

2006 ABR Part II - Therapy Physics Type

- For what isotope is the ratio of dose at d=5 cm to the dose at d=1 cm the lowest? Co, Cs, I, Pd? *Pd (low E)*
- How often are electron energies checked according to TG-40? Once a week. Once a week if they are used twice a week, etc.
- DVH - which plan has the lowest fraction of volume receiving 15-20 Gy?

- What measurement device is best for a simulation room survey? ion chamber, ion chamber w/ electrometer, GM, scintillation counter? *need quantitative measurement*

- If a patient is prescribed 200 cGy a fraction with 30% open and 20% wedged for each field, what dose does the patient receive if the wedge is put in the wrong field? WTR=0.25. *D_w = 200 x 0.4 = 80 cGy ⇒ MU = 200 / CF = 200 / 0.25 = 800 MU*

- What is the definition of wedge angle? *D₀ = 200 x 0.5 = 100 cGy ⇒ MU = 100 / CF = 100 / 0.5 = 200 MU*

- Given lots of TG-51 parameters, calculate cGy/MU for photons. *D₀ = 200 x 0.5 = 100 cGy ⇒ MU = 100 / CF = 100 / 0.5 = 200 MU*

- Given lots of TG-51 parameters, calculate cGy/MU for electrons. *D₀ = 200 x 0.5 = 100 cGy ⇒ MU = 100 / CF = 100 / 0.5 = 200 MU*

- With 6 MV incident on x1 mm tissue then x2 mm bone then x3 mm lung, what is the dose to the proximal (or distal, I forget) part of the lung? *proximal: -0.25 cm x 2% = -0.005 cm*

- Shown CT with depths of tissue and lung, single direct field, and attenuation coefficients, what is the dose w/ and without heterogeneity corrections? *CF = 1 / TAR(1.0) = 1 / 0.45 = 2.22*

- Given mixed energy, electron and photon, dose to surface = 40 Gy and PDDs at surface for each given, and dose to d=5 cm = 55 Gy, PDDs for each at d=5 given, what are the relative contributions of photons and electrons at dmax? *CF_{ph} = TAR(2.0) / TAR(1.0) = 0.45 / 0.45 = 1.0*

- Mammosite balloon w/ diameter = 4 cm and Rx point at 1 cm from surface of balloon. What is the minimum balloon to skin distance to minimize the hot spot to 150%? *D₀ = 200 x 0.5 = 100 cGy ⇒ MU = 100 / CF = 100 / 0.5 = 200 MU*

- What thickness of Al to compensate for 5 cm of missing tissue? *T = 5 cm x 0.08 cm/cm = 0.4 cm*

- Dose at point S is 6 mrem/hr. How much concrete shielding to get dose at point Z less than 2 mrem/hr. Point S is 6 m from iso and Point Z is 12 m from iso. Given TVL of concrete. *D₀ = 200 x 0.5 = 100 cGy ⇒ MU = 100 / CF = 100 / 0.5 = 200 MU*

- If the daily output is greater than what % is patient treatment suspended immediately according to TG-40? *5%*

- What is the overall uncertainty in dose delivered to a point in a patient with all uncertainties taken into consideration? Kahn - 5.6%

- What method cannot be used to verify an IMRT plan? Film, point hand calc?

- What is the purpose of the bending magnet?

partid: mean dose < 2500 cGy in at least one gland or 20cc of both glands < 2000 cGy

brainstem < 5400 cGy; 1cc < 6000 cGy

optical chiasm/optical nerves: < 5400 cGy, 1cc < 6000 cGy

temporal lobes: < 6000 cGy, 1% < 6500 cGy

cord: < 4500 cGy, 1cc < 5000 cGy


backbone: < 6000 cGy

EFS: < 3500 cGy

lens: < 4500 cGy

19. Where are the electrons generated in a linac? electron gun

20. What does Gamma measure?

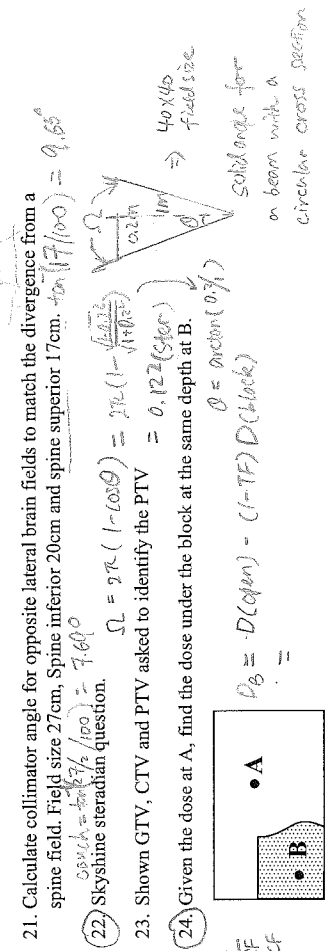

21. Calculate collimator angle for opposite lateral brain fields to match the divergence from a spine field. Field size 27cm, Spine inferior 20cm and spine superior 17cm. $\tan^{-1}(17/20) = 40.1^\circ$

22. Skyshine steradian question. $\Omega = 2\pi(1 - \cos\theta) = 2\pi(1 - \frac{17^2}{17^2 + 27^2}) = 7.69$

23. Shown GIV, CTV and PTV asked to identify the PTV = 0.122 (40%) \Rightarrow 40% of field size

24. Given the dose at A, find the dose under the block at the same depth at B. $D_B = D(A) - (1 - TF) D(block)$

25. When to check the wedge interlock monthly


26. IMRT Head and Neck treatment. What are the dose constraints for critical organs.

27. The tolerance dose for the kidney TD5/5: 2300 cGy TD5/5: 2800 \Rightarrow 2000 cGy

28. Scanning PDD curves given and asked to identify which is which.

29. What is the reference depth used in photon beam calibrations (per TG-51) 10 cm

30. Shielding problem. Distances given: Linac to A=6m, Linac to B=12m. Survey meter measures xx mrem/hr at point A. Dose delivered at each treatment is also given. How many patients can be treated to limit the exposure at point B to below 2 mRem/wk or 2 mR/hr

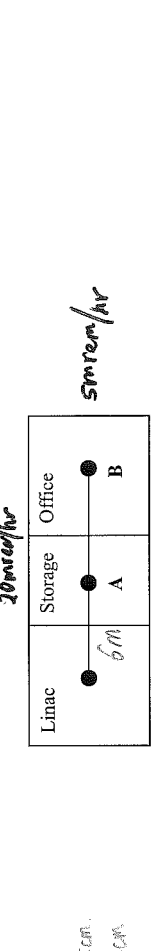

31. Gamma strength problem related to HDR treatment.

32. Question on changing Brachytherapy sources from ^{192}Ir to ^{125}I (or vice versa) and calculating activity/dose rate. ^{192}Ir : 14.9 Rcm/hr-mCi \cdot (4000) \cdot $f(0.495 \text{ cGy/hr} \cdot \text{cm}^2) \cdot (70^\circ) = D$

33. IMRT dose verification using small volume chamber (0.1cc). What should its resolution (or measured error) be in order to be able to use for dose verification (ans: 0.1%, 0.5%, 1%, 3%, 10%)

$I : SKCU \cdot \Lambda(\text{cm}^2/\text{hr} \cdot \text{cm}^2) \cdot 60(\text{s}) \cdot 910 \cdot FIC(\theta) = D$

$0.94 \sim 1.036$

photon hot, electron cold

34. Beam abutment question. Patient treated with 10MV photons and 16MeV electrons. Field size given. At 5cm depth what would be the case (photon side hot spot: electron side cold spot, photon side cold spot: electron side hot spot, both sides hot spots, both sides cold spots or no hot spots)

35. Morning (daily) QA for a HDR brachytherapy treatment source per TG-40

36. Daily output tolerance for X-ray and electrons (3%, 5%, 3%, 3%, 2%, 3%, 5%, 5% etc) at depth d3 what is the energy

37. $E_p = E_0 (1 - d/R_p)$ given that at depth d1, the energy is E1 and at depth d2 the energy is E2, at depth d3 what is the energy

38. Question on backscattering using block for electron beams. How does it change with energy E and Z. (increase when E and Z increases, decreases when E and Z decreases. Increases when E increases and decreases when Z increases and vice versa)

39. This time there were about 4-5 questions about the TG-51. We were provided all the detailed information about the different factors and asked to calculate the Mu's/cGy to deliver at Dmax. 2 questions about the Photon beam and 2 question about the e-beam. In some questions you have to calculate the Pion & Ppol.

40. HDR shielding calculation. Everything was provided. Just use the formula and answer was there. \Rightarrow check

41. One beam profile diagram was provided with profile line variation at the surface. The reason for that....Ans was---Water fluctuation.

42. Shielding calculation. the thickness was calculated as per the 6 MV beam and the Exposure level was given at particular point. question was to calculate the exposure level if 18 MV beam is used for the same thickness. TVLs were given.

$$D_{\text{dose}} = D \cdot \left(\frac{0.1}{0.1} \right)^{\frac{\text{thickness}}{\text{TVL}_{\text{beam}}}}$$

$$D_{\text{dose}} = D \cdot \left(\frac{0.1}{0.1} \right)^{\frac{\text{thickness}}{\text{TVL}_{\text{beam}}}} = \frac{D_{\text{dose}}}{\left(\frac{0.1}{0.1} \right)^{\frac{\text{thickness}}{\text{TVL}_{\text{beam}}}}}$$

✓ Khan's book:
 $R = \frac{P \cdot d \cdot t}{W \cdot T}$ depends on W @ m² cm
 From McGinley: McGinley use 4.8 R/
 $W = I_0 \cdot f \cdot A \cdot t \cdot \left(\frac{0.96 \text{ g/cm}^2}{\rho} \right) \cdot (A \cdot \text{cm}^2) \cdot (t \cdot \text{hr})$
 $= (4.69 \text{ Rcm}^2/\text{hr}) \cdot (A \cdot \text{cm}^2) \cdot (t \cdot \text{hr})$
 $t = \frac{(\text{Dose per patient}) \cdot (\# \text{ of patients})}{(\text{dose rate @ 10cm})}$
 $\rightarrow 1 \text{ Gy/min for 10Ci source can be assumed.}$

For example:
 10 Gy per patient, 25 patients per week
 $\Rightarrow t = \frac{10 \times 25}{1} = 250 \text{ min.}$
 $TW = 4.69 \times 0.96 \times 10000 \times \frac{250}{60} = 1.876 \times 10^5 \text{ cGy/hr @ 10cm}$
 $18.76 \text{ cGy/hr @ 1m.}$

To calculate dose at more dose
 $H = \frac{(10 \text{ Ci}) \cdot T_0 \cdot \text{Area}}{d^2 \cdot d_0^2}$
 d_0 : distance from source to wall
 d : more length.
 McGinley mention that dose rate in the more fall off slower than TVS.

HDR

TG-50: Table V.

Daily QA: for remote afterloading facility:

- verify dose delivery accuracy
- dose, time, source strength, time accuracy
- overall system function.
- simulated treatment
- treatment status indicator lights
- critical source control forwarded
- safety
- door interlock
- door indicator monitor
- area indication
- A/V communication
- emergency equipment
- positional accuracy 1mm
- temporal accuracy

TG-51:

- (1) correct function of:
 battery. A/V treatment status. A/V communication.
 indication monitors. simulated treatment.
 door interlock alarms.
- (2) Accuracy of:
 delayed source strength programmed in TPS and treatment units
 timer, radiation output using tertiary standard or timer spot check.
 source position.
 Availability, condition, function of emergency kit and tools.
 instructions.
 survey meters.
- (3)

Table VIII QA for remote afterloading
 door interlock: lights, alarms
 console functions, switches, batteries.
 visual inspection of source guide
 verify accuracy of ribbon preparation

photon production
 $\chi(x, r, r) A^2 X$
 threshold energy for (x, r)

meV
Al 131
Fe 104
Co 69
Pb 674

2007 Therapy Part II Type

Simple Questions: (each one counts 1 point, total 53 questions/points)

1. Neutron dose equivalent (mSv) outside field per photon Gy at isocenter for 20MV beam.
 $1.0 \times 10^{-6} \text{ mSv/Gy}$
2. Scatter and leakage shielding thickness calculations are equal. The shielding that should then be used is (A) TL + IHVL, B other options including Ts + TL, Ts + ITVL.
 $1.0 \times 10^{-6} \text{ mSv/Gy}$
3. Parts definitely not included in EPID - options were ion chamber, CCD camera, mirror, silicon screen, some other dose detection device.
 liquid
4. TBI - what is not true - A. Dose Uniformity < 15%, B. Tissue Equivalent Compensators are used, C. High SSD, D. AP preferred over lateral, E. Lower dose conformity with increased energy.
 high E, better uniformity
5. S/rho and rho given for lead. Calc thickness of lead used to shield 20MeV beam.
 $(S/\rho) \cdot \rho = S \rightarrow \text{meV/cm} \Rightarrow (0.021 \text{ MeV/cm}) / (11.34 \text{ g/cm}^3) = (0.00185) \text{ cm}$
6. How many TVL's in a linac head?
 $3 \text{ TVL} \approx 0.001$
7. PDD for wedge increases over open field due to: A. Photon interactions in the wedge B, C, D, E....
8. Purpose of the guard ring in a plane parallel chamber is to? (A) Define the collection volume appeared to me to be the only reasonable answer. + no purpose reduce charge leakage.
9. Electrons at extended SSD, which is true?
 A. Width of the 90% extends proportionately B. Penumbra increases C. Output follows ISL with 100 to source ...
10. Why does the equivalent square technique work? A. Because scatter doses are equal between square and rectangular fields. Other options involved statement about collimators and scatter that sounded wrong
11. TG51: what's upper limit for Pion? 1%, 3%, 5%, 10%.
12. TG51: where is cylindrical chamber's center placed for photon beam calibration? $d = 10 \text{ cm}$, photon? no shift
13. TG51: to cross calibrate parallel-plate chamber, what should use?
 Co60, high energy photon, high energy electron, low energy electron.
14. TG51: KQ depends on what? (choices included beam energy, ion chamber, both) both.

15. TG51: What's energy specification for electron beams?
 most probable energy $E_0 = 1.6 \times 10^{-13} \text{ J}$

16. TG51: total consecutive measurements were done with 20% difference, the reason is: 100 SSD vs 100 SAD; etc.

depths of PDD
 15-40
 2mm @ isocenter
 depth

$$\Phi(H \text{ of } r) = \Phi_{\text{air}} + \Phi_{\text{scat}} + \Phi_{\text{th}}$$

$$\text{per cm}^2 = \frac{Q}{4\pi r^2} + 540 \frac{Q}{S} + 1.26 \frac{Q}{S}$$

Q : neutrons per Gy (1/Gy)

Q : neutron dose equiv.
 at distance do (14m) from target. (mSv/Gy)
 range 0.82 m to 3.3 for 13 accelerators

17. TG51: where is the effective point of measurement of parallel-plate chamber?
 surface
18. How do you convert ionization curve to %dd curve? using stopping power correction of stopping power ratio of water to air
19. Agent used in PET? 18FDG

20. 9MeV electron beam. At 4 cm depth, how much lead should be used to shield deeper structure? No other information. $Q_{\text{MeV}} \Rightarrow R_p = 4.5 \text{ cm}$ $E = 9(1 - \frac{1}{1.6}) = 1 \text{ MeV} \Rightarrow 0.5 \text{ mm lead}$

21. Difference between physical wedge and dynamic wedge. Beam hardening.

22. IMRT: Difference between simulated annealing and gradient reduction in IMRT? Faster, more accurate in dose calculation in build up, better with step-and-shoot than with sliding window, achieve global minimum instead of local, etc.

23. IMRT: one fluence map is shown for 5 fields prostate IMRT, identify the field. AP, RPO, RAO, LAO, LPO.

24. Klystron's function.

25. Gas pressure low fault is related to which part in Linac? Gun, Waveguide, Magnetron, Accelerating tube, etc.
 vacuum!

26. Linac's outputs are off the same way for all the beams, what is the problem? klystron, bending magnet, RF waveguide, monitor chamber - I said monitor chamber because it would be the most consistent

27. What's PTV?

28. Which organ shows partial volume effect? Brachial Plexus, Kidney, Optic nerve, etc.
 lung 1750 3000 4500 6000 7500 9000
 kidney 2500 3000 5000 7500 9000
 brachial plexus 6000 6100 6200 6300 6400
 optic nerve 6500

29. To compare light field vs. radiation field, film is used. Ask distances for SSD and film SAD. SSD=100, SAD=100; SSD=100-dmax, SAD=100; etc. According to them: film @ SAD.

30. Photon field abuts electron field, where is the hot spot? photon.
 plastic sheet thick enough to provide more electronic buildup

31. The Transport Index represents the exposure rate... (choices included "on the surface" and "at one meter") on the external surface $\Rightarrow 0.005 \text{ mSv/hr}$ white 2mSv yellow 10mSv yellow 100mSv yellow 1000mSv yellow

32. Mayneord's Factor is more accurate for: 6MV, 6x6, 110 SSD; 6MV, 30x30, 150 SSD; 15MV, 6x6, 110 SSD; 15MV, 6x6, 150 SSD; etc.
 in green, "solid ordering"

33. What "stereotactic" means in stereotactic radiosurgery \Rightarrow use 3D coordinate to localize small targets

34. TG43: what is A? dose rate constant (cGy/hr/g) @ (1cm, 90°)

35. Tolerance for simulator laser vs. gantry center (or some other mechanical center)?
 $\frac{\text{fiducial}}{\text{fiducial}} = \frac{\text{fiducial}}{\text{fiducial}}$ $\rightarrow 2 \text{ mm}$ 2mm radiation center

coincidence of coll. gantry, couch axes with iso center: 2 mm diameter

F errors if $\left\{ \begin{array}{l} \text{large field change} \\ \text{large SSD change} \\ \text{large depth} \end{array} \right.$

36. Amount of X-ray contamination of 18 MeV electron beam? 1%, 4%, 10%, etc.

37. IMRT shielding: how much more shielding needed? All wall + TVL; Primary + TVL; Secondary + HVL; Secondary + TVL, etc.

38. If you were going to use a thimble chamber to calibrate an Ir192 source what type of beam would need to be used in determining the calibration factor? Calibrate with 192Ir, Calibrate with 380 keV X-ray, Cobalt-60 etc.

39. 45Gy photon treatment to neck. Choose electron energy for boost to treat nodes at 3cm depth and spare cord at 5cm depth. $R_p < 5cm$ $R_{sp} > 5cm$ $E = 3 \times 3.8 = 11.4MeV$

40. Treat 4.3 cm depth with 12 MeV and 200 cGy, dose at dmax. $E = 17MeV$ $R_{200} = 5/1.8 = 2.8cm$

41. Multi detector CT, when cone beam increases size, what's true: Collimator decreases, scatter photon increases, etc. (not quite sure about the answers)

42. Shielding: What's peak energy of photons near door? 200 keV, 500 keV, etc.

43. Shielding: Electron only machine has 4 electron energies, each with 3.5%, 2%, 1.5%, and 1% X-ray contamination. Workload 200 Gy/week, what is weekly workload for photon contamination?

44. Decay rate of 192Ir per day. 1% per day

45. Weekly dose limit for unrestricted area. 0.02mSv/pk 0.02mSv in any hour

46. GM counter property. \Rightarrow high sensitivity, but has quenching issue - slow recovery time

47. A question involving 10mg Ra - simple application of $\Gamma \propto A/d^2$ - but needed to know (i.e. not given) exposure rate const. = 8.25 Rem2/mg.hr

48. Breast Tangent pair. Field widths at 100 SAD = 10.5 cm. LAO has gantry angle 45 degrees. What gantry angle does RPO have such that posterior borders will be parallel?

49. Difference between Acceptance Test and Commission of Linac.

50. Tolerance for deviation in a light field for a CT sim

51. How much dose is given for an I-125 seed 1.44DoT1/2(1 - e^{-ln2t/T1/2})

52. What is the dose rate at 1m from a patient receiving external beam treatment

53. If the high voltage power source is pushing too much, what is the most likely observed result on the accelerator.

54. Which modality (photons or electrons) and energy is used to cross calibrate a parallel-plate chamber with a cylindrical chamber.

55. Electron beam quality is specified by (R50, Dref etc, dmax etc)

56. Given a table of PDD's 4 MV and 18 MV what is the ratio of max dose 4MV/18MV.

57. Effect on point outside treatment field when using dynamic wedge versus hard wedge.

Complex Questions: (each one counts 3 points, 27 questions, and total points 81)

1. HDR, three dwell positions (1, 2 and 3 - 2 in middle) 1cm apart in single channel. Dose points A, B and C 1cm perpendicular to dwell positions 1, 2 and 3 respectively. What is the ratio of dwell times 1 to 2 to make dose A equal dose B?

2. AP/PA doses given from each field to cord for 200 cGy to tumor (62cGy, 150cGy respectively). Cord block put in PA, new cord dose is 18% of original. How many fractions need cord block to limit cord dose to 40Gy? $D_c = 62 + 18 = 80$ $D_c = 21 \times 0.18 = 3.8$ $3.8/16 = 0.24$ $21 \times 0.24 = 5.04$

3. A lead pig with 2 cm wall thickness is inside a 30cm diameter polyurethane foam shipping drum. HVL of lead was given (=3.5mm). Exposure rate constant of 192 Ir was given (0.32 mR/mCi hr at 1 meter). Calculate max activity to keep exposure rate below 50mR/hr on the drum surface.

4. TBI, diode reading 450cGy on surface, prescribed midline 600cGy POP laterals, 30cm separation. TMRs were given with 350cmSSD. What is error in midline dose? A. 2.6% higher, etc.

5. Three isocentric beams 120 deg apart, AP and post obliques. Each goes through 15 cm depth to isocenter. 180Gy at isocenter weighted equally for three beams. Post beams transfer 9cm lung (electron density= 0.33), TMRs given at 3,6,9,12,15 cm. Calculate MU(post obliques)/MU(AP).

6. Ratio of Maximum Dose between 25MV and 4MV for same dose to midline using POP setup with SSD=100cm. PDD's given.

7. Given Kersey's formula and the distances and ratio of maze areas, neutron dose at isocenter (mSv) per photon cGy at isocenter, what is neutron dose (mSv) at door per photon cGy at iso

8. HDR 192Ir. Patient treated with time 420sec with Activity 3.75Ci on Aug 1st. Source got replaced with activity 9.43Ci on Aug 16th. Calculate treatment time on Aug 21st. No 192Ir half life given.

9. Given dose to point A 200 cGy, calculate thickness of block to achieve point B dose 90 cGy. TMR, %DD, and HVL given, depth may be different for B.

we R50 calculate R50 or look up table

longer beam on time

more scattering, leakage

to area that is an intended of the field

According to

Volume

able to perpendicular

green: EDN < physical wedge

Complex Questions: (each one counts 3 points, 27 questions, and total points 81)

38. If you were going to use a thimble chamber to calibrate an Ir192 source what type of beam would need to be used in determining the calibration factor? Calibrate with 192Ir, Calibrate with 380 keV X-ray, Cobalt-60 etc.

if $Ci = 5$

39. 45Gy photon treatment to neck. Choose electron energy for boost to treat nodes at 3cm depth and spare cord at 5cm depth. $R_p < 5cm$ $R_{sp} > 5cm$ $E = 3 \times 3.8 = 11.4MeV$

40. Treat 4.3 cm depth with 12 MeV and 200 cGy, dose at dmax. $E = 17MeV$ $R_{200} = 5/1.8 = 2.8cm$

41. Multi detector CT, when cone beam increases size, what's true: Collimator decreases, scatter photon increases, etc. (not quite sure about the answers)

42. Shielding: What's peak energy of photons near door? 200 keV, 500 keV, etc.

43. Shielding: Electron only machine has 4 electron energies, each with 3.5%, 2%, 1.5%, and 1% X-ray contamination. Workload 200 Gy/week, what is weekly workload for photon contamination?

44. Decay rate of 192Ir per day. 1% per day

45. Weekly dose limit for unrestricted area. 0.02mSv/pk 0.02mSv in any hour

46. GM counter property. \Rightarrow high sensitivity, but has quenching issue - slow recovery time

47. A question involving 10mg Ra - simple application of $\Gamma \propto A/d^2$ - but needed to know (i.e. not given) exposure rate const. = 8.25 Rem2/mg.hr

48. Breast Tangent pair. Field widths at 100 SAD = 10.5 cm. LAO has gantry angle 45 degrees. What gantry angle does RPO have such that posterior borders will be parallel?

49. Difference between Acceptance Test and Commission of Linac.

50. Tolerance for deviation in a light field for a CT sim

51. How much dose is given for an I-125 seed 1.44DoT1/2(1 - e^{-ln2t/T1/2})

52. What is the dose rate at 1m from a patient receiving external beam treatment

53. If the high voltage power source is pushing too much, what is the most likely observed result on the accelerator.



54. Which modality (photons or electrons) and energy is used to cross calibrate a parallel-plate chamber with a cylindrical chamber.

55. Electron beam quality is specified by (R50, Dref etc, dmax etc)

56. Given a table of PDD's 4 MV and 18 MV what is the ratio of max dose 4MV/18MV.

57. Effect on point outside treatment field when using dynamic wedge versus hard wedge.

Complex Questions: (each one counts 3 points, 27 questions, and total points 81)

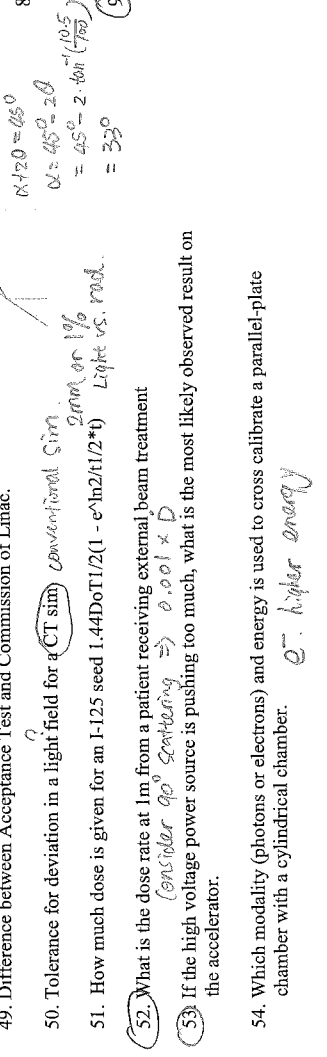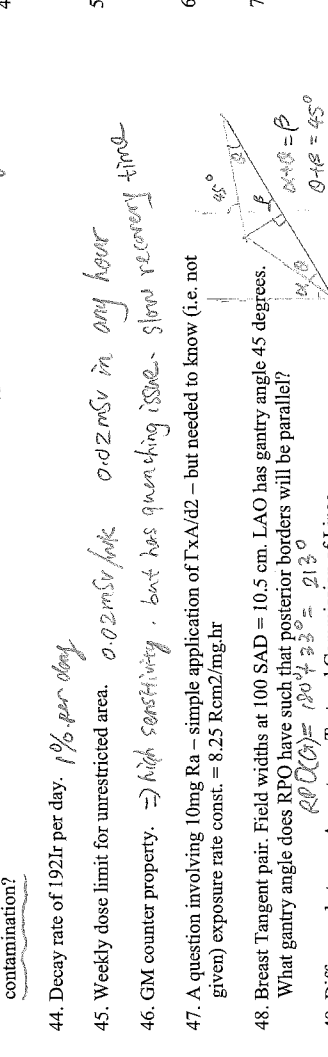

wedge angle:

the angle between wedge isodose line

and a line \perp to C.A.X of beam at depth of 10cm.

Not 50% isodose \leftarrow old definition

\Rightarrow because we greater depth, the isodose angle become smaller

because the increased scatter will reduce the wedge effect.

wedge angle:

the angle between wedge isodose line


and a line \perp to C.A.X of beam at depth of 10cm.

Not 50% isodose \leftarrow old definition


\Rightarrow because we greater depth, the isodose angle become smaller

because the increased scatter will reduce the wedge effect.


FS	5, 7, 10, 15, 20
OF	
TMR(7cm)	
%dd(7cm)	



22. Point A and B are candidates for machine isocenter. Point C is outside the primary shielding and distances AC(=7m) and BC(=5m) are given. If isocenter is set at A, measurement at C is within the MPD specification. If isocenter is changed to B, how much more shielding (TVL) is needed for the wall to maintain same reading at C, given TVL.

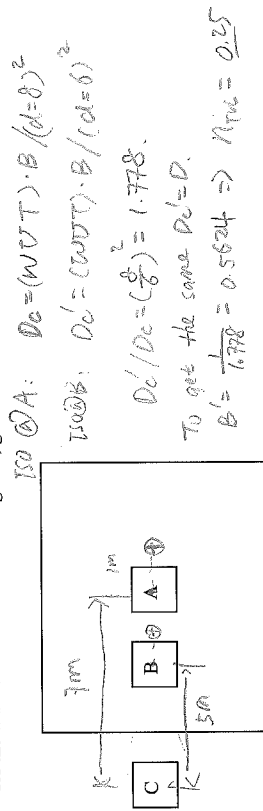


23. From source to point A, there are: 100 cm SSD to surface, then 3 cm tissue, 2 cm inhomogeneity ($\rho_e=0.25$), 3 cm tissue, another 3 cm inhomogeneity ($\rho_e=2.5$), finally 4 cm tissue. So depth is 15 cm. 4MV beam delivers 200 cGy to point A with inhomogeneities. What's the dose to point A without the inhomogeneities? (TMRs were given).

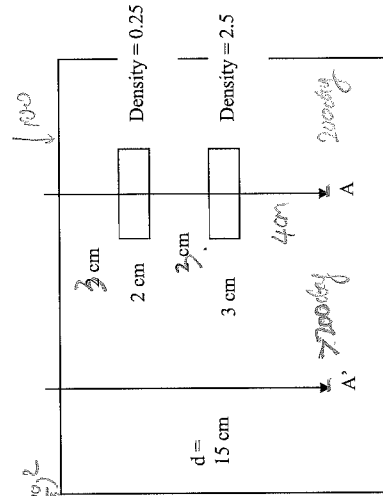


TMR ratio:
 $d_{\text{eff}} = 3 + 2 \times 0.25 + 3 + 3 \times 2.5 + 4 = 18 \text{ cm}$
 $CF = \frac{TMR(d=18, r=15 \text{ cm})}{TMR(d=15, r=15 \text{ cm})} < 1$
 $D_A' = D_A / CF = 200 / CF$
 $CF = \left(\frac{D_{\text{with TM}}}{D_{\text{no TM}}} \right) \Rightarrow \text{check!}$

Handwritten calculations for Question 10:
 $DA = DC$
 $= (D_e \cdot m) \cdot (1 - TE) \cdot D_{\text{block}}$
 $= (D_e \cdot m) \cdot (1 - TE) \cdot D_{\text{block}} - (1 - TE) \cdot D_{\text{block}}$
 $= D_{\text{block}} - (1 - TE) \cdot D_{\text{block}} - (1 - TE) \cdot D_{\text{block}}$
 $= D_{\text{block}} - 2 \cdot (1 - TE) \cdot D_{\text{block}}$
 $= D_{\text{block}} \cdot (1 - 2 \cdot (1 - TE))$
 $= D_{\text{block}} \cdot (2 \cdot TE - 1)$
 $Sc(100 \text{ cm})$



10. 36 inch space is available for 6 TVL shielding. Given Pb TVL (2 inch) and Concrete TVL (18 inch), what is the minimum thickness of Pb needed?

Handwritten calculation:
 $n_{Pb} \cdot 2 + (6 - n_{Pb}) \cdot 18 \leq 36$
 $\Rightarrow n_{Pb} \geq 4.5$
 $4.5 \times 2 = 9 \text{ inch}$



11. Sim film taken at 102cm SSD, SFD 140cm. Want to treat at 120cm SSD. $m_{92} = \frac{140}{102}$. What distance to film should be used when cutting blocks. $8FB = 120 \times \frac{140}{102} = 165 \text{ cm}$.

12. Field size is measured 56 cm on patient skin and collimator 40 cm with table at its lowest position 167 cm from the source. What's patient size (including setup bag etc.)?

Handwritten calculation:
 $\frac{167}{56} = \frac{56}{f} \Rightarrow f = 140$
 $167 - 140 = 27 \text{ cm}$

13. Given diagram of one dimension blocked field with distance from CAX and table of SARs (0cm 6cm 9cm 10cm etc), calculate SAR. (Block I)

14. Superficial X-ray, measurement at end of cone gives a reading of 150. Measurement at 10cm from the end of the cone gives a reading of 52.3. What is the effective SSD at the end of the cone?

Handwritten calculation:
 $\frac{150}{52.3} = \left(\frac{f+d_{\text{eff}}}{f+10} \right)^2 \Rightarrow f+d_{\text{eff}} = 14.49 \text{ cm}$

15. Dose to cord from AP/PA 100 SAD setup. Given 22cm separation, cord 4cm deep, and 200cGy to isocenter. $AP: D_{\text{ne}} = 100 = MU \cdot Sc \cdot Sp(r) \cdot TMR(r, d=11) \cdot (100)^2$. $PA: 100 = MU \cdot Sc \cdot Sp(r) \cdot TMR(r, d=11)$.

16. Film exposed for dosimetry. Given transmitted light is 200 times smaller than original, what is the dose? OD vs dose table was given. $OD = \log 200 = 2$

17. Single field 125 cm SSD, 4x17, 300cGy was prescribed to 5cm deep. Given PDD table and TMR table, calculate MU. No Output factor vs. field size! No machine calibration condition.

Handwritten calculation:
 $MU = \frac{300}{Sc \cdot Sp \cdot TMR(6.5 \times 17.5, d=5)} \cdot \left(\frac{100}{125} \right)^2$ or $Sc \cdot Sp \cdot PDD(6.5, f=12.5, d=5) \cdot \left(\frac{100}{125} \right)^2$

18. 15 x 20 POP, calculate MU for dose required. No Output factor vs. field size! No machine calibration condition, SSD or SAD!

19. Multiple beams plan: AP weighted to 100% at dmax, laterals weighted to 100% at dmax. 200 cGy delivered to 238% isodose line. What is the dose delivered by AP beam? $AP: D_{\text{AP}} = D_{\text{plan}} \cdot PDD(f, r, d)$

20. Given readings at 10 cm depth for 10 x 10 and 20 x 20 fields with 100 cm SAD, and two TMRs, calculate the Scp(20).

21. 15 x 15 field with 3 x 15 block in the center, which has 5% transmission factor. Depth at 7 cm, dose to point A given with 1.01 OCR, calculate dose to CAX under block, given table like:


Handwritten calculations for Question 21:
 $D_{\text{CAX}} = D_{\text{plan}} \cdot Scp(20) \cdot TMR(10 \times 10, d=7) \cdot (100)^2$
 $D_{\text{CAX}} = D_{\text{plan}} \cdot Scp(20) \cdot TMR(10 \times 10, d=7) \cdot (100)^2$
 $D_{\text{CAX}} = D_{\text{plan}} \cdot Scp(20) \cdot TMR(10 \times 10, d=7) \cdot (100)^2$

24. Given primary workload, distance to office, and TVL, calculate shielding thickness to achieve 1/10 of MPD. U, T, MPD were not given.

W d. T=1 B = $\frac{Pd^2}{WUT}$ P = 0.02 mS/week
 Assume U = 1/4 = 0.25

25. If dose to point A (depth 10 cm) is 200 cGy, calculate dose to point B ignore beam divergence. %DD(10)=65%, %DD(12.5)=56%, 100 SSD alone CAX.

In this case h = -2.5 d = 12.5 always defined at point surface

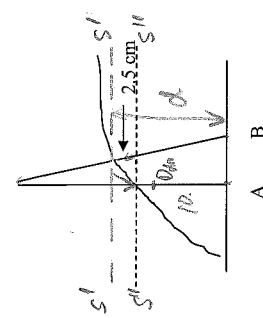

SSD = 100 cm @ CAX.

$D_B = D_A \cdot P'$ $P_{corr} = P' \cdot \left(\frac{D_{ref}}{D_d} \right)$

$D_B = D_{ref} \cdot P_{corr}$ $= P' \cdot \left(\frac{SSD + d_m}{SSD + d_B + h} \right)^2 = P' \cdot \left(\frac{100 + 1.5}{100 + 1.5 - 2.5} \right)^2$

P' is always relative to surface at S-S'

$P'(d) = P'(12.5)$

26. Lung correction given dose with no correction - the corrected dose has 2 cm of lung and 4 cm of dense medium (4x tissue) - what is the dose at that second point?

$6mV = 2.5\% / cm$ lung $\Rightarrow (-2.5\%) \times 2 + (2.5\%) \cdot 4 = 5\% \text{ less dose}$

27. Orthovoltage shielding calculation given the workload.

28. What would cause the biggest change of the depth of the 80% IDL for a 9 MeV electron? (choices included: add 1 cm bolus, change to 18 MeV, increase FS)

$R_{90} = \frac{9}{2.8} = 3.21$

$R_{90} = \frac{18}{2.8} = 6.42$ change by 1 cm

General Observations:

- Shielding questions -- lots of them!
- Lots and lots of dosimetry calculations:
- If you have the PDD or TMR data, how many MUs required?
- Know when to use Mayneord F factor and when to ratio TMRs
- Know relative depth doses for all electrons and photons
- Know definition of terms in TG-51:
- Numerous gap cales
- Lots of SSD and SAD treatments, max dose, midplane dose.

One or two, electron beams problems. Not too many. All the fields were rectangle and you had an additional calculation to convert to the equivalent square. TG 51 questions but not difficult. Raphex is very good for the easy questions and Khan and McGinley are good for the others. Lots of practice with the windows calculator. Some problems with long sets of calculations.

For TMR/TAR:

$CF = \frac{T(d, r_A)}{T(d+h, r_A)} = \frac{T(12.5, r_A @ d=12.5)}{T(12.5-2.5, r_A)} < 1$

P'' relative to S''-S'

$P'' = PDD(10) = 65\%$

$P_{corr} = P'' \cdot CF$

or using TMR

$d_{eff} = 2 \times 0.25 + 4 \times 4 = 16.5$


$d = 2 + 4 = 6$

$\Delta d = 10.5 \text{ cm}$

$6mV \ 3.5\% / cm$ for attenuation





$3.5\% \times 10.5 = 36\%$

Down ↓ for large field size

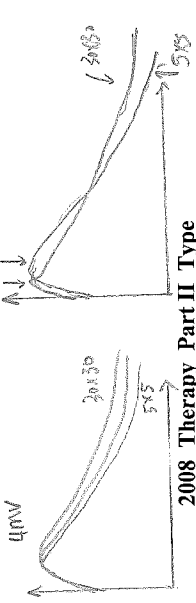

For proton beam PDD with field size, E. see reference course notes

2008_Therapy_Part II_Type

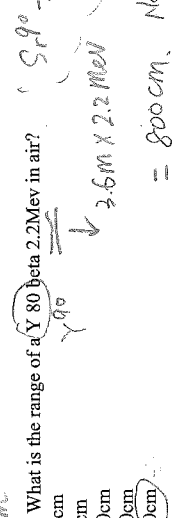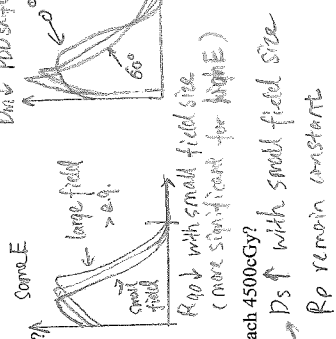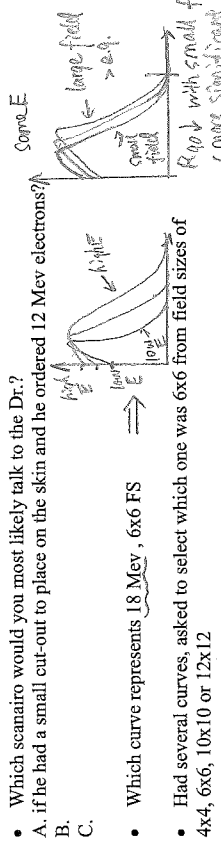

What is the range of a Y 80 beta 2.2 MeV in air? $S.P. \rightarrow 0.5 \text{ MeV} \Rightarrow 200 \text{ cm}$
 $3.5 \text{ m} \times 2.2 \text{ MeV} = 800 \text{ cm}$ No answer match!

Effective energy of an electron Ez 4 MeV, depth is 1.7 cm and an Eo is 7.1 MeV Two energies given. $E_2 = E_0 (1 - \frac{z}{R_p}) \Rightarrow 4 = 7.1 (1 - \frac{1.7}{R_p}) \Rightarrow R_p = 3.9 \text{ cm}$

Picture of squares, 3 cm, then 2 cm then 1 cm which equals tissue, bone and air. What is the effective depth when the beam is directed through each material.

A universal wedge has a 0.65 wedge factor. A 60 degree wedge is needed. 100 Mu are given, for open and 200 Mu given for the wedge field. What is the average WF? $WF = \frac{WF_{open} + WF_{wedge}}{2} = \frac{1.0 + 0.65}{2} = 0.825$

Overall uncertainty according to TG40? $6\% (5\% \text{ 4\% } 3\%)$ $WF = 0.565$ $WF = 0.435$ $WF = 0.65$ $WF = 0.767$

If the collimator rotation is off 1.2 mm, the couch rotation is off 1.4 mm and the gantry rotation is off 1.5. according to AAPM what is the overall uncertainty? $\sqrt{1.2^2 + 1.4^2 + 1.5^2} = 2.38 \text{ mm}$

Gap calculation: SAD 90 depth = 10, FS = 24 cm, but the treatment distance is changed to 100 SAD, d = 10, FS = 32 cm Assume two fields are the same

Calculate the steradian of a 50 cm diameter area on a standard linear accelerator.

a. .137
b. .122
c. .187

$\Omega = 2\pi (1 - \cos \theta)$
 $\Omega = 2\pi (1 - \frac{1}{\sqrt{1 + 0.5^2}})$
 $\Omega = 0.1876 \text{ ster}$

gap 2 = $\frac{16}{60} \times 10 \times 2 = 3.2 \text{ cm}$

Two isotopes Pd (lambda = .016) (rho =) and I125 (lambda =) half life is 17 days for Pd and 60 days for I125. After 120 days what is the ratio of doses? $T_{1/2} = \frac{\ln 2}{\lambda}$

Monte carlo calculations stop calculating at what energy and bundles everything into one

10 kev \rightarrow no contribution to dose
 100 kev \rightarrow
 200 kev \rightarrow
 500 kev \rightarrow
 1 Mev

How often according to TG40 should the wedge latch be checked? Monthly

What are Monte Carlo space files???

A. It registers where electrons are in space for calculation?????

A picture of a DVH

Shows critical organs, PTV and GTV curves. Choose which curve represents the GTV

13.05 cG exposure, $W/e = 33.3/70$ 2.58 x 10 R/C What is the volume of gas in the chamber?
 $X = \frac{Q}{M} \Rightarrow X = \frac{Q}{W}$
 $IR = 2.58 \times 10^{-4} \text{ C/kg} = \frac{13.05 \times 10^{-6}}{1.29 \text{ kg/m}^3 \text{ V(m}^3\text{)}}$
 $\Rightarrow V = \frac{13.05 \times 10^{-6}}{2.58 \times 10^{-4} \times 1.29} = 3.92 \times 10^{-5} \text{ m}^3$
 $= 3.92 \times 10^{-5} \times 10^6 \text{ cm}^3$
 $= 39.2 \text{ (cc)}$

HDR shielding question. How much thickness for 10 patients per week, 5 days a week, 500cGy/patient. The drawing showed a distance of 2 meters (I think that's what it meant).

$W = 500 \text{ cGy} \times 10 \times 5 = 25000 \text{ cGy/wk}$ \leftarrow wrong!!!
 $t = \frac{P_{\text{dot}}}{WUT}$
 $t = \frac{10 \times 5 \times 569}{154 \text{ hr/wk}} = 250 \text{ min}$
 $W = \frac{P_{\text{dot}}}{WUT}$
 $W = \frac{10 \times 5 \times 569}{154 \text{ hr/wk}} = 250 \text{ min}$
 $W = 1. \text{ for HDR}$
 $T = ?$ According to area
 $P = \left\{ \begin{array}{l} 1 \text{ ms/hr} \text{ for occupancy} < 2 \text{ ml/hr} \\ 0.1 \text{ ms/hr} \text{ for } 0.02 \text{ ms/wk} \text{ more conservative} \end{array} \right.$

Calculate the steradian of a 50 cm diameter area on a standard linear accelerator.

a. .137
b. .122
c. .187

$\Omega = 2\pi (1 - \cos \theta)$
 $\Omega = 2\pi (1 - \frac{1}{\sqrt{1 + 0.5^2}})$
 $\Omega = 0.1876 \text{ ster}$

gap 2 = $\frac{16}{60} \times 10 \times 2 = 3.2 \text{ cm}$

Two isotopes Pd (lambda = .016) (rho =) and I125 (lambda =) half life is 17 days for Pd and 60 days for I125. After 120 days what is the ratio of doses? $T_{1/2} = \frac{\ln 2}{\lambda}$

Monte carlo calculations stop calculating at what energy and bundles everything into one

10 kev \rightarrow no contribution to dose
 100 kev \rightarrow
 200 kev \rightarrow
 500 kev \rightarrow
 1 Mev

How often according to TG40 should the wedge latch be checked? Monthly

What are Monte Carlo space files???

A. It registers where electrons are in space for calculation?????

A picture of a DVH

Shows critical organs, PTV and GTV curves. Choose which curve represents the GTV

13.05 cG exposure, $W/e = 33.3/70$ 2.58 x 10 R/C What is the volume of gas in the chamber?
 $X = \frac{Q}{M} \Rightarrow X = \frac{Q}{W}$
 $IR = 2.58 \times 10^{-4} \text{ C/kg} = \frac{13.05 \times 10^{-6}}{1.29 \text{ kg/m}^3 \text{ V(m}^3\text{)}}$
 $\Rightarrow V = \frac{13.05 \times 10^{-6}}{2.58 \times 10^{-4} \times 1.29} = 3.92 \times 10^{-5} \text{ m}^3$
 $= 3.92 \times 10^{-5} \times 10^6 \text{ cm}^3$
 $= 39.2 \text{ (cc)}$

HDR shielding question. How much thickness for 10 patients per week, 5 days a week, 500cGy/patient. The drawing showed a distance of 2 meters (I think that's what it meant).

$W = 500 \text{ cGy} \times 10 \times 5 = 25000 \text{ cGy/wk}$ \leftarrow wrong!!!
 $t = \frac{P_{\text{dot}}}{WUT}$
 $t = \frac{10 \times 5 \times 569}{154 \text{ hr/wk}} = 250 \text{ min}$
 $W = \frac{P_{\text{dot}}}{WUT}$
 $W = \frac{10 \times 5 \times 569}{154 \text{ hr/wk}} = 250 \text{ min}$
 $W = 1. \text{ for HDR}$
 $T = ?$ According to area
 $P = \left\{ \begin{array}{l} 1 \text{ ms/hr} \text{ for occupancy} < 2 \text{ ml/hr} \\ 0.1 \text{ ms/hr} \text{ for } 0.02 \text{ ms/wk} \text{ more conservative} \end{array} \right.$

Calculate the steradian of a 50 cm diameter area on a standard linear accelerator.

a. .137
b. .122
c. .187

$\Omega = 2\pi (1 - \cos \theta)$
 $\Omega = 2\pi (1 - \frac{1}{\sqrt{1 + 0.5^2}})$
 $\Omega = 0.1876 \text{ ster}$

gap 2 = $\frac{16}{60} \times 10 \times 2 = 3.2 \text{ cm}$

Two isotopes Pd (lambda = .016) (rho =) and I125 (lambda =) half life is 17 days for Pd and 60 days for I125. After 120 days what is the ratio of doses? $T_{1/2} = \frac{\ln 2}{\lambda}$

Monte carlo calculations stop calculating at what energy and bundles everything into one

10 kev \rightarrow no contribution to dose
 100 kev \rightarrow
 200 kev \rightarrow
 500 kev \rightarrow
 1 Mev

How often according to TG40 should the wedge latch be checked? Monthly

What are Monte Carlo space files???

A. It registers where electrons are in space for calculation?????

A picture of a DVH

Shows critical organs, PTV and GTV curves. Choose which curve represents the GTV

13.05 cG exposure, $W/e = 33.3/70$ 2.58 x 10 R/C What is the volume of gas in the chamber?
 $X = \frac{Q}{M} \Rightarrow X = \frac{Q}{W}$
 $IR = 2.58 \times 10^{-4} \text{ C/kg} = \frac{13.05 \times 10^{-6}}{1.29 \text{ kg/m}^3 \text{ V(m}^3\text{)}}$
 $\Rightarrow V = \frac{13.05 \times 10^{-6}}{2.58 \times 10^{-4} \times 1.29} = 3.92 \times 10^{-5} \text{ m}^3$
 $= 3.92 \times 10^{-5} \times 10^6 \text{ cm}^3$
 $= 39.2 \text{ (cc)}$

HDR shielding question. How much thickness for 10 patients per week, 5 days a week, 500cGy/patient. The drawing showed a distance of 2 meters (I think that's what it meant).

$W = 500 \text{ cGy} \times 10 \times 5 = 25000 \text{ cGy/wk}$ \leftarrow wrong!!!
 $t = \frac{P_{\text{dot}}}{WUT}$
 $t = \frac{10 \times 5 \times 569}{154 \text{ hr/wk}} = 250 \text{ min}$
 $W = \frac{P_{\text{dot}}}{WUT}$
 $W = \frac{10 \times 5 \times 569}{154 \text{ hr/wk}} = 250 \text{ min}$
 $W = 1. \text{ for HDR}$
 $T = ?$ According to area
 $P = \left\{ \begin{array}{l} 1 \text{ ms/hr} \text{ for occupancy} < 2 \text{ ml/hr} \\ 0.1 \text{ ms/hr} \text{ for } 0.02 \text{ ms/wk} \text{ more conservative} \end{array} \right.$

Calculate the steradian of a 50 cm diameter area on a standard linear accelerator.

a. .137
b. .122
c. .187

$\Omega = 2\pi (1 - \cos \theta)$
 $\Omega = 2\pi (1 - \frac{1}{\sqrt{1 + 0.5^2}})$
 $\Omega = 0.1876 \text{ ster}$

gap 2 = $\frac{16}{60} \times 10 \times 2 = 3.2 \text{ cm}$

Two isotopes Pd (lambda = .016) (rho =) and I125 (lambda =) half life is 17 days for Pd and 60 days for I125. After 120 days what is the ratio of doses? $T_{1/2} = \frac{\ln 2}{\lambda}$

Monte carlo calculations stop calculating at what energy and bundles everything into one

10 kev \rightarrow no contribution to dose
 100 kev \rightarrow
 200 kev \rightarrow
 500 kev \rightarrow
 1 Mev

How often according to TG40 should the wedge latch be checked? Monthly

What are Monte Carlo space files???

A. It registers where electrons are in space for calculation?????

A picture of a DVH

Shows critical organs, PTV and GTV curves. Choose which curve represents the GTV

13.05 cG exposure, $W/e = 33.3/70$ 2.58 x 10 R/C What is the volume of gas in the chamber?
 $X = \frac{Q}{M} \Rightarrow X = \frac{Q}{W}$
 $IR = 2.58 \times 10^{-4} \text{ C/kg} = \frac{13.05 \times 10^{-6}}{1.29 \text{ kg/m}^3 \text{ V(m}^3\text{)}}$
 $\Rightarrow V = \frac{13.05 \times 10^{-6}}{2.58 \times 10^{-4} \times 1.29} = 3.92 \times 10^{-5} \text{ m}^3$
 $= 3.92 \times 10^{-5} \times 10^6 \text{ cm}^3$
 $= 39.2 \text{ (cc)}$

HDR shielding question. How much thickness for 10 patients per week, 5 days a week, 500cGy/patient. The drawing showed a distance of 2 meters (I think that's what it meant).

$W = 500 \text{ cGy} \times 10 \times 5 = 25000 \text{ cGy/wk}$ \leftarrow wrong!!!
 $t = \frac{P_{\text{dot}}}{WUT}$
 $t = \frac{10 \times 5 \times 569}{154 \text{ hr/wk}} = 250 \text{ min}$
 $W = \frac{P_{\text{dot}}}{WUT}$
 $W = \frac{10 \times 5 \times 569}{154 \text{ hr/wk}} = 250 \text{ min}$
 $W = 1. \text{ for HDR}$
 $T = ?$ According to area
 $P = \left\{ \begin{array}{l} 1 \text{ ms/hr} \text{ for occupancy} < 2 \text{ ml/hr} \\ 0.1 \text{ ms/hr} \text{ for } 0.02 \text{ ms/wk} \text{ more conservative} \end{array} \right.$

Calculate the steradian of a 50 cm diameter area on a standard linear accelerator.

a. .137
b. .122
c. .187

$\Omega = 2\pi (1 - \cos \theta)$
 $\Omega = 2\pi (1 - \frac{1}{\sqrt{1 + 0.5^2}})$
 $\Omega = 0.1876 \text{ ster}$

gap 2 = $\frac{16}{60} \times 10 \times 2 = 3.2 \text{ cm}$

Two isotopes Pd (lambda = .016) (rho =) and I125 (lambda =) half life is 17 days for Pd and 60 days for I125. After 120 days what is the ratio of doses? $T_{1/2} = \frac{\ln 2}{\lambda}$

Monte carlo calculations stop calculating at what energy and bundles everything into one

10 kev \rightarrow no contribution to dose
 100 kev \rightarrow
 200 kev \rightarrow
 500 kev \rightarrow
 1 Mev

How often according to TG40 should the wedge latch be checked? Monthly

What are Monte Carlo space files???

A. It registers where electrons are in space for calculation?????

A picture of a DVH

Shows critical organs, PTV and GTV curves. Choose which curve represents the GTV

13.05 cG exposure, $W/e = 33.3/70$ 2.58 x 10 R/C What is the volume of gas in the chamber?
 $X = \frac{Q}{M} \Rightarrow X = \frac{Q}{W}$
 $IR = 2.58 \times 10^{-4} \text{ C/kg} = \frac{13.05 \times 10^{-6}}{1.29 \text{ kg/m}^3 \text{ V(m}^3\text{)}}$
 $\Rightarrow V = \frac{13.05 \times 10^{-6}}{2.58 \times 10^{-4} \times 1.29} = 3.92 \times 10^{-5} \text{ m}^3$
 $= 3.92 \times 10^{-5} \times 10^6 \text{ cm}^3$
 $= 39.2 \text{ (cc)}$

HDR shielding question. How much thickness for 10 patients per week, 5 days a week, 500cGy/patient. The drawing showed a distance of 2 meters (I think that's what it meant).

$W = 500 \text{ cGy} \times 10 \times 5 = 25000 \text{ cGy/wk}$ \leftarrow wrong!!!
 $t = \frac{P_{\text{dot}}}{WUT}$
 $t = \frac{10 \times 5 \times 569}{154 \text{ hr/wk}} = 250 \text{ min}$
 $W = \frac{P_{\text{dot}}}{WUT}$
 $W = \frac{10 \times 5 \times 569}{154 \text{ hr/wk}} = 250 \text{ min}$
 $W = 1. \text{ for HDR}$
 $T = ?$ According to area
 $P = \left\{ \begin{array}{l} 1 \text{ ms/hr} \text{ for occupancy} < 2 \text{ ml/hr} \\ 0.1 \text{ ms/hr} \text{ for } 0.02 \text{ ms/wk} \text{ more conservative} \end{array} \right.$

Calculate the steradian of a 50 cm diameter area on a standard linear accelerator.

a. .137
b. .122
c. .187

$\Omega = 2\pi (1 - \cos \theta)$
 $\Omega = 2\pi (1 - \frac{1}{\sqrt{1 + 0.5^2}})$
 $\Omega = 0.1876 \text{ ster}$

gap 2 = $\frac{16}{60} \times 10 \times 2 = 3.2 \text{ cm}$

Two isotopes Pd (lambda = .016) (rho =) and I125 (lambda =) half life is 17 days for Pd and 60 days for I125. After 120 days what is the ratio of doses? $T_{1/2} = \frac{\ln 2}{\lambda}$

Monte carlo calculations stop calculating at what energy and bundles everything into one

10 kev \rightarrow no contribution to dose
 100 kev \rightarrow
 200 kev \rightarrow
 500 kev \rightarrow
 1 Mev

How often according to TG40 should the wedge latch be checked? Monthly

What are Monte Carlo space files???

A. It registers where electrons are in space for calculation?????

A picture of a DVH

Shows critical organs, PTV and GTV curves. Choose which curve represents the GTV

13.05 cG exposure, $W/e = 33.3/70$ 2.58 x 10 R/C What is the volume of gas in the chamber?
 $X = \frac{Q}{M} \Rightarrow X = \frac{Q}{W}$
 $IR = 2.58 \times 10^{-4} \text{ C/kg} = \frac{13.05 \times 10^{-6}}{1.29 \text{ kg/m}^3 \text{ V(m}^3\text{)}}$
 $\Rightarrow V = \frac{13.05 \times 10^{-6}}{2.58 \times 10^{-4} \times 1.29} = 3.92 \times 10^{-5} \text{ m}^3$
 $= 3.92 \times 10^{-5} \times 10^6 \text{ cm}^3$
 $= 39.2 \text{ (cc)}$

HDR shielding question. How much thickness for 10 patients per week, 5 days a week, 500cGy/patient. The drawing showed a distance of 2 meters (I think that's what it meant).

$W = 500 \text{ cGy} \times 10 \times 5 = 25000 \text{ cGy/wk}$ \leftarrow wrong!!!
 $t = \frac{P_{\text{dot}}}{WUT}$
 $t = \frac{10 \times 5 \times 569}{154 \text{ hr/wk}} = 250 \text{ min}$
 $W = \frac{P_{\text{dot}}}{WUT}$
 $W = \frac{10 \times 5 \times 569}{154 \text{ hr/wk}} = 250 \text{ min}$
 $W = 1. \text{ for HDR}$
 $T = ?$ According to area
 $P = \left\{ \begin{array}{l} 1 \text{ ms/hr} \text{ for occupancy} < 2 \text{ ml/hr} \\ 0.1 \text{ ms/hr} \text{ for } 0.02 \text{ ms/wk} \text{ more conservative} \end{array} \right.$

Calculate the steradian of a 50 cm diameter area on a standard linear accelerator.

a. .137
b. .122
c. .187

$\Omega = 2\pi (1 - \cos \theta)$
 $\Omega = 2\pi (1 - \frac{1}{\sqrt{1 + 0.5^2}})$
 $\Omega = 0.1876 \text{ ster}$

gap 2 = $\frac{16}{60} \times 10 \times 2 = 3.2 \text{ cm}$

Two isotopes Pd (lambda = .016) (rho =) and I125 (lambda =) half life is 17 days for Pd and 60 days for I125. After 120 days what is the ratio of doses? $T_{1/2} = \frac{\ln 2}{\lambda}$

Monte carlo calculations stop calculating at what energy and bundles everything into one

10 kev \rightarrow no contribution to dose
 100 kev \rightarrow
 200 kev \rightarrow
 500 kev \rightarrow
 1 Mev

How often according to TG40 should the wedge latch be checked? Monthly

What are Monte Carlo space files???

A. It registers where electrons are in space for calculation?????

A picture of a DVH

Shows critical organs, PTV and GTV curves. Choose which curve represents the GTV

13.05 cG exposure, $W/e = 33.3/70$ 2.58 x 10 R/C What is the volume of gas in the chamber?
 $X = \frac{Q}{M} \Rightarrow X = \frac{Q}{W}$
 $IR = 2.58 \times 10^{-4} \text{ C/kg} = \frac{13.05 \times 10^{-6}}{1.29 \text{ kg/m}^3 \text{ V(m}^3\text{)}}$
 $\Rightarrow V = \frac{13.05 \times 10^{-6}}{2.58 \times 10^{-4} \times 1.29} = 3.92 \times 10^{-5} \text{ m}^3$
 $= 3.92 \times 10^{-5} \times 10^6 \text{ cm}^3$
 $= 39.2 \text{ (cc)}$

HDR shielding question. How much thickness for 10 patients per week, 5 days a week, 500cGy/patient. The drawing showed a distance of 2 meters (I think that's what it meant).

$W = 500 \text{ cGy} \times 10 \times 5 = 25000 \text{ cGy/wk}$ \leftarrow wrong!!!
 $t = \frac{P_{\text{dot}}}{WUT}$
 $t = \frac{10 \times 5 \times 569}{154 \text{ hr/wk}} = 250 \text{ min}$
 $W = \frac{P_{\text{dot}}}{WUT}$
 $W = \frac{10 \times 5 \times 569}{154 \text{ hr/wk}} = 250 \text{ min}$
 $W = 1. \text{ for HDR}$
 $T = ?$ According to area
 $P = \left\{ \begin{array}{l} 1 \text{ ms/hr} \text{ for occupancy} < 2 \text{ ml/hr} \\ 0.1 \text{ ms/hr} \text{ for } 0.02 \text{ ms/wk} \text{ more conservative} \end{array} \right.$


Calculate the steradian of a 50 cm diameter area on a standard linear accelerator.

a. .137
b. .122
c. .187


$\Omega = 2\pi (1 - \cos \theta)$
 $\Omega = 2\pi (1 - \frac{1}{\sqrt{1 + 0.5^2}})$
 $\Omega = 0.1876 \text{ ster}$

cooling system
 gantry: { accelerator guide, bending magnet, accelerate solenoid, primary coll, energy slit, target }

stand: { klystron, klystron solenoid, circulator, of driver, of load, pulse transformer }

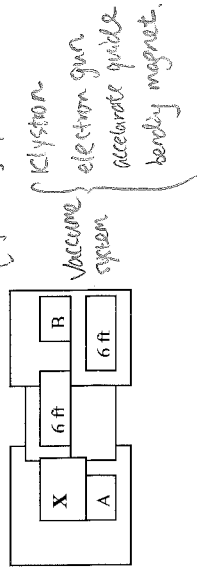

- For an instantaneous exposure it gives 30 mR. If a secretary is sitting at point B and the wall is shielded for 6X how many patients a week can be treated for a weekly dose of 0.02mSv? \Rightarrow more details in next page.
- Shielding question that gives a thickness of concrete and the room is shielded for 6X. How much more shielding is required for 18X? $\left[\left(\frac{4 \times 10^4 \text{ cGy}}{\text{TLD dose}} \right) \cdot \text{TLD dose} - \text{th} \right] = \left[\frac{\text{th}}{2 \text{ cm}} \times 4 \text{ cm} - \text{th} \right]$
- Why do the doctors leave a strip around each side of the treated area on a sarcoma for lymphatic drainage?



dose which if distributed uniformly across the entire target, for in risk, carries the same biological effects as actual inhomogeneous dose distribution

$$(N)TLP = \frac{1 + \left[\frac{E_{D50}}{E_{D0}} \right]^{1.650}}{1.650}$$

- What is the dose to point B?

- Range of S-90 in air 0.5m \Rightarrow 3.6m x 0.5 = 180cm
- Universal Wedge, WF = 0.2, what % MU needed for 30 degree effective wedge
- What does a fMRI measure \rightarrow physics \rightarrow tissue magnetic relaxation
- What is primary purpose of a bending magnet?
- IR delivered, 3x10-10 C measured... what's the size of the chamber? \Rightarrow see previous page.
- 30 cm2 field directed at roof, what is solid angle subtended at a point on the ground?
- HDR Cylinder with 5 sources 1 cm apart. Point A is midline, 4 cm from sources and receives 200 cGy. Point B is 2 cm lateral to Point A. What is Point B dose?
- Increasing the current to the magnetron does what?

Assume same density time

$$D_A = D_0 \left(\frac{1}{\sqrt{2442}} + \frac{1}{\sqrt{1442}} + \frac{1}{\sqrt{42}} + \frac{1}{\sqrt{1442}} + \frac{1}{\sqrt{2442}} \right)$$

$$D_B = D_0 \left(\frac{1}{\sqrt{2442}} + \frac{1}{\sqrt{1442}} + \frac{1}{\sqrt{42}} + \frac{1}{\sqrt{1442}} + \frac{1}{\sqrt{2442}} \right)$$

magnetron power output \rightarrow change in electron beam energy shift \Rightarrow peak power out \Rightarrow efficiency

Solid angle (Ω) = $2\pi(1 - \cos\theta)$ units (steradians)

Page 90
 Cartwright book

primary barrier will be more than adequate to shield against scatter radiation leakage even with TMRT

TMRT only increase leakage radiation

$$S = \left(\frac{P}{P_0} \right) \cdot P$$

$$d(cm) = \frac{E}{S}$$

90 Gy to TMRT

$$B_L(\text{no TMRT}) = \frac{P \cdot d^2 \cdot 0.001}{W \cdot T}$$

$$B_L(\text{TMRT}) = \frac{P \cdot d^2 \cdot 0.001}{W \cdot T}$$

$$\frac{B_L(\text{TMRT})}{B_L(\text{no TMRT})} = \frac{W}{W'} \Rightarrow \log \left(\frac{B_L(\text{TMRT})}{B_L(\text{no TMRT})} \right) = -\log \frac{W}{W'} + \log B_L(\text{no TMRT})$$

$$\Rightarrow \log \frac{W}{W'} = -\log \frac{B_L(\text{TMRT})}{B_L(\text{no TMRT})} + \log B_L(\text{no TMRT})$$

- Retrofit a linac to perform IMRT... how much shielding do you need to add? what is TVL?
- What is the source of electrons in an electron treatment?
- Given density of lead and mass atten coef for a random energy... how far is the vendor off?
- You check the source strength from the vendor 2 weeks after receipt. Given calibration factor, and reading... how far is the vendor off?
- Given DVH curve... which curve has the least homogeneous dose?
- Given DVH curve... points to a line, what is it? Answers were PTV, GTV, OAR, Volume receiving 100 of dose

- SRS treatment, 4mm cone... what is max dose? Answers were 10 Gy, 20 Gy, 40 Gy, etc
- All readings, voltages, kV, Nd, w, temp & pressure... how many cGy per MU?
- You calibrate a machine with the outside temp and pressure... But this is the inside temp and pressure... how far off is your output?
- Treating with parallel opposed wedge fields for 60 Gy in 30 fx and the MU per beam in 160 MU. After 10 fx... realize WF was not in calc. How many MUs required for remaining 20 fx to get to 60 Gy?

- Electron $E_0 = 7.1$ MeV, mean E at 2 cm = 4 MeV... what is range?
- According to TG51... you need to adjust you %DD by what?
- What happens to surface dose and %DD by adding a physical wedge? Surface dose \uparrow , %DD \downarrow
- Three layer material. First layer is 3 cm thick, HU = 0. Second layer is 4 cm thick, HU = 800. Third layer is 2 cm thick, HU = -100. What is effective depth?

- Why cant MRI be used for hetero corrections? \Rightarrow No electron density
- You have a half beam 6 MV photon beam and a parallel 9 MeV electron cutout? What should you convince the doctor to not use a 25 cm x 3 cm electron cutout?
- What is definition of EUD? \Rightarrow equivalent uniform dose
- What part of curve is an ion chamber used for calibration operated in? saturation
- Why would a doctor use Pd103 instead of 1125 for prostate implant? same half-life, fast delivery
- Which part of linac is not water cooled?
- Given an axial cut with weird dimensions drawn all over it... had to determine LPO angle?

Easy geometry

- Probably 10 MU calcs that I thought were very hard,
- Probably 5 or 6 TG43 brachy physics calcs
- According to TG40... how often do you check wedge interlocks?
- Probably 5 or 6 shielding calcs
- You use a 3x3 electron cutout... what doesn't happen? Dmax decreases, output decreases, flatness decreases, range decreases NO
- Probably 3-4 questions where you had to know that Total Dose = 1.44 times Half Life time Initial Dose Rate

- giving a dose rate constant of 1125 (Ir192)? measured experimental 0.7, two numbers calculated by Monte Carlo method (0.64, 0.67), something like that, ask according to TG-43, which one to use in planning system, 0.64, 0.67, 0.7, 0.65 (the experiment one, one of the Monte Carlo one, or the average of the two Monte Carlo) \Rightarrow $0.64 + 0.67 + 0.7 + 0.65 = 2.66 \Rightarrow \frac{2.66}{4} = 0.665$
- The universal wedge question like the one we had in the old exams, given a universal wedge, wedge factor = 0.25, to make a 30 degree wedge, what's the MU ratio of the wedge field and open = 0.6715

$$(1.5) \cdot 305 / 3600 \text{ (hr)} \cdot 0.6 \text{ mS/hr} \cdot \left(\frac{6}{T_2}\right)^2 = 2 \text{ mS/wk}$$

$$n = 320$$

field. I didn't know we need to assume the universal wedge angle is 60 degree until today. I thought something is missing in this question when I was working on it from the old exams.


3. one of the shielding questions like the old one, an office will be add next to the storage room, distance to the point in storage room is 6meters, to the point in office is 12meters, the reading in the point at storage room is 0.6mSv/hour, how many patient can they treat per week to get less 2mSv/week in that point in the office, the barrier between storage room and office has no attenuation, beam shoot on the barriers only 30s per patient, clinic is running 5 days per week. somehow I just can't get a number close to one of the answers.

4. Some of the questions have the answers are very close, I remembered one of the TG-51 calculation questions, the answer is like, 0.62, 0.63, 0.64...something like that, I got the answer is like 0.624 first time.

1. TG-51 calc. Given raw data. Need to calculate Pion and Ppol. Need to know standard pressure in kPa. Find dose at isocenter if 100 MU were given. Also given rcav which I didn't use. $\rightarrow 101.3 \text{ kPa} = 760 \text{ mmHg}$
2. Shielding - lots.
3. HDR calculation using point source formalism from TG-43 (given dose rate constant, radial dose function, some other stuff)
4. Treating a stereotactic lesion in the head with a 4 mm diameter beam. What is the largest dose you can prescribe?

5. Standard Gap Calc between a treatment with an SSD setup and a treatment with an SAD setup. Answer was 1.95 cm gap on skin. Options included 1.9 cm and 2 cm. I chose 2.
6. Photon and electron field
7. Concrete is used for neutron shielding for what reason? (thermalizes neutrons was my answer) *high hydrogen increase thermal neutron capture*
8. Using lead and concrete to shield Primary wall. From the inside, what is the order of the materials? (lead then concrete, concrete then lead, other combinations)
9. Given 125I half life of 59.4 days, given exposure rate constant in cGy/hr/U or cGy/U/hr.

- After 30 days what is the dose rate to the tumor in mSv/hr?
10. 20 keV beam. The density of copper is given in g/cm^3 , and the μ/ρ for copper is given in cm^2/g . If 3 mm of copper attenuates the beam to 63% of its original intensity, what is the TVL for copper? $0.37 = e^{-\Delta z / \text{TVL}} \Rightarrow \Delta z = 0.35 \Rightarrow \text{TVL} = 6.1$
11. Shielding: the distance from isocenter to point S is 6m, and iso to point Z is 12m. Point S is in a store room and point Z is in a room being considered as new office space. A survey meter measures 0.27 cGy/hr at point S. A beam is aimed toward this primary wall for 30 seconds per treatment. For a maximum dose of 0.087 cGy/week at point Z, what is the maximum number of patients you can treat per day? Consider only photon interactions.



$$D = X(r) \cdot f(\omega/r) = \frac{Q(\omega) \cdot f}{n(\omega, v)}$$

$$7 \times 7.0 = 49.0 \text{ g/L}$$

0.259/102

$$O = (0.05 \text{ day/hr}) \cdot \frac{308}{26008}$$

$$= 4.67 \times 10^{-4} \text{ g/ltr.}$$

(08000000) 17 days

0.0006 m
= 0.016 g/day

$$Q_{\text{max}} = 96$$


$$0.001 = 0.015 \text{ m/s}^2$$

[illegible]

$$0.02 \text{ mEq/L} \times 15 = 0.3 \text{ mEq/L}$$

$P = 32$ day

12. Given 5 HDR sources, 1 cm between each source dwell position, 4 cm between middle source and point A. The dose at point A is given. What is the dose at point B. Equal dwell times for all sources. (Also given source active length which is less than τ distance, so I treated as pt sources)




$$f' = \frac{25}{20} \times 100 = 125$$

$$SSD' = f' - d = 125 - 12 = 113 \text{ cm}$$

13. A setup calls for a 25 cm field length at 100 SAD. The SSD is 88 cm. However, the field requires a wedge that has a field size limit of 20 cm at isocenter. What must the new SSD be in order to accommodate the wedge?

14. Find the RPO angle given the following (diagram). The line represents the central ray of the beam through the patient.

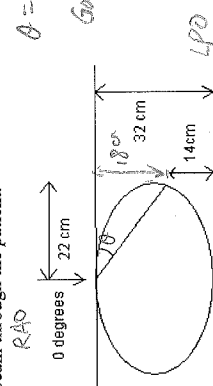



$$A_{\text{max}} = \tan^{-1}\left(\frac{18}{2}\right) = 39.2^\circ$$

$$\text{Gravity} = 90^\circ + 393^\circ = 1293^\circ$$

15. Parallel opposed fields with equal weighting. 60 Gy in 30 fractions is prescribed to the isocenter. The fields are equally weighted. (SAD setup with iso at midsep). The patient separation is given, as well as the depth to the cord. The TMRs at three different depths are given. Find the maximum number of fractions that can be given with the limitation being the cord tolerance dose. \Rightarrow Find Dose/par fr \Rightarrow $\frac{4400}{30}$ Dose = 146.6
16. Memory foggy on this one: You measure a brachy source and get a measurement in air at 1 meter of (given)/R/S. The chamber volume is given, the chamber calibration factor is given (in cGy/Cr). You are given the density of air in kg/m³. The stated activity from the manufacturer is given. Given 0.876cGy/R, given 33.95 I/C, NOT given 2.58E-4 C/Kg = 1R. What is the relationship between your measured dose rate and the dose rate rated by the

17. For a photon skyline calc, What is the solid angle of a circular beam with a 50 cm diameter? (0.187)
18. A beam travels through tissue (see diagram). What is the radiographic depth?

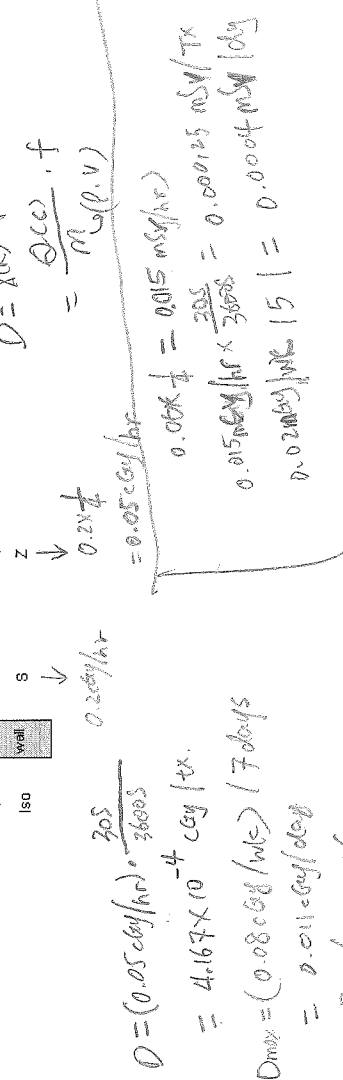

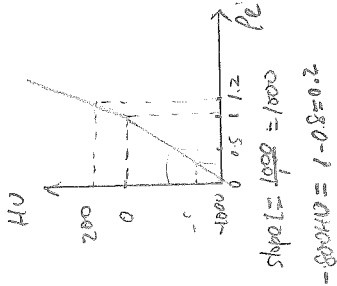

3 cm	HU = 0	$P_e = 1$
4 cm	HU = -800	$P_e = 0.2 \sim 0.25$
2 cm	HU = -200	$P_e = 1.15 \sim 1.2$

$$W' = 0.5W + (0.5W) \cdot C$$

$$= 0.5W + 0.5W \times 5$$

$$= 3W$$


$$TVL = \log \frac{W}{W'} = (0.48 TVL)$$

19. A Shielding calculation was performed assuming no IMRT. If you will now be doing 50% IMRT, how much additional shielding will you need to add?
20. A universal wedge with a wedge factor of 0.25 is used to deliver a beam with an effective wedge factor of 30 degrees. What is the fraction of MU's delivered by the wedged portion of the field. (There were 2 questions like this. For this question, I tried using both the Tatcher universal wedge equation and the equation from Greene and Williams (Linear Accelerators for Radiation Therapy). BOTH answers were in there. Maybe both will be counted as correct???)

21. Shown a setup with AP, Lt Lat, and Rt Lat fields. The Rt and Lt Laterals were wedged. The isodose distribution looks like the picture below. Another picture with a uniform isodose distribution is shown. You must choose which field weights and wedge weights to change in order to make the picture below look like a uniform isodose distribution. You are given a choice between answers like this:


RT LAT wt LT LAT wt AP wt RT lat wedge Lt lat wedge

decrease increase same increase increase

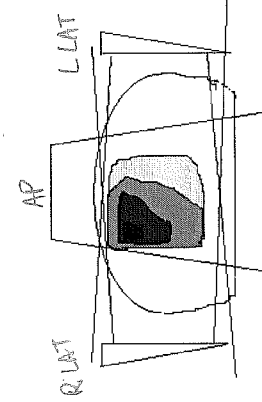


22. Electrons are produced in a linac by (thermionic emission from anode, thyratron anode, heating a filament, etc) emitted from cathode in electron gun.
23. When the current in the magnetron increases: The magnetron voltage increases, other answers I can't remember.
24. Overall error expected according to TG-40
25. definition of QA
26. definition of wedge factor
27. Meaning of Equivalent Uniform dose (given a non-uniform dose distribution, find the uniform dose that gives the same biological effect)

28. Shown DVH and must choose the DVH line representing most heterogeneous dose distribution




29. Which structure does line 2 represent on this DVH for an IMRT plan? (organ at risk, GTV, PTV, etc) It was an obvious PTV



When target is close to a joint, at least a part of the joint should be shielded. A strip of tissue should be spared along the entire extremity, delivering the entire dose to the entire system, high dose to the entire system.

30. Why, when treating an extremity, do we block out a sliver of skin? (spare lymphatic system, aid in skin healing after radiation, other choices)
31. When treating a lung tumor, what is the dose associated with radiation pneumonitis? (V20=30%, V50=10% etc) \rightarrow 1mSv/cy
32. Neutron dose from 15 MV photons: (2%, 5%, etc)
33. All of the following change when an electron beam is made significantly smaller by adding a cutout EXCEPT: (Rp, dmax dose, etc)
34. When an electron beam has an oblique incidence on the surface, what happens? (how does it change dmax, Range, etc) (Khan p.321, 3rd ed.)
35. According to Bragg-Gray cavity theory, the diameter of the air cavity should be (greater than the range of radiation in cavity, same as range of radiation in cavity, less than range of radiation in cavity— Khan p.114) \Rightarrow page 18 of review course
36. In which region would a cylindrical ion chamber be operated on a voltage versus ion pairs collected graph?



dmax \downarrow
Dose rate \uparrow
Rp \uparrow
 \downarrow penetration (Rp)
increase dose at
greater depth

37. In Monte Carlo Treatment Planning Algorithms, what is the cutoff energy under which the path a particle will no longer be mapped discretely, and instead it will be lumped in with a general energy distribution function. (100keV, 10 keV, 1keV, two other options)

38. How much do shift your curve to get a PDD (PDI?) curve? Options included 0.6cav upstream. It was the only one that made sense.

39. What is the purpose of the bending magnet. Options included: to accommodate a horizontal waveguide, and to focus the electron beam on the target.

40. There was a question that required you to know that the bending magnet was NOT between the target and primary collimator. It may have been included in the previous question.

41. On fluoro images in the simulator, wires used toward the outer edges of the field of view can appear to be (farther apart?) than they actually are. This is due to: image intensifier, \rightarrow magnification?

automatic brightness control, scatter grid, another choice I don't remember.

42. A dose calc where you have SSD, Dose rate at Dmax for 100 ssd setup, and a depth of 10 (PDD given). For the given setup, they give you the MU required to give the dose. for the same dose delivered to an SAD field at a depth of 10 (They stated the TMR), how many MU's do you need? Need to do a back calculation to get the output factors that are not mentioned, then do the SAD calc and include the output factors.

43. Prescription is 200 cGy/day delivered by parallel opposed, equally weighted beams. They say they gave 147 MU per beam, but left out a wedge factor of 0.8 for the first 10 treatments. The patient is to receive 30 treatments total. What is the MU required (per beam) for the remaining 20 treatments in order to deliver the prescribed dose for the entire course of treatment? $real\ MU = 147 / 0.8 = 184\ MU_s$

$$MU = \frac{D_{o+} \cdot N_c (1-WF)}{N_2} = \frac{D_{o+} \cdot WF \cdot 2}{N_2} = \frac{200 + \frac{200 \times 0.8}{20}}{\frac{100}{147} \times 0.8 \times 2} = 202$$

20 cGy to each per fx: $MU^* = \frac{20}{0.8 \times 0.8} = 31\ MU_s / 2 = 19\ MU_s \Rightarrow 203\ MU$
No questions on TBI this time. No questions about occupational or public dose limits. Lots of dose calcs. No electron calcs that I can remember. A sizable amount of rather obscure information was included in the simple questions. Most of the complex questions were more reasonable but I ran out of time and had to guess on the last few. Don't waste time on the simple questions you don't know!!

\Rightarrow Verify:


$$dose\ in\ first\ 10\ fx: 200 \times 0.8 \times 10 = 1600$$

$$20\ fx: (202 \times \frac{100}{147} \times 0.8) \times 2 \times 20 = 4397$$

2009 Part II Recall:

- For regular photon Linac, the major contribution of photon dose at maze door:
 - Leakage through maze wall
 - Leakage scattered through wall
 - Patient scattered
- For ion-chamber used for calibration, what is the limit for chamber leakage:
 - 10^{-12}
 - 10^{-14}
 - 10^{-10}
 - 10^{-8}
- Based on TG-66, the tolerance for the alignment of gantry laser with the image isocenter is: $\pm 1\text{mm}$; $\pm 2\text{mm}$ and so on
- A question about electron TG-51 calibration. Calculate cross-calibration p.p.l chamber: $K_{\text{ecl}} \cdot N_{\text{D,W}}$. Given reading M, correction factors, R50, KR50' formula for ppl and dose calibration factor for cylindrical chamber.

$$1.5 = \frac{1.0 - 0.45}{\log(D_1) - \log(D_0)} = \frac{0.55}{\log\left(\frac{D_1}{D_0}\right)}$$


$$\log\left(\frac{D_1}{D_0}\right) = \frac{0.55}{1.5} = 0.36667$$
- Physics wedge will:
 - increase skin dose, increase PDD
 - reduce skin dose, increase PDD
 - increase skin dose, decrease PDD
 - D.
- IMRT film QA, two areas with optical density 1.0 and 0.45; film gradient is 1.5, what is the ratio of doses on these two areas?
 - 2:1
 - 3:1
 - 3.5:1
- What material has the highest neutron production rate: Tin, Lucite, Lead and others
- Gap calculation: Field A: SAD treatment, SSD=90, d=10 and field size (FS) at SSD=24cm, Field B SSD=100, FS=15 at SSD, what is skin gap to match dose at depth=10cm? Answers: A 1.9cm B 2.1cm C 2cm
 
- Conformity index = 2.7 and GTV volume = 5.4cm^3 , what is the volume of tissue irradiated.

$$\frac{12}{90} = \frac{1}{10}$$

$$\frac{7.5}{100} = \frac{1}{10}$$

$$V_1 = \frac{12 \times 10}{90} + \frac{7.5 \times 10}{100}$$

$$= 2.08$$
- For megavoltage CT, what is the calibration curve HU to electron density.

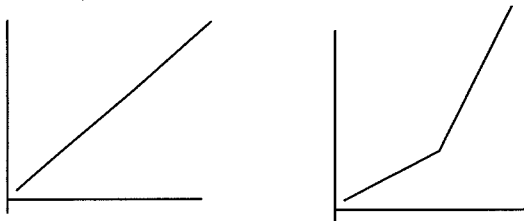

- Spiral CT, collimator: 4 slices with 1mm thickness, gantry rotation time = 1.5s, what is total time to scan 100mm?

pitch = $\frac{\text{Table travel speed per rotation}}{\text{collimator size}}$

$\frac{12\text{mm}}{4\text{mm}} = 3$

$\frac{100\text{mm}}{3} = 33.33\text{mm}$


$\frac{33.33\text{mm}}{1.5\text{s}} = 22.22\text{mm/s}$

$\frac{100\text{mm}}{22.22\text{mm/s}} = 4.5\text{s}$

$$e^{-\mu \cdot 2.8} = 0.5$$

$$\mu = 0.2475$$

12. HVL = 2.8cm for some material, $\mu^{\text{water}} = 0.19 \text{ cm}^{-1}$. What is the CT number for the material: A: 1000HU B: 2000HU C: 100HU D 0
13. Give a CT slice, showing 3cm chest wall, 11cm lung, 1cm tissue to point A, dose to point A is 200cGy and calculated without inhomogeneity correction. What is the real dose to point A? answers include 246cGy, 255cGy
14. What is difference between PDD (%10) and (%dd)x in TG-51:
 A. e- contamination is significant at d=10cm
 B. (%dd) is used to find KQ where (%dd) is used to convert/calculate dose at dmax.
15. where is effective point of measure of p.p.l chamber?
 A. proximal side of cavity
 B. distal side of cavity
16. Wedge calculation: total 60Gy in 30 fx. In first 10fx, 147MU given and then realize missing wedge factor 0.8. To compensate the dose in next 20fx, what is new MU: A. 202MU'
17. Gamma knife: localization error: 1.5mm and some other error 0.5mm, for quadratic total error? (square root of two errors)
18. HDR calibration: Give Sk on some date from vendor, then current measured after two weeks and chamber calibration factor is also given. What is difference between measured and vendor value? (Need to know dose = current * calibration factor * inversed decay correction)
19. Two shielding questions: For 6MV and 18MV, both TVL_1 and TVLe given. Concrete thickness 95cm. To find extra thickness if the room shield is needed if energy change from 6x to 16x. (need to know thickness = $\text{TVL}_1 + (n-1) \cdot \text{TVLe}$).
 The other question is very similar, but given TVL for both 6MV and 16MV, some thickness of thickness of shielding, find difference exposure readings behind the wall. (I can not recall this clearly. But the question is basically to ask you calculate transmission between different energies)
20. For primary wall shielding, Point A is 6m away from isocenter, point B is 12m away from isocenter. The beam is only 30s on the wall for each patient. Dose measured at point A is 0.06mSv/hr. Work load at iso was given. How many patients can be treated that dose at point B will not be greater than 0.02mSv/hr (The same question as No.11 of 2008 exam)
 (Ans: A. 26; B. 30)
21. For electron beam, f slope for gap = 0.0111 was given, SSD=100cm, dm = 2cm, what is effective SSD?



22. TG-51, given all parameters, T, P, readings at 150V, 300V, Ppol, Pecl, KQ, Nd,w, and SSD=100cm, PDD(10)=0.753, find dose at dm.

23. A few simple calculation of TG-43, give Sk, dose rate constant, G(r, θ) following IVS, g(r) and F(r, θ) given. Basically you need to convert units (cGy ↔ Gy, hr ↔ min), then you can calculate dose rate and find total dose and so on.

24. What happen if megatron current is increased?
A. RF power reduce B. Beam energy increase

25. If bending magnet is not working, what observation you will have:
A. Dose rate reduce B. field symmetry change C. beam energy change

26. What is the limiting dose that when 30% of kidney get irradiation and will have irrisisipible damage.
C. 2000cGy D. 3500cGy .. I don't remember if there is 5000cGy in answer

27. When using regular fractionation (1.8Gy/fx, some number of fx) , what is the TD5/5 of xxxx (a word that I don't recognize, probably some side effect) for parotid. (answers include: 10Gy, 30Gy, 50Gy)

28. BED calculation: 54Gy /30fx. Alfa/belta =10Gy, calculate dose per fx if want to deliver in 20fx.
 $BED = nd(1 + \frac{d}{\alpha/\beta}) = 54 \times (1 + \frac{1.8}{10}) = 20 \cdot d(1 + \frac{d}{10})$

29. Brachy source shield by 2cm lead (HVL = 5.5mm), container diameter 30cm, T=3.26Rm2/hr/mCi (I don't remember the number and unit). What is the max activity can be in the container to make the exposure less than 50mR/hr at the surface.
 $3.26 \times A \times e^{-\frac{2.0}{5.5} \times 200} \times (\frac{1}{15})^2 = 50mR \Rightarrow 0.05R \Rightarrow 43.02$
 $d = \frac{-20 \pm \sqrt{20^2 + 2 \times 4 \times 63.72}}{4}$
 $d = 2.54$

30. In cone beam CT, if some detectors only works intermittent (I don't recognize that word) , what artifact the image will have: A. band B. ring C. streaking D.

31. calculate leakage workload: # of patient 20 per day, 5 days per week, dose per patent = xxx Gy. 65% are conventional tx, 35% are IMRT, and C_{IMRT} =4, average treatment PDD = 65%, what is the workload?
 $(\frac{200}{0.65} \times 0.65 + \frac{200 \times 4 \times 0.35}{0.65}) \times 100 = 480 \text{ Gy}$
 $(200 + \frac{200}{0.65} \times 4 \times 0.35) \times 100 = 631 \text{ Gy}$

32. film cut question, SAD =100cm, separation =22cm, film at 135cm. then want to move to SSD=100cm, what is film distance? Answers: 144cm (I did not get the exact answer, but close to one of this number 146cm?)

33. e- treatment for a superficial lesion with diameter of 4.5cm, 200cGy to 80% ID₅₀, what is MU? Give cone factor of 6x6 (0.98), 10x10 (1.0) and 15x15 (1.02). So you need to decide which cone to use.

34. What kind of heterogeneity correction is used in collapsed cone calculation?

$$\frac{x}{100+11} = \frac{y}{?}$$

$$? = \frac{(100+11)y}{100}$$

$$\frac{x}{100} = \frac{y}{135}$$

$$\frac{x'}{y} = \frac{11}{100+11}$$

35. IMRT QA point verification should be at: A. low dose high gradient B. High dose low gradient and so on.

36. How many ____% of brachy seeds need to be surveyed and at what percentage different ____ that you need to report to vendor?

37.

35. IMRT QA point verification should be at: A. low dose high gradient B. High dose low gradient and so on.
36. How many ____% of brachy seeds need to be surveyed and at what percentage different ____ that you need to report to vendor?
37. Which is the most sensitive device to detect ^{125}I :
A: G-M counter B. Thin-window G-M counter
38. A 9-inch polyethylene sphere surrounding BF3 with cadmium rod is best to measure:
A. thermal neutron B. fast neutron