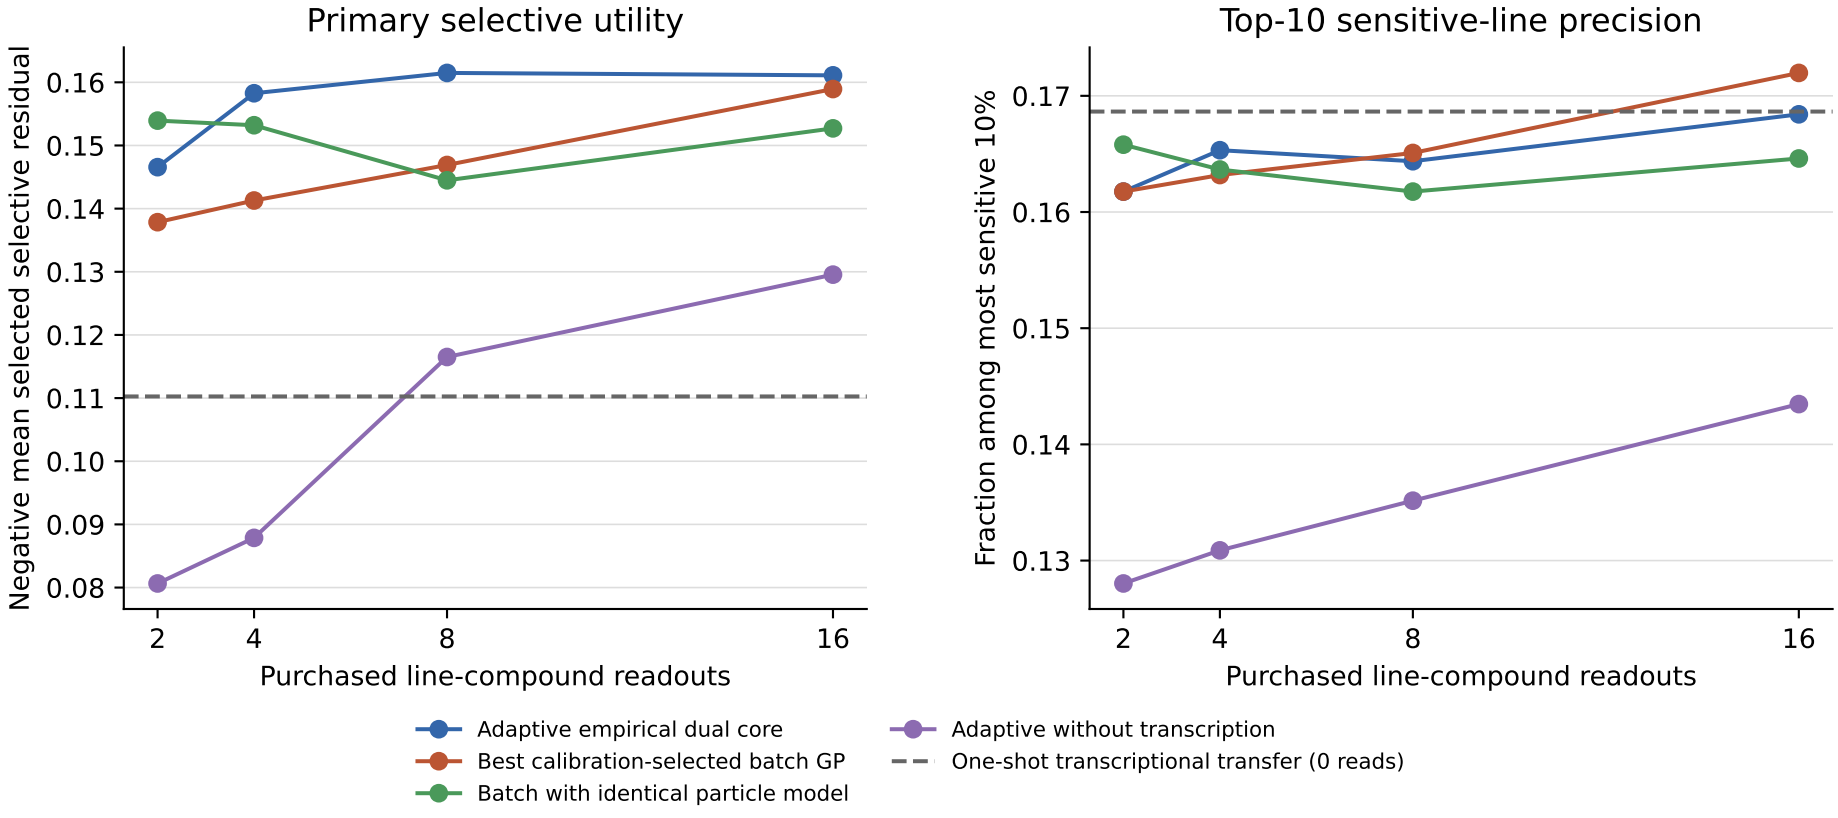
Primary selective utility
Negative mean selected selective residual
0.16
0.15
0.14
0.13
0.12
0.11
0.10
0.09
0.08
2
4
8
16
Purchased line-compound readouts
Top-10 sensitive-line precision
Fraction among most sensitive 10%
0.17
0.16
0.15
0.14
0.13
2
4
8
16
Purchased line-compound readouts
Adaptive empirical dual core
Best calibration-selected batch GP
Batch with identical particle model
Adaptive without transcription
One-shot transcriptional transfer (0 reads)