Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(PL 12.30)\QuantResults\1,4.batch.bin				
Analysis Time	2026-01-08 오전 11:42:59	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:42:59	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

1,4-Dioxane

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
1,4 ST-01.D	Cal	2.359	1216	2375	0.011
1,4 ST-02.D	Cal	2.364	2407	2376	0.020
1,4 ST-03.D	Cal	2.364	6246	2414	0.050
1,4 ST-04.D	Cal	2.353	9976	2432	0.079
1,4 ST-05.D	Cal	2.348	11755	2237	0.101
1,4 ST-06.D	Cal	2.359	19209	2353	0.156
1,4 ST-07.D	Cal	2.353	24535	2316	0.203
BK-.D	Blank			2392	ND
FBK(PL 25-12-30).D	Blank			2332	ND
PL-01.D	Sample			1843	ND
PL-02.D	Sample			1901	ND
MBK.D	Blank			2423	ND
-C-C-V-1.D	QC	2.348	12152	2340	0.100

1,4-Dioxane

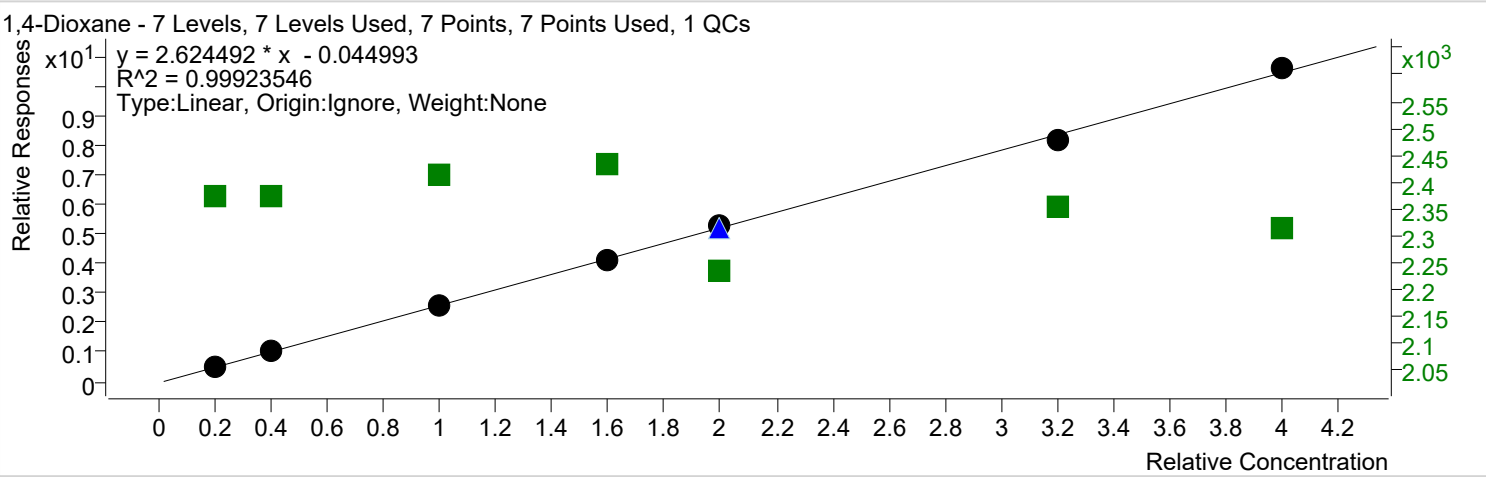

Cal. Path	Type	Level	Enable	Conc.	Response
W:\2026\1. 2026-01\1,4(PL 12.30)\1,4 ST-01.D	Calibration	1	x	0.200	1216
W:\2026\1. 2026-01\1,4(PL 12.30)\1,4 ST-02.D	Calibration	2	x	0.400	2407
W:\2026\1. 2026-01\1,4(PL 12.30)\1,4 ST-03.D	Calibration	3	x	1.000	6246
W:\2026\1. 2026-01\1,4(PL 12.30)\1,4 ST-04.D	Calibration	4	x	1.600	9976
W:\2026\1. 2026-01\1,4(PL 12.30)\1,4 ST-05.D	Calibration	5	x	2.000	11755
W:\2026\1. 2026-01\1,4(PL 12.30)\-C-C-V-1.D	QC	5	x	2.000	12152
W:\2026\1. 2026-01\1,4(PL 12.30)\1,4 ST-06.D	Calibration	6	x	3.200	19209
W:\2026\1. 2026-01\1,4(PL 12.30)\1,4 ST-07.D	Calibration	7	x	4.000	24535

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(PL 12.30)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-08 오전 11:42:59	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:45:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:42:59	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오후 12:08:51	**Data File**	1,4 ST-01.D
Type	Cal	**Name**	1,4 ST-01
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

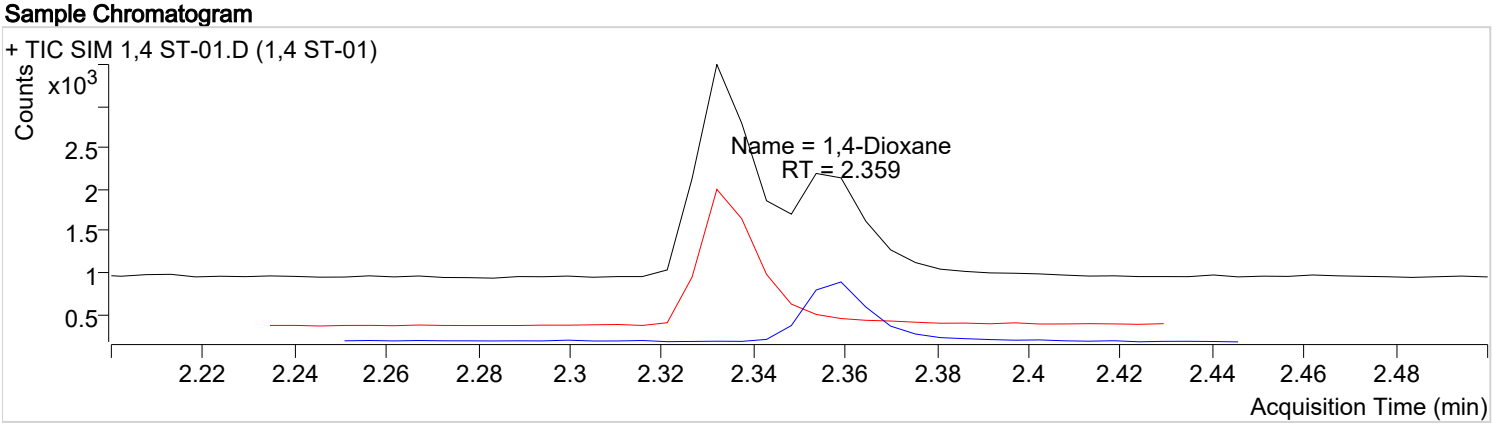

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.359	1216	2375	0.011 mg/L

1,4-Dioxane

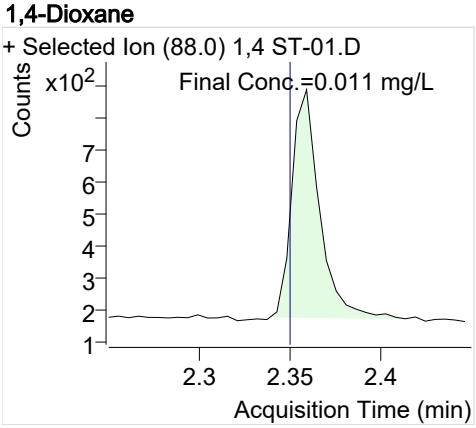

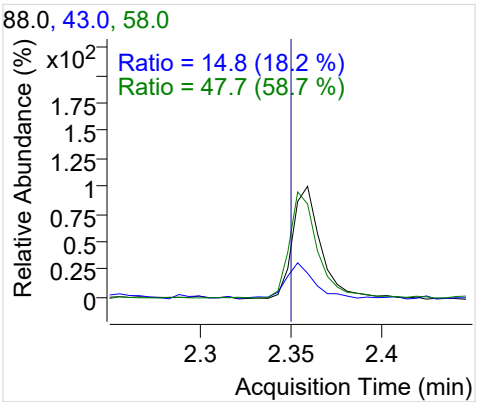



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(PL 12.30)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-08 오전 11:42:59	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:45:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:42:59	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오후 12:17:49	**Data File**	1,4 ST-02.D
Type	Cal	**Name**	1,4 ST-02
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

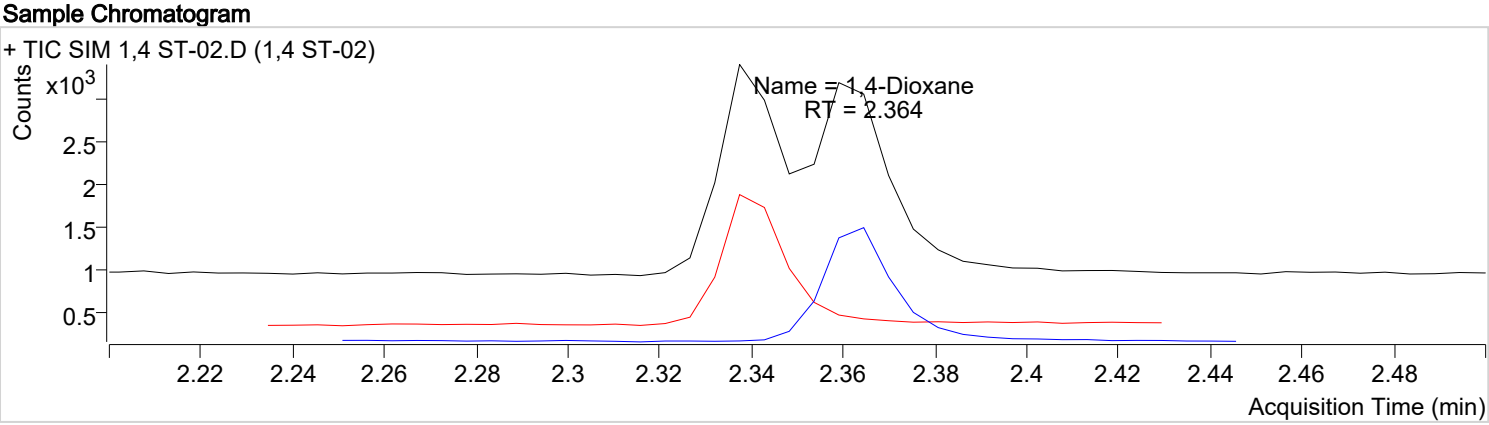

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.364	2407	2376	0.020 mg/L

1,4-Dioxane

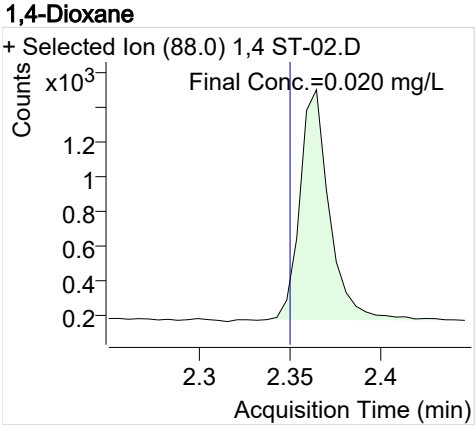

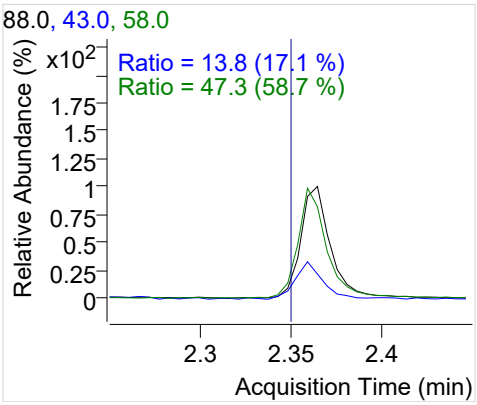



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(PL 12.30)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-08 오전 11:42:59	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:45:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:42:59	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오후 12:26:46	**Data File**	1,4 ST-03.D
Type	Cal	**Name**	1,4 ST-03
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

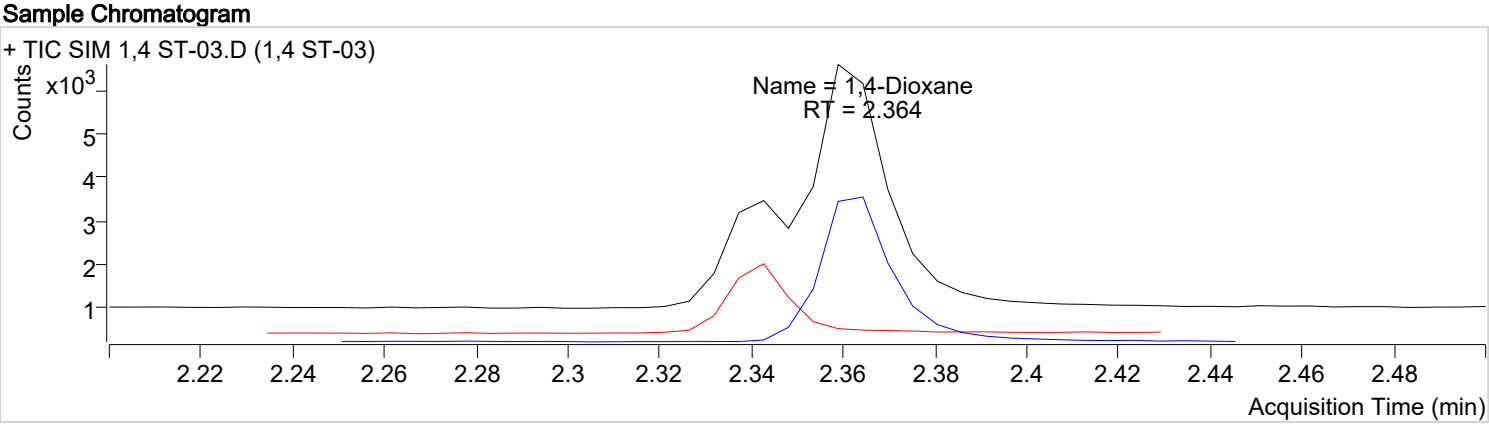

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.364	6246	2414	0.050 mg/L

1,4-Dioxane

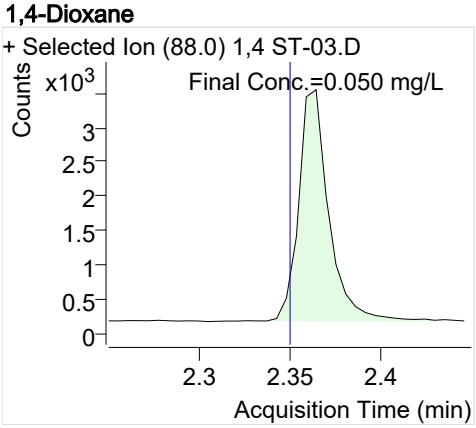

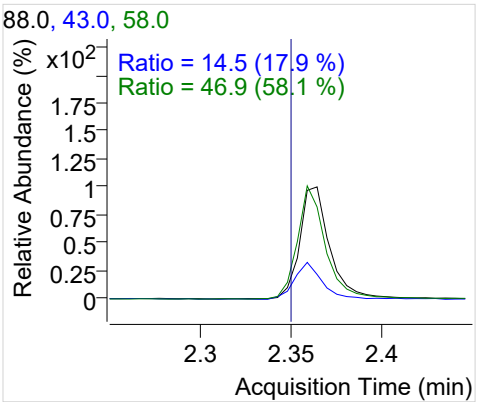



Quant Sample Report

Batch Data Path	W:\2026\1. 2026-01\1,4(PL 12.30)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-08 오전 11:42:59	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:45:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:42:59	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오후 12:35:48	**Data File**	1,4 ST-04.D
Type	Cal	**Name**	1,4 ST-04
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

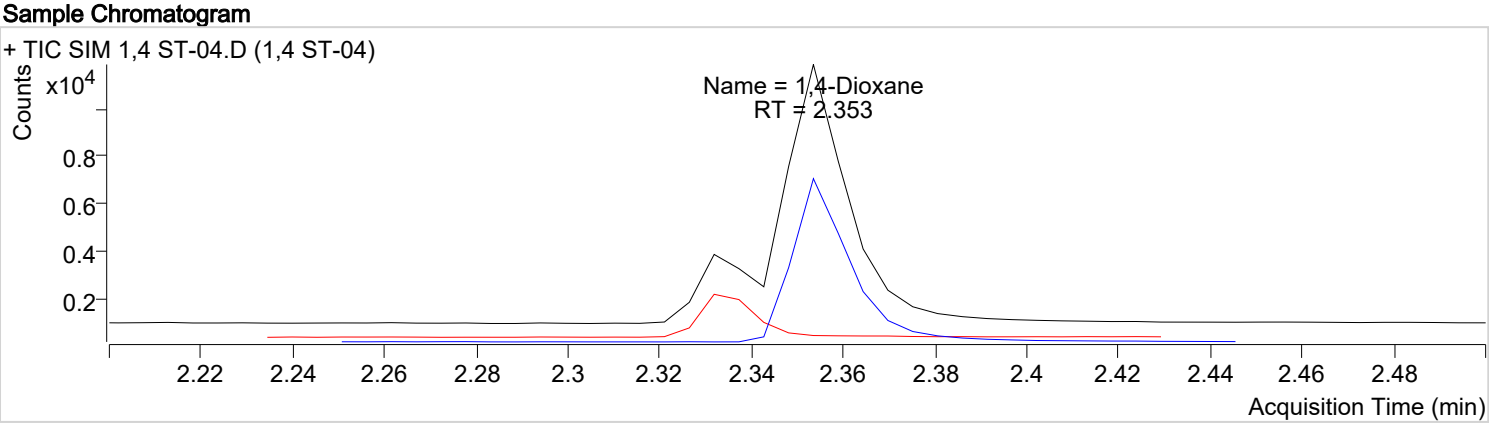

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.353	9976	2432	0.079 mg/L

1,4-Dioxane

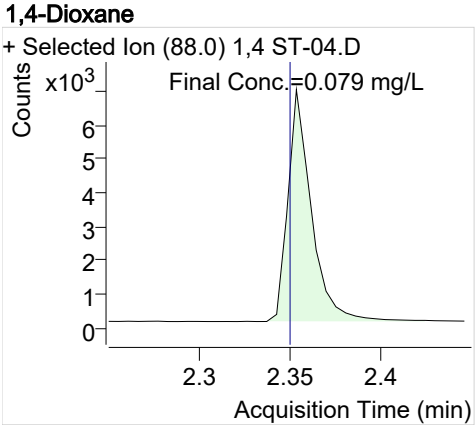

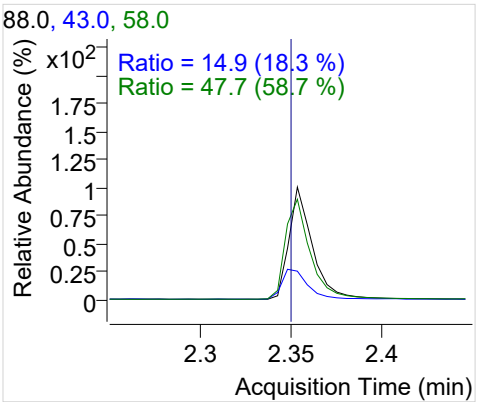



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(PL 12.30)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-08 오전 11:42:59	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:45:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:42:59	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오후 12:44:46	**Data File**	1,4 ST-05.D
Type	Cal	**Name**	1,4 ST-05
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

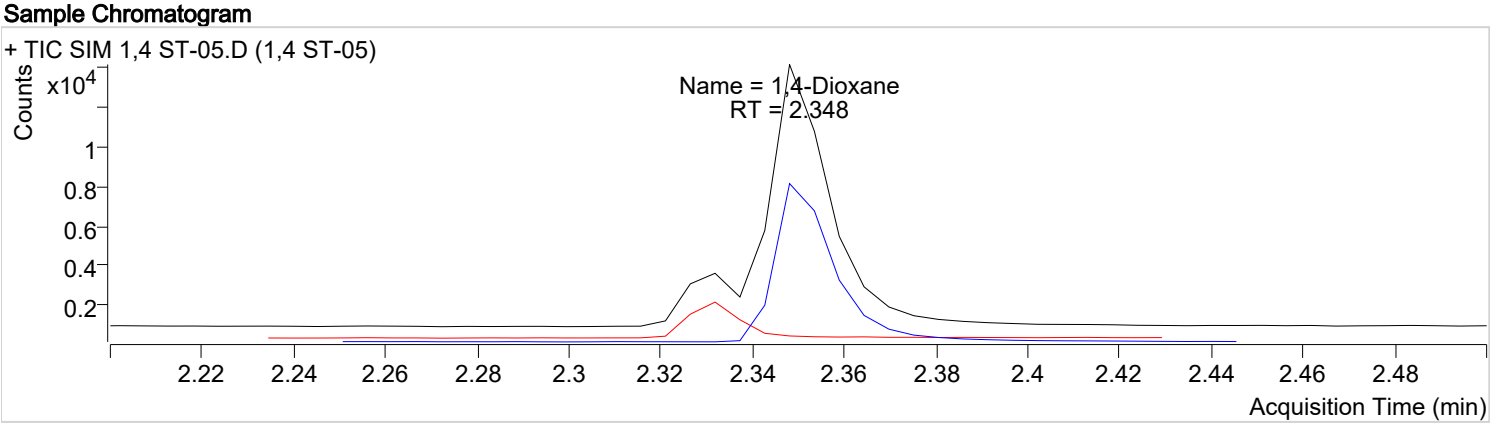

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.348	11755	2237	0.101 mg/L

1,4-Dioxane

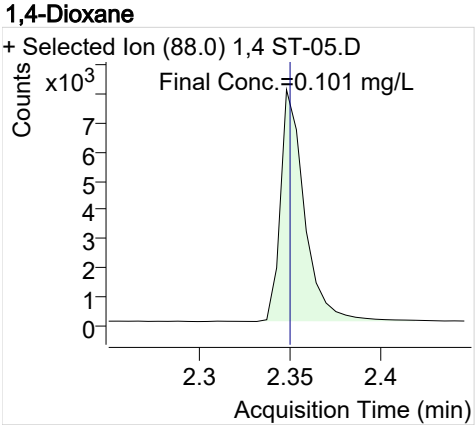



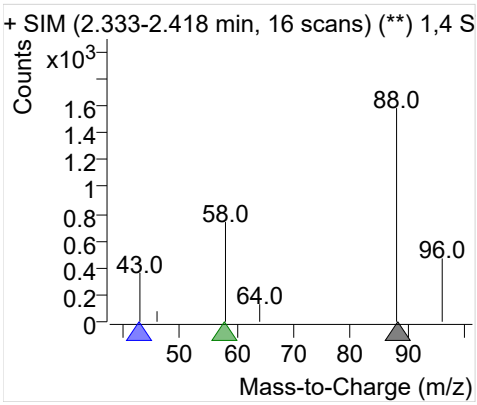

Quant Sample Report

Batch Data Path	W:\2026\1. 2026-01\1,4(PL 12.30)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-08 오전 11:42:59	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:45:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:42:59	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오후 12:53:52	**Data File**	1,4 ST-06.D
Type	Cal	**Name**	1,4 ST-06
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

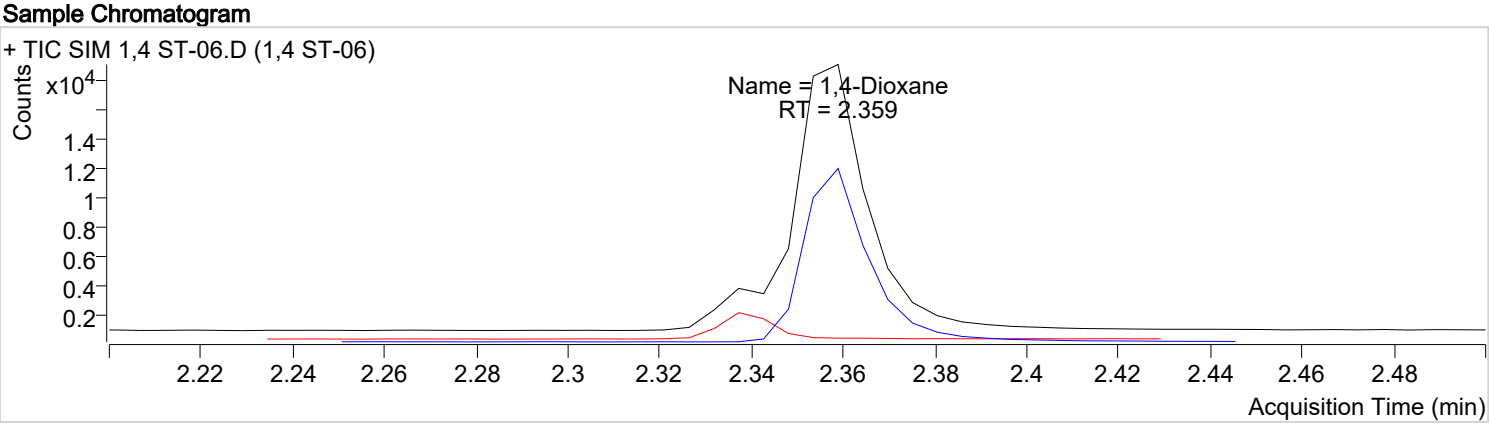

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.359	19209	2353	0.156 mg/L

1,4-Dioxane

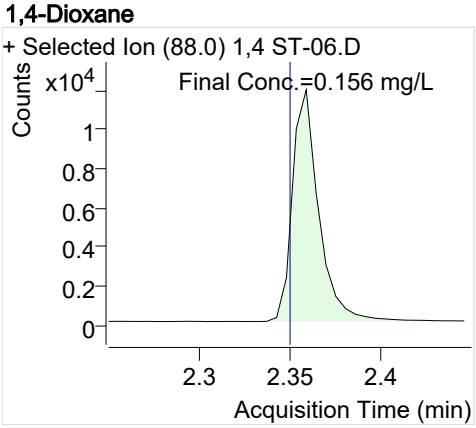

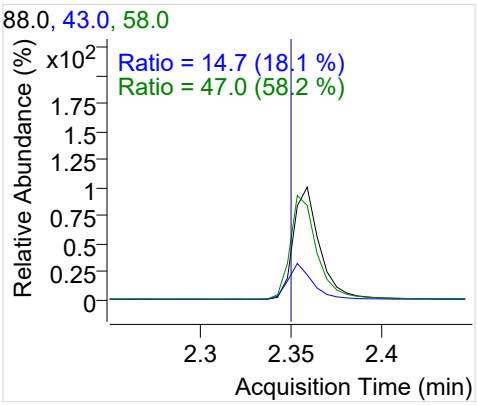



Quant Sample Report

Batch Data Path	W:\2026\1. 2026-01\1,4(PL 12.30)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-08 오전 11:42:59	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:45:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:42:59	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오후 1:02:54	**Data File**	1,4 ST-07.D
Type	Cal	**Name**	1,4 ST-07
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

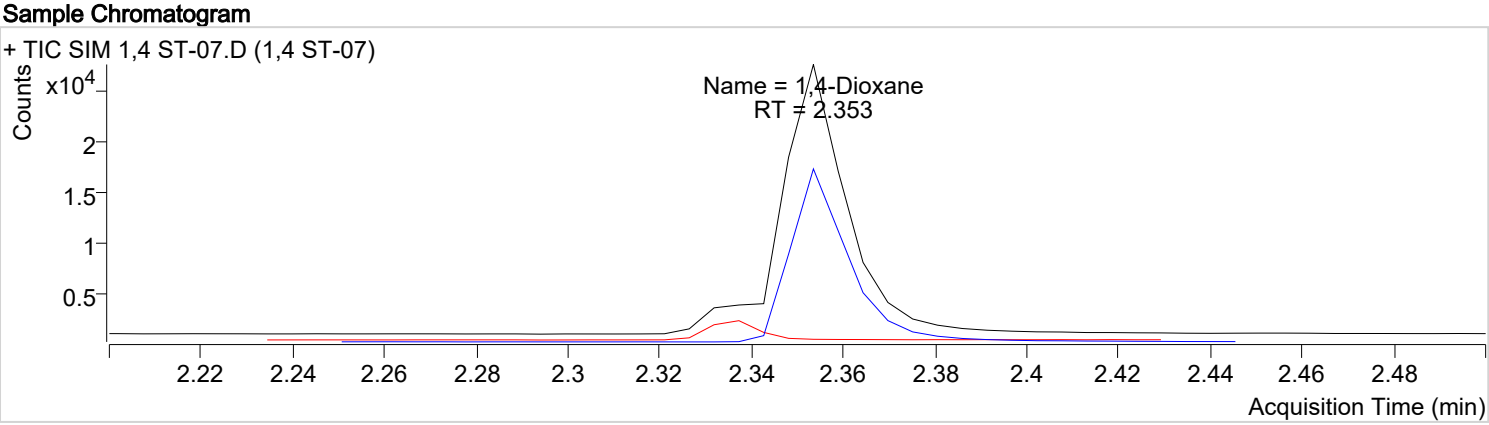

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.353	24535	2316	0.203 mg/L

1,4-Dioxane

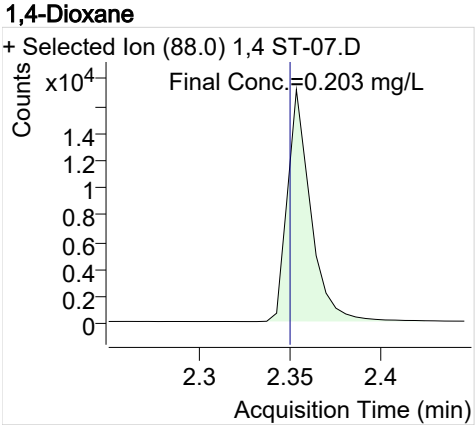

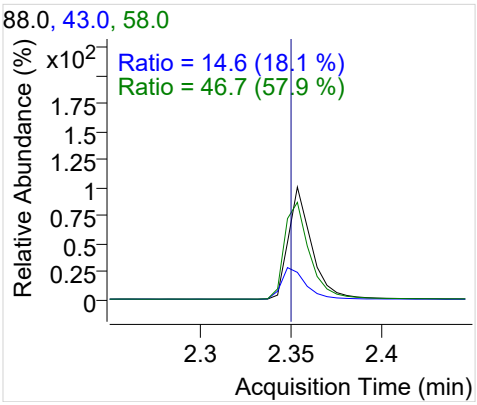



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(PL 12.30)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-08 오전 11:42:59	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:45:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:42:59	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오후 1:21:00	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

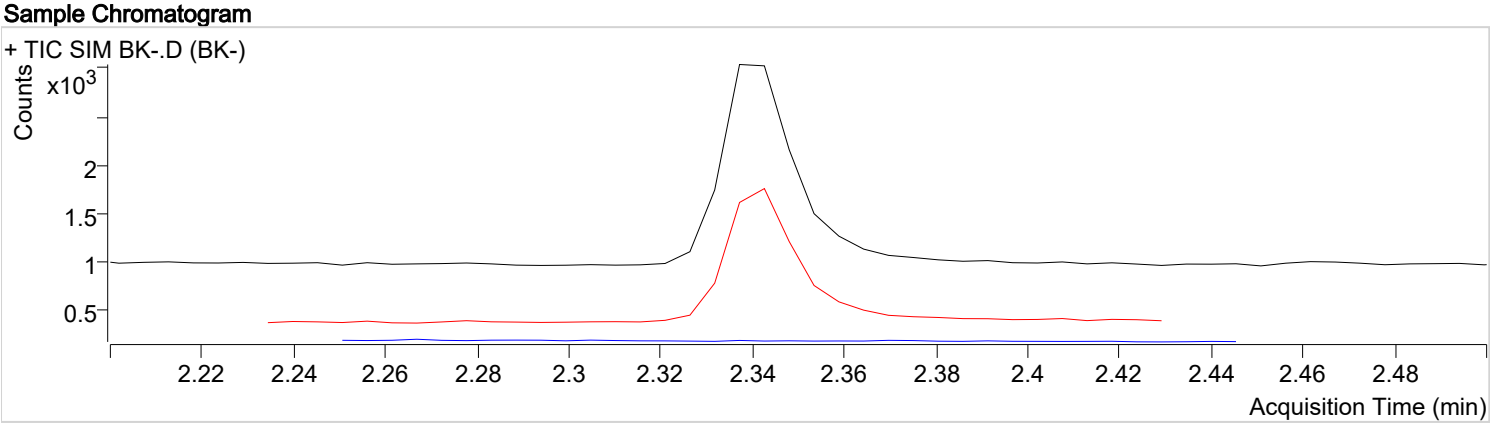

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			2392	ND mg/L

1,4-Dioxane

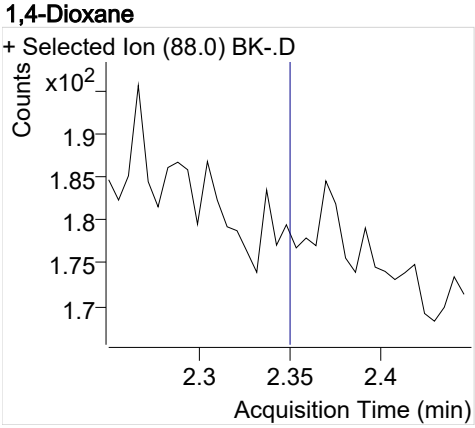



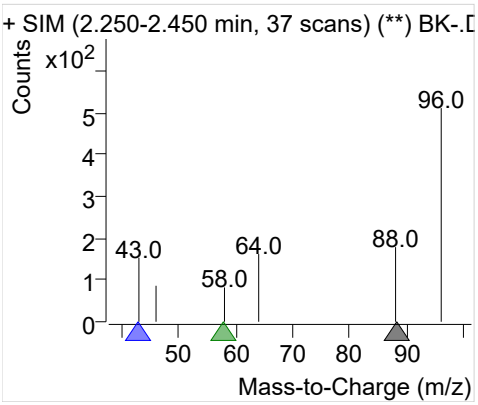

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(PL 12.30)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-08 오전 11:42:59	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:45:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:42:59	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오후 1:30:03	**Data File**	FBK(PL 25-12-30).D
Type	Blank	**Name**	FBK(PL 25-12-30)
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

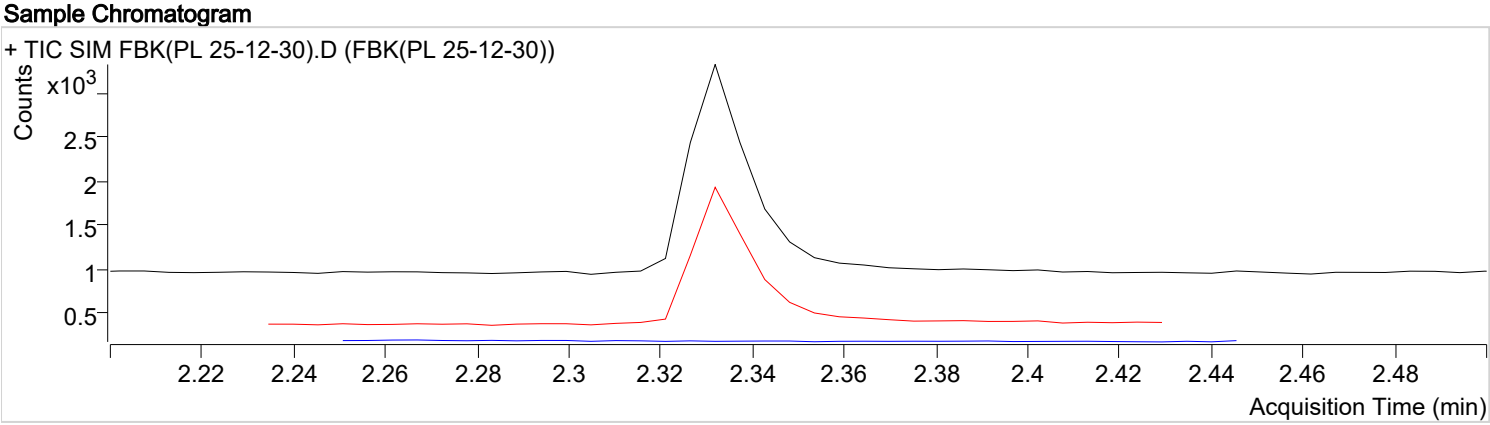

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			2332	ND mg/L

1,4-Dioxane

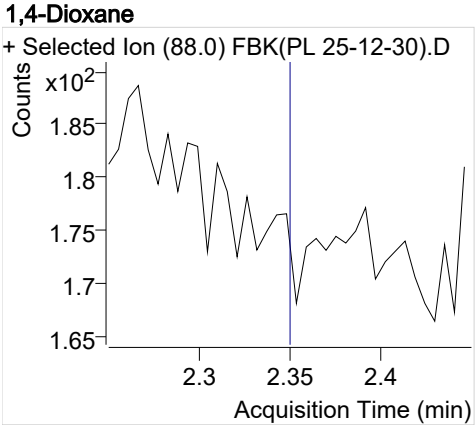





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(PL 12.30)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-08 오전 11:42:59	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:45:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:42:59	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오후 1:39:04	**Data File**	PL-01.D
Type	Sample	**Name**	PL-01
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

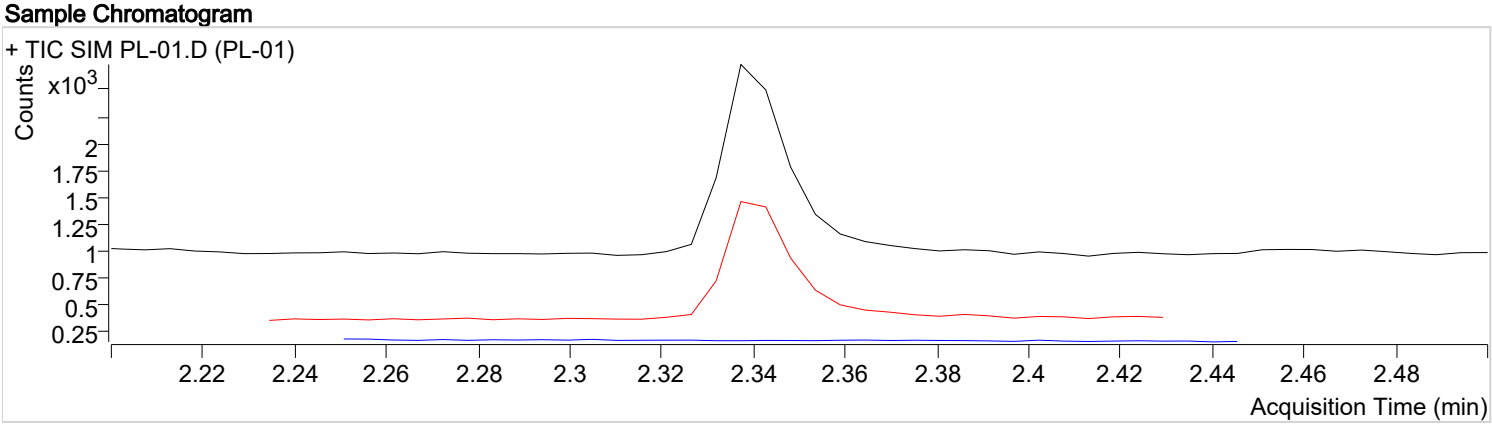

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1843	ND mg/L

1,4-Dioxane

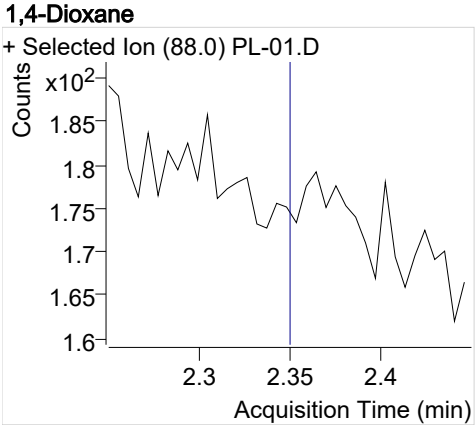

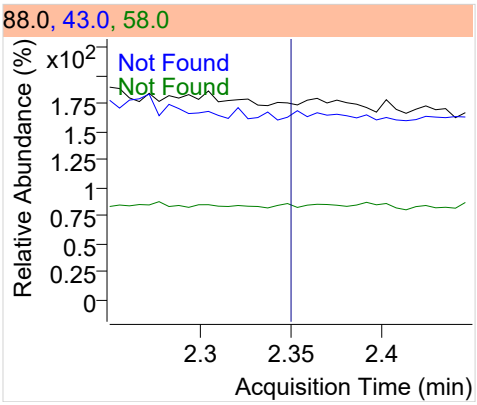

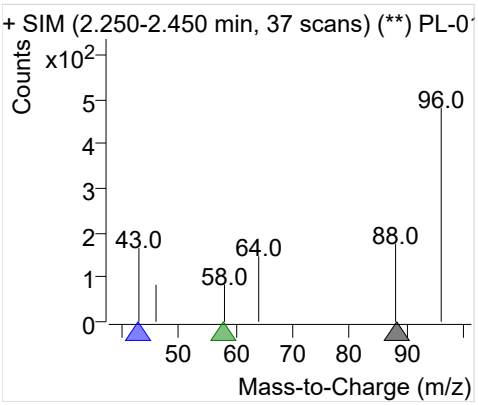

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(PL 12.30)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-08 오전 11:42:59	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:45:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:42:59	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오후 1:48:07	**Data File**	PL-02.D
Type	Sample	**Name**	PL-02
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

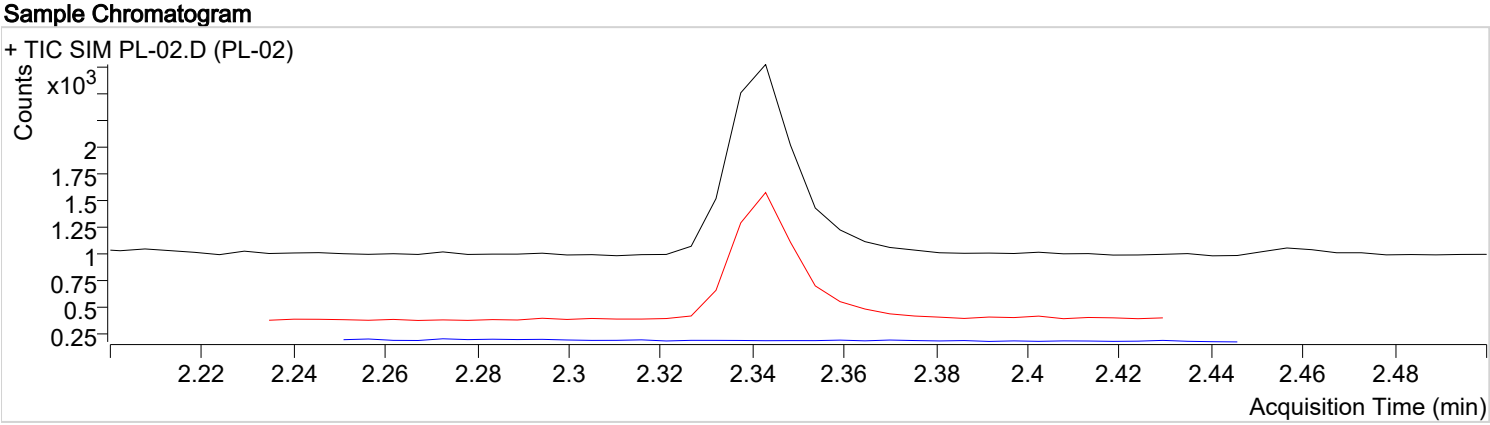

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1901	ND mg/L

1,4-Dioxane

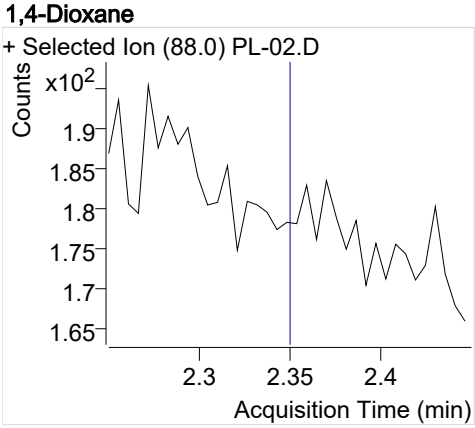



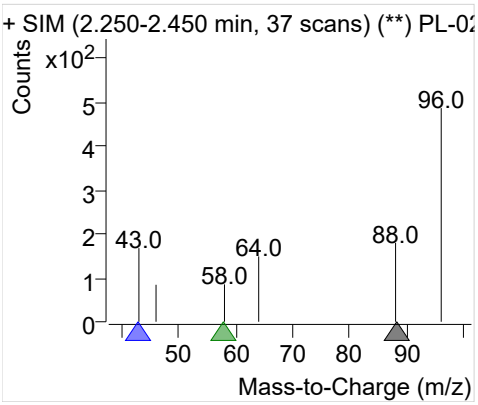

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(PL 12.30)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-08 오전 11:42:59	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:45:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:42:59	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오후 1:57:07	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

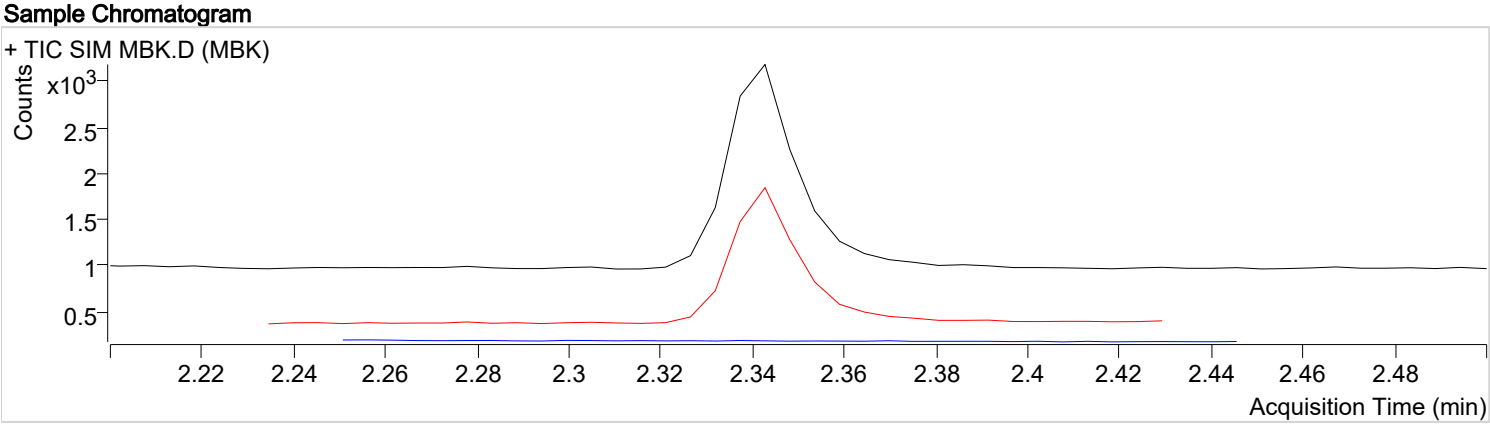

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			2423	ND mg/L

1,4-Dioxane

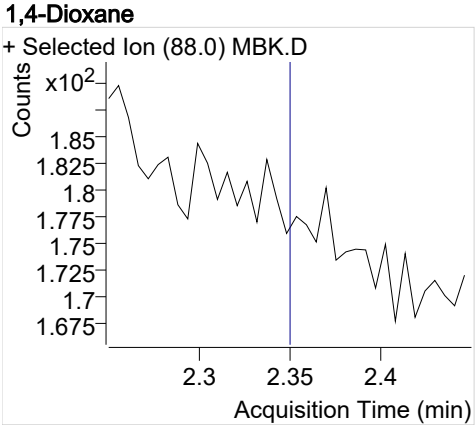



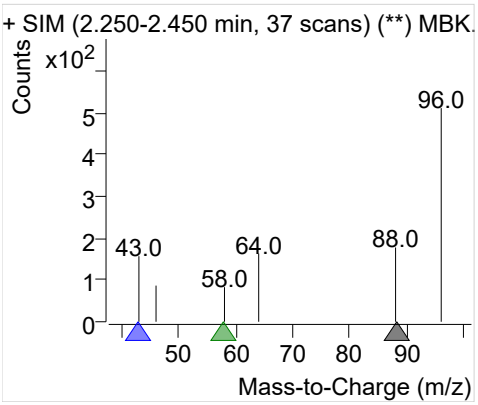

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(PL 12.30)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-08 오전 11:42:59	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:45:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:42:59	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오후 2:24:04	**Data File**	-C-C-V-1.D
Type	QC	**Name**	-C-C-V-1
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

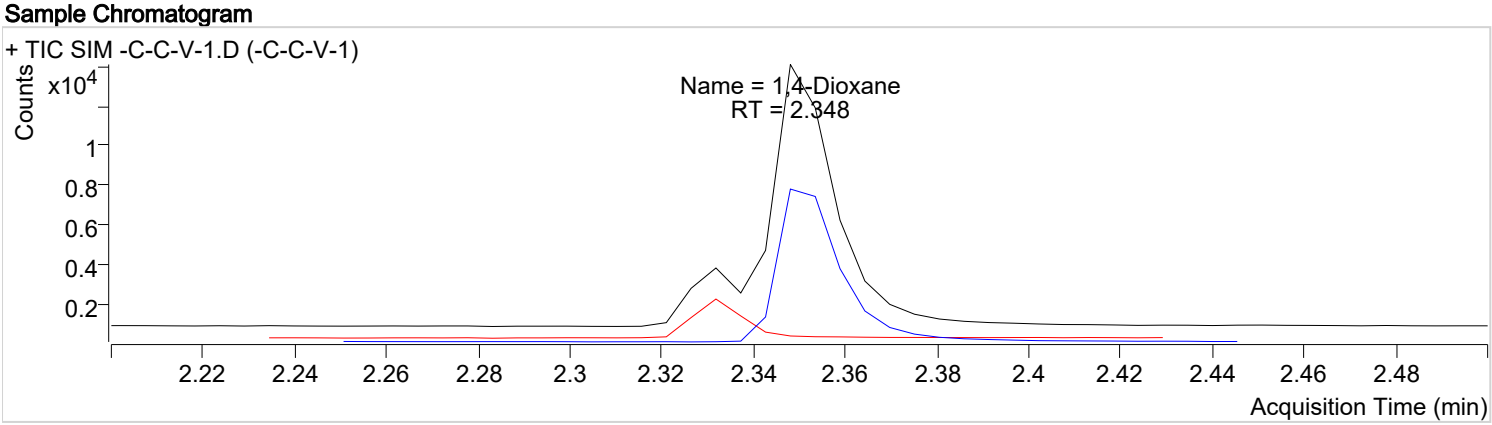

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.348	12152	2340	0.100 mg/L

1,4-Dioxane

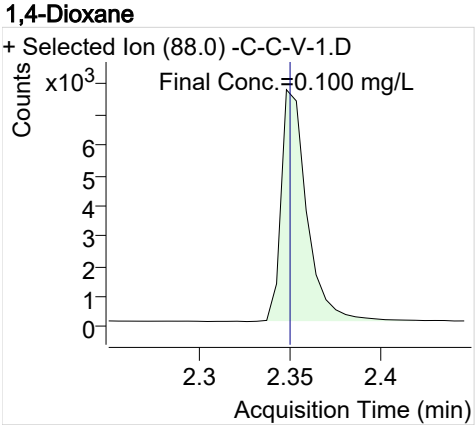

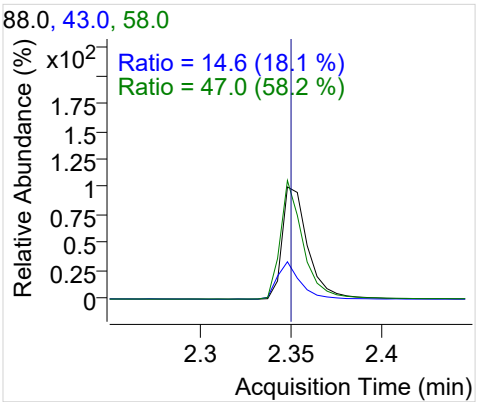

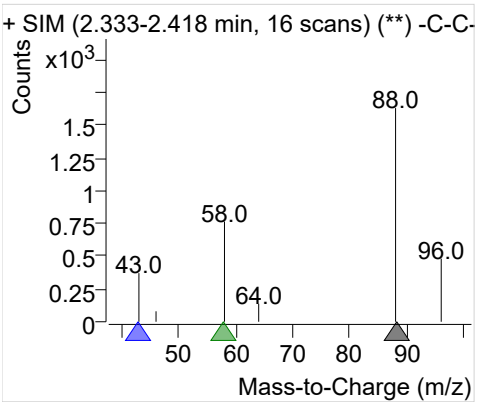

Generated at 오전 9:45 on 2026-04-10