Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(KD 1.15)\QuantResults\1,4.batch.bin				
Analysis Time	2026-01-19 오후 4:42:46	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-19 오후 4:42:46	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

1,4-Dioxane

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
1,4 ST-01.D	Cal	2.354	713	1430	0.010
1,4 ST-02.D	Cal	2.348	995	1033	0.020
1,4 ST-03.D	Cal	2.348	3770	1516	0.050
1,4 ST-04.D	Cal	2.353	7555	1857	0.081
1,4 ST-05.D	Cal	2.354	9018	1803	0.100
1,4 ST-06.D	Cal	2.343	9333	1173	0.158
1,4 ST-07.D	Cal	2.348	16613	1645	0.201
BK-.D	Blank			1835	ND
FBK(KD 26-01-15).D	Blank			1321	ND
KD-01.D	Sample	2.354	0	1245	ND
KG-02.D	Sample	2.353	0	1804	ND
MBK.D	Blank			1882	ND
CCV.D	QC	2.348	7096	1392	0.102

1,4-Dioxane

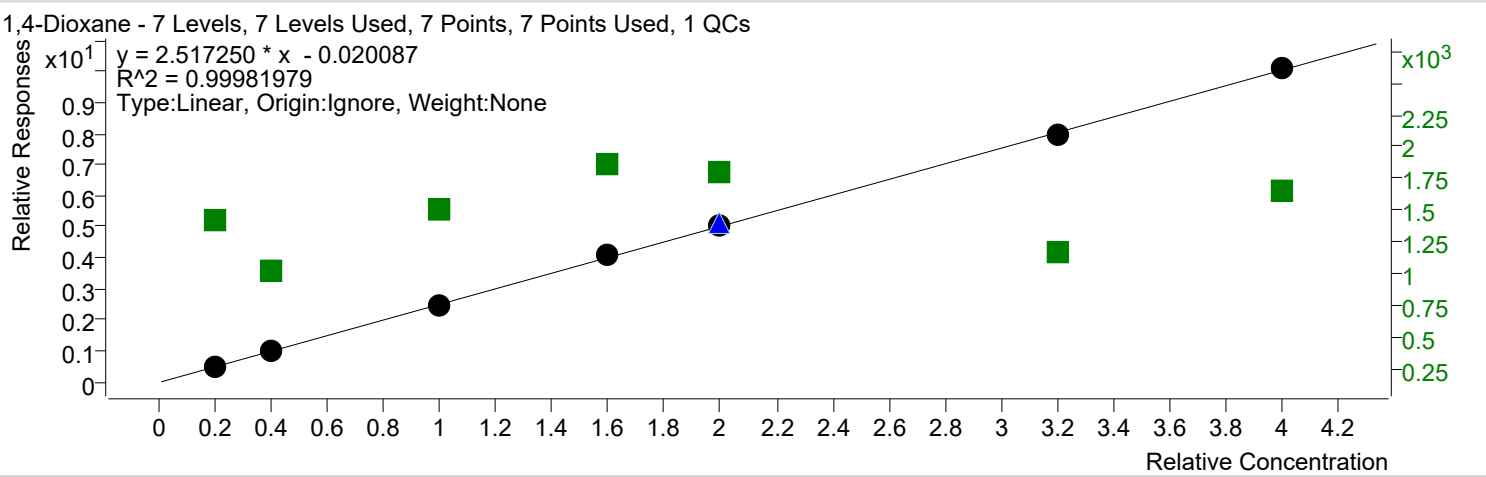

Cal. Path	Type	Level	Enable	Conc.	Response
W:\2026\1. 2026-01\1,4(KD 1.15)\1,4 ST-01.D	Calibration	1	x	0.200	713
W:\2026\1. 2026-01\1,4(KD 1.15)\1,4 ST-02.D	Calibration	2	x	0.400	995
W:\2026\1. 2026-01\1,4(KD 1.15)\1,4 ST-03.D	Calibration	3	x	1.000	3770
W:\2026\1. 2026-01\1,4(KD 1.15)\1,4 ST-04.D	Calibration	4	x	1.600	7555
W:\2026\1. 2026-01\1,4(KD 1.15)\1,4 ST-05.D	Calibration	5	x	2.000	9018
W:\2026\1. 2026-01\1,4(KD 1.15)\CCV.D	QC	5	x	2.000	7096
W:\2026\1. 2026-01\1,4(KD 1.15)\1,4 ST-06.D	Calibration	6	x	3.200	9333
W:\2026\1. 2026-01\1,4(KD 1.15)\1,4 ST-07.D	Calibration	7	x	4.000	16613

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(KD 1.15)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-19 오후 4:42:46	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:43:48	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-19 오후 4:42:46	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오전 11:49:23	**Data File**	1,4 ST-01.D
Type	Cal	**Name**	1,4 ST-01
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

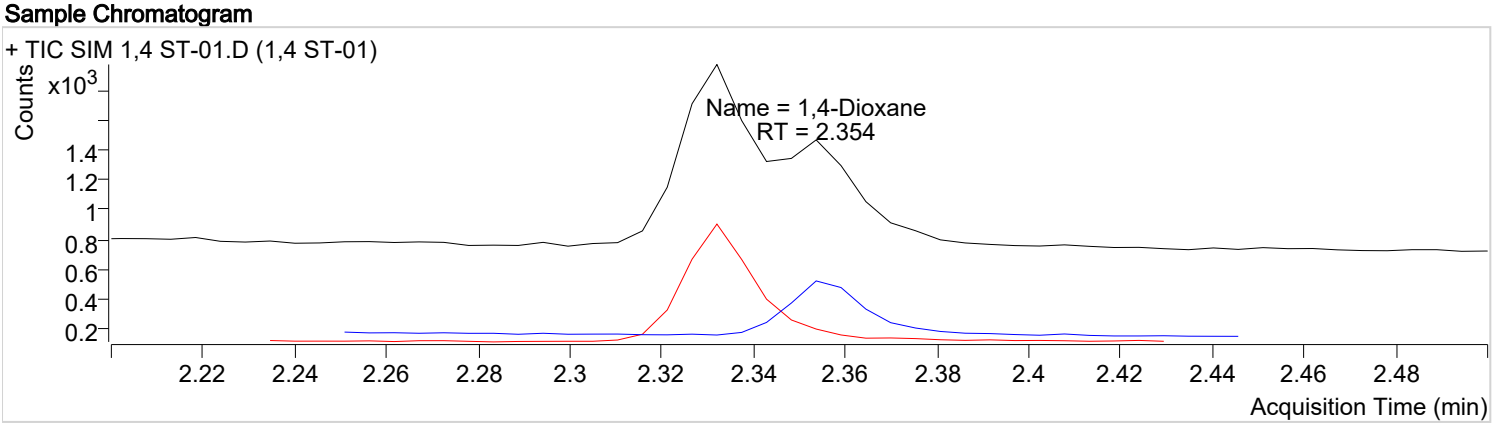

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.354	713	1430	0.010 mg/L

1,4-Dioxane

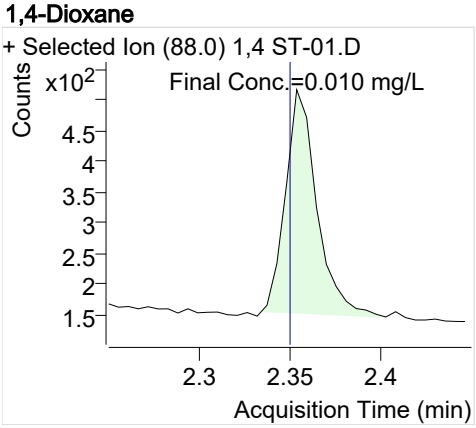





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(KD 1.15)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-19 오후 4:42:46	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:43:48	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-19 오후 4:42:46	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오전 11:58:26	**Data File**	1,4 ST-02.D
Type	Cal	**Name**	1,4 ST-02
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

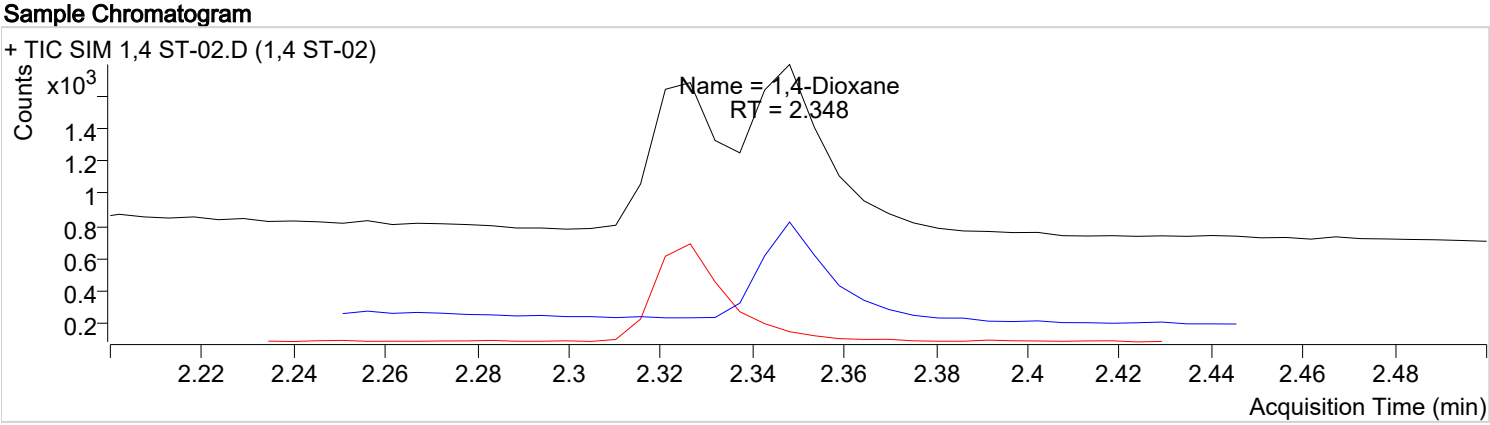

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.348	995	1033	0.020 mg/L

1,4-Dioxane

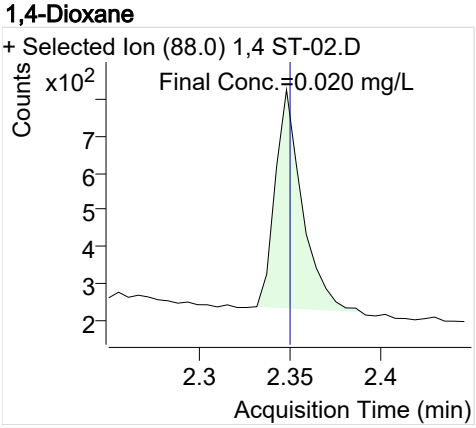





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(KD 1.15)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-19 오후 4:42:46	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:43:48	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-19 오후 4:42:46	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 12:07:30	**Data File**	1,4 ST-03.D
Type	Cal	**Name**	1,4 ST-03
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

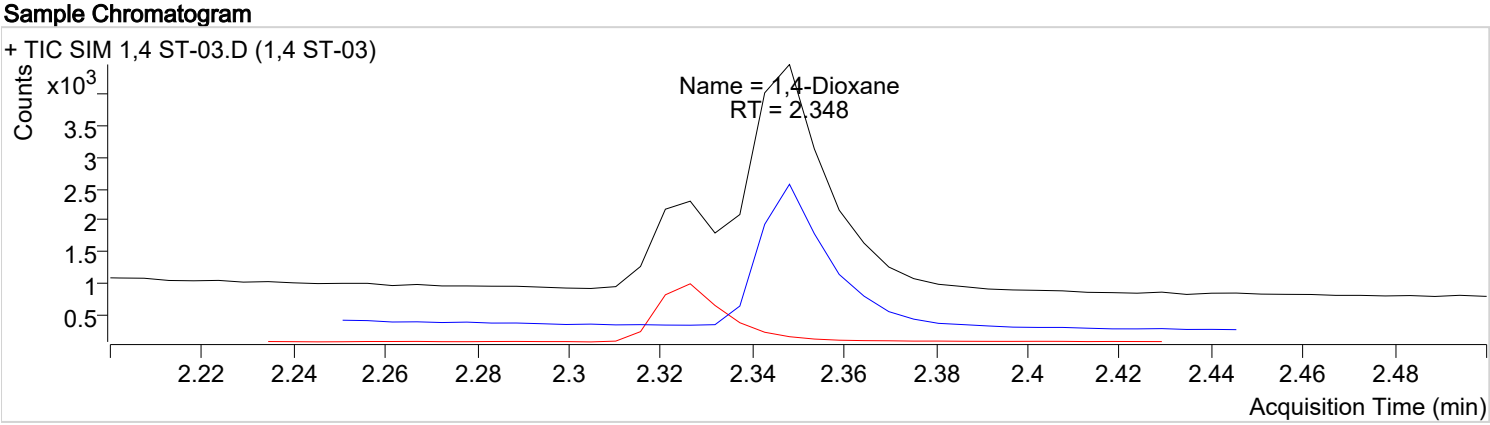

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.348	3770	1516	0.050 mg/L

1,4-Dioxane

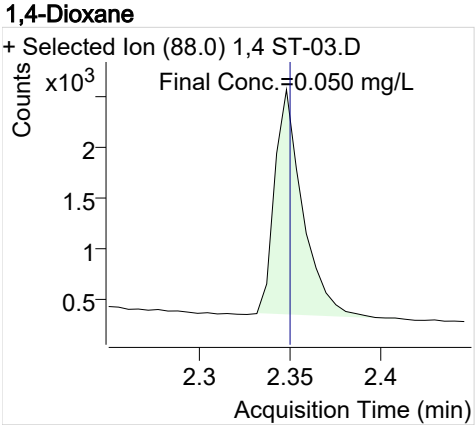

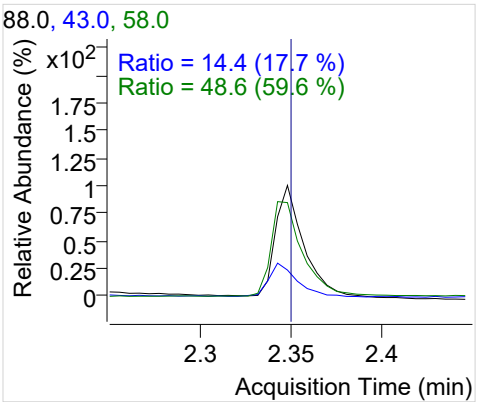

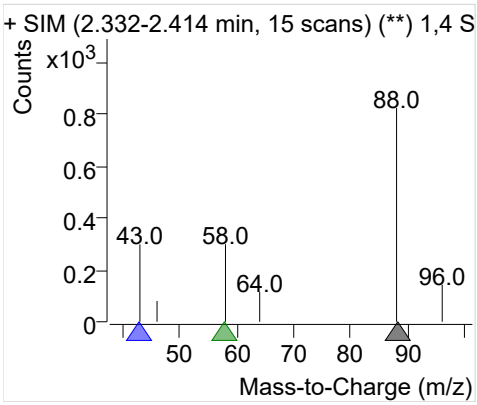

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(KD 1.15)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-19 오후 4:42:46	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:43:48	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-19 오후 4:42:46	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 12:16:38	**Data File**	1,4 ST-04.D
Type	Cal	**Name**	1,4 ST-04
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

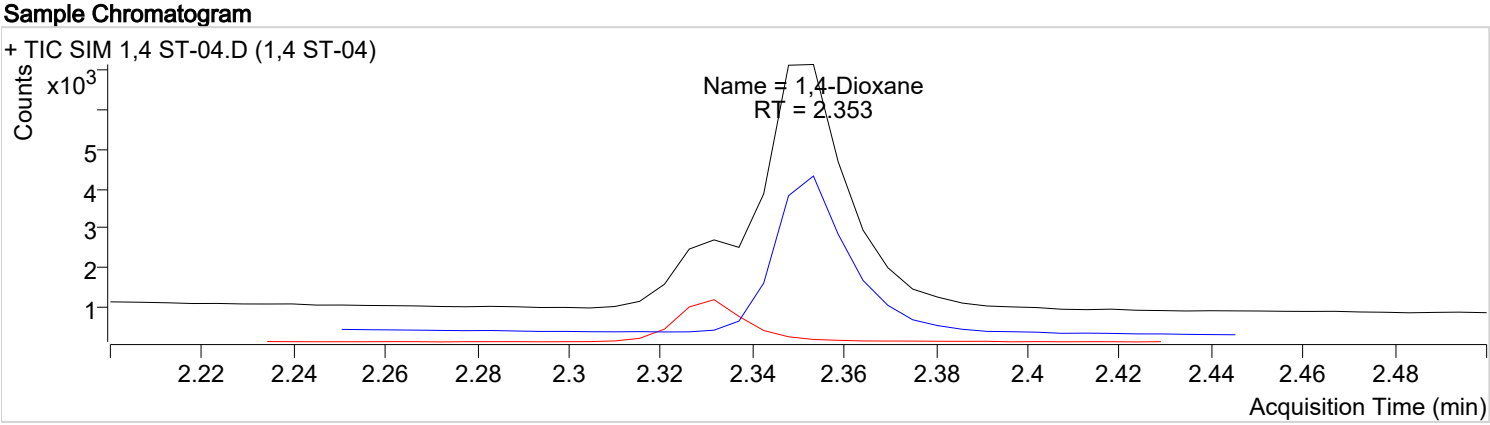

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.353	7555	1857	0.081 mg/L

1,4-Dioxane

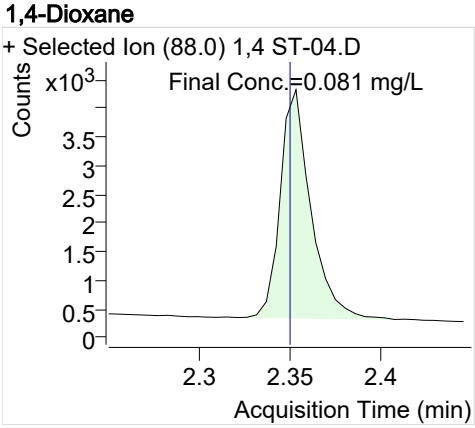





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(KD 1.15)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-19 오후 4:42:46	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:43:48	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-19 오후 4:42:46	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 12:25:45	**Data File**	1,4 ST-05.D
Type	Cal	**Name**	1,4 ST-05
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

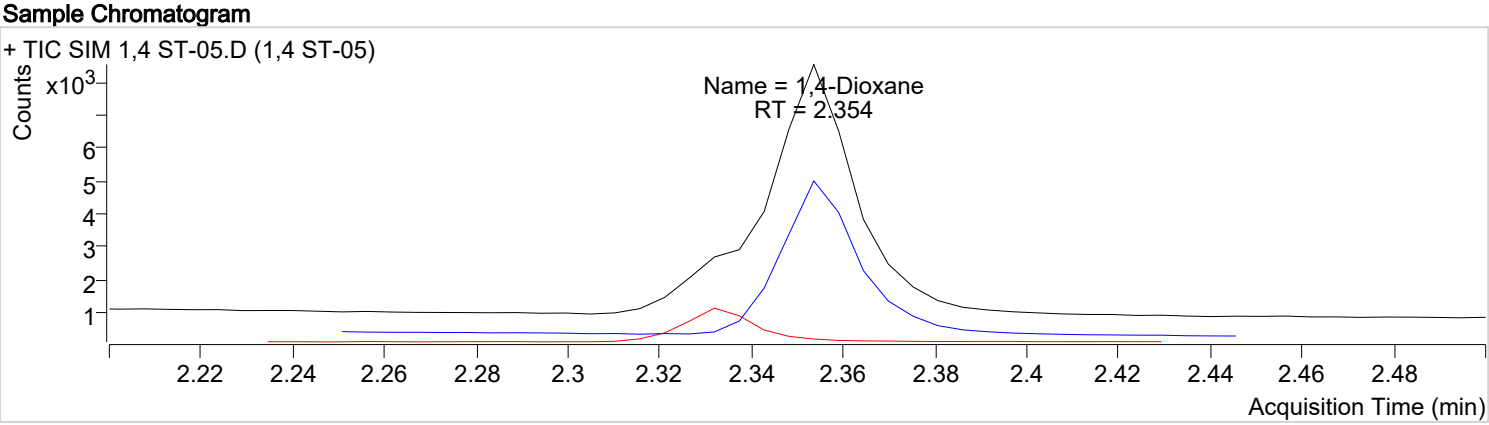

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.354	9018	1803	0.100 mg/L

1,4-Dioxane

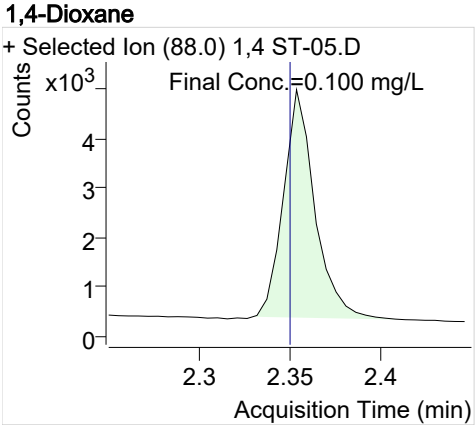

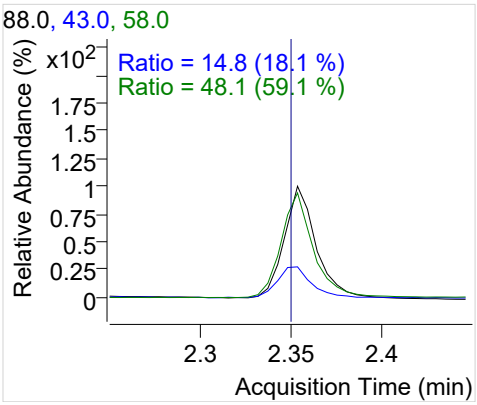

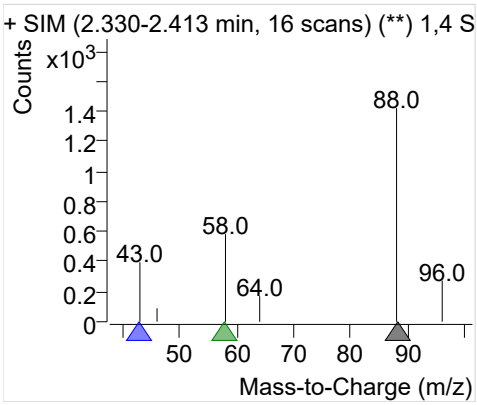

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(KD 1.15)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-19 오후 4:42:46	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:43:48	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-19 오후 4:42:46	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 12:34:53	**Data File**	1,4 ST-06.D
Type	Cal	**Name**	1,4 ST-06
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

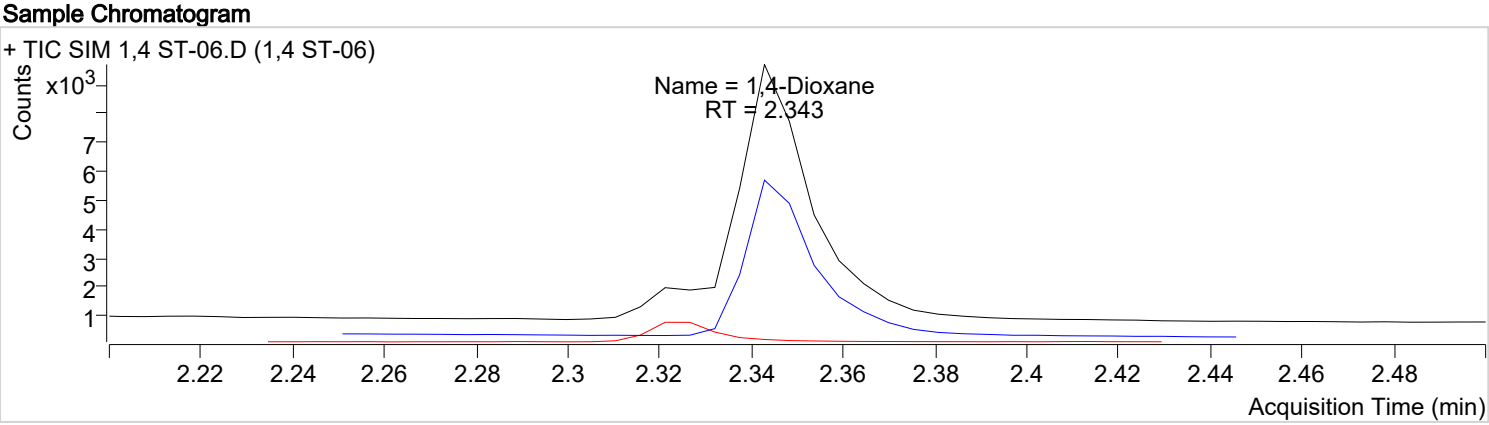

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.343	9333	1173	0.158 mg/L

1,4-Dioxane

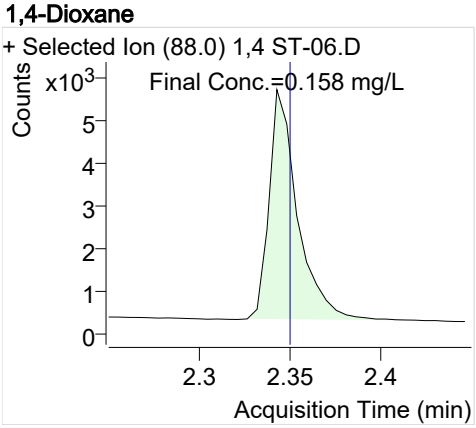

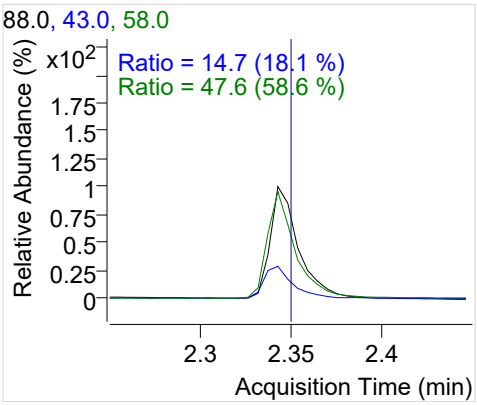



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(KD 1.15)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-19 오후 4:42:46	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:43:48	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-19 오후 4:42:46	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 12:44:03	**Data File**	1,4 ST-07.D
Type	Cal	**Name**	1,4 ST-07
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

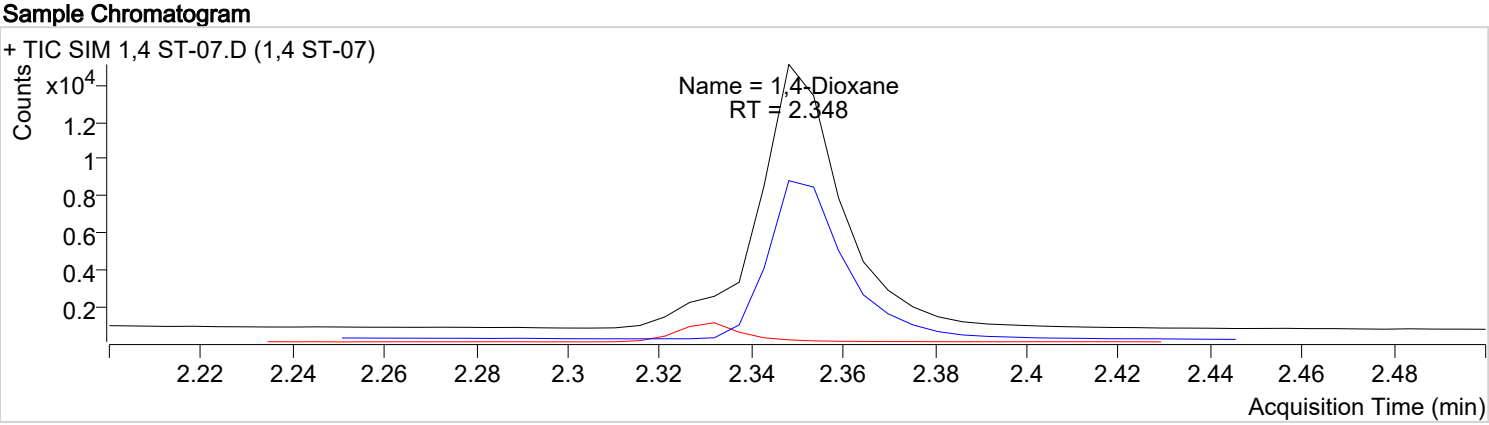

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.348	16613	1645	0.201 mg/L

1,4-Dioxane

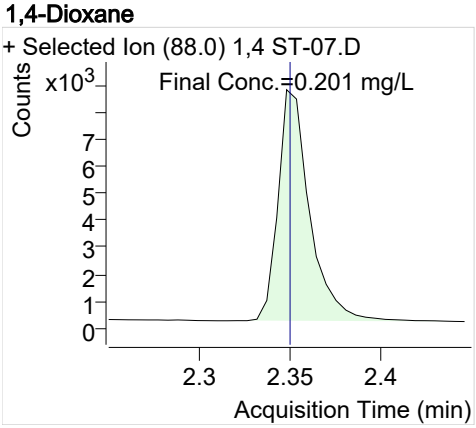

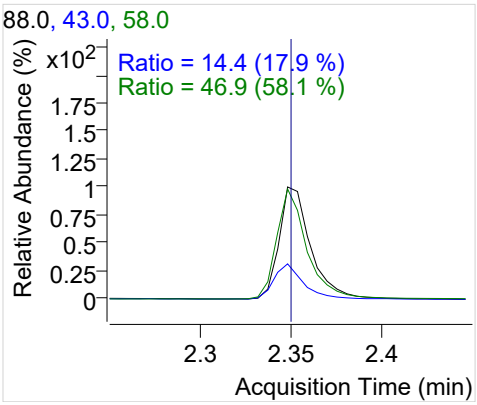

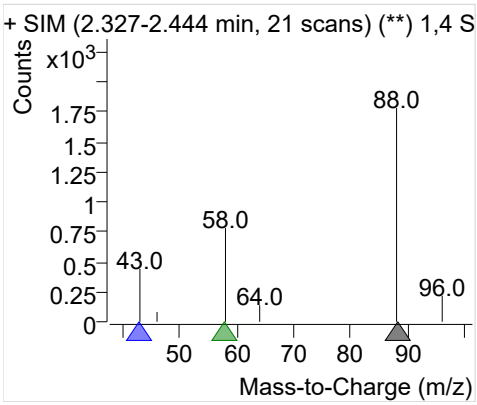

Generated at 오전 9:43 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(KD 1.15)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-19 오후 4:42:46	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:43:48	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-19 오후 4:42:46	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 1:02:22	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

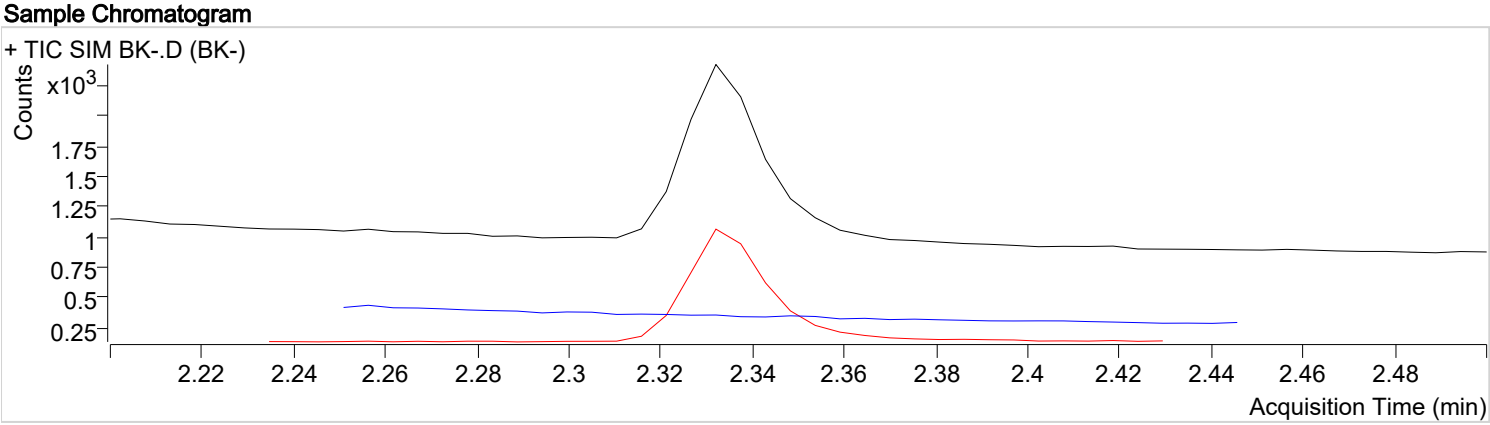

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1835	ND mg/L

1,4-Dioxane

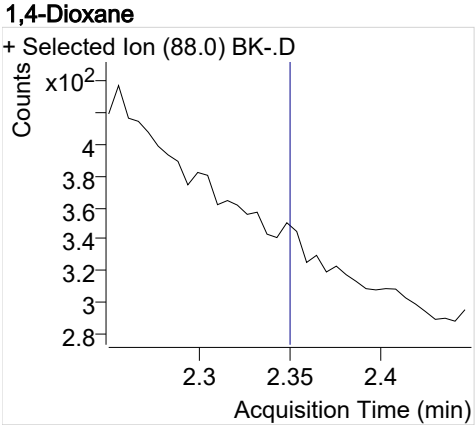



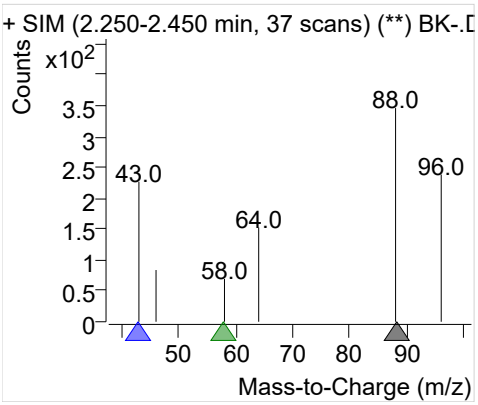

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(KD 1.15)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-19 오후 4:42:46	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:43:48	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-19 오후 4:42:46	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 1:11:31	**Data File**	FBK(KD 26-01-15).D
Type	Blank	**Name**	FBK(KD 26-01-15)
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

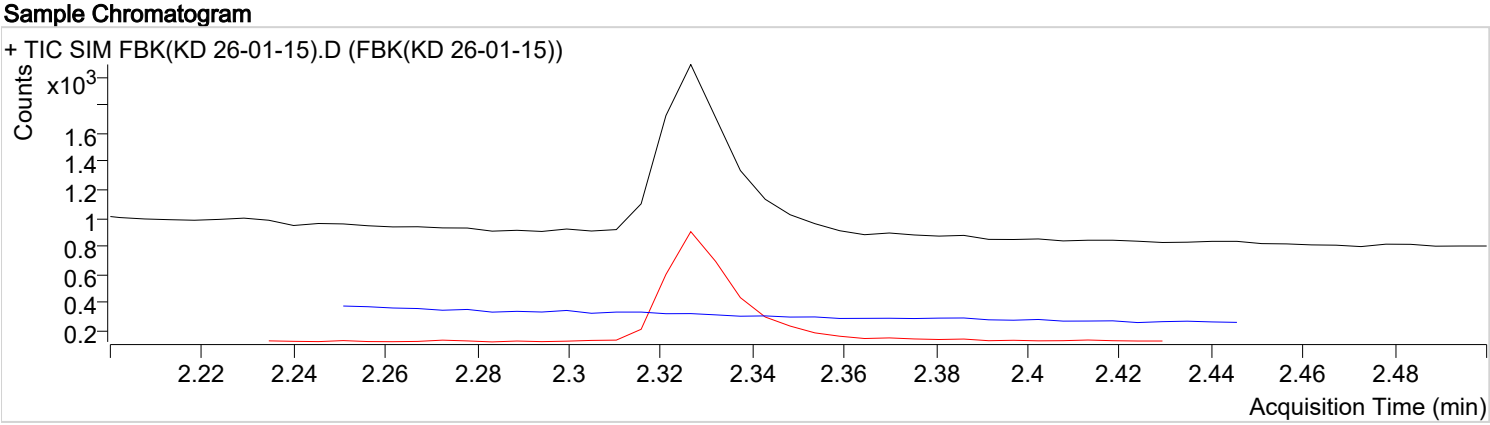

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1321	ND mg/L

1,4-Dioxane

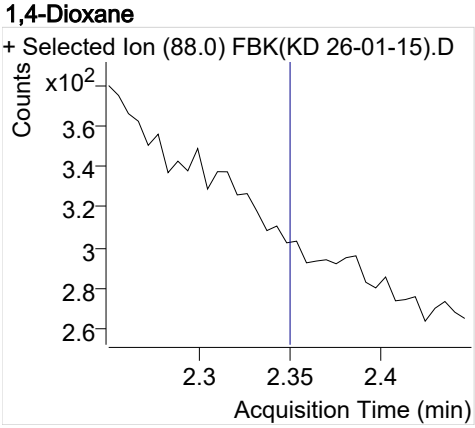



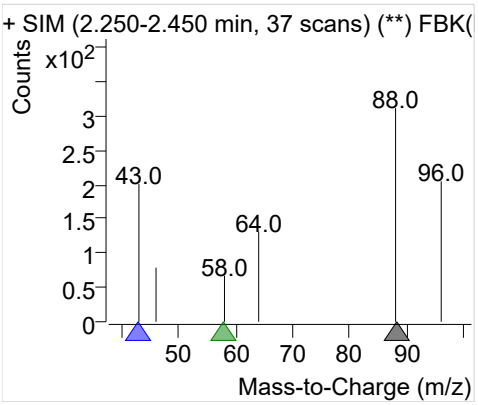

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(KD 1.15)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-19 오후 4:42:46	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:43:48	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-19 오후 4:42:46	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 1:20:38	**Data File**	KD-01.D
Type	Sample	**Name**	KD-01
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

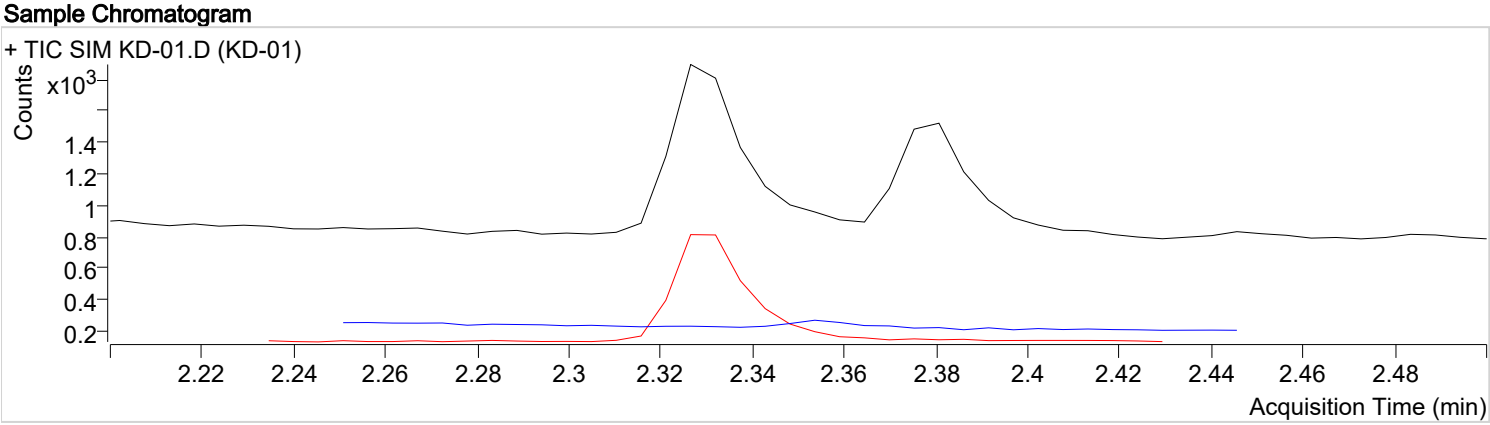

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.354	0	1245	ND mg/L

1,4-Dioxane

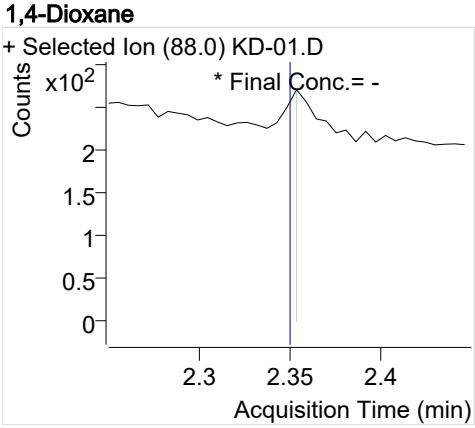



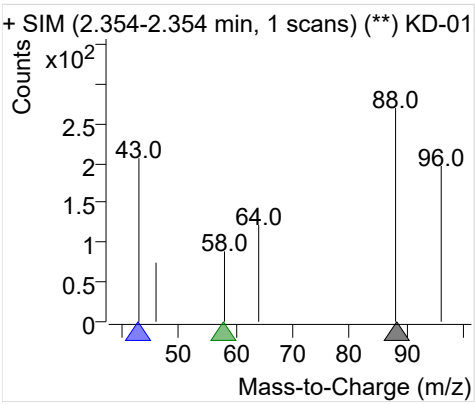

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(KD 1.15)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-19 오후 4:42:46	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:43:48	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-19 오후 4:42:46	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 1:29:47	**Data File**	KG-02.D
Type	Sample	**Name**	KG-02
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

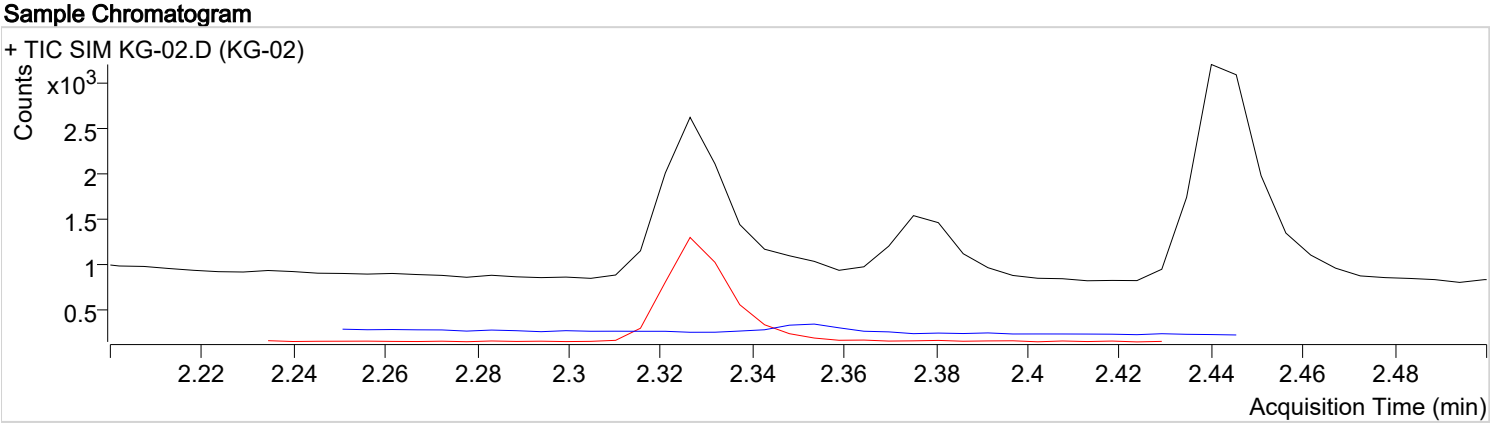

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.353	0	1804	ND mg/L

1,4-Dioxane

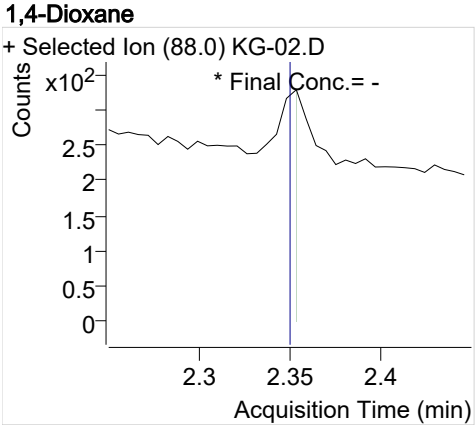





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\1,4(KD 1.15)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-19 오후 4:42:46	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:43:48	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-19 오후 4:42:46	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 1:38:55	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

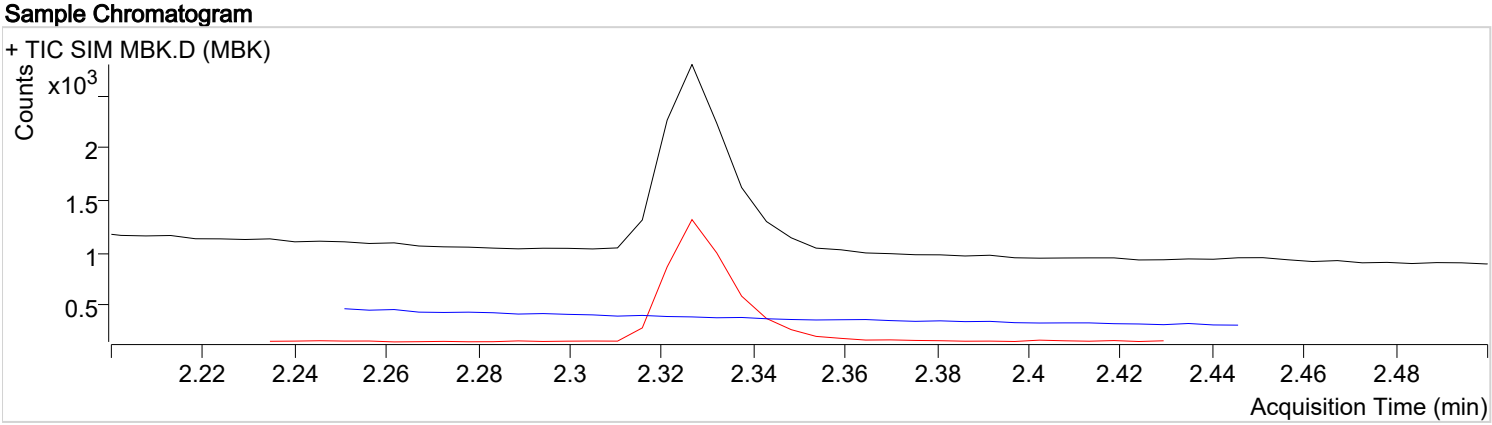

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1882	ND mg/L

1,4-Dioxane

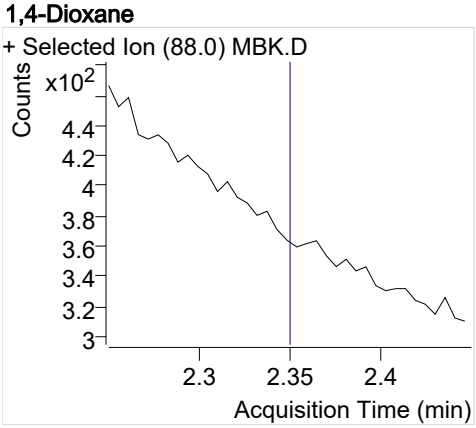

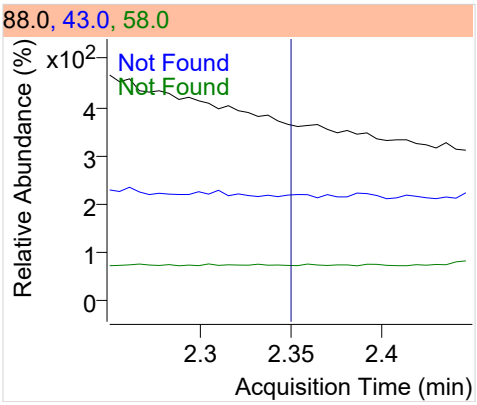

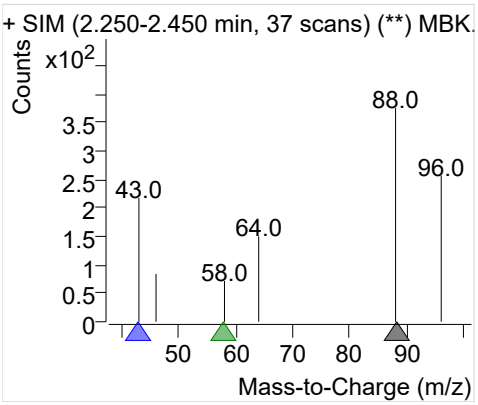

Quant Sample Report

Batch Data Path	W:\2026\1. 2026-01\1,4(KD 1.15)\QuantResults\1,4.batch.bin		
Analysis Time	2026-01-19 오후 4:42:46	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:43:48	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-19 오후 4:42:46	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 1:48:07	**Data File**	CCV.D
Type	QC	**Name**	CCV
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

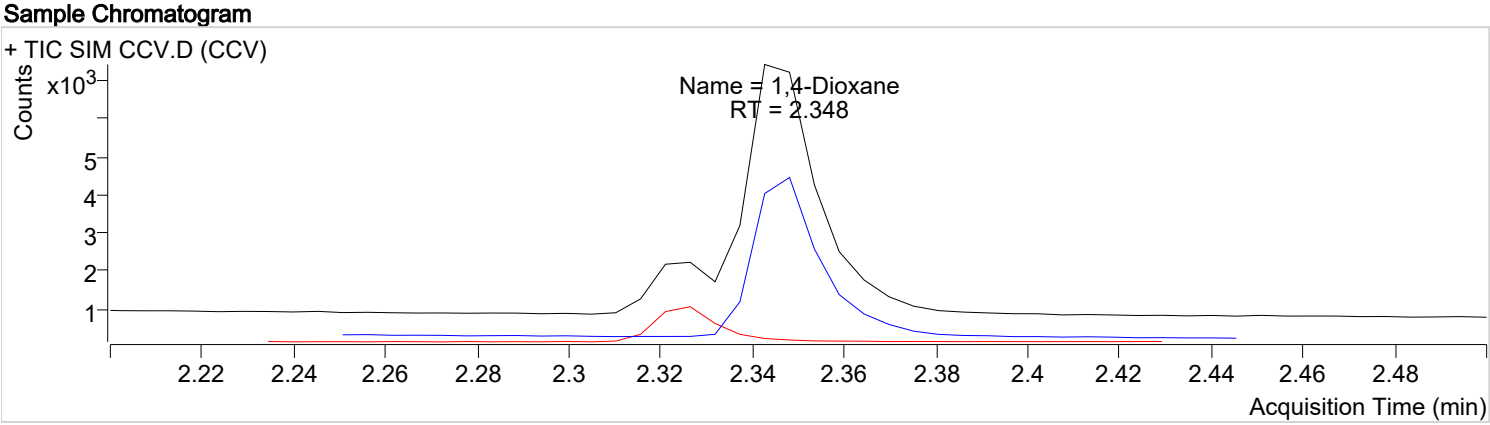

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.348	7096	1392	0.102 mg/L

1,4-Dioxane

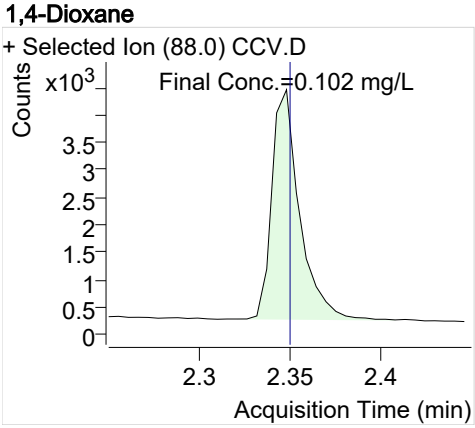



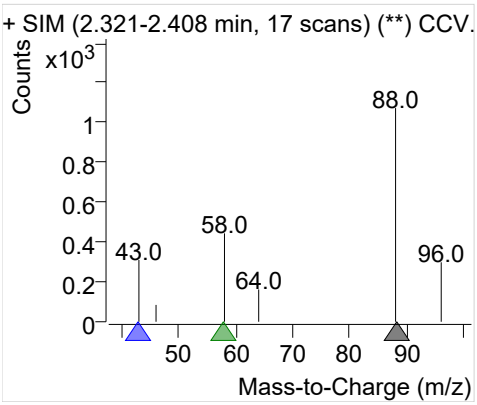

Generated at 오전 9:43 on 2026-04-10