Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin				
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

1,4-Dioxane

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
1,4 ST-01.D	Cal	2.348	1096	2286	0.010
1,4 ST-02.D	Cal	2.354	2499	2499	0.020
1,4 ST-03.D	Cal	2.348	5918	2373	0.050
1,4 ST-04.D	Cal	2.348	9462	2342	0.080
1,4 ST-05.D	Cal	2.354	11864	2345	0.100
1,4 ST-06.D	Cal	2.348	17265	2115	0.161
1,4 ST-07.D	Cal	2.348	23313	2306	0.199
BK-.D	Blank			2229	ND
FBK(KD 26-02-04).D	Blank			2125	ND
FBK(JR 26-02-05).D	Blank			2566	ND
KD-01.D	Sample			1864	ND
KD-04.D	Sample			2130	ND
JR-01.D	Sample	2.353	0	1689	ND
JR-02.D	Sample	2.353	0	1990	ND
JR-03.D	Sample	2.418	0	1517	ND
JR-04.D	Sample			1939	ND
JR-05.D	Sample			2066	ND
JR-06.D	Sample			1706	ND
JR-07.D	Sample	2.289	0	1655	ND
JR-08.D	Sample	2.299	0	2278	ND
MBK.D	Blank			1681	ND
-C-C-V-.D	QC	2.348	7752	1489	0.103

1,4-Dioxane

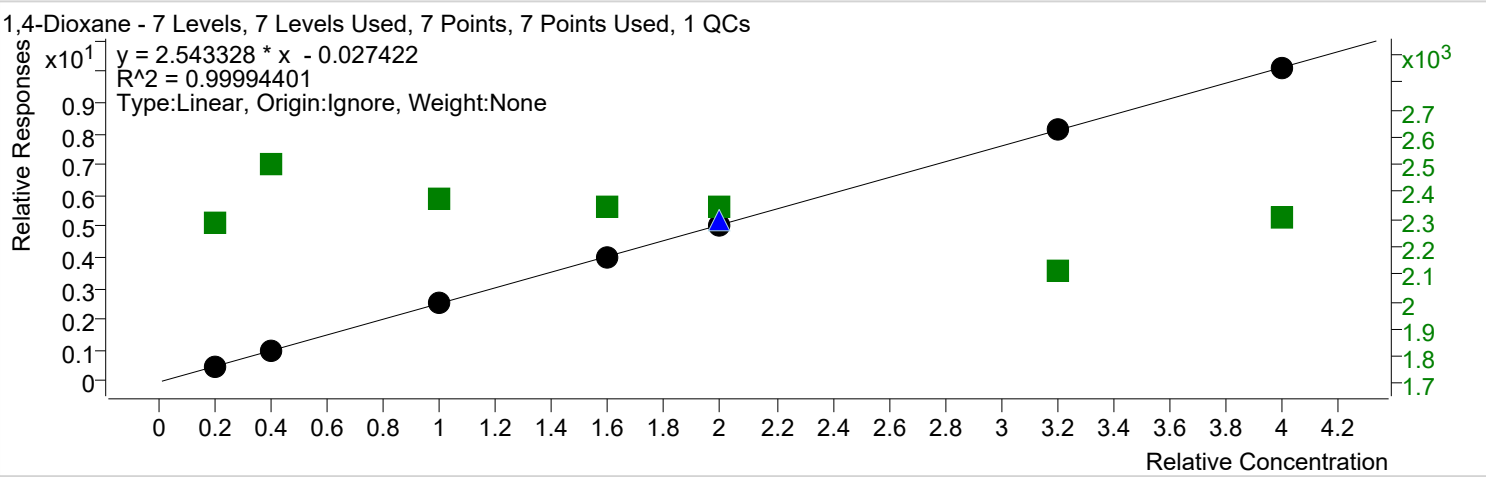

Cal. Path	Type	Level	Enable	Conc.	Response
\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\1,4 ST-01.D	Calibration	1	x	0.200	1096
\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\1,4 ST-02.D	Calibration	2	x	0.400	2499
\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\1,4 ST-03.D	Calibration	3	x	1.000	5918
\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\1,4 ST-04.D	Calibration	4	x	1.600	9462
\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\1,4 ST-05.D	Calibration	5	x	2.000	11864
\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\-C-C-V-.D	QC	5	x	2.000	7752
\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\1,4 ST-06.D	Calibration	6	x	3.200	17265
\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\1,4 ST-07.D	Calibration	7	x	4.000	23313

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오전 10:15:25	**Data File**	1,4 ST-01.D
Type	Cal	**Name**	1,4 ST-01
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

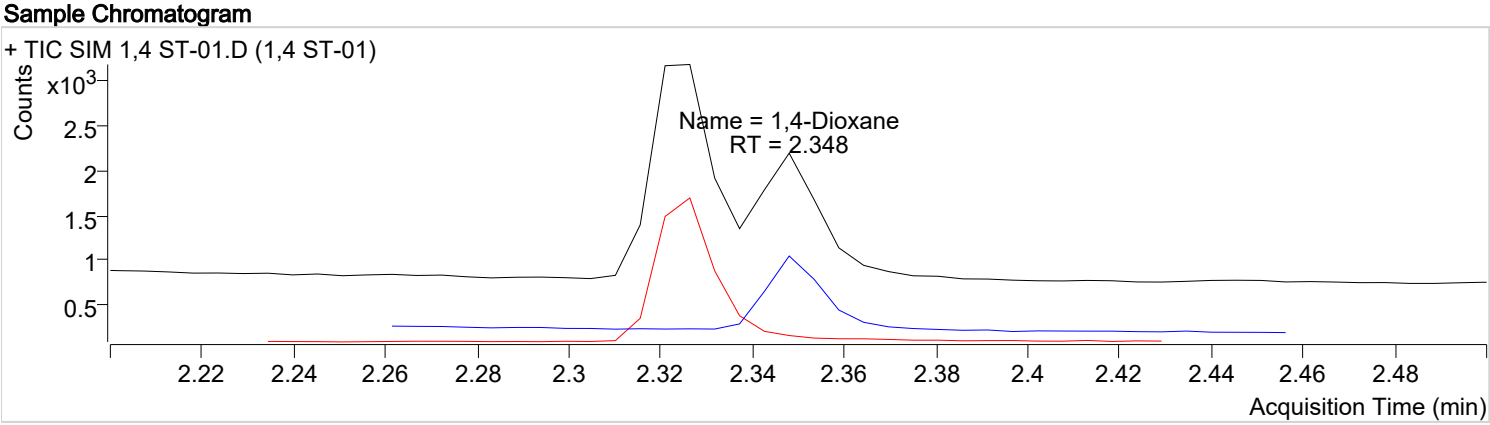

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.348	1096	2286	0.010 mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오전 10:24:23	**Data File**	1,4 ST-02.D
Type	Cal	**Name**	1,4 ST-02
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

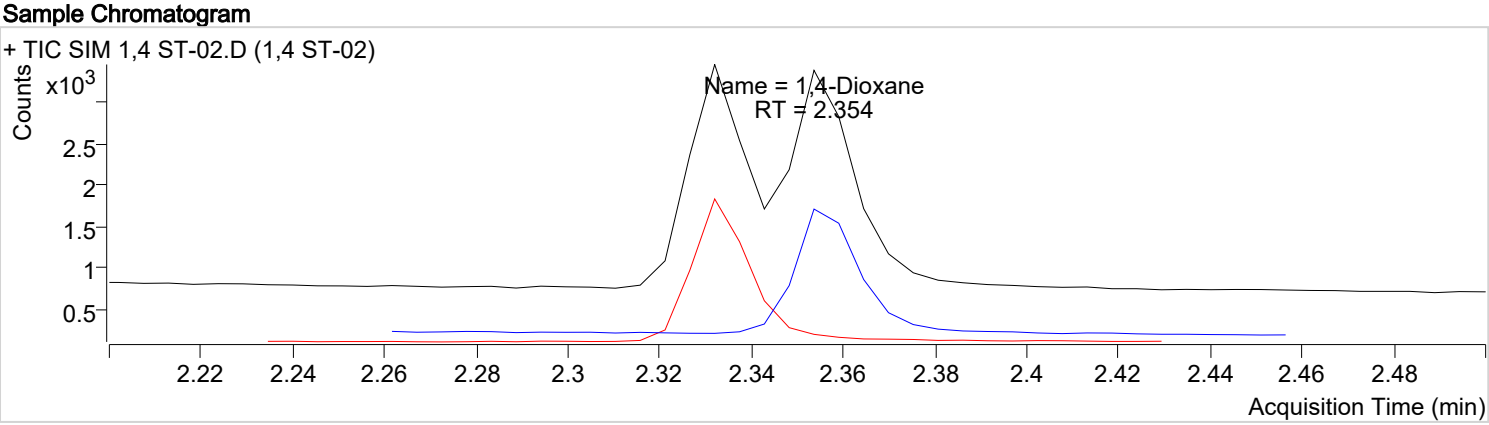

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.354	2499	2499	0.020 mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오전 10:33:23	**Data File**	1,4 ST-03.D
Type	Cal	**Name**	1,4 ST-03
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

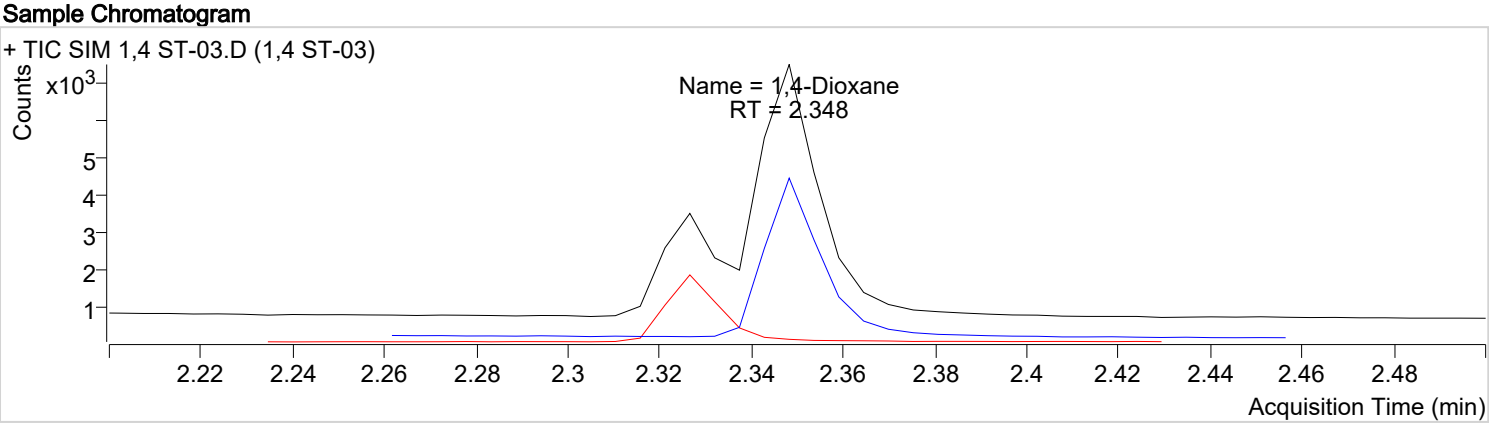

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.348	5918	2373	0.050 mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오전 10:42:26	**Data File**	1,4 ST-04.D
Type	Cal	**Name**	1,4 ST-04
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

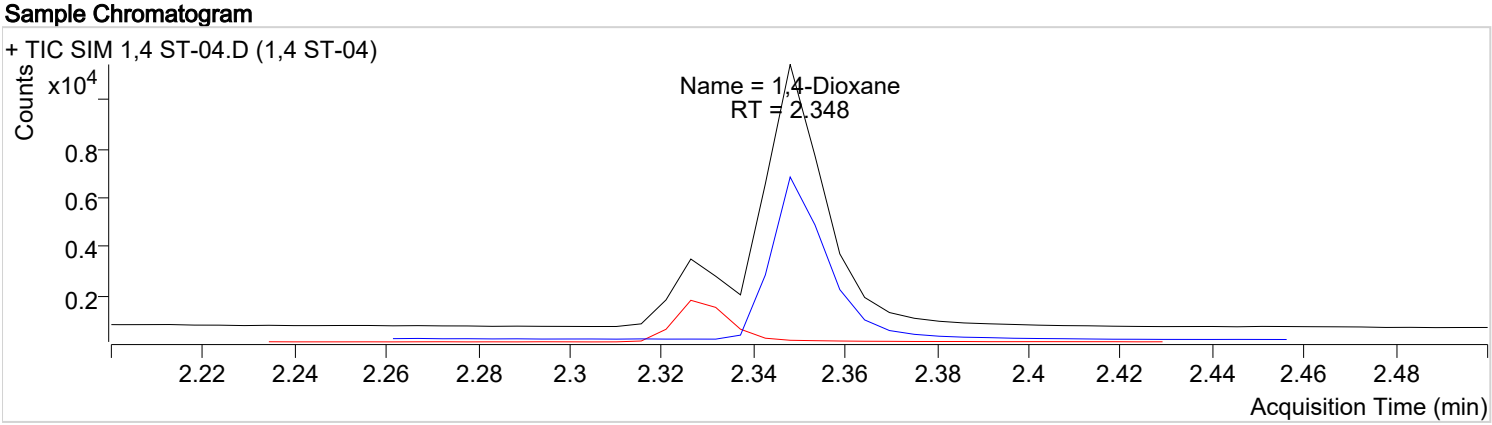

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.348	9462	2342	0.080 mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오전 10:51:29	**Data File**	1,4 ST-05.D
Type	Cal	**Name**	1,4 ST-05
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

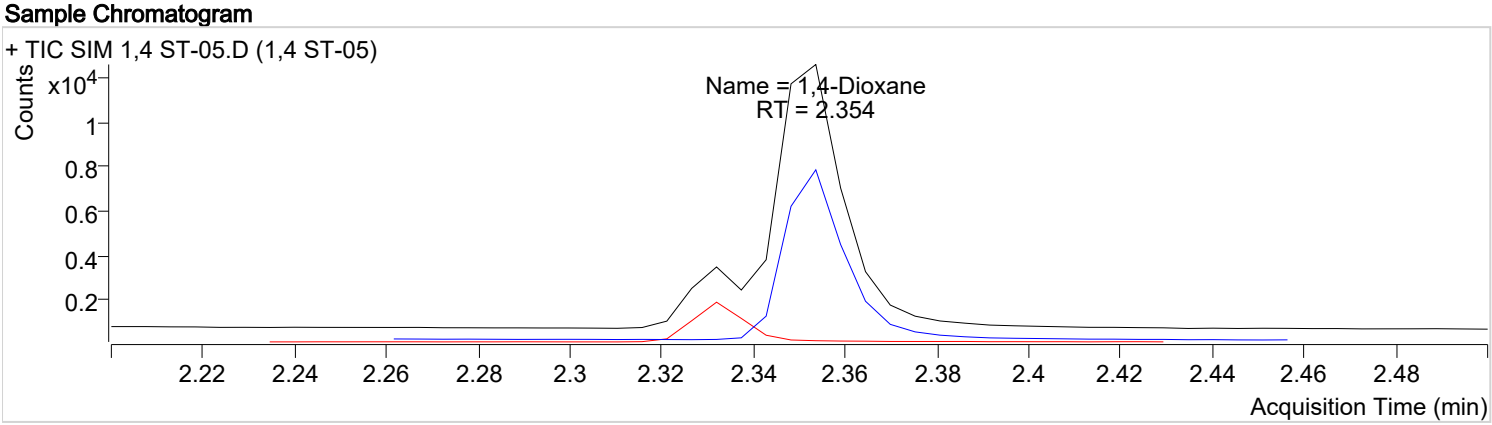

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.354	11864	2345	0.100 mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오전 11:00:32	**Data File**	1,4 ST-06.D
Type	Cal	**Name**	1,4 ST-06
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

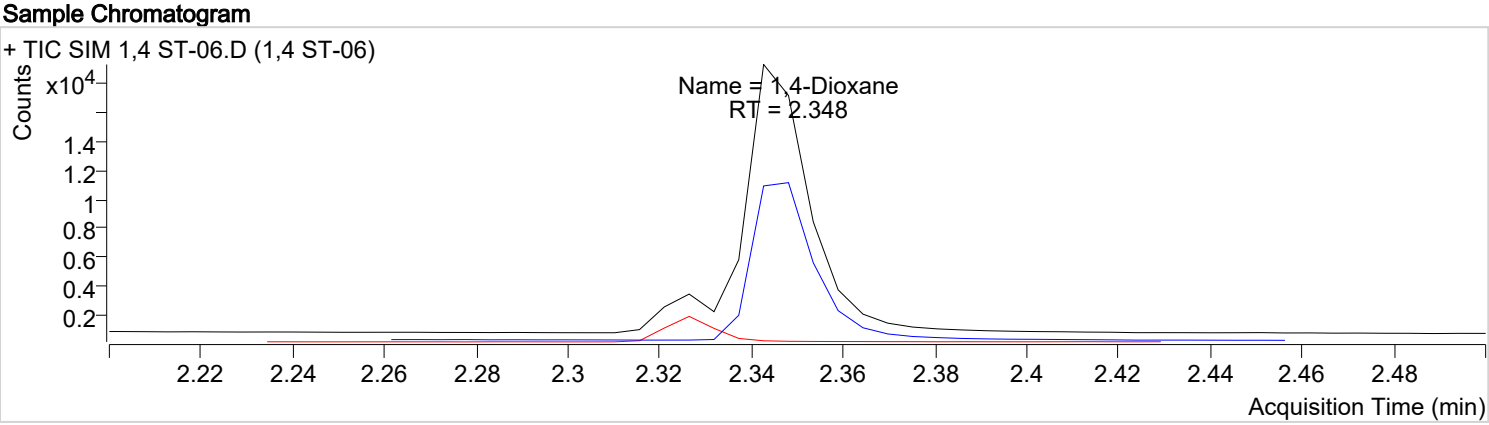

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.348	17265	2115	0.161 mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오전 11:09:38	**Data File**	1,4 ST-07.D
Type	Cal	**Name**	1,4 ST-07
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

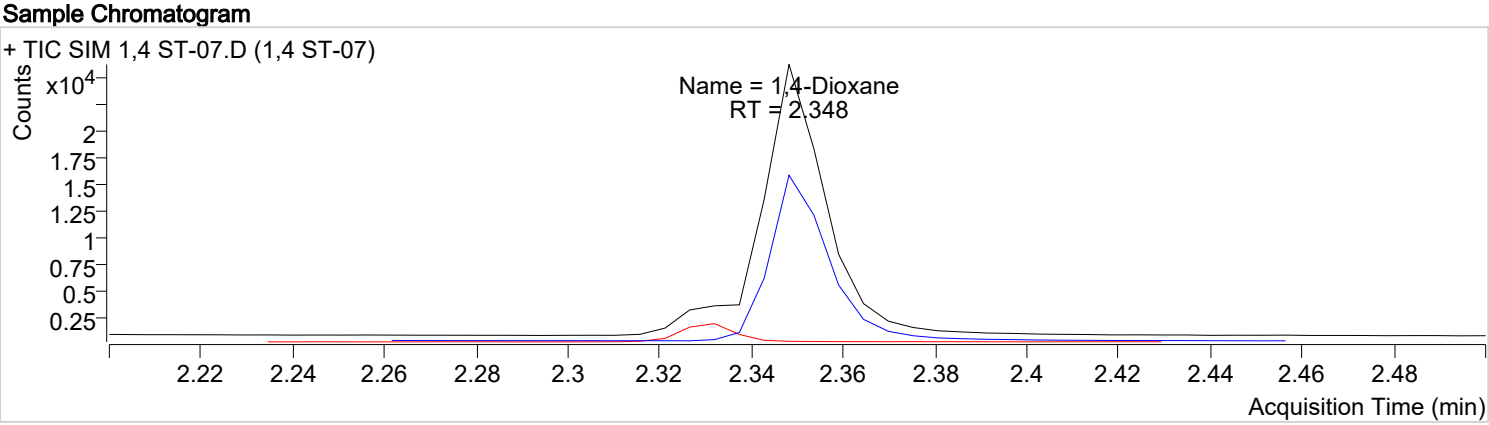

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.348	23313	2306	0.199 mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오전 11:27:47	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

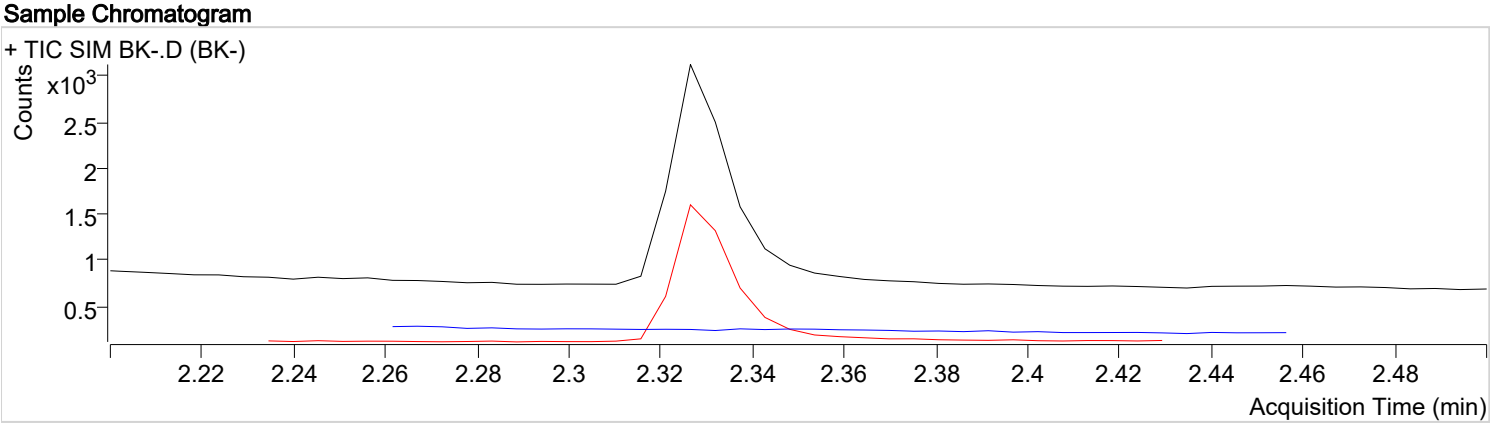

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			2229	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오전 11:36:53	**Data File**	FBK(KD 26-02-04).D
Type	Blank	**Name**	FBK(KD 26-02-04)
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

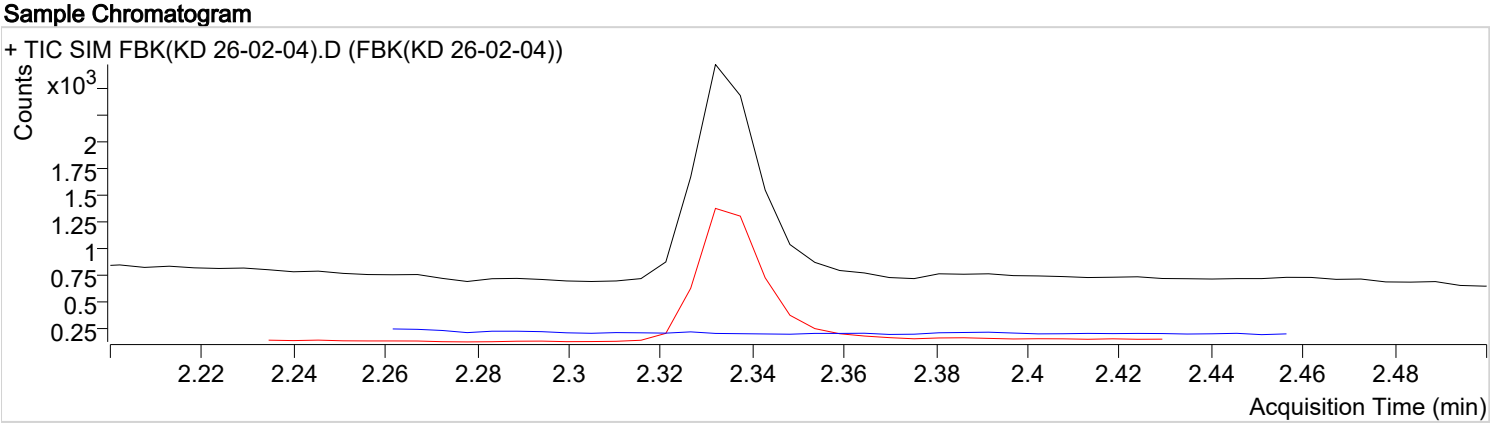

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			2125	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오전 11:45:59	**Data File**	FBK(JR 26-02-05).D
Type	Blank	**Name**	FBK(JR 26-02-05)
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

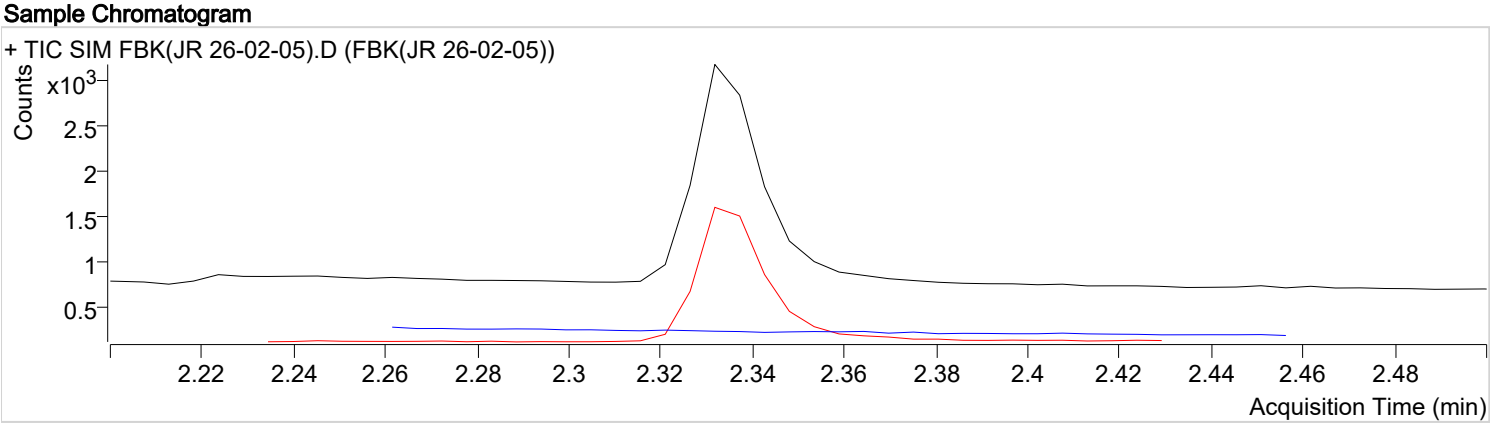

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			2566	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오전 11:55:06	**Data File**	KD-01.D
Type	Sample	**Name**	KD-01
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

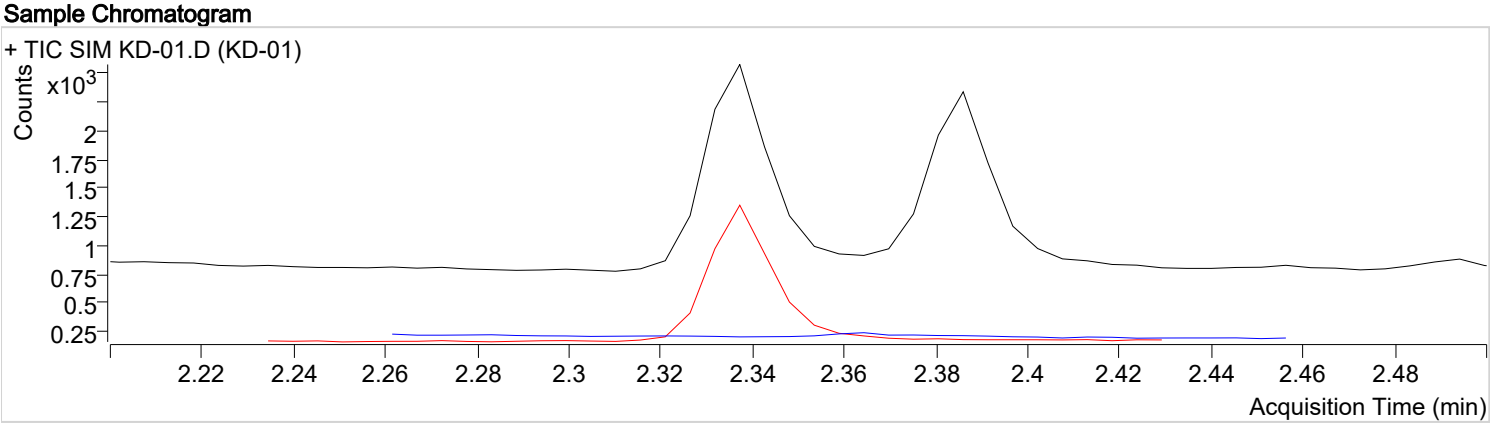

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1864	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오후 12:04:15	**Data File**	KD-04.D
Type	Sample	**Name**	KD-04
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

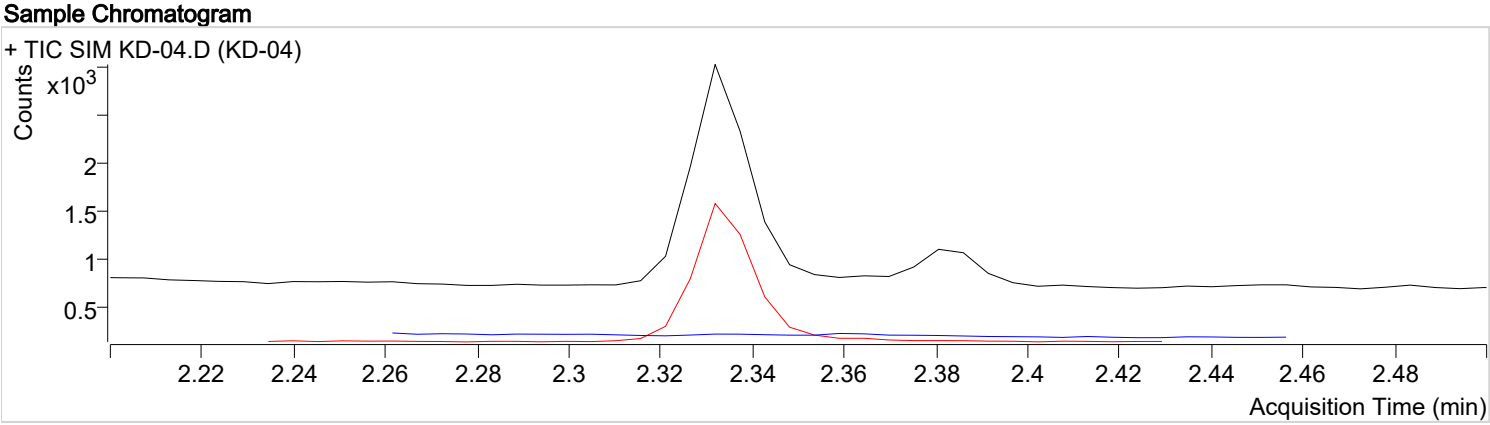

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			2130	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오후 12:13:22	**Data File**	JR-01.D
Type	Sample	**Name**	JR-01
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

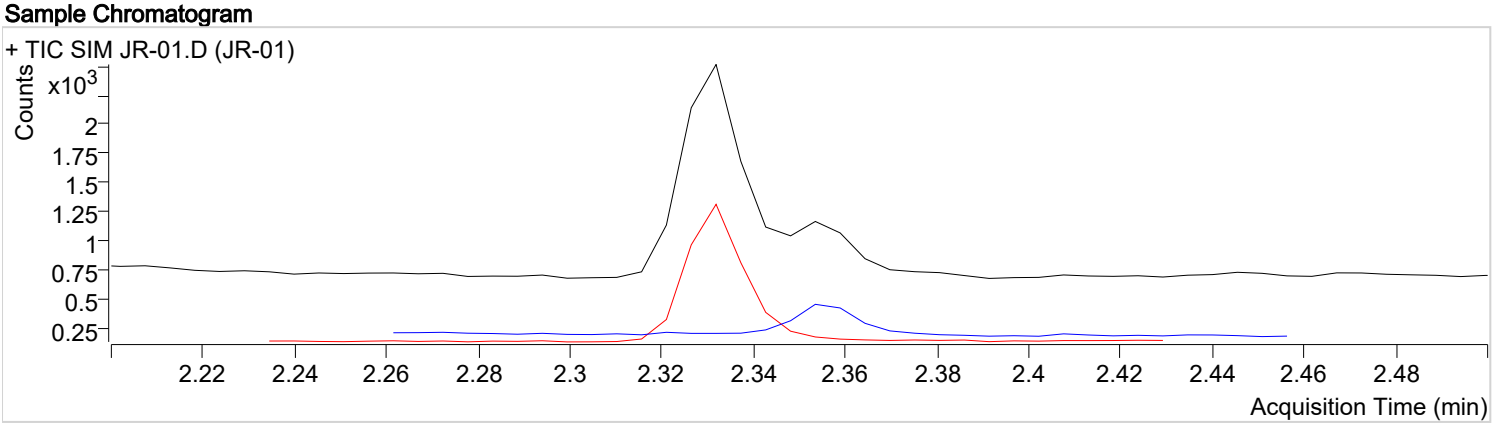

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.353	0	1689	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오후 12:22:27	**Data File**	JR-02.D
Type	Sample	**Name**	JR-02
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

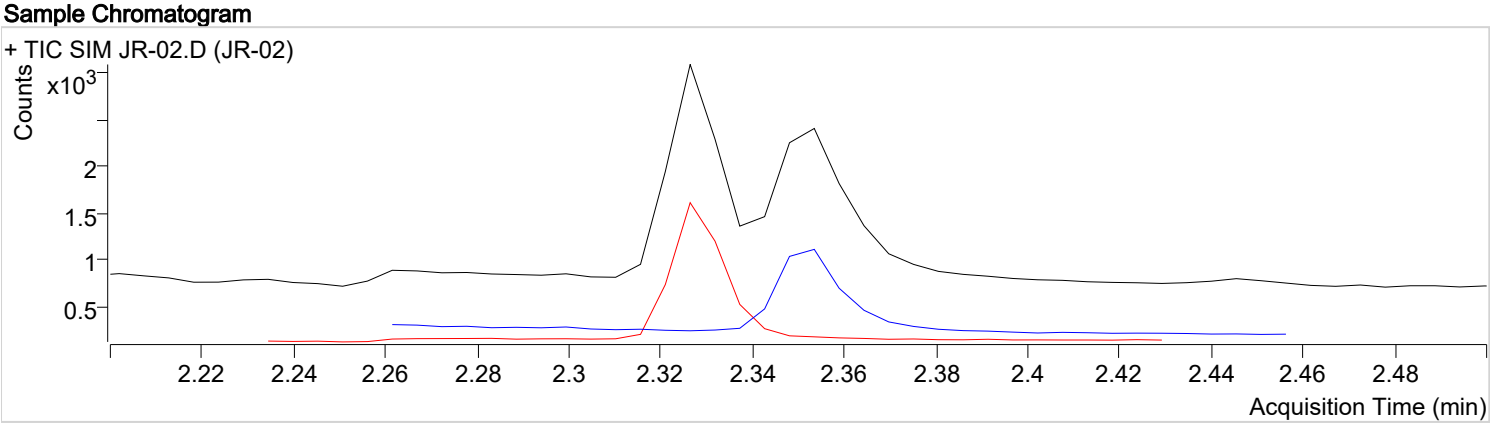

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.353	0	1990	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오후 12:31:33	**Data File**	JR-03.D
Type	Sample	**Name**	JR-03
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

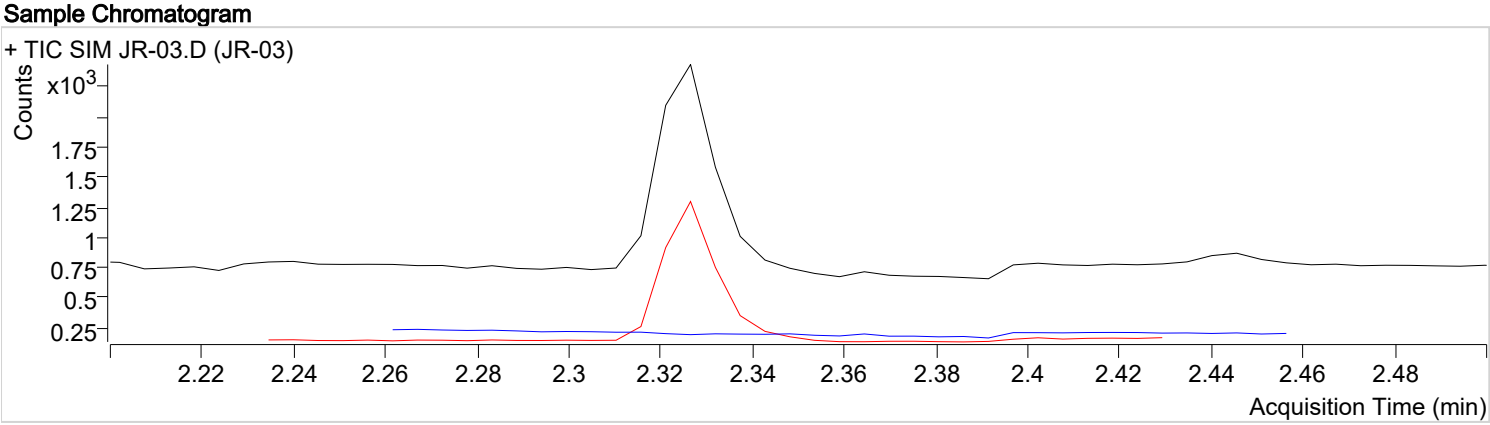

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.418	0	1517	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오후 12:40:39	**Data File**	JR-04.D
Type	Sample	**Name**	JR-04
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

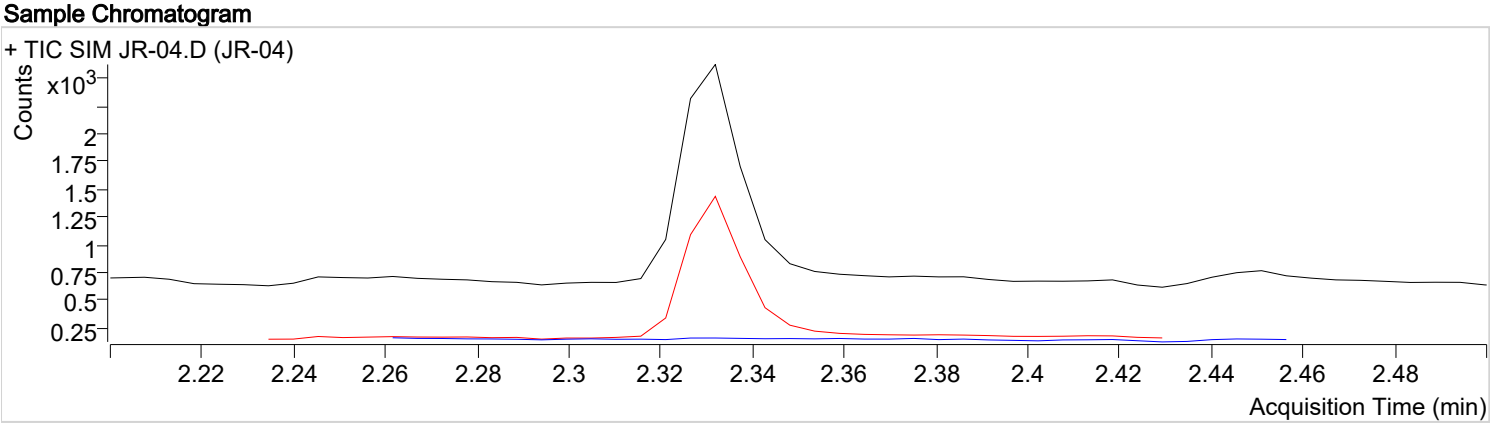

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1939	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오후 12:49:44	**Data File**	JR-05.D
Type	Sample	**Name**	JR-05
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

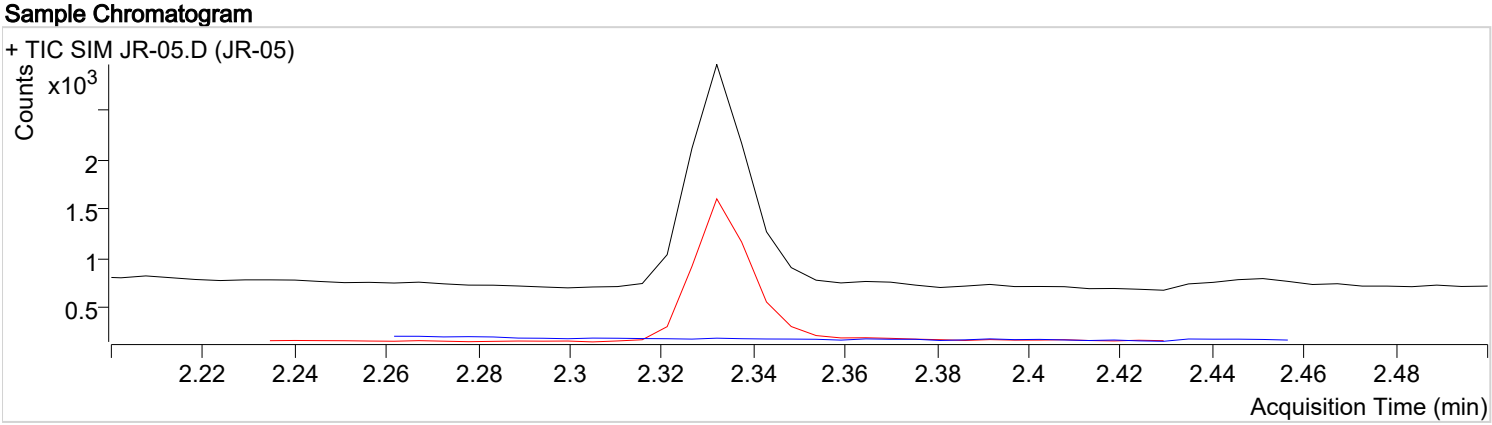

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			2066	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오후 12:58:55	**Data File**	JR-06.D
Type	Sample	**Name**	JR-06
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

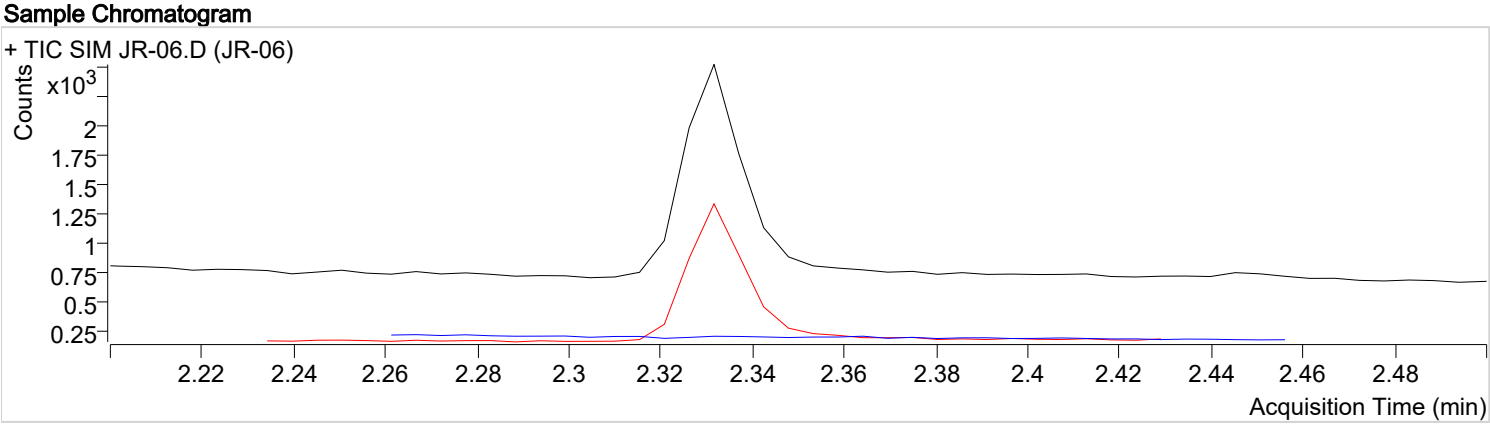

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1706	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오후 1:08:04	**Data File**	JR-07.D
Type	Sample	**Name**	JR-07
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

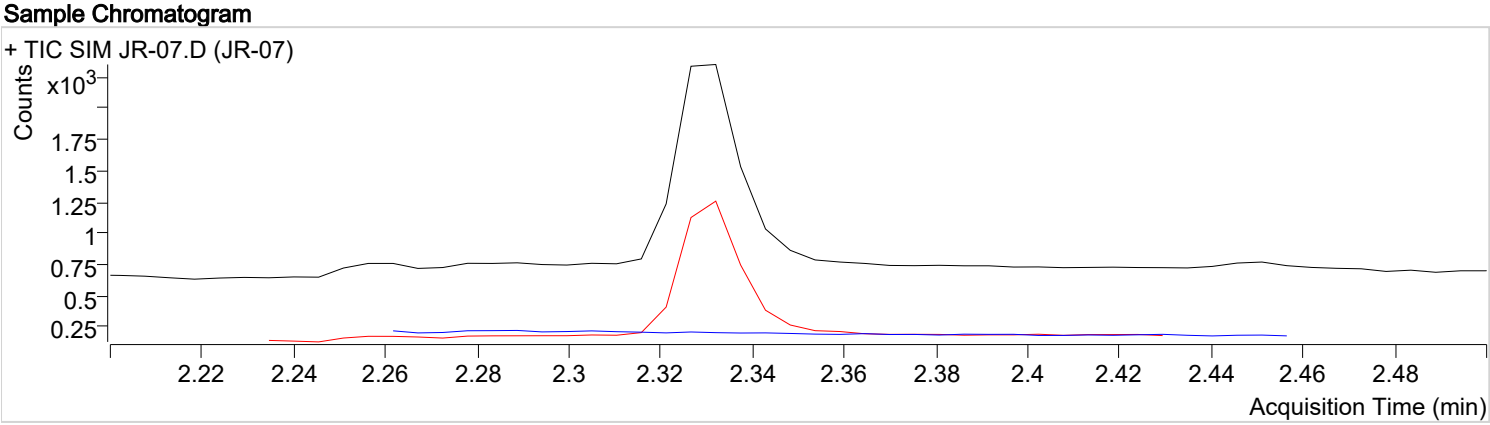

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.289	0	1655	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오후 1:17:11	**Data File**	JR-08.D
Type	Sample	**Name**	JR-08
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

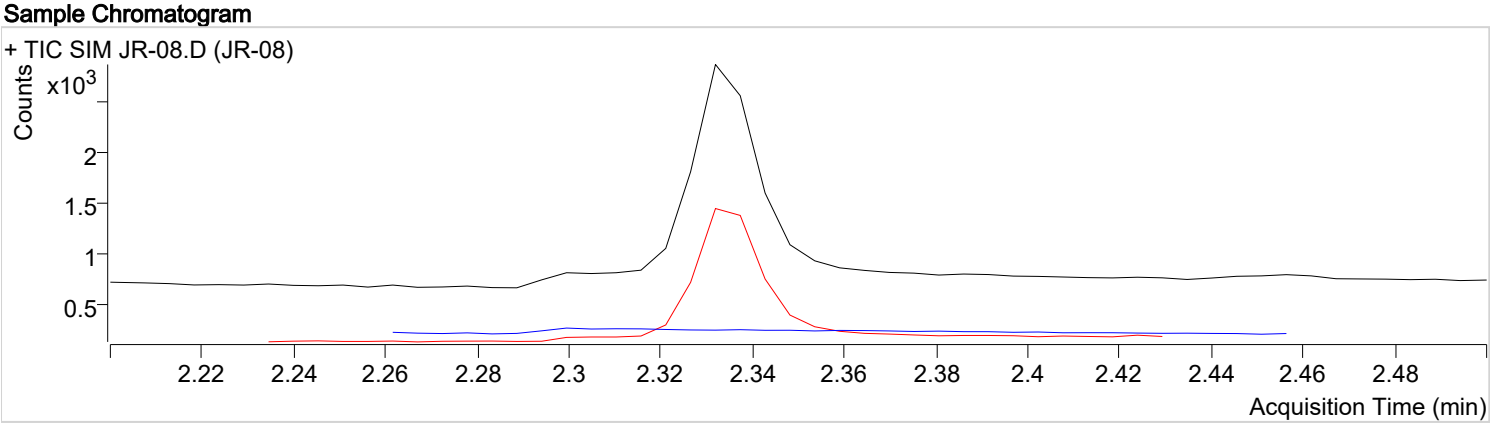

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.299	0	2278	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오후 1:26:15	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

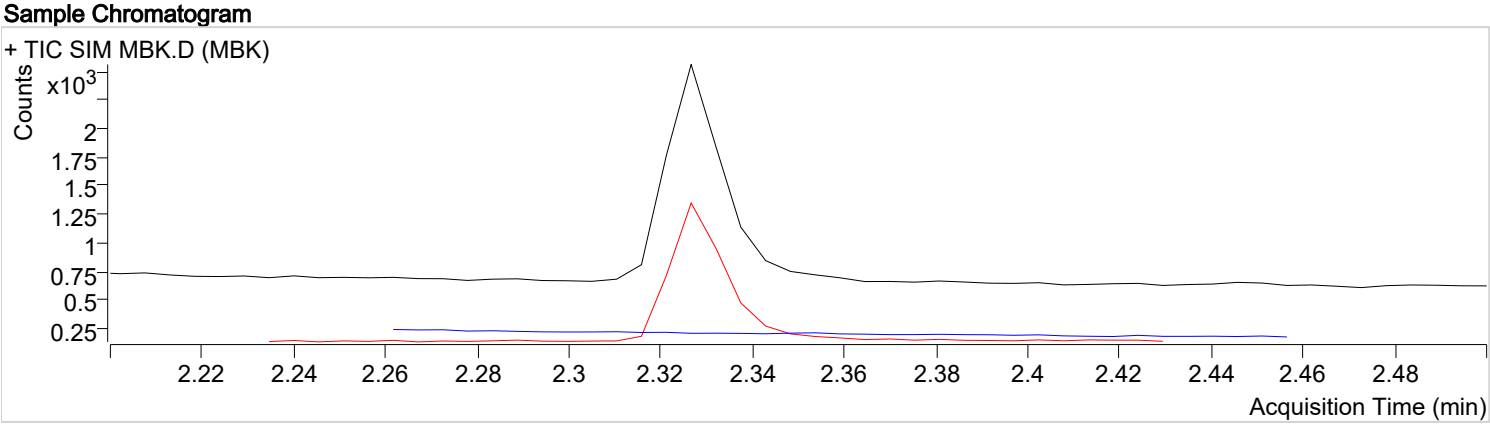

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1681	ND mg/L

1,4-Dioxane







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(KD 2.4, JR 2.5)\QuantResults\1,4.batch.bin		
Analysis Time	2026-02-06 오후 3:56:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:49:57	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-06 오후 3:56:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-06 오후 1:44:35	**Data File**	-C-C-V-.D
Type	QC	**Name**	-C-C-V-
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

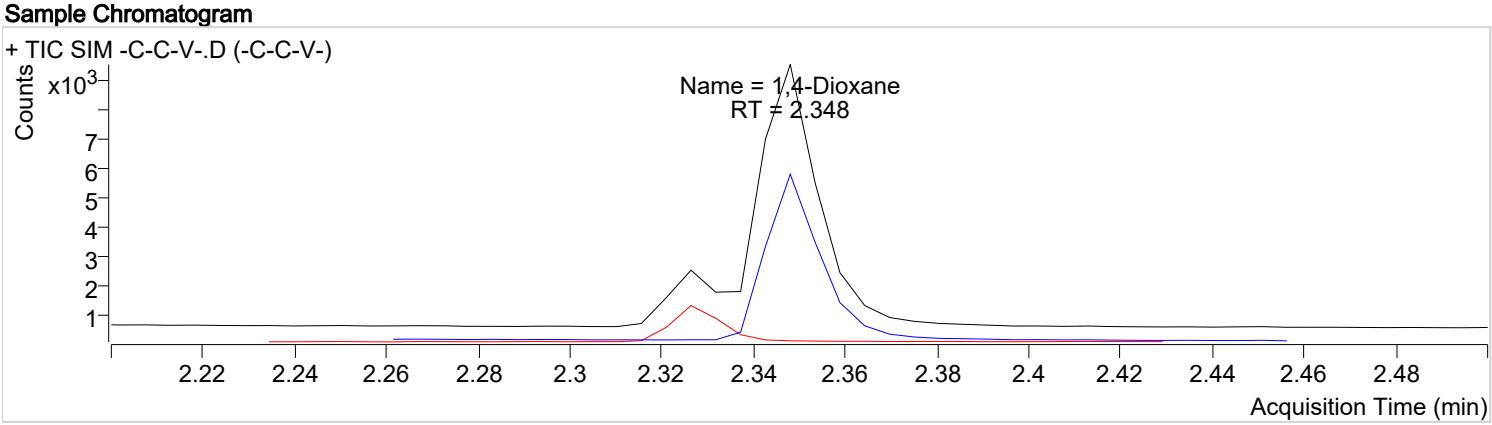

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.348	7752	1489	0.103 mg/L

1,4-Dioxane