Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin				
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

1,4-Dioxane

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
1,4 ST-01.D	Cal	2.359	2053	5110	0.009
1,4 ST-02.D	Cal	2.364	3956	5327	0.018
1,4 ST-03.D	Cal	2.359	10589	5269	0.050
1,4 ST-04.D	Cal	2.353	17795	5386	0.083
1,4 ST-05.D	Cal	2.359	23106	5719	0.102
1,4 ST-06.D	Cal	2.354	34501	5449	0.160
1,4 ST-07.D	Cal	2.353	42424	5416	0.198
BK-.D	Blank			4881	ND
FBK(HS 26-02-25).D	Blank			5467	ND
FBK(DL 26-02-26).D	Blank			4372	ND
FBK(LT 26-02-26).D	Blank			5251	ND
FBK(PL 26-02-27).D	Blank			5805	ND
HS 26-02-25.D	Sample			5621	ND
DL-01.D	Sample			4746	ND
LT-01.D	Sample	2.364	0	4760	ND
LT-02.D	Sample	2.364	0	4732	ND
LT-03.D	Sample	2.359	0	3747	ND
PL-01.D	Sample			4209	ND
PL-02.D	Sample			5464	ND
MBK.D	Blank			5300	ND
-CCV-.D	QC	2.359	22133	5555	0.100

1,4-Dioxane

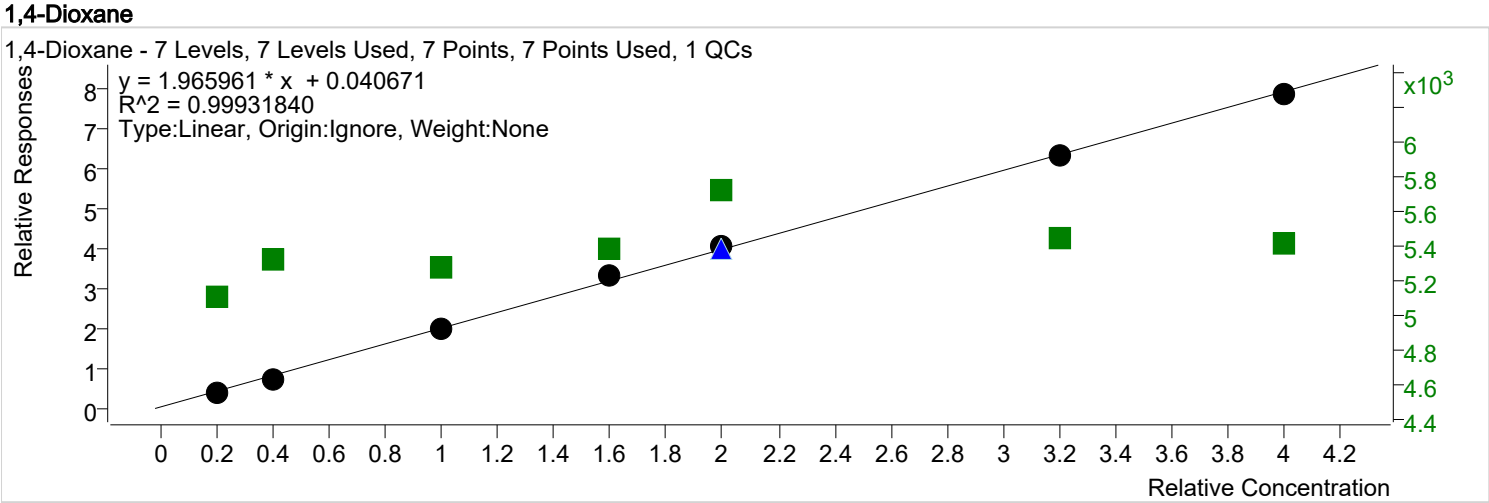

Cal. Path	Type	Level	Enable	Conc.	Response
\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\1,4 ST-01.D	Calibration	1	x	0.200	2053
\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\1,4 ST-02.D	Calibration	2	x	0.400	3956
\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\1,4 ST-03.D	Calibration	3	x	1.000	10589
\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\1,4 ST-04.D	Calibration	4	x	1.600	17795
\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\1,4 ST-05.D	Calibration	5	x	2.000	23106
\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\-CCV-.D	QC	5	x	2.000	22133
\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\1,4 ST-06.D	Calibration	6	x	3.200	34501
\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\1,4 ST-07.D	Calibration	7	x	4.000	42424

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 2:21:41	**Data File**	1,4 ST-01.D
Type	Cal	**Name**	1,4 ST-01
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

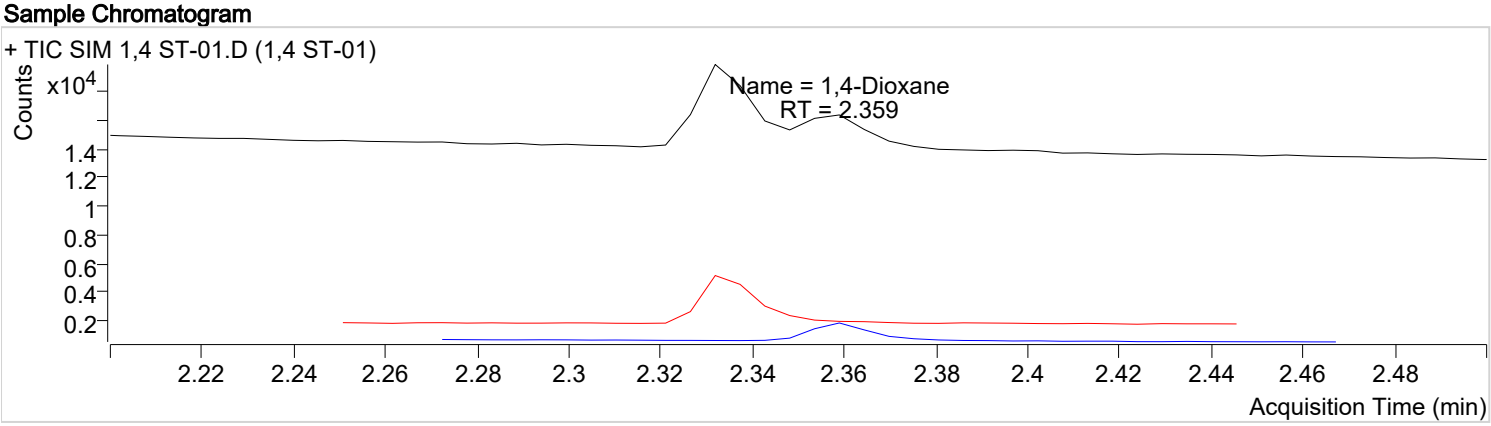

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.359	2053	5110	0.009 mg/L

1,4-Dioxane

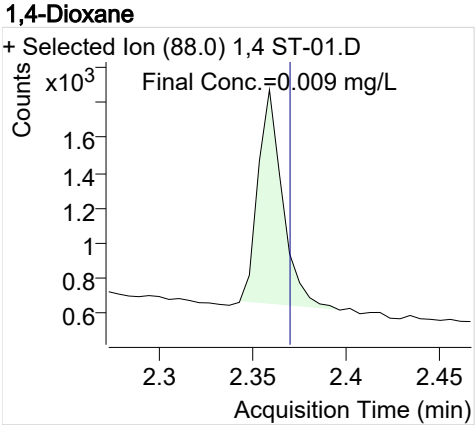

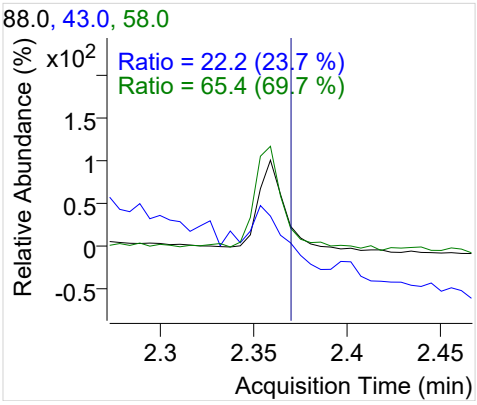

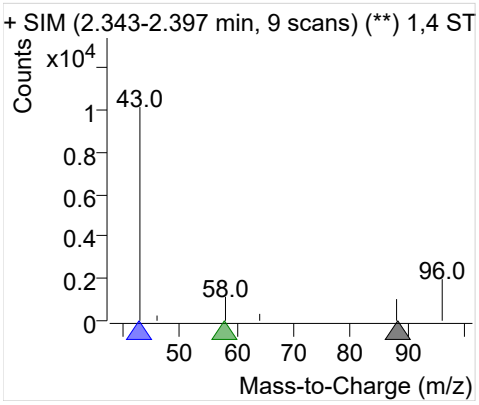

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 2:30:48	**Data File**	1,4 ST-02.D
Type	Cal	**Name**	1,4 ST-02
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

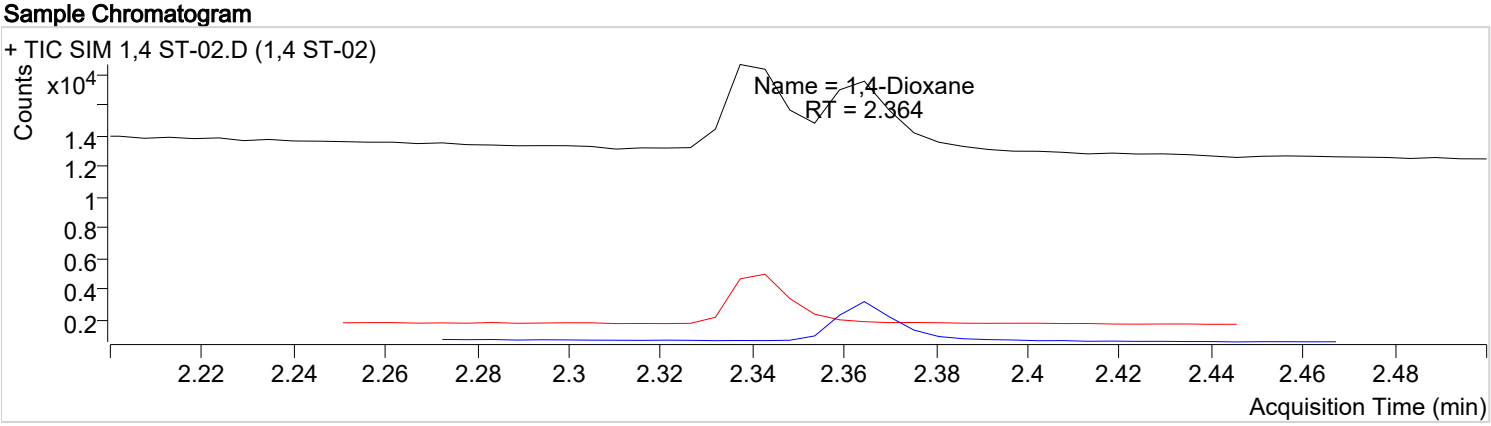

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.364	3956	5327	0.018 mg/L

1,4-Dioxane

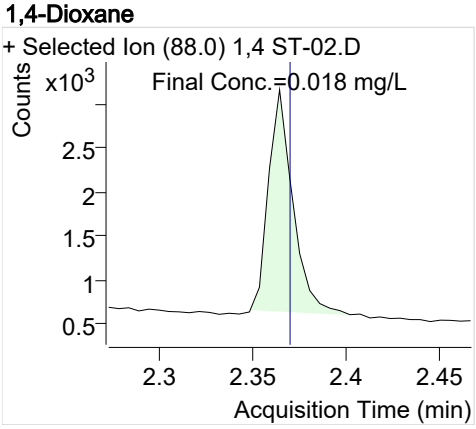

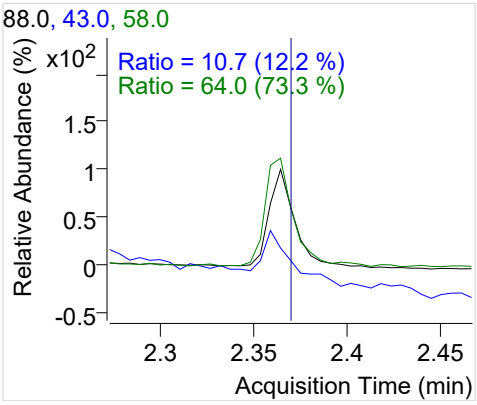

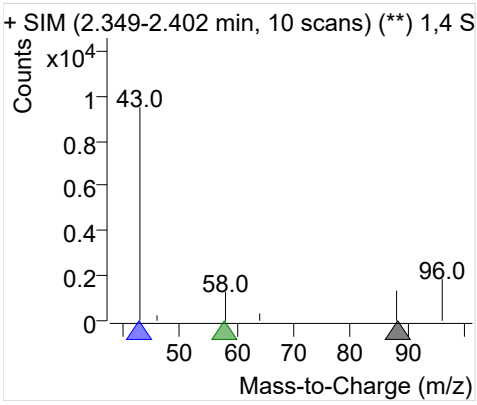

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 2:39:50	**Data File**	1,4 ST-03.D
Type	Cal	**Name**	1,4 ST-03
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

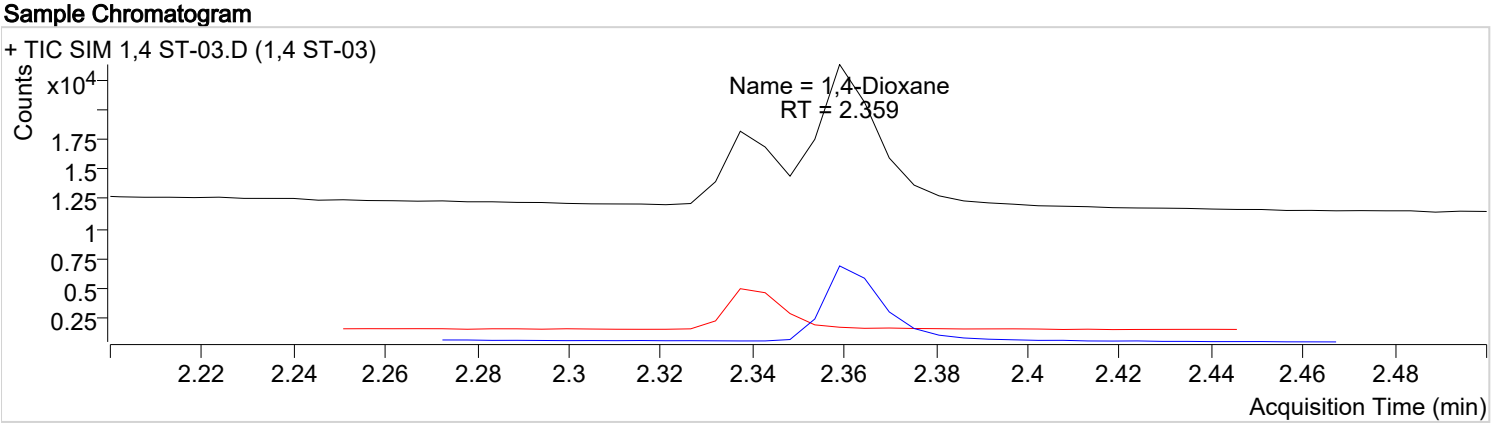

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.359	10589	5269	0.050 mg/L

1,4-Dioxane





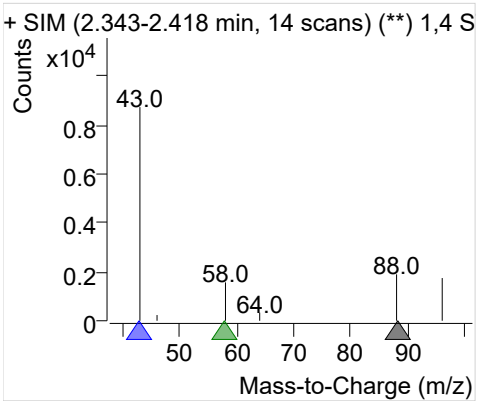

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 2:48:55	**Data File**	1,4 ST-04.D
Type	Cal	**Name**	1,4 ST-04
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

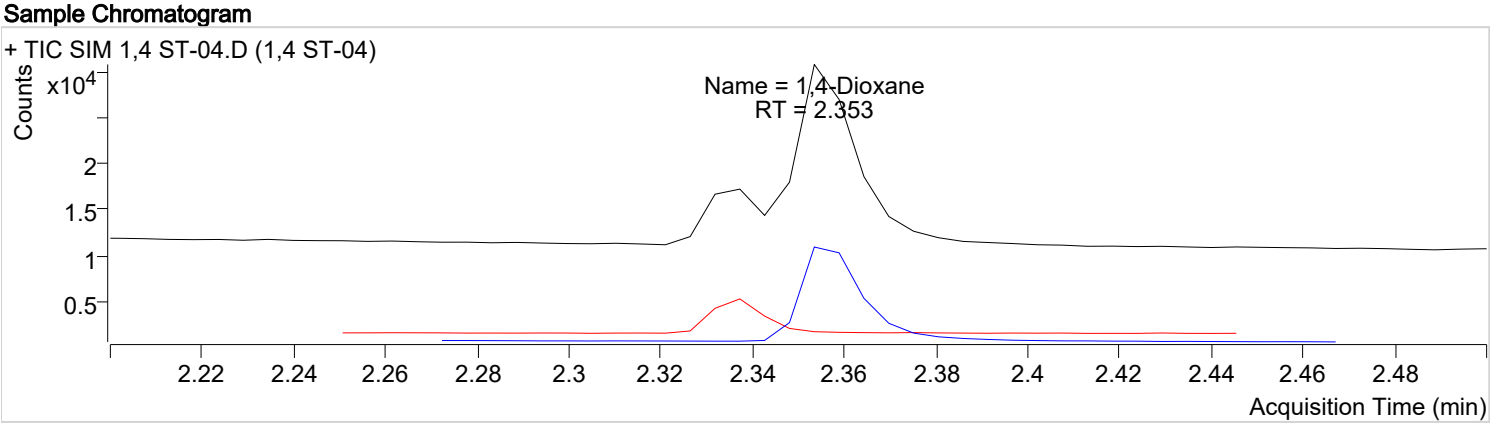

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.353	17795	5386	0.083 mg/L

1,4-Dioxane





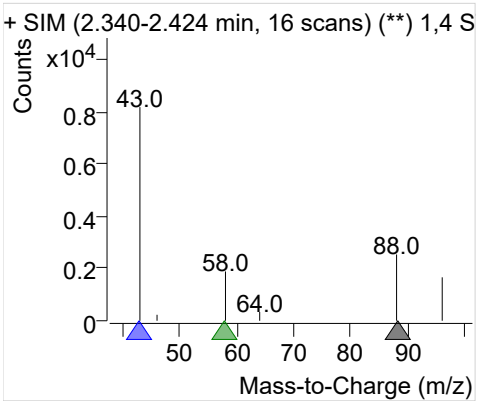

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 2:58:01	**Data File**	1,4 ST-05.D
Type	Cal	**Name**	1,4 ST-05
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

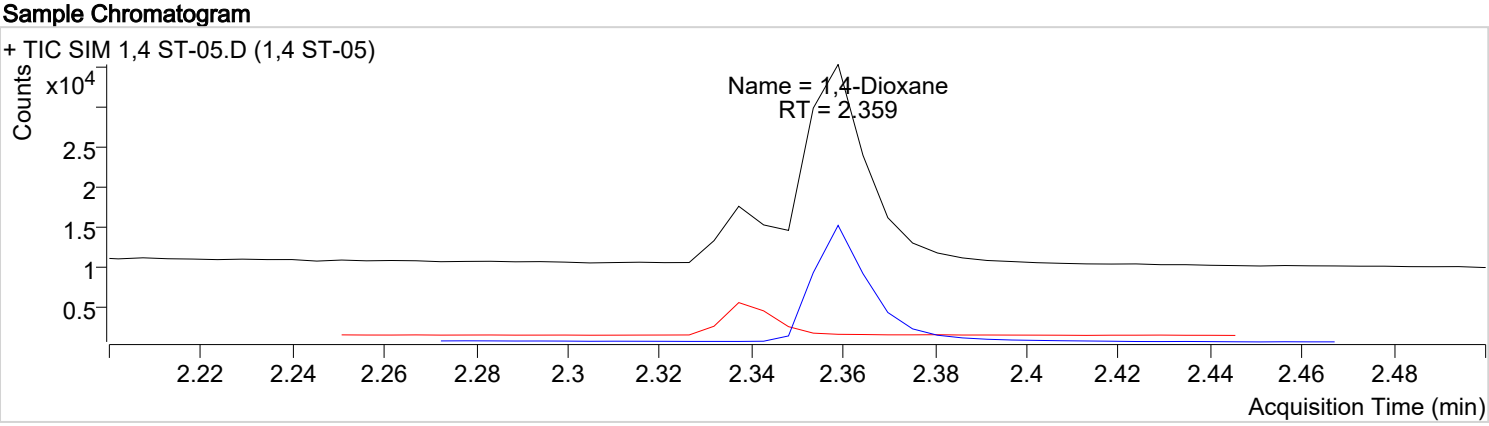

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.359	23106	5719	0.102 mg/L

1,4-Dioxane





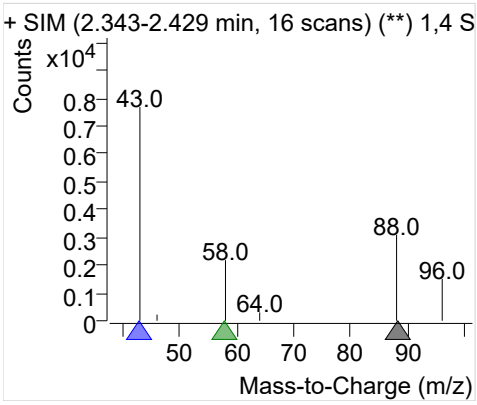

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 3:07:06	**Data File**	1,4 ST-06.D
Type	Cal	**Name**	1,4 ST-06
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

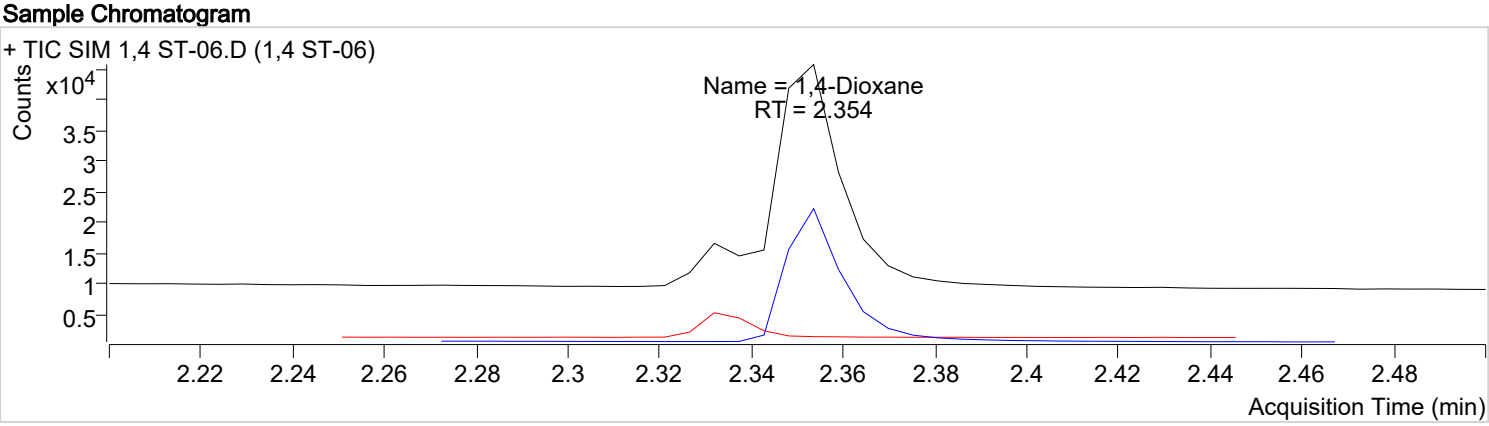

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.354	34501	5449	0.160 mg/L

1,4-Dioxane





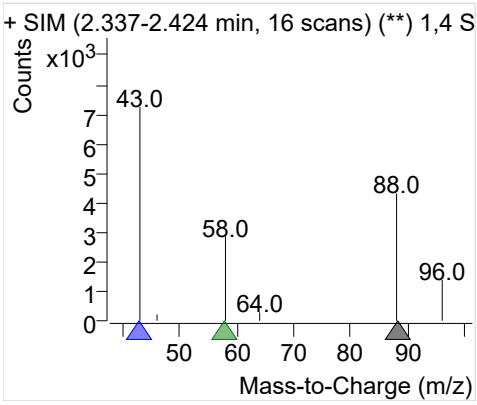

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 3:16:08	**Data File**	1,4 ST-07.D
Type	Cal	**Name**	1,4 ST-07
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

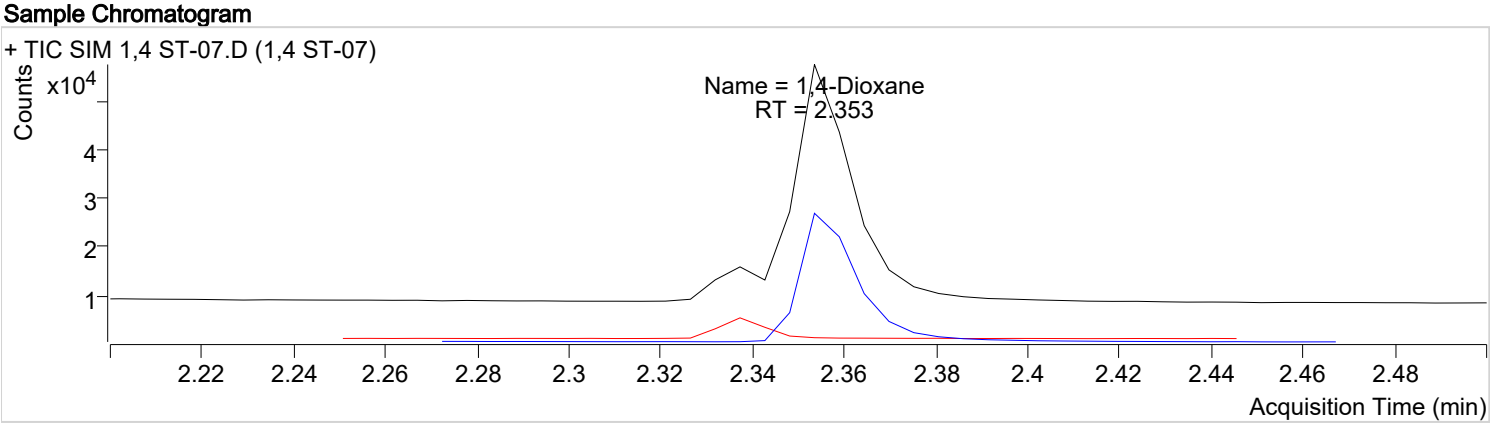

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.353	42424	5416	0.198 mg/L

1,4-Dioxane





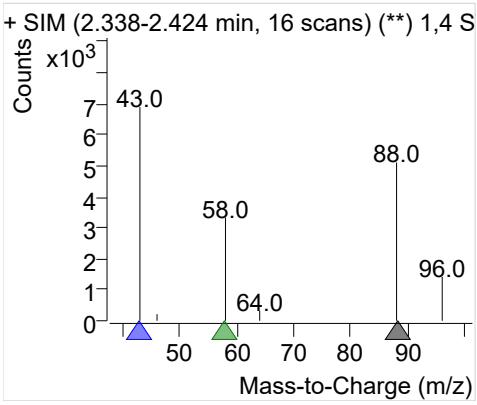

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 3:34:22	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

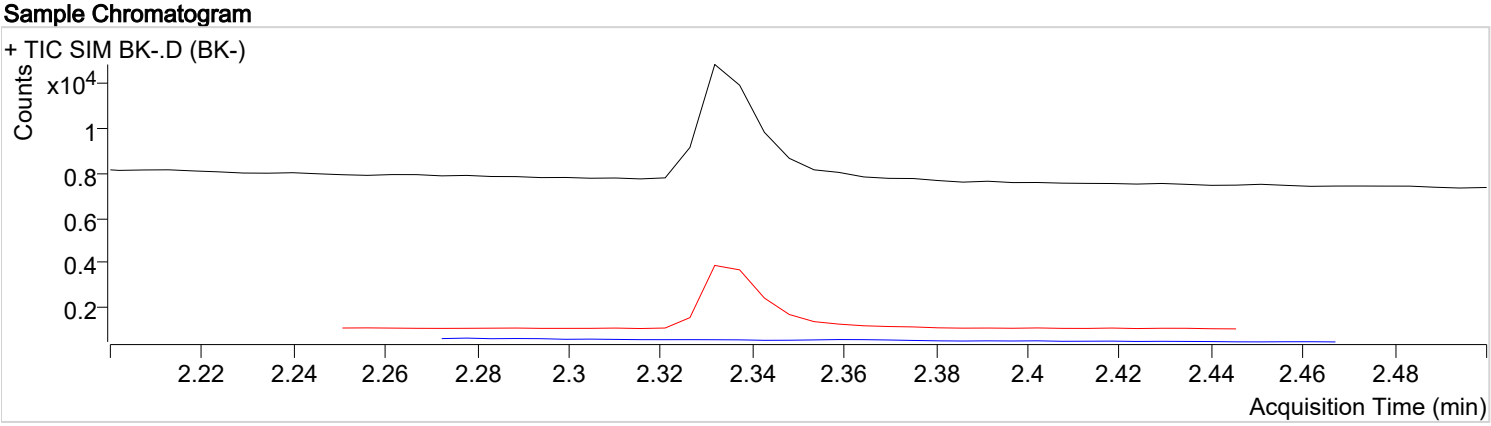

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			4881	ND mg/L

1,4-Dioxane





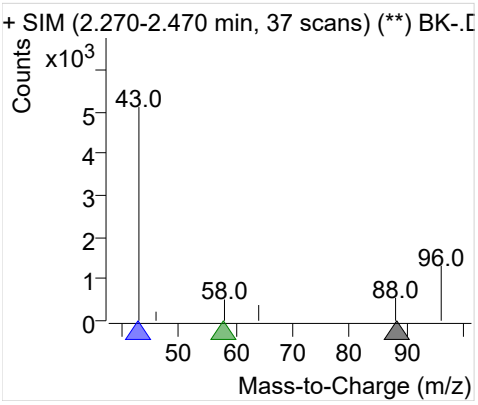

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 3:43:31	**Data File**	FBK(HS 26-02-25).D
Type	Blank	**Name**	FBK(HS 26-02-25)
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

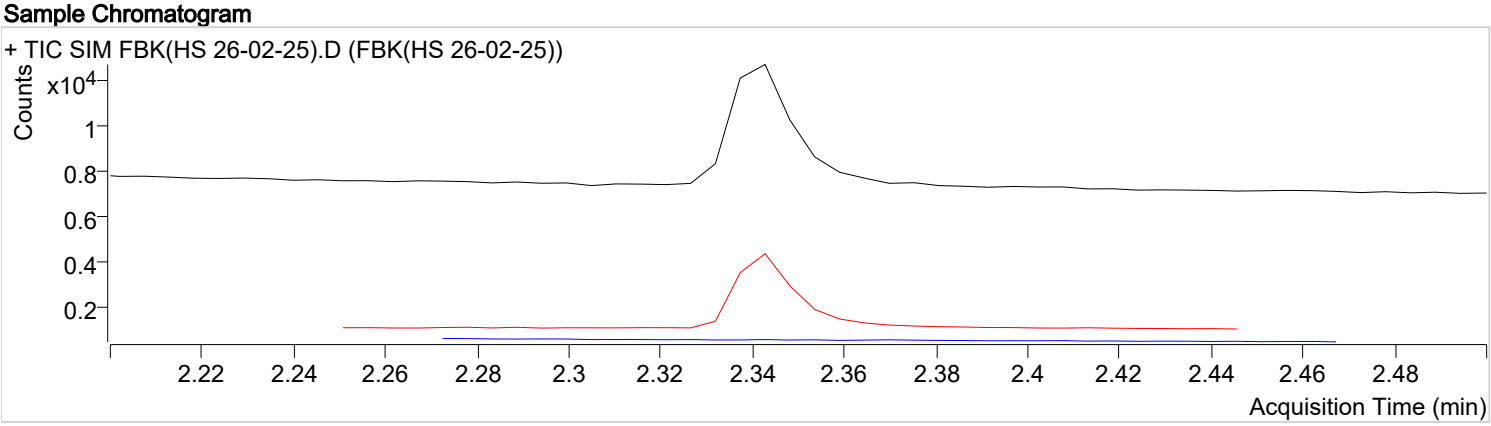

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			5467	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 3:52:33	**Data File**	FBK(DL 26-02-26).D
Type	Blank	**Name**	FBK(DL 26-02-26)
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

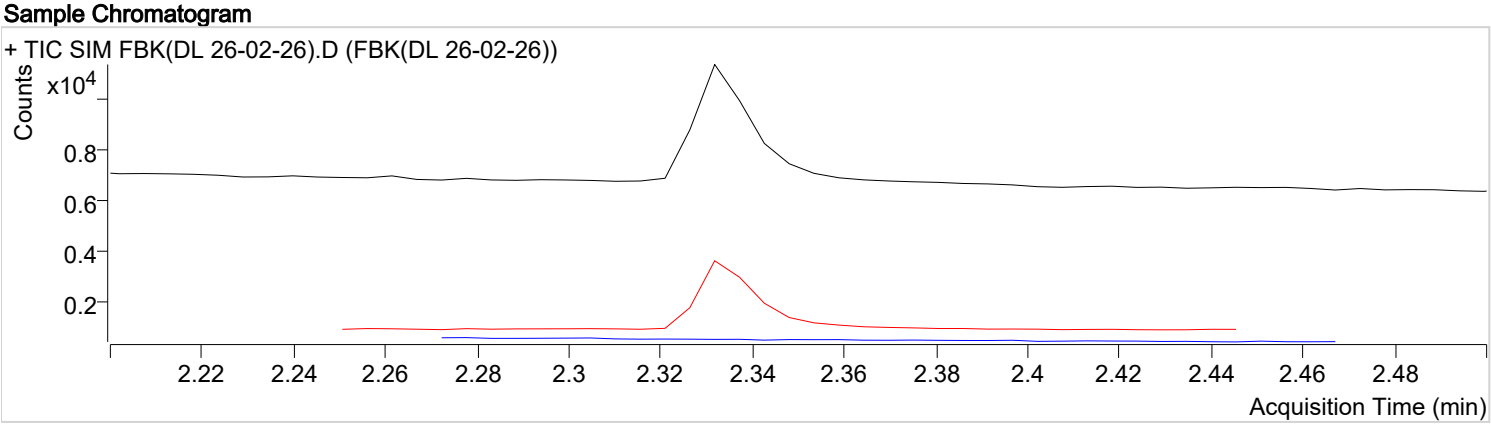

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			4372	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 4:01:38	**Data File**	FBK(LT 26-02-26).D
Type	Blank	**Name**	FBK(LT 26-02-26)
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

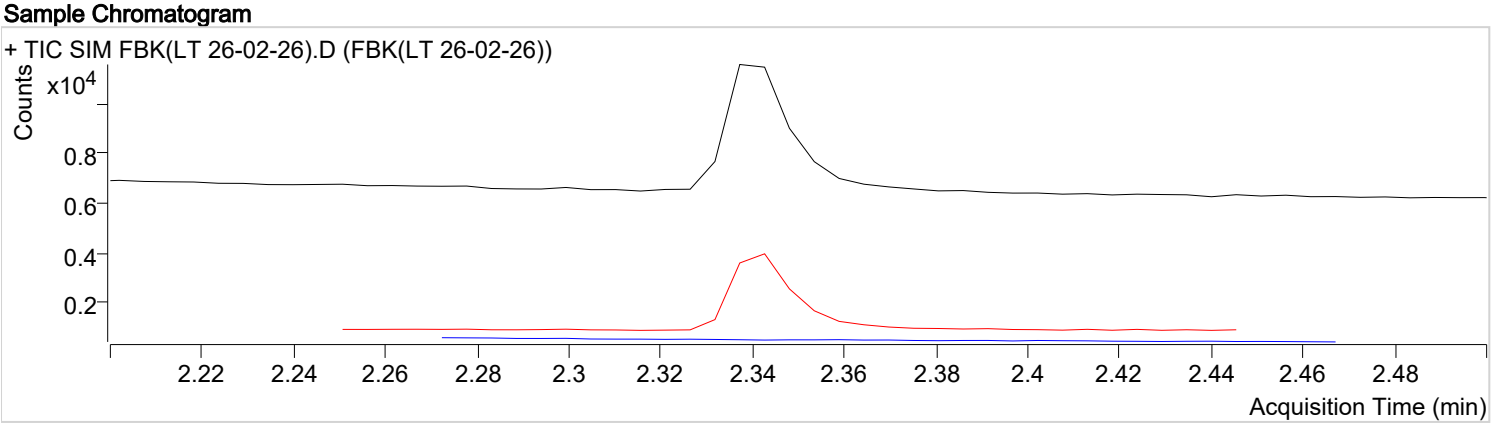

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			5251	ND mg/L

1,4-Dioxane

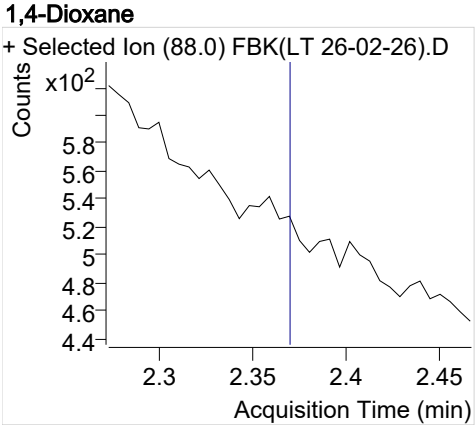



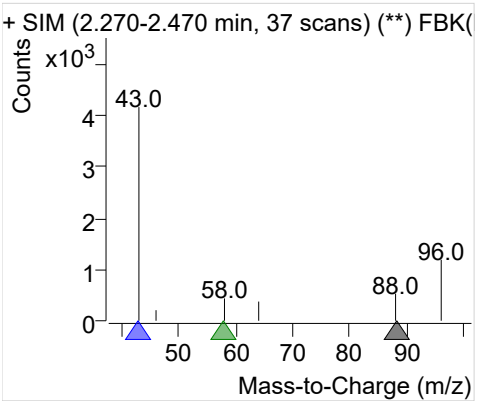

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 4:10:41	**Data File**	FBK(PL 26-02-27).D
Type	Blank	**Name**	FBK(PL 26-02-27)
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

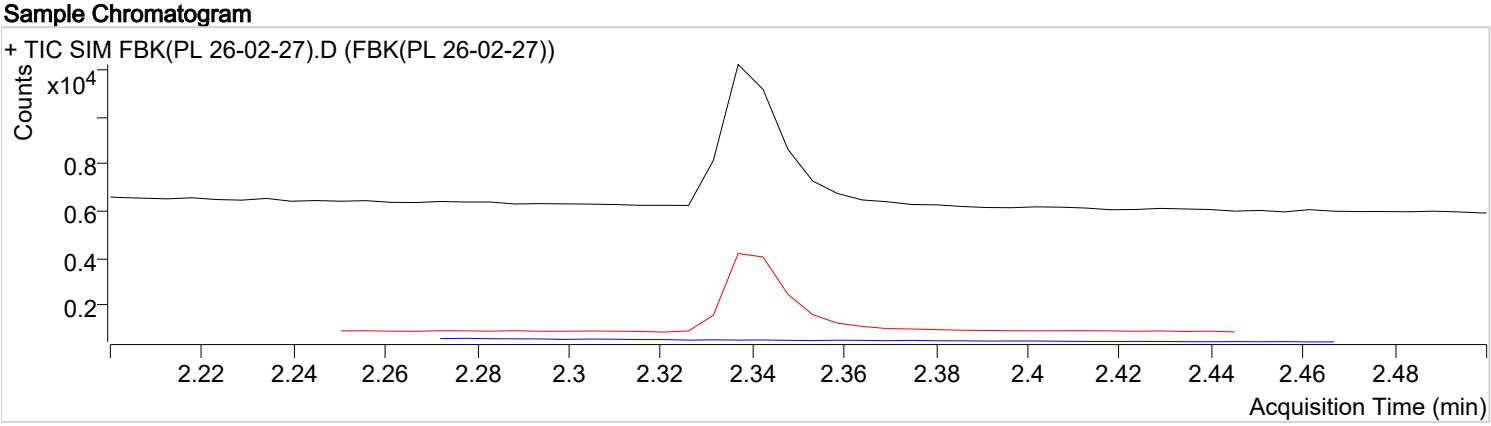

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			5805	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 4:19:48	**Data File**	HS 26-02-25.D
Type	Sample	**Name**	HS 26-02-25
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

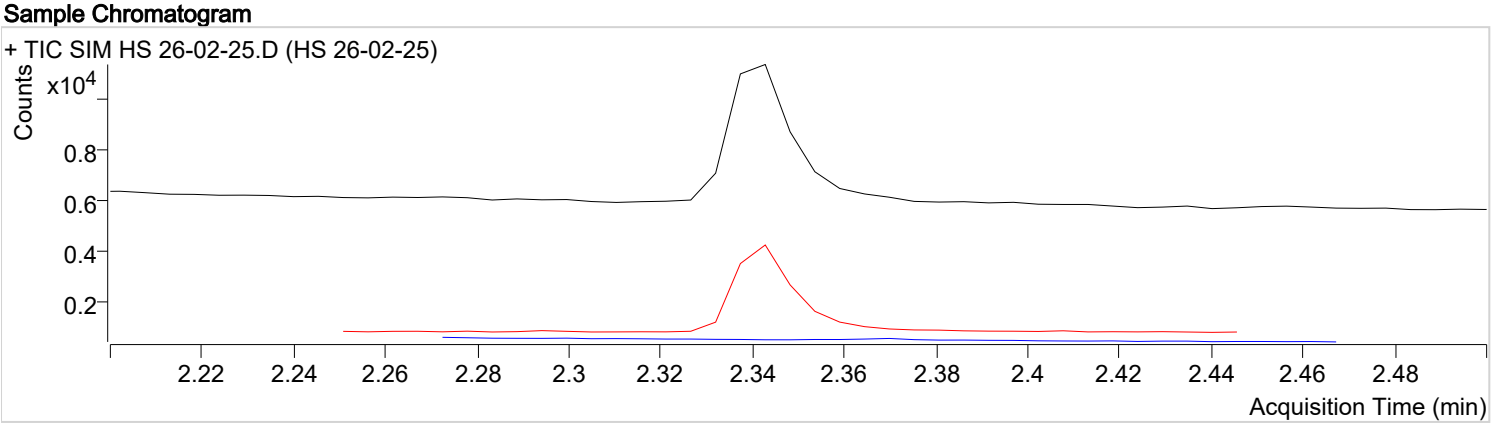

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			5621	ND mg/L

1,4-Dioxane





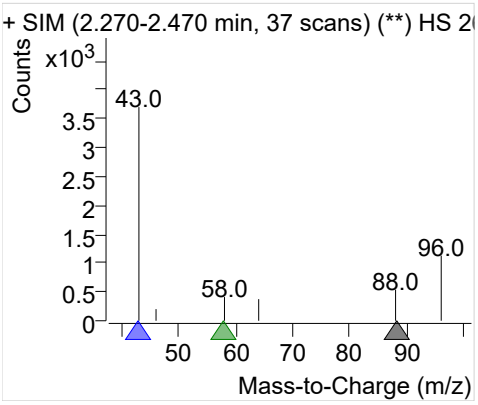

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 4:28:53	**Data File**	DL-01.D
Type	Sample	**Name**	DL-01
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

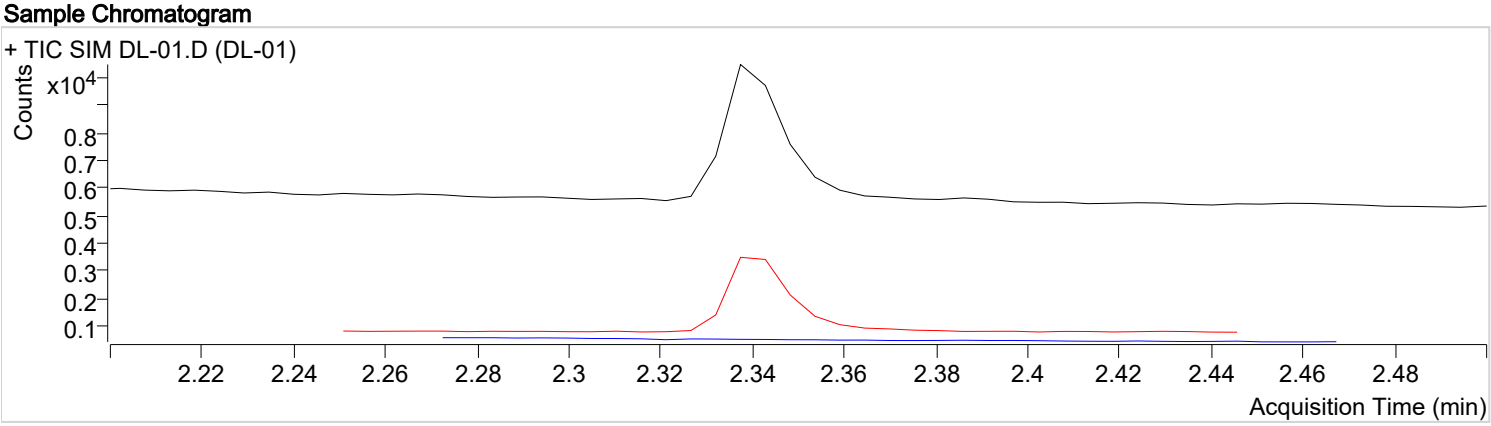

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			4746	ND mg/L

1,4-Dioxane





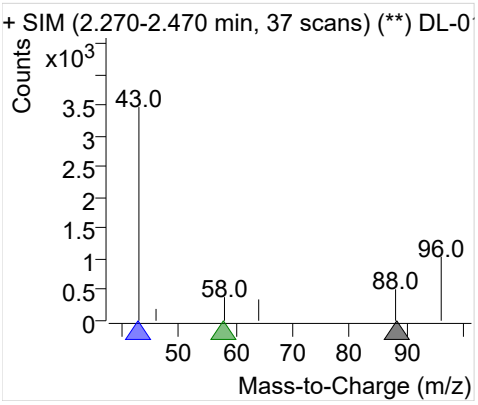

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 4:37:54	**Data File**	LT-01.D
Type	Sample	**Name**	LT-01
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

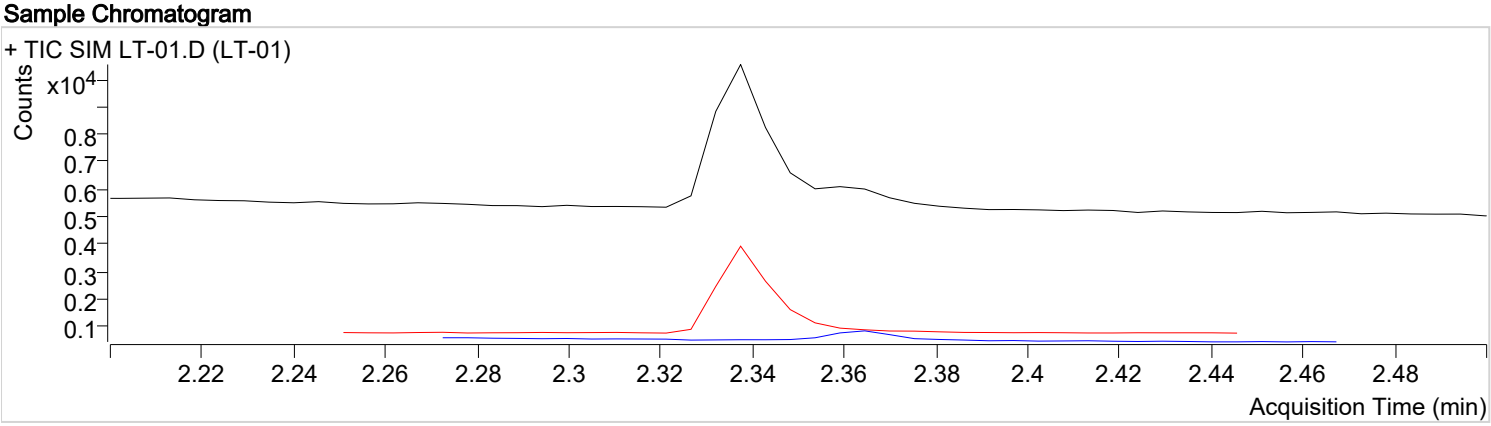

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.364	0	4760	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 4:46:58	**Data File**	LT-02.D
Type	Sample	**Name**	LT-02
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

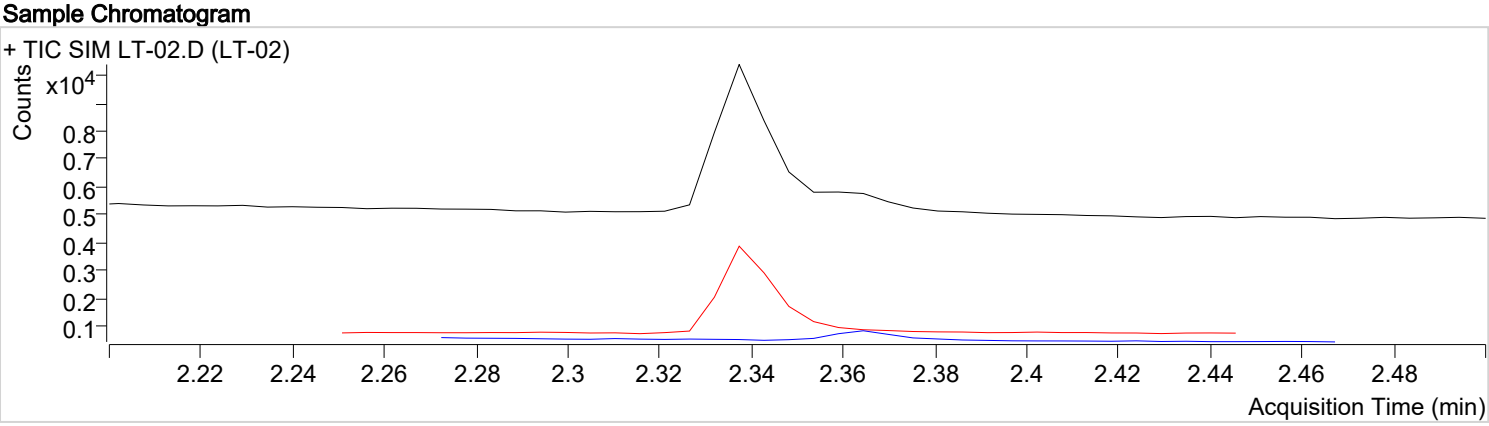

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.364	0	4732	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 4:56:05	**Data File**	LT-03.D
Type	Sample	**Name**	LT-03
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

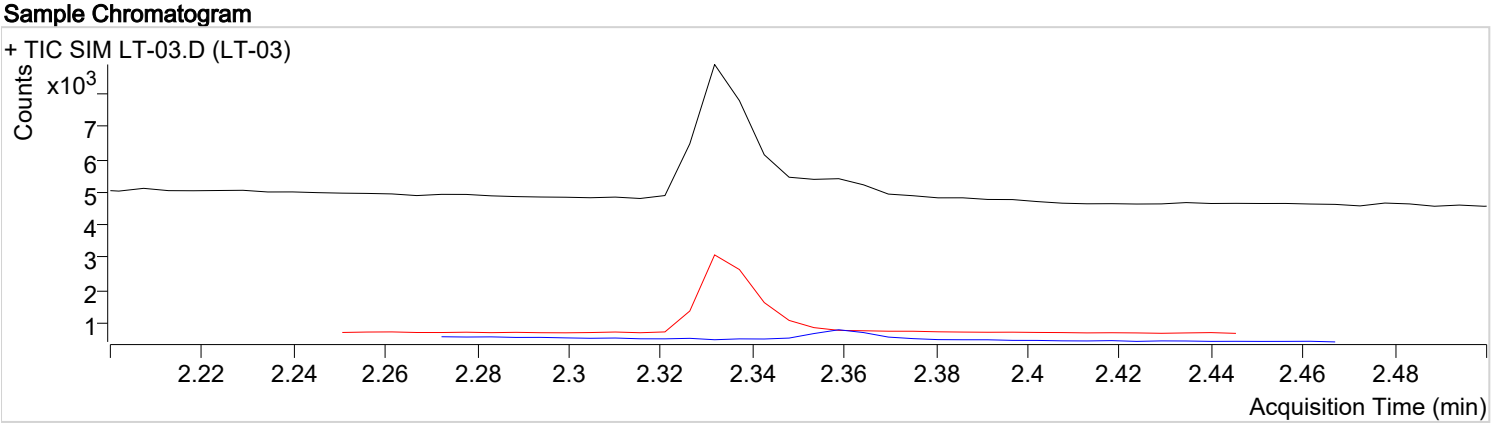

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.359	0	3747	ND mg/L

1,4-Dioxane







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 5:05:08	**Data File**	PL-01.D
Type	Sample	**Name**	PL-01
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

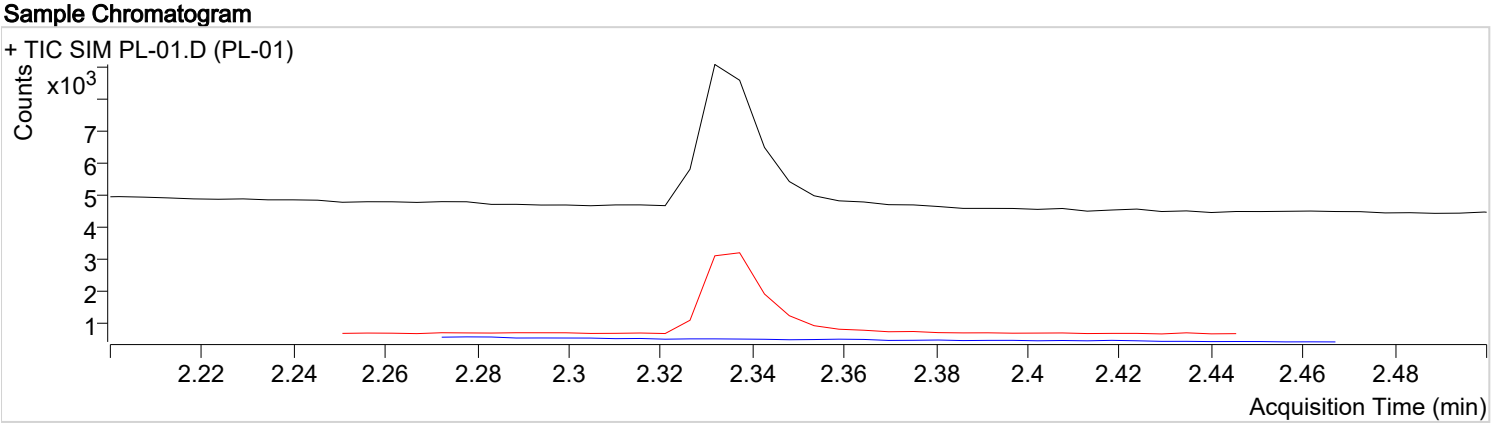

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			4209	ND mg/L

1,4-Dioxane





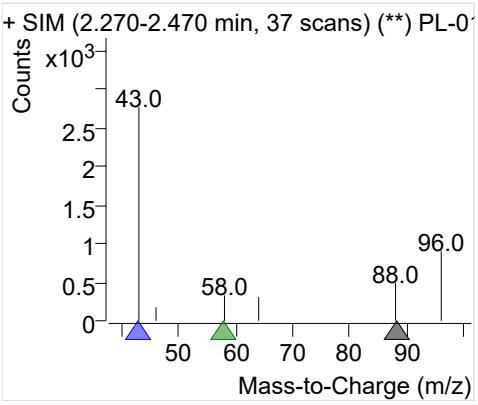

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 5:14:14	**Data File**	PL-02.D
Type	Sample	**Name**	PL-02
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

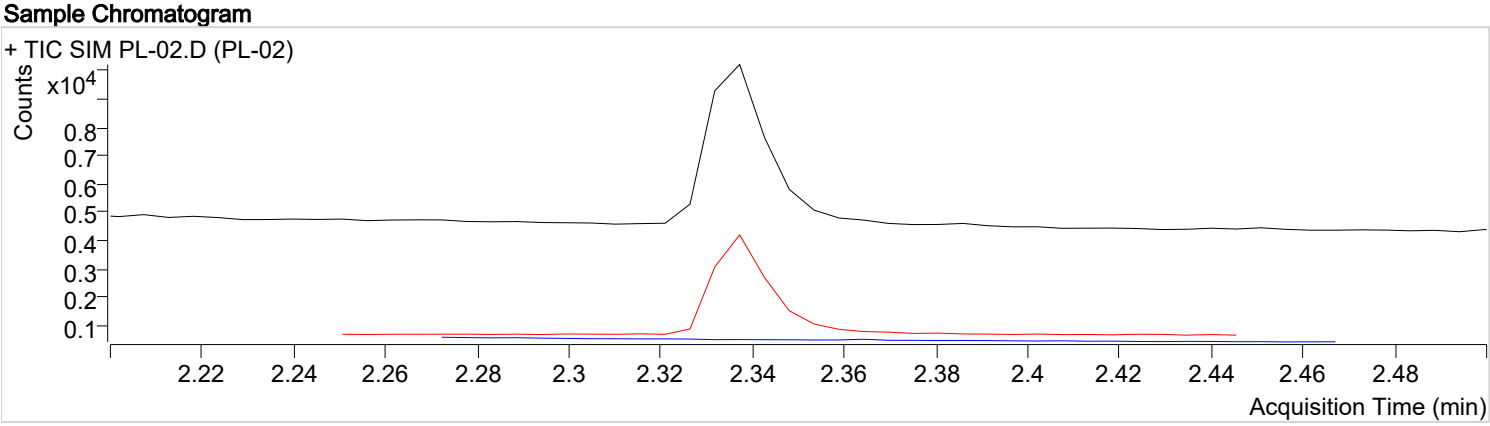

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			5464	ND mg/L

1,4-Dioxane





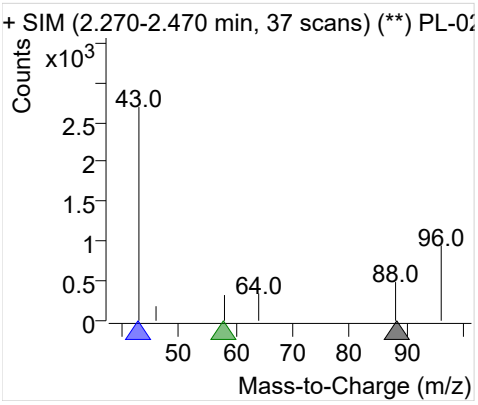

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 5:23:17	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

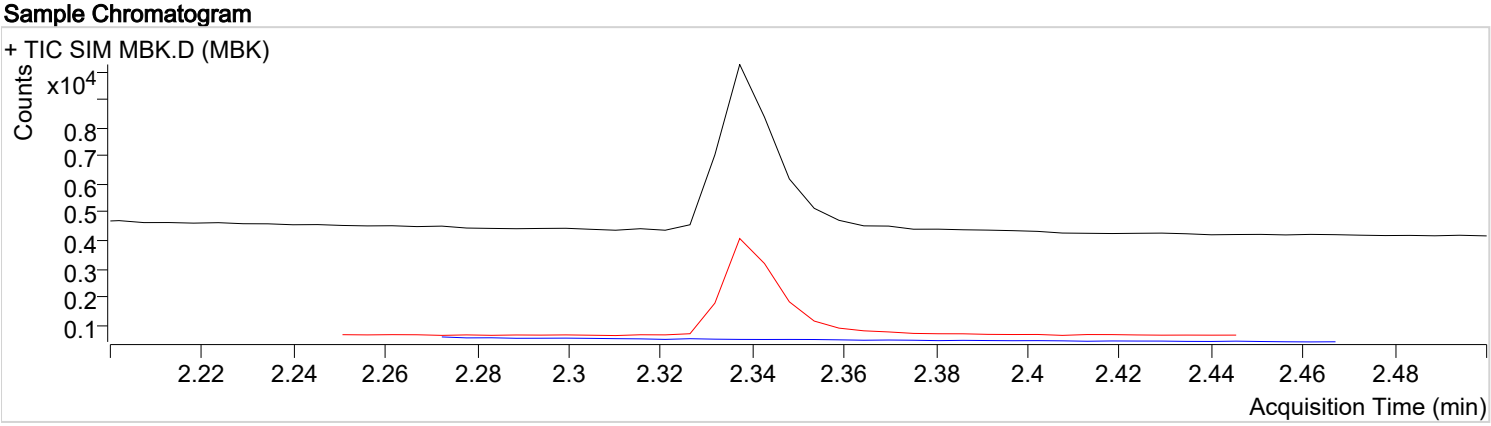

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			5300	ND mg/L

1,4-Dioxane





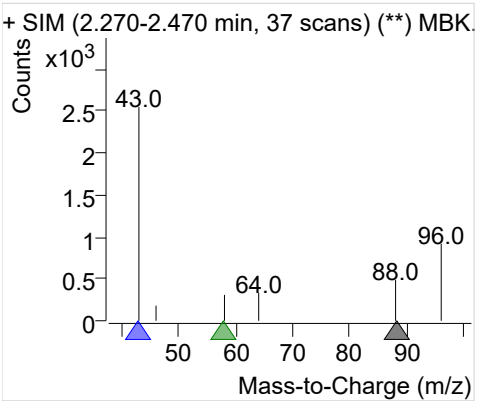

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\1,4(HS 2.25 DL 2.26 LT 2.26 PL 2.27)\QuantResults\1.4.batch.bin		
Analysis Time	2026-02-28 오전 9:52:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 9:48:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:52:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 5:41:31	**Data File**	-CCV-.D
Type	QC	**Name**	-CCV-
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

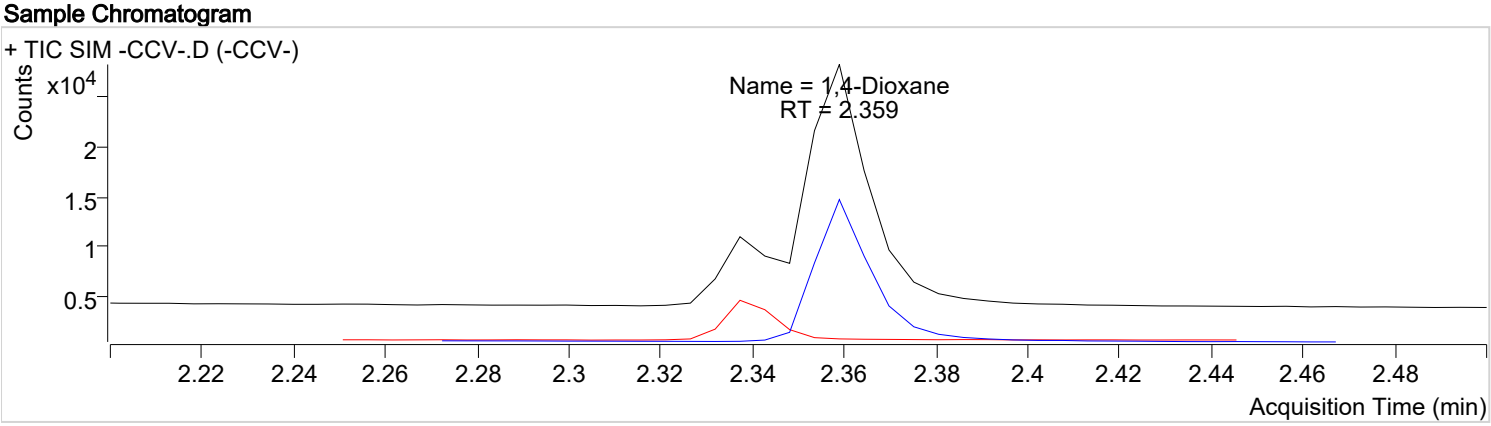

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.359	22133	5555	0.100 mg/L
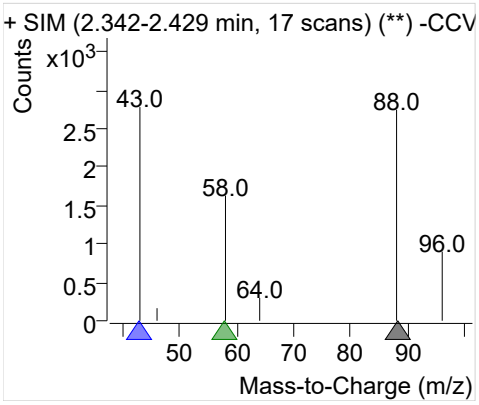
1,4-Dioxane