Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin				
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

1,4-Dioxane

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
1,4 ST-01.D	Cal	2.354	1837	4437	0.009
1,4 ST-02.D	Cal	2.353	3561	4408	0.019
1,4 ST-03.D	Cal	2.353	9211	4547	0.050
1,4 ST-04.D	Cal	2.348	13169	3978	0.082
1,4 ST-05.D	Cal	2.354	18999	4608	0.103
1,4 ST-06.D	Cal	2.348	25677	4078	0.158
1,4 ST-07.D	Cal	2.353	35109	4449	0.199
BK-.D	Blank			4766	ND
FBK(RE 26-03-04).D	Blank			4643	ND
FBK(KD 26-03-04).D	Blank			4911	ND
RE-01.D	Sample	2.354	0	3525	ND
RE-02.D	Sample	2.364	0	4614	ND
RE-03.D	Sample	2.353	0	3967	ND
RE-04.D	Sample	2.353	0	3923	ND
RE-09.D	Sample	2.364	0	4112	ND
RE-10.D	Sample			3946	ND
RE-11.D	Sample	2.370	0	4820	ND
RE-12.D	Sample			4305	ND
KD-01.D	Sample	2.359	0	4440	ND
KD-02.D	Sample			4428	ND
KD-03.D	Sample			3995	ND
MBK.D	Blank			4078	ND
-C-C-V-.D	QC	2.348	14949	3735	0.100

1,4-Dioxane

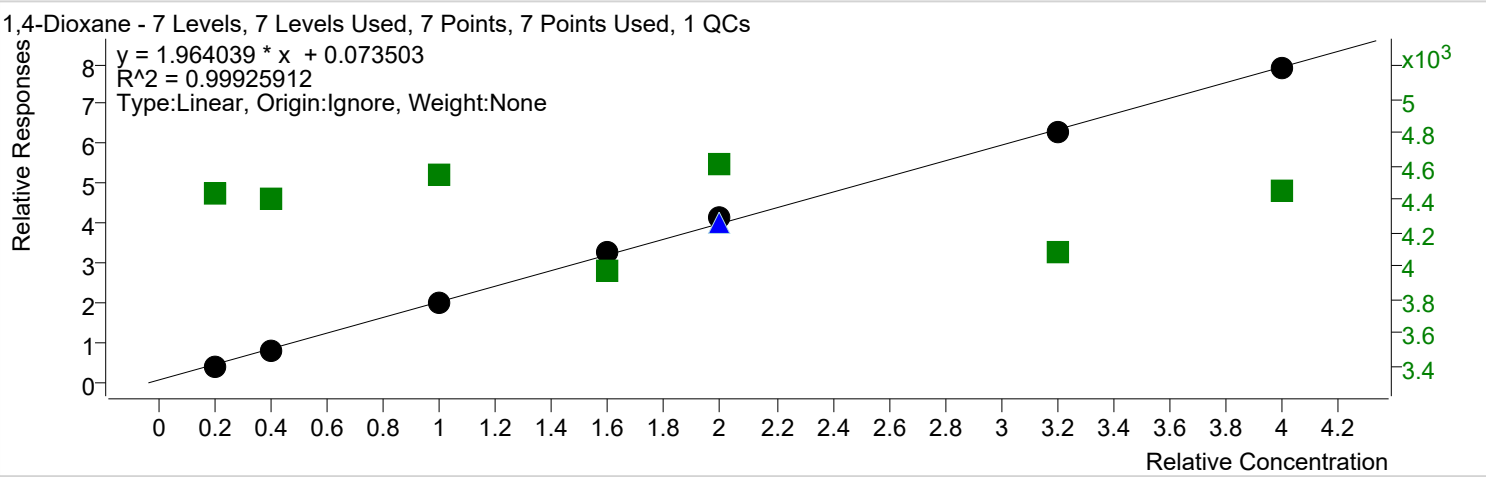

Cal. Path	Type	Level	Enable	Conc.	Response
\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\1,4 ST-01.D	Calibration	1	x	0.200	1837
\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\1,4 ST-02.D	Calibration	2	x	0.400	3561
\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\1,4 ST-03.D	Calibration	3	x	1.000	9211
\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\1,4 ST-04.D	Calibration	4	x	1.600	13169
\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\1,4 ST-05.D	Calibration	5	x	2.000	18999
\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\-C-C-V-.D	QC	5	x	2.000	14949
\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\1,4 ST-06.D	Calibration	6	x	3.200	25677
\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\1,4 ST-07.D	Calibration	7	x	4.000	35109

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오전 10:17:36	**Data File**	1,4 ST-01.D
Type	Cal	**Name**	1,4 ST-01
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

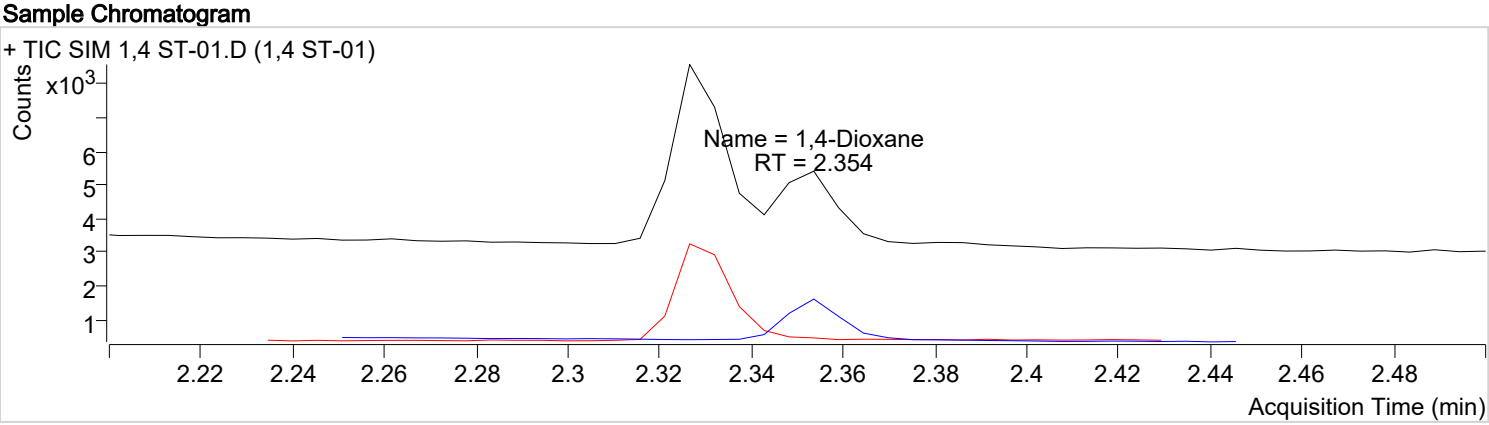

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.354	1837	4437	0.009 mg/L

1,4-Dioxane





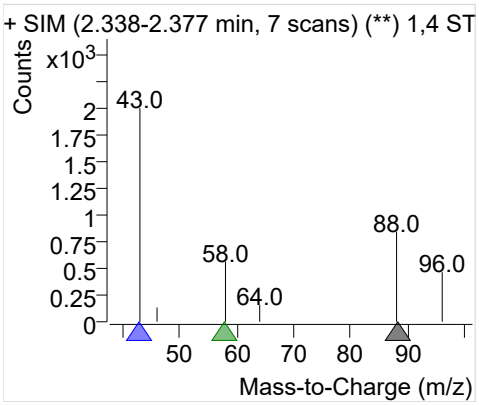

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오전 10:26:28	**Data File**	1,4 ST-02.D
Type	Cal	**Name**	1,4 ST-02
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

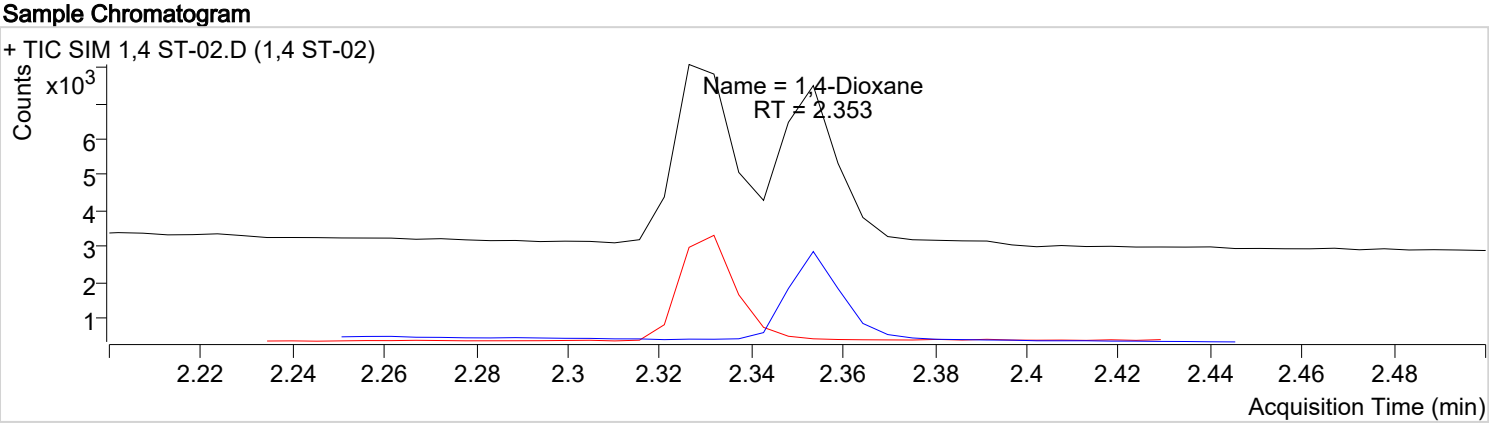

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.353	3561	4408	0.019 mg/L

1,4-Dioxane





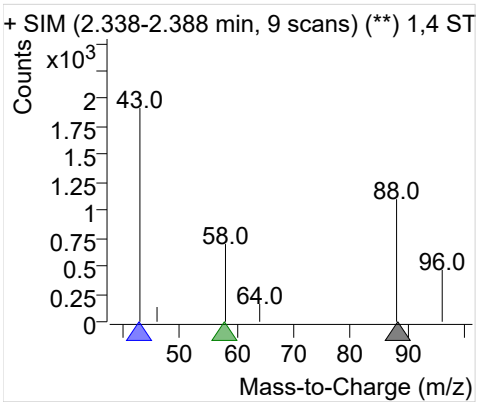

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오전 10:35:18	**Data File**	1,4 ST-03.D
Type	Cal	**Name**	1,4 ST-03
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

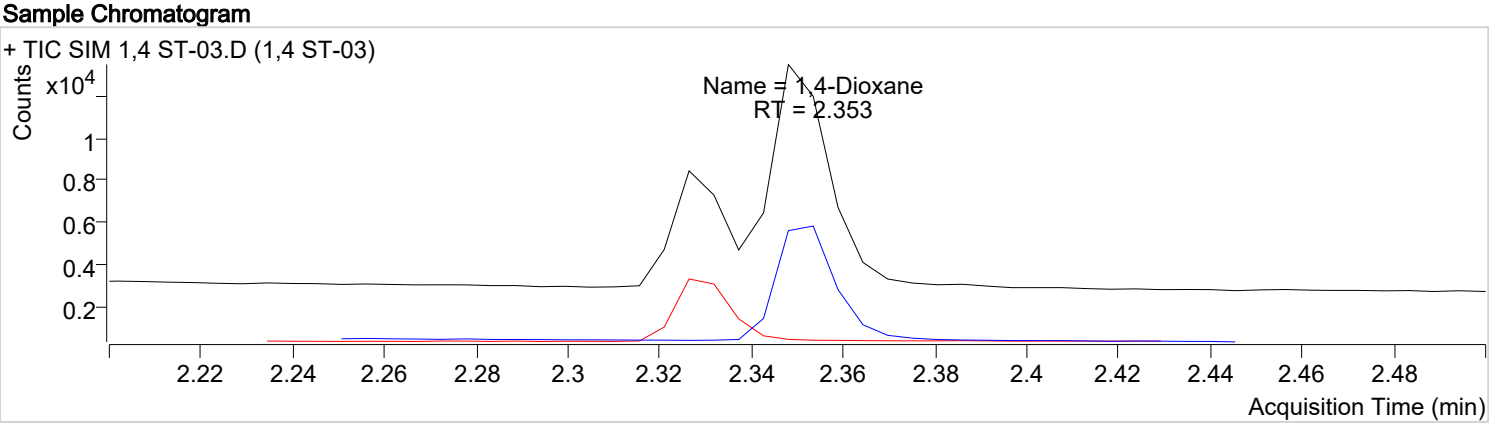

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.353	9211	4547	0.050 mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오전 10:44:12	**Data File**	1,4 ST-04.D
Type	Cal	**Name**	1,4 ST-04
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

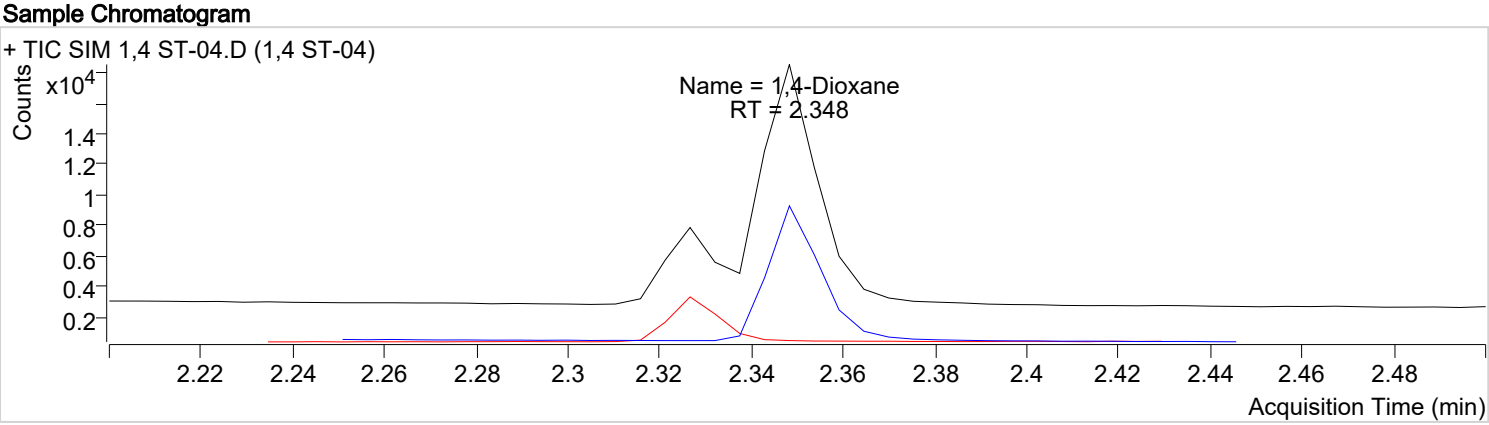

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.348	13169	3978	0.082 mg/L

1,4-Dioxane







Generated at 오전 10:04 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오전 10:53:06	**Data File**	1,4 ST-05.D
Type	Cal	**Name**	1,4 ST-05
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

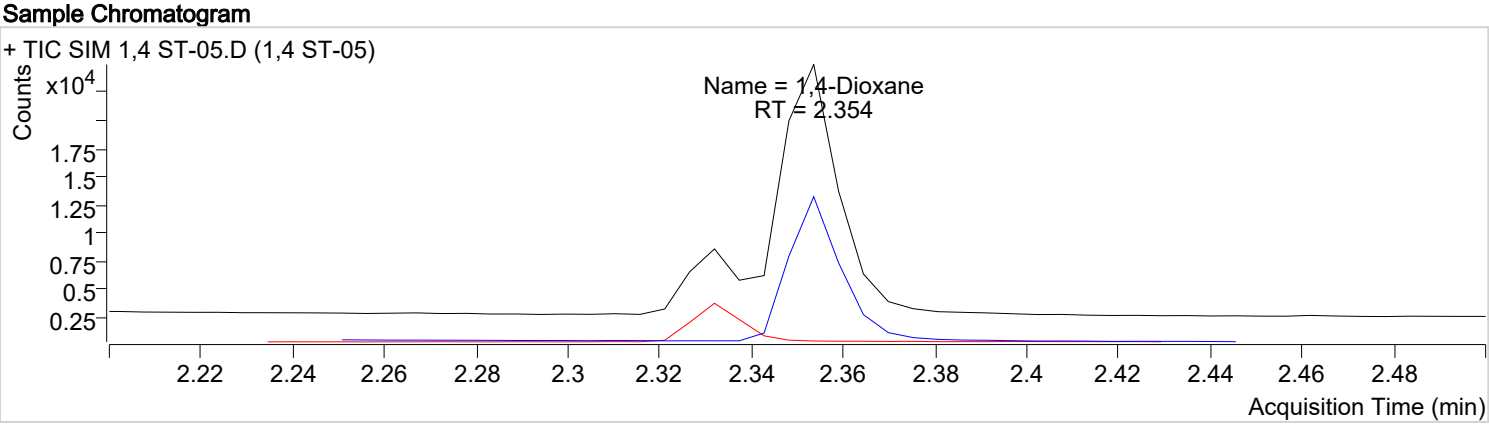

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.354	18999	4608	0.103 mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오전 11:02:02	**Data File**	1,4 ST-06.D
Type	Cal	**Name**	1,4 ST-06
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

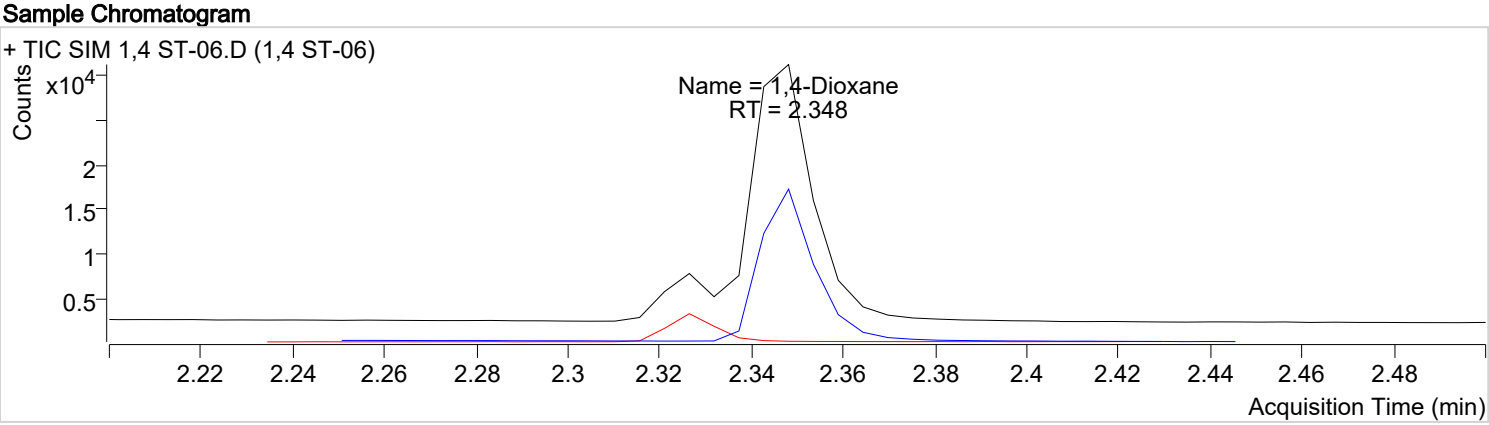

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.348	25677	4078	0.158 mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오전 11:10:57	**Data File**	1,4 ST-07.D
Type	Cal	**Name**	1,4 ST-07
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

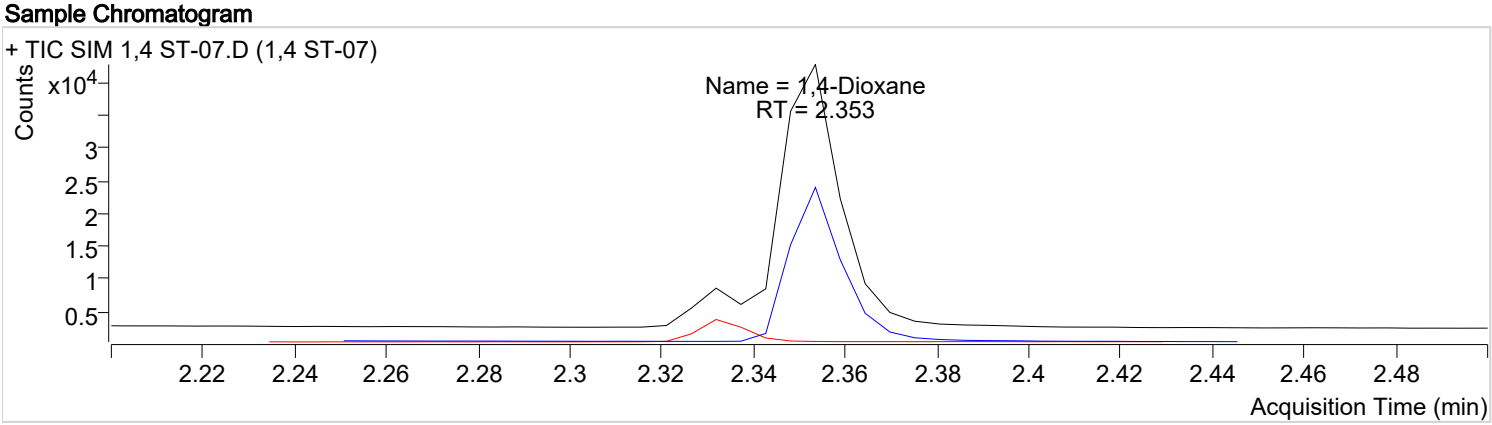

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.353	35109	4449	0.199 mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오전 11:28:51	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

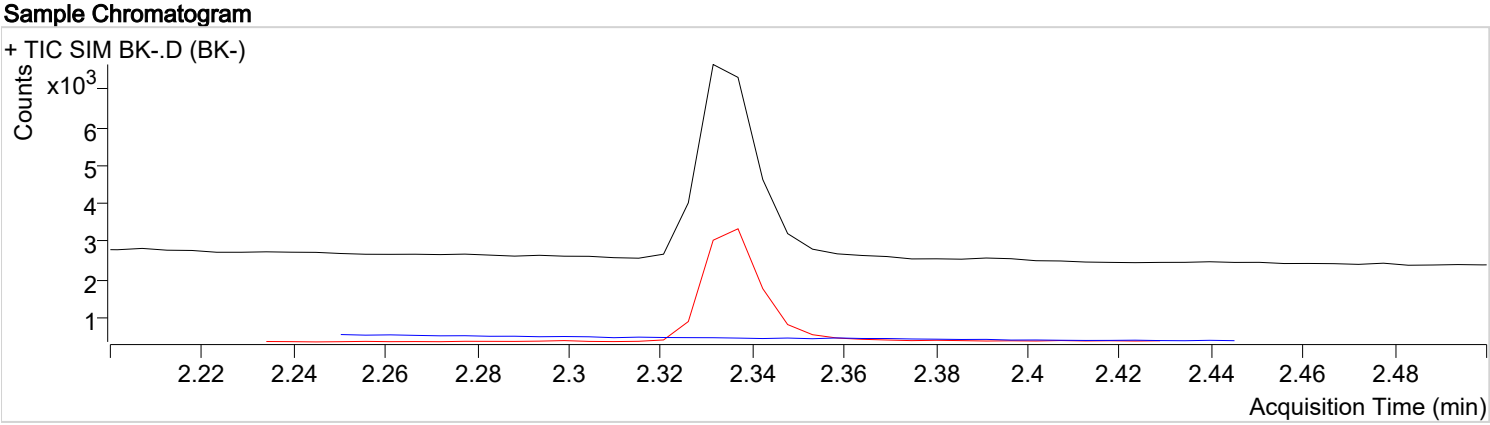

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			4766	ND mg/L

1,4-Dioxane





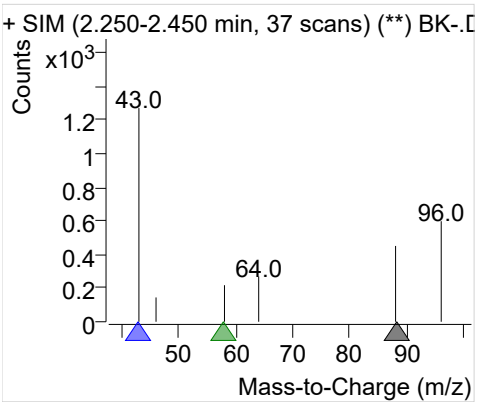

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오전 11:37:49	**Data File**	FBK(RE 26-03-04).D
Type	Blank	**Name**	FBK(RE 26-03-04)
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

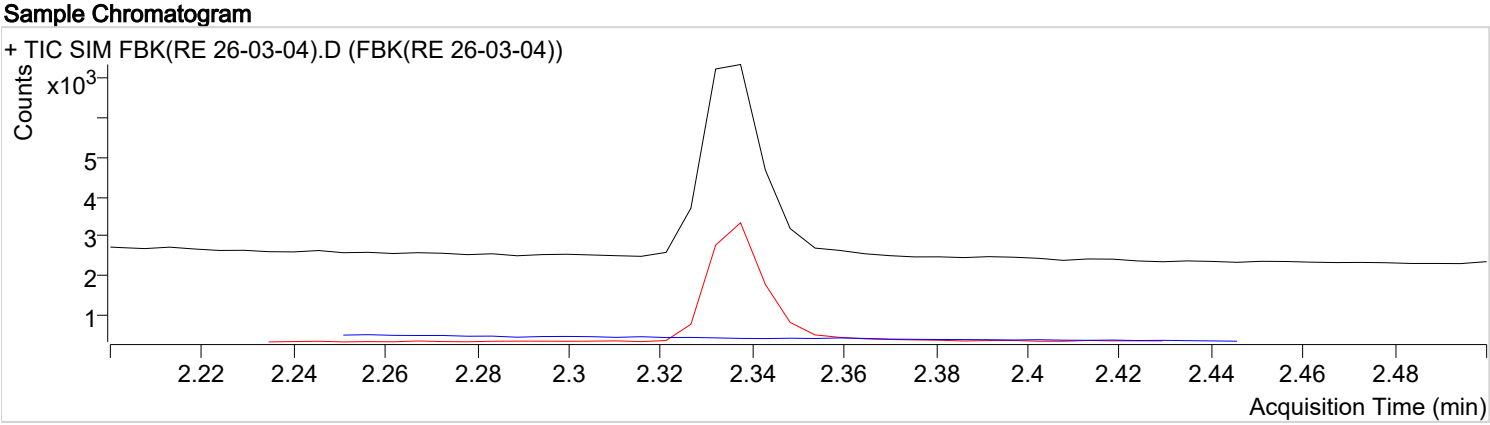

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			4643	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오전 11:46:42	**Data File**	FBK(KD 26-03-04).D
Type	Blank	**Name**	FBK(KD 26-03-04)
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

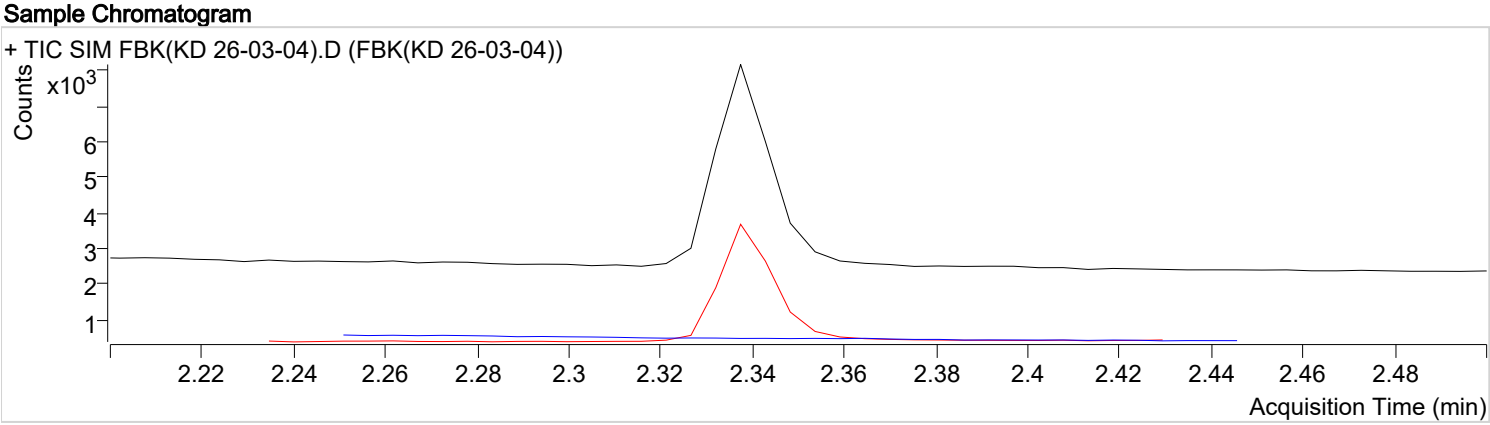

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			4911	ND mg/L

1,4-Dioxane





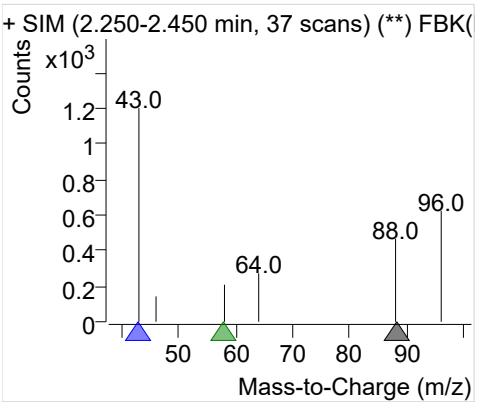

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오전 11:55:38	**Data File**	RE-01.D
Type	Sample	**Name**	RE-01
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

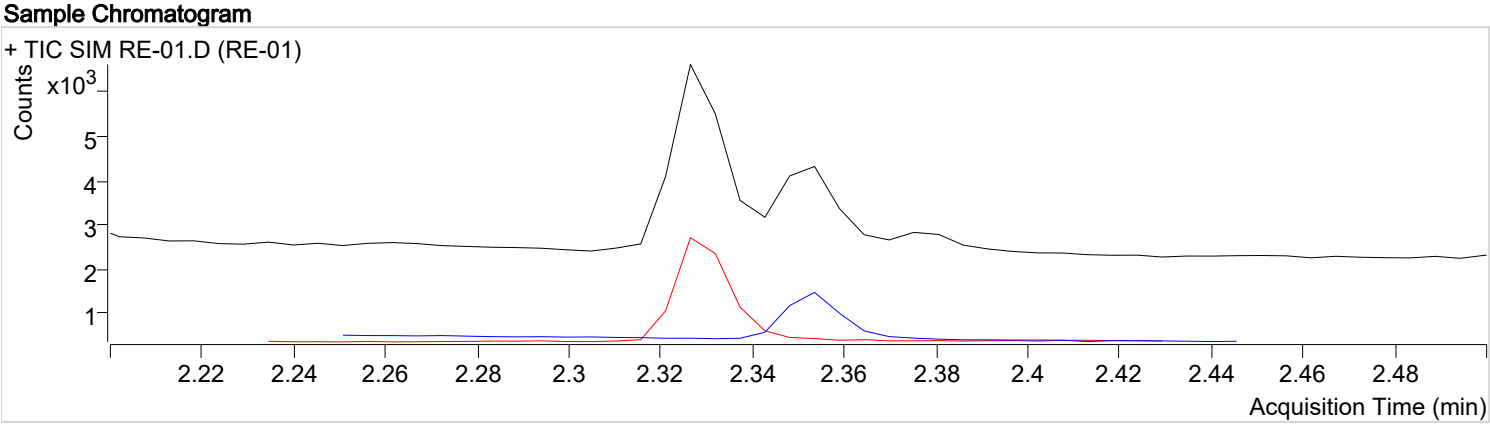

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.354	0	3525	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오후 12:04:35	**Data File**	RE-02.D
Type	Sample	**Name**	RE-02
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

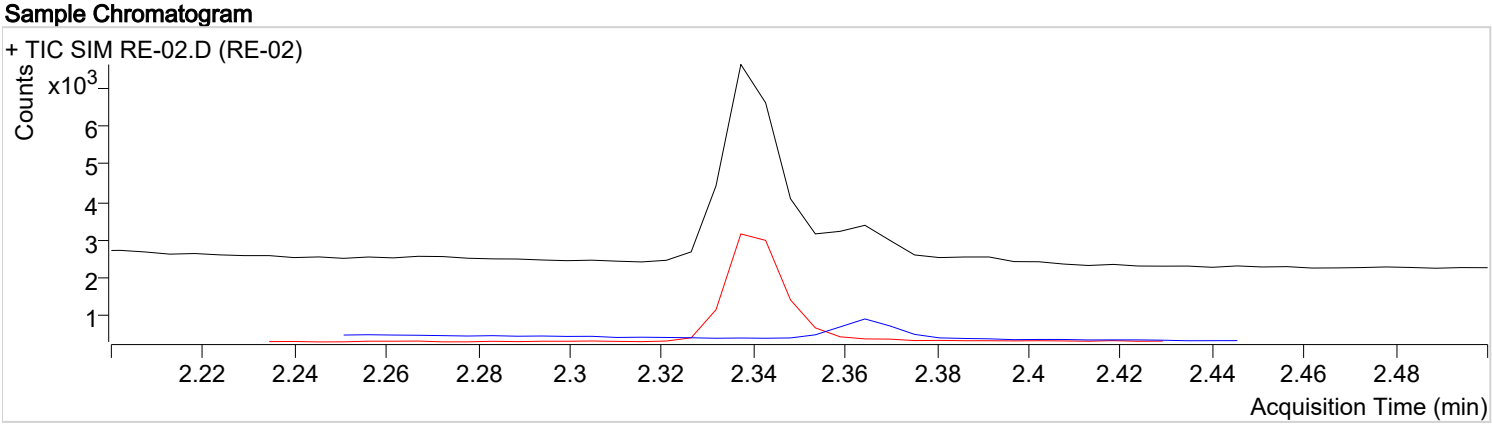

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.364	0	4614	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오후 12:13:30	**Data File**	RE-03.D
Type	Sample	**Name**	RE-03
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

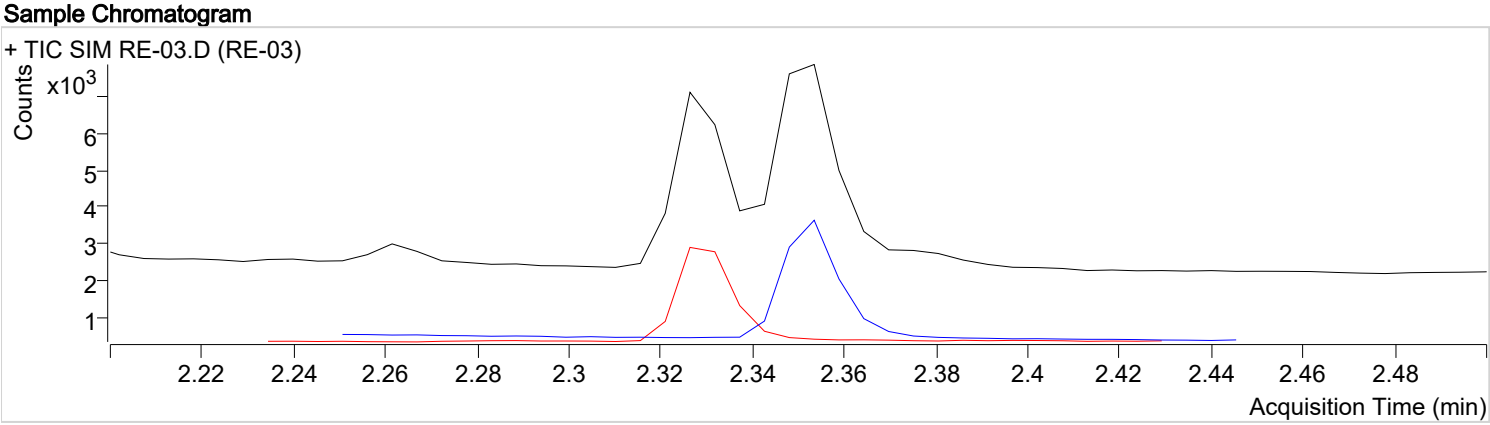

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.353	0	3967	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오후 12:22:28	**Data File**	RE-04.D
Type	Sample	**Name**	RE-04
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

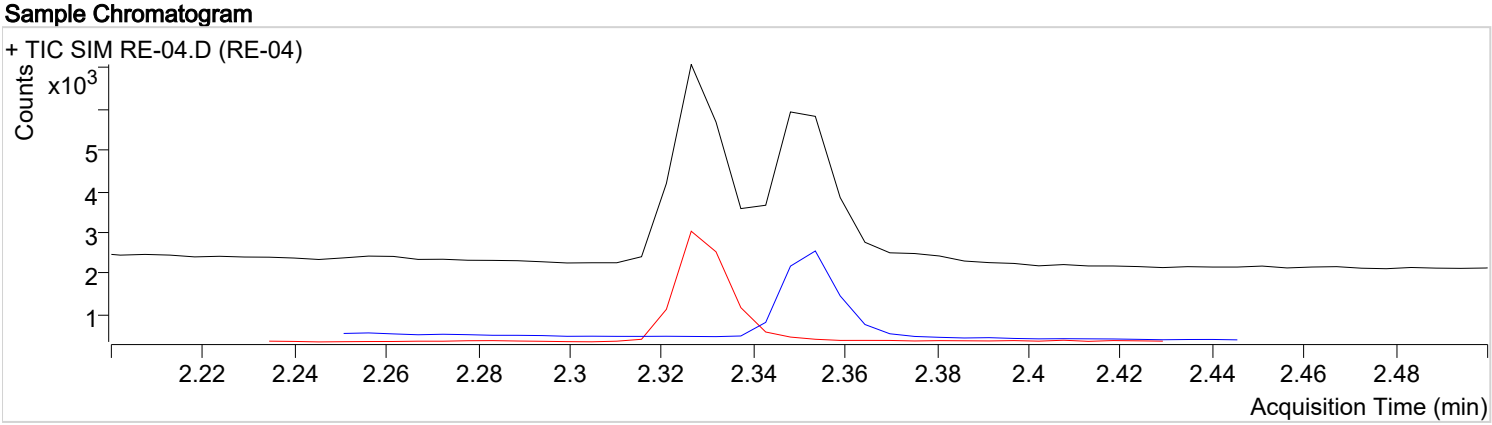

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.353	0	3923	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오후 12:31:22	**Data File**	RE-09.D
Type	Sample	**Name**	RE-09
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

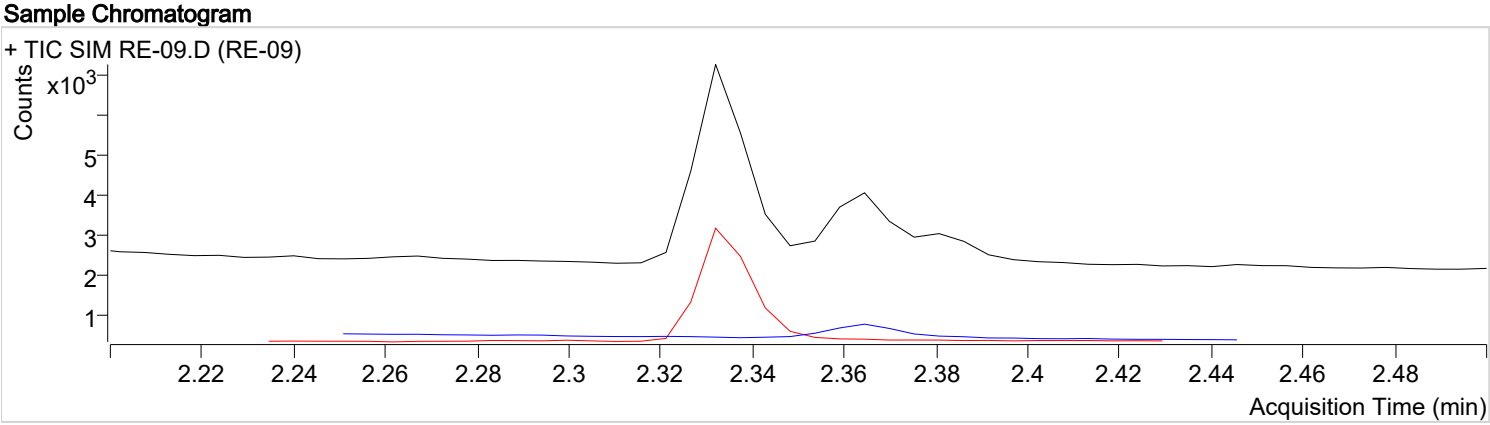

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.364	0	4112	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오후 12:40:21	**Data File**	RE-10.D
Type	Sample	**Name**	RE-10
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

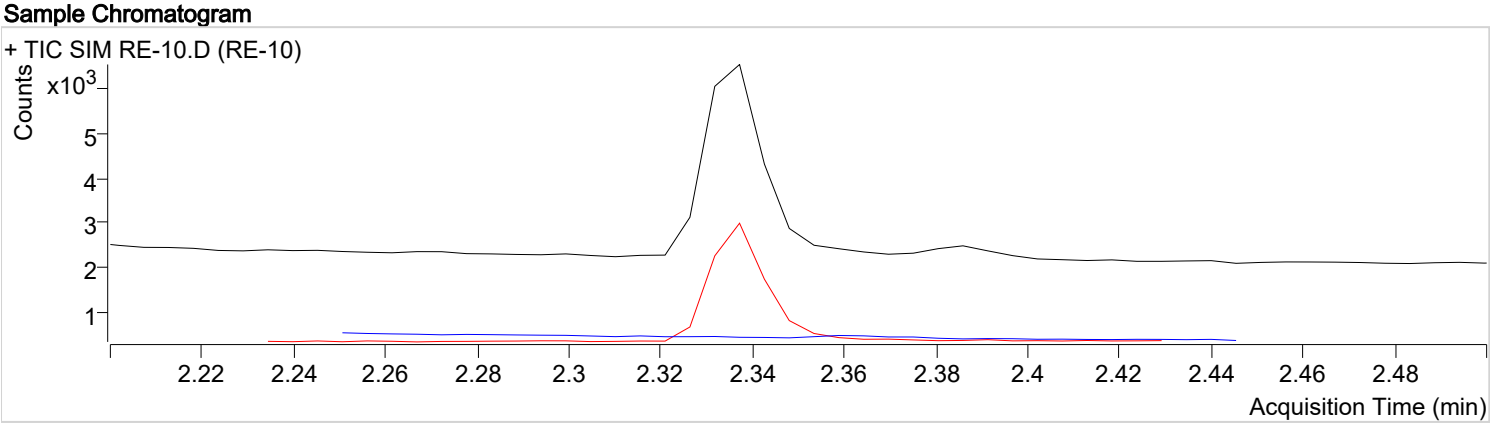

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			3946	ND mg/L

1,4-Dioxane





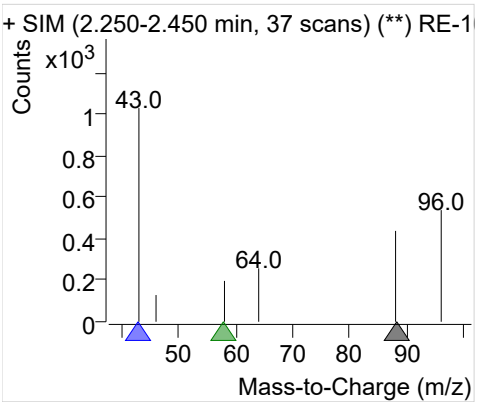

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오후 12:49:19	**Data File**	RE-11.D
Type	Sample	**Name**	RE-11
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

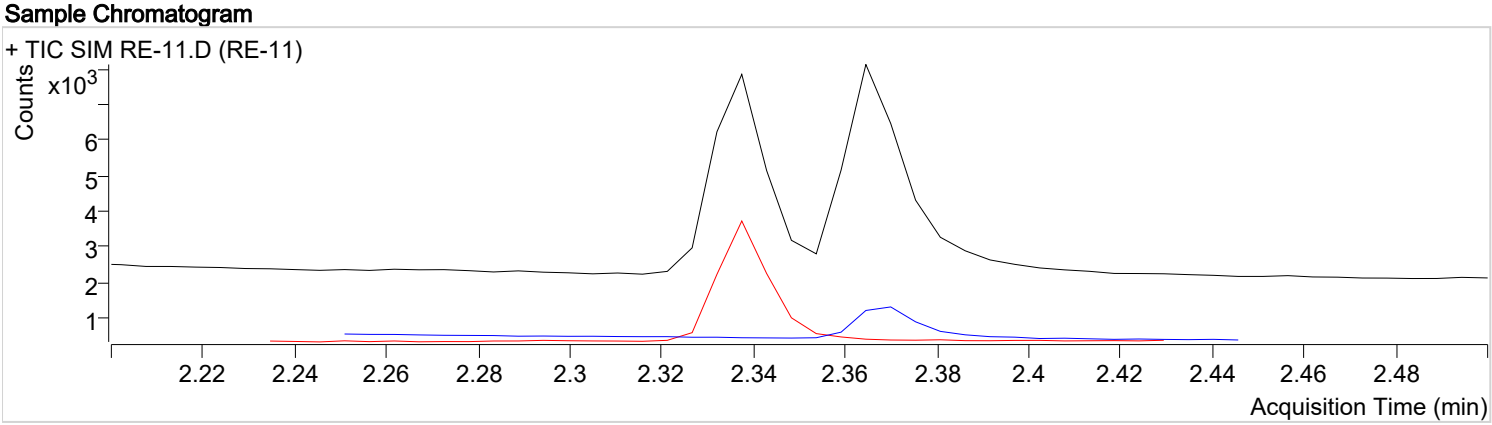

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.370	0	4820	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오후 12:58:14	**Data File**	RE-12.D
Type	Sample	**Name**	RE-12
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

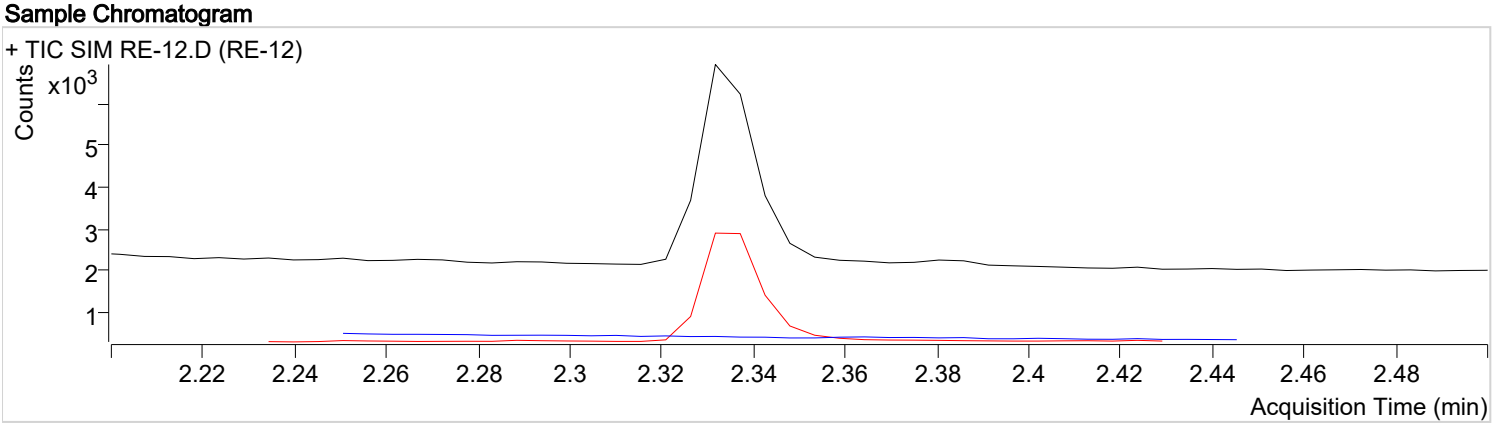

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			4305	ND mg/L

1,4-Dioxane





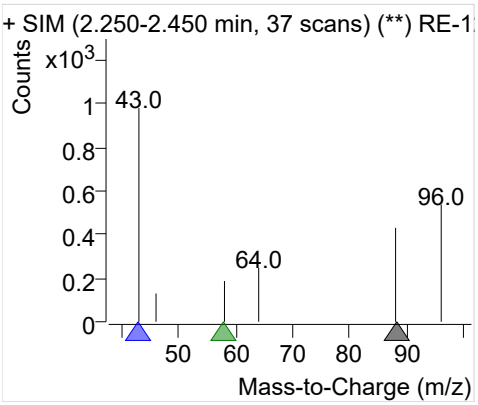

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오후 1:07:13	**Data File**	KD-01.D
Type	Sample	**Name**	KD-01
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

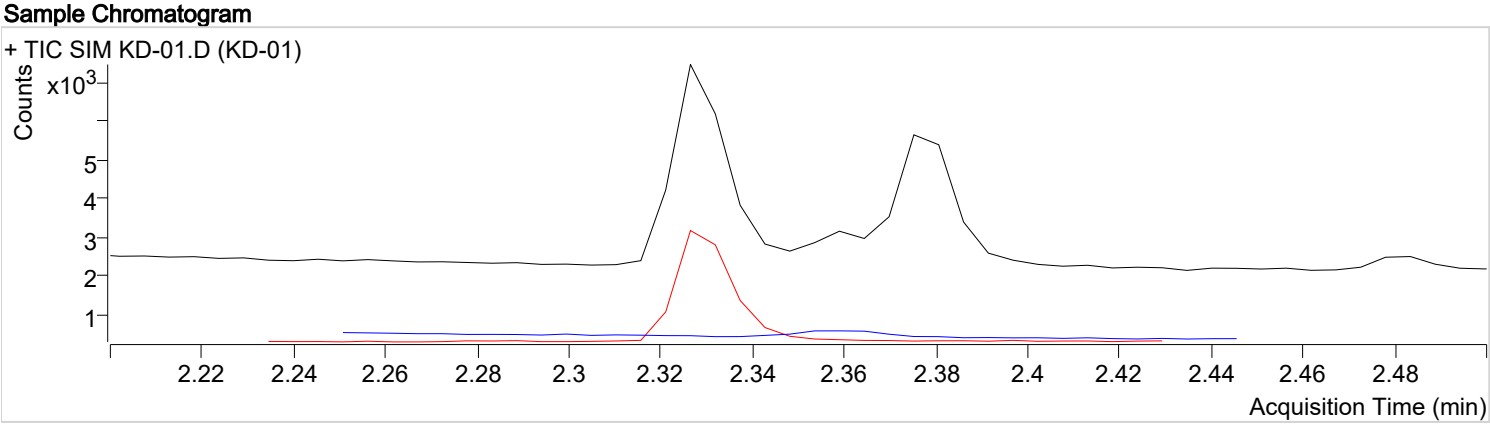

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.359	0	4440	ND mg/L

1,4-Dioxane





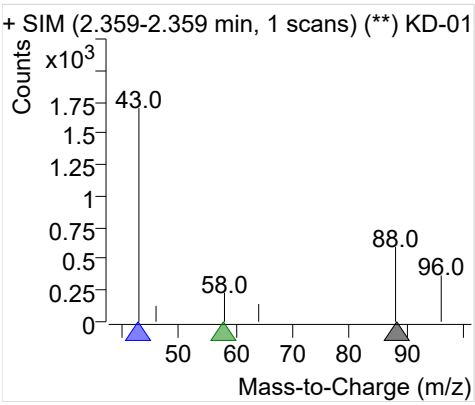

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오후 1:47:39	**Data File**	KD-02.D
Type	Sample	**Name**	KD-02
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

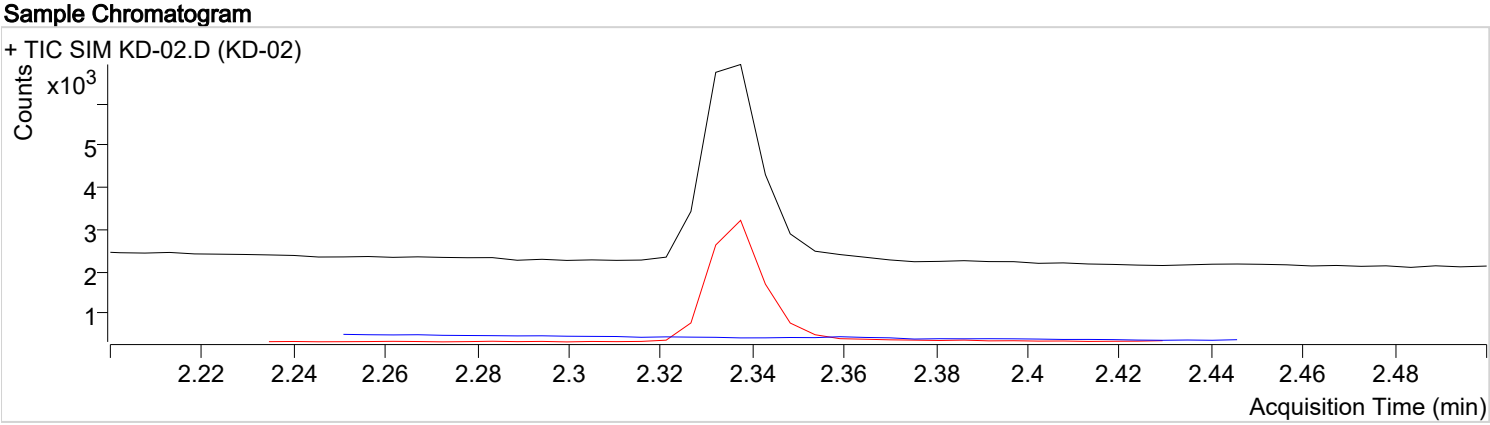

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			4428	ND mg/L

1,4-Dioxane





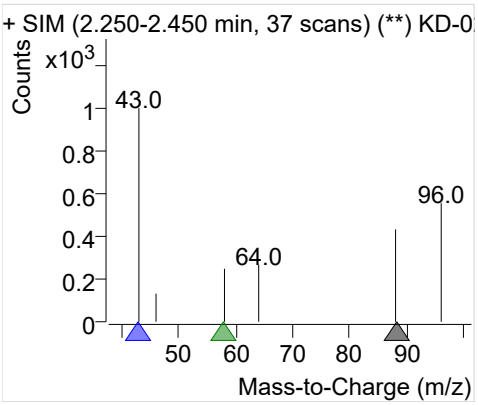

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오후 1:56:37	**Data File**	KD-03.D
Type	Sample	**Name**	KD-03
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

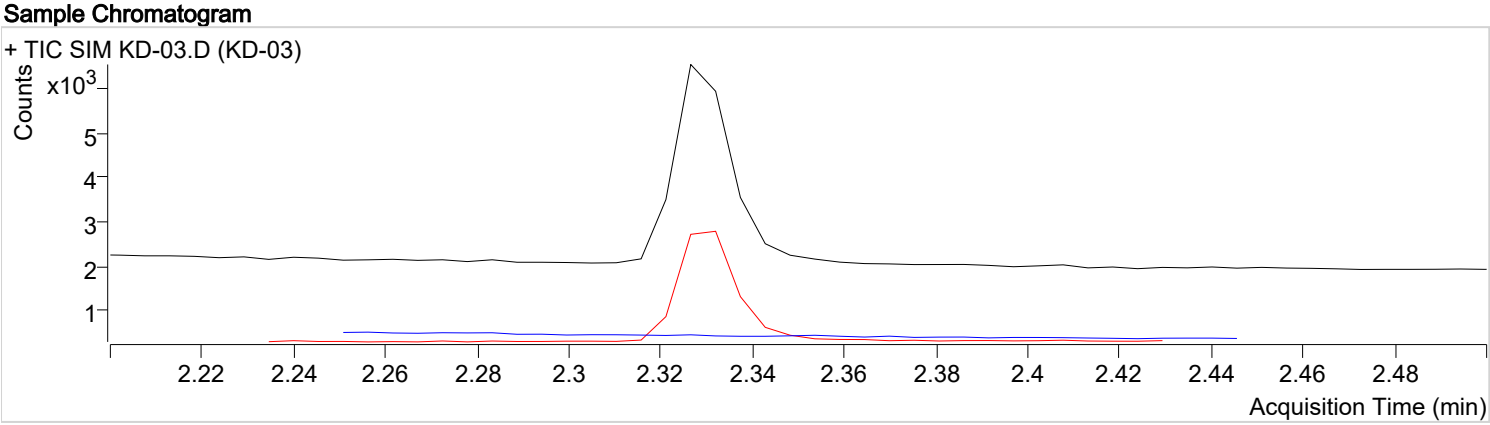

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			3995	ND mg/L

1,4-Dioxane





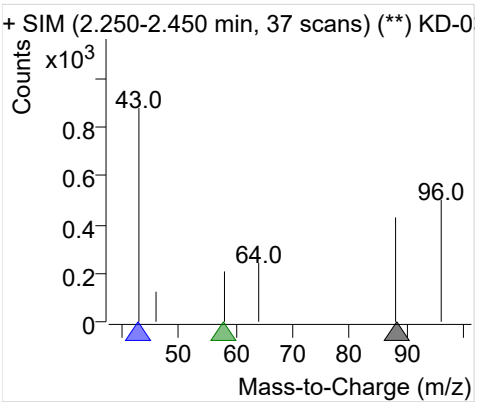

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오후 2:05:34	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

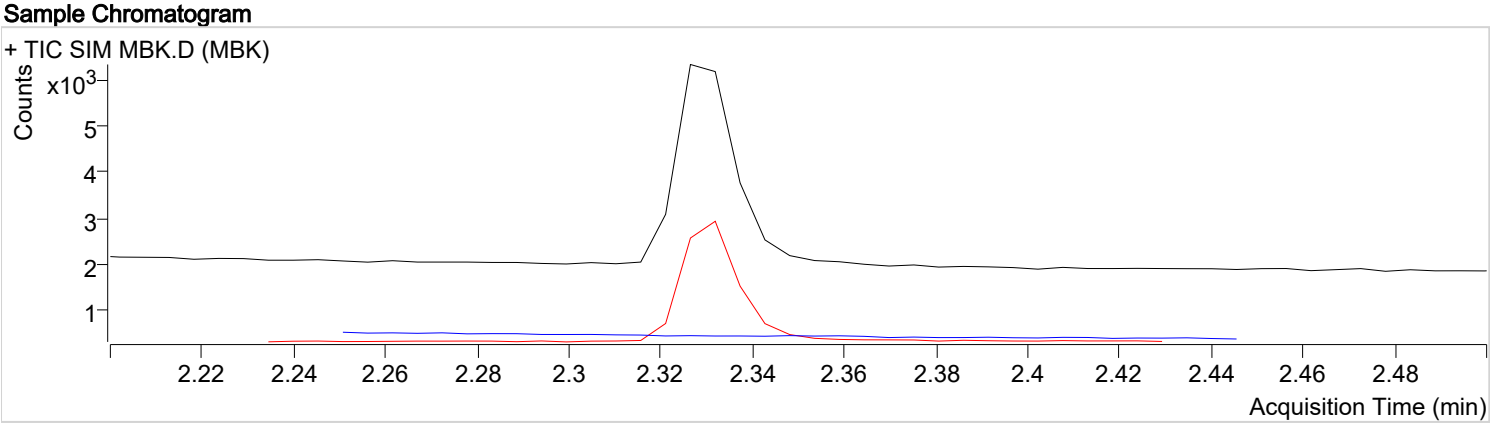

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			4078	ND mg/L

1,4-Dioxane





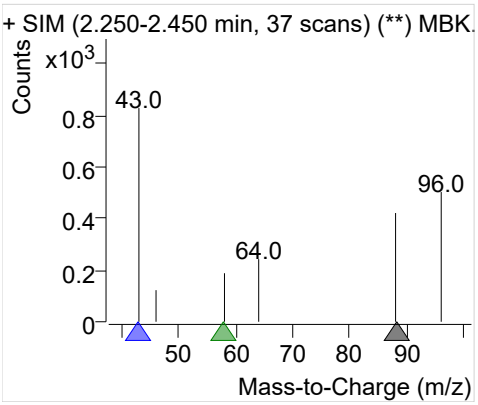

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.4, KD 3.4)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-06 오후 2:42:48	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:42:48	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-06 오후 2:14:31	**Data File**	-C-C-V-.D
Type	QC	**Name**	-C-C-V-
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

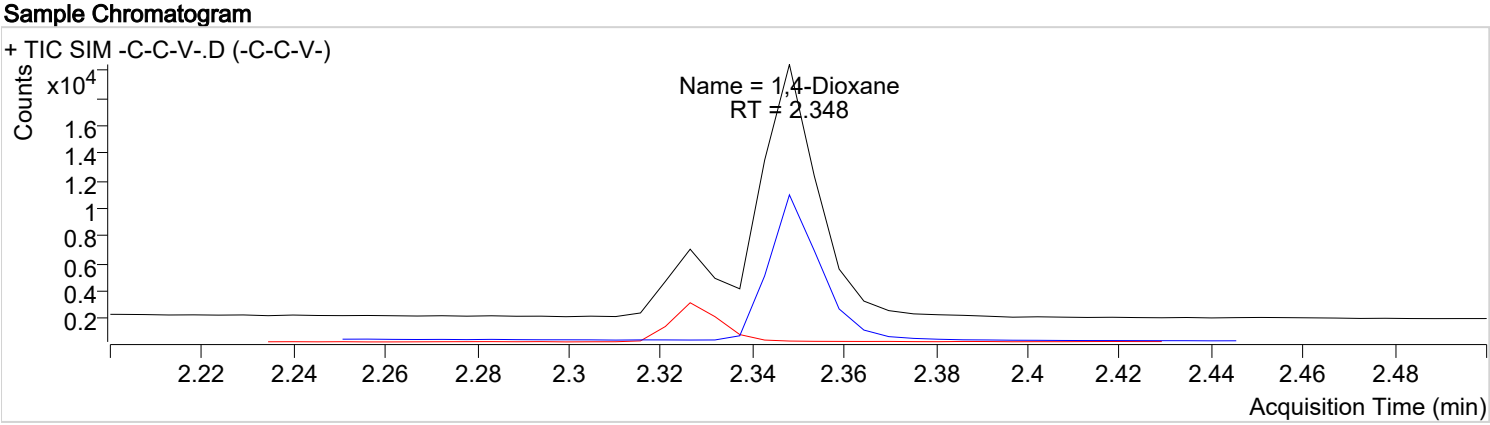

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.348	14949	3735	0.100 mg/L

1,4-Dioxane





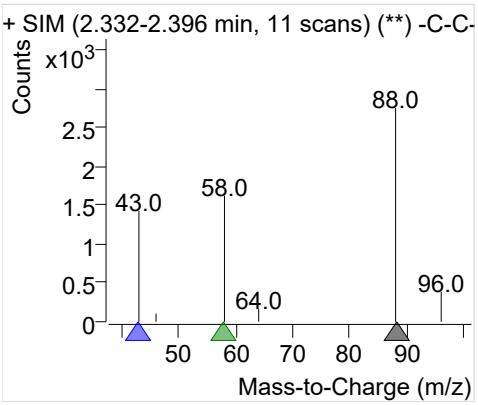

Generated at 오전 10:04 on 2026-04-10