Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin				
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

1,4-Dioxane

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
1,4 ST-01.D	Cal	2.359	1105	2310	0.010
1,4 ST-02.D	Cal	2.359	2382	2541	0.019
1,4 ST-03.D	Cal	2.353	5879	2433	0.050
1,4 ST-04.D	Cal	2.359	9494	2392	0.082
1,4 ST-05.D	Cal	2.348	10868	2202	0.102
1,4 ST-06.D	Cal	2.348	17743	2329	0.157
1,4 ST-07.D	Cal	2.348	22174	2271	0.201
BK-.D	Blank			1527	ND
FBK(RE 26-03-11).D	Blank			1400	ND
RE-07.D	Sample			896	ND
RE-08.D	Sample			1155	ND
RE-17.D	Sample			1054	ND
RE-18.D	Sample			957	ND
RE-19.D	Sample			933	ND
RE-20.D	Sample			793	ND
RE-21.D	Sample			912	ND
RE-22.D	Sample			861	ND
RE-23.D	Sample			931	ND
MBK.D	Blank			1225	ND
-C-C-V-.D	QC	2.353	5329	1097	0.100

1,4-Dioxane

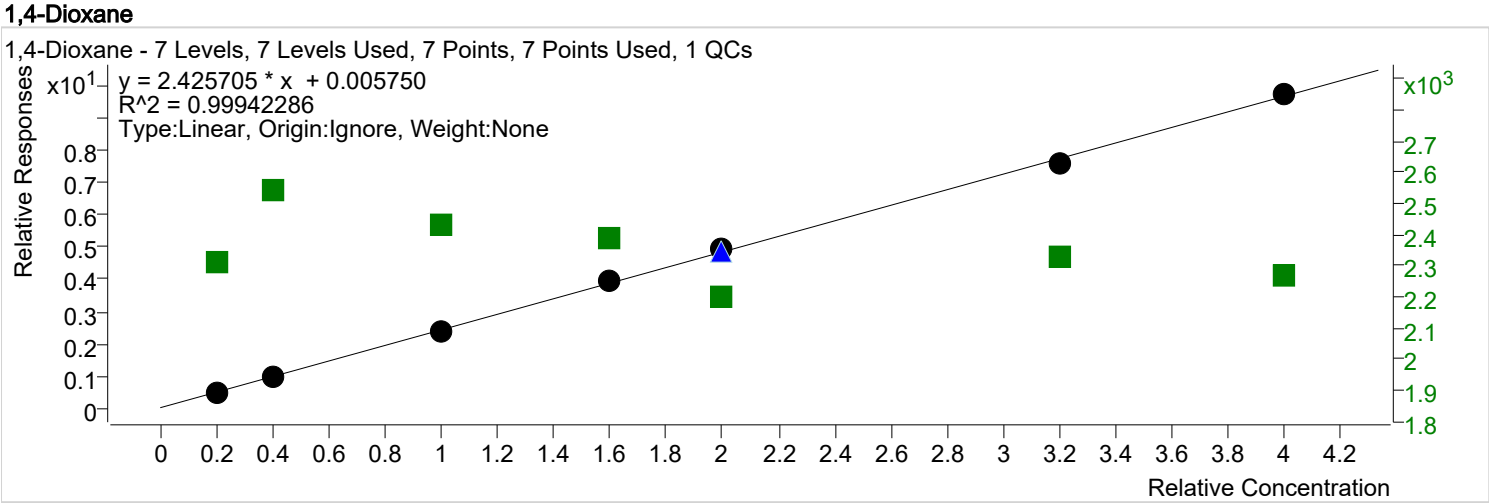

Cal. Path	Type	Level	Enable	Conc.	Response
\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\1,4 ST-01.D	Calibration	1	x	0.200	1105
\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\1,4 ST-02.D	Calibration	2	x	0.400	2382
\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\1,4 ST-03.D	Calibration	3	x	1.000	5879
\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\1,4 ST-04.D	Calibration	4	x	1.600	9494
\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\1,4 ST-05.D	Calibration	5	x	2.000	10868
\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\-C-C-V-.D	QC	5	x	2.000	5329
\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\1,4 ST-06.D	Calibration	6	x	3.200	17743
\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\1,4 ST-07.D	Calibration	7	x	4.000	22174

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오전 10:20:50	**Data File**	1,4 ST-01.D
Type	Cal	**Name**	1,4 ST-01
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

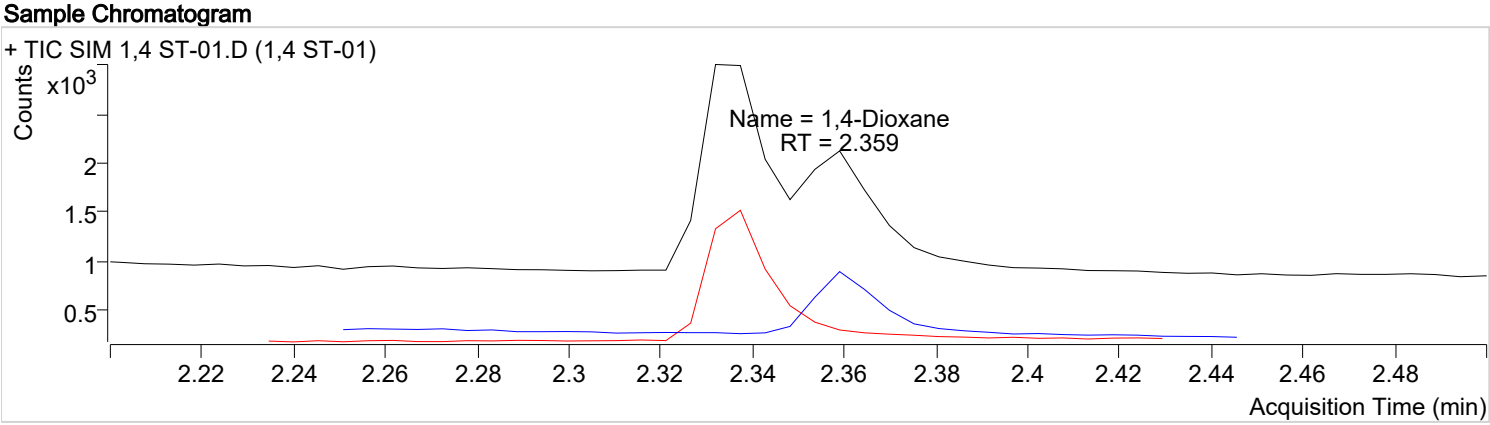

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.359	1105	2310	0.010 mg/L

1,4-Dioxane

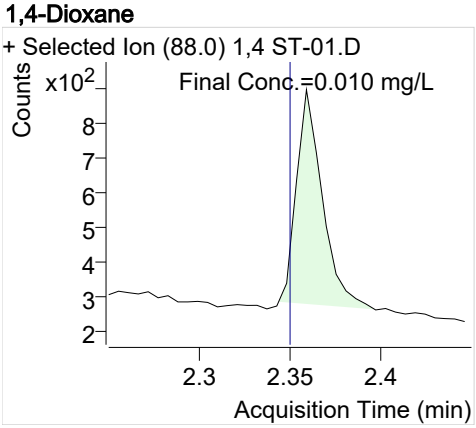





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오전 10:29:37	**Data File**	1,4 ST-02.D
Type	Cal	**Name**	1,4 ST-02
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

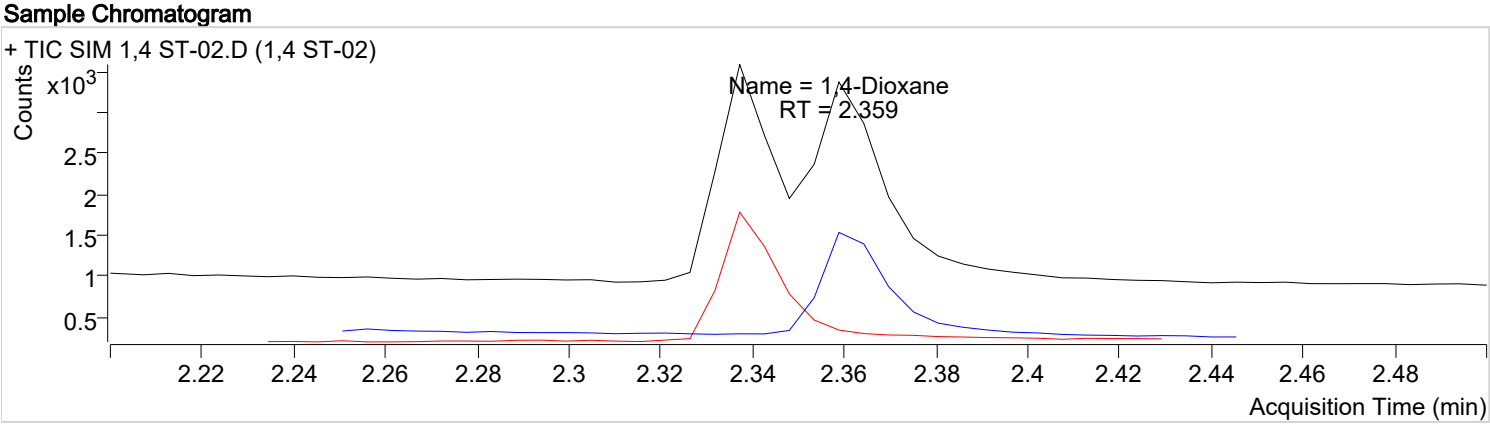

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.359	2382	2541	0.019 mg/L

1,4-Dioxane

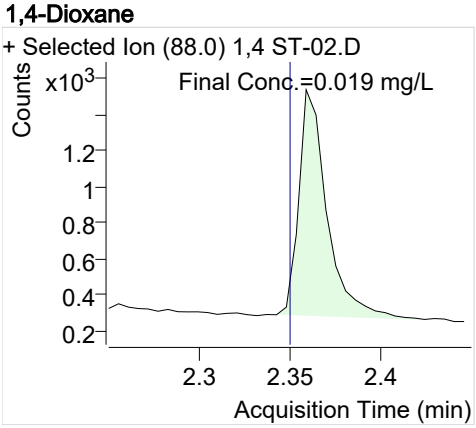





Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오전 10:38:28	**Data File**	1,4 ST-03.D
Type	Cal	**Name**	1,4 ST-03
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

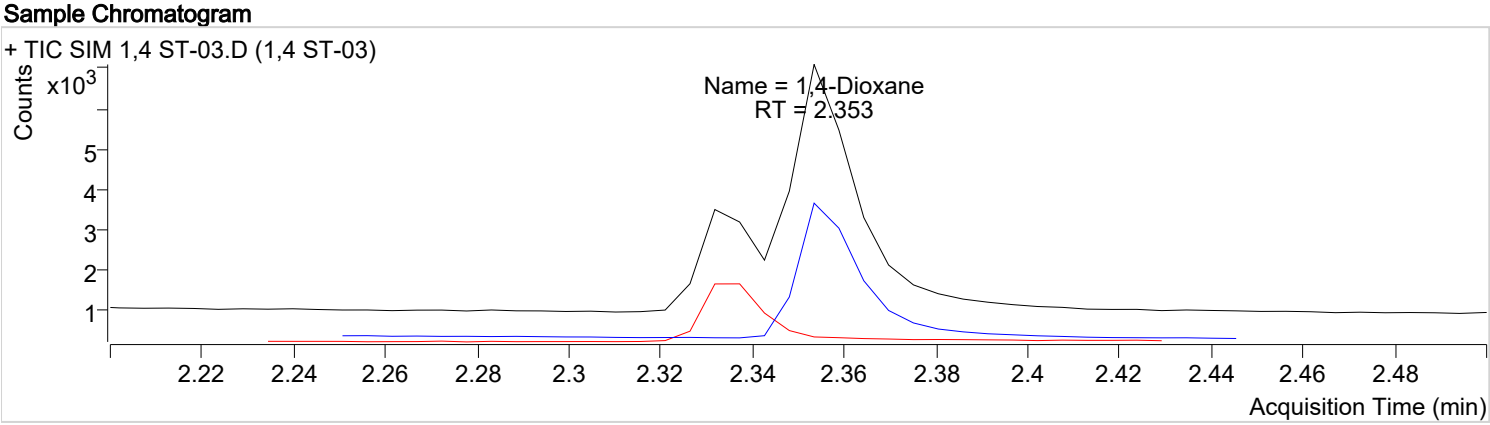

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.353	5879	2433	0.050 mg/L

1,4-Dioxane

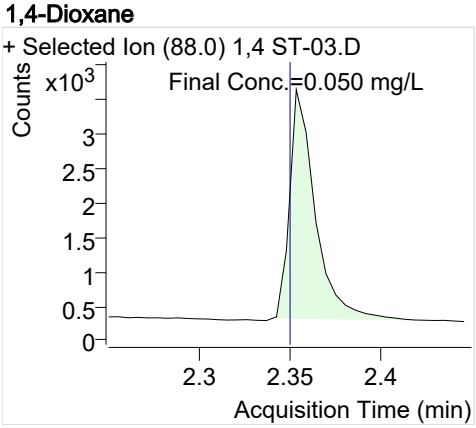





Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오전 10:47:21	**Data File**	1,4 ST-04.D
Type	Cal	**Name**	1,4 ST-04
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

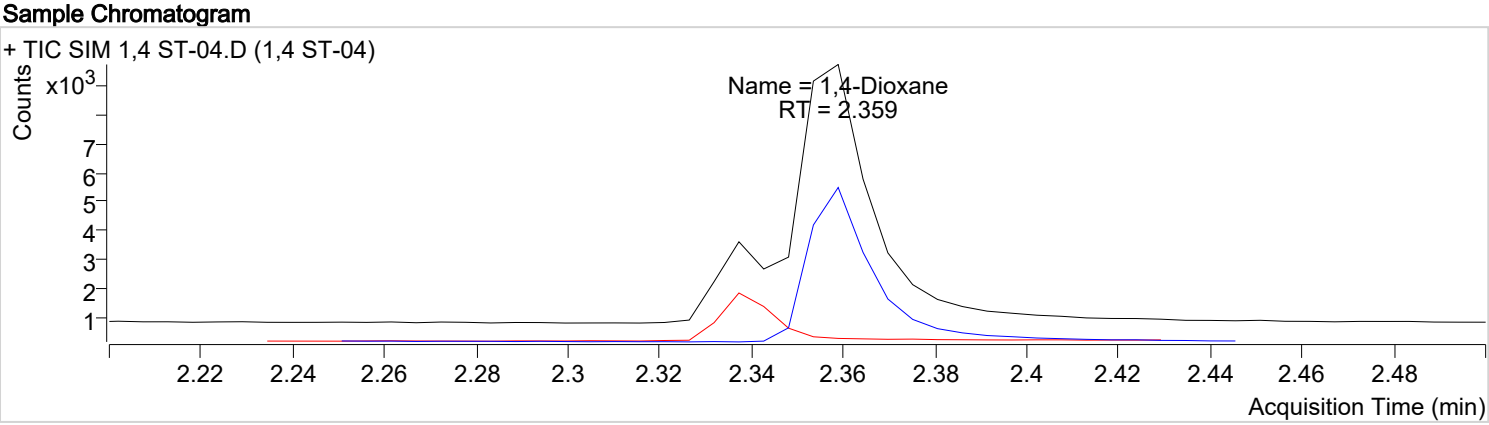

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.359	9494	2392	0.082 mg/L

1,4-Dioxane

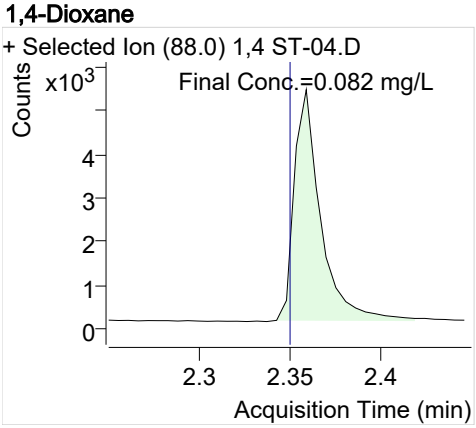

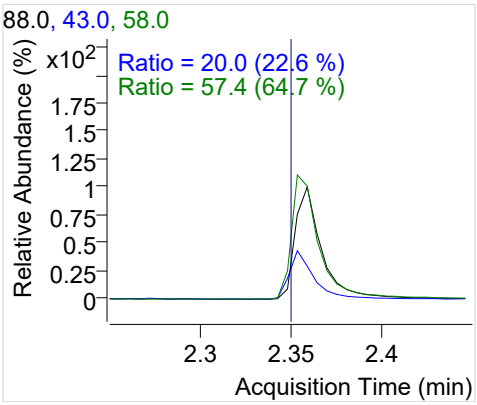



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오전 10:56:18	**Data File**	1,4 ST-05.D
Type	Cal	**Name**	1,4 ST-05
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

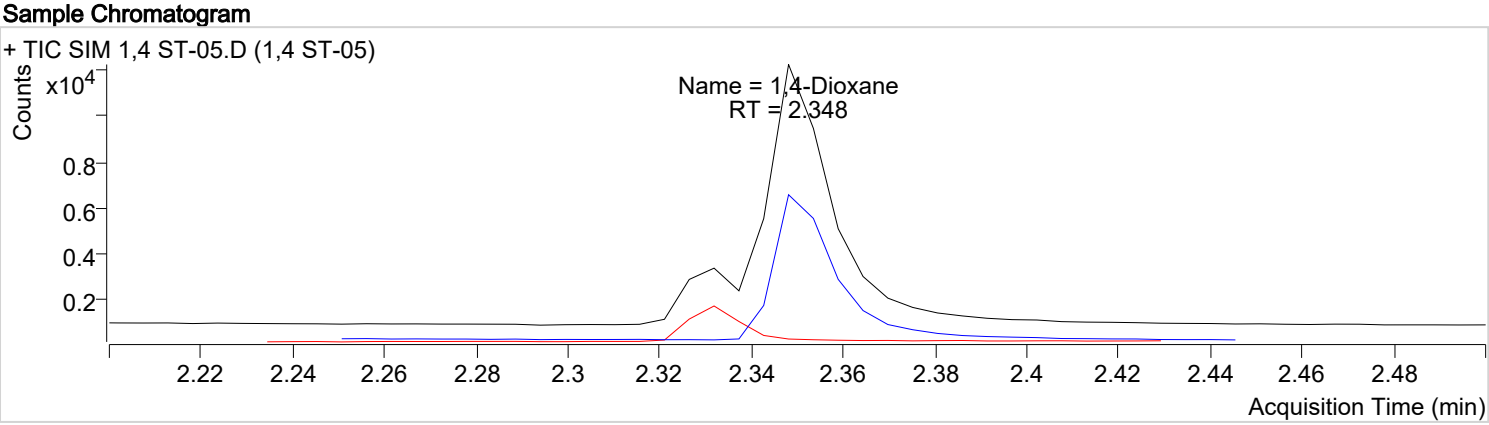

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.348	10868	2202	0.102 mg/L

1,4-Dioxane

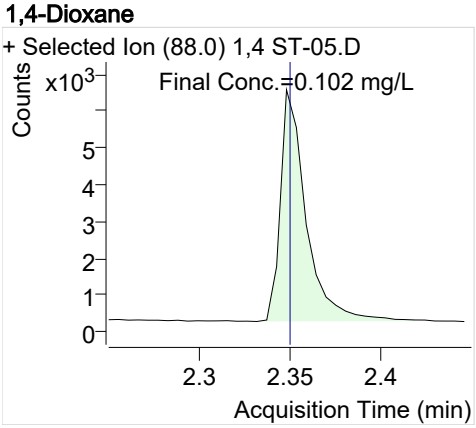

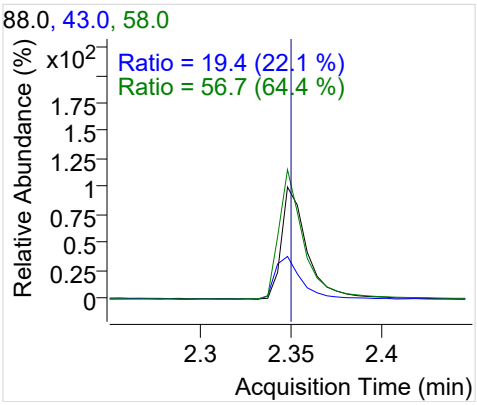

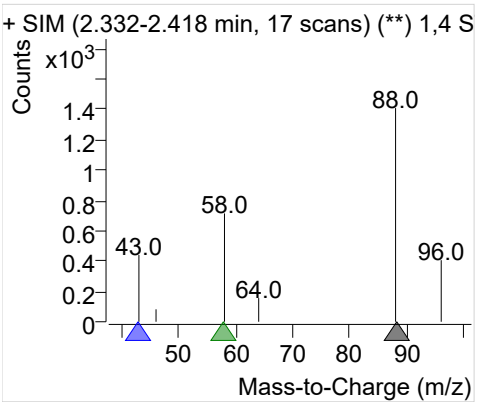

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오전 11:05:10	**Data File**	1,4 ST-06.D
Type	Cal	**Name**	1,4 ST-06
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

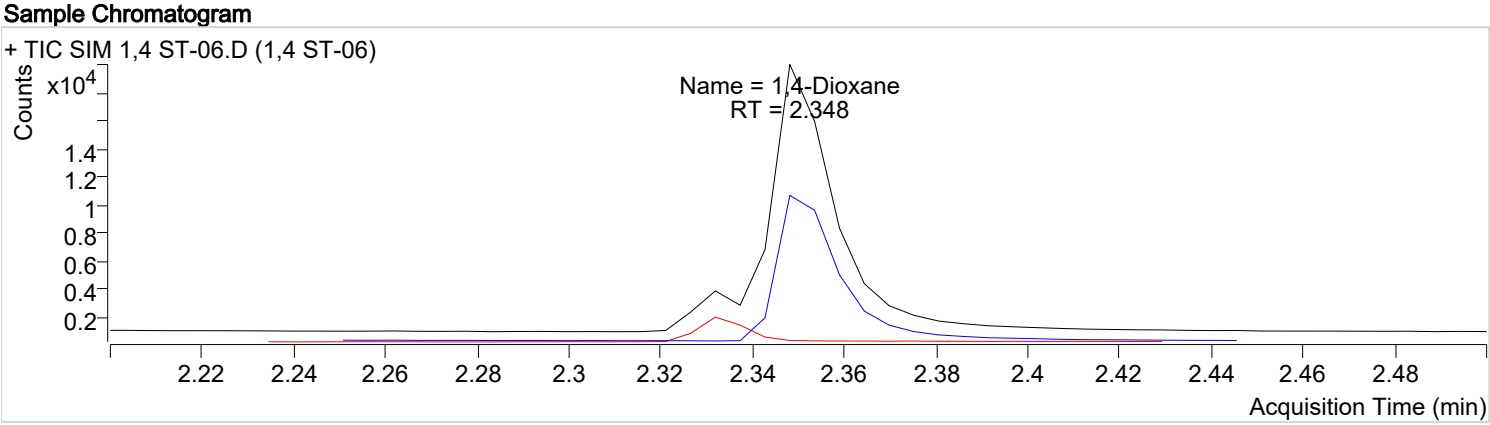

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.348	17743	2329	0.157 mg/L

1,4-Dioxane







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오전 11:14:02	**Data File**	1,4 ST-07.D
Type	Cal	**Name**	1,4 ST-07
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

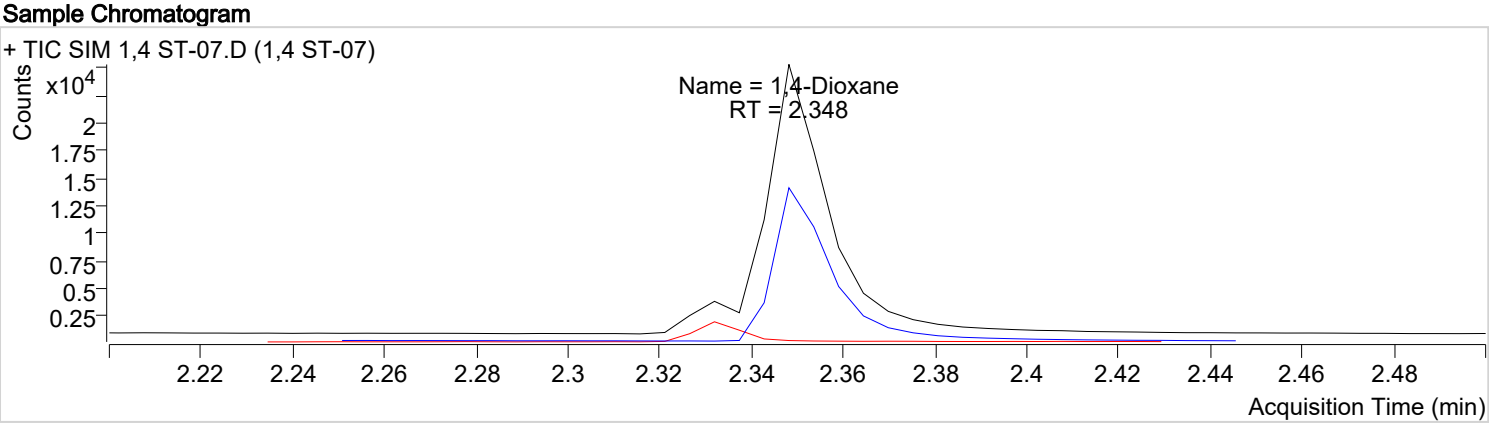

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.348	22174	2271	0.201 mg/L

1,4-Dioxane

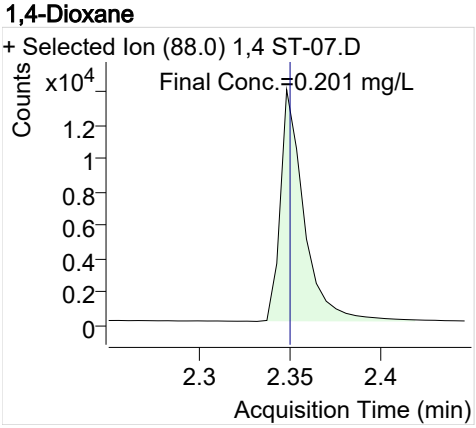

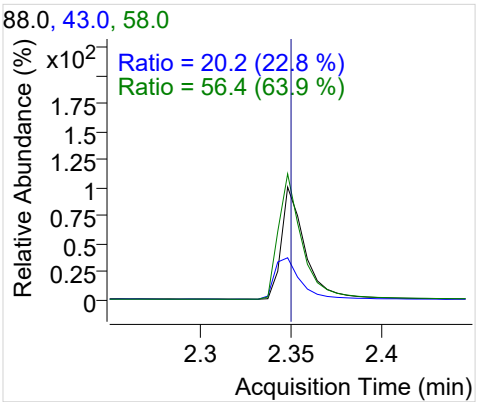



Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오전 11:31:43	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

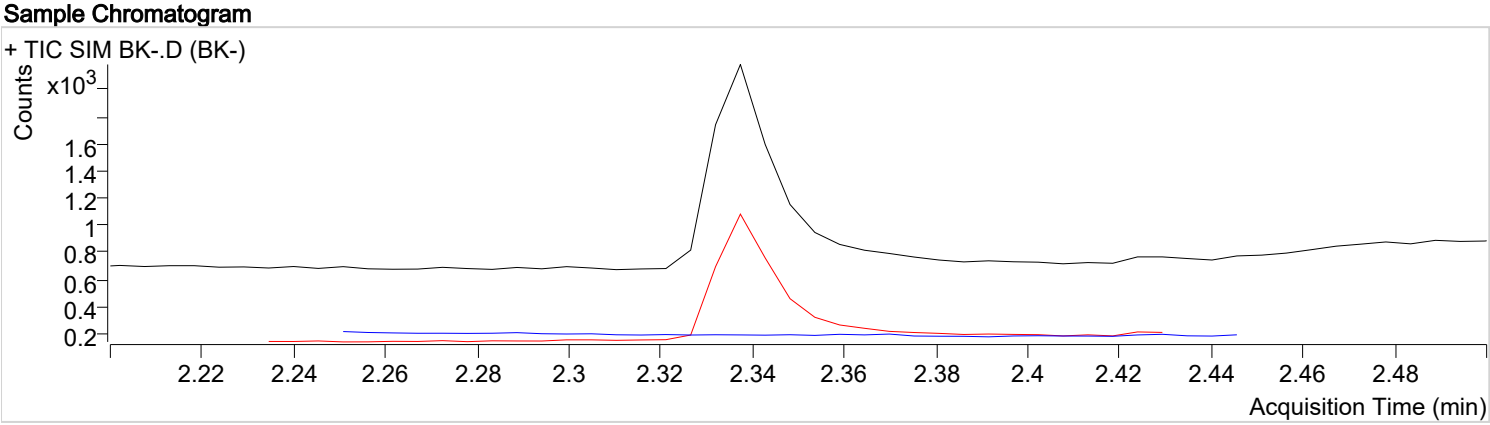

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1527	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오전 11:40:36	**Data File**	FBK(RE 26-03-11).D
Type	Blank	**Name**	FBK(RE 26-03-11)
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

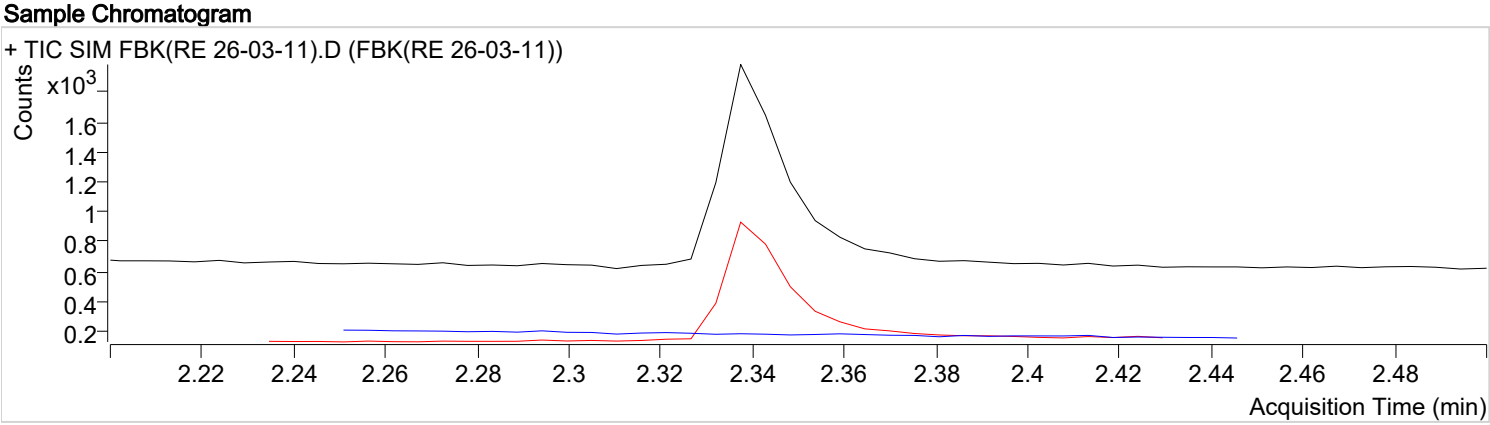

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1400	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오전 11:49:27	**Data File**	RE-07.D
Type	Sample	**Name**	RE-07
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

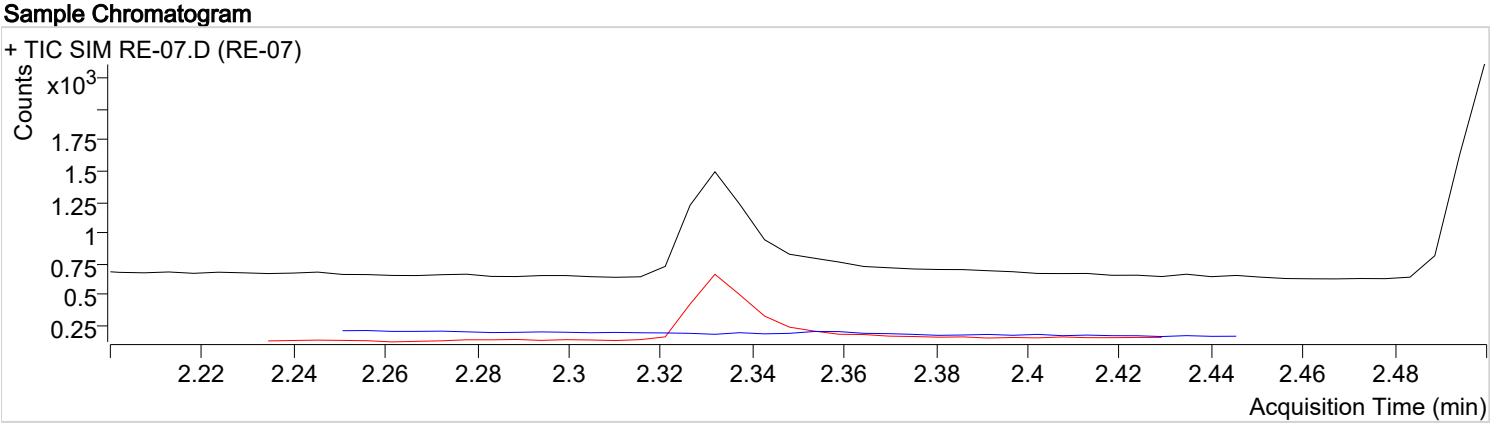

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			896	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오전 11:58:19	**Data File**	RE-08.D
Type	Sample	**Name**	RE-08
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

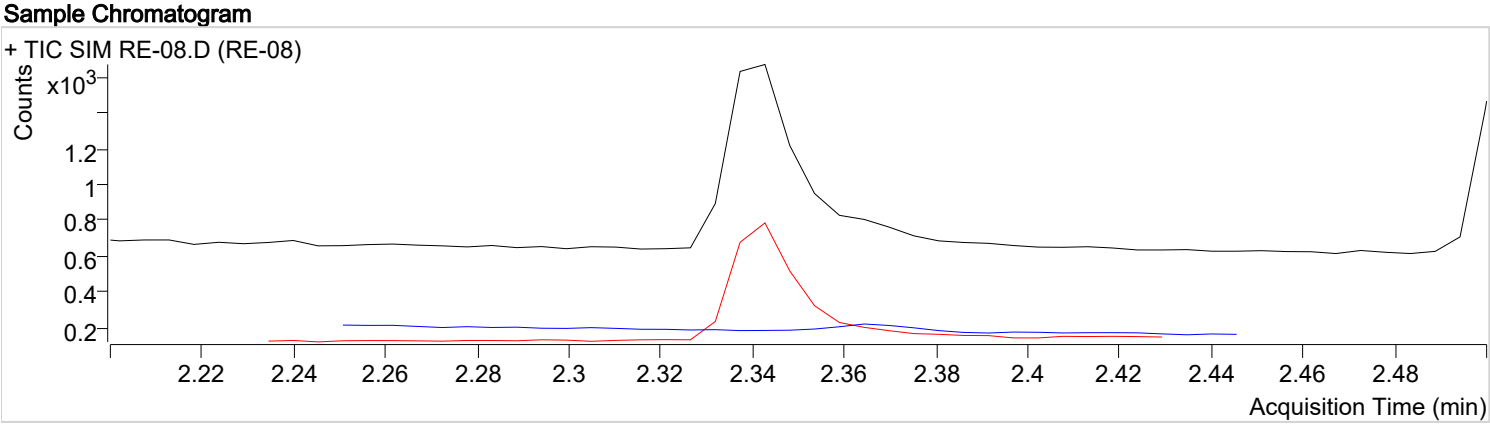

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1155	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 12:07:10	**Data File**	RE-17.D
Type	Sample	**Name**	RE-17
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

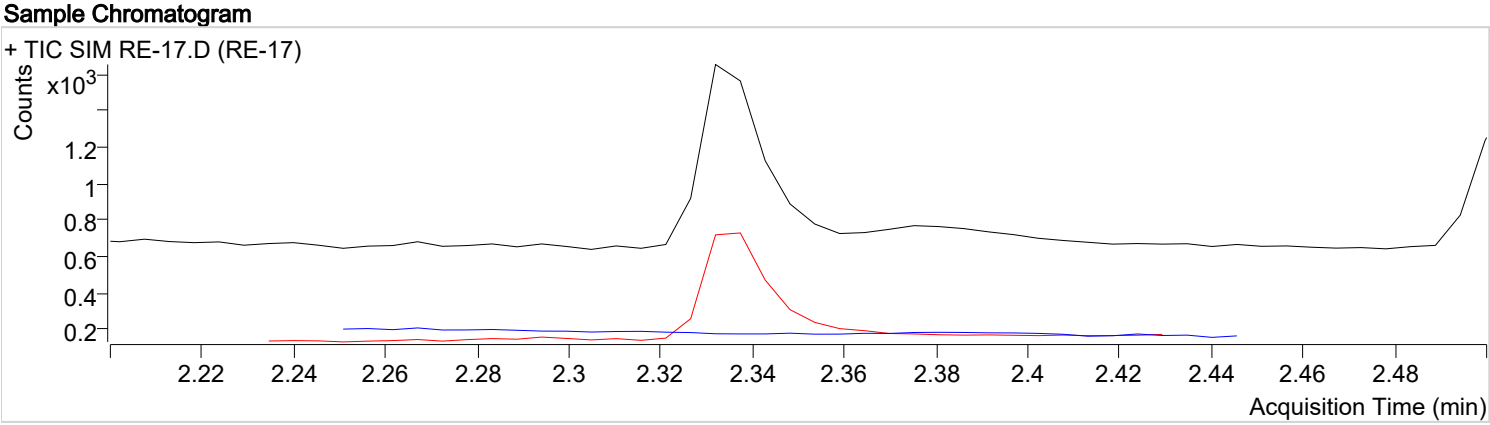

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1054	ND mg/L

1,4-Dioxane







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 12:16:01	**Data File**	RE-18.D
Type	Sample	**Name**	RE-18
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

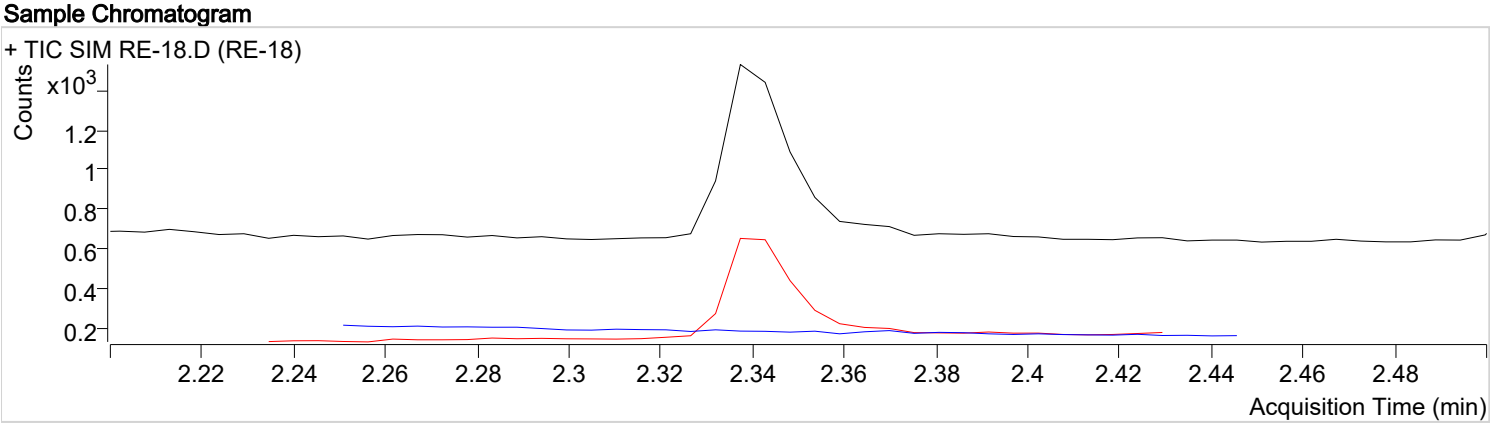

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			957	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 12:24:52	**Data File**	RE-19.D
Type	Sample	**Name**	RE-19
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

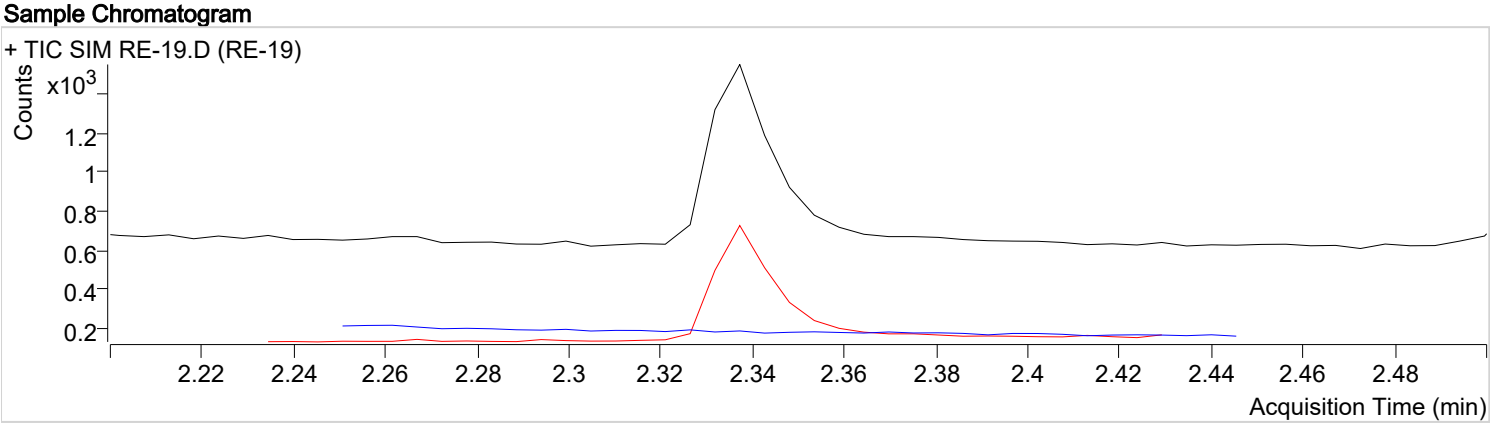

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			933	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 12:33:46	**Data File**	RE-20.D
Type	Sample	**Name**	RE-20
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

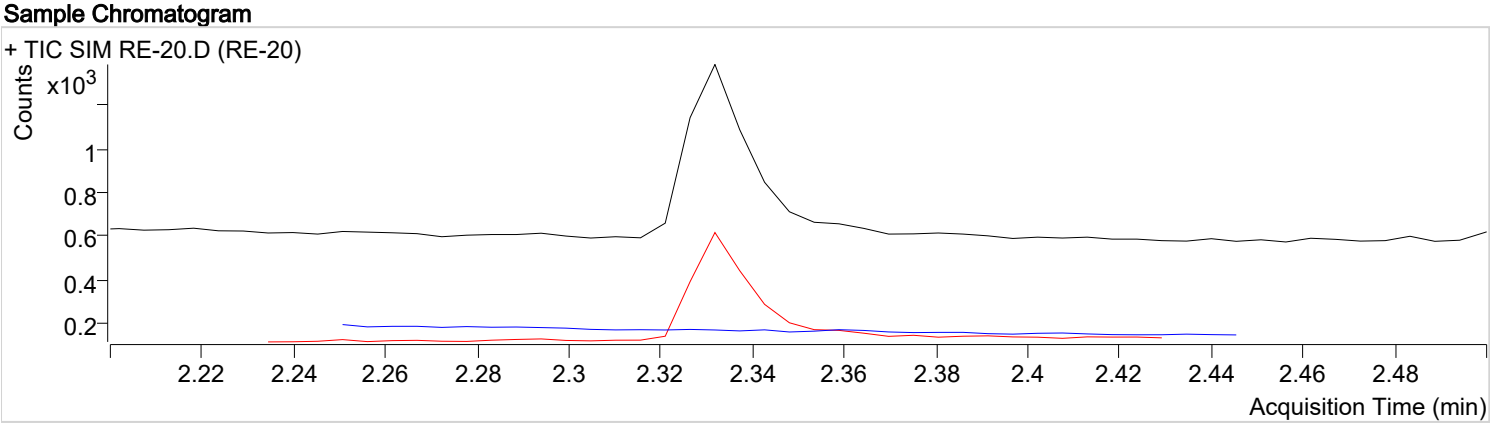

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			793	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 12:42:36	**Data File**	RE-21.D
Type	Sample	**Name**	RE-21
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

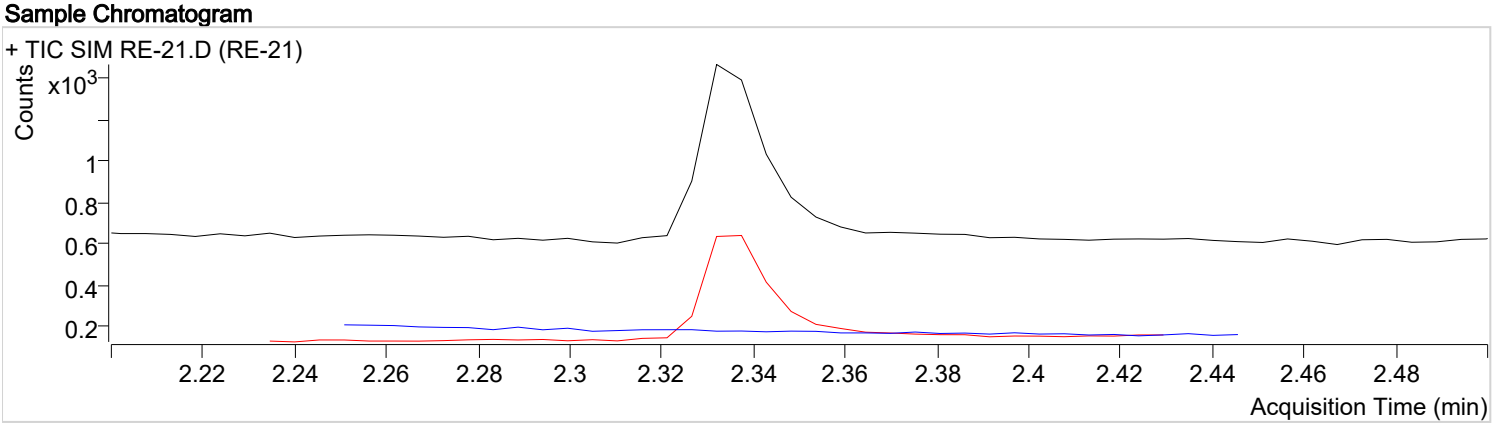

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			912	ND mg/L

1,4-Dioxane

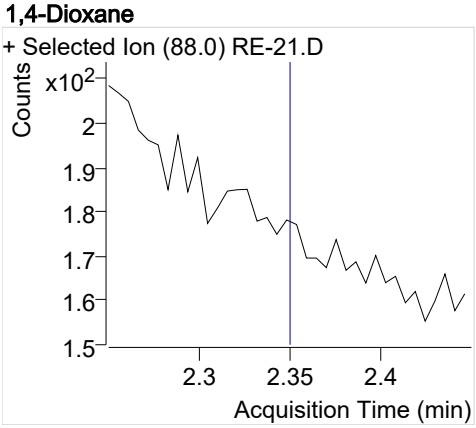





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 12:51:29	**Data File**	RE-22.D
Type	Sample	**Name**	RE-22
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

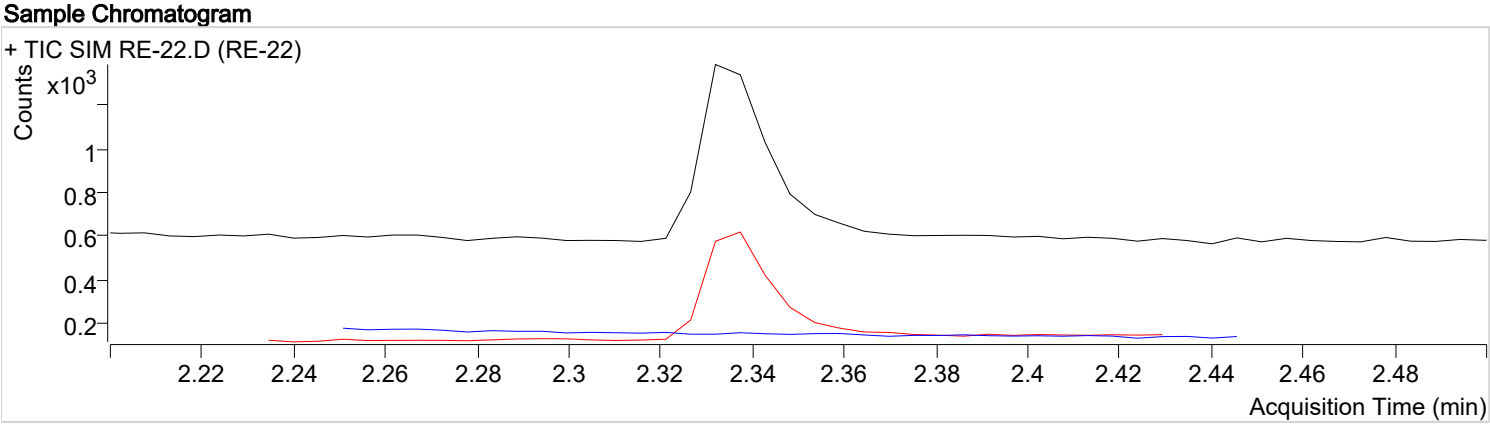

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			861	ND mg/L

1,4-Dioxane







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 1:00:22	**Data File**	RE-23.D
Type	Sample	**Name**	RE-23
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

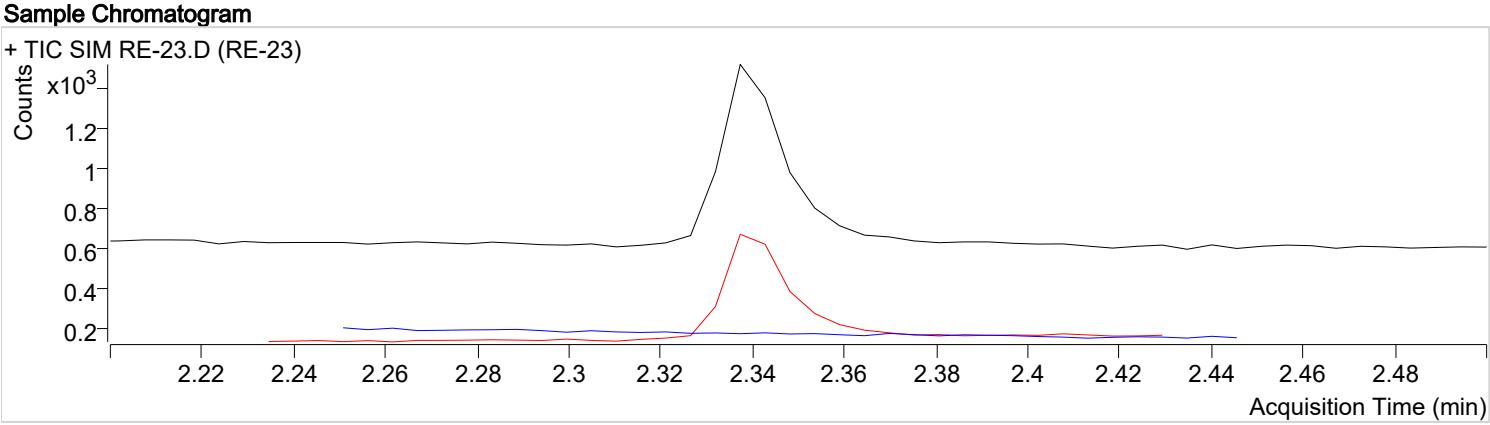

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			931	ND mg/L

1,4-Dioxane







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 1:18:17	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

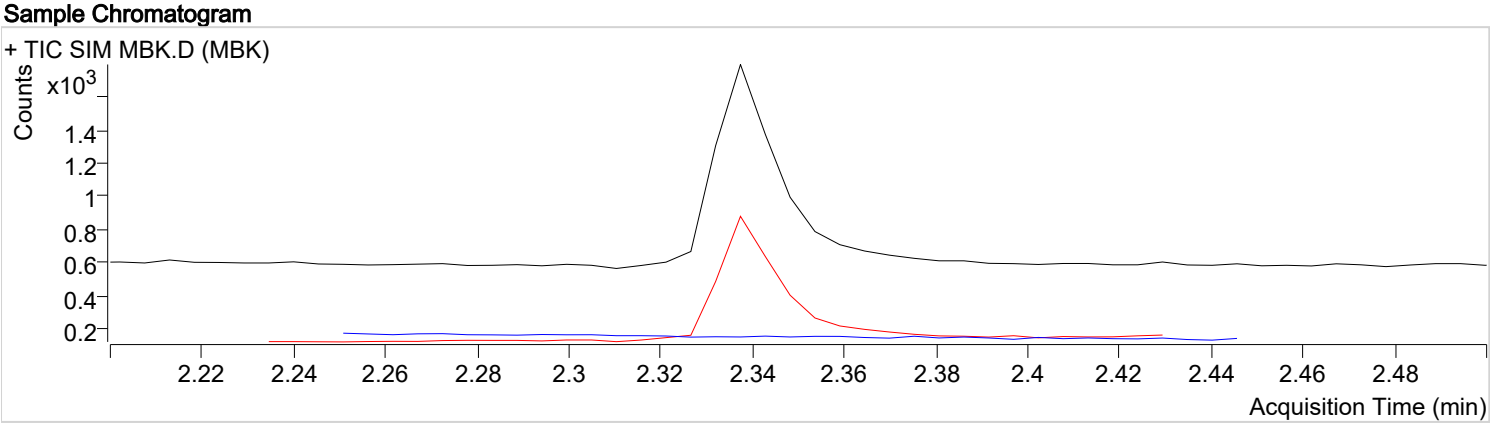

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1225	ND mg/L

1,4-Dioxane







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(RE 3.11)\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-18 오후 12:35:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:04:39	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:35:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 1:36:12	**Data File**	-C-C-V-.D
Type	QC	**Name**	-C-C-V-
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

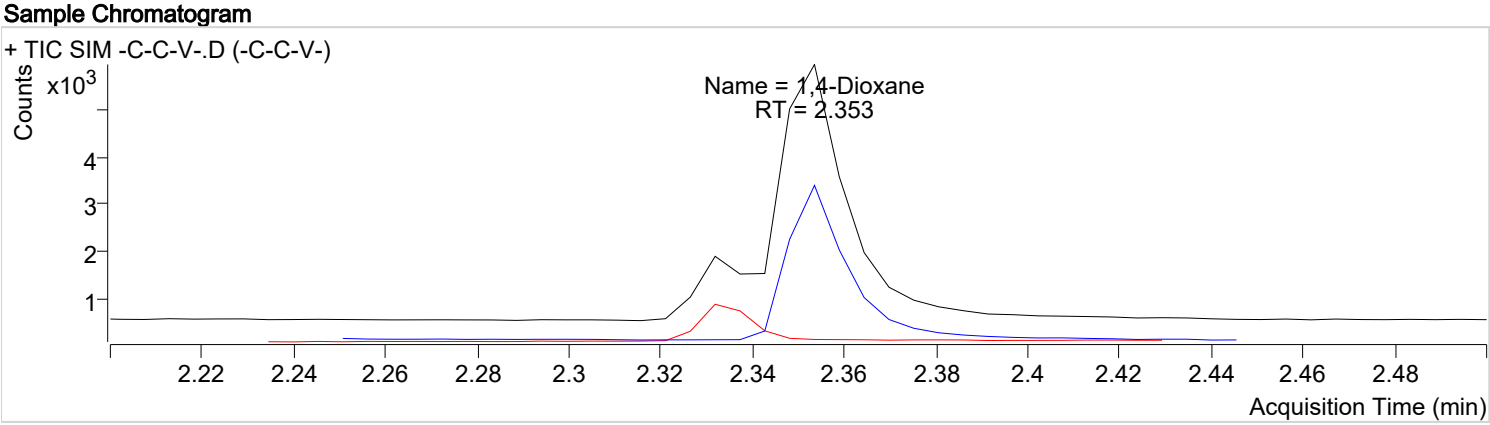

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.353	5329	1097	0.100 mg/L

1,4-Dioxane

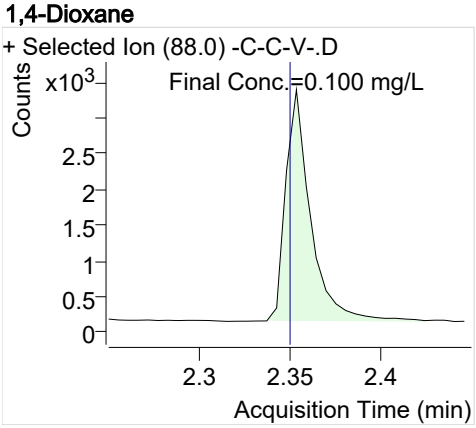

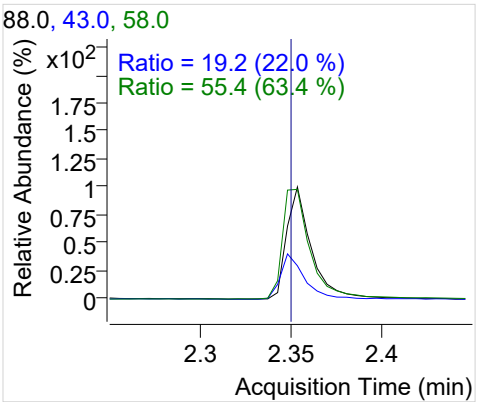

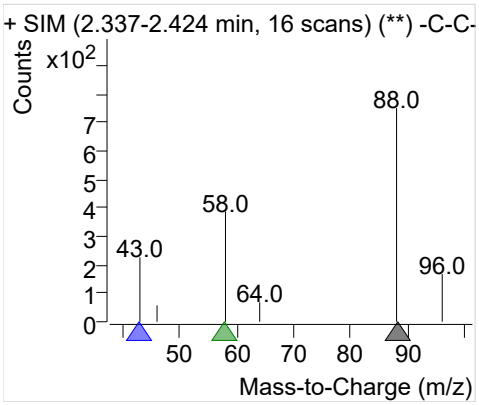

Generated at 오전 10:04 on 2026-04-10