Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\QuantResults\1,4.batch.bin				
Analysis Time	2026-03-31 오후 1:50:58	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:50:58	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

1,4-Dioxane

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
1,4 ST-01.D	Cal	2.364	637	1615	0.009
1,4 ST-02.D	Cal	2.370	1430	1828	0.019
1,4 ST-03.D	Cal	2.354	3002	1462	0.051
1,4 ST-04.D	Cal	2.359	5787	1795	0.081
1,4 ST-05.D	Cal	2.364	7819	1914	0.103
1,4 ST-06.D	Cal	2.354	10533	1655	0.160
1,4 ST-07.D	Cal	2.353	13797	1759	0.198
BK-.D	Blank			1667	ND
FBK(LG NJ 26-03-26).D	Blank			1690	ND
LG NJ-01.D	Sample			1752	ND
LG NJ-02.D	Sample			1450	ND
LG NJ-03.D	Sample			1683	ND
LG NJ-04.D	Sample			1648	ND
LG NJ-05.D	Sample			1654	ND
LG NJ-06.D	Sample			1739	ND
MBK.D	Blank			1616	ND
-CCV-.D	QC	2.359	6488	1573	0.104

1,4-Dioxane

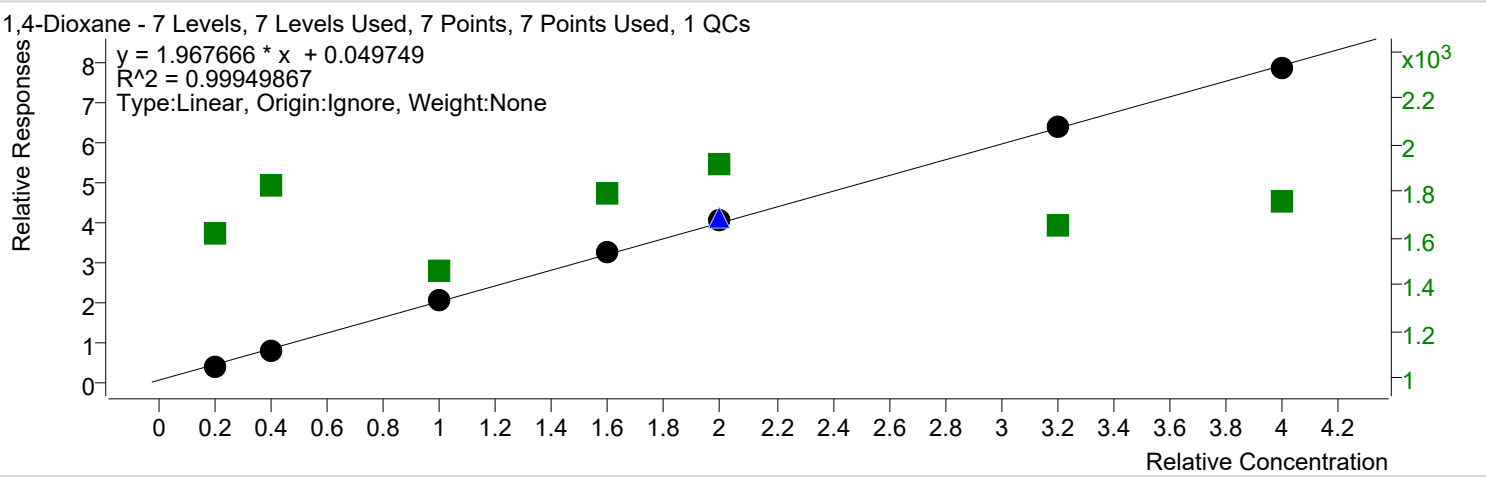

Cal. Path	Type	Level	Enable	Conc.	Response
\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\1,4 ST-01.D	Calibration	1	x	0.200	637
\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\1,4 ST-02.D	Calibration	2	x	0.400	1430
\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\1,4 ST-03.D	Calibration	3	x	1.000	3002
\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\1,4 ST-04.D	Calibration	4	x	1.600	5787
\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\1,4 ST-05.D	Calibration	5	x	2.000	7819
\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\-CCV-.D	QC	5	x	2.000	6488
\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\1,4 ST-06.D	Calibration	6	x	3.200	10533
\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\1,4 ST-07.D	Calibration	7	x	4.000	13797

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-31 오후 1:50:58	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:02:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:50:58	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 3:54:00	**Data File**	1,4 ST-01.D
Type	Cal	**Name**	1,4 ST-01
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

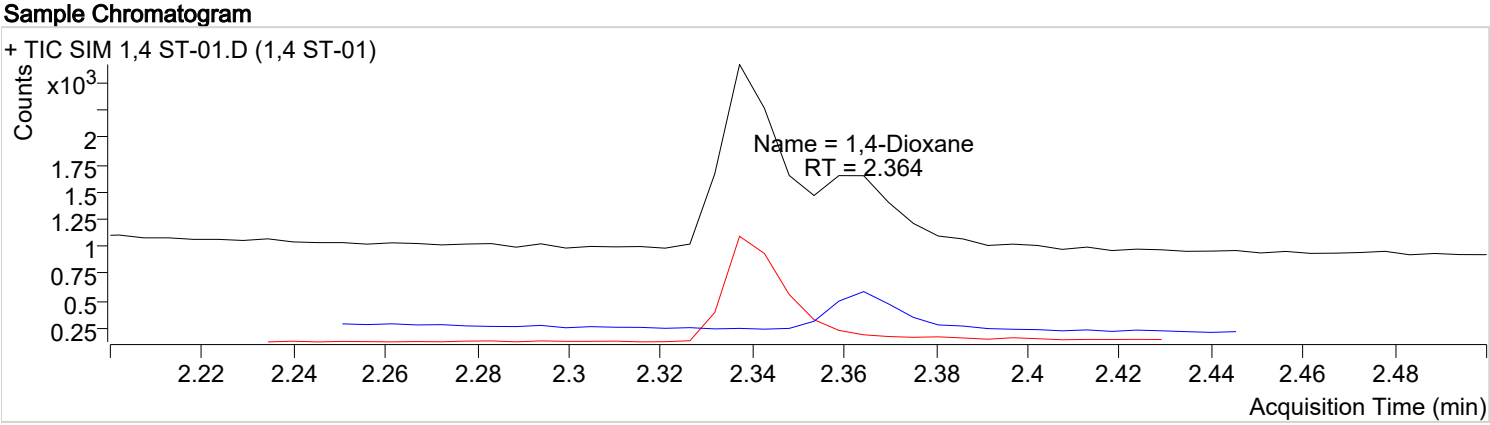

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.364	637	1615	0.009 mg/L

1,4-Dioxane

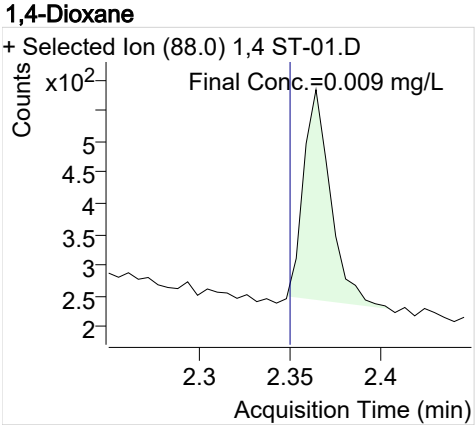

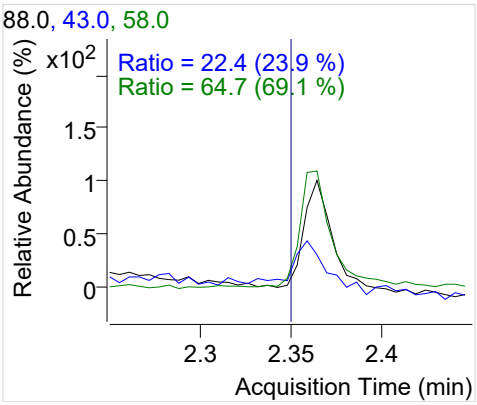

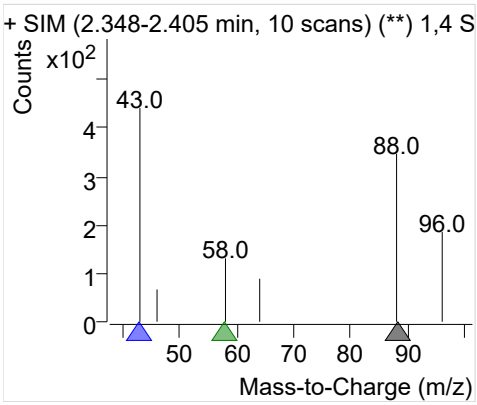

Generated at 오전 10:02 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-31 오후 1:50:58	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:02:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:50:58	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 4:03:04	**Data File**	1,4 ST-02.D
Type	Cal	**Name**	1,4 ST-02
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

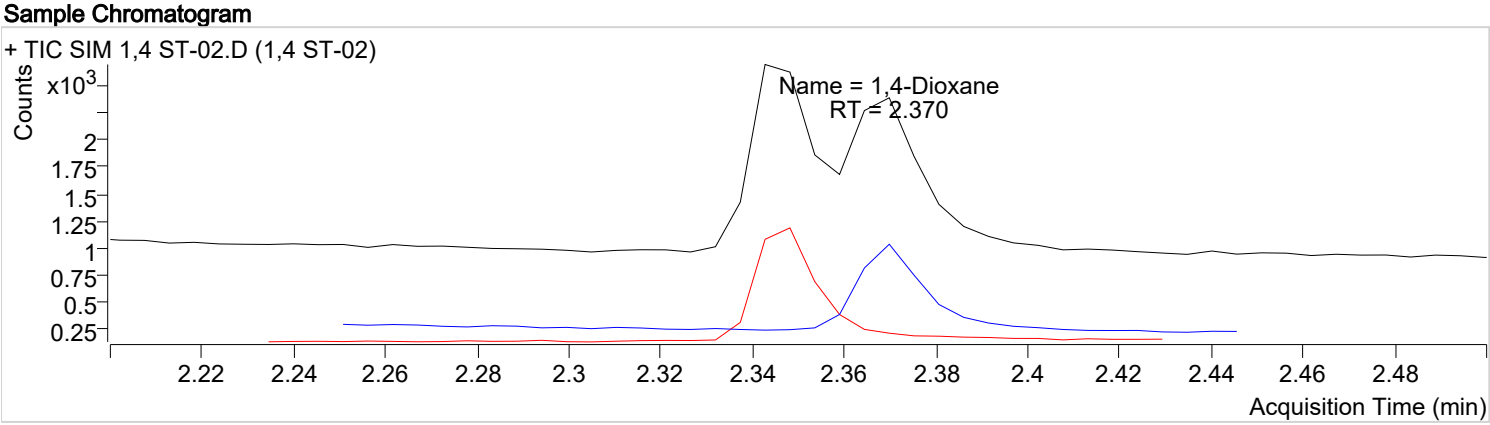

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.370	1430	1828	0.019 mg/L

1,4-Dioxane

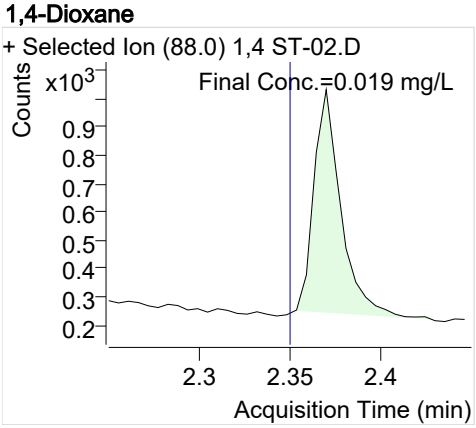

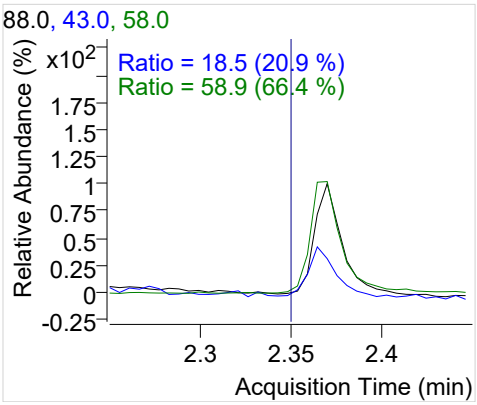

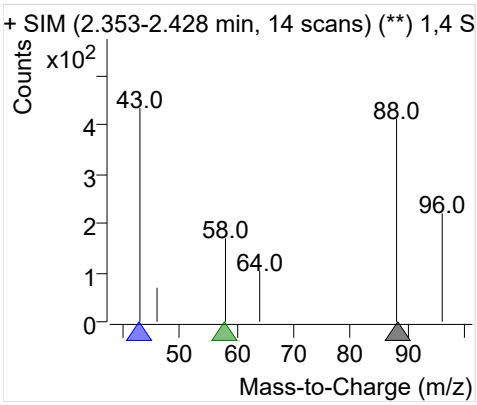

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-31 오후 1:50:58	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:02:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:50:58	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 4:12:05	**Data File**	1,4 ST-03.D
Type	Cal	**Name**	1,4 ST-03
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

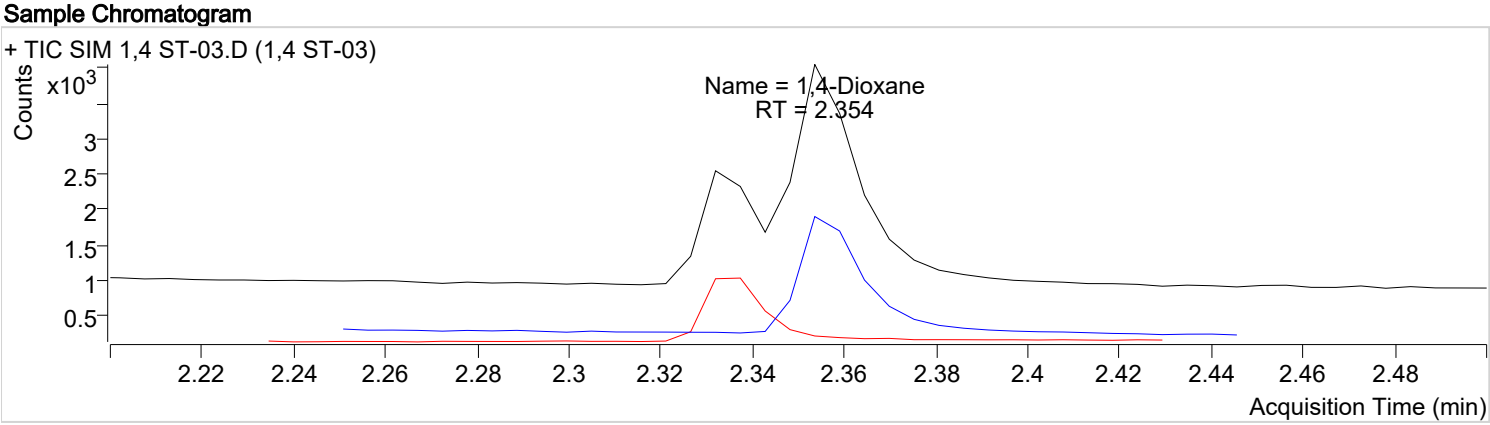

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.354	3002	1462	0.051 mg/L

1,4-Dioxane

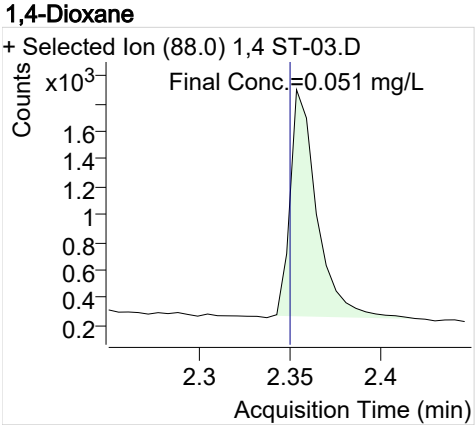





Generated at 오전 10:02 on 2026-04-10

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-31 오후 1:50:58	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:02:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:50:58	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 4:21:02	**Data File**	1,4 ST-04.D
Type	Cal	**Name**	1,4 ST-04
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

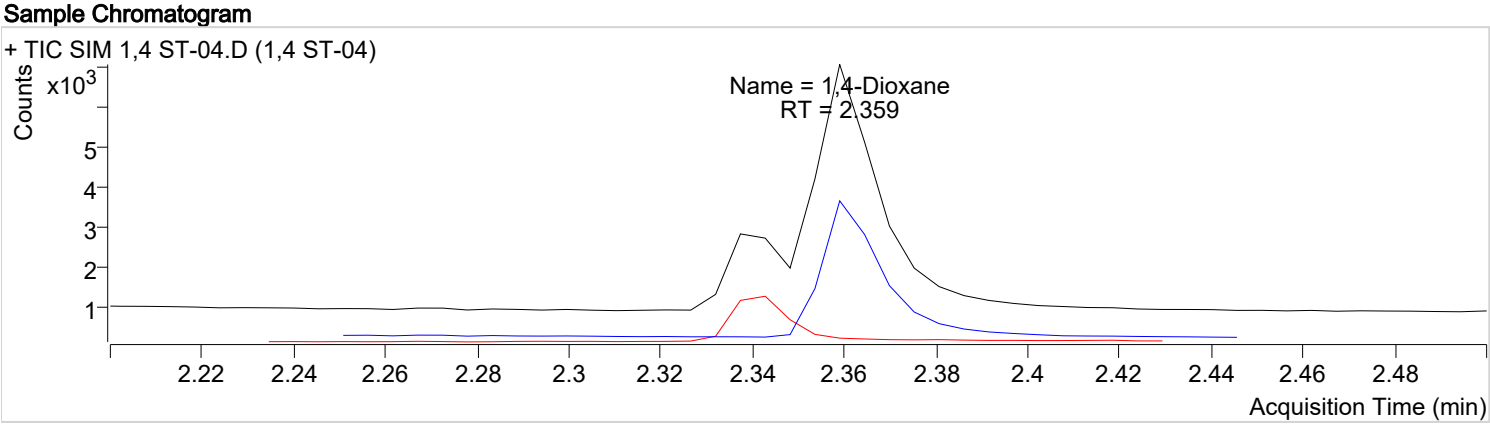

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.359	5787	1795	0.081 mg/L

1,4-Dioxane

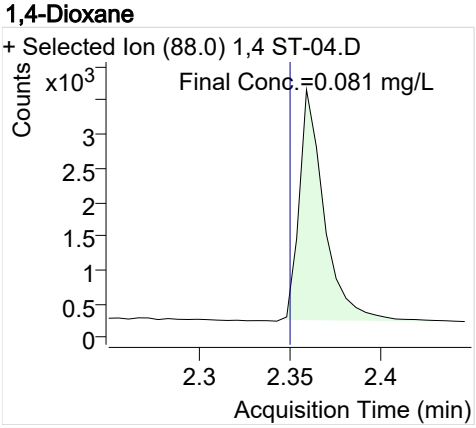

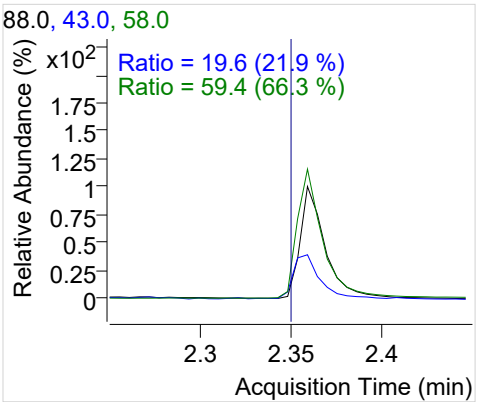

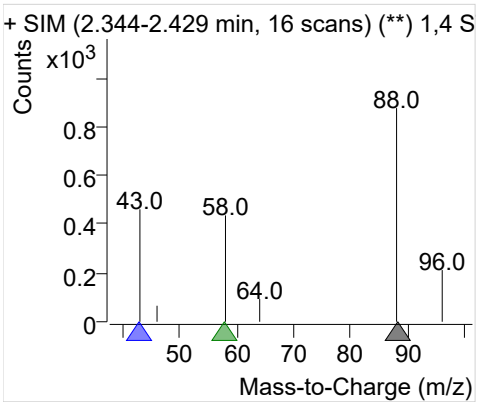

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-31 오후 1:50:58	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:02:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:50:58	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 4:30:03	**Data File**	1,4 ST-05.D
Type	Cal	**Name**	1,4 ST-05
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

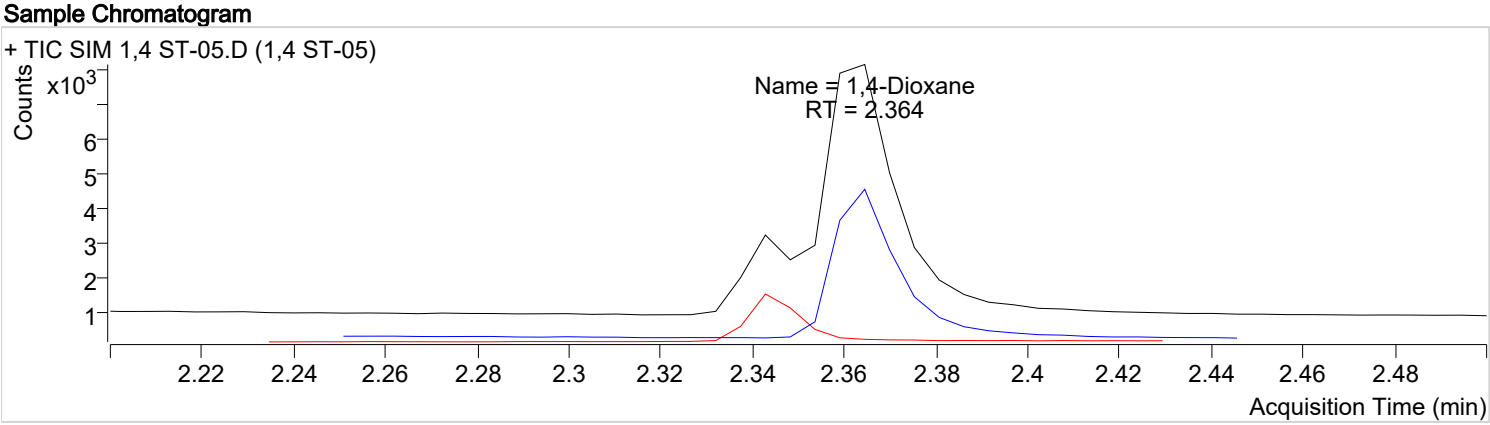

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.364	7819	1914	0.103 mg/L

1,4-Dioxane

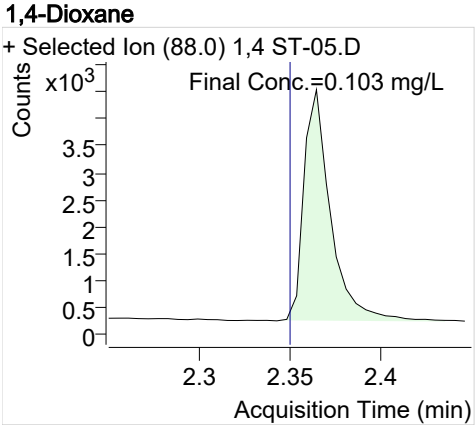





Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-31 오후 1:50:58	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:02:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:50:58	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 4:39:01	**Data File**	1,4 ST-06.D
Type	Cal	**Name**	1,4 ST-06
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

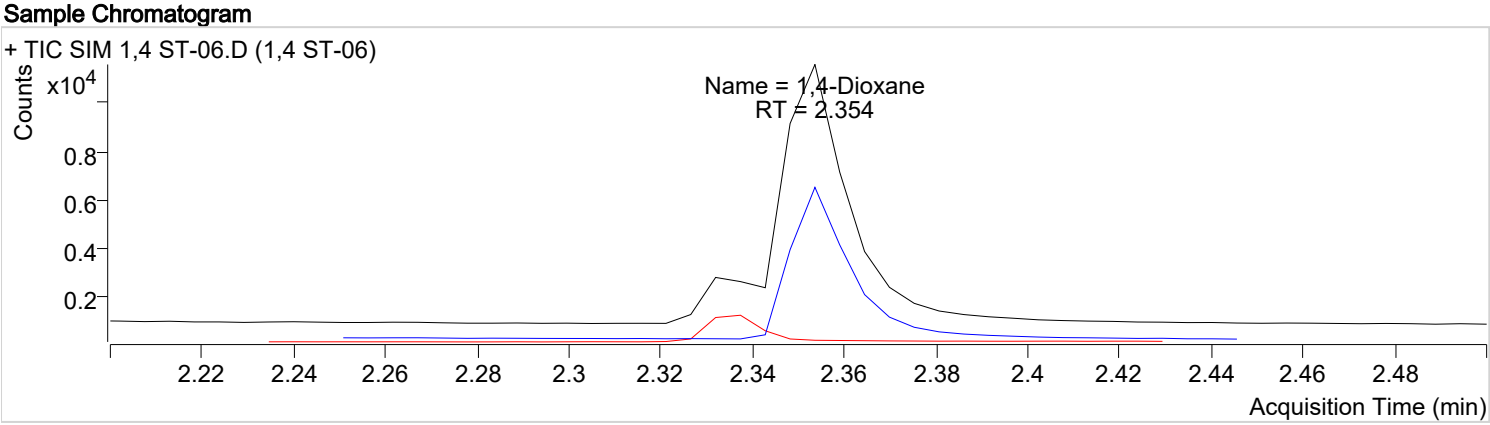

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.354	10533	1655	0.160 mg/L

1,4-Dioxane

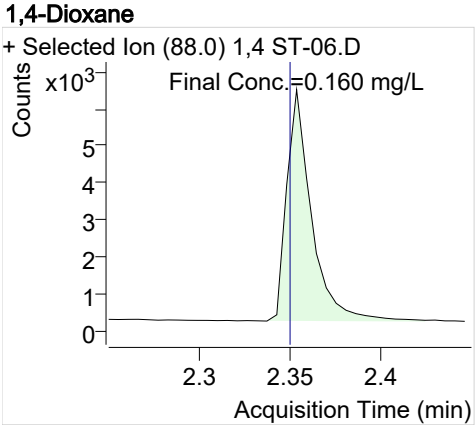

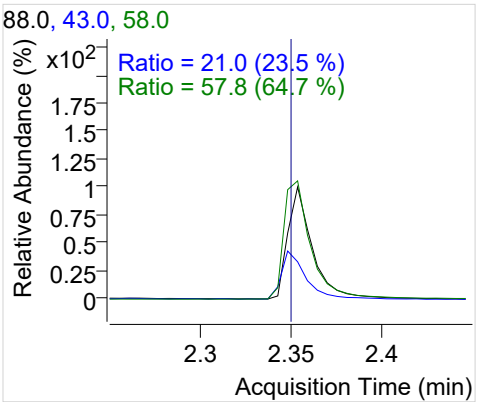

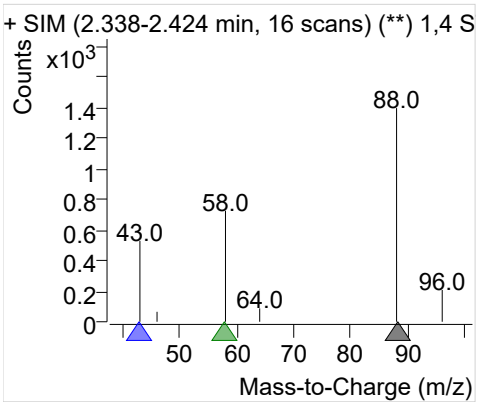

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-31 오후 1:50:58	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:02:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:50:58	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 4:48:01	**Data File**	1,4 ST-07.D
Type	Cal	**Name**	1,4 ST-07
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

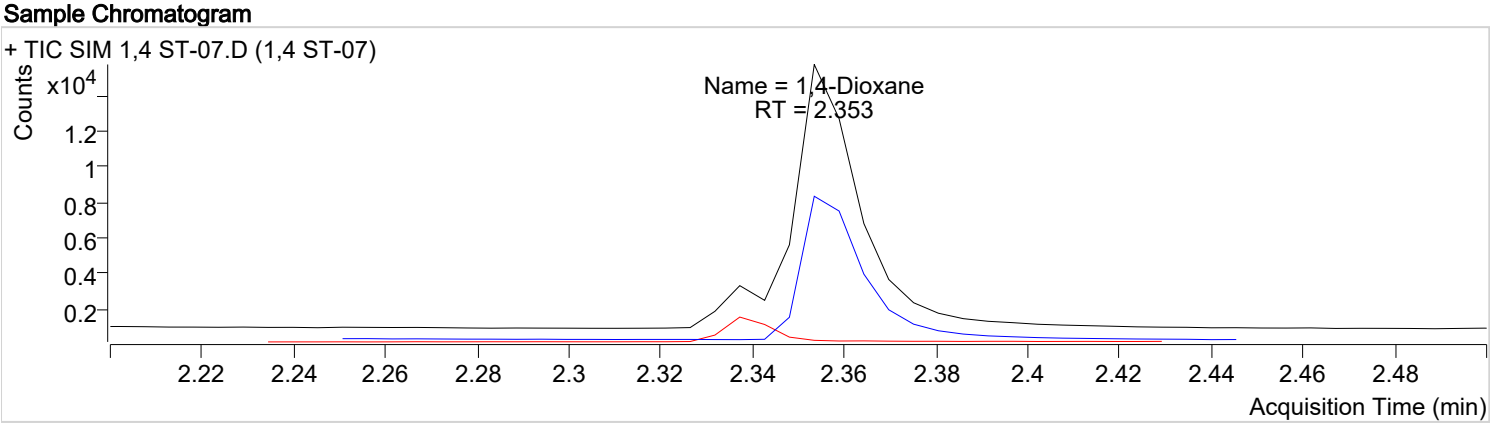

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.353	13797	1759	0.198 mg/L

1,4-Dioxane

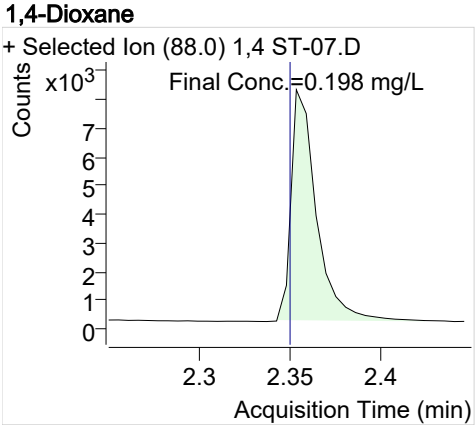





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-31 오후 1:50:58	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:02:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:50:58	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 5:05:59	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

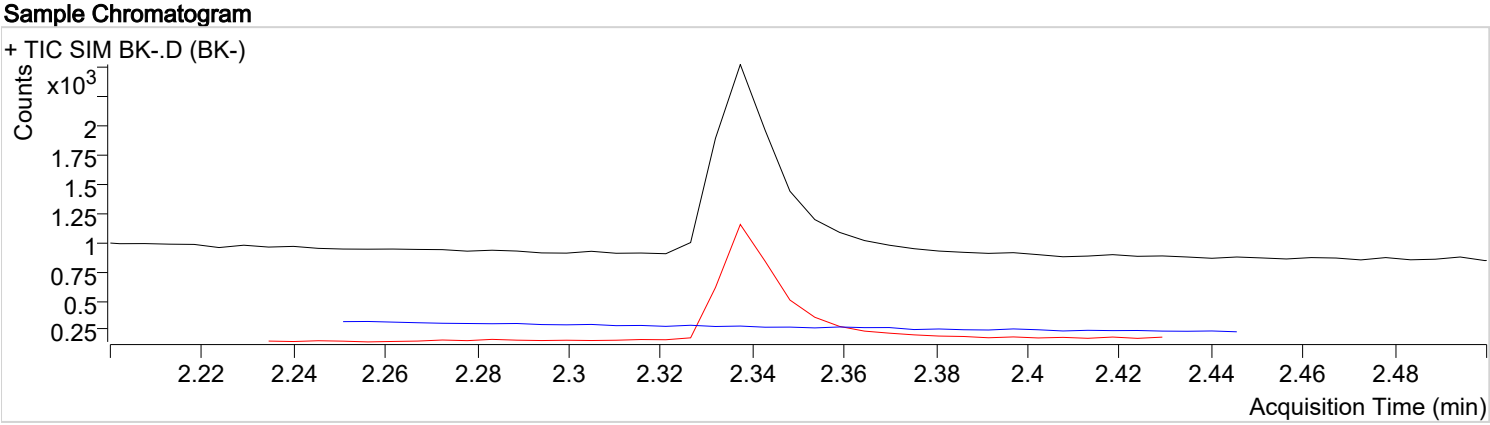

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1667	ND mg/L

1,4-Dioxane

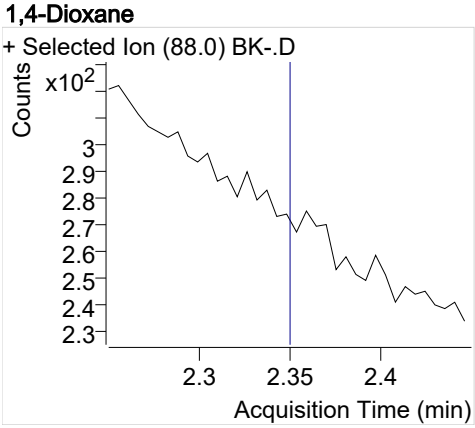



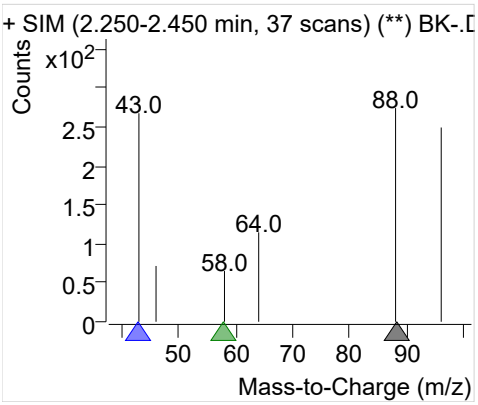

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-31 오후 1:50:58	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:02:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:50:58	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 5:14:59	**Data File**	FBK(LG NJ 26-03-26).D
Type	Blank	**Name**	FBK(LG NJ 26-03-26)
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

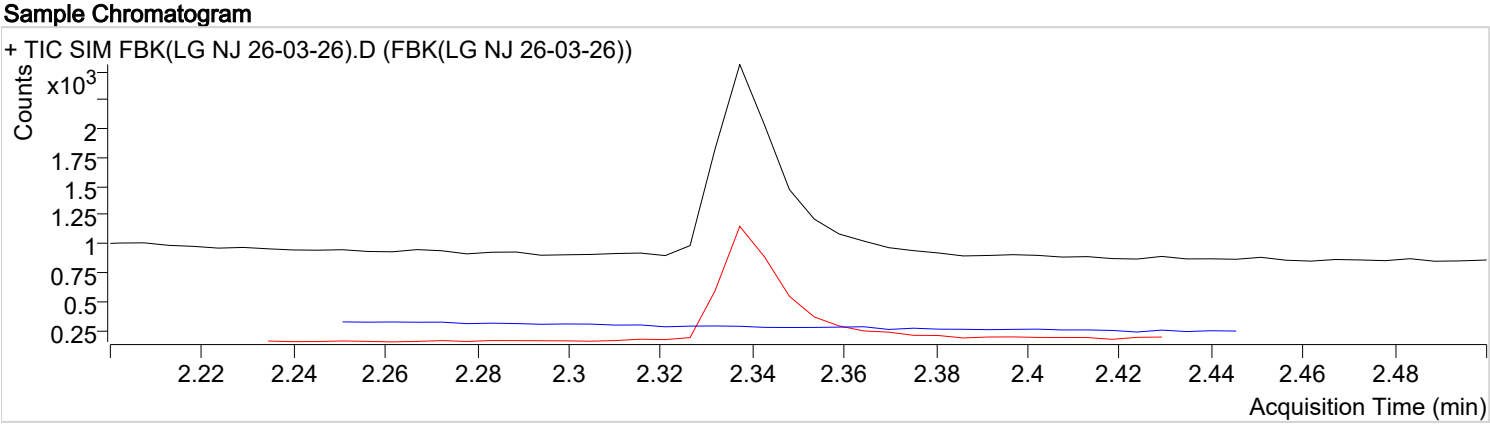

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1690	ND mg/L

1,4-Dioxane

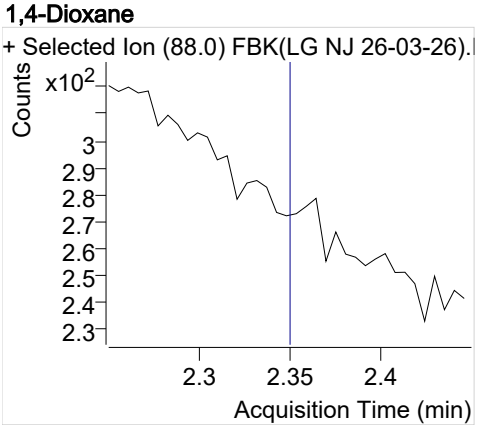



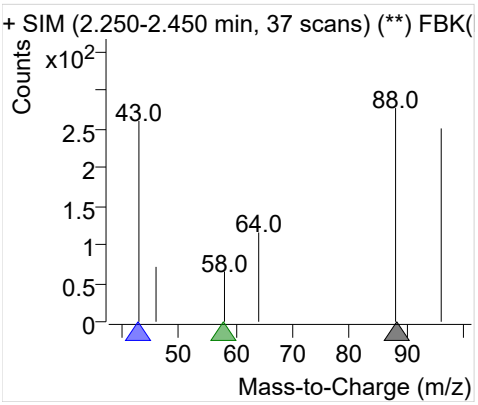

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-31 오후 1:50:58	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:02:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:50:58	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 5:23:57	**Data File**	LG NJ-01.D
Type	Sample	**Name**	LG NJ-01
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

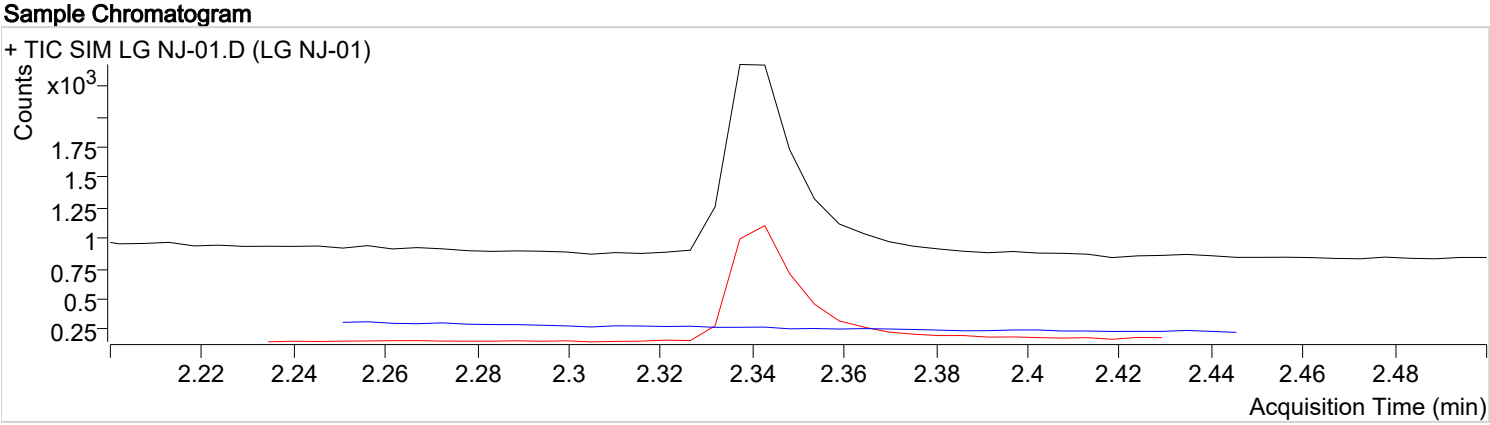

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1752	ND mg/L

1,4-Dioxane

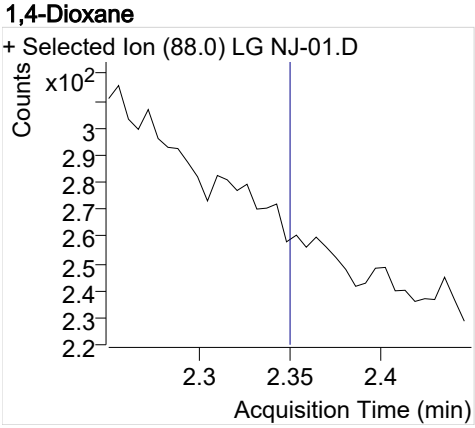





Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-31 오후 1:50:58	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:02:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:50:58	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 5:32:54	**Data File**	LG NJ-02.D
Type	Sample	**Name**	LG NJ-02
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

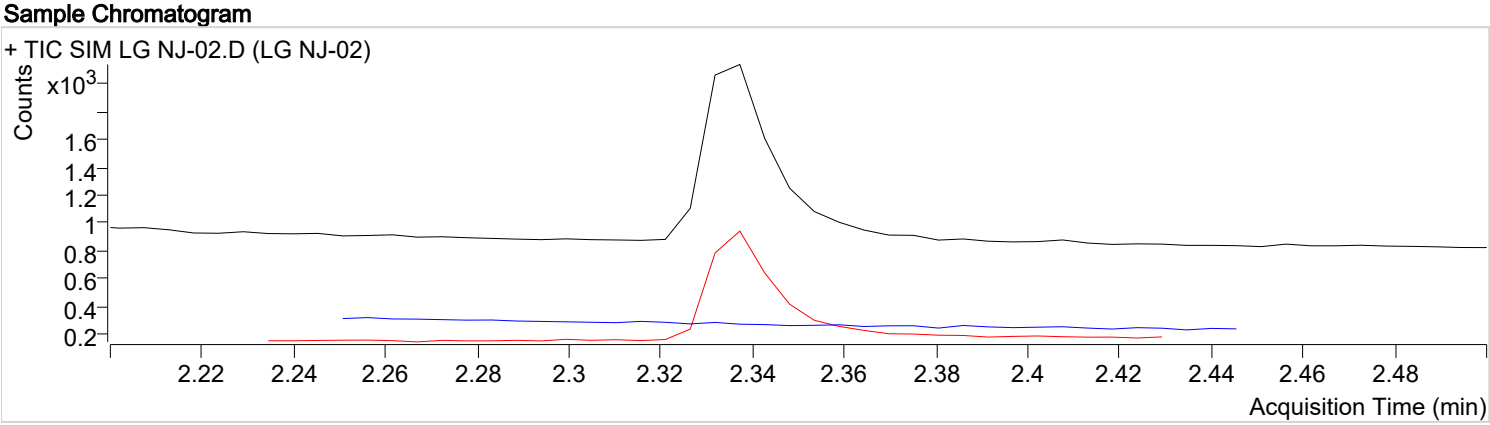

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1450	ND mg/L

1,4-Dioxane

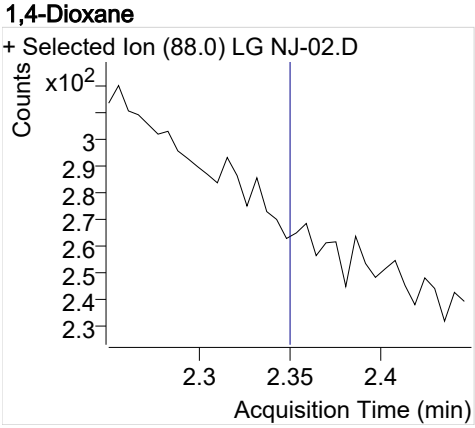





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-31 오후 1:50:58	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:02:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:50:58	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 5:41:54	**Data File**	LG NJ-03.D
Type	Sample	**Name**	LG NJ-03
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

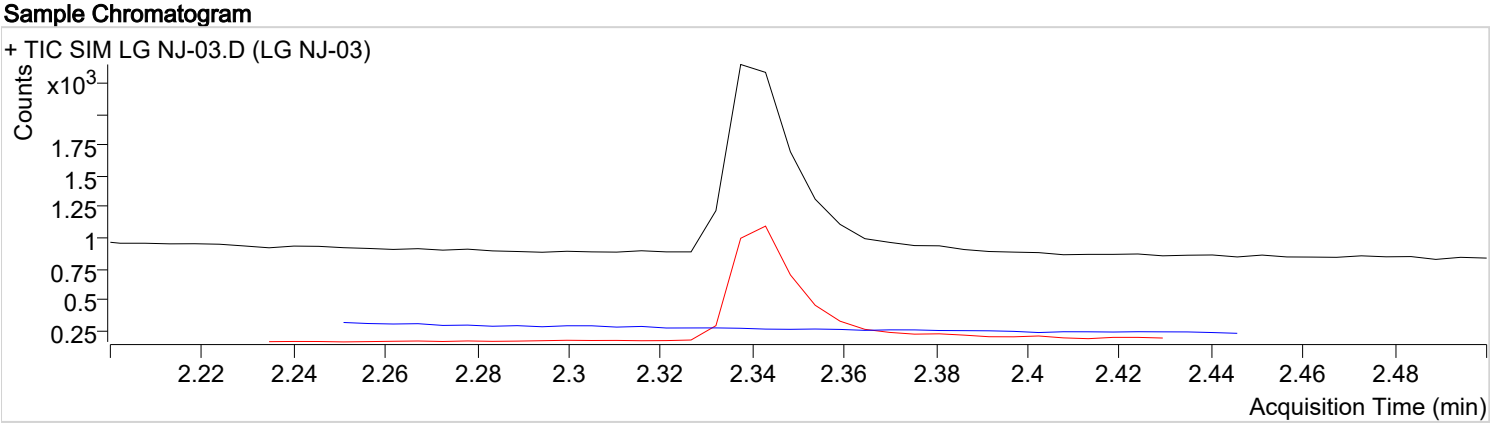

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1683	ND mg/L

1,4-Dioxane

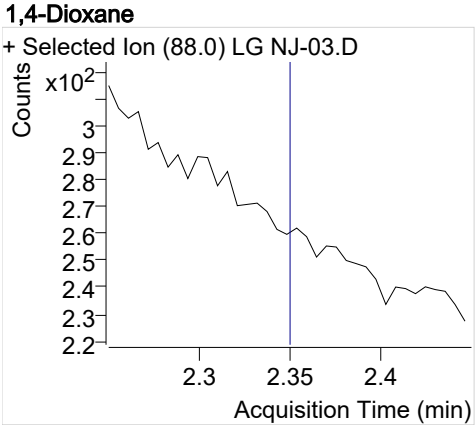





Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-31 오후 1:50:58	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:02:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:50:58	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 5:50:53	**Data File**	LG NJ-04.D
Type	Sample	**Name**	LG NJ-04
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

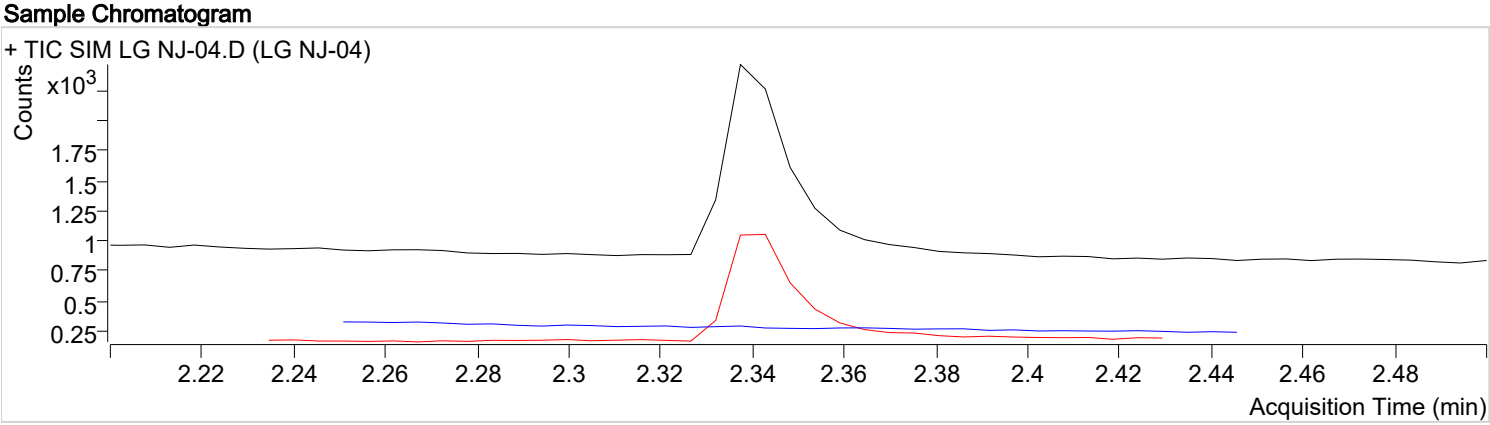

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1648	ND mg/L

1,4-Dioxane

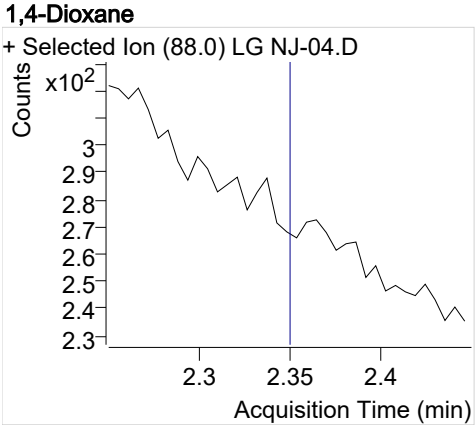





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-31 오후 1:50:58	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:02:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:50:58	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 5:59:52	**Data File**	LG NJ-05.D
Type	Sample	**Name**	LG NJ-05
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

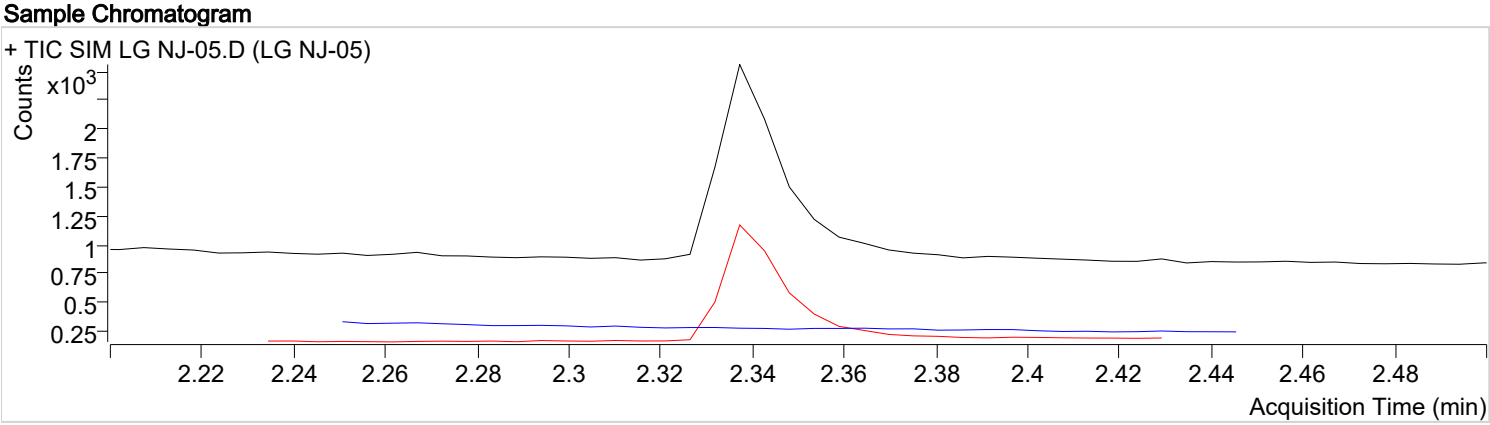

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1654	ND mg/L

1,4-Dioxane

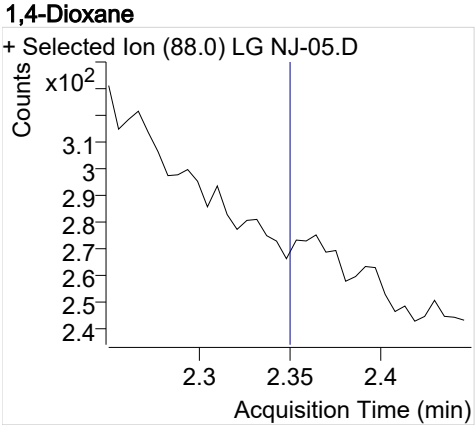





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-31 오후 1:50:58	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:02:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:50:58	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 6:08:51	**Data File**	LG NJ-06.D
Type	Sample	**Name**	LG NJ-06
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

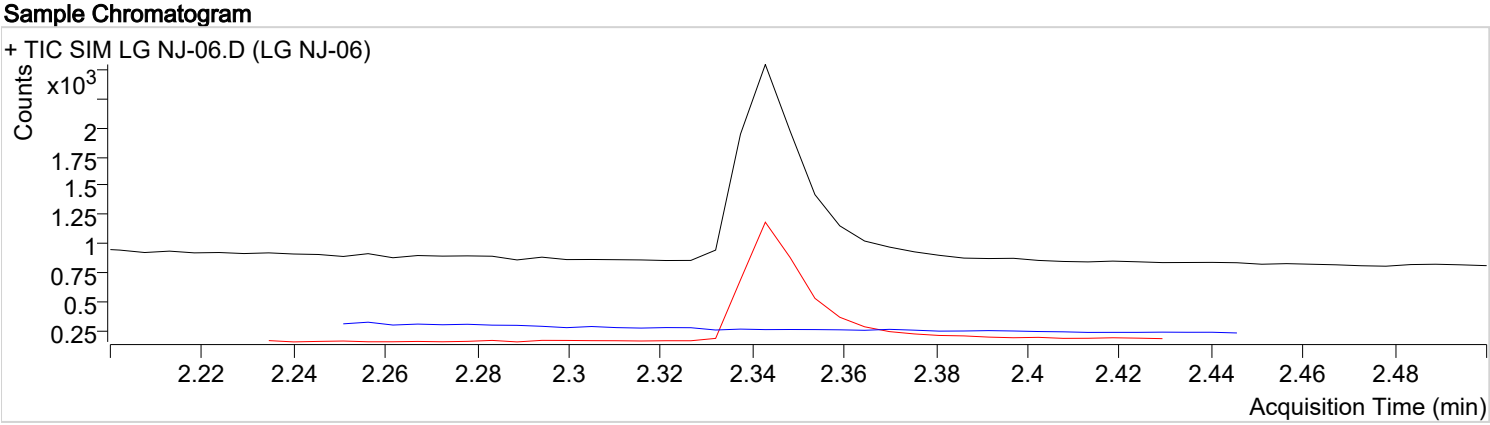

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1739	ND mg/L

1,4-Dioxane

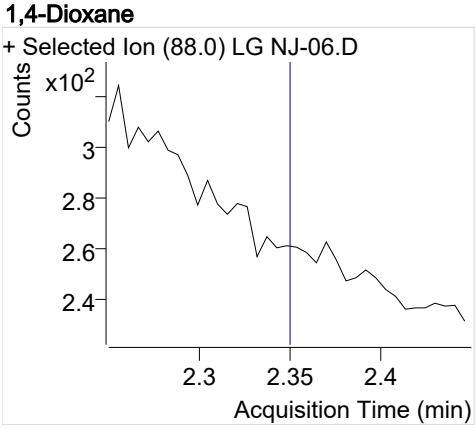





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-31 오후 1:50:58	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:02:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:50:58	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 6:17:51	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

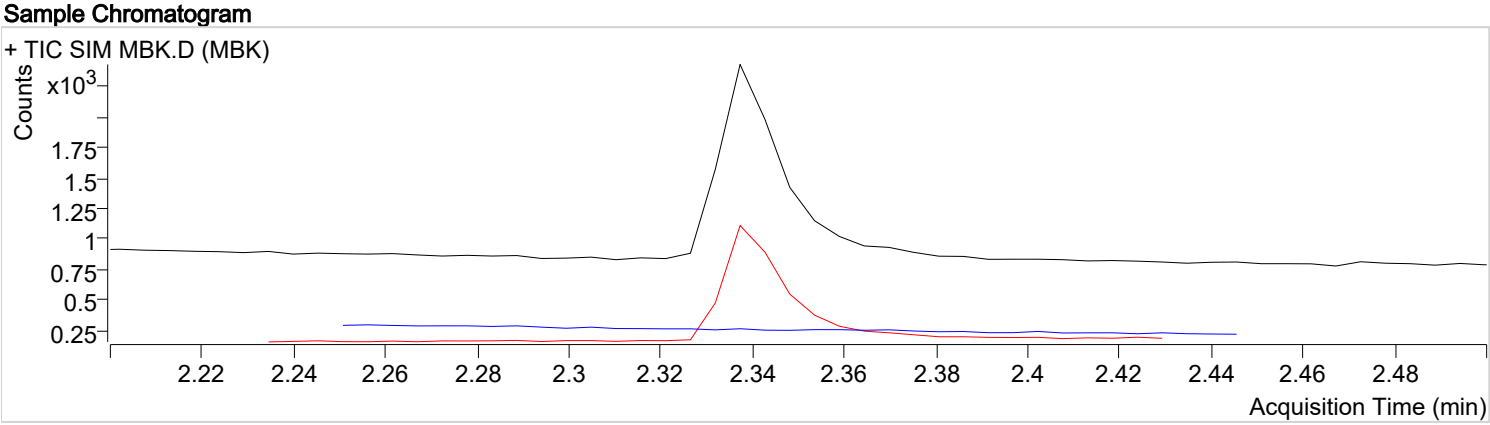

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane			1616	ND mg/L

1,4-Dioxane

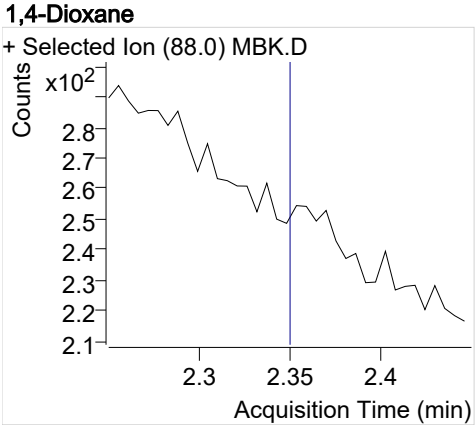



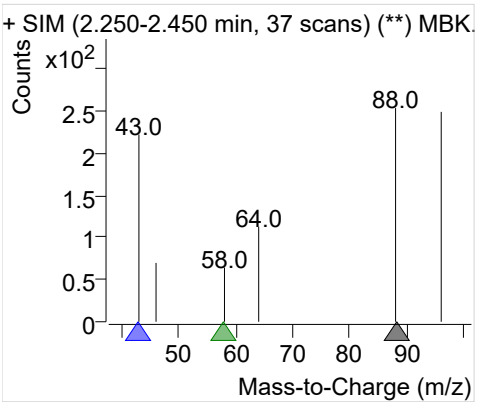

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\1,4(NJ 3.26) RE\QuantResults\1,4.batch.bin		
Analysis Time	2026-03-31 오후 1:50:58	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:02:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:50:58	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 6:35:45	**Data File**	-CCV-.D
Type	QC	**Name**	-CCV-
Dil.	0.05	**Acq. Method File**	VOCS(1,4)-LQ

Sample Chromatogram

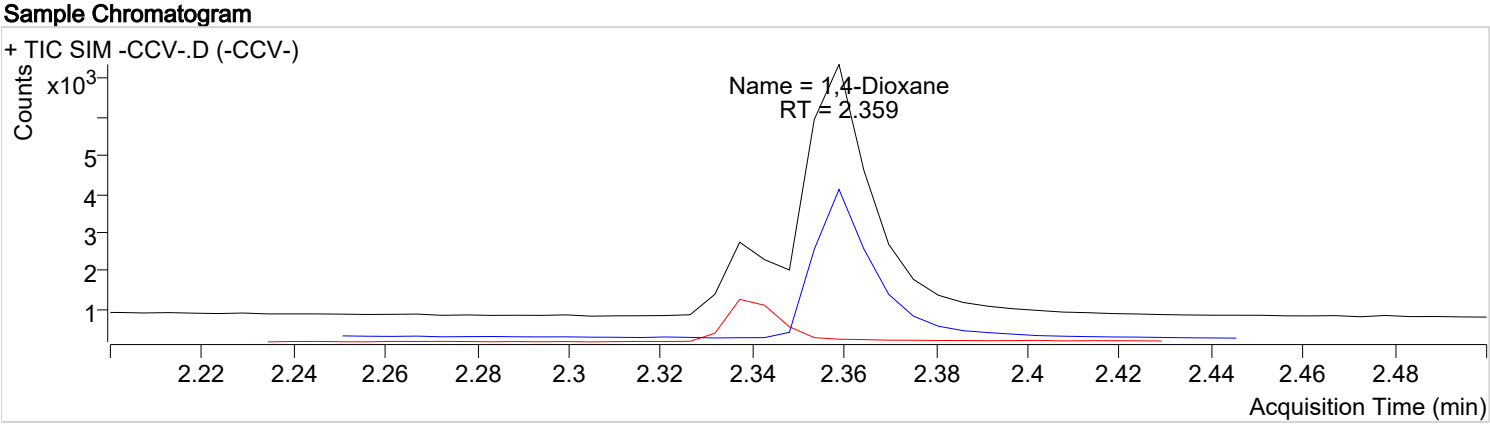

Name	RT	Resp.	ISTD Resp	Final Units Conc.
1,4-Dioxane	2.359	6488	1573	0.104 mg/L

1,4-Dioxane

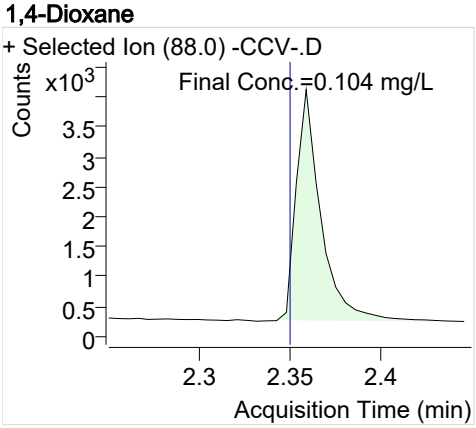



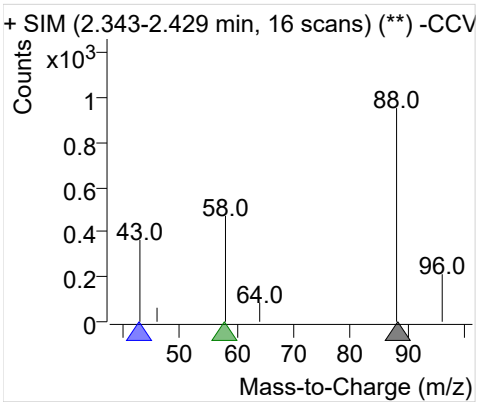

Generated at 오전 10:02 on 2026-04-10