Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(RE 3.11)\QuantResults\DEHA.batch.bin				
Analysis Time	2026-03-18 오후 12:47:49	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:47:49	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Di(2-ethylhexyl)adipate

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
DEHA ST-01.d	Cal	6.928	7077	110694	0.7180
DEHA ST-02.d	Cal	6.928	15416	112372	1.0962
DEHA ST-03.d	Cal	6.928	43619	121796	2.2368
DEHA ST-04.d	Cal	6.928	99640	116398	4.8073
DEHA ST-05.d	Cal	6.928	232521	123072	10.1416
BK-.d	Blank			116363	ND
FBK(RE 26-03-11).d	Blank			116832	ND
RE-07.d	Sample			118472	ND
RE-08.d	Sample			105546	ND
RE-17.d	Sample			113083	ND
RE-18.d	Sample			105607	ND
RE-19.d	Sample			129891	ND
RE-20.d	Sample			111374	ND
RE-21.d	Sample			98116	ND
RE-22.d	Sample			112675	ND
RE-23.d	Sample			116034	ND
MBK.d	Blank			129719	ND
CCV.d	QC	6.934	79978	111240	4.0997

Di(2-ethylhexyl)adipate

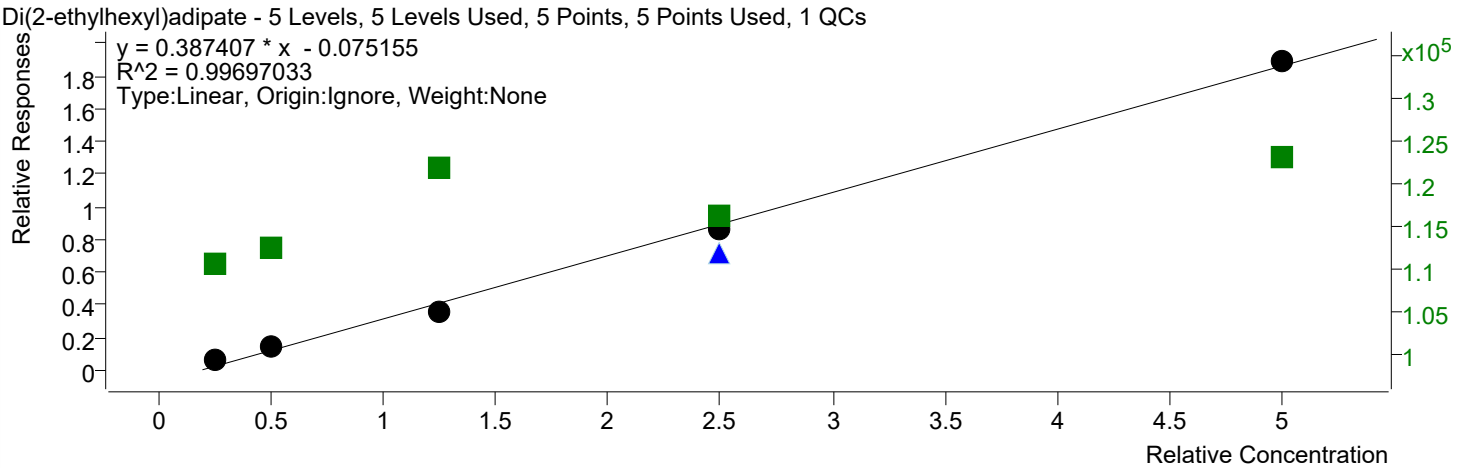

Cal. Path	Type	Level	Enable	Conc.	Response
V:\2026\2026-03\DEHA(RE 3.11)\DEHA ST-01.d	Calibration	1	x	0.500	7077
V:\2026\2026-03\DEHA(RE 3.11)\DEHA ST-02.d	Calibration	2	x	1.000	15416
V:\2026\2026-03\DEHA(RE 3.11)\DEHA ST-03.d	Calibration	3	x	2.500	43619
V:\2026\2026-03\DEHA(RE 3.11)\DEHA ST-04.d	Calibration	4	x	5.000	99640
V:\2026\2026-03\DEHA(RE 3.11)\CCV.d	QC	4	x	5.000	79978
V:\2026\2026-03\DEHA(RE 3.11)\DEHA ST-05.d	Calibration	5	x	10.000	232521

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(RE 3.11)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-03-18 오후 12:47:49	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:08:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:47:49	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 3:00:48	**Data File**	DEHA ST-01.d
Type	Cal	**Name**	DEHA ST-01
Dil.	1	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

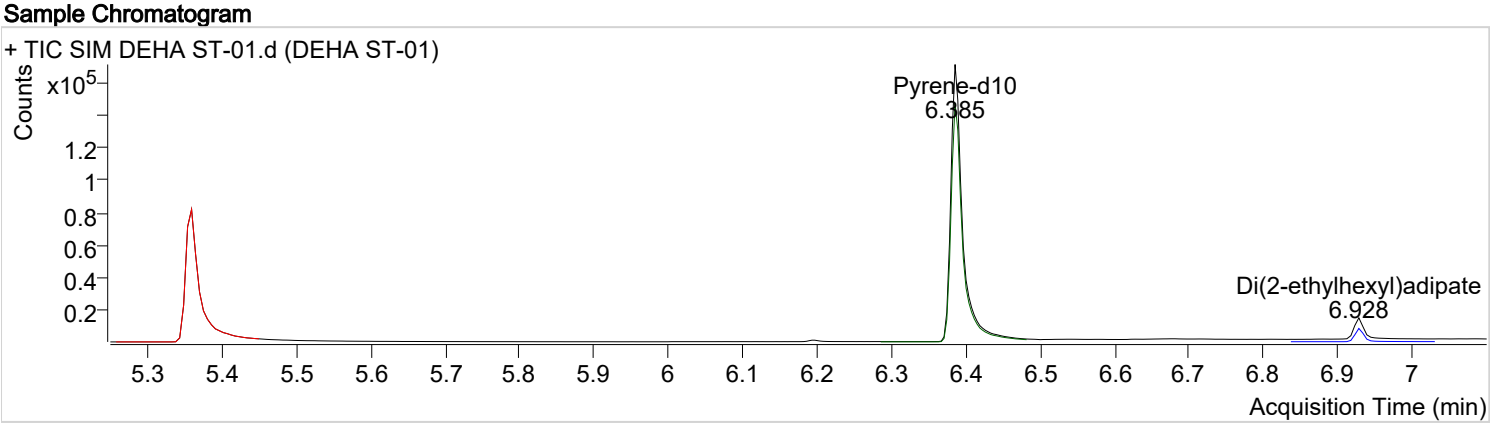

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate	6.928	7077	110694	0.7180 mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(RE 3.11)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-03-18 오후 12:47:49	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:08:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:47:49	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 3:11:24	**Data File**	DEHA ST-02.d
Type	Cal	**Name**	DEHA ST-02
Dil.	1	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

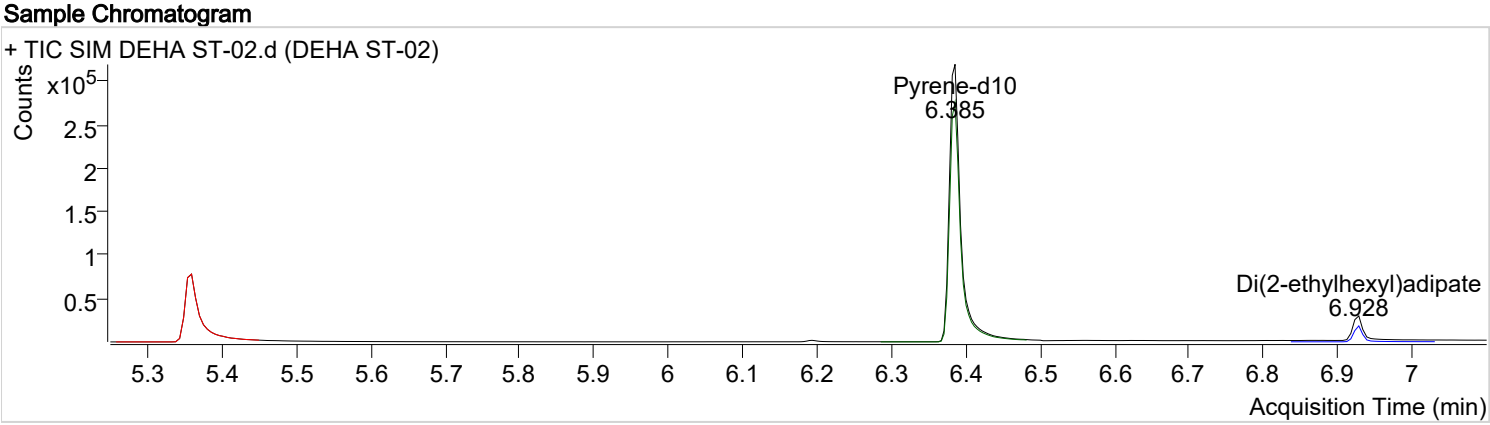

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate	6.928	15416	112372	1.0962 mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(RE 3.11)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-03-18 오후 12:47:49	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:08:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:47:49	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 3:21:58	**Data File**	DEHA ST-03.d
Type	Cal	**Name**	DEHA ST-03
Dil.	1	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

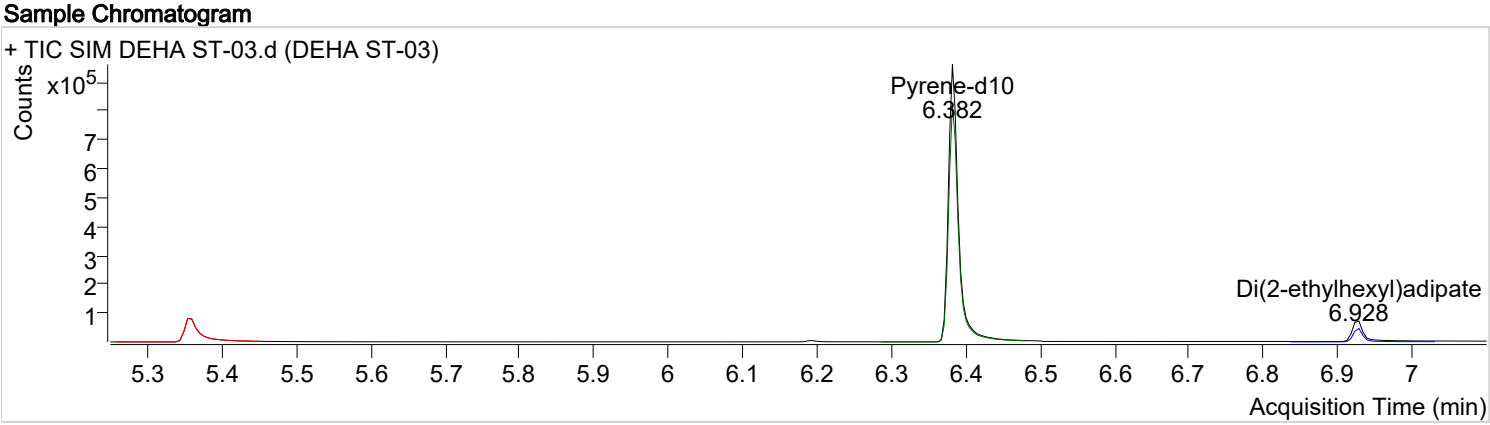

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate	6.928	43619	121796	2.2368 mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Batch Data Path	V:\2026\2026-03\DEHA(RE 3.11)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-03-18 오후 12:47:49	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:08:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:47:49	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 3:32:33	**Data File**	DEHA ST-04.d
Type	Cal	**Name**	DEHA ST-04
Dil.	1	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

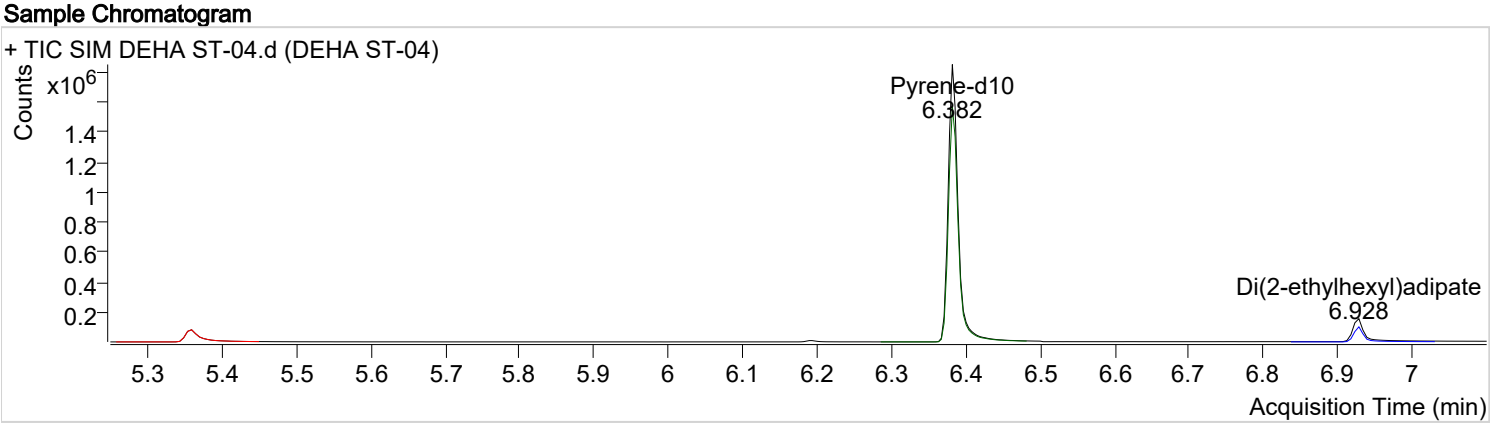

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate	6.928	99640	116398	4.8073 mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(RE 3.11)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-03-18 오후 12:47:49	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:08:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:47:49	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 3:43:11	**Data File**	DEHA ST-05.d
Type	Cal	**Name**	DEHA ST-05
Dil.	1	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

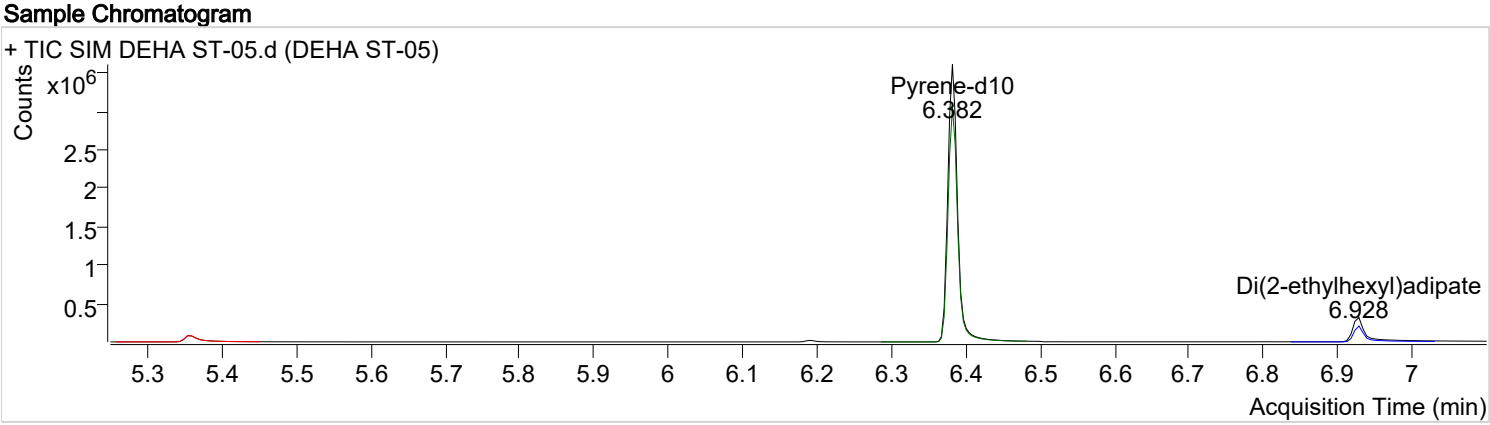

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate	6.928	232521	123072	10.1416 mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(RE 3.11)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-03-18 오후 12:47:49	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:08:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:47:49	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 4:04:30	**Data File**	BK-.d
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

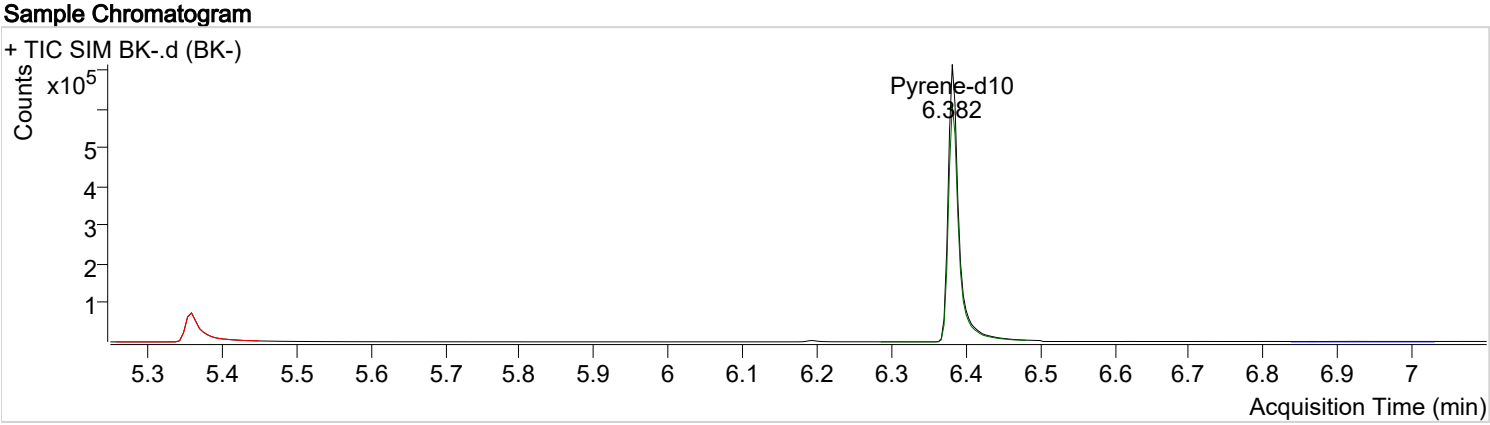

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			116363	ND mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(RE 3.11)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-03-18 오후 12:47:49	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:08:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:47:49	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 4:15:07	**Data File**	FBK(RE 26-03-11).d
Type	Blank	**Name**	FBK(RE 26-03-11)
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

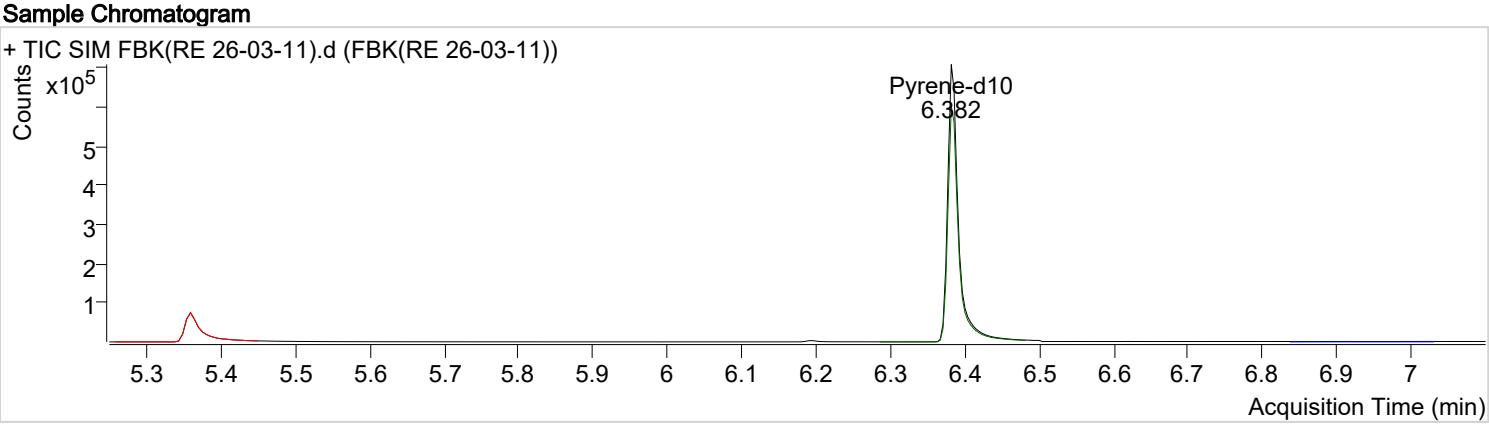

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			116832	ND mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Batch Data Path	V:\2026\2026-03\DEHA(RE 3.11)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-03-18 오후 12:47:49	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:08:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:47:49	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 4:25:45	**Data File**	RE-07.d
Type	Sample	**Name**	RE-07
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

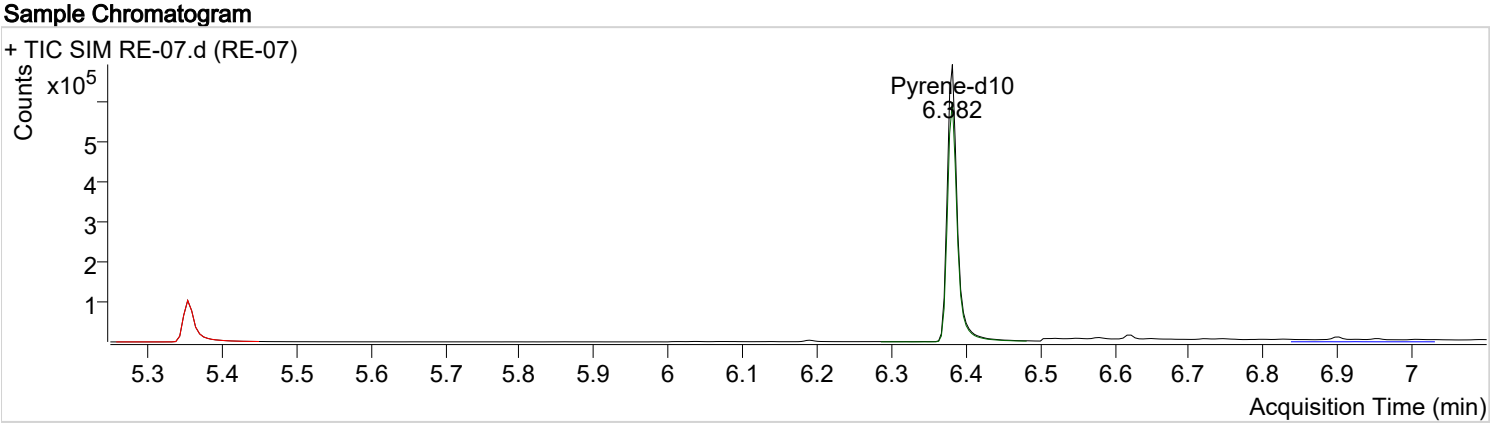

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			118472	ND mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Batch Data Path	V:\2026\2026-03\DEHA(RE 3.11)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-03-18 오후 12:47:49	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:08:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:47:49	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 4:36:23	**Data File**	RE-08.d
Type	Sample	**Name**	RE-08
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

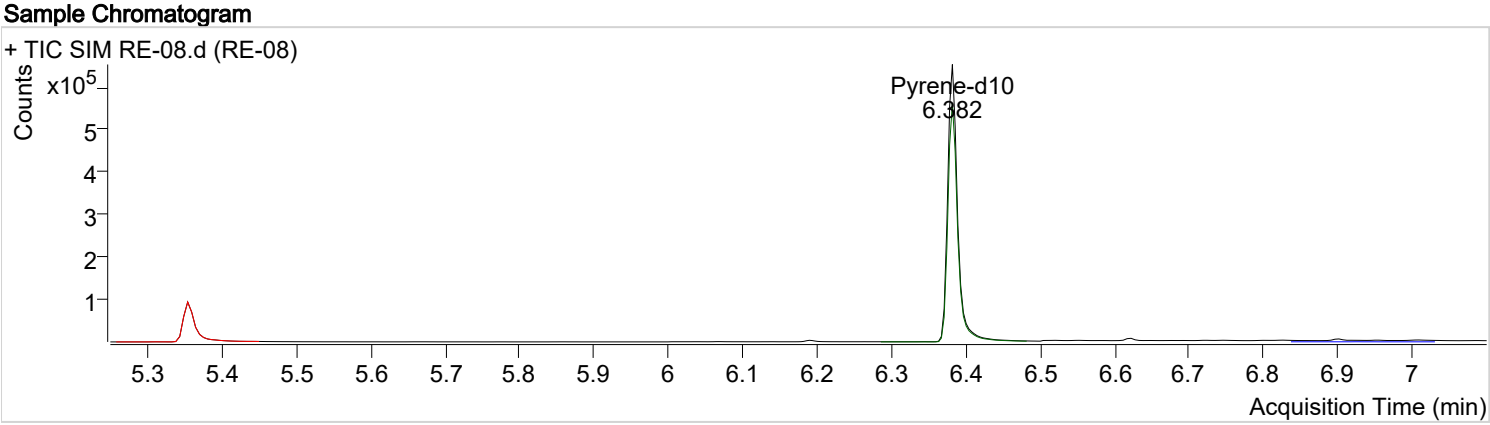

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			105546	ND mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Batch Data Path	V:\2026\2026-03\DEHA(RE 3.11)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-03-18 오후 12:47:49	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:08:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:47:49	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 4:46:59	**Data File**	RE-17.d
Type	Sample	**Name**	RE-17
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

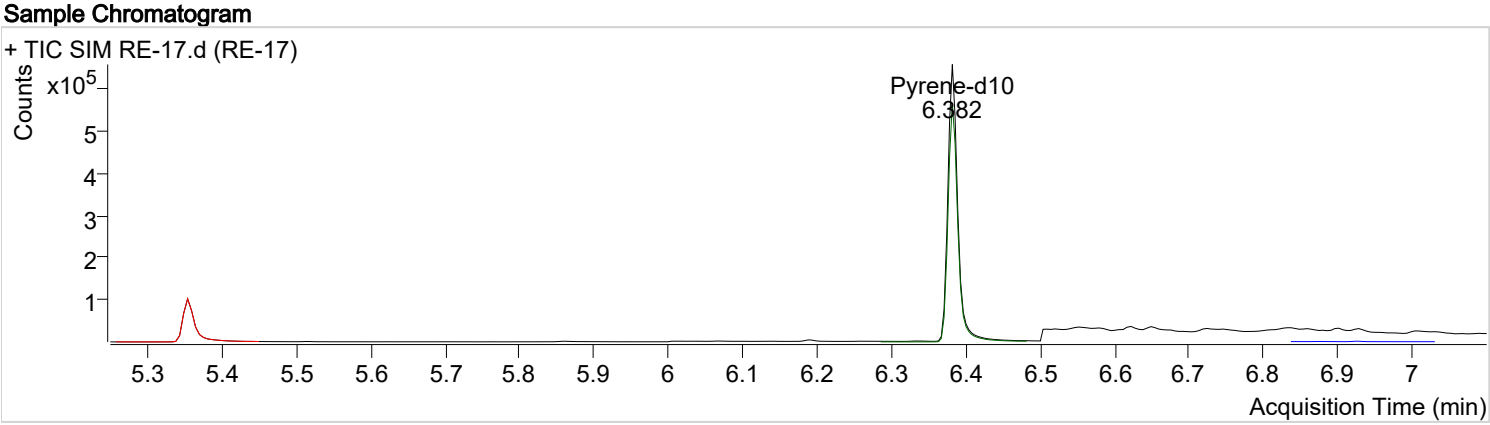

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			113083	ND mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(RE 3.11)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-03-18 오후 12:47:49	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:08:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:47:49	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 4:57:39	**Data File**	RE-18.d
Type	Sample	**Name**	RE-18
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

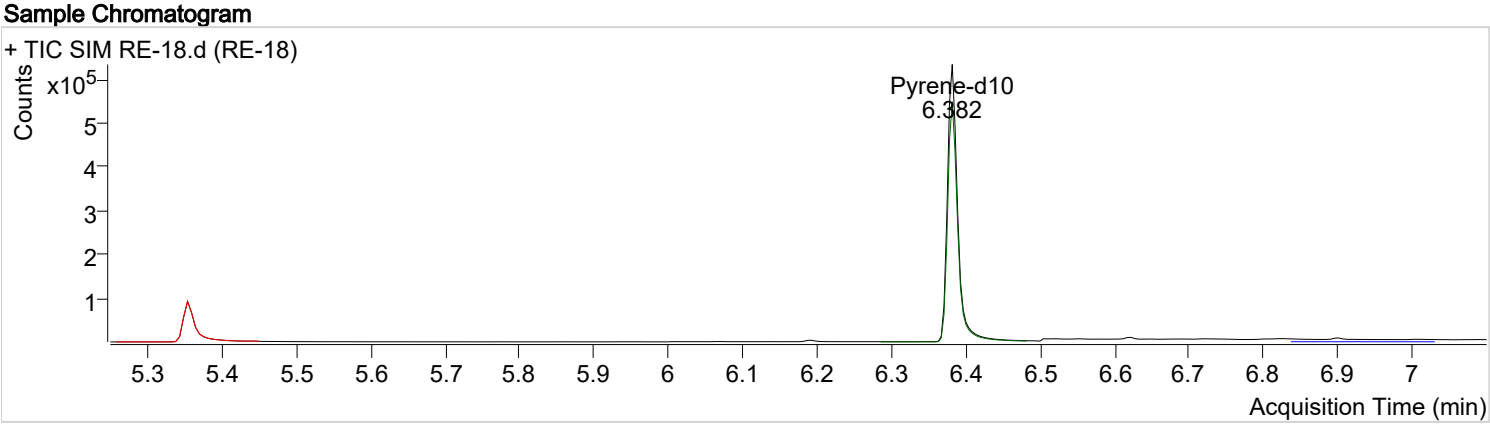

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			105607	ND mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Batch Data Path	V:\2026\2026-03\DEHA(RE 3.11)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-03-18 오후 12:47:49	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:08:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:47:49	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 5:08:20	**Data File**	RE-19.d
Type	Sample	**Name**	RE-19
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

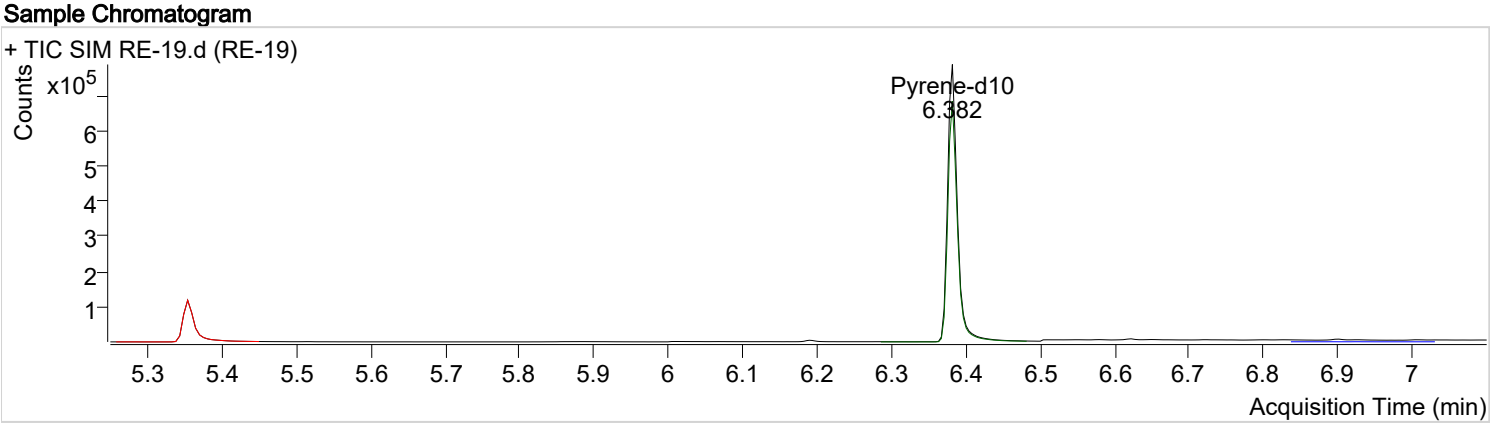

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			129891	ND mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(RE 3.11)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-03-18 오후 12:47:49	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:08:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:47:49	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 5:18:57	**Data File**	RE-20.d
Type	Sample	**Name**	RE-20
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

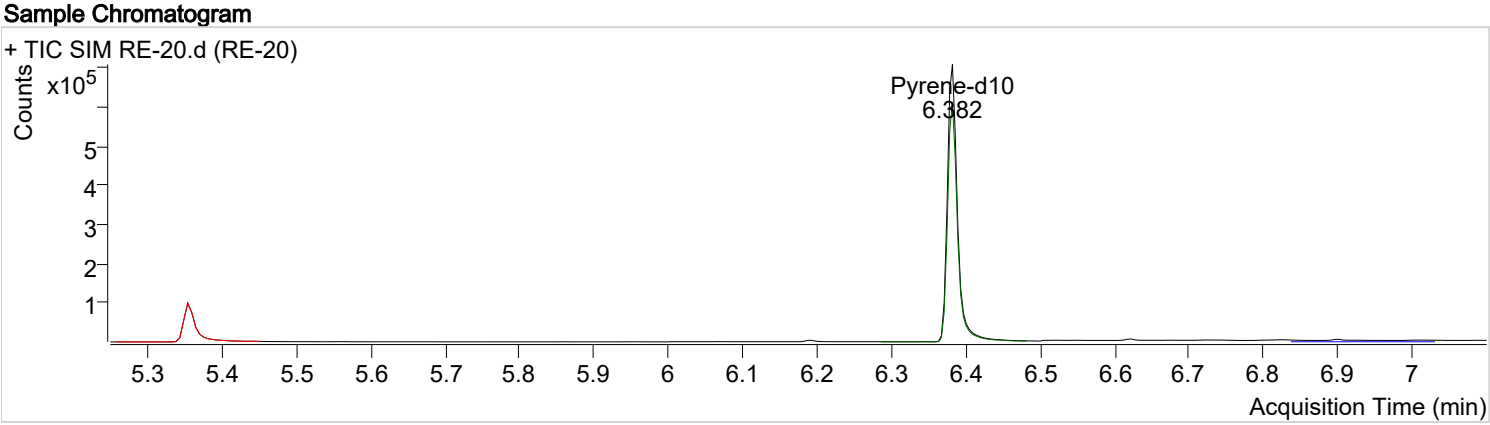

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			111374	ND mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(RE 3.11)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-03-18 오후 12:47:49	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:08:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:47:49	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 5:29:34	**Data File**	RE-21.d
Type	Sample	**Name**	RE-21
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

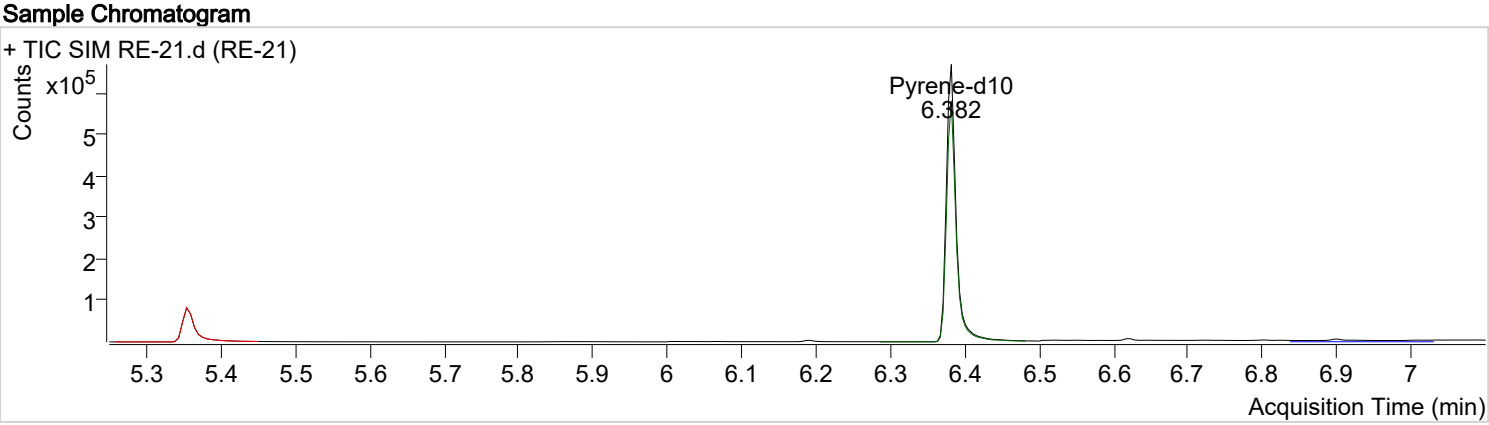

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			98116	ND mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Batch Data Path	V:\2026\2026-03\DEHA(RE 3.11)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-03-18 오후 12:47:49	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:08:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:47:49	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 5:40:14	**Data File**	RE-22.d
Type	Sample	**Name**	RE-22
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

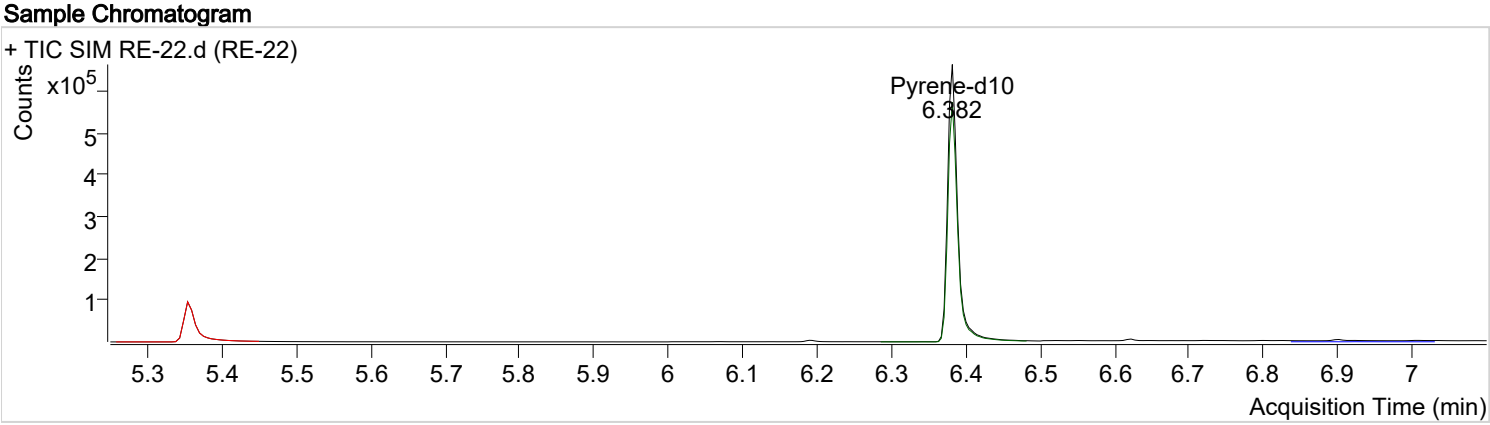

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			112675	ND mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Batch Data Path	V:\2026\2026-03\DEHA(RE 3.11)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-03-18 오후 12:47:49	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:08:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:47:49	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 5:50:53	**Data File**	RE-23.d
Type	Sample	**Name**	RE-23
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

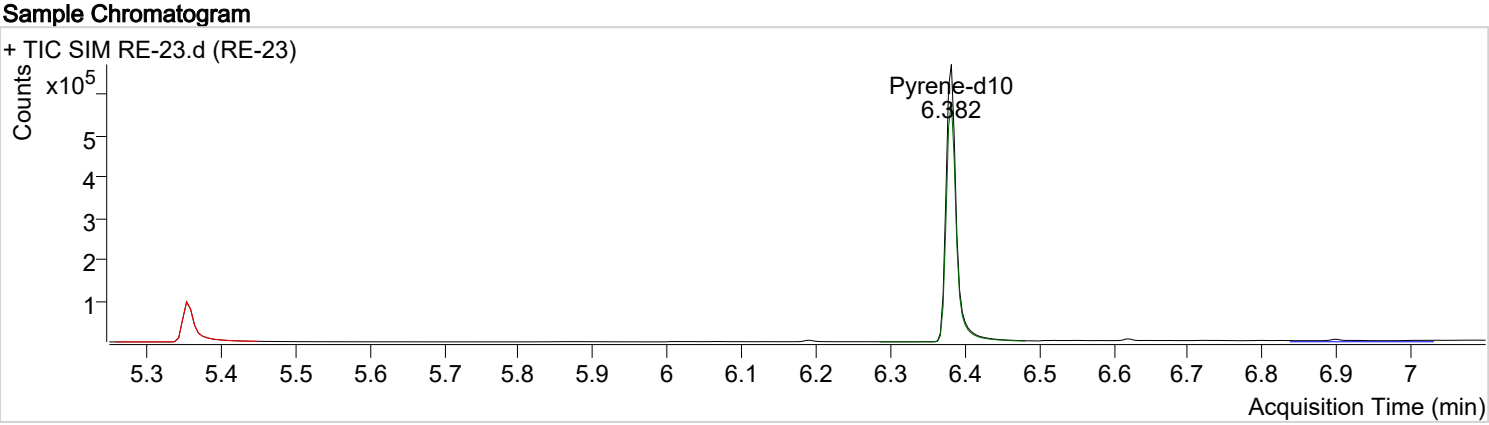

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			116034	ND mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(RE 3.11)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-03-18 오후 12:47:49	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:08:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:47:49	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 6:01:27	**Data File**	MBK.d
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

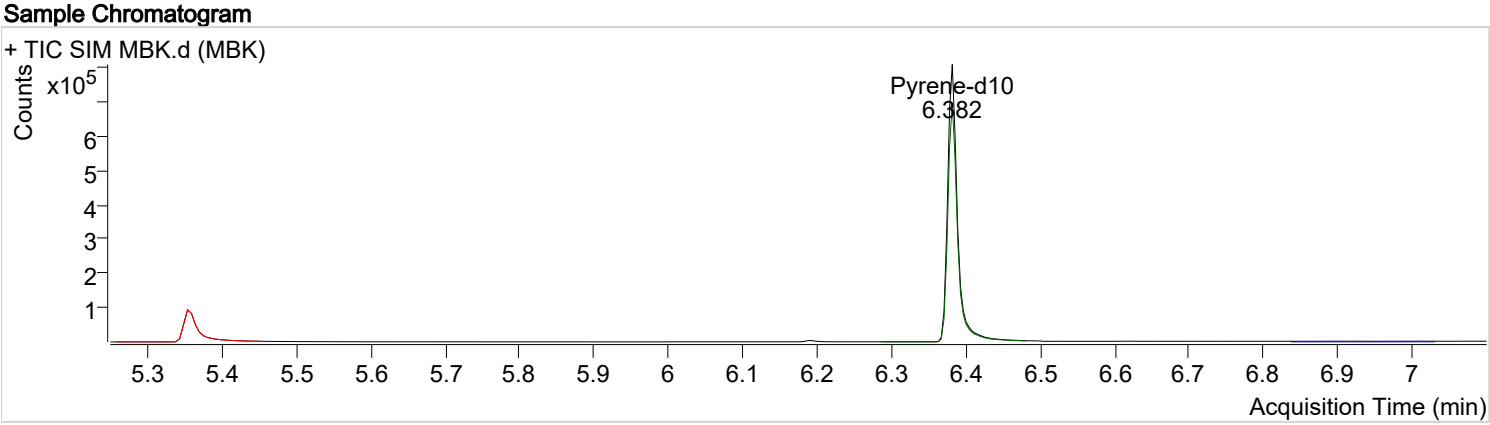

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			129719	ND mg/L

Di(2-ethylhexyl)adipate

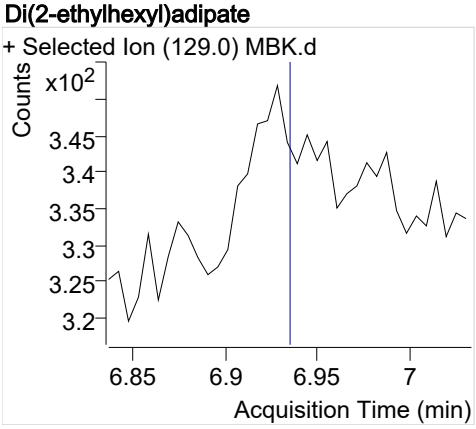

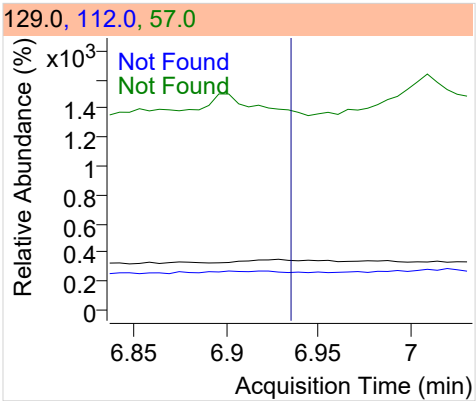

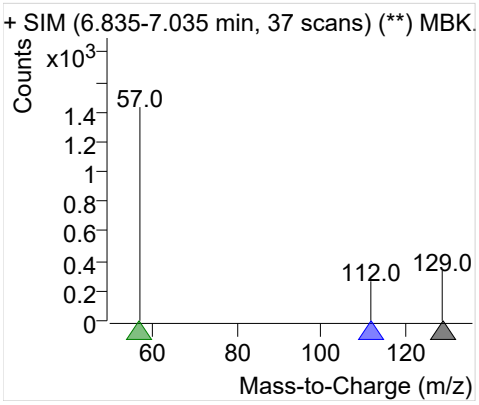

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(RE 3.11)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-03-18 오후 12:47:49	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:08:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:47:49	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 6:12:02	**Data File**	CCV.d
Type	QC	**Name**	CCV
Dil.	1	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

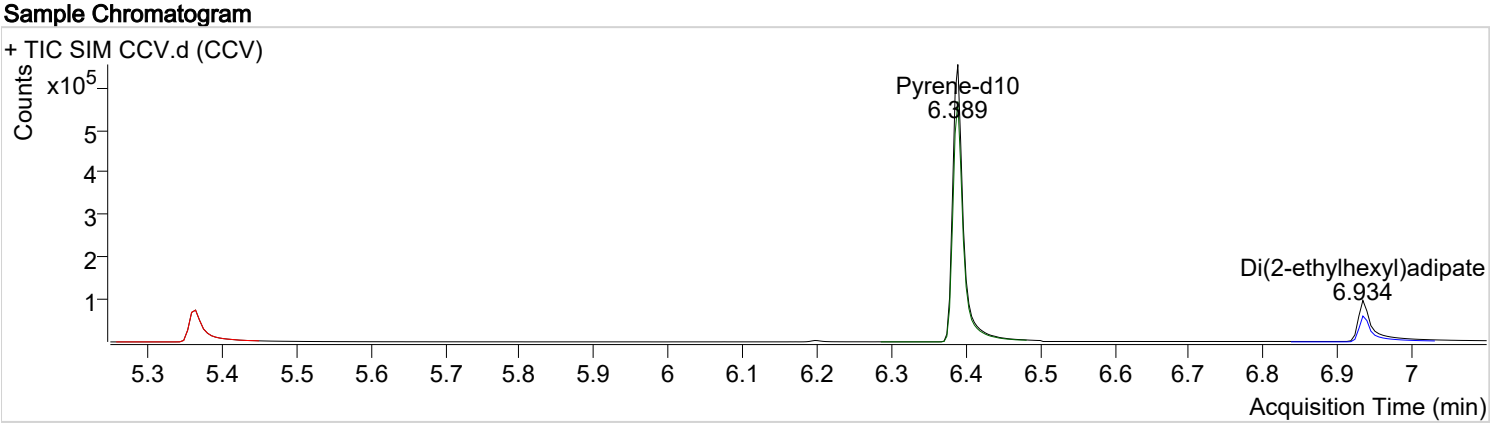

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate	6.934	79978	111240	4.0997 mg/L
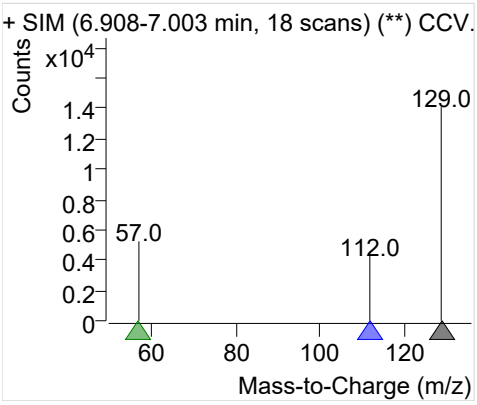
Di(2-ethylhexyl)adipate