Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin				
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Di(2-ethylhexyl)adipate

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
DEHA ST-01.d	Cal	6.928	6150	80112	0.4182
DEHA ST-02.d	Cal	6.928	13456	84215	0.9707
DEHA ST-03.d	Cal	6.928	35735	86444	2.6586
DEHA ST-04.d	Cal	6.928	70962	93283	4.9704
DEHA ST-05.d	Cal	6.928	157166	103827	9.9822
BK-.d	Blank			103290	ND
FBK(HH 26-03-24).d	Blank			102965	ND
HH-01.d	Sample			104073	ND
HH-02.d	Sample			106272	ND
HH-03.d	Sample			105891	ND
HH-04.d	Sample			109111	ND
FBK(NJ 26-03-26).d	Blank			108819	ND
NJ-01.d	Sample			110873	ND
NJ-02.d	Sample			105500	ND
NJ-03.d	Sample			109484	ND
NJ-04.d	Sample			104627	ND
NJ-05.d	Sample			107596	ND
NJ-06.d	Sample			108686	ND
MBK.d	Blank			108632	ND
CCV.d	QC	6.928	87746	110064	5.2134

Di(2-ethylhexyl)adipate

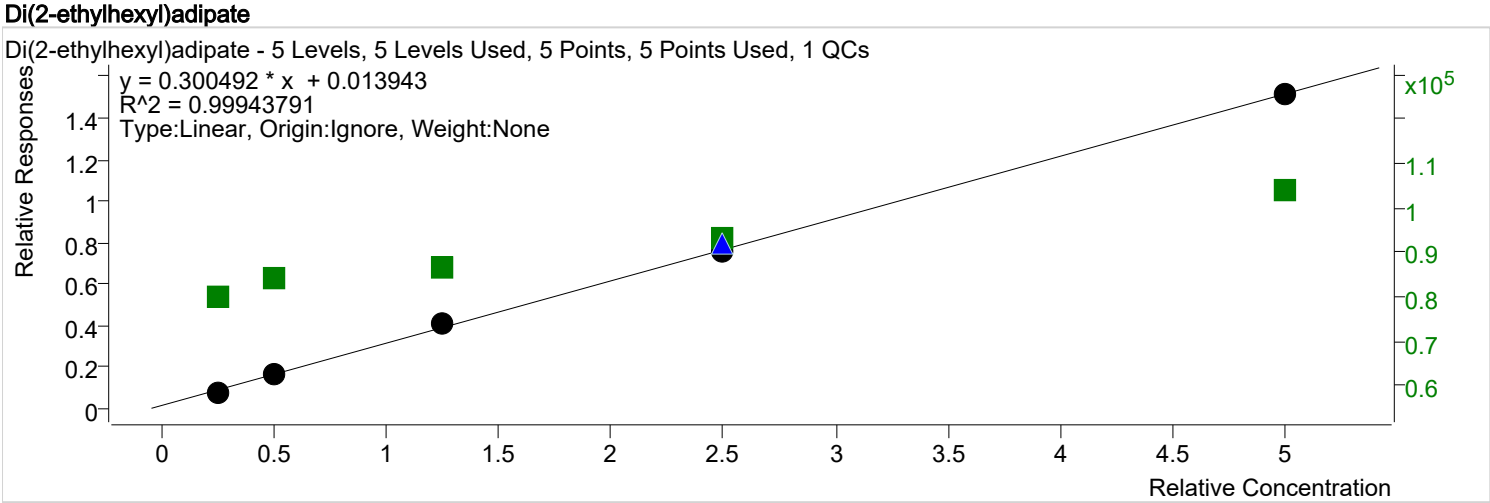

Cal. Path	Type	Level	Enable	Conc.	Response
V:\2026\2026-03\DEHA(NJ 3.26)\DEHA ST-01.d	Calibration	1	x	0.500	6150
V:\2026\2026-03\DEHA(NJ 3.26)\DEHA ST-02.d	Calibration	2	x	1.000	13456
V:\2026\2026-03\DEHA(NJ 3.26)\DEHA ST-03.d	Calibration	3	x	2.500	35735
V:\2026\2026-03\DEHA(NJ 3.26)\DEHA ST-04.d	Calibration	4	x	5.000	70962
V:\2026\2026-03\DEHA(NJ 3.26)\CCV.d	QC	4	x	5.000	87746
V:\2026\2026-03\DEHA(NJ 3.26)\DEHA ST-05.d	Calibration	5	x	10.000	157166

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 9:32:32	**Data File**	DEHA ST-01.d
Type	Cal	**Name**	DEHA ST-01
Dil.	1	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

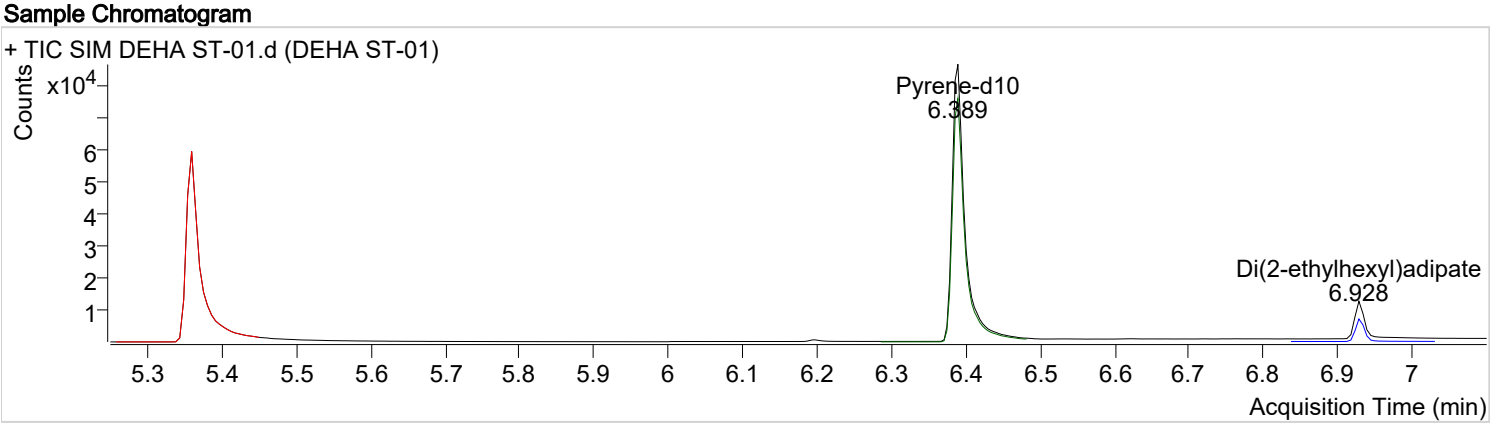

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate	6.928	6150	80112	0.4182 mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 9:43:06	**Data File**	DEHA ST-02.d
Type	Cal	**Name**	DEHA ST-02
Dil.	1	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

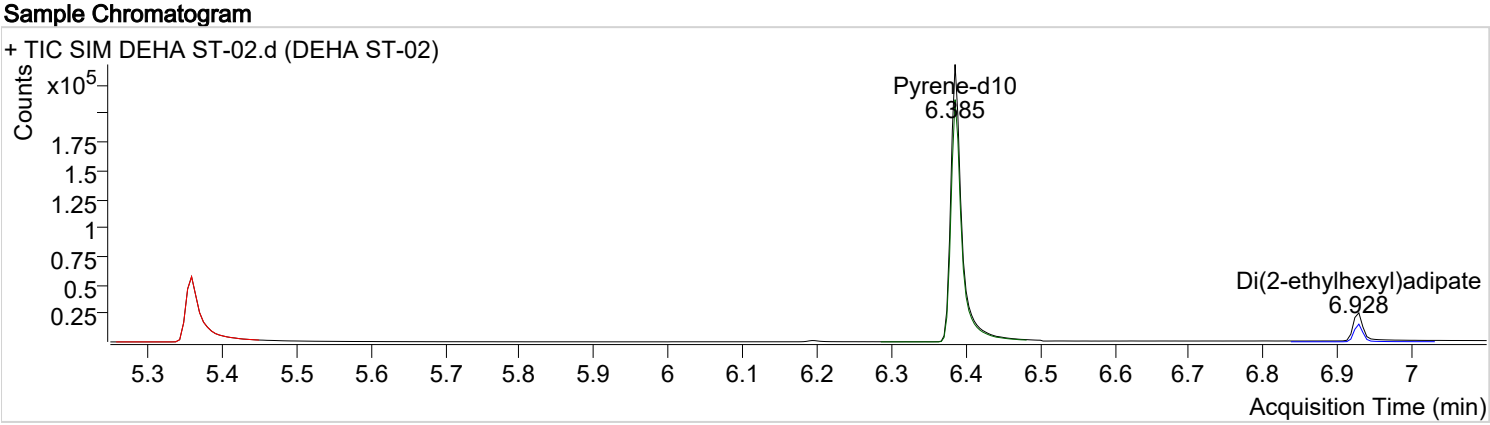

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate	6.928	13456	84215	0.9707 mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 9:53:46	**Data File**	DEHA ST-03.d
Type	Cal	**Name**	DEHA ST-03
Dil.	1	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

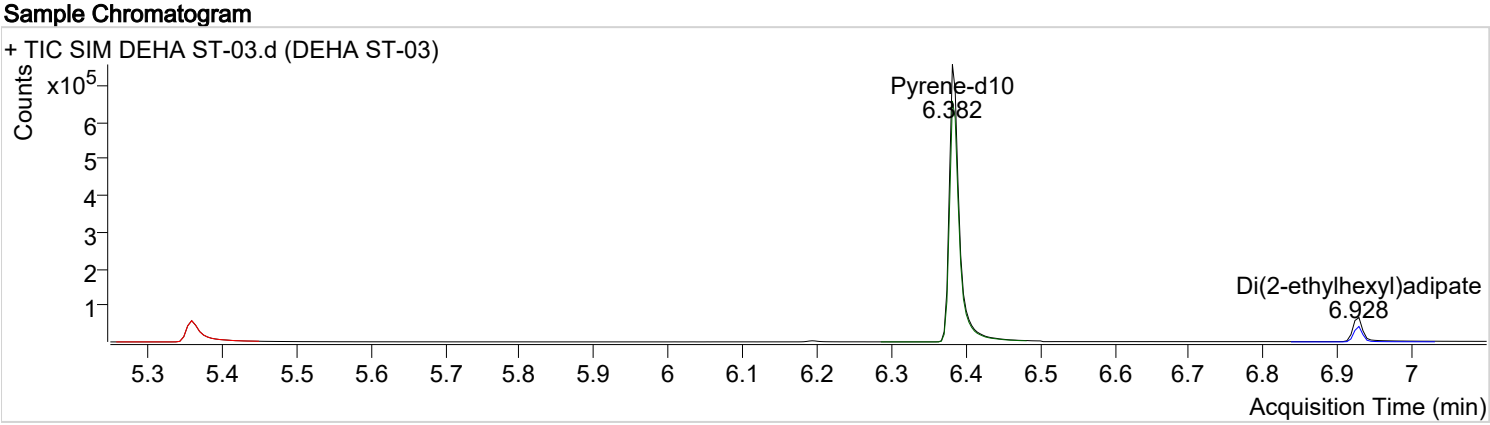

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate	6.928	35735	86444	2.6586 mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 10:04:26	**Data File**	DEHA ST-04.d
Type	Cal	**Name**	DEHA ST-04
Dil.	1	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

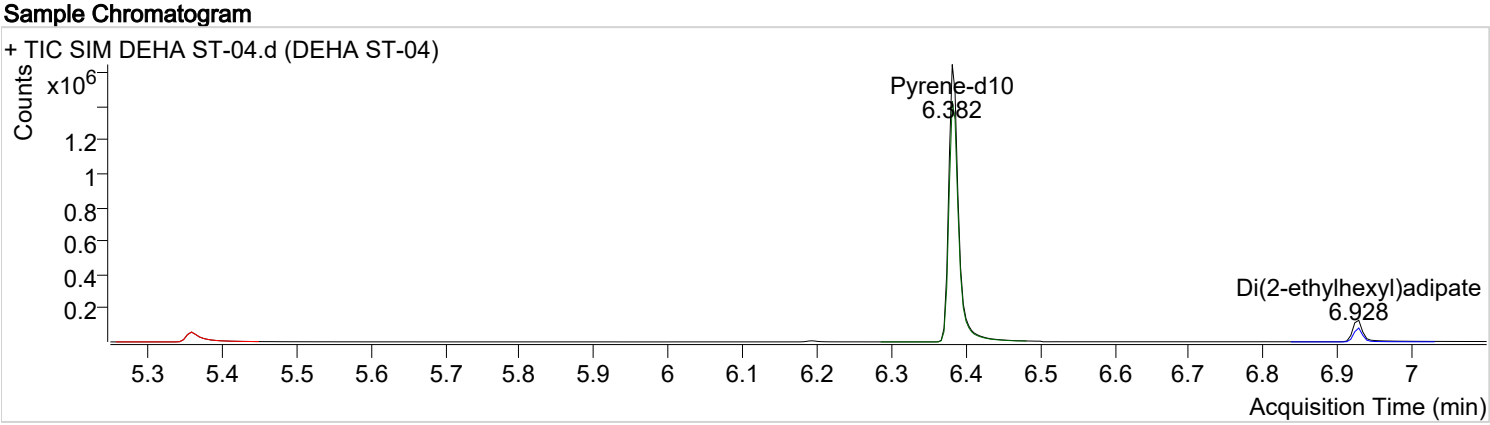

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate	6.928	70962	93283	4.9704 mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 10:15:08	**Data File**	DEHA ST-05.d
Type	Cal	**Name**	DEHA ST-05
Dil.	1	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

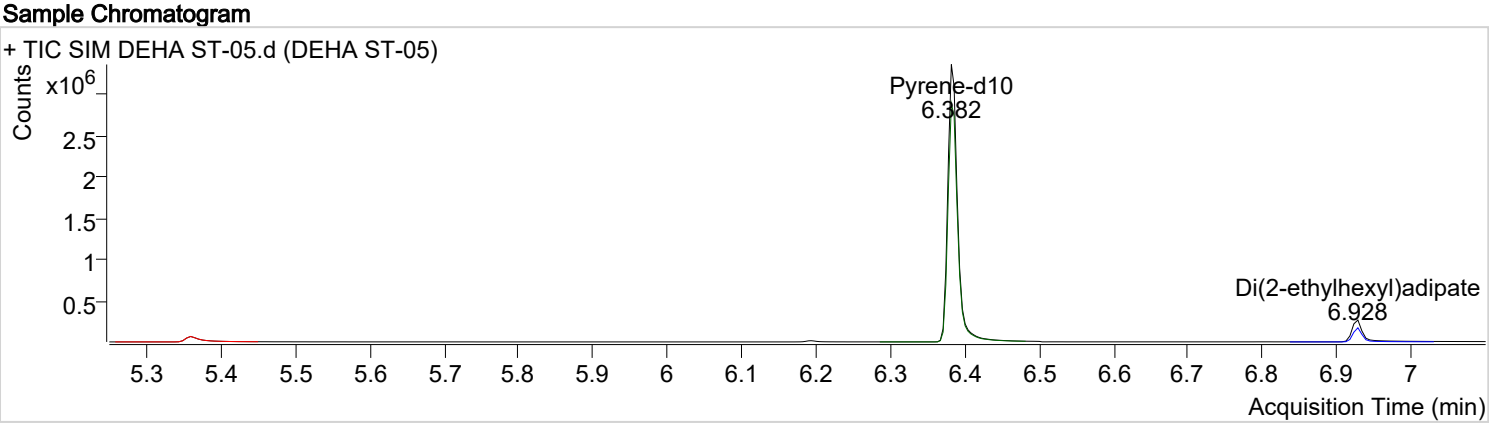

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate	6.928	157166	103827	9.9822 mg/L

Di(2-ethylhexyl)adipate

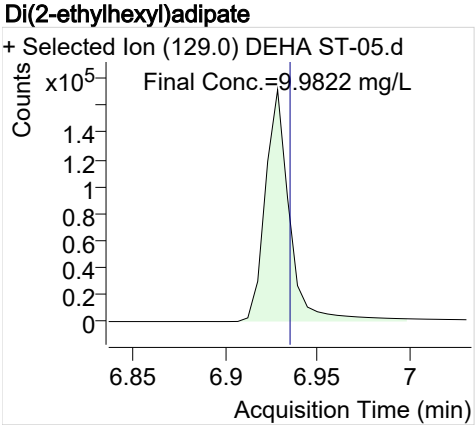





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 10:36:31	**Data File**	BK-.d
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

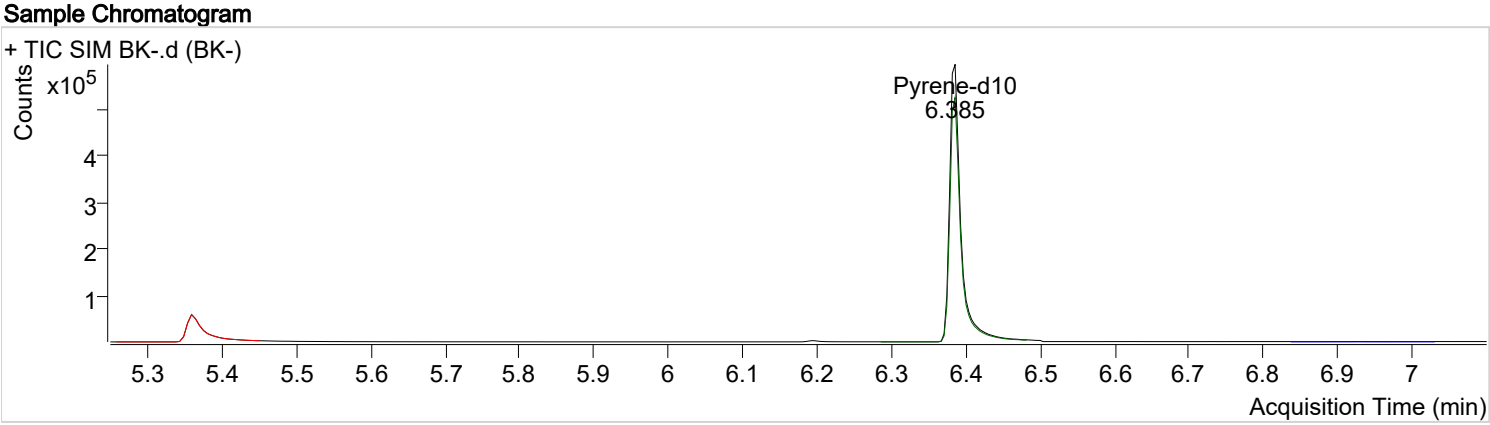

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			103290	ND mg/L

Di(2-ethylhexyl)adipate

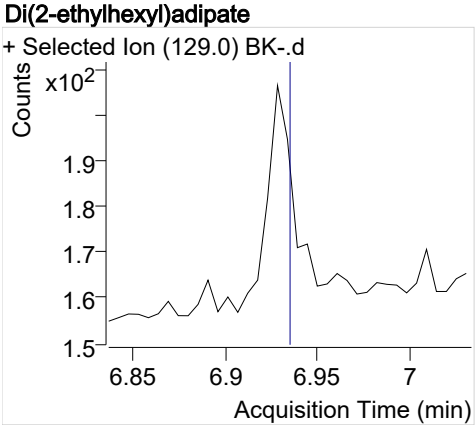





Quant Sample Report

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 10:47:13	**Data File**	FBK(HH 26-03-24).d
Type	Blank	**Name**	FBK(HH 26-03-24)
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

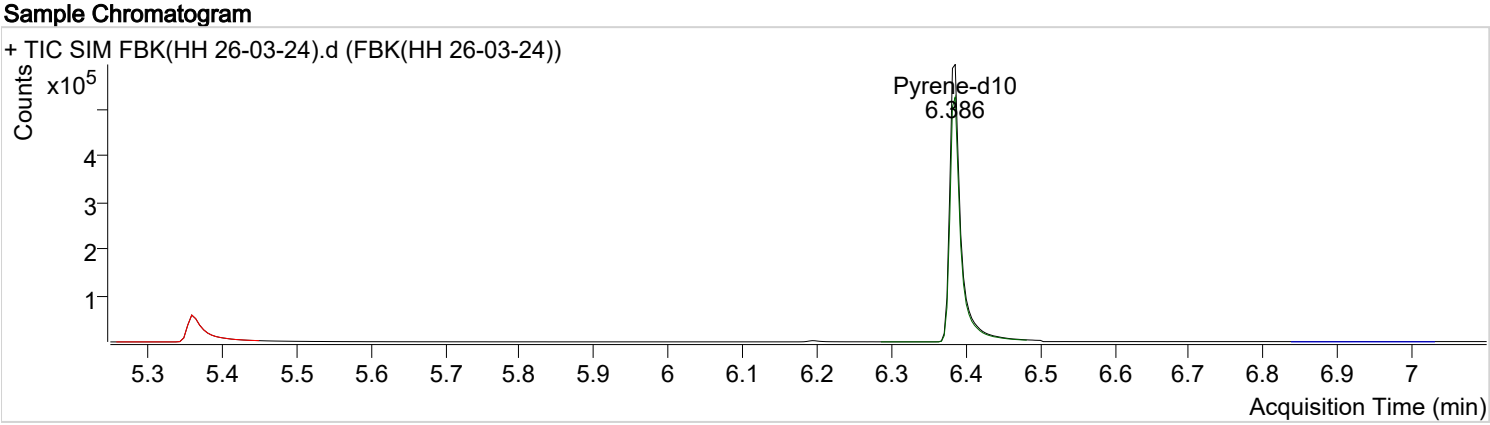

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			102965	ND mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 10:57:51	**Data File**	HH-01.d
Type	Sample	**Name**	HH-01
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

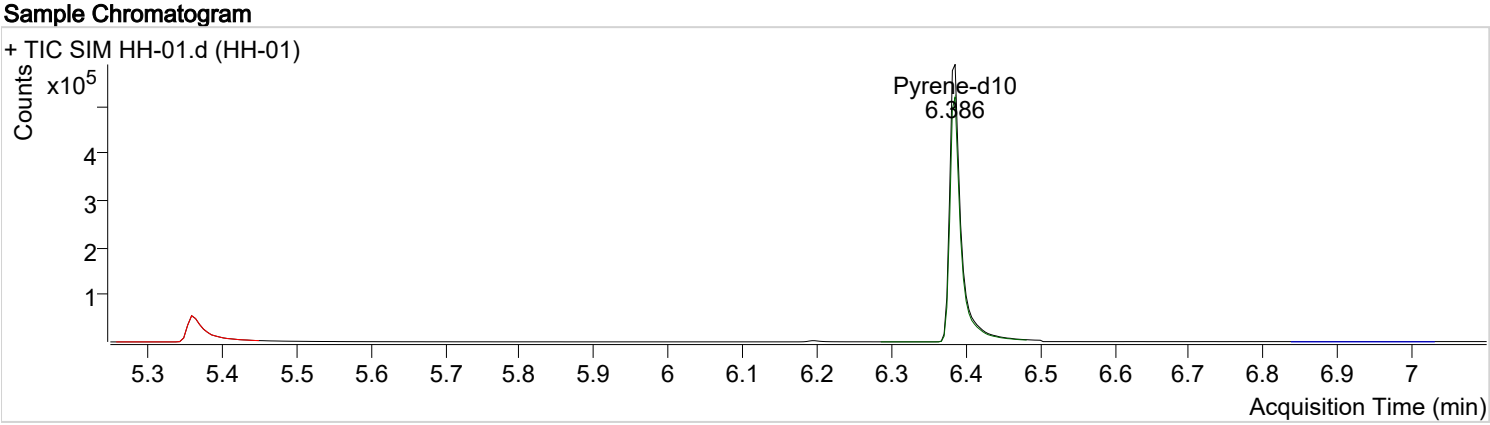

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			104073	ND mg/L

Di(2-ethylhexyl)adipate





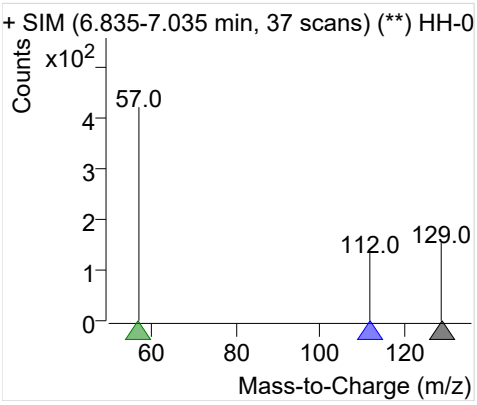

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 11:08:31	**Data File**	HH-02.d
Type	Sample	**Name**	HH-02
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

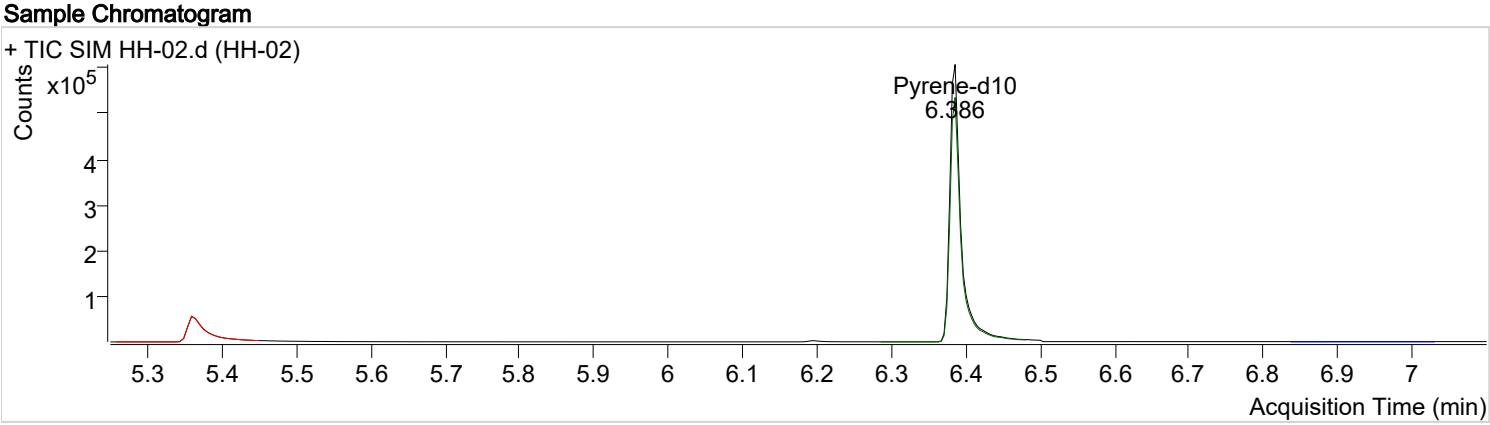

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			106272	ND mg/L

Di(2-ethylhexyl)adipate





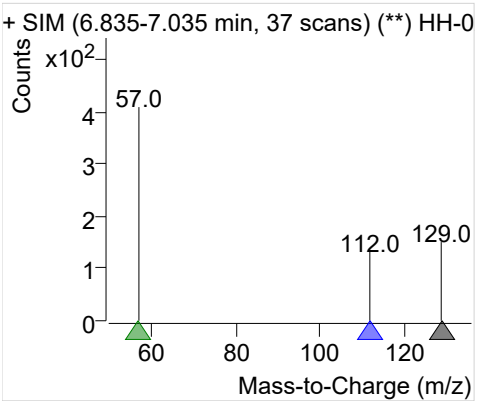

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 11:19:10	**Data File**	HH-03.d
Type	Sample	**Name**	HH-03
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

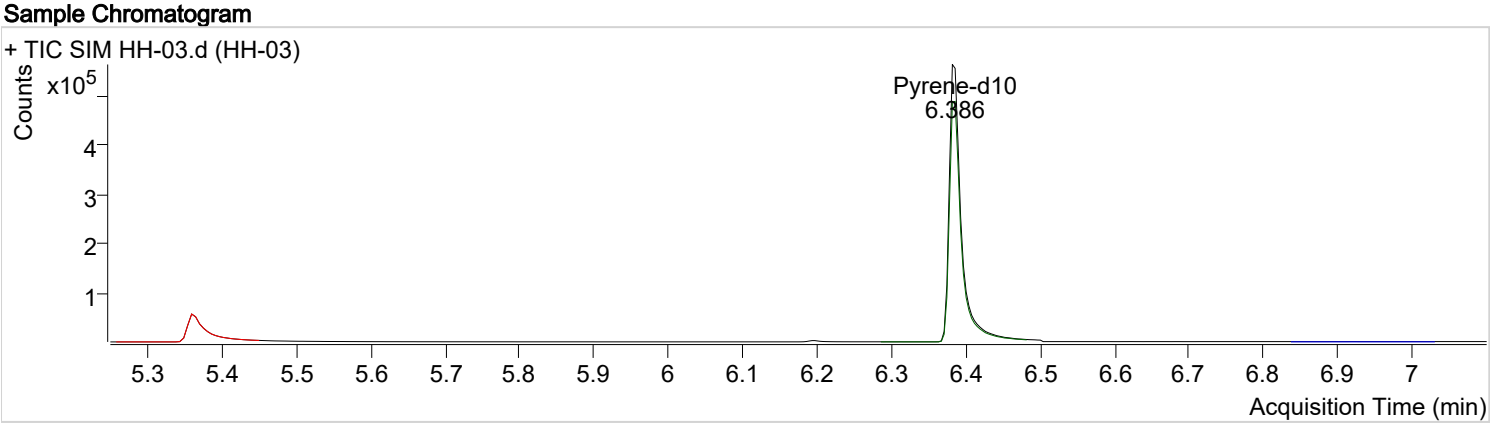

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			105891	ND mg/L

Di(2-ethylhexyl)adipate





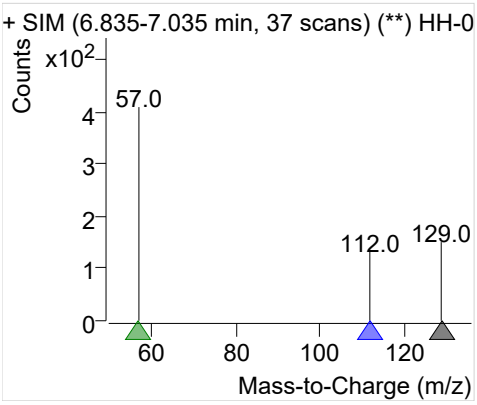

Quant Sample Report

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 11:29:49	**Data File**	HH-04.d
Type	Sample	**Name**	HH-04
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

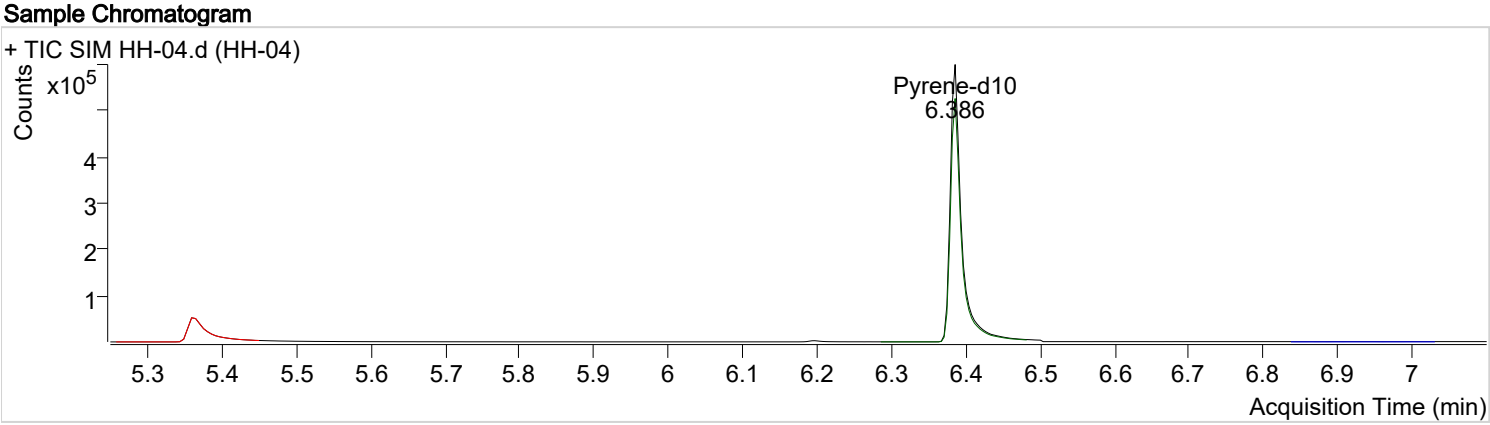

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			109111	ND mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 11:40:26	**Data File**	FBK(NJ 26-03-26).d
Type	Blank	**Name**	FBK(NJ 26-03-26)
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

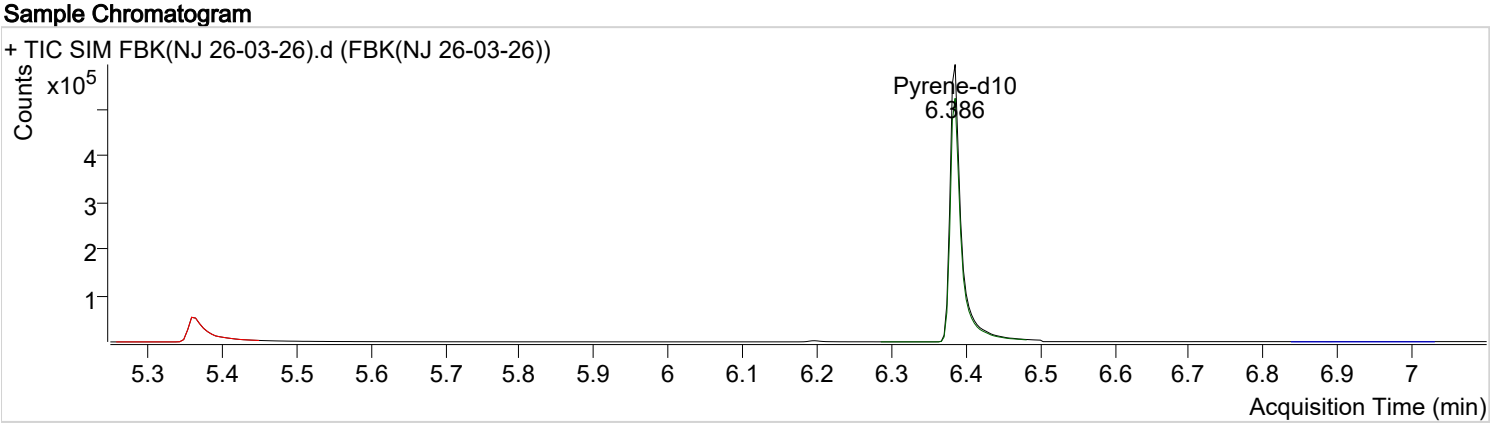

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			108819	ND mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 11:51:07	**Data File**	NJ-01.d
Type	Sample	**Name**	NJ-01
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

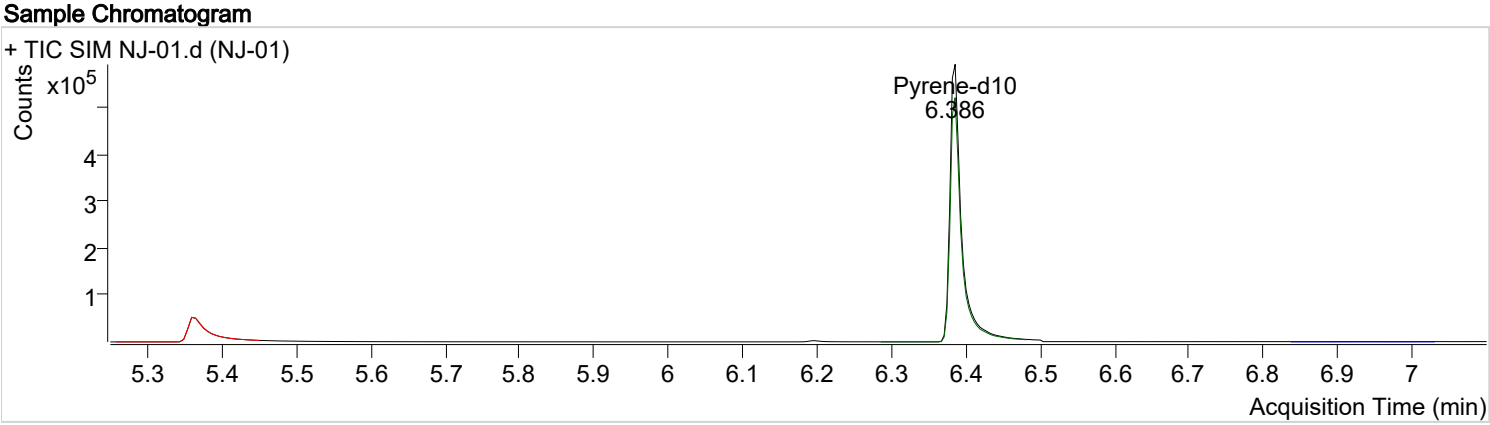

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			110873	ND mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오후 12:01:46	**Data File**	NJ-02.d
Type	Sample	**Name**	NJ-02
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

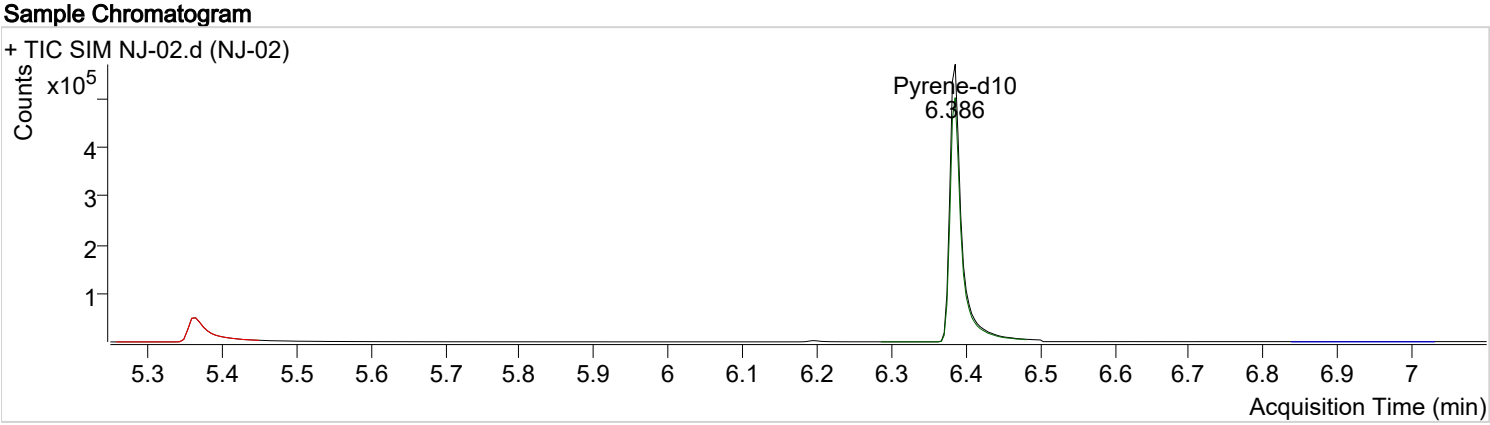

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			105500	ND mg/L

Di(2-ethylhexyl)adipate





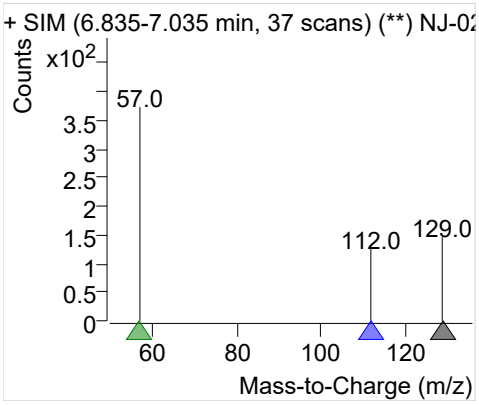

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오후 12:12:22	**Data File**	NJ-03.d
Type	Sample	**Name**	NJ-03
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

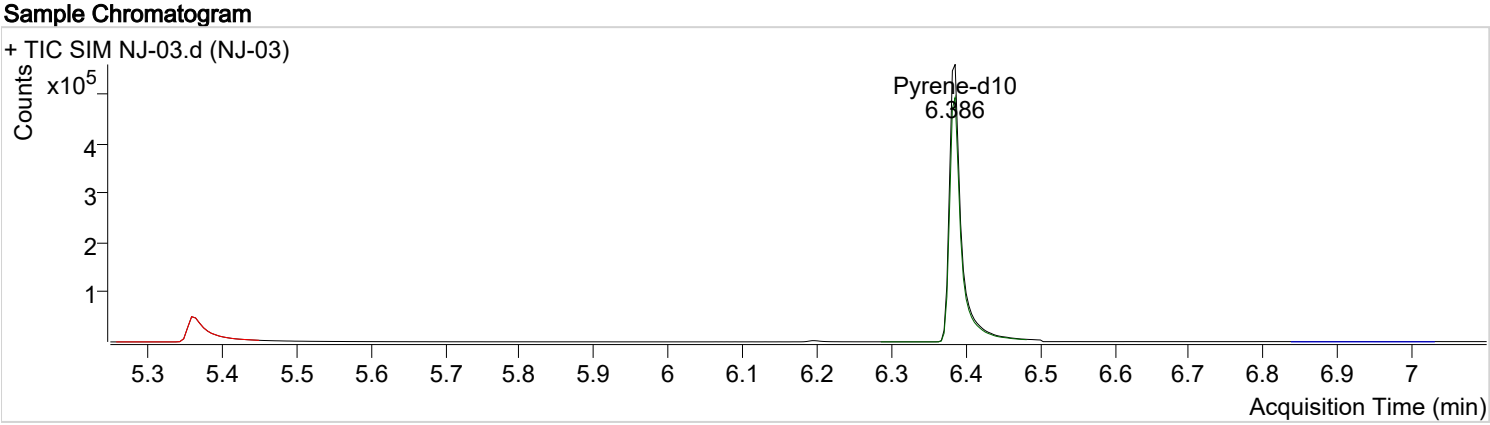

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			109484	ND mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오후 12:23:02	**Data File**	NJ-04.d
Type	Sample	**Name**	NJ-04
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

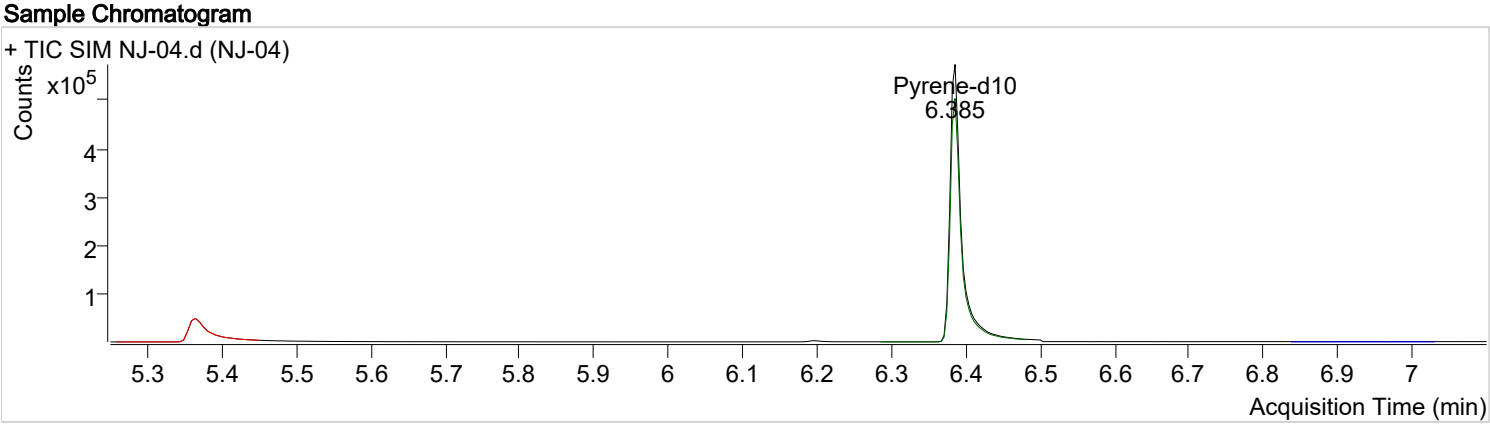

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			104627	ND mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오후 12:33:43	**Data File**	NJ-05.d
Type	Sample	**Name**	NJ-05
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

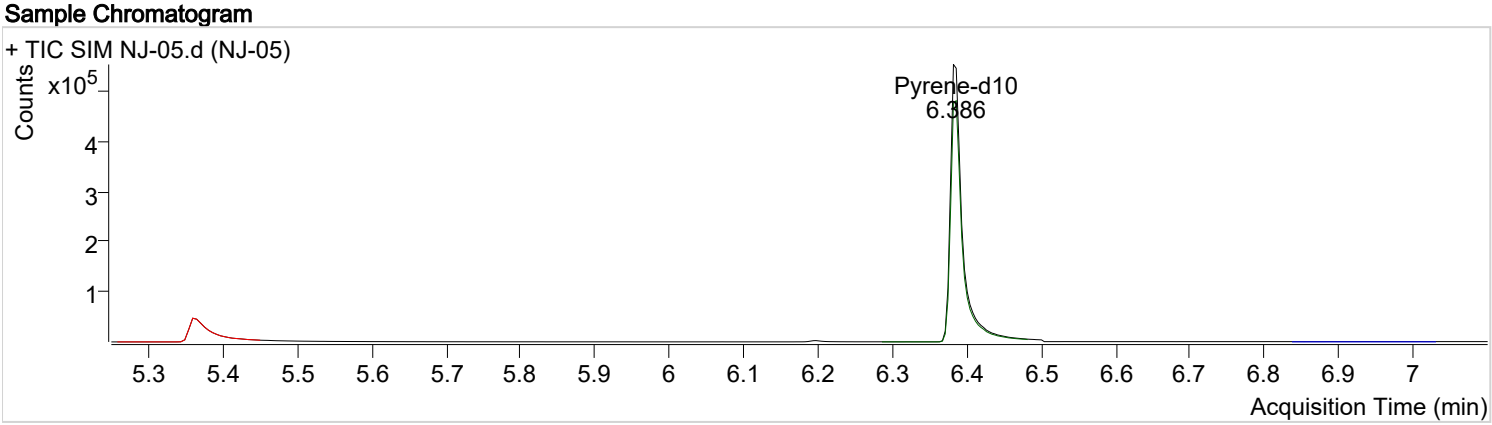

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			107596	ND mg/L

Di(2-ethylhexyl)adipate

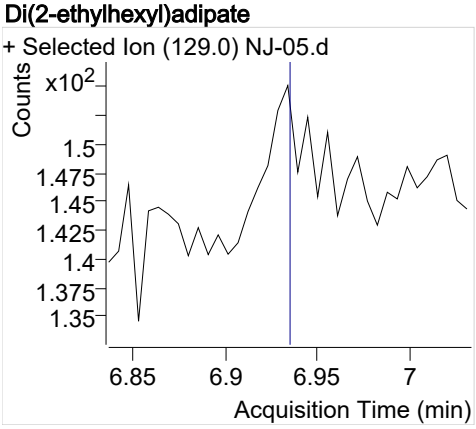





Quant Sample Report

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오후 12:44:22	**Data File**	NJ-06.d
Type	Sample	**Name**	NJ-06
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

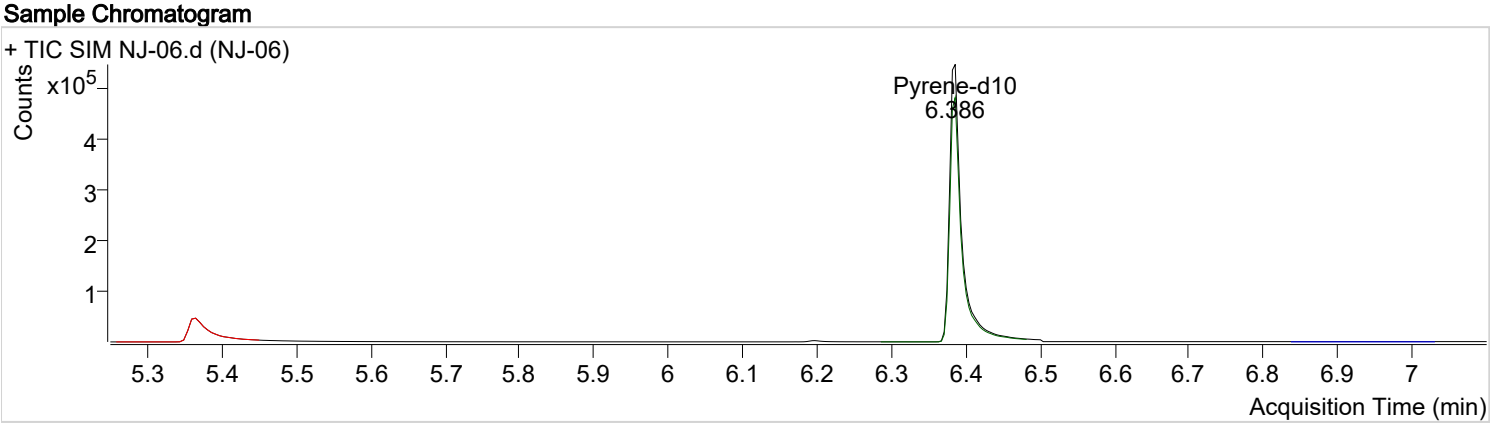

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			108686	ND mg/L

Di(2-ethylhexyl)adipate





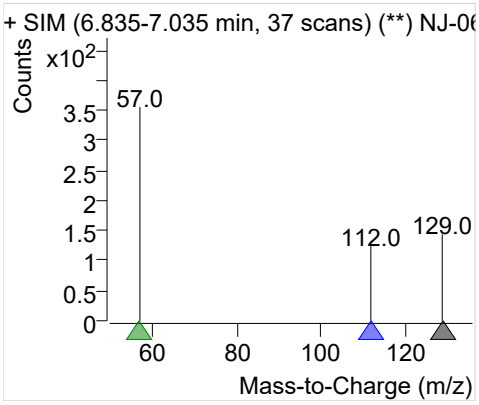

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오후 12:55:03	**Data File**	MBK.d
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

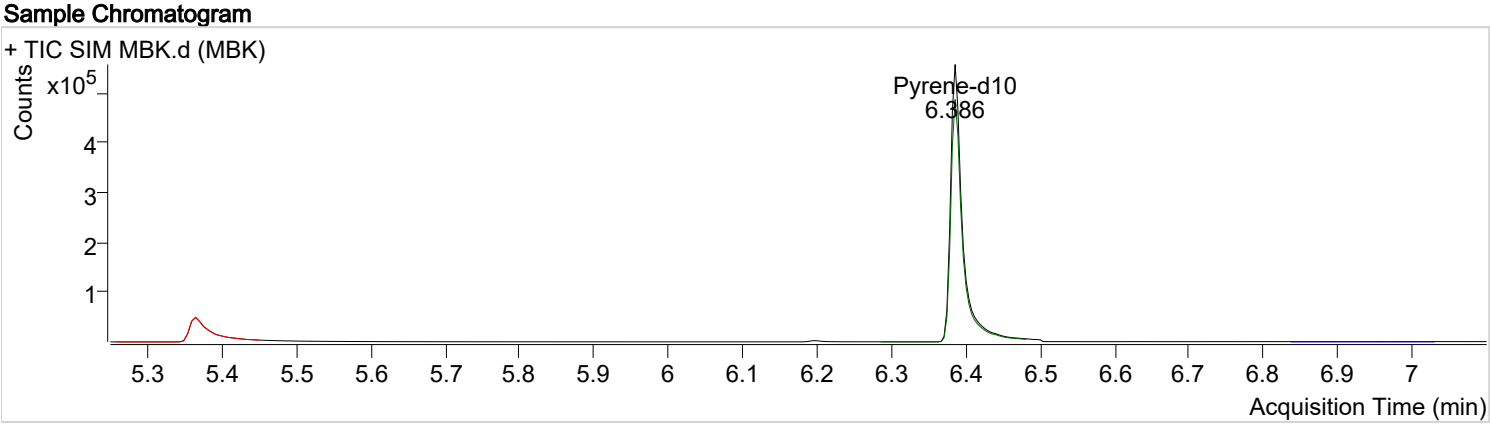

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate			108632	ND mg/L

Di(2-ethylhexyl)adipate







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\DEHA(NJ 3.26)\QuantResults\DEHA.batch.bin		
Analysis Time	2026-04-01 오후 4:21:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:06:07	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:21:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오후 1:05:45	**Data File**	CCV.d
Type	QC	**Name**	CCV
Dil.	1	**Acq. Method File**	ORG(DEHA) METHOD

Sample Chromatogram

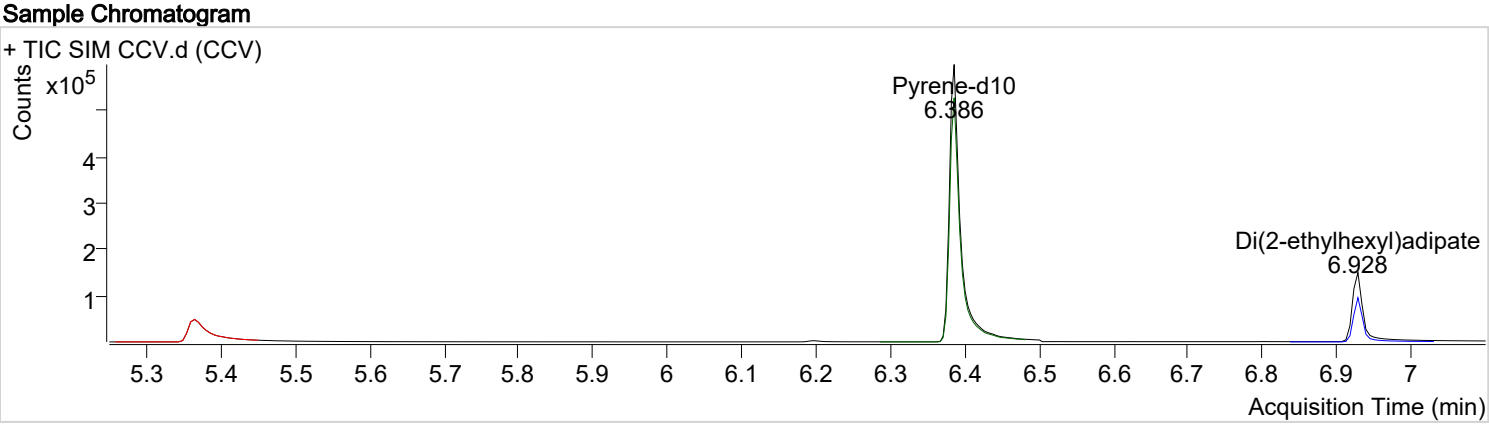

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Di(2-ethylhexyl)adipate	6.928	87746	110064	5.2134 mg/L
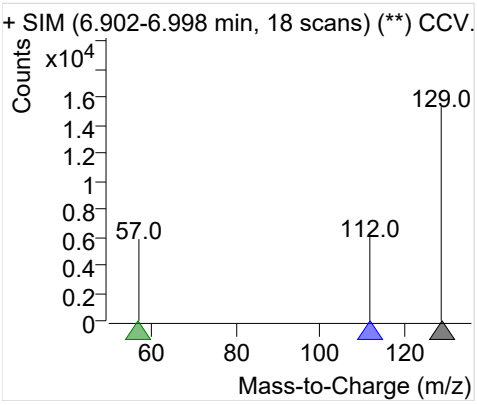
Di(2-ethylhexyl)adipate