Quantitative Analysis Results Summary Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin				
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Di-Phtalate

Data File	Type	RT	Resp.	Final Conc.
DEHP ST-01.D	Cal	9.683	51169	0.0021
DEHP ST-02.D	Cal	9.683	114654	0.0068
DEHP ST-03.D	Cal	9.683	127037	0.0078
DEHP ST-04.D	Cal	9.683	160265	0.0103
DEHP ST-05.D	Cal	9.683	226059	0.0152
DEHP ST-06.D	Cal	9.683	284229	0.0196
BK-.D	Blank			ND
FBK(KD 26-02-04).D	Blank			ND
FBK(JR 26-02-05).D	Blank			ND
JR-01.D	Sample			ND
JR-02.D	Sample			ND
JR-03.D	Sample			ND
JR-04.D	Sample			ND
JR-05.D	Sample			ND
JR-06.D	Sample			ND
JR-07.D	Sample			ND
JR-08.D	Sample			ND
KD-01.D	Sample			ND
KD-02.D	Sample			ND
KD-04.D	Sample			ND
MBK.D	Blank			ND
CCV.D	QC	9.689	136744	0.0085

Di-Phtalate

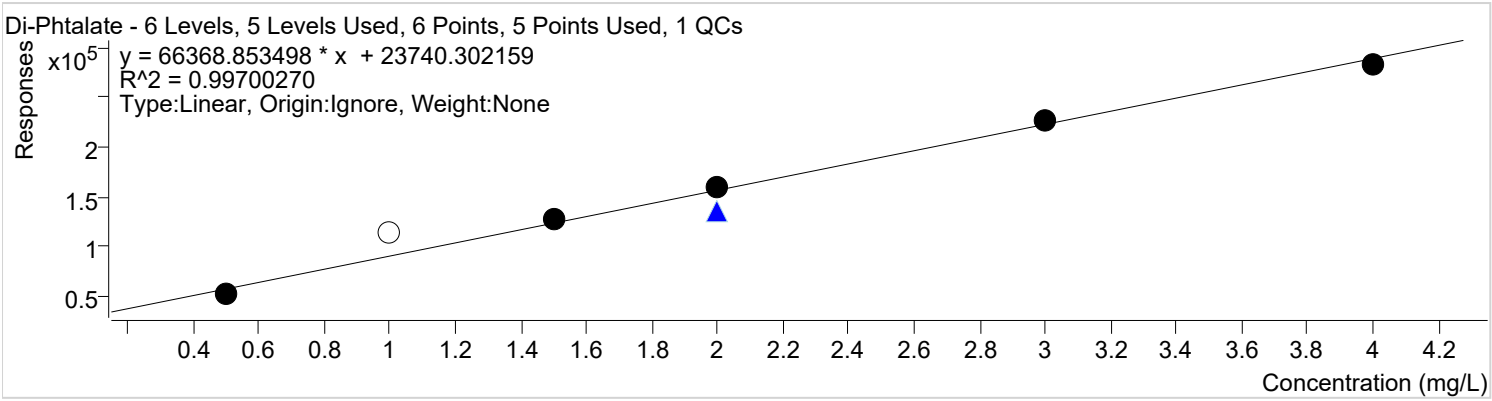

Cal. Path	Type	Level	Enable	Conc.	Response
\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\DEHP ST-01.D	Calibration	1	x	0.500	51169
\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\DEHP ST-02.D	Calibration	2		1.000	114654
\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\DEHP ST-03.D	Calibration	3	x	1.500	127037
\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\DEHP ST-04.D	Calibration	4	x	2.000	160265
\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\CCV.D	QC	4	x	2.000	136744
\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\DEHP ST-05.D	Calibration	5	x	3.000	226059
\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\DEHP ST-06.D	Calibration	6	x	4.000	284229

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 5:11:20	**Data File**	DEHP ST-01.D
Type	Cal	**Name**	DEHP ST-01
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

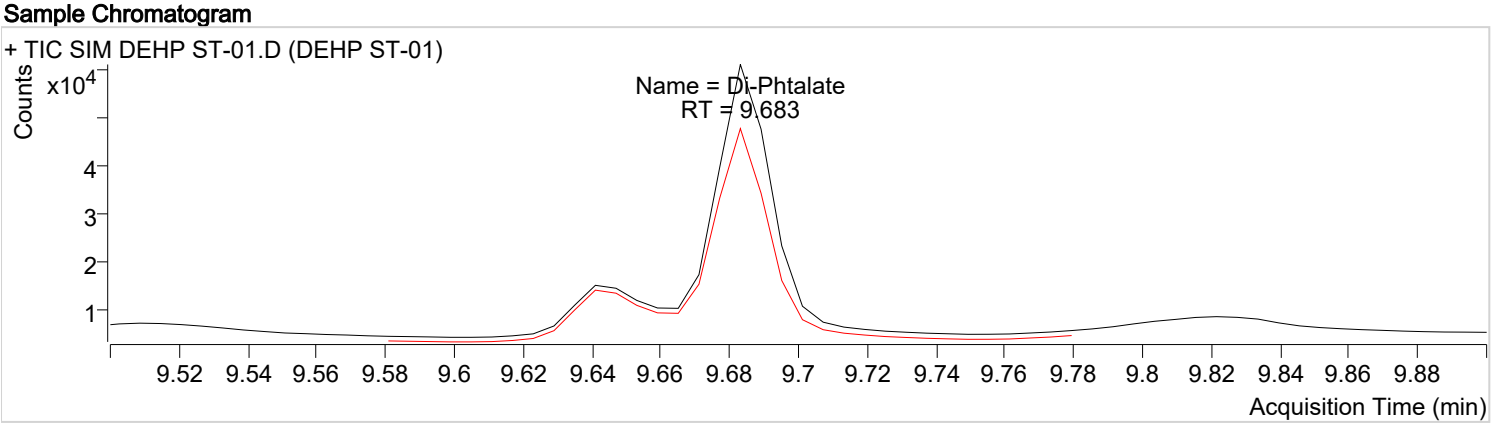

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.683	51169	0.0021	mg/L

Di-Phtalate

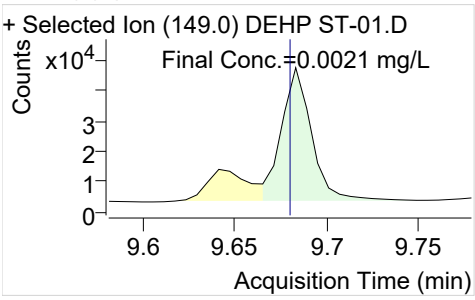

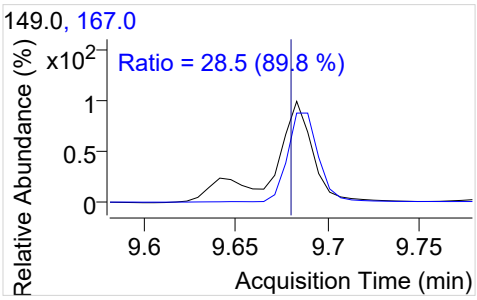

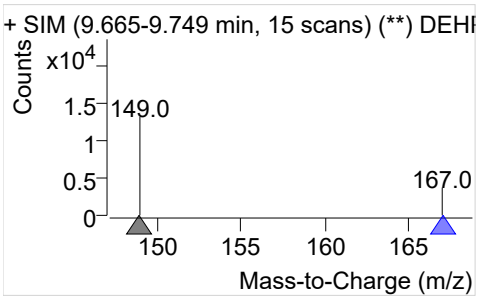

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 5:25:03	**Data File**	DEHP ST-02.D
Type	Cal	**Name**	DEHP ST-02
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

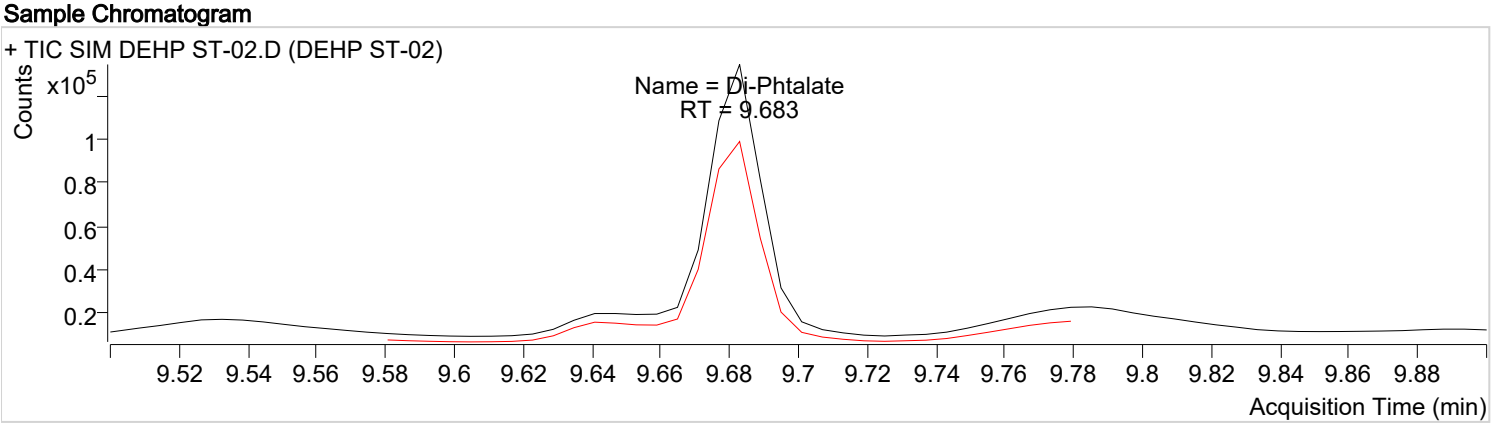

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.683	114654	0.0068	mg/L

Di-Phtalate

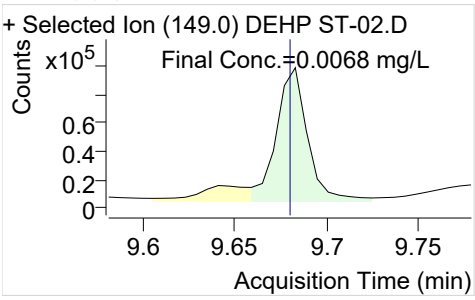

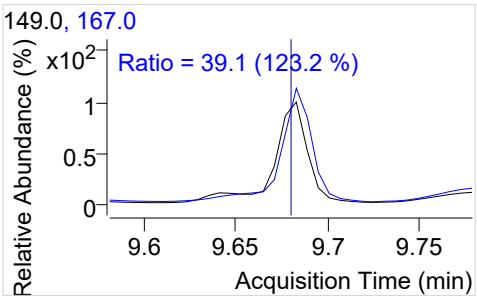

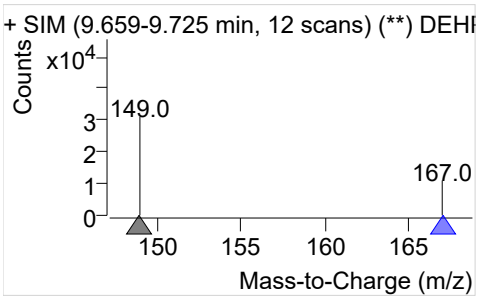

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 5:38:48	**Data File**	DEHP ST-03.D
Type	Cal	**Name**	DEHP ST-03
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

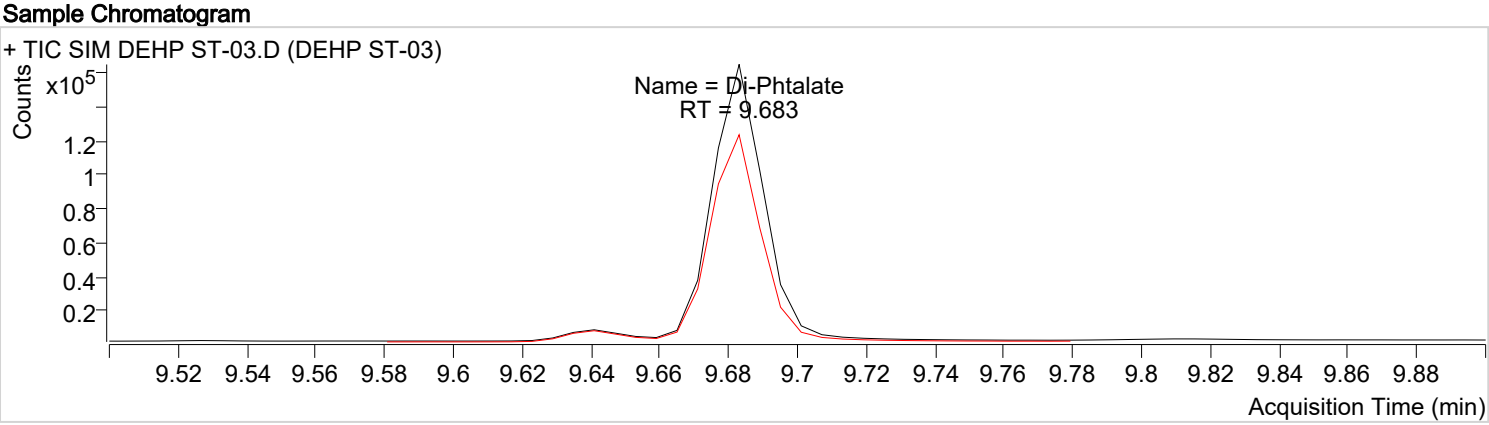

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.683	127037	0.0078	mg/L

Di-Phtalate

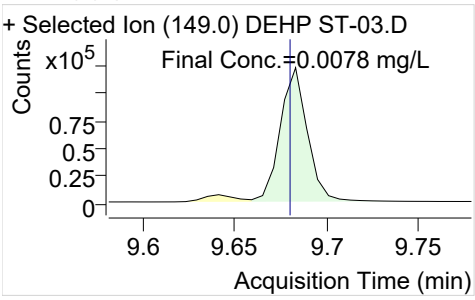



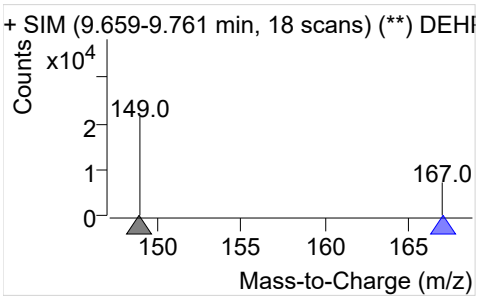

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 5:52:32	**Data File**	DEHP ST-04.D
Type	Cal	**Name**	DEHP ST-04
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

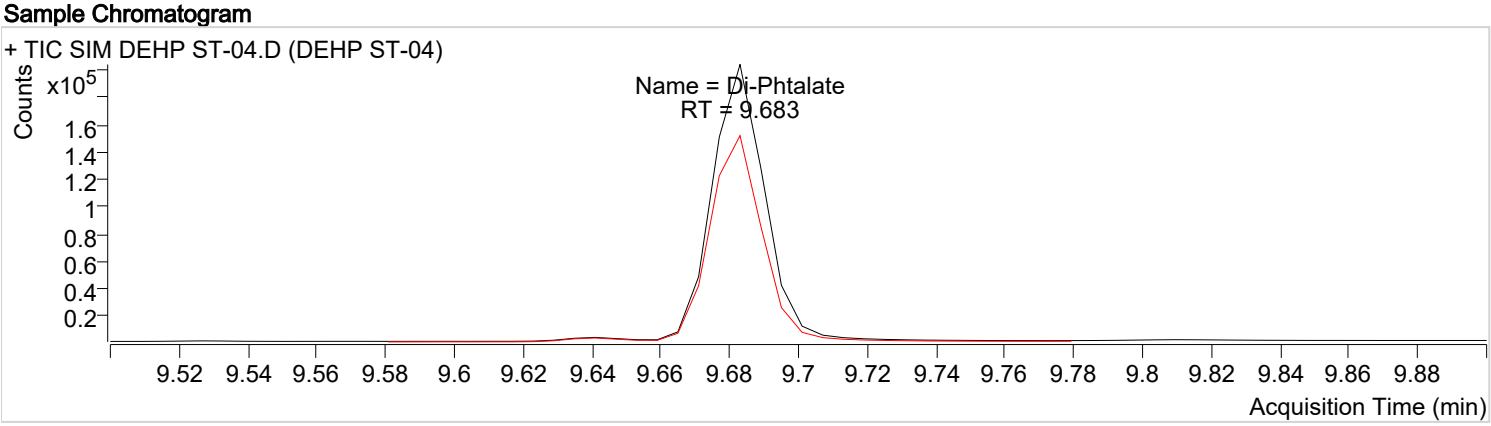

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.683	160265	0.0103	mg/L

Di-Phtalate



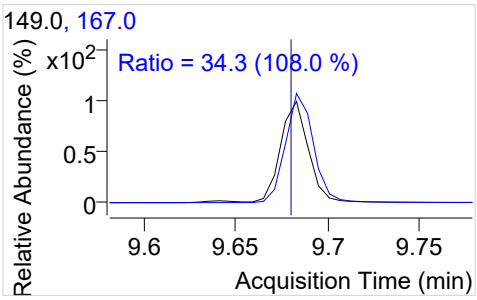

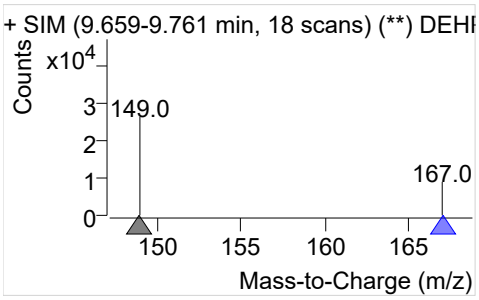

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 6:06:18	**Data File**	DEHP ST-05.D
Type	Cal	**Name**	DEHP ST-05
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

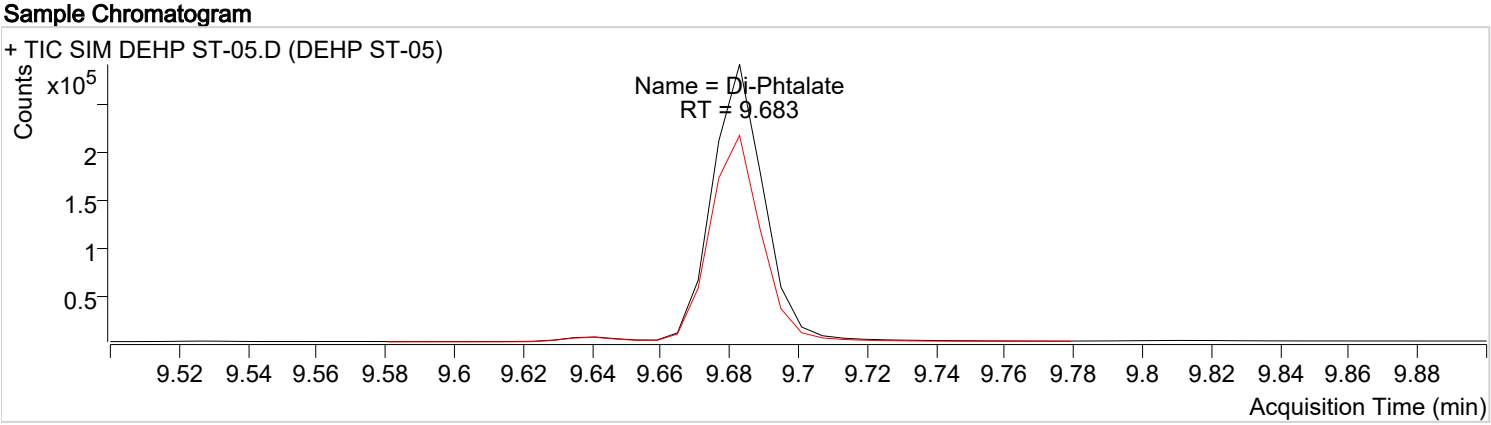

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.683	226059	0.0152	mg/L

Di-Phtalate

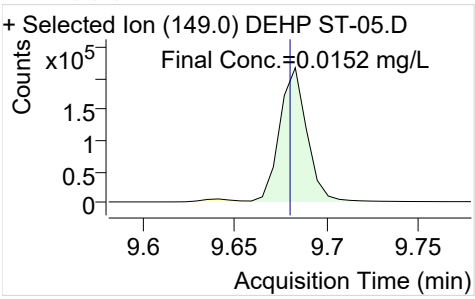



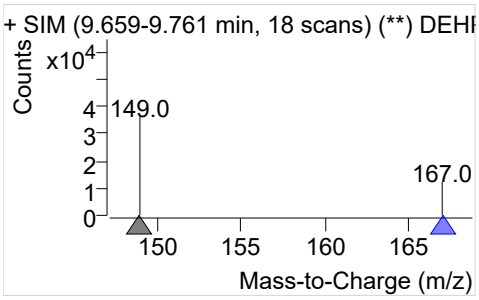

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 6:20:03	**Data File**	DEHP ST-06.D
Type	Cal	**Name**	DEHP ST-06
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

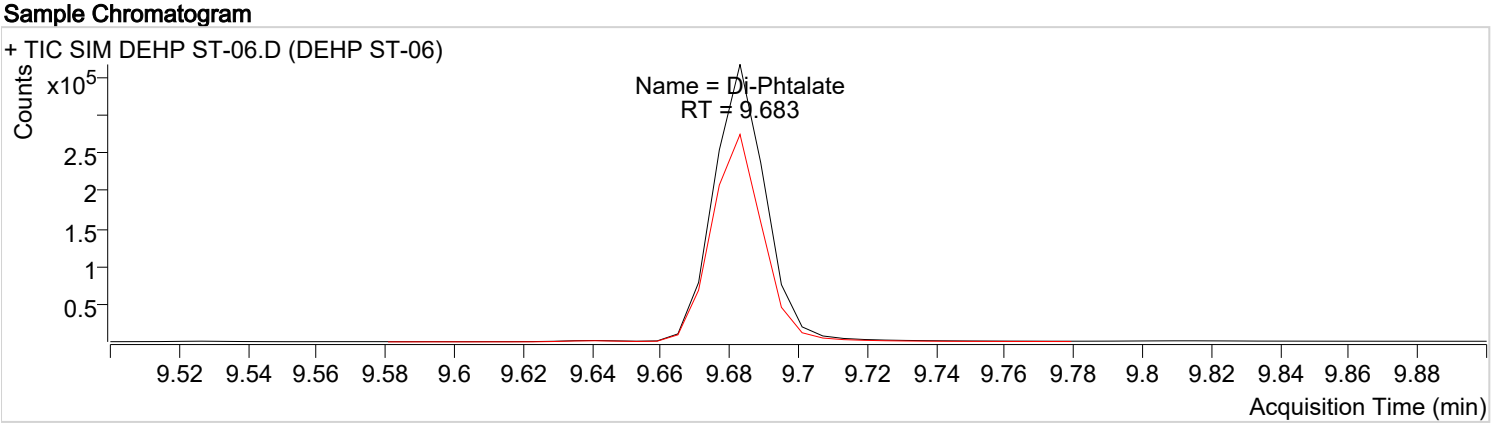

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.683	284229	0.0196	mg/L

Di-Phtalate

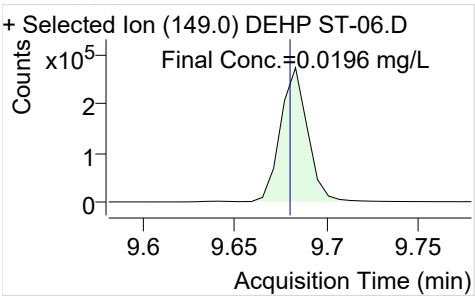

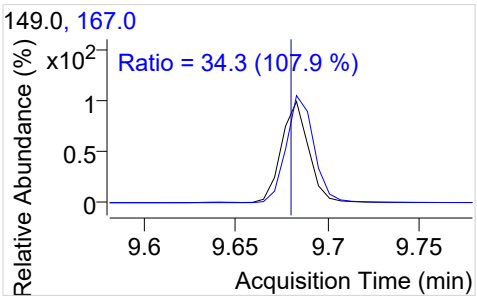

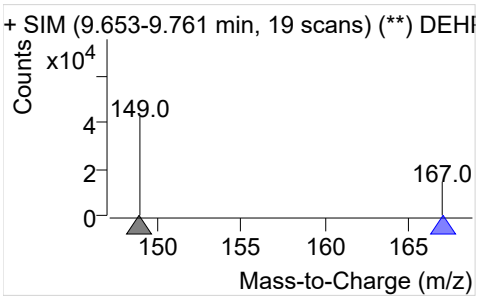

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 6:47:30	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

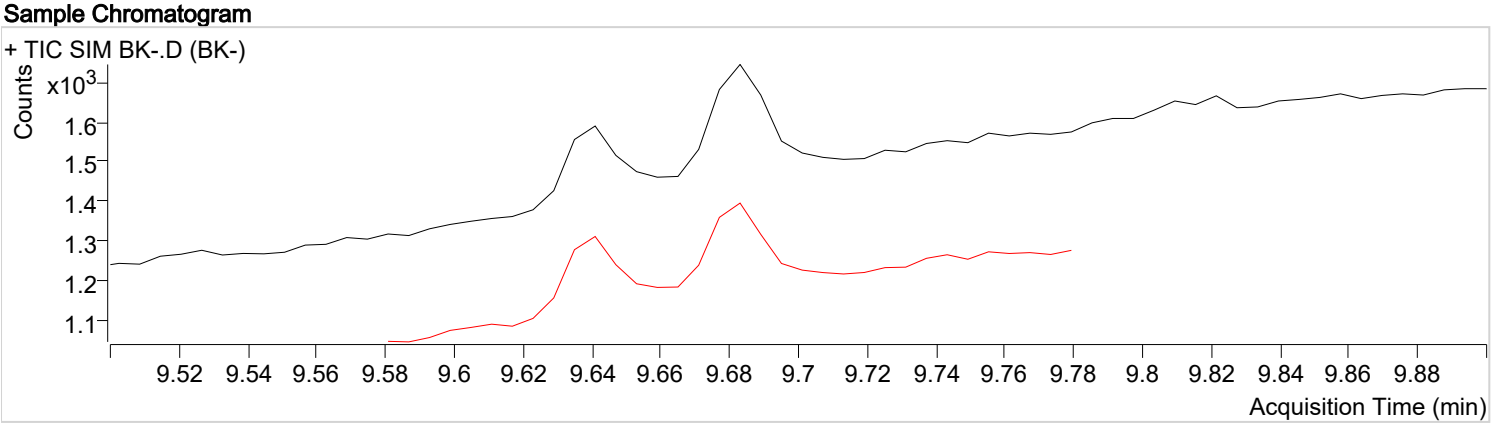

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 7:01:14	**Data File**	FBK(KD 26-02-04).D
Type	Blank	**Name**	FBK(KD 26-02-04)
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

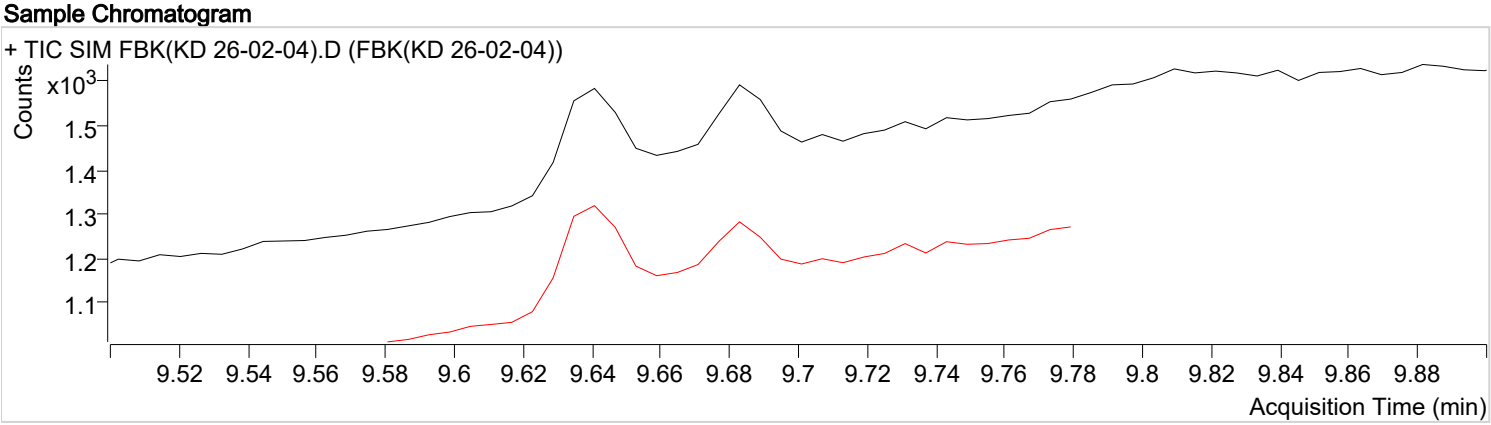

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 7:14:57	**Data File**	FBK(JR 26-02-05).D
Type	Blank	**Name**	FBK(JR 26-02-05)
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

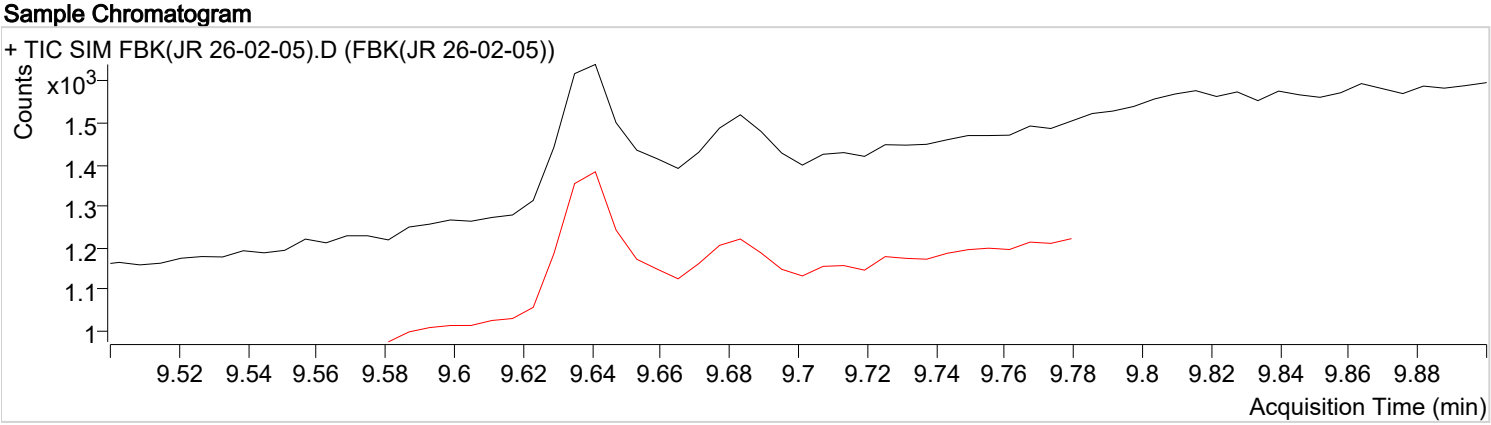

Di-Phtalate







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 7:28:42	**Data File**	JR-01.D
Type	Sample	**Name**	JR-01
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

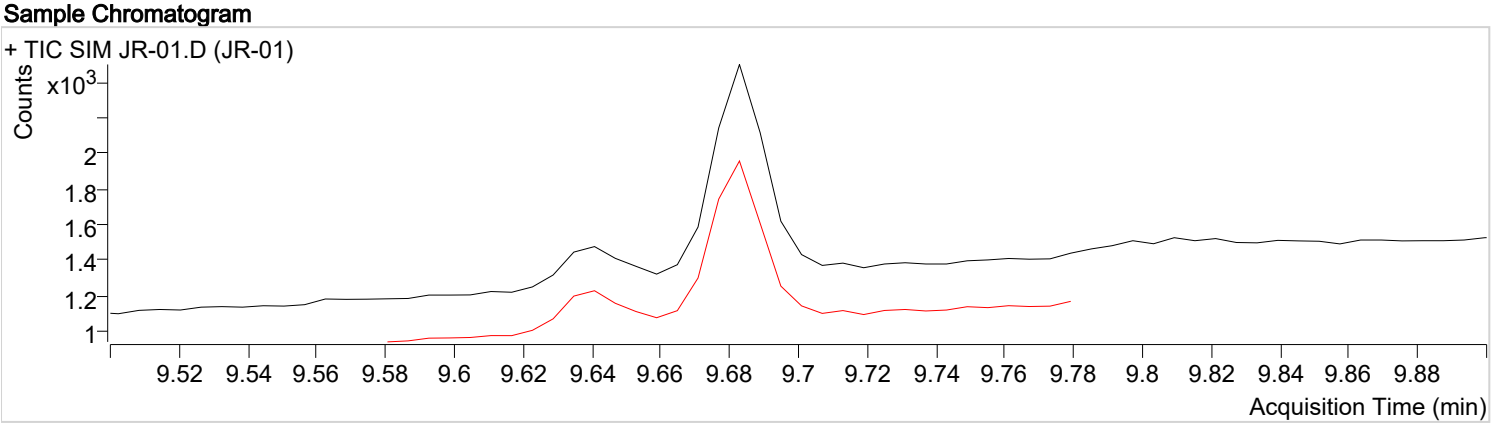

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 7:42:25	**Data File**	JR-02.D
Type	Sample	**Name**	JR-02
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

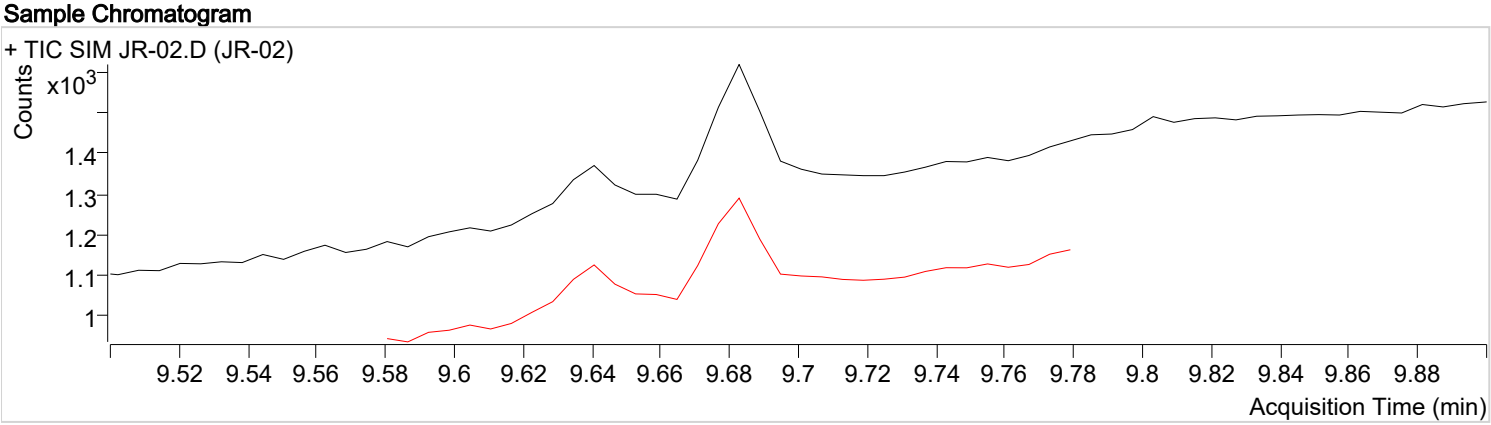

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 7:56:08	**Data File**	JR-03.D
Type	Sample	**Name**	JR-03
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

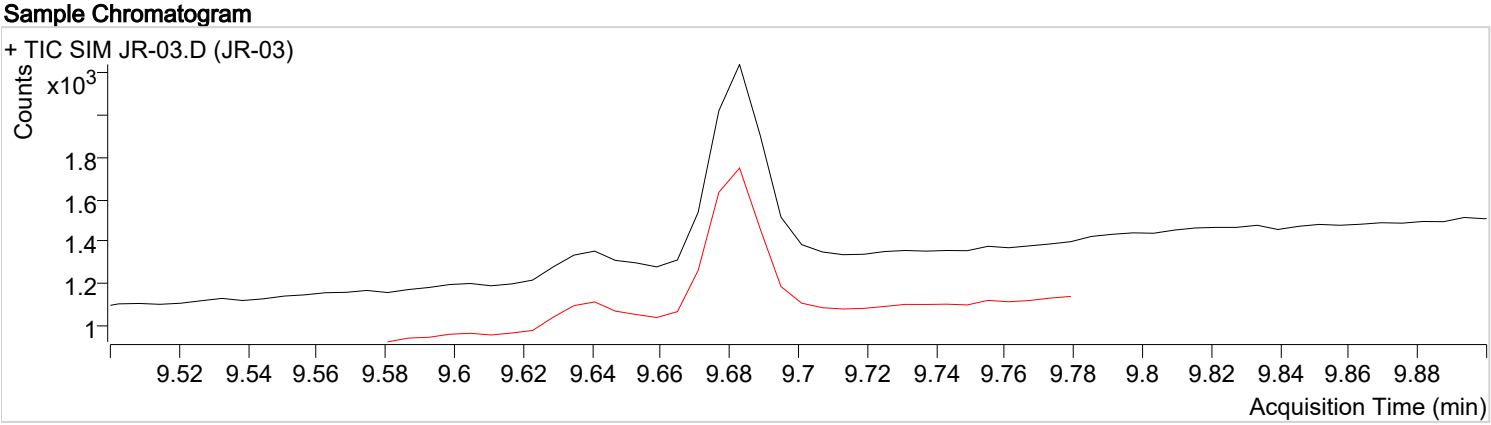

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 8:09:52	**Data File**	JR-04.D
Type	Sample	**Name**	JR-04
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

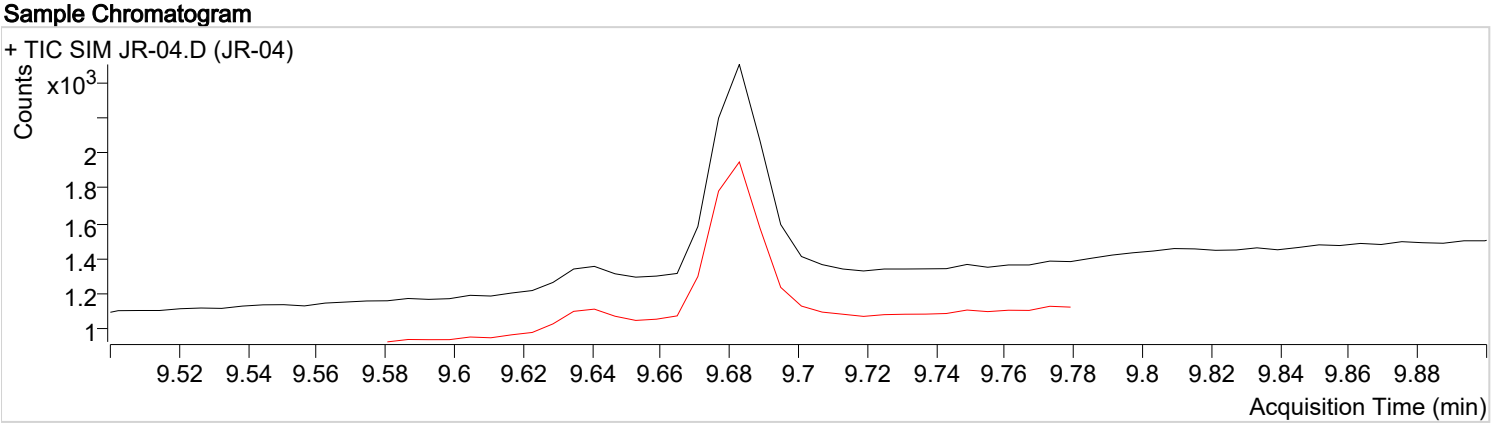

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 8:23:34	**Data File**	JR-05.D
Type	Sample	**Name**	JR-05
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

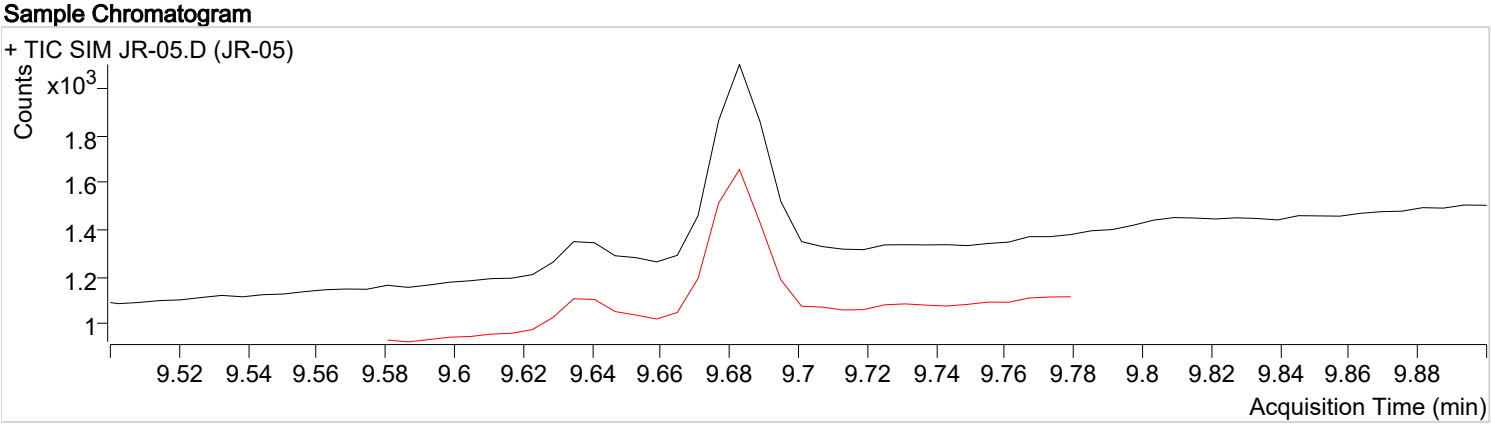

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 8:37:18	**Data File**	JR-06.D
Type	Sample	**Name**	JR-06
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

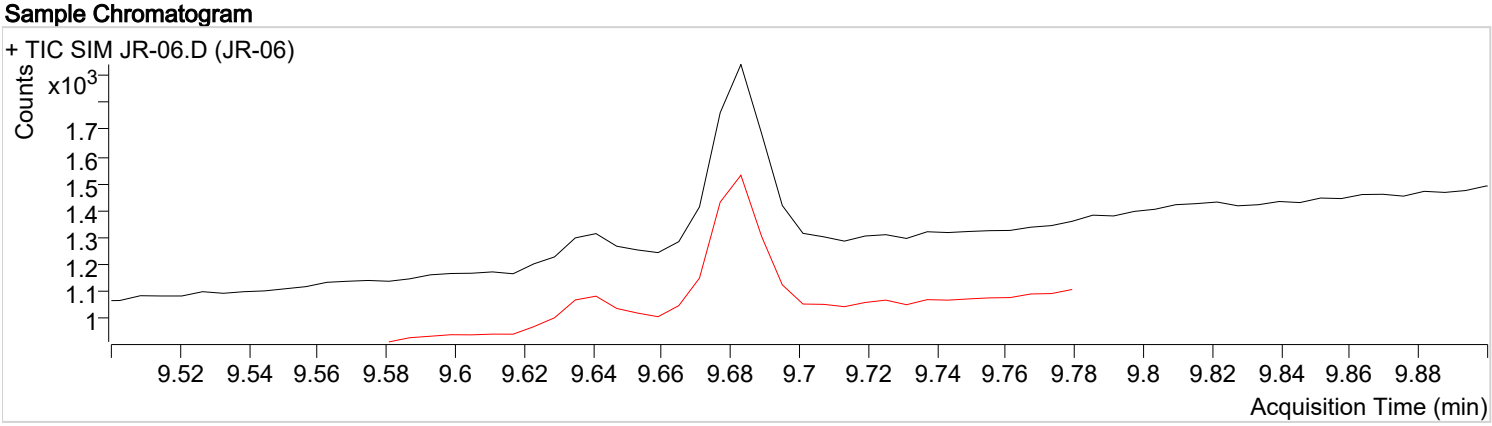

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 8:51:01	**Data File**	JR-07.D
Type	Sample	**Name**	JR-07
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

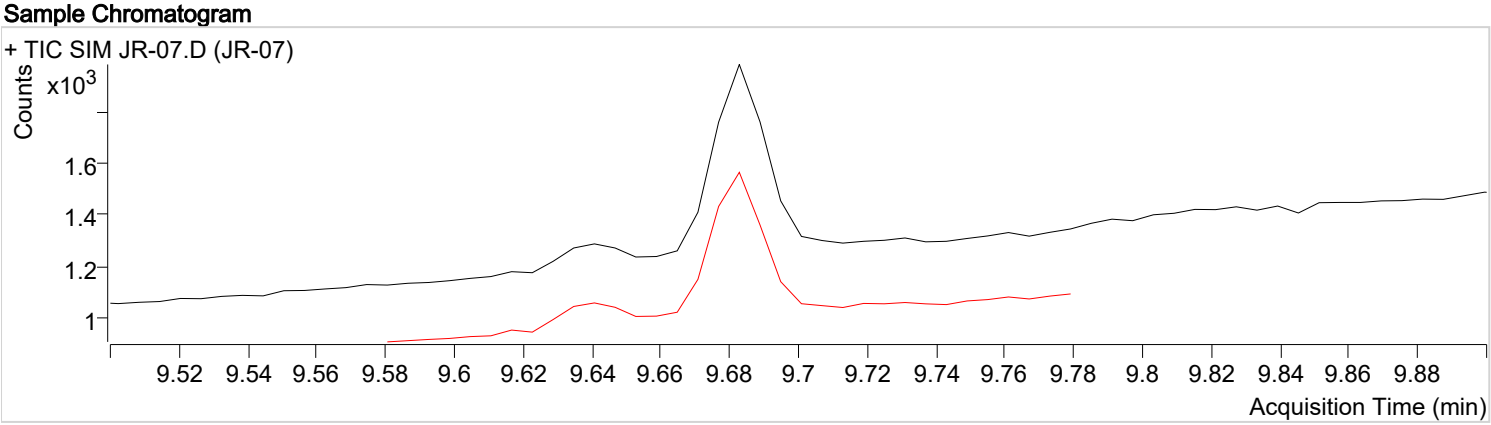

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 9:04:46	**Data File**	JR-08.D
Type	Sample	**Name**	JR-08
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

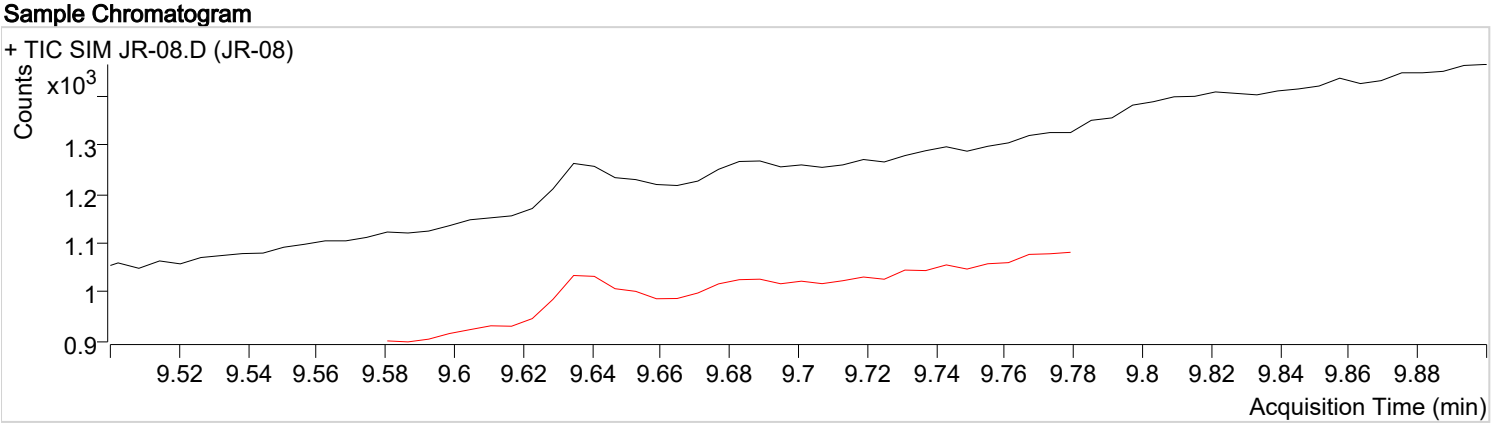

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 9:18:30	**Data File**	KD-01.D
Type	Sample	**Name**	KD-01
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

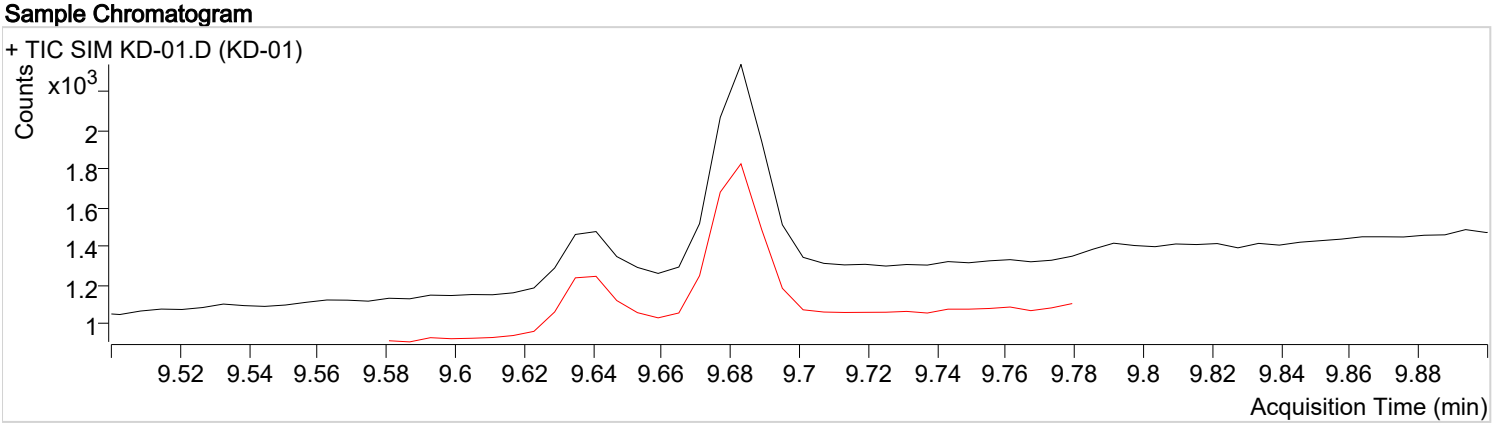

Di-Phtalate





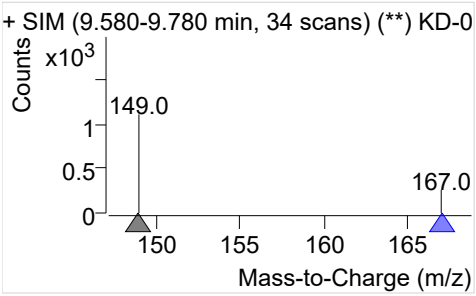

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 9:32:17	**Data File**	KD-02.D
Type	Sample	**Name**	KD-02
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

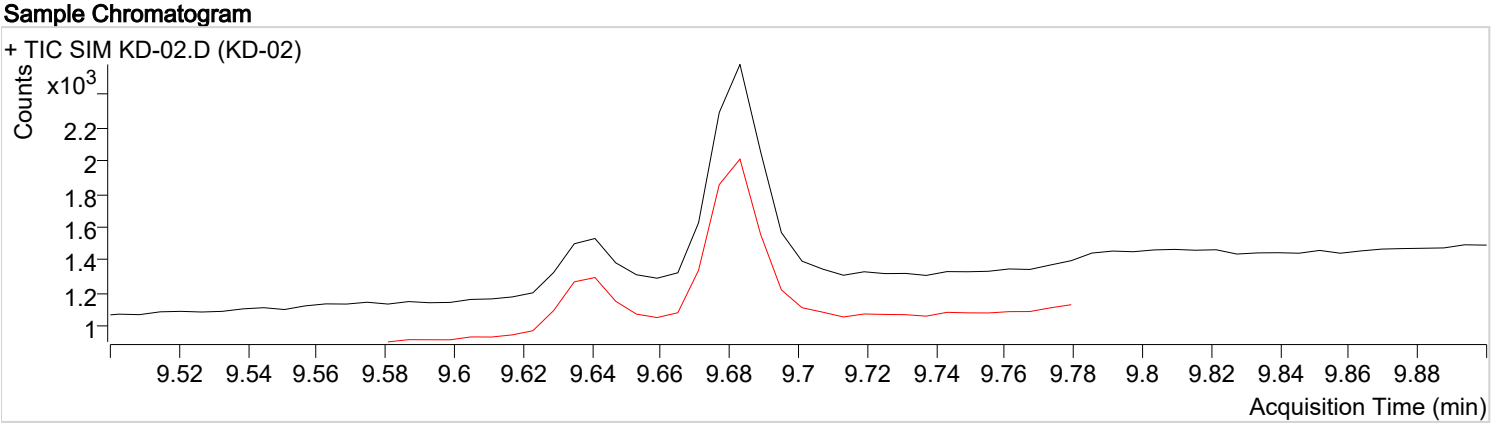

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 9:46:02	**Data File**	KD-04.D
Type	Sample	**Name**	KD-04
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

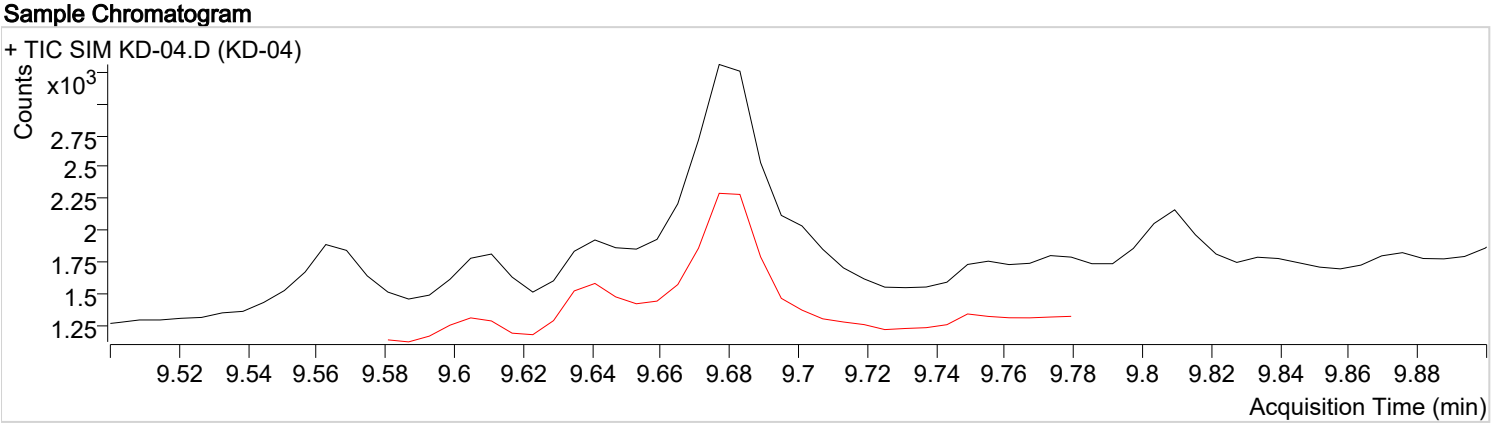

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 9:59:44	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

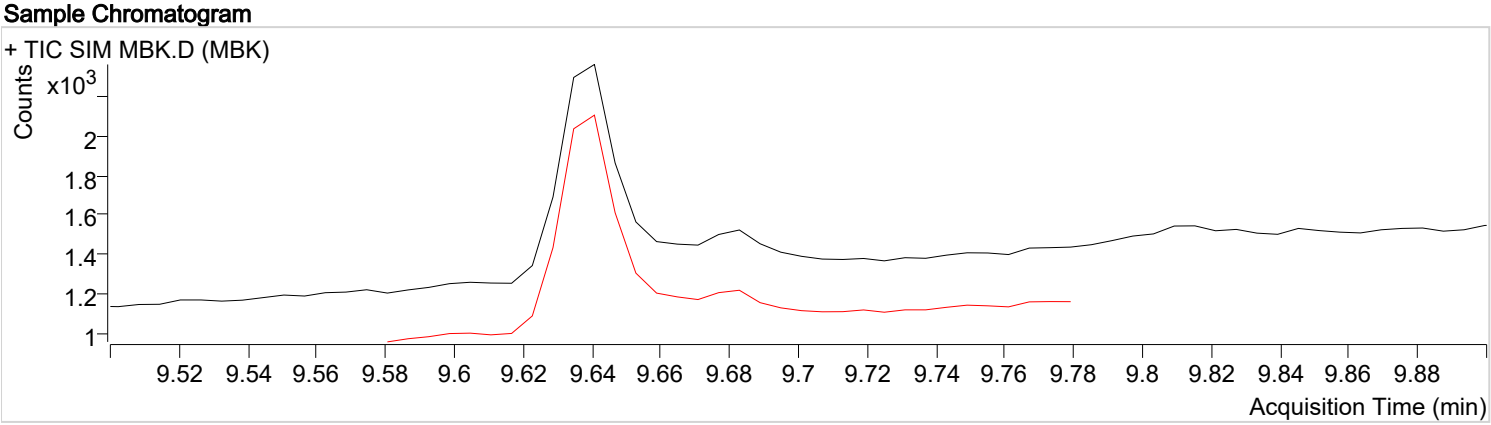

Di-Phtalate





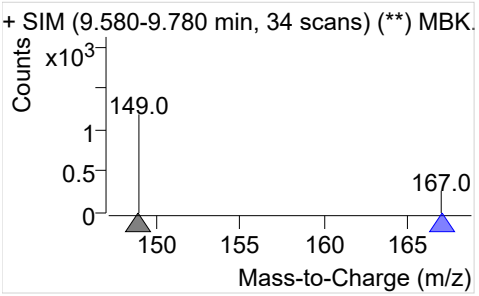

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(KD 2.4, JR 2.5)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-10 오전 11:02:00	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:52:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-10 오전 11:02:00	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-09 오후 10:13:29	**Data File**	CCV.D
Type	QC	**Name**	CCV
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

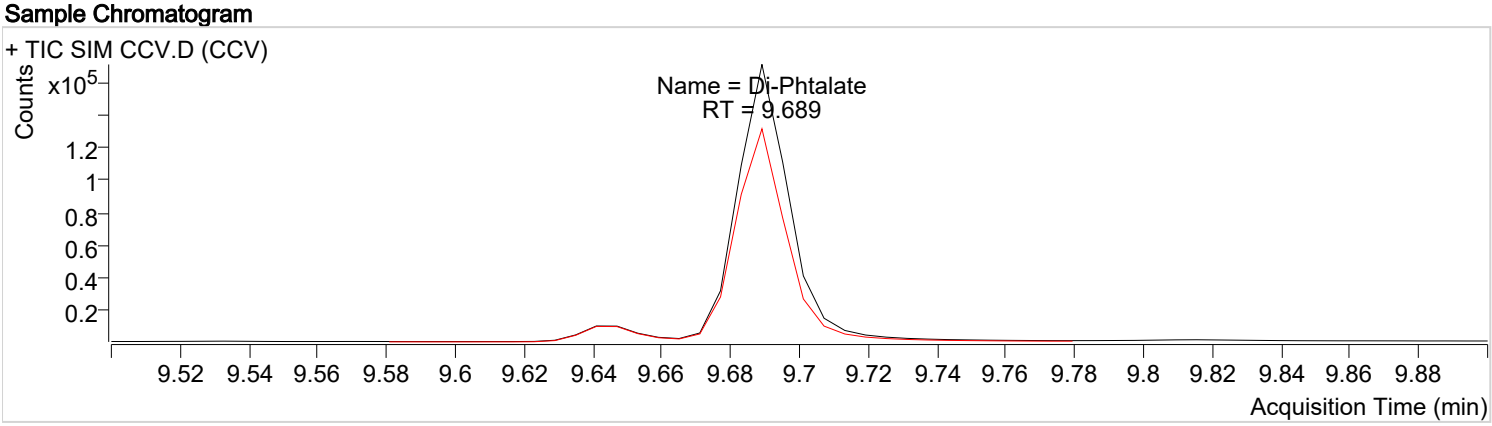

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.689	136744	0.0085	mg/L
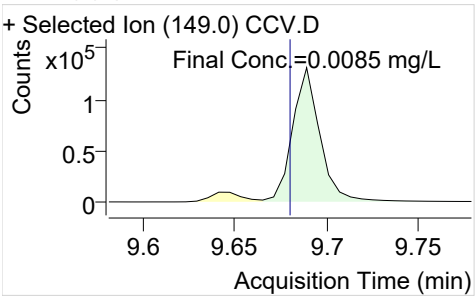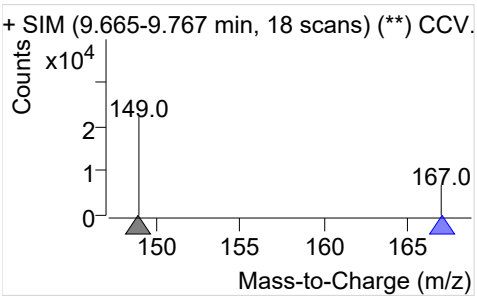
Di-Phtalate