Quantitative Analysis Results Summary Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin				
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Di-Phtalate

Data File	Type	RT	Resp.	Final Conc.
DEHP ST-01.D	Cal	9.689	12039	0.0024
DEHP ST-02.D	Cal	9.683	24751	0.0046
DEHP ST-03.D	Cal	9.683	40536	0.0074
DEHP ST-04.D	Cal	9.683	59362	0.0108
DEHP ST-05.D	Cal	9.689	83486	0.0150
DEHP ST-06.D	Cal	9.689	109808	0.0197
BK-.D	Blank			ND
FBK(GS 26-02-10).D	Blank			ND
KH 26-02-10.D	Sample			ND
GS-01.D	Sample			ND
GS-02.D	Sample			ND
GS-03.D	Sample			ND
GS-04.D	Sample			ND
GS-05.D	Sample			ND
GS-06.D	Sample			ND
GS-07.D	Sample			ND
GS-08.D	Sample			ND
GS-09.D	Sample			ND
GS-10.D	Sample			ND
GS-11.D	Sample			ND
GS-12.D	Sample			ND
GS-13.D	Sample			ND
GS-14.D	Sample			ND
GS-15.D	Sample			ND
GS-16.D	Sample			ND
MBK-1.D	Blank			ND
-CCV-1.D	QC	9.683	56822	0.0103
GS-17.D	Sample			ND
GS-18.D	Sample			ND
GS-19.D	Sample			ND
GS-20.D	Sample			ND
GS-21.D	Sample			ND
GS-22.D	Sample			ND
GS-23.D	Sample			ND
GS-24.D	Sample			ND
MBK-2.D	Blank			ND
-CCV-2.D	QC	9.683	53349	0.0097

Di-Phtalate

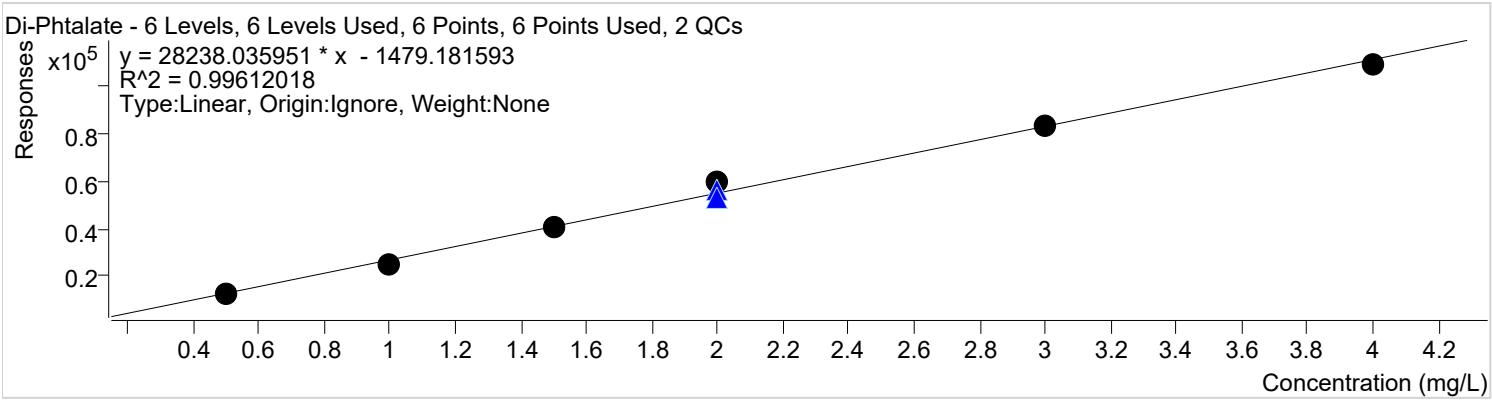

Cal. Path	Type	Level	Enable	Conc.	Response
\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\DEHP ST-01.D	Calibration	1	x	0.500	12039
\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\DEHP ST-02.D	Calibration	2	x	1.000	24751
\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\DEHP ST-03.D	Calibration	3	x	1.500	40536
\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\DEHP ST-04.D	Calibration	4	x	2.000	59362
\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\-CCV-1.D	QC	4	x	2.000	56822
\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\-CCV-2.D	QC	4	x	2.000	53349
\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\DEHP ST-05.D	Calibration	5	x	3.000	83486
\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\DEHP ST-06.D	Calibration	6	x	4.000	109808

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 4:39:13	**Data File**	DEHP ST-01.D
Type	Cal	**Name**	DEHP ST-01
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

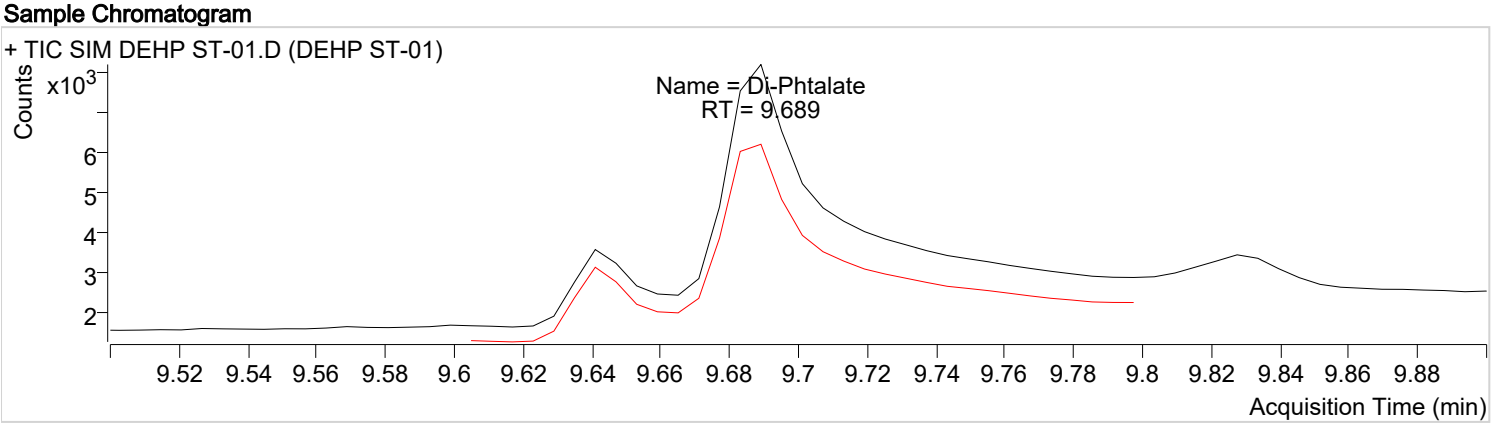

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.689	12039	0.0024	mg/L

Di-Phtalate



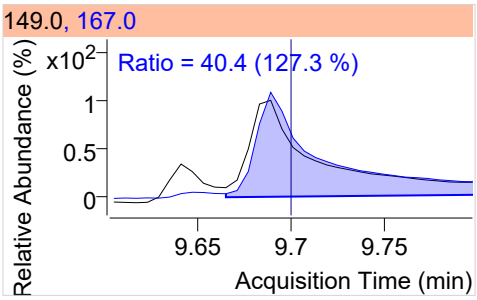

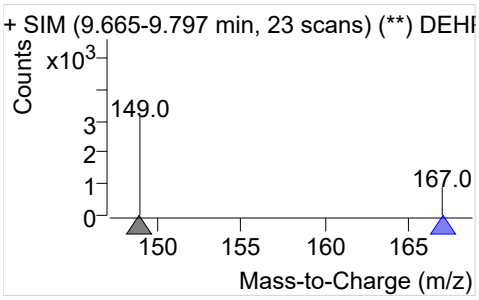

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 4:52:59	**Data File**	DEHP ST-02.D
Type	Cal	**Name**	DEHP ST-02
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

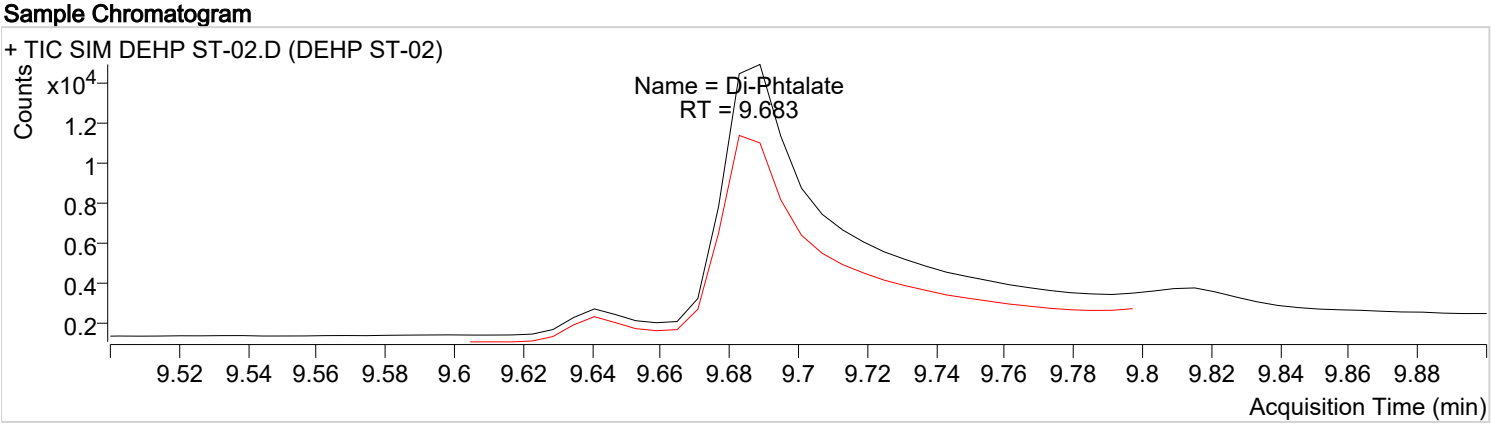

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.683	24751	0.0046	mg/L

Di-Phtalate

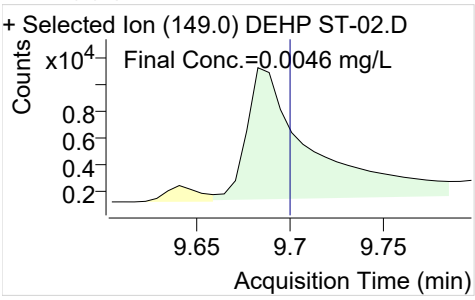

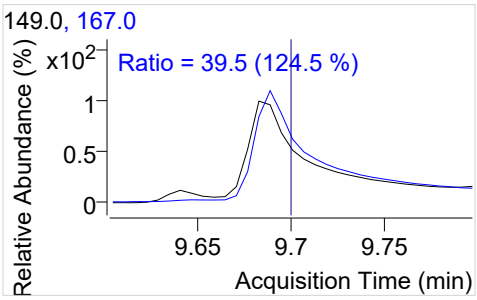

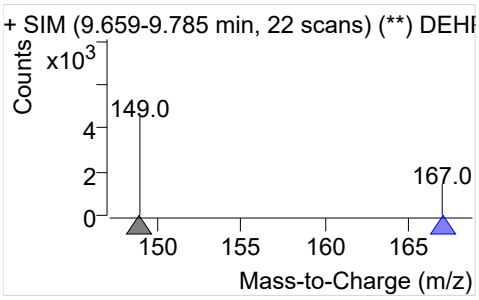

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 5:06:44	**Data File**	DEHP ST-03.D
Type	Cal	**Name**	DEHP ST-03
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

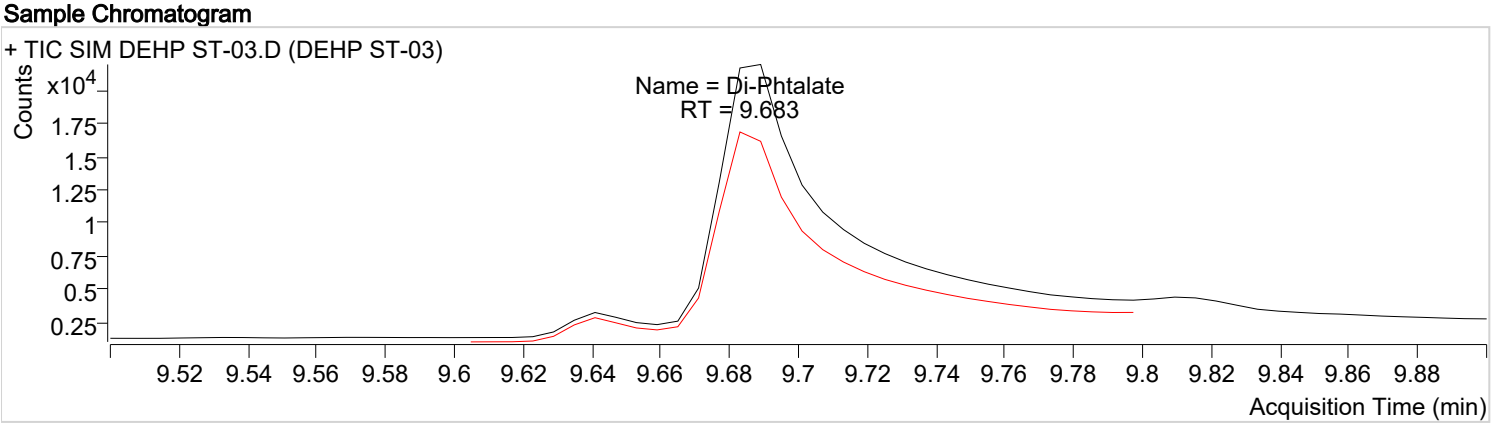

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.683	40536	0.0074	mg/L

Di-Phtalate

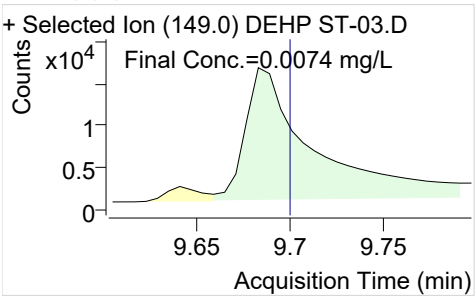

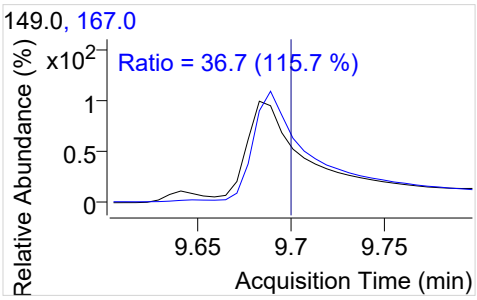

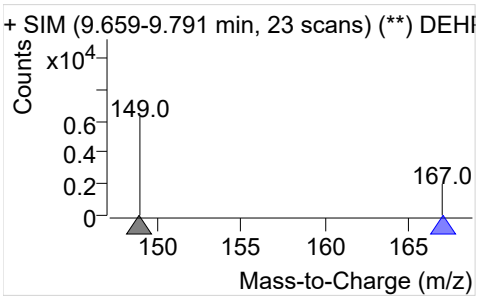

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 5:20:29	**Data File**	DEHP ST-04.D
Type	Cal	**Name**	DEHP ST-04
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

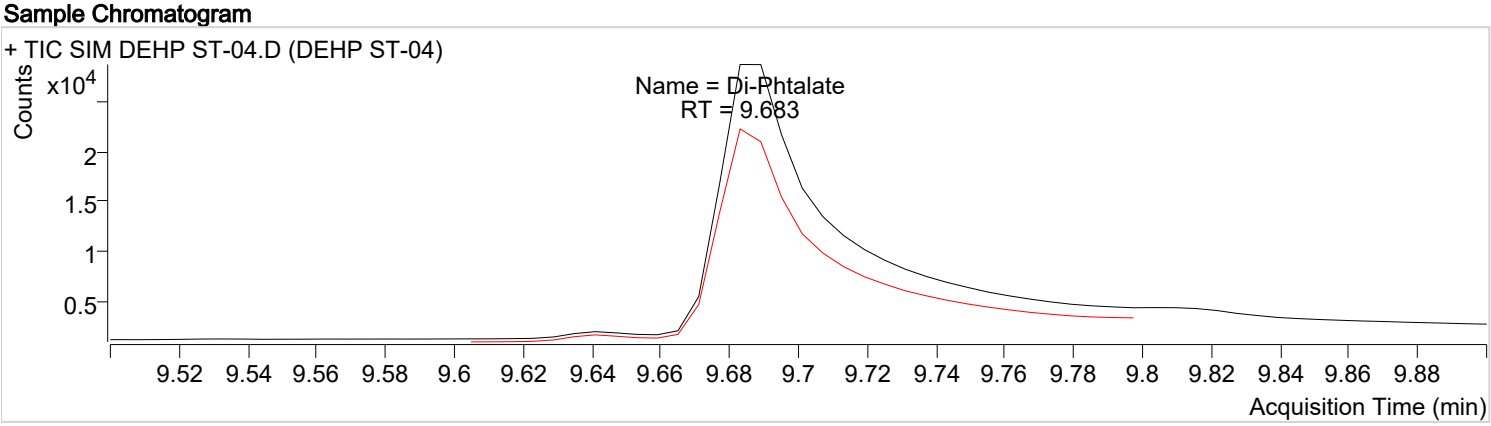

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.683	59362	0.0108	mg/L

Di-Phtalate

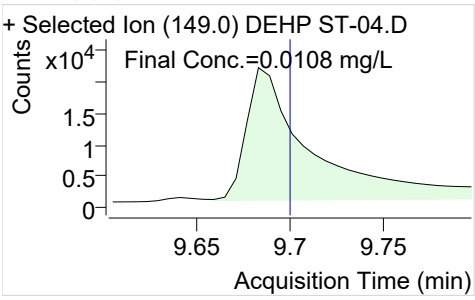

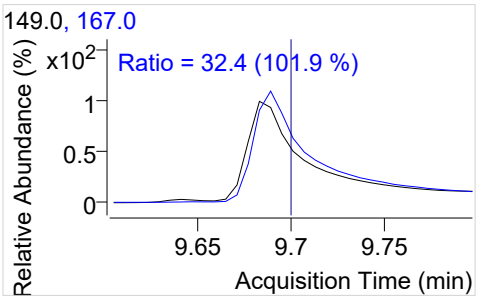

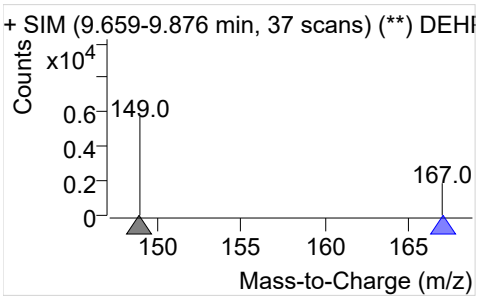

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 5:34:15	**Data File**	DEHP ST-05.D
Type	Cal	**Name**	DEHP ST-05
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

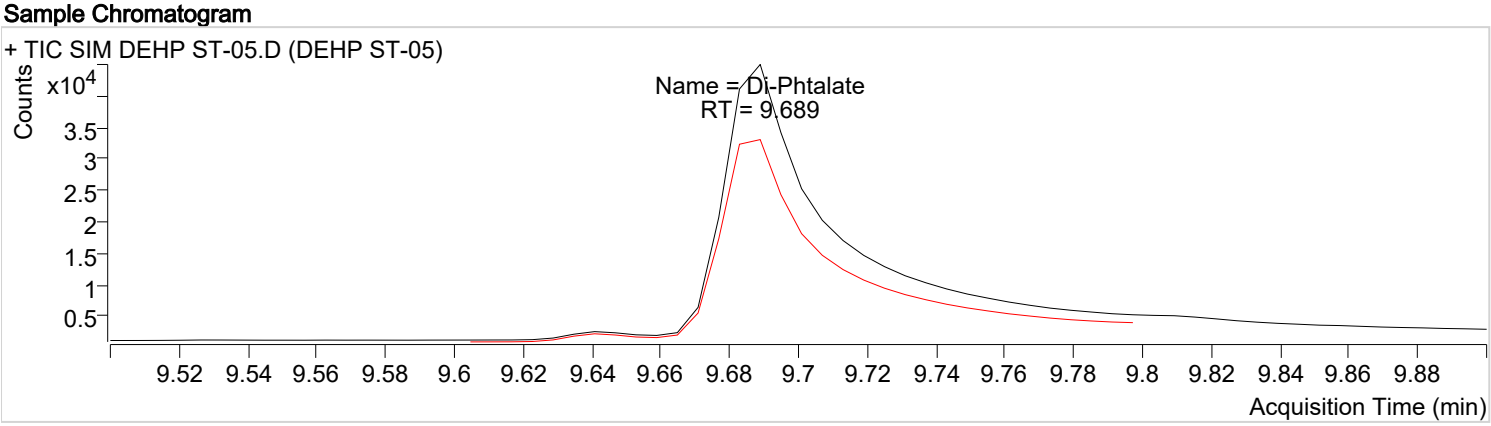

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.689	83486	0.0150	mg/L

Di-Phtalate

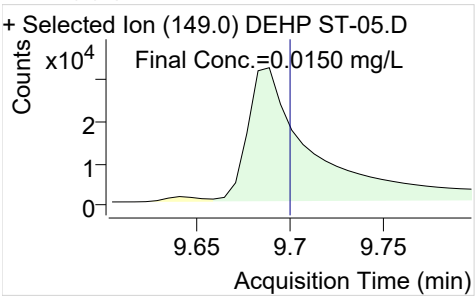

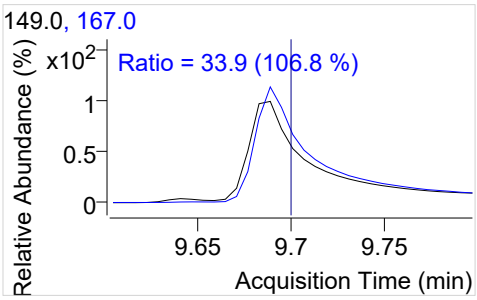

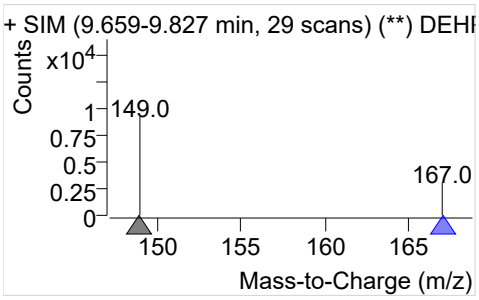

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 5:48:03	**Data File**	DEHP ST-06.D
Type	Cal	**Name**	DEHP ST-06
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

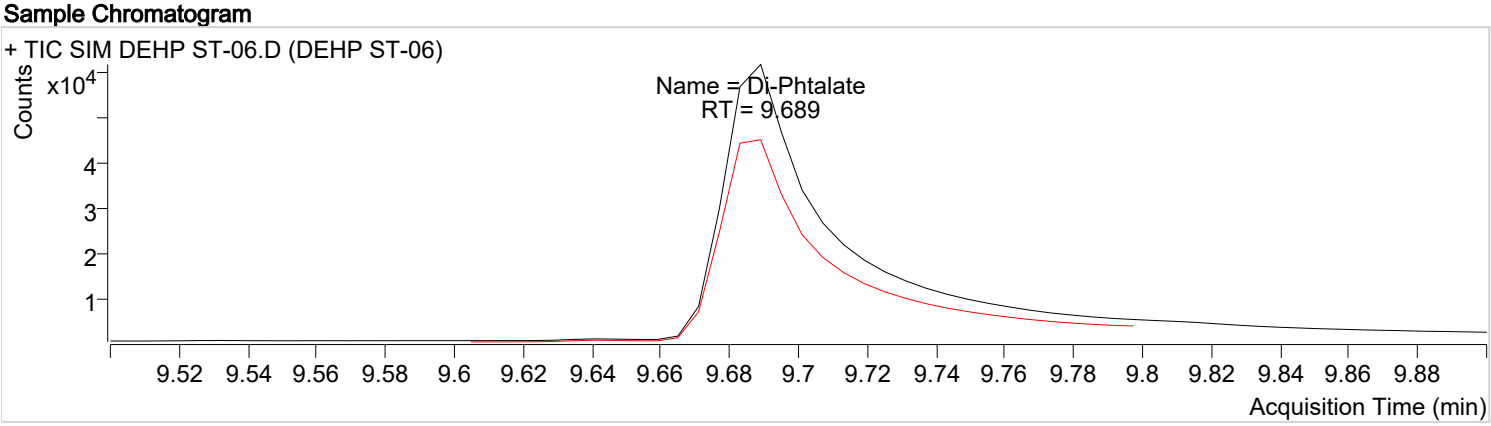

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.689	109808	0.0197	mg/L

Di-Phtalate

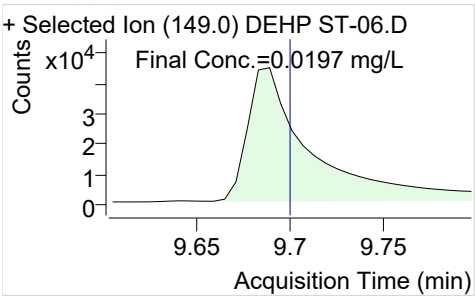

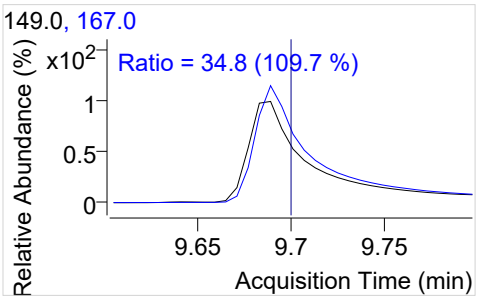

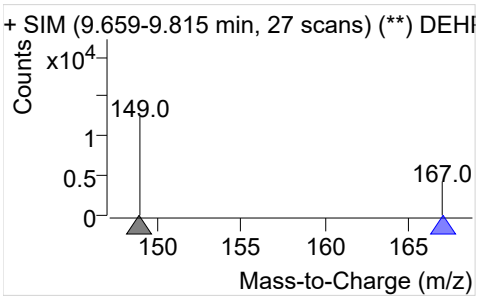

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 6:15:31	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

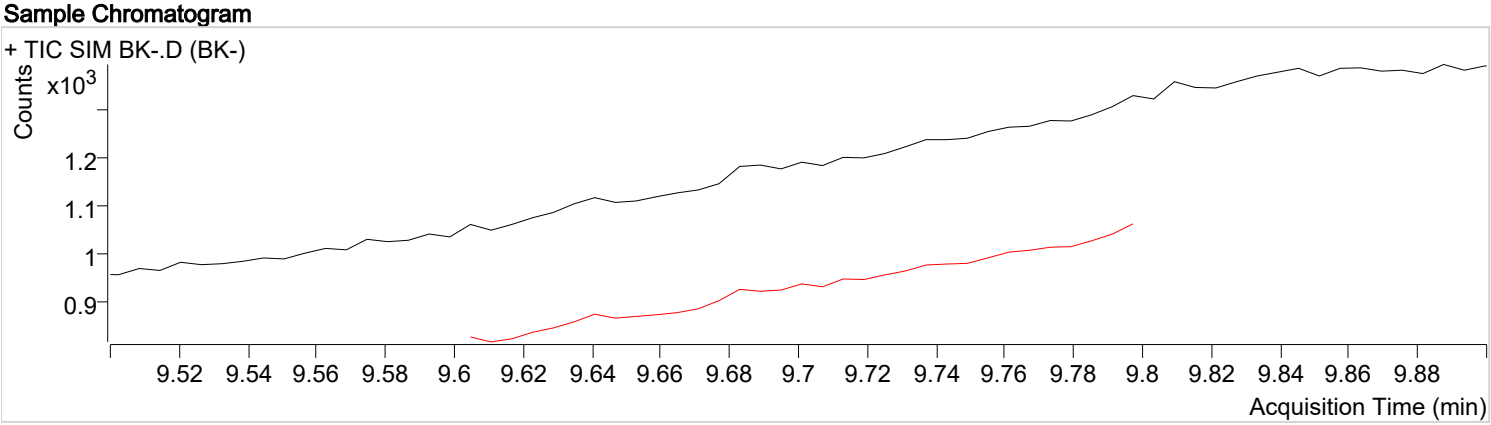

Di-Phtalate





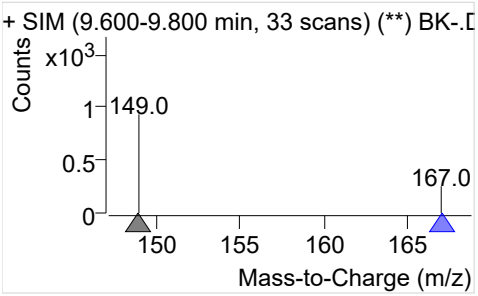

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 6:29:16	**Data File**	FBK(GS 26-02-10).D
Type	Blank	**Name**	FBK(GS 26-02-10)
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

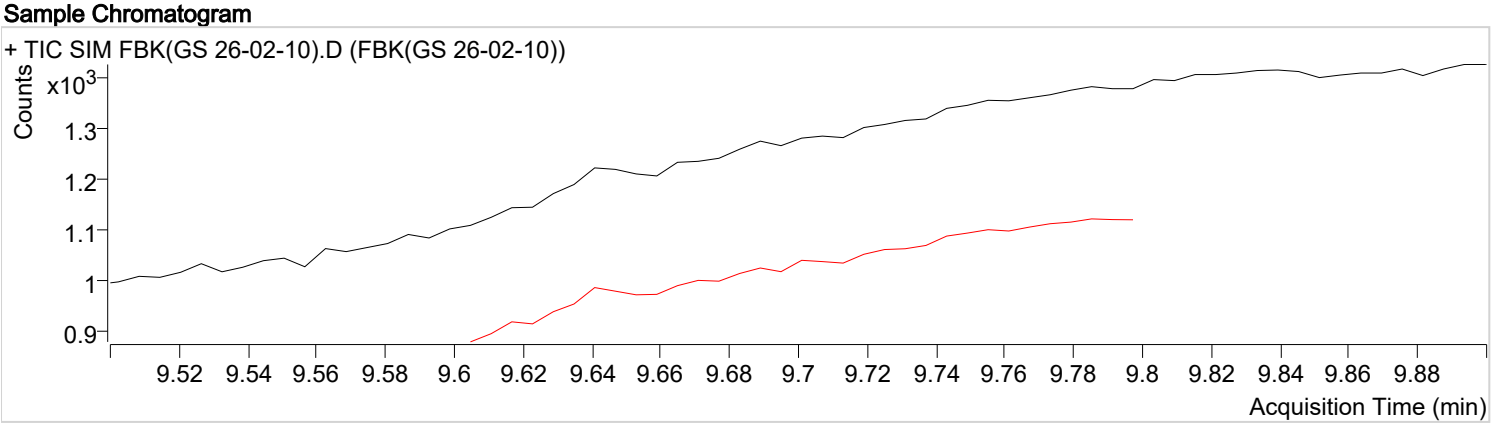

Di-Phtalate





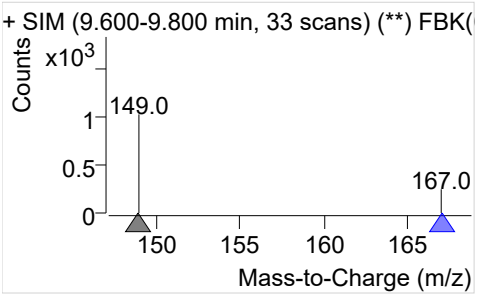

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 6:43:03	**Data File**	KH 26-02-10.D
Type	Sample	**Name**	KH 26-02-10
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

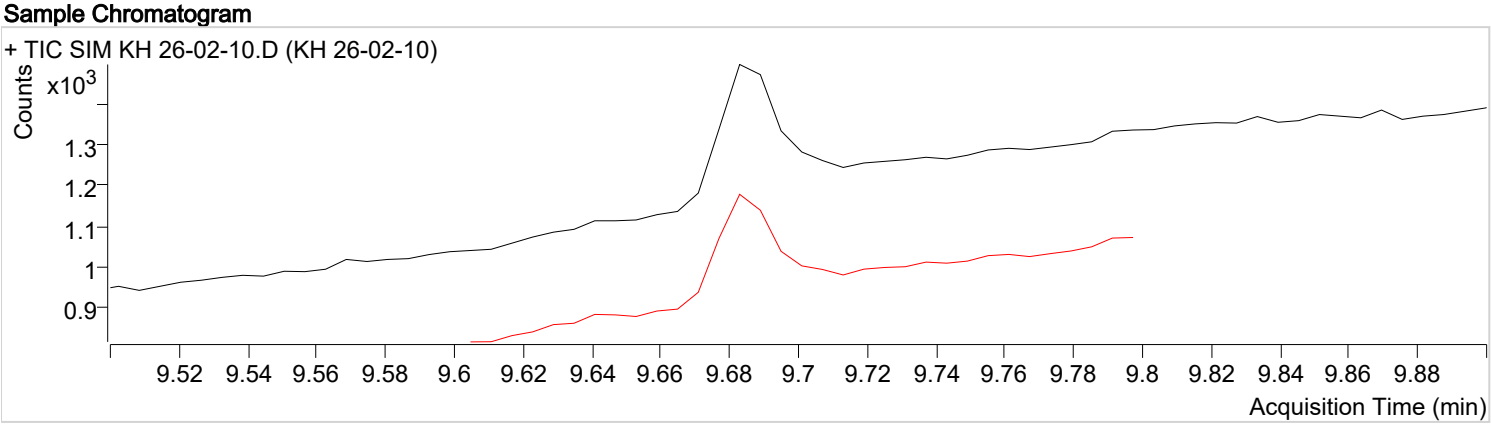

Di-Phtalate





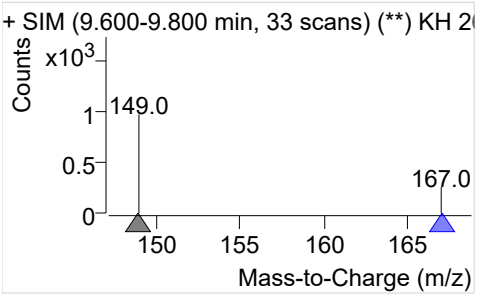

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 6:56:45	**Data File**	GS-01.D
Type	Sample	**Name**	GS-01
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

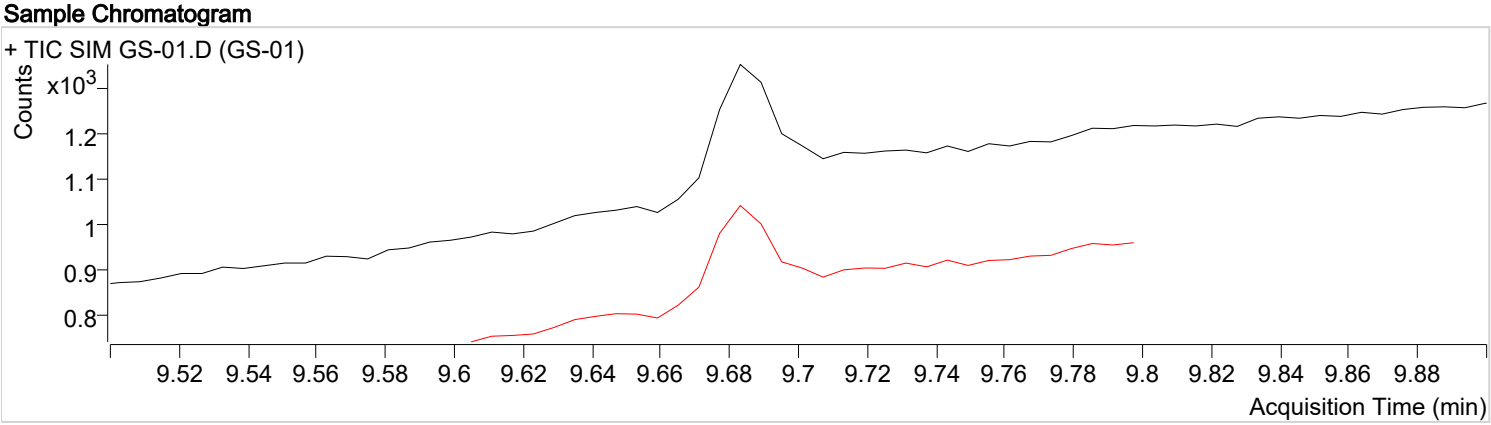

Di-Phtalate





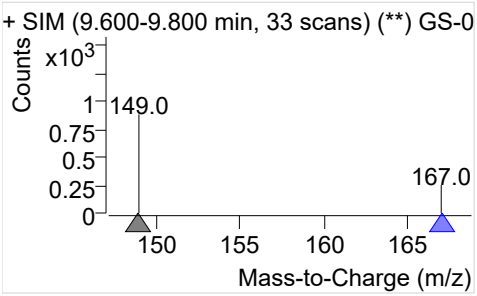

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 7:10:30	**Data File**	GS-02.D
Type	Sample	**Name**	GS-02
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

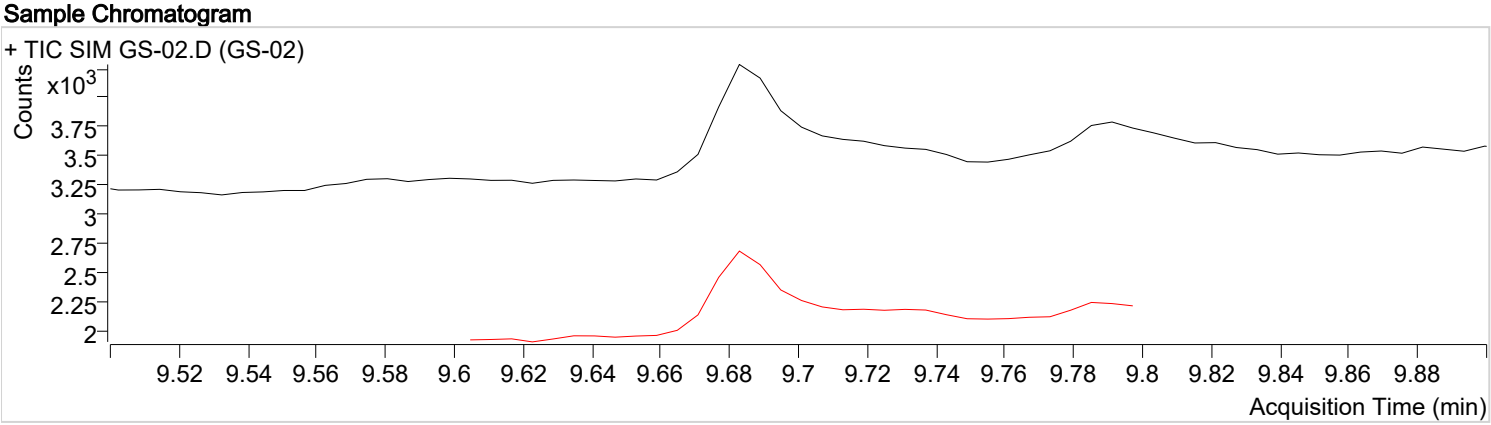

Di-Phtalate





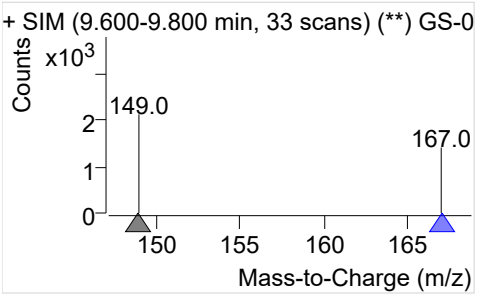

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 7:24:14	**Data File**	GS-03.D
Type	Sample	**Name**	GS-03
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

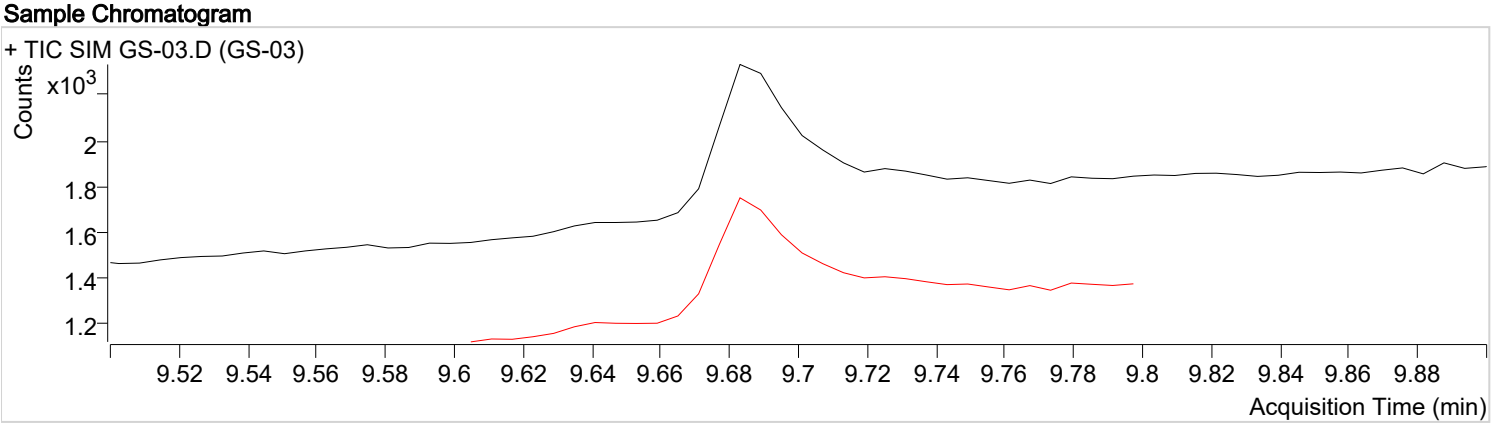

Di-Phtalate





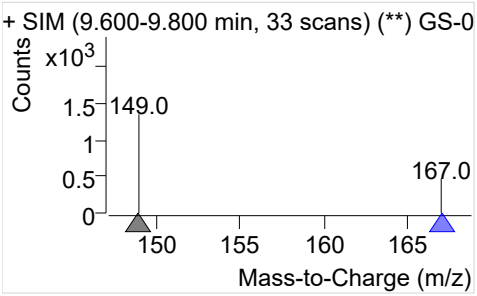

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 7:37:56	**Data File**	GS-04.D
Type	Sample	**Name**	GS-04
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

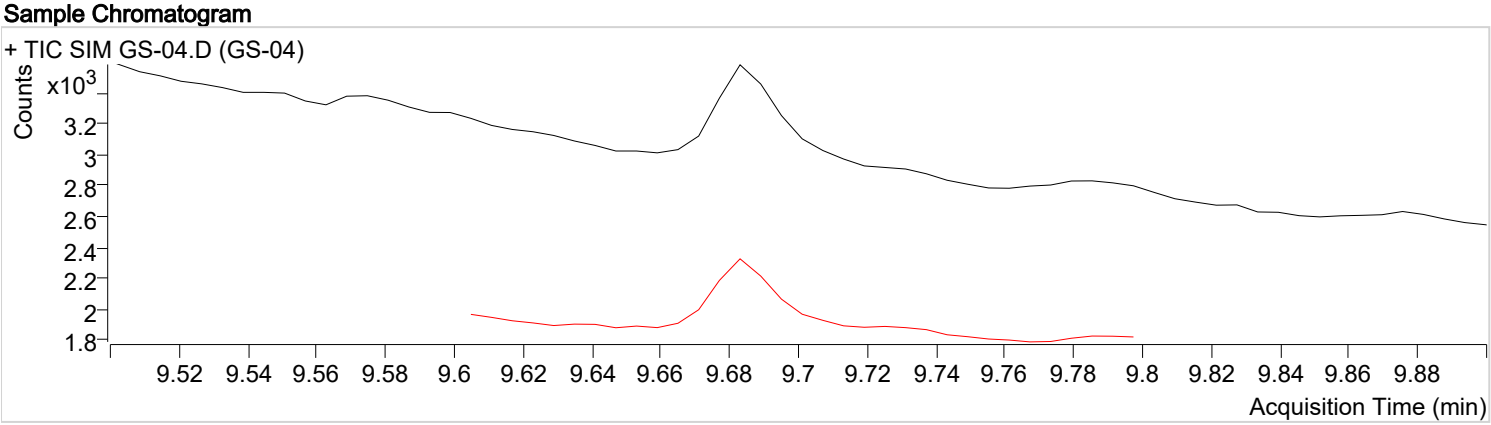

Di-Phtalate





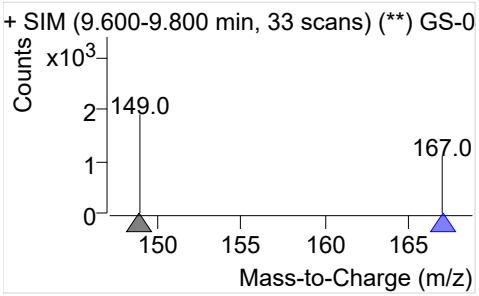

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 7:51:41	**Data File**	GS-05.D
Type	Sample	**Name**	GS-05
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

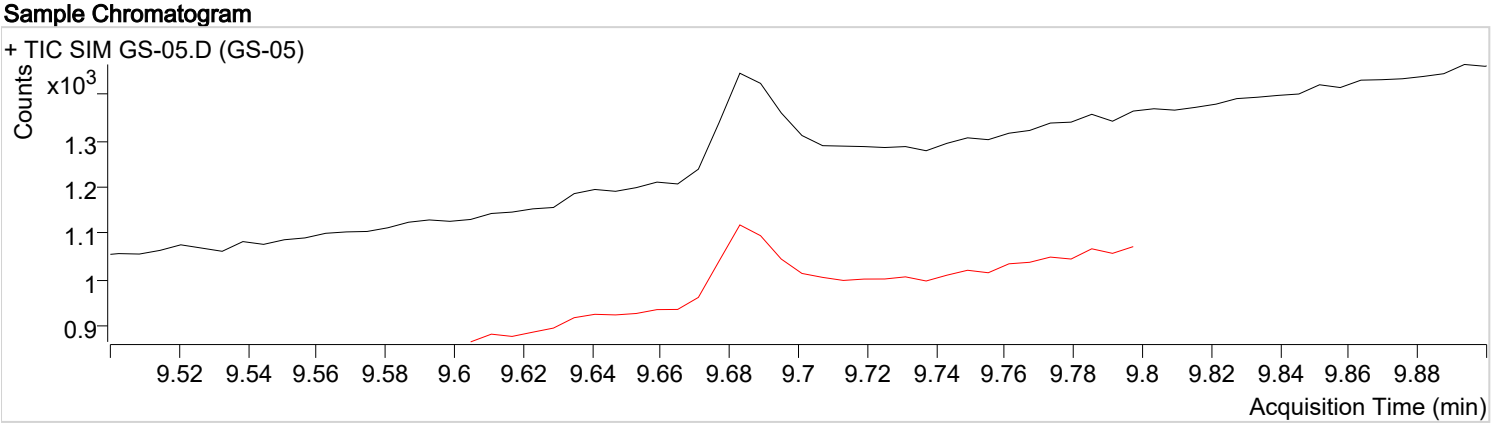

Di-Phtalate





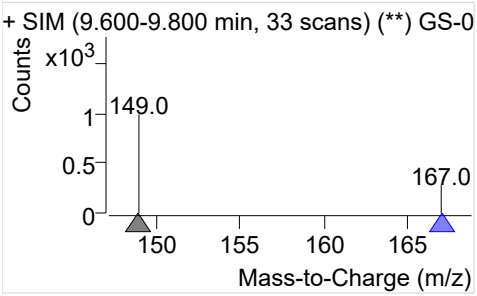

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 8:05:25	**Data File**	GS-06.D
Type	Sample	**Name**	GS-06
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

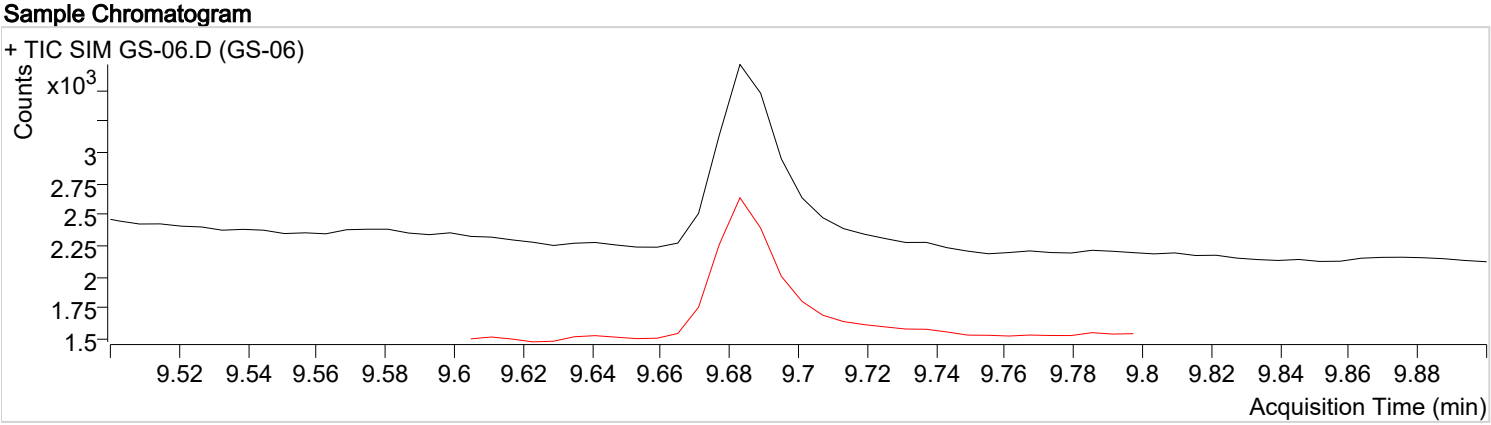

Di-Phtalate





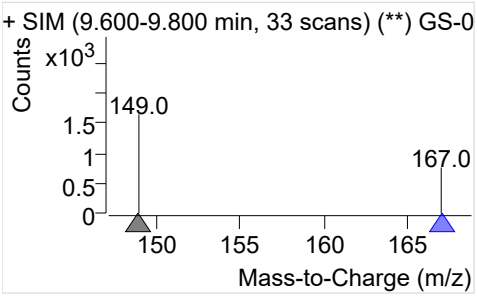

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 8:19:11	**Data File**	GS-07.D
Type	Sample	**Name**	GS-07
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

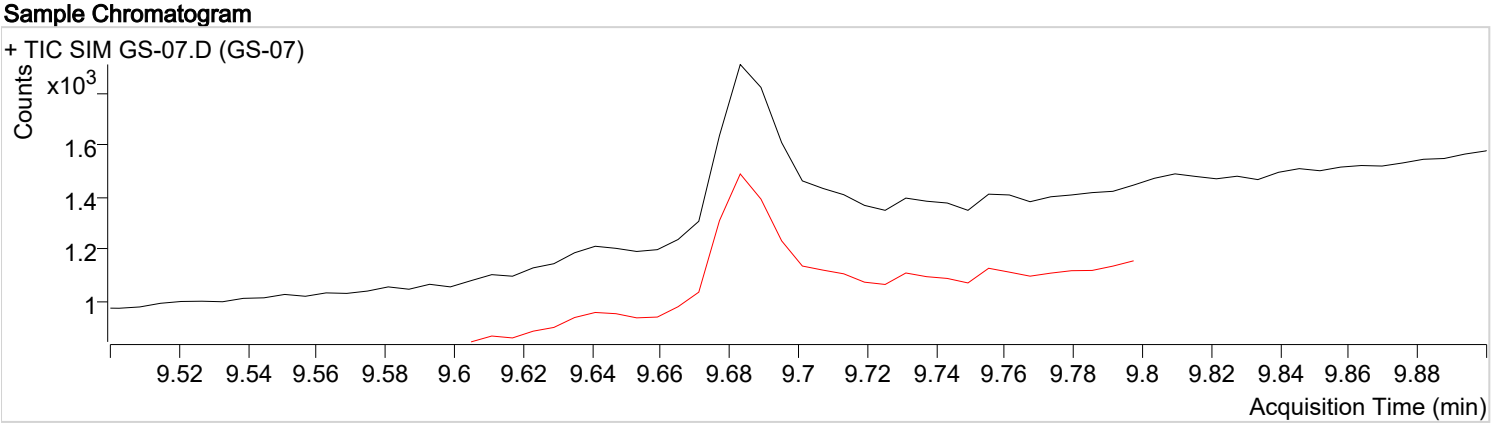

Di-Phtalate





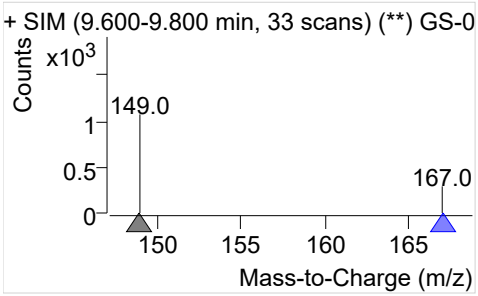

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 8:32:55	**Data File**	GS-08.D
Type	Sample	**Name**	GS-08
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

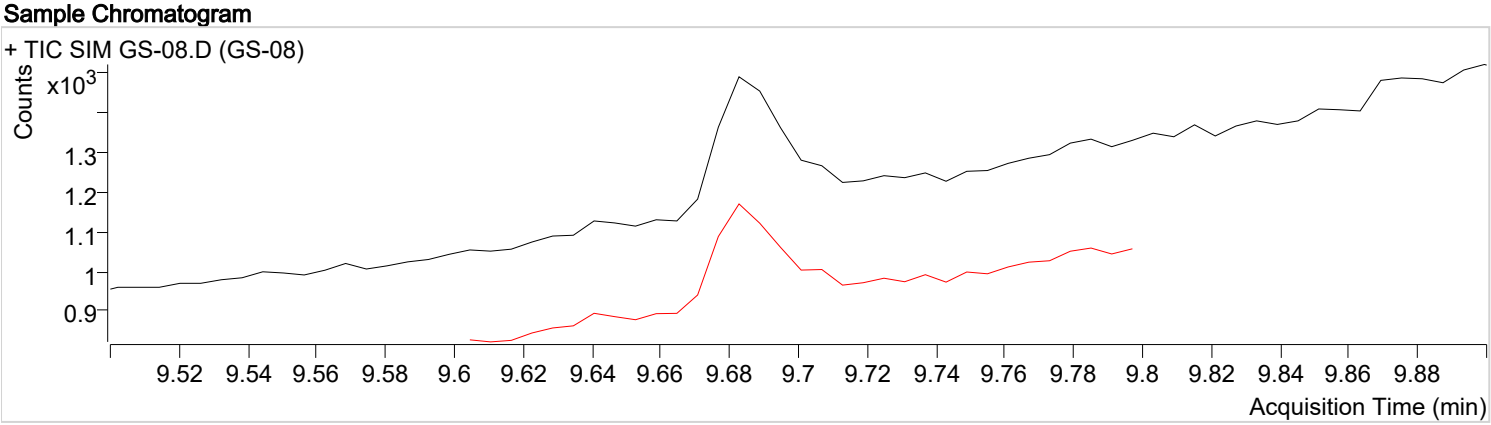

Di-Phtalate





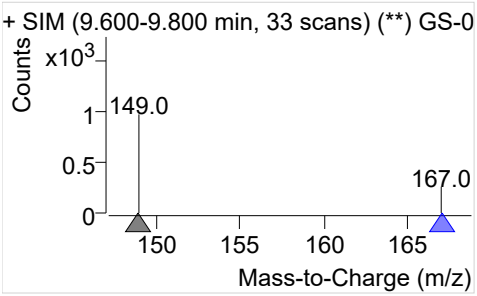

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 8:46:39	**Data File**	GS-09.D
Type	Sample	**Name**	GS-09
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

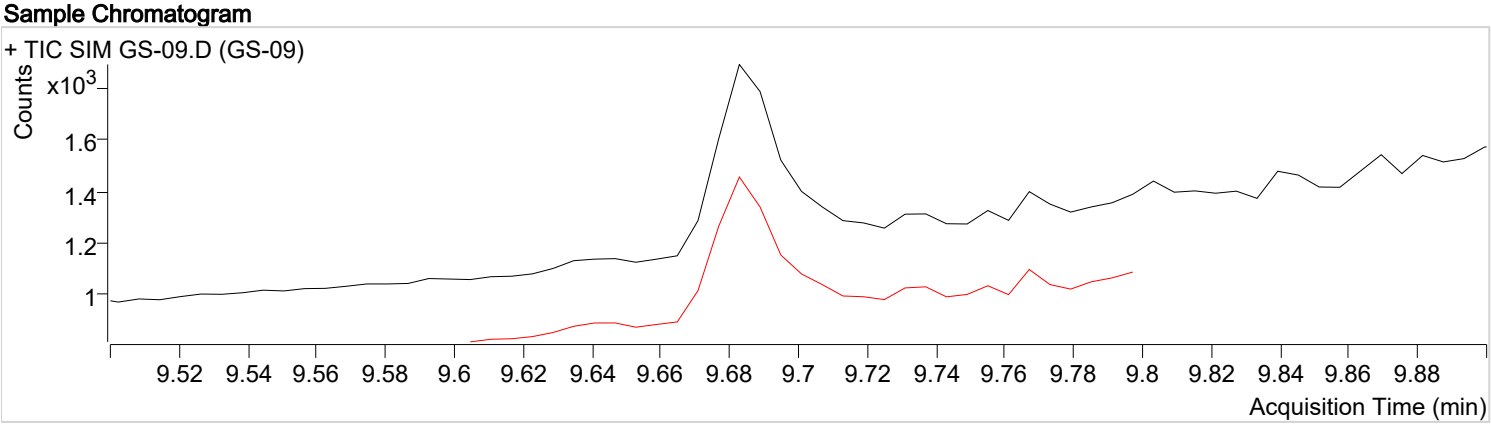

Di-Phtalate





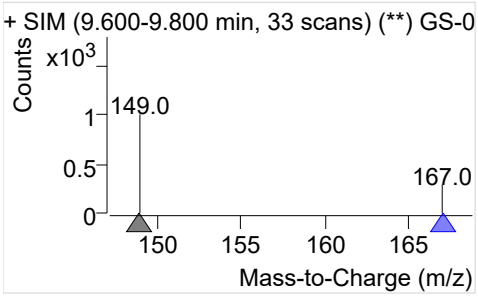

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 9:00:23	**Data File**	GS-10.D
Type	Sample	**Name**	GS-10
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

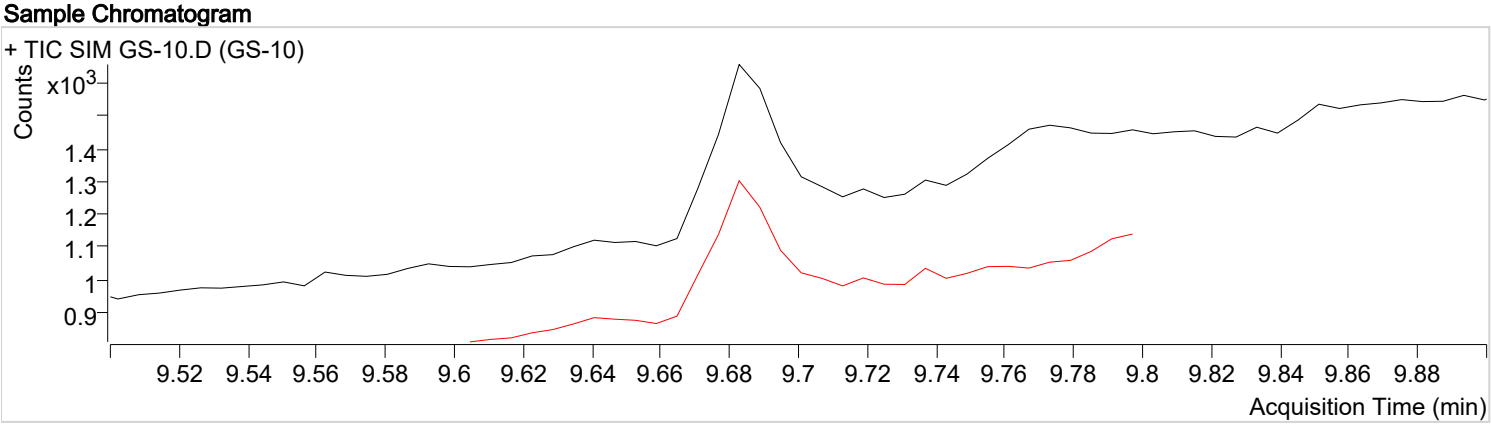

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 9:14:09	**Data File**	GS-11.D
Type	Sample	**Name**	GS-11
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

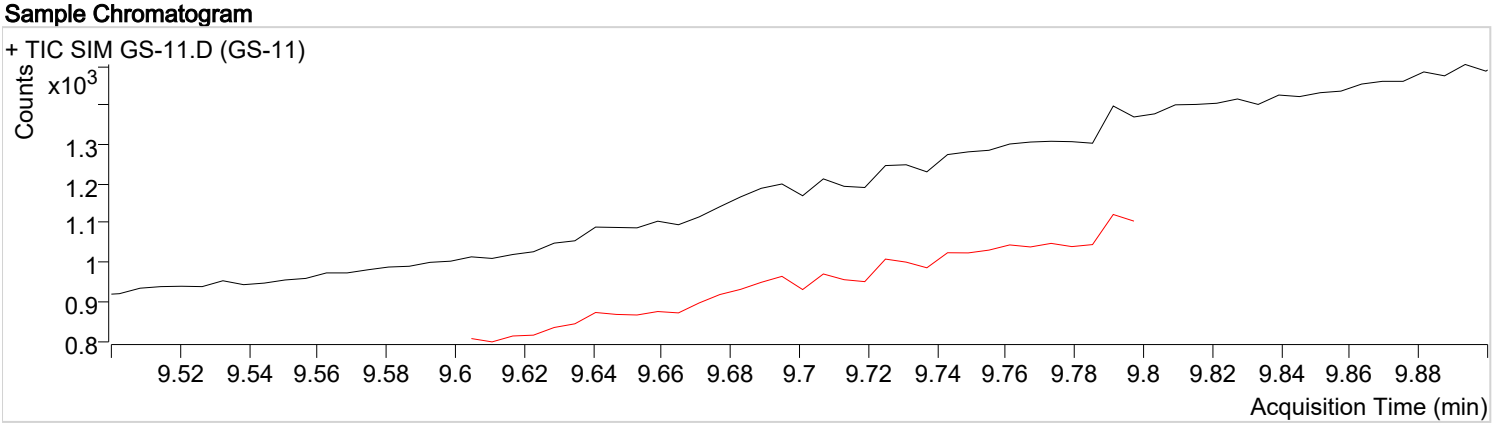

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 9:27:52	**Data File**	GS-12.D
Type	Sample	**Name**	GS-12
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

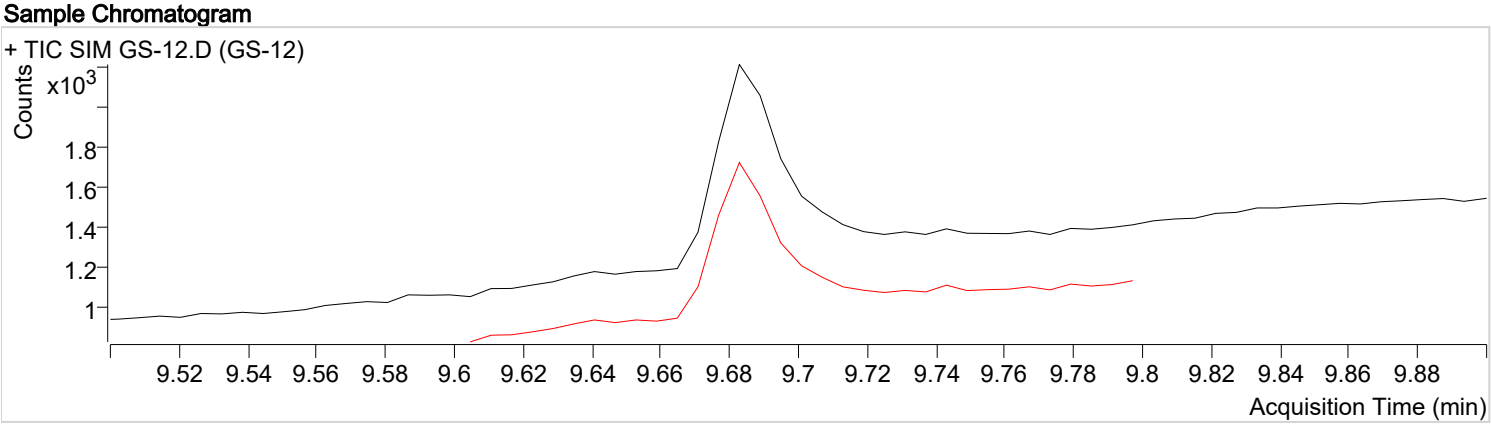

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 9:41:38	**Data File**	GS-13.D
Type	Sample	**Name**	GS-13
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

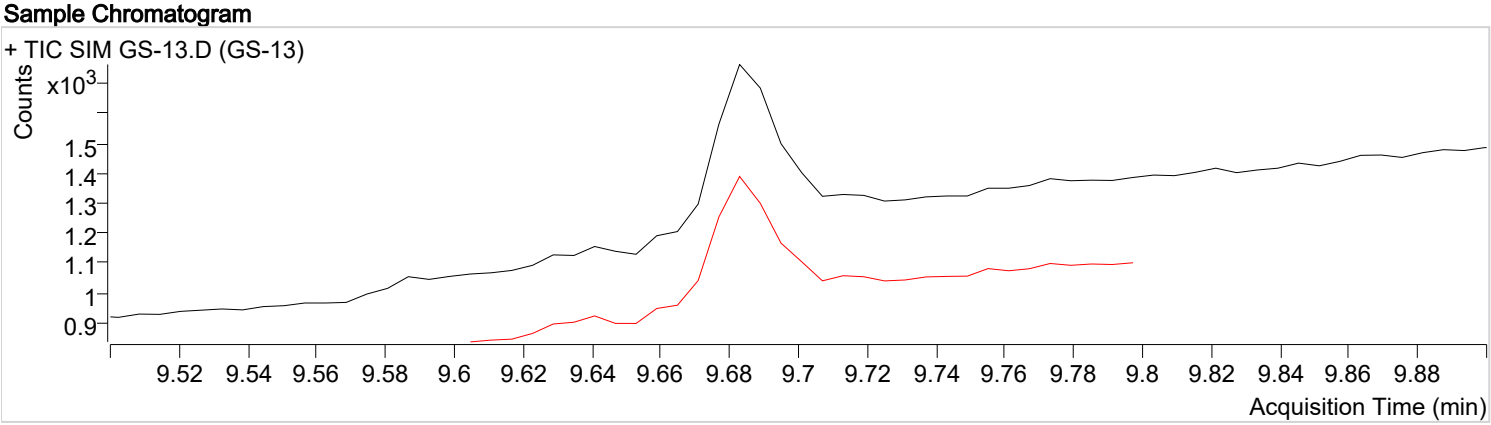

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 9:55:21	**Data File**	GS-14.D
Type	Sample	**Name**	GS-14
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

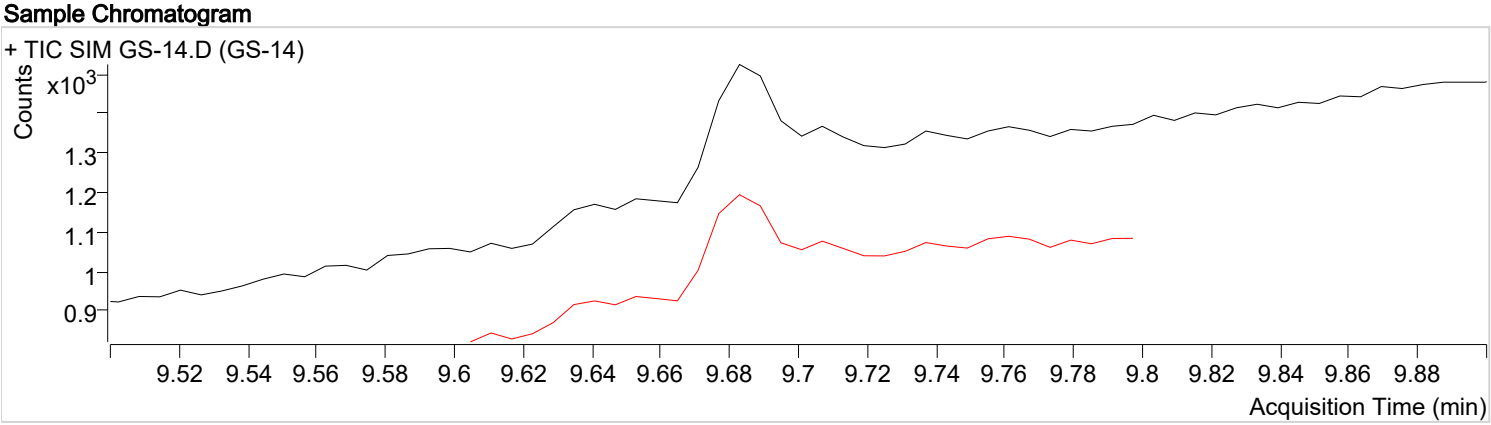

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 10:09:04	**Data File**	GS-15.D
Type	Sample	**Name**	GS-15
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

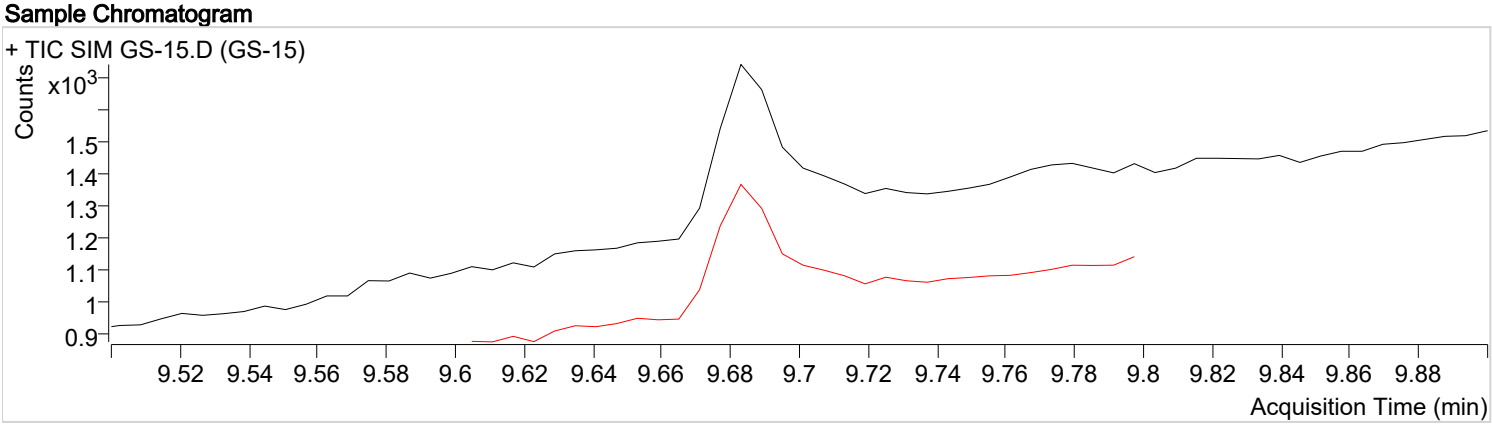

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 10:22:49	**Data File**	GS-16.D
Type	Sample	**Name**	GS-16
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

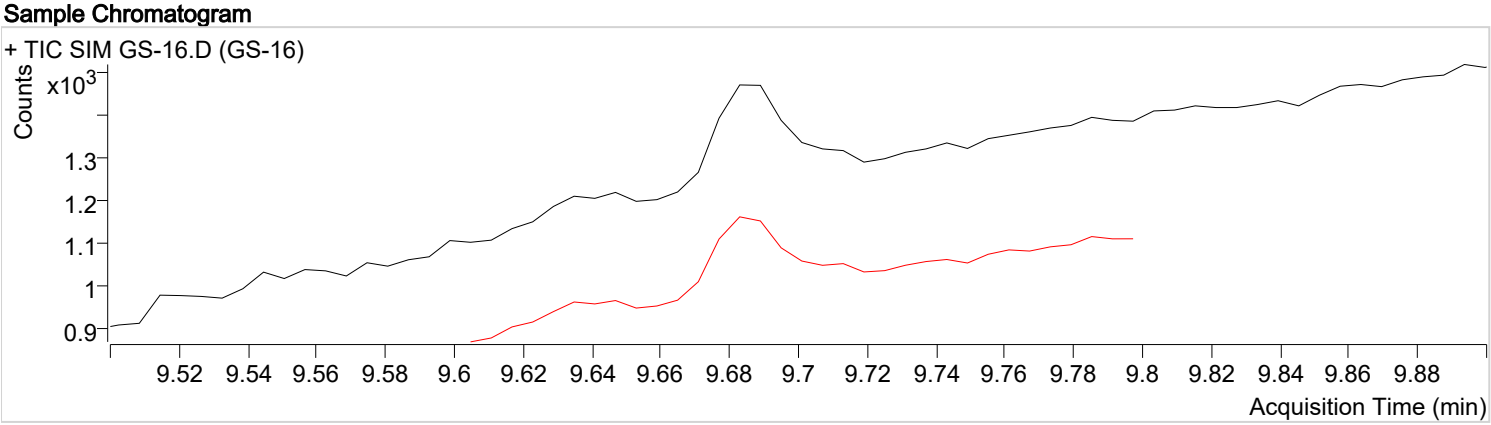

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 10:36:32	**Data File**	MBK-1.D
Type	Blank	**Name**	MBK-1
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

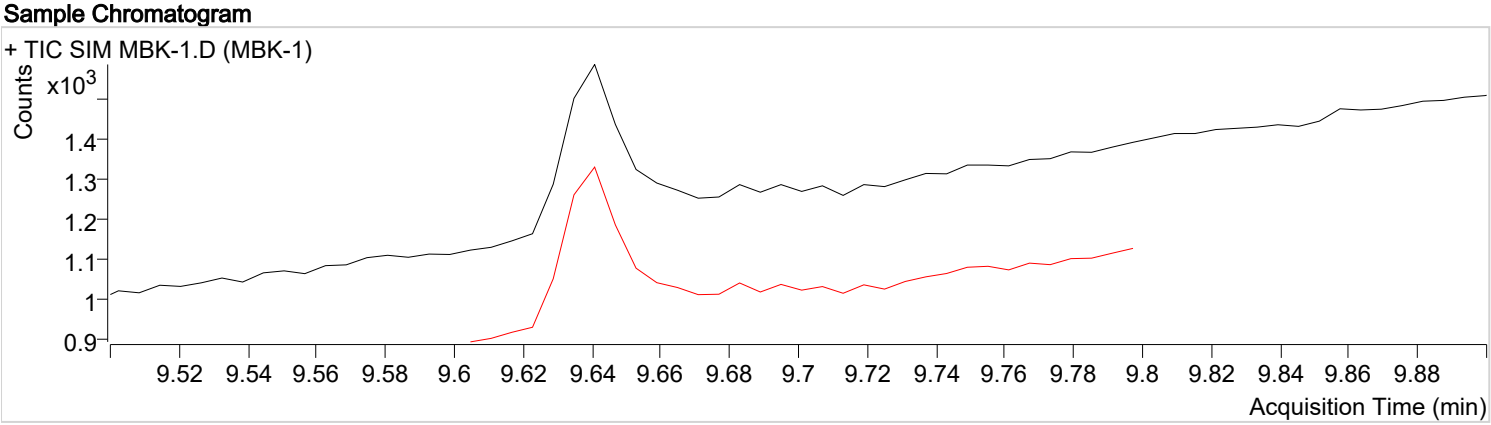

Di-Phtalate





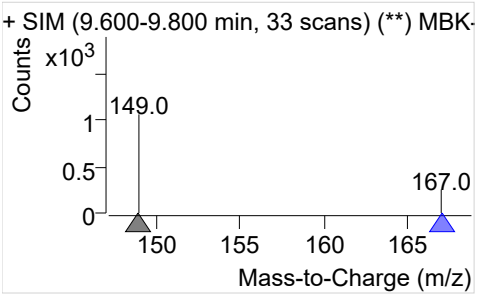

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 11:03:59	**Data File**	-CCV-1.D
Type	QC	**Name**	-CCV-1
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

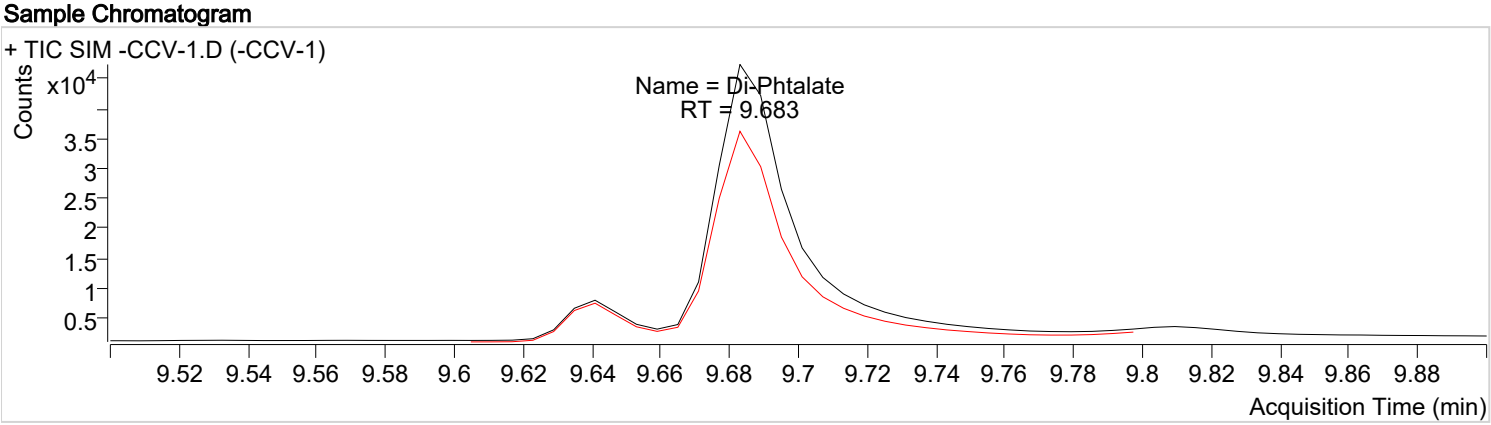

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.683	56822	0.0103	mg/L

Di-Phtalate



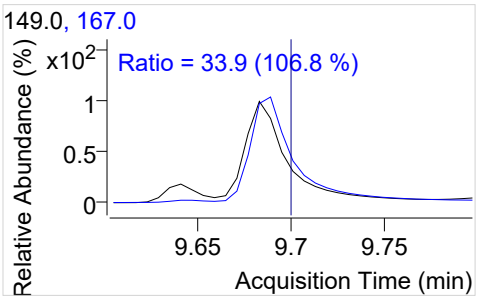

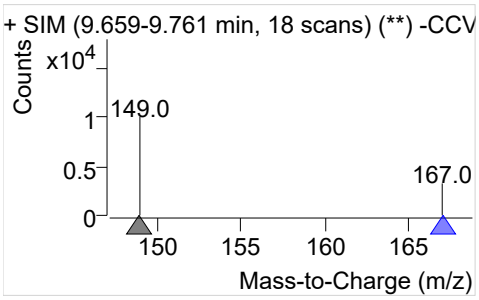

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 11:31:27	**Data File**	GS-17.D
Type	Sample	**Name**	GS-17
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

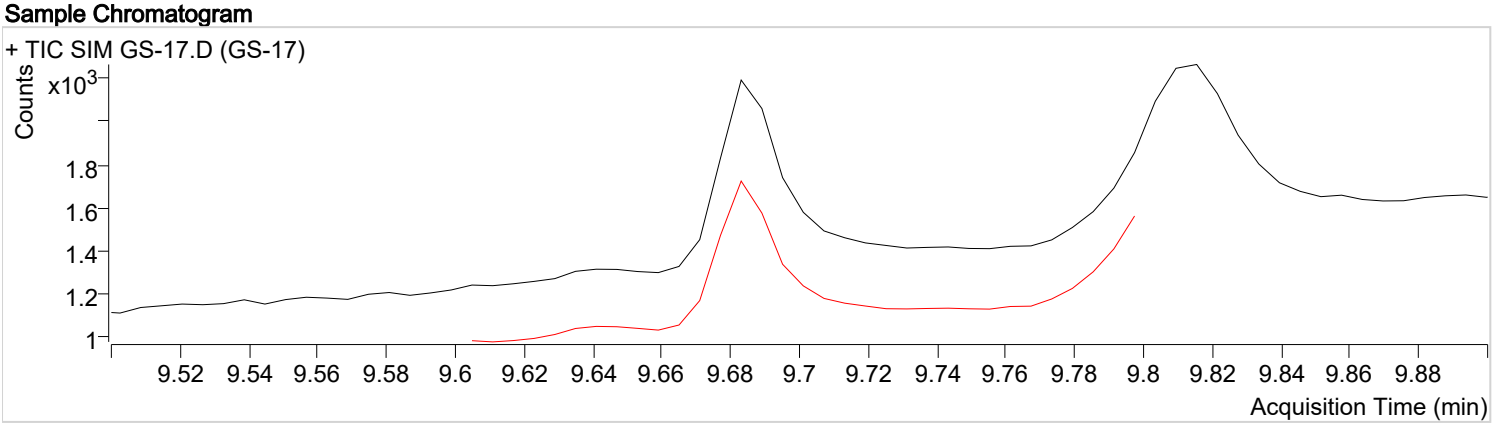

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 11:45:11	**Data File**	GS-18.D
Type	Sample	**Name**	GS-18
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

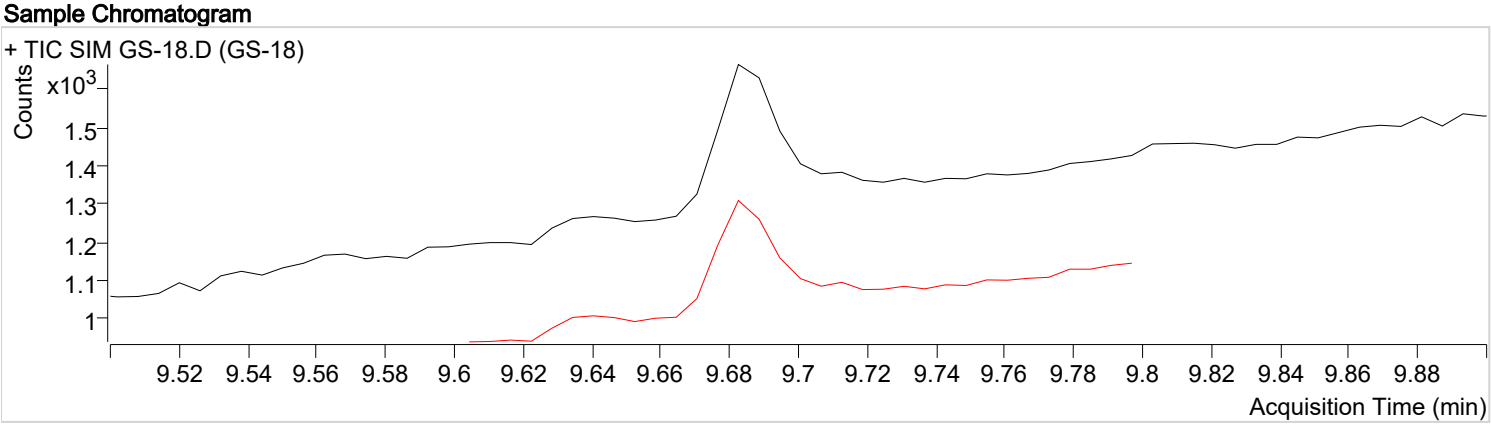

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 11:58:54	**Data File**	GS-19.D
Type	Sample	**Name**	GS-19
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

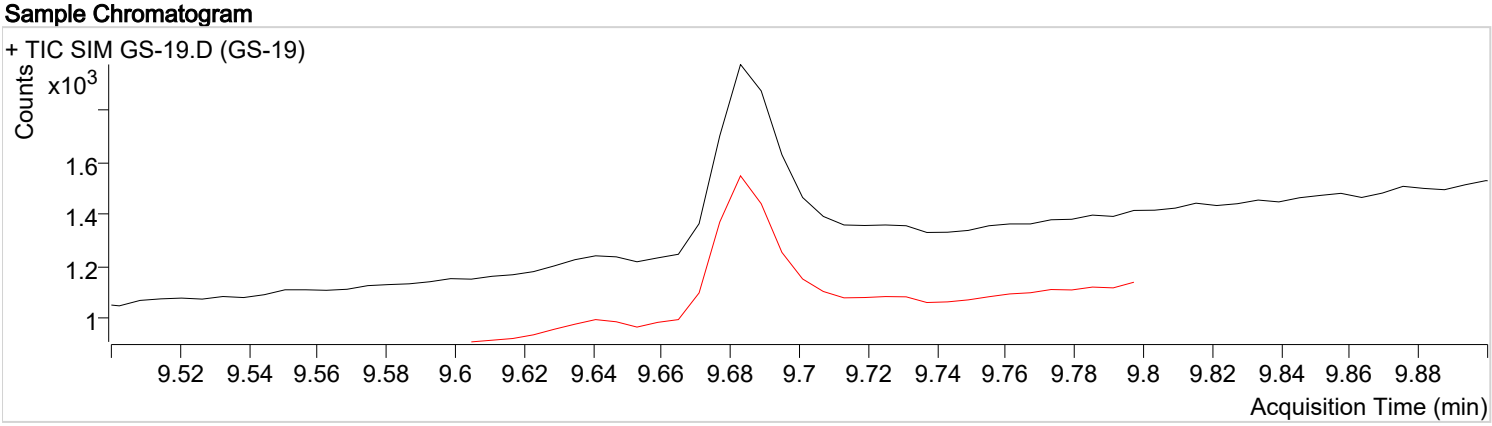

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-13 오전 12:12:38	**Data File**	GS-20.D
Type	Sample	**Name**	GS-20
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

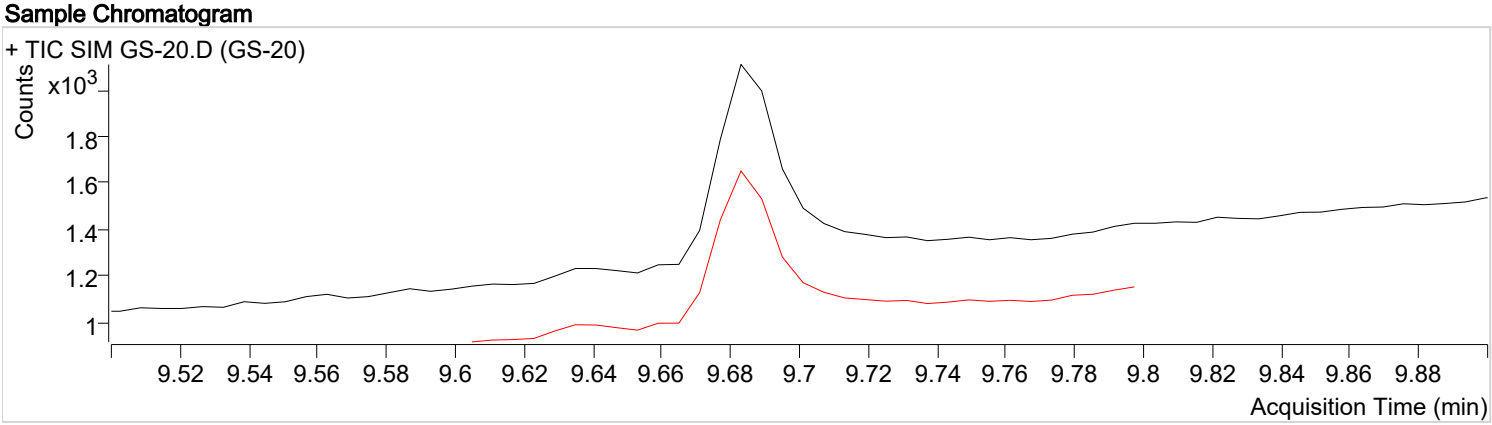

Di-Phtalate





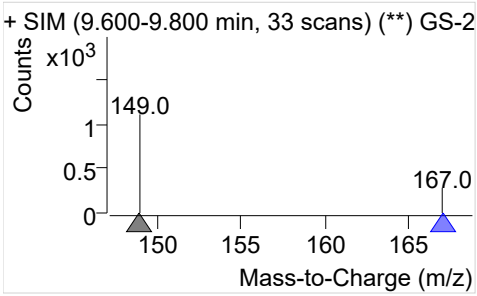

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-13 오전 12:26:23	**Data File**	GS-21.D
Type	Sample	**Name**	GS-21
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

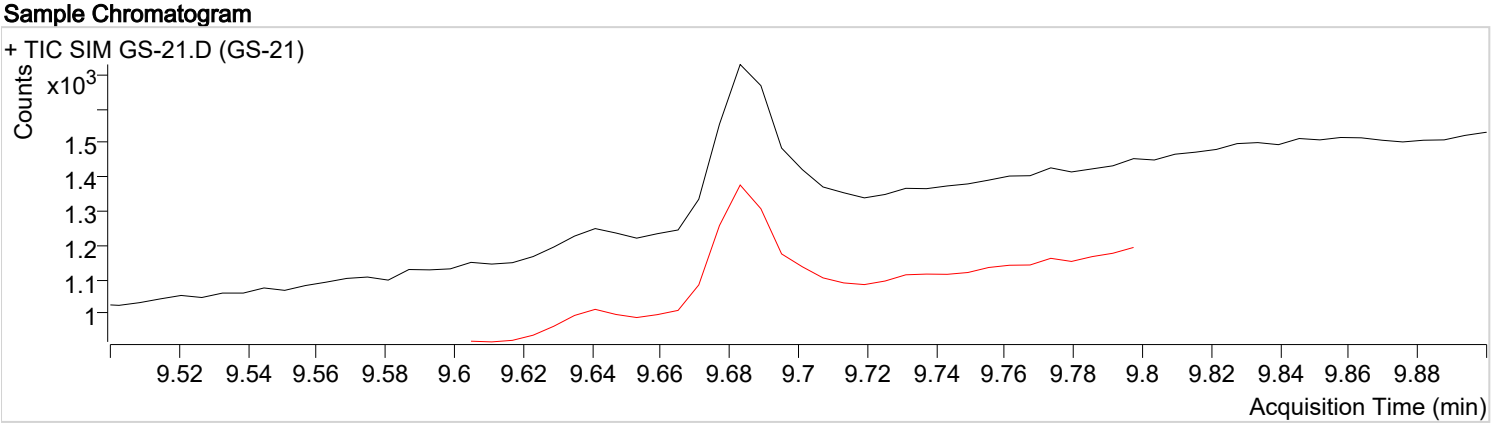

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-13 오전 12:40:08	**Data File**	GS-22.D
Type	Sample	**Name**	GS-22
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

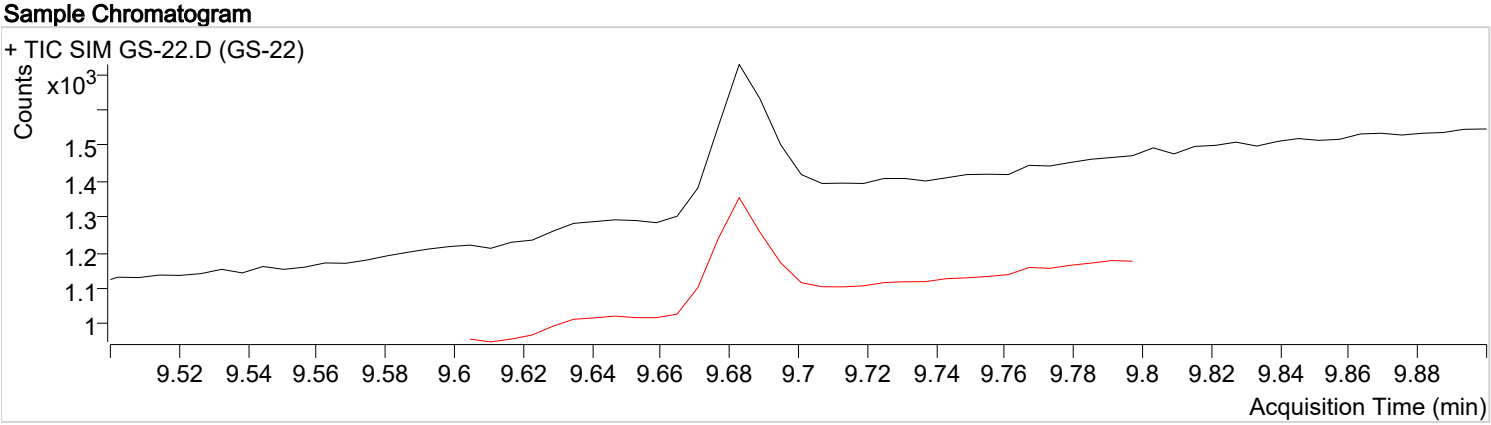

Di-Phtalate





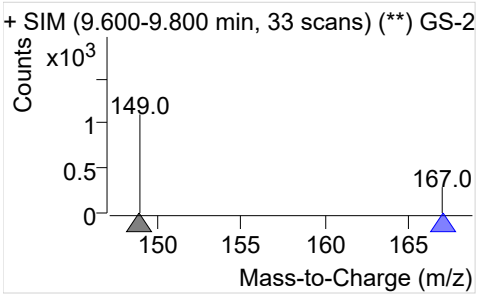

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-13 오전 12:53:52	**Data File**	GS-23.D
Type	Sample	**Name**	GS-23
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

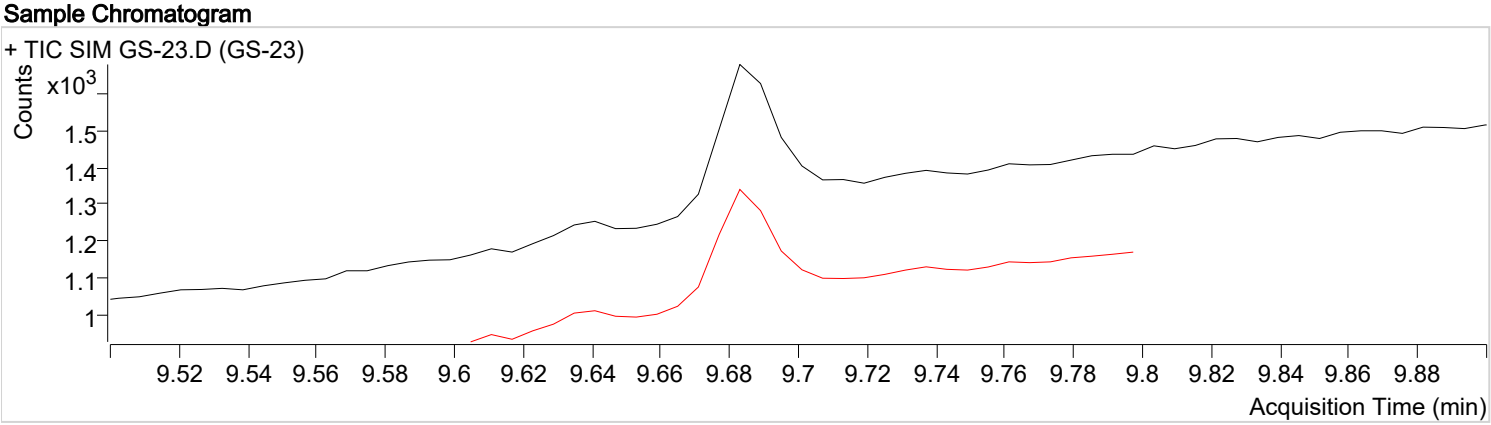

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-13 오전 1:07:34	**Data File**	GS-24.D
Type	Sample	**Name**	GS-24
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

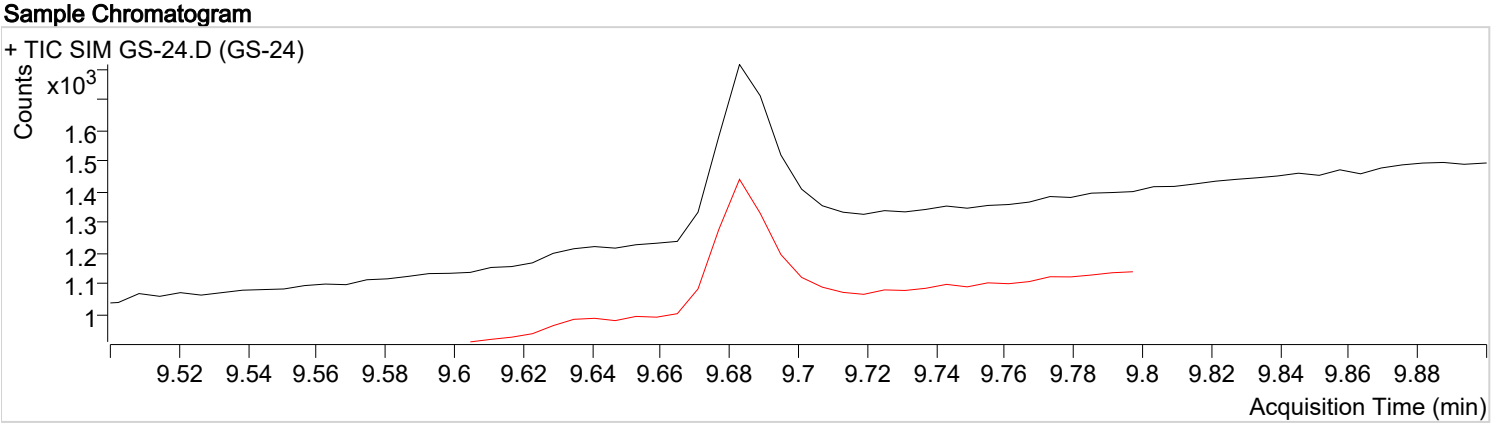

Di-Phtalate





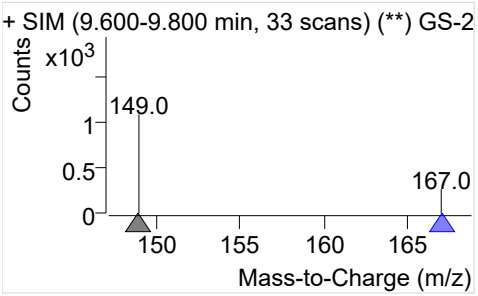

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-13 오전 1:21:18	**Data File**	MBK-2.D
Type	Blank	**Name**	MBK-2
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

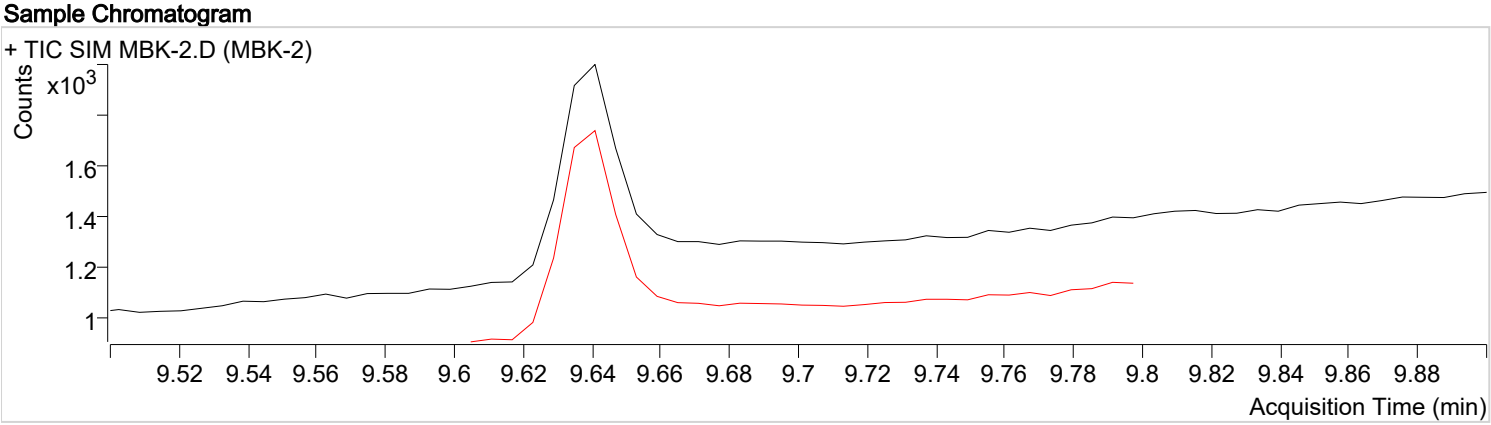

Di-Phtalate





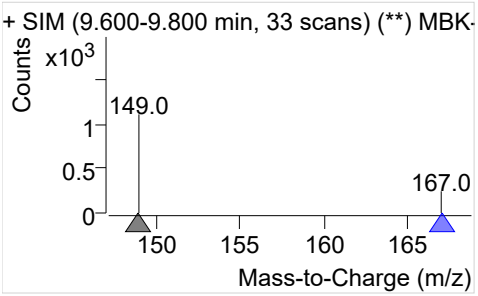

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\DEHP(GS 2.10, KH 2.10)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-02-13 오후 12:36:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:51:02	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:36:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-13 오전 1:48:48	**Data File**	-CCV-2.D
Type	QC	**Name**	-CCV-2
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

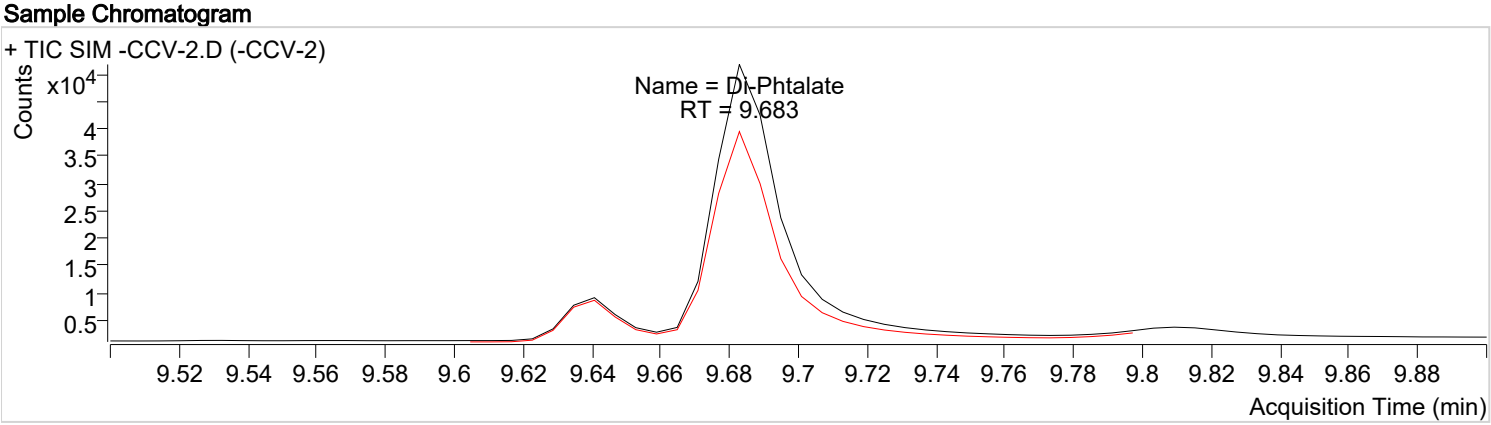

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.683	53349	0.0097	mg/L
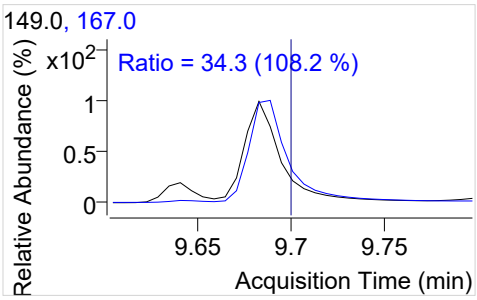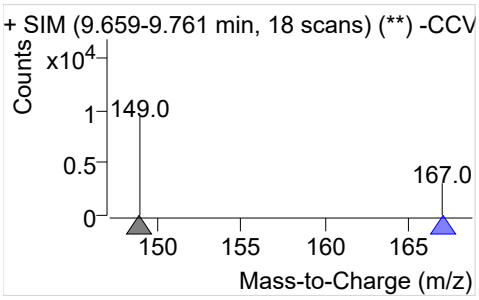
Di-Phtalate