Quantitative Analysis Results Summary Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin				
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Di-Phtalate

Data File	Type	RT	Resp.	Final Conc.
DEHP ST-01.D	Cal	9.677	21561	0.0026
DEHP ST-02.D	Cal	9.677	46572	0.0050
DEHP ST-03.D	Cal	9.677	71789	0.0074
DEHP ST-04.D	Cal	9.677	99492	0.0101
DEHP ST-05.D	Cal	9.677	147983	0.0147
DEHP ST-06.D	Cal	9.677	205508	0.0202
BK-.D	Blank			ND
FBK(RE 26-03-04).D	Blank			ND
FBK(KD 26-03-04).D	Blank			ND
RE-01.D	Sample			ND
RE-02.D	Sample			ND
RE-03.D	Sample	9.635	0	ND
RE-04.D	Sample			ND
RE-09.D	Sample	9.635	0	ND
RE-10.D	Sample	9.635	0	ND
RE-11.D	Sample			ND
RE-12.D	Sample			ND
KD-01.D	Sample	9.635	0	ND
KD-02.D	Sample			ND
KD-03.D	Sample	9.635	0	ND
MBK.D	Blank			ND
C-C-V-.D	QC	9.677	91080	0.0093

Di-Phtalate

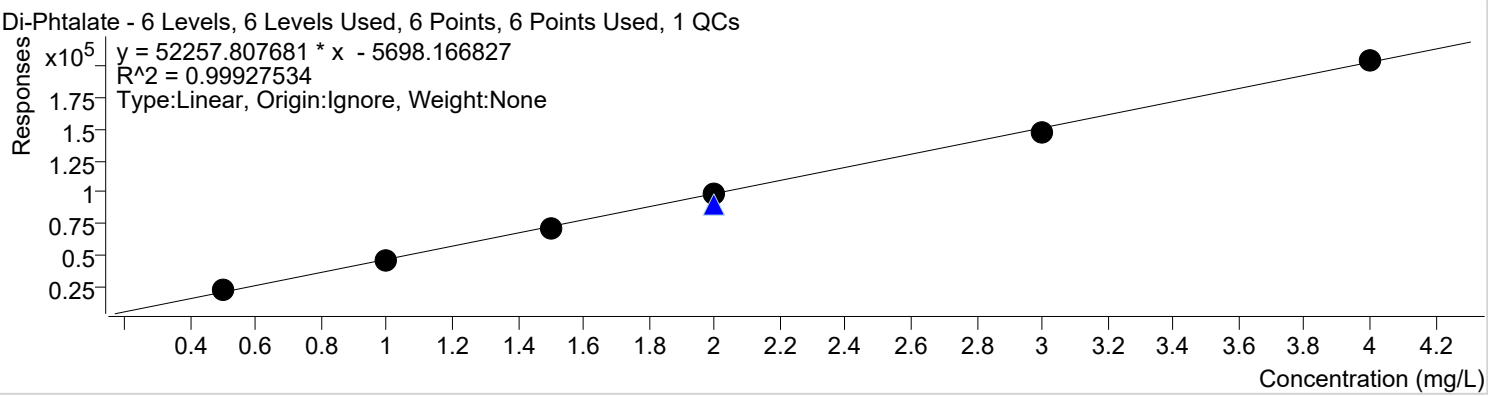

Cal. Path	Type	Level	Enable	Conc.	Response
\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\DEHP ST-01.D	Calibration	1	x	0.500	21561
\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\DEHP ST-02.D	Calibration	2	x	1.000	46572
\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\DEHP ST-03.D	Calibration	3	x	1.500	71789
\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\DEHP ST-04.D	Calibration	4	x	2.000	99492
\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\C-C-V-.D	QC	4	x	2.000	91080
\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\DEHP ST-05.D	Calibration	5	x	3.000	147983
\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\DEHP ST-06.D	Calibration	6	x	4.000	205508

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오전 10:44:04	**Data File**	DEHP ST-01.D
Type	Cal	**Name**	DEHP ST-01
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

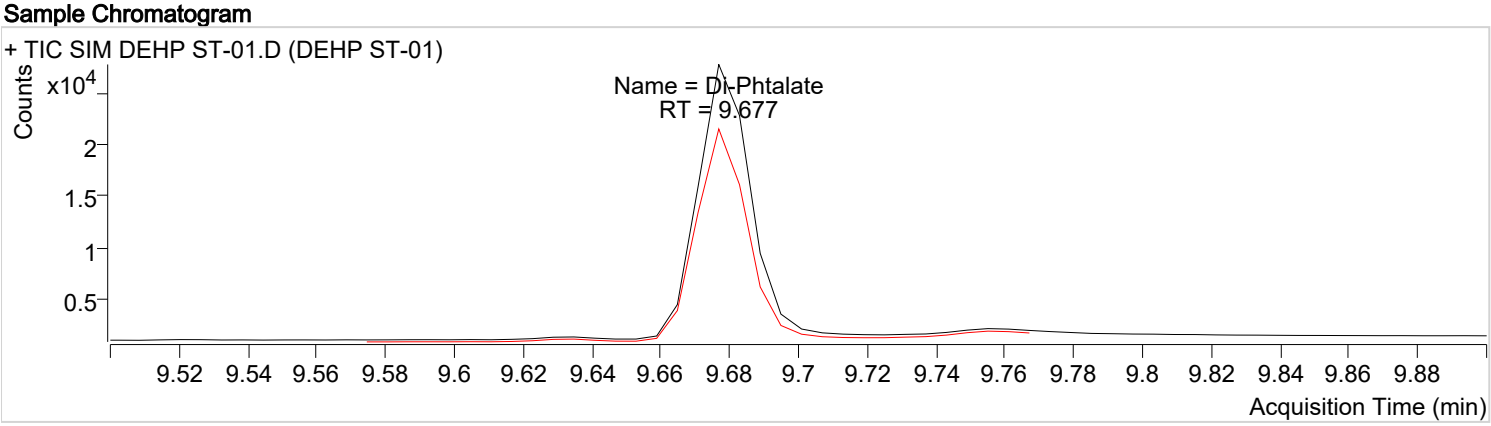

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.677	21561	0.0026	mg/L

Di-Phtalate

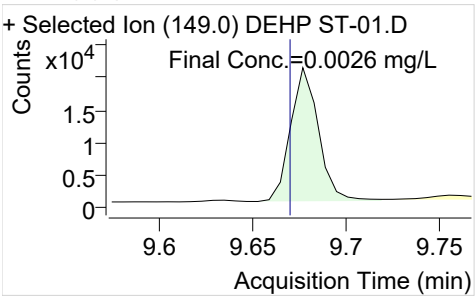

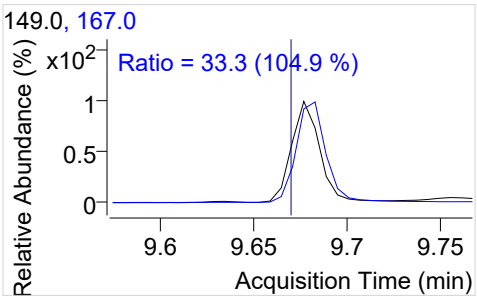

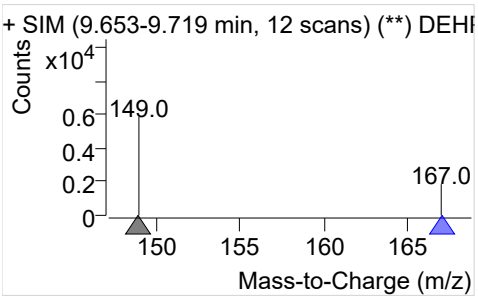

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오전 10:57:42	**Data File**	DEHP ST-02.D
Type	Cal	**Name**	DEHP ST-02
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

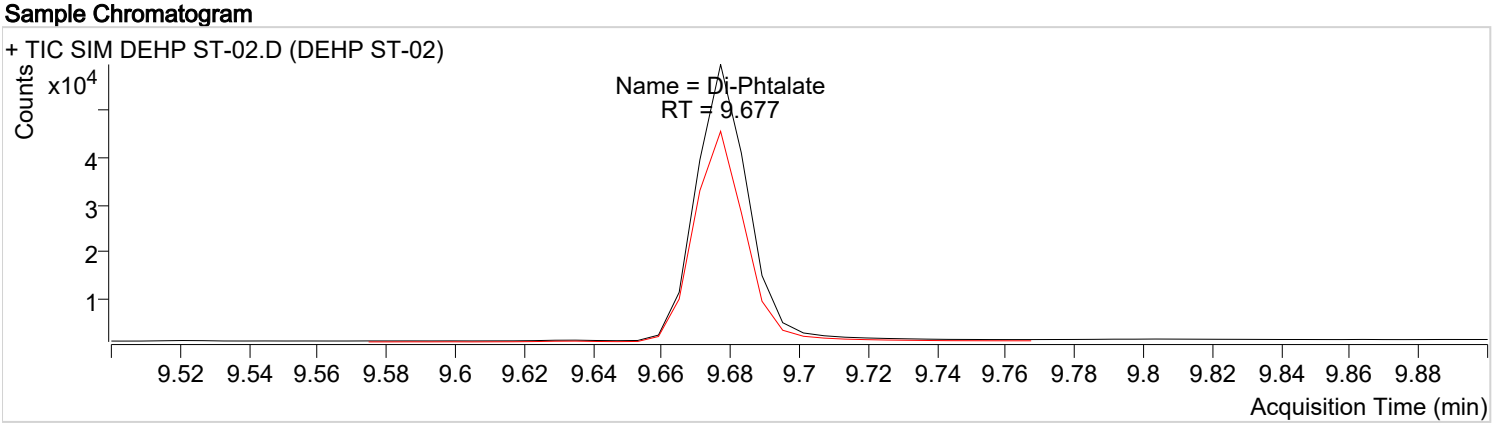

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.677	46572	0.0050	mg/L

Di-Phtalate



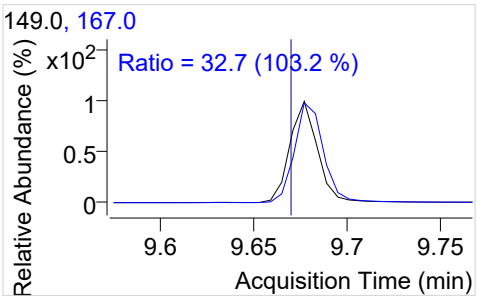

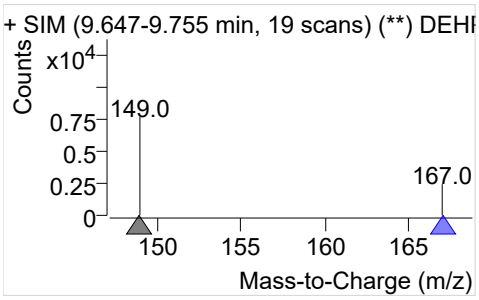

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오전 11:11:21	**Data File**	DEHP ST-03.D
Type	Cal	**Name**	DEHP ST-03
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

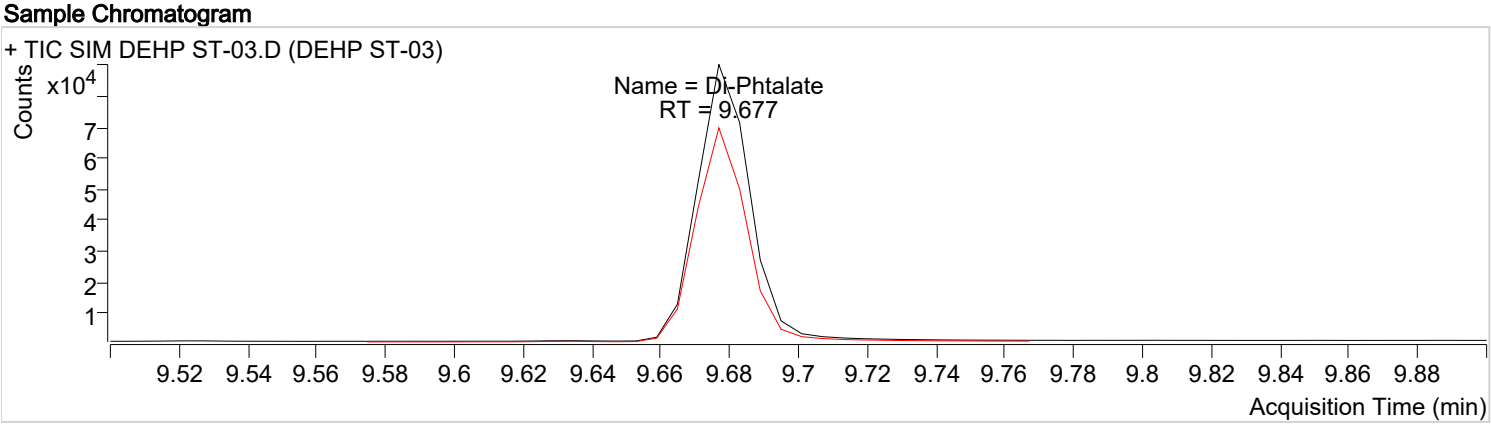

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.677	71789	0.0074	mg/L

Di-Phtalate

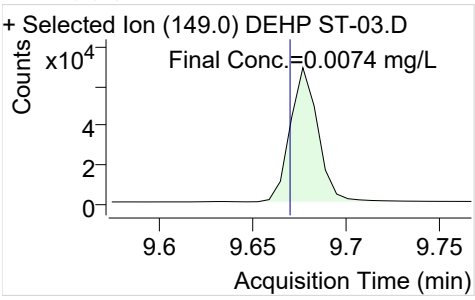

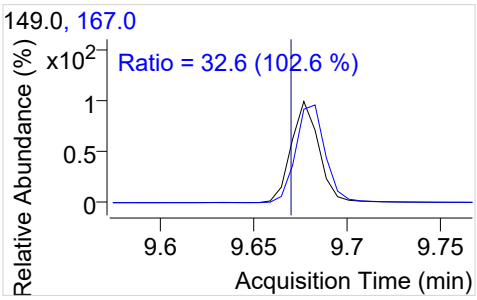

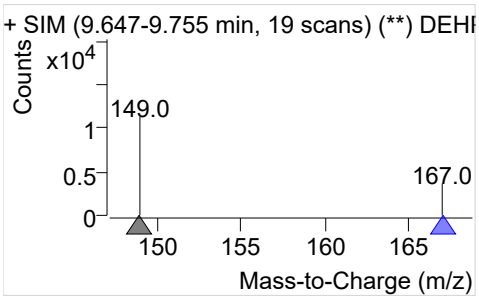

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오전 11:25:00	**Data File**	DEHP ST-04.D
Type	Cal	**Name**	DEHP ST-04
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

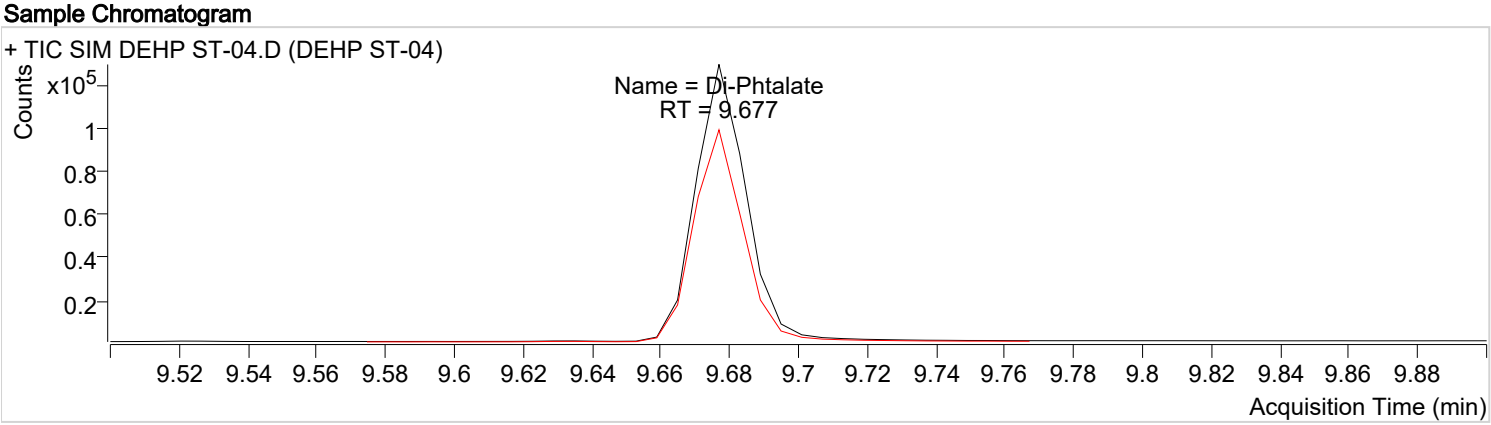

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.677	99492	0.0101	mg/L

Di-Phtalate

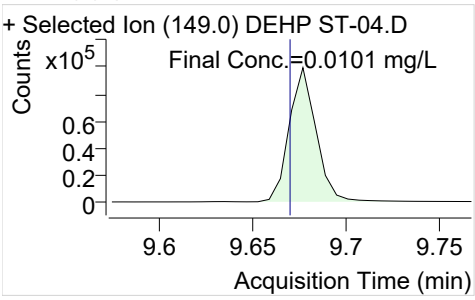



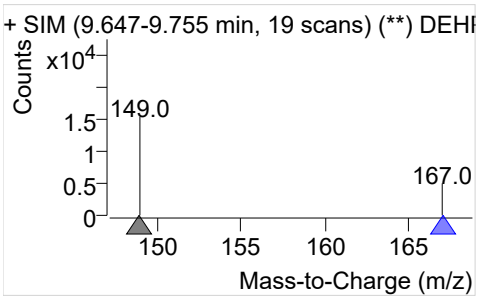

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오전 11:38:43	**Data File**	DEHP ST-05.D
Type	Cal	**Name**	DEHP ST-05
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

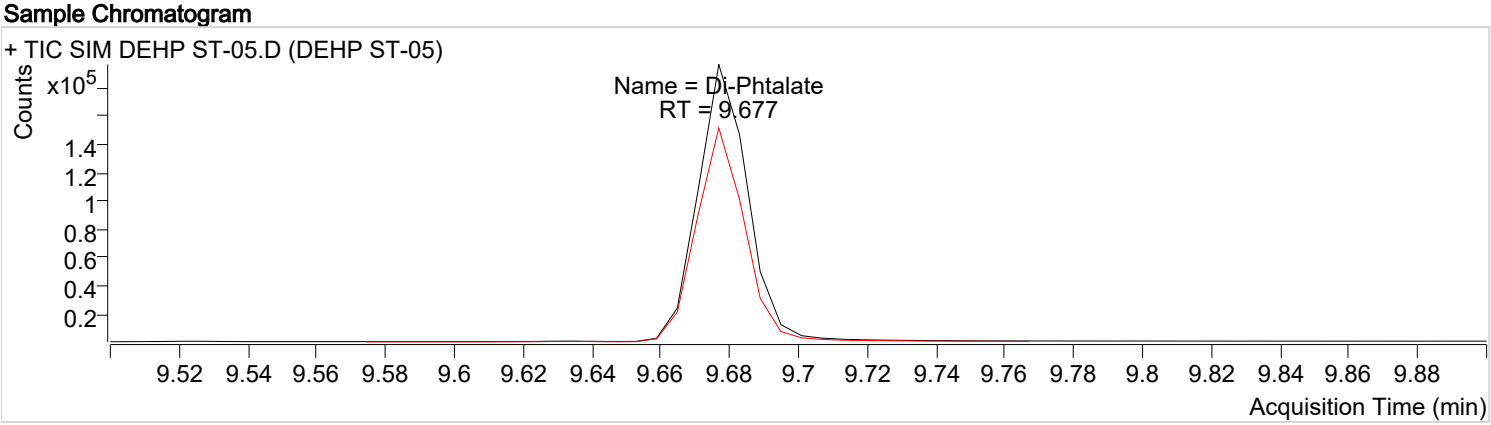

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.677	147983	0.0147	mg/L

Di-Phtalate



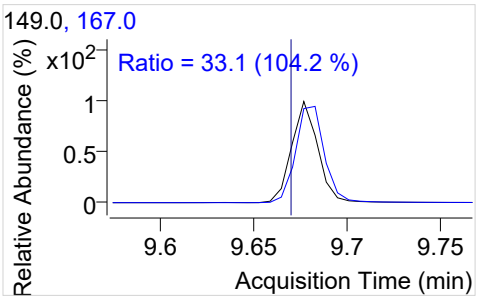

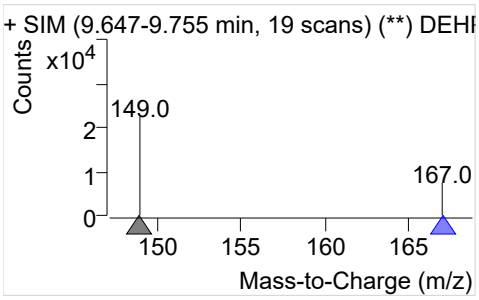

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오전 11:52:25	**Data File**	DEHP ST-06.D
Type	Cal	**Name**	DEHP ST-06
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

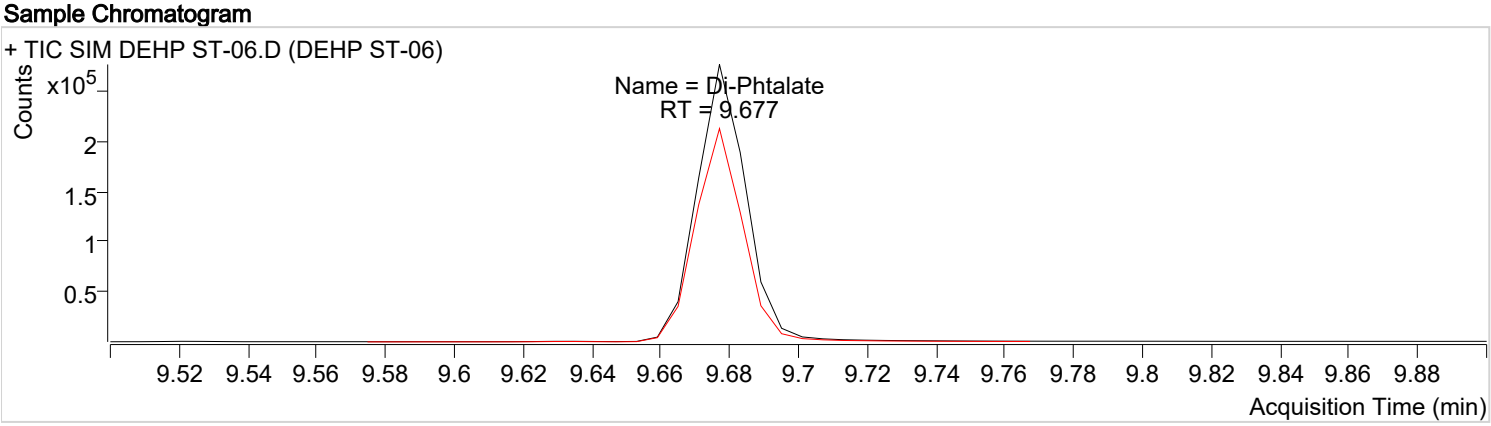

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.677	205508	0.0202	mg/L

Di-Phtalate



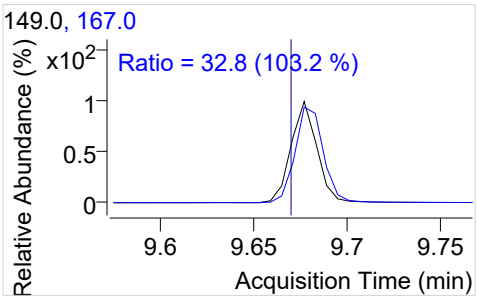

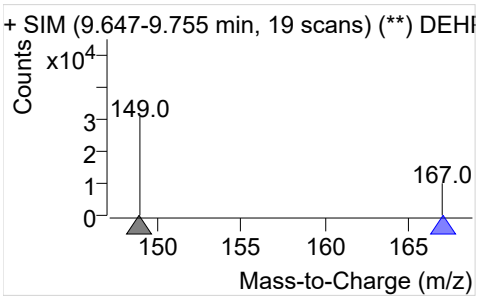

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오후 12:19:47	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

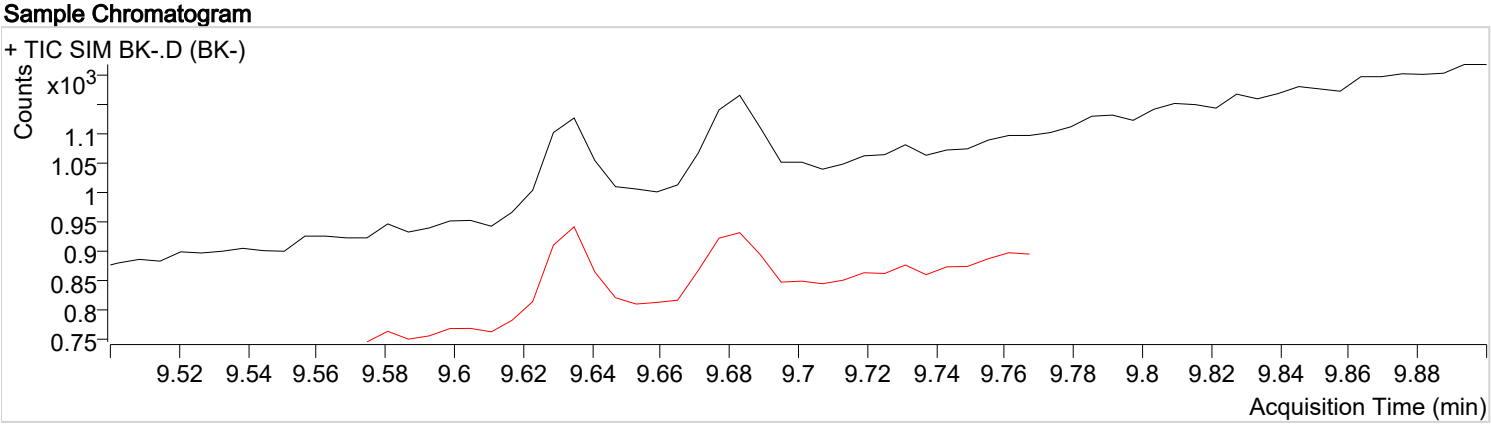

Di-Phtalate





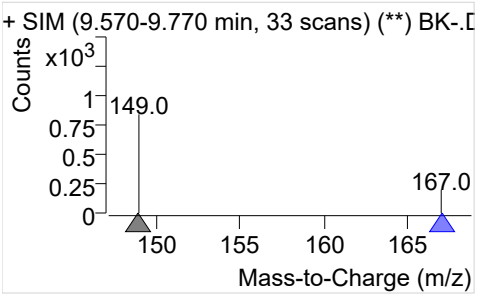

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오후 12:33:28	**Data File**	FBK(RE 26-03-04).D
Type	Blank	**Name**	FBK(RE 26-03-04)
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

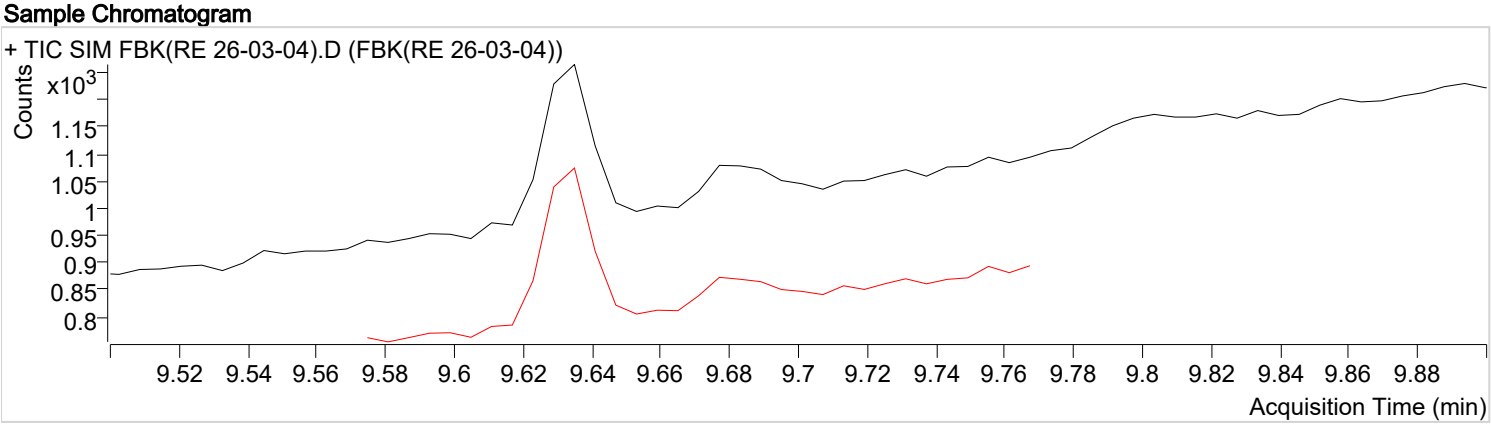

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오후 12:47:08	**Data File**	FBK(KD 26-03-04).D
Type	Blank	**Name**	FBK(KD 26-03-04)
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

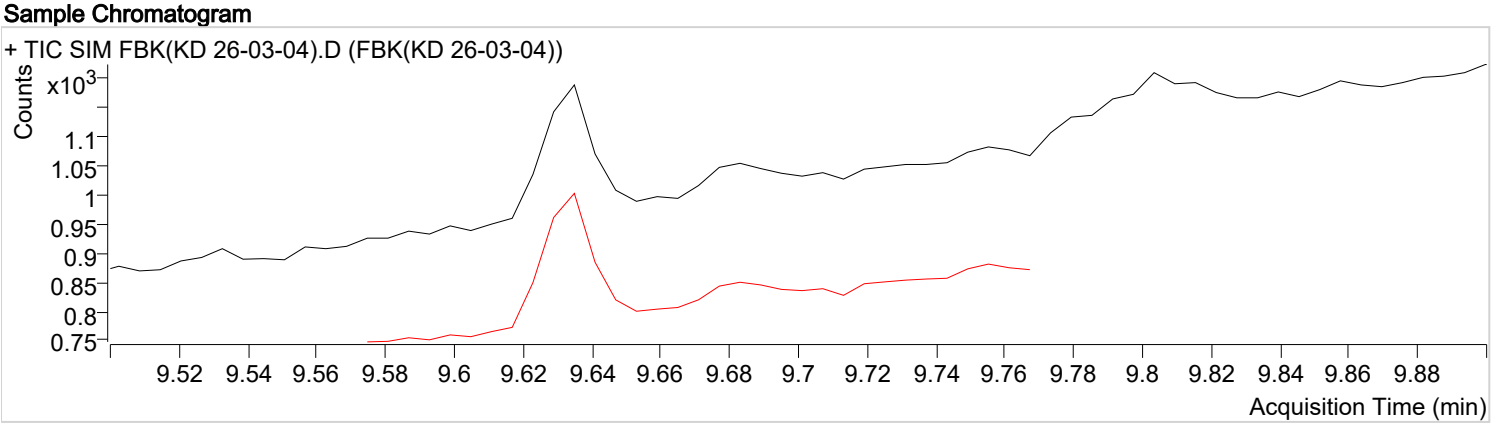

Di-Phtalate





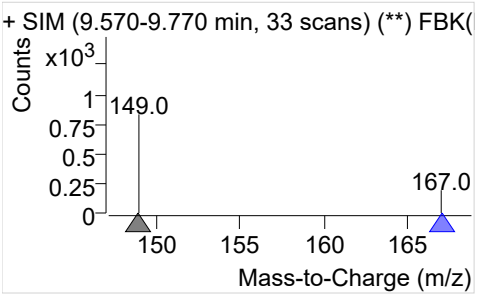

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오후 1:00:48	**Data File**	RE-01.D
Type	Sample	**Name**	RE-01
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

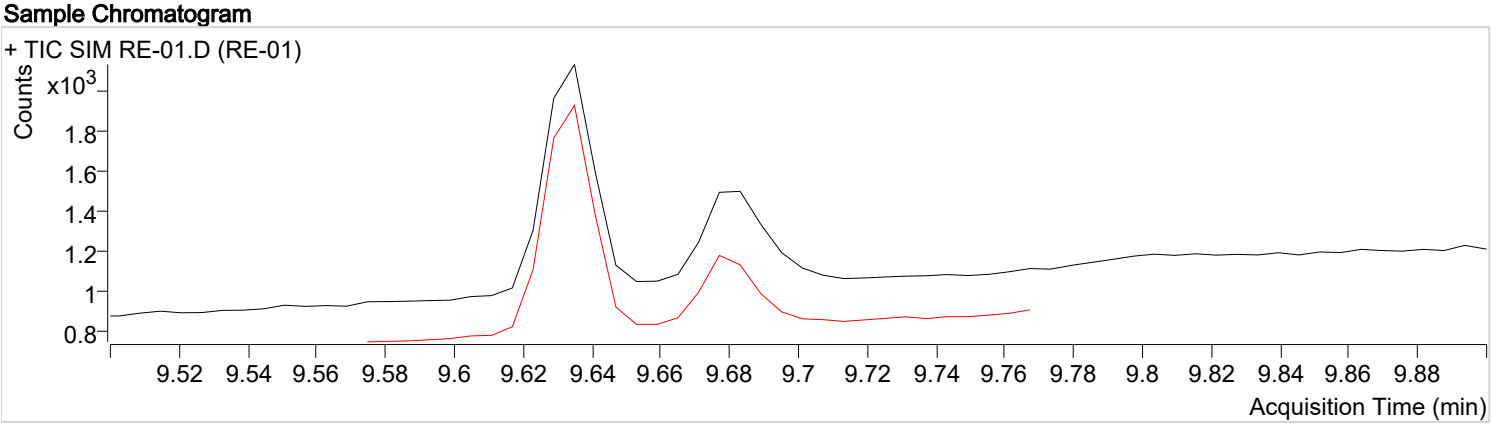

Di-Phtalate





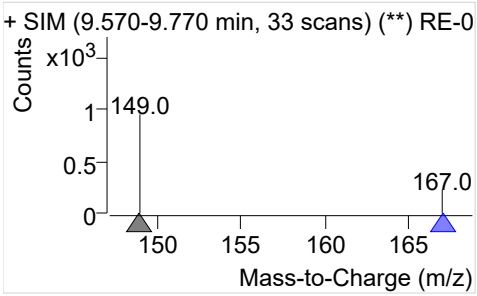

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오후 1:14:27	**Data File**	RE-02.D
Type	Sample	**Name**	RE-02
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

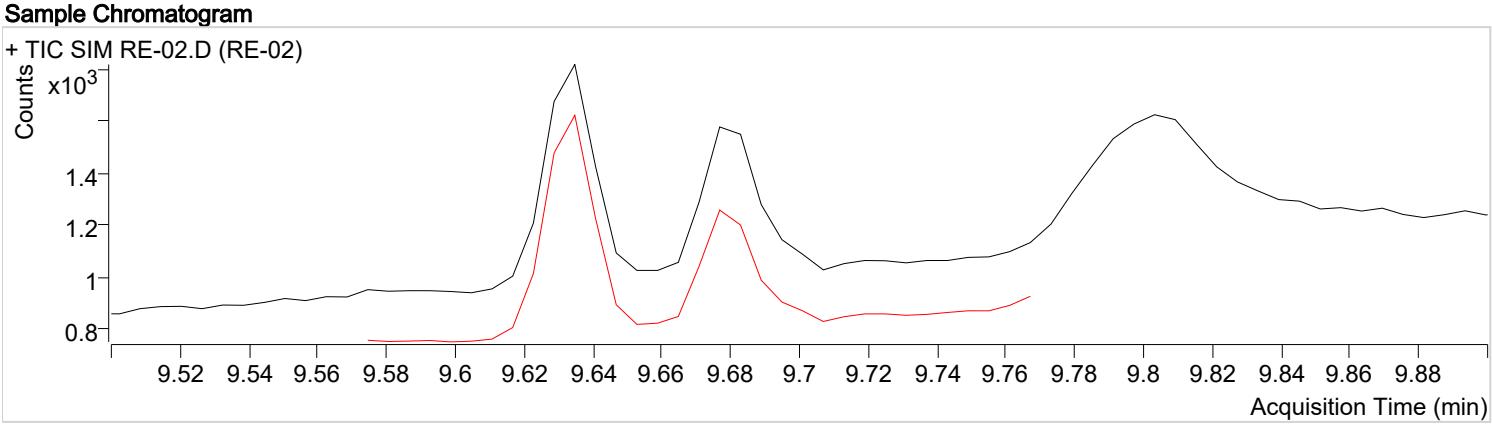

Di-Phtalate





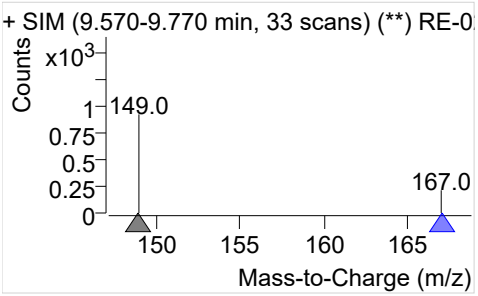

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오후 1:28:07	**Data File**	RE-03.D
Type	Sample	**Name**	RE-03
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

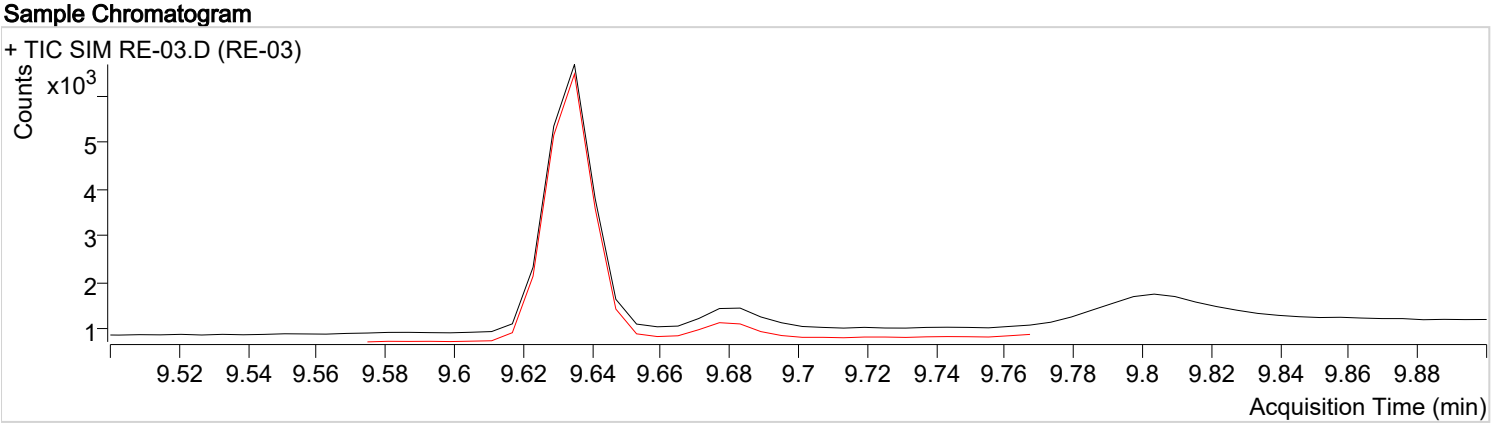

Di-Phtalate





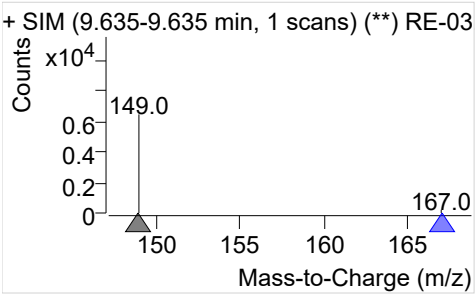

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오후 1:41:50	**Data File**	RE-04.D
Type	Sample	**Name**	RE-04
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

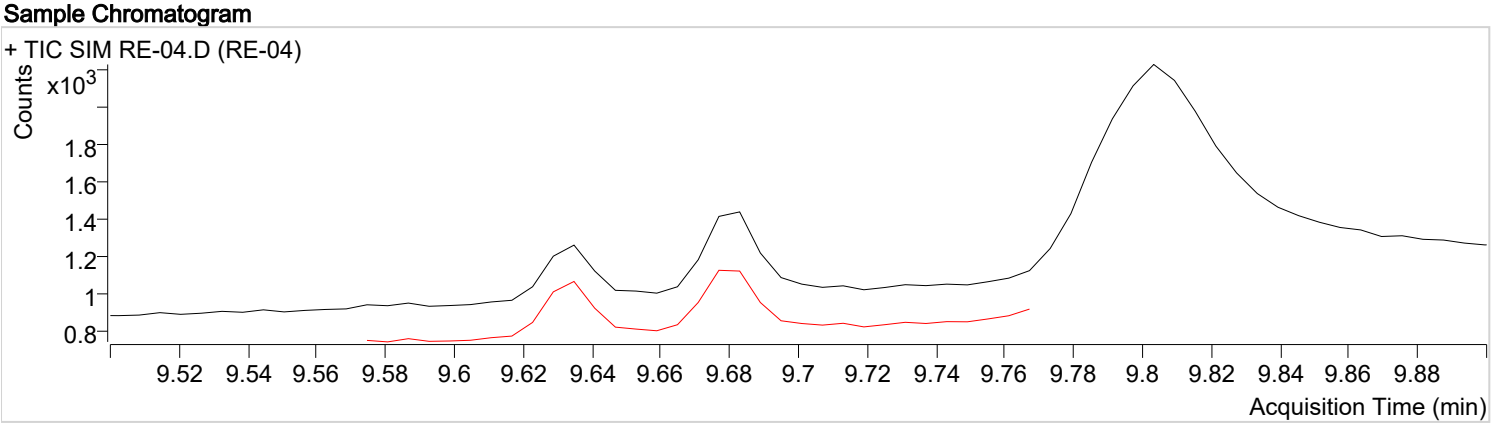

Di-Phtalate





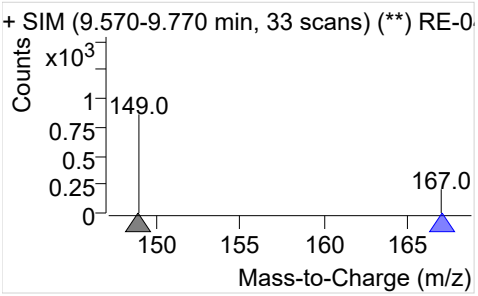

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오후 1:55:30	**Data File**	RE-09.D
Type	Sample	**Name**	RE-09
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

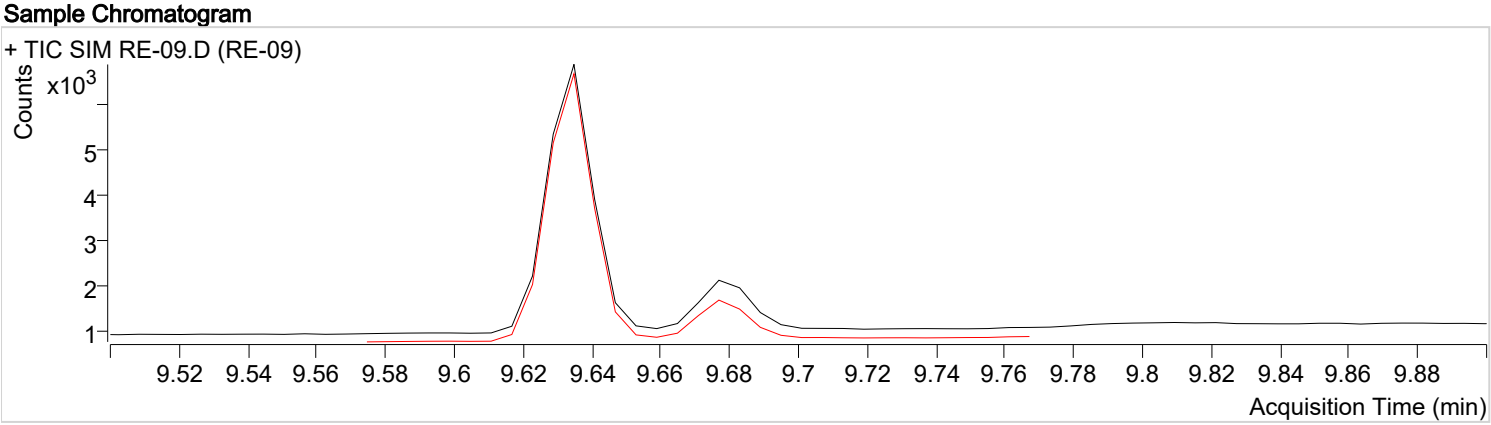

Di-Phtalate





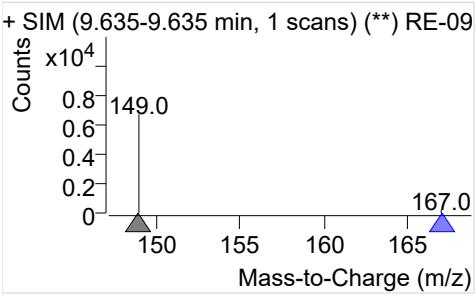

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오후 2:09:11	**Data File**	RE-10.D
Type	Sample	**Name**	RE-10
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

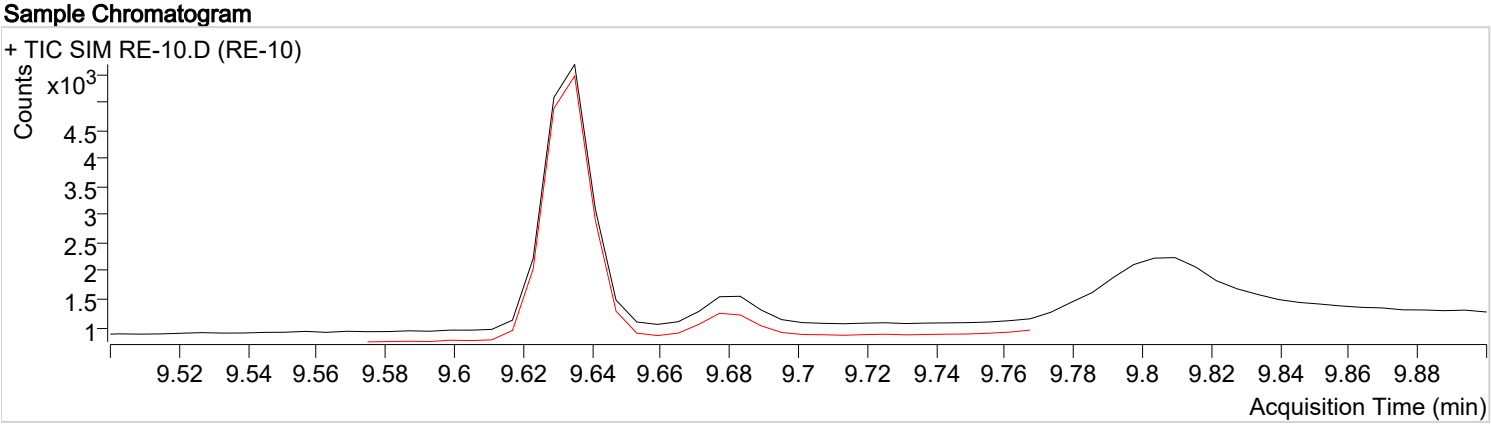

Di-Phtalate





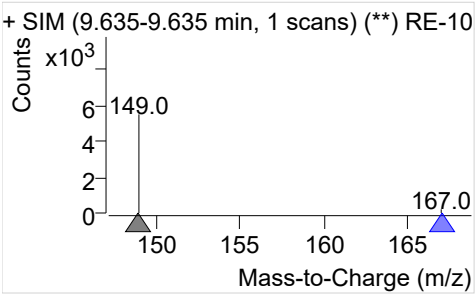

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오후 2:22:53	**Data File**	RE-11.D
Type	Sample	**Name**	RE-11
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

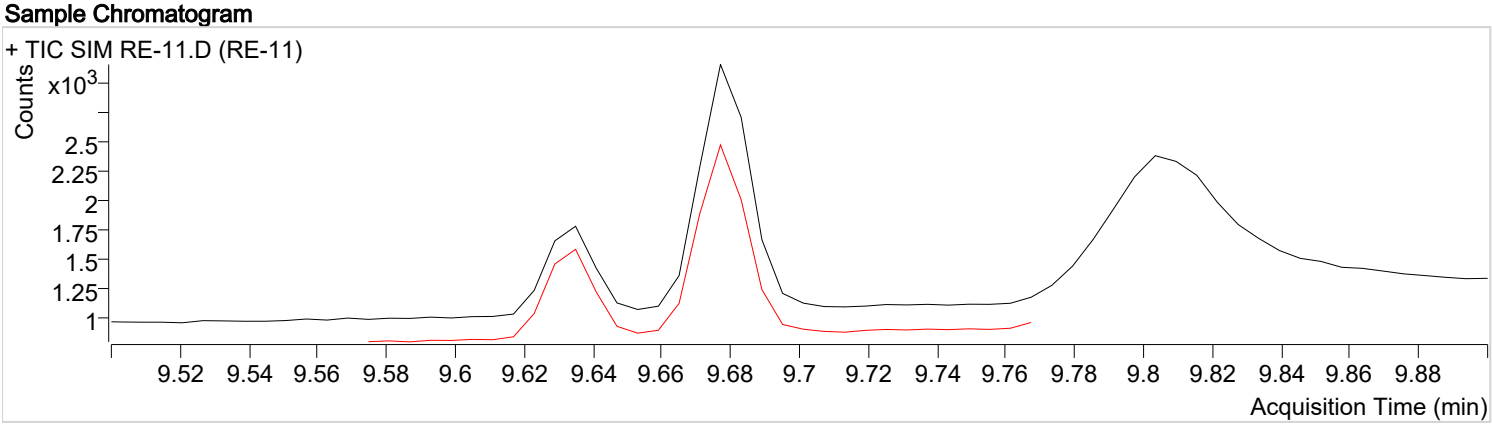

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오후 2:36:36	**Data File**	RE-12.D
Type	Sample	**Name**	RE-12
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

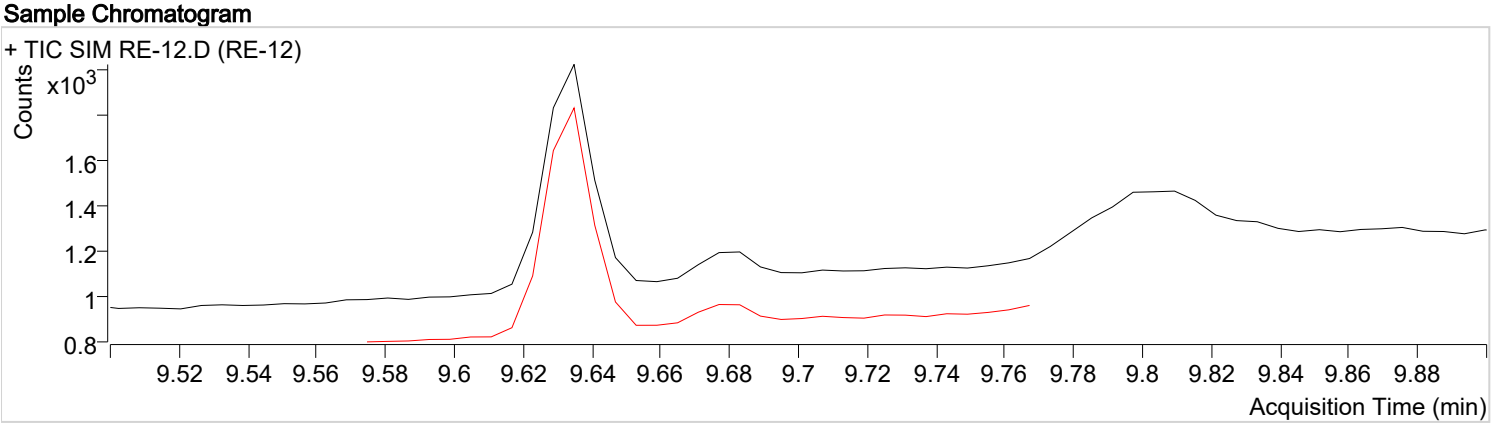

Di-Phtalate





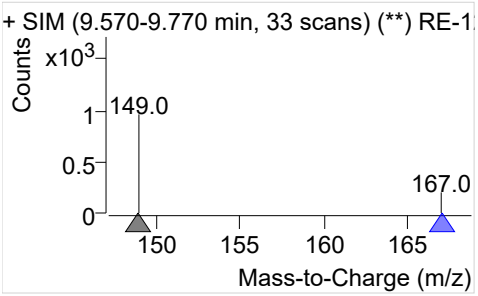

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오후 2:50:17	**Data File**	KD-01.D
Type	Sample	**Name**	KD-01
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

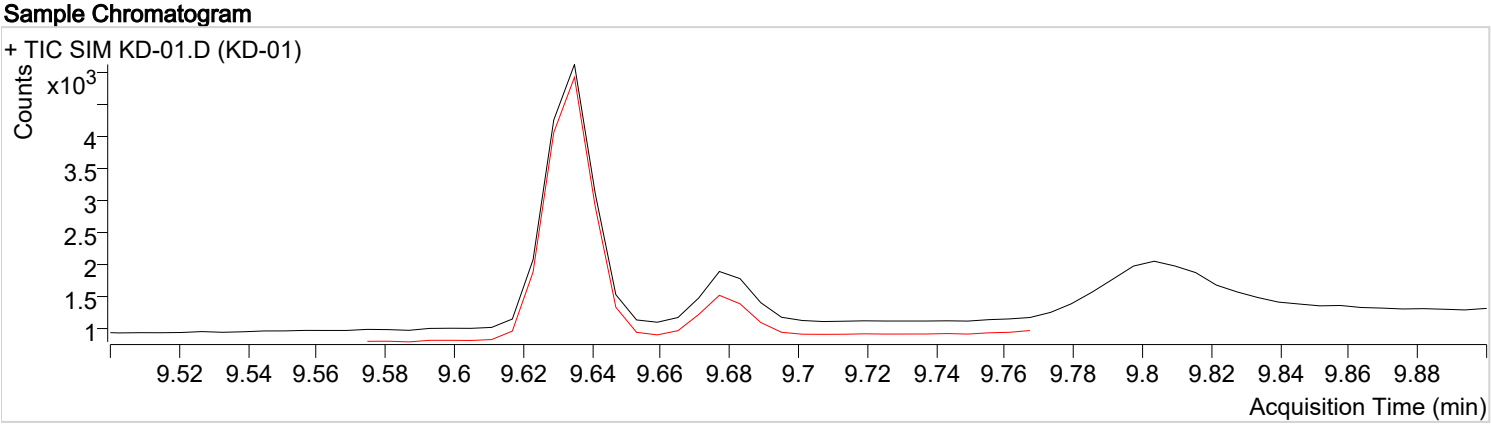

Di-Phtalate







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오후 3:03:59	**Data File**	KD-02.D
Type	Sample	**Name**	KD-02
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

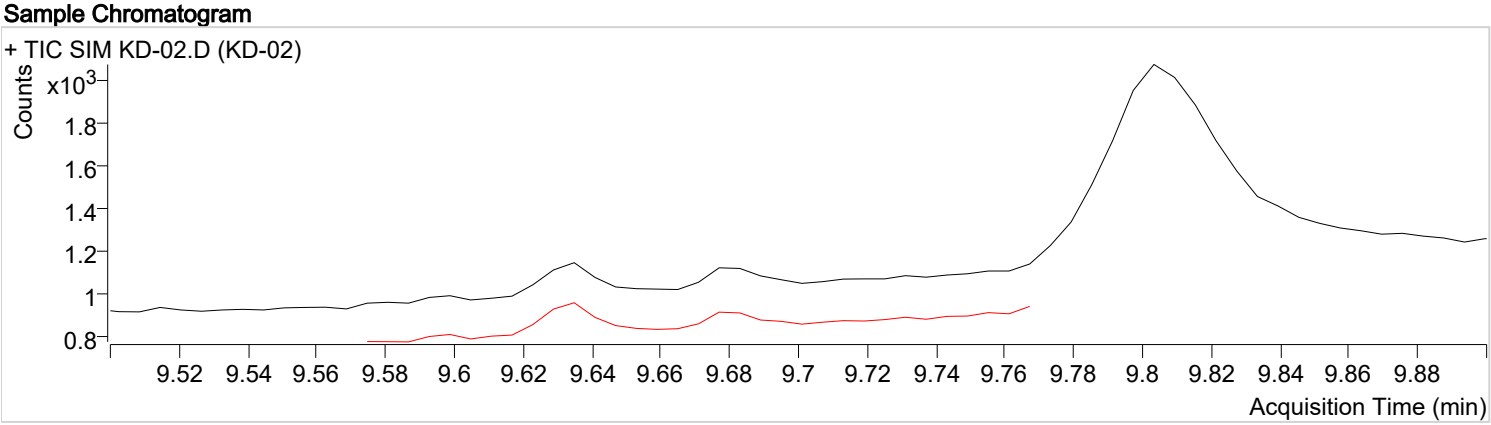

Di-Phtalate





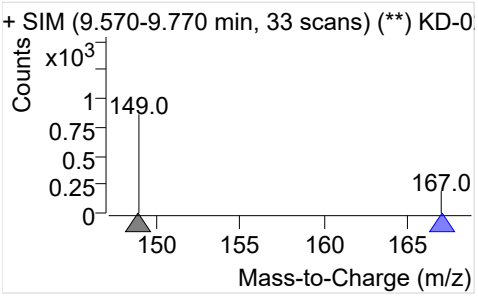

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오후 3:17:41	**Data File**	KD-03.D
Type	Sample	**Name**	KD-03
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

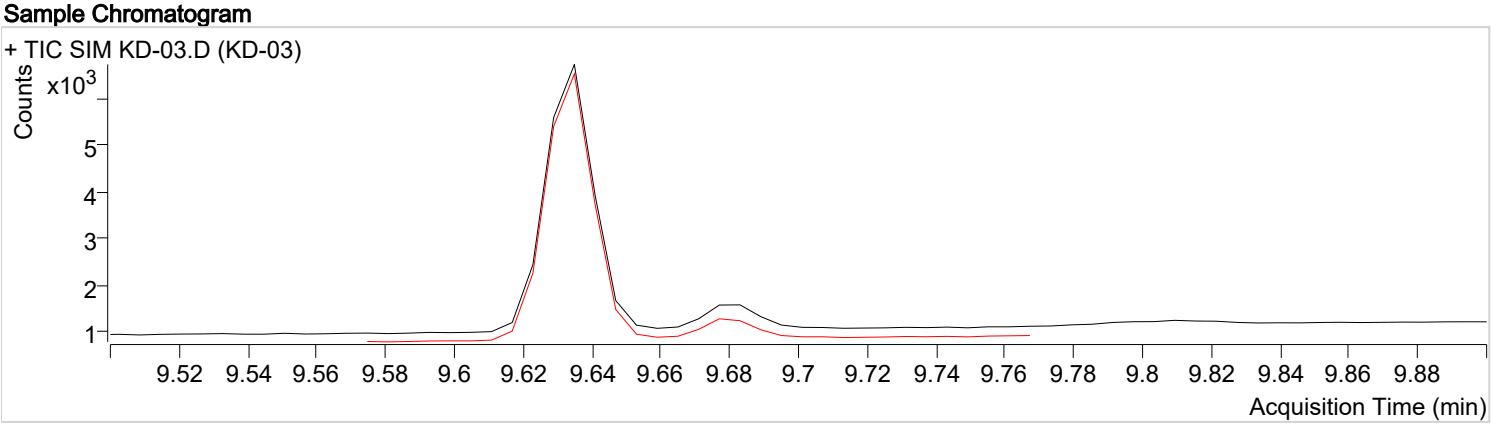

Di-Phtalate





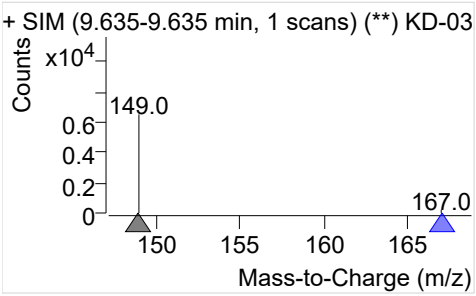

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오후 3:31:23	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

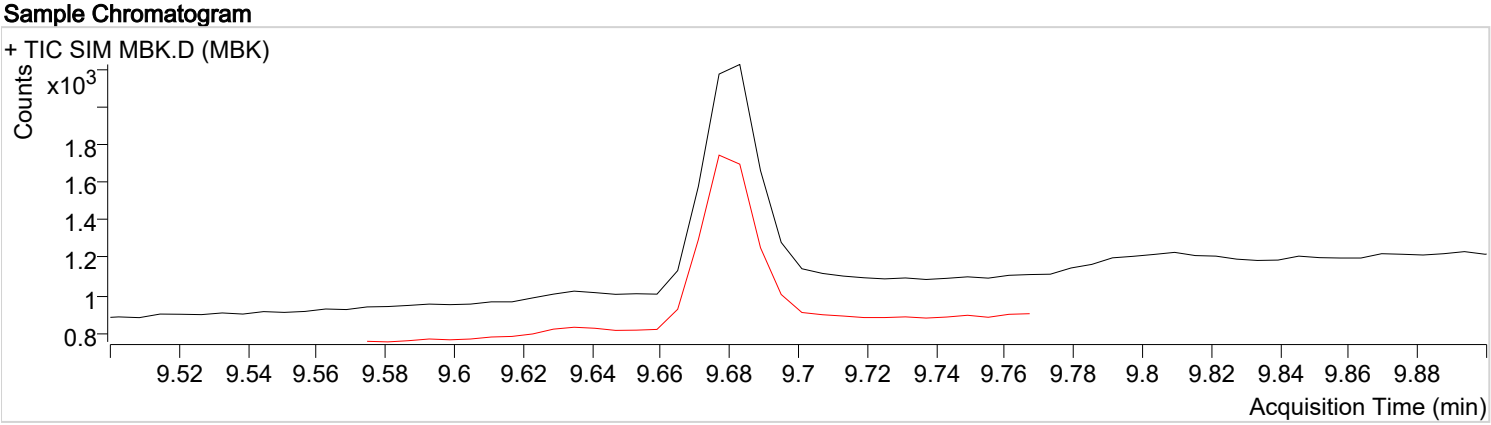

Di-Phtalate





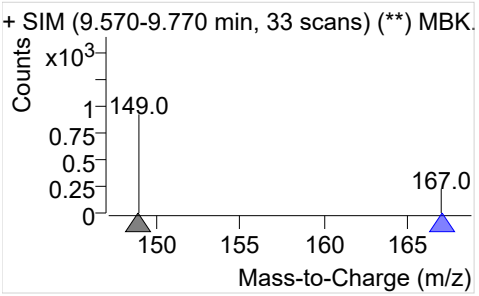

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP (RE 3.4 KD 3.4)RR\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-10 오후 4:33:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:54:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:33:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-08 오후 3:58:47	**Data File**	C-C-V-.D
Type	QC	**Name**	C-C-V-
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

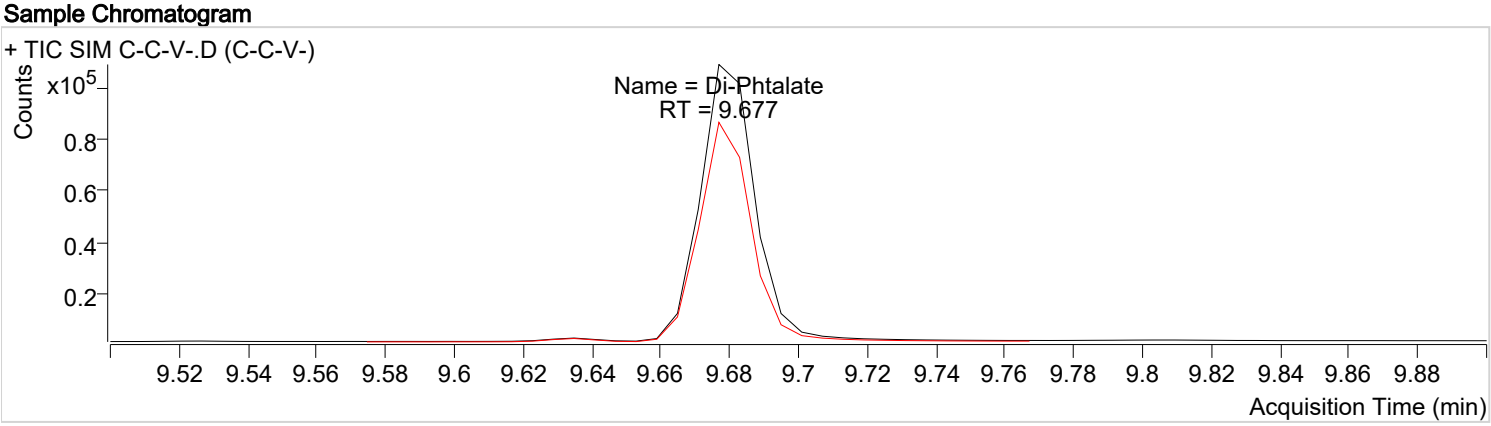

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.677	91080	0.0093	mg/L
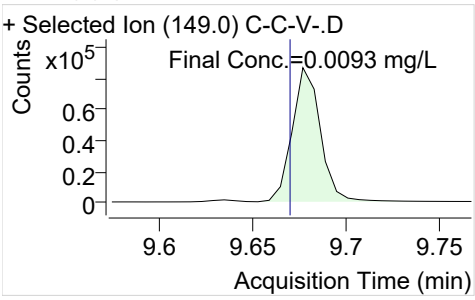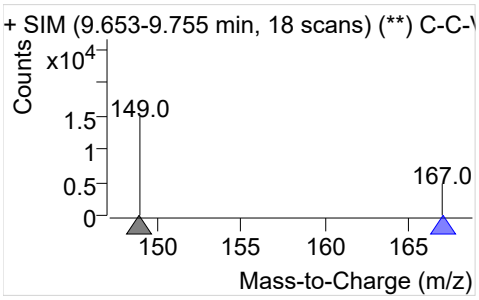
Di-Phtalate