Quantitative Analysis Results Summary Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin				
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Di-Phtalate

Data File	Type	RT	Resp.	Final Conc.
DEHP ST-01.D	Cal	9.677	41966	0.0015
DEHP ST-02.D	Cal	9.677	90676	0.0053
DEHP ST-03.D	Cal	9.677	123975	0.0079
DEHP ST-04.D	Cal	9.677	159913	0.0107
DEHP ST-05.D	Cal	9.677	220036	0.0154
DEHP ST-06.D	Cal	9.677	270539	0.0193
BK.D	Blank			ND
FBK(RE 26-03-17).D	Blank			ND
FBK(RE 26-03-18).D	Blank			ND
FBK(HS 26-03-18).D	Blank			ND
RE-05.D	Sample			ND
RE-06.D	Sample			ND
RE-13.D	Sample			ND
RE-14.D	Sample			ND
RE-24.D	Sample			ND
RE-25.D	Sample			ND
HS 26-03-18.D	Sample			ND
MBK.D	Blank			ND
-C-C-V-.D	QC	9.677	144583	0.0095

Di-Phtalate

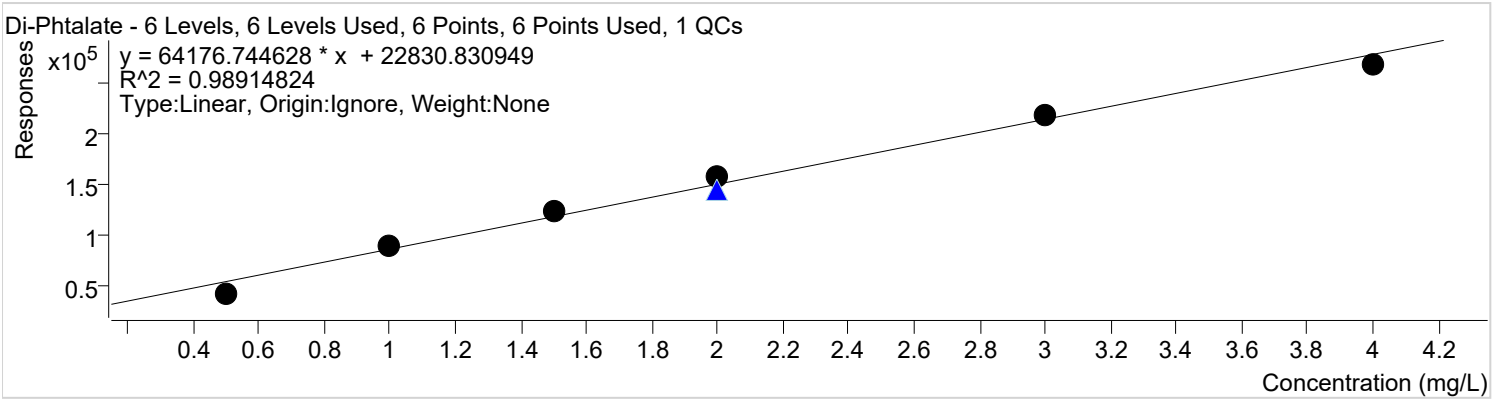

Cal. Path	Type	Level	Enable	Conc.	Response
\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\DEHP ST-01.D	Calibration	1	x	0.500	41966
\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\DEHP ST-02.D	Calibration	2	x	1.000	90676
\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\DEHP ST-03.D	Calibration	3	x	1.500	123975
\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\DEHP ST-04.D	Calibration	4	x	2.000	159913
\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\-C-C-V-.D	QC	4	x	2.000	144583
\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\DEHP ST-05.D	Calibration	5	x	3.000	220036
\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\DEHP ST-06.D	Calibration	6	x	4.000	270539

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:56:54	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 1:01:43	**Data File**	DEHP ST-01.D
Type	Cal	**Name**	DEHP ST-01
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

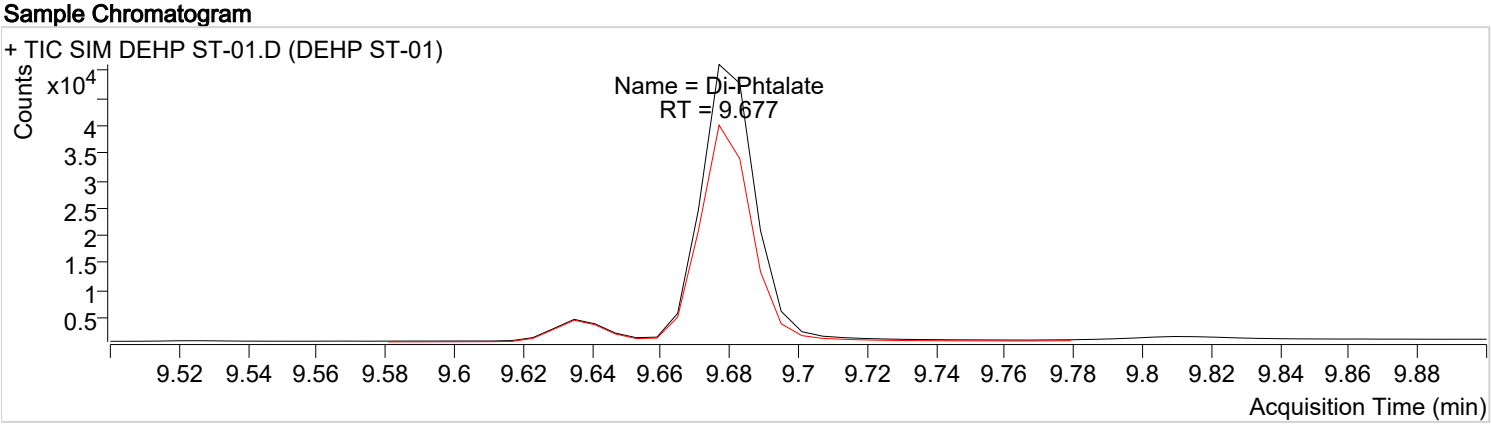

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.677	41966	0.0015	mg/L

Di-Phtalate

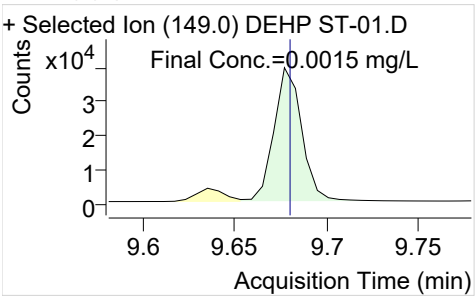



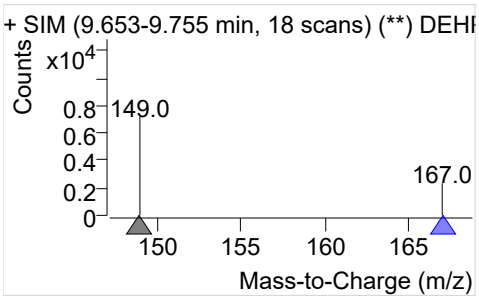

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:56:54	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 1:15:28	**Data File**	DEHP ST-02.D
Type	Cal	**Name**	DEHP ST-02
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

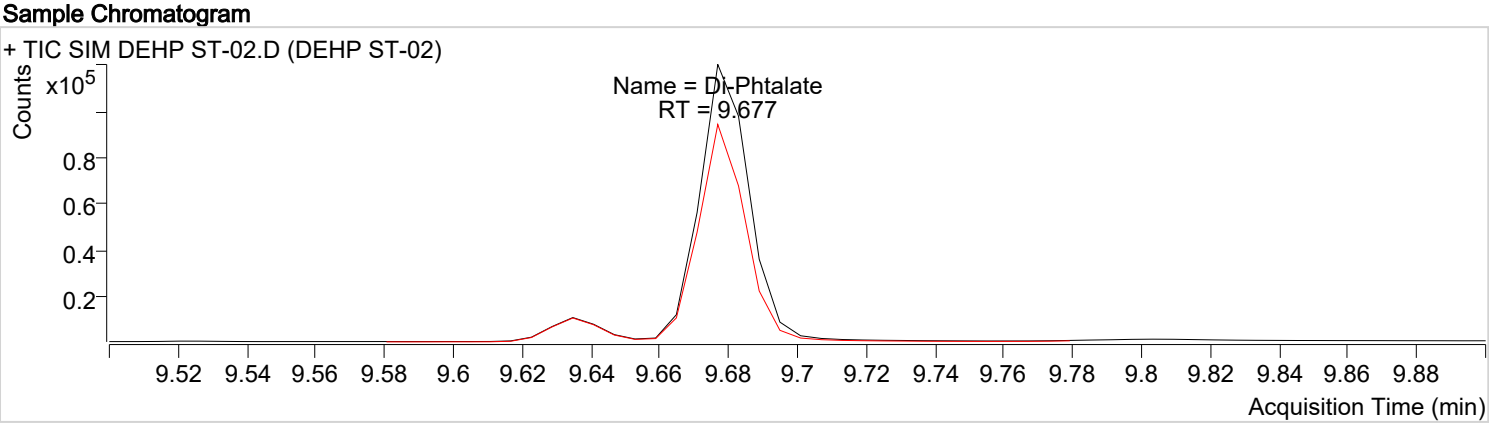

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.677	90676	0.0053	mg/L

Di-Phtalate

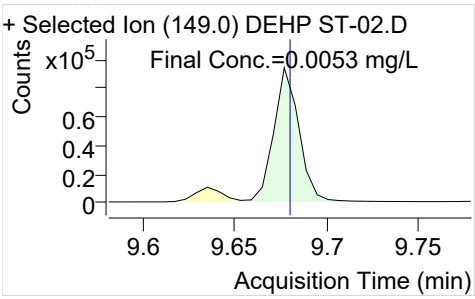



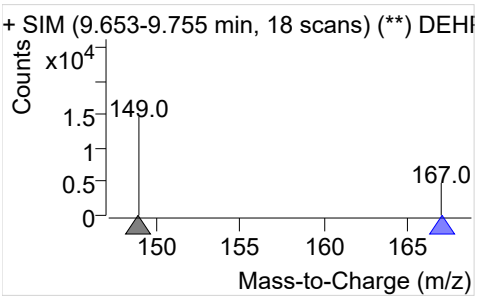

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:56:54	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 1:29:11	**Data File**	DEHP ST-03.D
Type	Cal	**Name**	DEHP ST-03
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

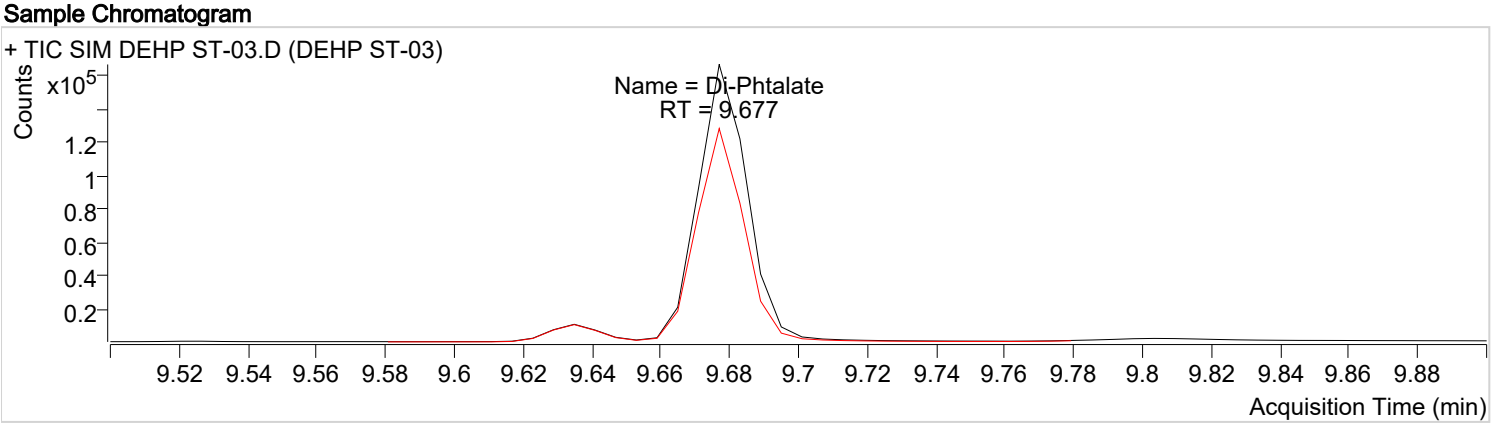

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.677	123975	0.0079	mg/L

Di-Phtalate

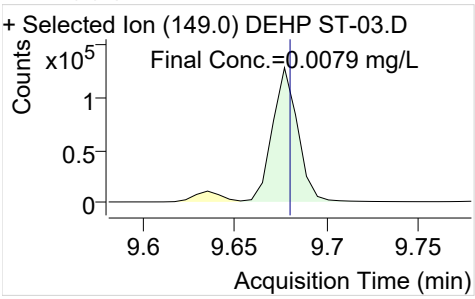



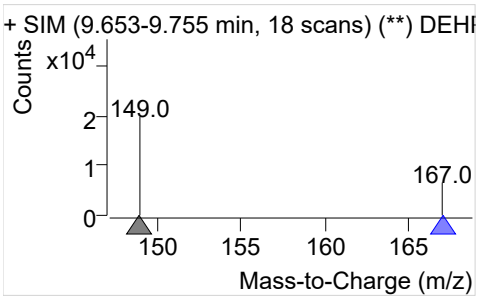

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:56:54	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 1:42:55	**Data File**	DEHP ST-04.D
Type	Cal	**Name**	DEHP ST-04
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

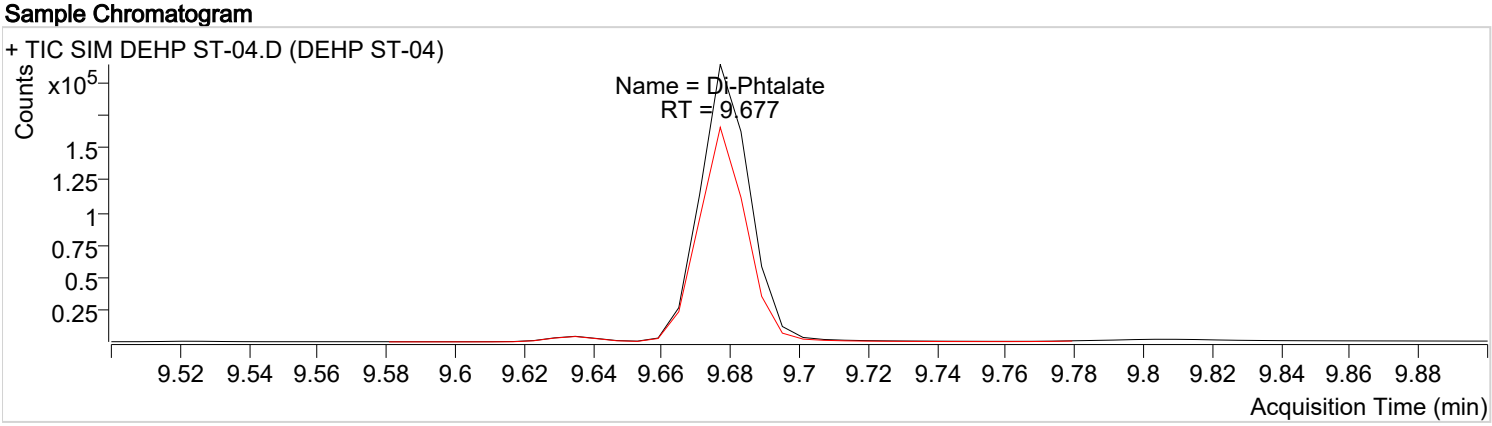

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.677	159913	0.0107	mg/L

Di-Phtalate

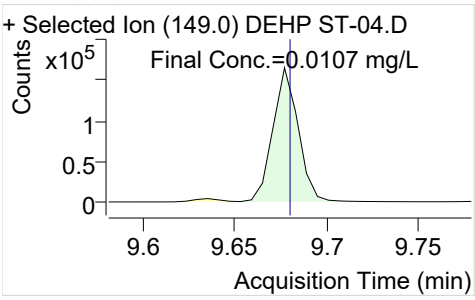

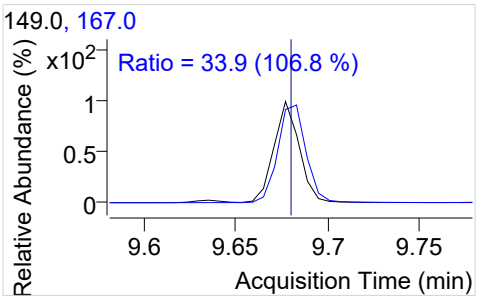

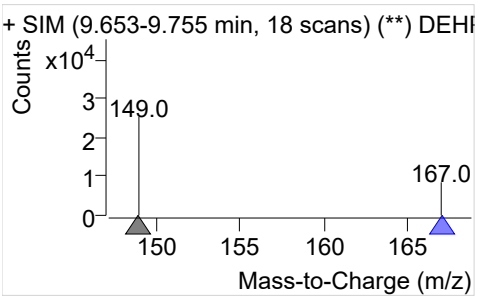

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:56:54	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 1:56:38	**Data File**	DEHP ST-05.D
Type	Cal	**Name**	DEHP ST-05
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

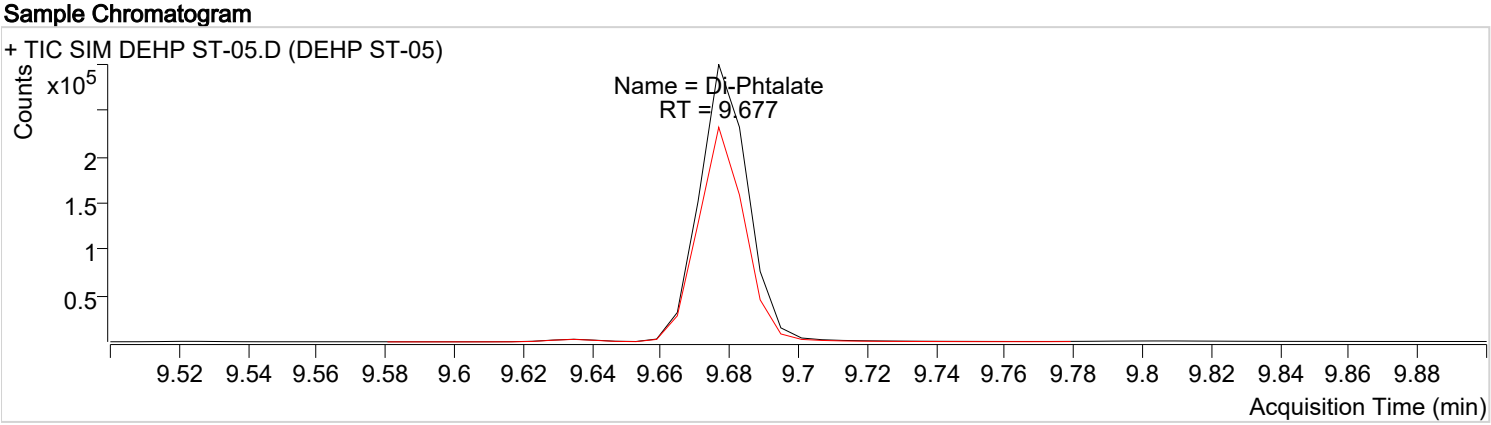

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.677	220036	0.0154	mg/L

Di-Phtalate

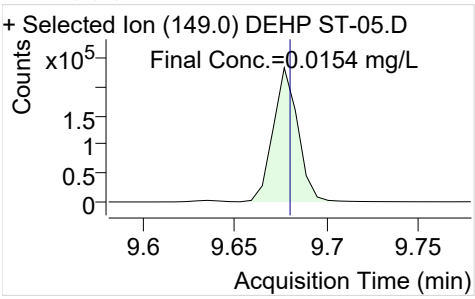



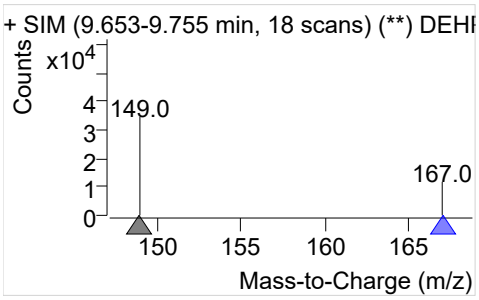

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:56:54	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 2:10:21	**Data File**	DEHP ST-06.D
Type	Cal	**Name**	DEHP ST-06
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

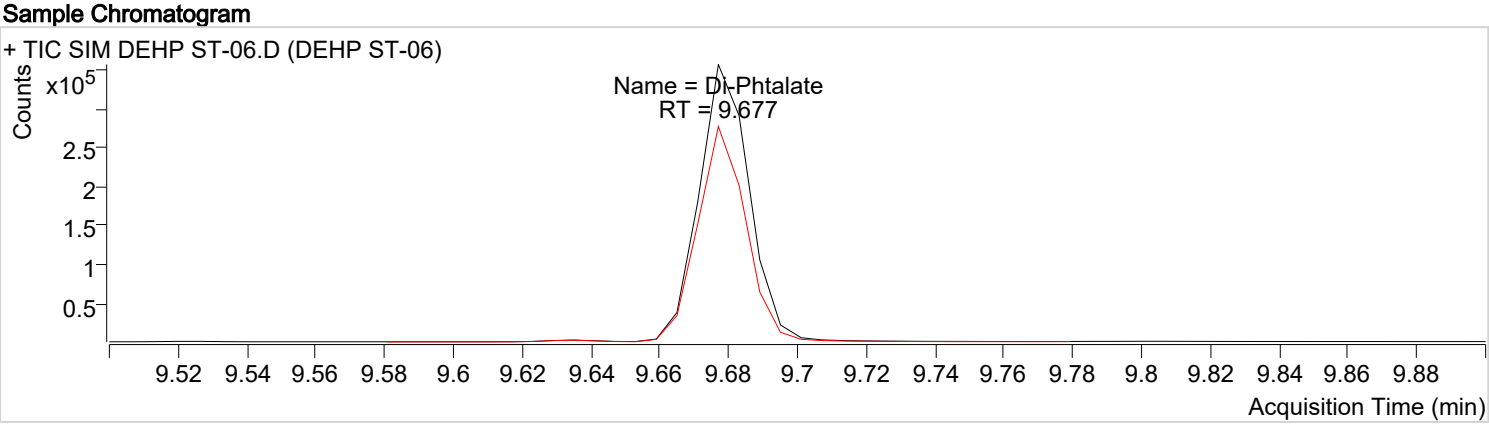

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.677	270539	0.0193	mg/L

Di-Phtalate

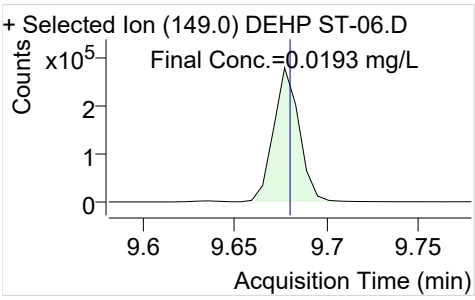

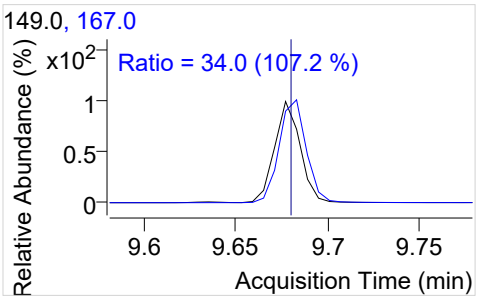

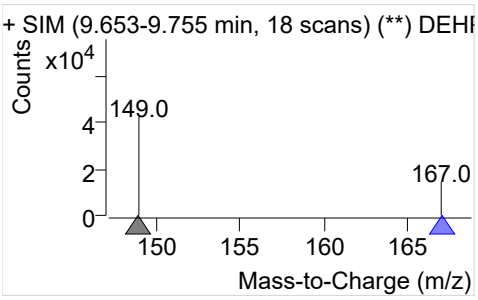

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:56:54	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 2:43:39	**Data File**	BK.D
Type	Blank	**Name**	BK
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

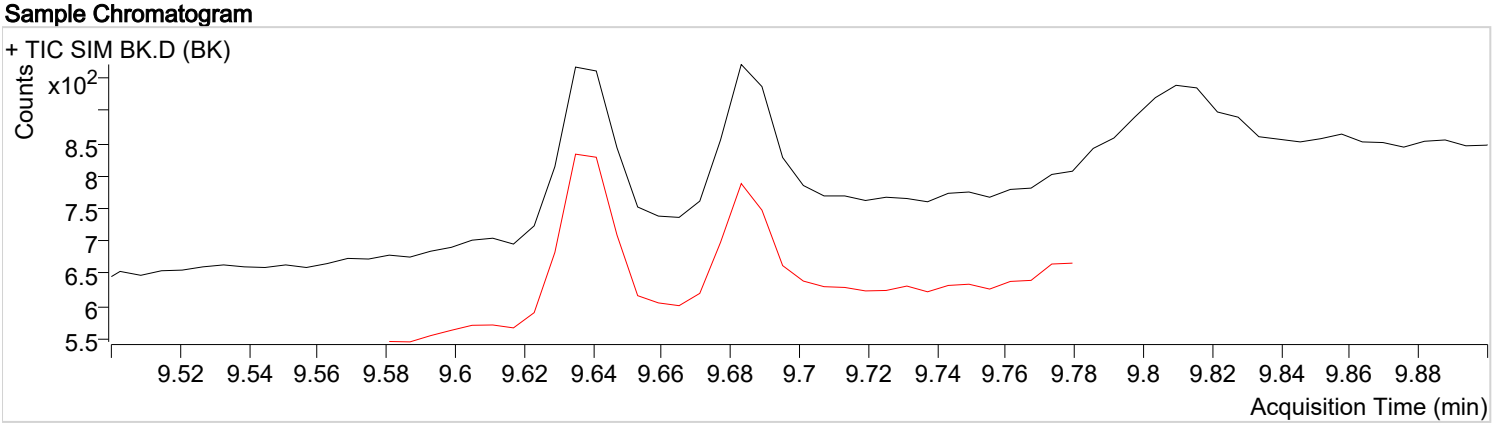

Di-Phtalate





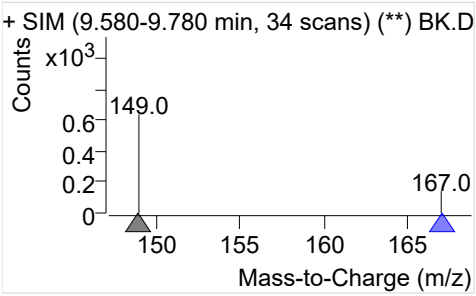

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:56:54	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 3:44:21	**Data File**	FBK(RE 26-03-17).D
Type	Blank	**Name**	FBK(RE 26-03-17)
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

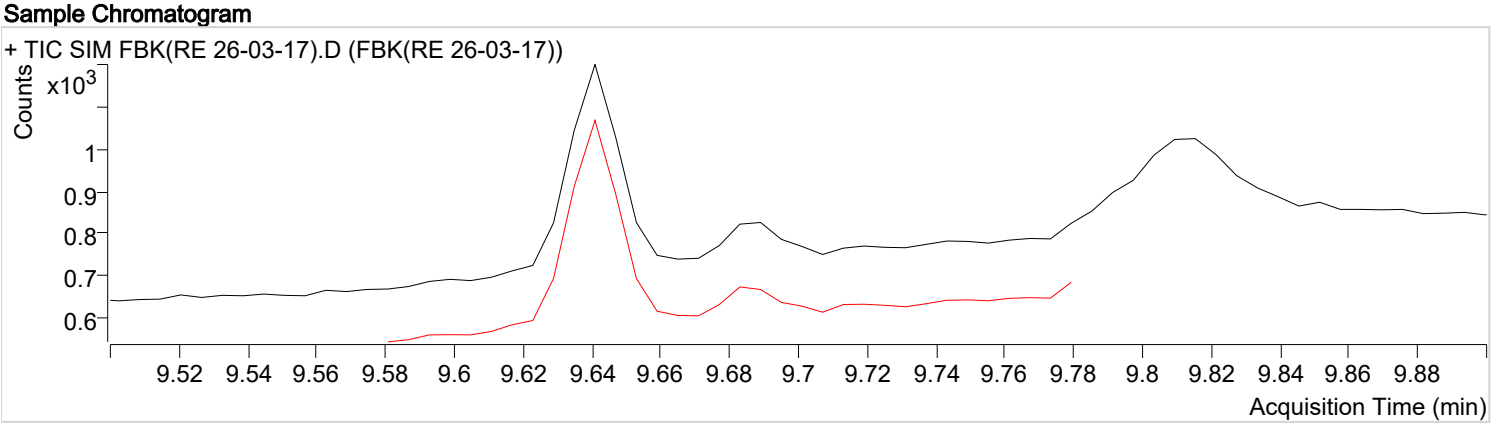

Di-Phtalate





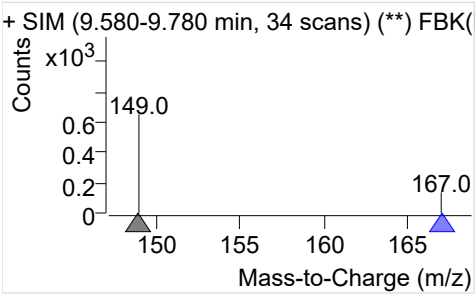

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:56:54	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 3:58:02	**Data File**	FBK(RE 26-03-18).D
Type	Blank	**Name**	FBK(RE 26-03-18)
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

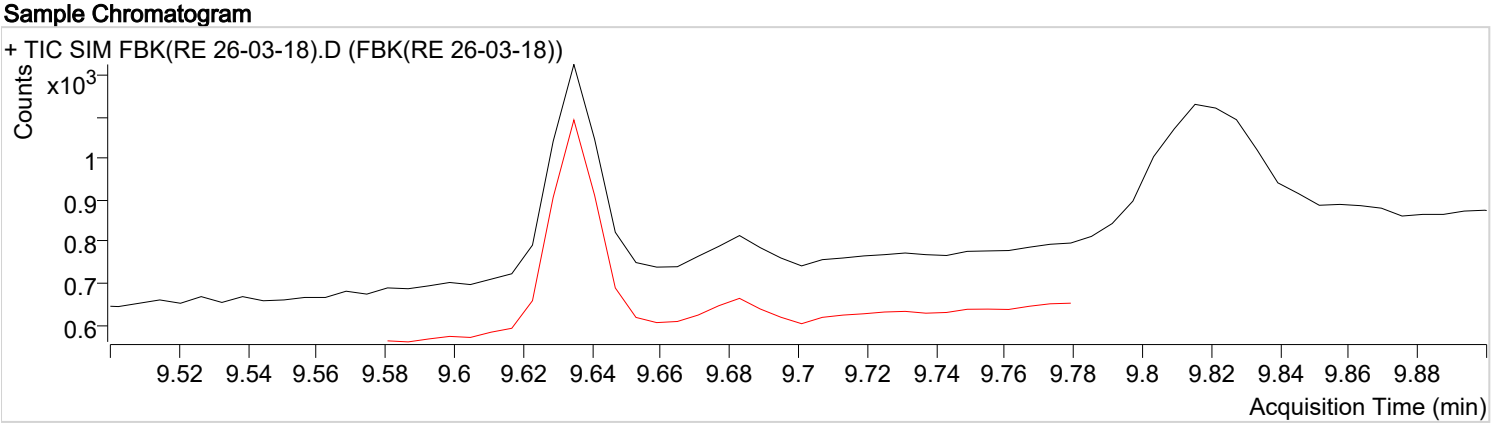

Di-Phtalate





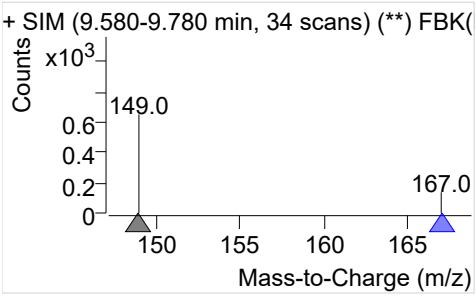

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:56:54	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 4:11:43	**Data File**	FBK(HS 26-03-18).D
Type	Blank	**Name**	FBK(HS 26-03-18)
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

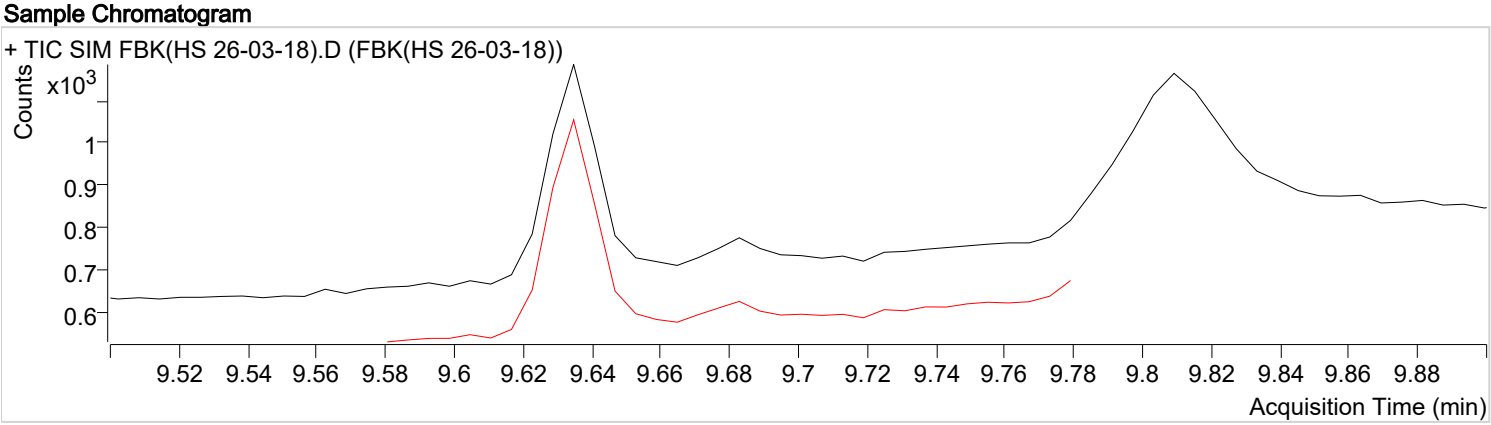

Di-Phtalate





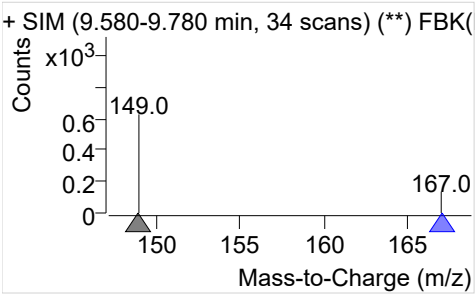

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:56:54	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 4:25:27	**Data File**	RE-05.D
Type	Sample	**Name**	RE-05
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

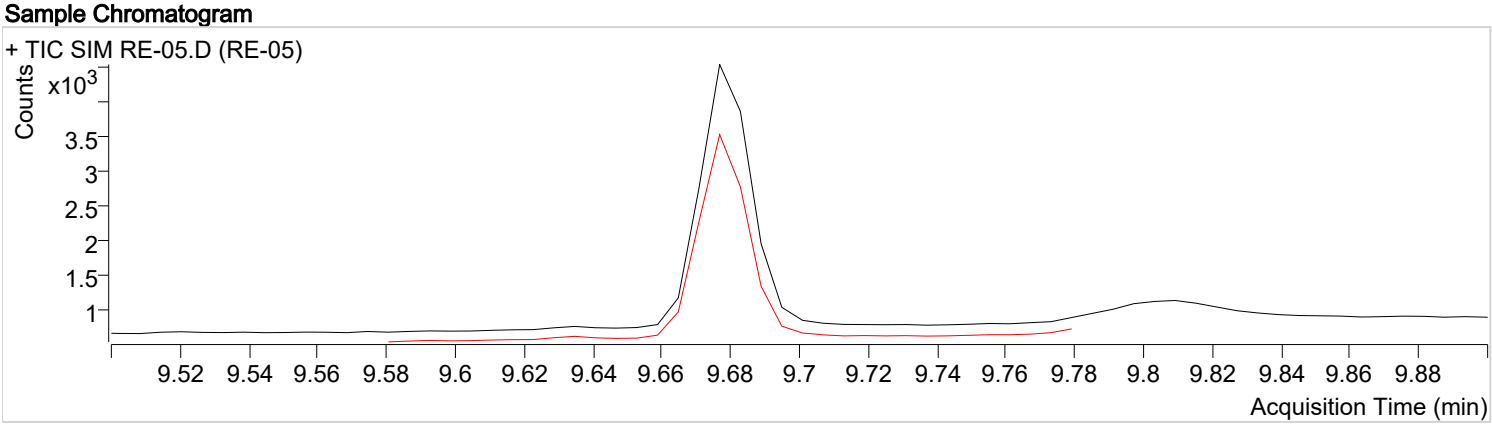

Di-Phtalate





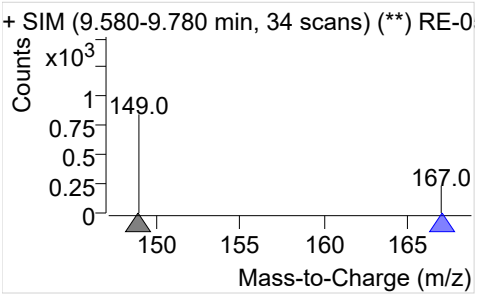

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:56:54	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 4:39:12	**Data File**	RE-06.D
Type	Sample	**Name**	RE-06
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

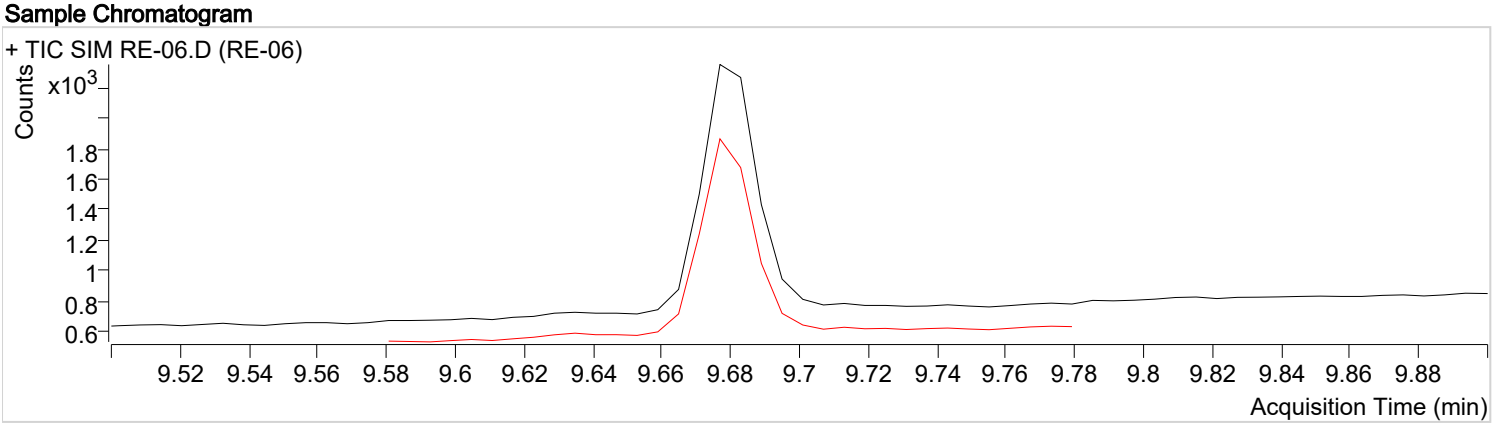

Di-Phtalate





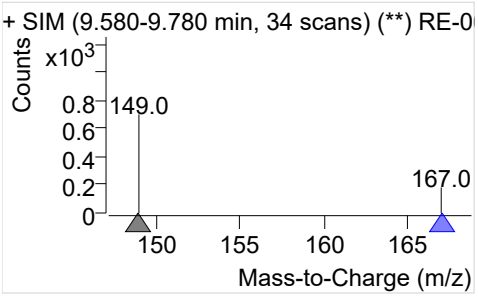

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:56:54	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 4:52:57	**Data File**	RE-13.D
Type	Sample	**Name**	RE-13
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

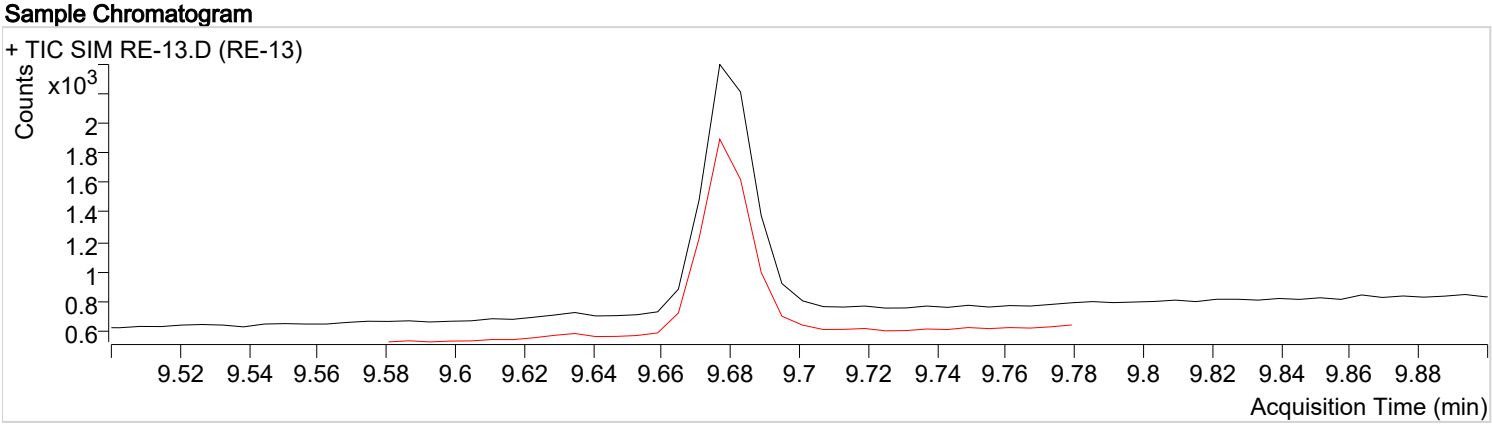

Di-Phtalate





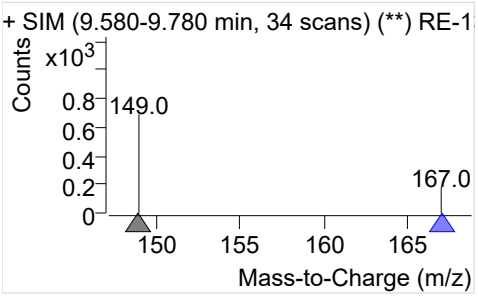

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:56:54	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 5:06:39	**Data File**	RE-14.D
Type	Sample	**Name**	RE-14
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

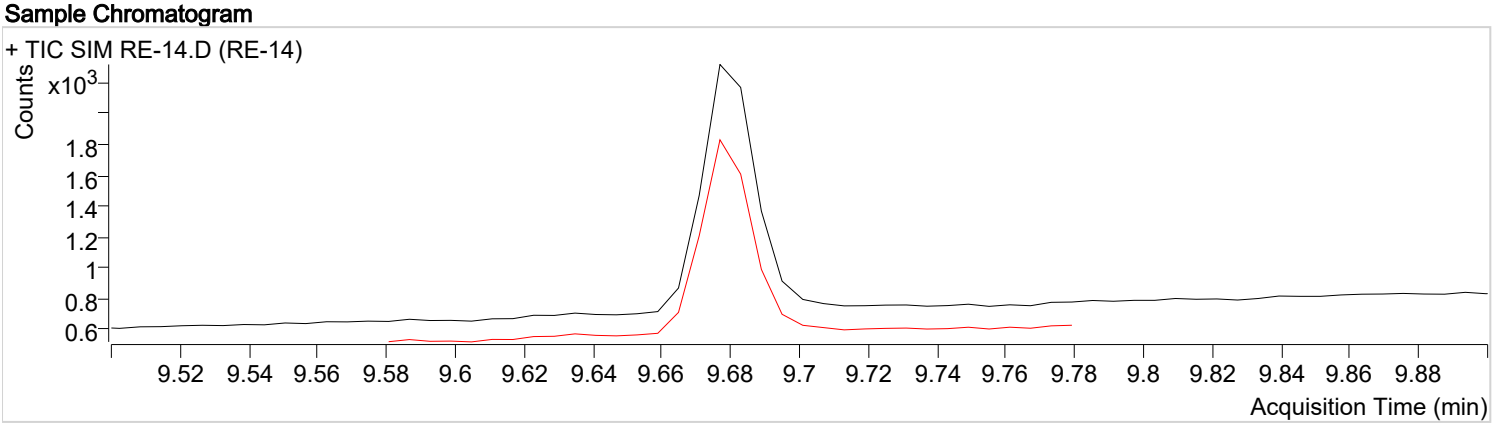

Di-Phtalate





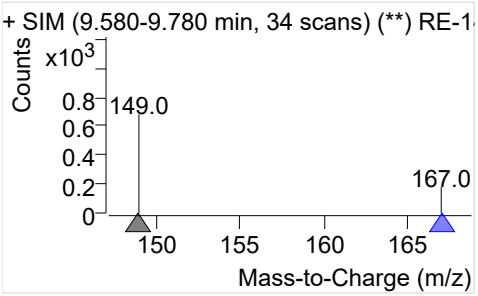

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:56:54	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 5:20:24	**Data File**	RE-24.D
Type	Sample	**Name**	RE-24
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

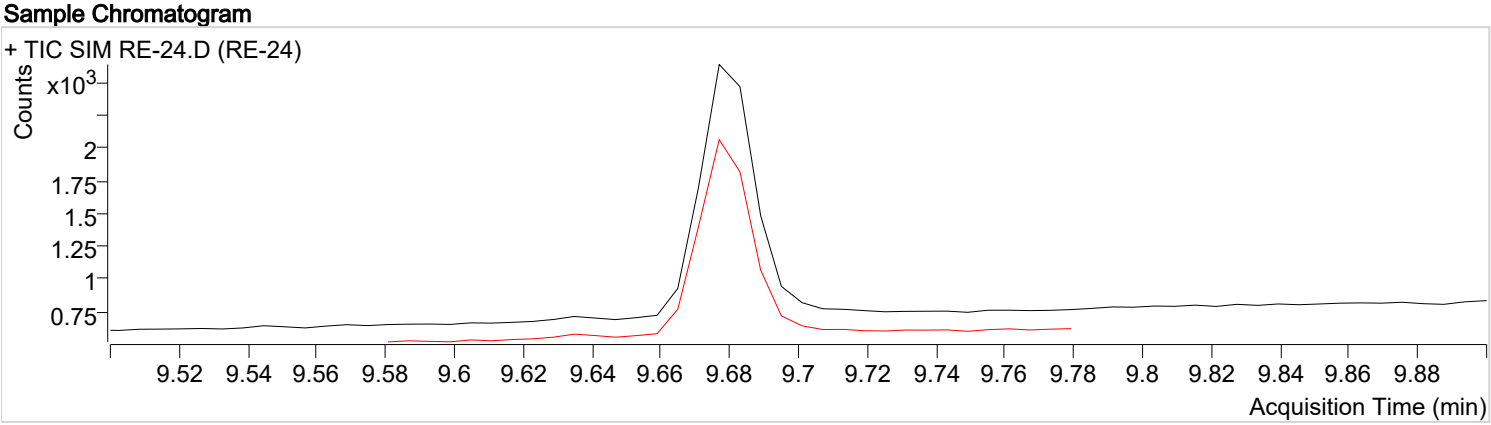

Di-Phtalate





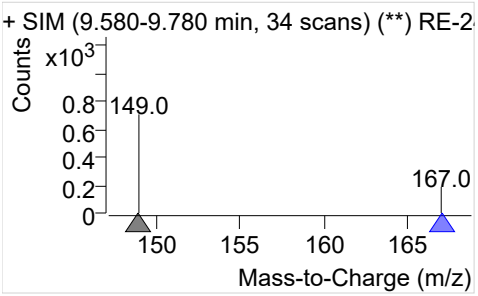

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:56:54	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 5:34:09	**Data File**	RE-25.D
Type	Sample	**Name**	RE-25
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

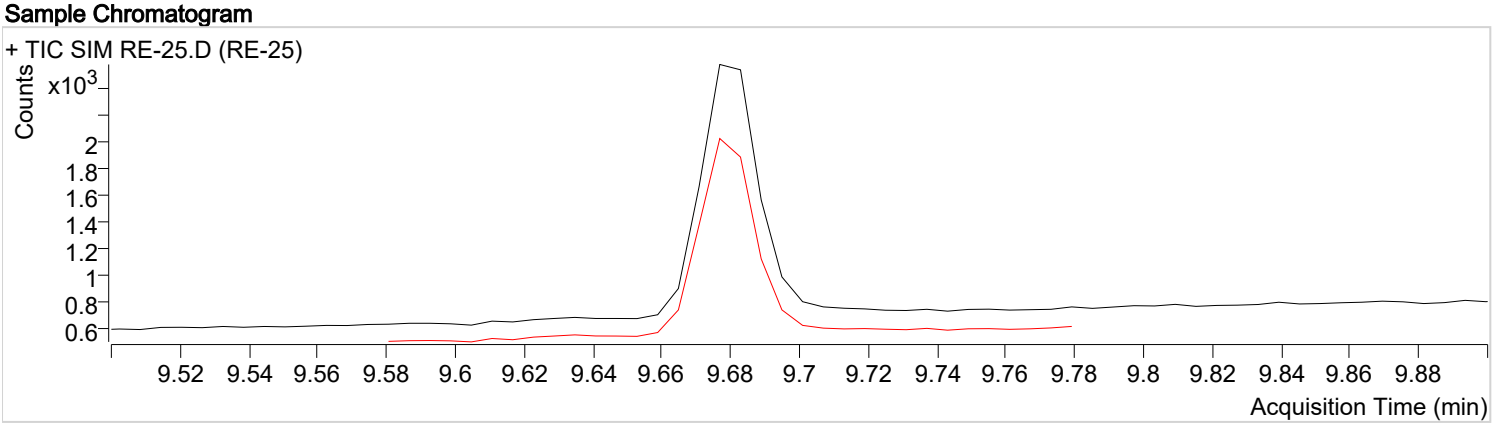

Di-Phtalate





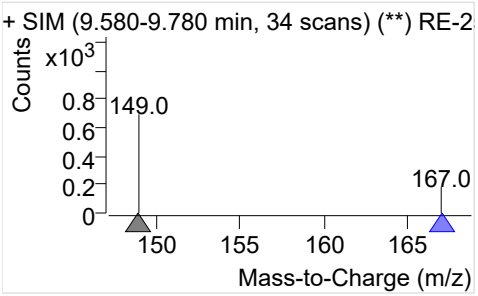

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:56:54	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 5:47:54	**Data File**	HS 26-03-18.D
Type	Sample	**Name**	HS 26-03-18
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

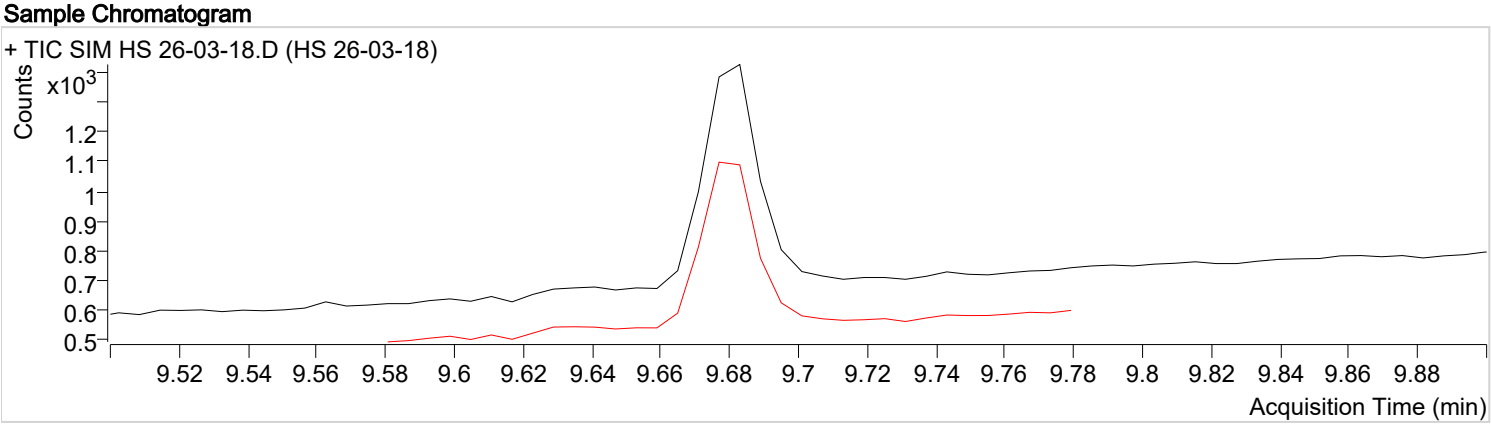

Di-Phtalate





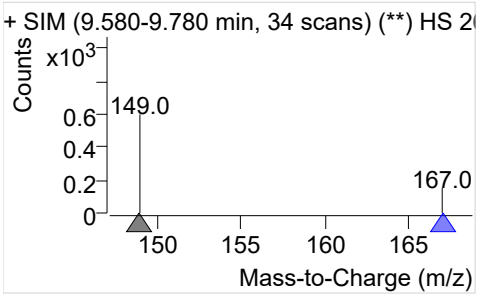

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:56:54	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 6:01:38	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

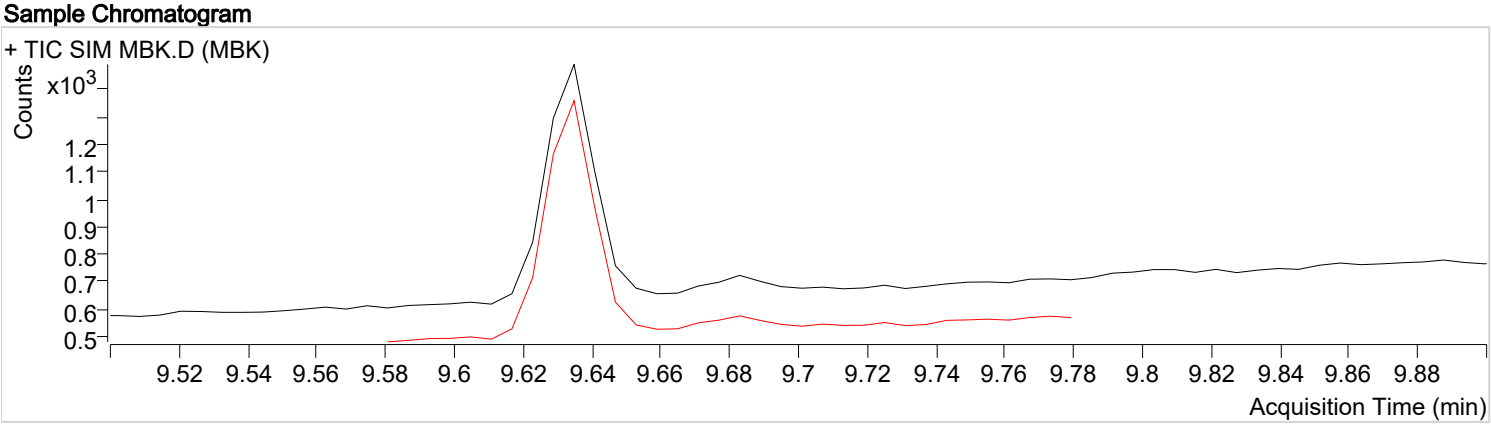

Di-Phtalate





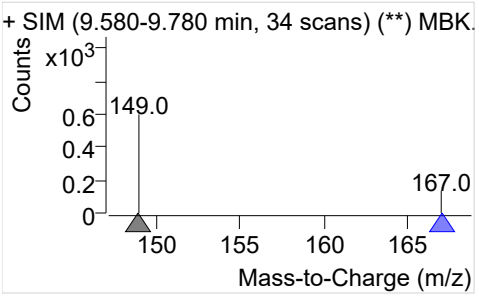

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\DEHP(RE 3.17.18 HS 3.18)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-03-24 오전 11:07:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:56:54	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:07:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 6:42:48	**Data File**	-C-C-V-.D
Type	QC	**Name**	-C-C-V-
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

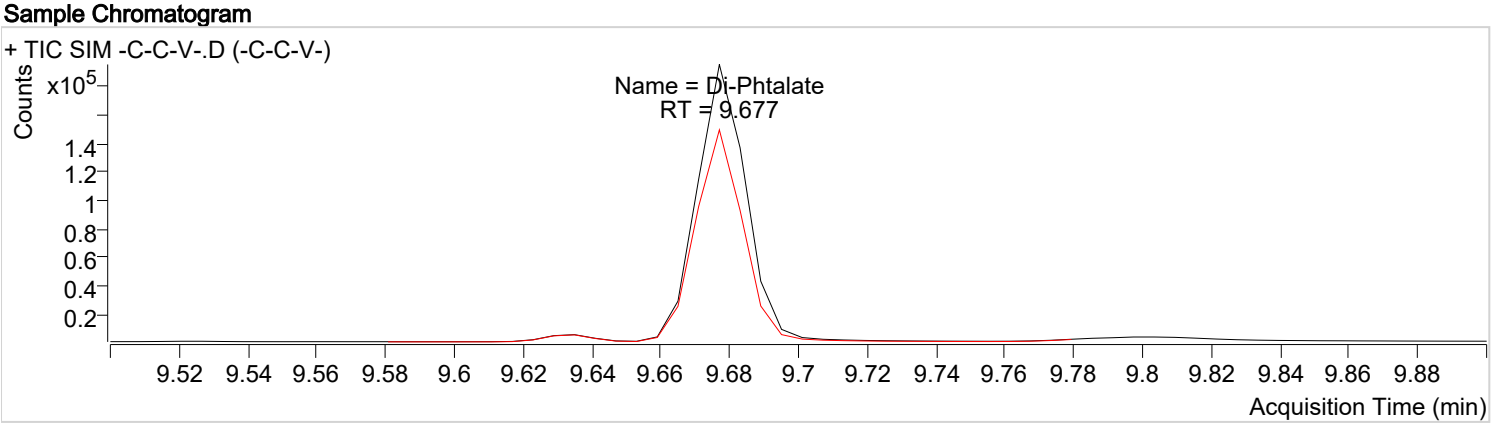

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	9.677	144583	0.0095	mg/L
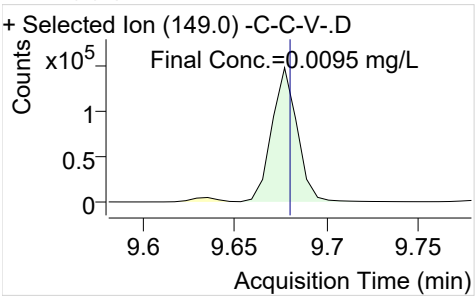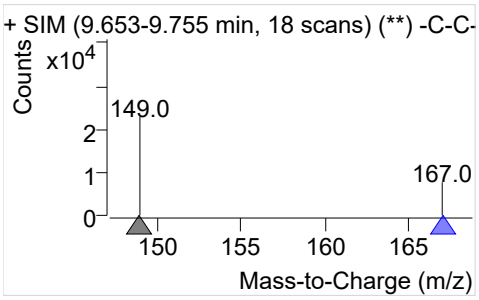
Di-Phtalate