Quantitative Analysis Results Summary Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-01\DEHP(PL 12.30)\QuantResults\DEHP.batch.bin				
Analysis Time	2026-01-08 오전 11:56:16	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:56:16	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Di-Phtalate

Data File	Type	RT	Resp.	Final Conc.
DEHP ST-01.d	Cal	5.694	21866	0.0030
DEHP ST-02.d	Cal	5.688	35736	0.0048
DEHP ST-03.d	Cal	5.688	48748	0.0066
DEHP ST-04.d	Cal	5.688	77380	0.0104
DEHP ST-05.d	Cal	5.688	112113	0.0151
BK-.d	Blank			ND
FBK(PL 25-12-30).d	Blank			ND
PL-01.d	Sample			ND
PL-02.d	Sample			ND
MBK-1.d	Blank			ND
C-C-V-1.d	QC	5.688	44373	0.0060

Di-Phtalate

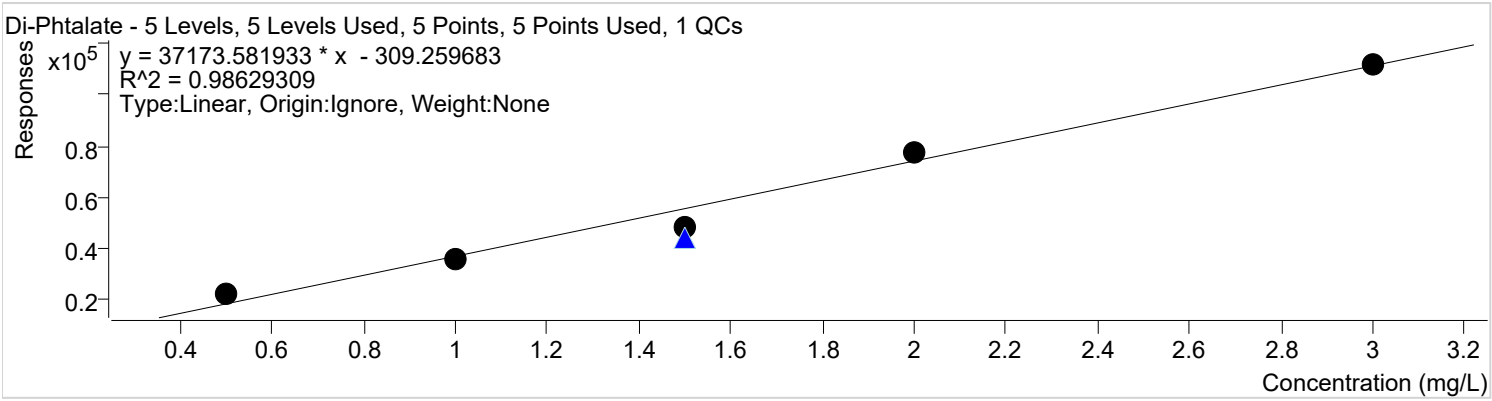

Cal. Path	Type	Level	Enable	Conc.	Response
V:\2026\2026-01\DEHP(PL 12.30)\DEHP ST-01.d	Calibration	1	x	0.500	21866
V:\2026\2026-01\DEHP(PL 12.30)\DEHP ST-02.d	Calibration	2	x	1.000	35736
V:\2026\2026-01\DEHP(PL 12.30)\DEHP ST-03.d	Calibration	3	x	1.500	48748
V:\2026\2026-01\DEHP(PL 12.30)\C-C-V-1.d	QC	3	x	1.500	44373
V:\2026\2026-01\DEHP(PL 12.30)\DEHP ST-04.d	Calibration	4	x	2.000	77380
V:\2026\2026-01\DEHP(PL 12.30)\DEHP ST-05.d	Calibration	5	x	3.000	112113

Quant Sample Report

Batch Data Path	V:\2026\2026-01\DEHP(PL 12.30)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-01-08 오전 11:56:16	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:58:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:56:16	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-06 오후 4:21:30	**Data File**	DEHP ST-01.d
Type	Cal	**Name**	DEHP ST-01
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

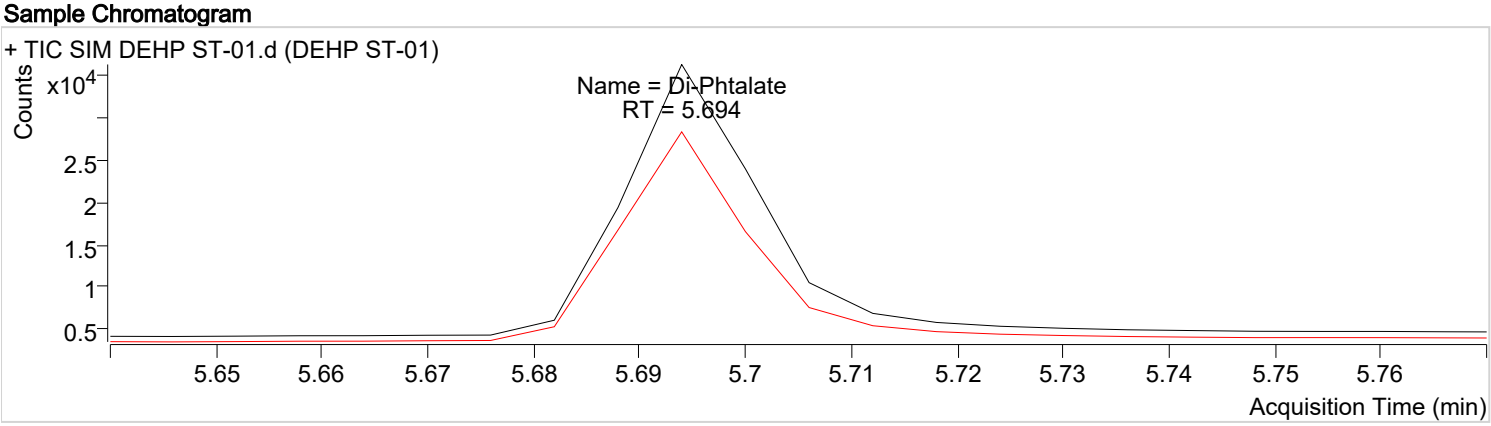

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	5.694	21866	0.0030	mg/L

Di-Phtalate

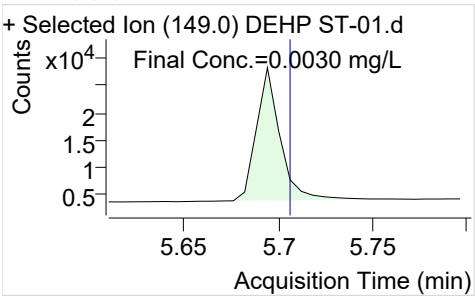

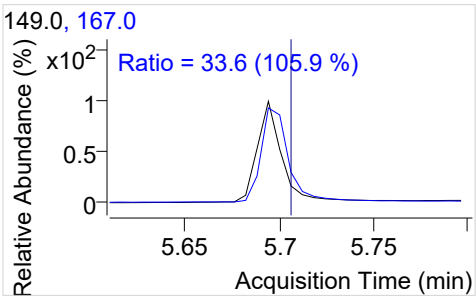

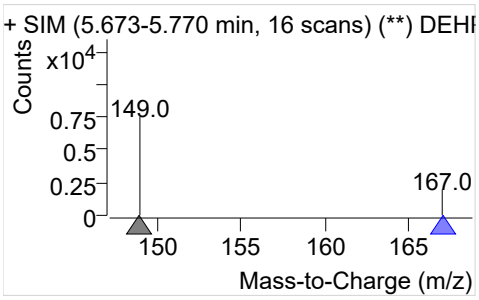

Quant Sample Report

Batch Data Path	V:\2026\2026-01\DEHP(PL 12.30)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-01-08 오전 11:56:16	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:58:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:56:16	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-06 오후 4:30:11	**Data File**	DEHP ST-02.d
Type	Cal	**Name**	DEHP ST-02
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

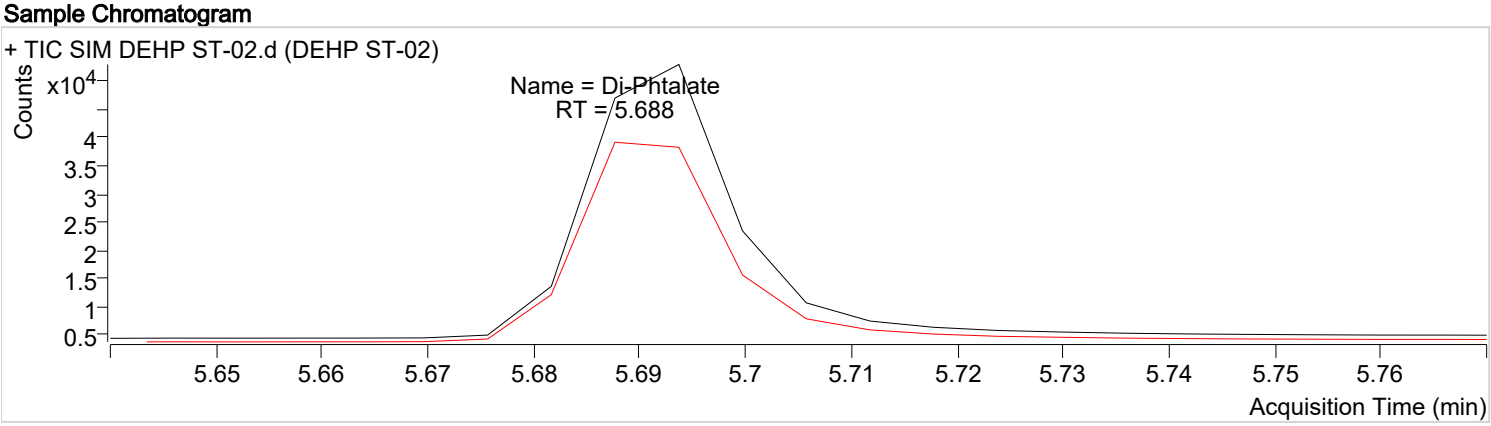

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	5.688	35736	0.0048	mg/L

Di-Phtalate

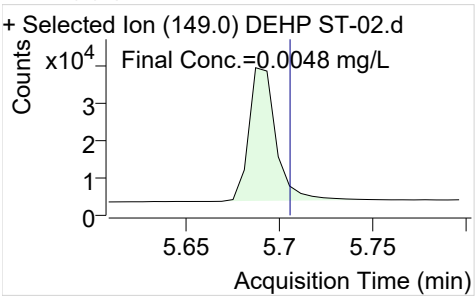

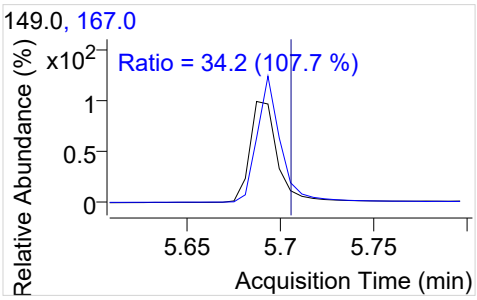

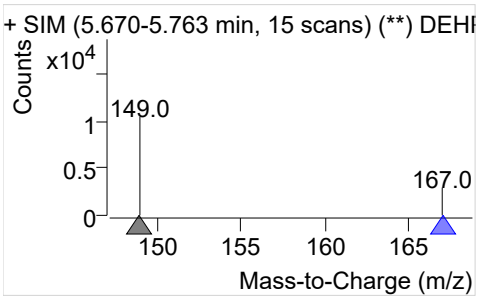

Quant Sample Report

Batch Data Path	V:\2026\2026-01\DEHP(PL 12.30)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-01-08 오전 11:56:16	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:58:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:56:16	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-06 오후 4:38:52	**Data File**	DEHP ST-03.d
Type	Cal	**Name**	DEHP ST-03
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

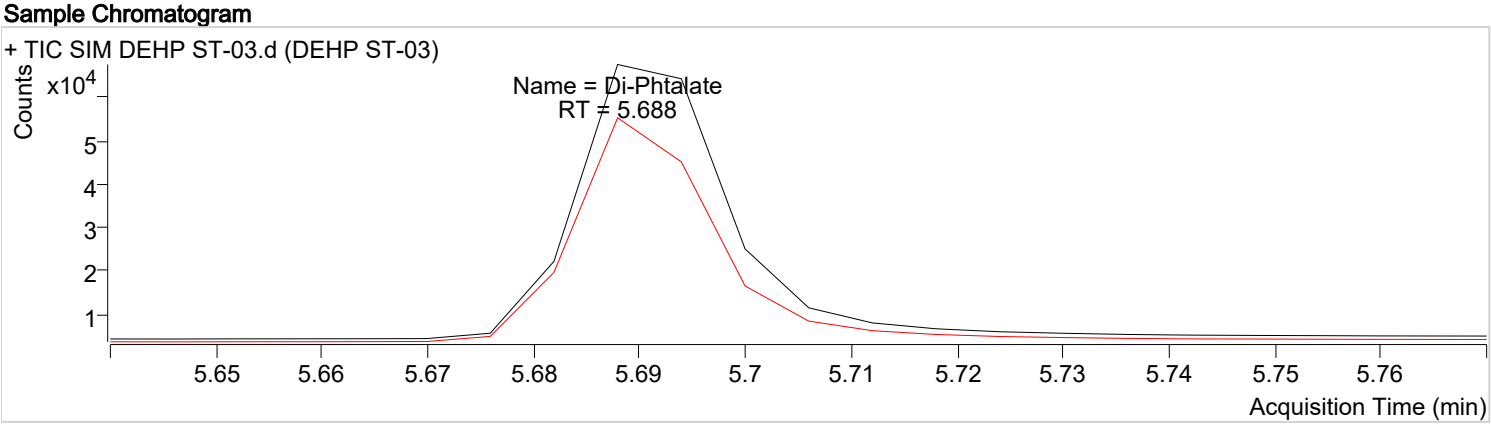

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	5.688	48748	0.0066	mg/L

Di-Phtalate

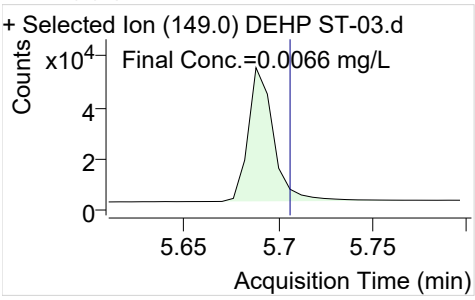

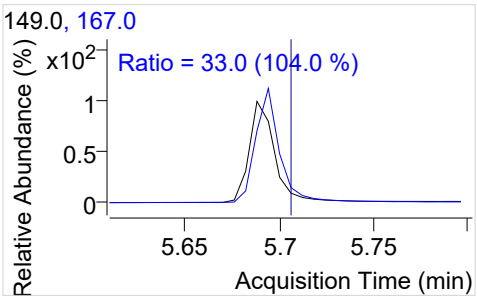

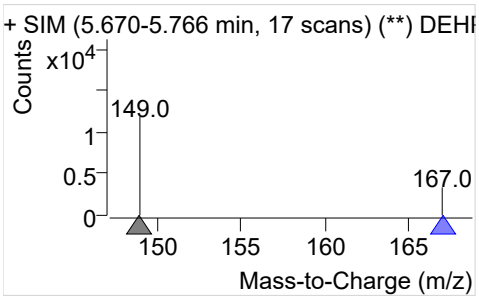

Quant Sample Report

Batch Data Path	V:\2026\2026-01\DEHP(PL 12.30)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-01-08 오전 11:56:16	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:58:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:56:16	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-06 오후 4:47:35	**Data File**	DEHP ST-04.d
Type	Cal	**Name**	DEHP ST-04
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

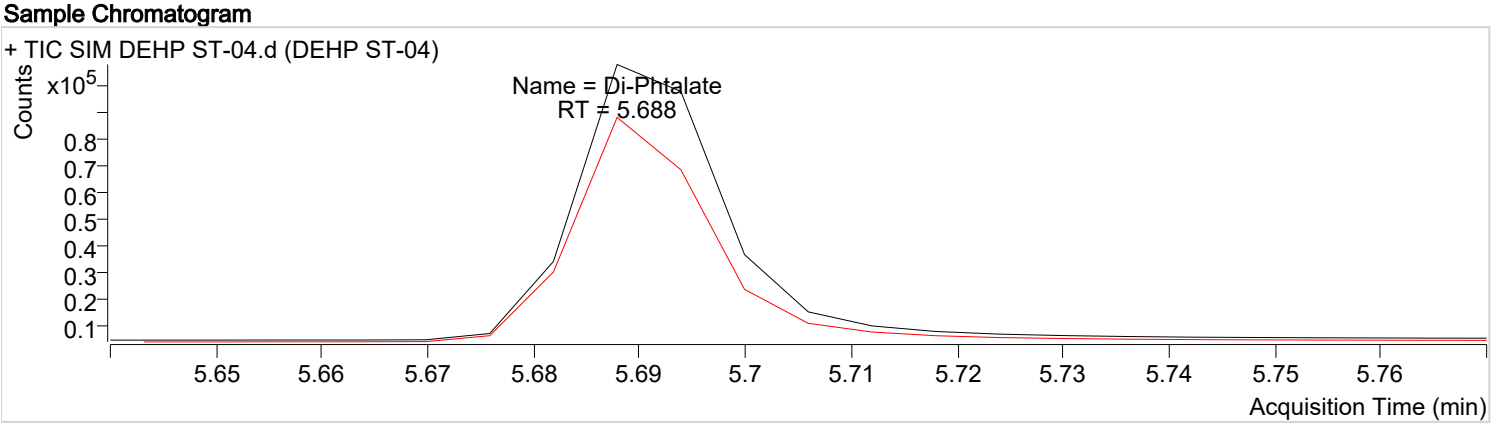

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	5.688	77380	0.0104	mg/L

Di-Phtalate

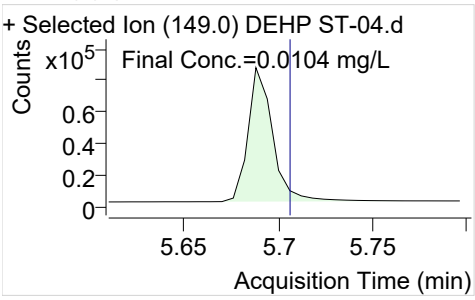

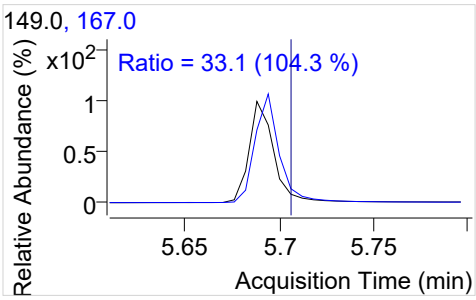

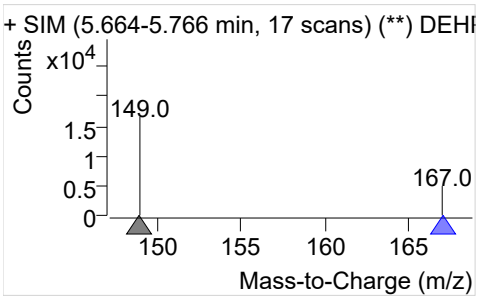

Quant Sample Report

Batch Data Path	V:\2026\2026-01\DEHP(PL 12.30)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-01-08 오전 11:56:16	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:58:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:56:16	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-06 오후 4:56:19	**Data File**	DEHP ST-05.d
Type	Cal	**Name**	DEHP ST-05
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

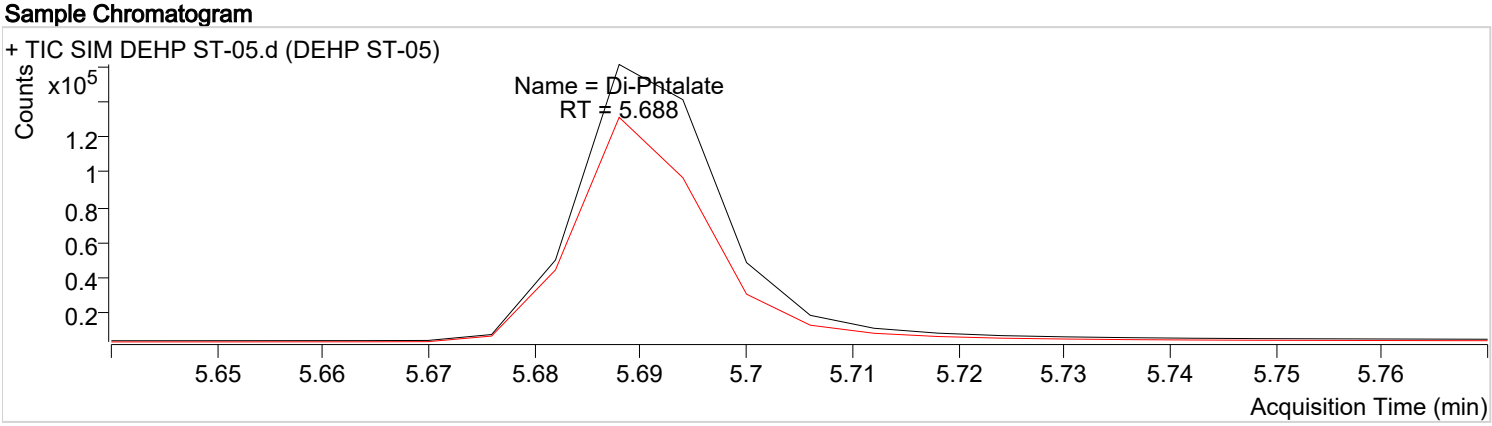

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	5.688	112113	0.0151	mg/L

Di-Phtalate

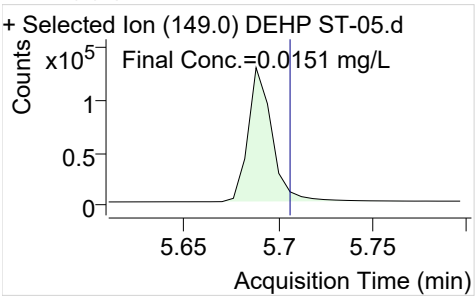

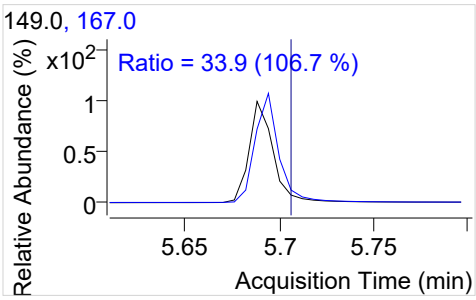

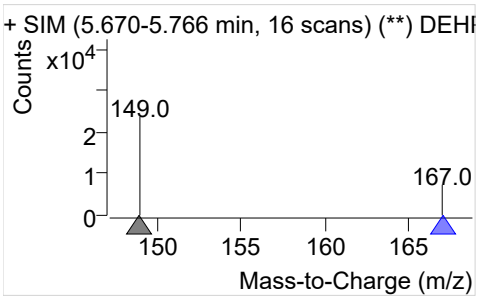

Quant Sample Report

Batch Data Path	V:\2026\2026-01\DEHP(PL 12.30)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-01-08 오전 11:56:16	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:58:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:56:16	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-06 오후 5:22:28	**Data File**	BK-.d
Type	Blank	**Name**	BK-
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

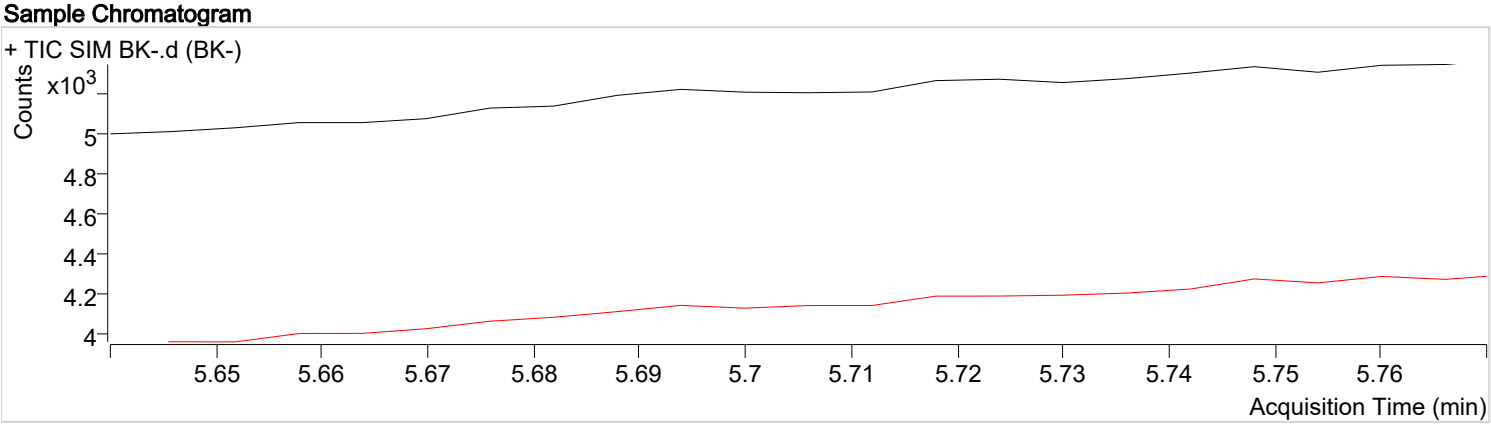

Di-Phtalate

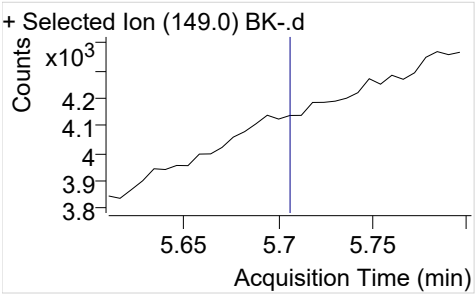

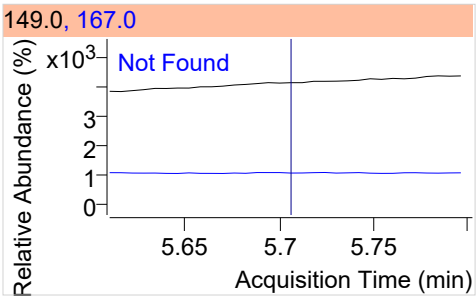

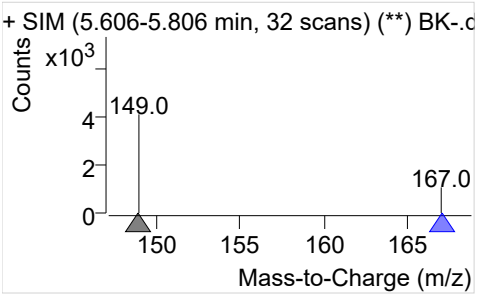

Quant Sample Report

Batch Data Path	V:\2026\2026-01\DEHP(PL 12.30)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-01-08 오전 11:56:16	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:58:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:56:16	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-06 오후 5:31:09	**Data File**	FBK(PL 25-12-30).d
Type	Blank	**Name**	FBK(PL 25-12-30)
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

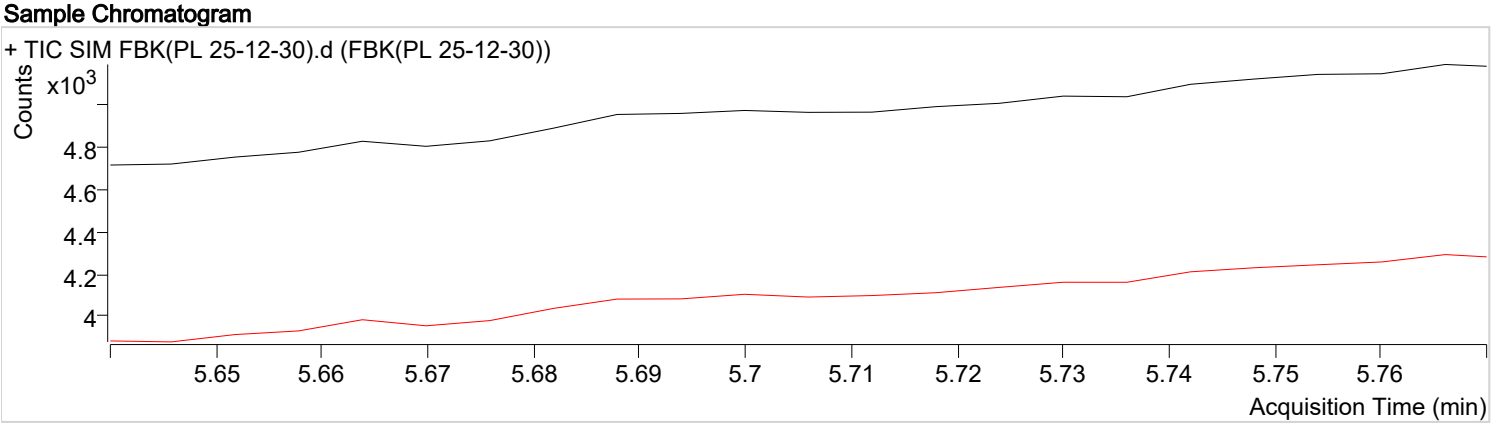

Di-Phtalate

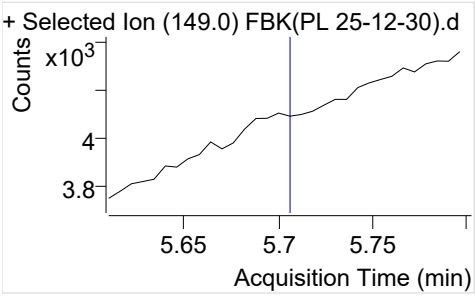

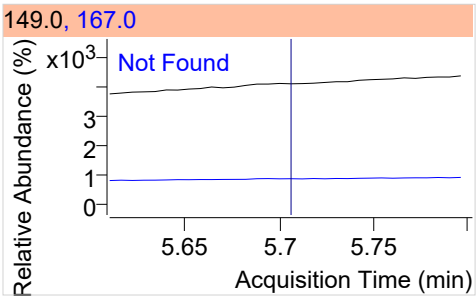

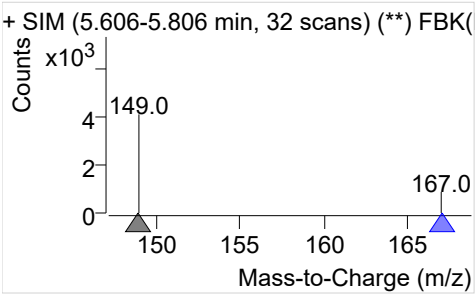

Quant Sample Report

Batch Data Path	V:\2026\2026-01\DEHP(PL 12.30)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-01-08 오전 11:56:16	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:58:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:56:16	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-06 오후 5:39:51	**Data File**	PL-01.d
Type	Sample	**Name**	PL-01
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

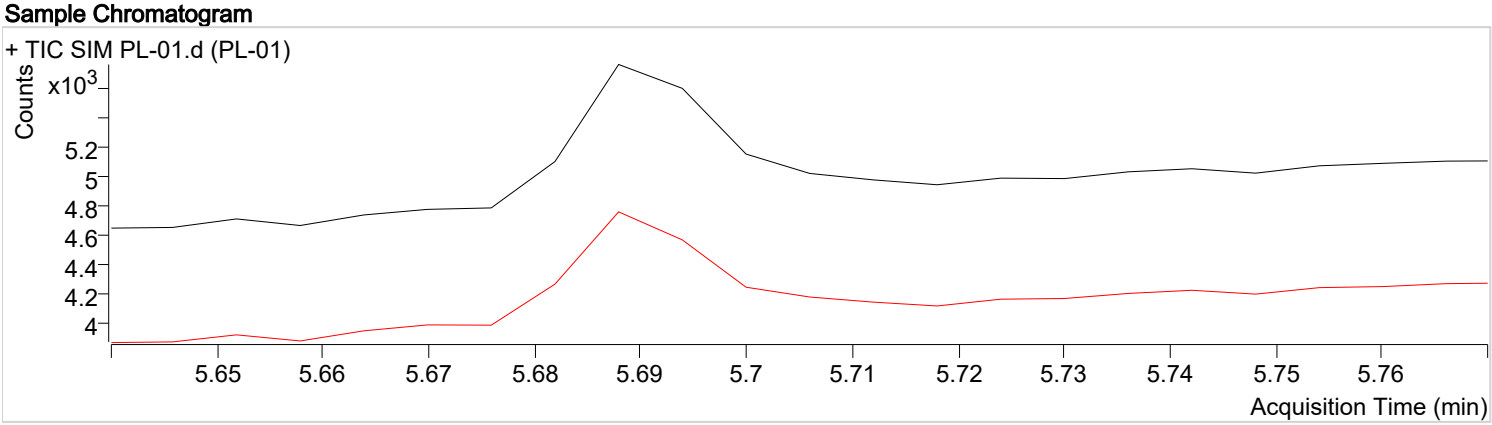

Di-Phtalate

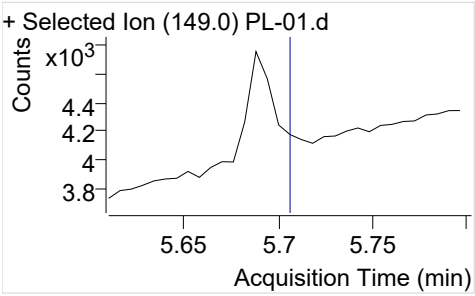

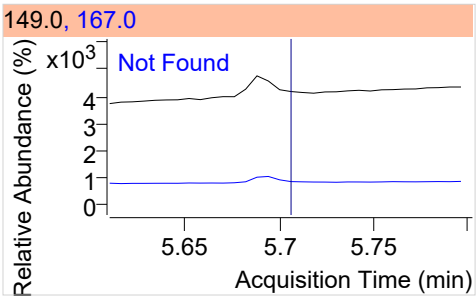

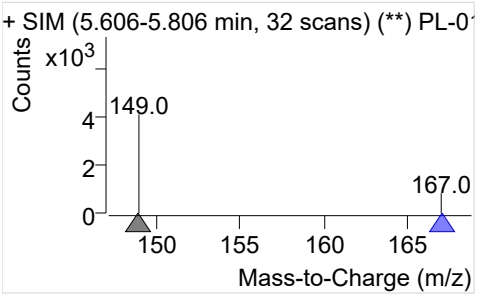

Quant Sample Report

Batch Data Path	V:\2026\2026-01\DEHP(PL 12.30)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-01-08 오전 11:56:16	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:58:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:56:16	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-06 오후 5:48:34	**Data File**	PL-02.d
Type	Sample	**Name**	PL-02
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

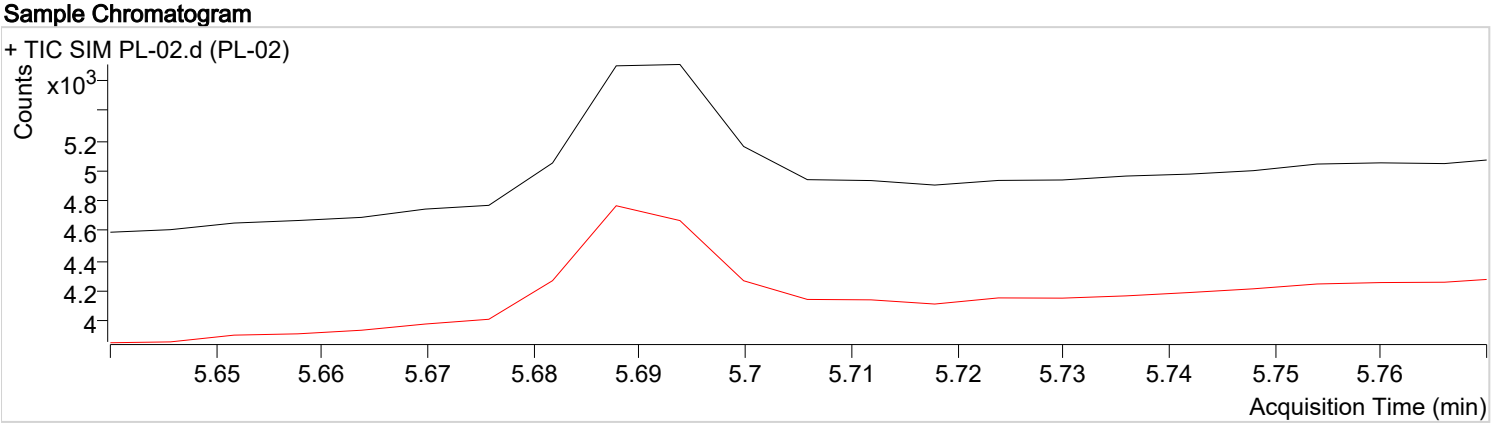

Di-Phtalate

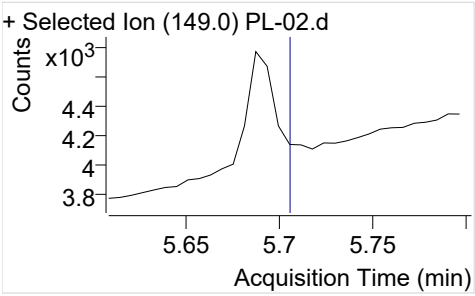

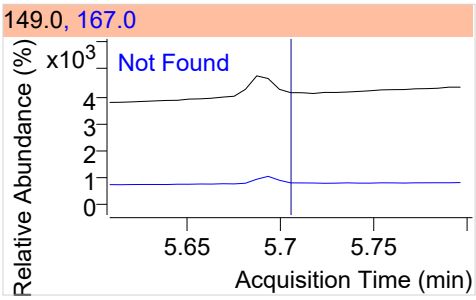

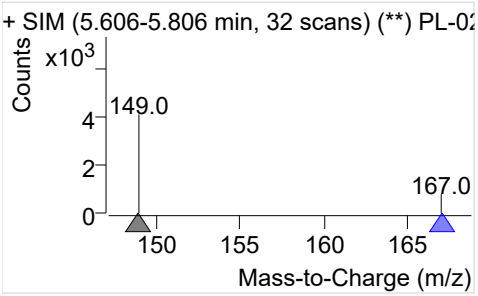

Quant Sample Report

Batch Data Path	V:\2026\2026-01\DEHP(PL 12.30)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-01-08 오전 11:56:16	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:58:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:56:16	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-06 오후 5:57:17	**Data File**	MBK-1.d
Type	Blank	**Name**	MBK-1
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

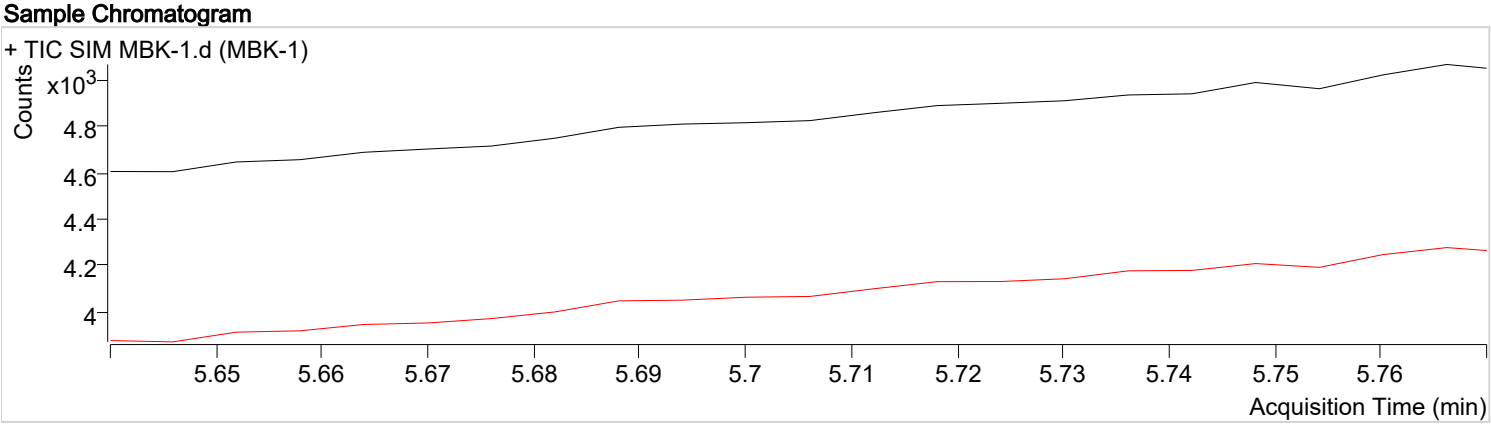

Di-Phtalate

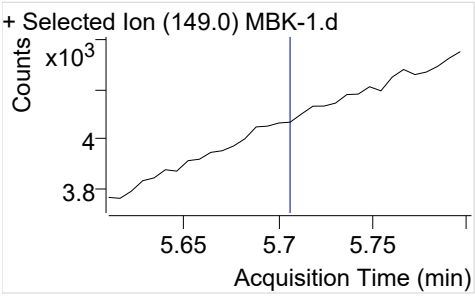

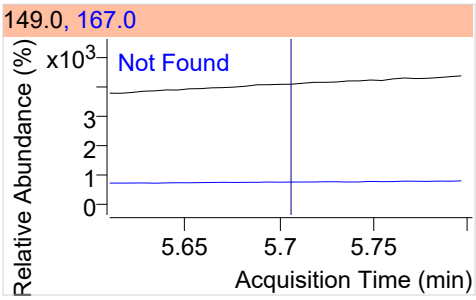

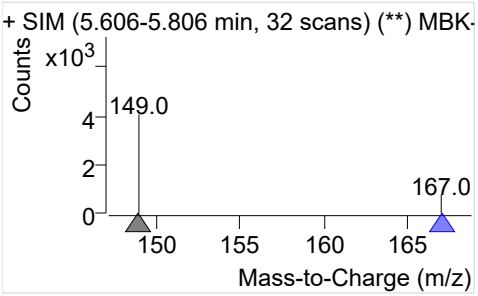

Quant Sample Report

Batch Data Path	V:\2026\2026-01\DEHP(PL 12.30)\QuantResults\DEHP.batch.bin		
Analysis Time	2026-01-08 오전 11:56:16	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:58:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:56:16	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-06 오후 6:23:28	**Data File**	C-C-V-1.d
Type	QC	**Name**	C-C-V-1
Dil.	0.005	**Acq. Method File**	ORG(DEHP)

Sample Chromatogram

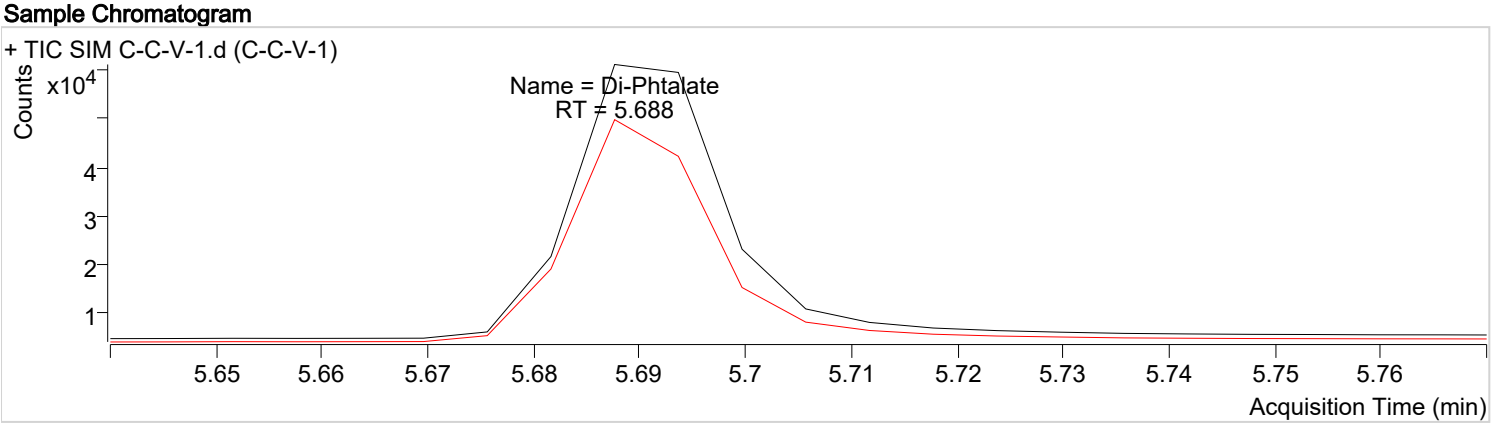

Name	RT	Resp.	Final Conc.	Units
Di-Phtalate	5.688	44373	0.0060	mg/L
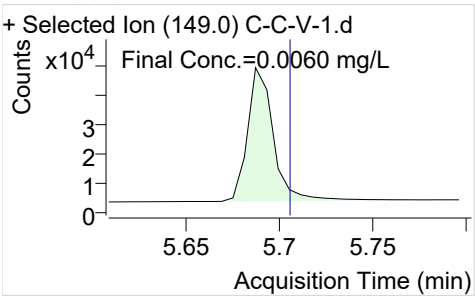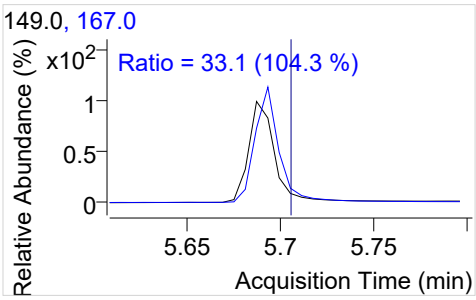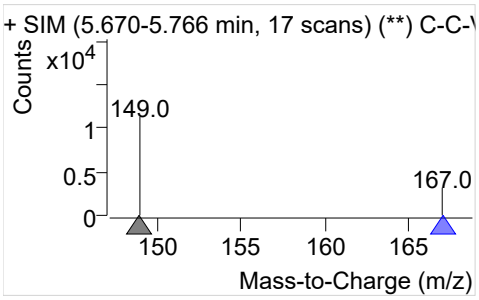
Di-Phtalate