Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\VOC10(JR 3.19 HH 3.24)\QuantResults\VOC10.batch.bin				
Analysis Time	2026-03-25 오후 4:37:11	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-25 오후 4:37:11	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Chloroform

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
VOC10 ST-01.D	Cal	5.715	8170	4240	0.011
VOC10 ST-02.D	Cal	5.720	15381	4116	0.021
VOC10 ST-03.D	Cal	5.720	45419	4816	0.052
VOC10 ST-04.D	Cal	5.715	76475	4329	0.096
VOC10 ST-05.D	Cal	5.720	131578	3570	0.199
VOC10 ST-06.D	Cal	5.715	252196	3387	0.401
BK-.D	Blank			4756	ND
FBK(HH 26-03-24).D	Blank			4388	ND
JR 26-03-19.D	Sample			4503	ND
HH-03.D	Sample	5.715	5664	4074	0.008
HH-04.D	Sample			4157	ND
MBK.D	Blank			3709	ND
CCV-.D	QC	5.720	119041	2836	0.227

Benzene

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
VOC10 ST-01.D	Cal	5.993	19919	4240	0.011
VOC10 ST-02.D	Cal	5.993	37557	4116	0.021
VOC10 ST-03.D	Cal	5.993	109085	4816	0.052
VOC10 ST-04.D	Cal	5.993	181801	4329	0.095
VOC10 ST-05.D	Cal	5.993	314123	3570	0.200
VOC10 ST-06.D	Cal	5.993	599803	3387	0.401
BK-.D	Blank			4756	ND
FBK(HH 26-03-24).D	Blank			4388	ND
JR 26-03-19.D	Sample			4503	ND
HH-03.D	Sample			4074	ND
HH-04.D	Sample			4157	ND
MBK.D	Blank			3709	ND
CCV-.D	QC	5.993	276933	2836	0.221

Toluene

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
VOC10 ST-01.D	Cal	6.851	22786	4240	0.011
VOC10 ST-02.D	Cal	6.851	42932	4116	0.021
VOC10 ST-03.D	Cal	6.851	128925	4816	0.053
VOC10 ST-04.D	Cal	6.851	210383	4329	0.095
VOC10 ST-05.D	Cal	6.851	364705	3570	0.200
VOC10 ST-06.D	Cal	6.851	692861	3387	0.401
BK-.D	Blank			4756	ND
FBK(HH 26-03-24).D	Blank			4388	ND
JR 26-03-19.D	Sample			4503	ND
HH-03.D	Sample			4074	ND
HH-04.D	Sample			4157	ND
MBK.D	Blank			3709	ND
CCV-.D	QC	6.851	315420	2836	0.218

Chloroform

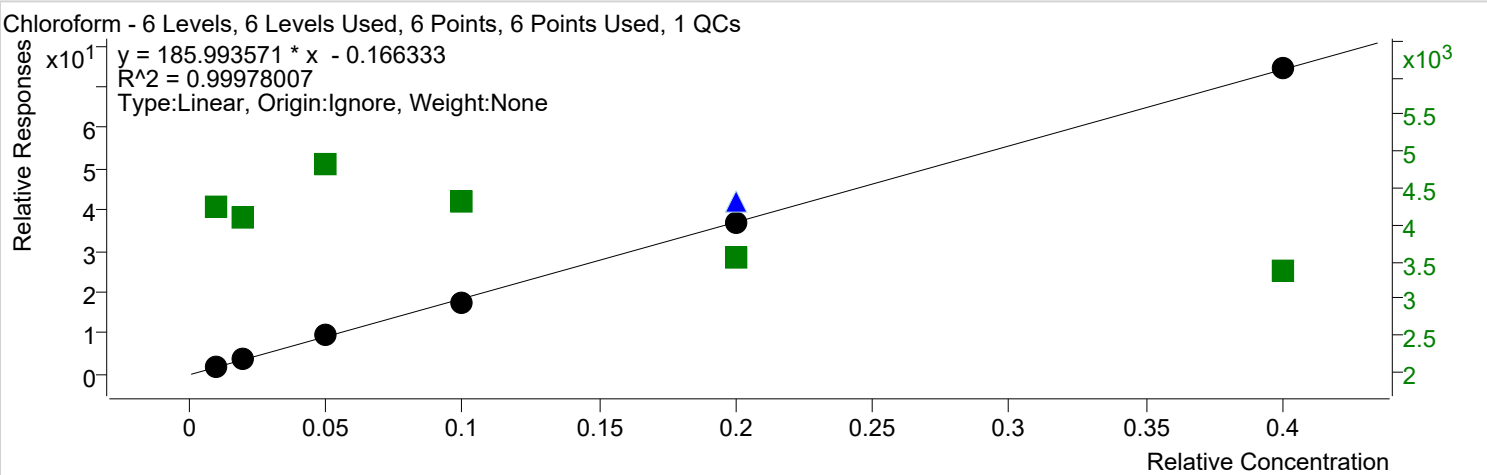

Cal. Path	Type	Level	Enable	Conc.	Response
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\VOC10 ST-01.D	Calibration	1	x	0.010	8170
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\VOC10 ST-02.D	Calibration	2	x	0.020	15381
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\VOC10 ST-03.D	Calibration	3	x	0.050	45419
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\VOC10 ST-04.D	Calibration	4	x	0.100	76475
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\VOC10 ST-05.D	Calibration	5	x	0.200	131578
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\CCV-.D	QC	5	x	0.200	119041
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\VOC10 ST-06.D	Calibration	6	x	0.400	252196

Benzene

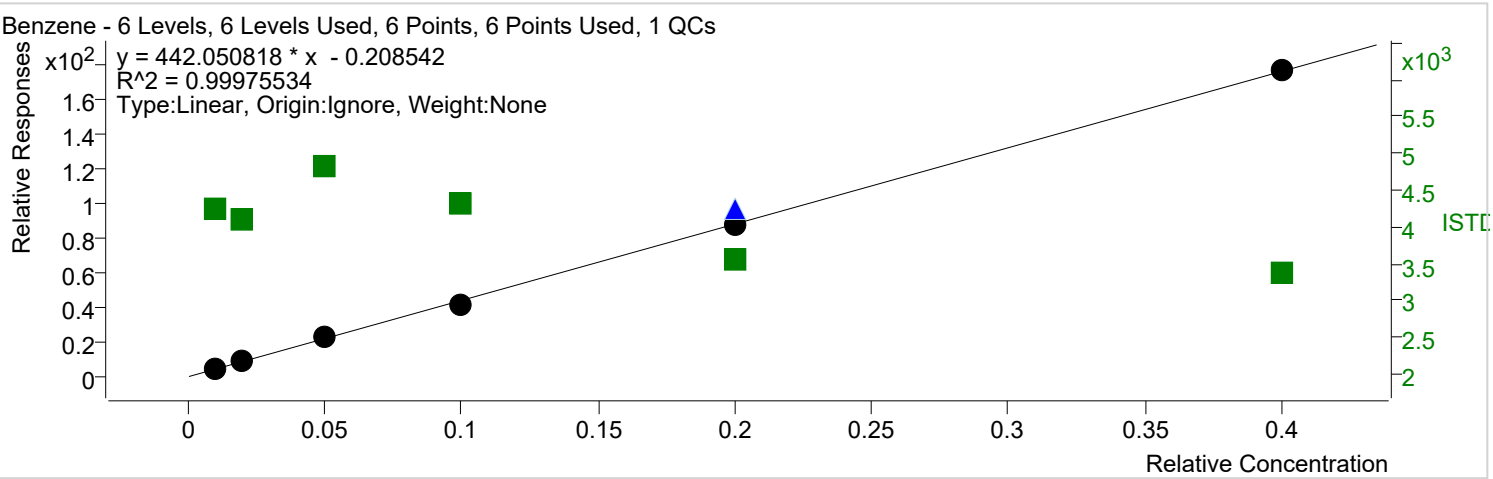

Cal. Path	Type	Level	Enable	Conc.	Response
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\VOC10 ST-01.D	Calibration	1	x	0.010	19919
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\VOC10 ST-02.D	Calibration	2	x	0.020	37557
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\VOC10 ST-03.D	Calibration	3	x	0.050	109085

Cal. Path	Type	Level	Enable	Conc.	Response
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\VOC10 ST-04.D	Calibration	4	x	0.100	181801
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\VOC10 ST-05.D	Calibration	5	x	0.200	314123
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\CCV-.D	QC	5	x	0.200	276933
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\VOC10 ST-06.D	Calibration	6	x	0.400	599803

Toluene

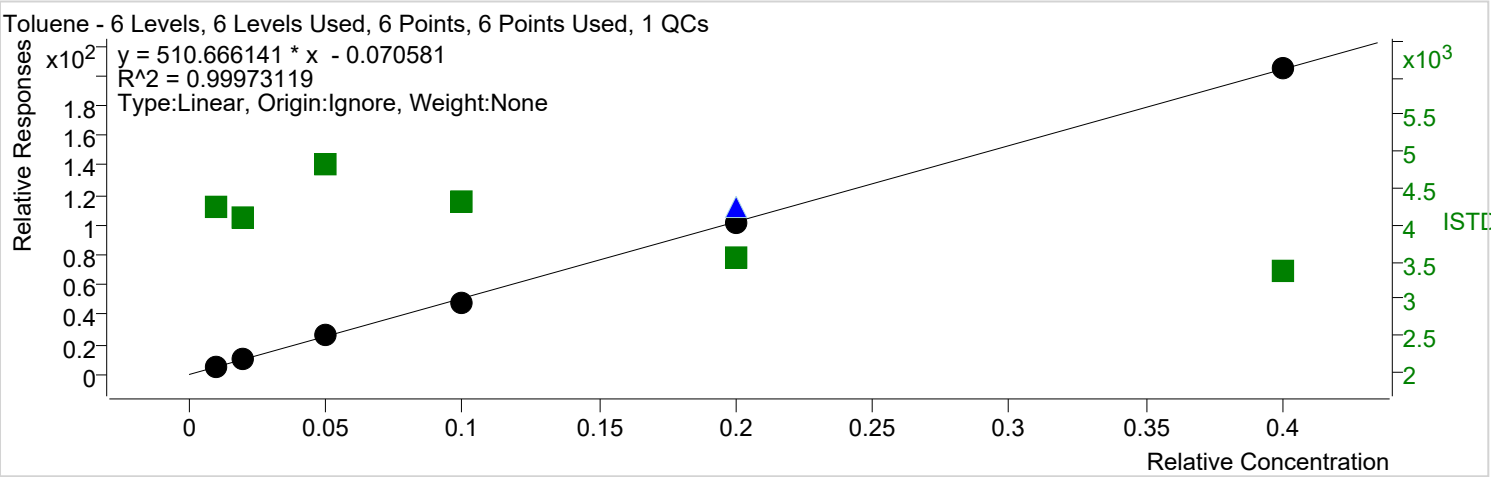

Cal. Path	Type	Level	Enable	Conc.	Response
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\VOC10 ST-01.D	Calibration	1	x	0.010	22786
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\VOC10 ST-02.D	Calibration	2	x	0.020	42932
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\VOC10 ST-03.D	Calibration	3	x	0.050	128925
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\VOC10 ST-04.D	Calibration	4	x	0.100	210383
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\VOC10 ST-05.D	Calibration	5	x	0.200	364705
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\CCV-.D	QC	5	x	0.200	315420
D:\DATA\2026년\3. 2026년 3월 \VOC10(JR 3.19 HH 3.24)\VOC10 ST-06.D	Calibration	6	x	0.400	692861

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\VOC10(JR 3.19 HH 3.24)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-03-25 오후 4:37:11	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-25 오후 4:37:11	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-25 오전 11:53:02	**Data File**	VOC10 ST-01.D
Type	Cal	**Name**	VOC10 ST-01
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

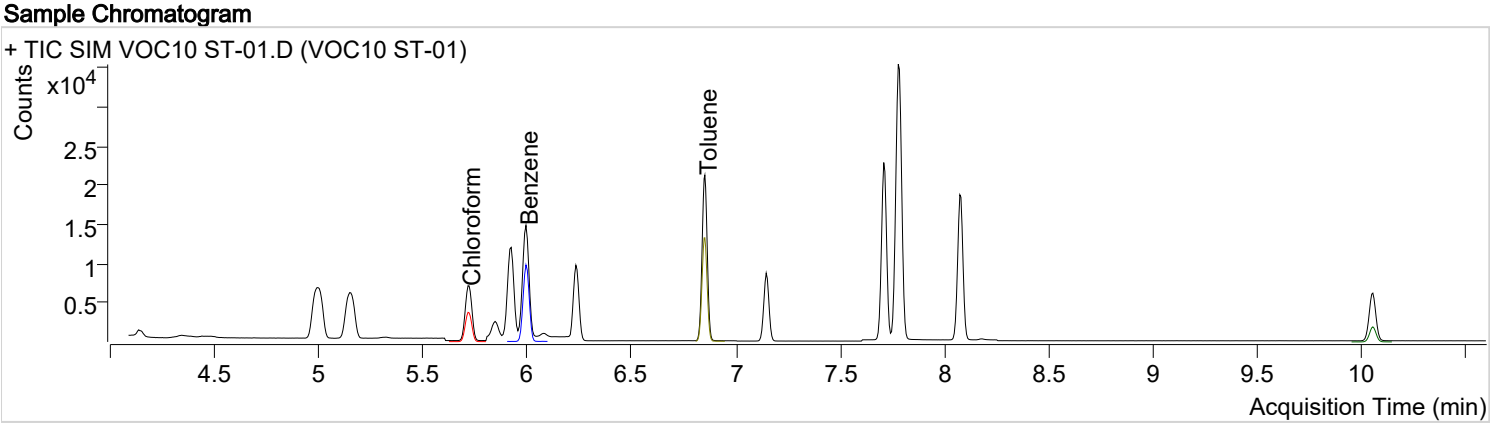

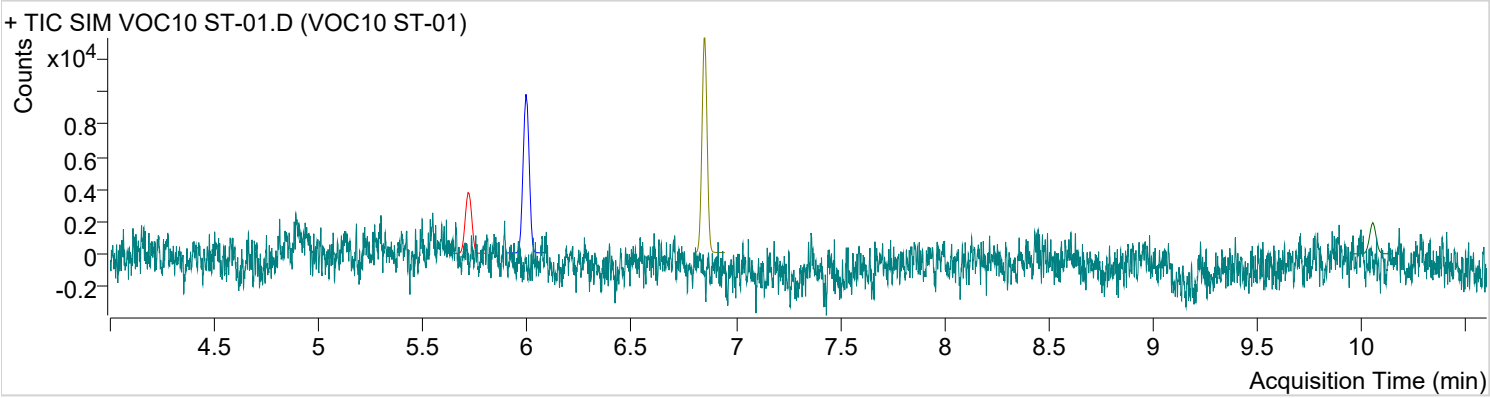

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Chloroform	5.715	8170	4240	0.011 mg/L
Benzene	5.993	19919	4240	0.011 mg/L
Toluene	6.851	22786	4240	0.011 mg/L

Chloroform



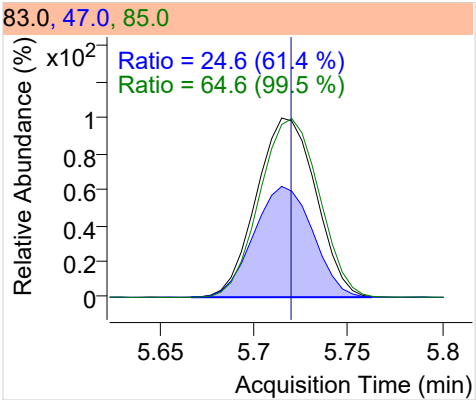

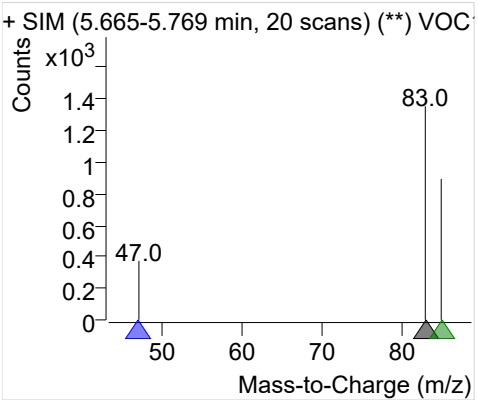

Benzene







Toluene







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\VOC10(JR 3.19 HH 3.24)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-03-25 오후 4:37:11	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-25 오후 4:37:11	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-25 오후 12:05:42	**Data File**	VOC10 ST-02.D
Type	Cal	**Name**	VOC10 ST-02
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

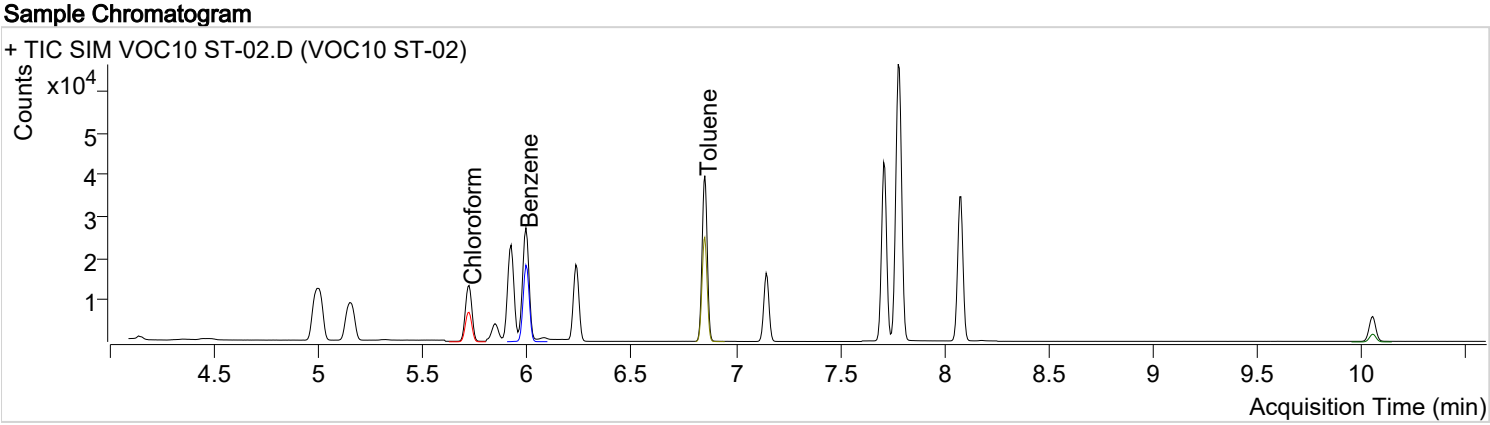

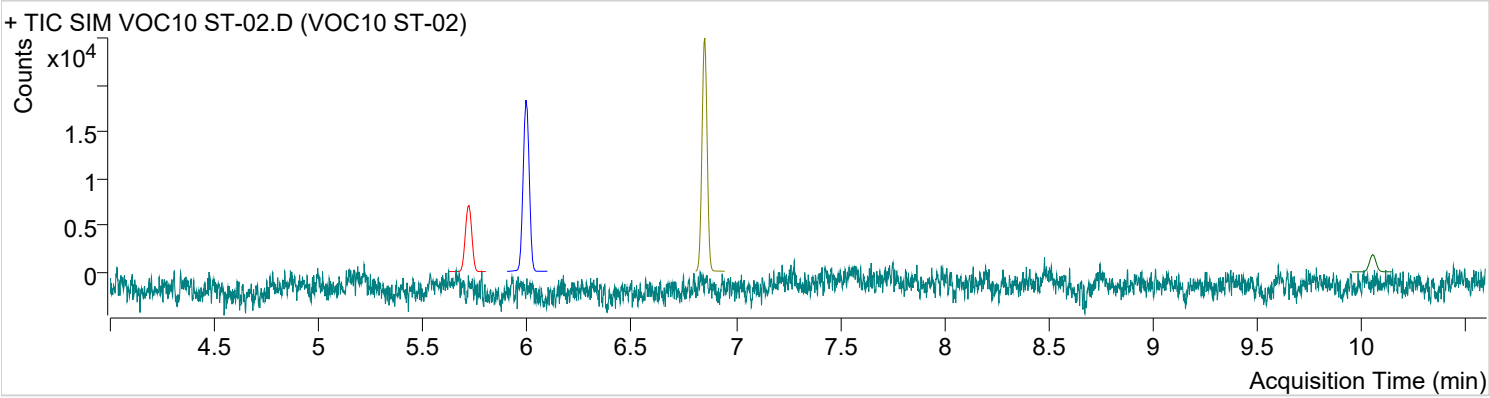

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Chloroform	5.720	15381	4116	0.021 mg/L
Benzene	5.993	37557	4116	0.021 mg/L
Toluene	6.851	42932	4116	0.021 mg/L

Chloroform



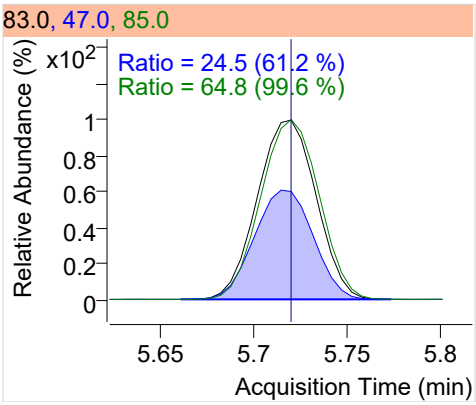

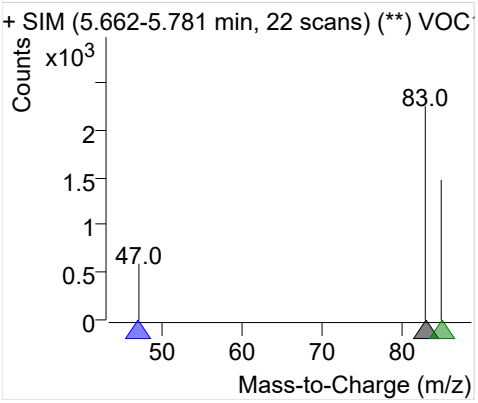

Benzene





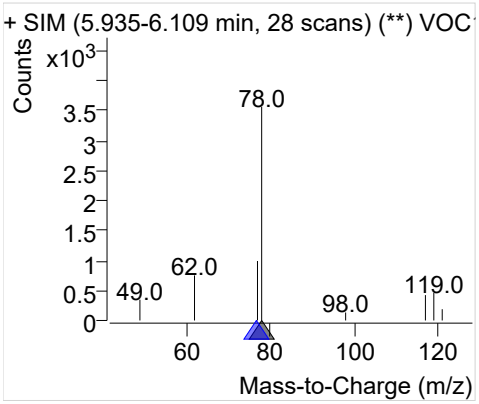

Toluene





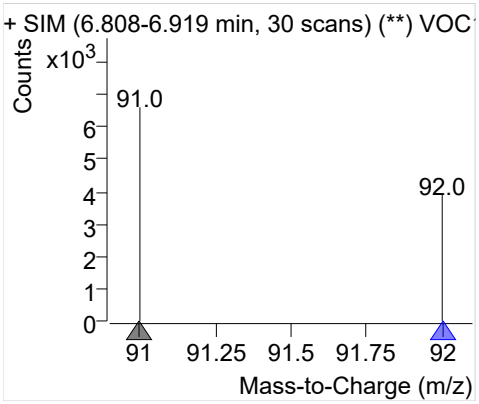

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\VOC10(JR 3.19 HH 3.24)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-03-25 오후 4:37:11	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-25 오후 4:37:11	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-25 오후 12:18:23	**Data File**	VOC10 ST-03.D
Type	Cal	**Name**	VOC10 ST-03
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

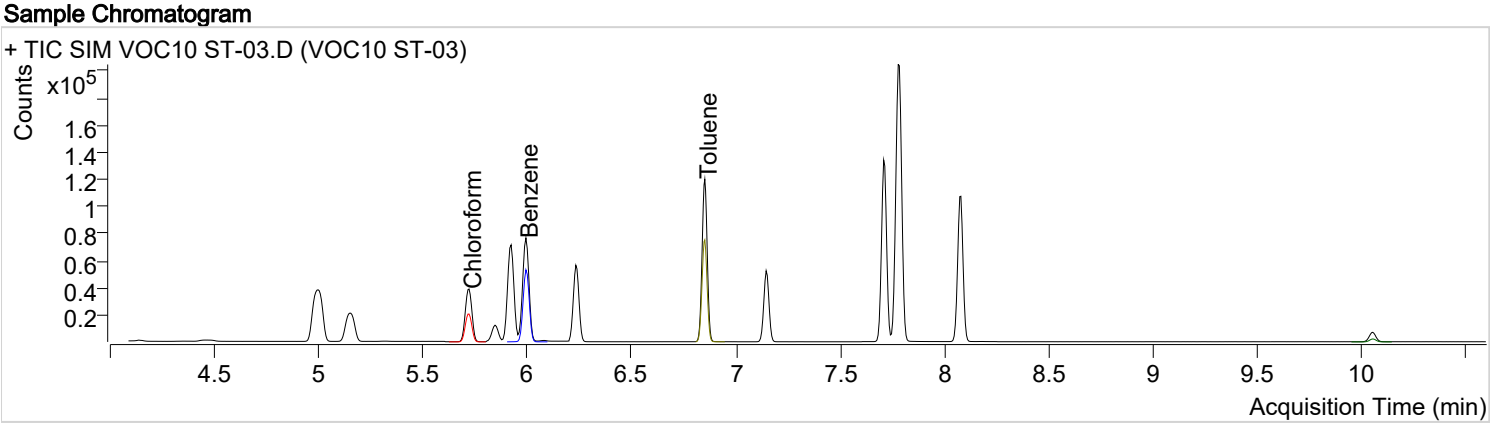

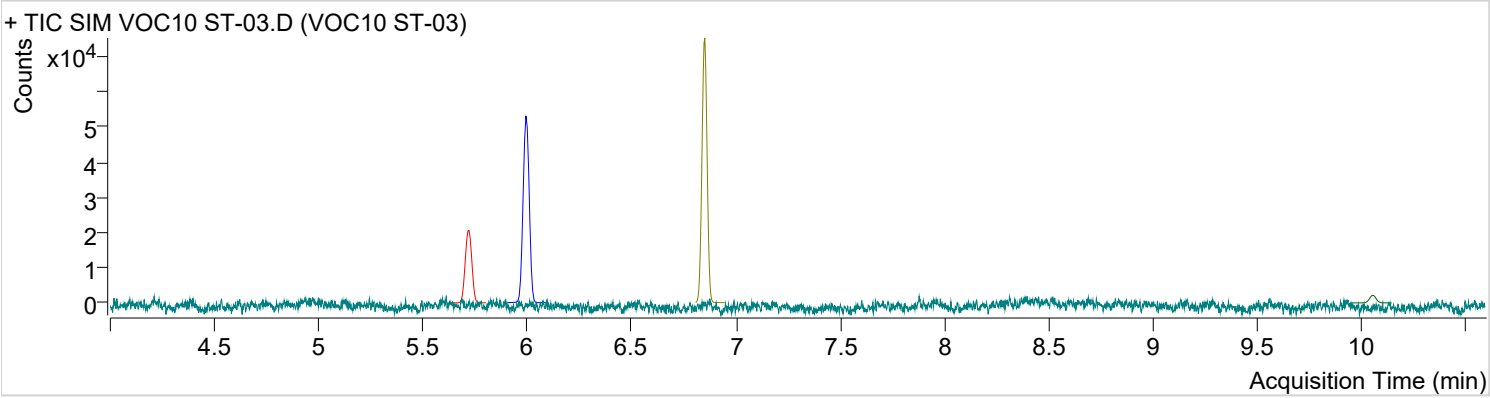

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Chloroform	5.720	45419	4816	0.052 mg/L
Benzene	5.993	109085	4816	0.052 mg/L
Toluene	6.851	128925	4816	0.053 mg/L

Chloroform



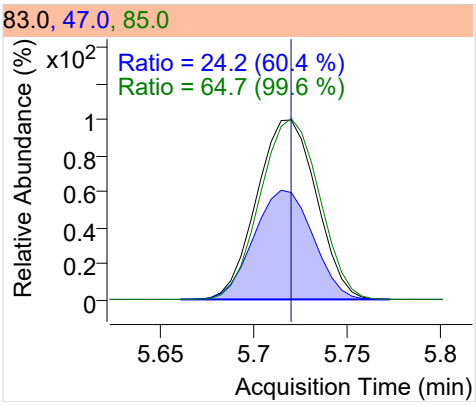

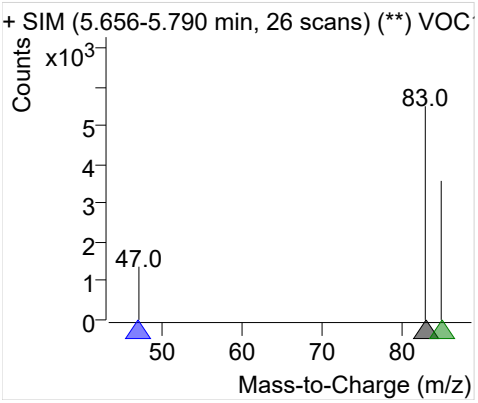

Benzene







Toluene







Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\VOC10(JR 3.19 HH 3.24)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-03-25 오후 4:37:11	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-25 오후 4:37:11	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-25 오후 12:31:03	**Data File**	VOC10 ST-04.D
Type	Cal	**Name**	VOC10 ST-04
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

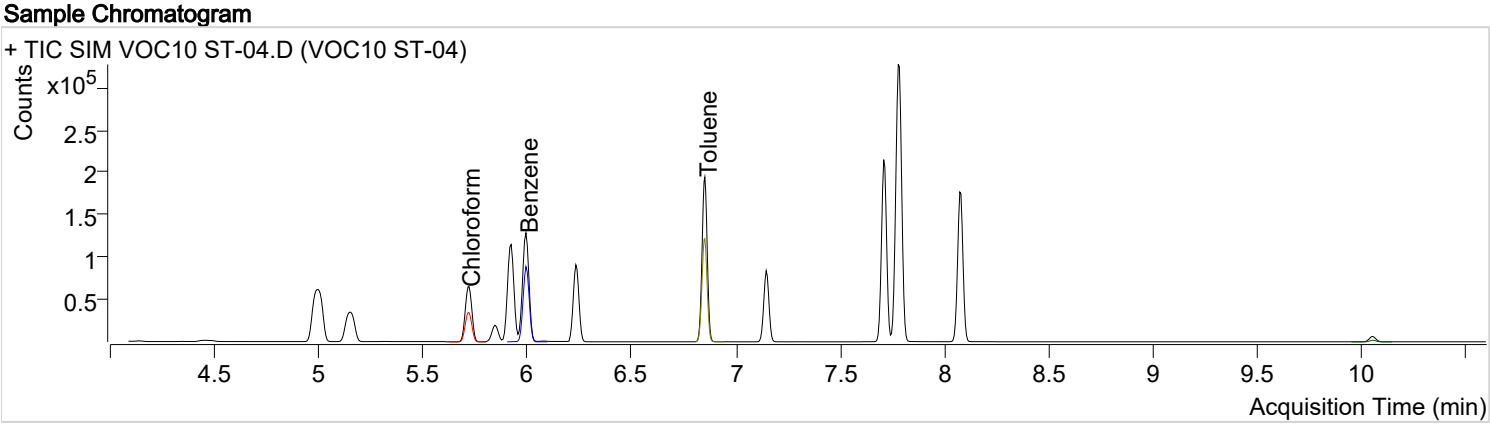

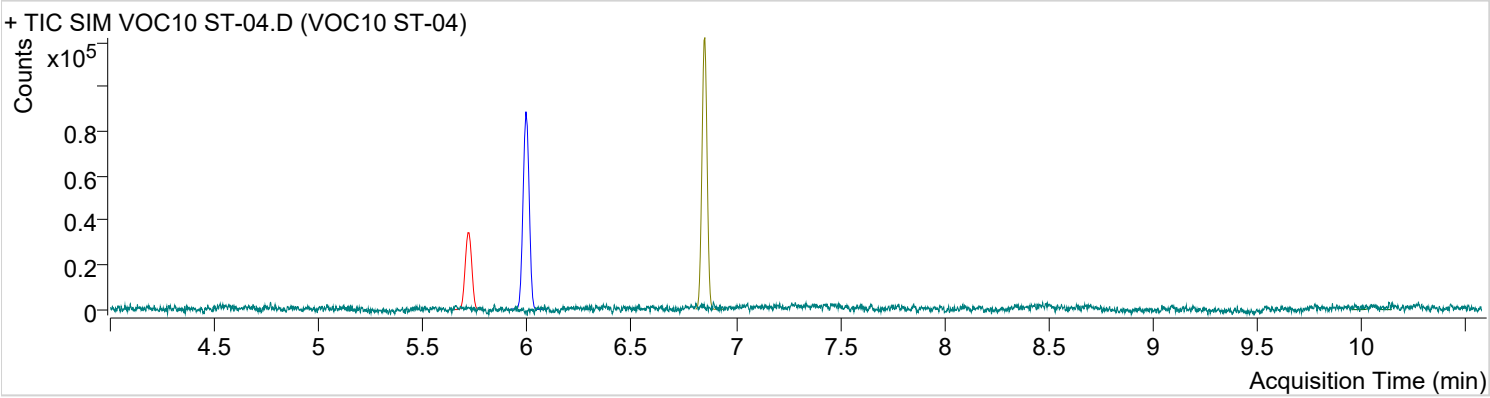

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Chloroform	5.715	76475	4329	0.096 mg/L
Benzene	5.993	181801	4329	0.095 mg/L
Toluene	6.851	210383	4329	0.095 mg/L

Chloroform



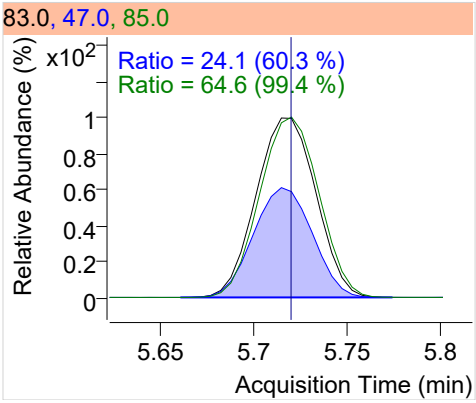

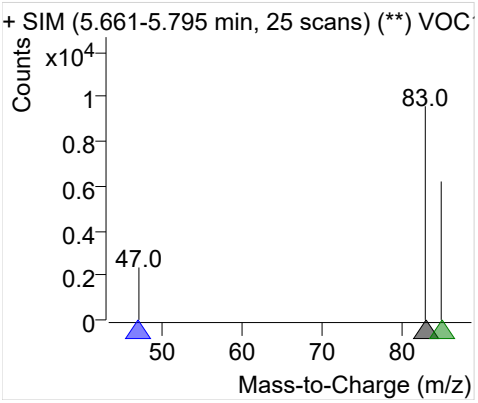

Benzene

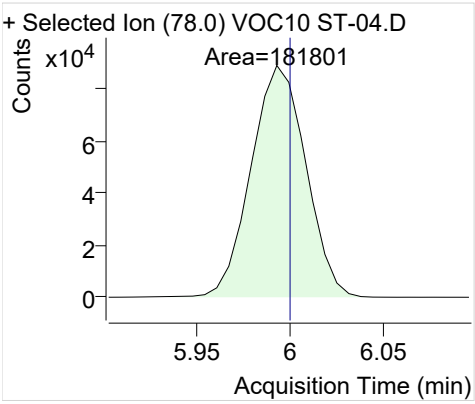





Toluene

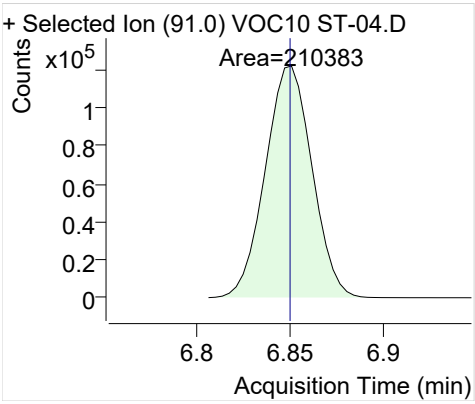





Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\VOC10(JR 3.19 HH 3.24)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-03-25 오후 4:37:11	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-25 오후 4:37:11	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-25 오후 12:43:55	**Data File**	VOC10 ST-05.D
Type	Cal	**Name**	VOC10 ST-05
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

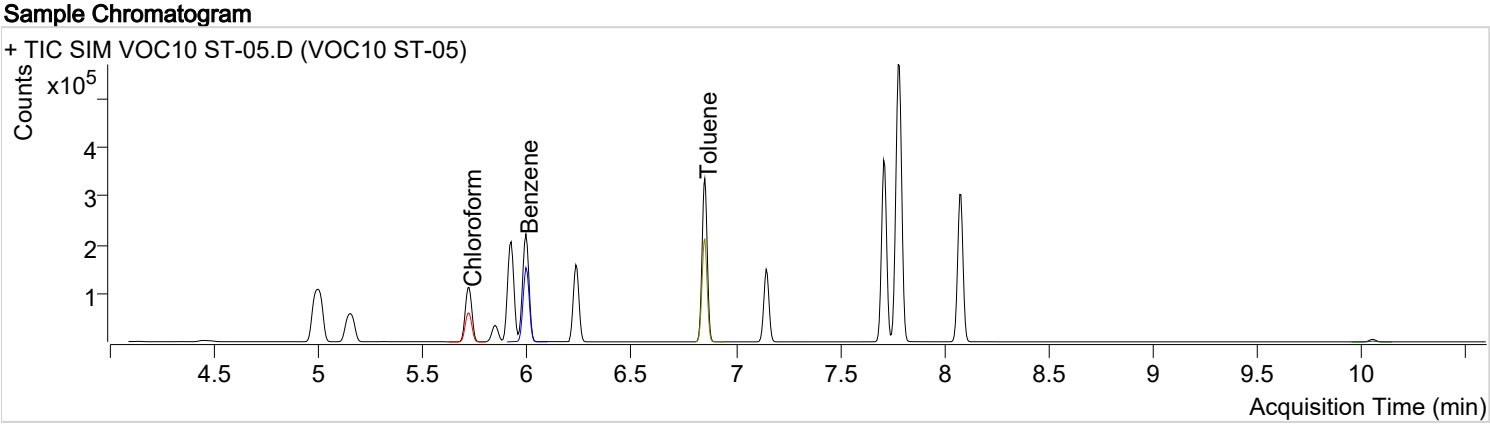

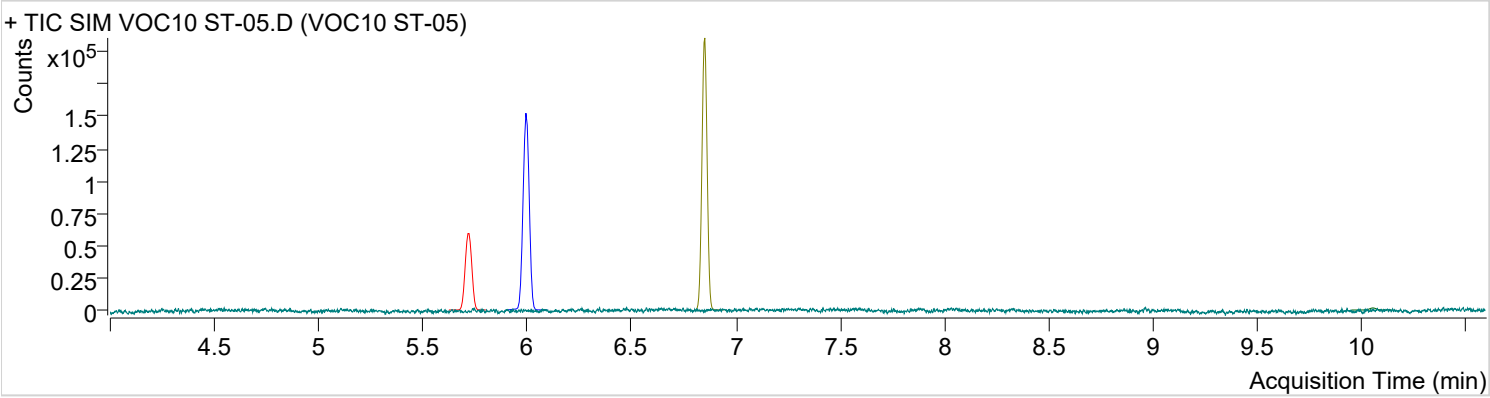

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Chloroform	5.720	131578	3570	0.199 mg/L
Benzene	5.993	314123	3570	0.200 mg/L
Toluene	6.851	364705	3570	0.200 mg/L

Chloroform



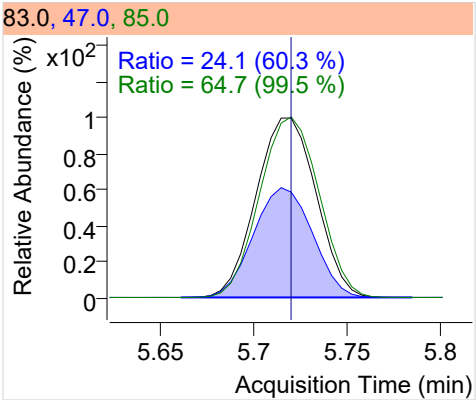

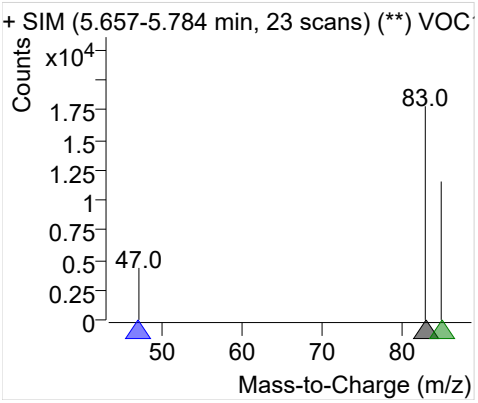

Benzene





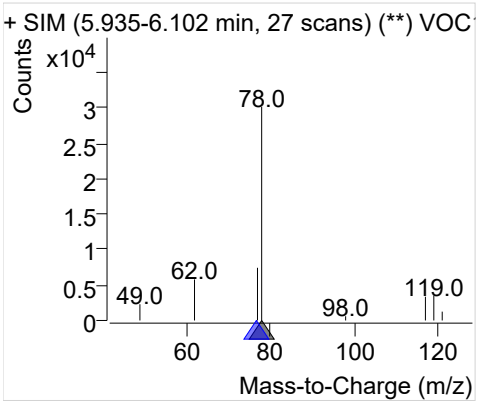

Toluene





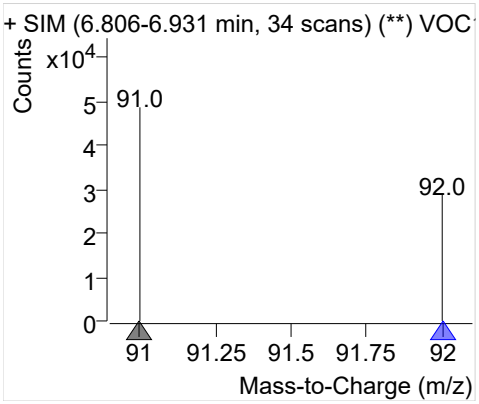

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\VOC10(JR 3.19 HH 3.24)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-03-25 오후 4:37:11	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-25 오후 4:37:11	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-25 오후 12:56:37	**Data File**	VOC10 ST-06.D
Type	Cal	**Name**	VOC10 ST-06
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

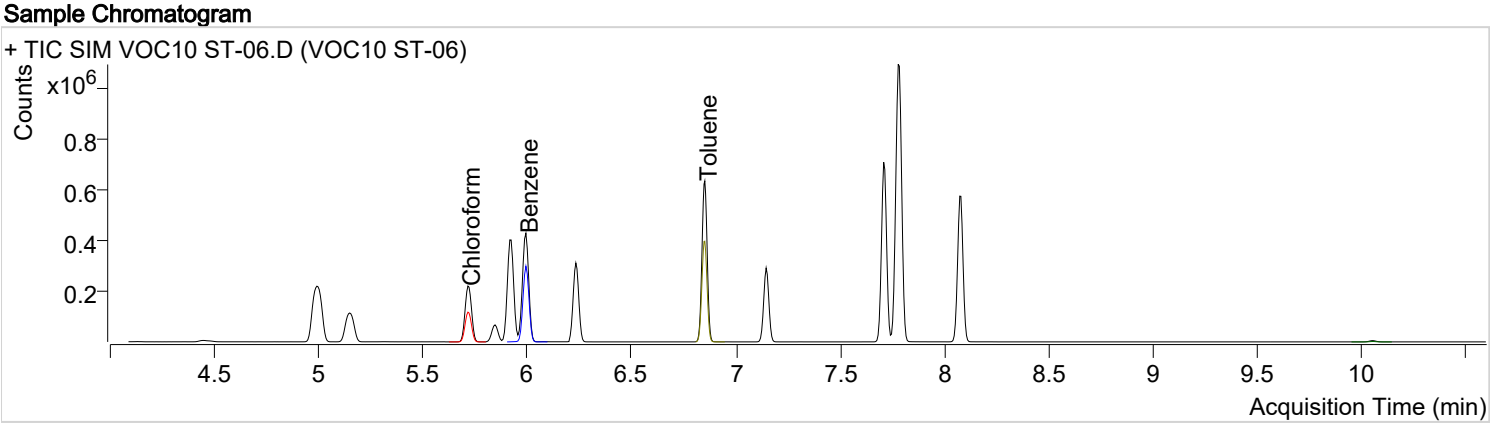

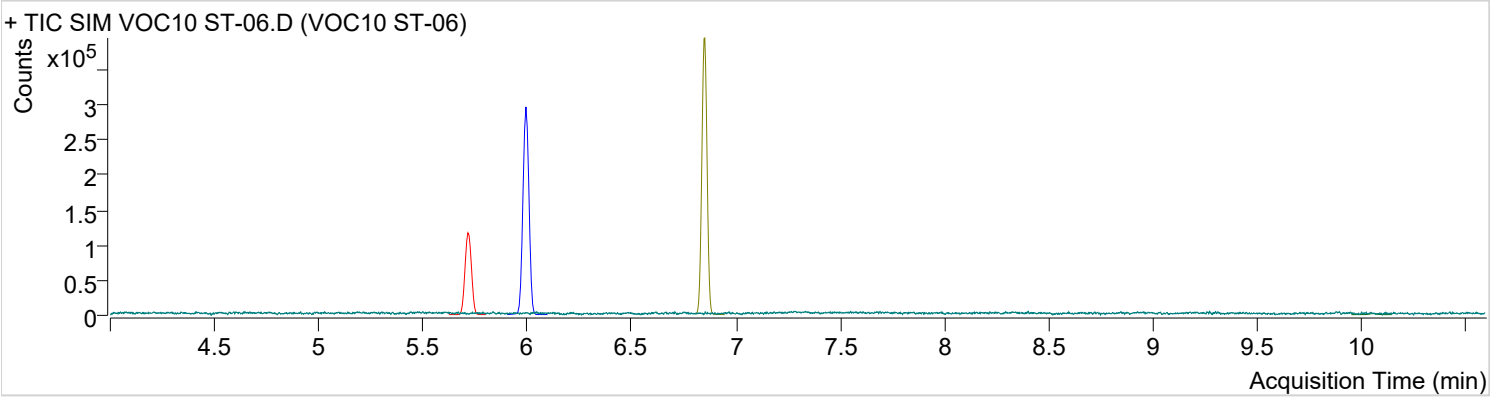

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Chloroform	5.715	252196	3387	0.401 mg/L
Benzene	5.993	599803	3387	0.401 mg/L
Toluene	6.851	692861	3387	0.401 mg/L

Chloroform



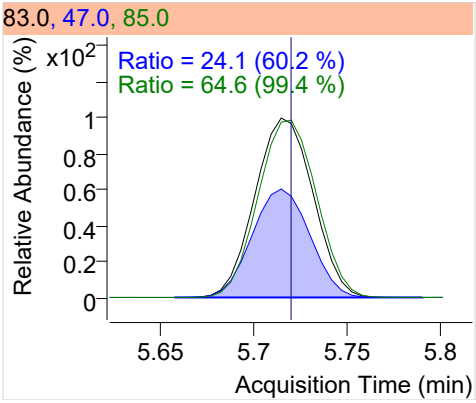

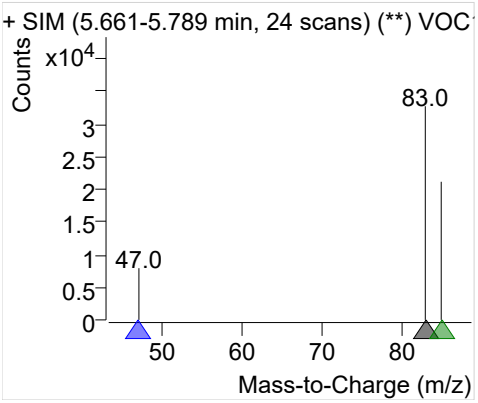

Benzene

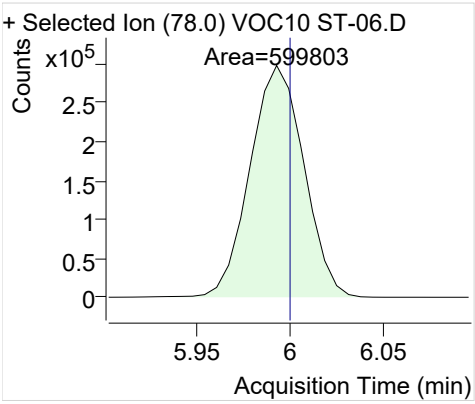





Toluene

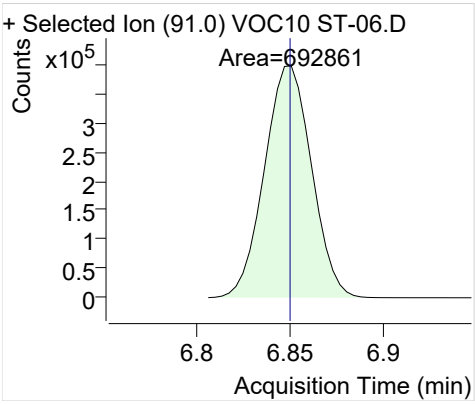





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\VOC10(JR 3.19 HH 3.24)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-03-25 오후 4:37:11	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-25 오후 4:37:11	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-25 오후 1:22:07	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

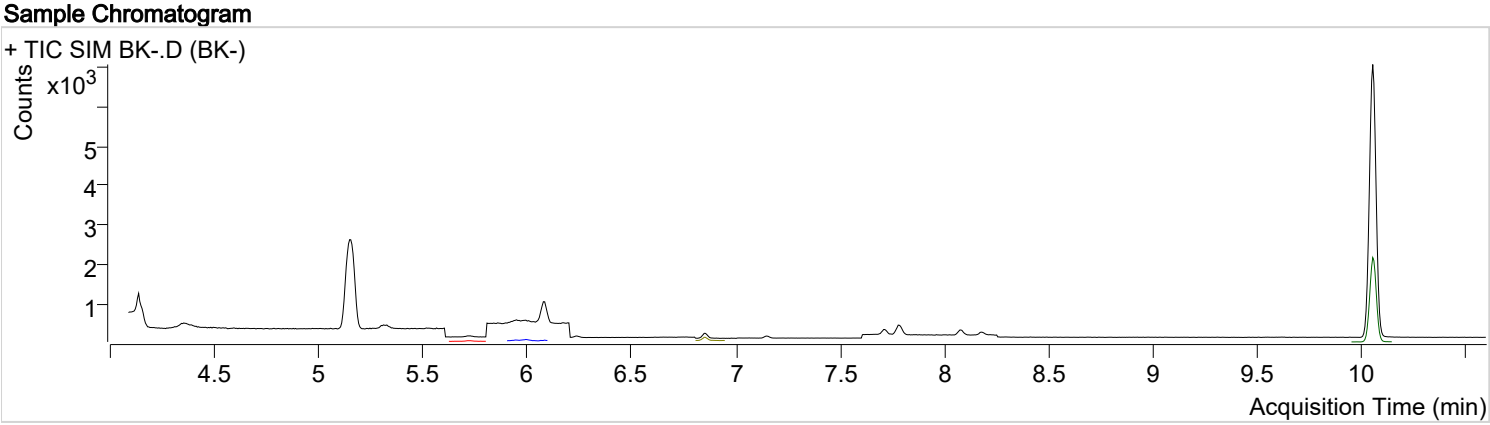

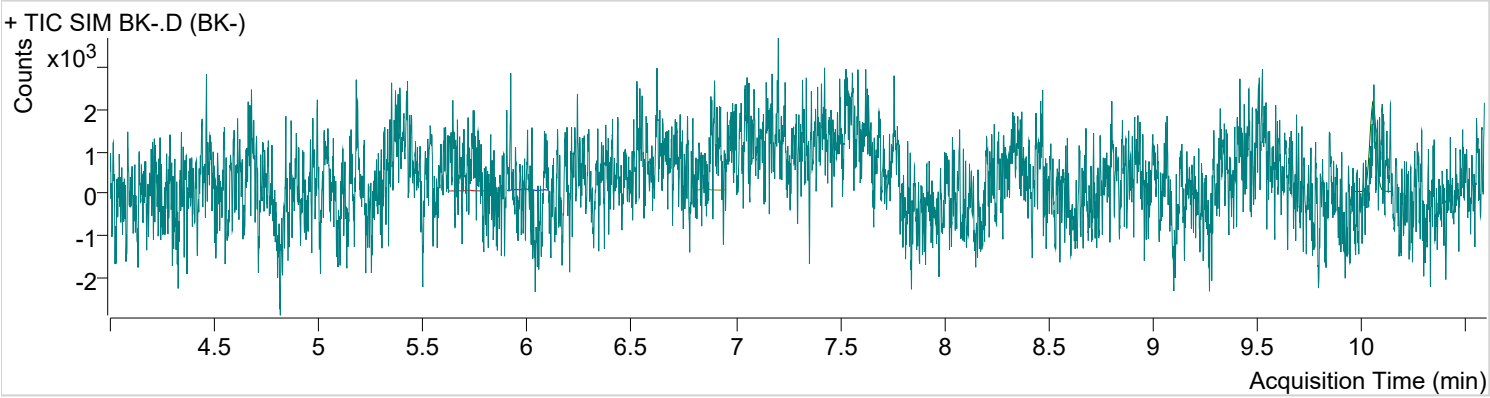

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Chloroform			4756	ND mg/L
Benzene			4756	ND mg/L
Toluene			4756	ND mg/L

Chloroform



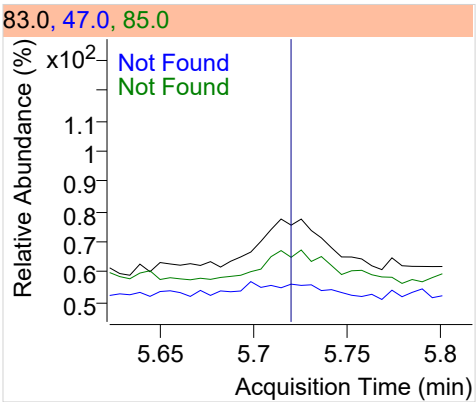

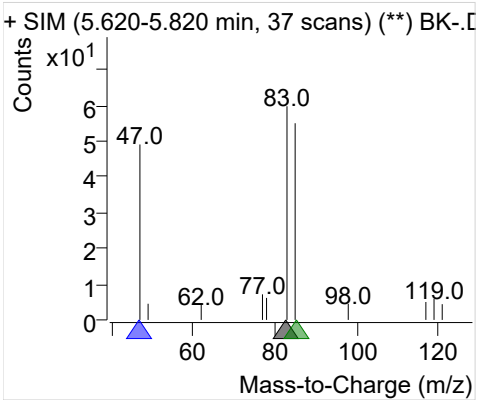

Benzene



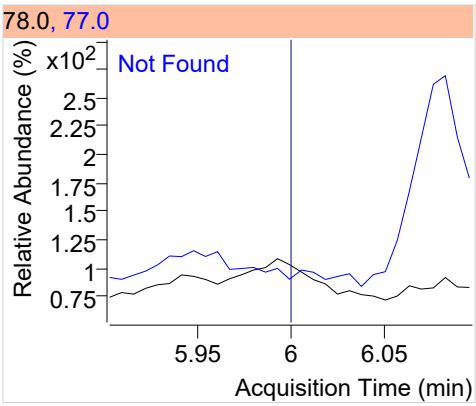



Toluene

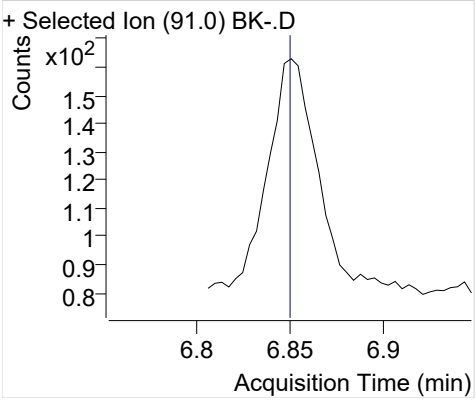



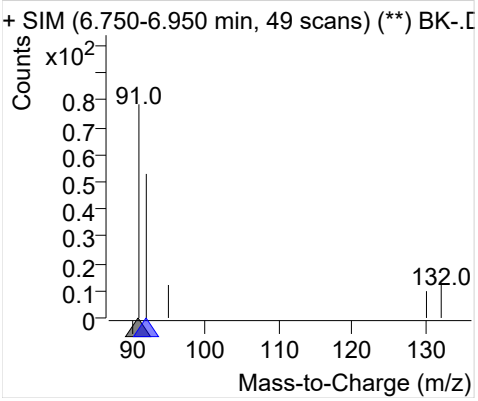

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\VOC10(JR 3.19 HH 3.24)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-03-25 오후 4:37:11	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-25 오후 4:37:11	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-25 오후 1:34:46	**Data File**	FBK(HH 26-03-24).D
Type	Blank	**Name**	FBK(HH 26-03-24)
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

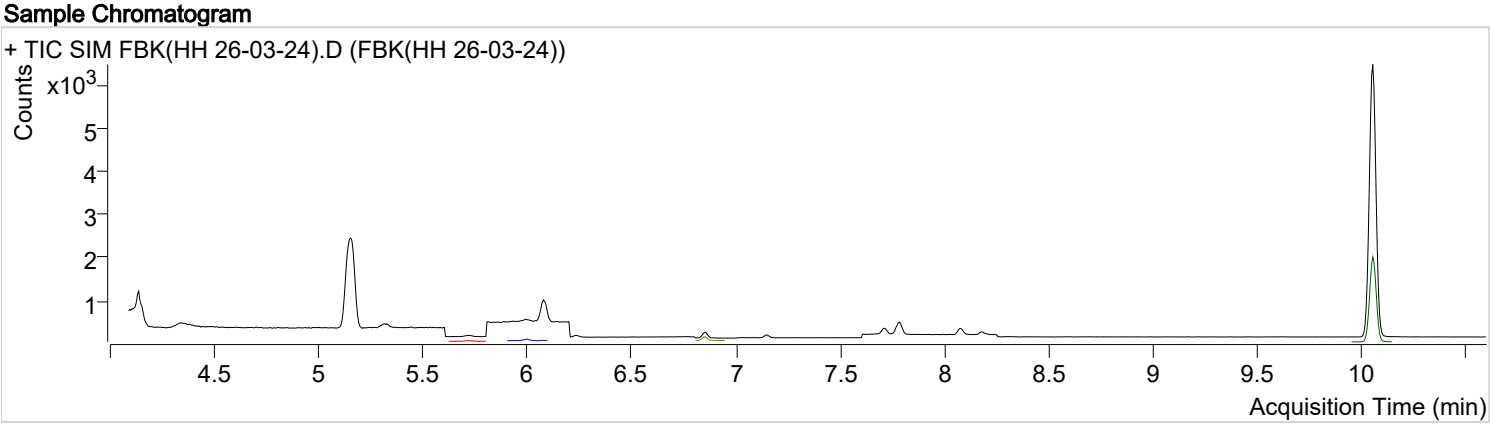

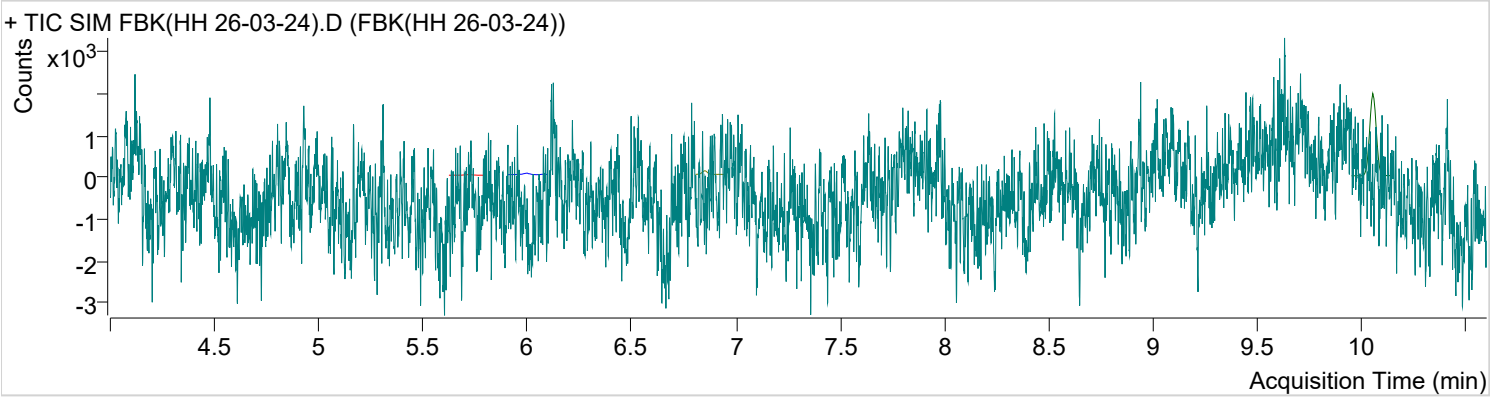

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Chloroform			4388	ND mg/L
Benzene			4388	ND mg/L
Toluene			4388	ND mg/L

Chloroform



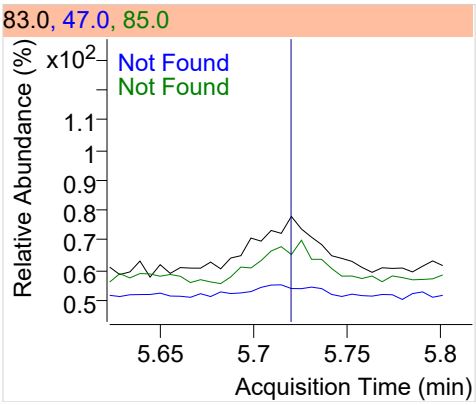

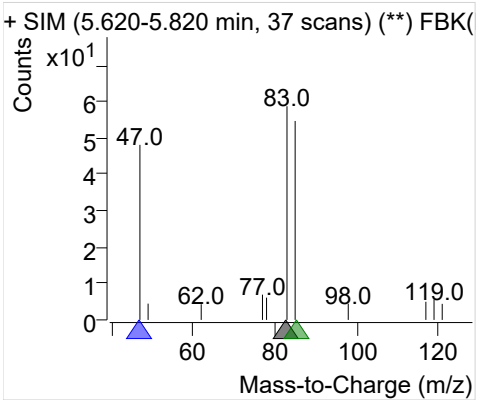

Benzene







Toluene







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\VOC10(JR 3.19 HH 3.24)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-03-25 오후 4:37:11	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-25 오후 4:37:11	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-25 오후 1:47:27	**Data File**	JR 26-03-19.D
Type	Sample	**Name**	JR 26-03-19
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

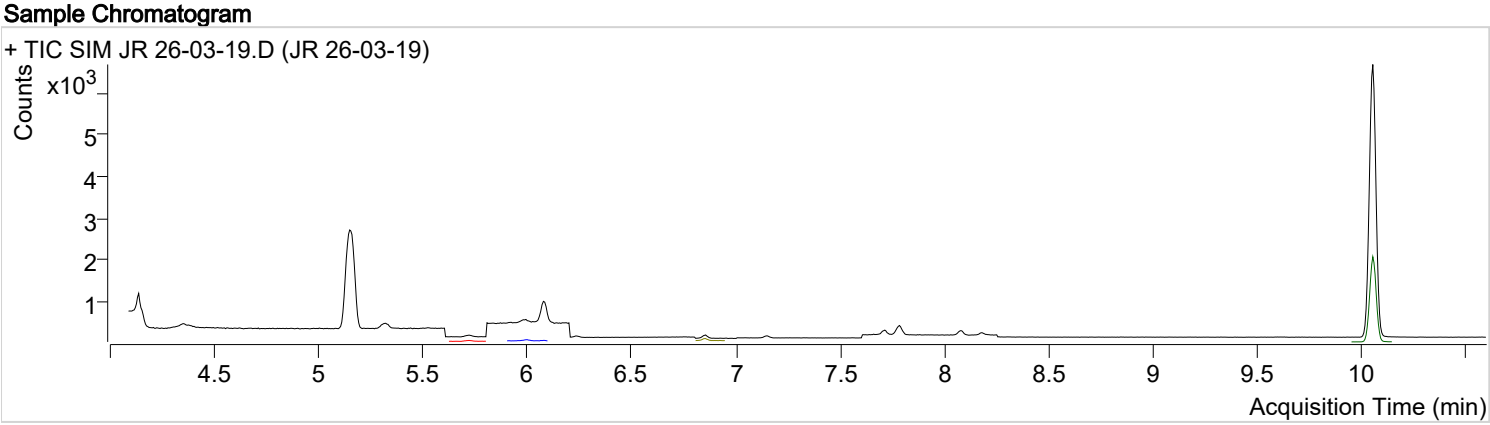

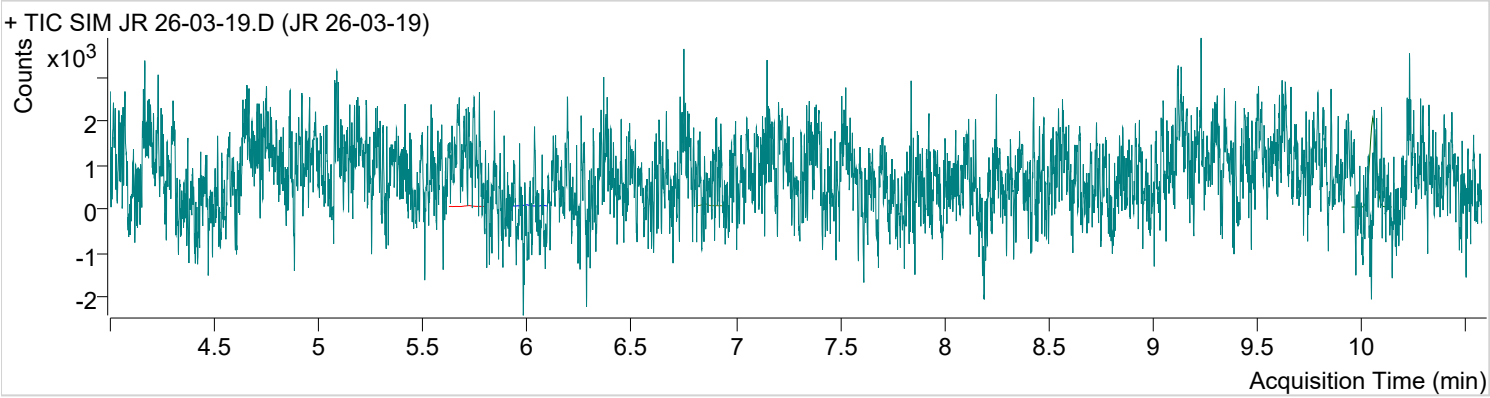

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Chloroform			4503	ND mg/L
Benzene			4503	ND mg/L
Toluene			4503	ND mg/L

Chloroform



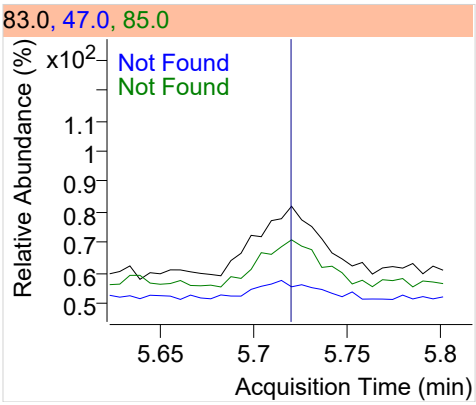

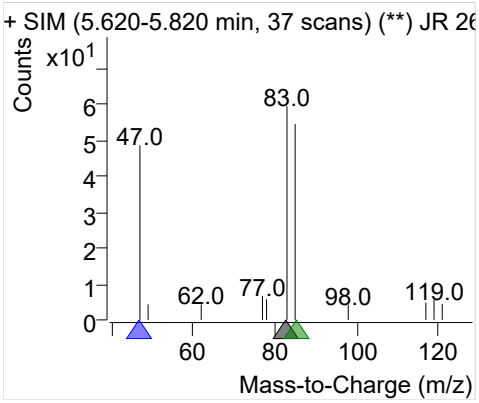

Benzene



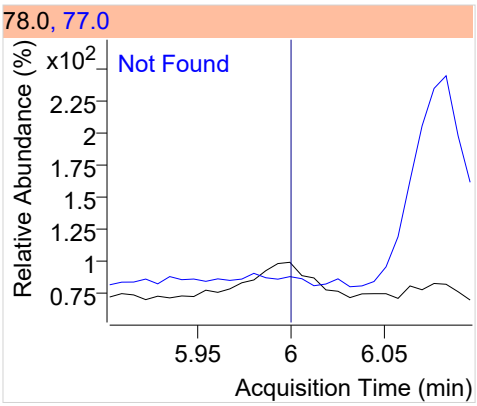



Toluene







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\VOC10(JR 3.19 HH 3.24)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-03-25 오후 4:37:11	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-25 오후 4:37:11	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-25 오후 2:25:31	**Data File**	HH-03.D
Type	Sample	**Name**	HH-03
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

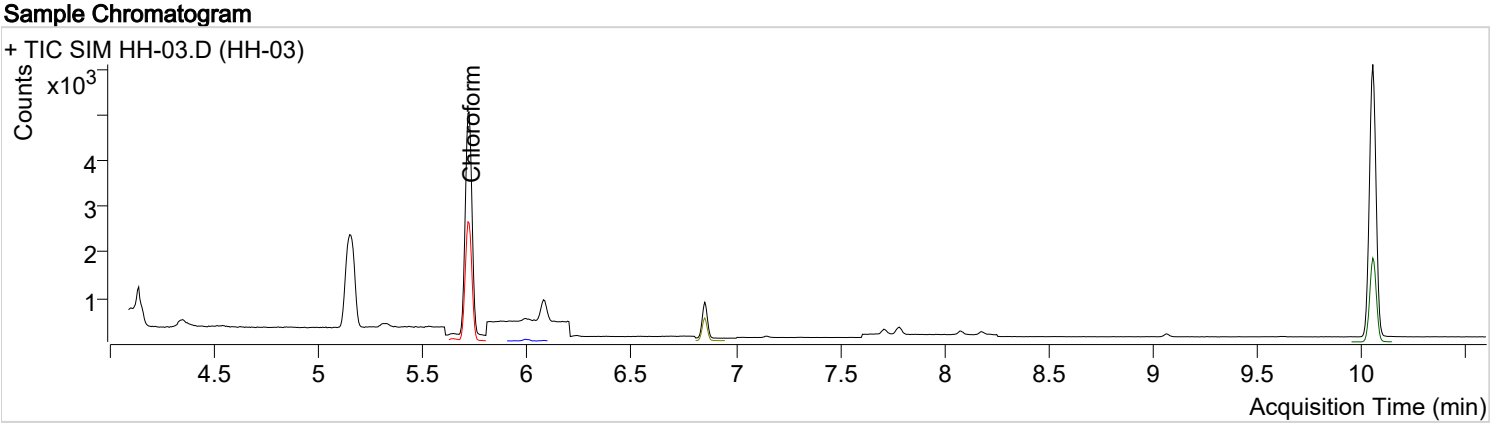

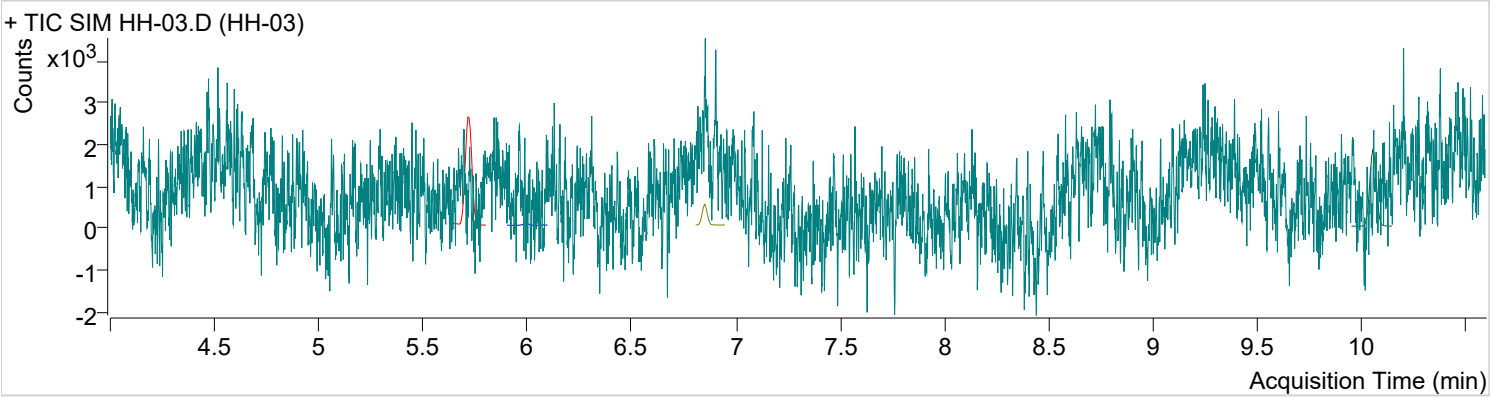

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Chloroform	5.715	5664	4074	0.008 mg/L
Benzene			4074	ND mg/L
Toluene			4074	ND mg/L

Chloroform



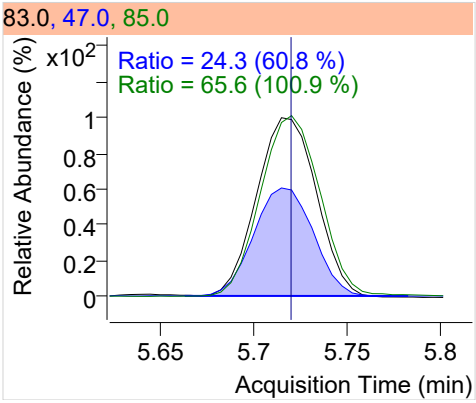

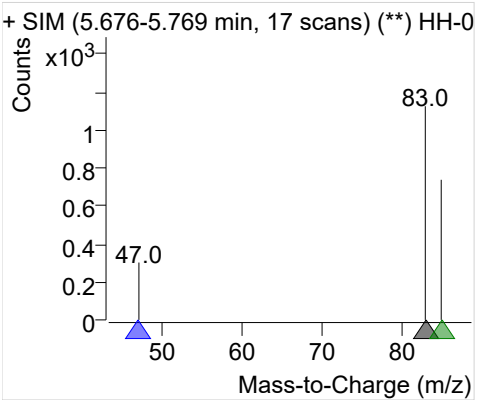

Benzene



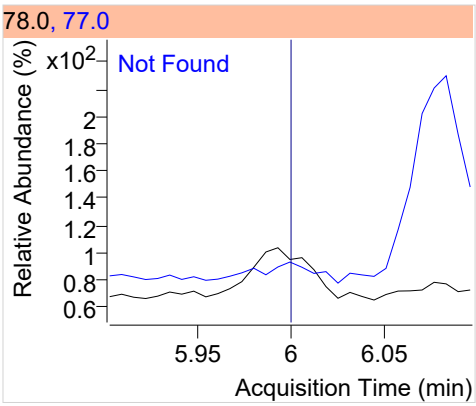



Toluene







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\VOC10(JR 3.19 HH 3.24)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-03-25 오후 4:37:11	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-25 오후 4:37:11	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-25 오후 2:38:12	**Data File**	HH-04.D
Type	Sample	**Name**	HH-04
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

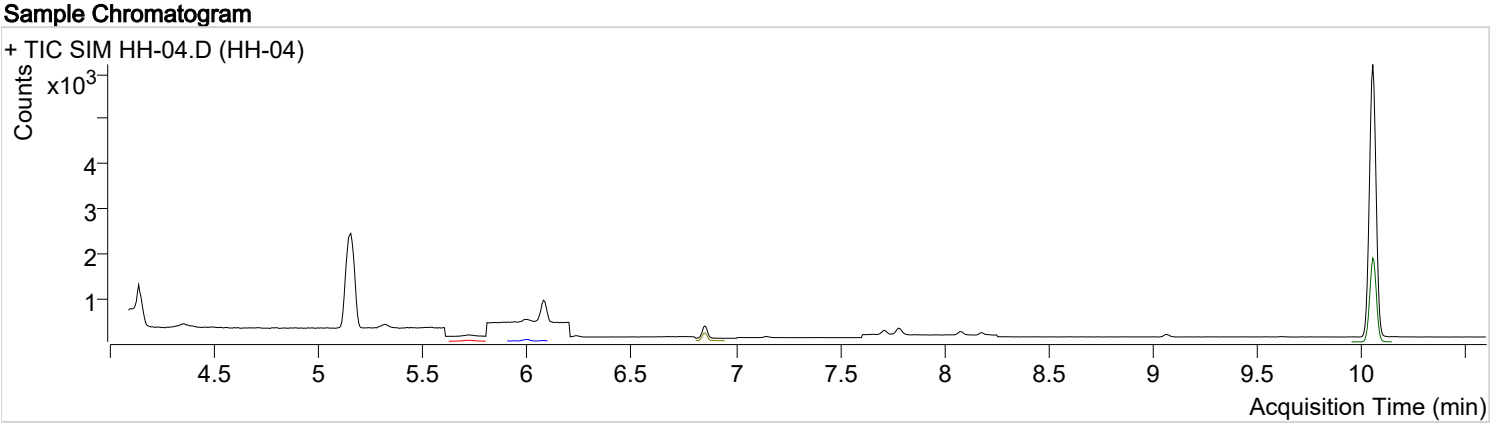

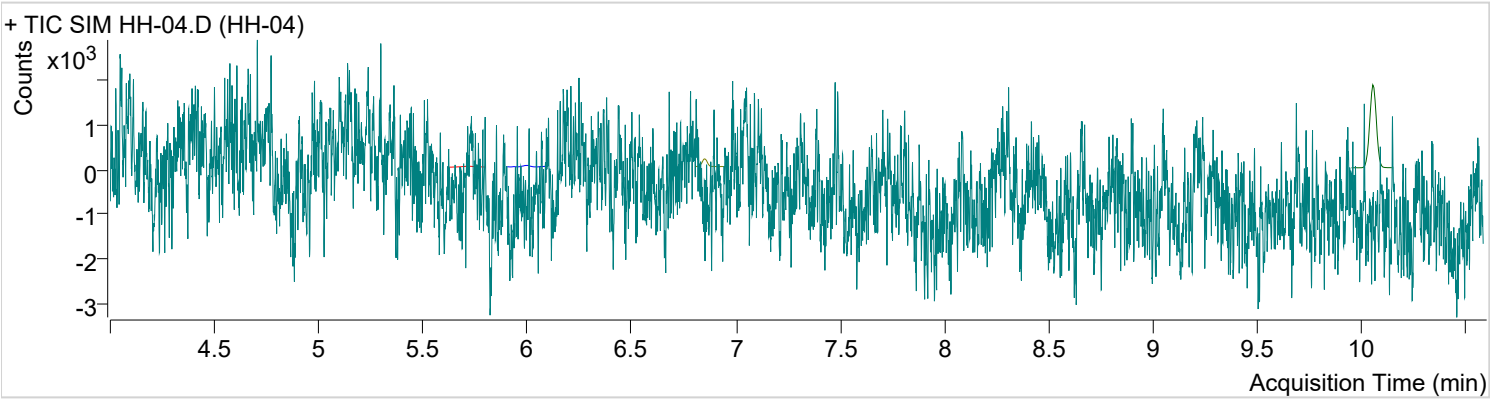

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Chloroform			4157	ND mg/L
Benzene			4157	ND mg/L
Toluene			4157	ND mg/L

Chloroform



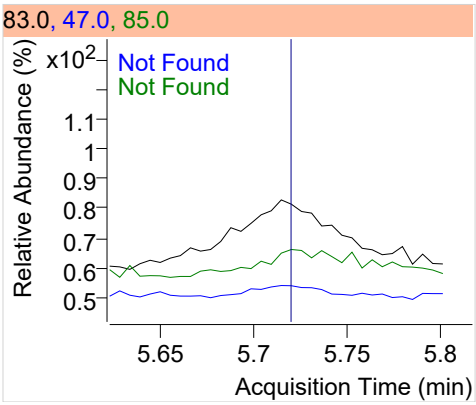

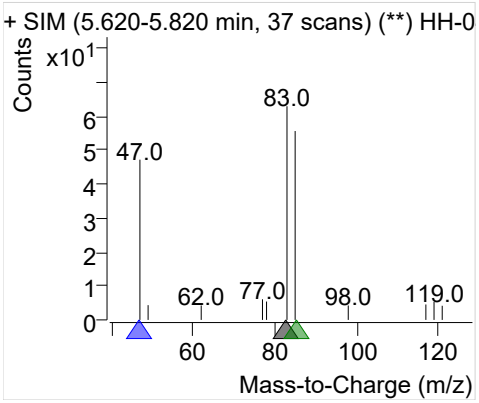

Benzene



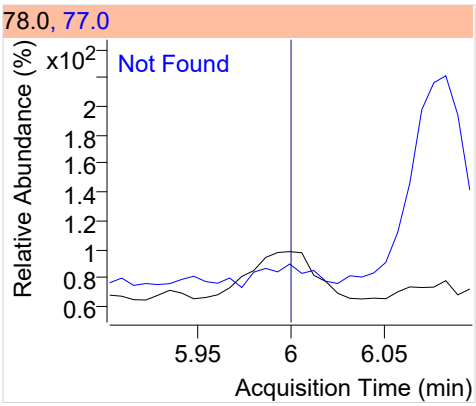



Toluene







Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\VOC10(JR 3.19 HH 3.24)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-03-25 오후 4:37:11	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-25 오후 4:37:11	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-25 오후 2:50:55	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

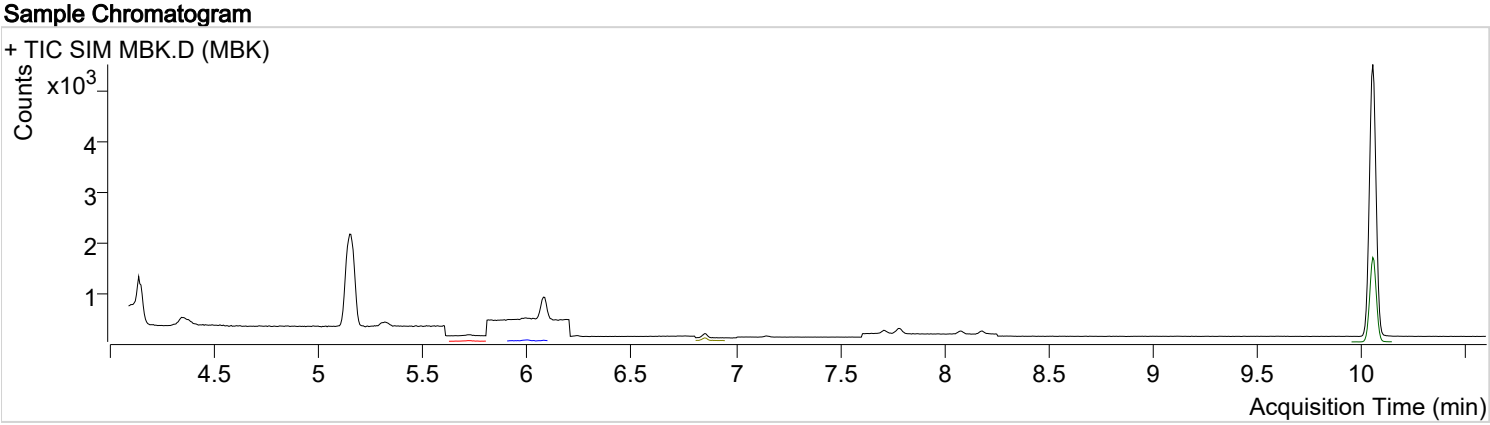

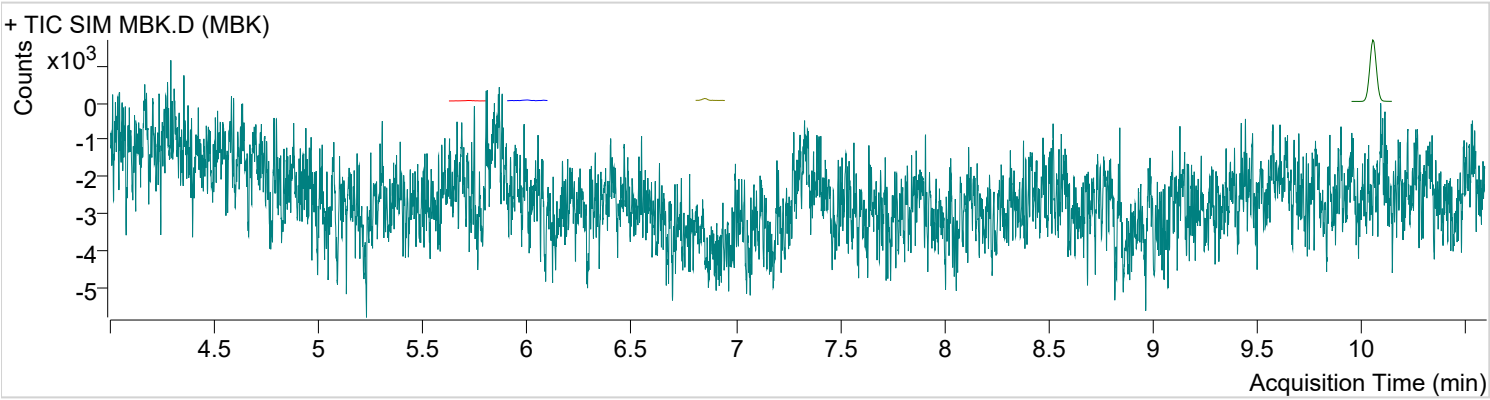

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Chloroform			3709	ND mg/L
Benzene			3709	ND mg/L
Toluene			3709	ND mg/L

Chloroform



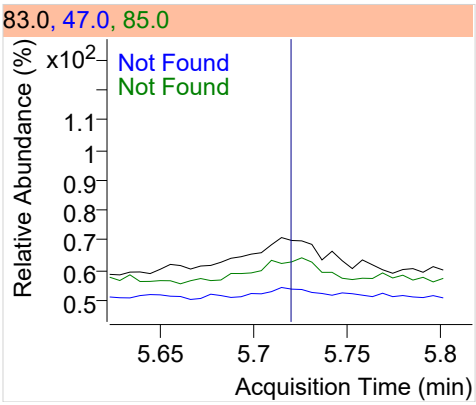

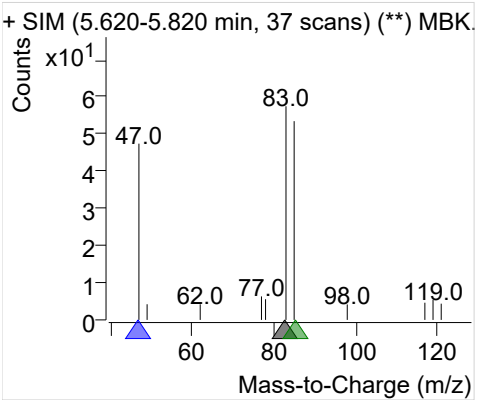

Benzene



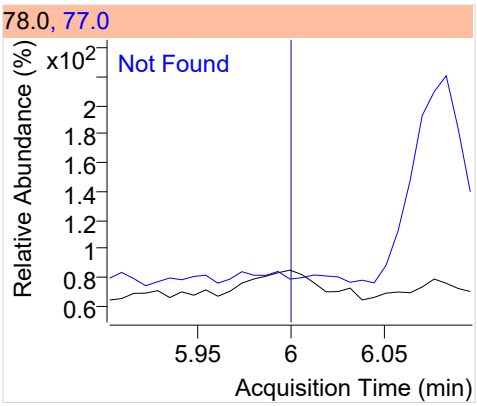



Toluene







Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\VOC10(JR 3.19 HH 3.24)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-03-25 오후 4:37:11	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-25 오후 4:37:11	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-25 오후 3:16:18	**Data File**	CCV-.D
Type	QC	**Name**	CCV-
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

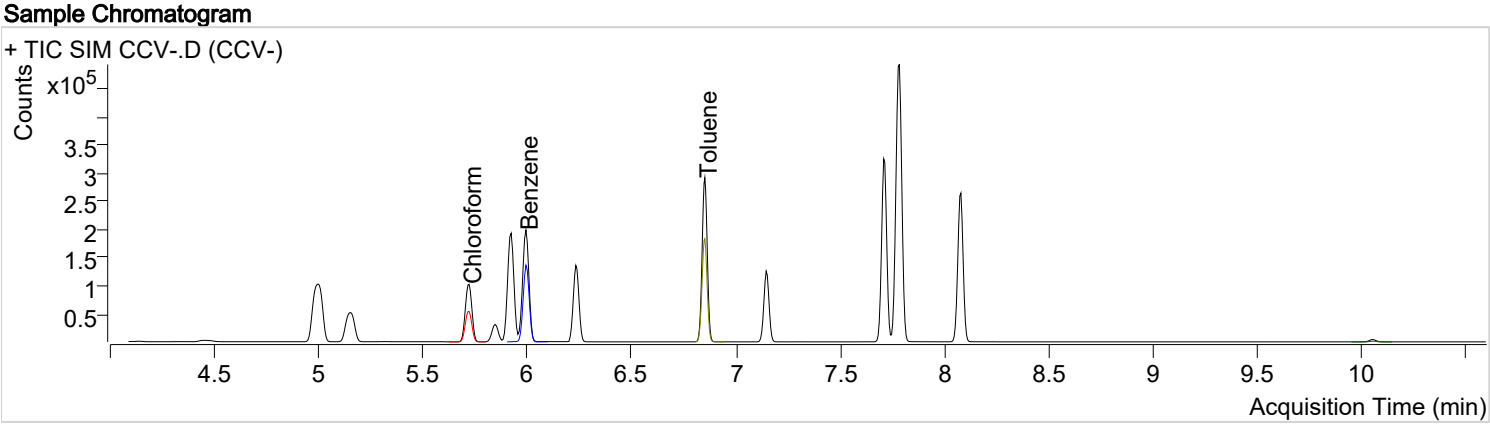

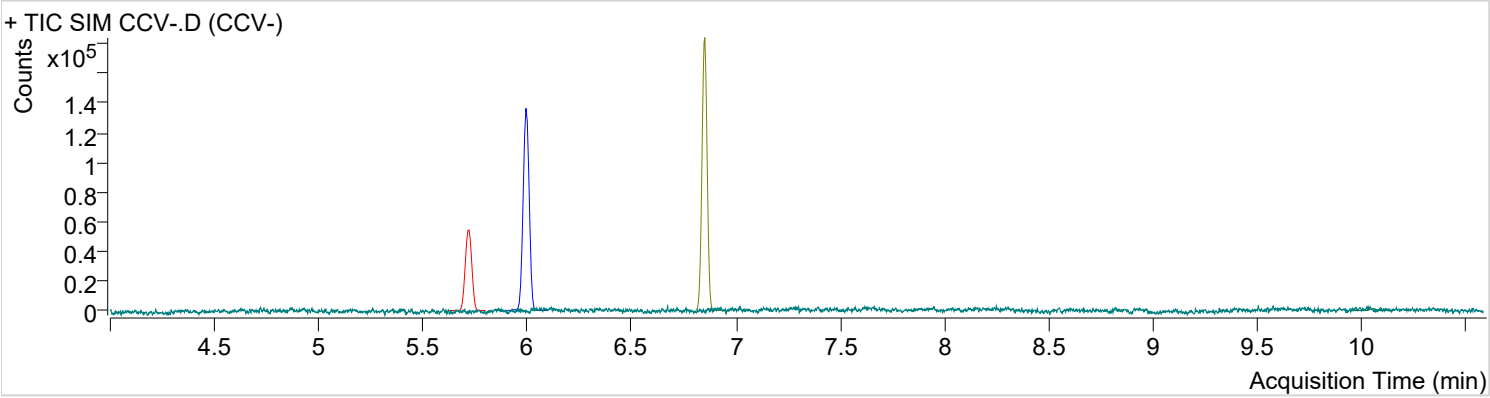

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Chloroform	5.720	119041	2836	0.227 mg/L
Benzene	5.993	276933	2836	0.221 mg/L
Toluene	6.851	315420	2836	0.218 mg/L

Chloroform



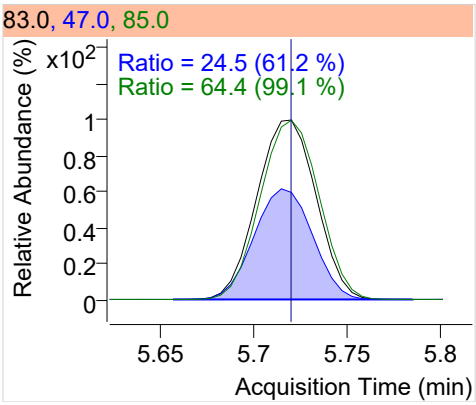

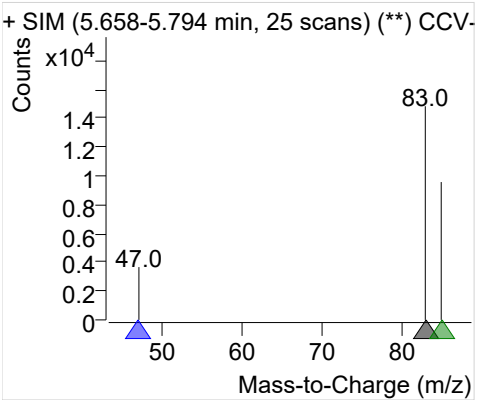

Benzene





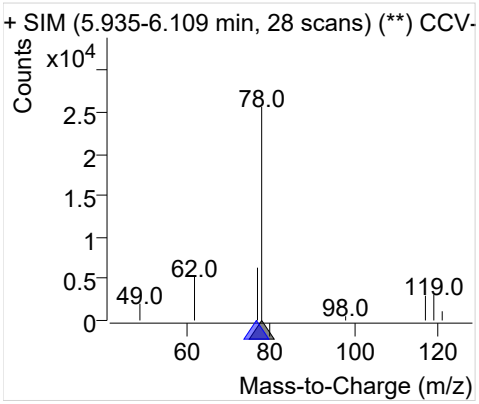
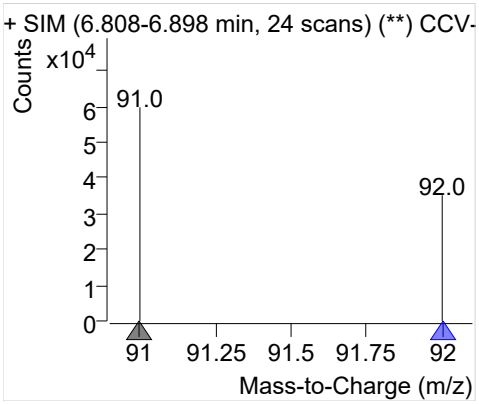
Toluene