Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC10(KD 1.15)\QuantResults\VOC10.batch.bin				
Analysis Time	2026-04-10 오전 10:56:29	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-10 오전 10:56:29	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Benzene

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
VOC10 ST-01.D	Cal	5.999	15540	2202	0.017
VOC10 ST-02.D	Cal	5.999	36633	2346	0.025
VOC10 ST-03.D	Cal	5.999	97880	2380	0.051
VOC10 ST-04.D	Cal	5.999	216663	2568	0.093
VOC10 ST-05.D	Cal	5.999	503740	2825	0.186
VOC10 ST-06.D	Cal	5.999	1052280	2602	0.408
BK-.D	Blank			3075	ND
JR 26-01-19.D	Sample			2819	ND
MBK.D	Blank			3618	ND
-CCV-.D	QC	5.999	502102	2975	0.176

Benzene

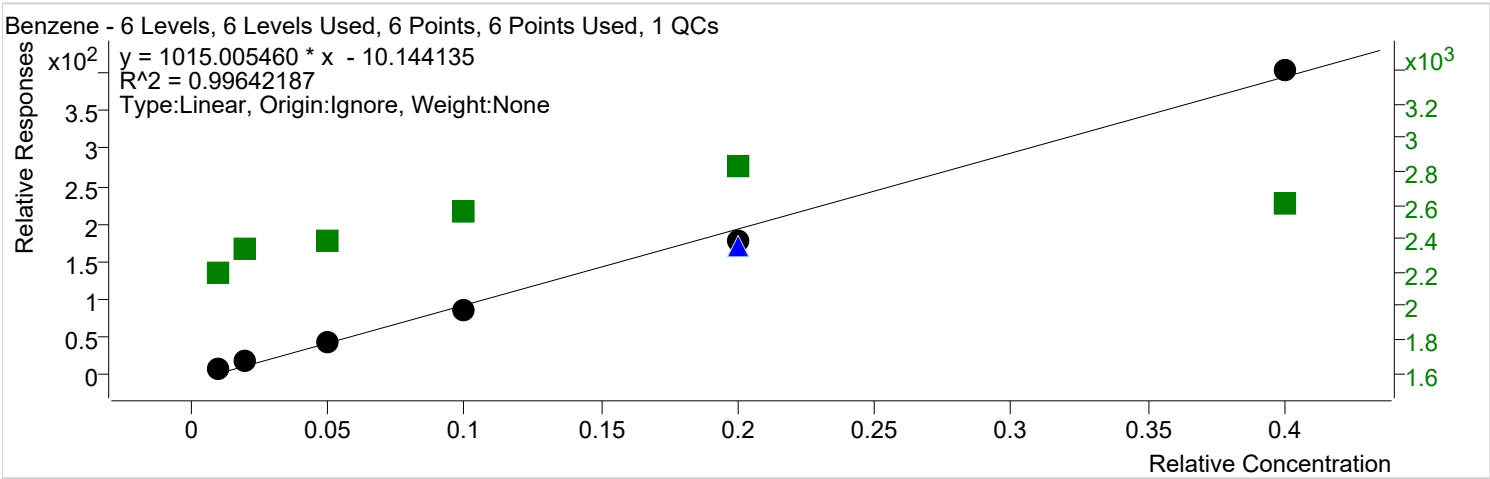

Cal. Path	Type	Level	Enable	Conc.	Response
D:\DATA\2026년\1. 2026년 1월 \VOC10(KD 1.15)\VOC10 ST-01.D	Calibration	1	x	0.010	15540
D:\DATA\2026년\1. 2026년 1월 \VOC10(KD 1.15)\VOC10 ST-02.D	Calibration	2	x	0.020	36633
D:\DATA\2026년\1. 2026년 1월 \VOC10(KD 1.15)\VOC10 ST-03.D	Calibration	3	x	0.050	97880
D:\DATA\2026년\1. 2026년 1월 \VOC10(KD 1.15)\VOC10 ST-04.D	Calibration	4	x	0.100	216663
D:\DATA\2026년\1. 2026년 1월 \VOC10(KD 1.15)\VOC10 ST-05.D	Calibration	5	x	0.200	503740
D:\DATA\2026년\1. 2026년 1월 \VOC10(KD 1.15)\-CCV-.D	QC	5	x	0.200	502102
D:\DATA\2026년\1. 2026년 1월 \VOC10(KD 1.15)\VOC10 ST-06.D	Calibration	6	x	0.400	1052280

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC10(KD 1.15)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-04-10 오전 10:56:29	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:57:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-10 오전 10:56:29	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 8:55:55	**Data File**	VOC10 ST-01.D
Type	Cal	**Name**	VOC10 ST-01
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

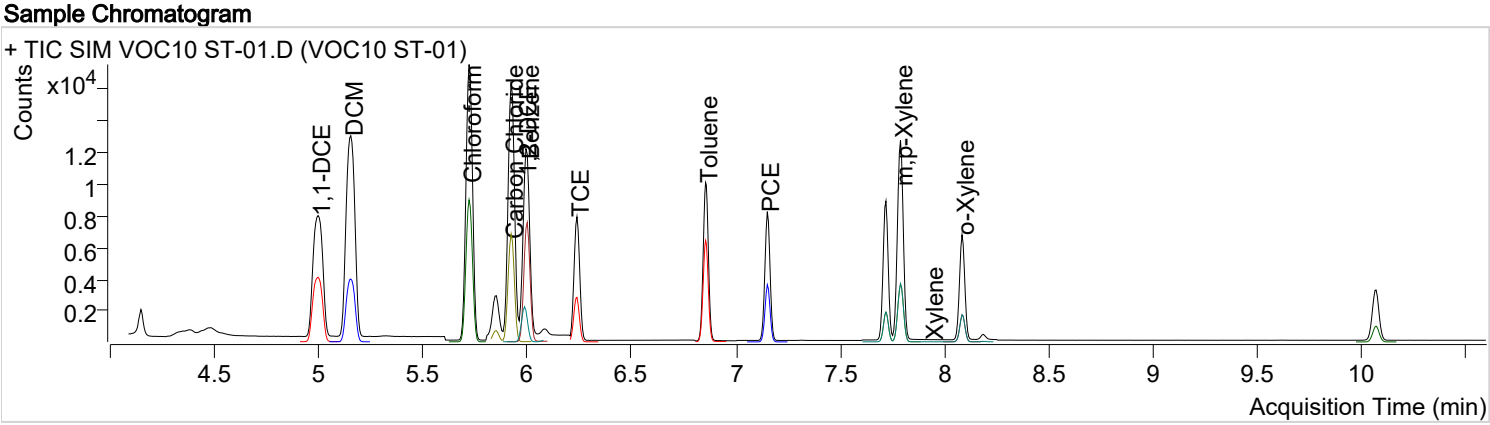

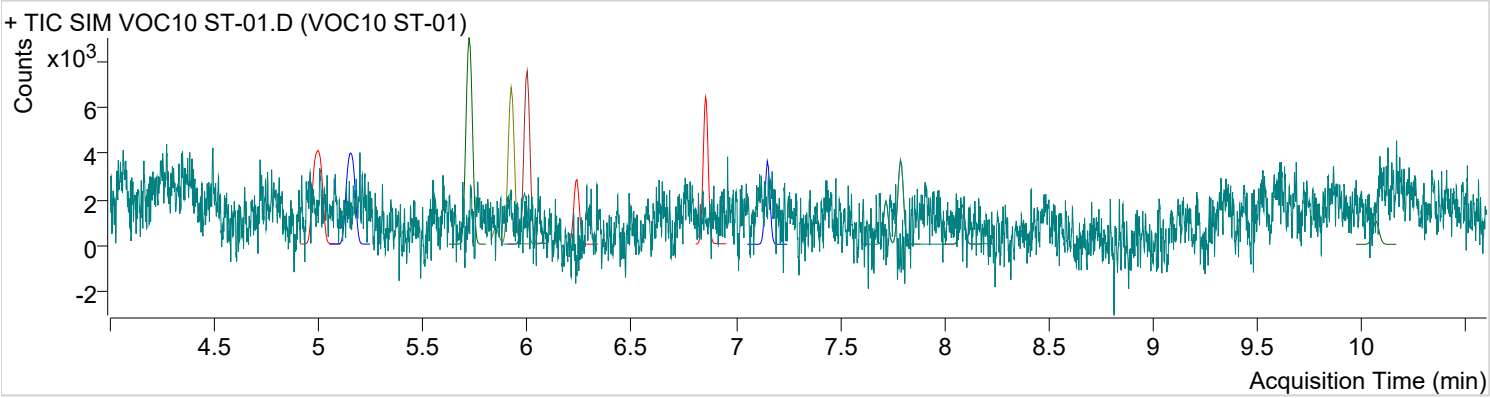

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene	5.999	15540	2202	0.017 mg/L

Benzene

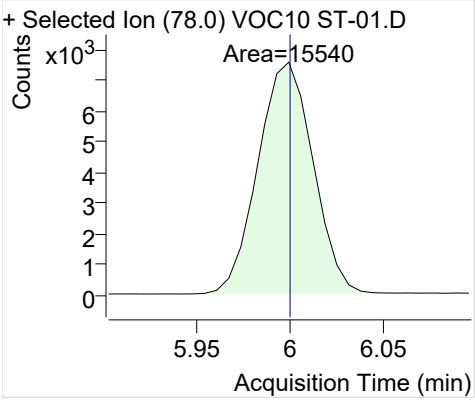

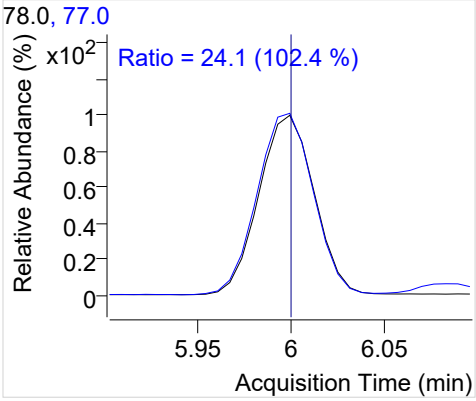

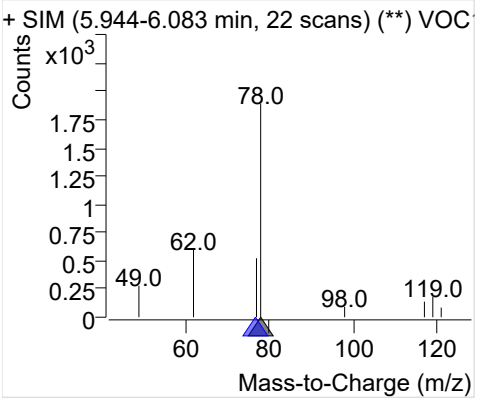

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC10(KD 1.15)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-04-10 오전 10:56:29	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:57:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-10 오전 10:56:29	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 9:08:45	**Data File**	VOC10 ST-02.D
Type	Cal	**Name**	VOC10 ST-02
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

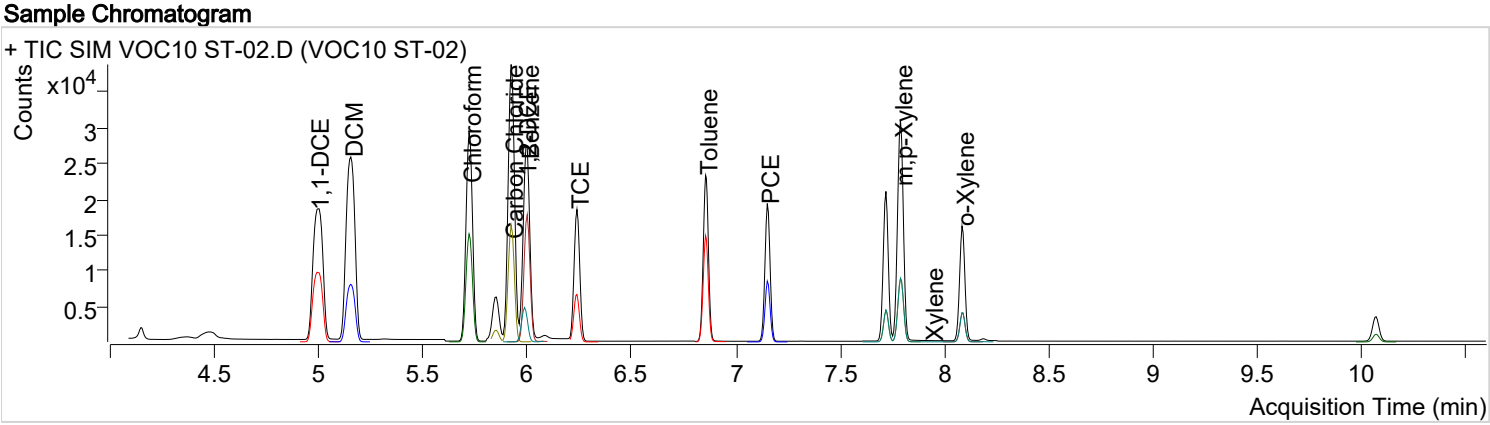

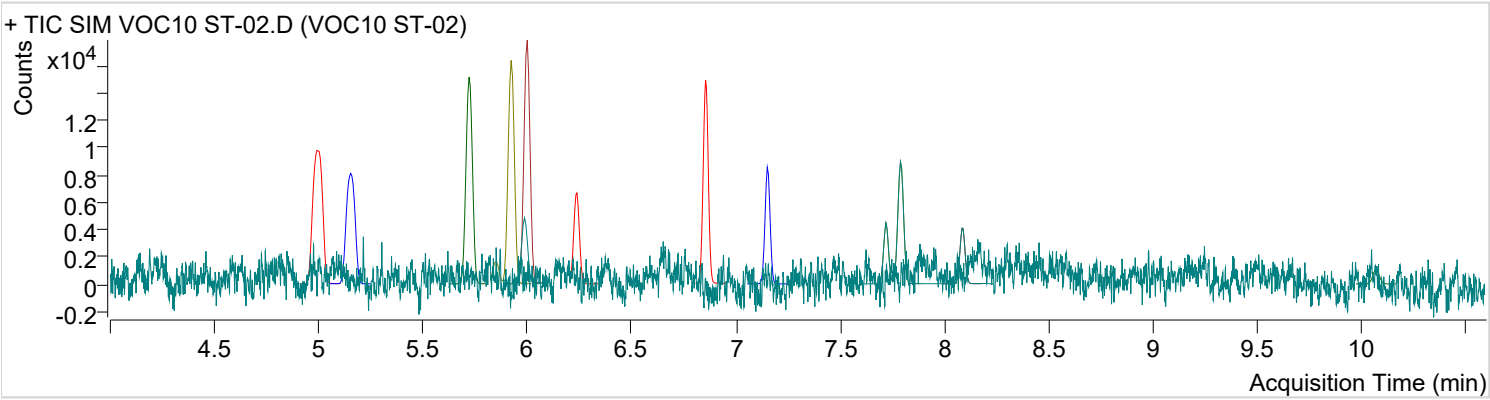

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene	5.999	36633	2346	0.025 mg/L

Benzene

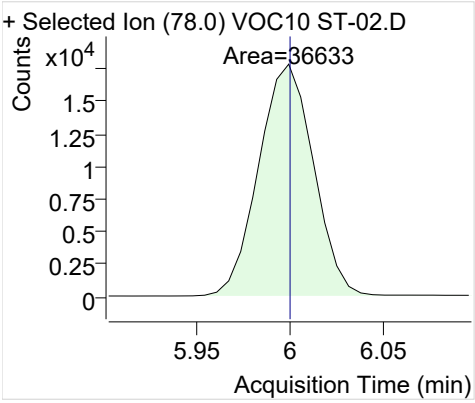

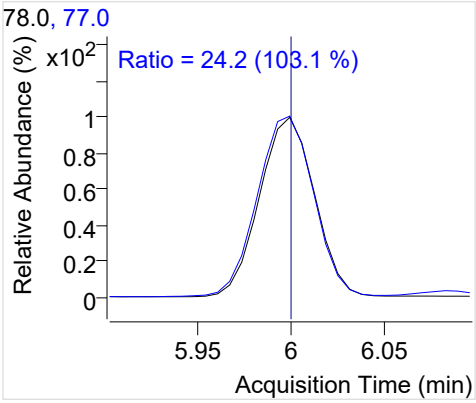

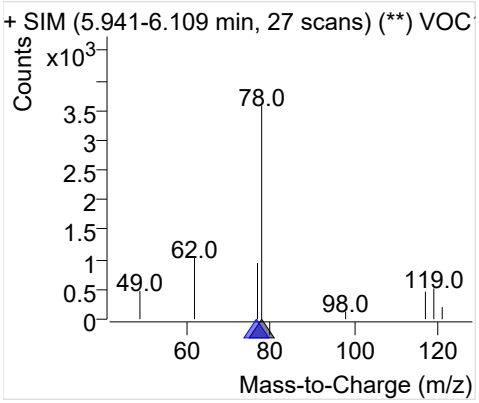

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC10(KD 1.15)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-04-10 오전 10:56:29	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:57:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-10 오전 10:56:29	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 9:21:36	**Data File**	VOC10 ST-03.D
Type	Cal	**Name**	VOC10 ST-03
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

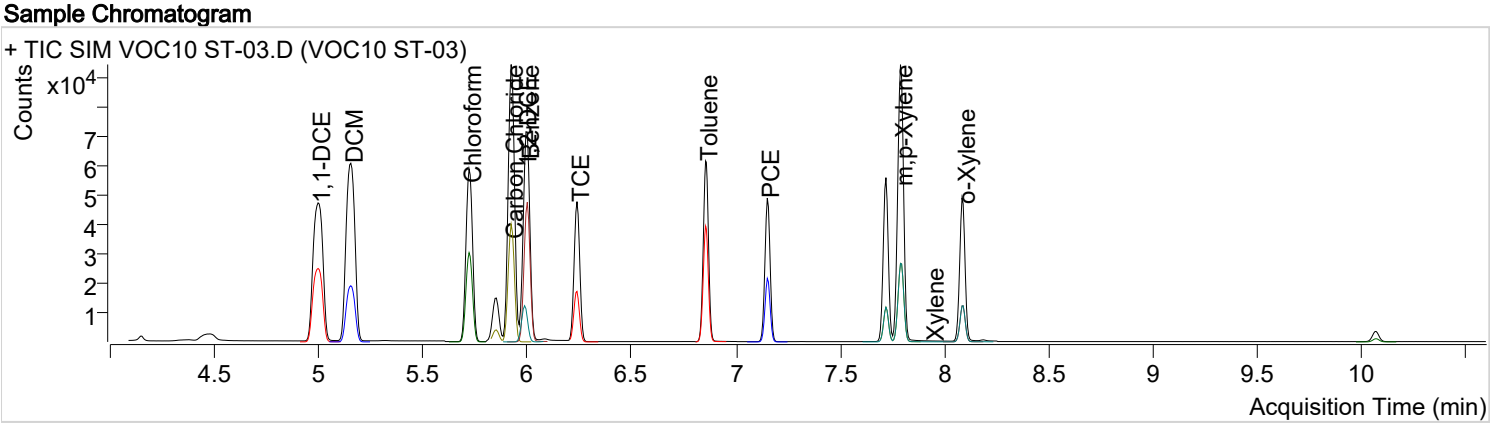

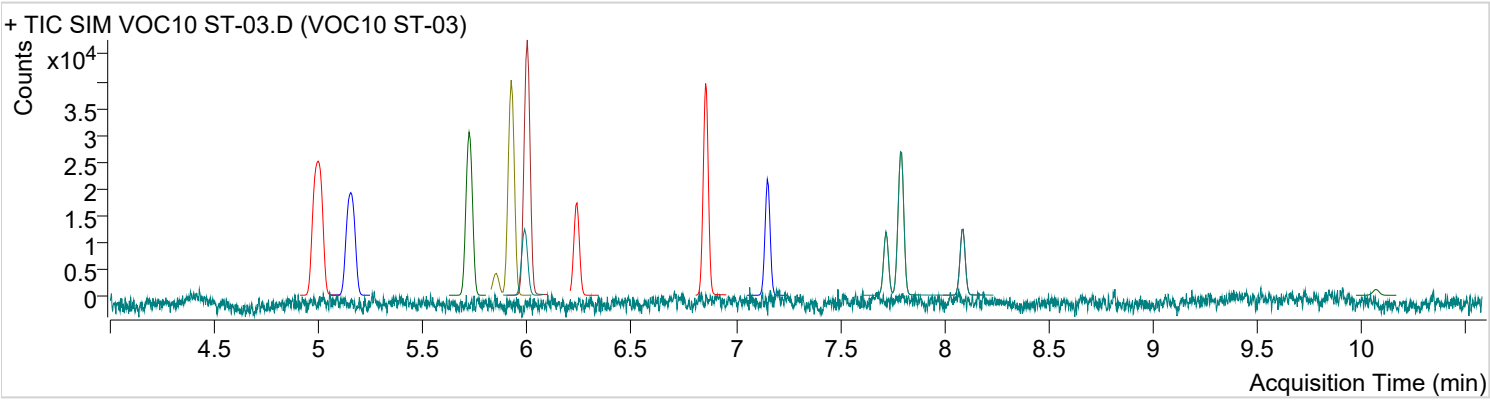

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene	5.999	97880	2380	0.051 mg/L

Benzene

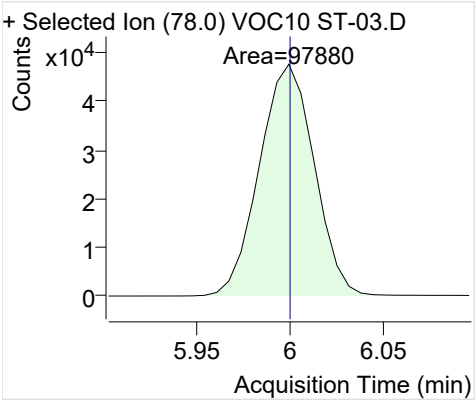

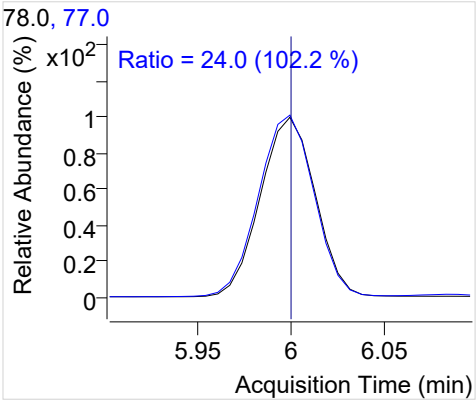

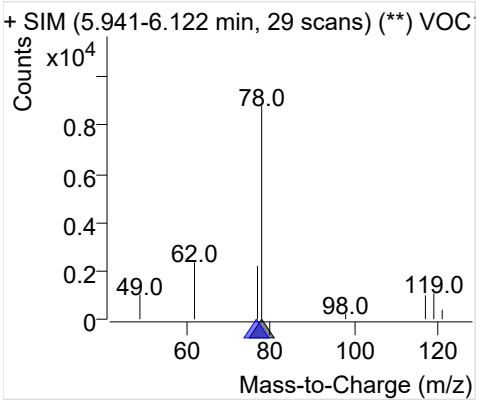

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC10(KD 1.15)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-04-10 오전 10:56:29	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:57:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-10 오전 10:56:29	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 9:34:27	**Data File**	VOC10 ST-04.D
Type	Cal	**Name**	VOC10 ST-04
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

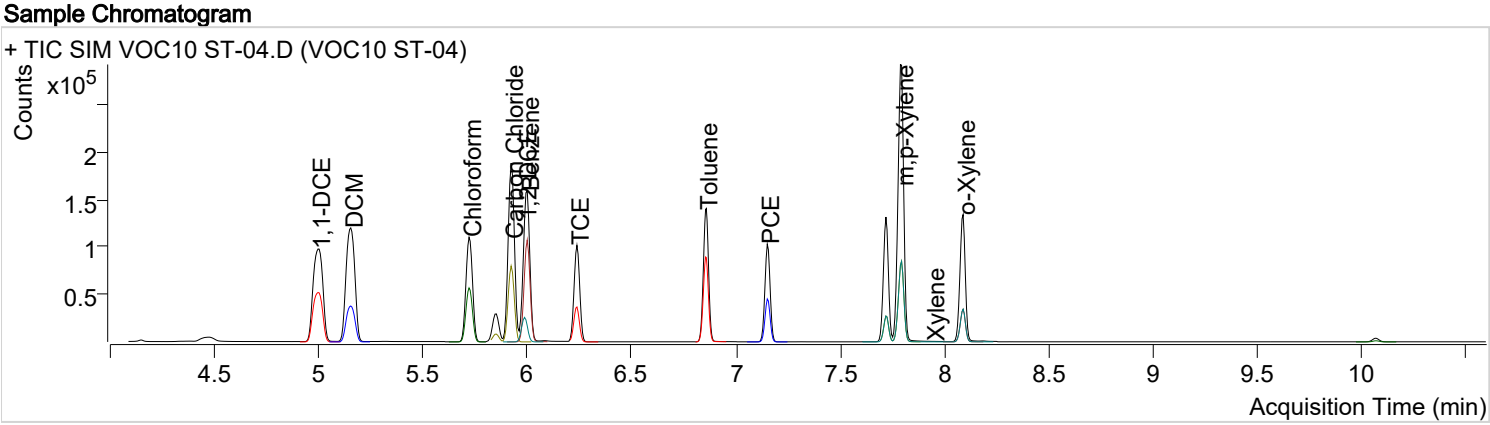

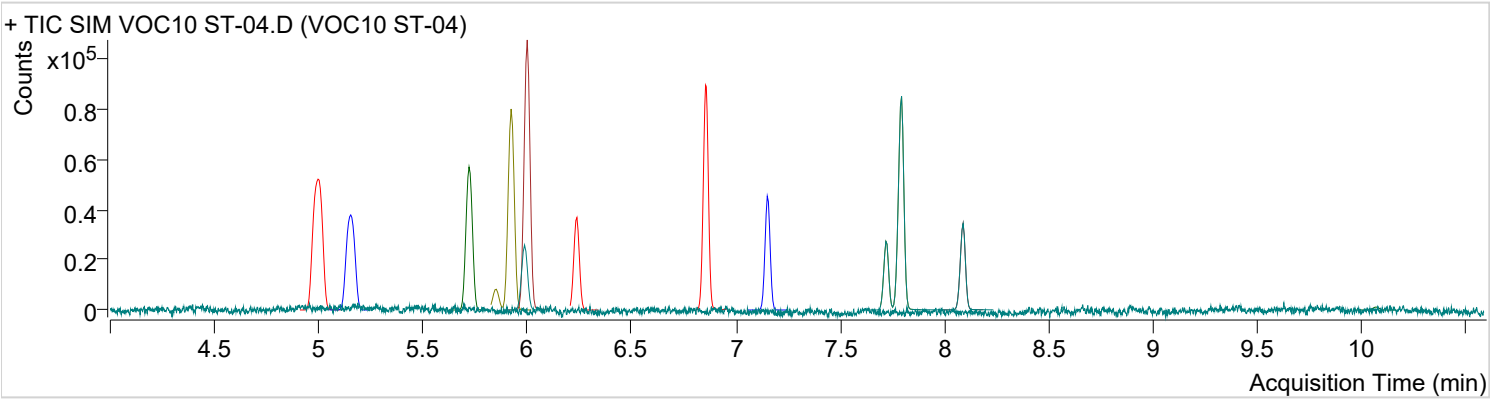

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene	5.999	216663	2568	0.093 mg/L

Benzene

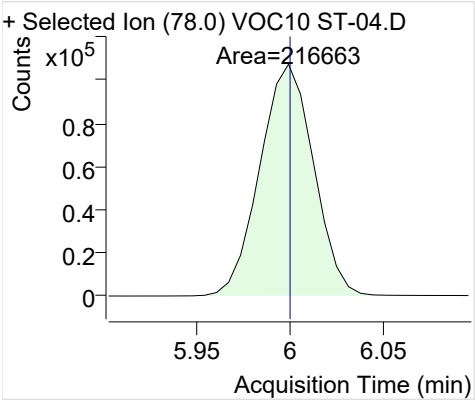

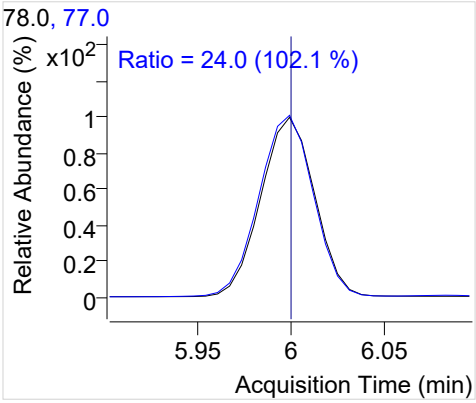

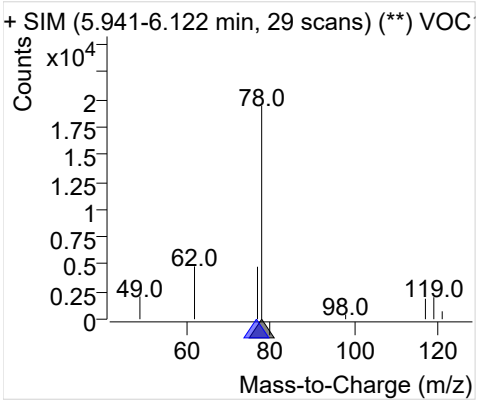

Generated at 오전 10:57 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC10(KD 1.15)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-04-10 오전 10:56:29	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:57:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-10 오전 10:56:29	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 9:47:19	**Data File**	VOC10 ST-05.D
Type	Cal	**Name**	VOC10 ST-05
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

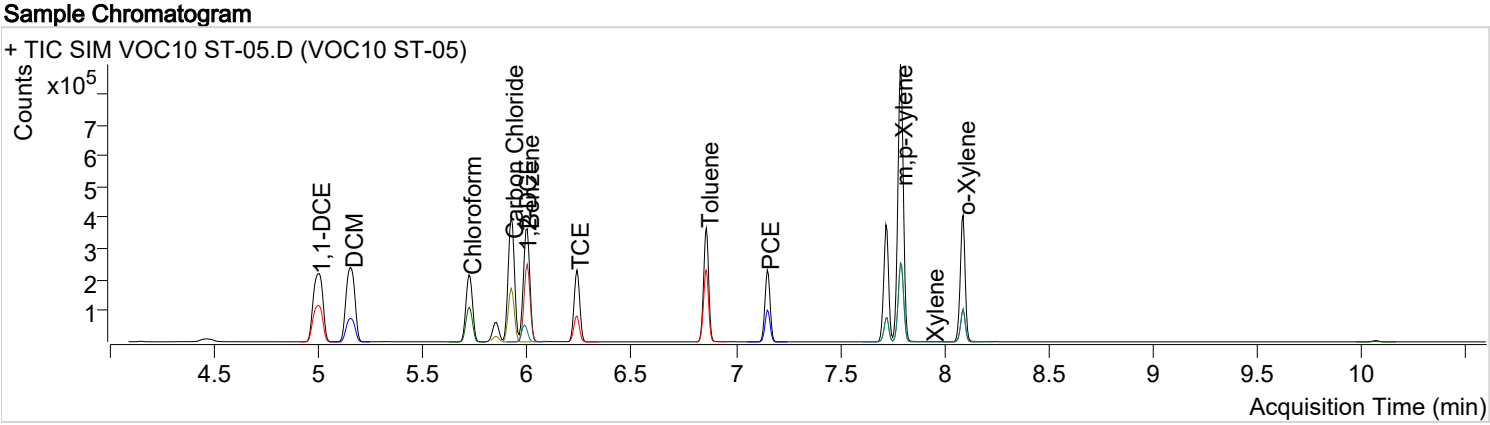

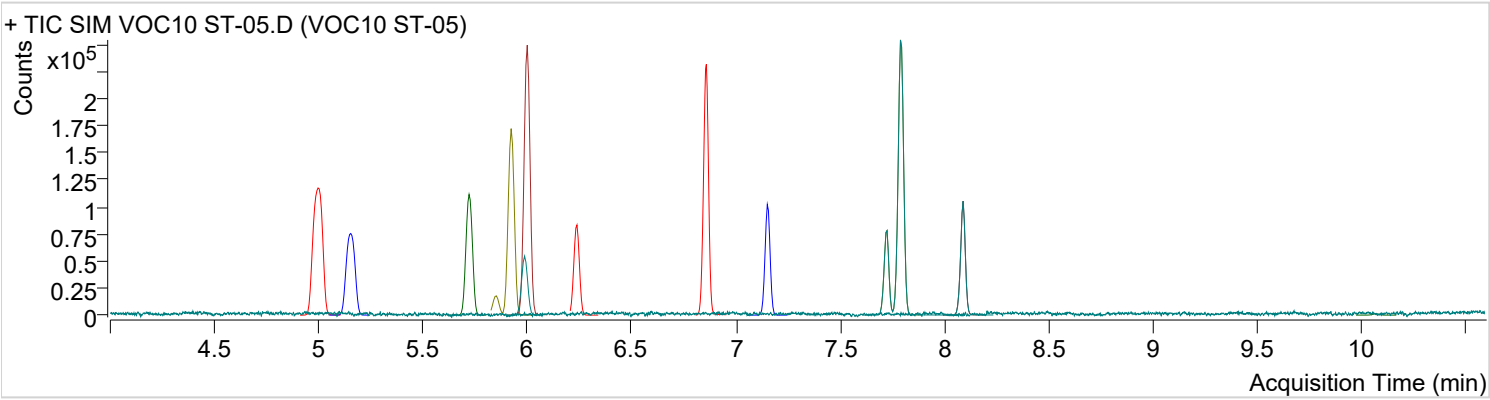

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene	5.999	503740	2825	0.186 mg/L

Benzene

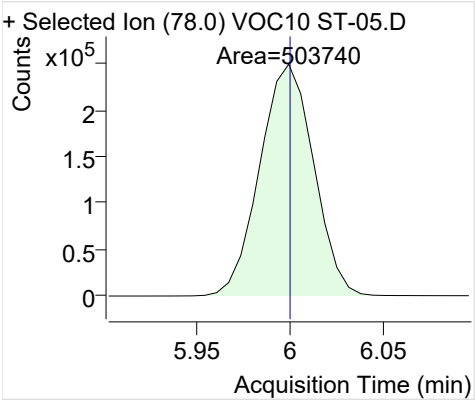

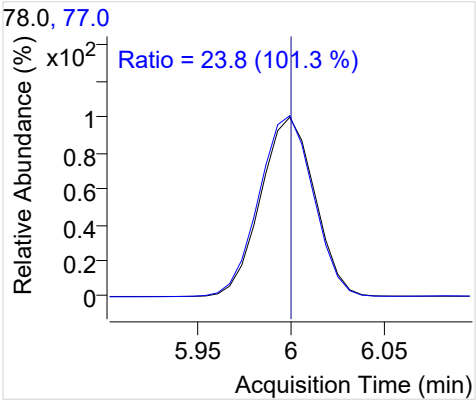

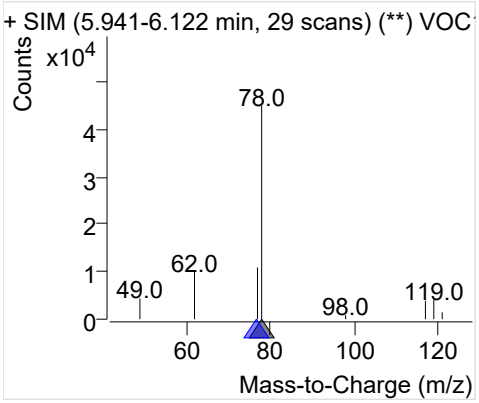

Generated at 오전 10:57 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC10(KD 1.15)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-04-10 오전 10:56:29	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:57:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-10 오전 10:56:29	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 10:04:31	**Data File**	VOC10 ST-06.D
Type	Cal	**Name**	VOC10 ST-06
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

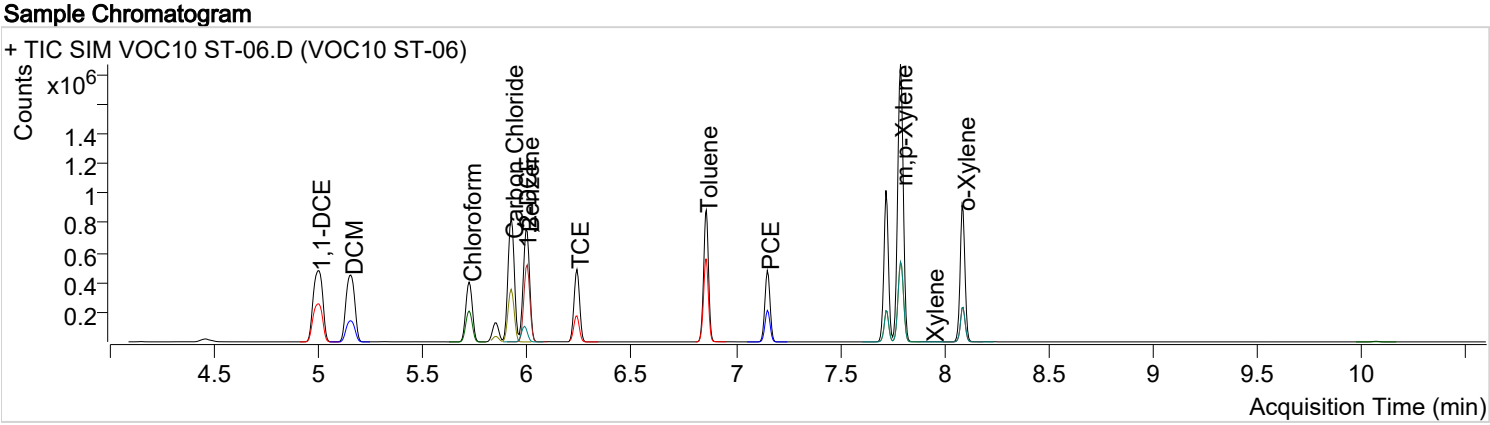

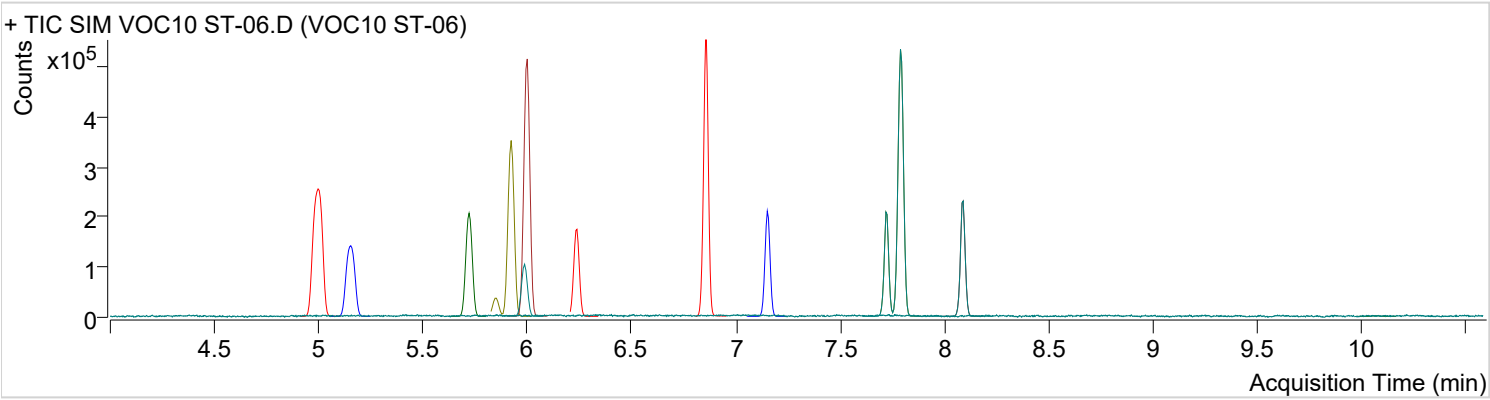

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene	5.999	1052280	2602	0.408 mg/L

Benzene

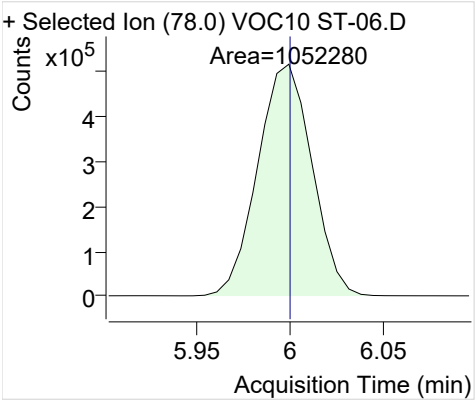

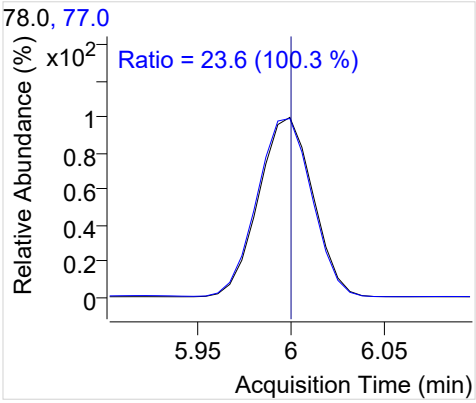

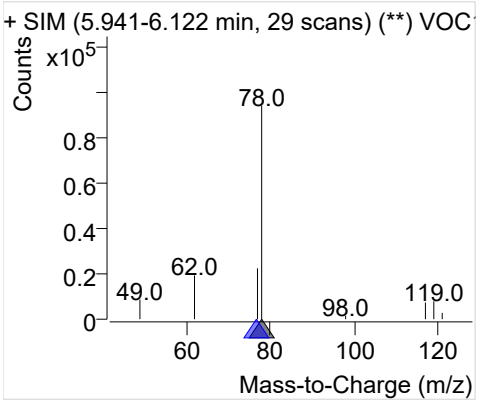

Generated at 오전 10:57 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC10(KD 1.15)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-04-10 오전 10:56:29	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:57:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-10 오전 10:56:29	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 10:29:50	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

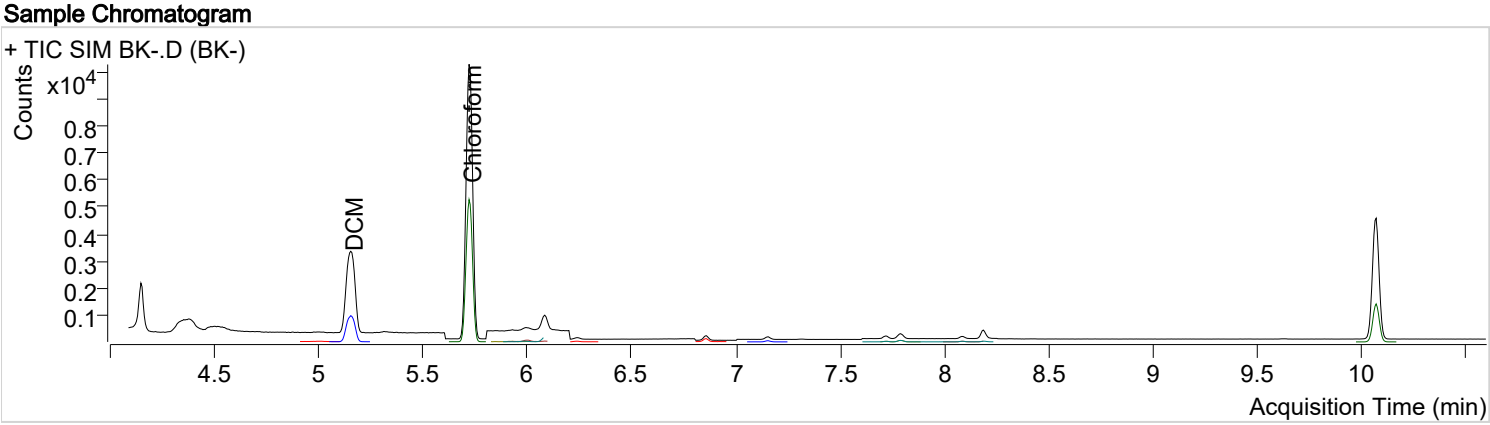

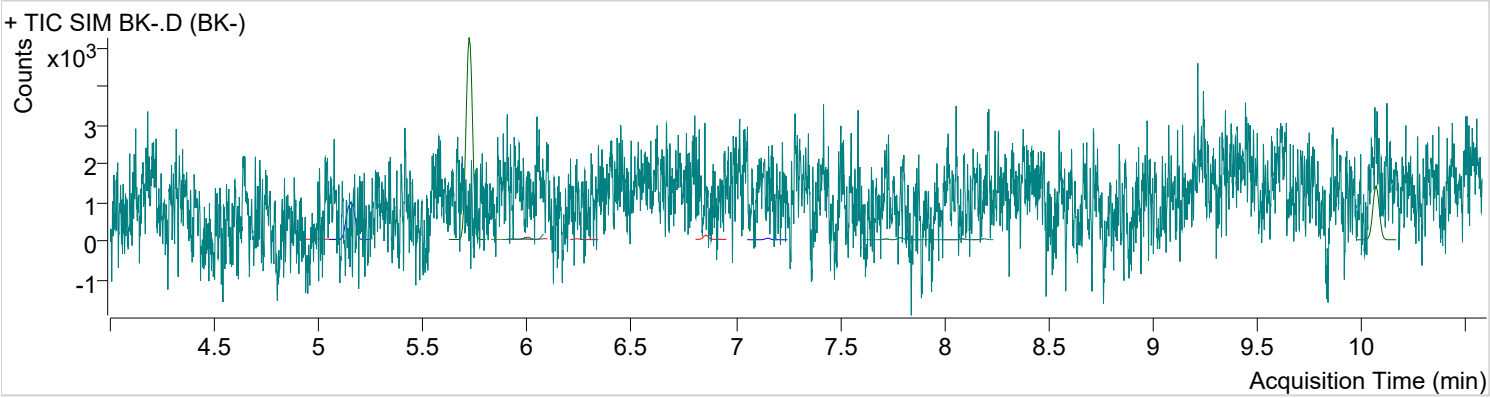

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene			3075	ND mg/L

Benzene

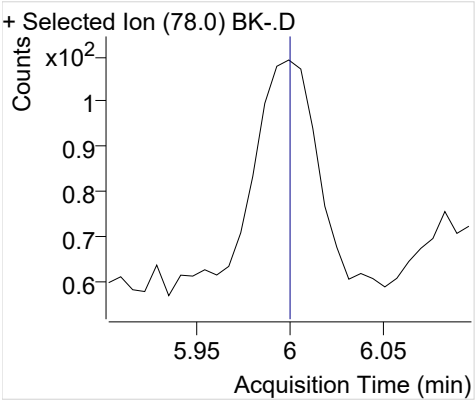

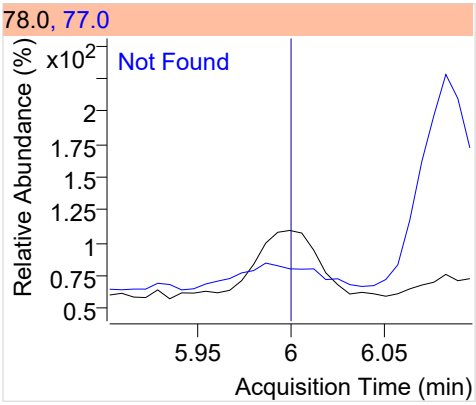

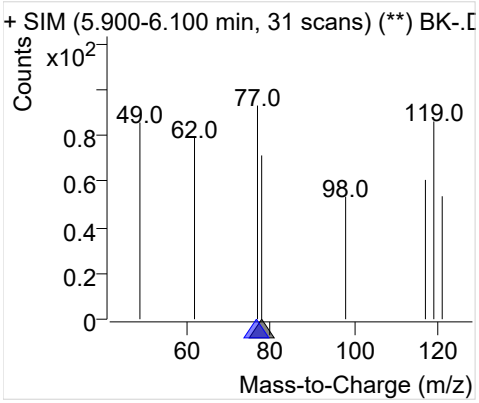

Generated at 오전 10:57 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC10(KD 1.15)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-04-10 오전 10:56:29	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:57:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-10 오전 10:56:29	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 11:20:32	**Data File**	JR 26-01-19.D
Type	Sample	**Name**	JR 26-01-19
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

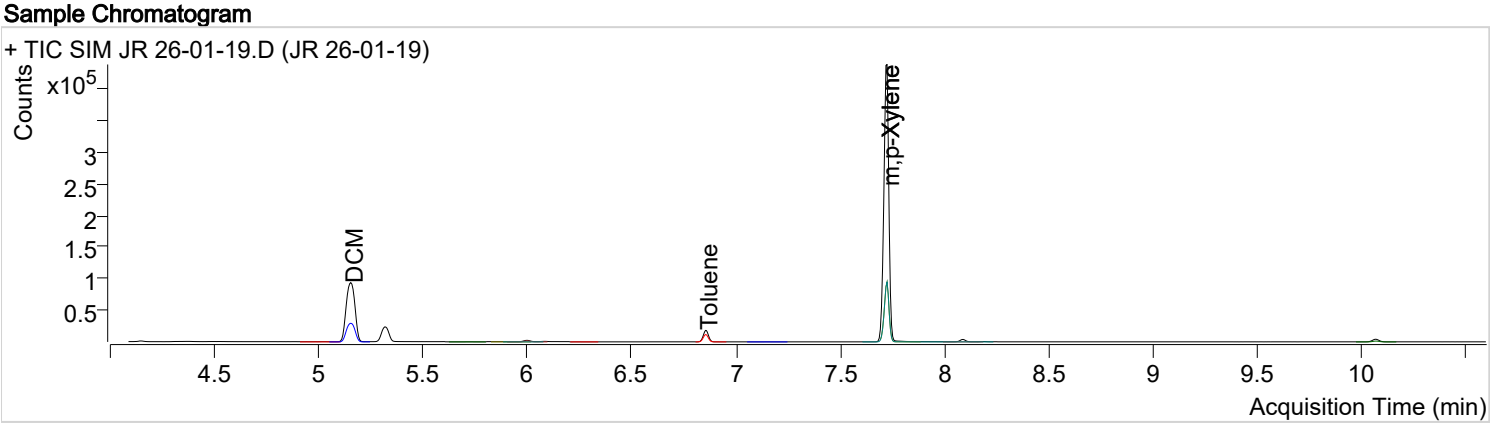

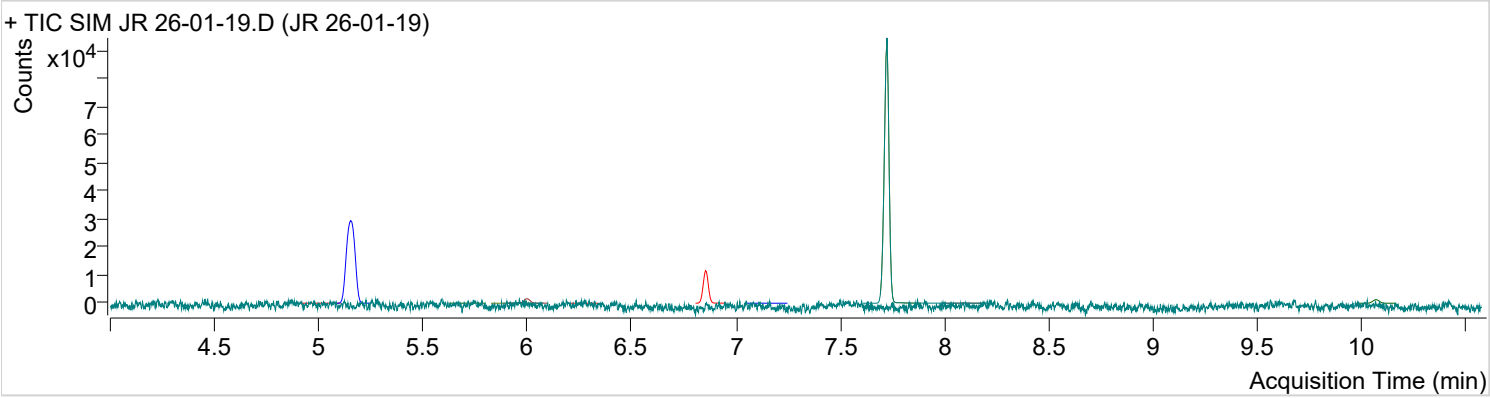

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene			2819	ND mg/L

Benzene

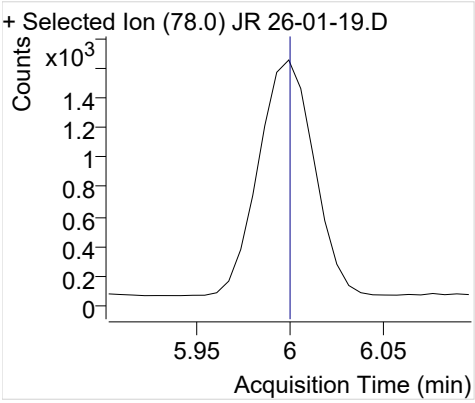

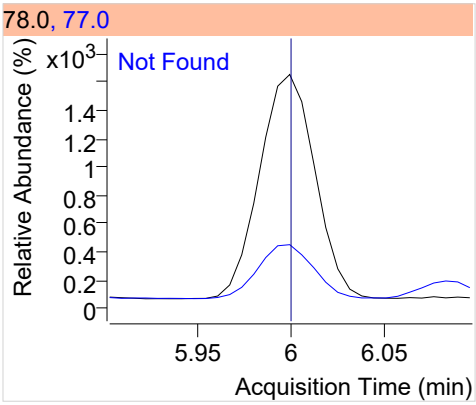

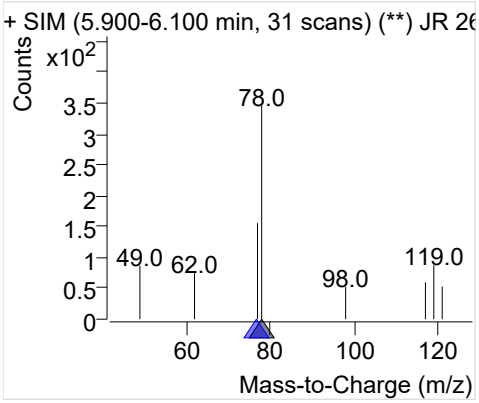

Generated at 오전 10:57 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC10(KD 1.15)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-04-10 오전 10:56:29	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:57:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-10 오전 10:56:29	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 11:33:12	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

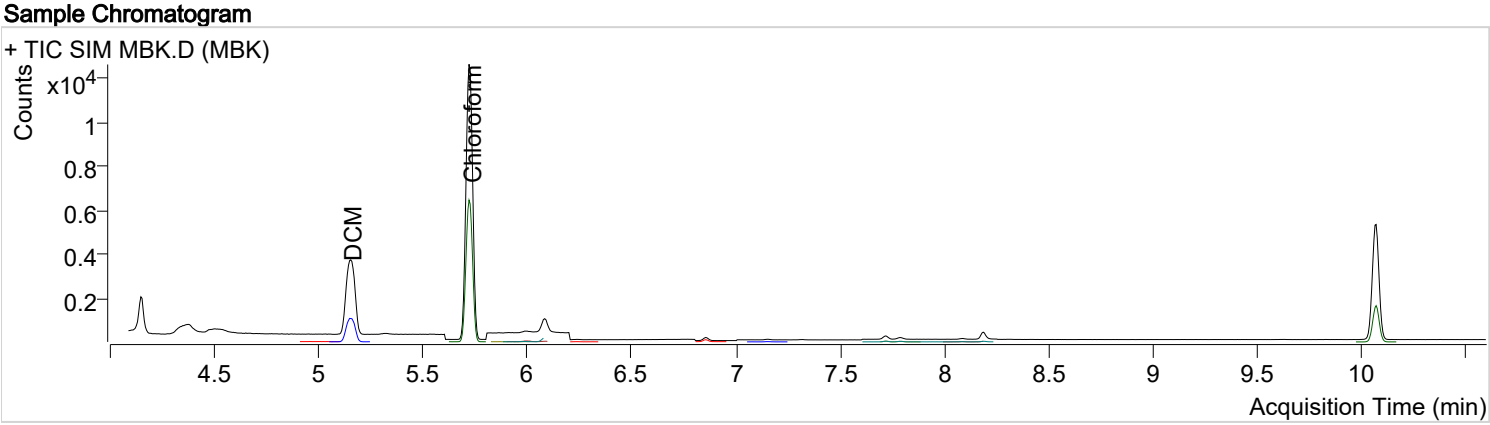

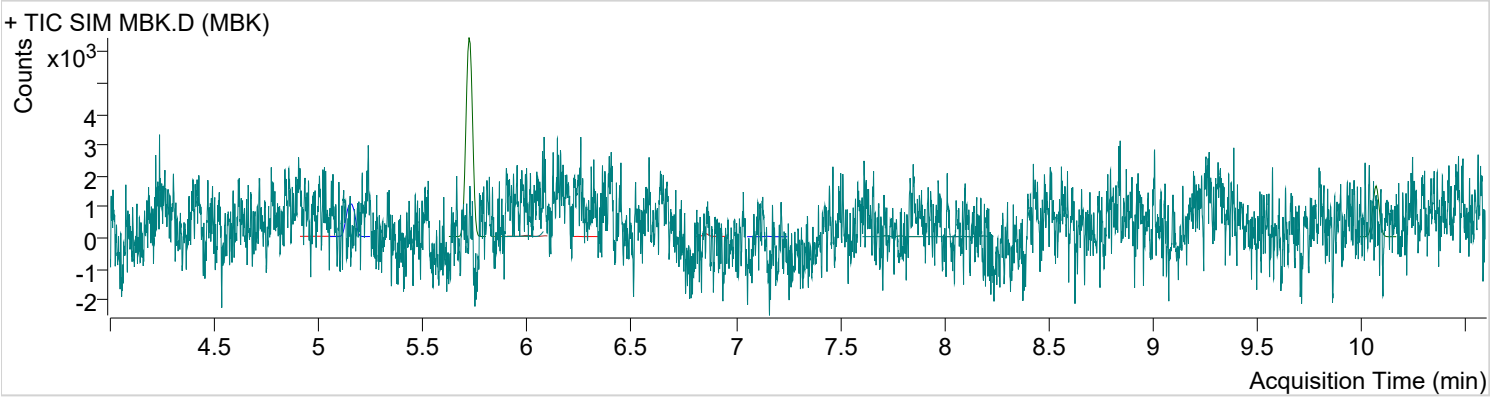

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene			3618	ND mg/L

Benzene

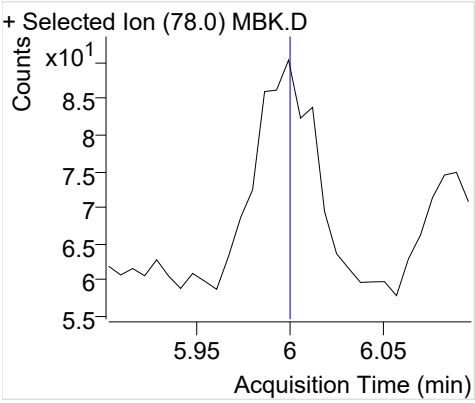

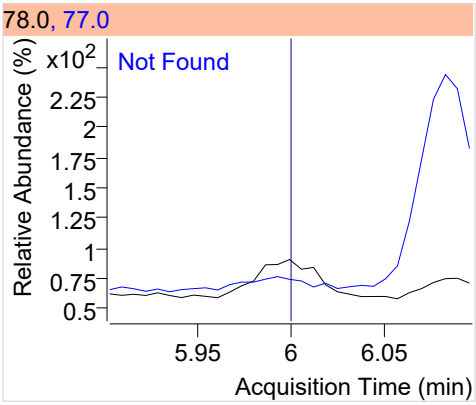

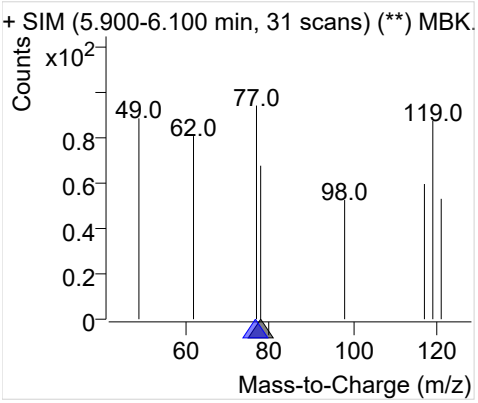

Generated at 오전 10:57 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC10(KD 1.15)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-04-10 오전 10:56:29	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:57:29	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-10 오전 10:56:29	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-19 오후 11:58:41	**Data File**	-CCV-.D
Type	QC	**Name**	-CCV-
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

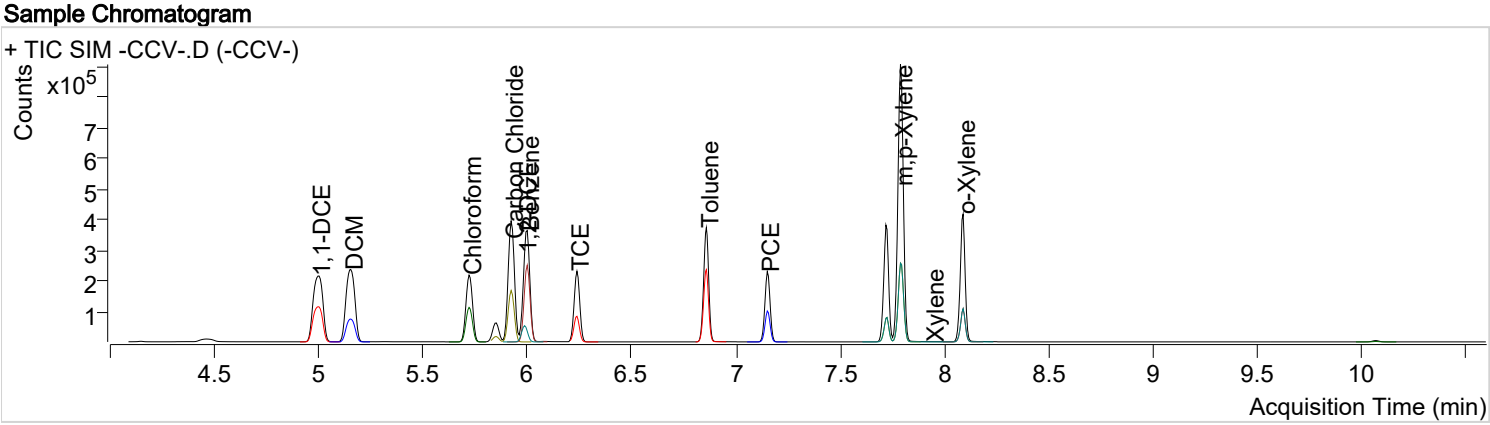

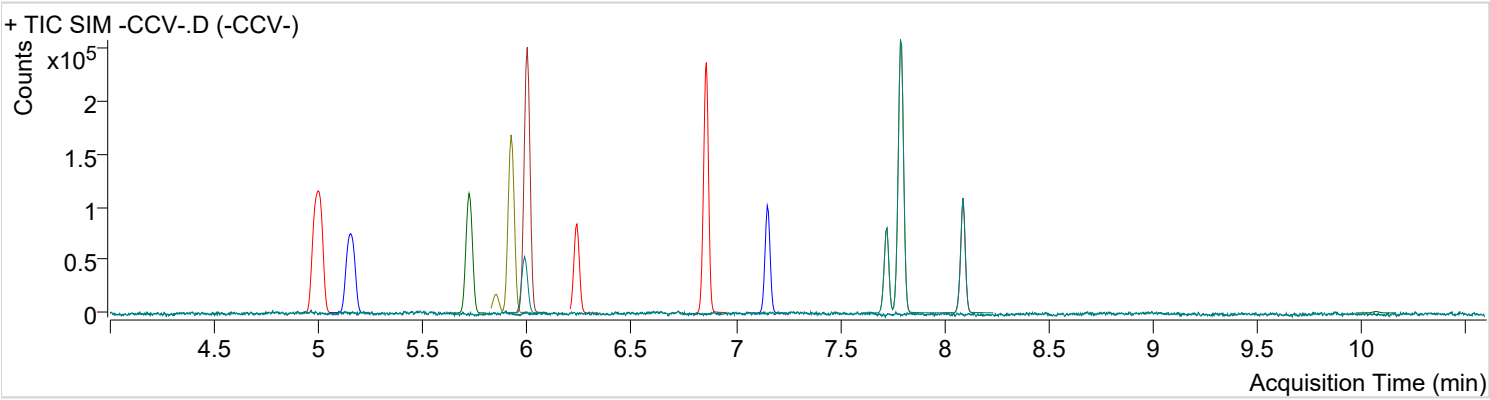

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene	5.999	502102	2975	0.176 mg/L

Benzene

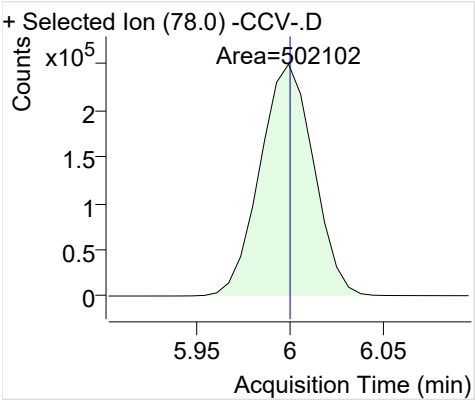

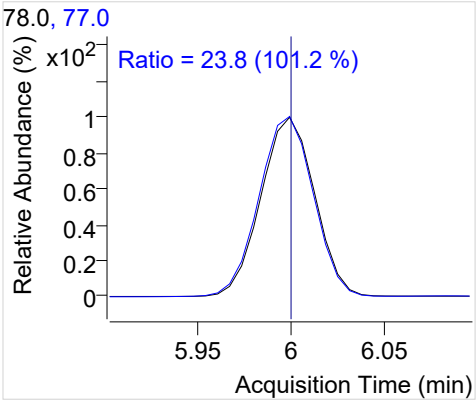

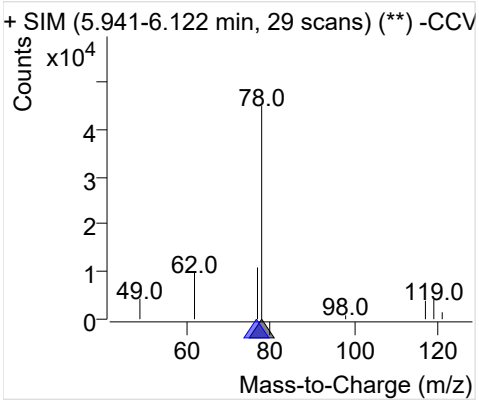

Generated at 오전 10:57 on 2026-04-10