Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\VOC10(JR 2.20)\QuantResults\VOC10.batch.bin				
Analysis Time	2026-02-24 오전 8:45:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:45:07	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Benzene

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
VOC10 ST-01.D	Cal	5.993	6852	2326	0.011
VOC10 ST-02.D	Cal	5.993	17290	2406	0.021
VOC10 ST-03.D	Cal	5.993	49511	2534	0.049
VOC10 ST-04.D	Cal	5.993	106066	2548	0.099
VOC10 ST-05.D	Cal	5.993	235264	2769	0.198
VOC10 ST-06.D	Cal	5.993	419138	2410	0.401
BK-.D	Blank			2849	ND
JR 26-02-20.D	Sample			2941	ND
MBK.D	Blank			2983	ND
CCV-.D	QC	5.993	246198	2704	0.212

Benzene

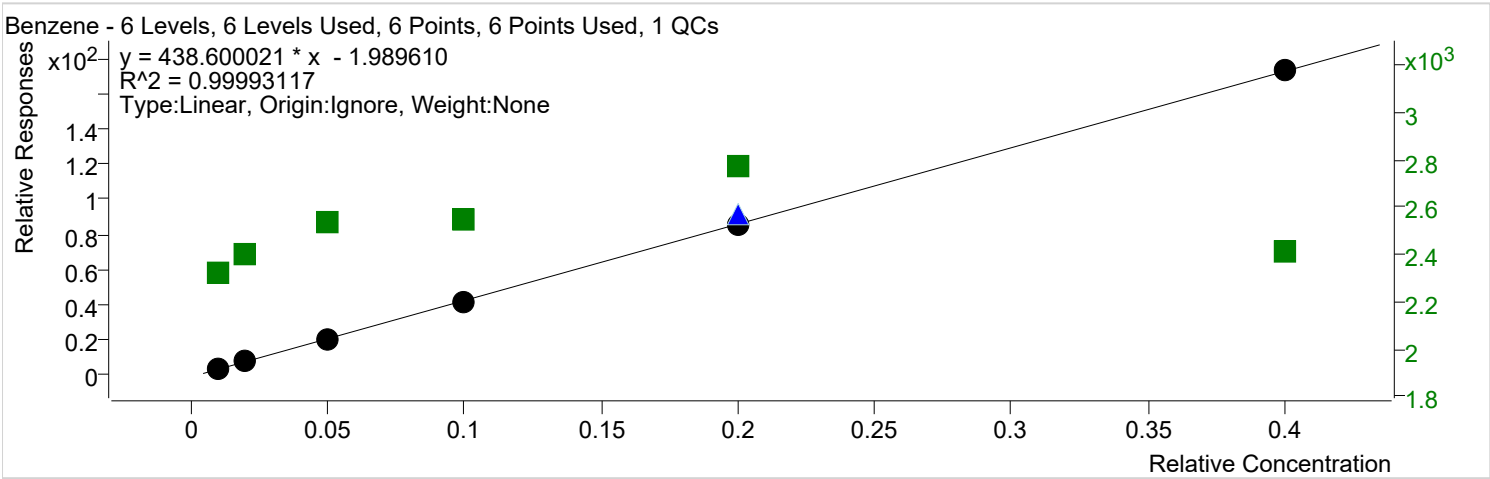

Cal. Path	Type	Level	Enable	Conc.	Response
D:\DATA\2026년\2. 2026년 2월 \VOC10(JR 2.20)\VOC10 ST-01.D	Calibration	1	x	0.010	6852
D:\DATA\2026년\2. 2026년 2월 \VOC10(JR 2.20)\VOC10 ST-02.D	Calibration	2	x	0.020	17290
D:\DATA\2026년\2. 2026년 2월 \VOC10(JR 2.20)\VOC10 ST-03.D	Calibration	3	x	0.050	49511
D:\DATA\2026년\2. 2026년 2월 \VOC10(JR 2.20)\VOC10 ST-04.D	Calibration	4	x	0.100	106066
D:\DATA\2026년\2. 2026년 2월 \VOC10(JR 2.20)\VOC10 ST-05.D	Calibration	5	x	0.200	235264
D:\DATA\2026년\2. 2026년 2월 \VOC10(JR 2.20)\CCV-.D	QC	5	x	0.200	246198
D:\DATA\2026년\2. 2026년 2월 \VOC10(JR 2.20)\VOC10 ST-06.D	Calibration	6	x	0.400	419138

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\VOC10(JR 2.20)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-02-24 오전 8:45:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:08:33	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:45:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 4:47:51	**Data File**	VOC10 ST-01.D
Type	Cal	**Name**	VOC10 ST-01
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

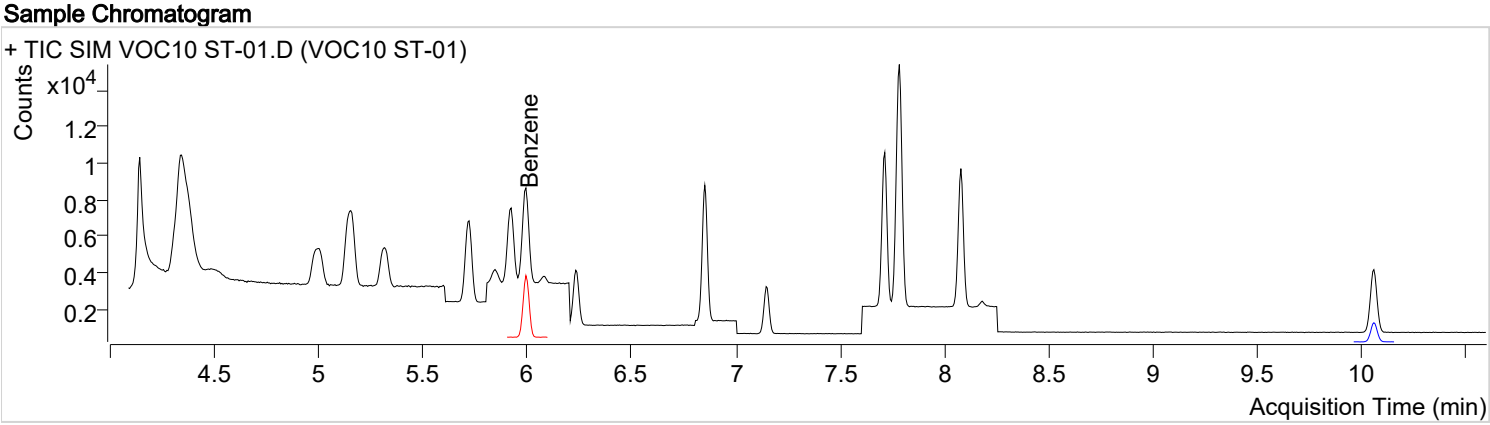

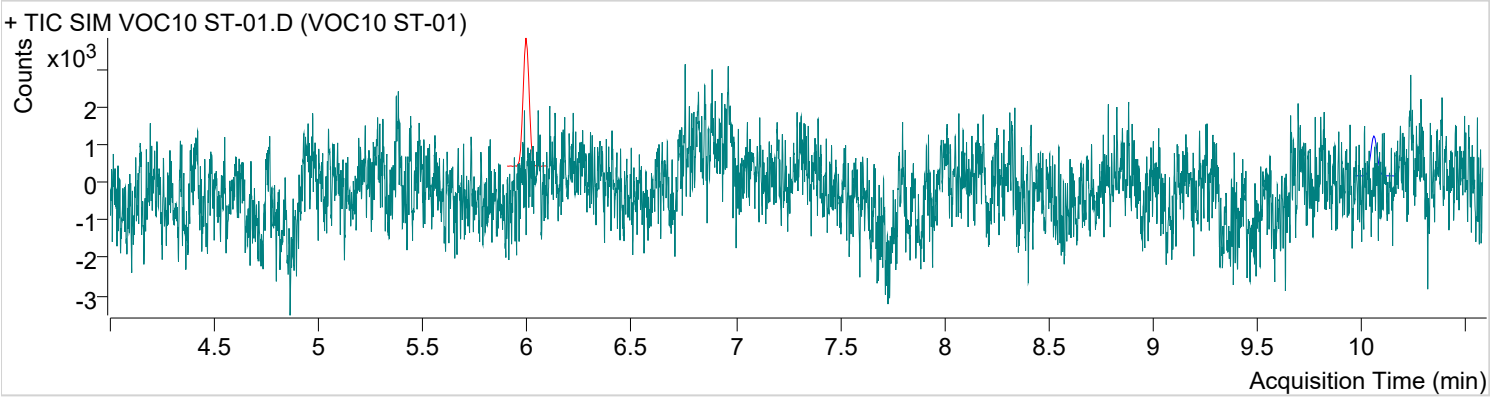

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene	5.993	6852	2326	0.011 mg/L

Benzene

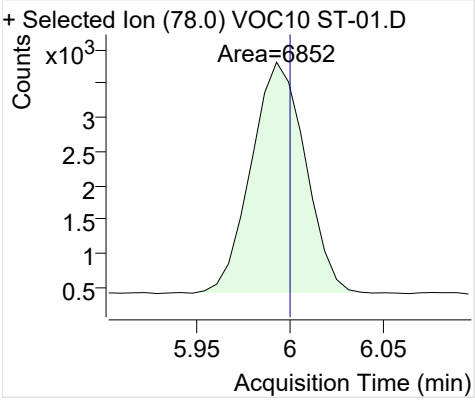

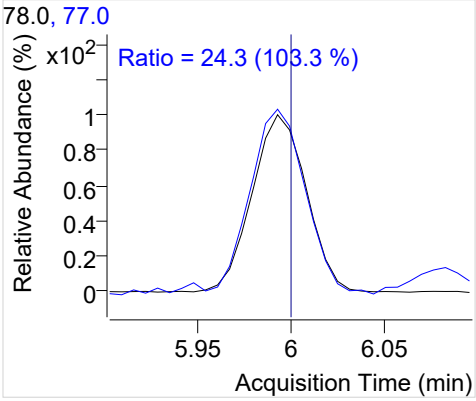

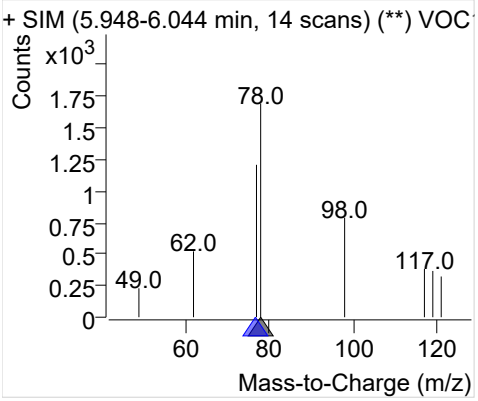

Generated at 오전 11:08 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\VOC10(JR 2.20)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-02-24 오전 8:45:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:08:33	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:45:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 5:00:35	**Data File**	VOC10 ST-02.D
Type	Cal	**Name**	VOC10 ST-02
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

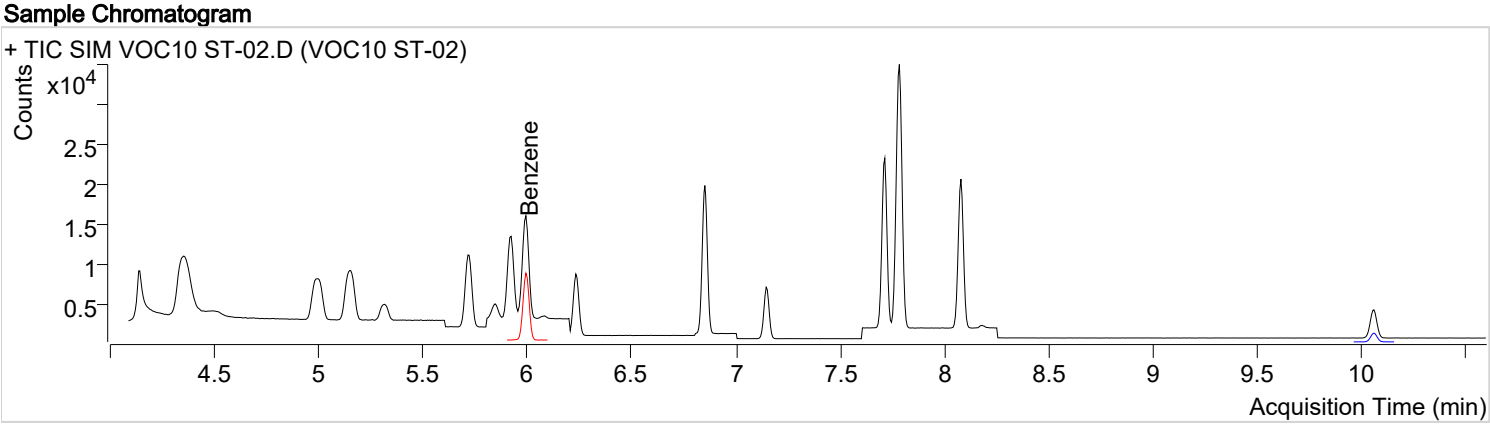

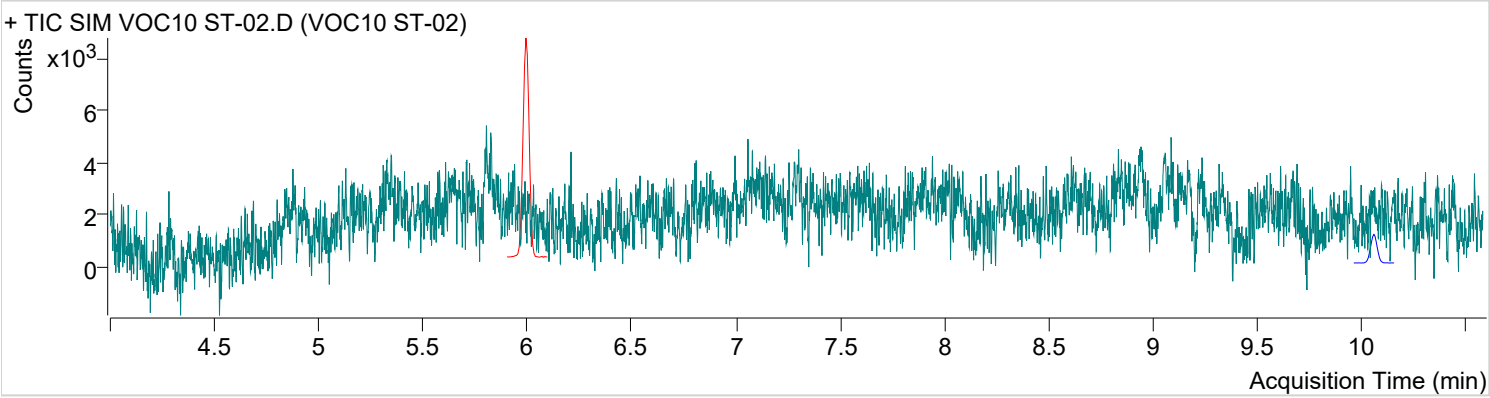

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene	5.993	17290	2406	0.021 mg/L

Benzene

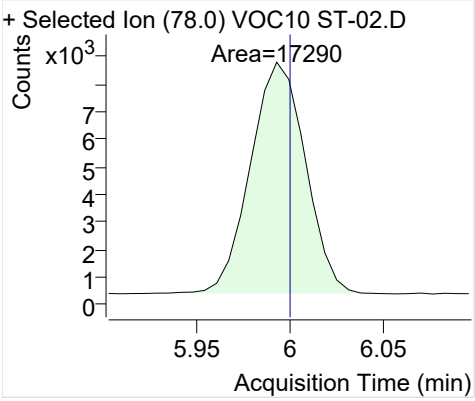

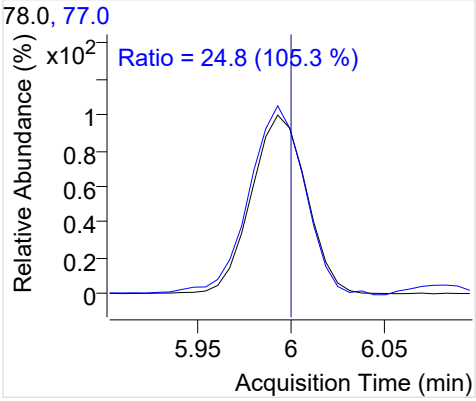

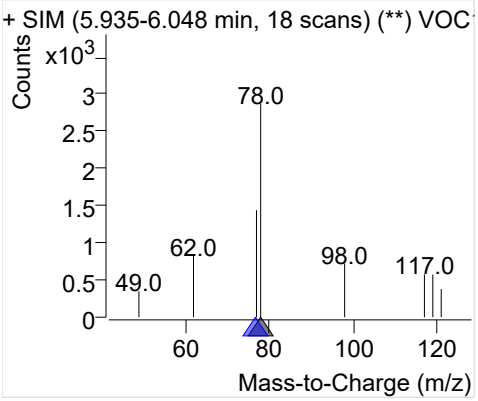

Generated at 오전 11:08 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\VOC10(JR 2.20)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-02-24 오전 8:45:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:08:33	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:45:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 5:13:19	**Data File**	VOC10 ST-03.D
Type	Cal	**Name**	VOC10 ST-03
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

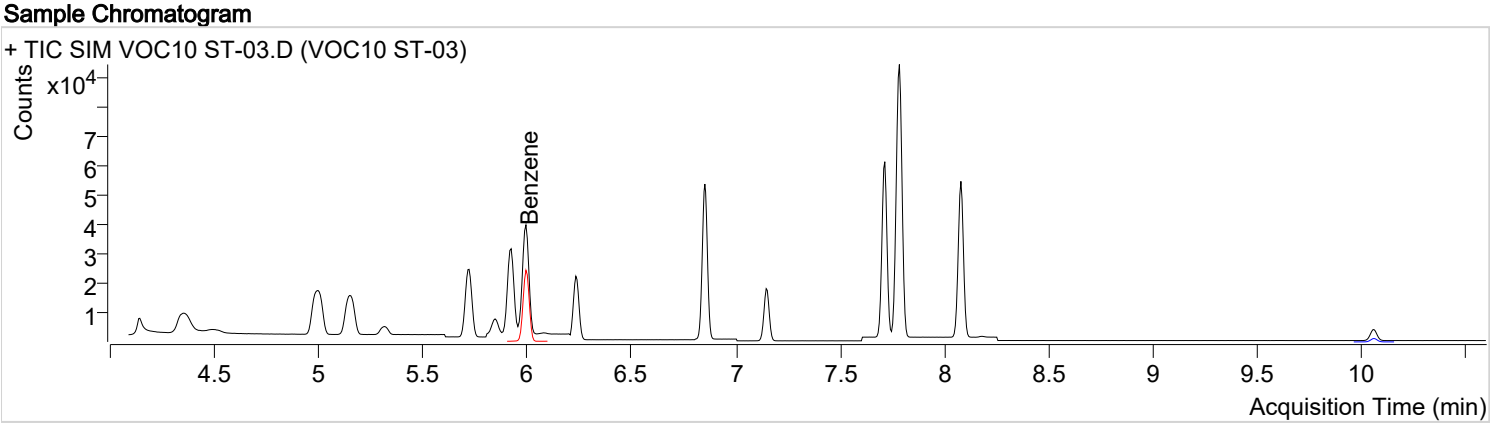

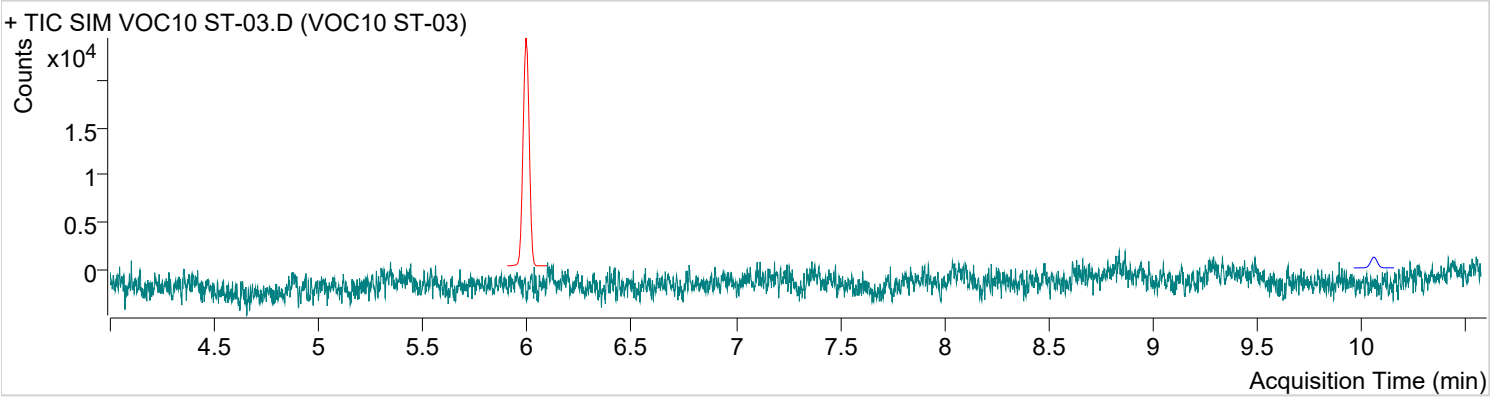

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene	5.993	49511	2534	0.049 mg/L

Benzene

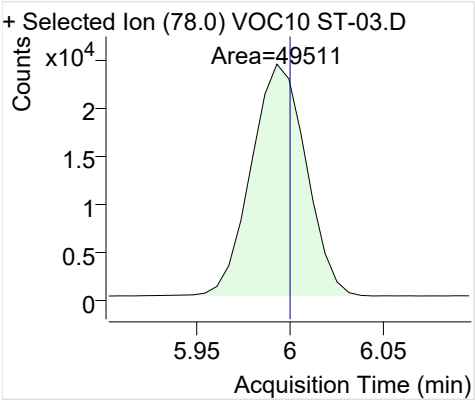

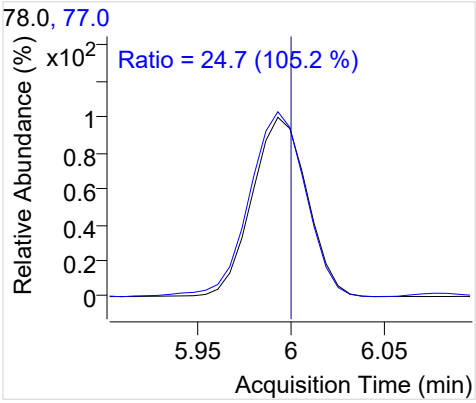

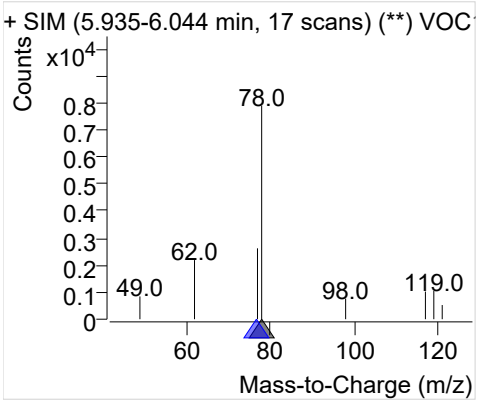

Generated at 오전 11:08 on 2026-04-10

Quant Sample Report

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\VOC10(JR 2.20)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-02-24 오전 8:45:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:08:33	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:45:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 5:26:02	**Data File**	VOC10 ST-04.D
Type	Cal	**Name**	VOC10 ST-04
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

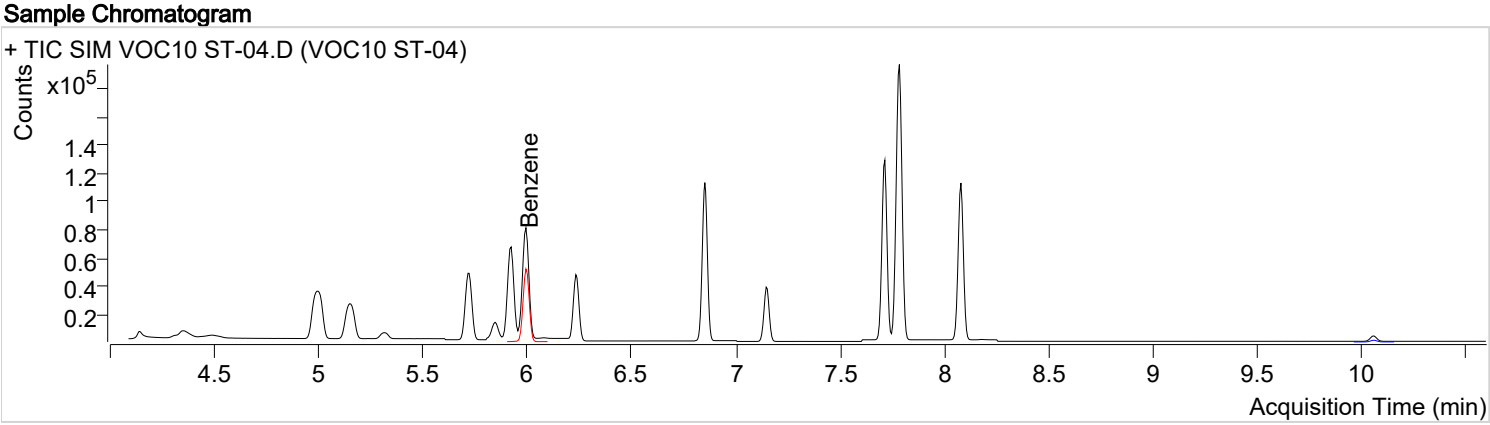

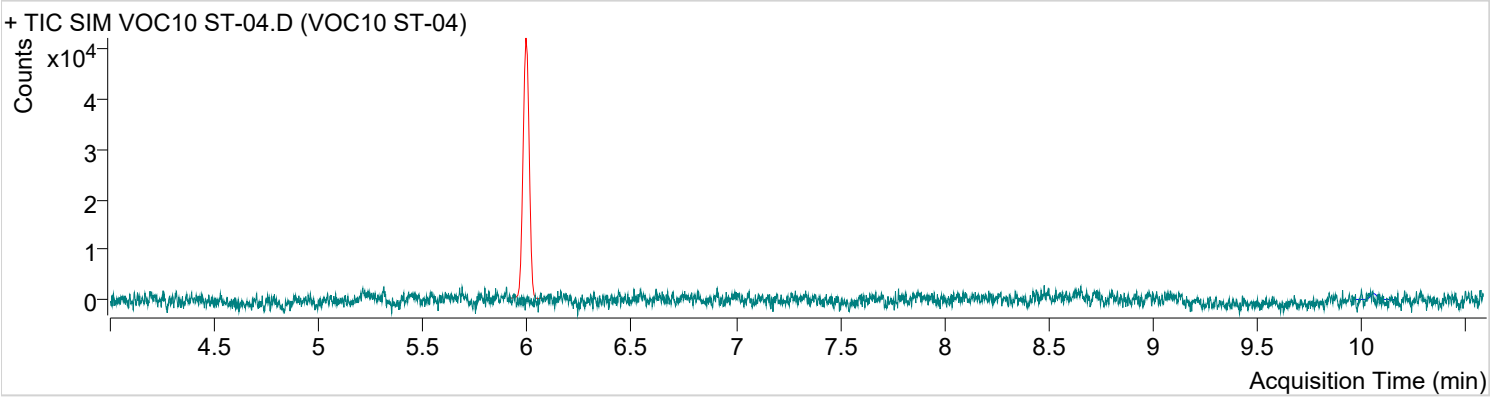

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene	5.993	106066	2548	0.099 mg/L

Benzene

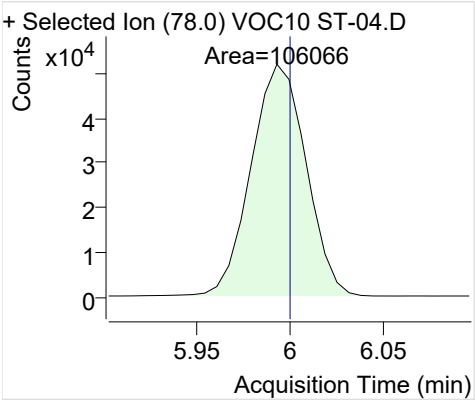

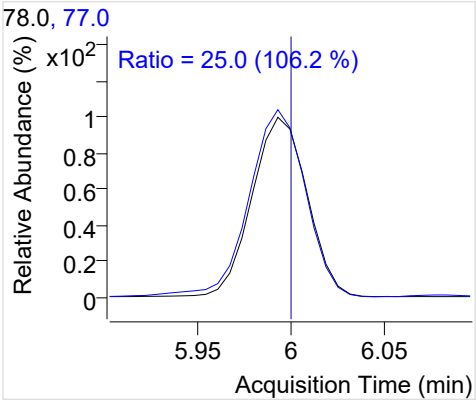

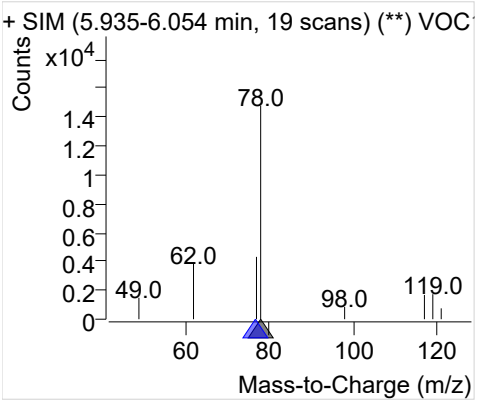

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\VOC10(JR 2.20)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-02-24 오전 8:45:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:08:33	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:45:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 5:38:44	**Data File**	VOC10 ST-05.D
Type	Cal	**Name**	VOC10 ST-05
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

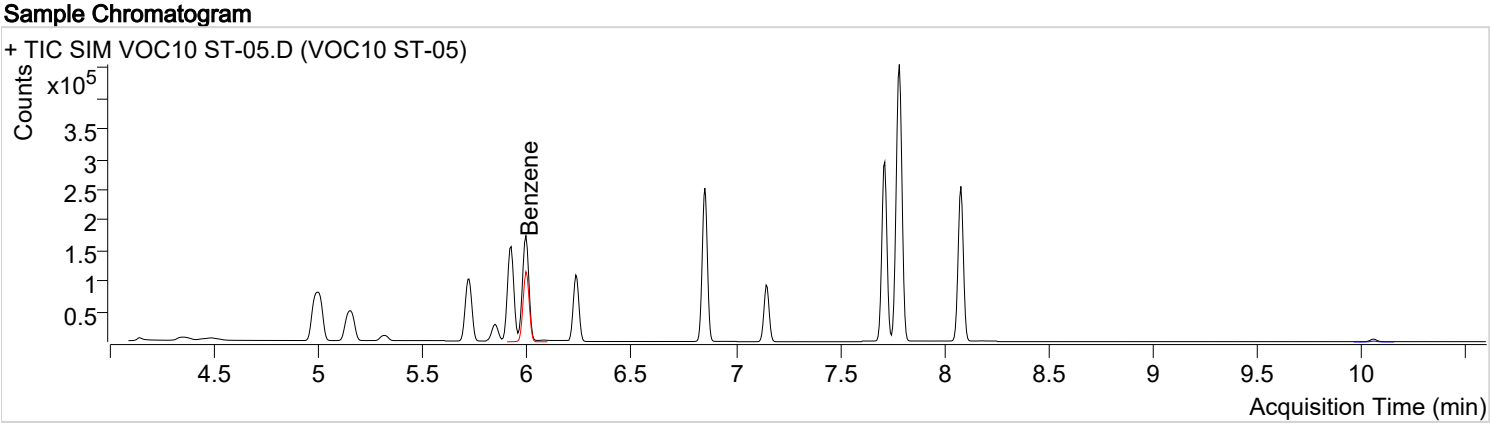

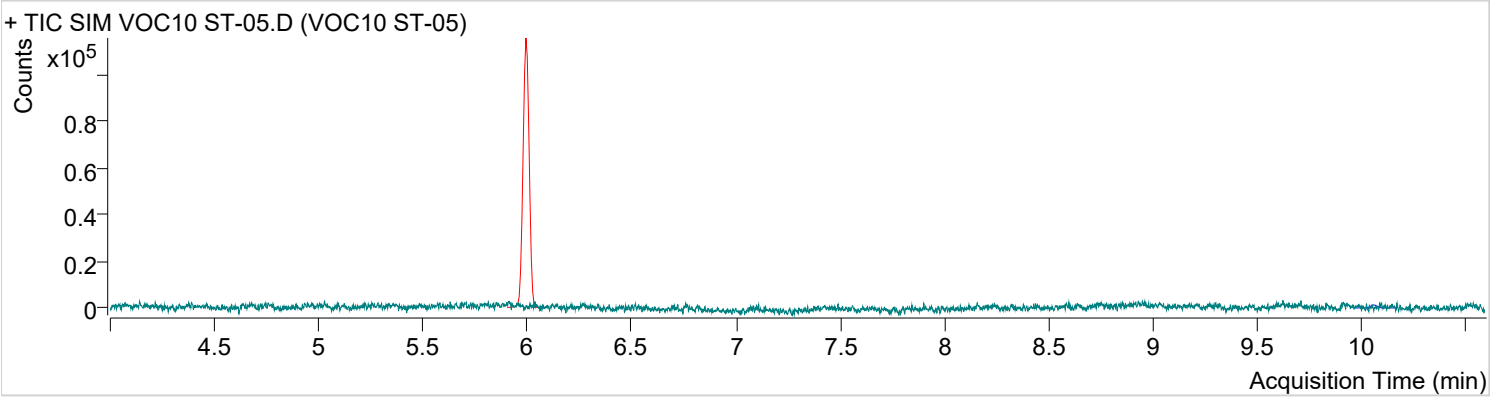

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene	5.993	235264	2769	0.198 mg/L

Benzene

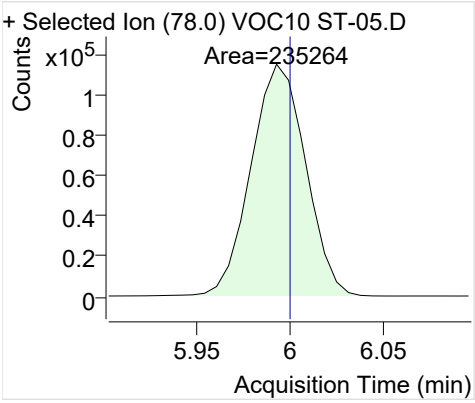

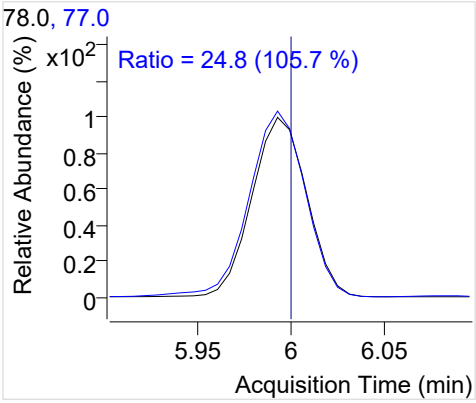

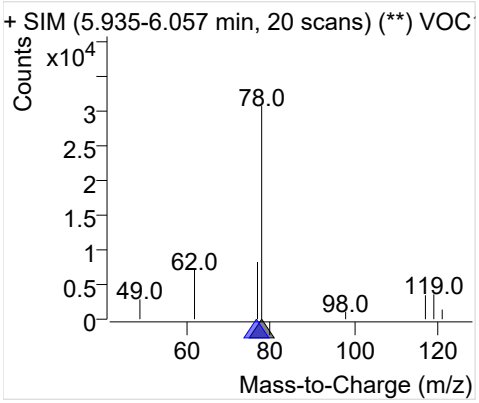

Generated at 오전 11:08 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\VOC10(JR 2.20)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-02-24 오전 8:45:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:08:33	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:45:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 5:51:27	**Data File**	VOC10 ST-06.D
Type	Cal	**Name**	VOC10 ST-06
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

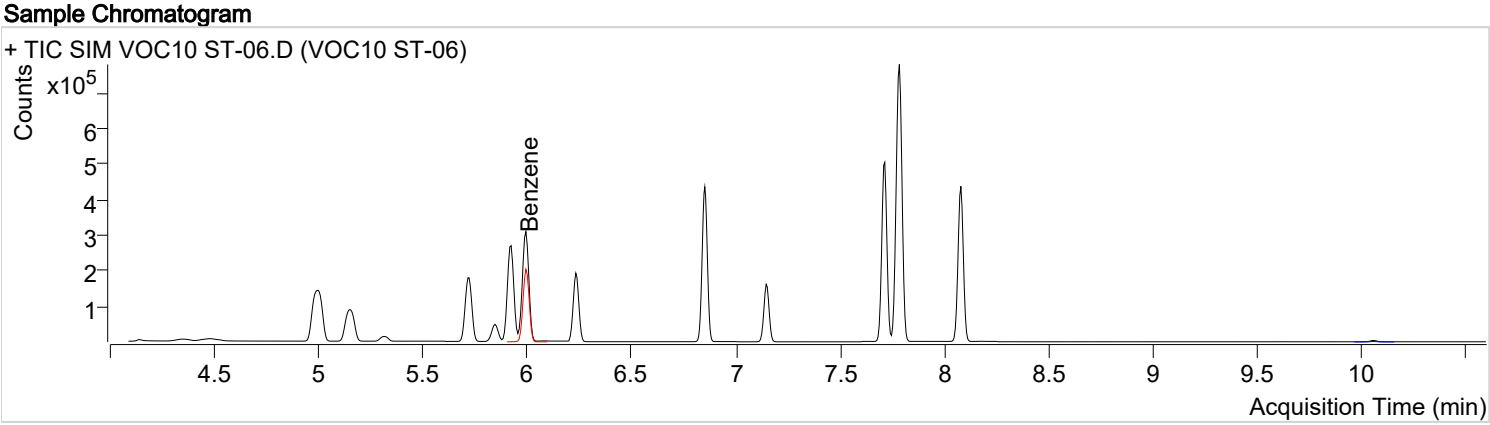

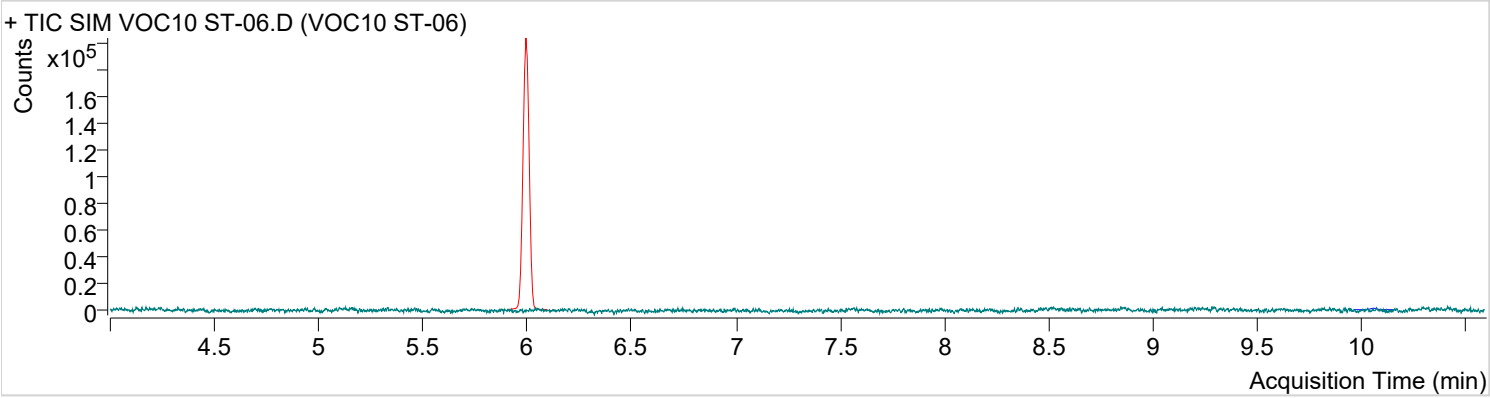

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene	5.993	419138	2410	0.401 mg/L

Benzene

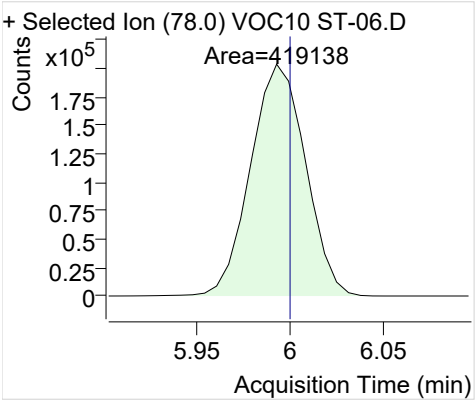

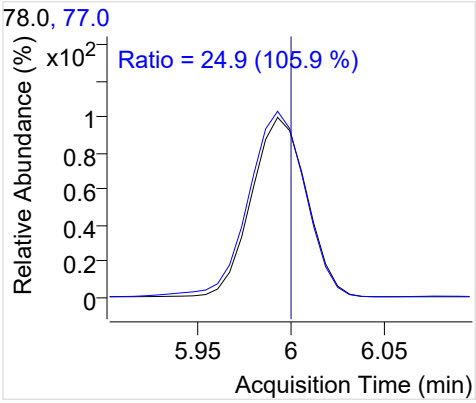

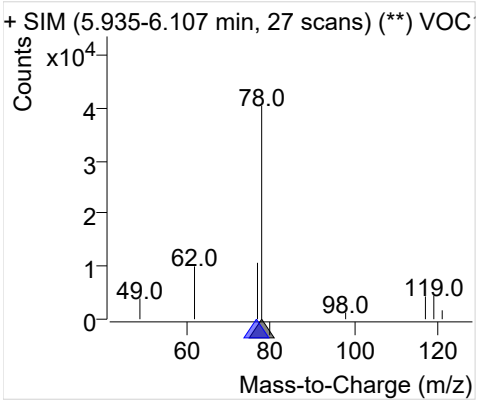

Generated at 오전 11:08 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\VOC10(JR 2.20)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-02-24 오전 8:45:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:08:33	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:45:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 6:16:57	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

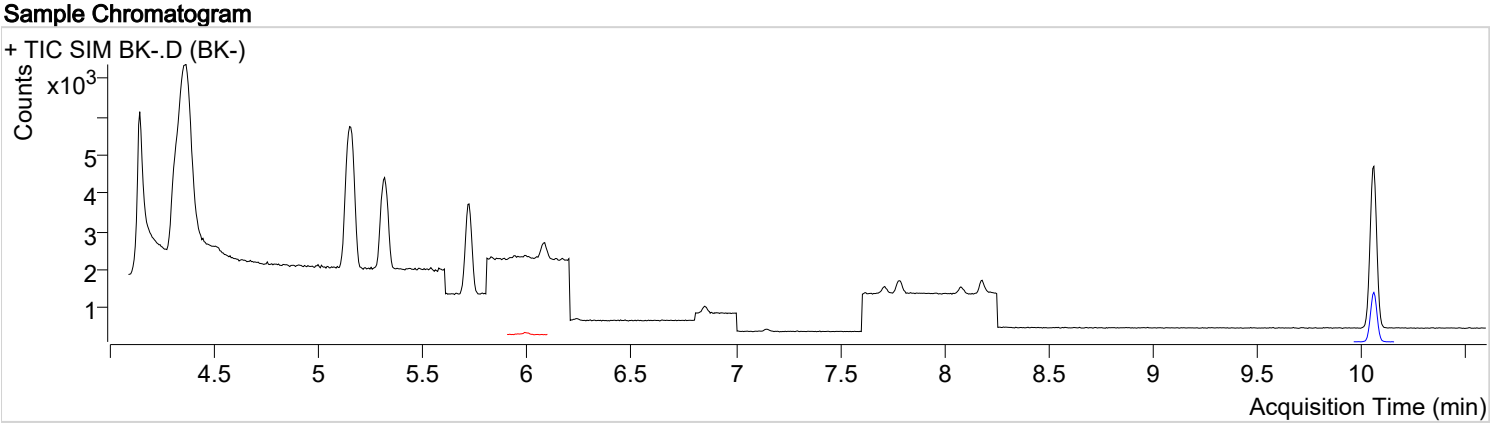

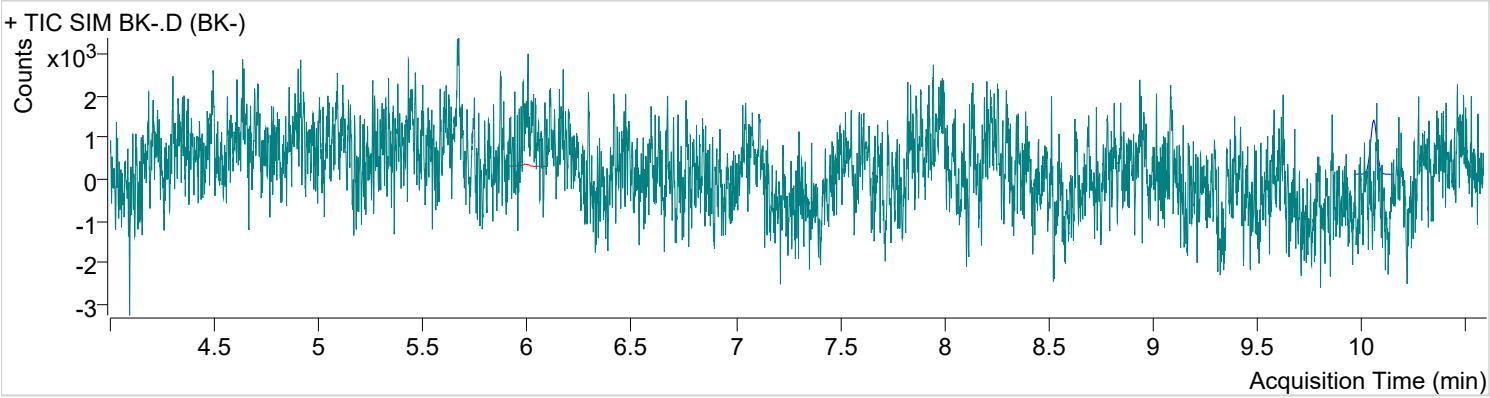

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene			2849	ND mg/L

Benzene

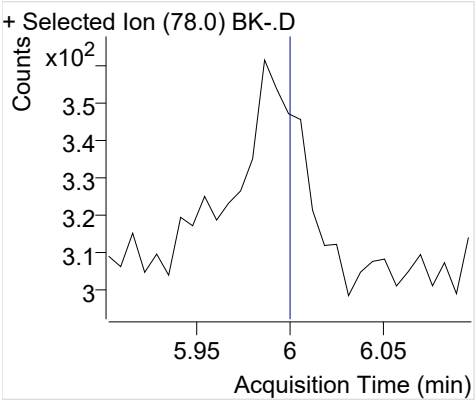

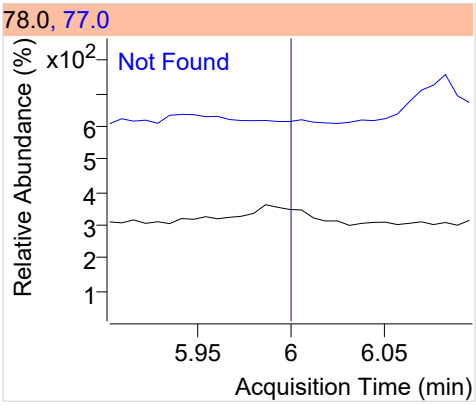

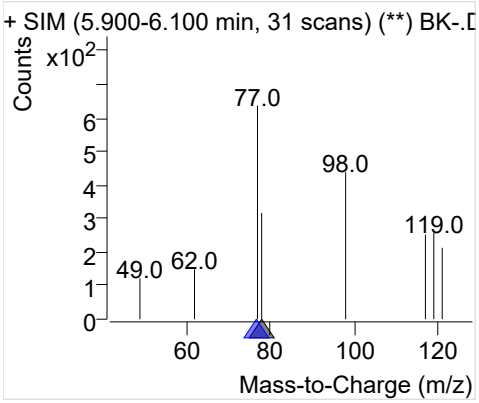

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\VOC10(JR 2.20)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-02-24 오전 8:45:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:08:33	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:45:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 6:29:41	**Data File**	JR 26-02-20.D
Type	Sample	**Name**	JR 26-02-20
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

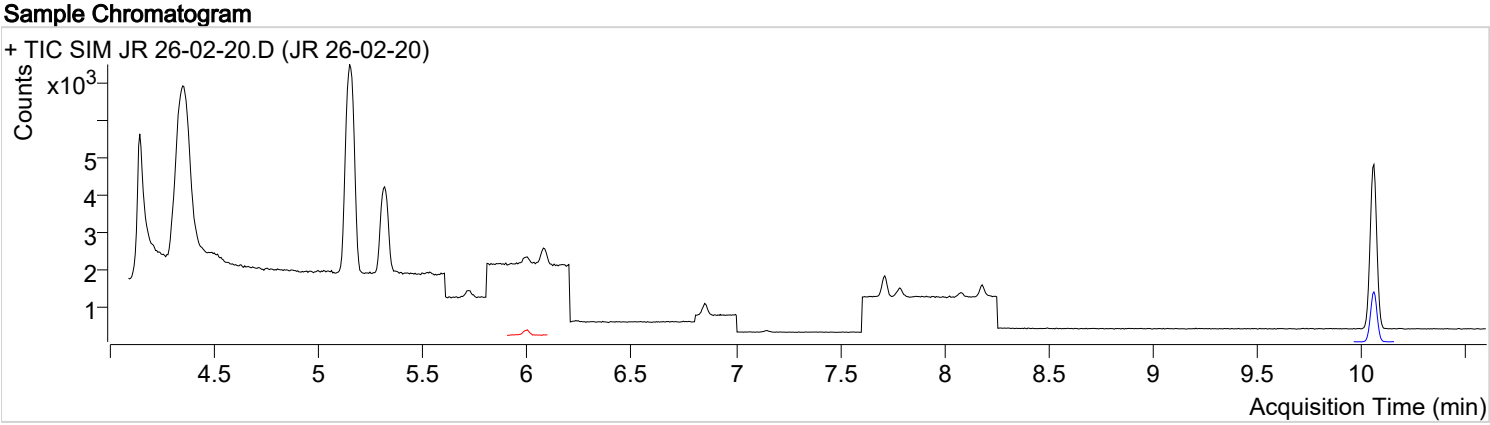

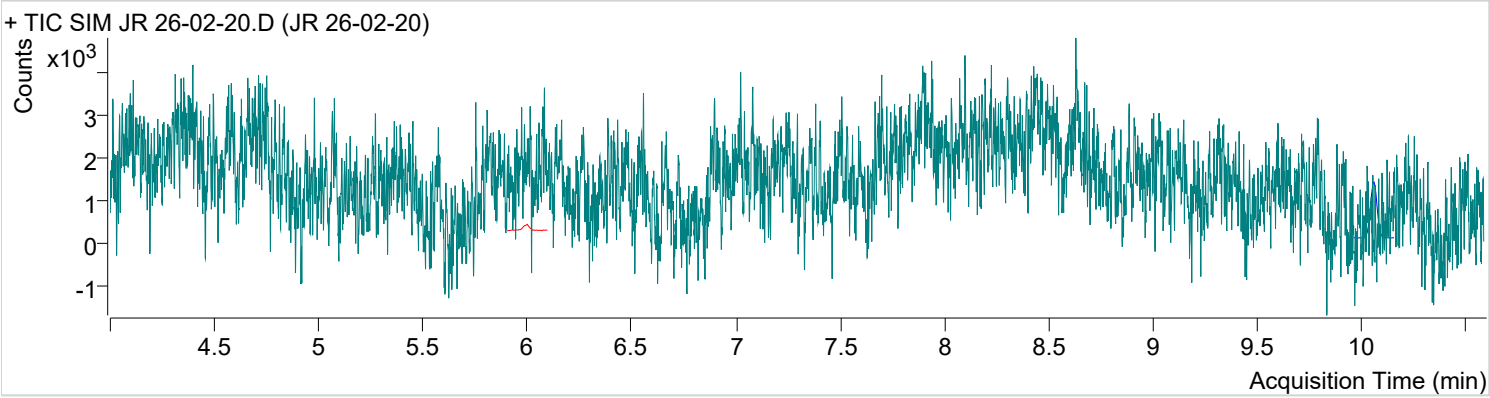

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene			2941	ND mg/L

Benzene

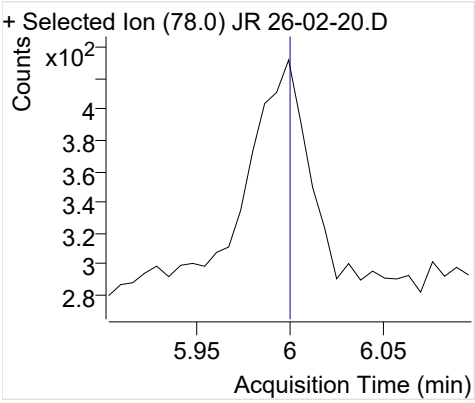

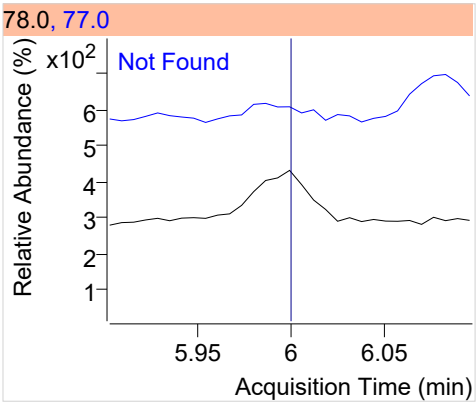

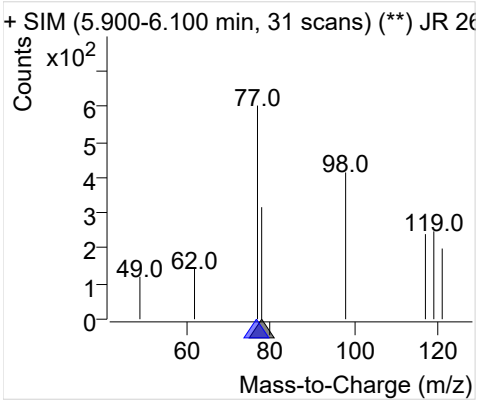

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\VOC10(JR 2.20)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-02-24 오전 8:45:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:08:33	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:45:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 6:42:25	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

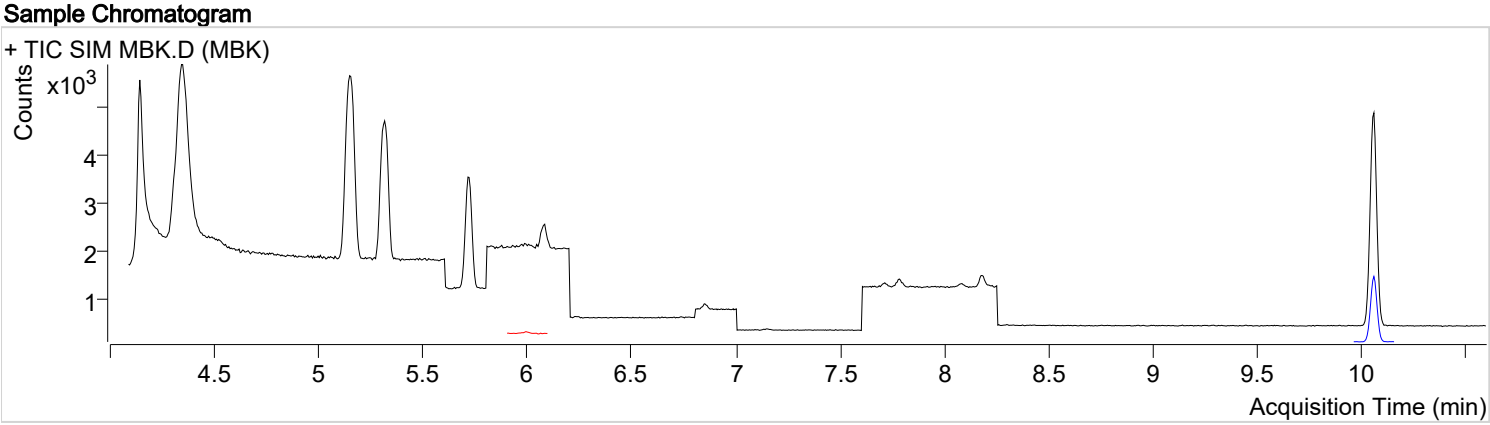

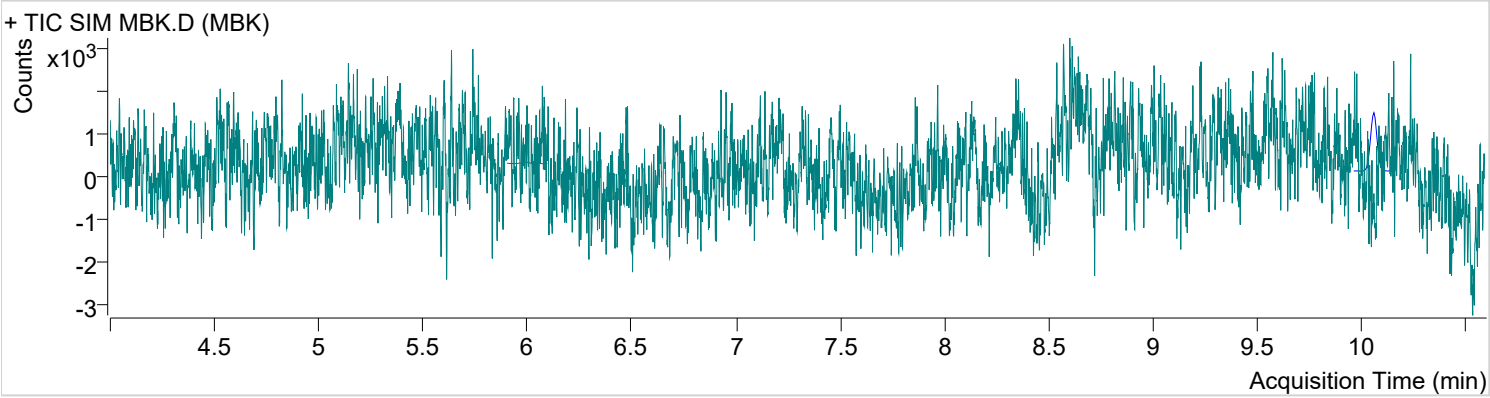

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene			2983	ND mg/L

Benzene

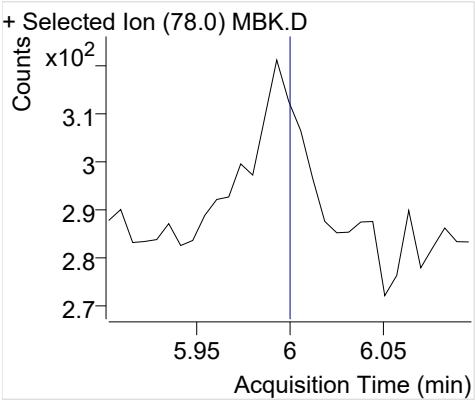

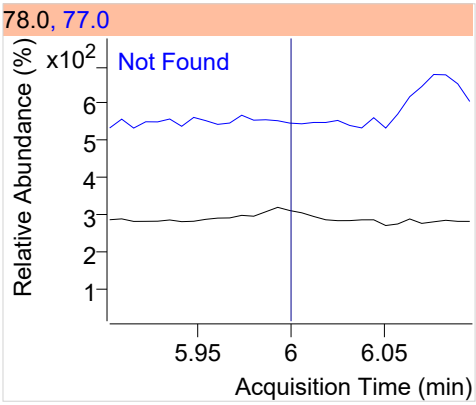

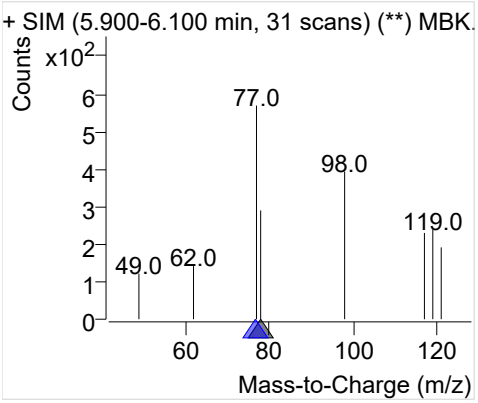

Generated at 오전 11:08 on 2026-04-10

Quant Sample Report

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\VOC10(JR 2.20)\QuantResults\VOC10.batch.bin		
Analysis Time	2026-02-24 오전 8:45:07	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:08:33	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:45:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 7:07:52	**Data File**	CCV-.D
Type	QC	**Name**	CCV-
Dil.	1	**Acq. Method File**	2025 VOCs(10) NEW

Sample Chromatogram

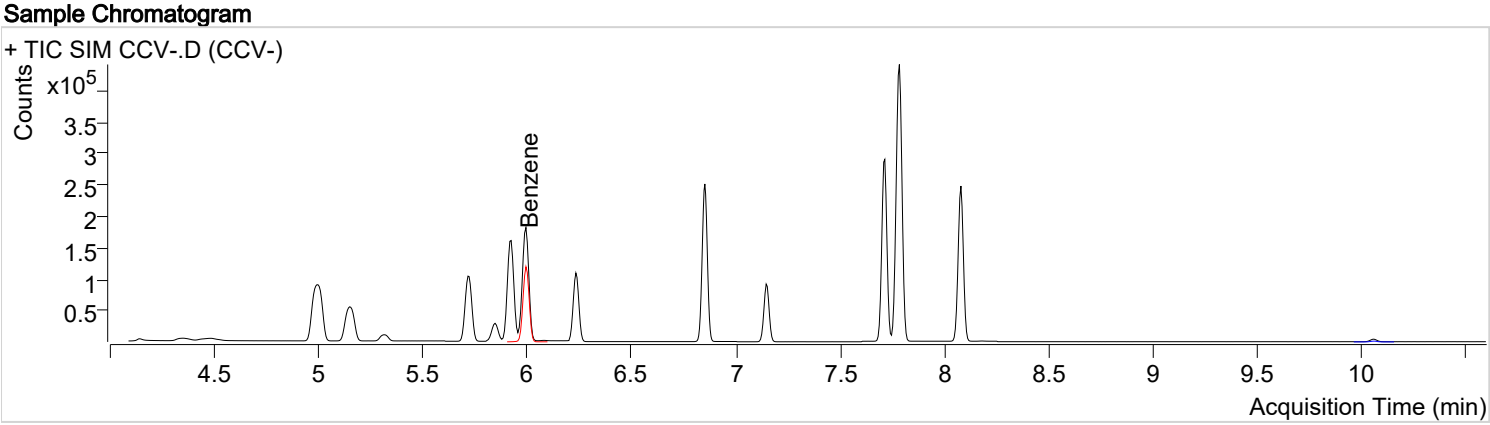

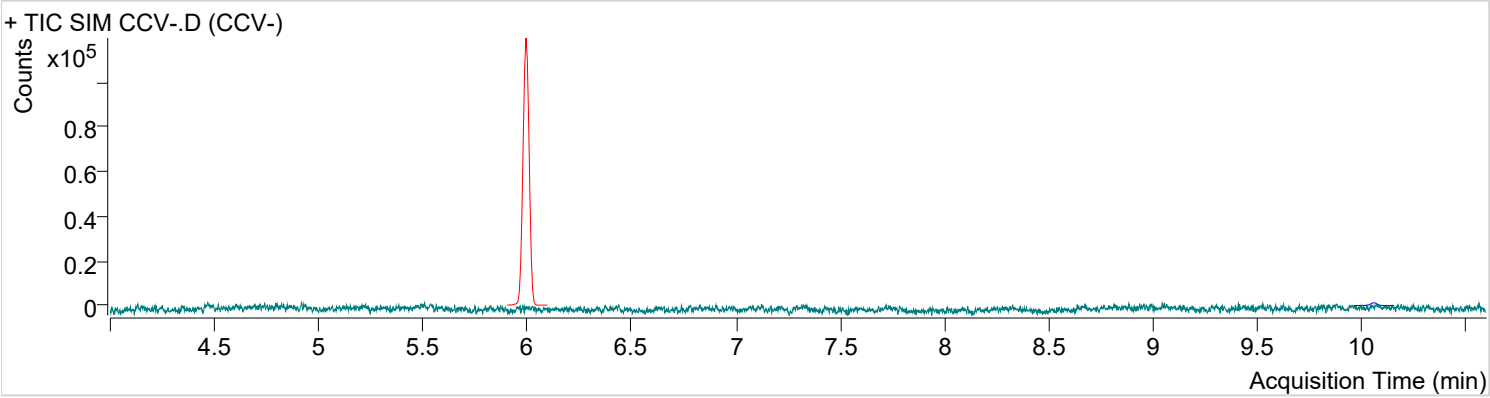

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Benzene	5.993	246198	2704	0.212 mg/L

Benzene

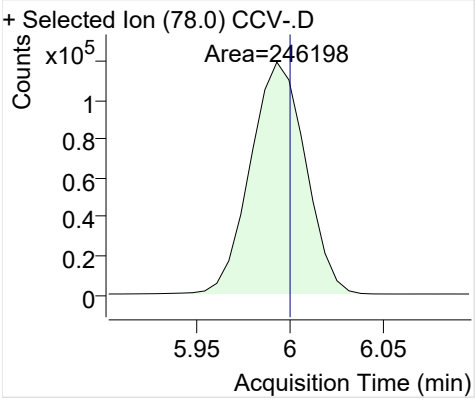

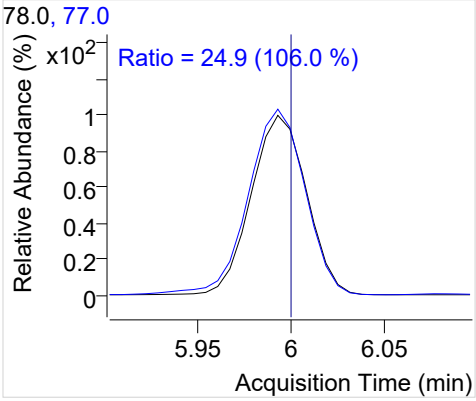

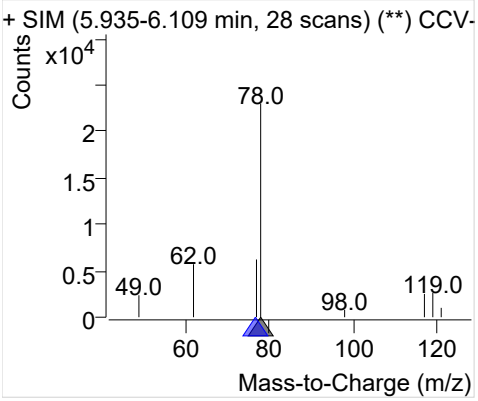

Generated at 오전 11:08 on 2026-04-10