Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(KD 1.15, HC 1.12)\QuantResults\VOC3.batch.bin				
Analysis Time	2026-01-23 오후 4:06:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-23 오후 4:06:05	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Vinylchloride

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
VOC3 ST-01.D	Cal	4.820	2213	1073	0.000
VOC3 ST-02.D	Cal	4.831	7497	991	0.003
VOC3 ST-03.D	Cal	4.831	37060	875	0.057
VOC3 ST-04.D	Cal	4.831	75725	1090	0.099
VOC3 ST-05.D	Cal	4.831	133000	878	0.226
VOC3 ST-06.D	Cal	4.831	319559	1252	0.387
BK-.D	Blank			1179	ND
FBK(HC 25-01-12).D	Blank			1164	ND
HC 25-01-12.D	Sample	4.831	14998	1136	0.011
MBK.D	Blank			1171	ND
-CCV-.D	QC	4.831	138031	1074	0.190

Vinylchloride

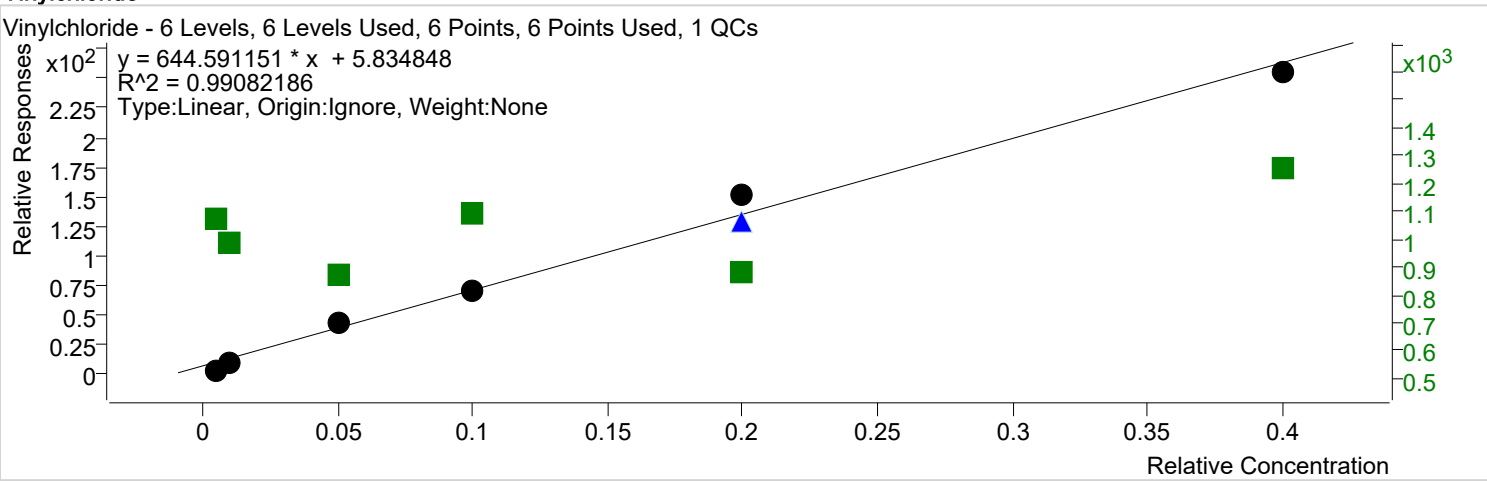

Cal. Path	Type	Level	Enable	Conc.	Response
D:\DATA\2026년\1. 2026년 1월 \VOC3(KD 1.15, HC 1.12)\VOC3 ST-01.D	Calibration	1	x	0.005	2213
D:\DATA\2026년\1. 2026년 1월 \VOC3(KD 1.15, HC 1.12)\VOC3 ST-02.D	Calibration	2	x	0.010	7497
D:\DATA\2026년\1. 2026년 1월 \VOC3(KD 1.15, HC 1.12)\VOC3 ST-03.D	Calibration	3	x	0.050	37060
D:\DATA\2026년\1. 2026년 1월 \VOC3(KD 1.15, HC 1.12)\VOC3 ST-04.D	Calibration	4	x	0.100	75725
D:\DATA\2026년\1. 2026년 1월 \VOC3(KD 1.15, HC 1.12)\VOC3 ST-05.D	Calibration	5	x	0.200	133000
D:\DATA\2026년\1. 2026년 1월 \VOC3(KD 1.15, HC 1.12)\-CCV-.D	QC	5	x	0.200	138031
D:\DATA\2026년\1. 2026년 1월 \VOC3(KD 1.15, HC 1.12)\VOC3 ST-06.D	Calibration	6	x	0.400	319559

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(KD 1.15, HC 1.12)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-23 오후 4:06:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:28:55	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-23 오후 4:06:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-18 오전 11:44:26	**Data File**	VOC3 ST-01.D
Type	Cal	**Name**	VOC3 ST-01
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

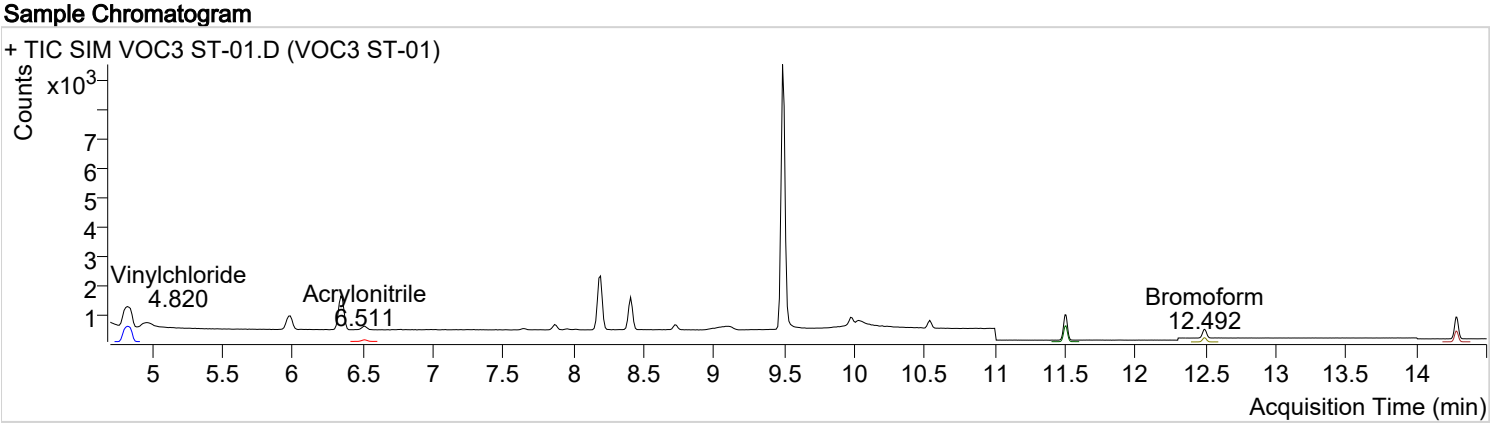

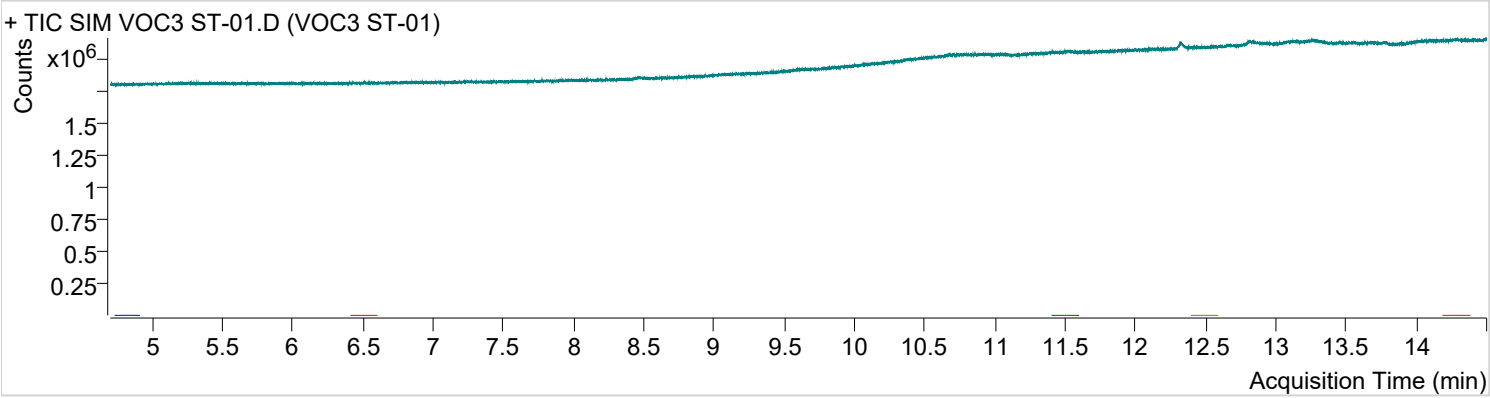

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.820	2213	1073	0.000 mg/L

Vinylchloride





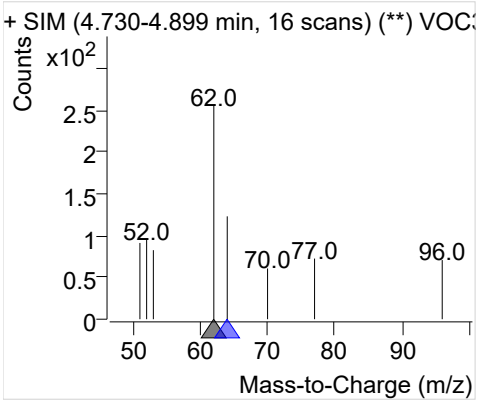

Generated at 오전 11:28 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(KD 1.15, HC 1.12)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-23 오후 4:06:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:28:55	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-23 오후 4:06:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-18 오후 12:02:08	**Data File**	VOC3 ST-02.D
Type	Cal	**Name**	VOC3 ST-02
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

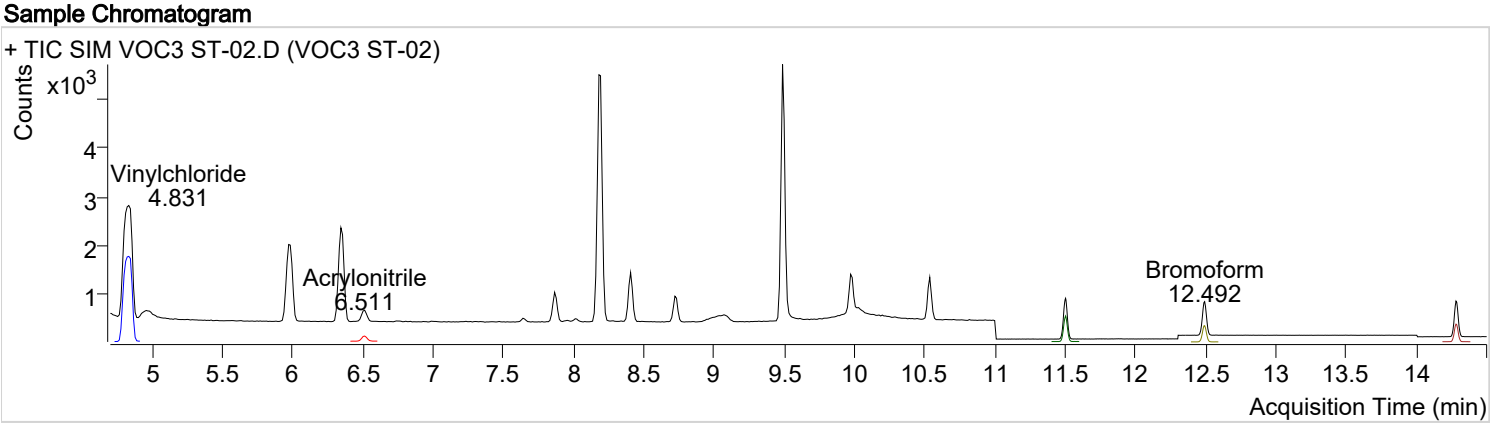

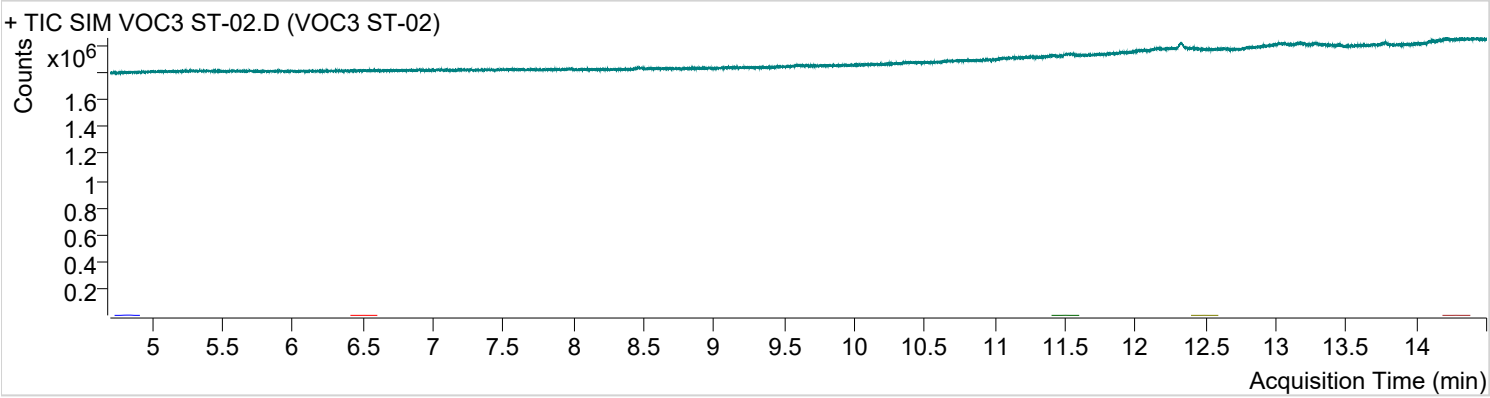

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.831	7497	991	0.003 mg/L

Vinylchloride





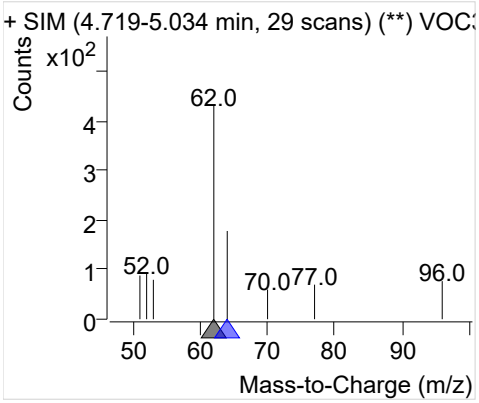

Generated at 오전 11:28 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(KD 1.15, HC 1.12)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-23 오후 4:06:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:28:55	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-23 오후 4:06:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-18 오후 12:19:51	**Data File**	VOC3 ST-03.D
Type	Cal	**Name**	VOC3 ST-03
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

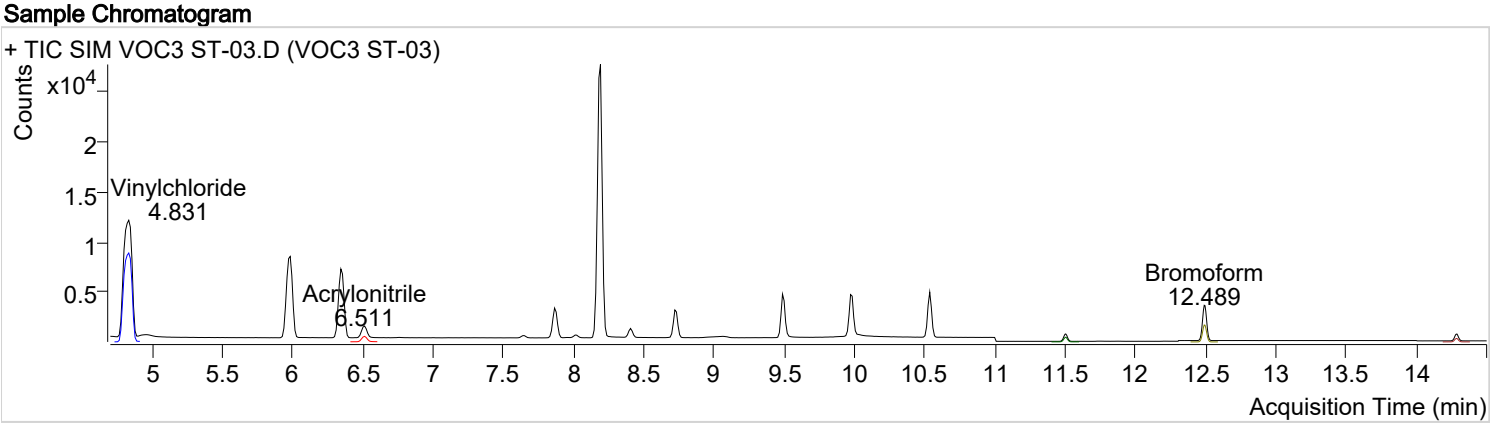

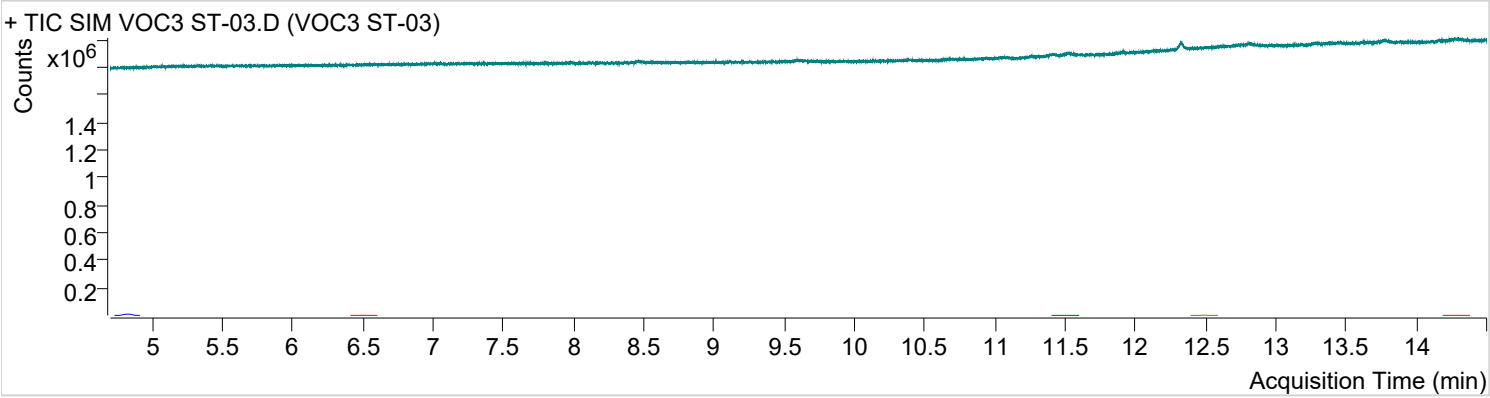

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.831	37060	875	0.057 mg/L

Vinylchloride





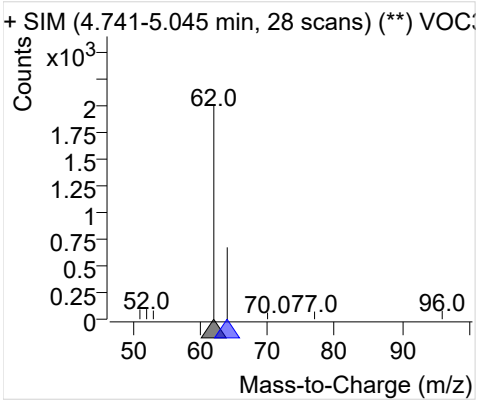

Generated at 오전 11:28 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(KD 1.15, HC 1.12)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-23 오후 4:06:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:28:55	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-23 오후 4:06:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-18 오후 12:37:31	**Data File**	VOC3 ST-04.D
Type	Cal	**Name**	VOC3 ST-04
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

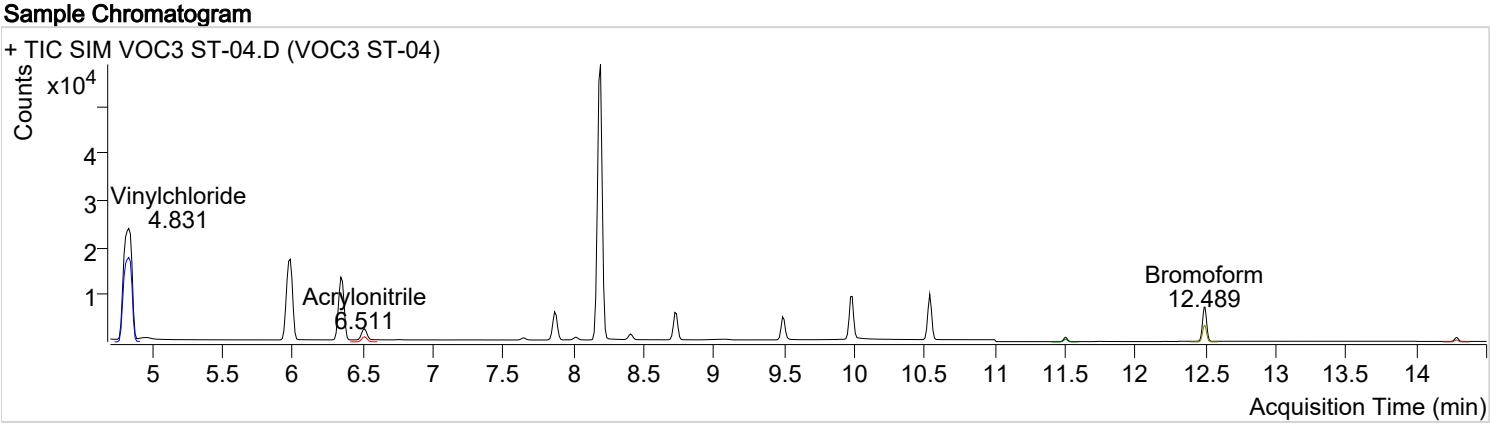

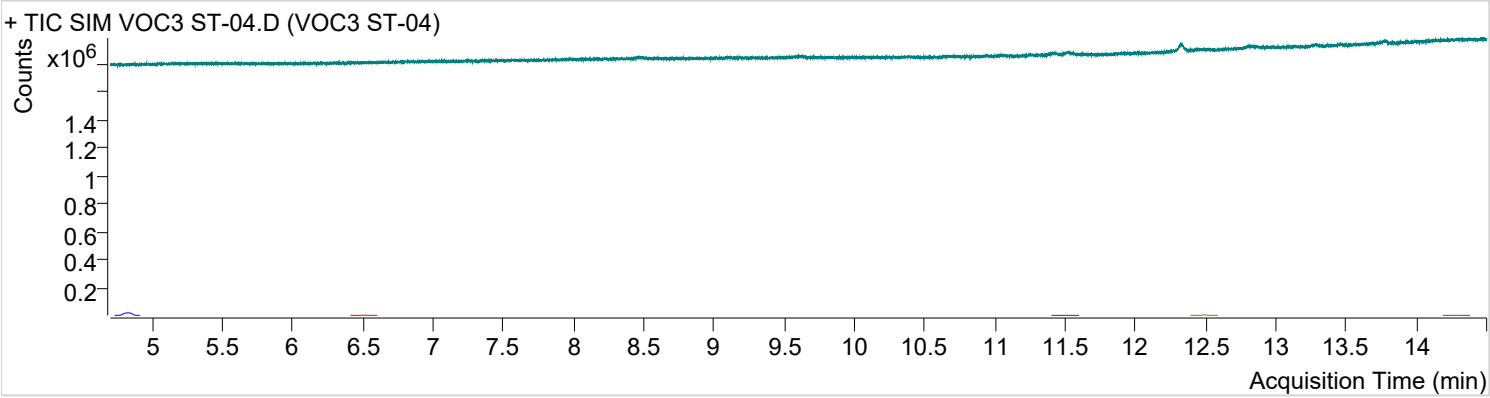

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.831	75725	1090	0.099 mg/L

Vinylchloride





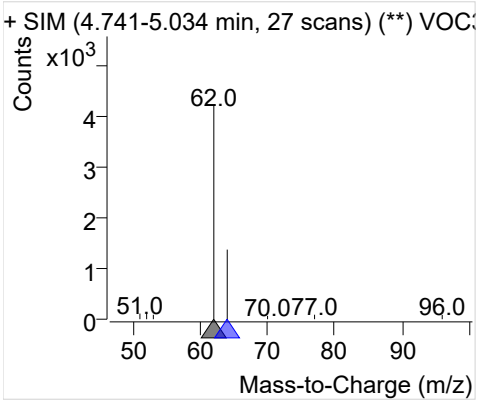

Generated at 오전 11:28 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(KD 1.15, HC 1.12)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-23 오후 4:06:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:28:55	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-23 오후 4:06:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-18 오후 12:55:14	**Data File**	VOC3 ST-05.D
Type	Cal	**Name**	VOC3 ST-05
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

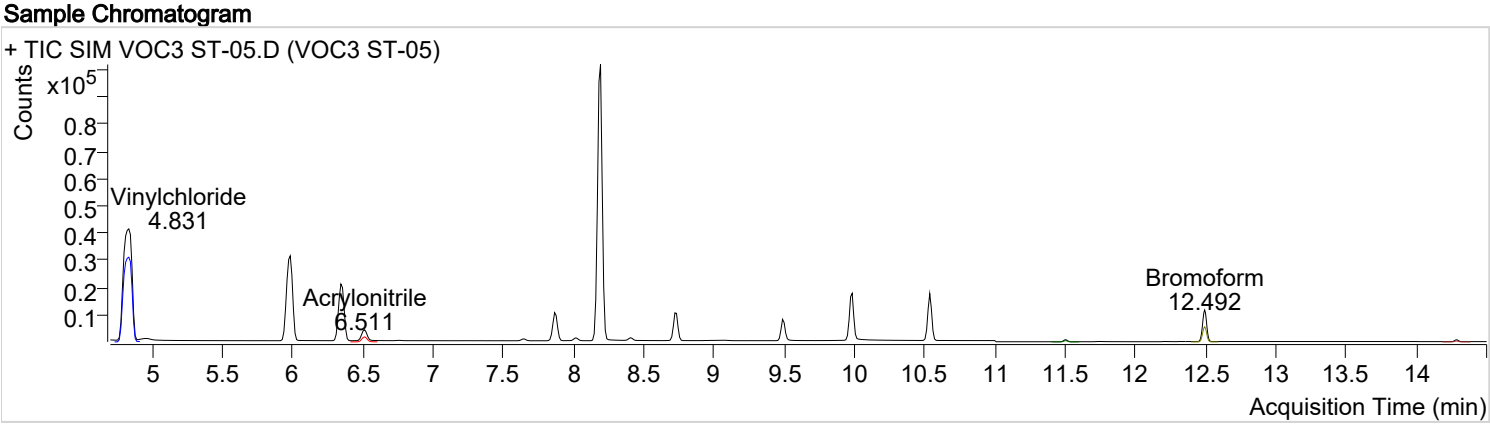

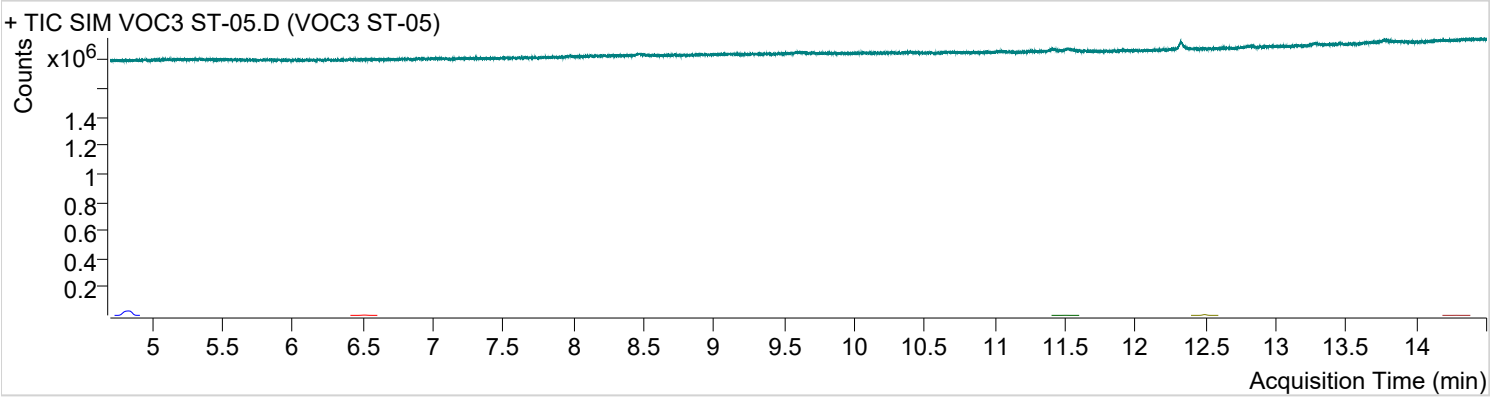

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.831	133000	878	0.226 mg/L

Vinylchloride





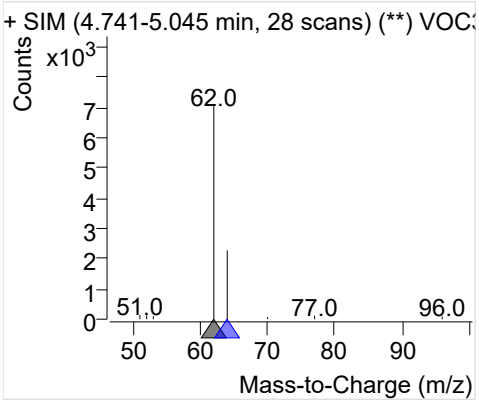

Generated at 오전 11:28 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(KD 1.15, HC 1.12)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-23 오후 4:06:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:28:55	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-23 오후 4:06:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-18 오후 1:12:57	**Data File**	VOC3 ST-06.D
Type	Cal	**Name**	VOC3 ST-06
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

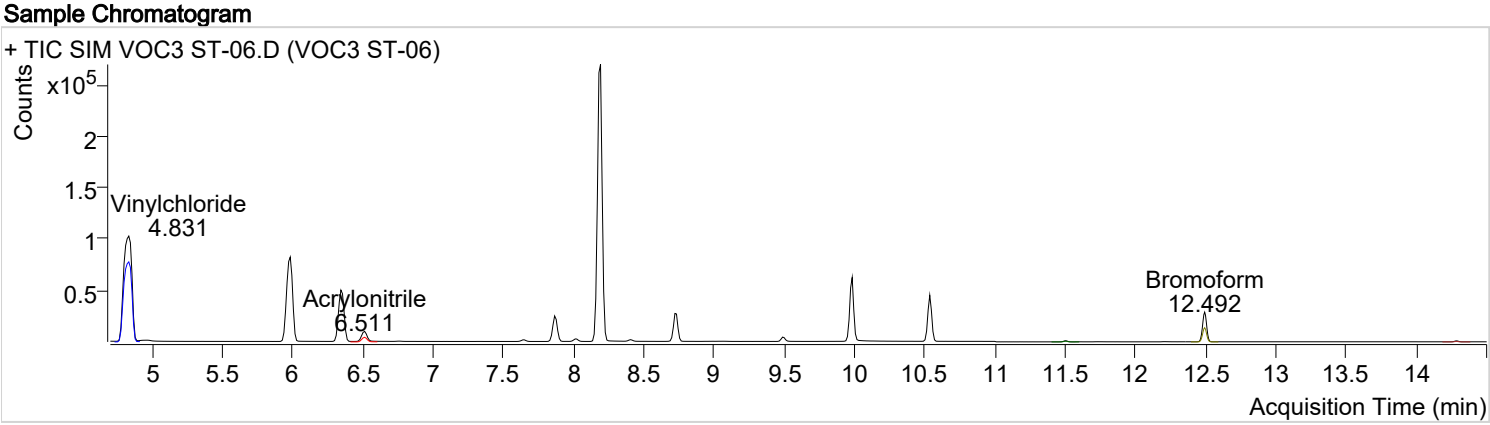

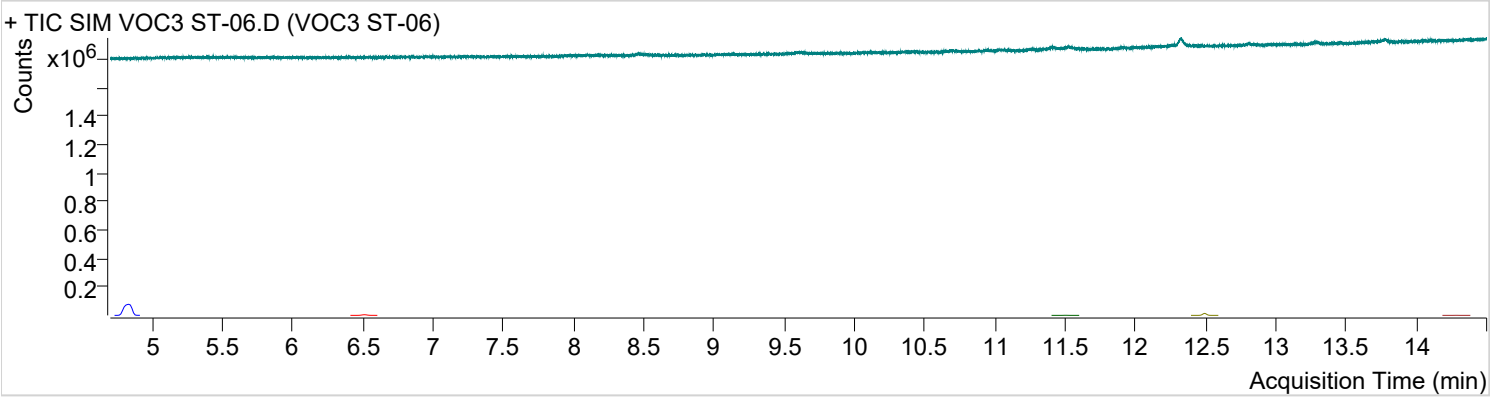

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.831	319559	1252	0.387 mg/L

Vinylchloride





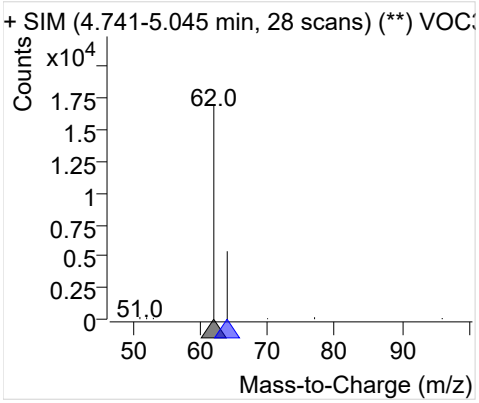

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(KD 1.15, HC 1.12)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-23 오후 4:06:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:28:55	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-23 오후 4:06:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-18 오후 1:48:20	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

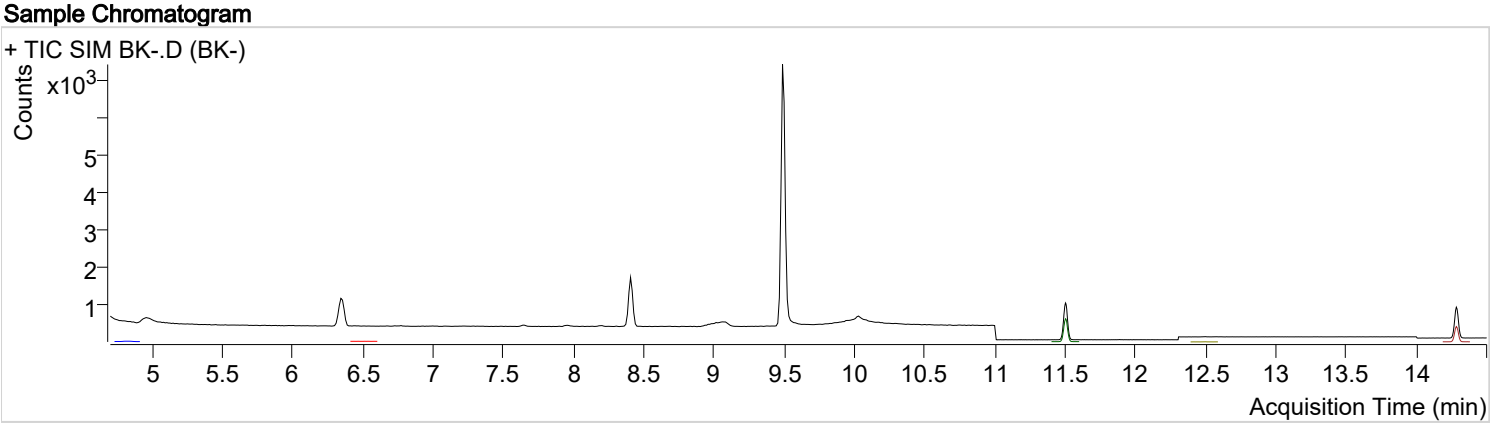

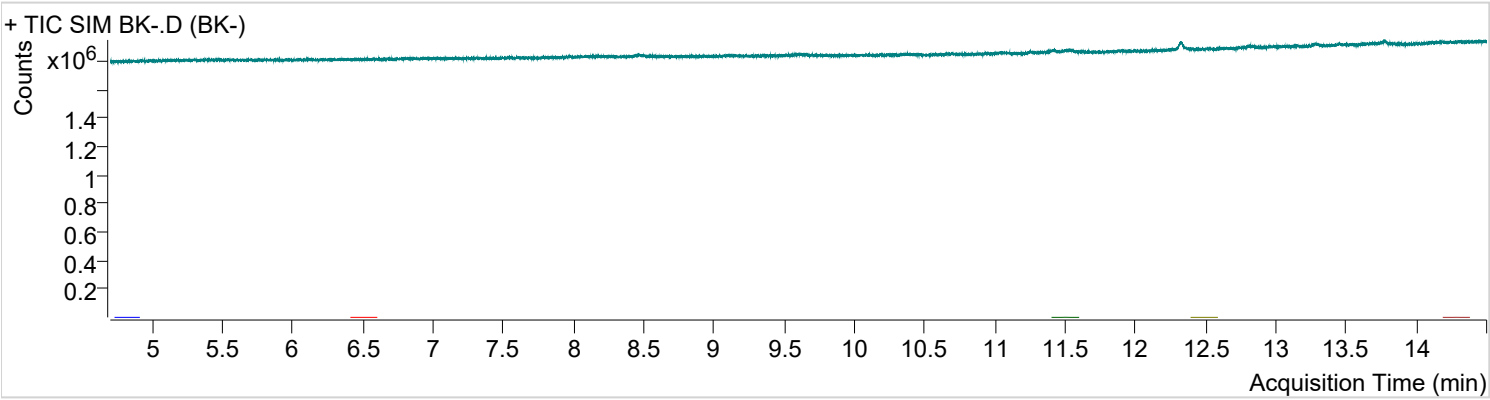

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride			1179	ND mg/L

Vinylchloride





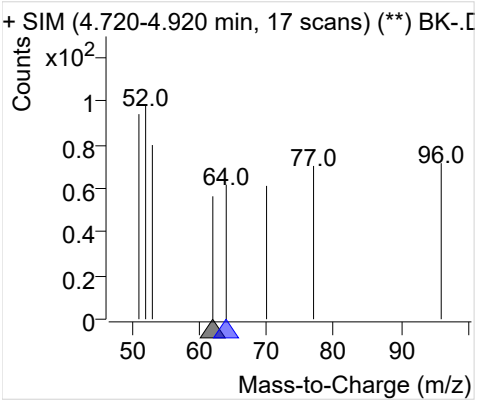

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(KD 1.15, HC 1.12)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-23 오후 4:06:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:28:55	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-23 오후 4:06:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-18 오후 2:06:03	**Data File**	FBK(HC 25-01-12).D
Type	Blank	**Name**	FBK(HC 25-01-12)
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

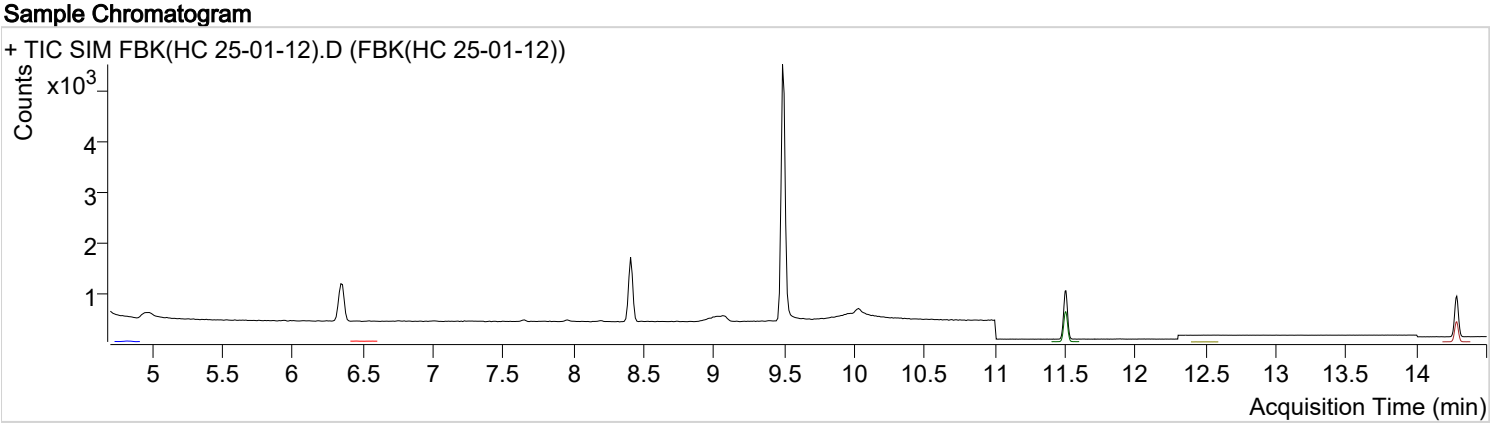

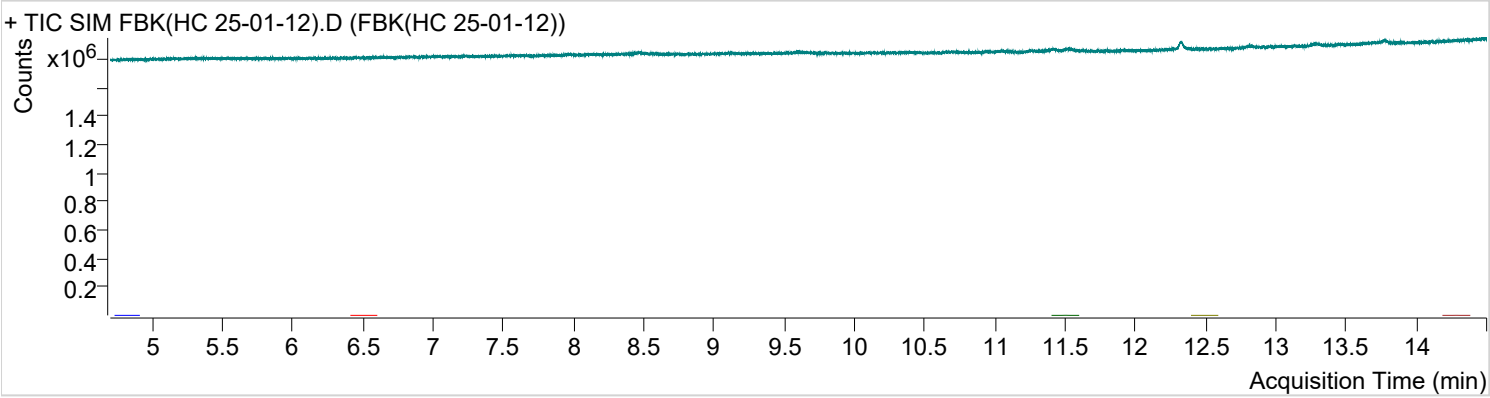

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride			1164	ND mg/L

Vinylchloride

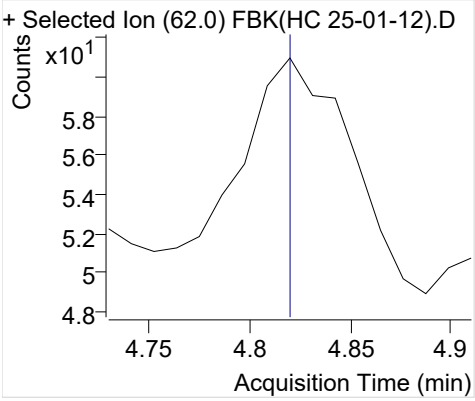



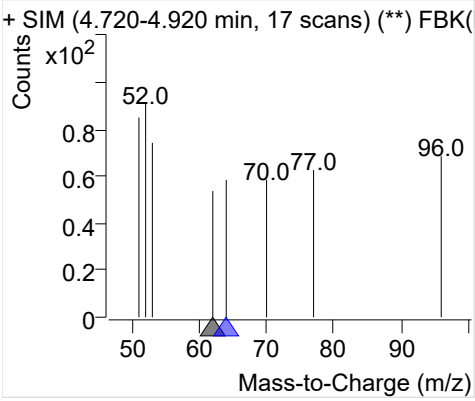

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(KD 1.15, HC 1.12)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-23 오후 4:06:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:28:55	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-23 오후 4:06:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-18 오후 2:41:27	**Data File**	HC 25-01-12.D
Type	Sample	**Name**	HC 25-01-12
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

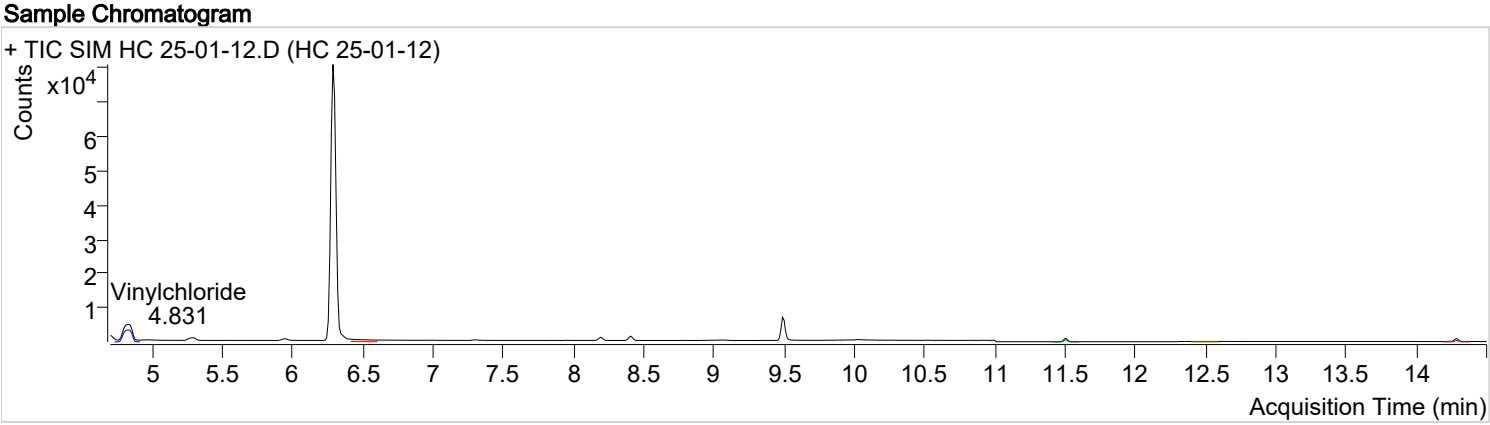

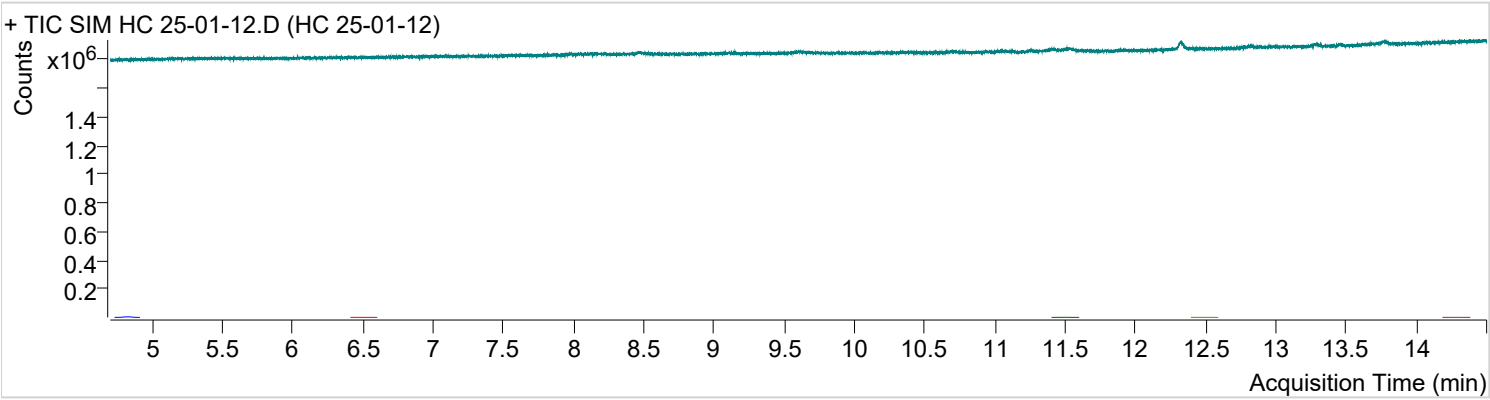

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.831	14998	1136	0.011 mg/L

Vinylchloride





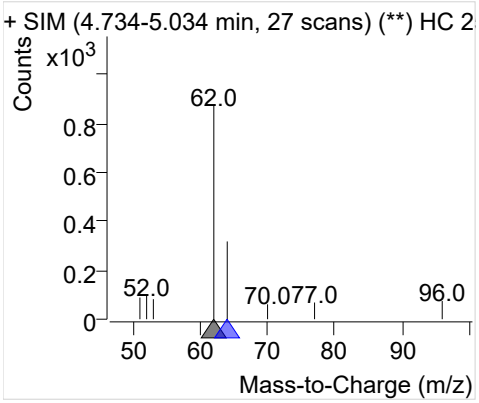

Generated at 오전 11:28 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(KD 1.15, HC 1.12)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-23 오후 4:06:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:28:55	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-23 오후 4:06:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-18 오후 3:16:43	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

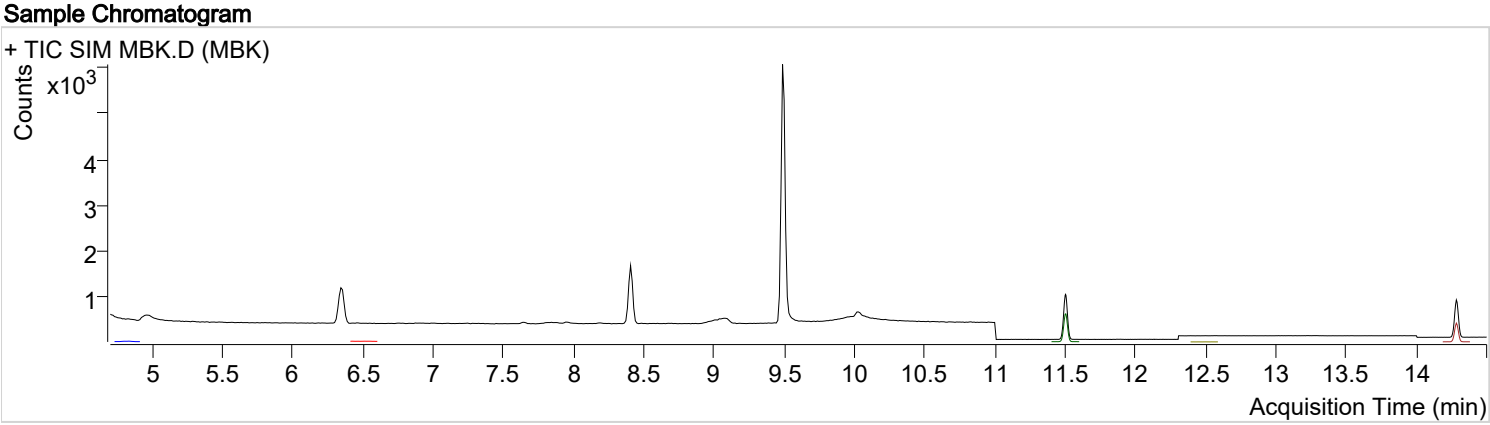

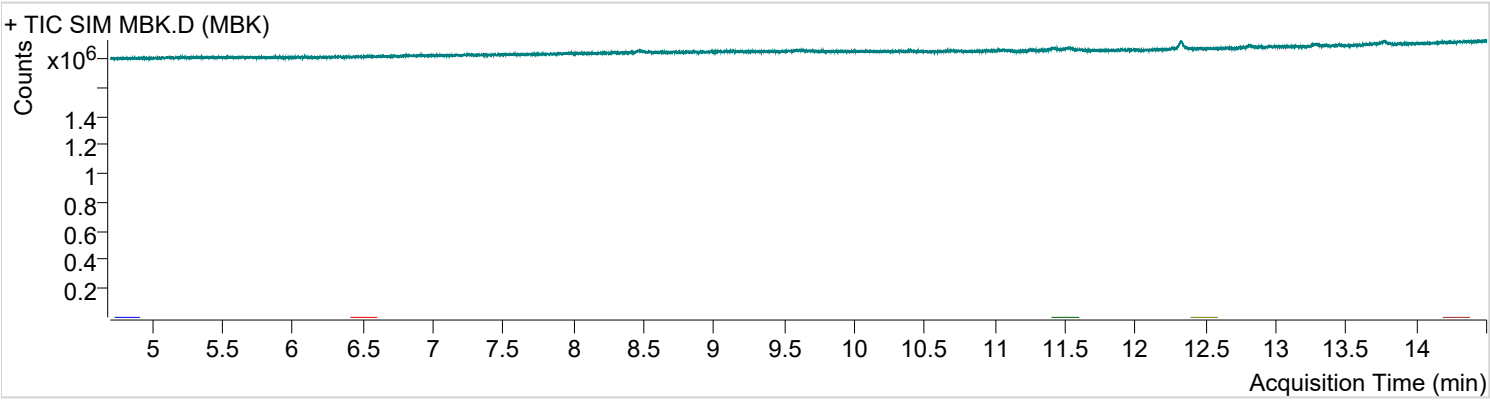

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride			1171	ND mg/L

Vinylchloride





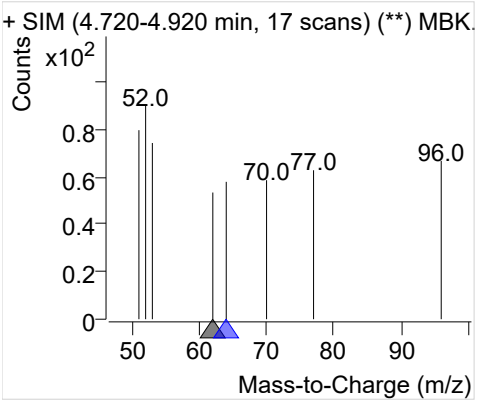

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(KD 1.15, HC 1.12)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-23 오후 4:06:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:28:55	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-23 오후 4:06:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-18 오후 3:52:09	**Data File**	-CCV-.D
Type	QC	**Name**	-CCV-
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

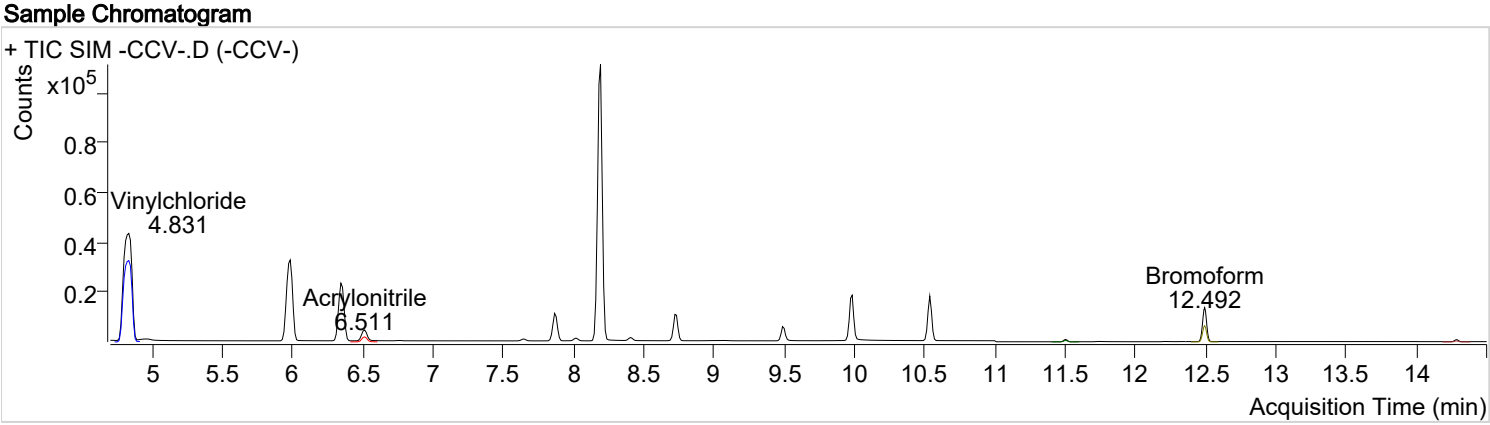

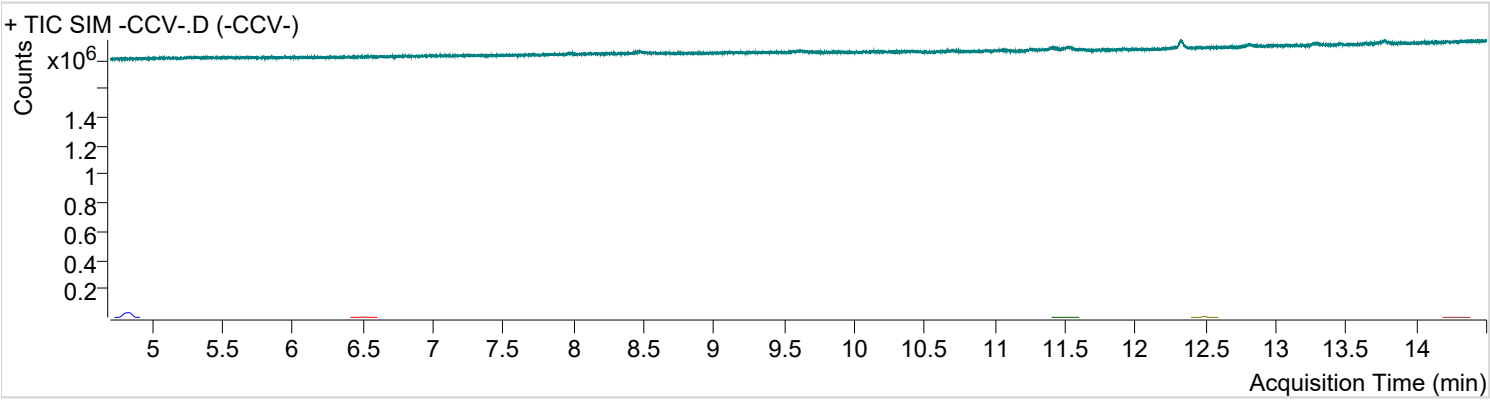

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.831	138031	1074	0.190 mg/L

Vinylchloride





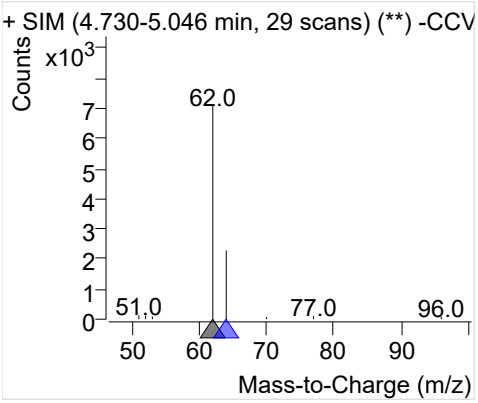

Generated at 오전 11:28 on 2026-04-10