Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 1.22, 1.26)\QuantResults\VOC3.batch.bin				
Analysis Time	2026-02-02 오후 3:22:38	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-02 오후 3:22:38	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Vinylchloride

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
VOC3 ST-01.D	Cal	4.831	4563	1825	0.000
VOC3 ST-02.D	Cal	4.831	9104	1872	0.004
VOC3 ST-03.D	Cal	4.831	40559	1568	0.051
VOC3 ST-04.D	Cal	4.831	80325	1549	0.108
VOC3 ST-05.D	Cal	4.831	163465	1671	0.209
VOC3 ST-06.D	Cal	4.831	310646	1711	0.394
BK-.D	Blank			1736	ND
FBK(HC 26-01-26) .D	Blank			1358	ND
LDPE 26-01-26.D	Sample	4.831	0	1236	ND
MBK-1.D	Blank			1009	ND
-CCV-1.D	QC	4.831	134544	1553	0.184

Vinylchloride

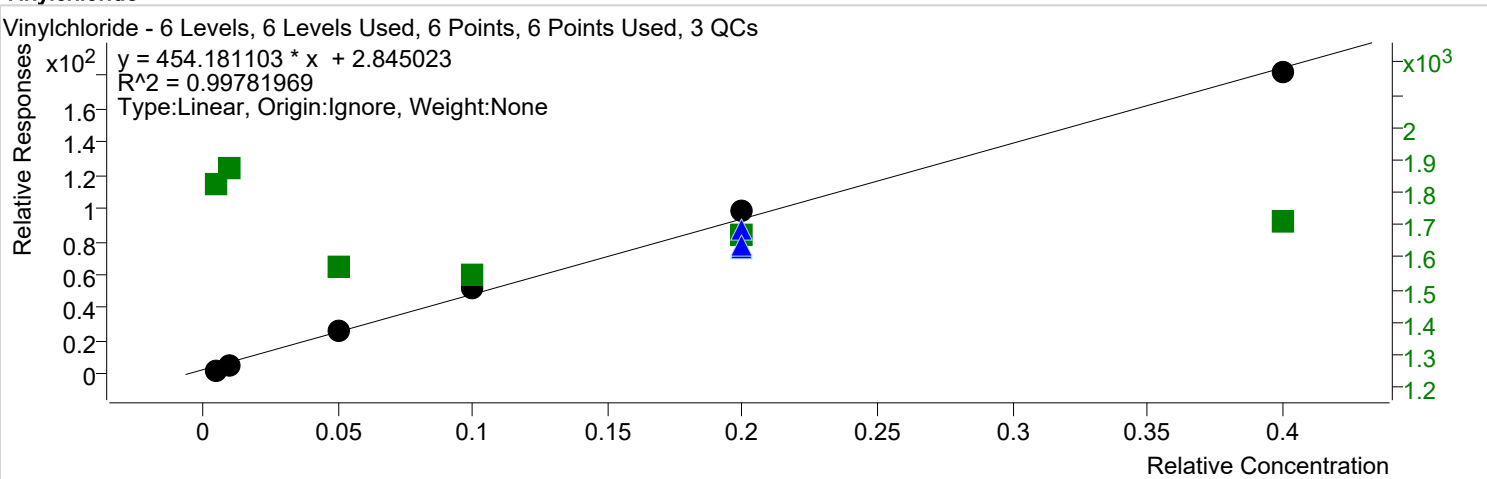

Cal. Path	Type	Level	Enable	Conc.	Response
D:\DATA\2026년\1. 2026년 1월 \VOC3(HC 1.22, 1.26)\VOC3 ST-01.D	Calibration	1	x	0.005	4563
D:\DATA\2026년\1. 2026년 1월 \VOC3(HC 1.22, 1.26)\VOC3 ST-02.D	Calibration	2	x	0.010	9104
D:\DATA\2026년\1. 2026년 1월 \VOC3(HC 1.22, 1.26)\VOC3 ST-03.D	Calibration	3	x	0.050	40559
D:\DATA\2026년\1. 2026년 1월 \VOC3(HC 1.22, 1.26)\VOC3 ST-04.D	Calibration	4	x	0.100	80325
D:\DATA\2026년\1. 2026년 1월 \VOC3(HC 1.22, 1.26)\VOC3 ST-05.D	Calibration	5	x	0.200	163465
D:\DATA\2026년\1. 2026년 1월 \VOC3(HC 1.22, 1.26)\-CCV-1.D	QC	5	x	0.200	134544
D:\DATA\2026년\1. 2026년 1월 \VOC3(HC 1.22, 1.26)\-CCV-2.D	QC	5	x	0.200	79949
D:\DATA\2026년\1. 2026년 1월 \VOC3(HC 1.22, 1.26)\CCV-3.D	QC	5	x	0.200	84166
D:\DATA\2026년\1. 2026년 1월 \VOC3(HC 1.22, 1.26)\VOC3 ST-06.D	Calibration	6	x	0.400	310646

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 1.22, 1.26)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-02-02 오후 3:22:38	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:24:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-02 오후 3:22:38	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-26 오후 5:55:25	**Data File**	VOC3 ST-01.D
Type	Cal	**Name**	VOC3 ST-01
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

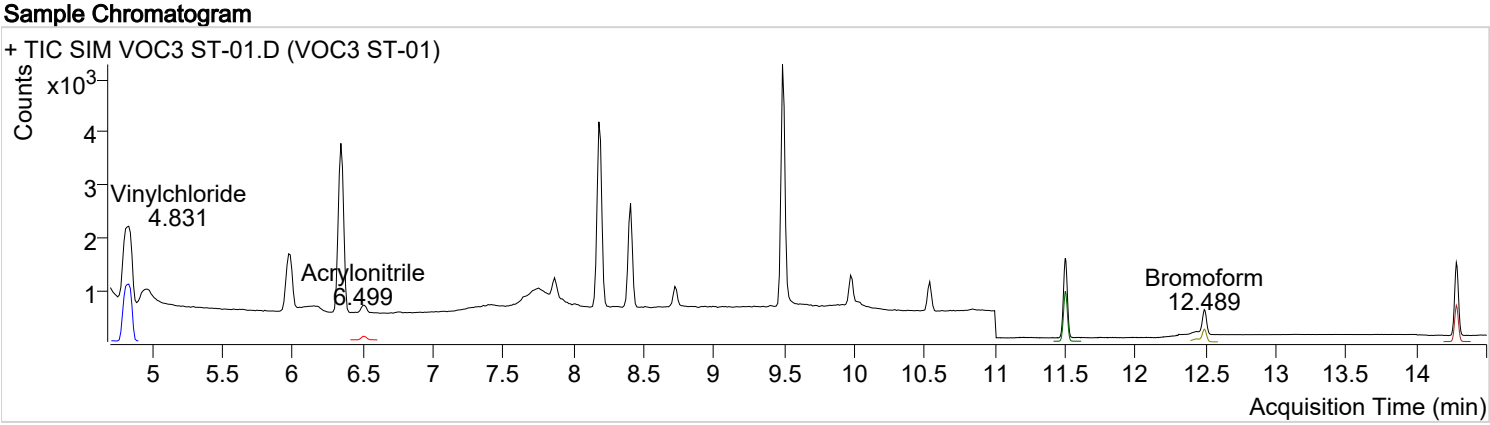

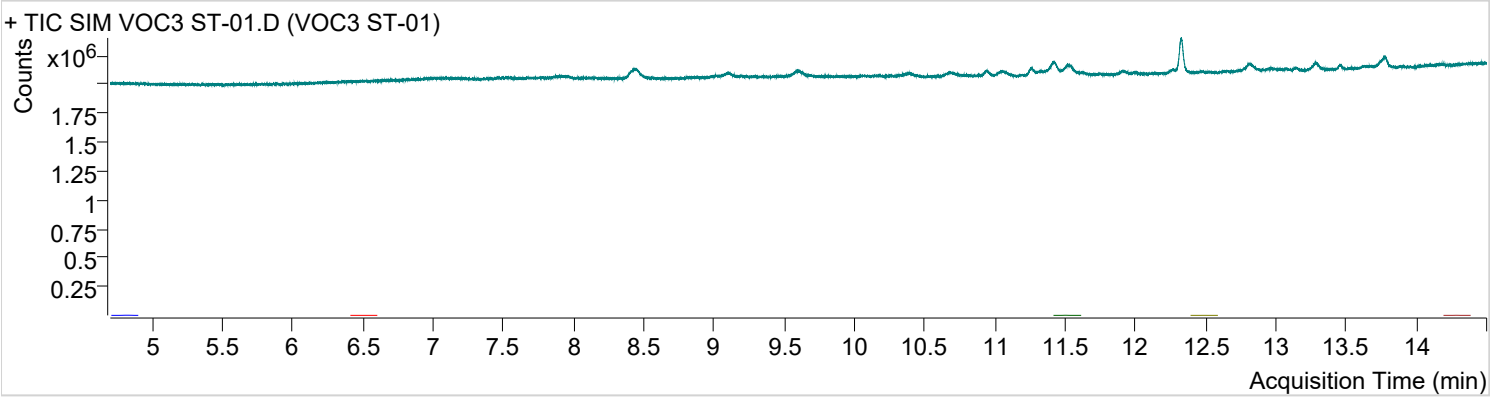

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.831	4563	1825	0.000 mg/L

Vinylchloride





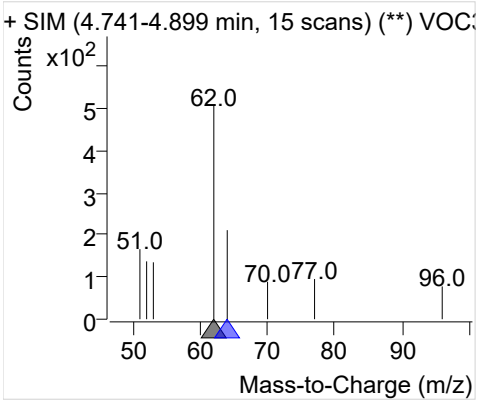

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 1.22, 1.26)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-02-02 오후 3:22:38	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:24:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-02 오후 3:22:38	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-26 오후 6:13:18	**Data File**	VOC3 ST-02.D
Type	Cal	**Name**	VOC3 ST-02
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

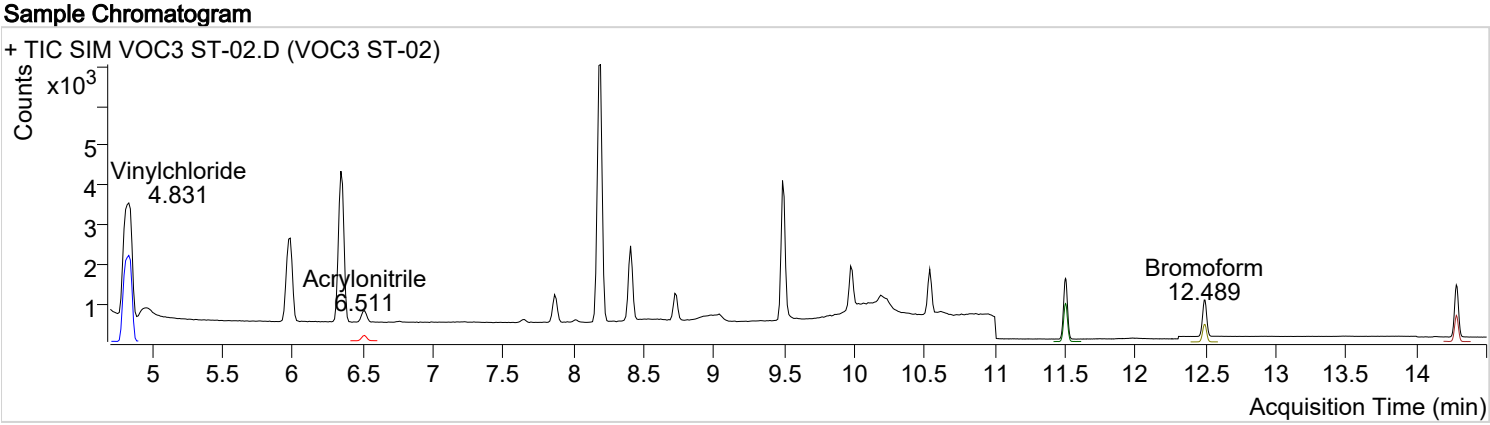

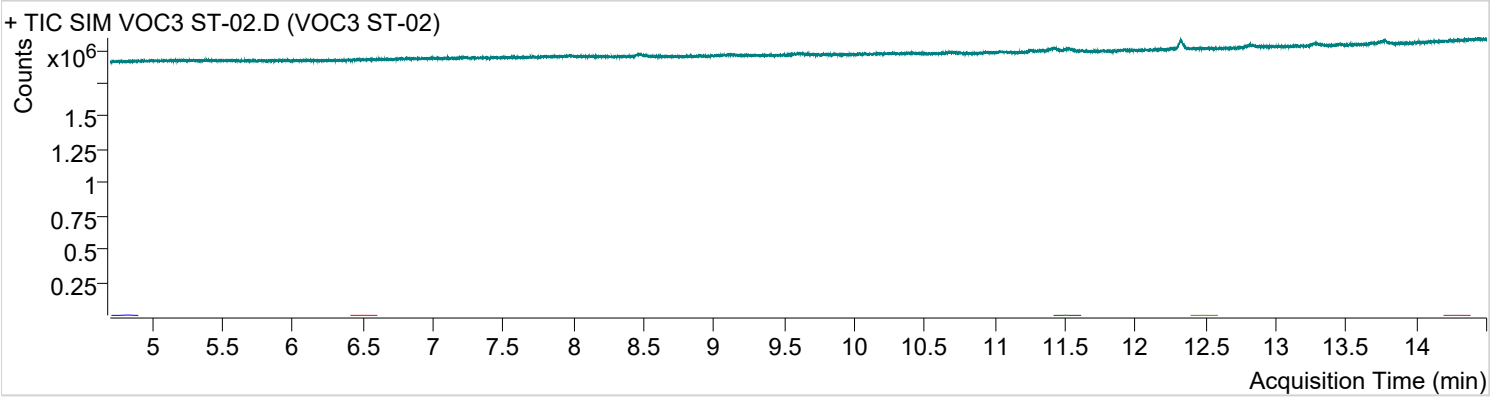

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.831	9104	1872	0.004 mg/L

Vinylchloride





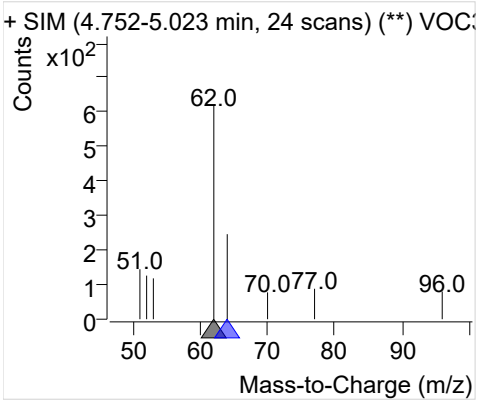

Generated at 오전 11:24 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 1.22, 1.26)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-02-02 오후 3:22:38	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:24:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-02 오후 3:22:38	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-26 오후 6:31:12	**Data File**	VOC3 ST-03.D
Type	Cal	**Name**	VOC3 ST-03
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

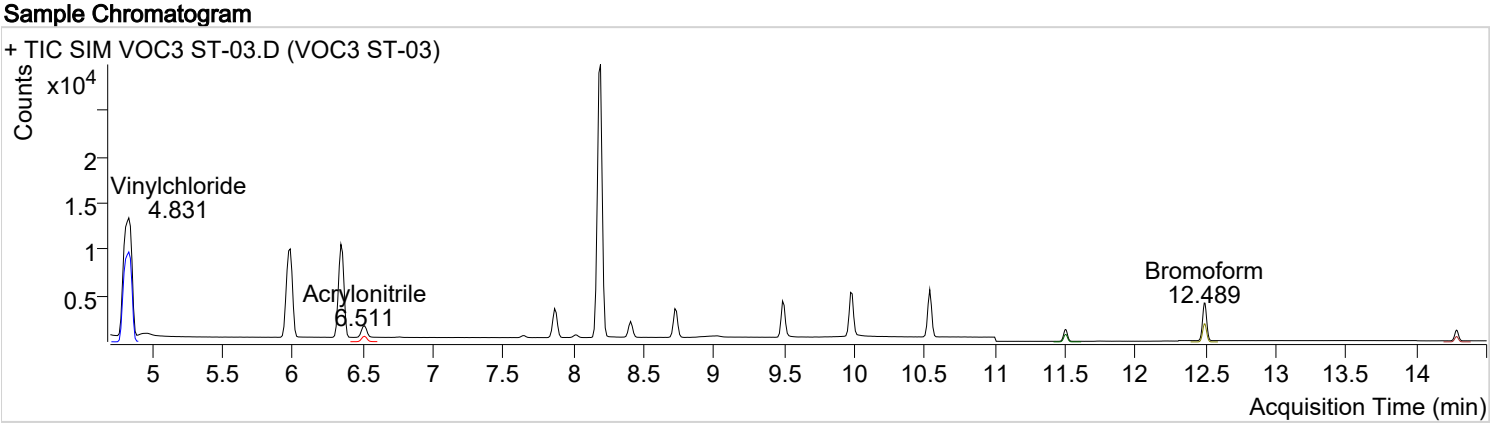

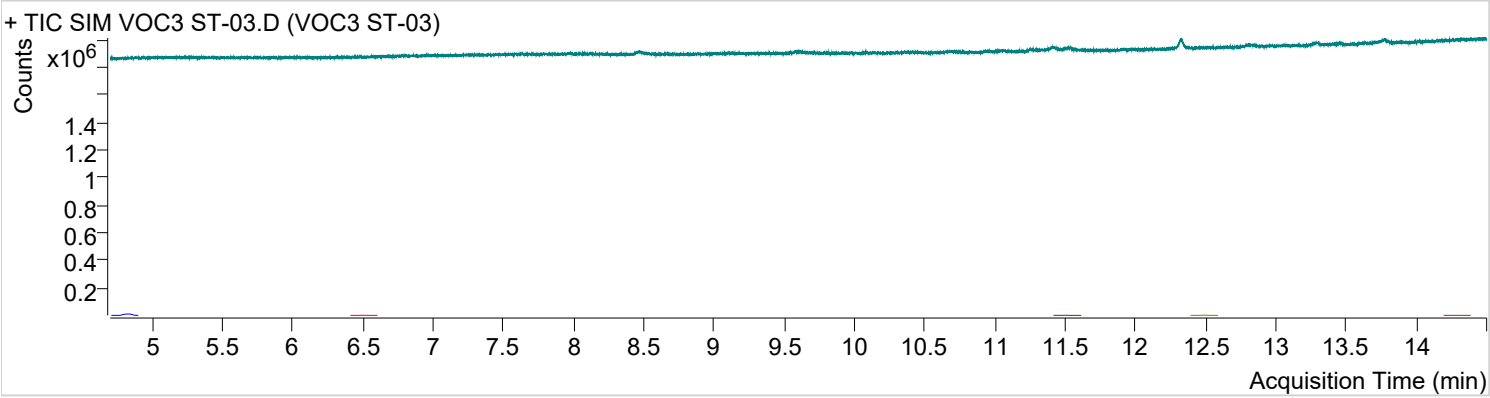

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.831	40559	1568	0.051 mg/L

Vinylchloride





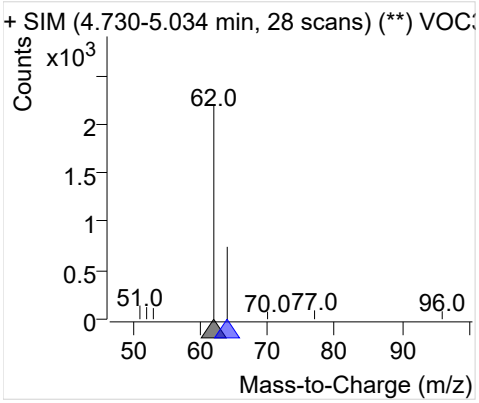

Generated at 오전 11:24 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 1.22, 1.26)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-02-02 오후 3:22:38	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:24:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-02 오후 3:22:38	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-26 오후 6:49:11	**Data File**	VOC3 ST-04.D
Type	Cal	**Name**	VOC3 ST-04
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

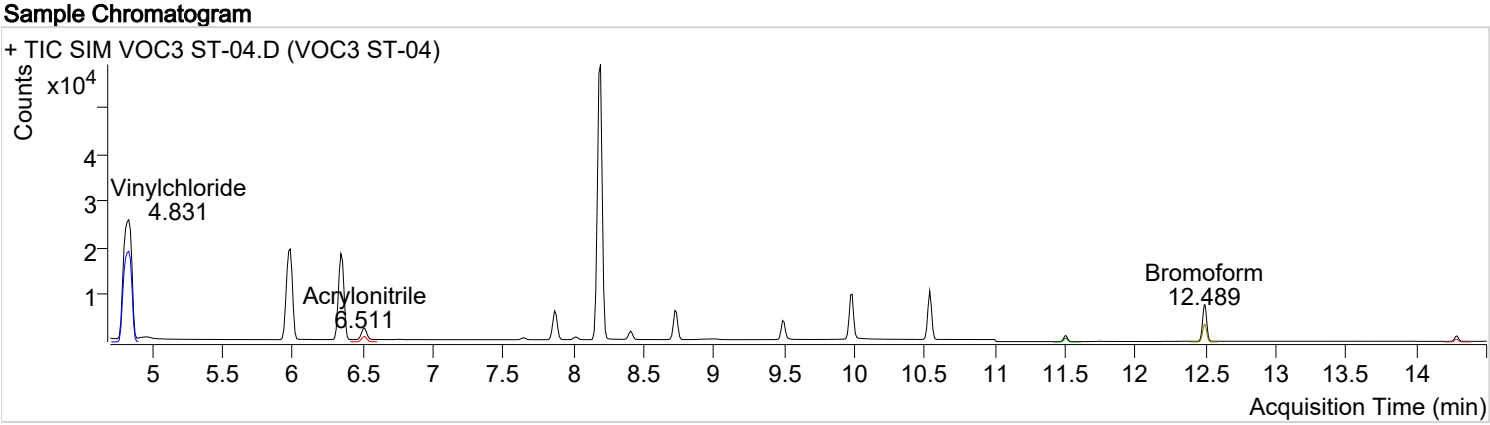

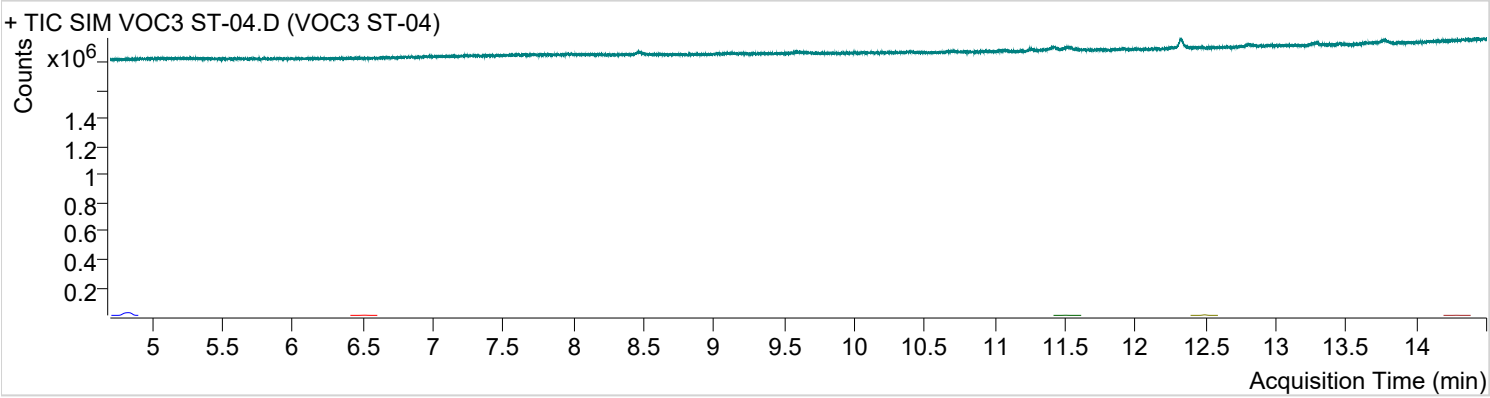

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.831	80325	1549	0.108 mg/L

Vinylchloride





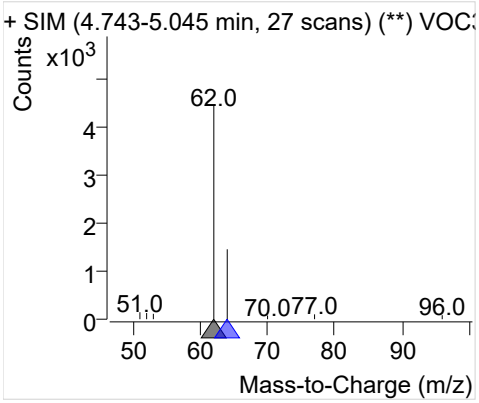

Generated at 오전 11:24 on 2026-04-10

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 1.22, 1.26)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-02-02 오후 3:22:38	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:24:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-02 오후 3:22:38	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-26 오후 7:07:05	**Data File**	VOC3 ST-05.D
Type	Cal	**Name**	VOC3 ST-05
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

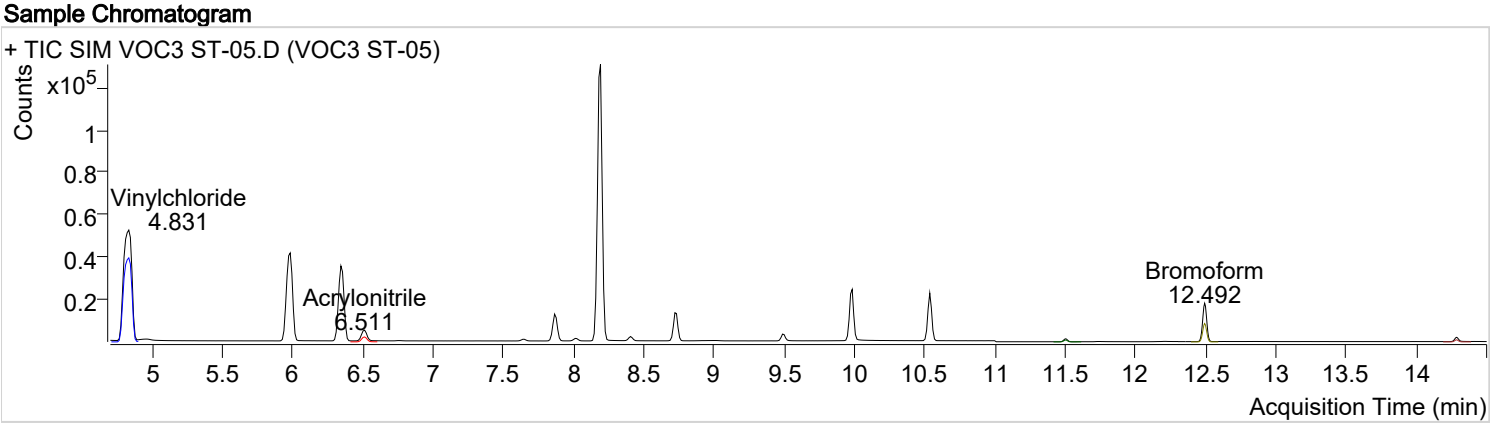

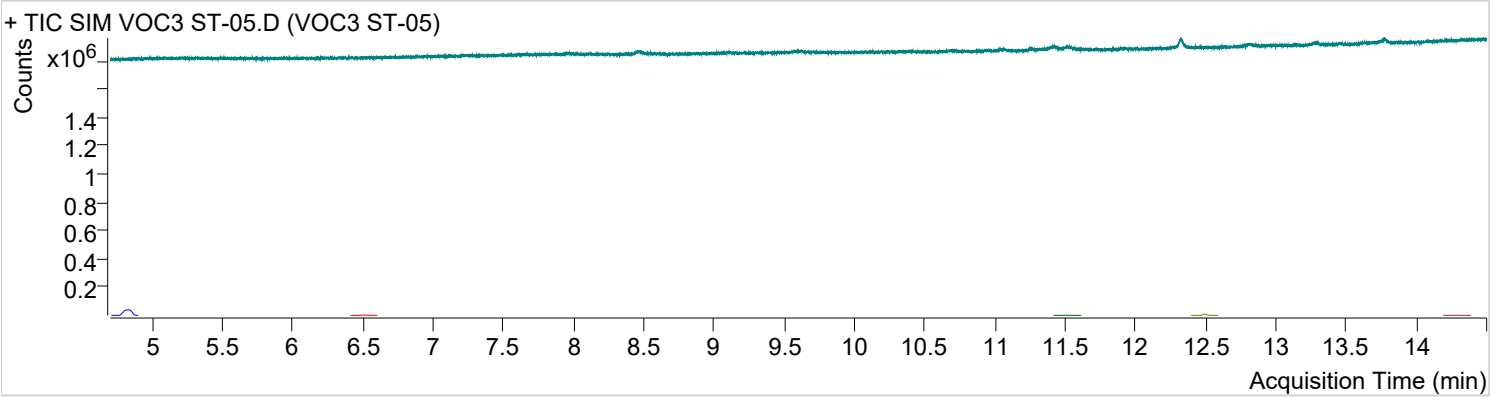

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.831	163465	1671	0.209 mg/L

Vinylchloride





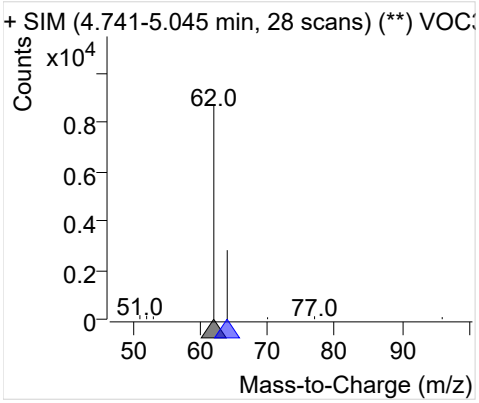

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 1.22, 1.26)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-02-02 오후 3:22:38	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:24:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-02 오후 3:22:38	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-26 오후 7:24:57	**Data File**	VOC3 ST-06.D
Type	Cal	**Name**	VOC3 ST-06
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

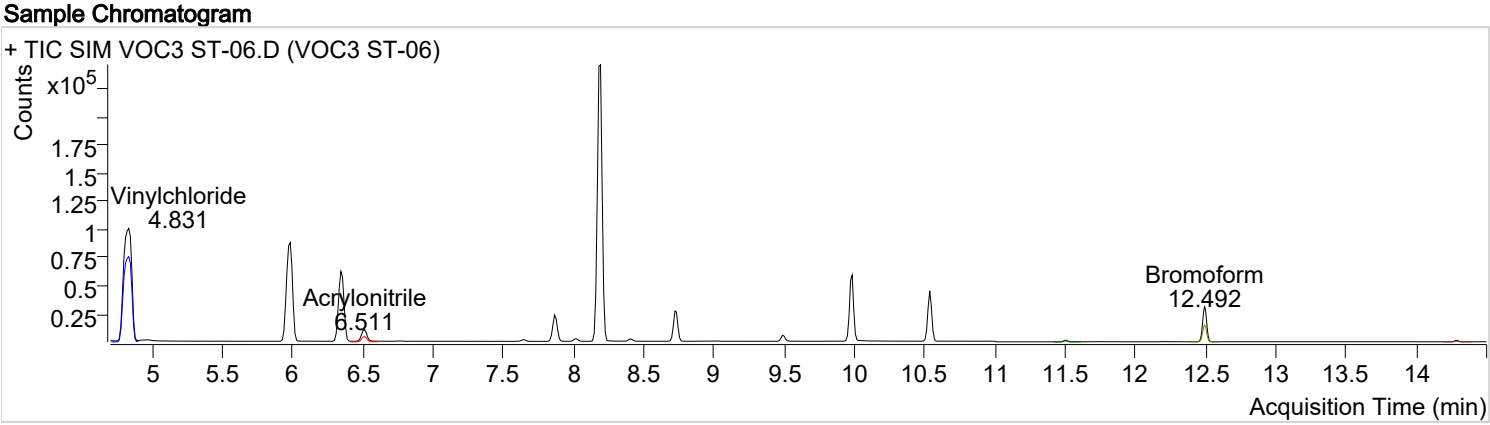

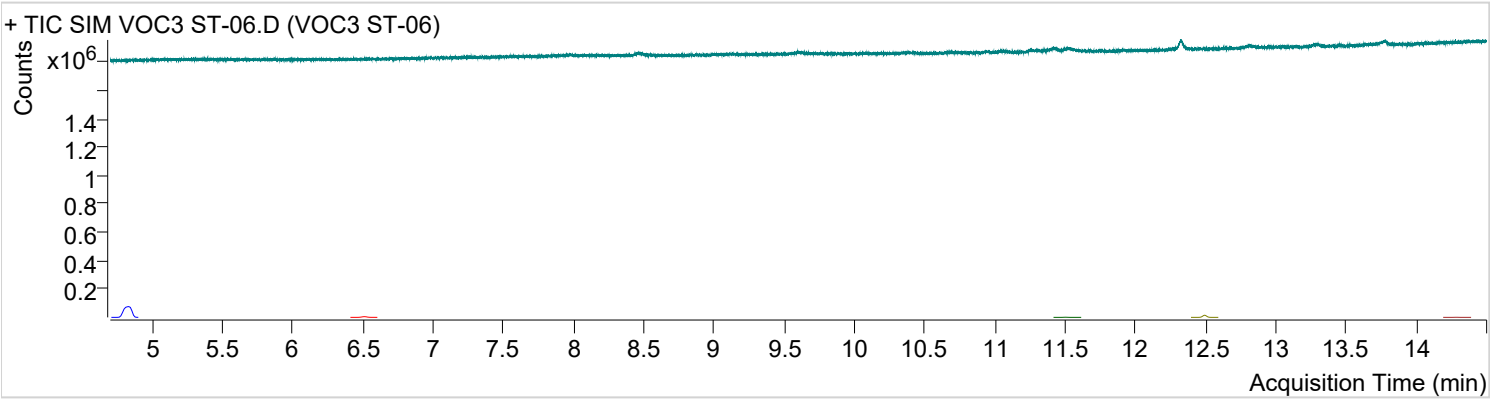

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.831	310646	1711	0.394 mg/L

Vinylchloride





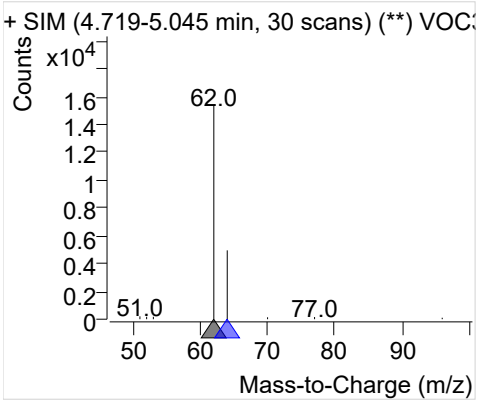

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 1.22, 1.26)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-02-02 오후 3:22:38	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:24:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-02 오후 3:22:38	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-26 오후 8:00:48	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

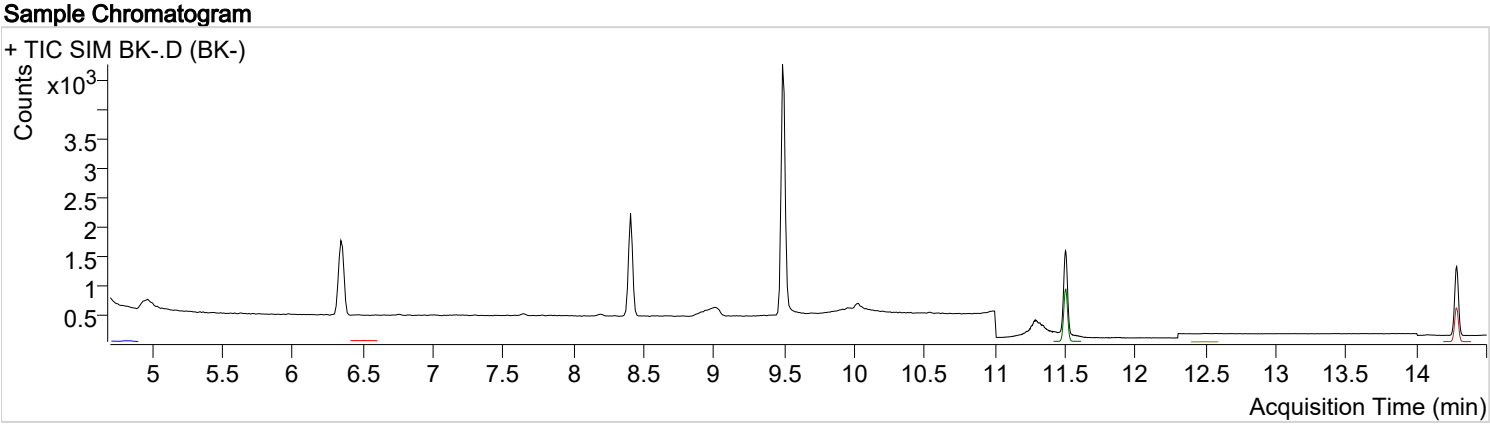

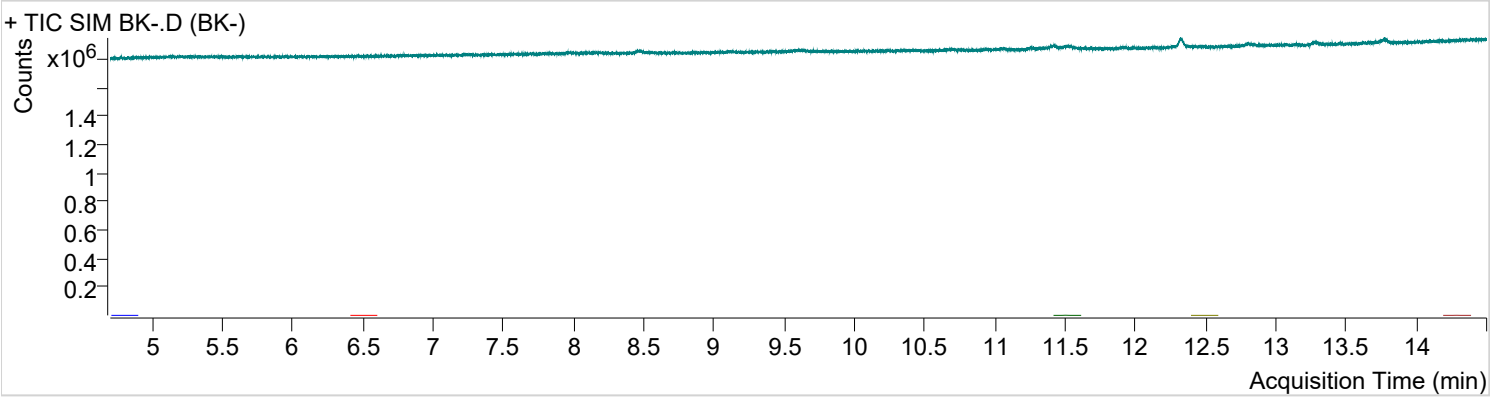

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride			1736	ND mg/L

Vinylchloride





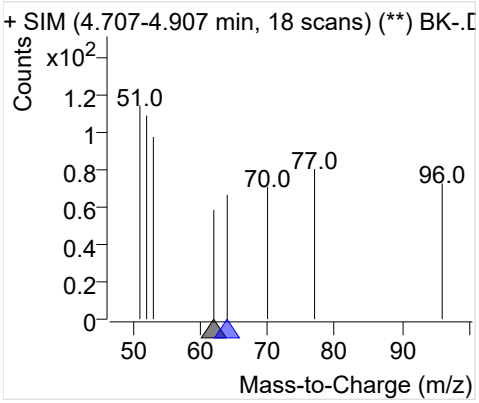

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 1.22, 1.26)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-02-02 오후 3:22:38	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:24:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-02 오후 3:22:38	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-26 오후 8:54:30	**Data File**	FBK(HC 26-01-26) .D
Type	Blank	**Name**	FBK(HC 26-01-26)
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

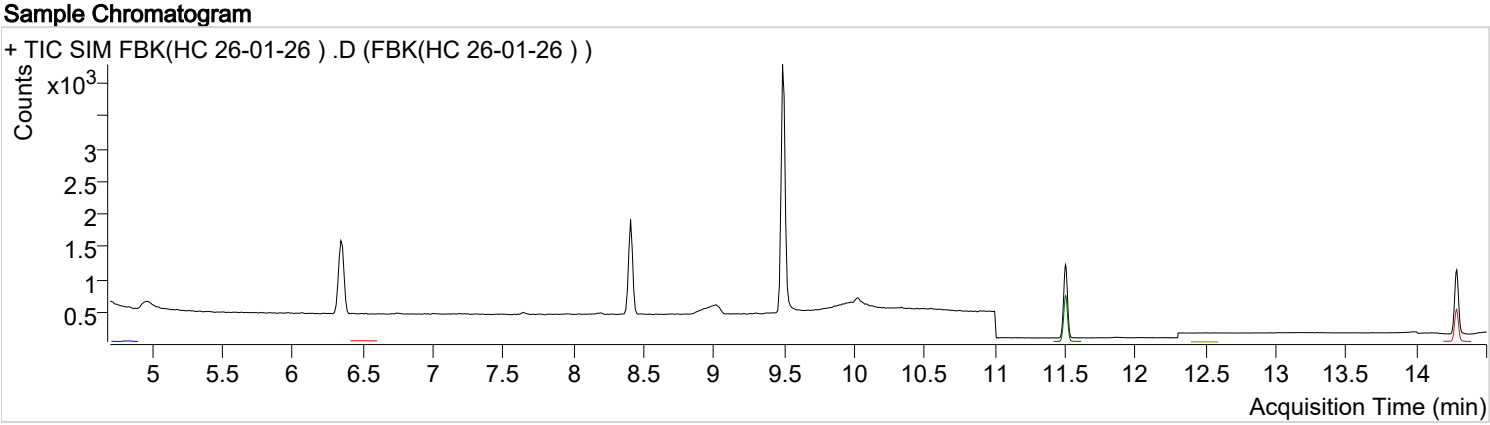

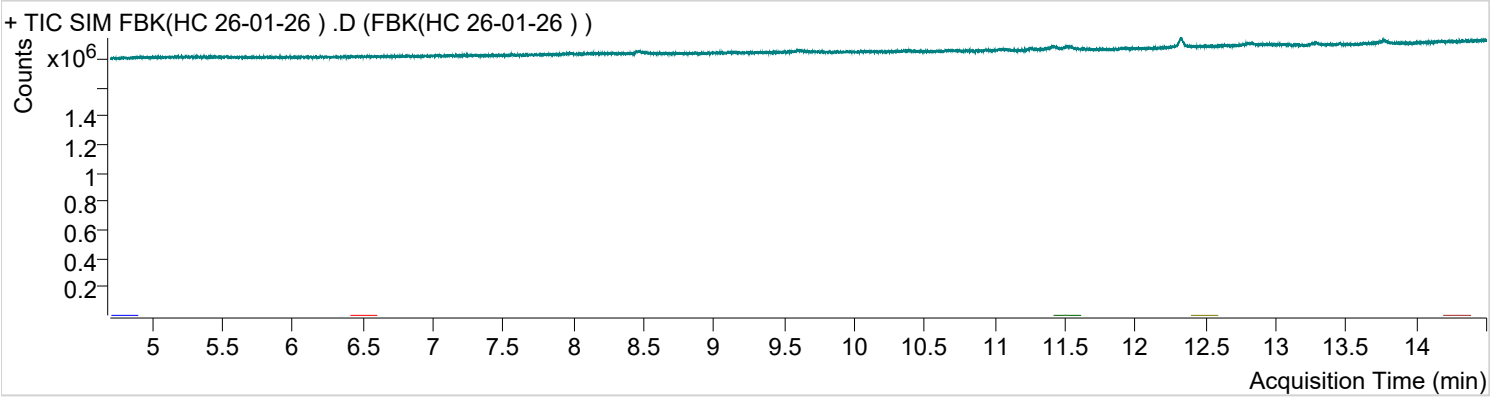

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride			1358	ND mg/L

Vinylchloride

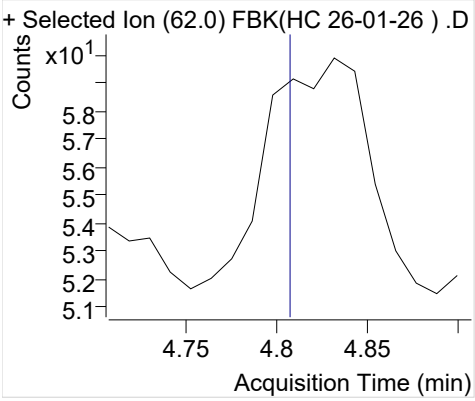



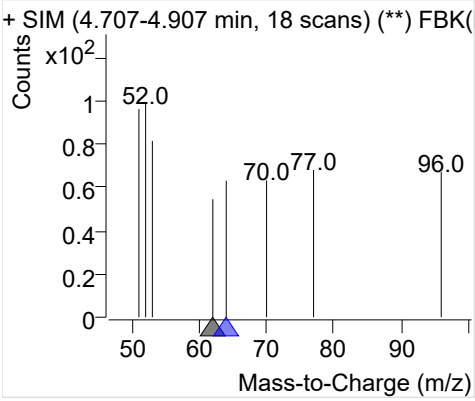

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 1.22, 1.26)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-02-02 오후 3:22:38	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:24:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-02 오후 3:22:38	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-26 오후 9:12:22	**Data File**	LDPE 26-01-26.D
Type	Sample	**Name**	LDPE 26-01-26
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

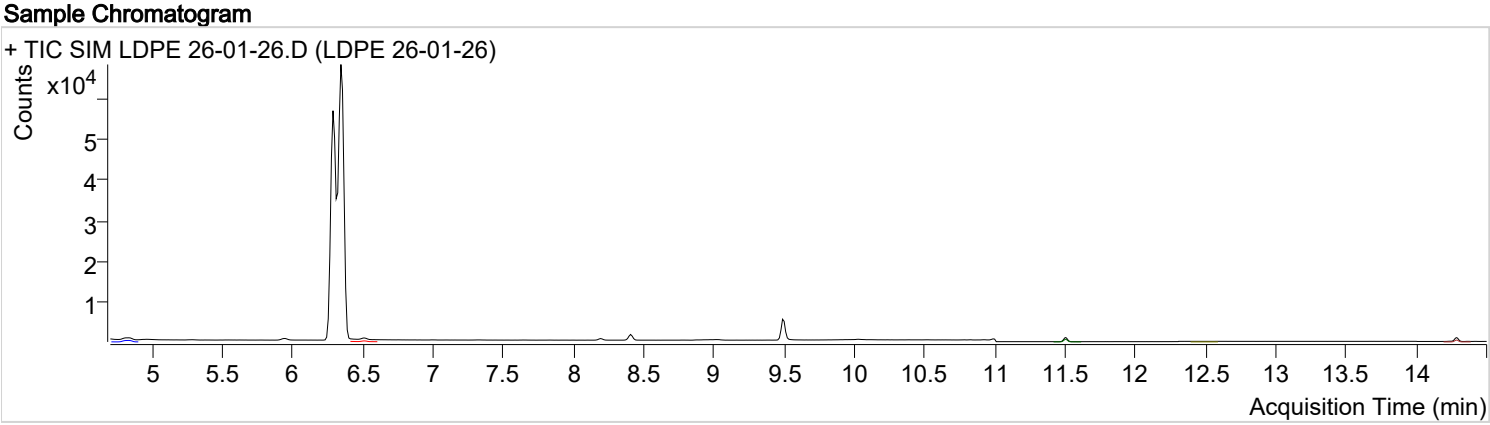

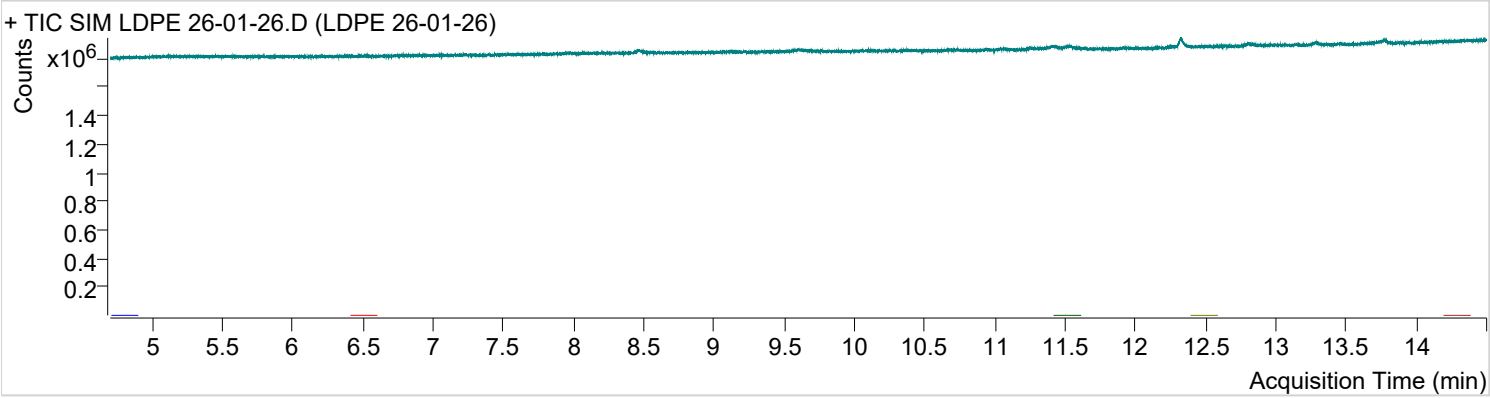

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.831	0	1236	ND mg/L

Vinylchloride



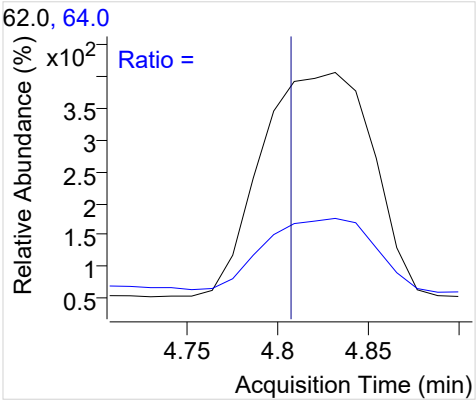

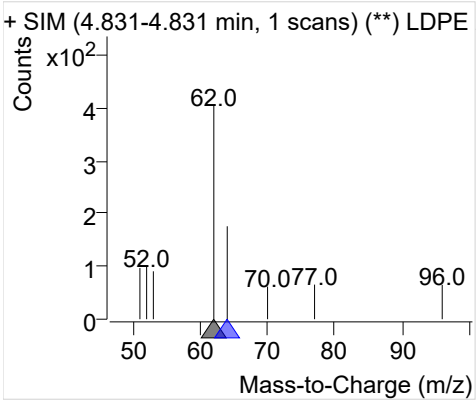

Generated at 오전 11:24 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 1.22, 1.26)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-02-02 오후 3:22:38	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:24:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-02 오후 3:22:38	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-27 오전 1:41:03	**Data File**	MBK-1.D
Type	Blank	**Name**	MBK-1
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

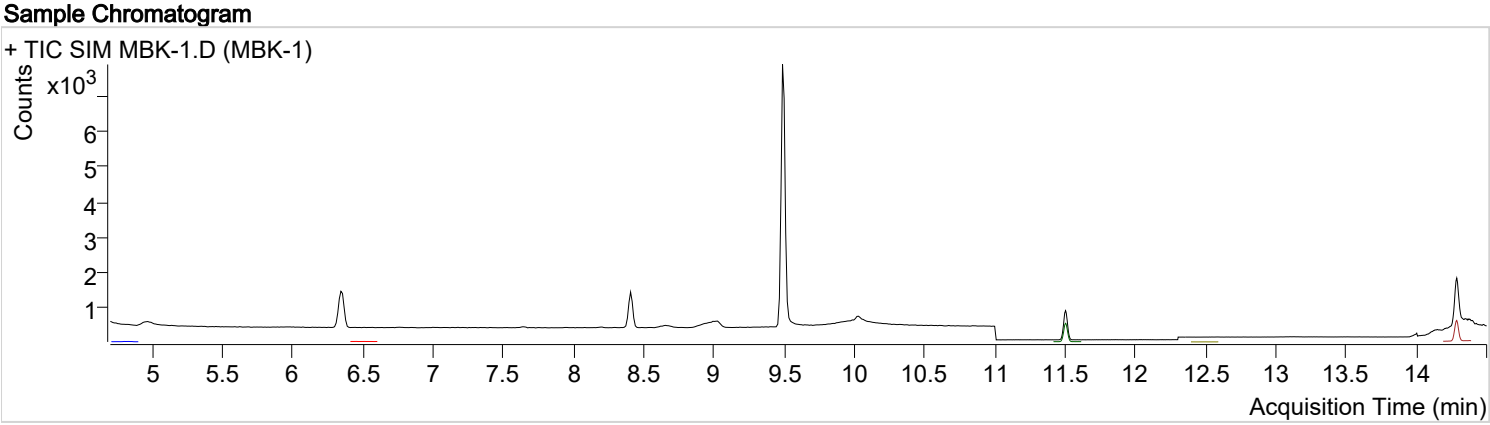

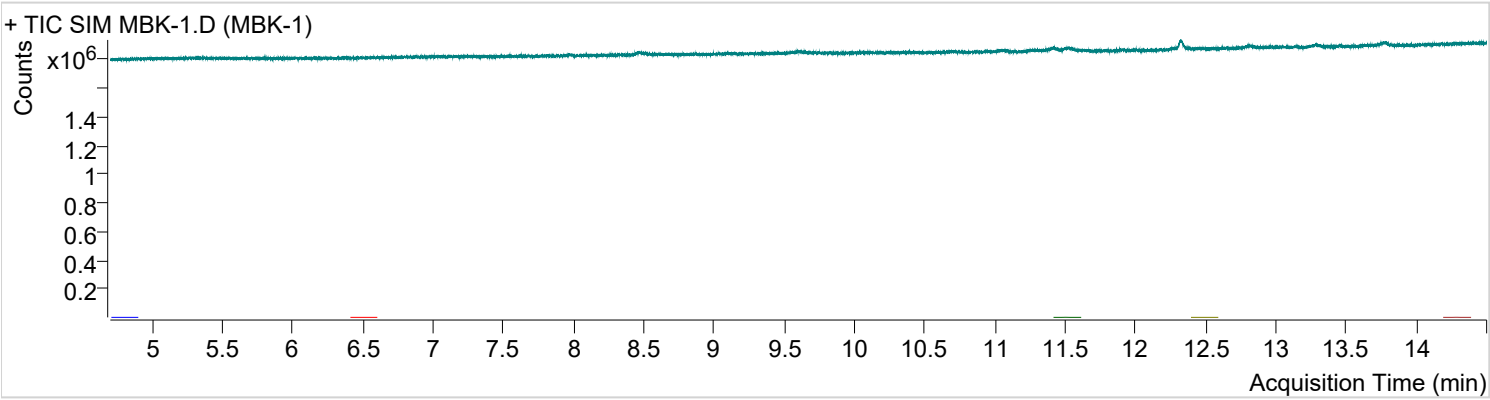

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride			1009	ND mg/L

Vinylchloride





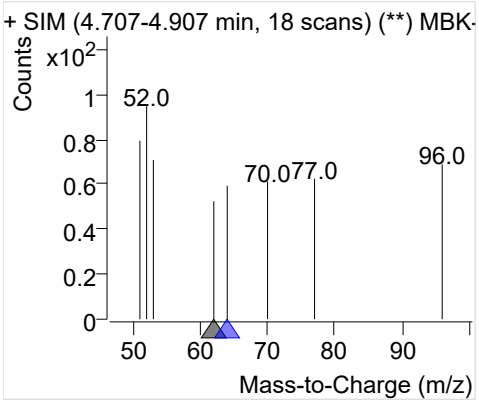

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 1.22, 1.26)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-02-02 오후 3:22:38	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:24:34	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-02 오후 3:22:38	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-27 오전 2:16:56	**Data File**	-CCV-1.D
Type	QC	**Name**	-CCV-1
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

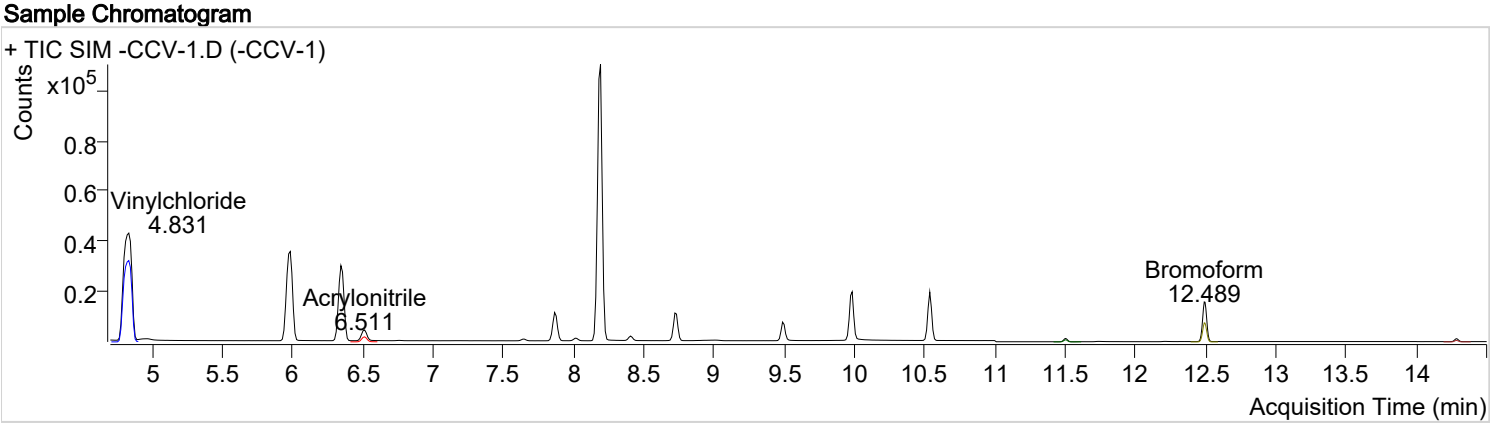

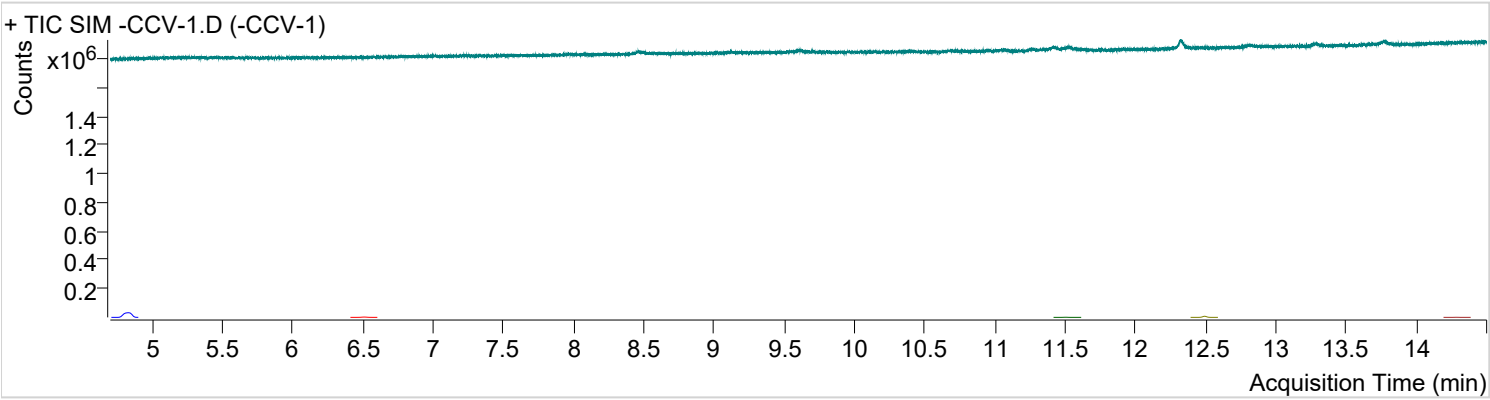

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.831	134544	1553	0.184 mg/L

Vinylchloride





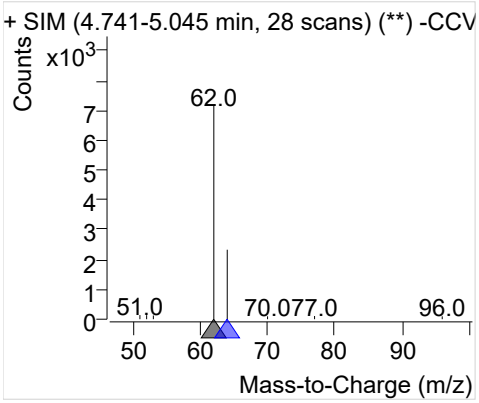

Generated at 오전 11:24 on 2026-04-10