Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 12.29 PL 12.30)\QuantResults\VOC3.batch.bin				
Analysis Time	2026-01-02 오후 1:27:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-02 오후 1:27:05	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Vinylchloride

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
VOC3 ST-01.D	Cal	4.831	650	383	0.008
VOC3 ST-02.D	Cal	4.820	1846	330	0.014
VOC3 ST-03.D	Cal	4.820	9919	420	0.039
VOC3 ST-04.D	Cal	4.820	24400	352	0.103
VOC3 ST-05.D	Cal	4.820	52685	377	0.201
BK-.D	Blank			599	ND
FBK(HC 25-12-29).D	Blank			449	ND
HC 25-12-29.D	Sample	4.820	10095	564	0.031
MBK.D	Blank			419	ND
CCV.D	QC	4.820	25433	357	0.106

Vinylchloride

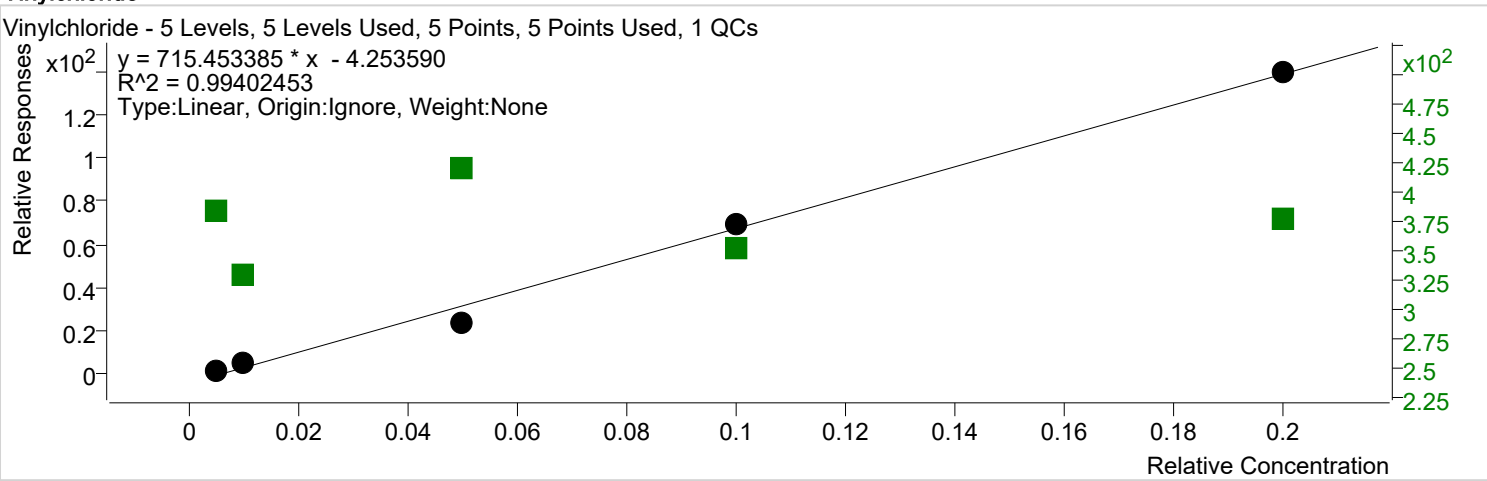

Cal. Path	Type	Level	Enable	Conc.	Response
D:\DATA\2026년\1. 2026년 1월 \VOC3(HC 12.29 PL 12.30)\VOC3 ST-01.D	Calibration	1	x	0.005	650
D:\DATA\2026년\1. 2026년 1월 \VOC3(HC 12.29 PL 12.30)\VOC3 ST-02.D	Calibration	2	x	0.010	1846
D:\DATA\2026년\1. 2026년 1월 \VOC3(HC 12.29 PL 12.30)\VOC3 ST-03.D	Calibration	3	x	0.050	9919
D:\DATA\2026년\1. 2026년 1월 \VOC3(HC 12.29 PL 12.30)\VOC3 ST-04.D	Calibration	4	x	0.100	24400
D:\DATA\2026년\1. 2026년 1월 \VOC3(HC 12.29 PL 12.30)\CCV.D	QC	4		0.100	25433
D:\DATA\2026년\1. 2026년 1월 \VOC3(HC 12.29 PL 12.30)\VOC3 ST-05.D	Calibration	5	x	0.200	52685

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 12.29 PL 12.30)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-02 오후 1:27:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:26:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-02 오후 1:27:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-01 오후 2:24:34	**Data File**	VOC3 ST-01.D
Type	Cal	**Name**	VOC3 ST-01
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

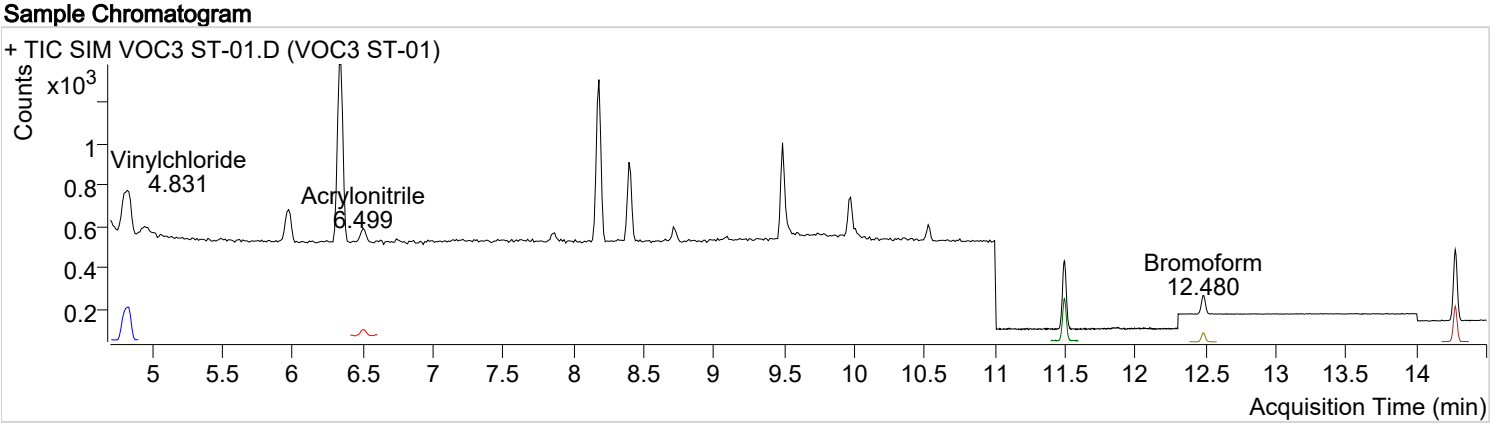

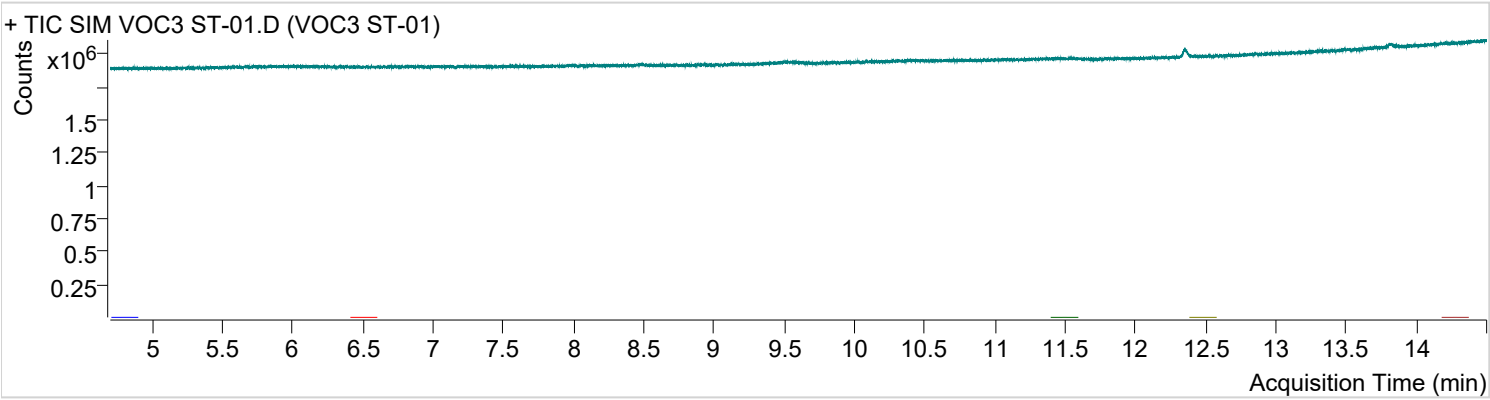

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.831	650	383	0.008 mg/L

Vinylchloride

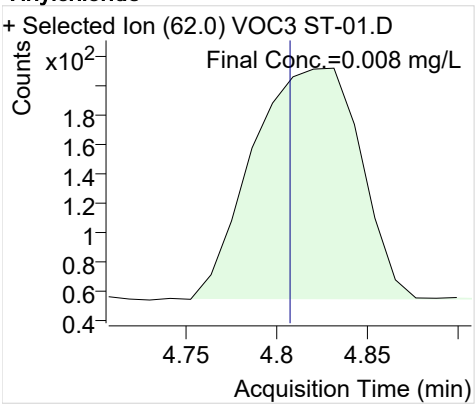



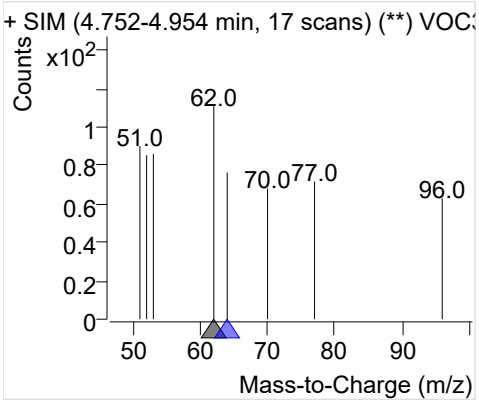

Generated at 오전 11:26 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 12.29 PL 12.30)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-02 오후 1:27:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:26:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-02 오후 1:27:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-01 오후 2:42:19	**Data File**	VOC3 ST-02.D
Type	Cal	**Name**	VOC3 ST-02
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

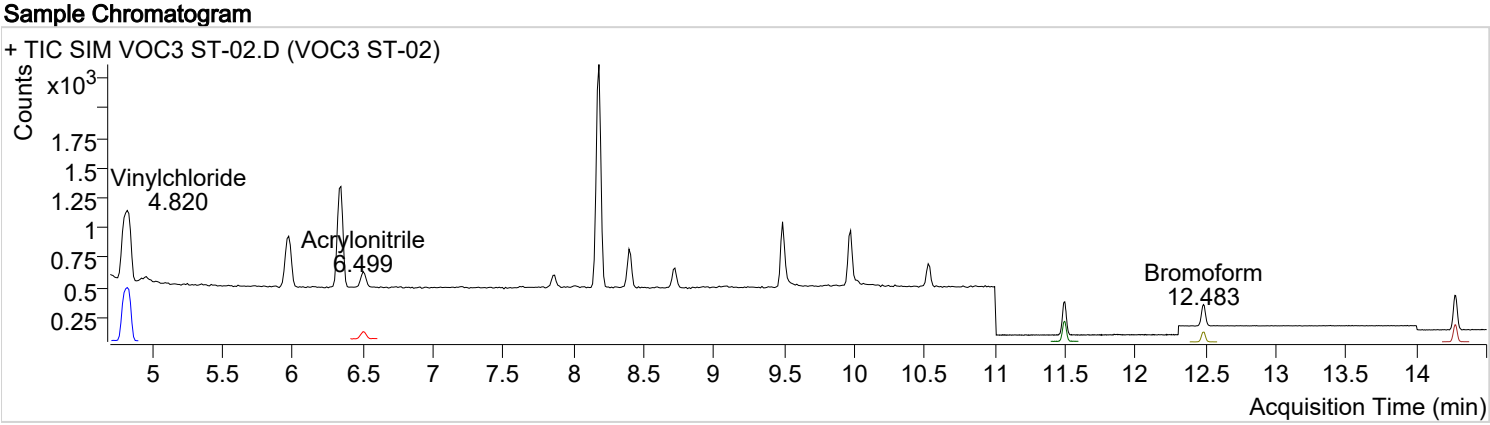

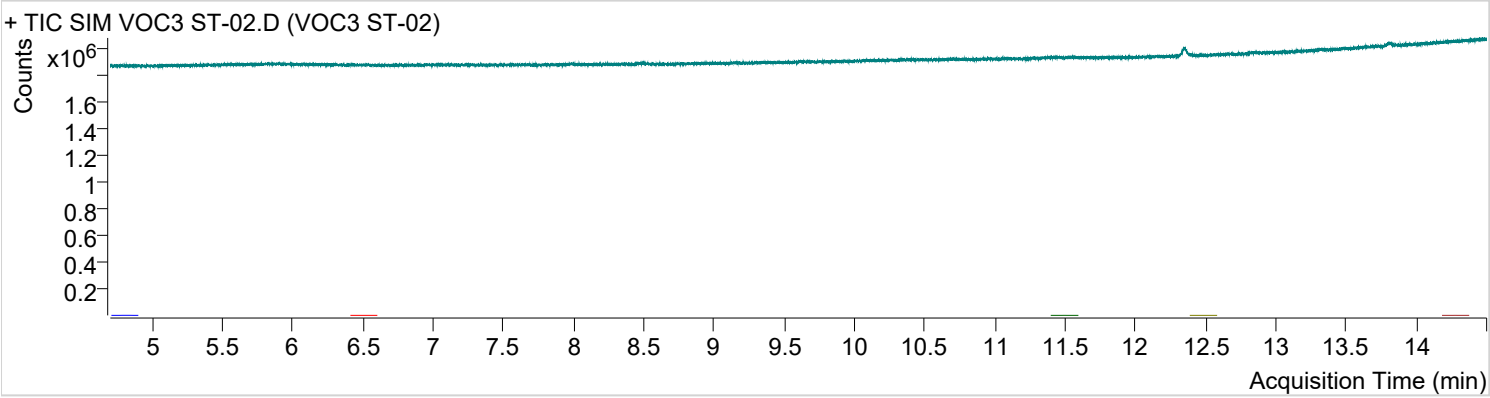

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.820	1846	330	0.014 mg/L

Vinylchloride

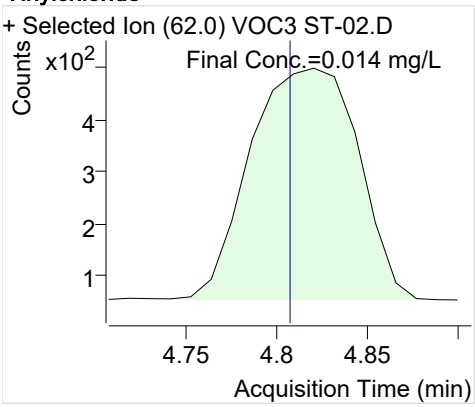



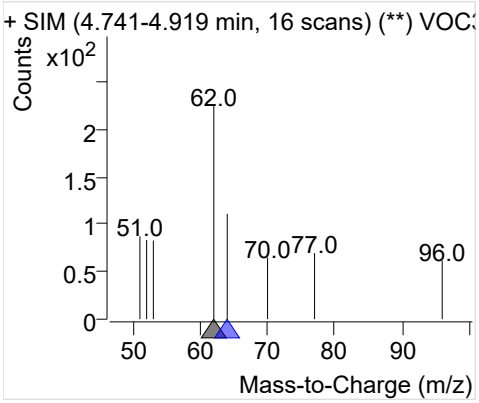

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 12.29 PL 12.30)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-02 오후 1:27:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:26:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-02 오후 1:27:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-01 오후 3:00:06	**Data File**	VOC3 ST-03.D
Type	Cal	**Name**	VOC3 ST-03
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

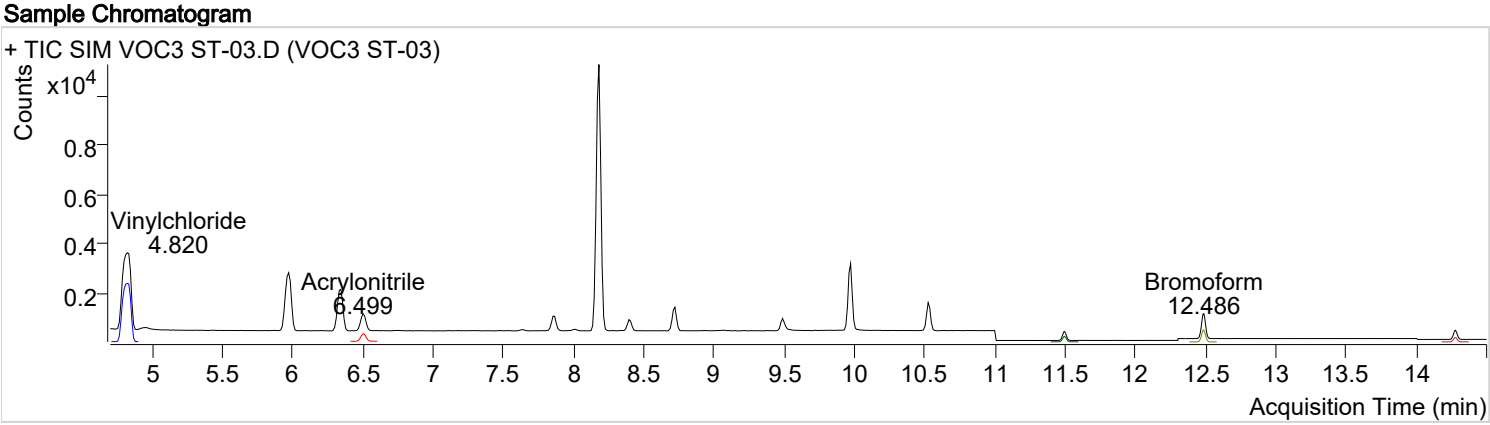

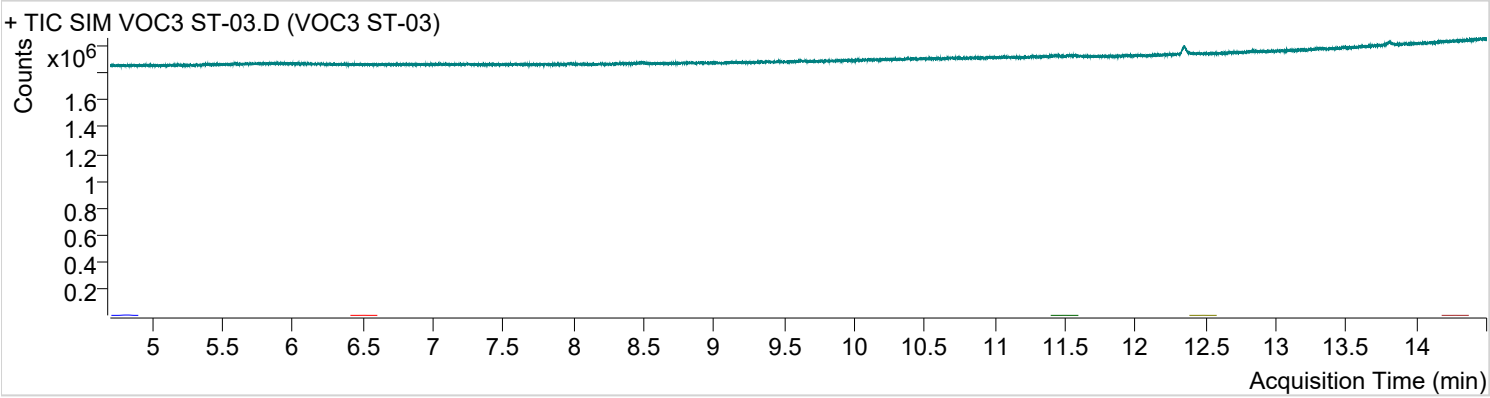

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.820	9919	420	0.039 mg/L

Vinylchloride

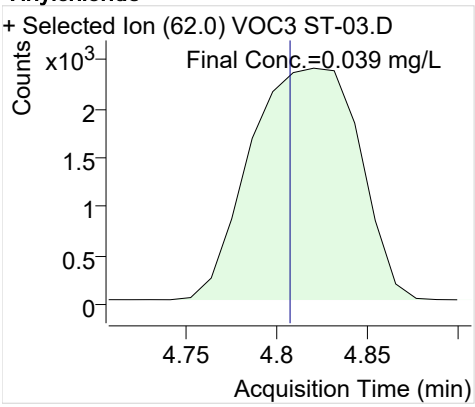



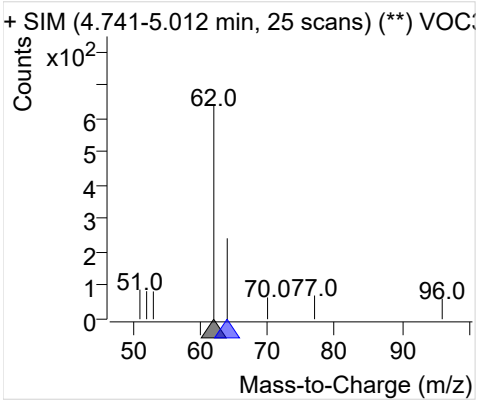

Generated at 오전 11:26 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 12.29 PL 12.30)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-02 오후 1:27:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:26:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-02 오후 1:27:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-01 오후 3:17:58	**Data File**	VOC3 ST-04.D
Type	Cal	**Name**	VOC3 ST-04
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

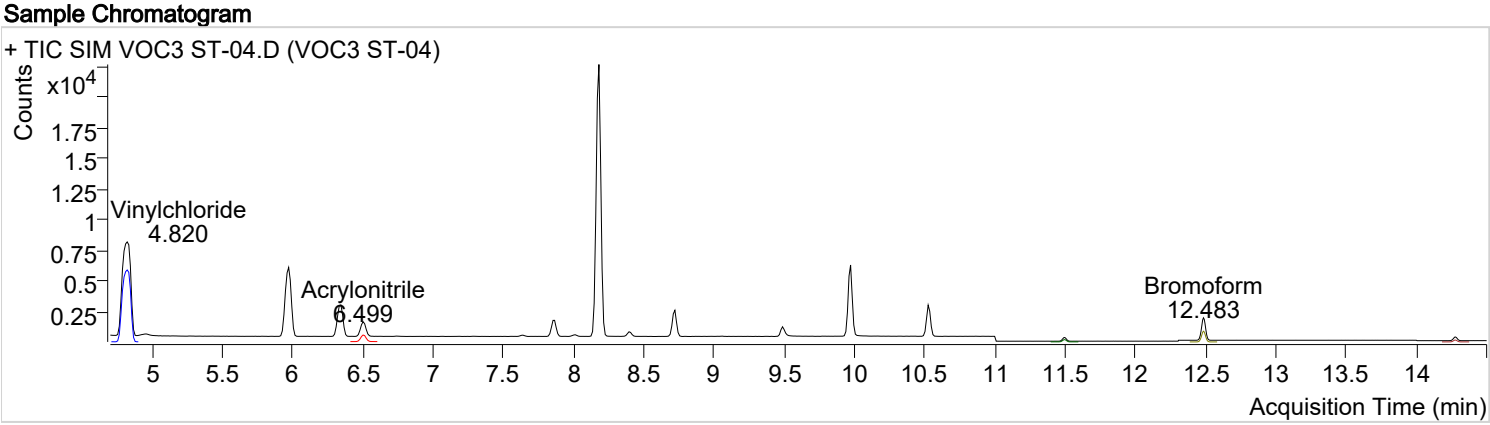

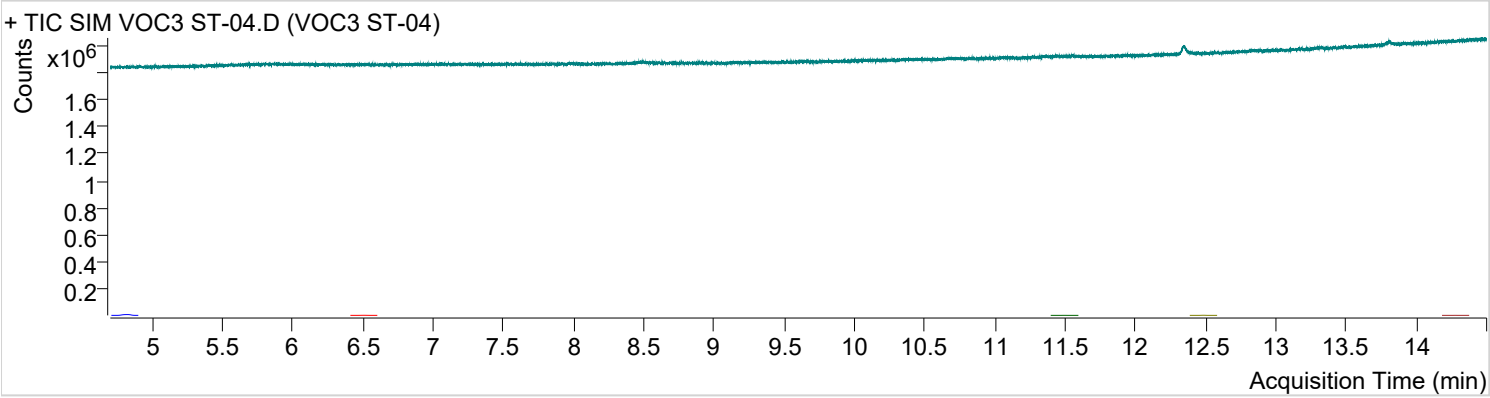

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.820	24400	352	0.103 mg/L

Vinylchloride

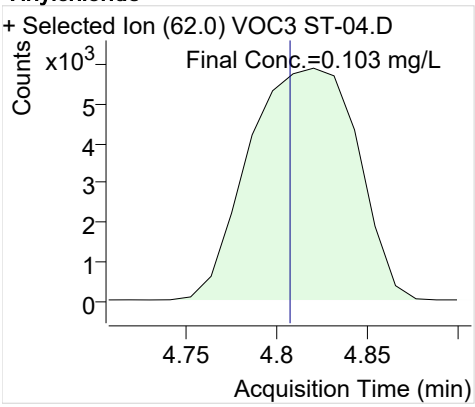



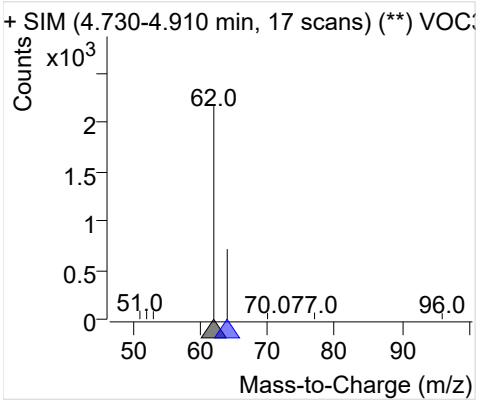

Generated at 오전 11:26 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 12.29 PL 12.30)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-02 오후 1:27:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:26:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-02 오후 1:27:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-01 오후 3:35:51	**Data File**	VOC3 ST-05.D
Type	Cal	**Name**	VOC3 ST-05
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

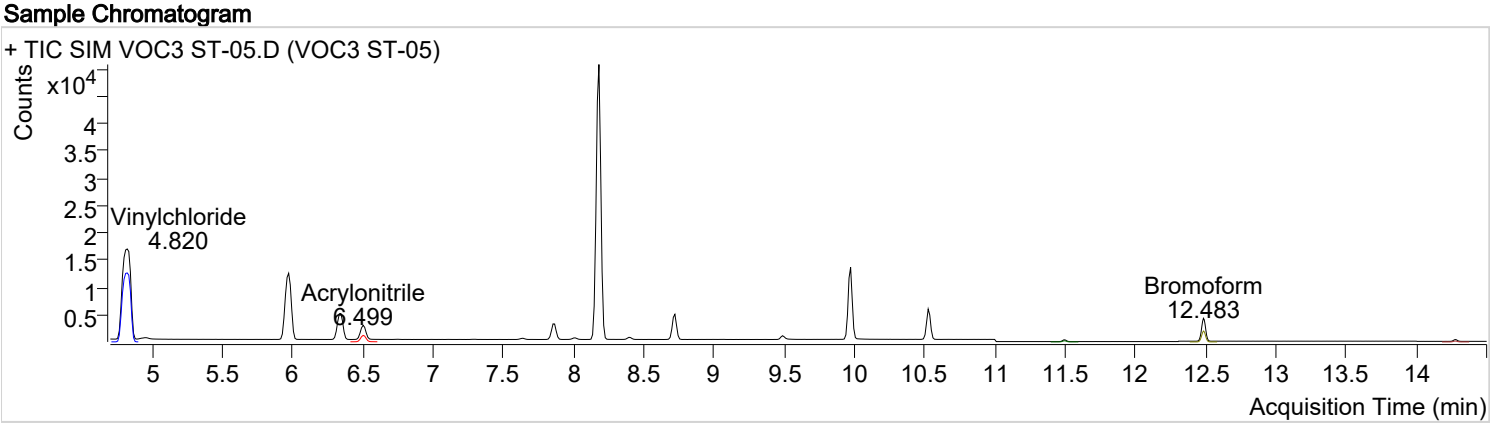

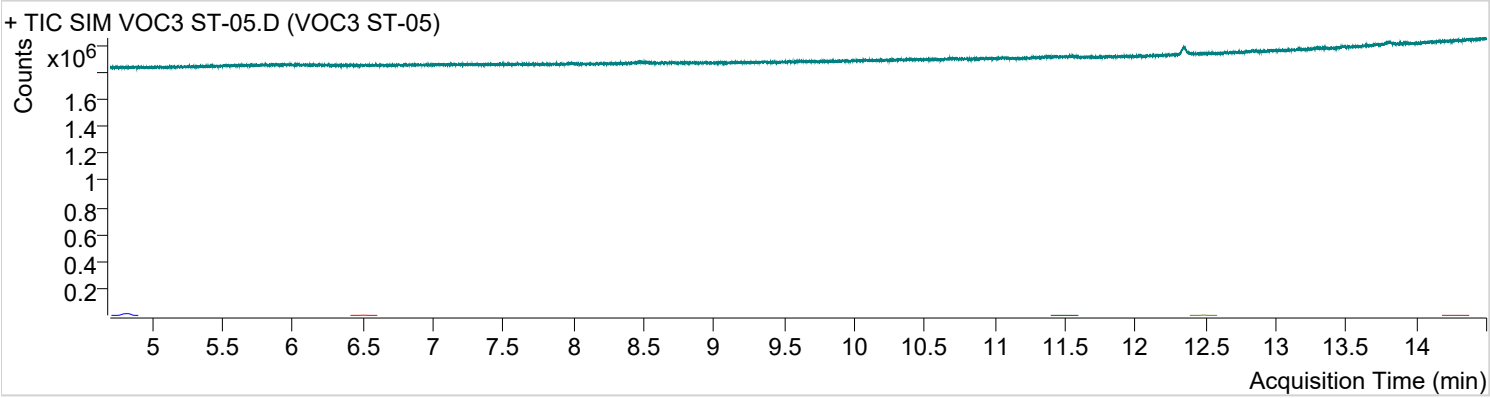

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.820	52685	377	0.201 mg/L

Vinylchloride

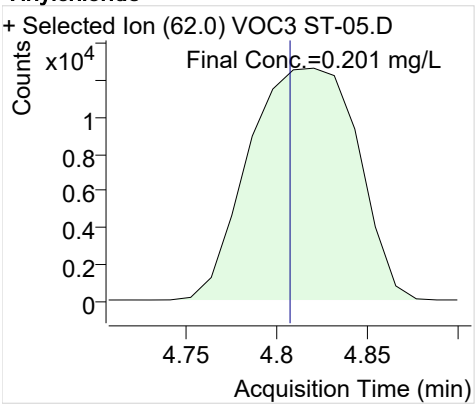



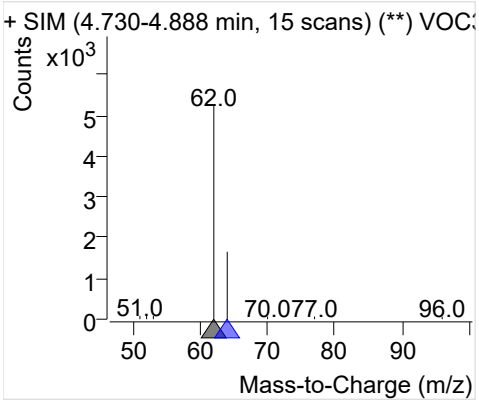

Generated at 오전 11:26 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 12.29 PL 12.30)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-02 오후 1:27:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:26:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-02 오후 1:27:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-01 오후 4:29:24	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

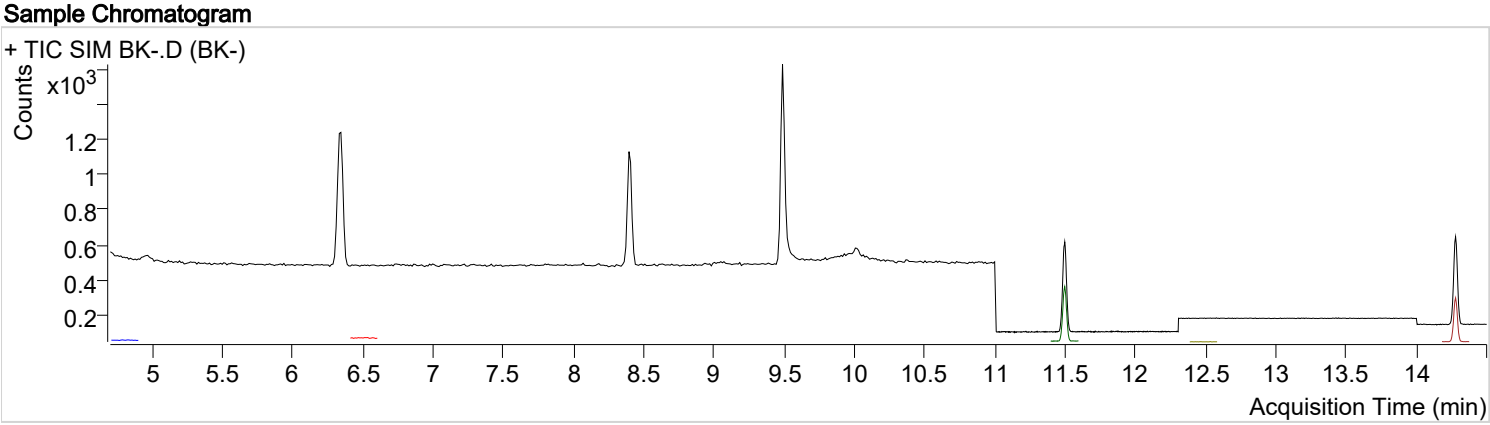

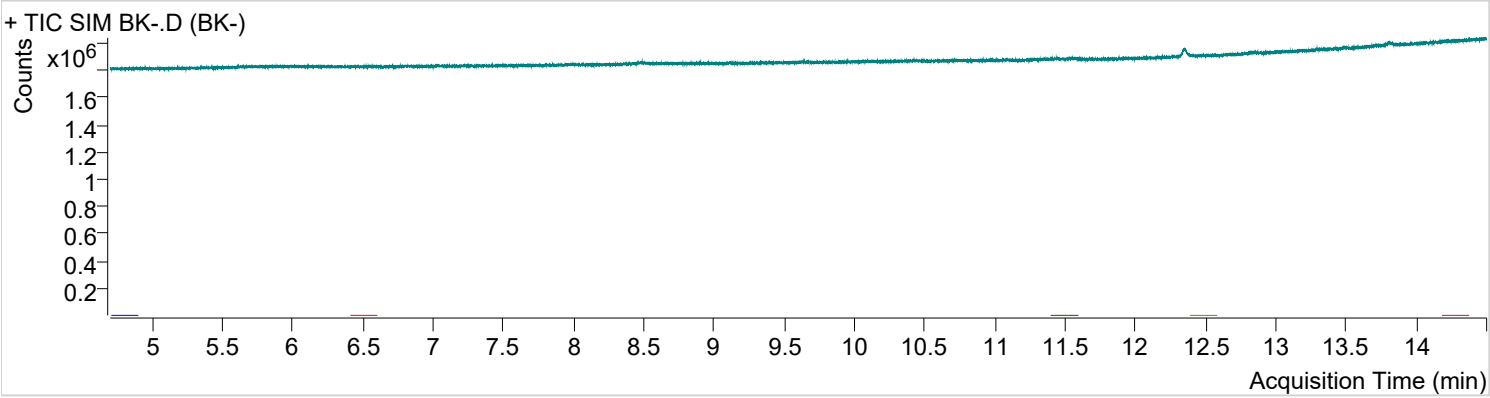

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride			599	ND mg/L

Vinylchloride

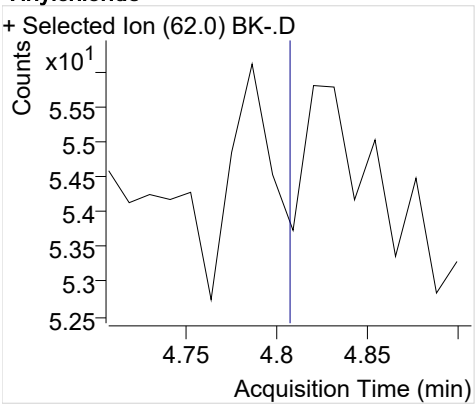



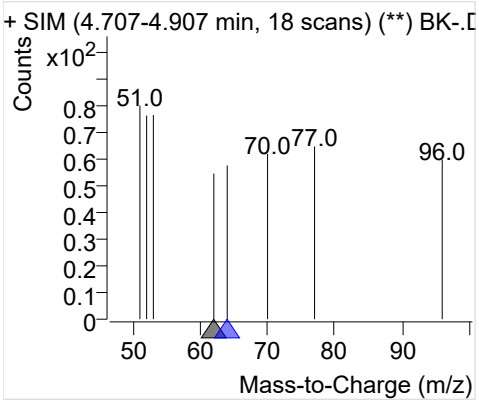

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 12.29 PL 12.30)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-02 오후 1:27:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:26:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-02 오후 1:27:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-01 오후 4:47:12	**Data File**	FBK(HC 25-12-29).D
Type	Blank	**Name**	FBK(HC 25-12-29)
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

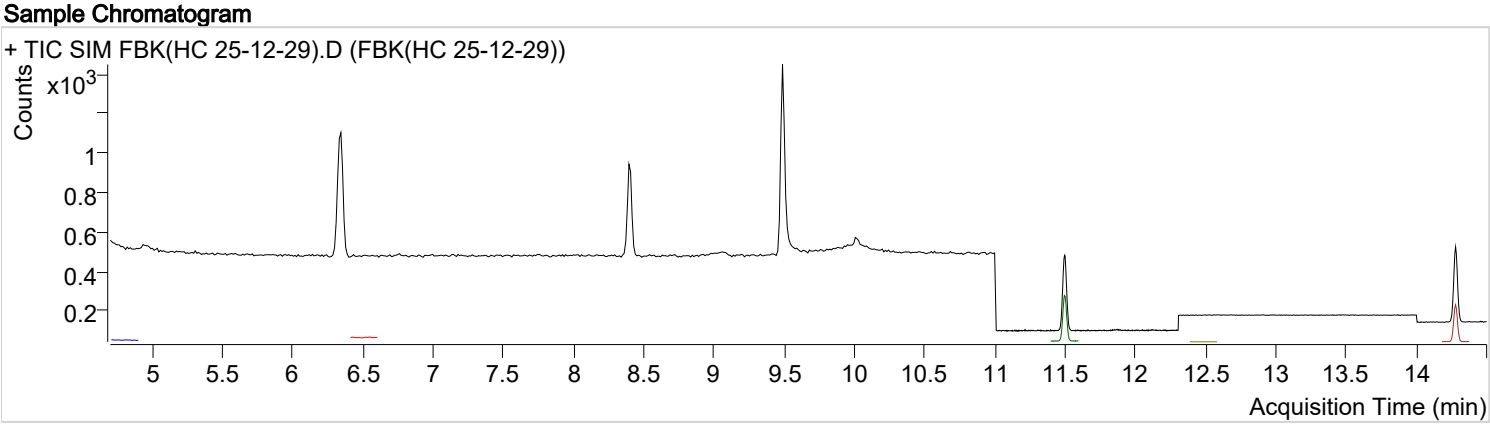

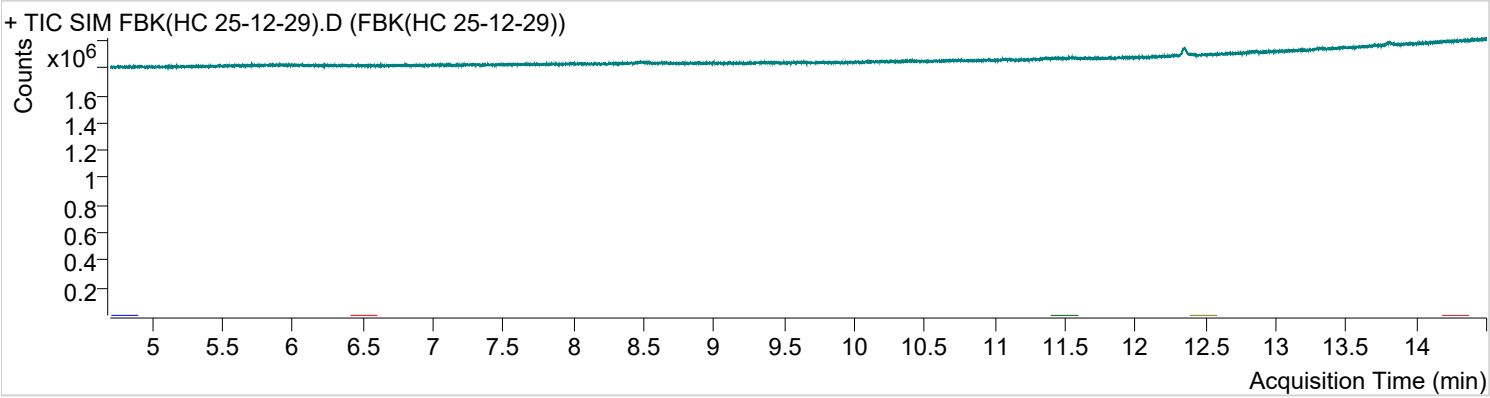

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride			449	ND mg/L

Vinylchloride

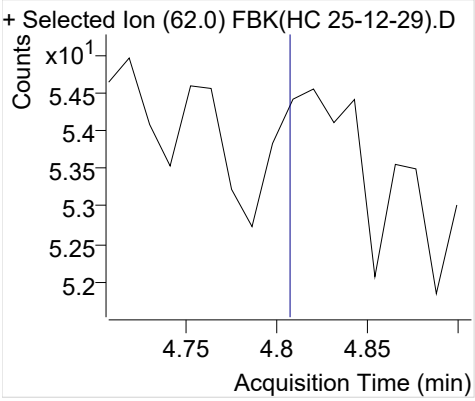



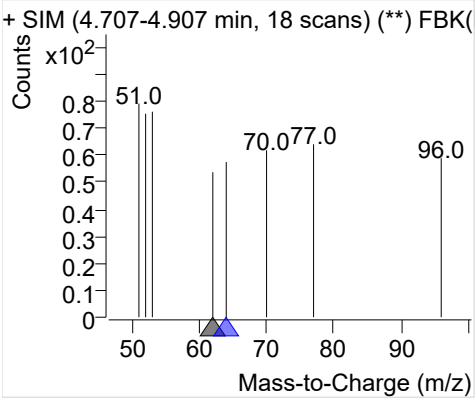

Generated at 오전 11:26 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 12.29 PL 12.30)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-02 오후 1:27:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:26:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-02 오후 1:27:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-01 오후 5:05:00	**Data File**	HC 25-12-29.D
Type	Sample	**Name**	HC 25-12-29
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

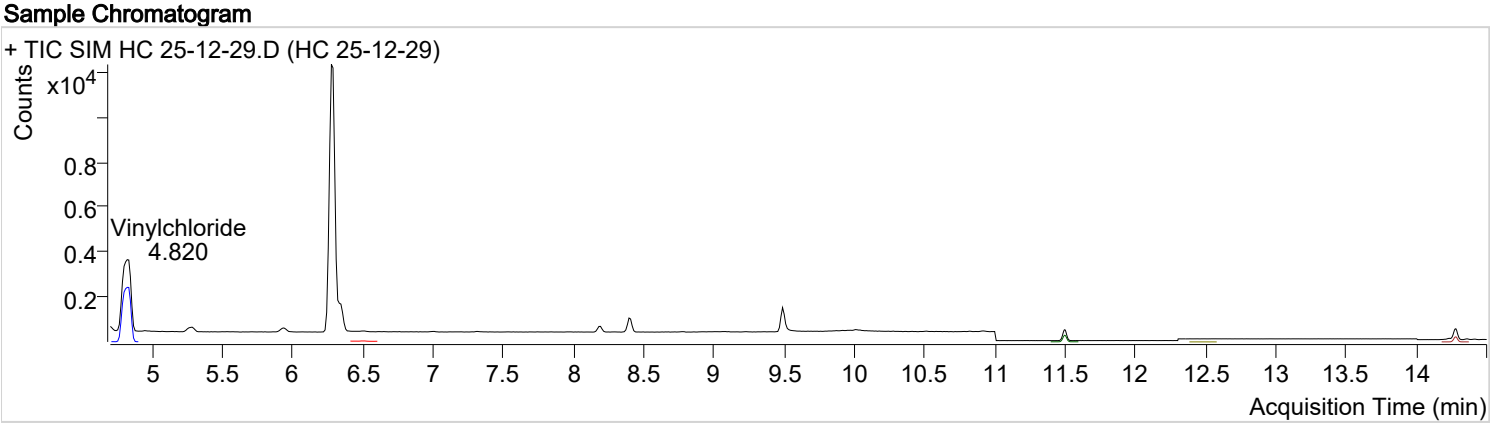

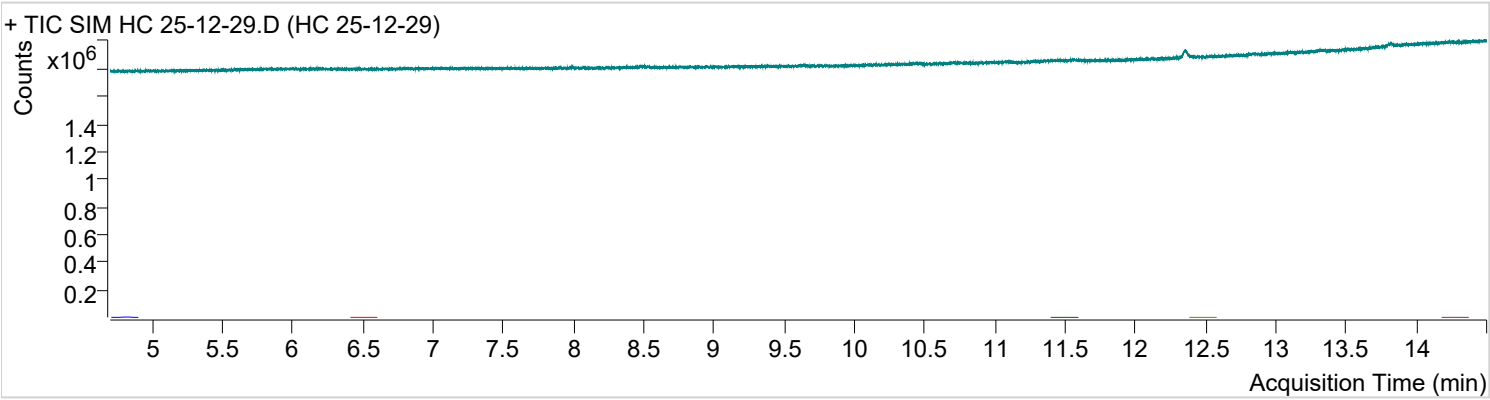

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.820	10095	564	0.031 mg/L

Vinylchloride

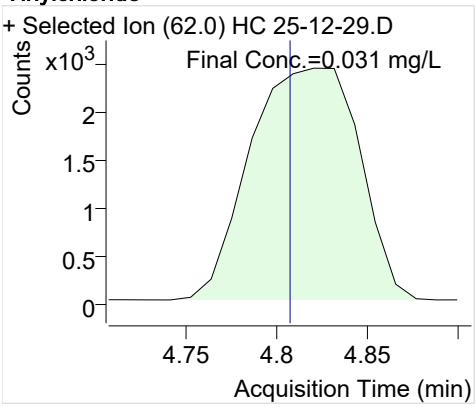



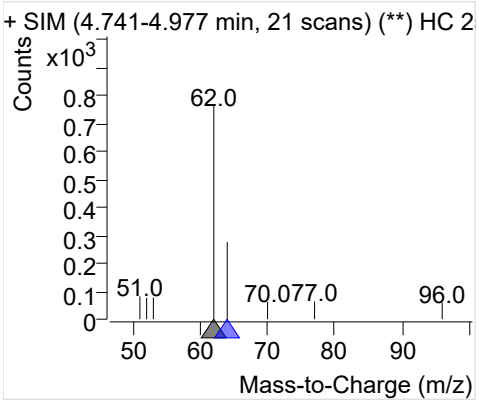

Generated at 오전 11:26 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 12.29 PL 12.30)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-02 오후 1:27:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:26:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-02 오후 1:27:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-01 오후 6:16:09	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

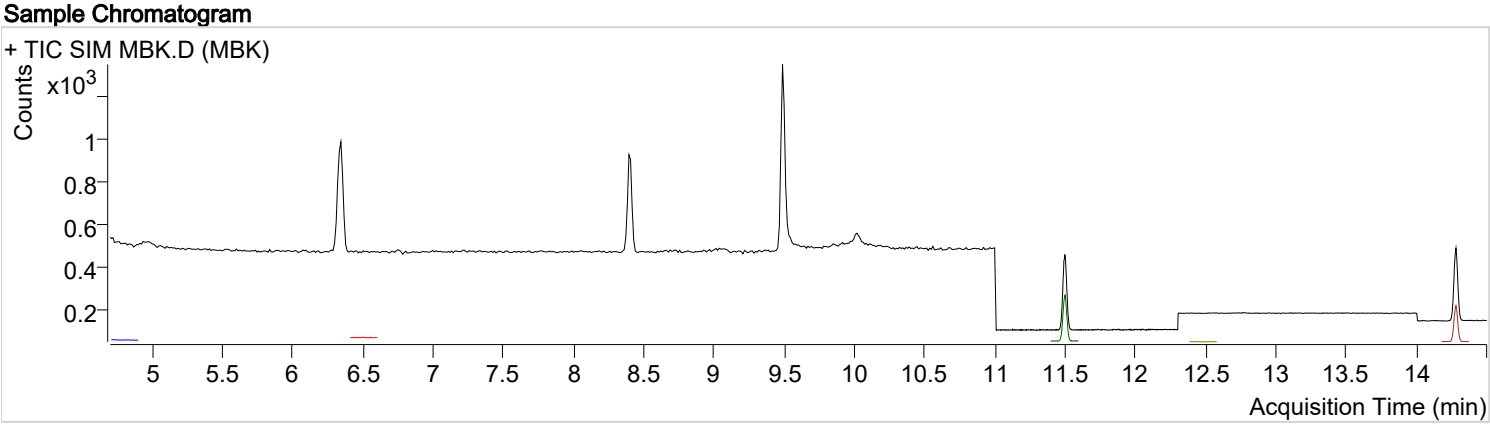

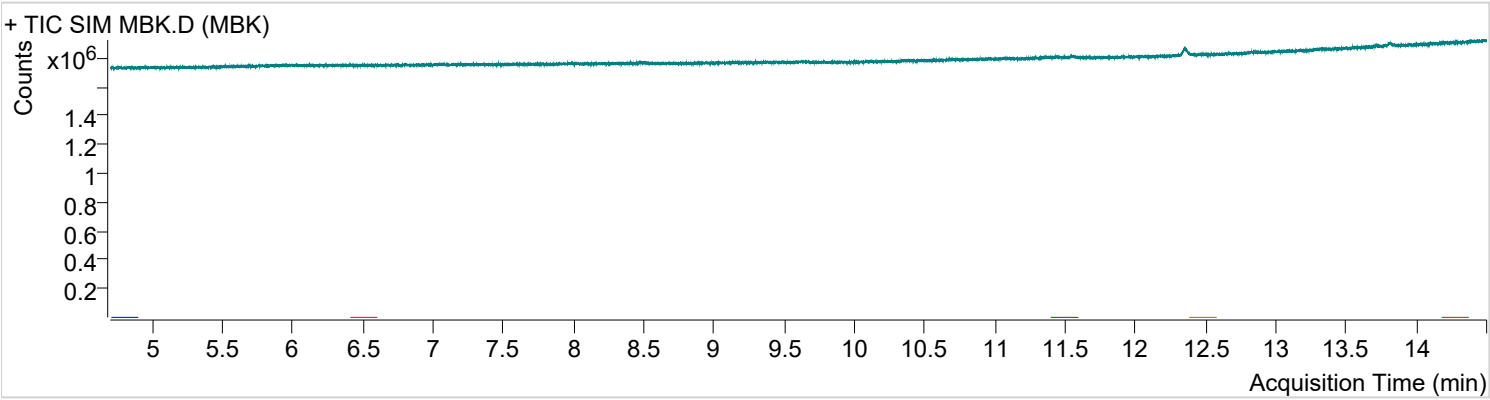

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride			419	ND mg/L

Vinylchloride

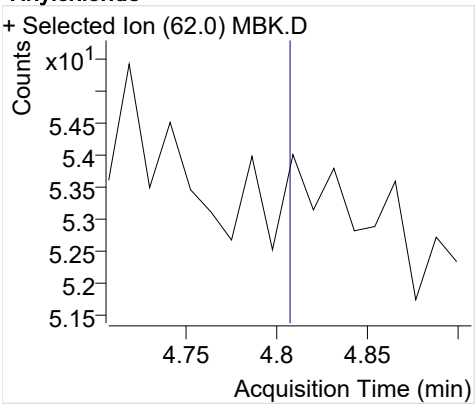



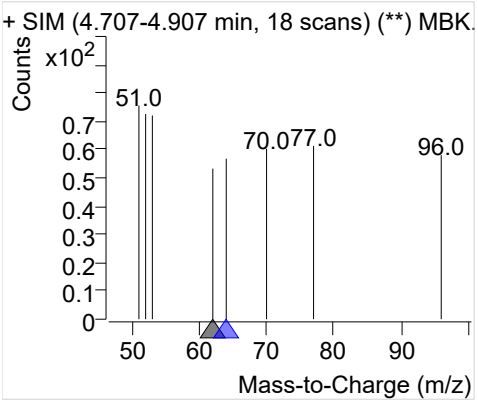

Generated at 오전 11:26 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC3(HC 12.29 PL 12.30)\QuantResults\VOC3.batch.bin		
Analysis Time	2026-01-02 오후 1:27:05	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 11:26:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-02 오후 1:27:05	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-01 오후 6:33:59	**Data File**	CCV.D
Type	QC	**Name**	CCV
Dil.	1	**Acq. Method File**	2025-VOCs(3) NEW

Sample Chromatogram

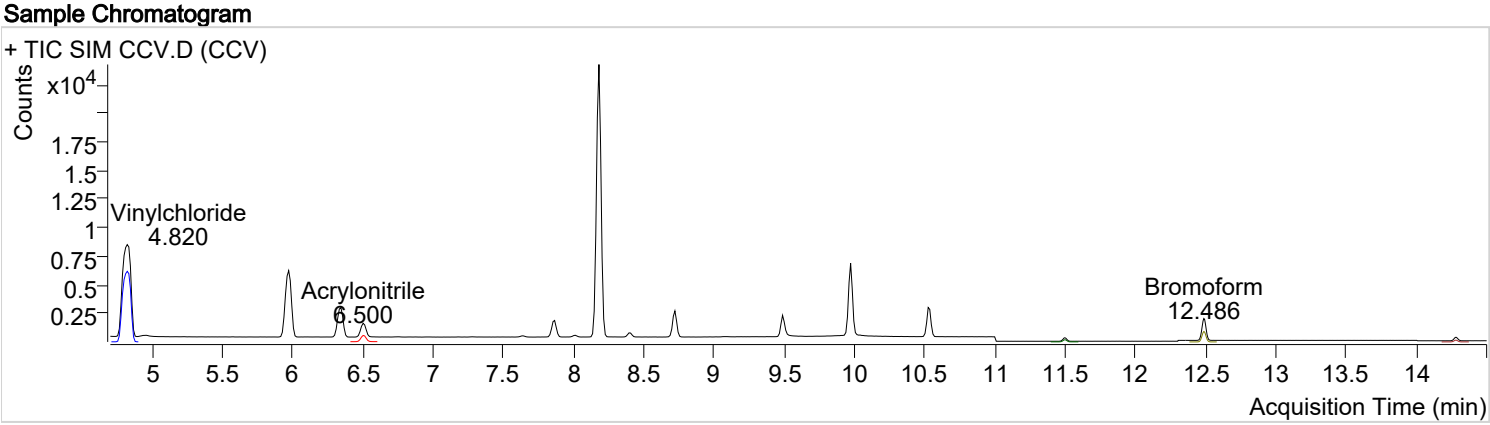

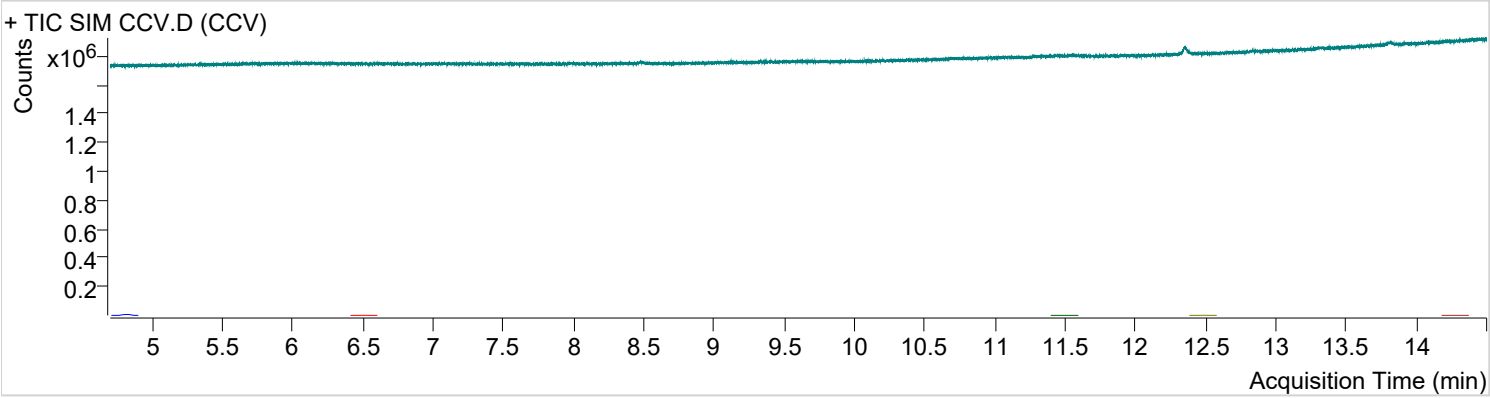

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Vinylchloride	4.820	25433	357	0.106 mg/L

Vinylchloride

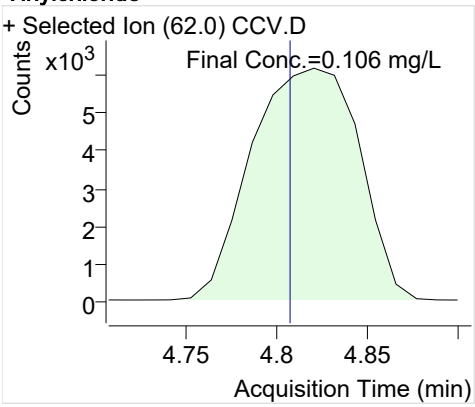



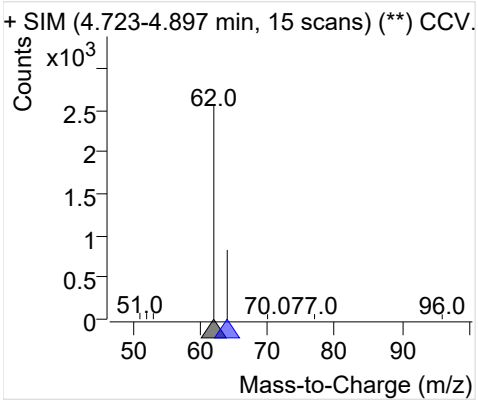

Generated at 오전 11:26 on 2026-04-10