Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\Naphthalene.batch.bin				
Analysis Time	2026-01-08 오후 12:02:33	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 12:02:33	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Naphthalene

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
Naphthalene ST-01.D	Cal	14.430	747	2254	0.001
Naphthalene ST-02.D	Cal	14.436	2683	1806	0.006
Naphthalene ST-03.D	Cal	14.430	3481	1834	0.008
Naphthalene ST-04.D	Cal	14.436	11525	1029	0.051
Naphthalene ST-05.D	Cal	14.436	34939	1607	0.100
BK-.D	Blank			1587	ND
FBK(PL 25-12-30).D	Blank			1419	ND
PL-01.D	Sample	14.436	593	1262	0.002
PL-02.D	Sample			1266	ND
MBK.D	Blank			1069	ND
CCV(N).D	QC	14.430	13470	1398	0.044

Naphthalene

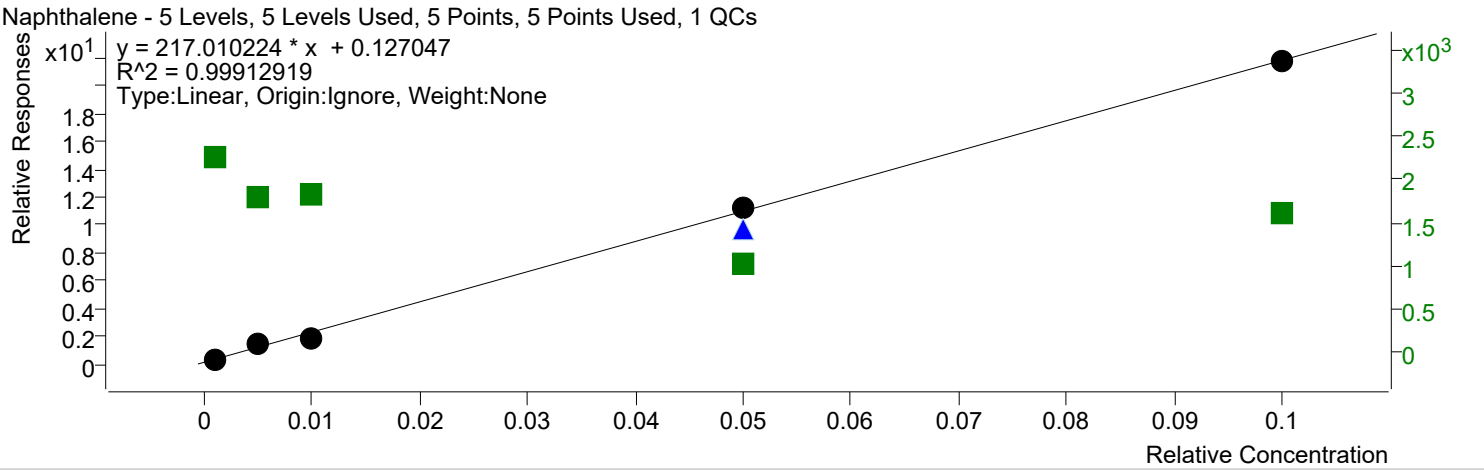

Cal. Path	Type	Level	Enable	Conc.	Response
D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\Naphthalene ST-01.D	Calibration	1	x	0.001	747
D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\Naphthalene ST-02.D	Calibration	2	x	0.005	2683
D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\Naphthalene ST-03.D	Calibration	3	x	0.010	3481
D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\Naphthalene ST-04.D	Calibration	4	x	0.050	11525
D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\CCV(N).D	QC	4	x	0.050	13470
D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\Naphthalene ST-05.D	Calibration	5	x	0.100	34939

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\Naphthalene.batch.bin		
Analysis Time	2026-01-08 오후 12:02:33	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:06:17	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 12:02:33	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-02 오전 11:56:02	**Data File**	Naphthalene ST-01.D
Type	Cal	**Name**	Naphthalene ST-01
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

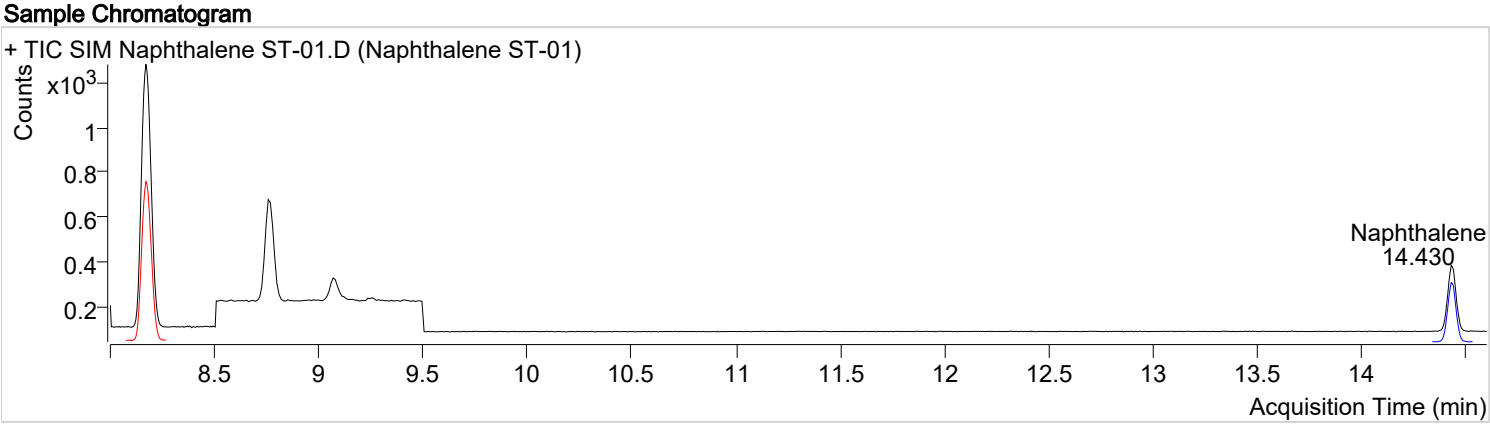

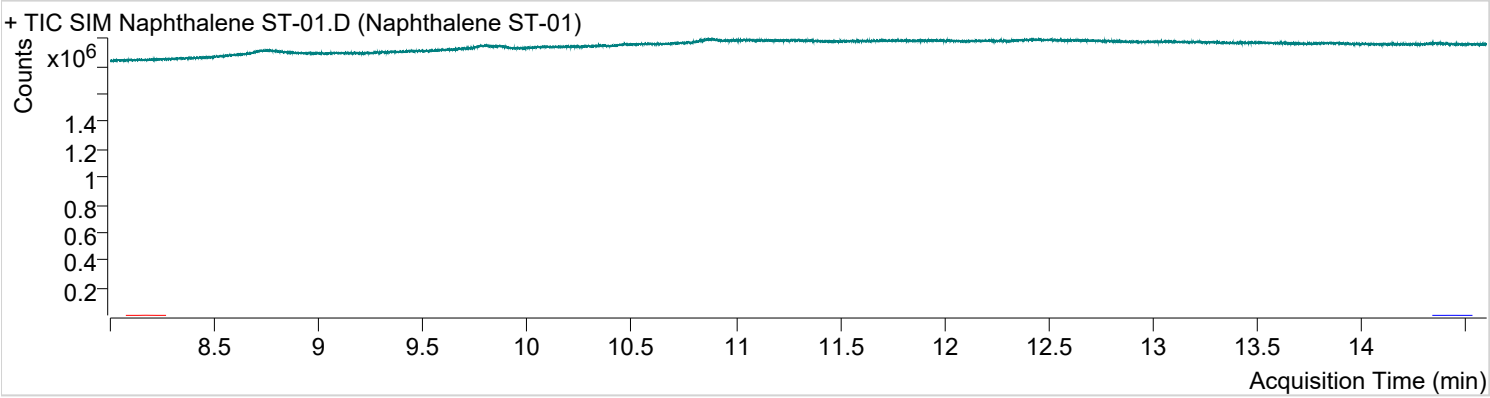

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	14.430	747	2254	0.001 mg/L

Naphthalene

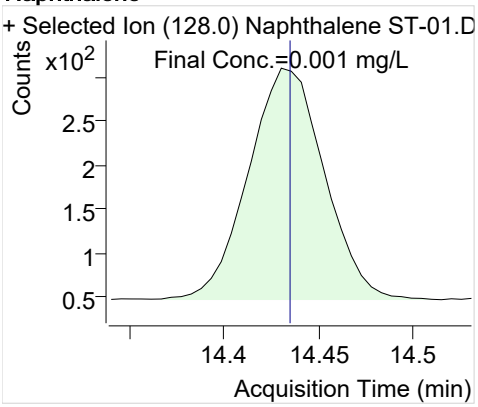

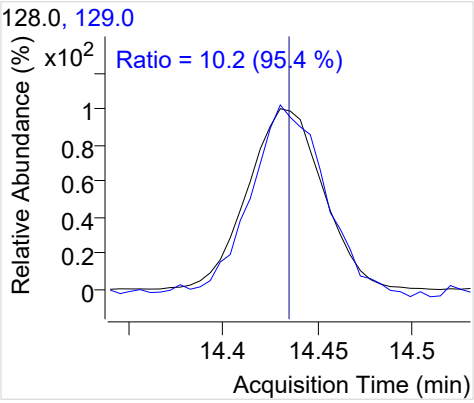



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\Naphthalene.batch.bin		
Analysis Time	2026-01-08 오후 12:02:33	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:06:17	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 12:02:33	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-02 오후 12:12:44	**Data File**	Naphthalene ST-02.D
Type	Cal	**Name**	Naphthalene ST-02
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

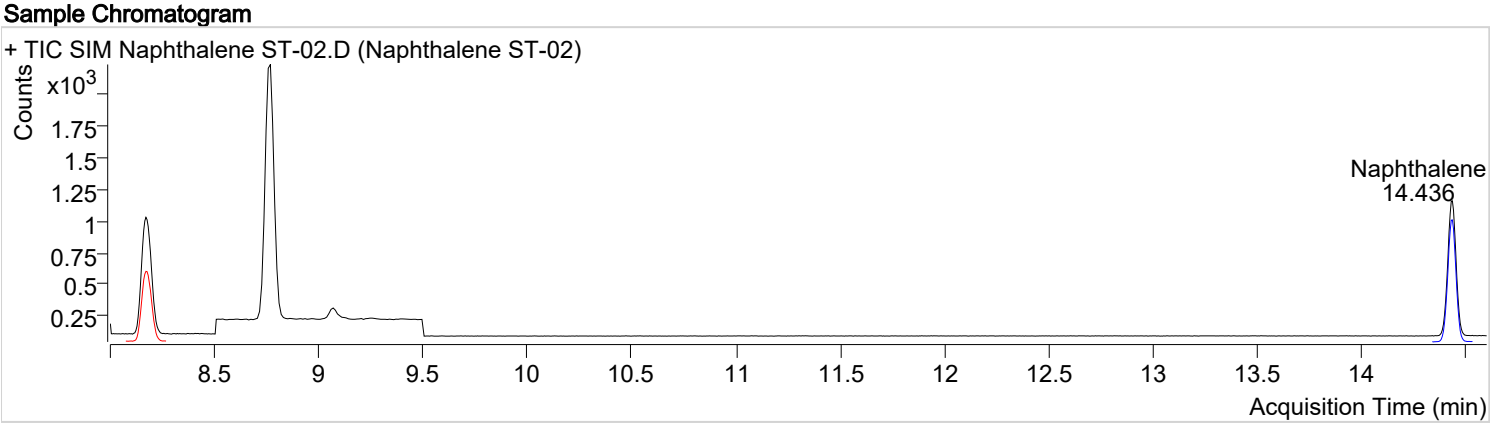

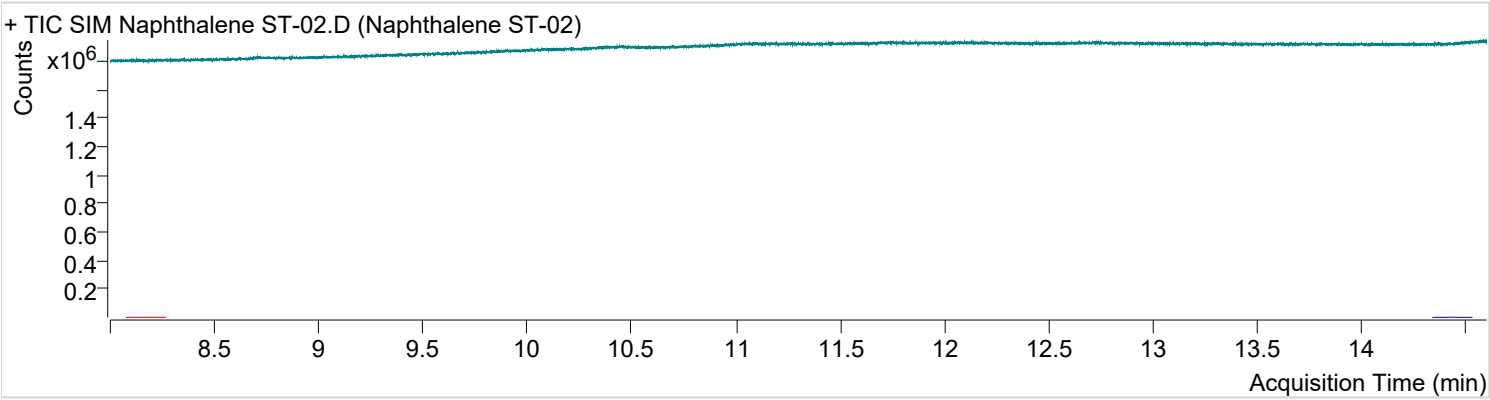

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	14.436	2683	1806	0.006 mg/L

Naphthalene

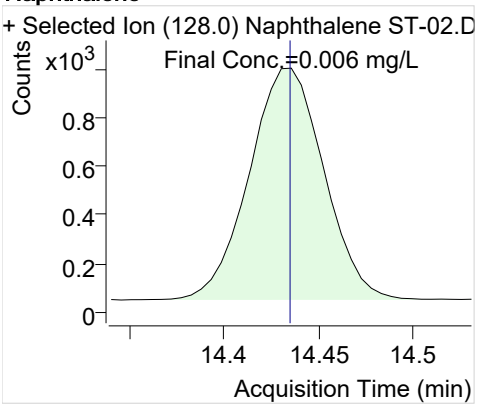

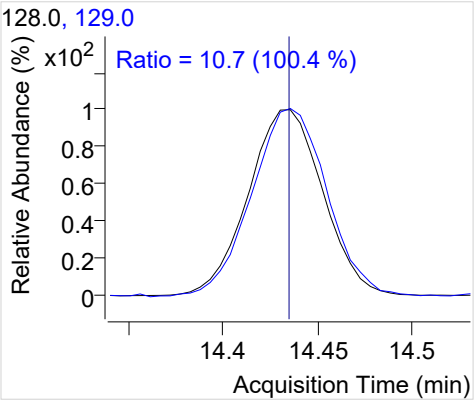



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\Naphthalene.batch.bin		
Analysis Time	2026-01-08 오후 12:02:33	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:06:17	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 12:02:33	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-02 오후 12:29:27	**Data File**	Naphthalene ST-03.D
Type	Cal	**Name**	Naphthalene ST-03
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

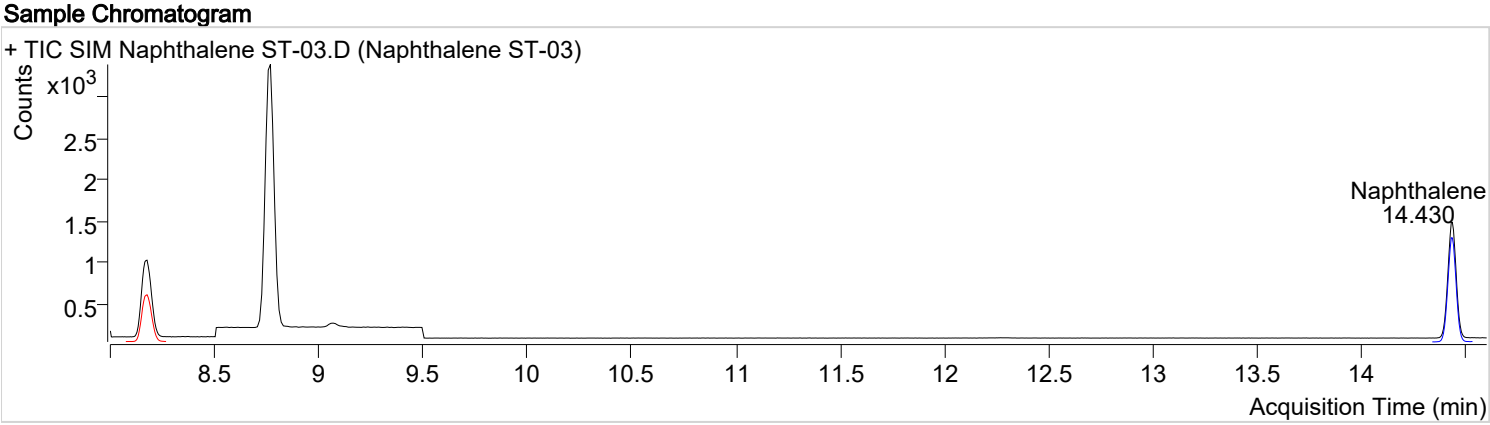

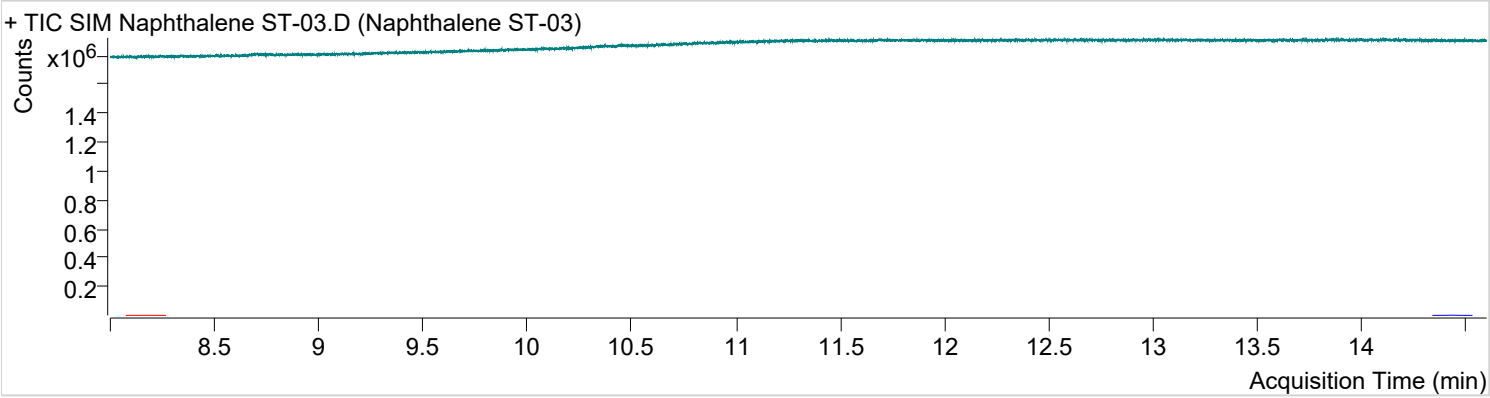

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	14.430	3481	1834	0.008 mg/L

Naphthalene

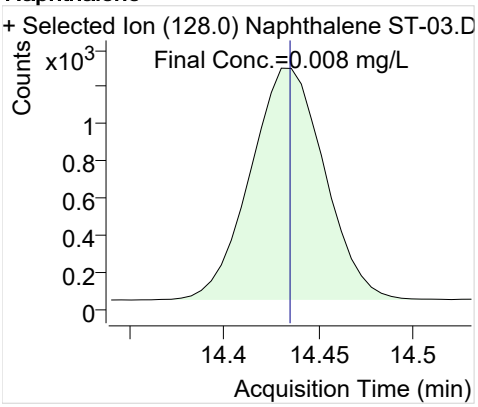

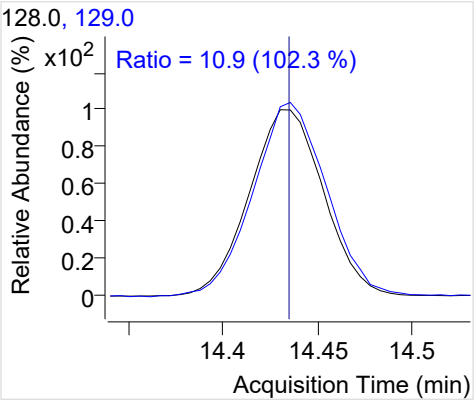



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\Naphthalene.batch.bin		
Analysis Time	2026-01-08 오후 12:02:33	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:06:17	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 12:02:33	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-02 오후 12:46:09	**Data File**	Naphthalene ST-04.D
Type	Cal	**Name**	Naphthalene ST-04
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

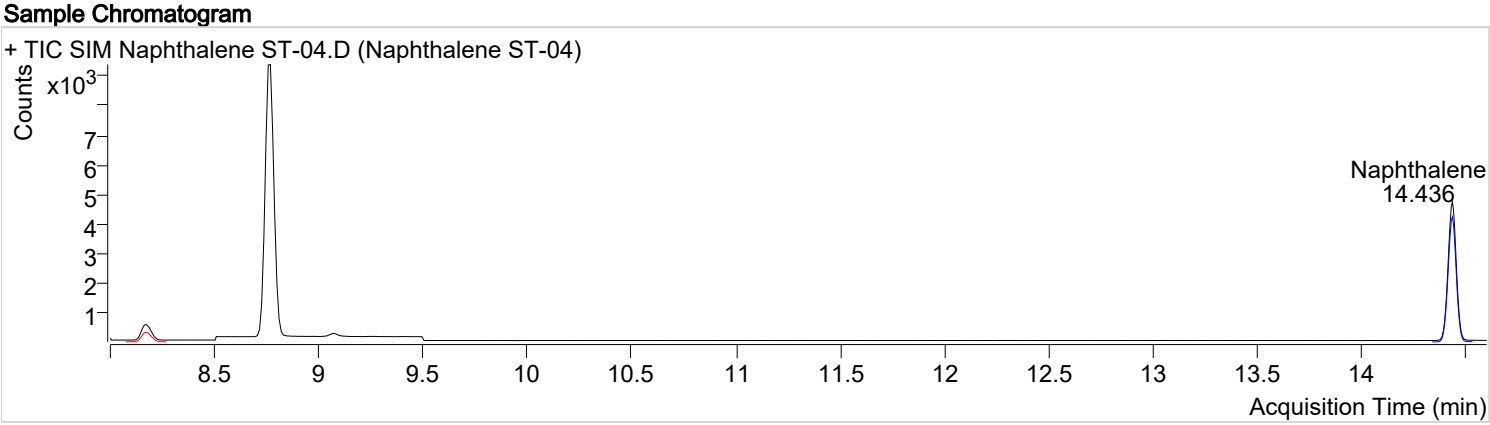

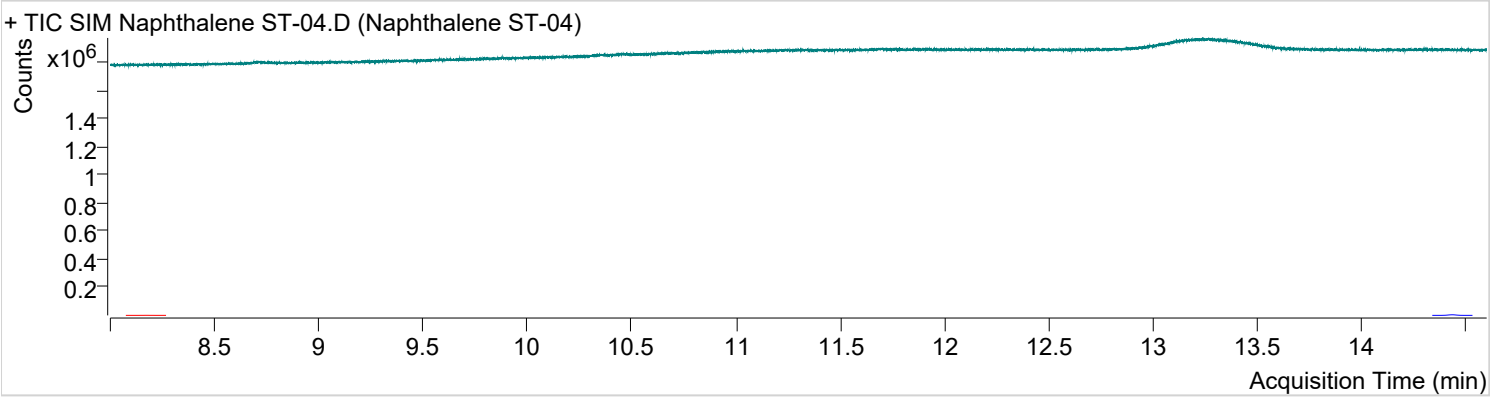

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	14.436	11525	1029	0.051 mg/L

Naphthalene

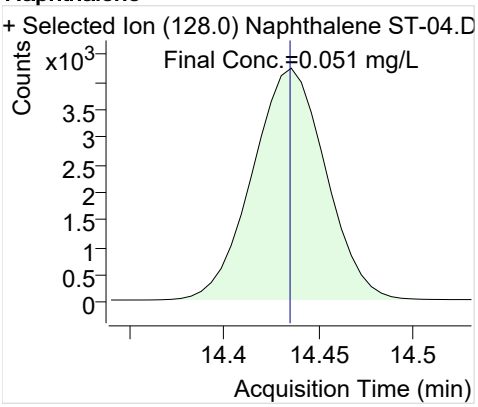

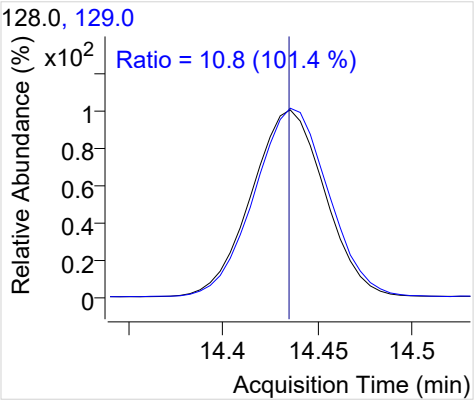



Generated at 오후 3:06 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\Naphthalene.batch.bin		
Analysis Time	2026-01-08 오후 12:02:33	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:06:17	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 12:02:33	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-02 오후 1:02:53	**Data File**	Naphthalene ST-05.D
Type	Cal	**Name**	Naphthalene ST-05
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

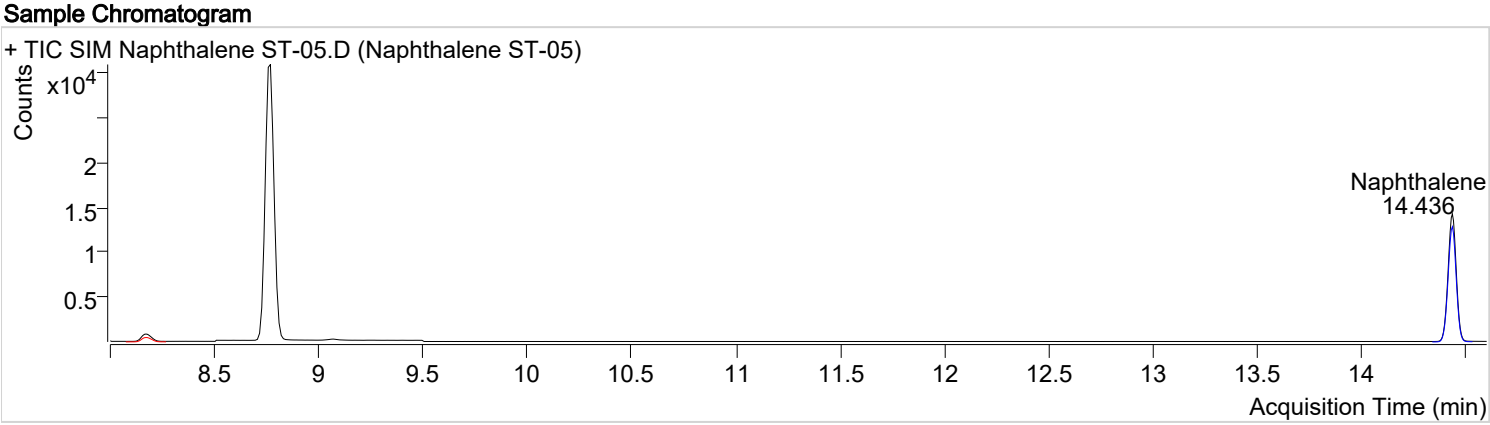

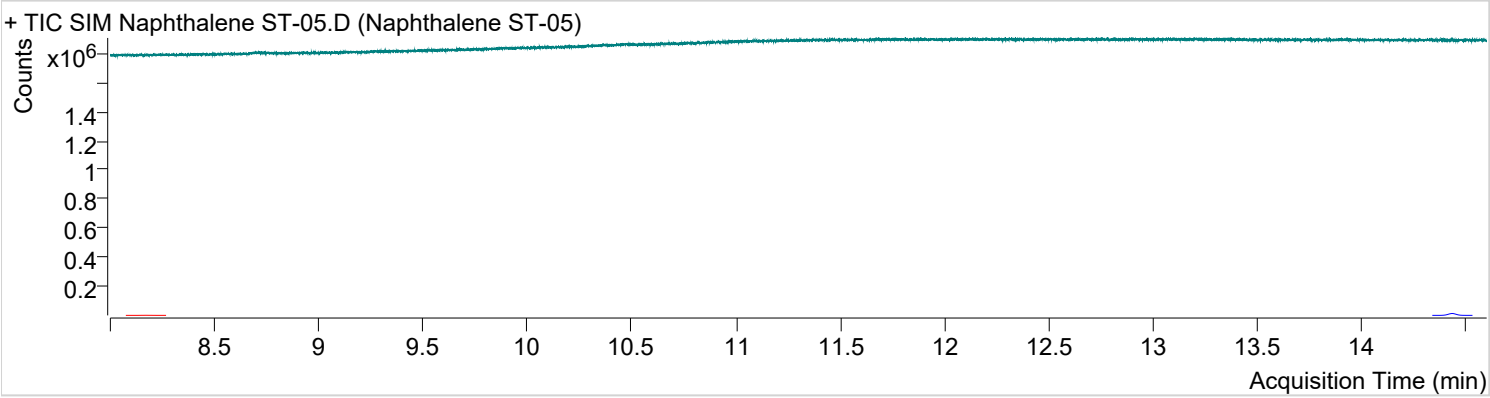

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	14.436	34939	1607	0.100 mg/L

Naphthalene

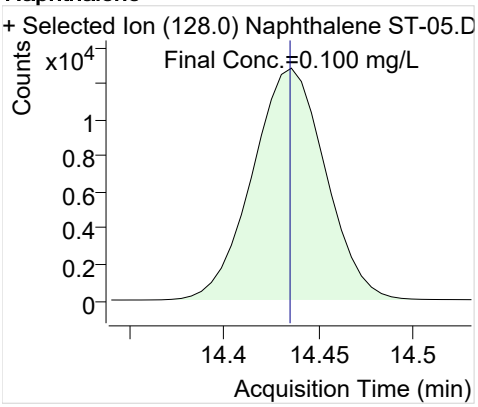

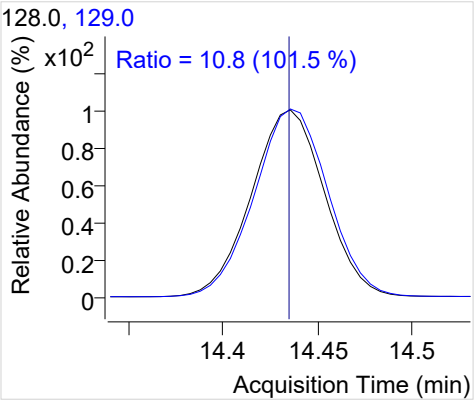



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\Naphthalene.batch.bin		
Analysis Time	2026-01-08 오후 12:02:33	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:06:17	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 12:02:33	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-02 오후 3:22:48	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

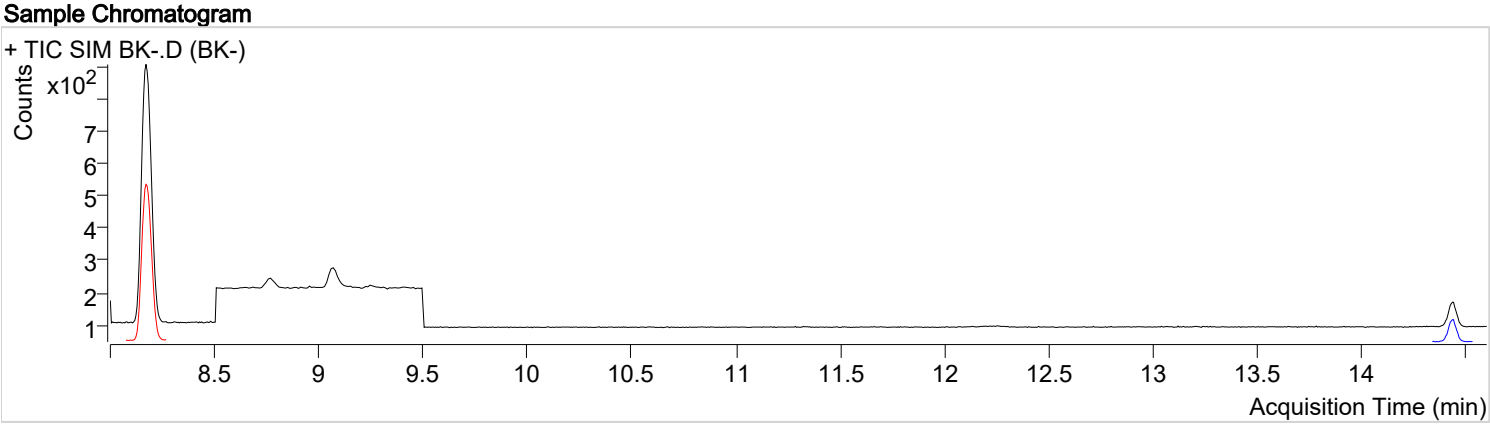

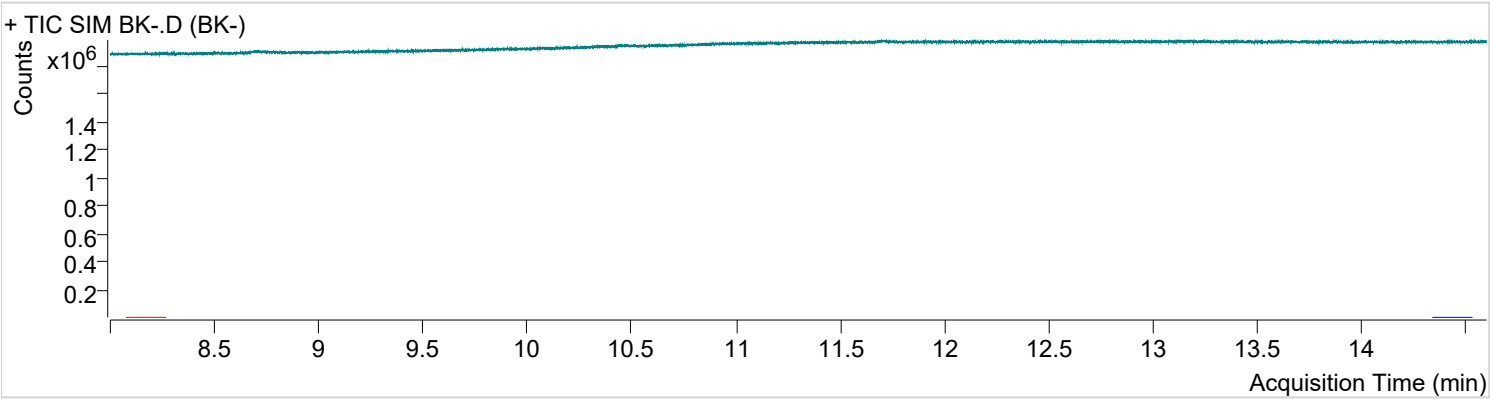

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			1587	ND mg/L

Naphthalene

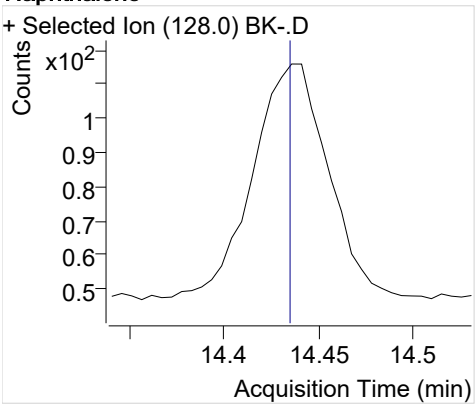

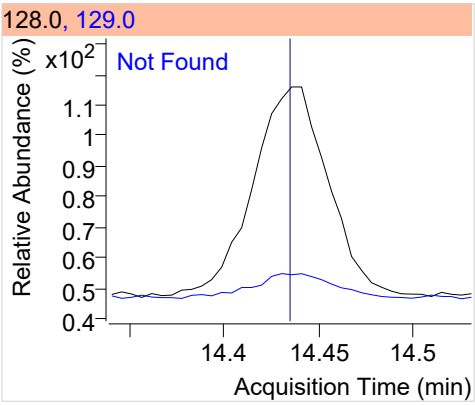



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\Naphthalene.batch.bin		
Analysis Time	2026-01-08 오후 12:02:33	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:06:17	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 12:02:33	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-02 오후 3:40:30	**Data File**	FBK(PL 25-12-30).D
Type	Blank	**Name**	FBK(PL 25-12-30)
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

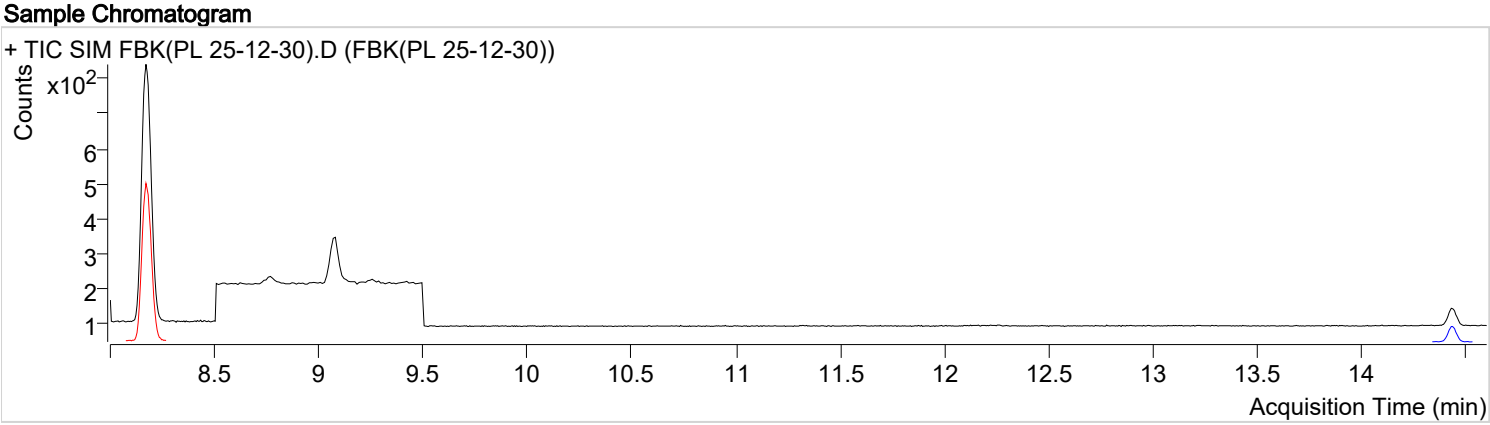

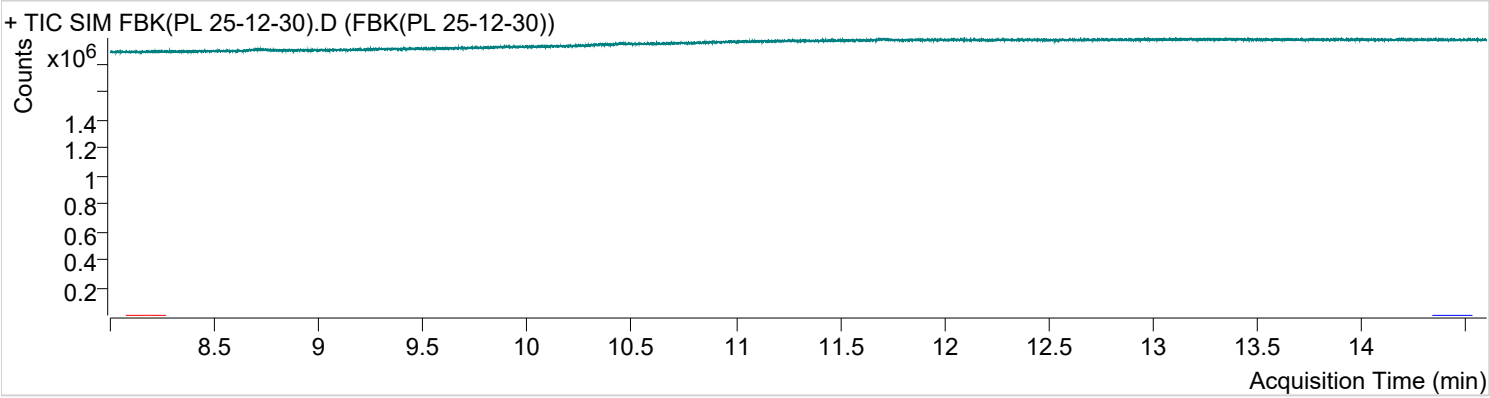

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			1419	ND mg/L

Naphthalene

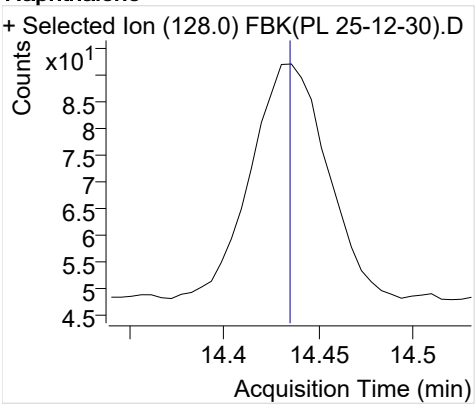

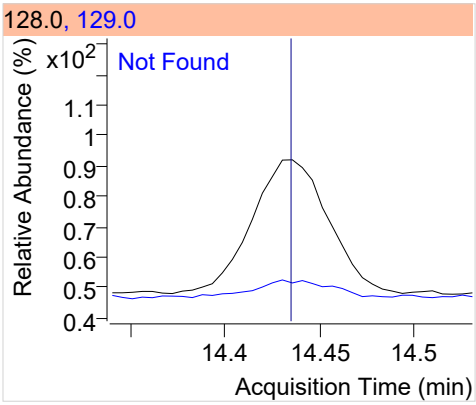

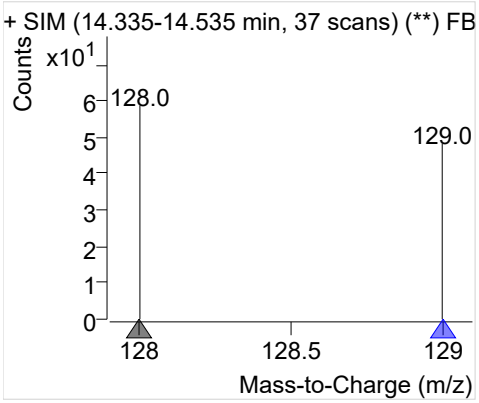

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\Naphthalene.batch.bin		
Analysis Time	2026-01-08 오후 12:02:33	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:06:17	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 12:02:33	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-02 오후 3:58:19	**Data File**	PL-01.D
Type	Sample	**Name**	PL-01
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

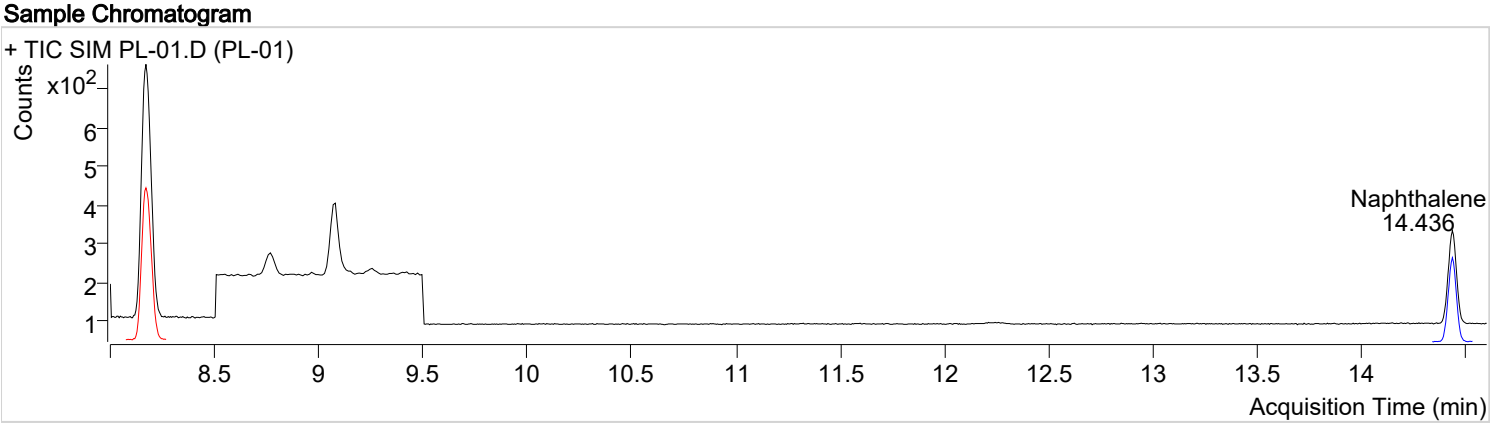

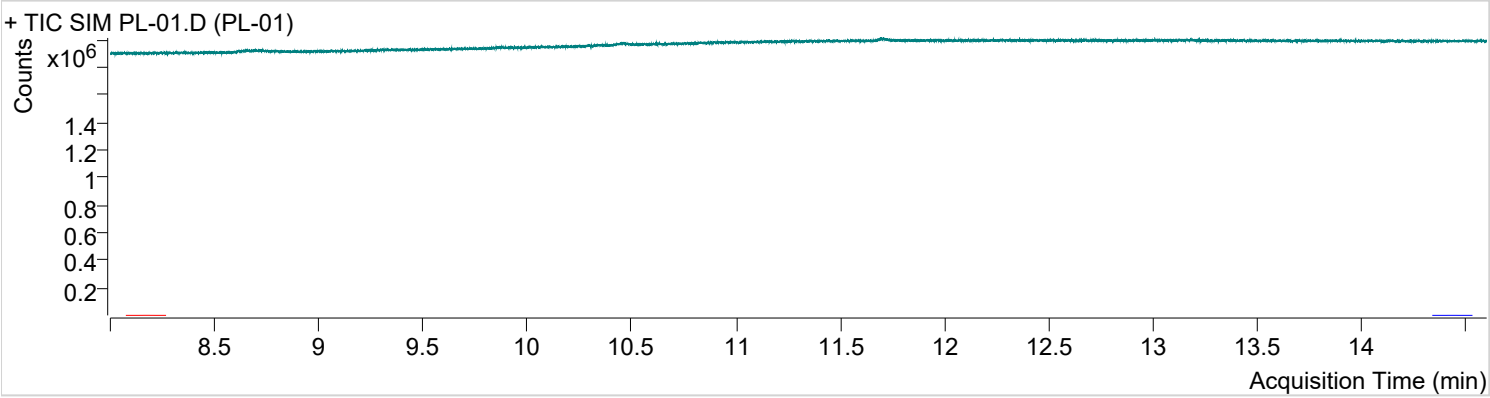

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	14.436	593	1262	0.002 mg/L

Naphthalene

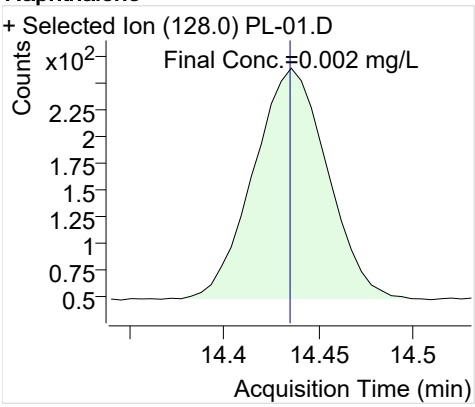

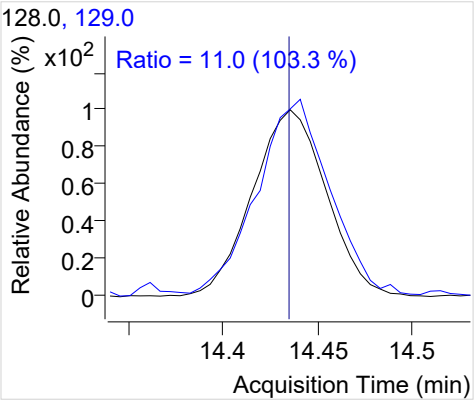



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\Naphthalene.batch.bin		
Analysis Time	2026-01-08 오후 12:02:33	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:06:17	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 12:02:33	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-02 오후 4:16:03	**Data File**	PL-02.D
Type	Sample	**Name**	PL-02
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

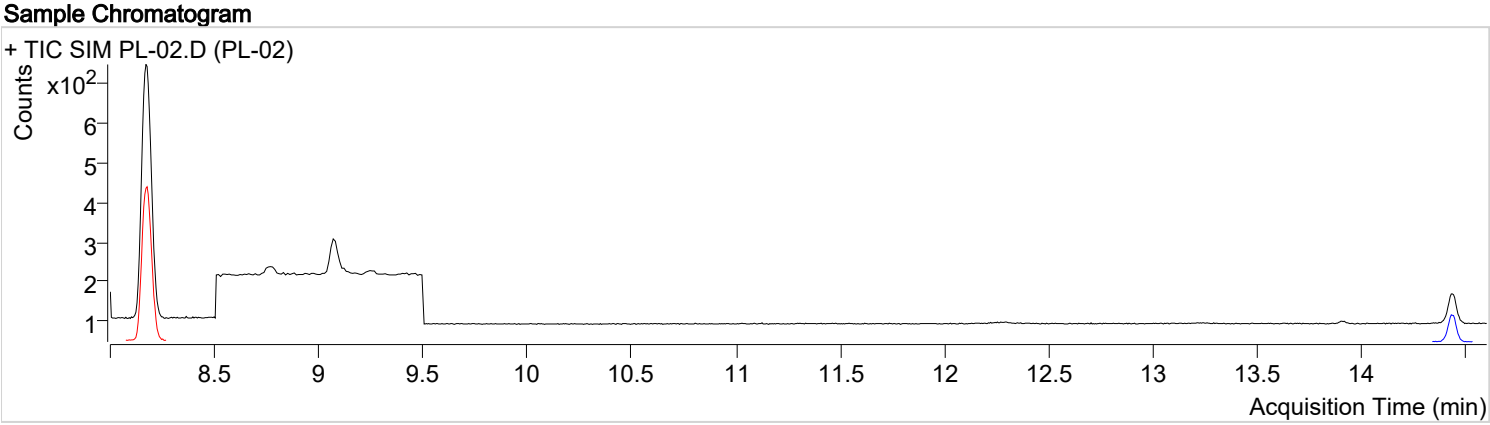

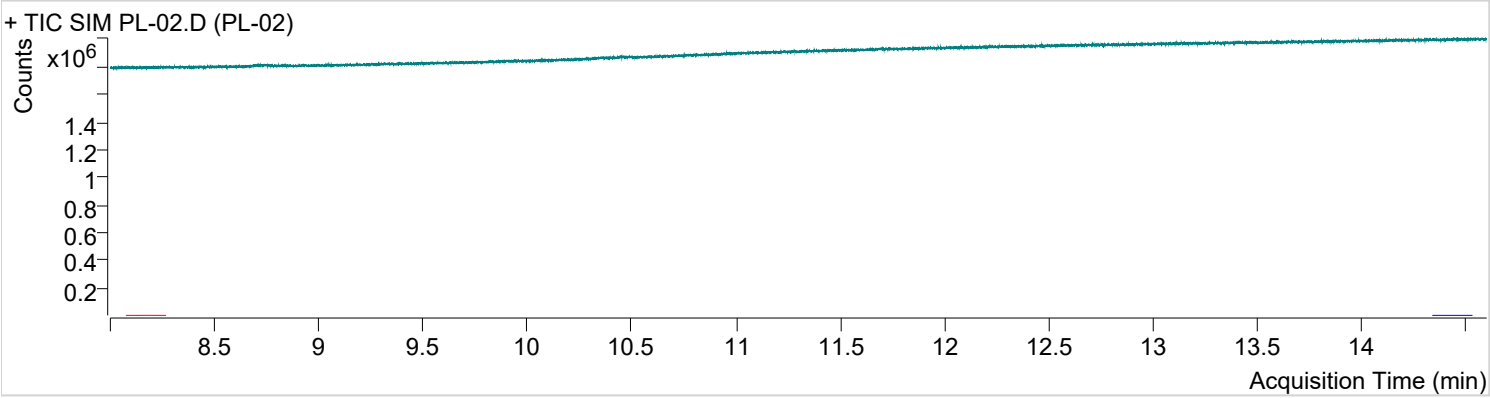

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			1266	ND mg/L

Naphthalene

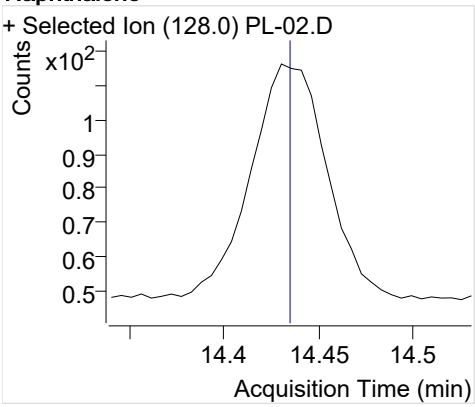

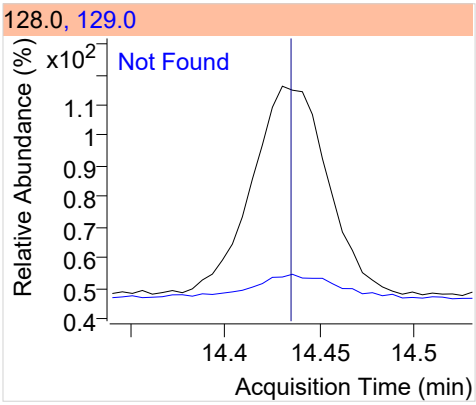



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\Naphthalene.batch.bin		
Analysis Time	2026-01-08 오후 12:02:33	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:06:17	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 12:02:33	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-02 오후 4:51:35	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

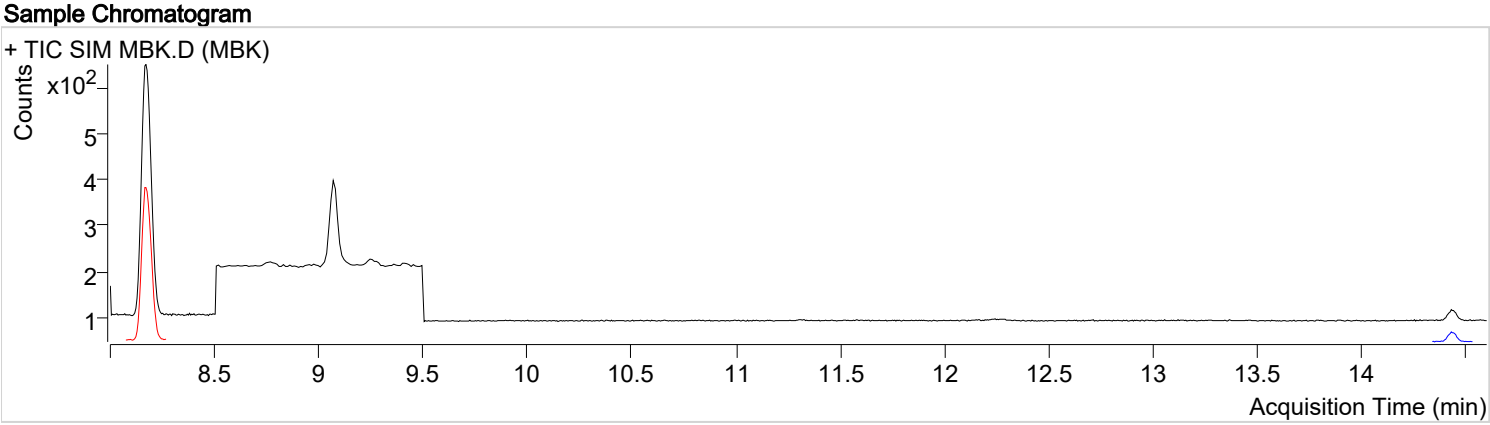

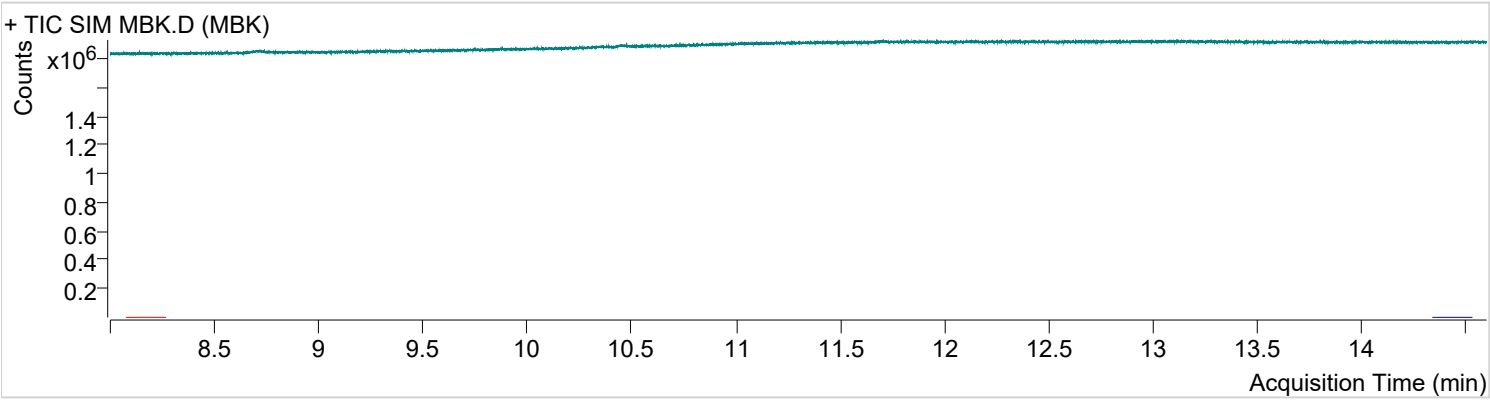

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			1069	ND mg/L

Naphthalene

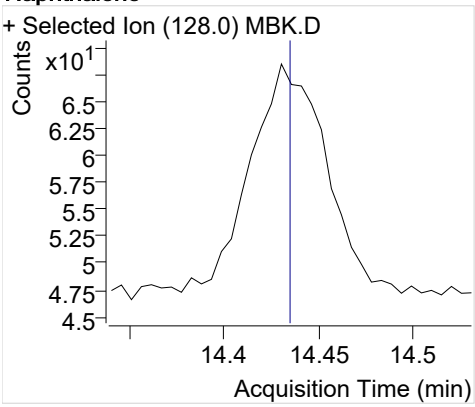

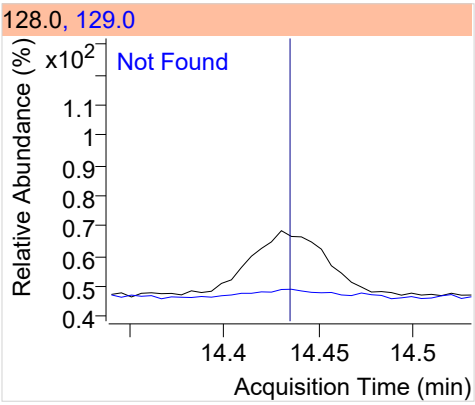



Generated at 오후 3:06 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\Naphthalene.batch.bin		
Analysis Time	2026-01-08 오후 12:02:33	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:06:17	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 12:02:33	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-02 오후 5:09:18	**Data File**	CCV(N).D
Type	QC	**Name**	CCV(N)
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

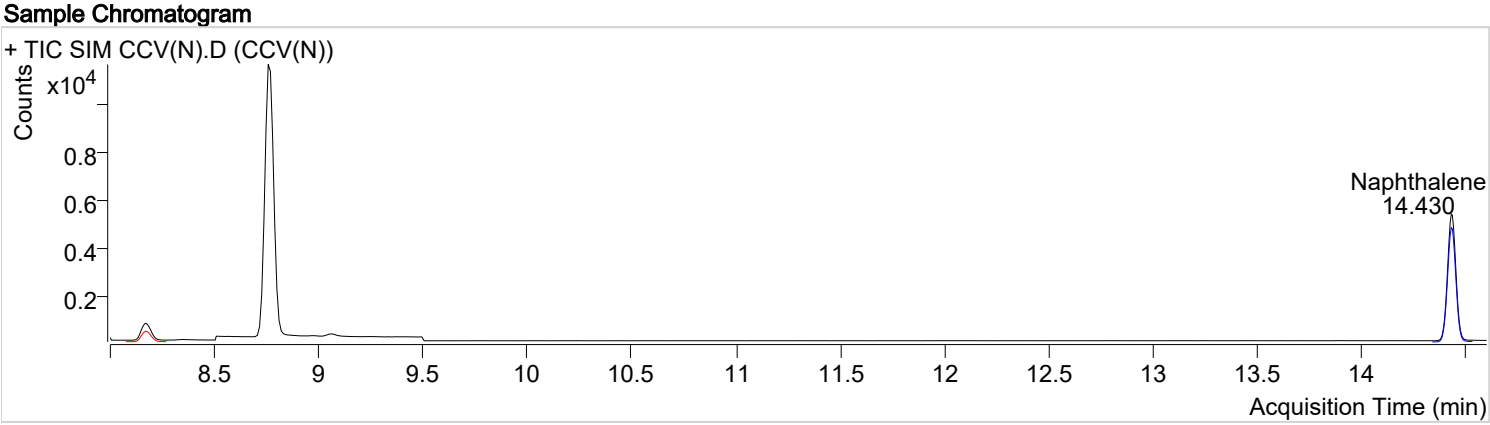

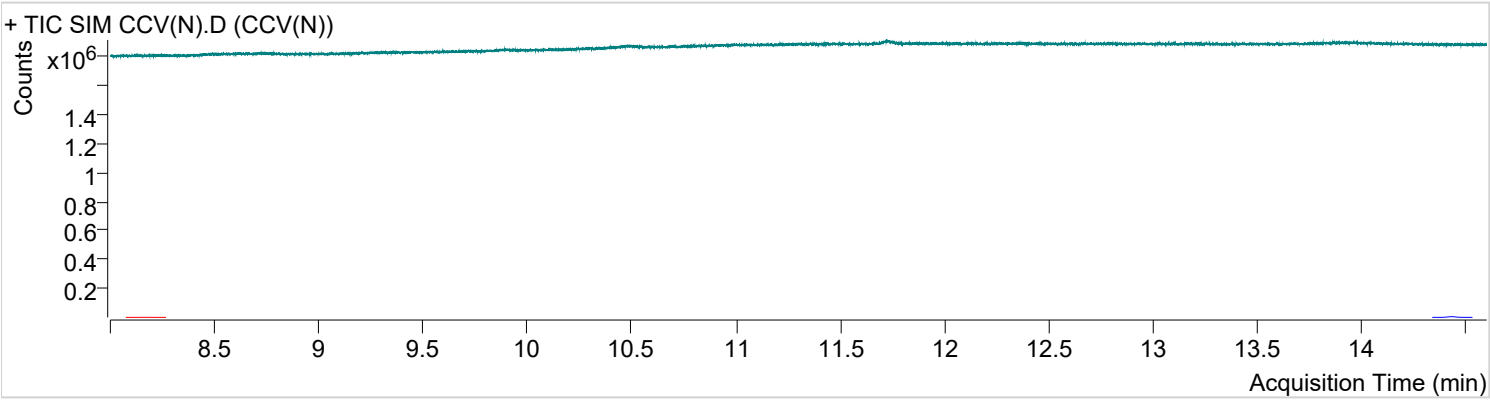

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	14.430	13470	1398	0.044 mg/L

Naphthalene

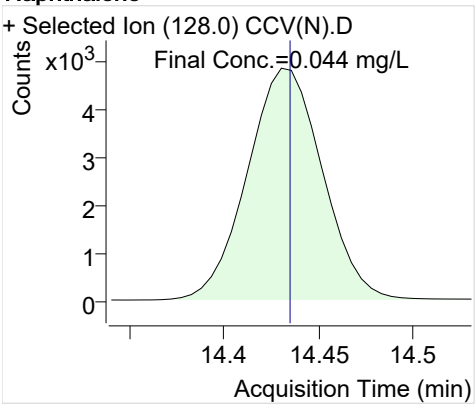

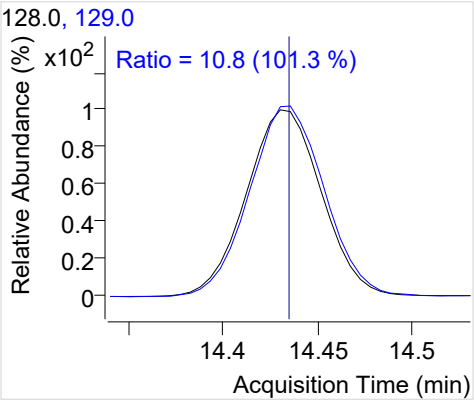



Generated at 오후 3:06 on 2026-04-10