Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin				
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Naphthalene

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
NA ST-01.d	Cal	10.829	4652	9219	0.001
NA ST-02.d	Cal	10.826	18568	8542	0.005
NA ST-03.d	Cal	10.822	39872	9047	0.009
NA ST-04.d	Cal	10.818	193495	8085	0.052
NA ST-05.d	Cal	10.815	402897	8877	0.099
BK-.d	Blank	10.826	1921	8657	0.000
FBK(GS 26-02-10).d	Blank	10.826	1221	8452	0.000
KH (26-02-10).d	Blank	10.826	0	7853	ND
GS-01.d	Sample	10.822	16127	8071	0.004
GS-02.d	Sample	10.815	435174	8266	0.115
GS-03.d	Sample	10.822	0	6998	ND
GS-04.d	Sample	10.822	0	8098	ND
GS-05.d	Sample	10.818	11208	7436	0.003
GS-06.d	Sample	10.826	0	6985	ND
GS-15.d	Sample	10.826	0	6032	ND
GS-02 R.d	Sample	10.815	90253	7272	0.135
MBK-1.d	Blank	10.826	755	8599	0.000
CCV N.d	QC	10.818	163451	6779	0.053
SOL 1.d	Sample	10.826	0	4445	ND
SOL 2.d	Sample	10.826	0	4708	ND
SOL 3.d	Sample	10.826	0	4832	ND

Naphthalene

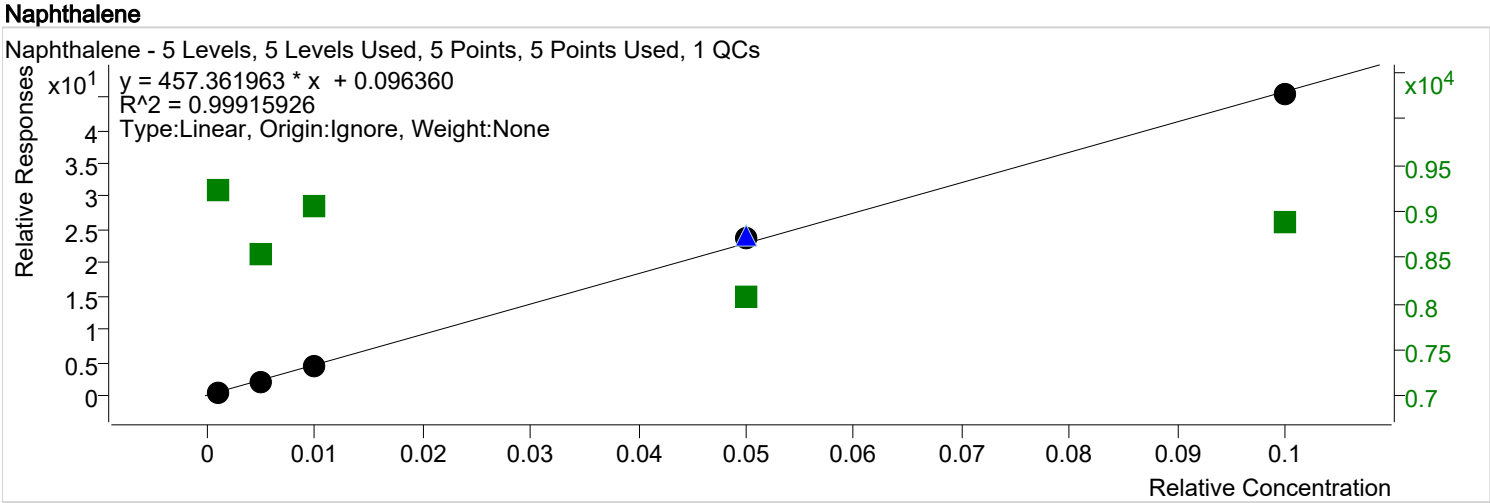

Cal. Path	Type	Level	Enable	Conc.	Response
V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\NA ST-01.d	Calibration	1	x	0.001	4652
V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\NA ST-02.d	Calibration	2	x	0.005	18568
V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\NA ST-03.d	Calibration	3	x	0.010	39872
V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\NA ST-04.d	Calibration	4	x	0.050	193495
V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\CCV N.d	QC	4	x	0.050	163451
V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\NA ST-05.d	Calibration	5	x	0.100	402897

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오전 10:07:32	**Data File**	NA ST-01.d
Type	Cal	**Name**	NA ST-01
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

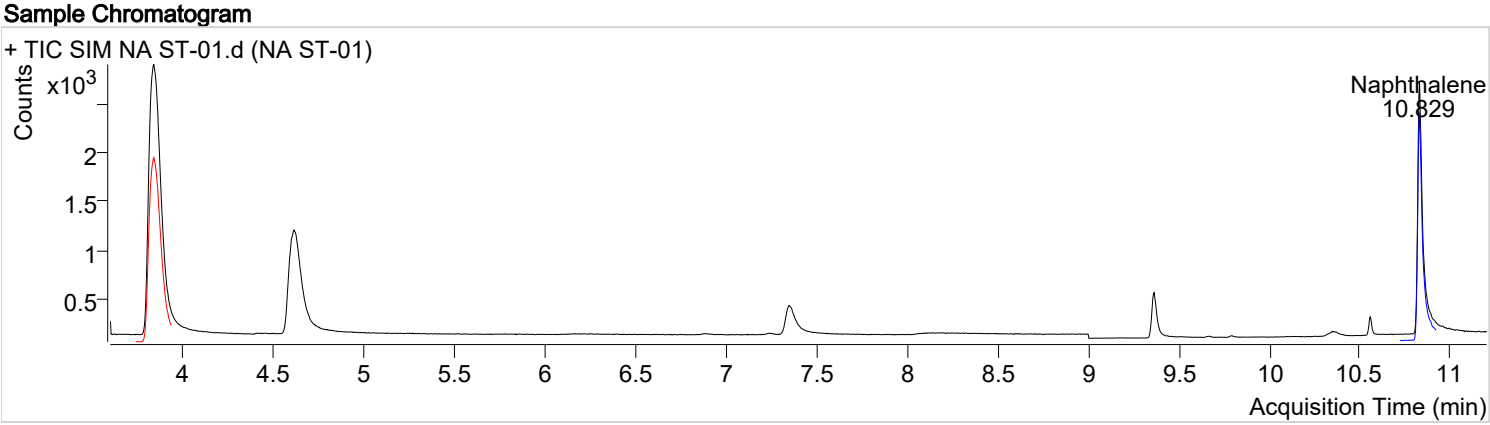

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.829	4652	9219	0.001 mg/L

Naphthalene







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오전 10:24:40	**Data File**	NA ST-02.d
Type	Cal	**Name**	NA ST-02
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

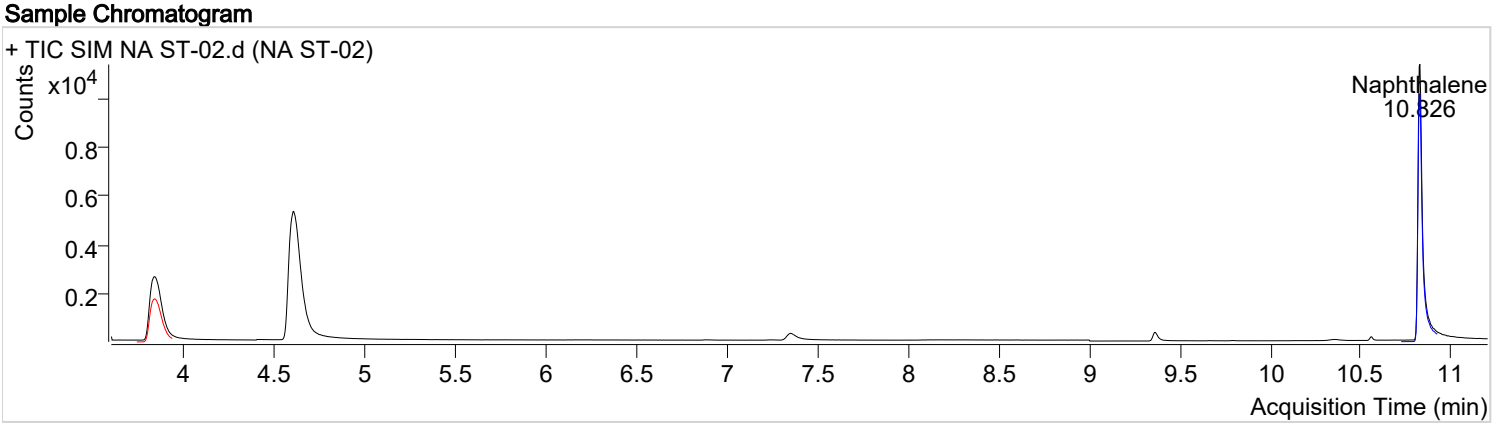

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.826	18568	8542	0.005 mg/L

Naphthalene







Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오전 10:41:48	**Data File**	NA ST-03.d
Type	Cal	**Name**	NA ST-03
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

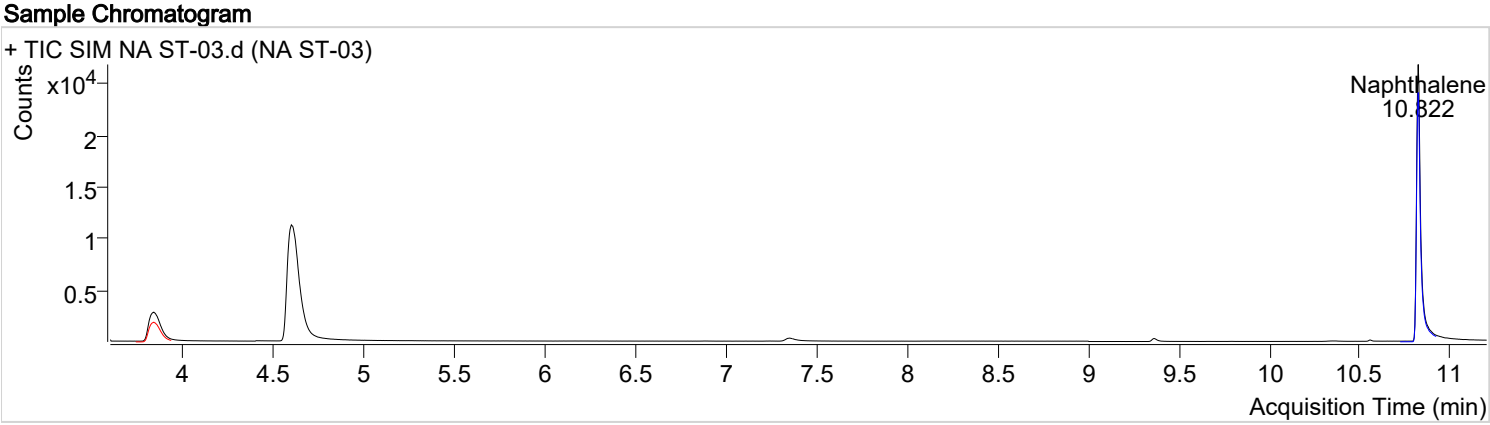

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.822	39872	9047	0.009 mg/L

Naphthalene







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오전 10:58:52	**Data File**	NA ST-04.d
Type	Cal	**Name**	NA ST-04
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

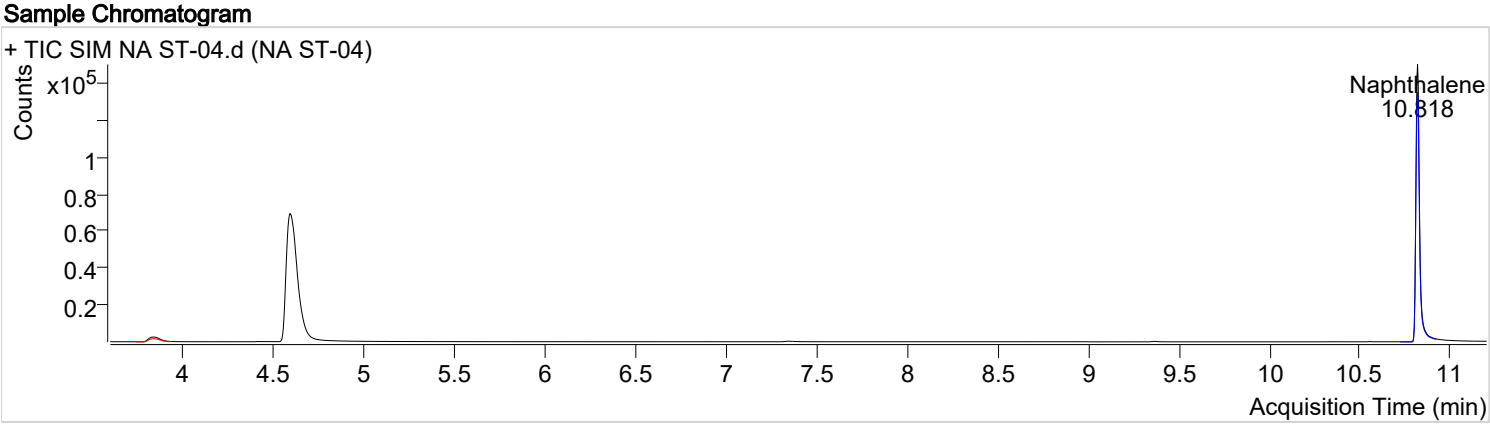

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.818	193495	8085	0.052 mg/L

Naphthalene







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오전 11:16:00	**Data File**	NA ST-05.d
Type	Cal	**Name**	NA ST-05
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

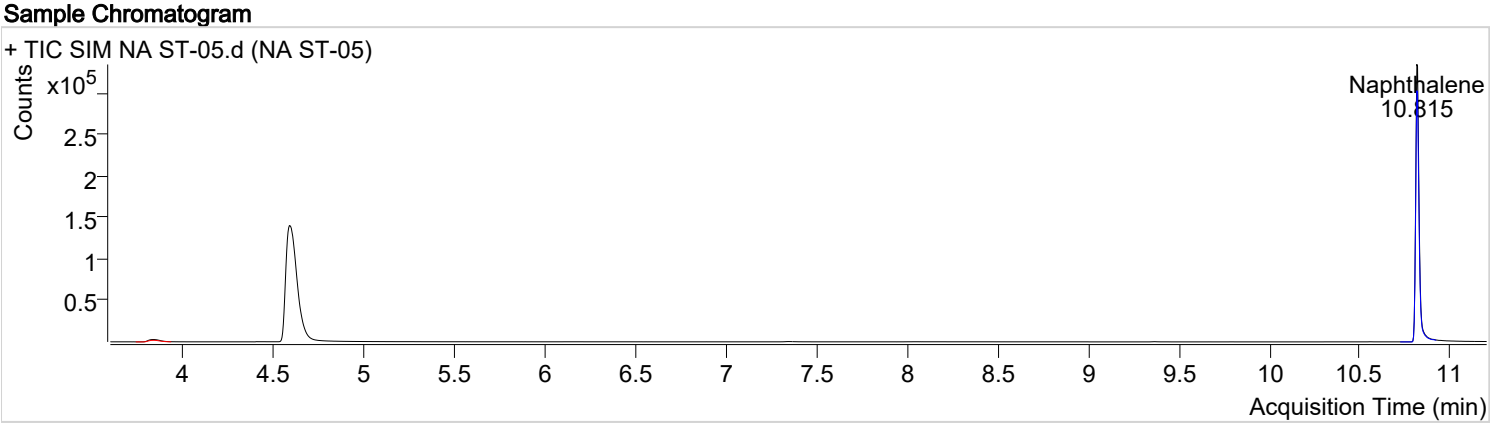

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.815	402897	8877	0.099 mg/L

Naphthalene

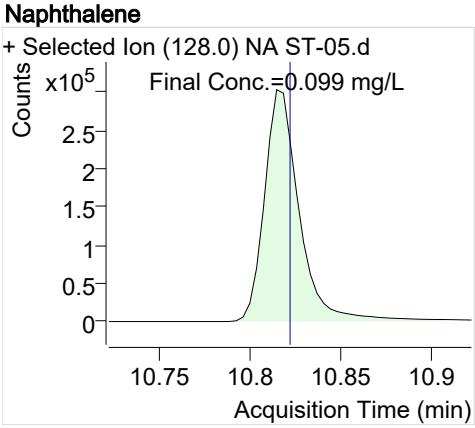





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오후 1:32:46	**Data File**	BK-.d
Type	Blank	**Name**	BK-
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

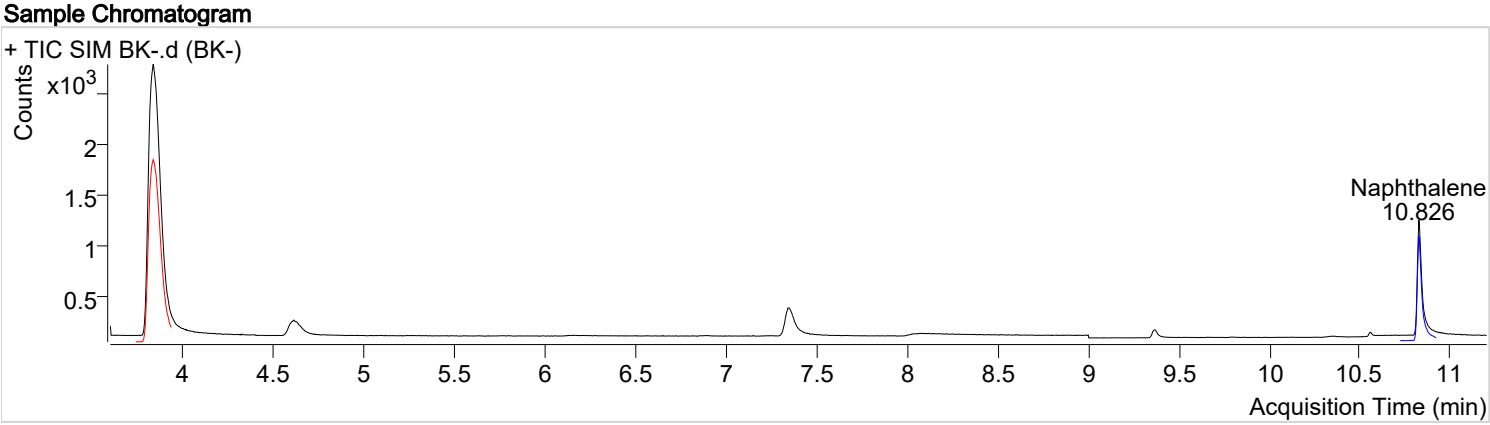

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.826	1921	8657	0.000 mg/L

Naphthalene







Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오후 1:49:54	**Data File**	FBK(GS 26-02-10).d
Type	Blank	**Name**	FBK(GS 26-02-10)
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

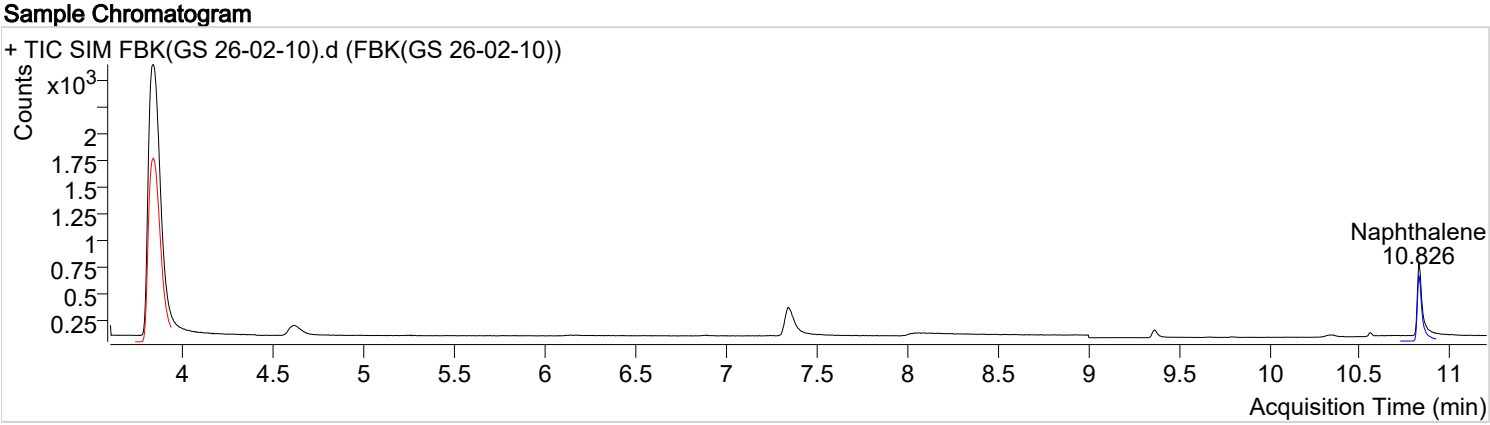

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.826	1221	8452	0.000 mg/L

Naphthalene



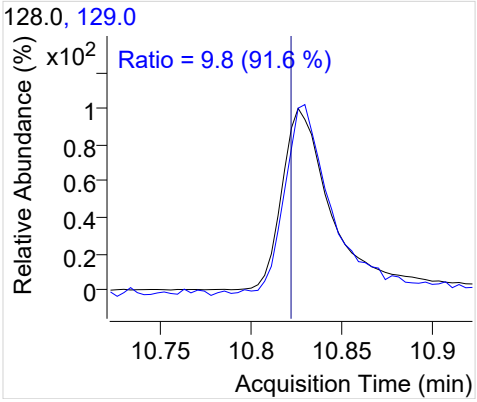

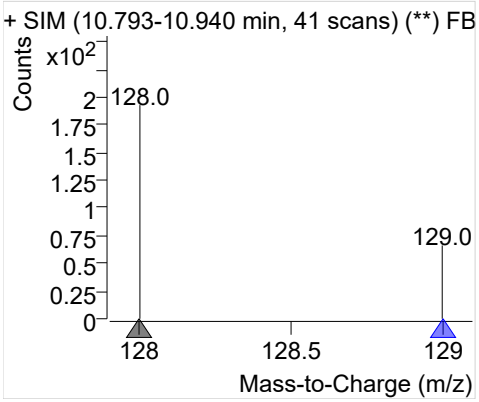

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오후 2:07:03	**Data File**	KH (26-02-10).d
Type	Blank	**Name**	KH (26-02-10)
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

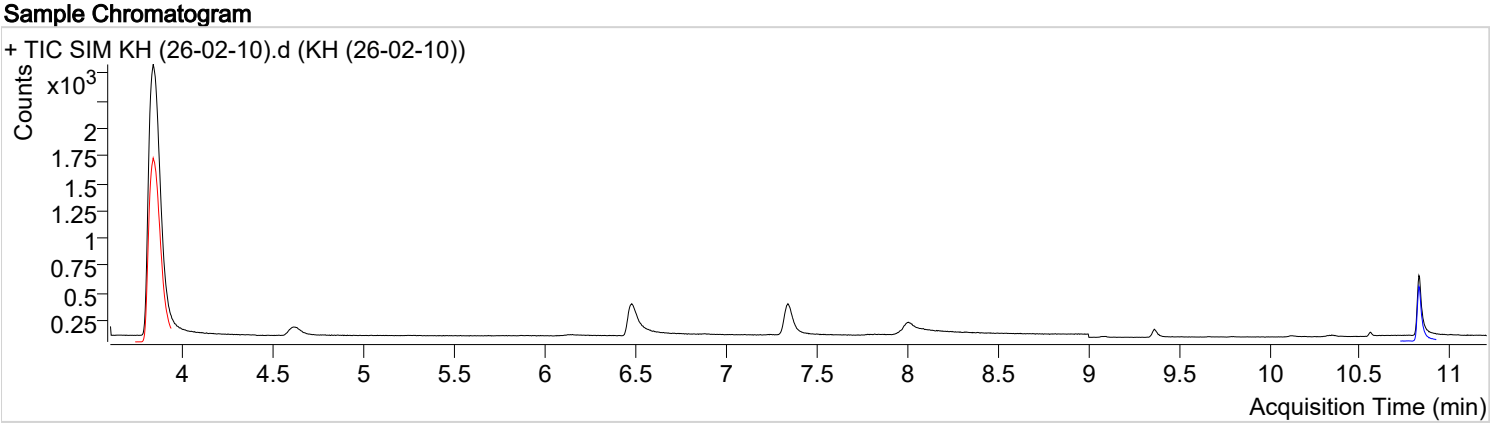

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.826	0	7853	ND mg/L

Naphthalene







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오후 2:20:25	**Data File**	GS-01.d
Type	Sample	**Name**	GS-01
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

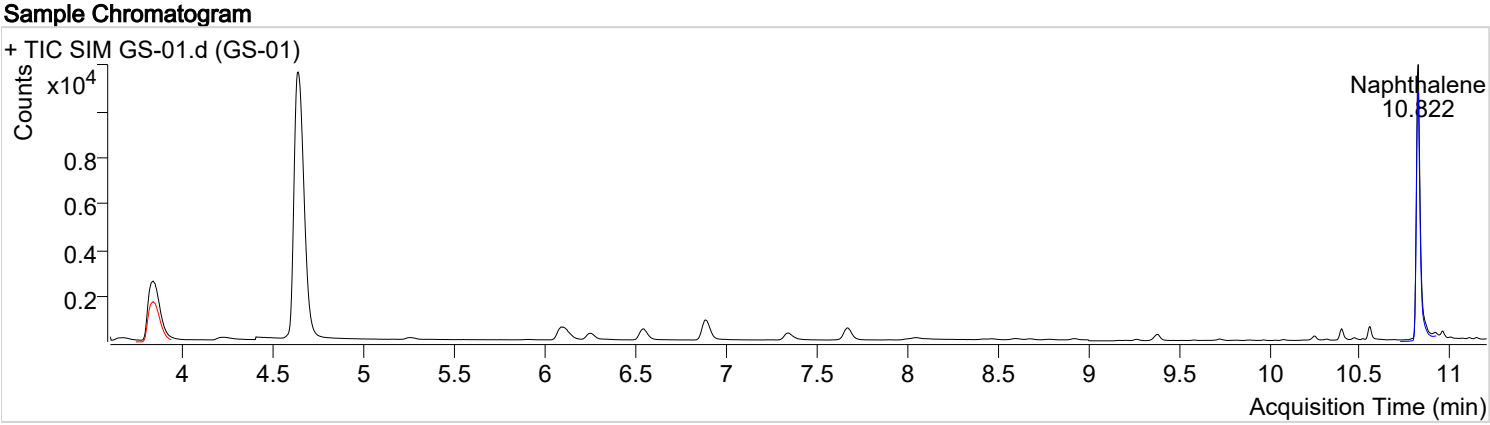

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.822	16127	8071	0.004 mg/L

Naphthalene







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오후 2:51:26	**Data File**	GS-02.d
Type	Sample	**Name**	GS-02
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

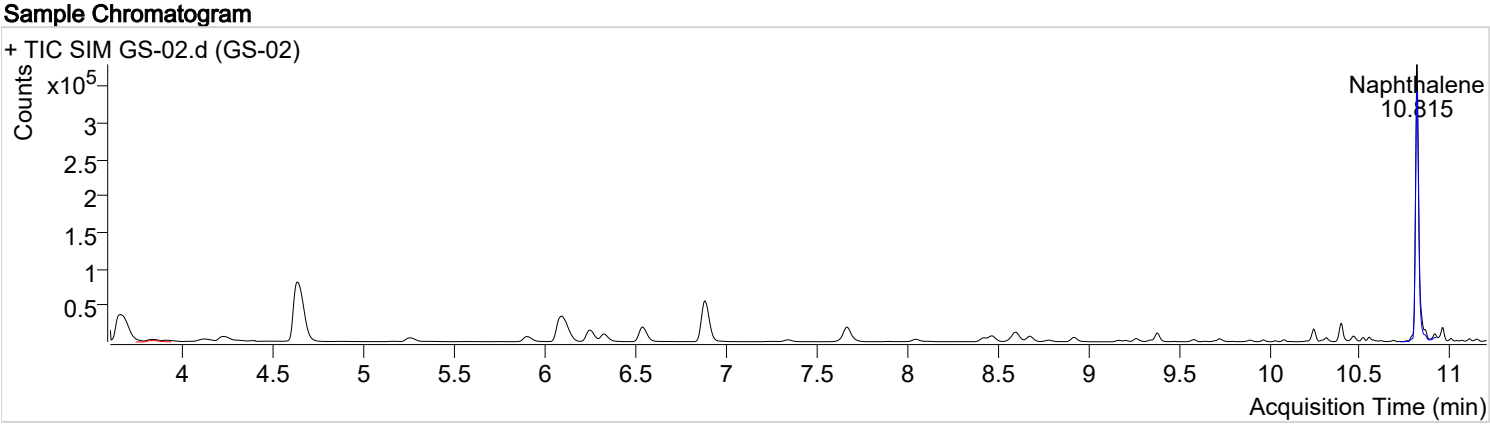

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.815	435174	8266	0.115 mg/L

Naphthalene







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오후 3:08:21	**Data File**	GS-03.d
Type	Sample	**Name**	GS-03
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

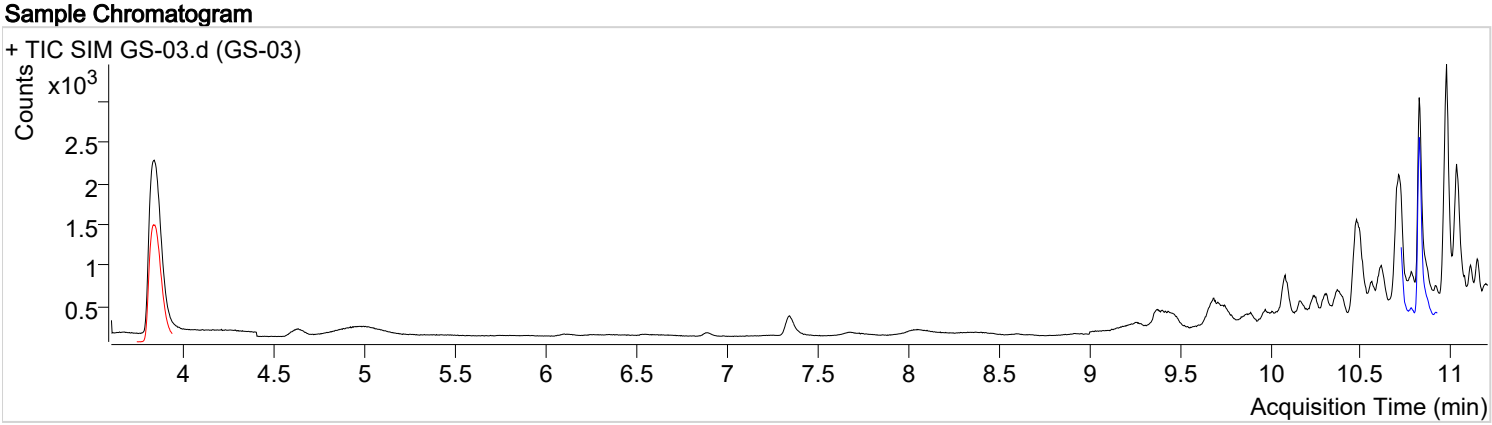

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.822	0	6998	ND mg/L

Naphthalene





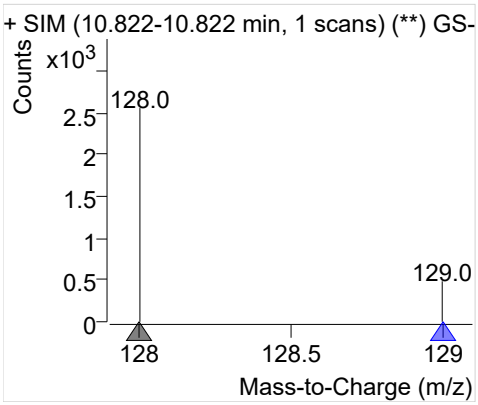

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오후 3:25:25	**Data File**	GS-04.d
Type	Sample	**Name**	GS-04
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

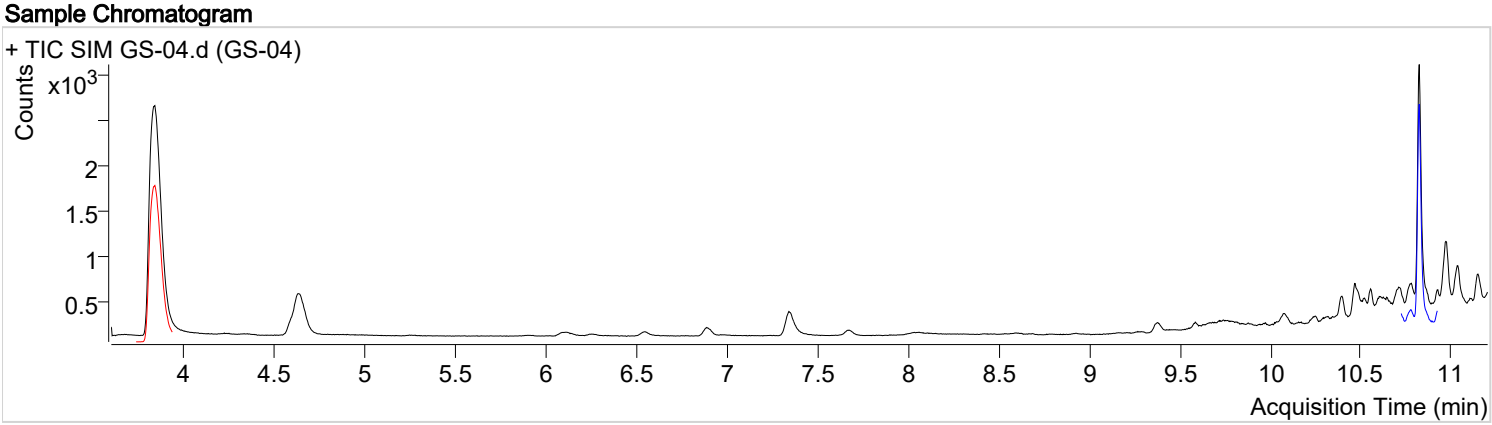

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.822	0	8098	ND mg/L

Naphthalene





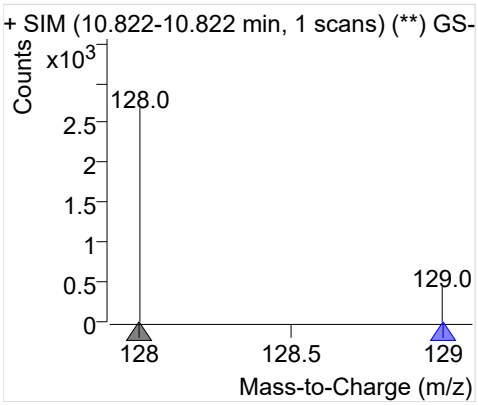

Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오후 3:38:49	**Data File**	GS-05.d
Type	Sample	**Name**	GS-05
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

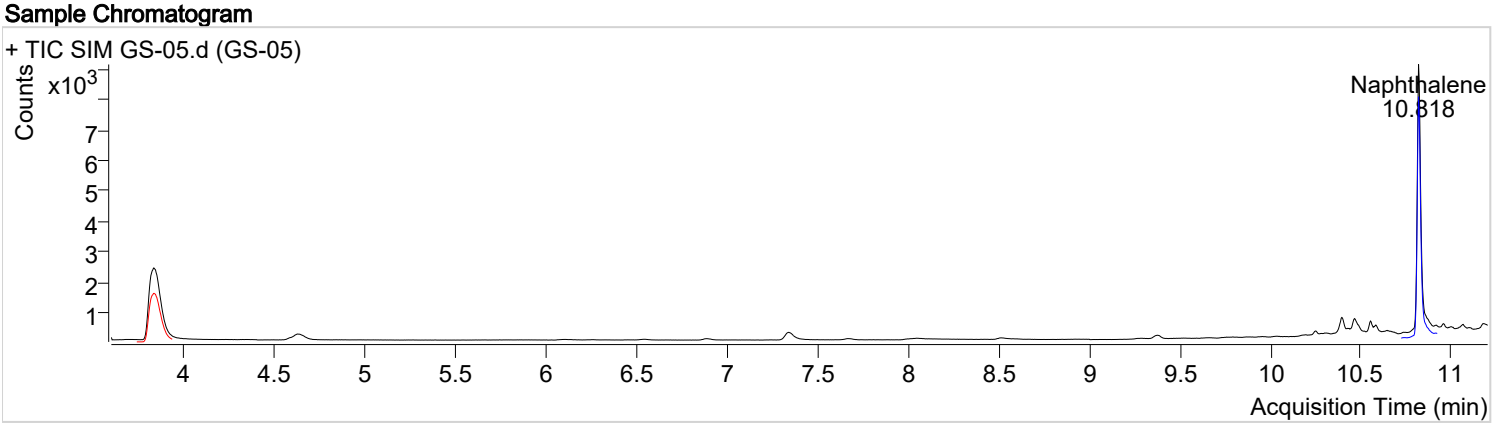

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.818	11208	7436	0.003 mg/L

Naphthalene





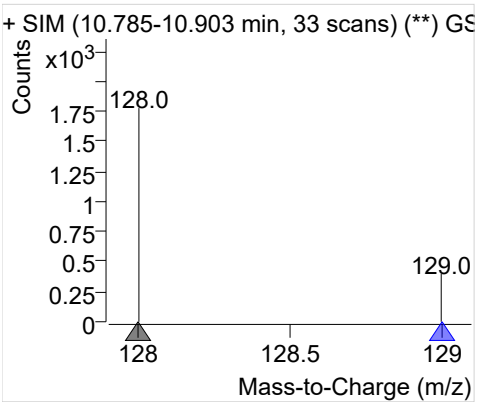

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오후 4:09:56	**Data File**	GS-06.d
Type	Sample	**Name**	GS-06
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

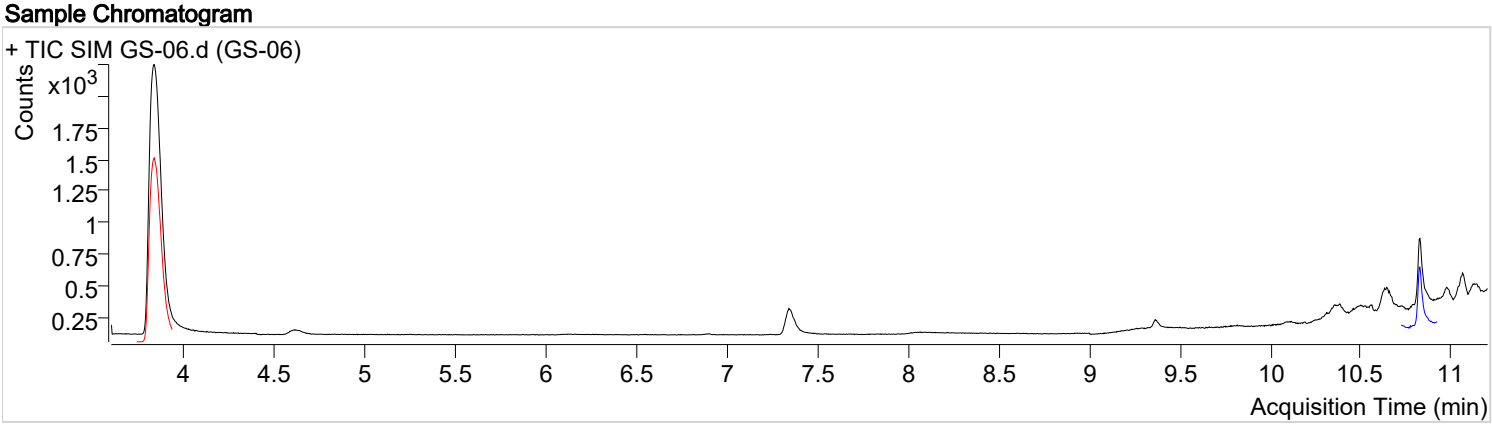

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.826	0	6985	ND mg/L

Naphthalene





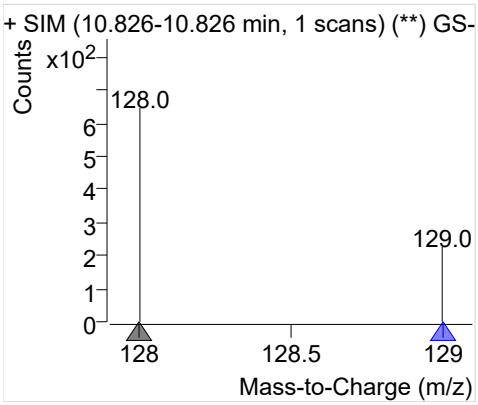

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오후 4:27:05	**Data File**	GS-15.d
Type	Sample	**Name**	GS-15
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

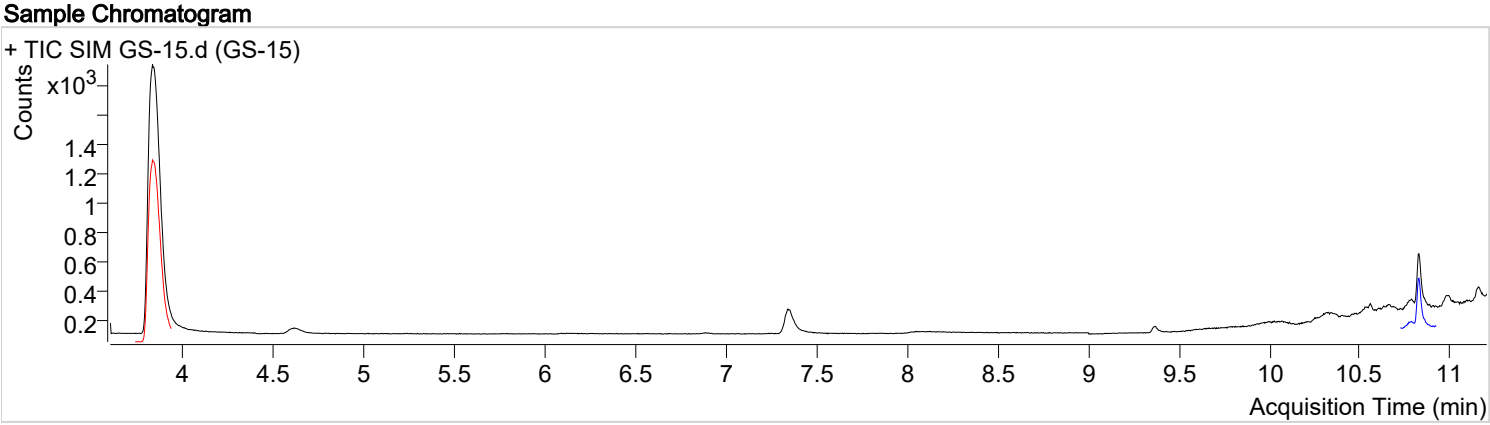

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.826	0	6032	ND mg/L

Naphthalene



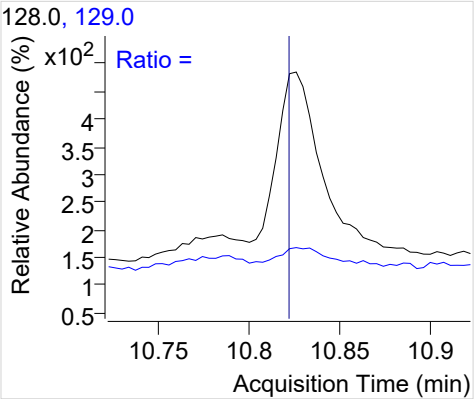

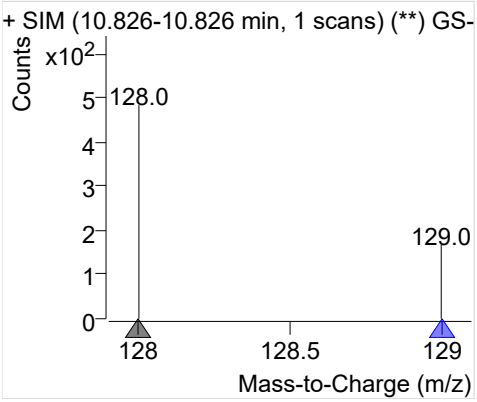

Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오후 4:44:12	**Data File**	GS-02 R.d
Type	Sample	**Name**	GS-02 R
Dil.	5	**Acq. Method File**	VOC2

Sample Chromatogram

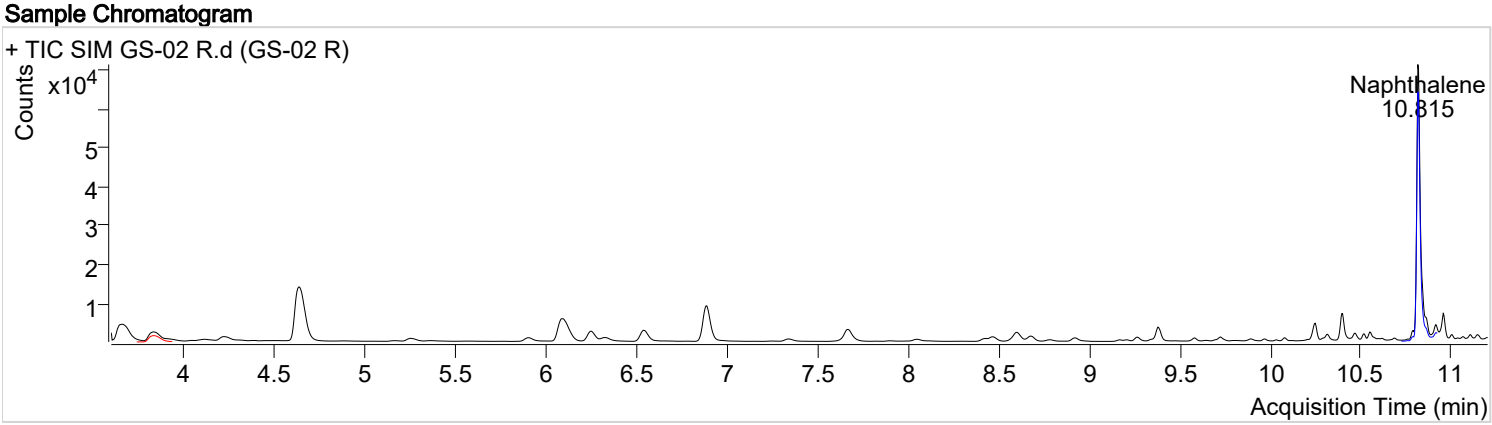

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.815	90253	7272	0.135 mg/L

Naphthalene







Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오후 5:01:21	**Data File**	MBK-1.d
Type	Blank	**Name**	MBK-1
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

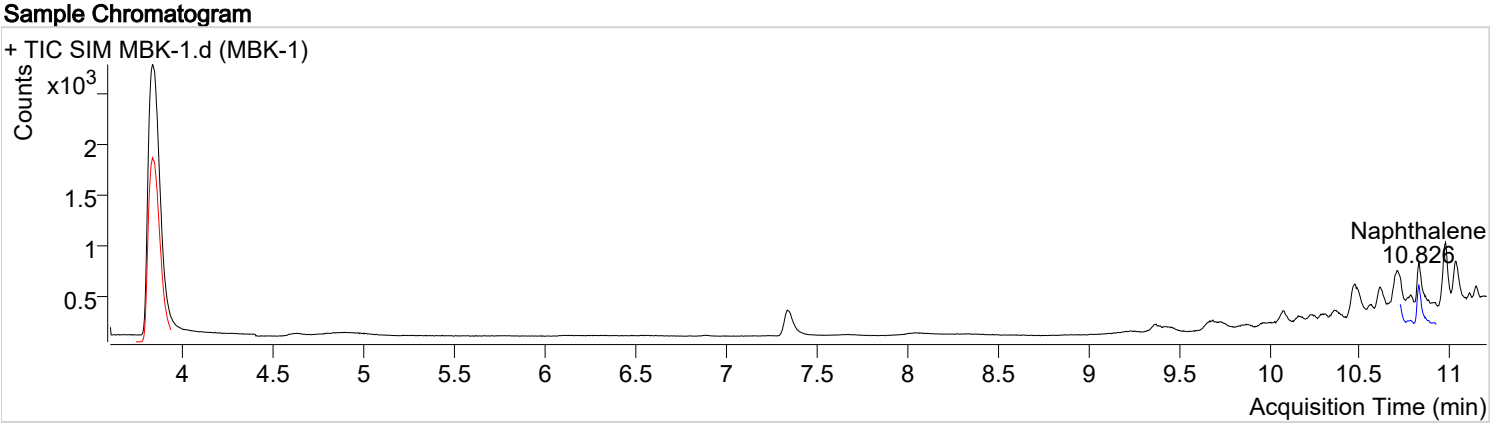

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.826	755	8599	0.000 mg/L

Naphthalene

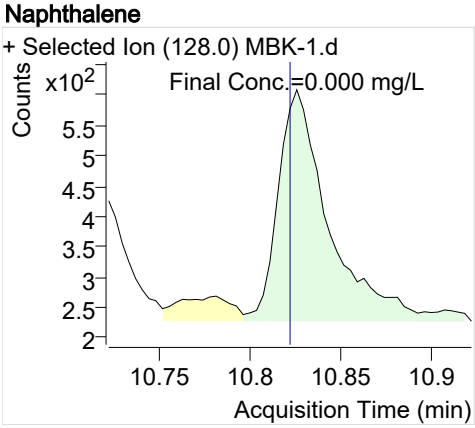

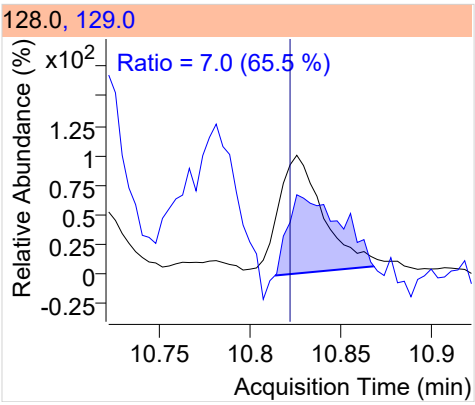

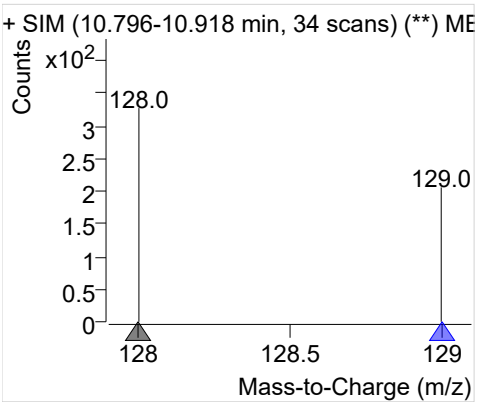

Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오후 5:18:29	**Data File**	CCV N.d
Type	QC	**Name**	CCV N
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

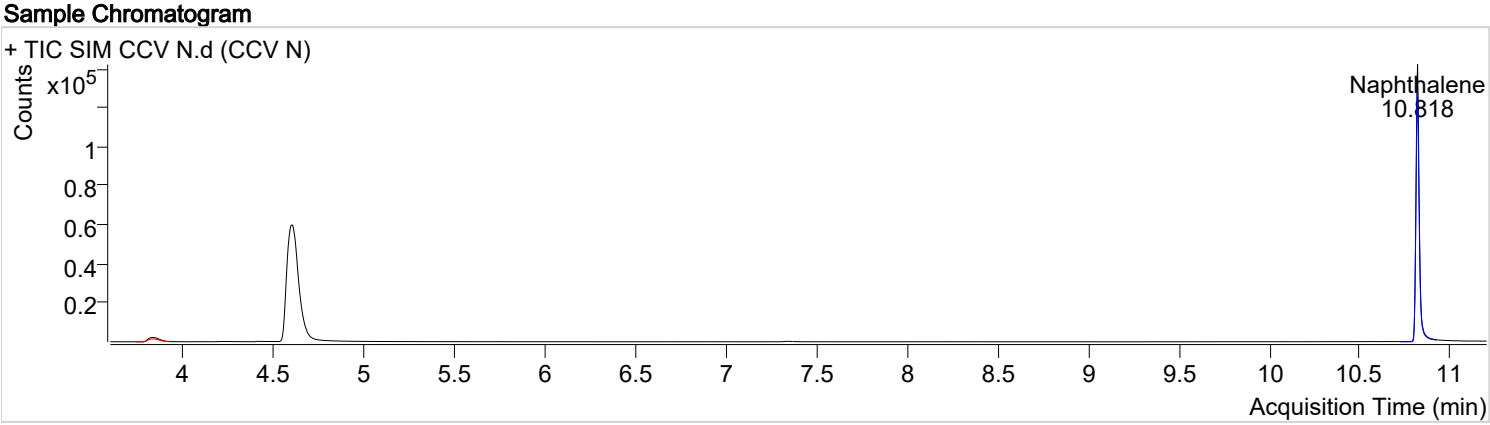

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.818	163451	6779	0.053 mg/L

Naphthalene







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오후 6:26:37	**Data File**	SOL 1.d
Type	Sample	**Name**	SOL 1
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

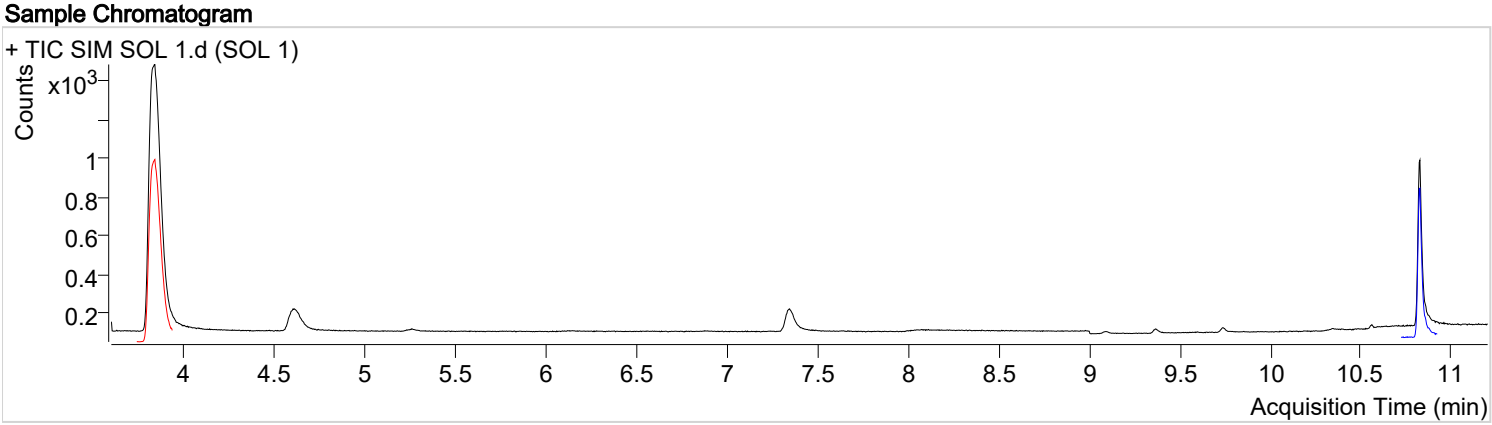

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.826	0	4445	ND mg/L

Naphthalene







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오후 6:43:33	**Data File**	SOL 2.d
Type	Sample	**Name**	SOL 2
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

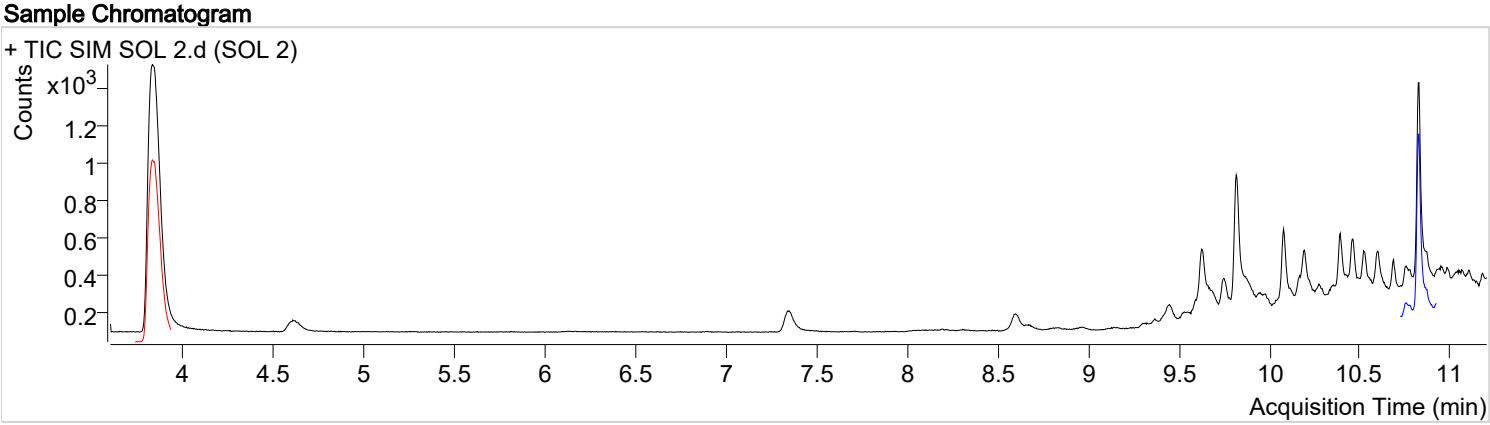

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.826	0	4708	ND mg/L

Naphthalene







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\NA.batch.bin		
Analysis Time	2026-02-13 오후 12:42:35	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:57:12	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:42:35	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-12 오후 7:00:29	**Data File**	SOL 3.d
Type	Sample	**Name**	SOL 3
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

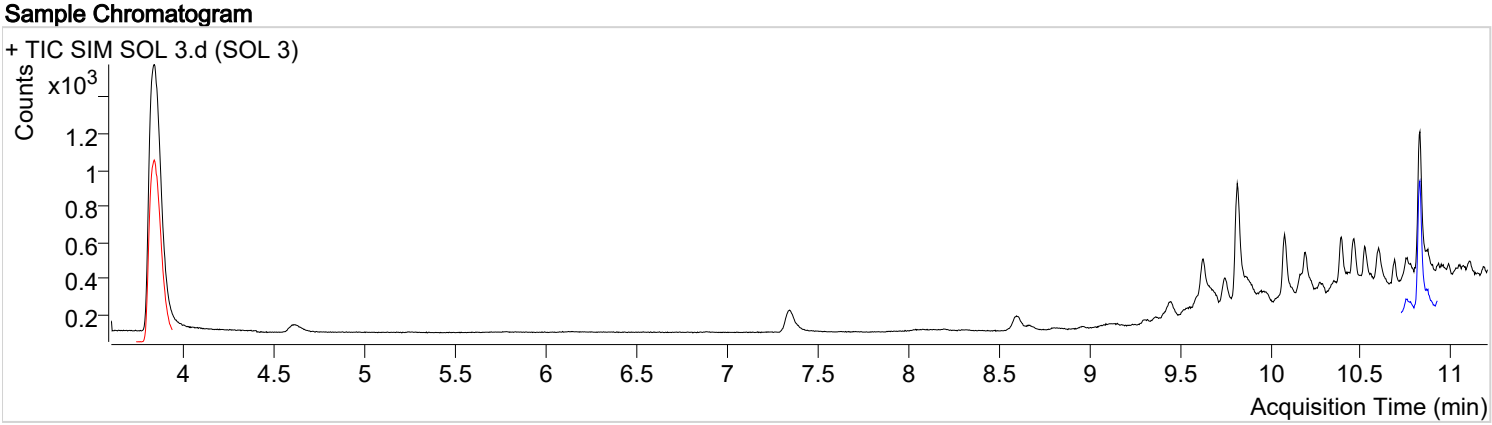

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.826	0	4832	ND mg/L

Naphthalene