Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.11)\QuantResults\NA.batch.bin				
Analysis Time	2026-03-23 오전 10:37:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 10:37:25	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Naphthalene

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
NA ST-01.d	Cal	10.830	6112	5384	0.002
NA ST-02.d	Cal	10.829	21378	6178	0.005
NA ST-03.d	Cal	10.826	45408	6429	0.009
NA ST-04.d	Cal	10.819	243230	6338	0.051
NA ST-05.d	Cal	10.819	469886	6210	0.100
BK-.d	Blank			5287	ND
FBK(RE 26-03-11).d	Blank			4484	ND
RE-07.d	Sample			4623	ND
RE-08.d	Sample			4083	ND
RE-17.d	Sample			4342	ND
RE-18.d	Sample			4474	ND
RE-19.d	Sample			4872	ND
RE-20.d	Sample			4814	ND
RE-21.d	Sample			5004	ND
RE-22.d	Sample			4386	ND
RE-23.d	Sample			4020	ND
MBK.d	Blank			4195	ND
CCV(N)-.d	QC	10.822	132322	4015	0.043

Naphthalene

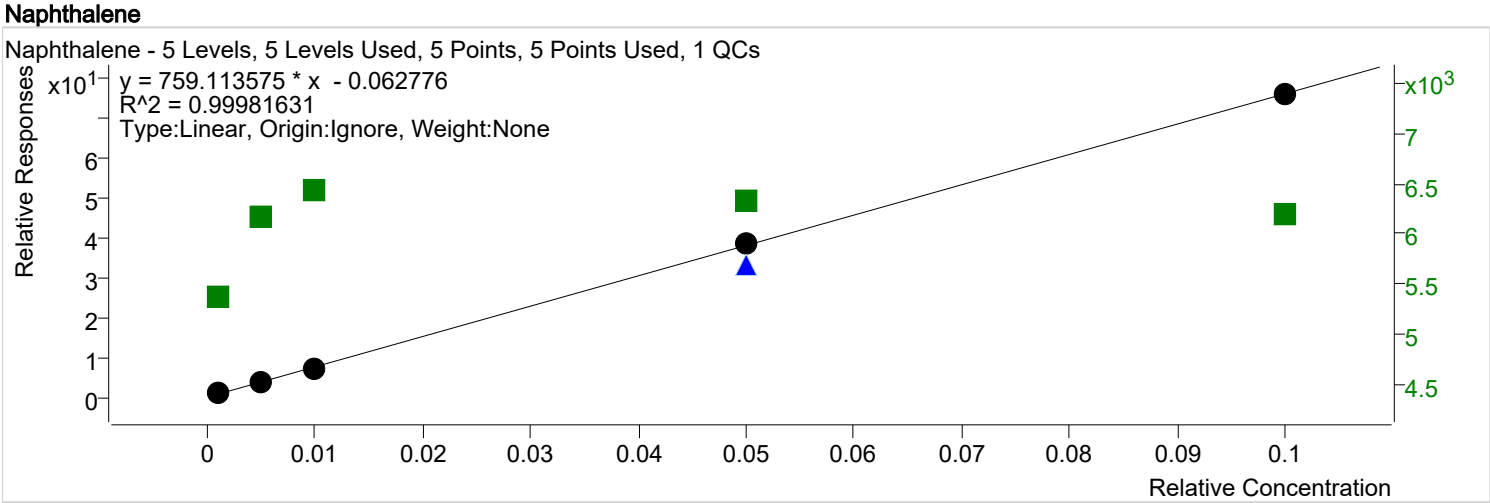

Cal. Path	Type	Level	Enable	Conc.	Response
V:\2026\2026-03\VOC2(RE 3.11)\NAST-01.d	Calibration	1	x	0.001	6112
V:\2026\2026-03\VOC2(RE 3.11)\NAST-02.d	Calibration	2	x	0.005	21378
V:\2026\2026-03\VOC2(RE 3.11)\NAST-03.d	Calibration	3	x	0.010	45408
V:\2026\2026-03\VOC2(RE 3.11)\NAST-04.d	Calibration	4	x	0.050	243230
V:\2026\2026-03\VOC2(RE 3.11)\CCV(N)-.d	QC	4	x	0.050	132322
V:\2026\2026-03\VOC2(RE 3.11)\NAST-05.d	Calibration	5	x	0.100	469886

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.11)\QuantResults\NA.batch.bin		
Analysis Time	2026-03-23 오전 10:37:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:00:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 10:37:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 3:47:19	**Data File**	NA ST-01.d
Type	Cal	**Name**	NA ST-01
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

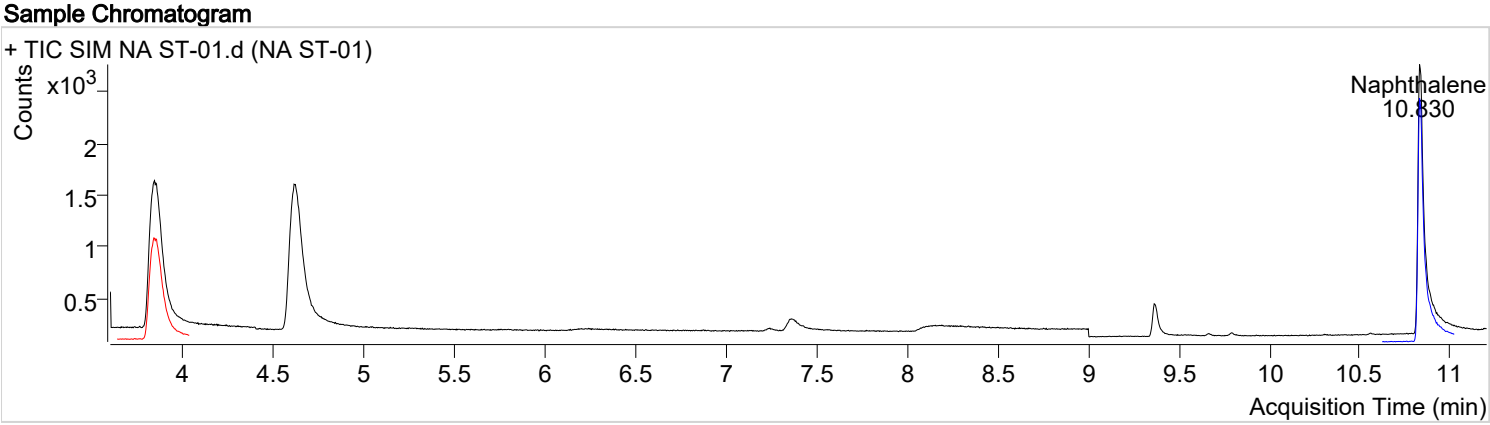

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.830	6112	5384	0.002 mg/L

Naphthalene





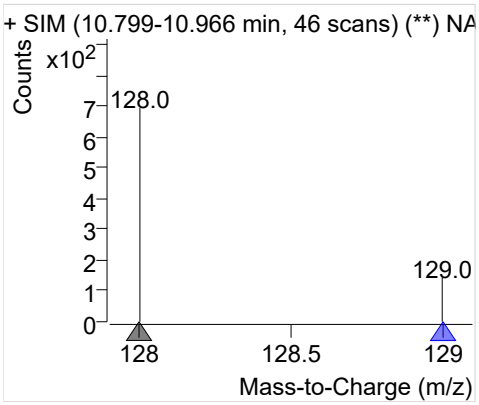

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.11)\QuantResults\NA.batch.bin		
Analysis Time	2026-03-23 오전 10:37:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:00:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 10:37:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 4:04:24	**Data File**	NA ST-02.d
Type	Cal	**Name**	NA ST-02
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

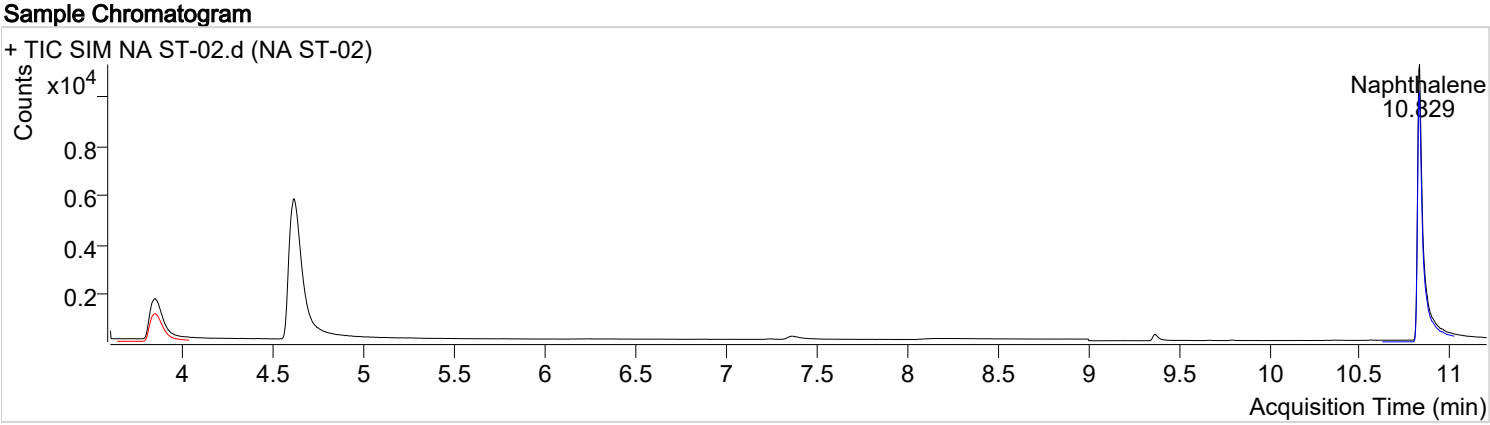

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.829	21378	6178	0.005 mg/L

Naphthalene





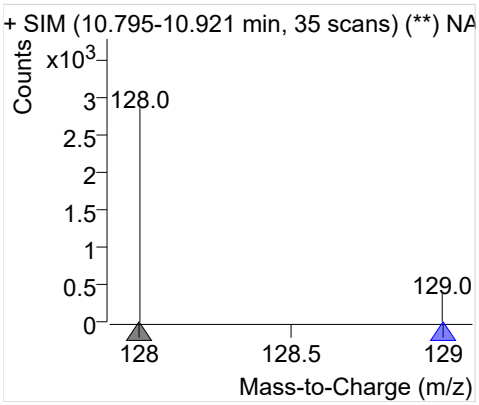

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.11)\QuantResults\NA.batch.bin		
Analysis Time	2026-03-23 오전 10:37:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:00:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 10:37:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 4:21:28	**Data File**	NA ST-03.d
Type	Cal	**Name**	NA ST-03
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

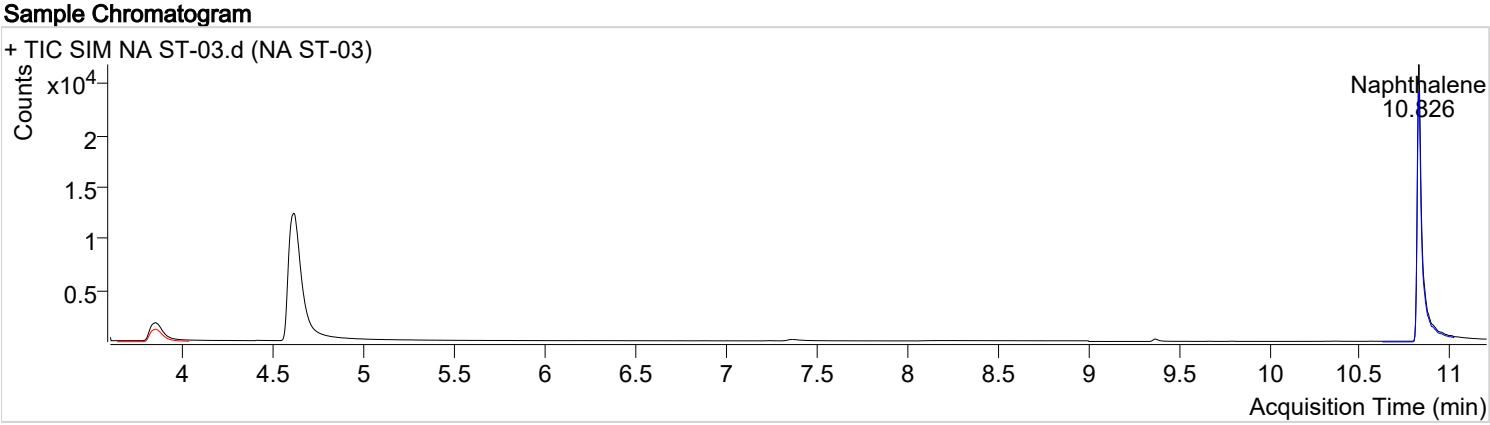

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.826	45408	6429	0.009 mg/L

Naphthalene





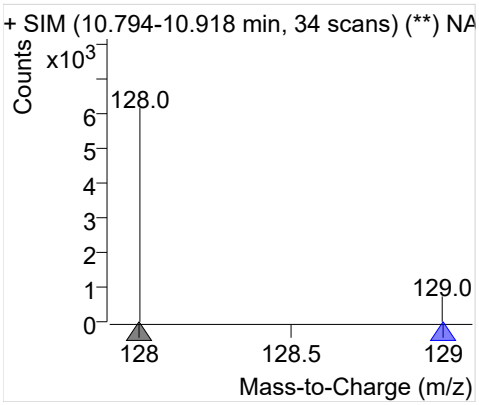

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.11)\QuantResults\NA.batch.bin		
Analysis Time	2026-03-23 오전 10:37:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:00:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 10:37:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 4:38:28	**Data File**	NA ST-04.d
Type	Cal	**Name**	NA ST-04
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

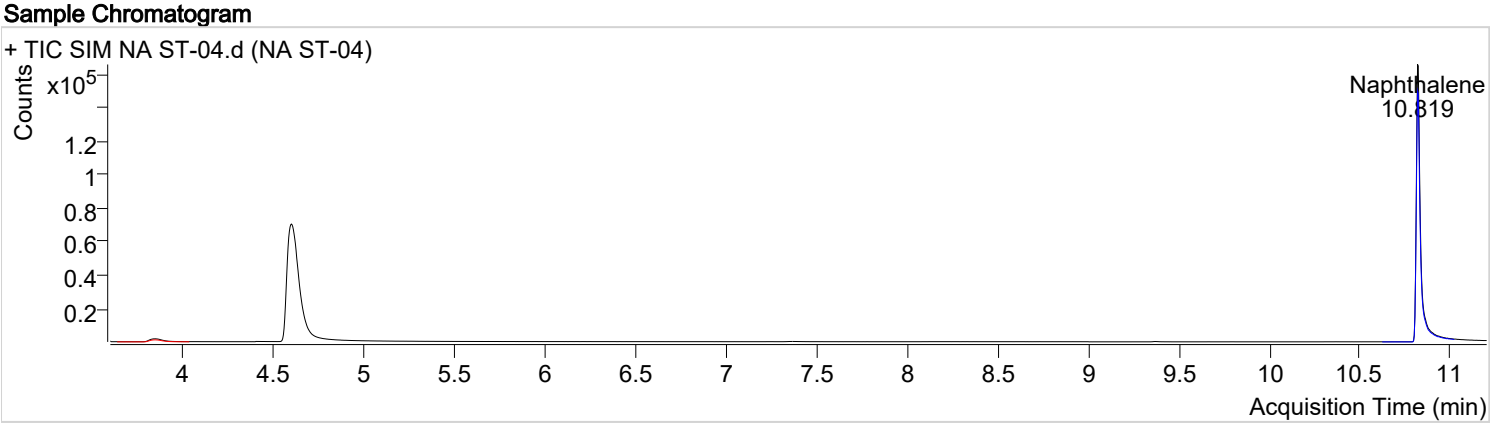

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.819	243230	6338	0.051 mg/L

Naphthalene





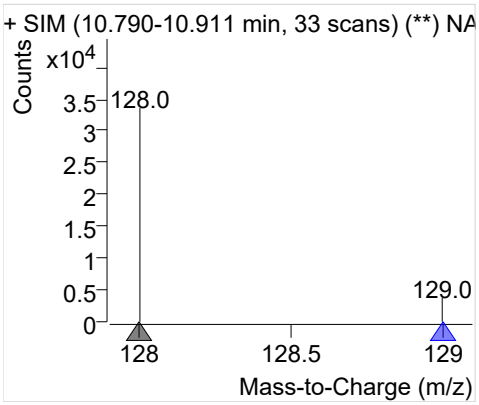

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.11)\QuantResults\NA.batch.bin		
Analysis Time	2026-03-23 오전 10:37:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:00:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 10:37:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 4:55:30	**Data File**	NA ST-05.d
Type	Cal	**Name**	NA ST-05
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

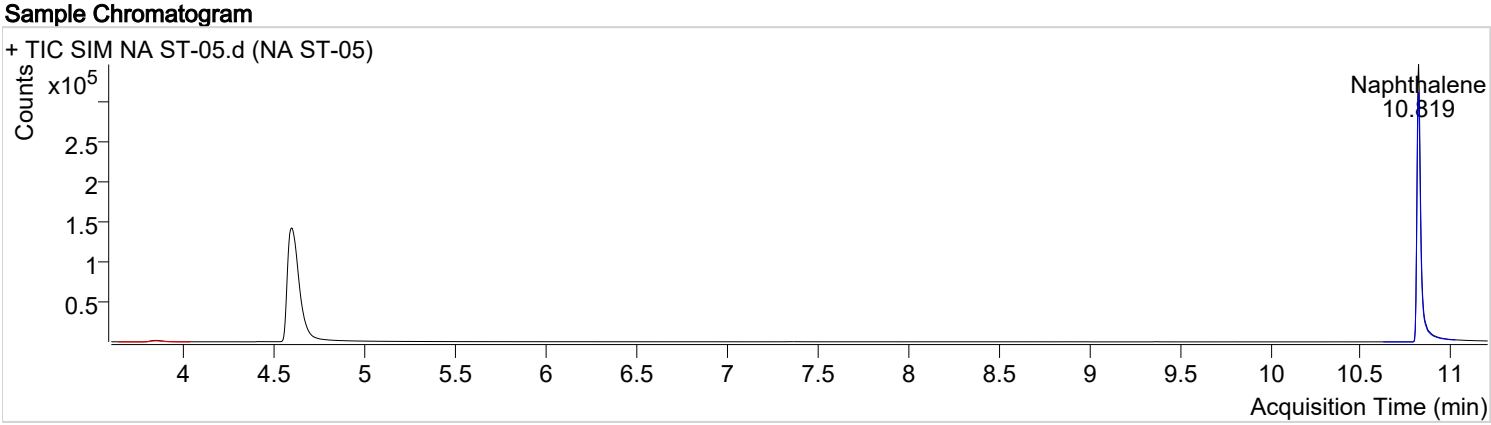

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.819	469886	6210	0.100 mg/L

Naphthalene





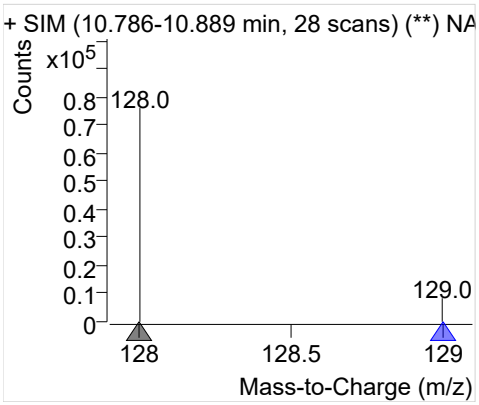

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.11)\QuantResults\NA.batch.bin		
Analysis Time	2026-03-23 오전 10:37:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:00:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 10:37:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 7:11:47	**Data File**	BK-.d
Type	Blank	**Name**	BK-
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

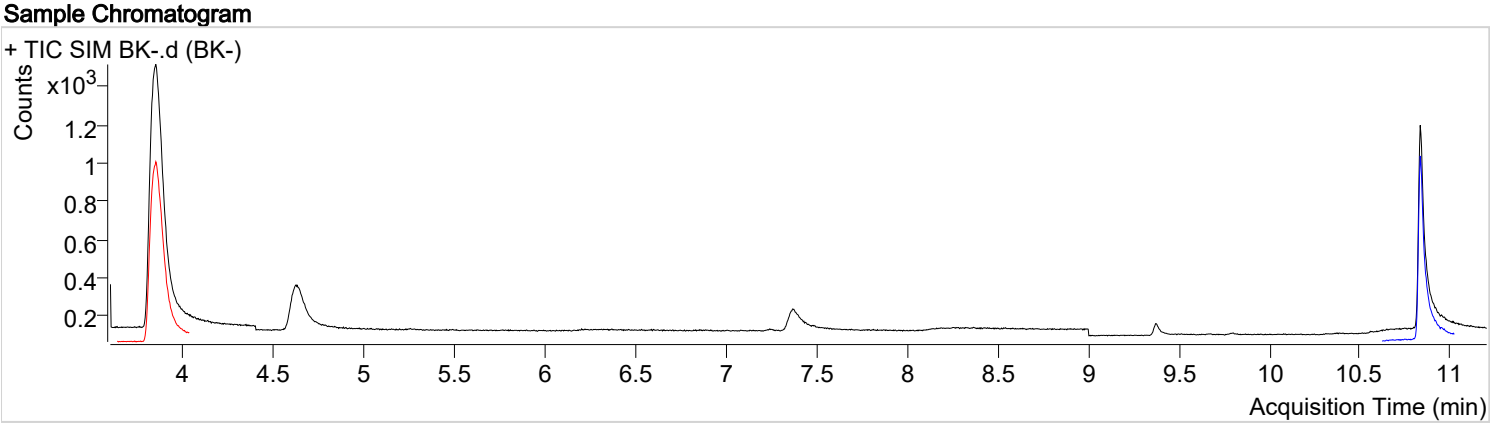

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			5287	ND mg/L

Naphthalene

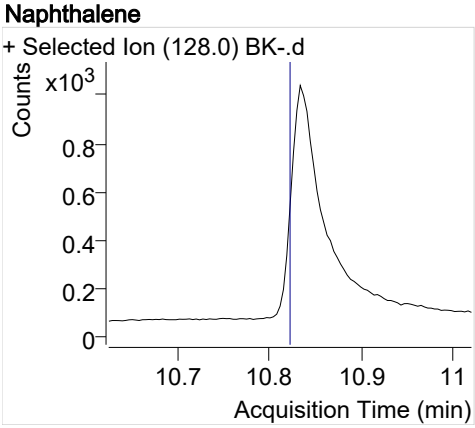

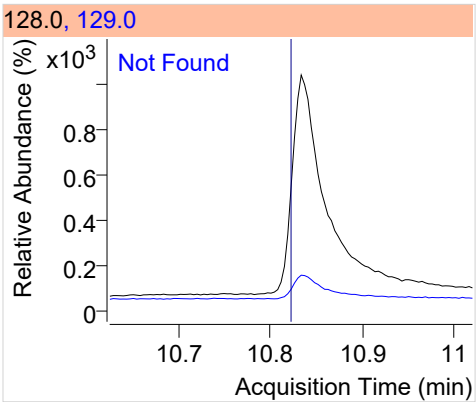

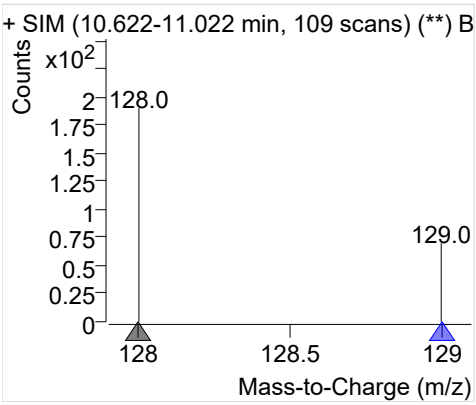

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.11)\QuantResults\NA.batch.bin		
Analysis Time	2026-03-23 오전 10:37:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:00:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 10:37:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 7:28:42	**Data File**	FBK(RE 26-03-11).d
Type	Blank	**Name**	FBK(RE 26-03-11)
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

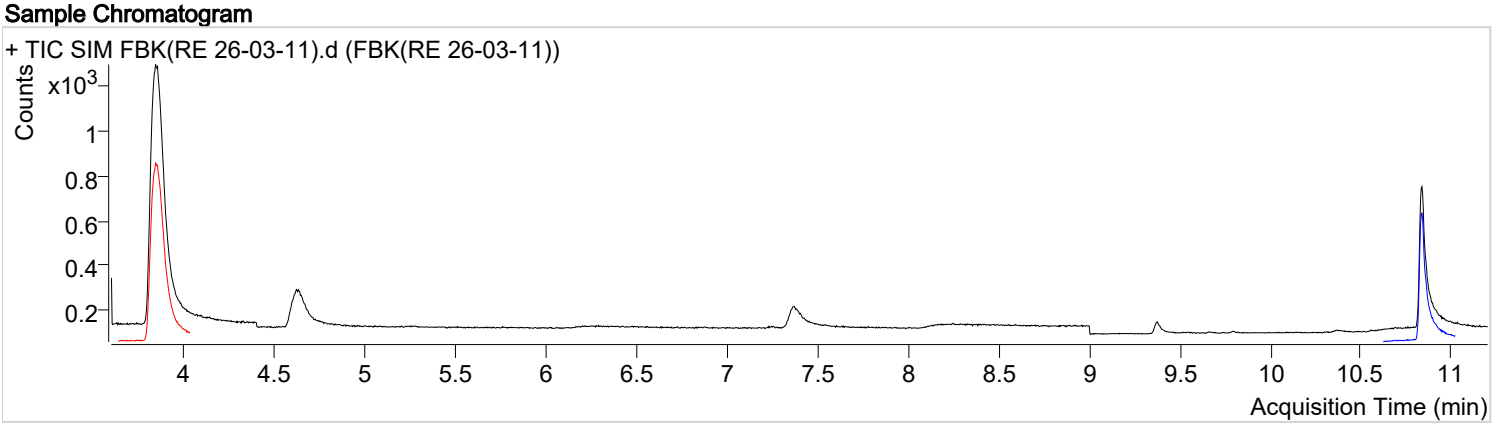

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			4484	ND mg/L

Naphthalene







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.11)\QuantResults\NA.batch.bin		
Analysis Time	2026-03-23 오전 10:37:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:00:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 10:37:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 7:45:45	**Data File**	RE-07.d
Type	Sample	**Name**	RE-07
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

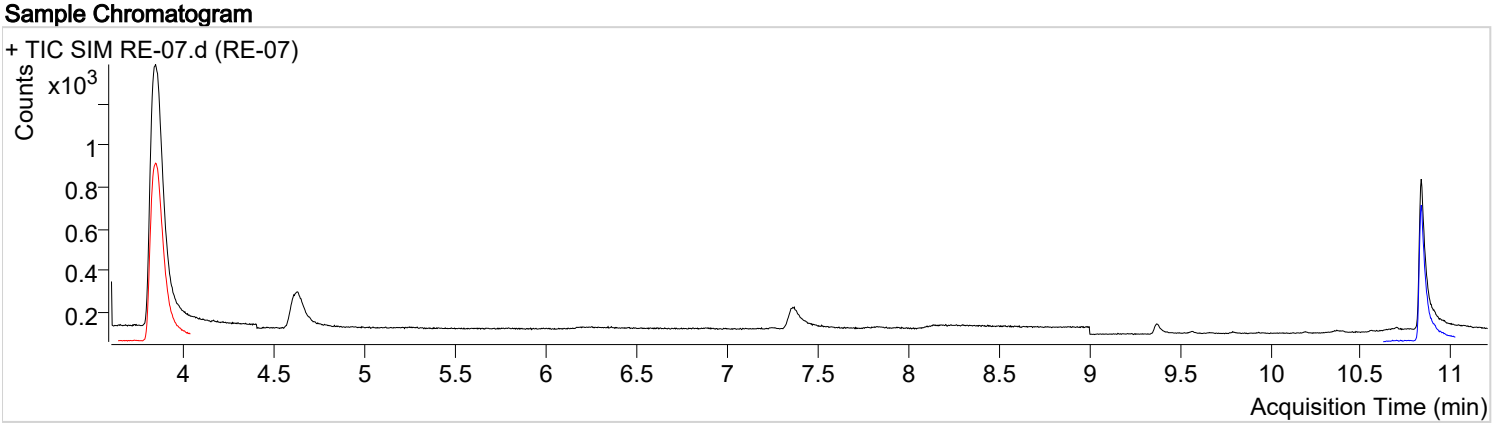

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			4623	ND mg/L

Naphthalene







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.11)\QuantResults\NA.batch.bin		
Analysis Time	2026-03-23 오전 10:37:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:00:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 10:37:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 8:02:47	**Data File**	RE-08.d
Type	Sample	**Name**	RE-08
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

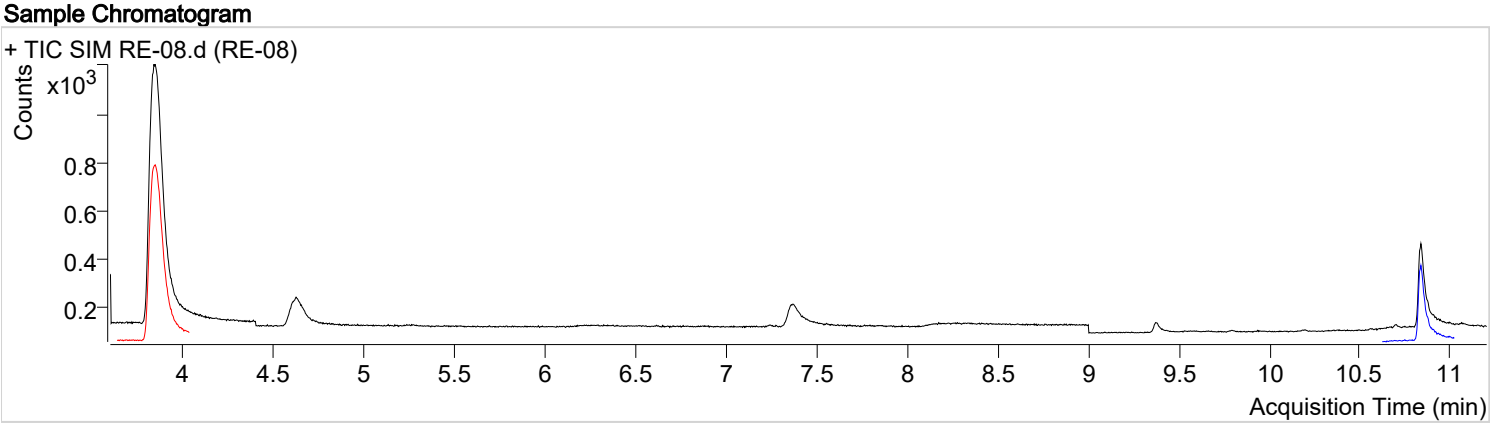

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			4083	ND mg/L

Naphthalene

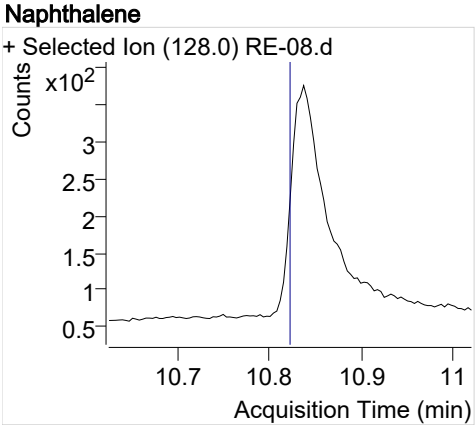

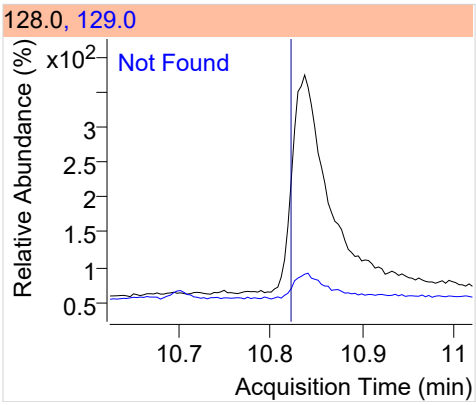



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.11)\QuantResults\NA.batch.bin		
Analysis Time	2026-03-23 오전 10:37:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:00:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 10:37:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 8:19:48	**Data File**	RE-17.d
Type	Sample	**Name**	RE-17
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

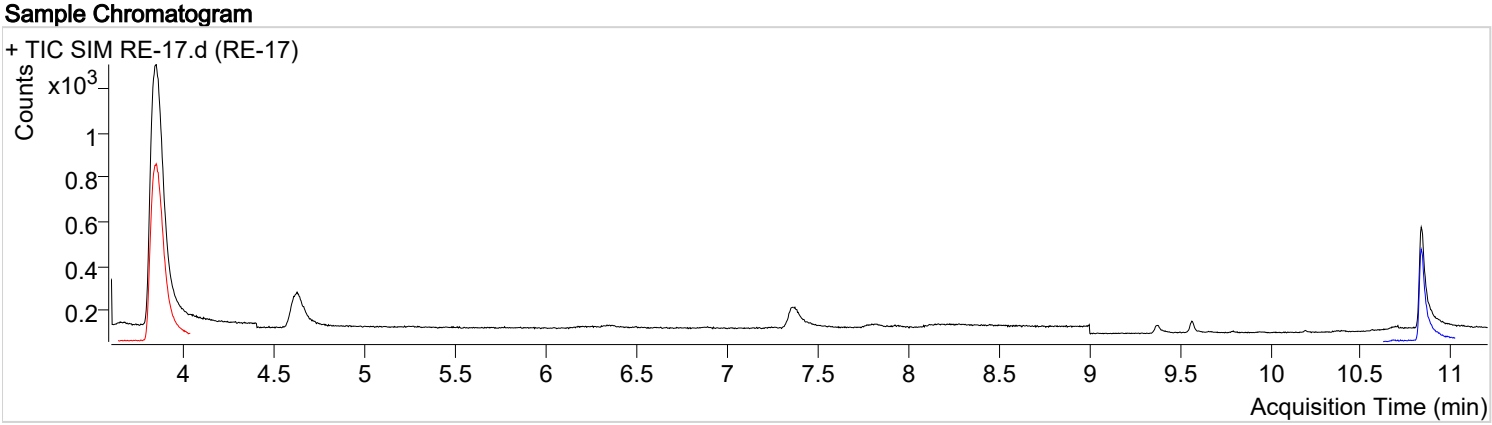

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			4342	ND mg/L

Naphthalene

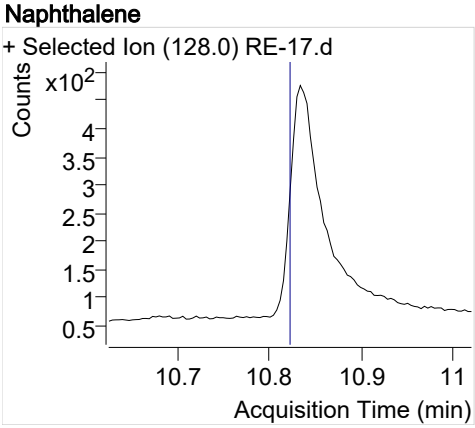

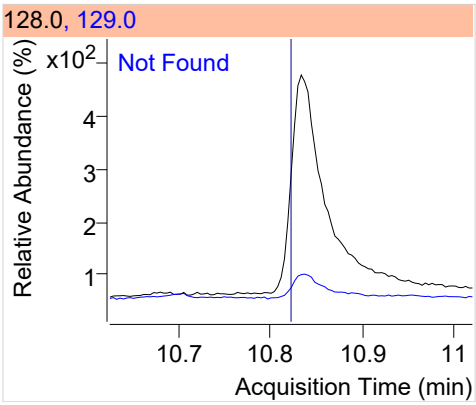



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.11)\QuantResults\NA.batch.bin		
Analysis Time	2026-03-23 오전 10:37:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:00:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 10:37:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 8:36:48	**Data File**	RE-18.d
Type	Sample	**Name**	RE-18
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

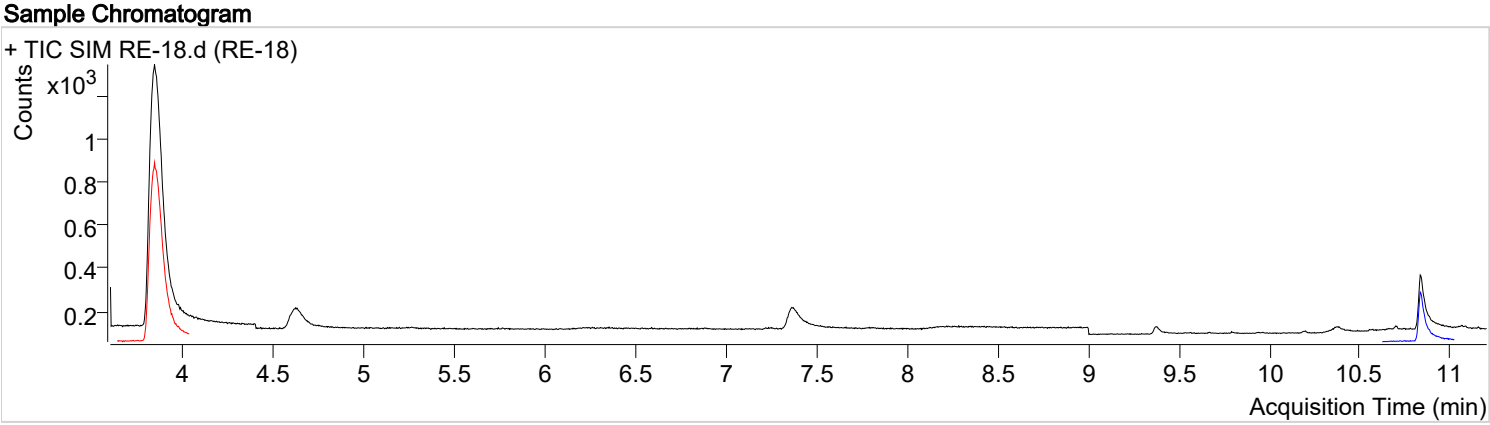

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			4474	ND mg/L

Naphthalene

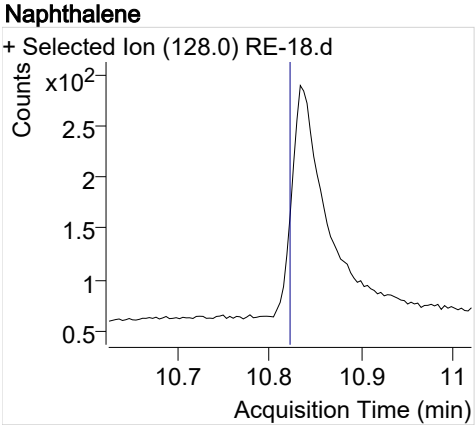

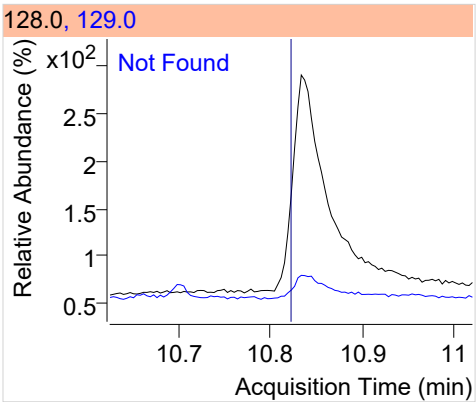

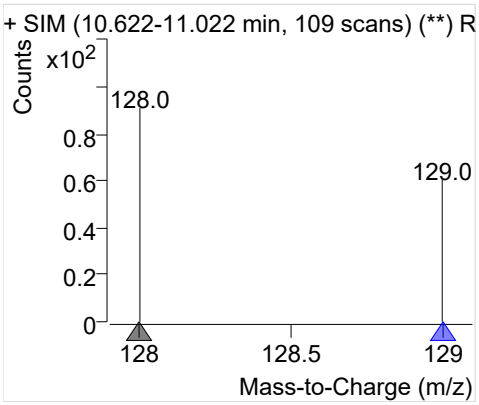

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.11)\QuantResults\NA.batch.bin		
Analysis Time	2026-03-23 오전 10:37:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:00:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 10:37:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 8:53:49	**Data File**	RE-19.d
Type	Sample	**Name**	RE-19
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

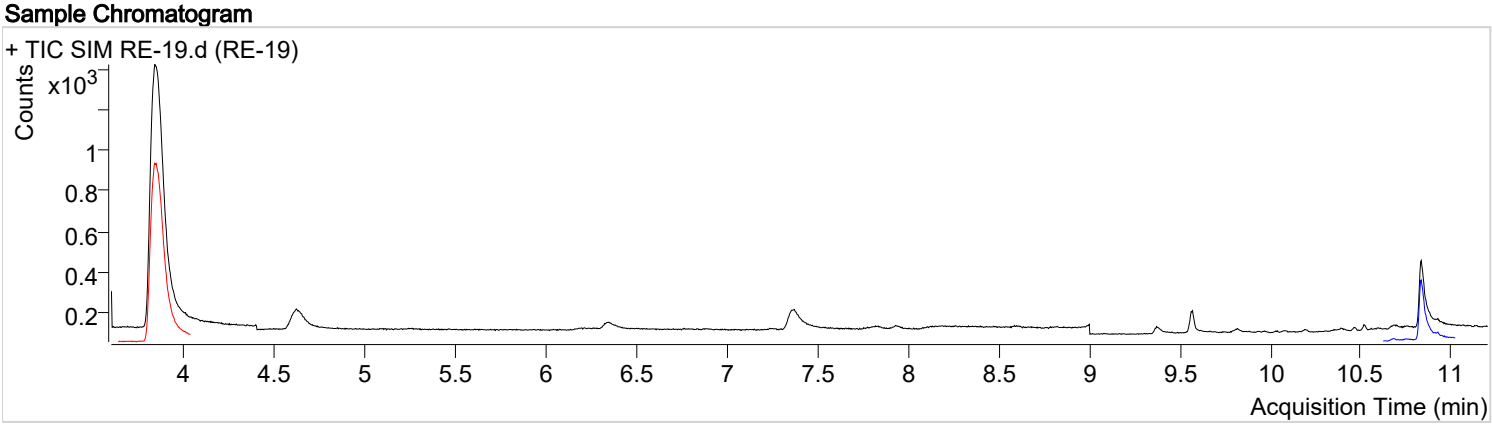

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			4872	ND mg/L

Naphthalene







Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.11)\QuantResults\NA.batch.bin		
Analysis Time	2026-03-23 오전 10:37:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:00:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 10:37:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 9:10:56	**Data File**	RE-20.d
Type	Sample	**Name**	RE-20
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

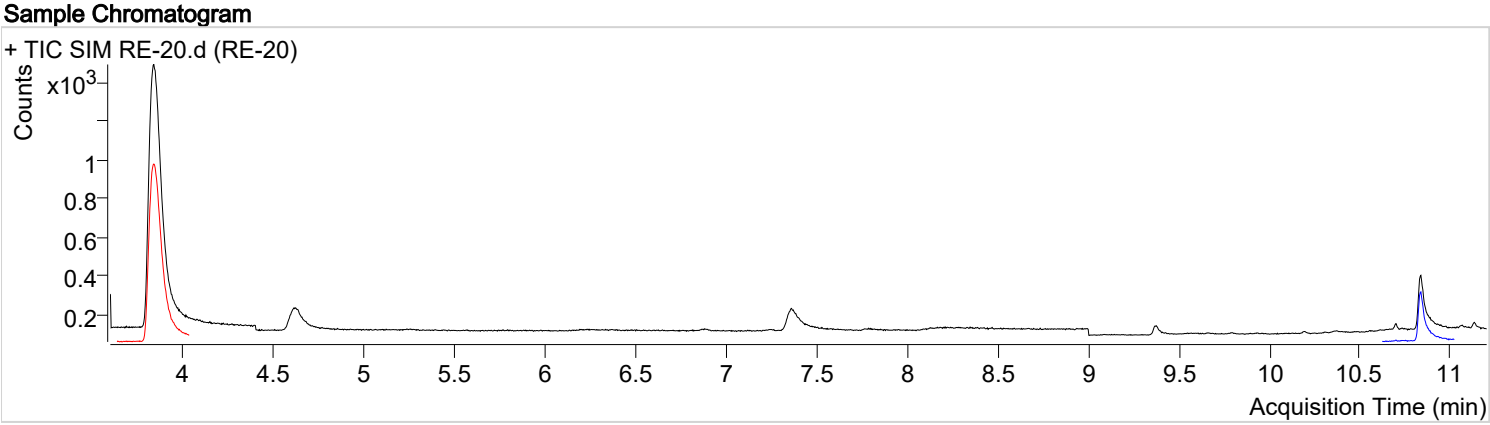

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			4814	ND mg/L

Naphthalene

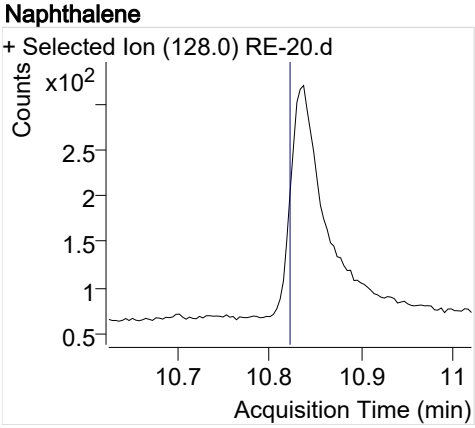

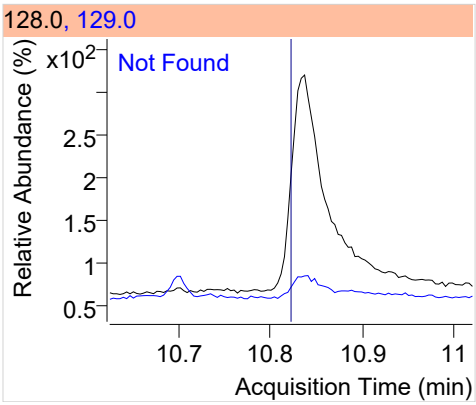



Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.11)\QuantResults\NA.batch.bin		
Analysis Time	2026-03-23 오전 10:37:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:00:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 10:37:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 9:27:59	**Data File**	RE-21.d
Type	Sample	**Name**	RE-21
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

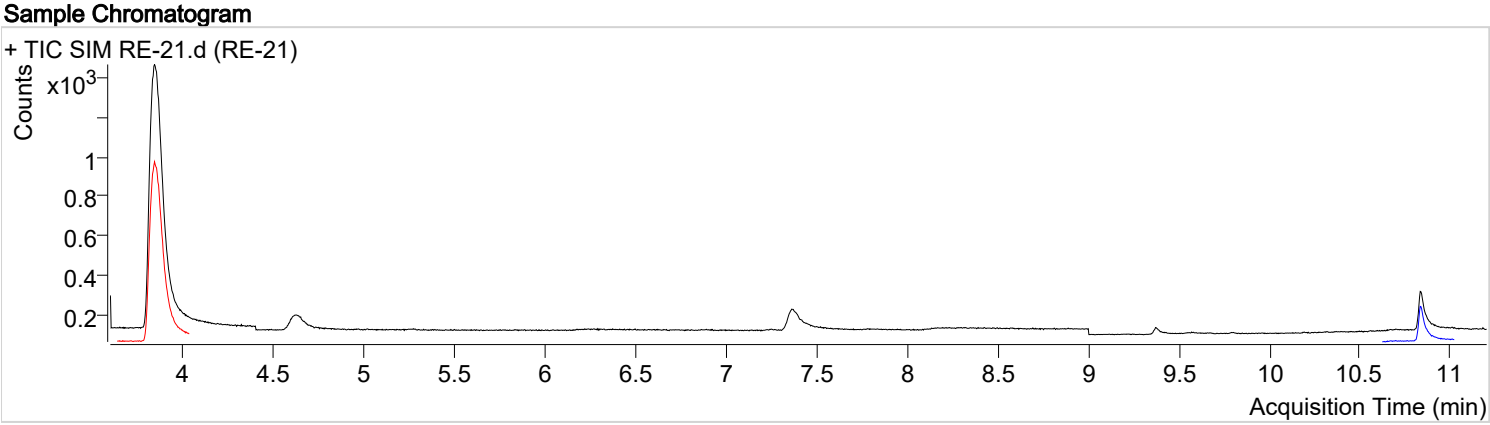

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			5004	ND mg/L

Naphthalene

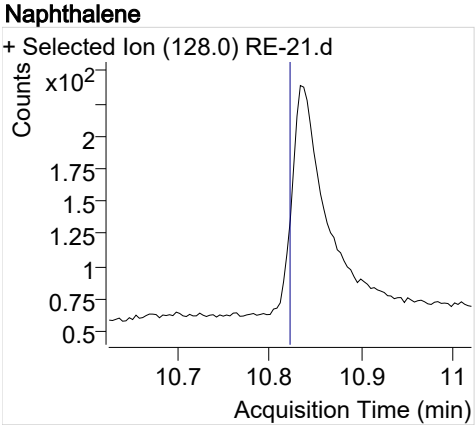

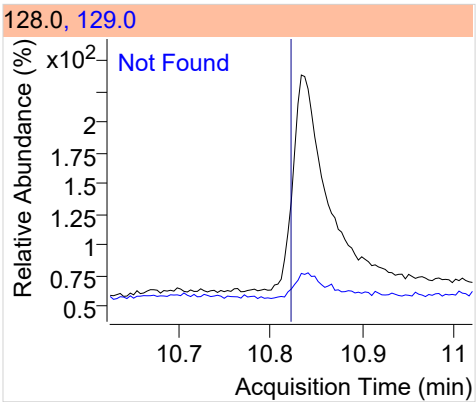



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.11)\QuantResults\NA.batch.bin		
Analysis Time	2026-03-23 오전 10:37:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:00:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 10:37:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 9:44:58	**Data File**	RE-22.d
Type	Sample	**Name**	RE-22
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

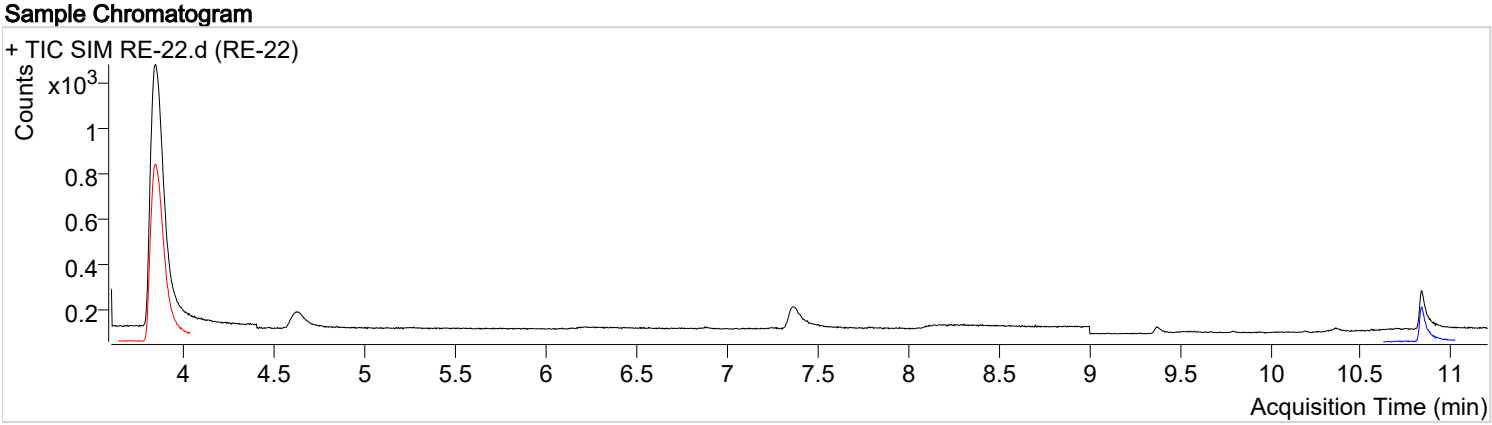

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			4386	ND mg/L

Naphthalene







Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.11)\QuantResults\NA.batch.bin		
Analysis Time	2026-03-23 오전 10:37:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:00:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 10:37:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 10:02:02	**Data File**	RE-23.d
Type	Sample	**Name**	RE-23
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

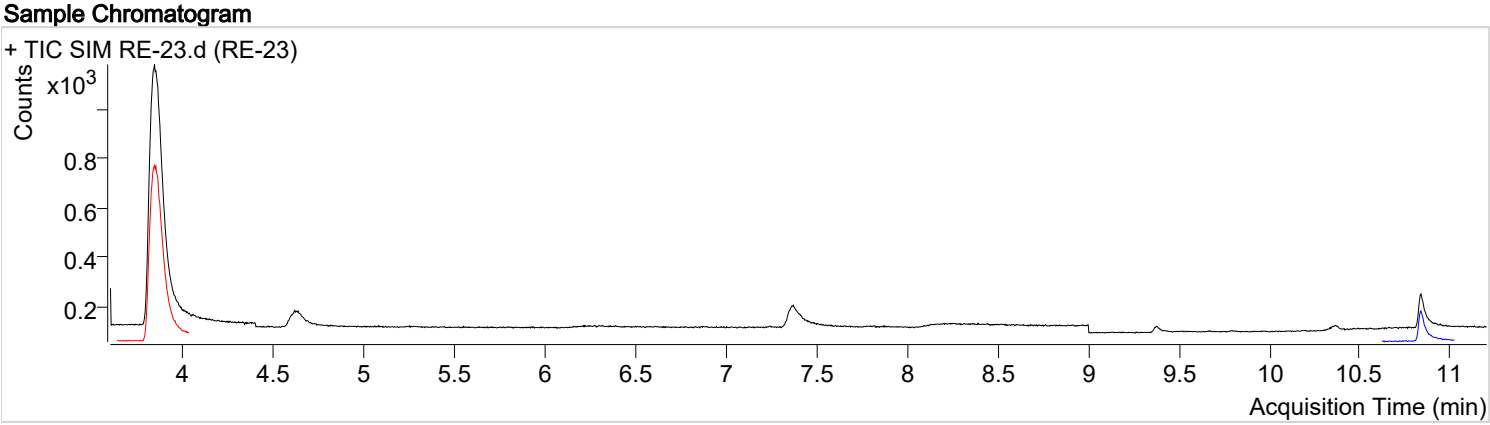

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			4020	ND mg/L

Naphthalene

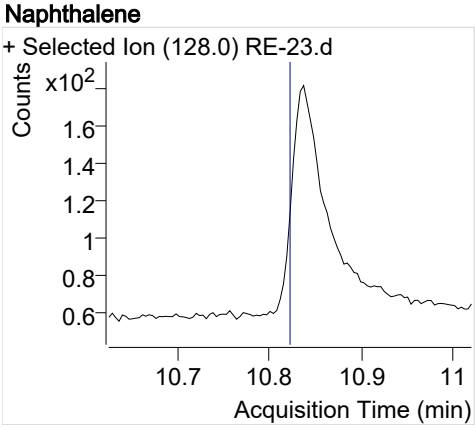

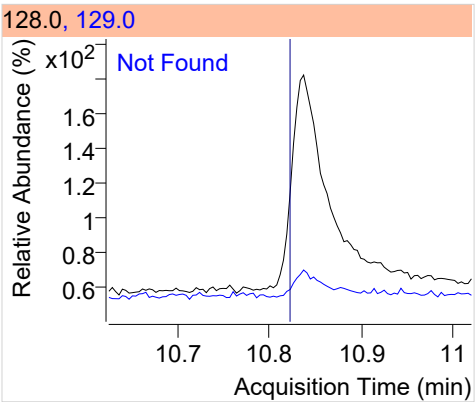



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.11)\QuantResults\NA.batch.bin		
Analysis Time	2026-03-23 오전 10:37:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:00:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 10:37:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 10:19:08	**Data File**	MBK.d
Type	Blank	**Name**	MBK
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

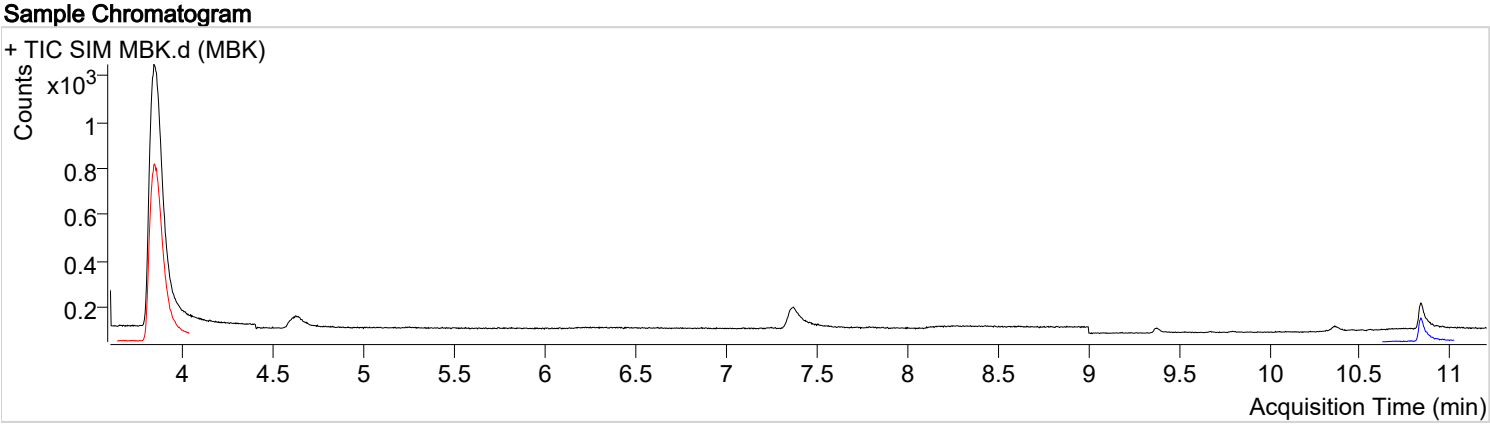

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			4195	ND mg/L

Naphthalene

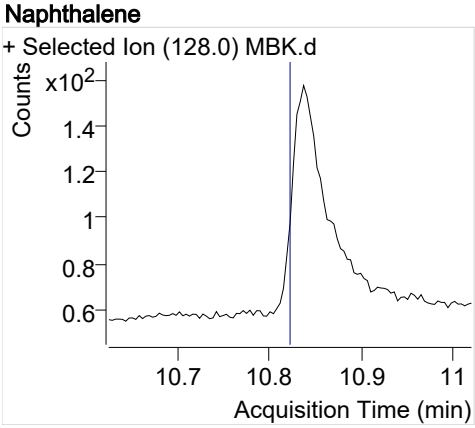

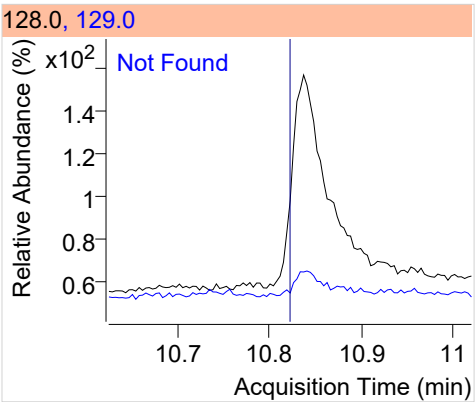



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.11)\QuantResults\NA.batch.bin		
Analysis Time	2026-03-23 오전 10:37:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:00:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 10:37:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-13 오후 10:53:15	**Data File**	CCV(N)-.d
Type	QC	**Name**	CCV(N)-
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

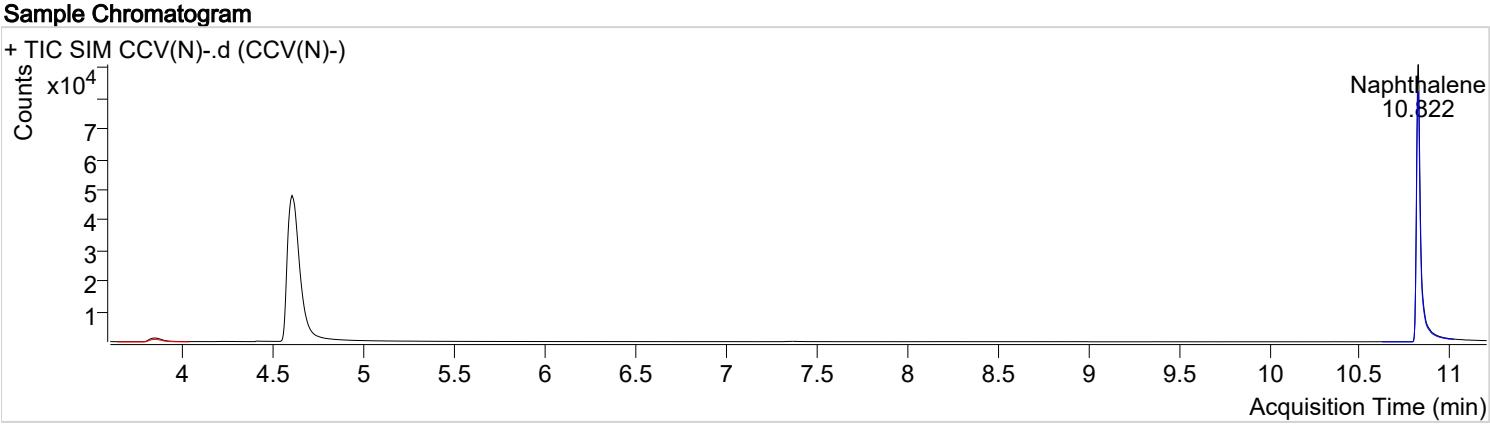

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.822	132322	4015	0.043 mg/L

Naphthalene





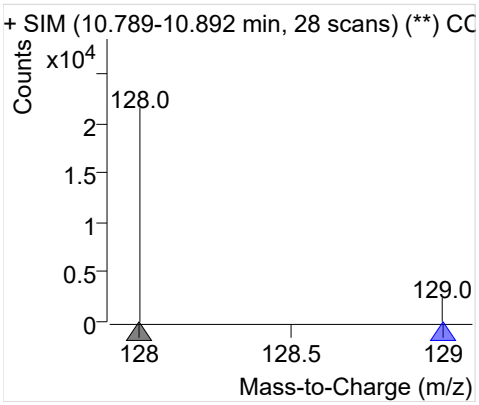

Generated at 오후 3:00 on 2026-04-10