Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\NA.batch.bin				
Analysis Time	2026-04-01 오후 4:45:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:45:39	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Naphthalene

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
NA ST-01.d	Cal	10.826	5488	4144	0.002
NA ST-02.d	Cal	10.822	11484	3549	0.005
NA ST-03.d	Cal	10.822	17371	2469	0.011
NA ST-04.d	Cal	10.818	111460	3705	0.047
NA ST-05.d	Cal	10.819	217311	3395	0.101
BK-.d	Blank	10.830	833	2936	0.000
FBK(NK 26-03-26).d	Blank	10.829	552	3356	0.000
NJ-01.d	Sample			2853	ND
NJ-02.d	Sample			2604	ND
NJ-03.d	Sample			2431	ND
NJ-04.d	Sample			2388	ND
NJ-05.d	Sample			2536	ND
NJ-06.d	Sample			2127	ND
MBK.d	Blank			2933	ND
CCV N.d	QC	10.819	90492	2395	0.060

Naphthalene

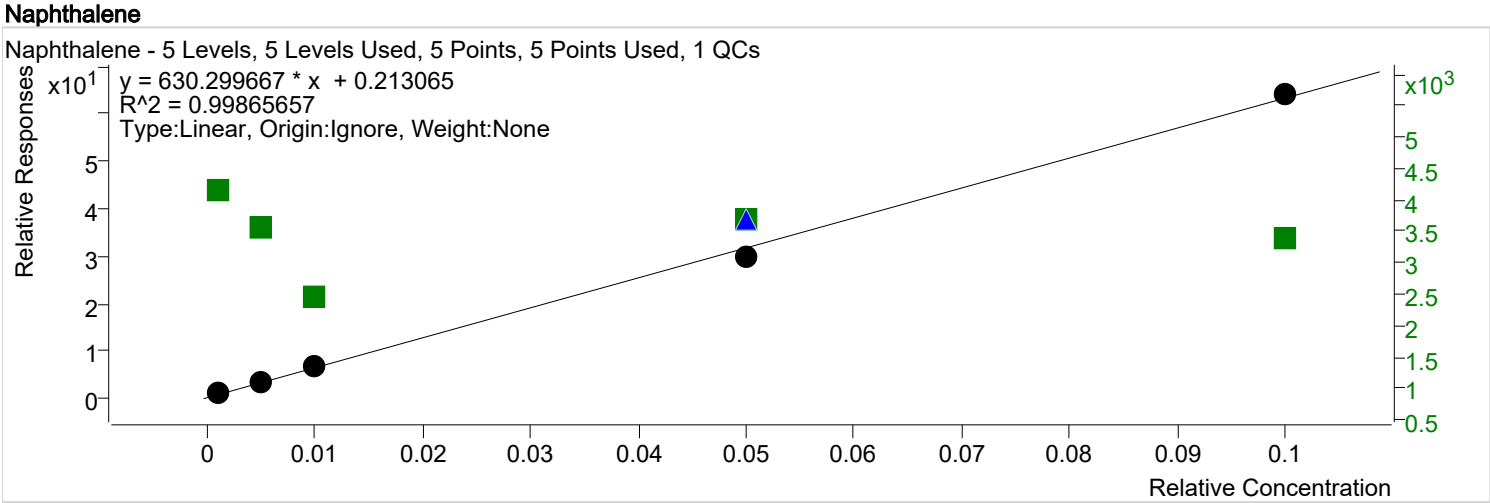

Cal. Path	Type	Level	Enable	Conc.	Response
V:\2026\2026-03\VOC2(NJ 3.26)\NAST-01.d	Calibration	1	x	0.001	5488
V:\2026\2026-03\VOC2(NJ 3.26)\NAST-02.d	Calibration	2	x	0.005	11484
V:\2026\2026-03\VOC2(NJ 3.26)\NAST-03.d	Calibration	3	x	0.010	17371
V:\2026\2026-03\VOC2(NJ 3.26)\NAST-04.d	Calibration	4	x	0.050	111460
V:\2026\2026-03\VOC2(NJ 3.26)\CCVN.d	QC	4	x	0.050	90492
V:\2026\2026-03\VOC2(NJ 3.26)\NAST-05.d	Calibration	5	x	0.100	217311

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\NA.batch.bin		
Analysis Time	2026-04-01 오후 4:45:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:59:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:45:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 2:34:41	**Data File**	NA ST-01.d
Type	Cal	**Name**	NA ST-01
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

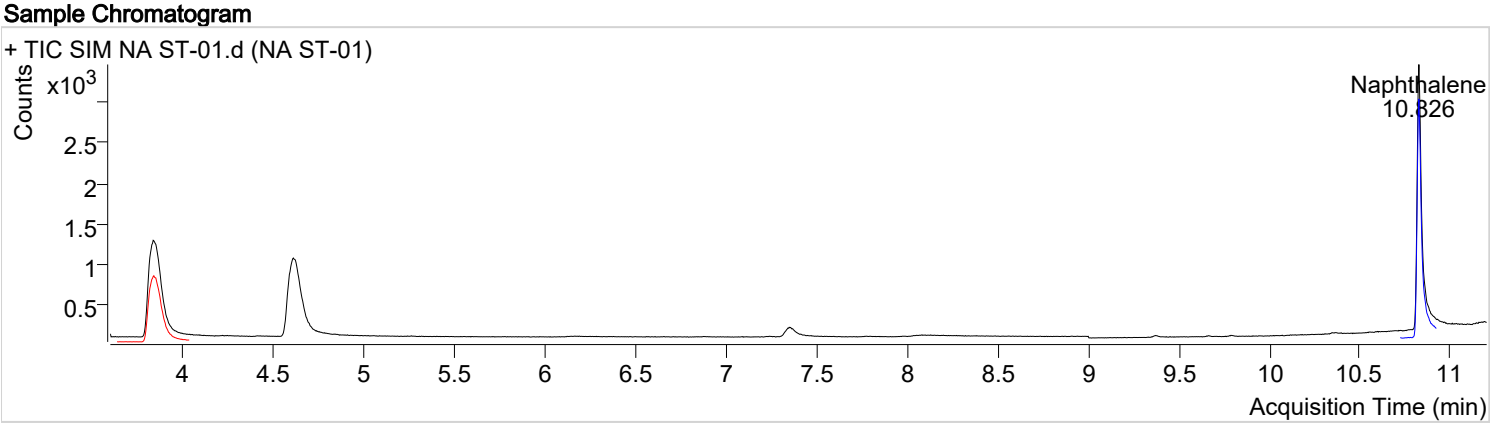

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.826	5488	4144	0.002 mg/L

Naphthalene





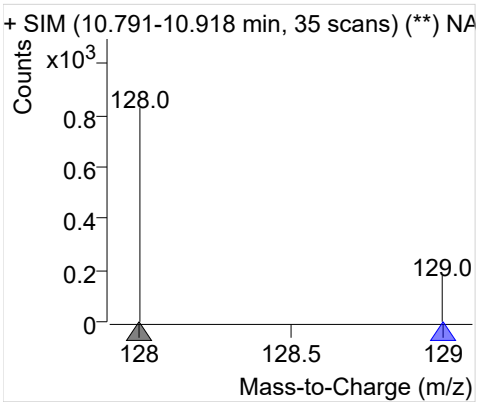

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\NA.batch.bin		
Analysis Time	2026-04-01 오후 4:45:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:59:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:45:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 2:51:38	**Data File**	NA ST-02.d
Type	Cal	**Name**	NA ST-02
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

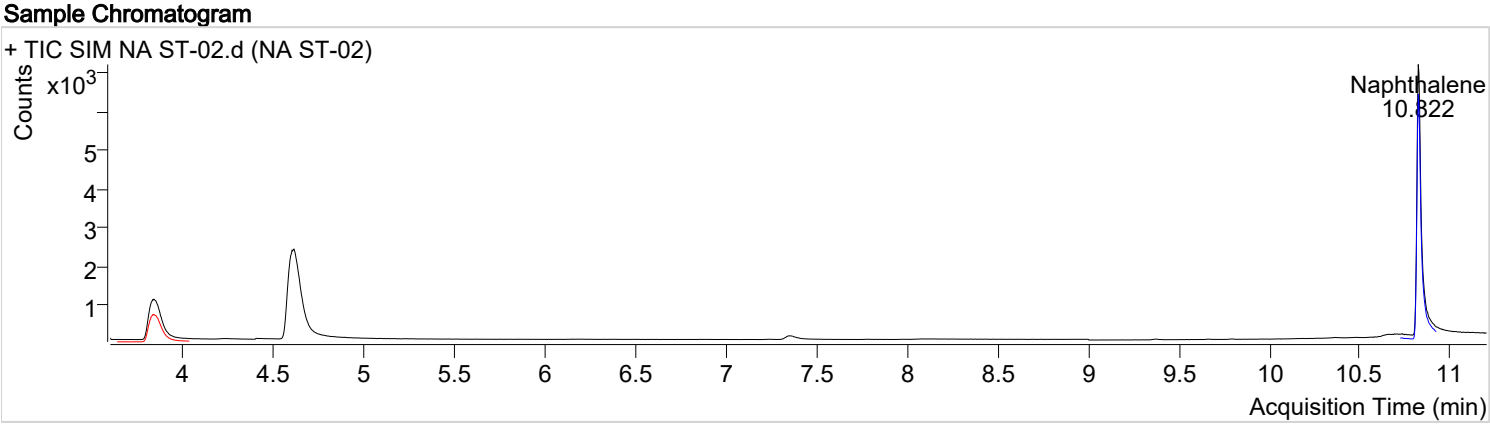

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.822	11484	3549	0.005 mg/L

Naphthalene





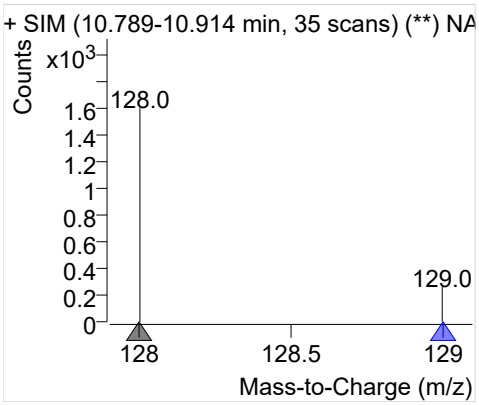

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\NA.batch.bin		
Analysis Time	2026-04-01 오후 4:45:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:59:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:45:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 3:08:44	**Data File**	NA ST-03.d
Type	Cal	**Name**	NA ST-03
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

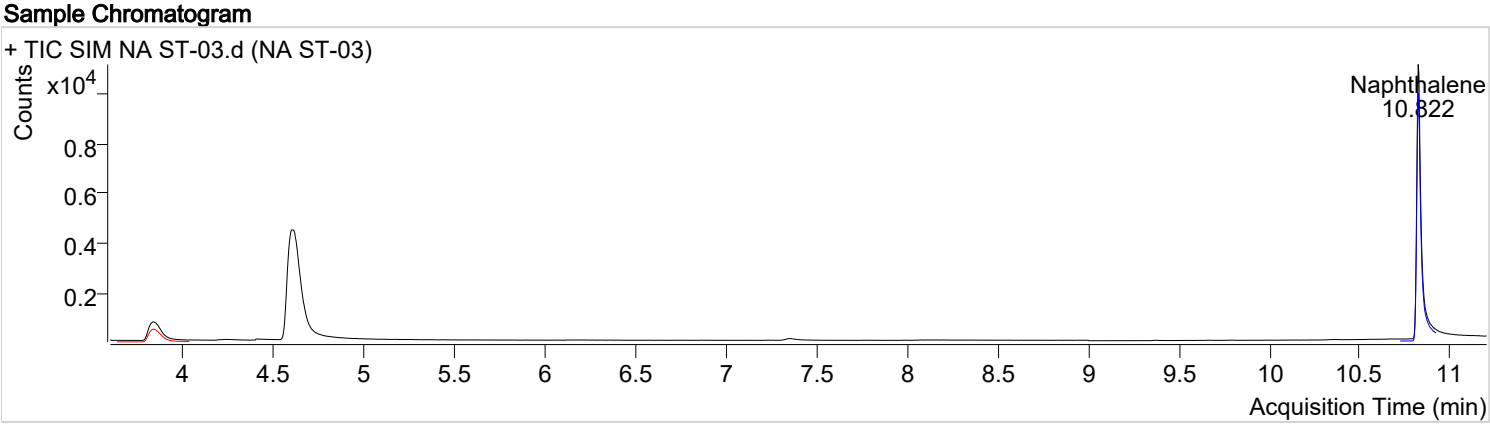

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.822	17371	2469	0.011 mg/L

Naphthalene

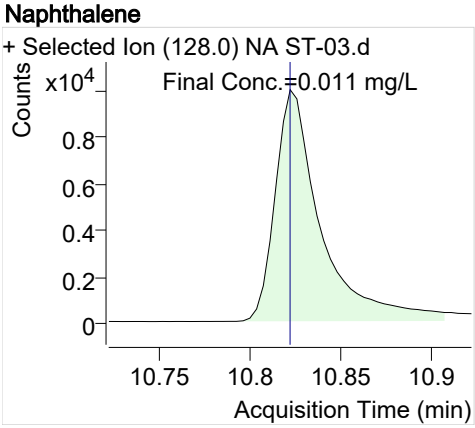

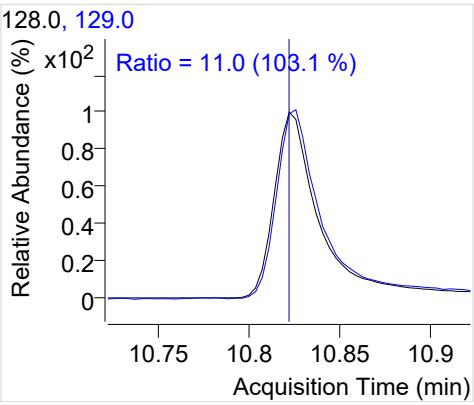

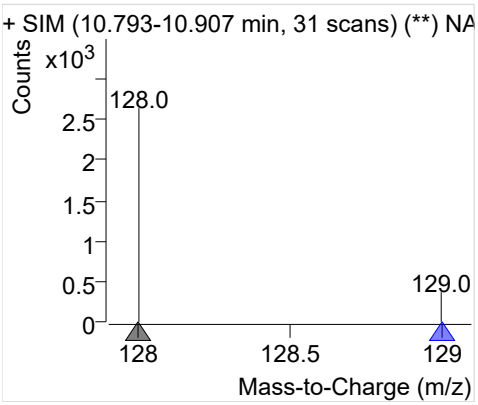

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\NA.batch.bin		
Analysis Time	2026-04-01 오후 4:45:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:59:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:45:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 3:25:52	**Data File**	NA ST-04.d
Type	Cal	**Name**	NA ST-04
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

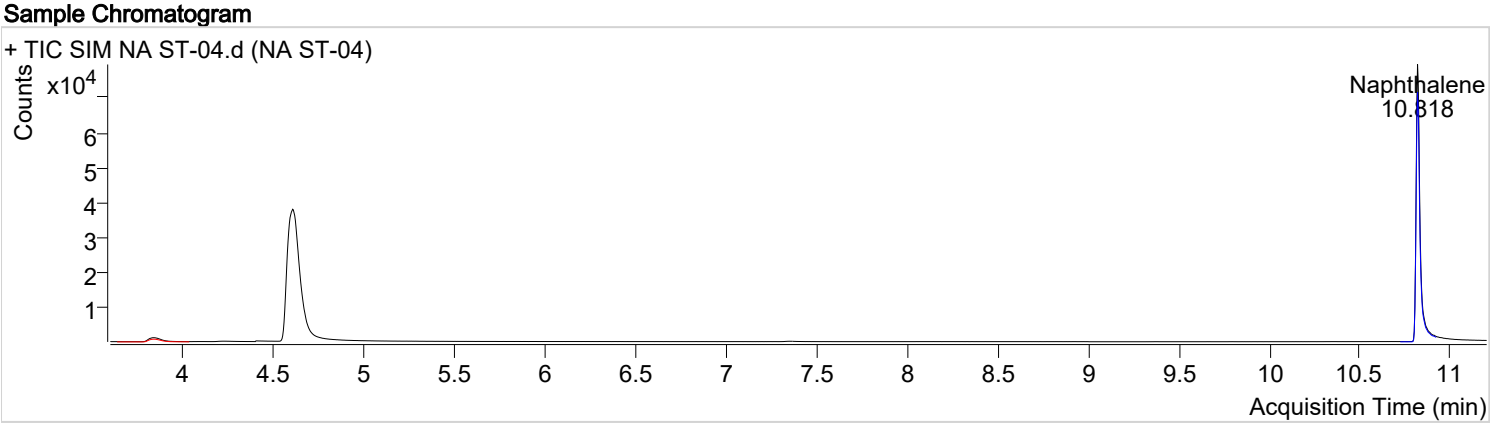

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.818	111460	3705	0.047 mg/L

Naphthalene





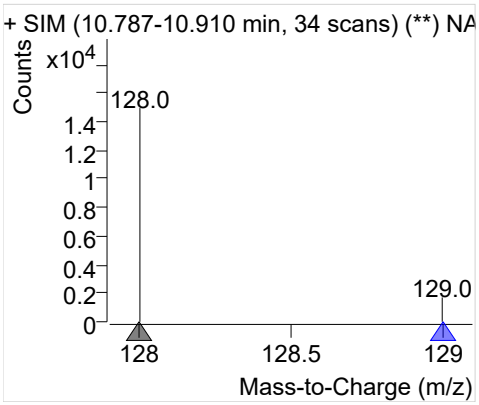

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\NA.batch.bin		
Analysis Time	2026-04-01 오후 4:45:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:59:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:45:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 3:42:56	**Data File**	NA ST-05.d
Type	Cal	**Name**	NA ST-05
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

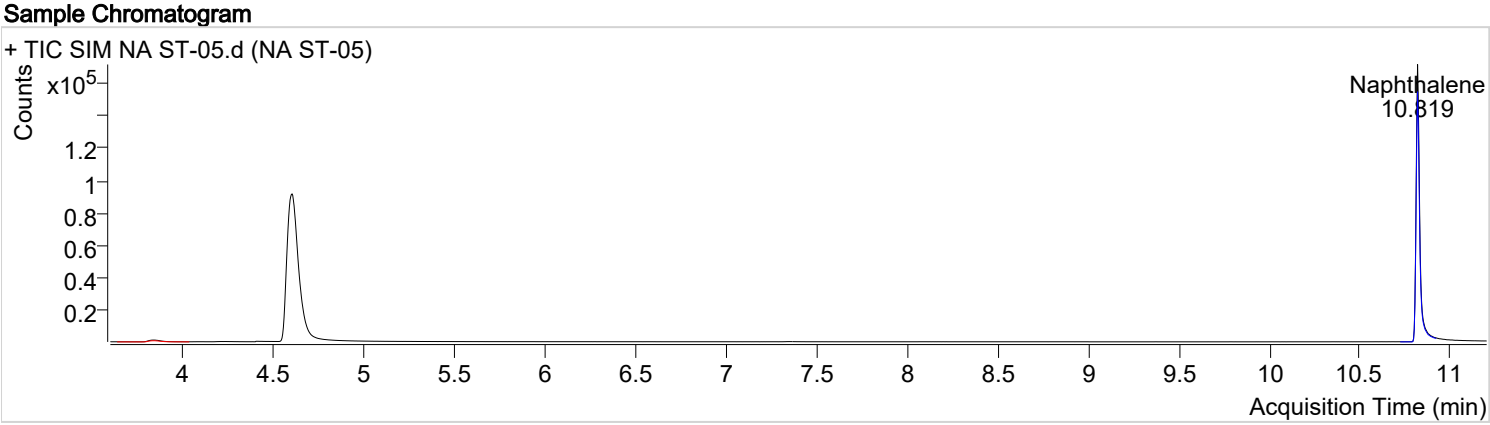

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.819	217311	3395	0.101 mg/L

Naphthalene





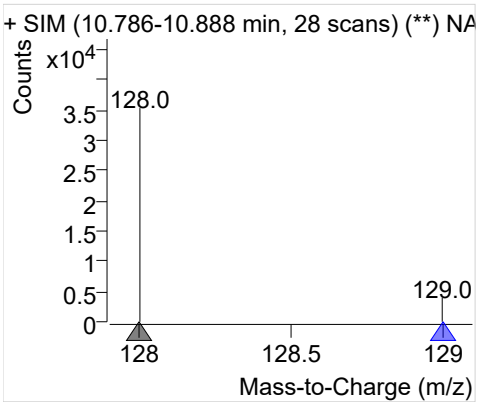

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\NA.batch.bin		
Analysis Time	2026-04-01 오후 4:45:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:59:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:45:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 5:59:19	**Data File**	BK-.d
Type	Blank	**Name**	BK-
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

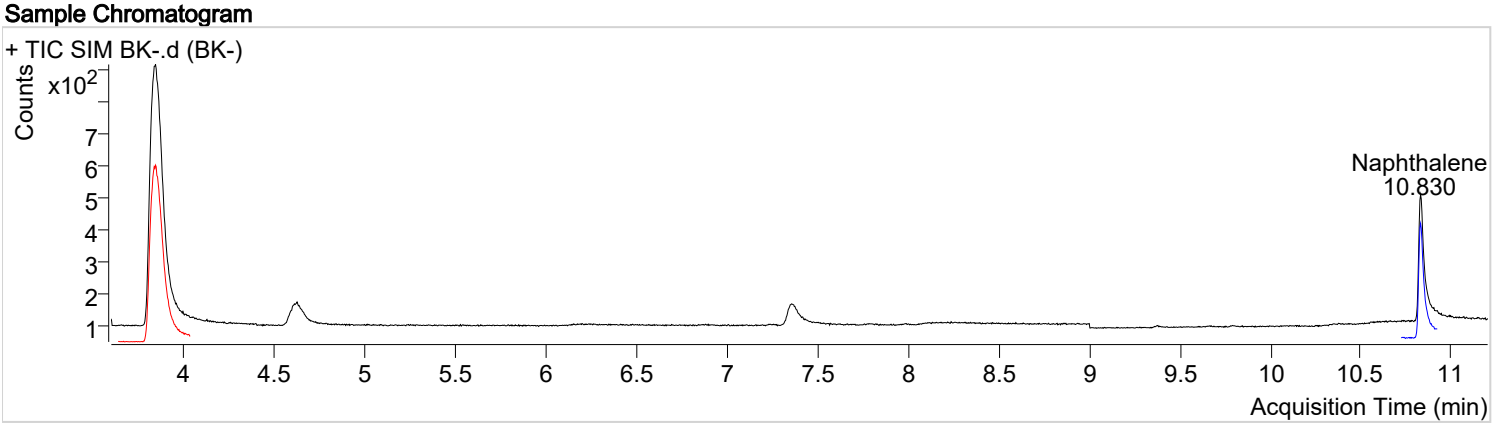

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.830	833	2936	0.000 mg/L

Naphthalene





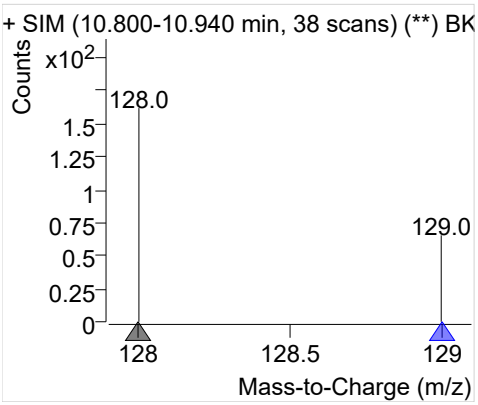

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\NA.batch.bin		
Analysis Time	2026-04-01 오후 4:45:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:59:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:45:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 6:16:20	**Data File**	FBK(NK 26-03-26).d
Type	Blank	**Name**	FBK(NK 26-03-26)
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

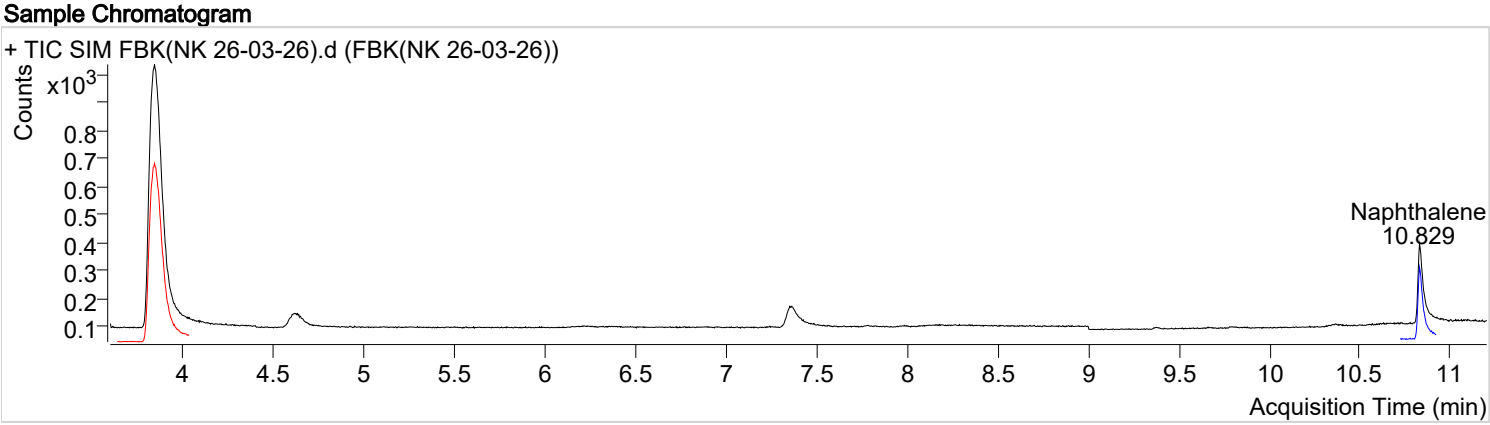

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.829	552	3356	0.000 mg/L

Naphthalene





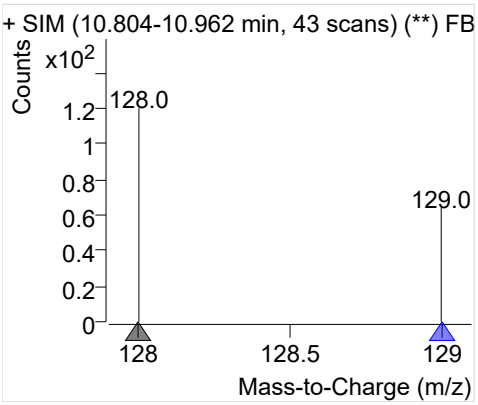

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\NA.batch.bin		
Analysis Time	2026-04-01 오후 4:45:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:59:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:45:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 6:33:23	**Data File**	NJ-01.d
Type	Sample	**Name**	NJ-01
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

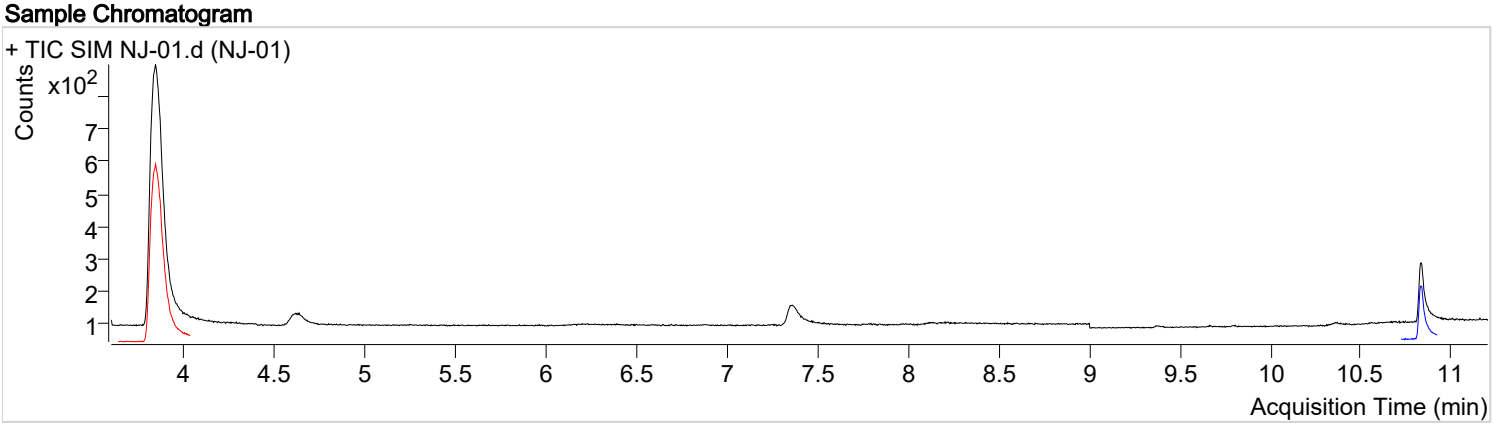

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			2853	ND mg/L

Naphthalene







Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\NA.batch.bin		
Analysis Time	2026-04-01 오후 4:45:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:59:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:45:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 6:50:26	**Data File**	NJ-02.d
Type	Sample	**Name**	NJ-02
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

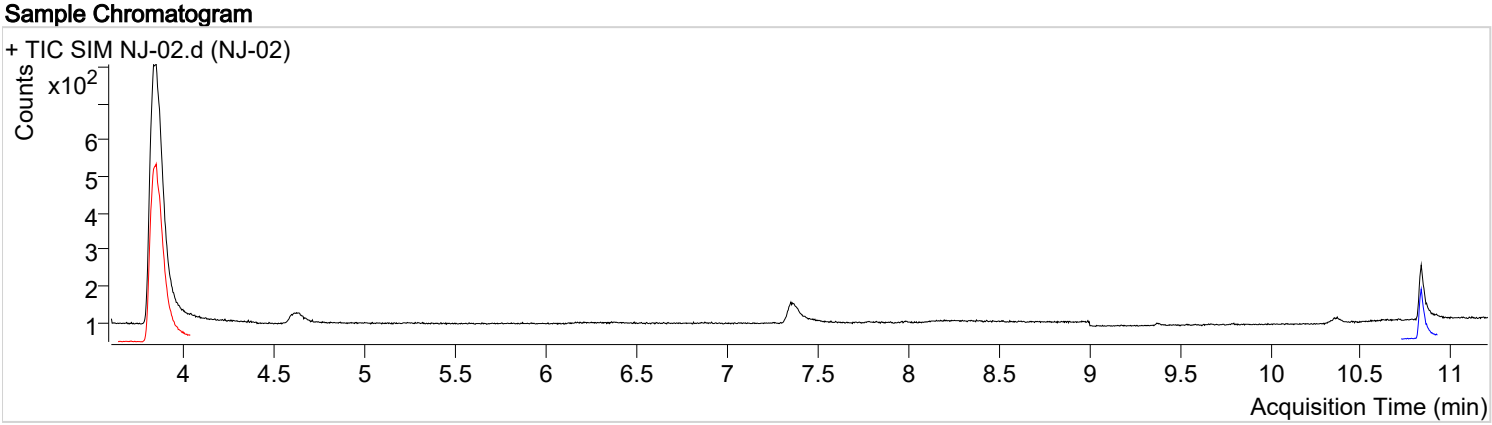

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			2604	ND mg/L

Naphthalene







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\NA.batch.bin		
Analysis Time	2026-04-01 오후 4:45:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:59:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:45:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 7:07:32	**Data File**	NJ-03.d
Type	Sample	**Name**	NJ-03
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

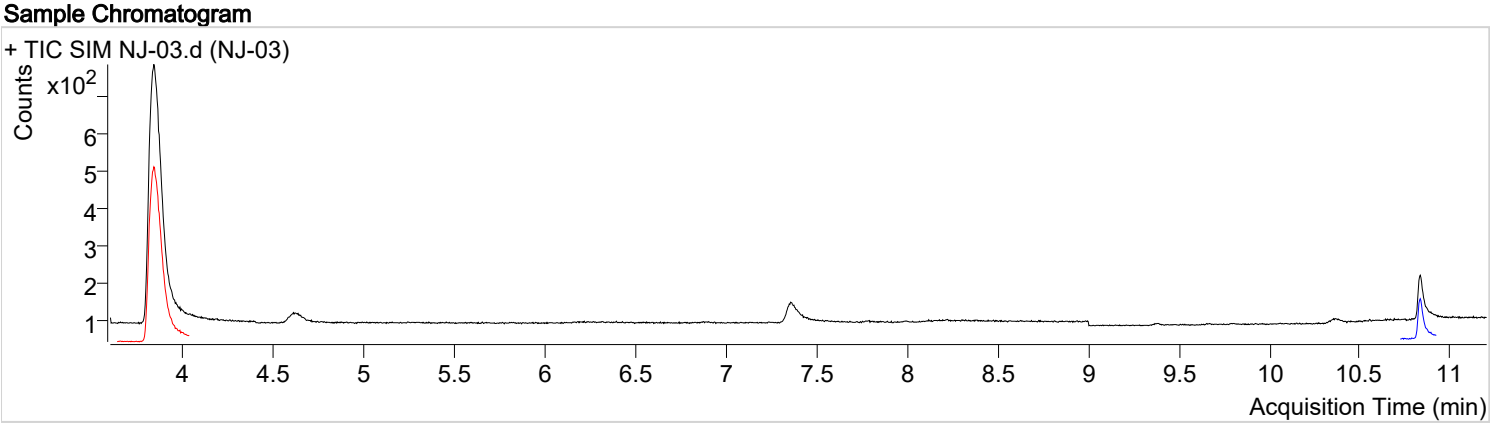

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			2431	ND mg/L

Naphthalene

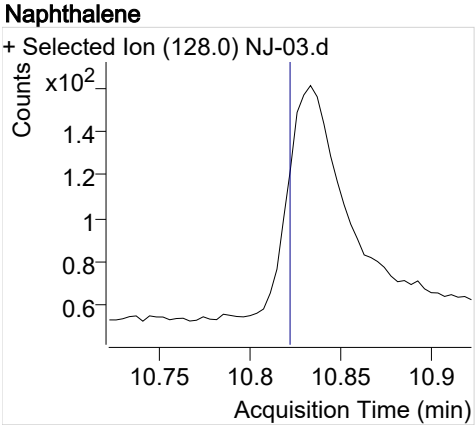

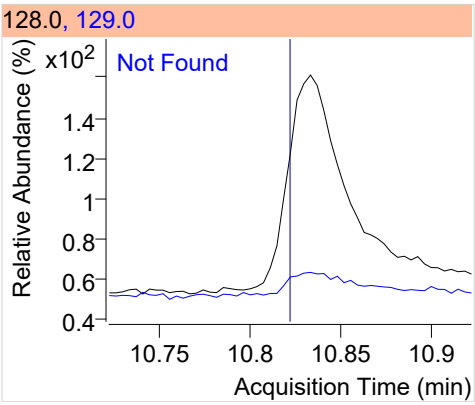

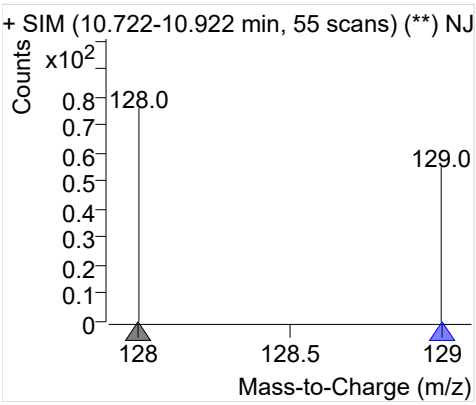

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\NA.batch.bin		
Analysis Time	2026-04-01 오후 4:45:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:59:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:45:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 7:24:34	**Data File**	NJ-04.d
Type	Sample	**Name**	NJ-04
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

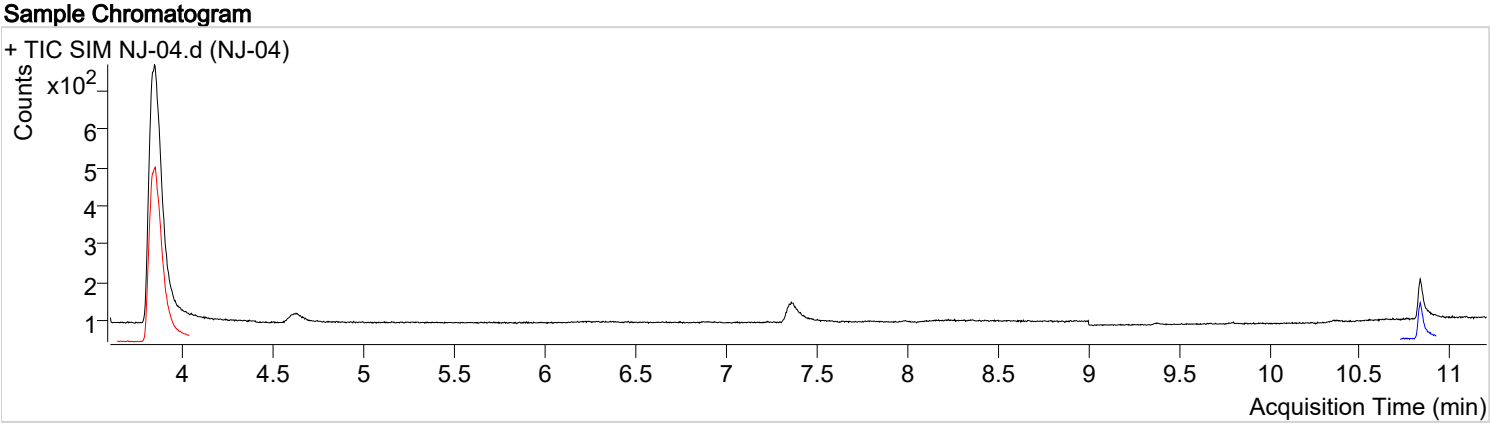

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			2388	ND mg/L

Naphthalene

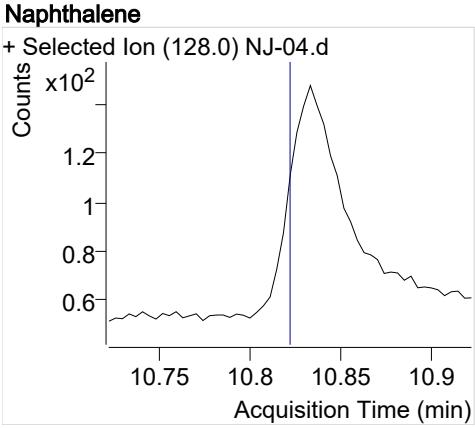

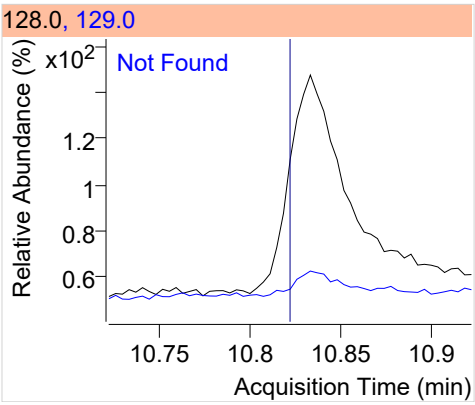

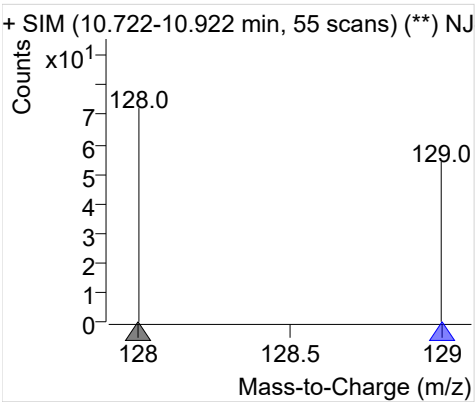

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\NA.batch.bin		
Analysis Time	2026-04-01 오후 4:45:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:59:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:45:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 7:41:39	**Data File**	NJ-05.d
Type	Sample	**Name**	NJ-05
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

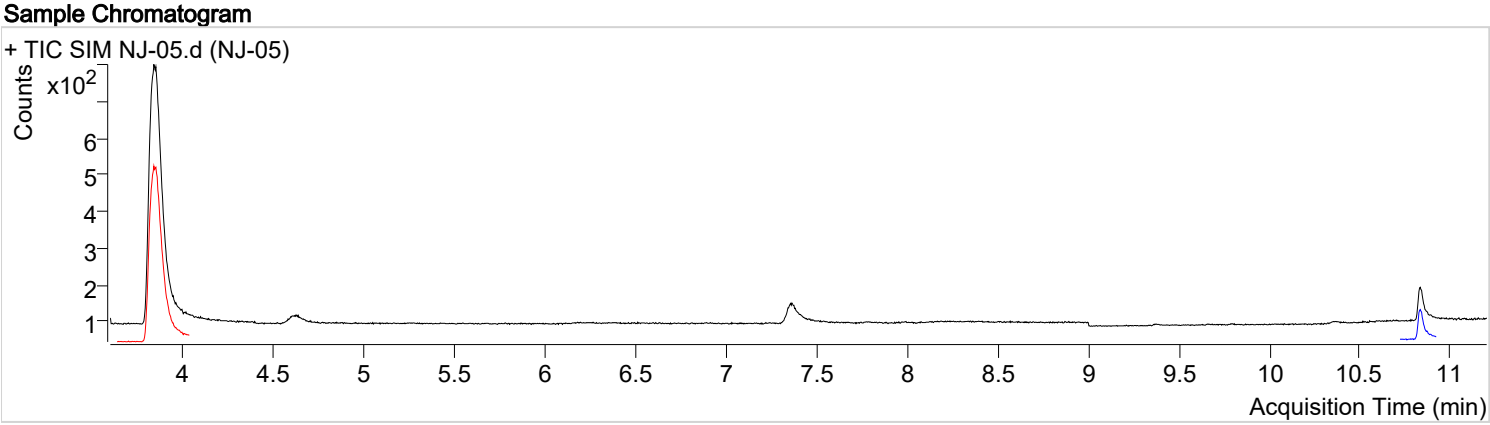

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			2536	ND mg/L

Naphthalene

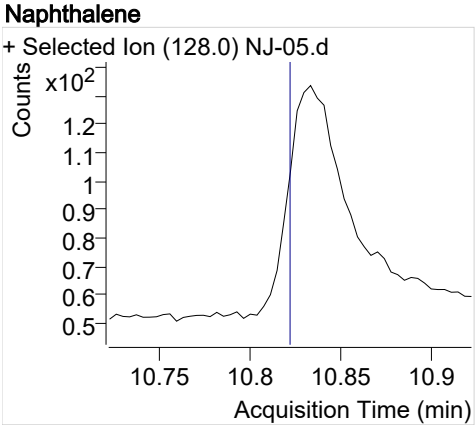

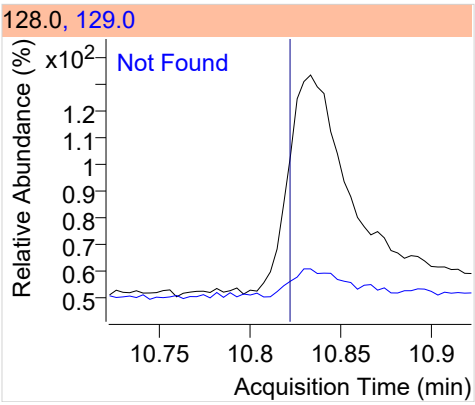

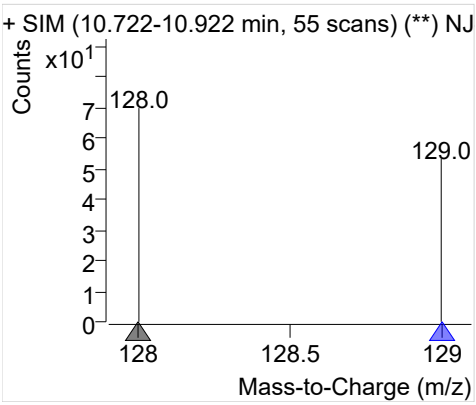

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\NA.batch.bin		
Analysis Time	2026-04-01 오후 4:45:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:59:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:45:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 7:58:51	**Data File**	NJ-06.d
Type	Sample	**Name**	NJ-06
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

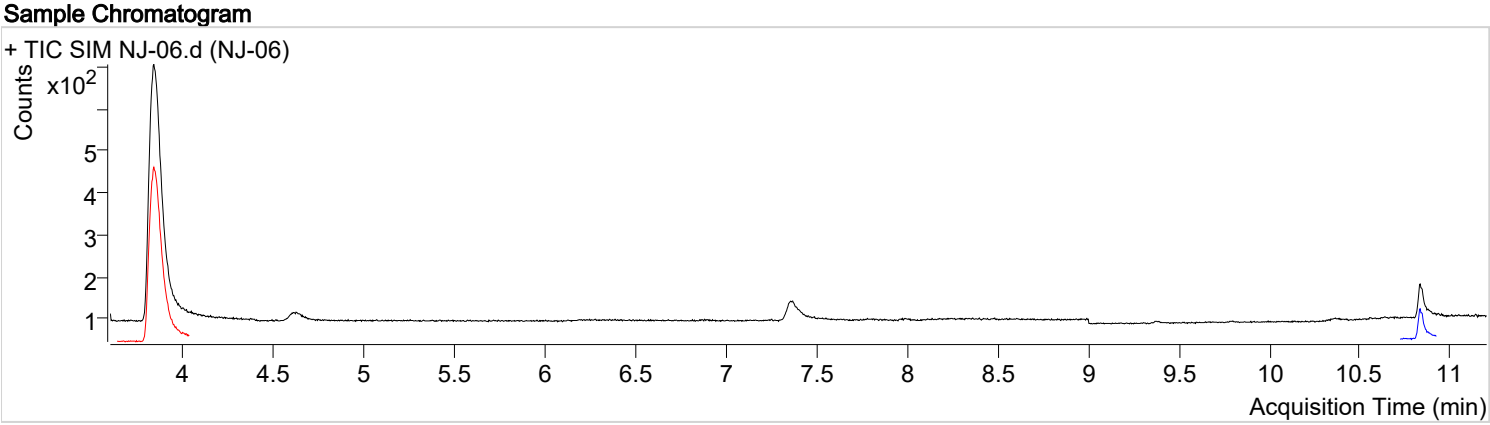

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			2127	ND mg/L

Naphthalene

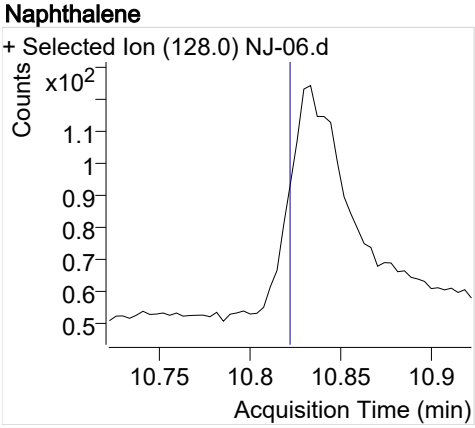

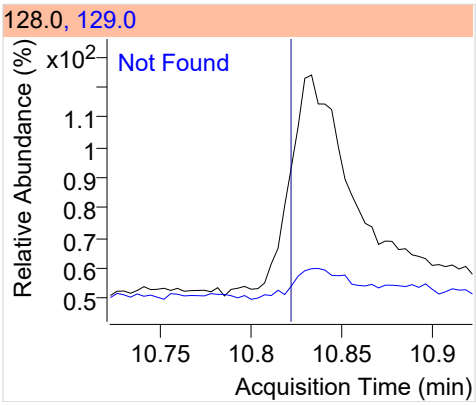

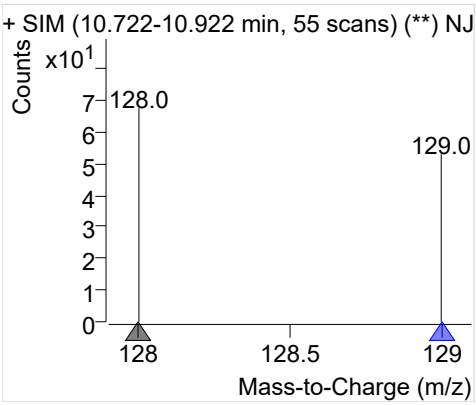

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\NA.batch.bin		
Analysis Time	2026-04-01 오후 4:45:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:59:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:45:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 8:15:51	**Data File**	MBK.d
Type	Blank	**Name**	MBK
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

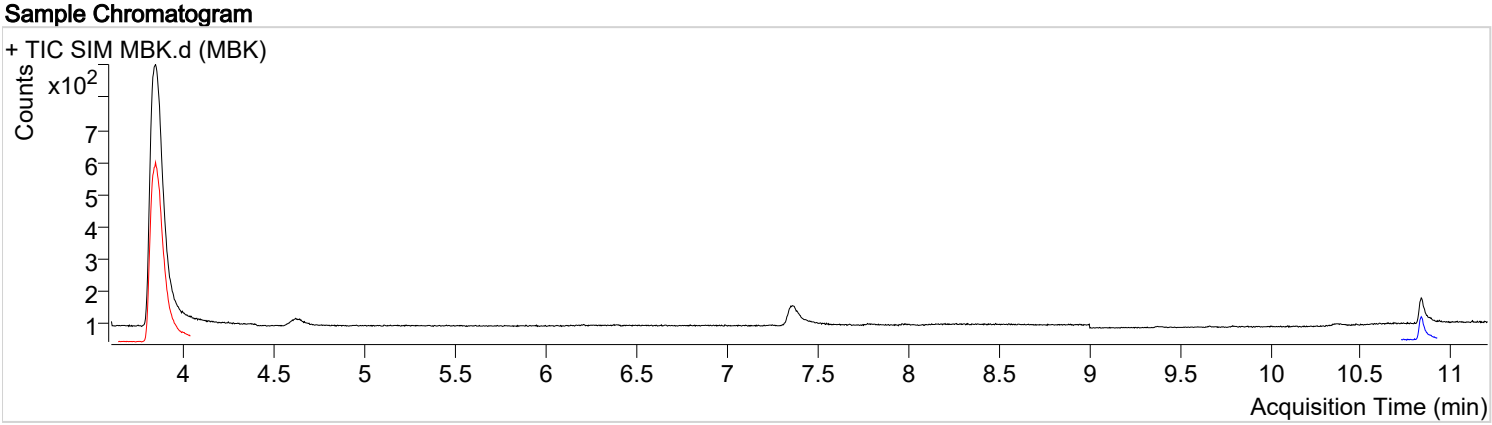

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene			2933	ND mg/L

Naphthalene





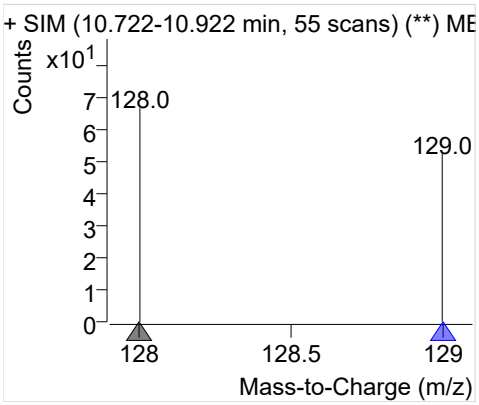

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\NA.batch.bin		
Analysis Time	2026-04-01 오후 4:45:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:59:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:45:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 8:32:57	**Data File**	CCV N.d
Type	QC	**Name**	CCV N
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

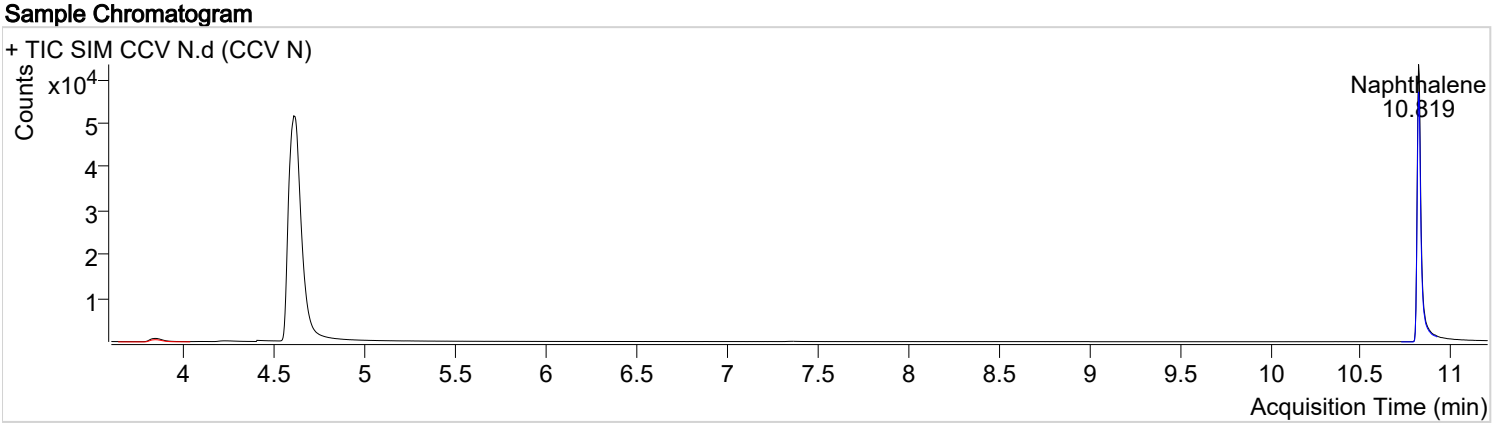

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Naphthalene	10.819	90492	2395	0.060 mg/L
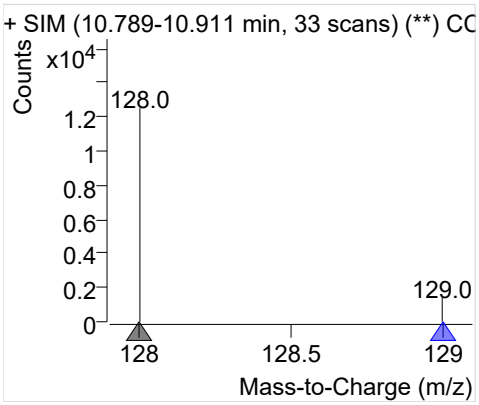
Naphthalene