Quantitative Analysis Results Summary Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\S.batch.bin				
Analysis Time	2026-01-08 오후 1:37:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 1:37:41	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Styrene

Data File	Type	RT	Resp.	Final Conc.
Styrene ST-01.D	Cal	8.768	762	0.013
Styrene ST-02.D	Cal	8.767	3213	0.016
Styrene ST-03.D	Cal	8.768	13121	0.030
Styrene ST-04.D	Cal	8.767	103269	0.151
Styrene ST-05.D	Cal	8.767	363667	0.502
BK-.D	Blank			ND
FBK(PL 25-12-30).D	Blank			ND
PL-01.D	Sample			ND
PL-02.D	Sample			ND
JR(25-01-02).D	Sample			ND
MBK.D	Blank			ND
CCV-(S).D	QC	8.767	144055	0.206

Styrene

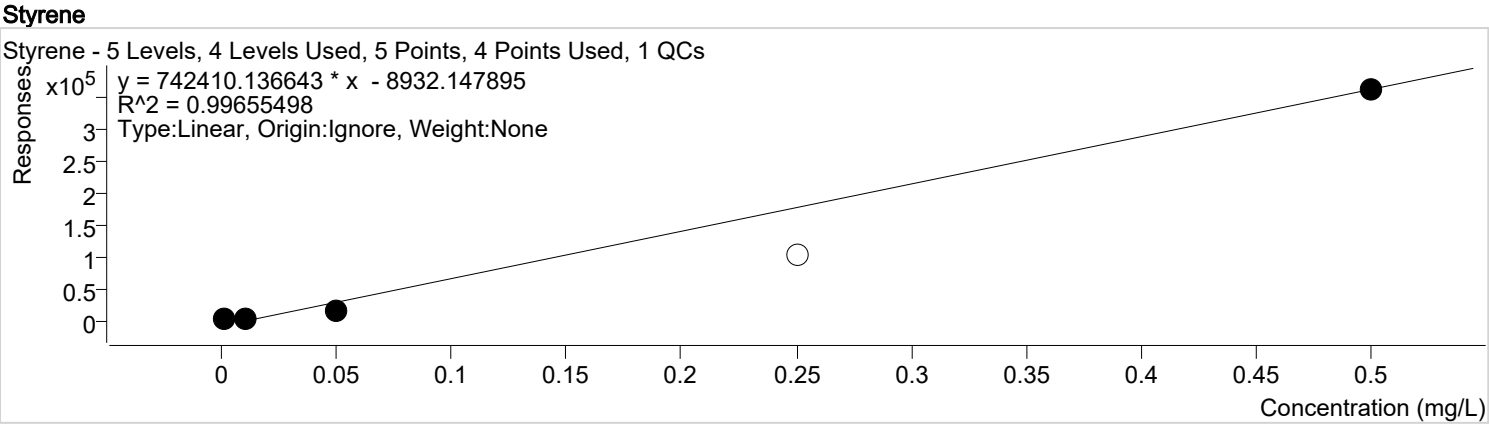

Cal. Path	Type	Level	Enable	Conc.	Response
D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\Styrene ST-01.D	Calibration	1	x	0.001	762
D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\Styrene ST-02.D	Calibration	2	x	0.010	3213
D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\Styrene ST-03.D	Calibration	3	x	0.050	13121
D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\Styrene ST-04.D	Calibration	4		0.250	103269
D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\CCV-(S).D	QC	4		0.250	144055
D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\Styrene ST-05.D	Calibration	5	x	0.500	363667

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\S.batch.bin		
Analysis Time	2026-01-08 오후 1:37:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:10:10	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 1:37:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-02 오후 1:36:28	**Data File**	Styrene ST-01.D
Type	Cal	**Name**	Styrene ST-01
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

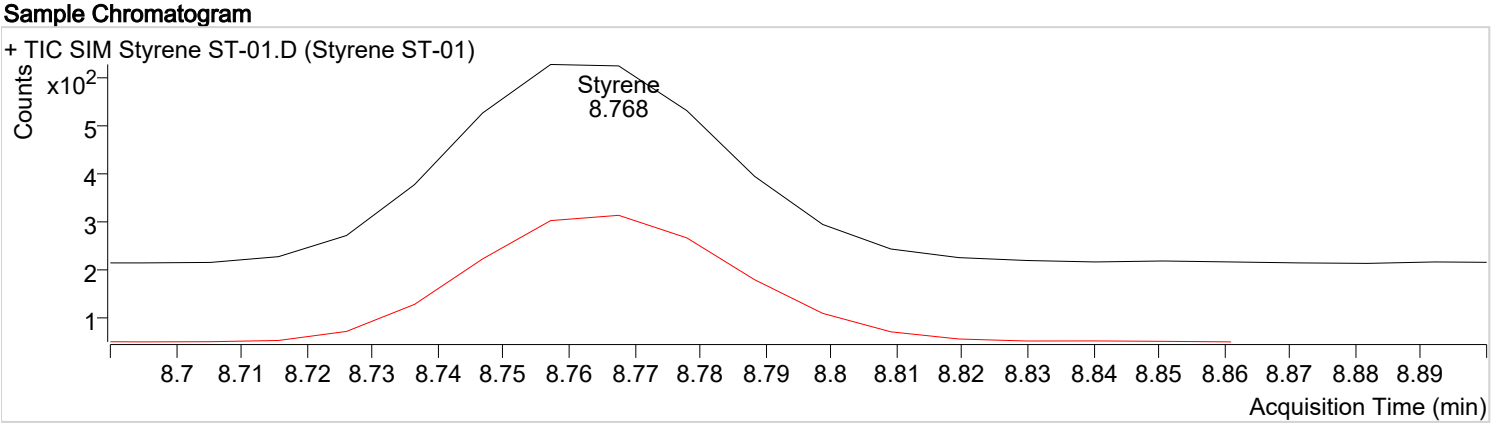

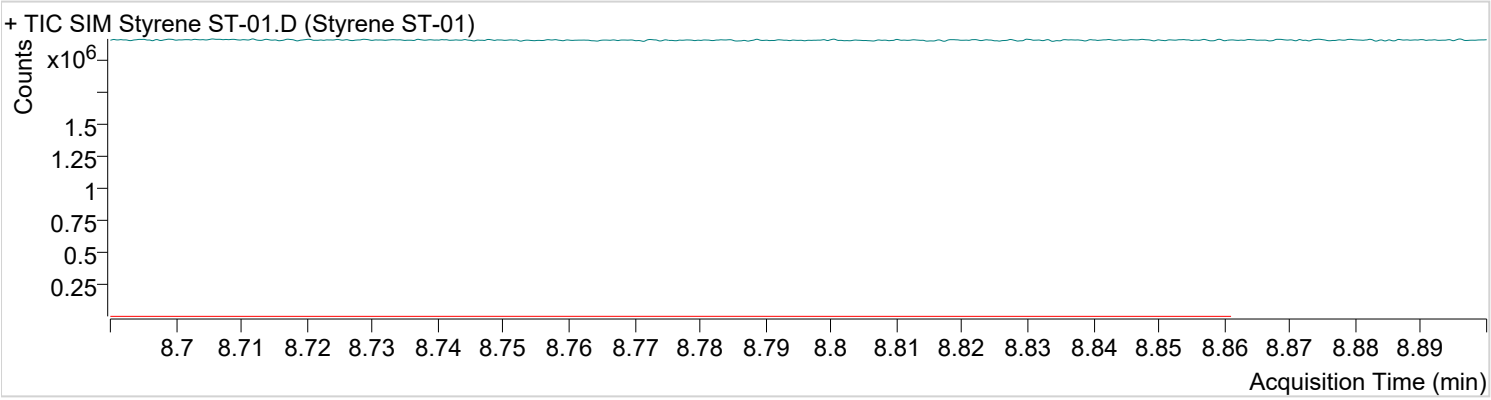

Name	RT	Resp.	Final Conc.	Units
Styrene	8.768	762	0.013	mg/L

Styrene



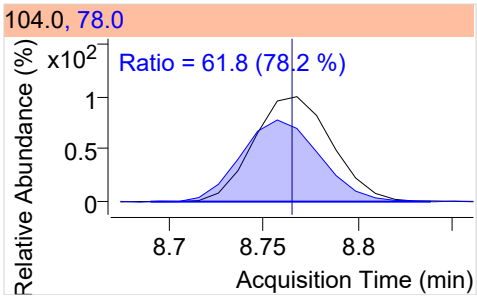

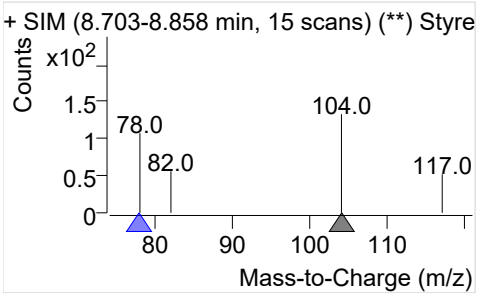

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\S.batch.bin		
Analysis Time	2026-01-08 오후 1:37:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:10:10	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 1:37:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-02 오후 1:53:10	**Data File**	Styrene ST-02.D
Type	Cal	**Name**	Styrene ST-02
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

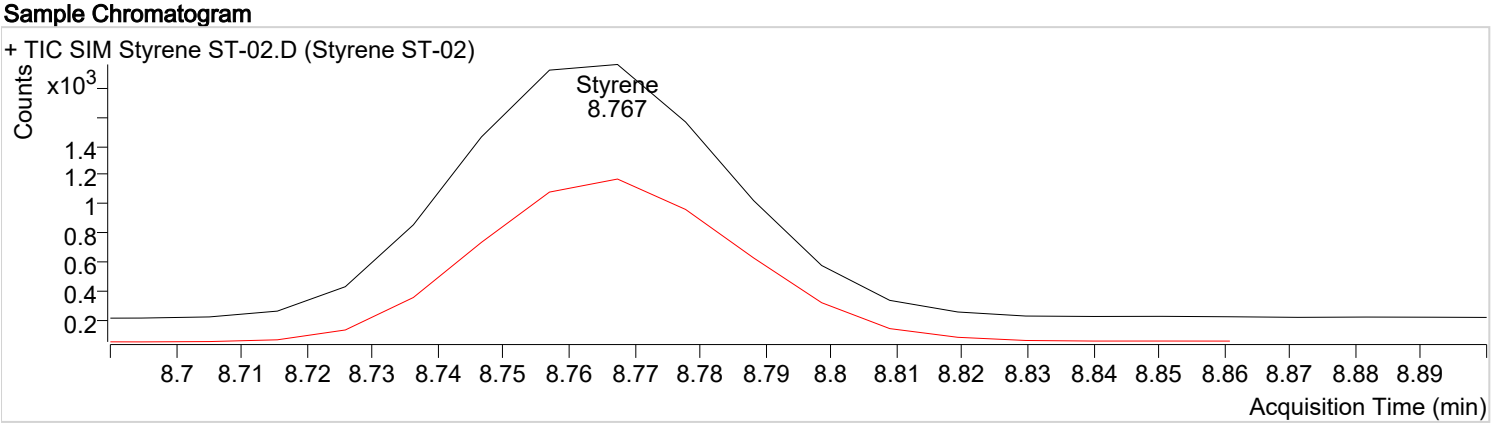

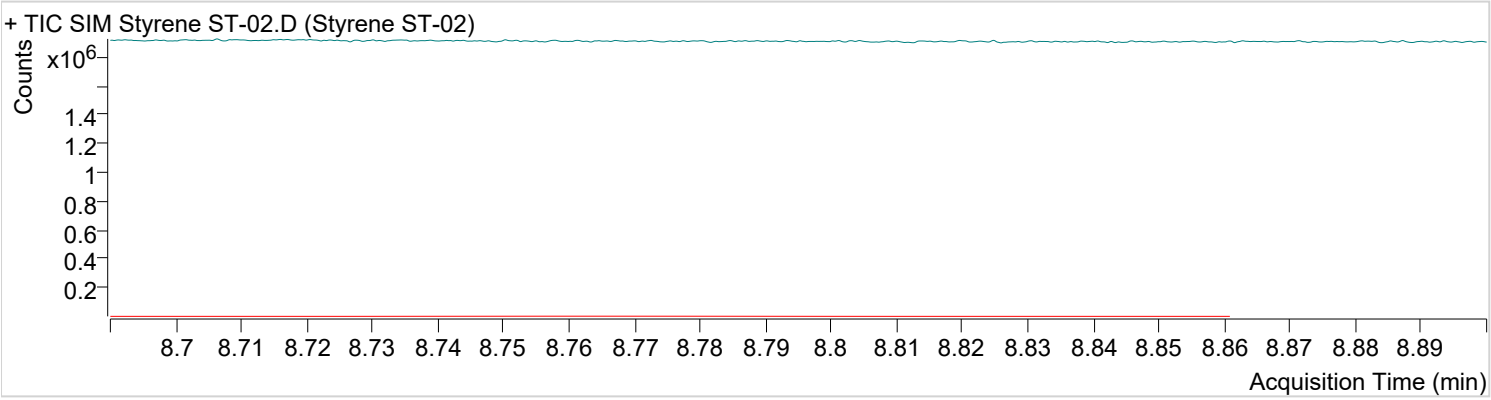

Name	RT	Resp.	Final Conc.	Units
Styrene	8.767	3213	0.016	mg/L

Styrene



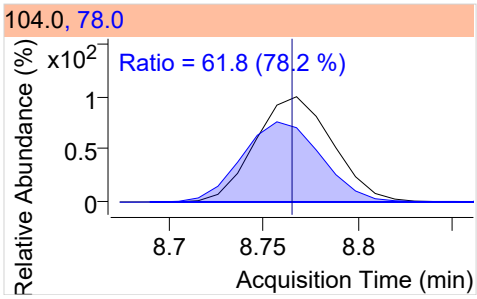

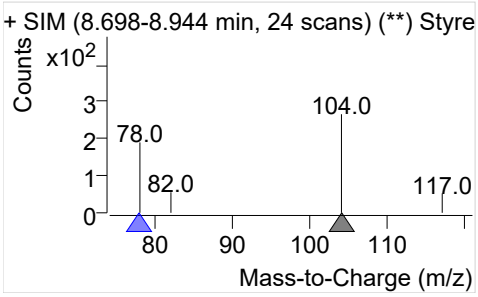

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\S.batch.bin		
Analysis Time	2026-01-08 오후 1:37:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:10:10	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 1:37:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-02 오후 2:09:53	**Data File**	Styrene ST-03.D
Type	Cal	**Name**	Styrene ST-03
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

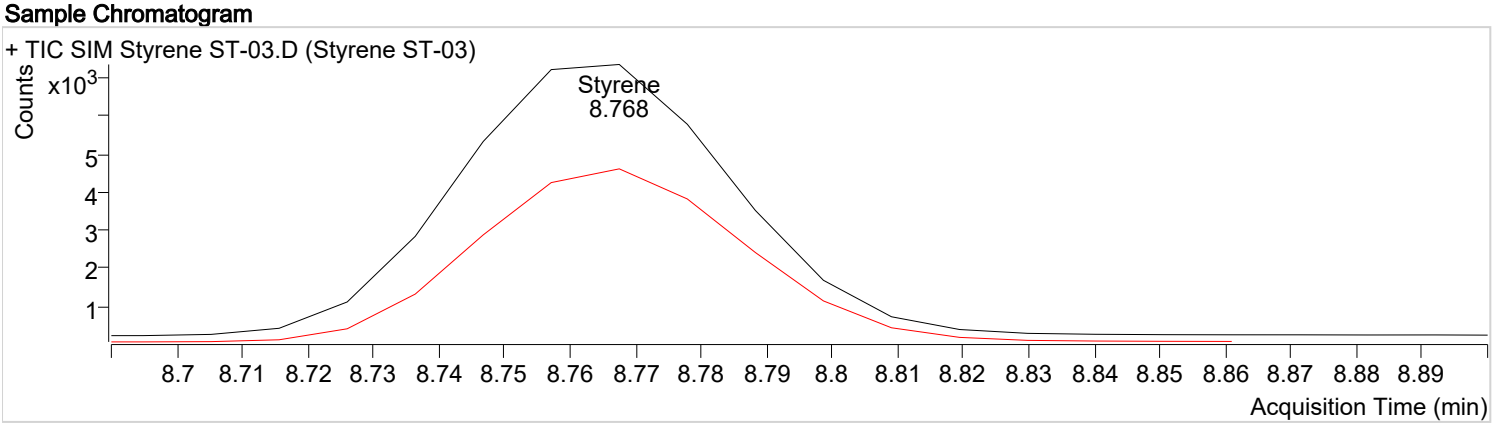

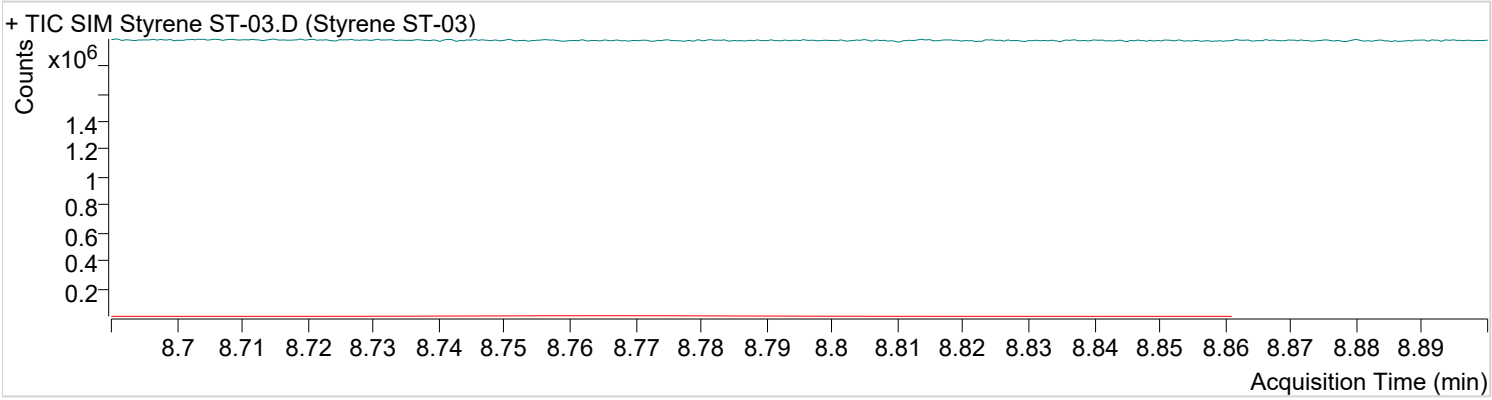

Name	RT	Resp.	Final Conc.	Units
Styrene	8.768	13121	0.030	mg/L

Styrene



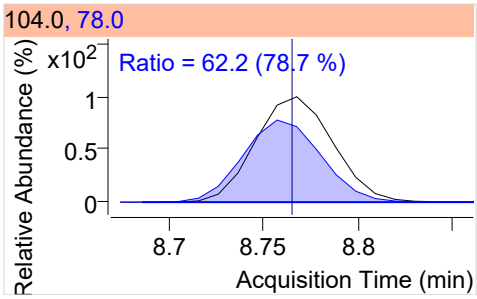

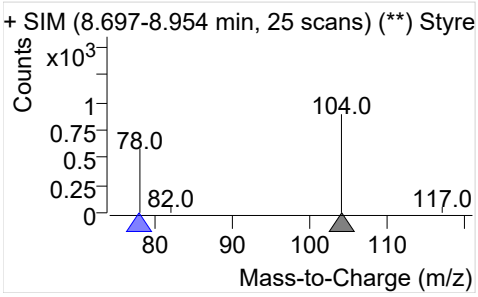

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\S.batch.bin		
Analysis Time	2026-01-08 오후 1:37:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:10:10	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 1:37:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-02 오후 2:26:41	**Data File**	Styrene ST-04.D
Type	Cal	**Name**	Styrene ST-04
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

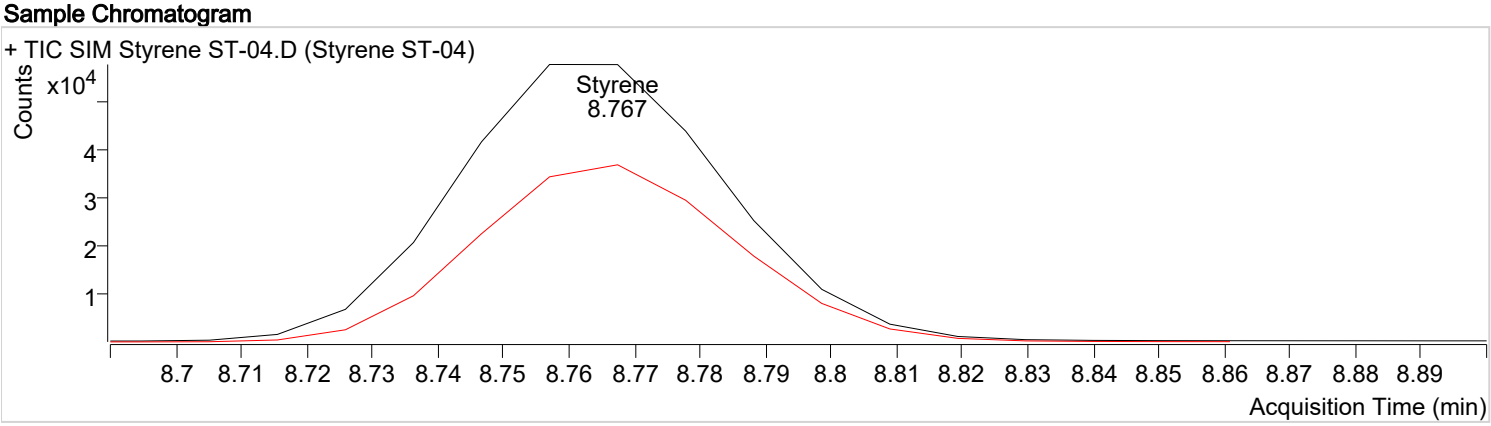

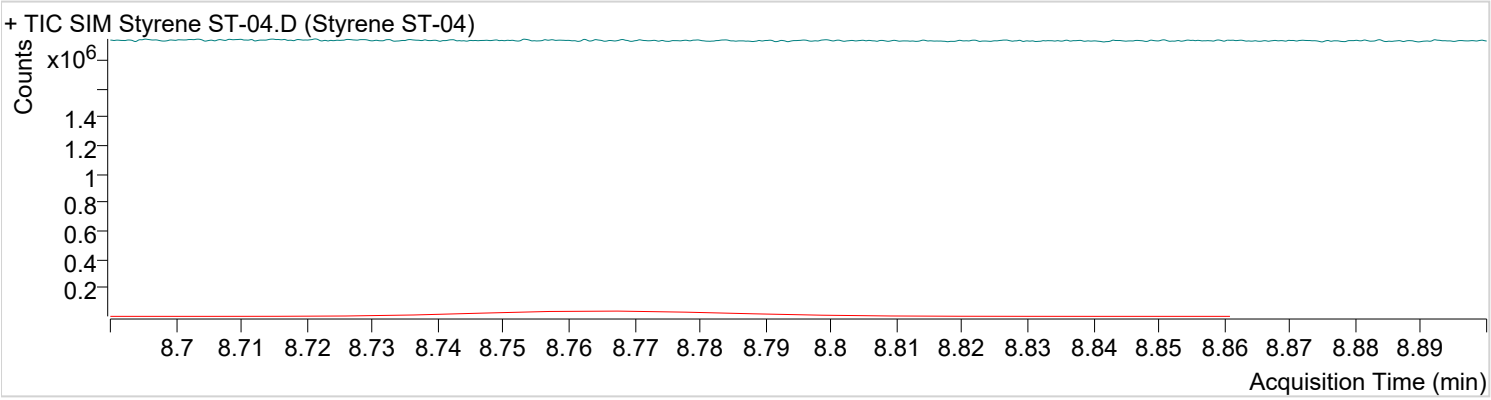

Name	RT	Resp.	Final Conc.	Units
Styrene	8.767	103269	0.151	mg/L

Styrene



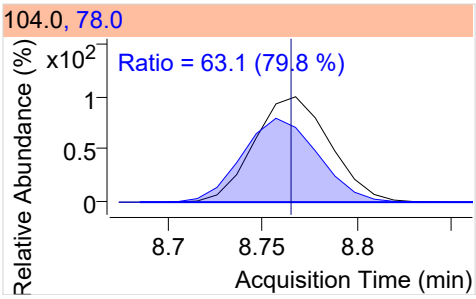

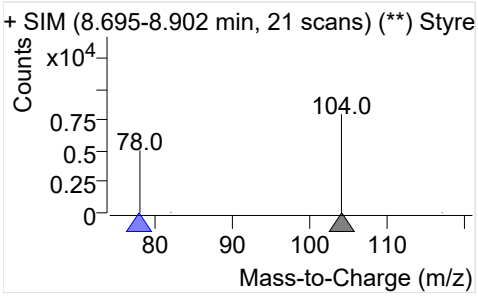

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\S.batch.bin		
Analysis Time	2026-01-08 오후 1:37:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:10:10	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 1:37:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-02 오후 2:43:24	**Data File**	Styrene ST-05.D
Type	Cal	**Name**	Styrene ST-05
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

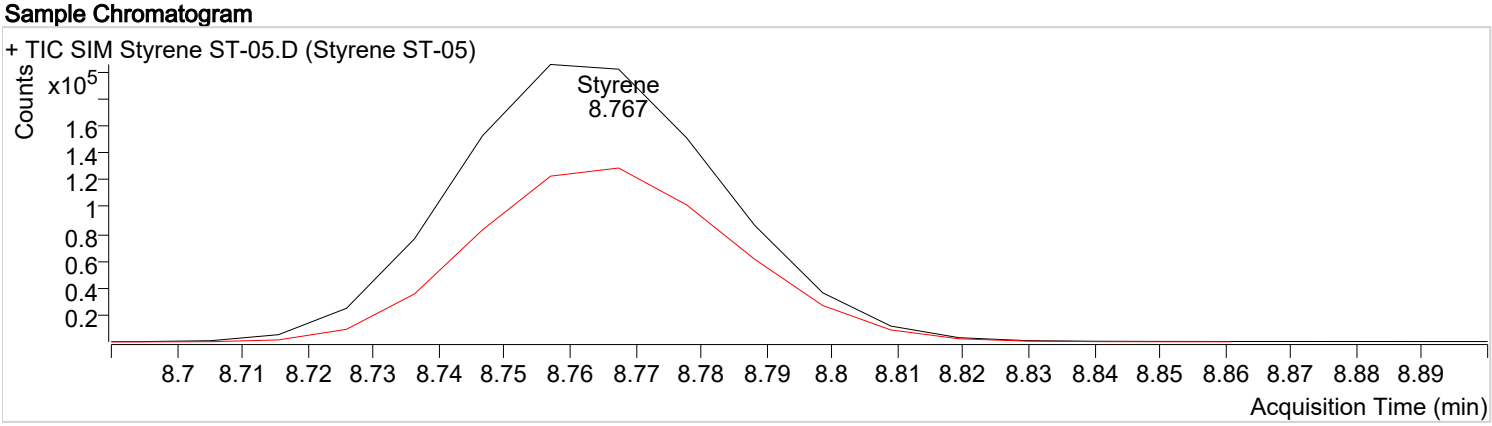

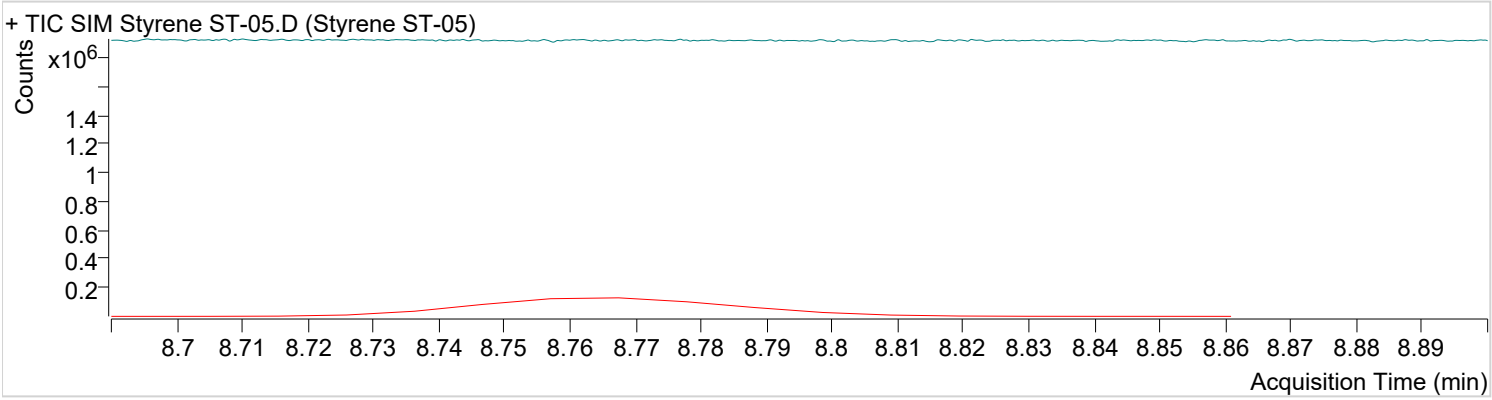

Name	RT	Resp.	Final Conc.	Units
Styrene	8.767	363667	0.502	mg/L

Styrene



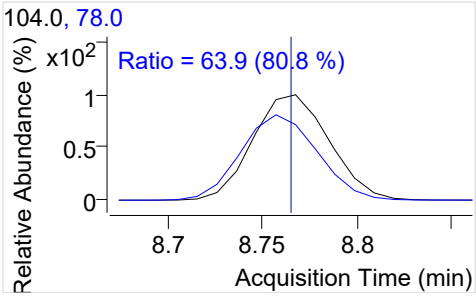

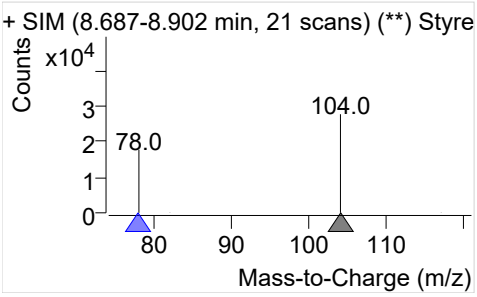

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\S.batch.bin		
Analysis Time	2026-01-08 오후 1:37:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:10:10	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 1:37:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-02 오후 3:22:48	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

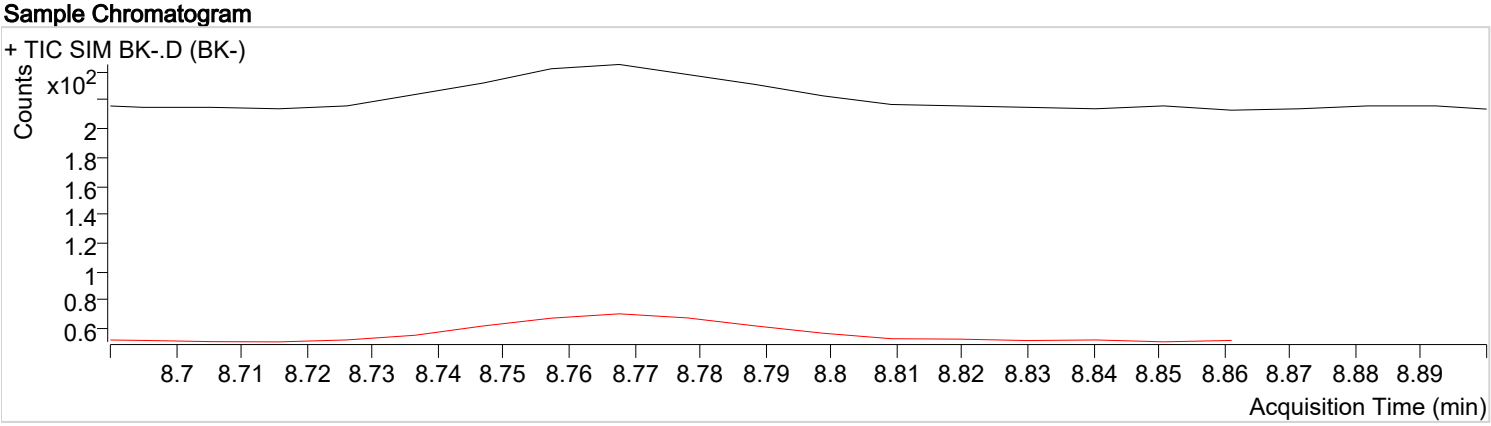

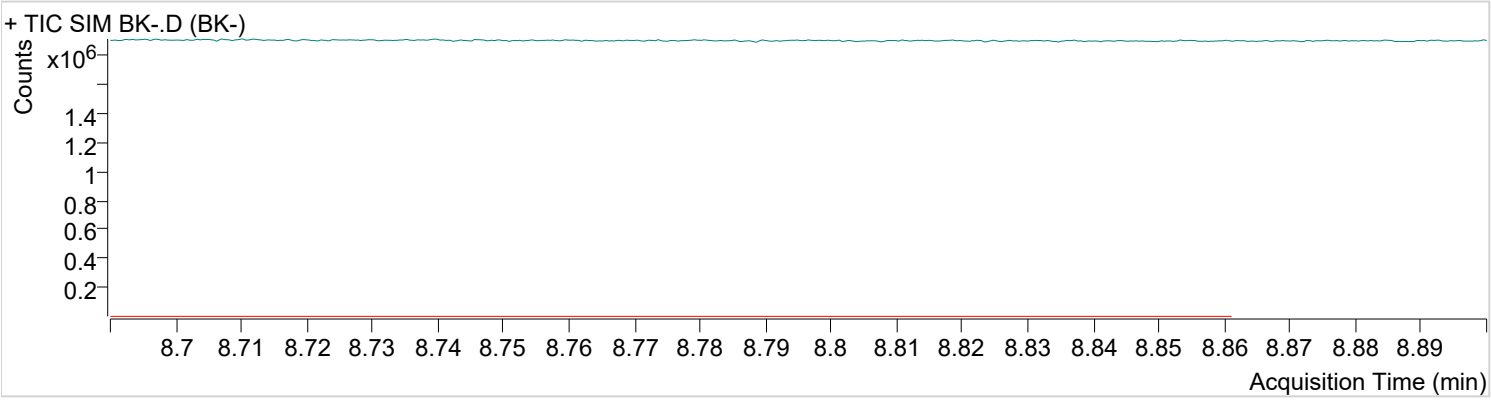

Styrene



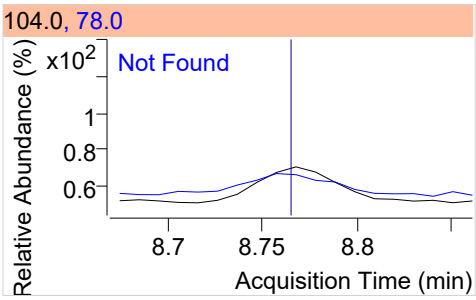

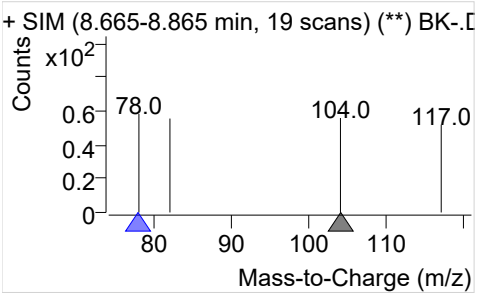

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\S.batch.bin		
Analysis Time	2026-01-08 오후 1:37:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:10:10	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 1:37:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-02 오후 3:40:30	**Data File**	FBK(PL 25-12-30).D
Type	Blank	**Name**	FBK(PL 25-12-30)
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

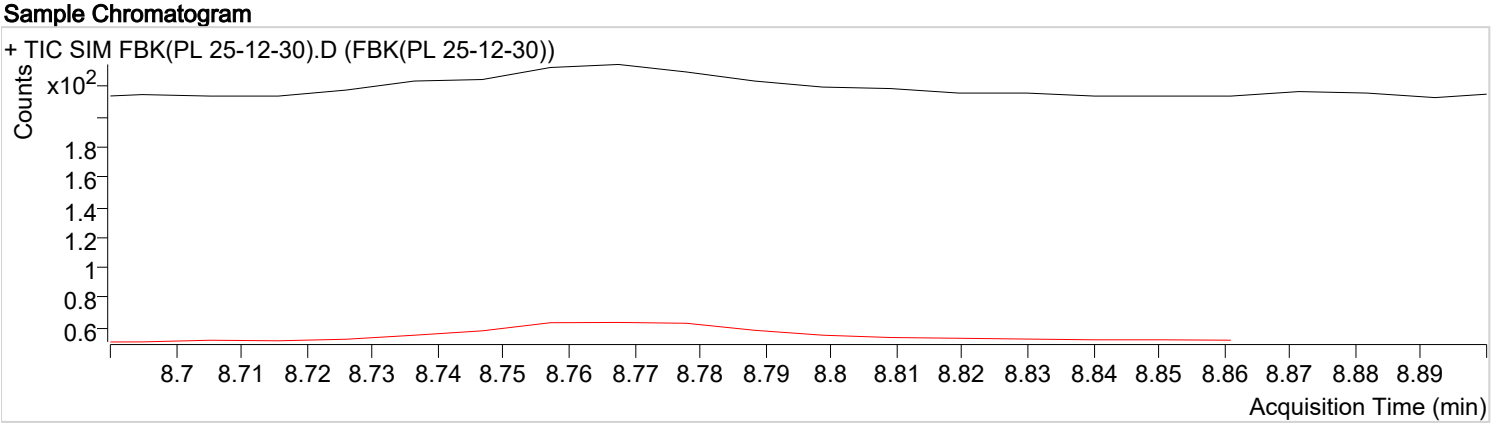

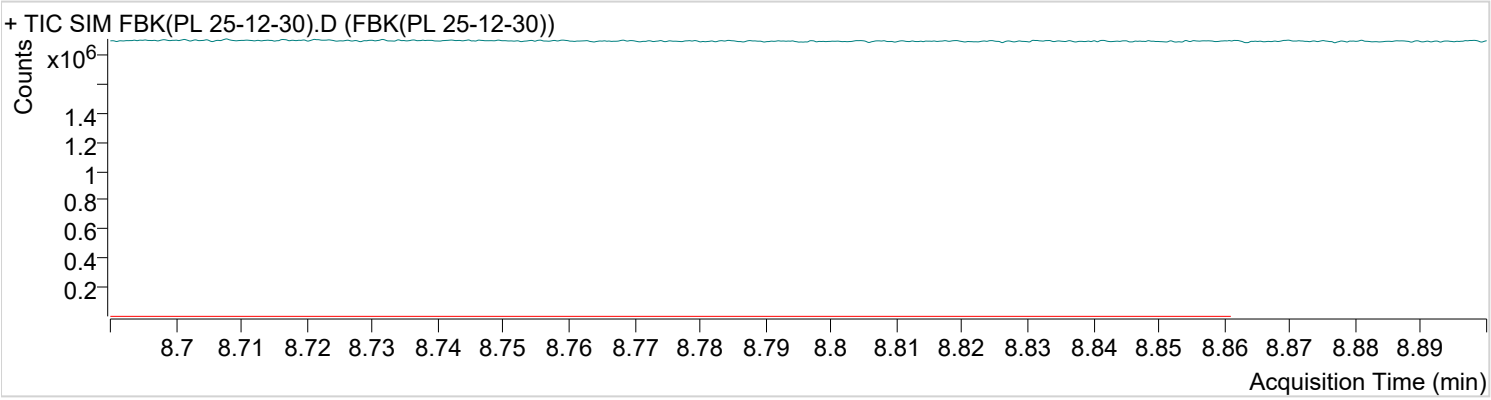

Styrene

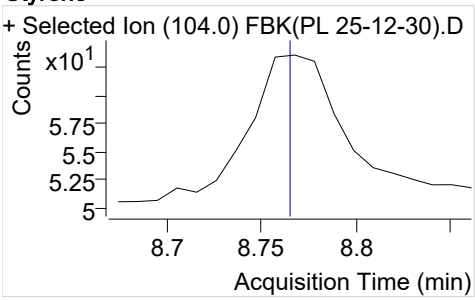

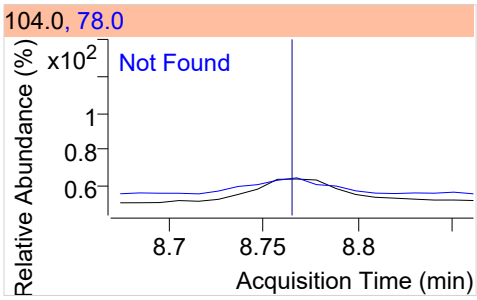

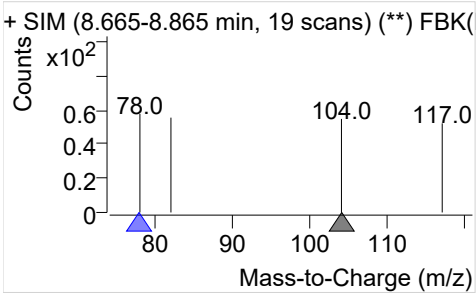

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\S.batch.bin		
Analysis Time	2026-01-08 오후 1:37:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:10:10	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 1:37:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-02 오후 3:58:19	**Data File**	PL-01.D
Type	Sample	**Name**	PL-01
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

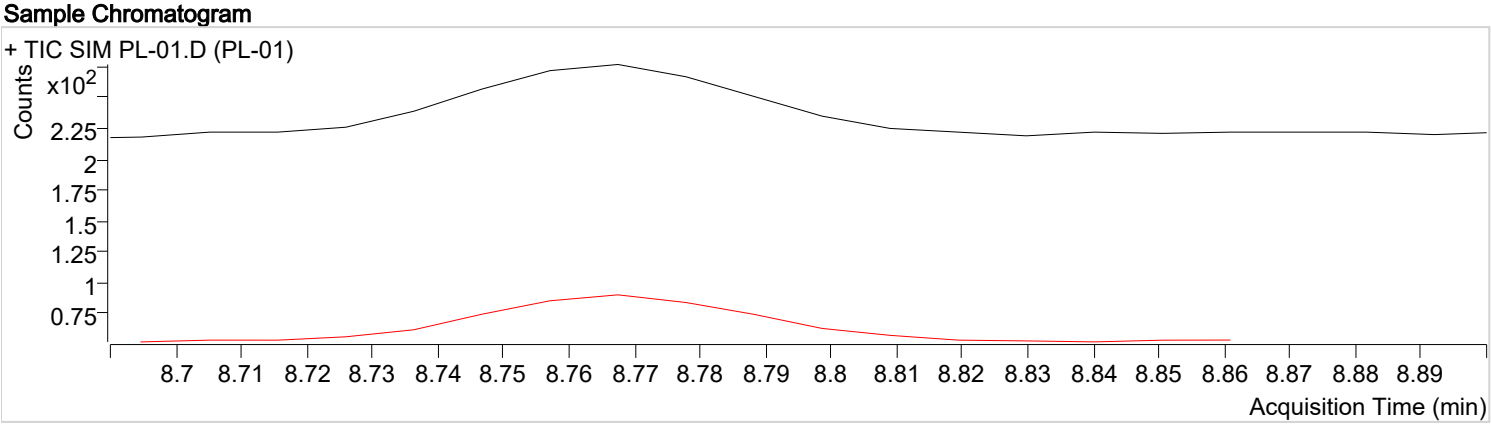

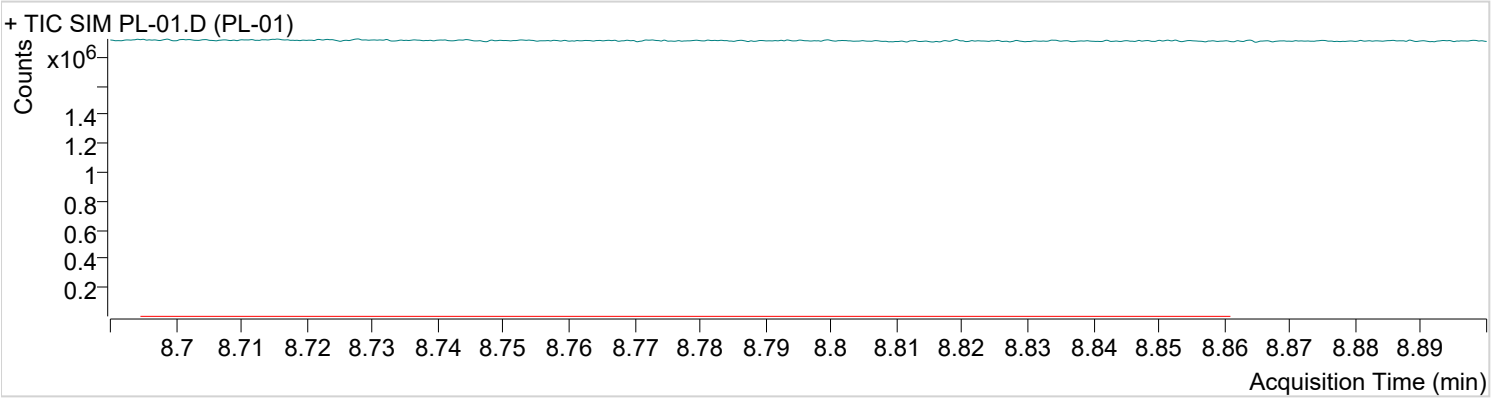

Styrene



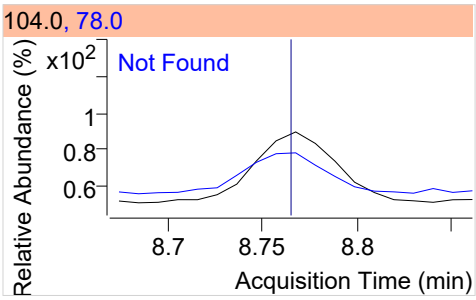

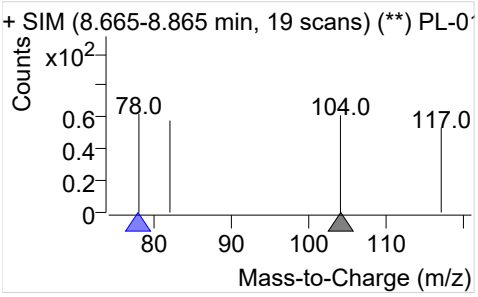

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\S.batch.bin		
Analysis Time	2026-01-08 오후 1:37:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:10:10	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 1:37:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-02 오후 4:16:03	**Data File**	PL-02.D
Type	Sample	**Name**	PL-02
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

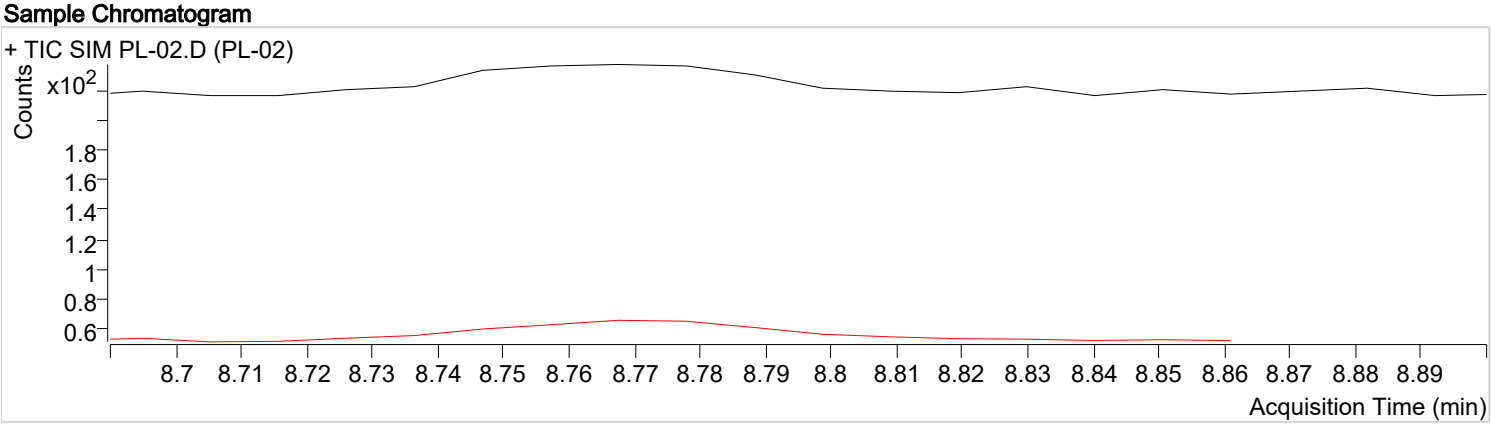

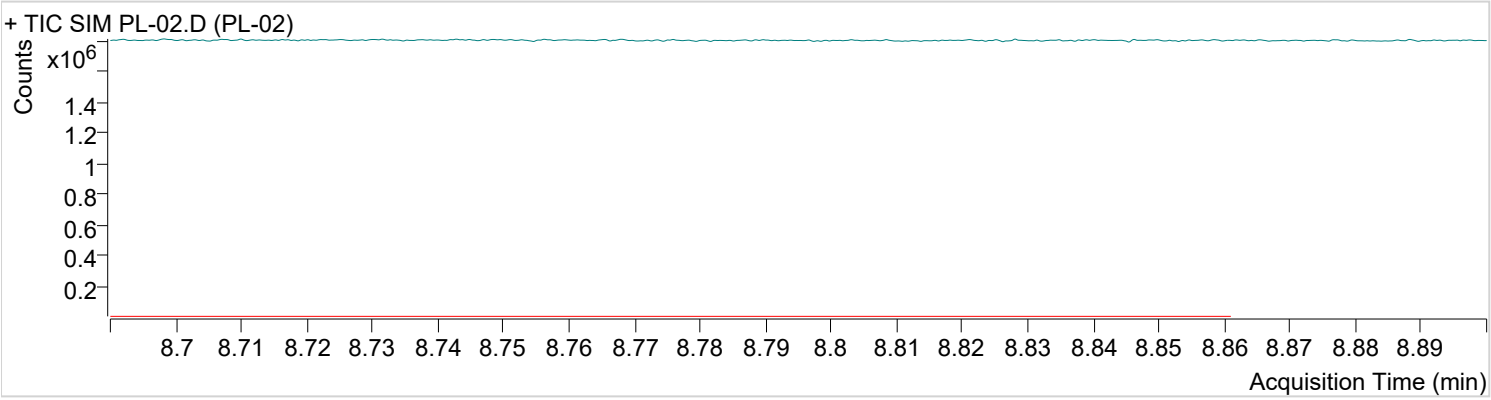

Styrene



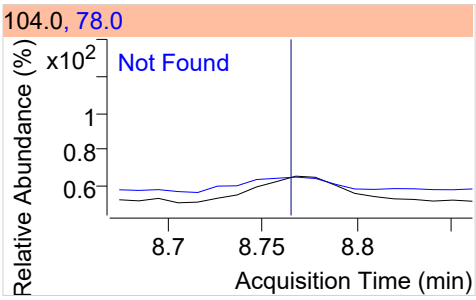

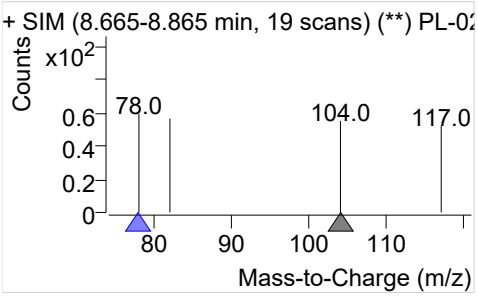

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\S.batch.bin		
Analysis Time	2026-01-08 오후 1:37:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:10:10	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 1:37:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-02 오후 4:33:47	**Data File**	JR(25-01-02).D
Type	Sample	**Name**	JR(25-01-02)
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

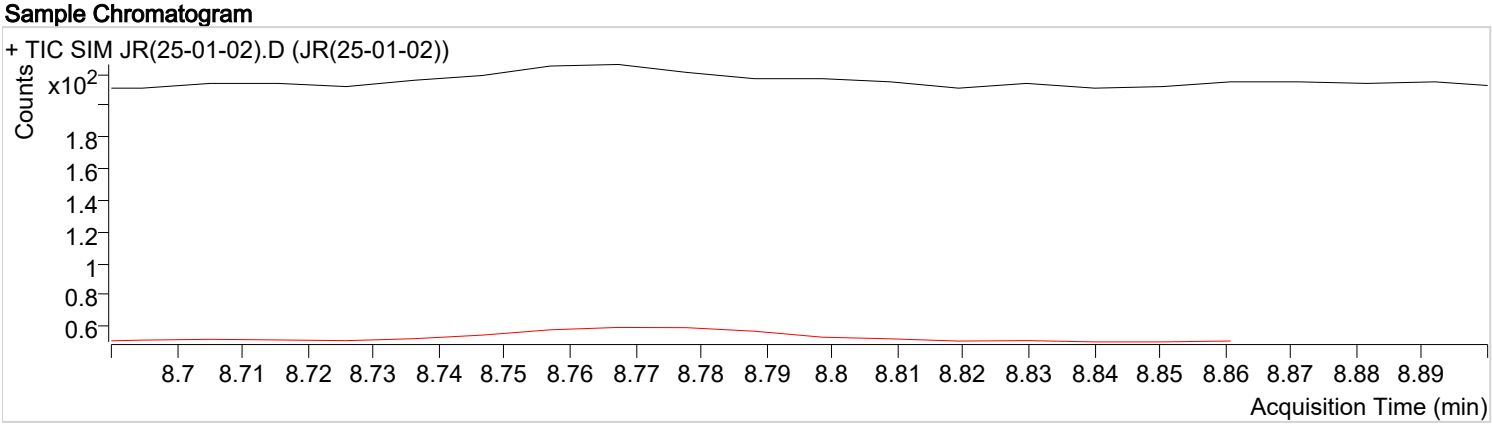

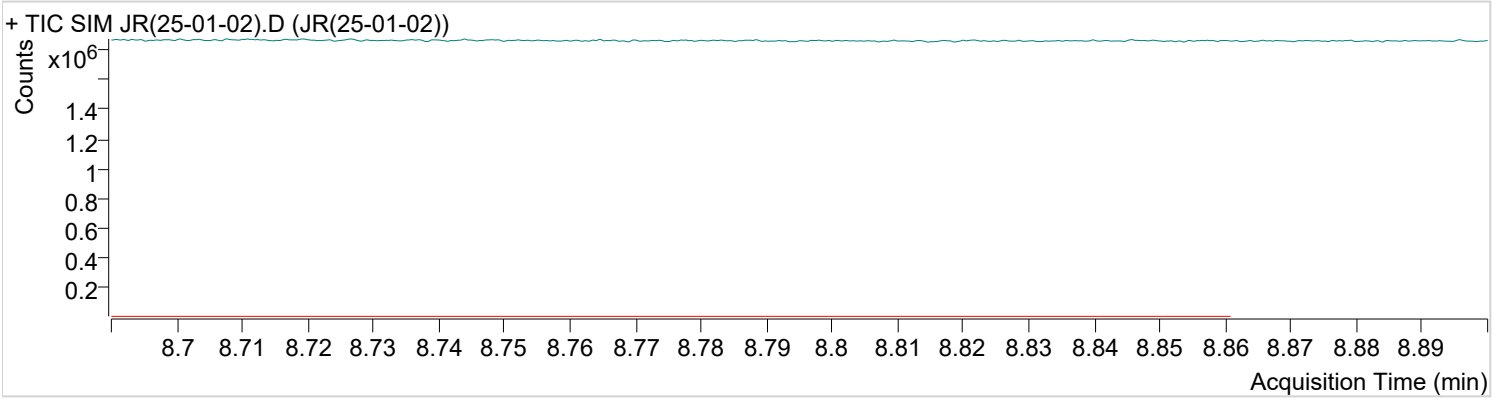

Styrene

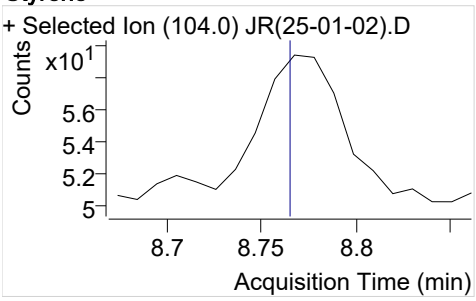

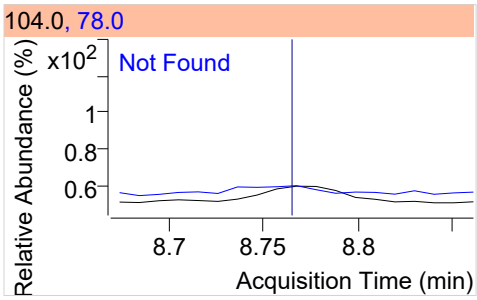

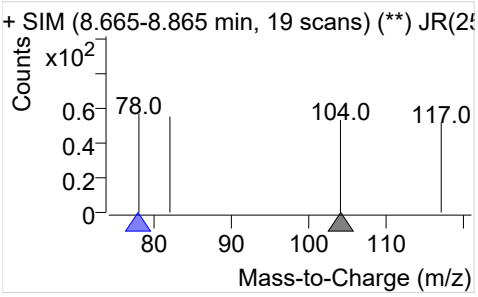

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\S.batch.bin		
Analysis Time	2026-01-08 오후 1:37:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:10:10	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 1:37:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-02 오후 4:51:35	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

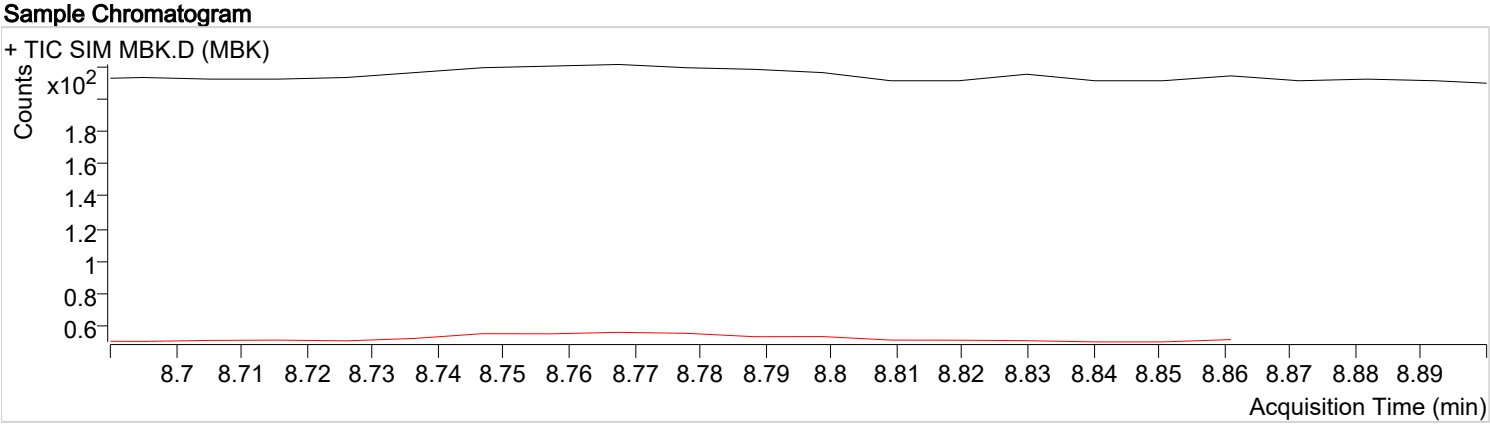

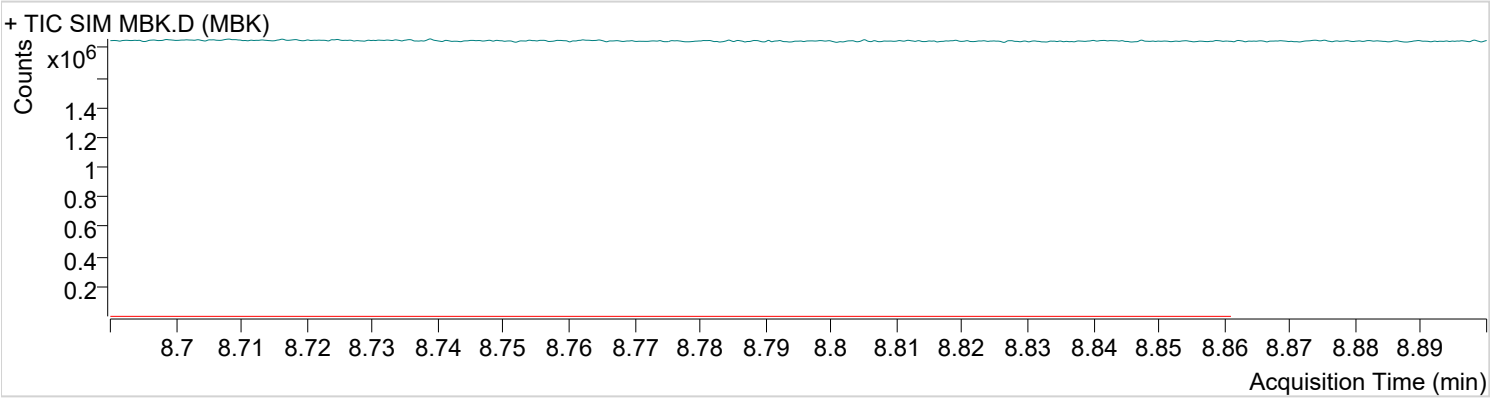

Styrene



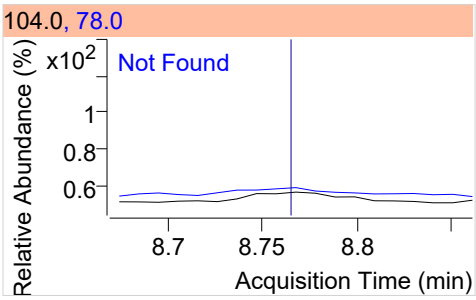

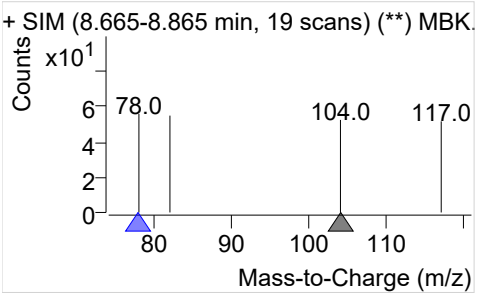

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(PL 12.30)\QuantResults\S.batch.bin		
Analysis Time	2026-01-08 오후 1:37:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:10:10	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오후 1:37:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-02 오후 6:02:34	**Data File**	CCV-(S).D
Type	QC	**Name**	CCV-(S)
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

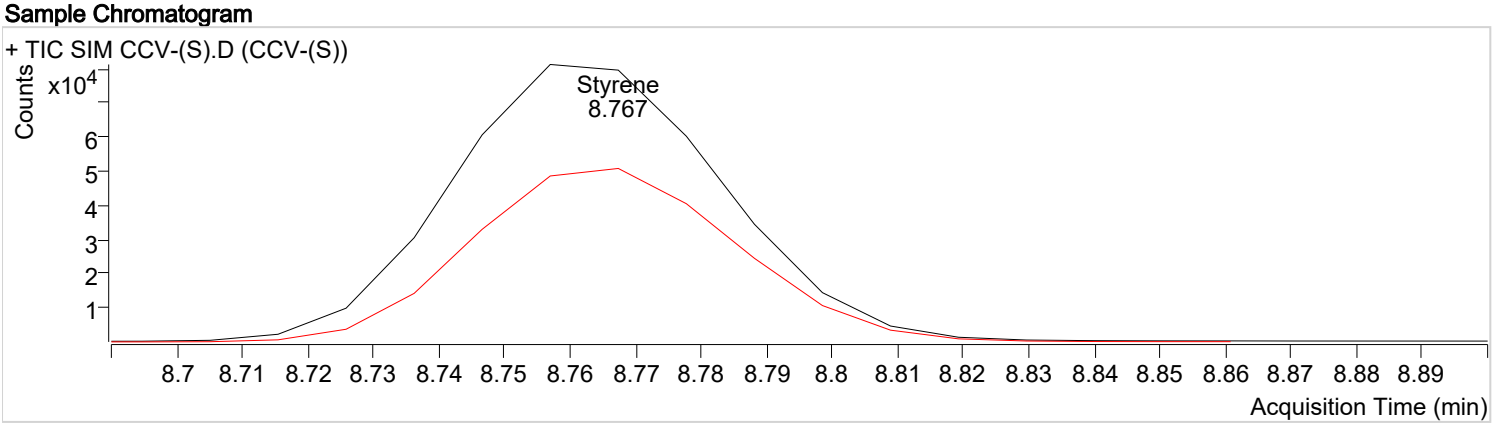

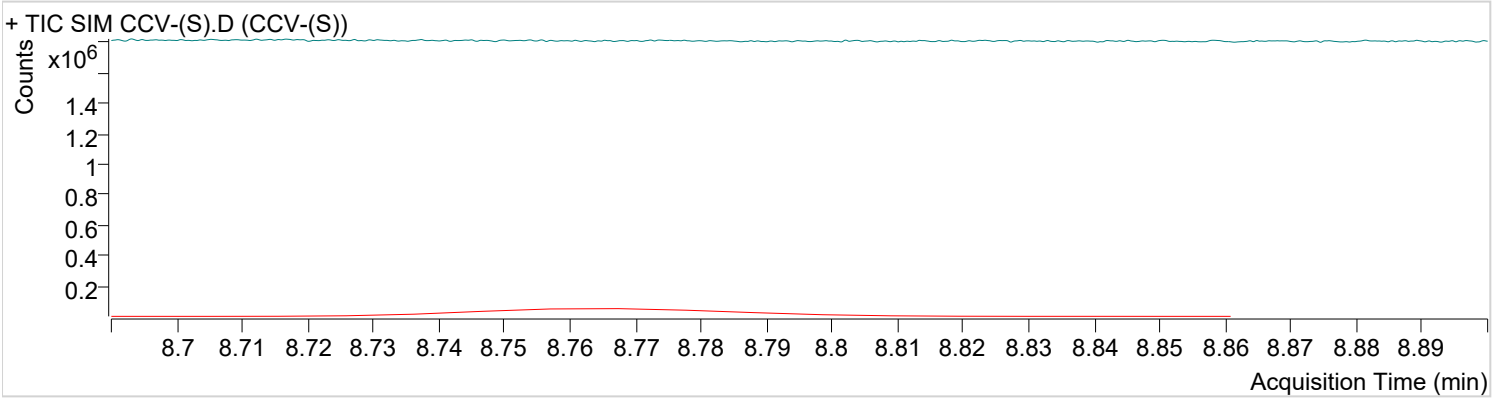

Name	RT	Resp.	Final Conc.	Units
Styrene	8.767	144055	0.206	mg/L

Styrene



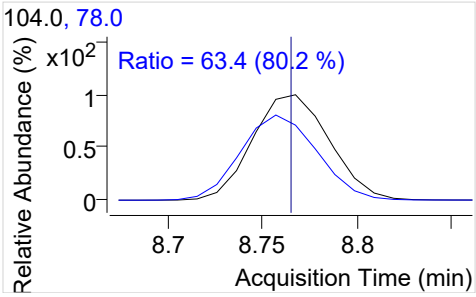

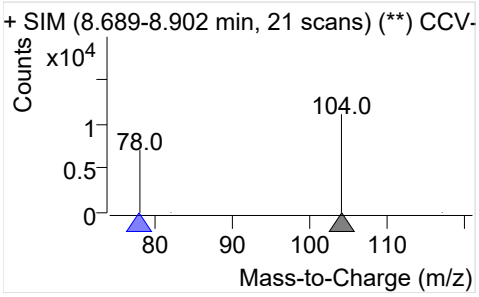

Generated at 오후 3:10 on 2026-04-10