Quantitative Analysis Results Summary Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(KD 1.15)\QuantResults\ST.batch.bin				
Analysis Time	2026-01-21 오후 4:57:44	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 4:57:44	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Styrene

Data File	Type	RT	Resp.	Final Conc.
Styrene ST-01.D	Cal	8.768	664	0.009
Styrene ST-02.D	Cal	8.768	12126	0.011
Styrene ST-03.D	Cal	8.768	135150	0.035
Styrene ST-04.D	Cal	8.768	1271941	0.259
Styrene ST-05.D	Cal	8.767	2481626	0.497
BK-.D	Blank			ND
FBK(KD 26-01-15).D	Blank			ND
KD-01.D	Sample			ND
JR 26-01-19.D	Sample	8.768	34183	0.015
MBK.D	Blank			ND
CCV S.D	QC	8.767	1197521	0.244

Styrene

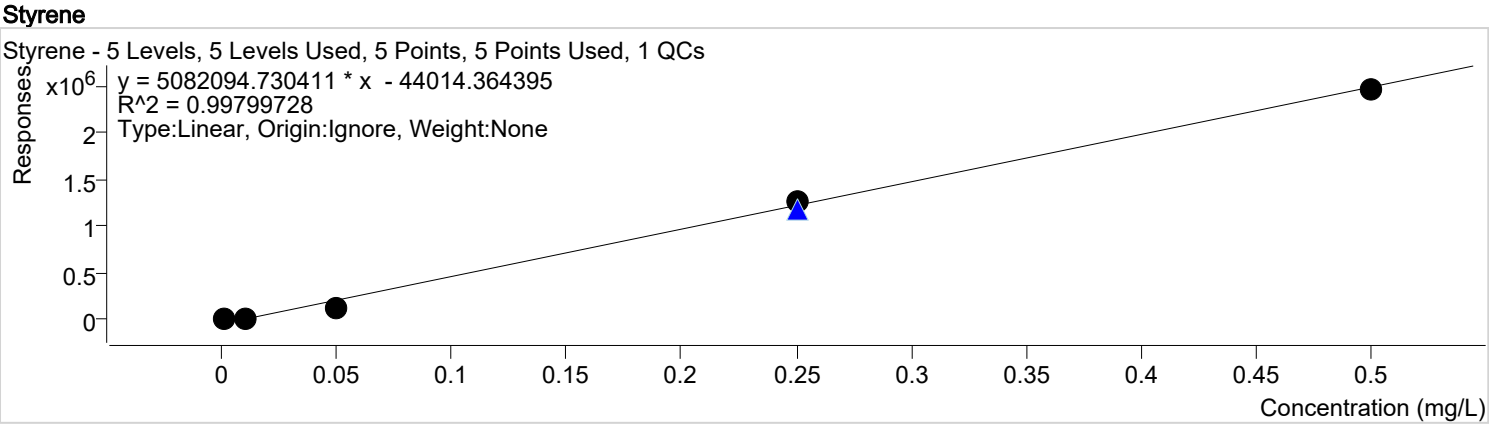

Cal. Path	Type	Level	Enable	Conc.	Response
D:\DATA\2026년\1. 2026년 1월\VOC2(KD 1.15)\Styrene ST-01.D	Calibration	1	x	0.001	664
D:\DATA\2026년\1. 2026년 1월\VOC2(KD 1.15)\Styrene ST-02.D	Calibration	2	x	0.010	12126
D:\DATA\2026년\1. 2026년 1월\VOC2(KD 1.15)\Styrene ST-03.D	Calibration	3	x	0.050	135150
D:\DATA\2026년\1. 2026년 1월\VOC2(KD 1.15)\Styrene ST-04.D	Calibration	4	x	0.250	1271941
D:\DATA\2026년\1. 2026년 1월\VOC2(KD 1.15)\CCV S.D	QC	4	x	0.250	1197521
D:\DATA\2026년\1. 2026년 1월\VOC2(KD 1.15)\Styrene ST-05.D	Calibration	5	x	0.500	2481626

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(KD 1.15)\QuantResults\ST.batch.bin		
Analysis Time	2026-01-21 오후 4:57:44	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:08:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 4:57:44	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-21 오전 11:46:47	**Data File**	Styrene ST-01.D
Type	Cal	**Name**	Styrene ST-01
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

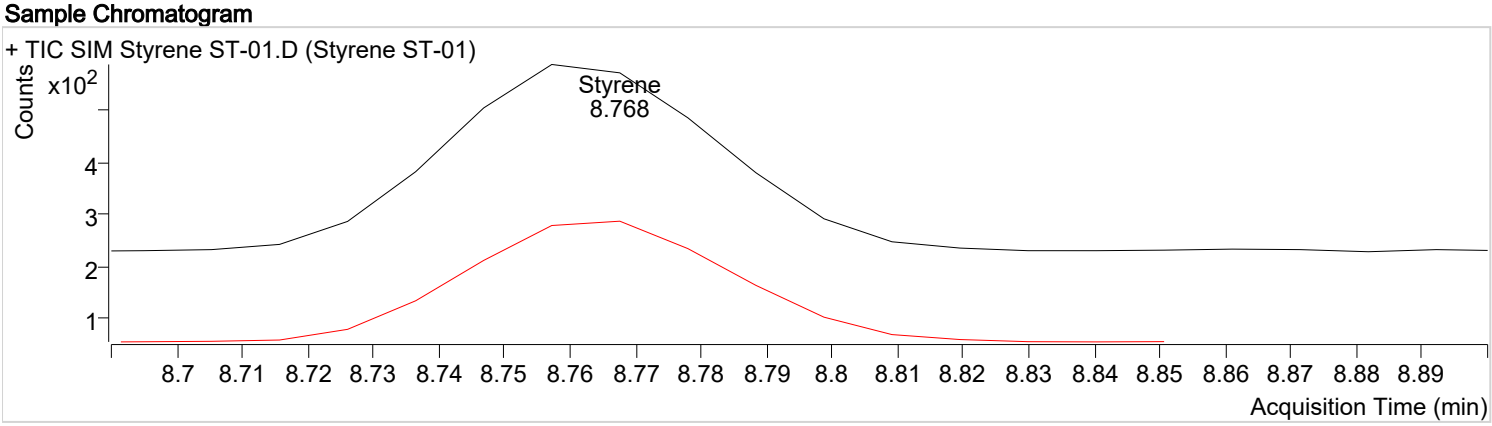

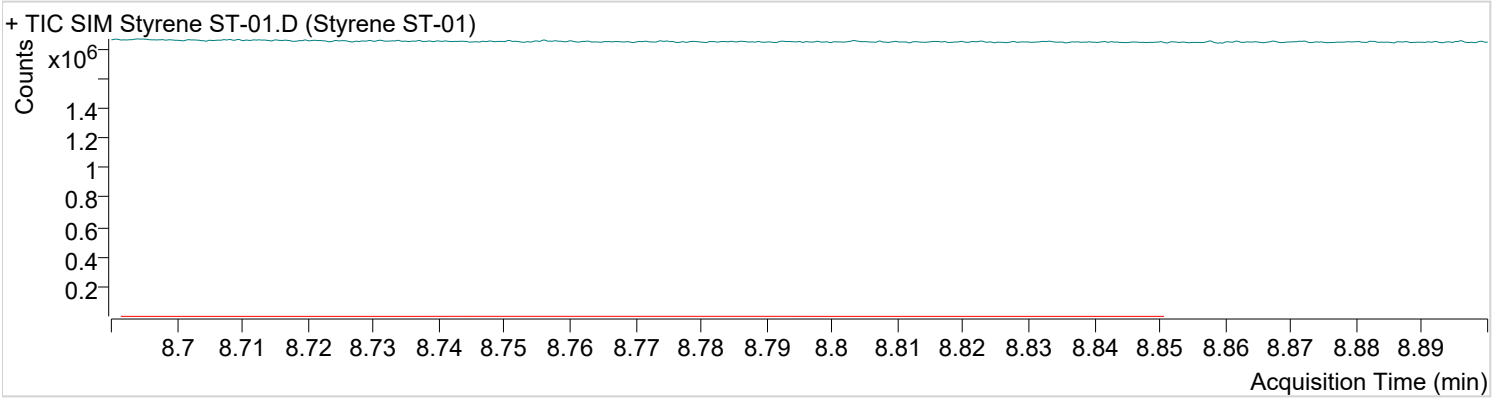

Name	RT	Resp.	Final Conc.	Units
Styrene	8.768	664	0.009	mg/L

Styrene

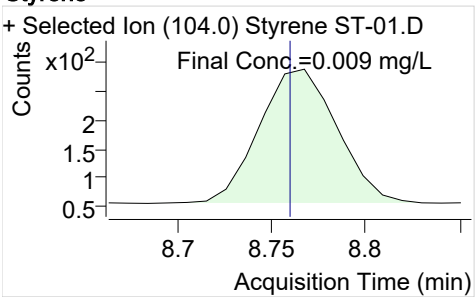

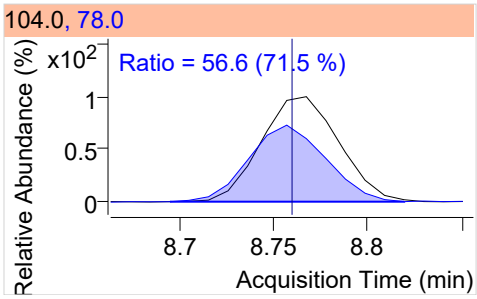

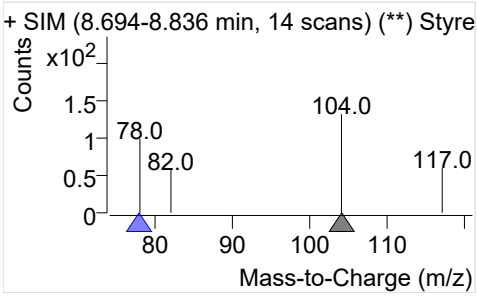

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(KD 1.15)\QuantResults\ST.batch.bin		
Analysis Time	2026-01-21 오후 4:57:44	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:08:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 4:57:44	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-21 오후 12:07:02	**Data File**	Styrene ST-02.D
Type	Cal	**Name**	Styrene ST-02
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

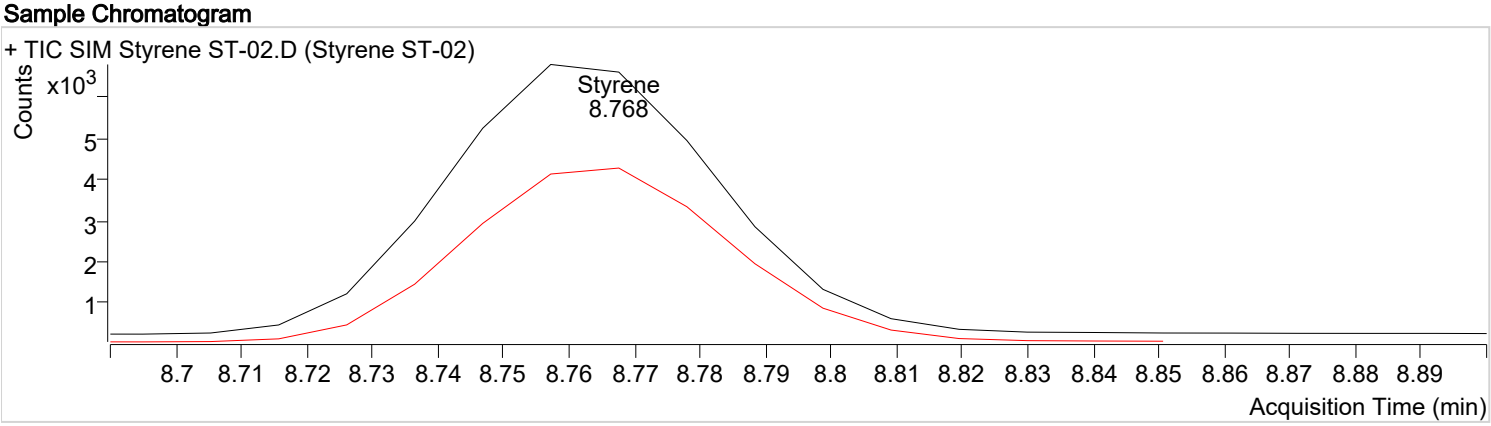

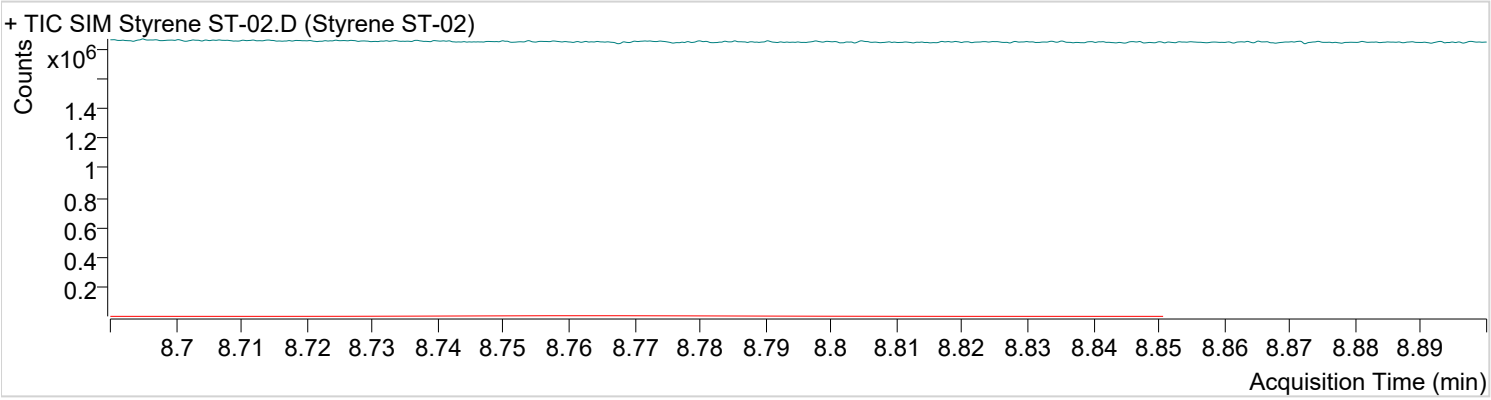

Name	RT	Resp.	Final Conc.	Units
Styrene	8.768	12126	0.011	mg/L

Styrene

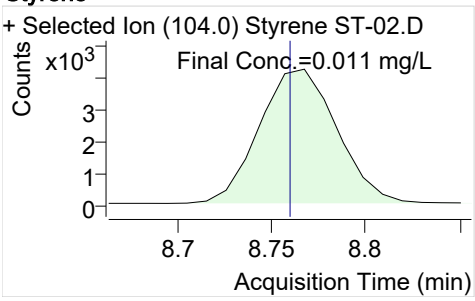

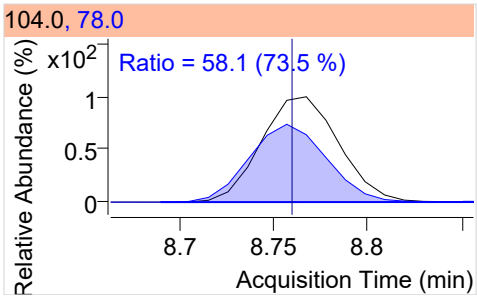

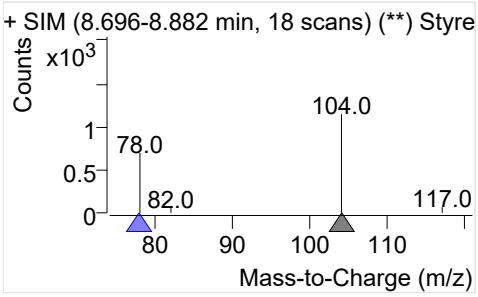

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(KD 1.15)\QuantResults\ST.batch.bin		
Analysis Time	2026-01-21 오후 4:57:44	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:08:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 4:57:44	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-21 오후 12:27:20	**Data File**	Styrene ST-03.D
Type	Cal	**Name**	Styrene ST-03
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

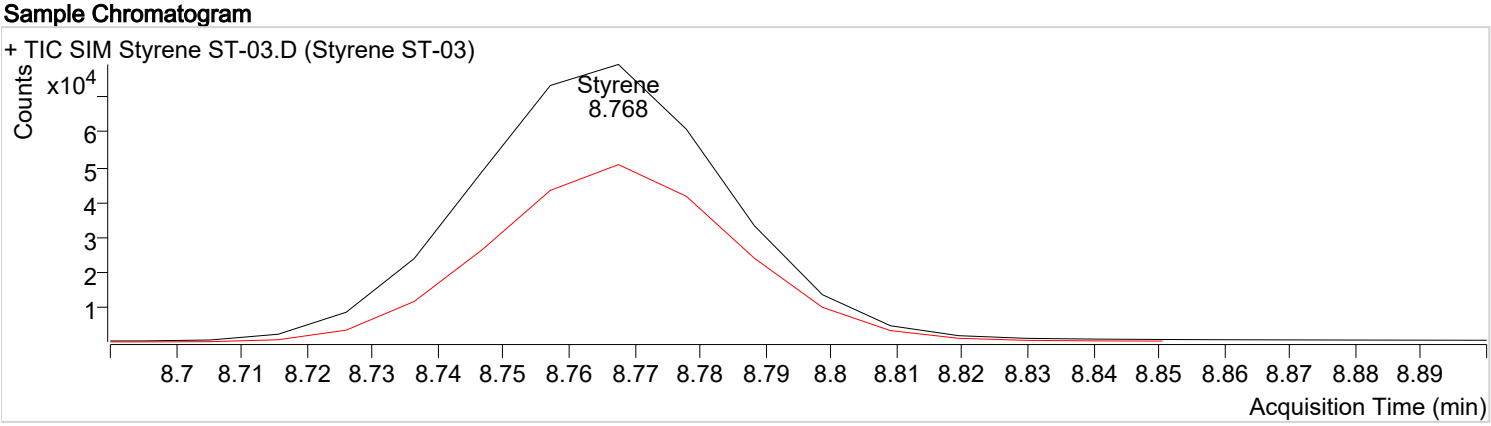

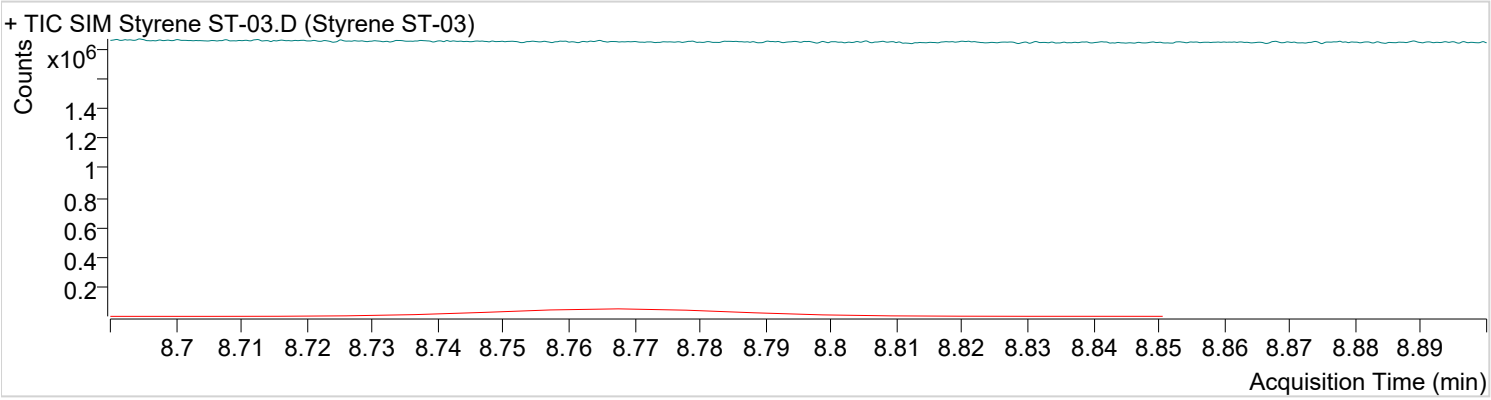

Name	RT	Resp.	Final Conc.	Units
Styrene	8.768	135150	0.035	mg/L

Styrene

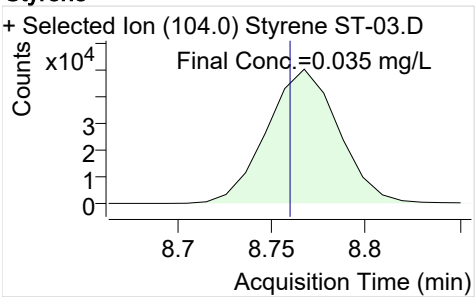

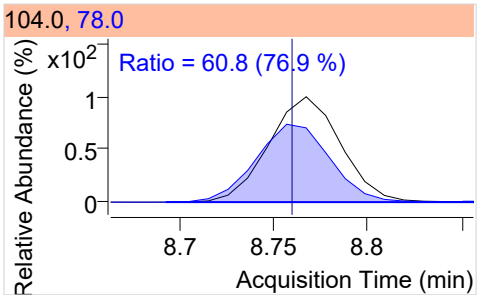

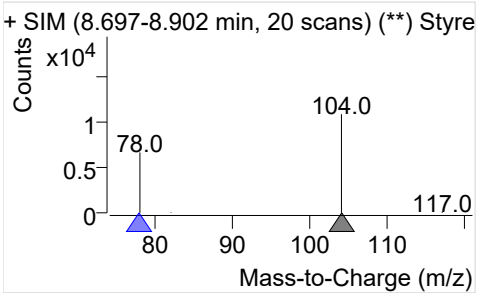

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(KD 1.15)\QuantResults\ST.batch.bin		
Analysis Time	2026-01-21 오후 4:57:44	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:08:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 4:57:44	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-21 오후 12:47:39	**Data File**	Styrene ST-04.D
Type	Cal	**Name**	Styrene ST-04
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

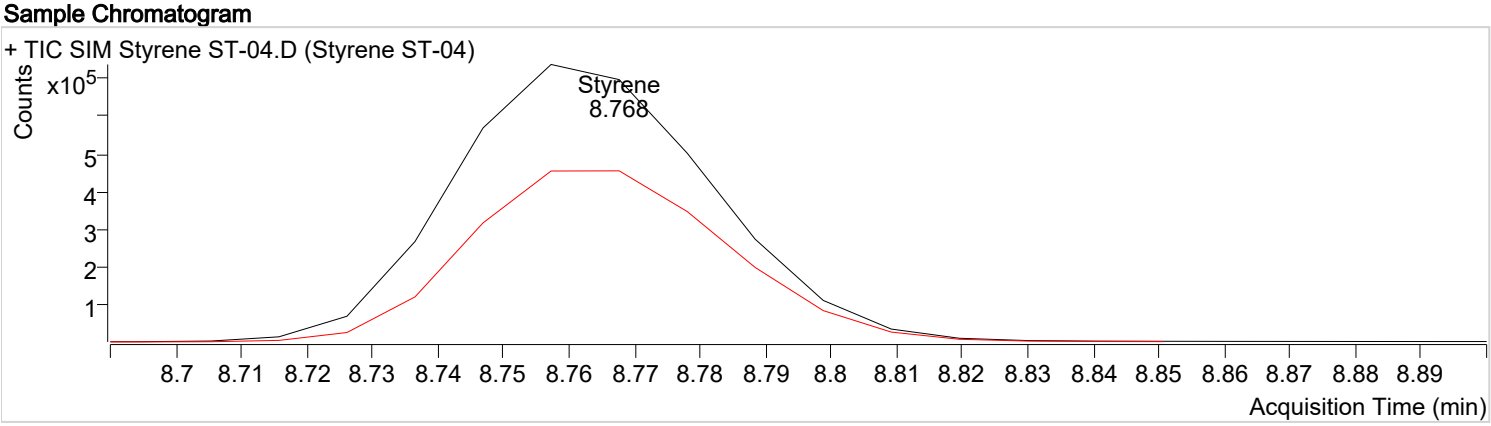

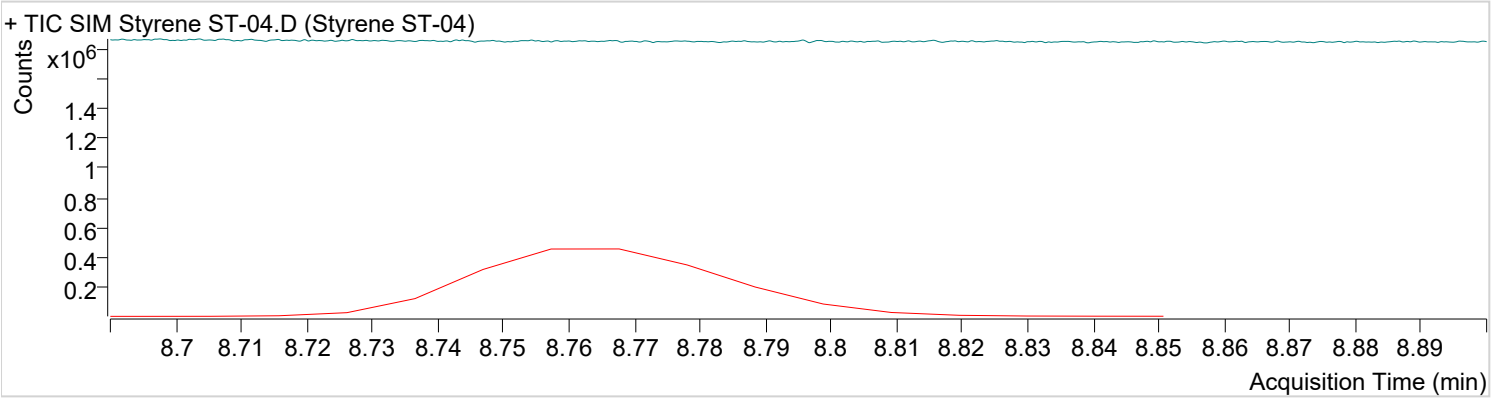

Name	RT	Resp.	Final Conc.	Units
Styrene	8.768	1271941	0.259	mg/L

Styrene

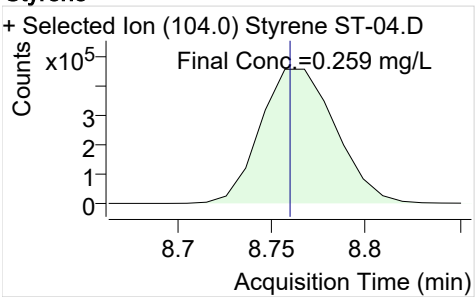

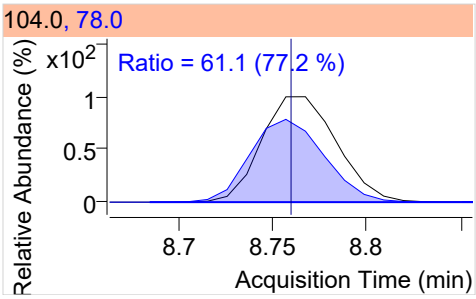

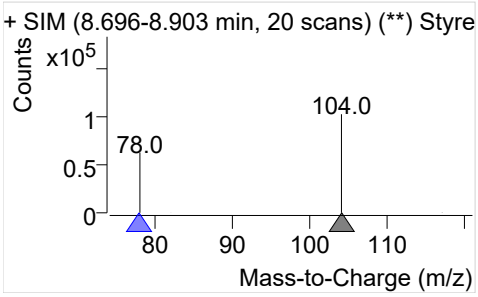

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(KD 1.15)\QuantResults\ST.batch.bin		
Analysis Time	2026-01-21 오후 4:57:44	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:08:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 4:57:44	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-21 오후 1:07:55	**Data File**	Styrene ST-05.D
Type	Cal	**Name**	Styrene ST-05
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

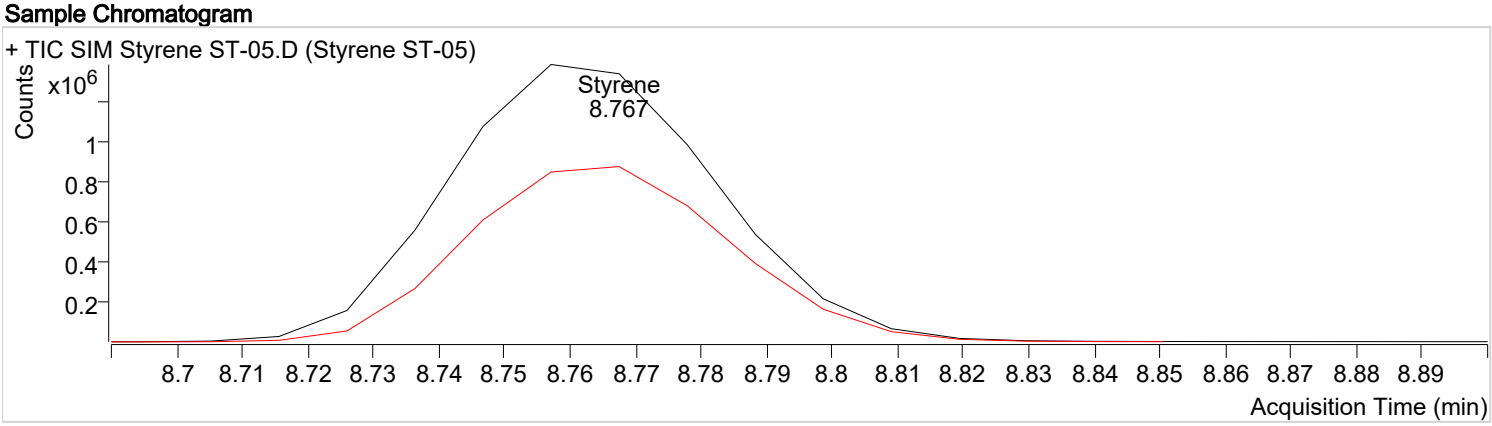

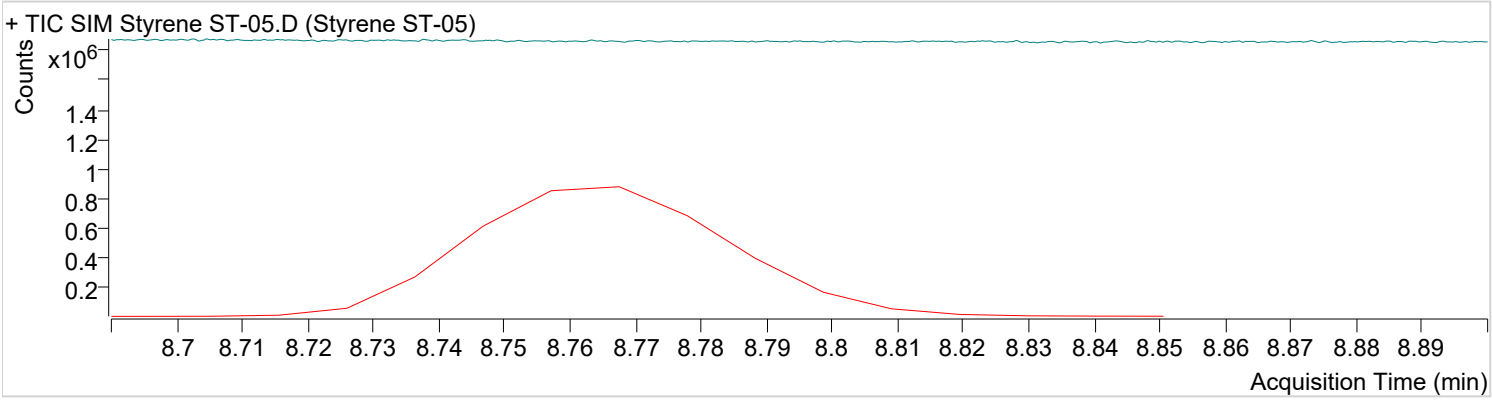

Name	RT	Resp.	Final Conc.	Units
Styrene	8.767	2481626	0.497	mg/L

Styrene

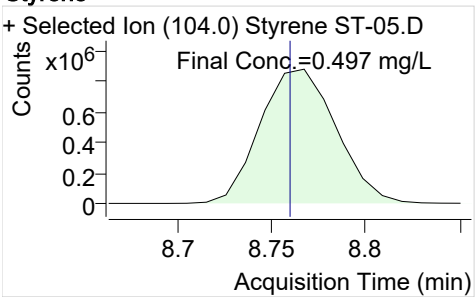

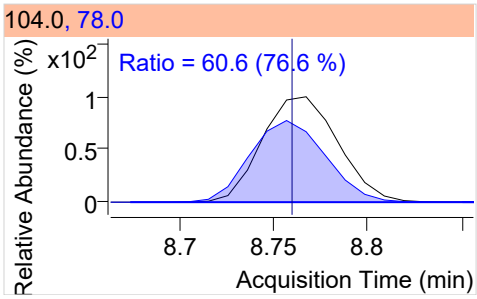

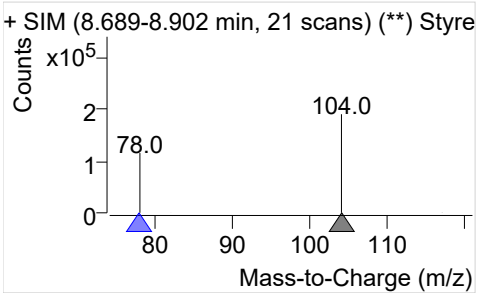

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(KD 1.15)\QuantResults\ST.batch.bin		
Analysis Time	2026-01-21 오후 4:57:44	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:08:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 4:57:44	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-21 오후 1:48:34	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

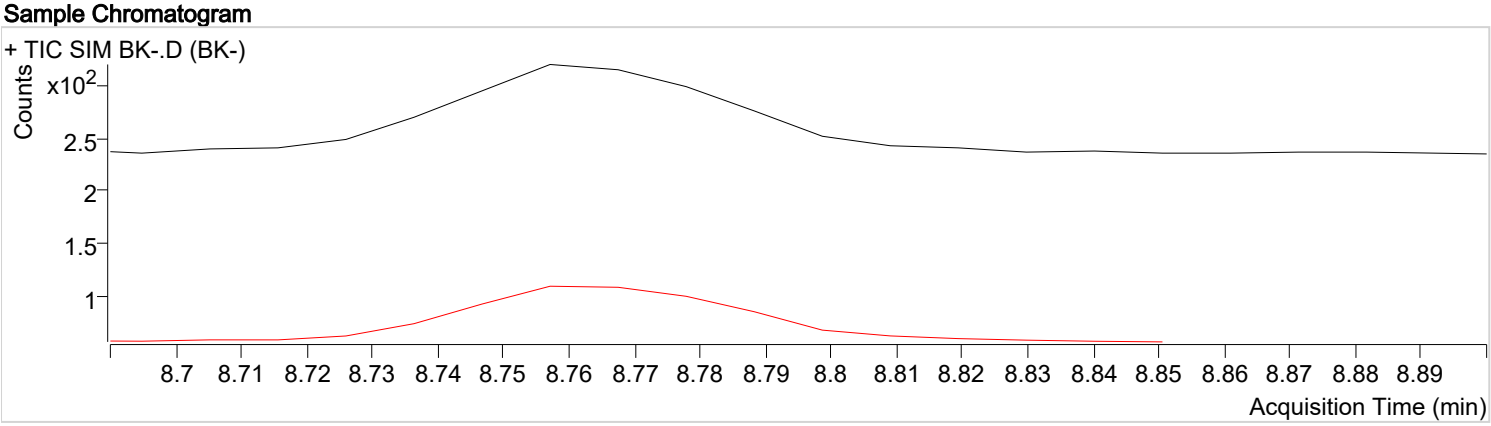

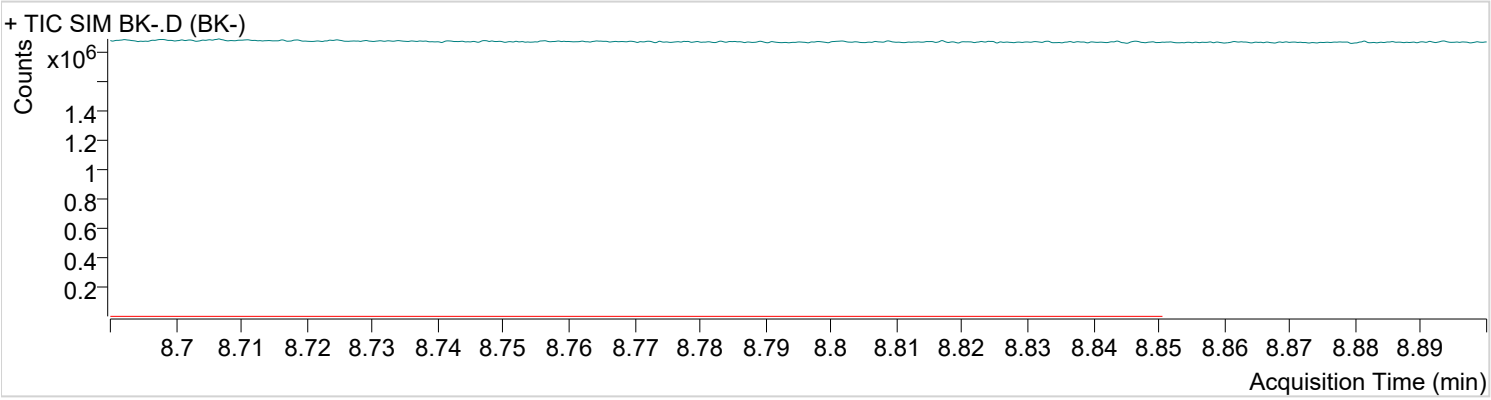

Styrene

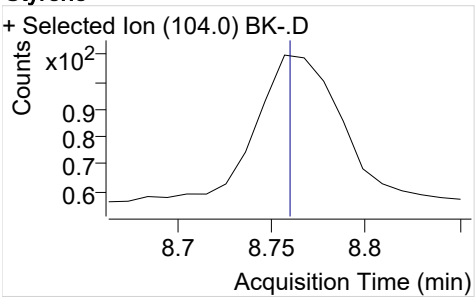

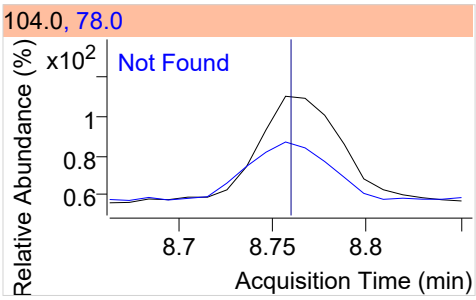

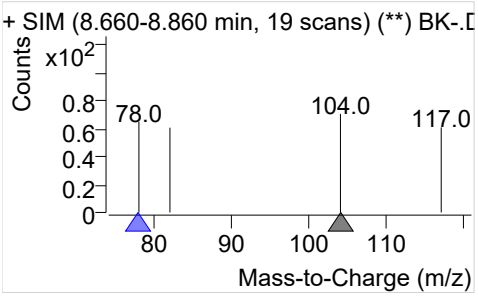

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(KD 1.15)\QuantResults\ST.batch.bin		
Analysis Time	2026-01-21 오후 4:57:44	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:08:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 4:57:44	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-21 오후 2:08:51	**Data File**	FBK(KD 26-01-15).D
Type	Blank	**Name**	FBK(KD 26-01-15)
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

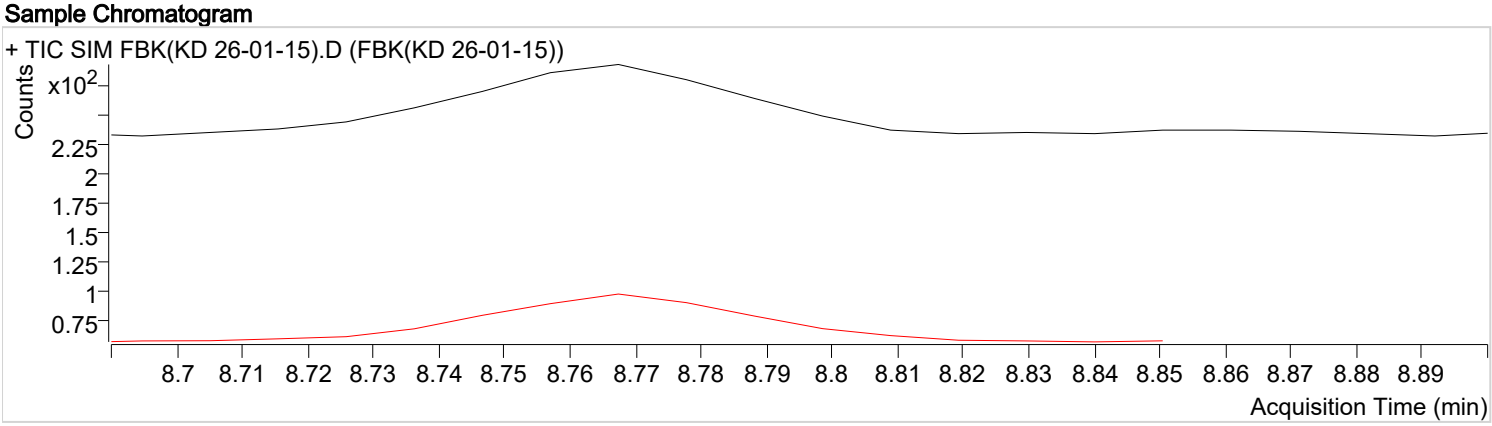

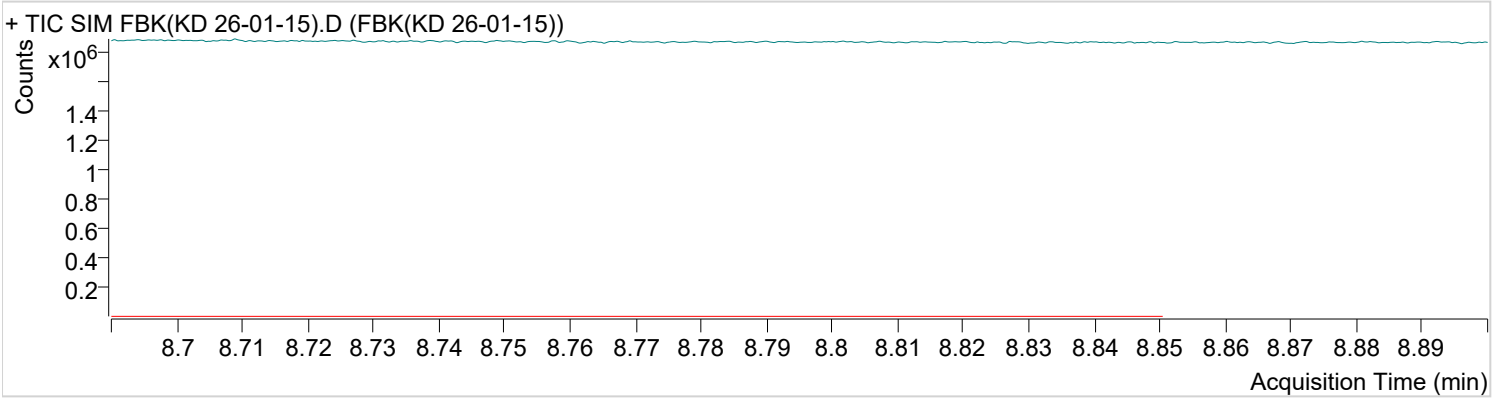

Styrene

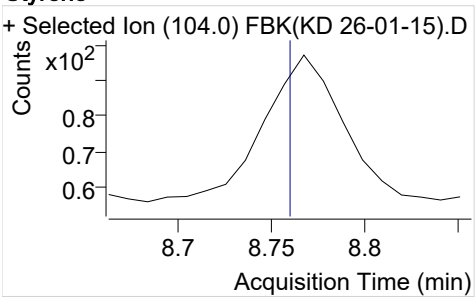

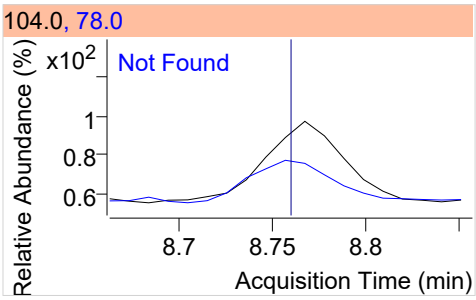

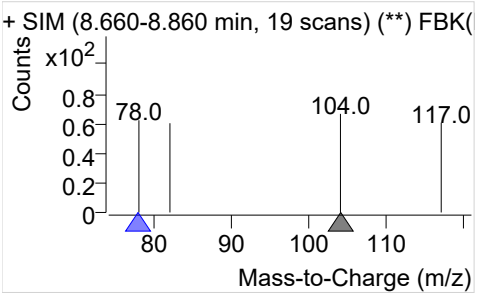

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(KD 1.15)\QuantResults\ST.batch.bin		
Analysis Time	2026-01-21 오후 4:57:44	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:08:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 4:57:44	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-21 오후 2:29:06	**Data File**	KD-01.D
Type	Sample	**Name**	KD-01
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

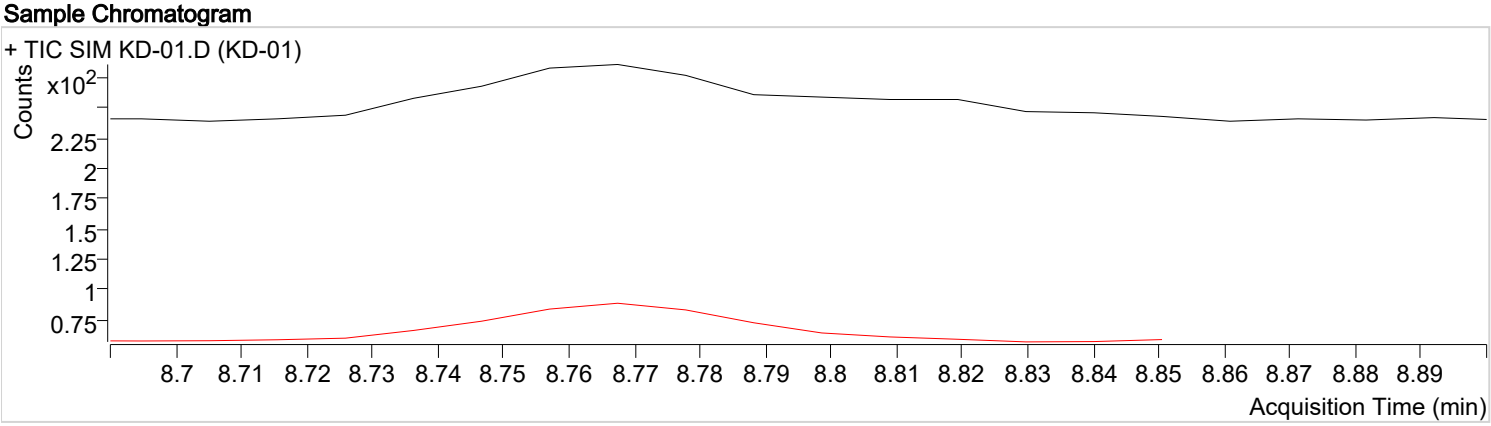

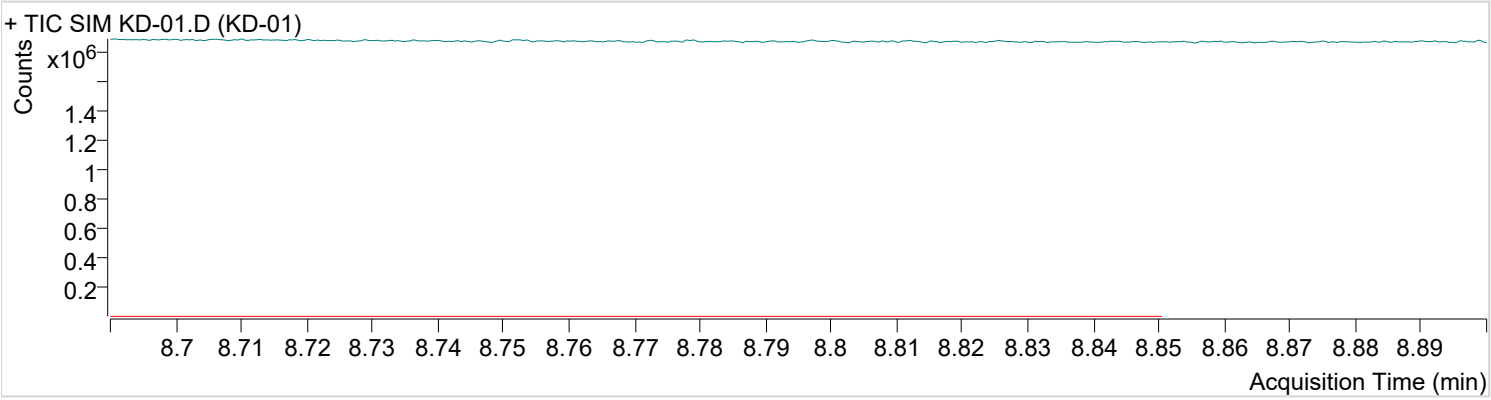

Styrene

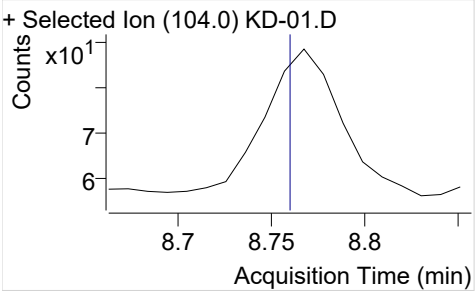

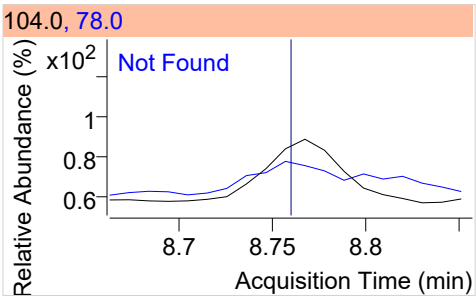

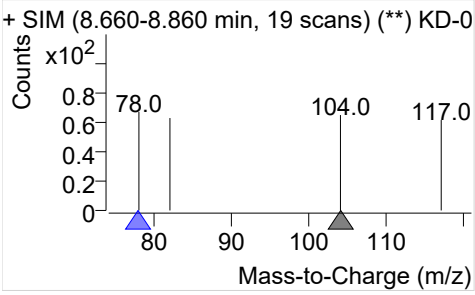

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(KD 1.15)\QuantResults\ST.batch.bin		
Analysis Time	2026-01-21 오후 4:57:44	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:08:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 4:57:44	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-21 오후 2:49:22	**Data File**	JR 26-01-19.D
Type	Sample	**Name**	JR 26-01-19
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

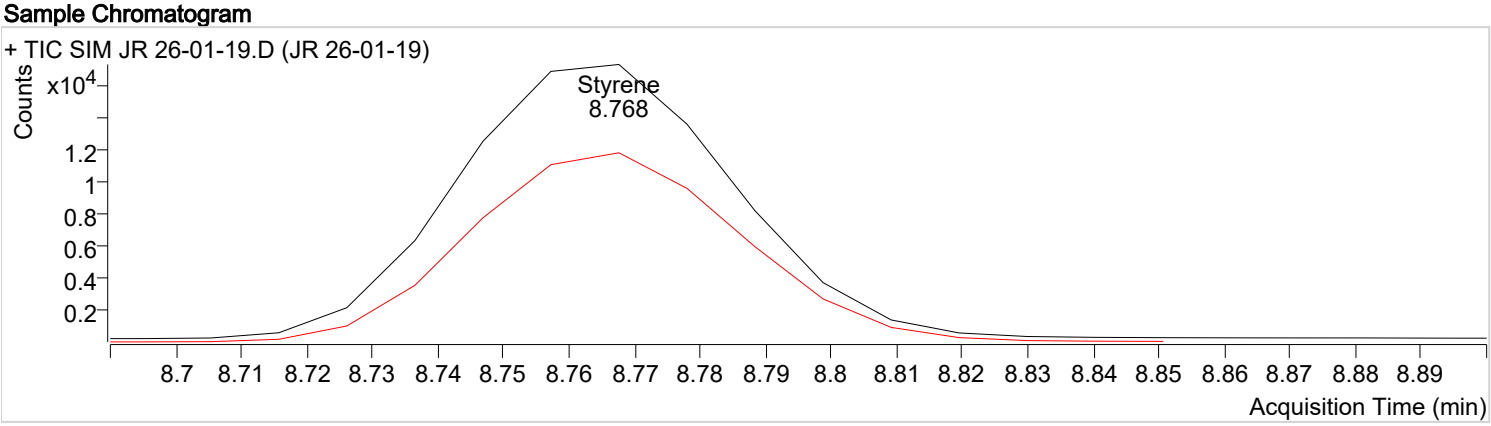

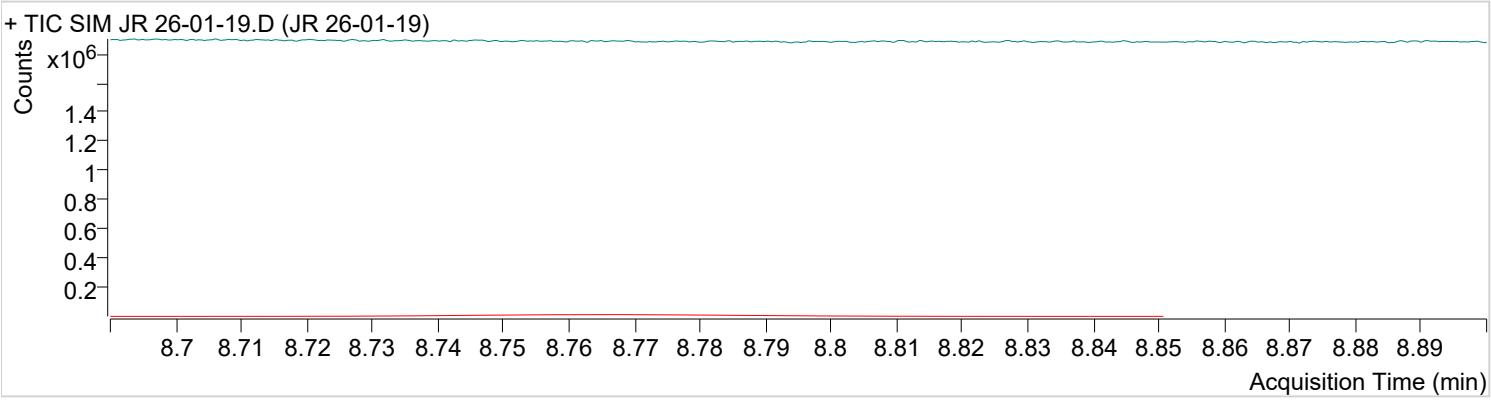

Name	RT	Resp.	Final Conc.	Units
Styrene	8.768	34183	0.015	mg/L

Styrene

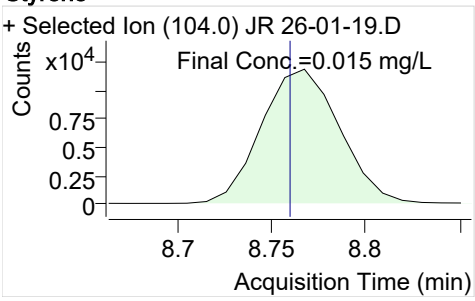

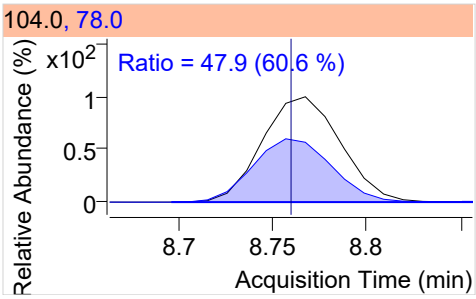

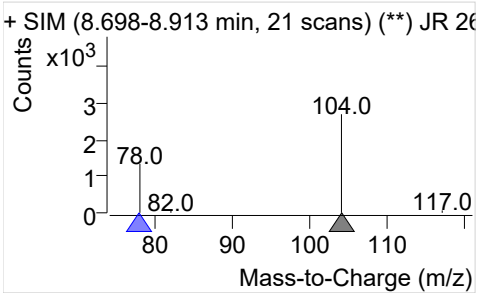

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(KD 1.15)\QuantResults\ST.batch.bin		
Analysis Time	2026-01-21 오후 4:57:44	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:08:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 4:57:44	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-21 오후 3:09:40	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

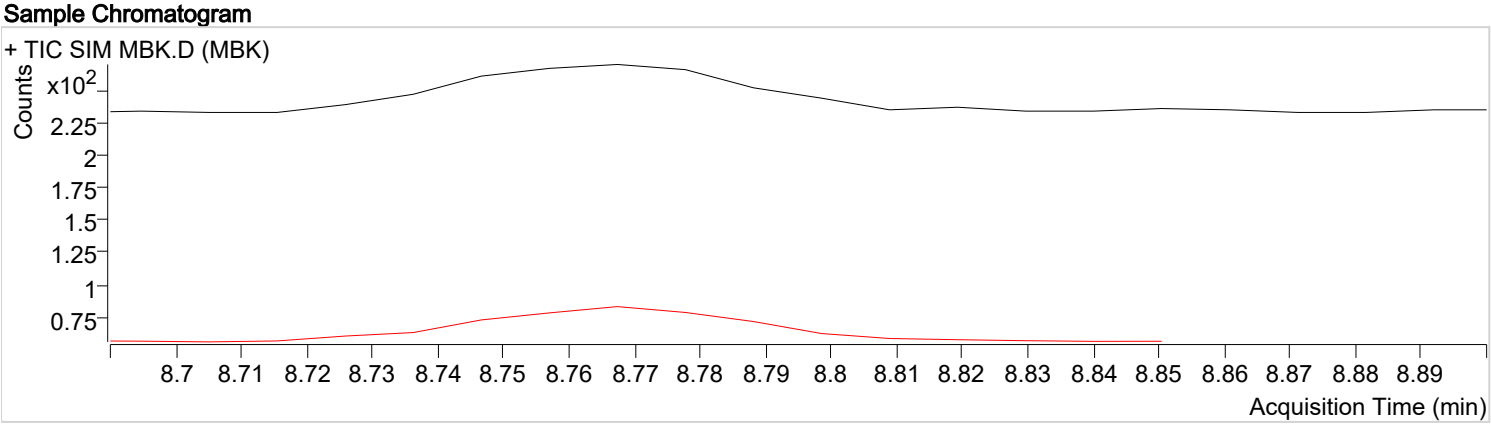

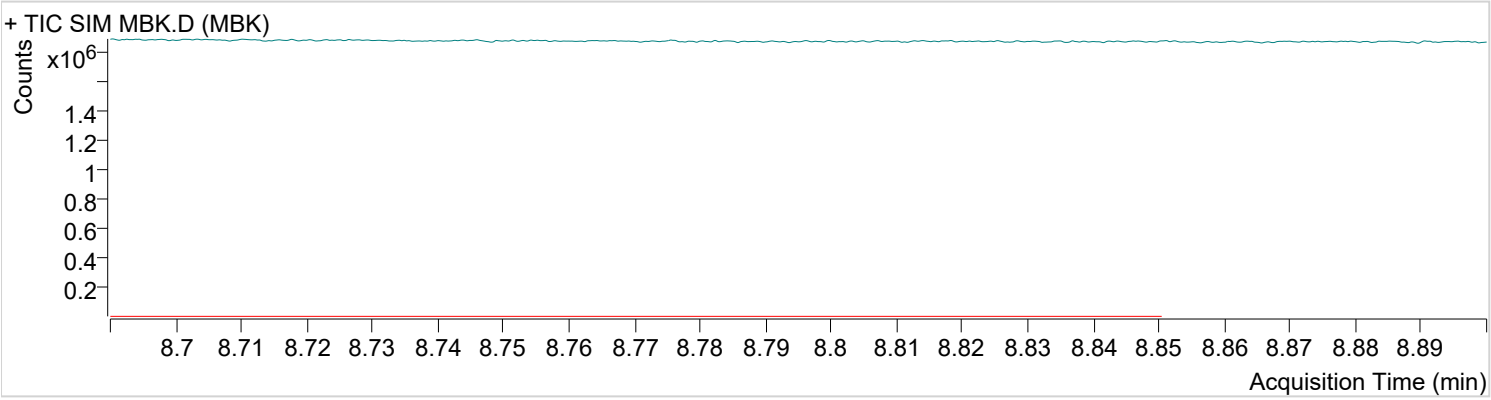

Styrene

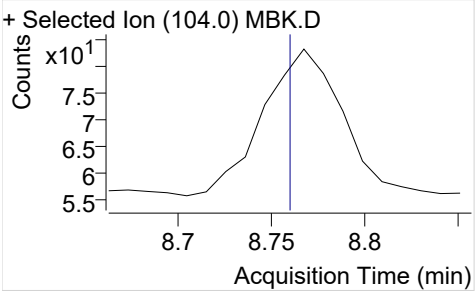

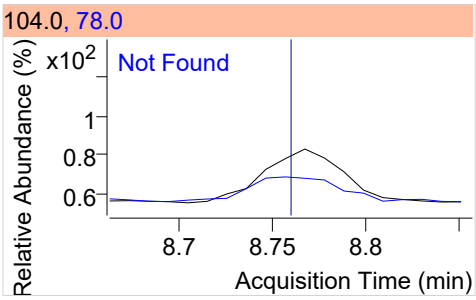

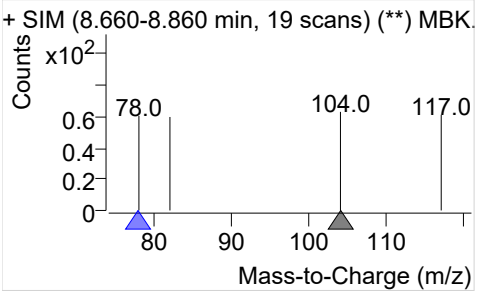

Quant Sample Report

Batch Data Path	D:\DATA\2026년\1. 2026년 1월\VOC2(KD 1.15)\QuantResults\ST.batch.bin		
Analysis Time	2026-01-21 오후 4:57:44	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:08:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 4:57:44	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-01-21 오후 4:10:27	**Data File**	CCV S.D
Type	QC	**Name**	CCV S
Dil.	1	**Acq. Method File**	VOCs(2) NEW

Sample Chromatogram

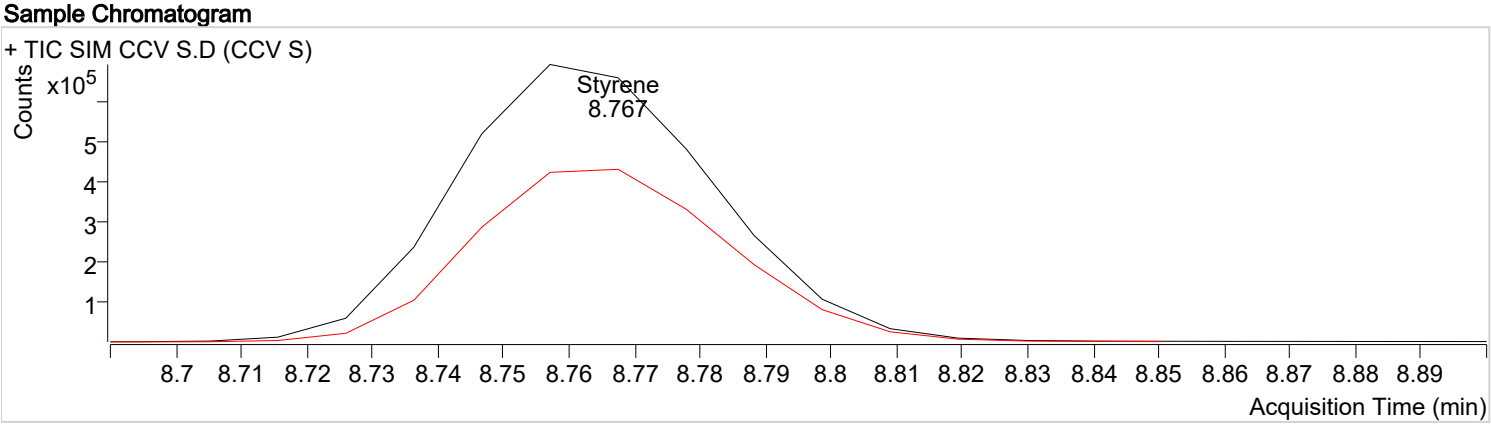

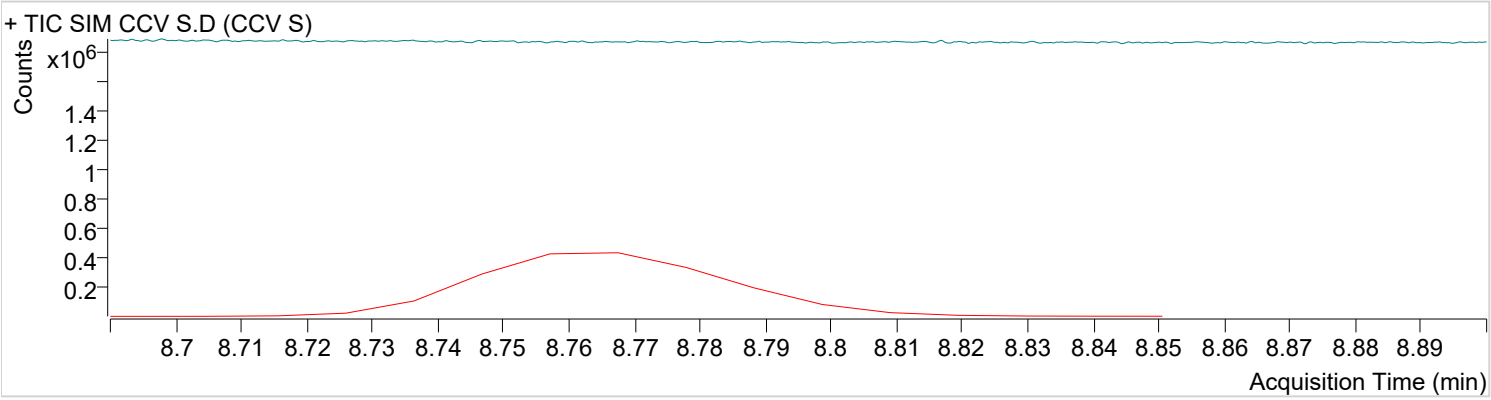

Name	RT	Resp.	Final Conc.	Units
Styrene	8.767	1197521	0.244	mg/L
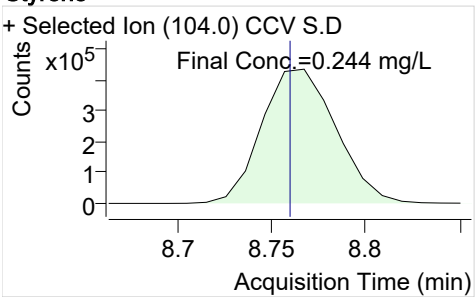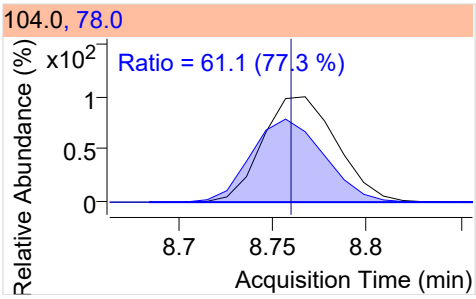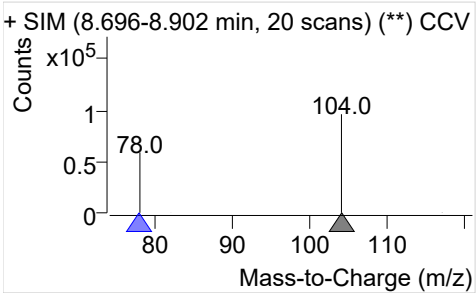
Styrene