Quantitative Analysis Results Summary Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin				
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Styrene

Data File	Type	RT	Resp.	Final Conc.
STY ST-01.d	Cal	4.611	2014	0.000
STY ST-02.d	Cal	4.600	29921	0.003
STY ST-03.d	Cal	4.592	198512	0.052
STY ST-04.d	Cal	4.589	959833	0.271
STY ST-05.d	Cal	4.585	1716361	0.489
BK-.d	Blank			ND
FBK(GS 26-02-10).d	Blank			ND
KH (26-02-10).d	Blank			ND
GS-01.d	Sample	4.636	0	ND
GS-02.d	Sample	4.633	0	ND
GS-03.d	Sample			ND
GS-04.d	Sample	4.629	0	ND
GS-05.d	Sample			ND
GS-06.d	Sample			ND
GS-15.d	Sample			ND
MBK-1.d	Blank			ND
CCV S.d	QC	4.592	887056	0.250
SOL 1.d	Sample			ND
SOL 2.d	Sample			ND
SOL 3.d	Sample			ND

Styrene

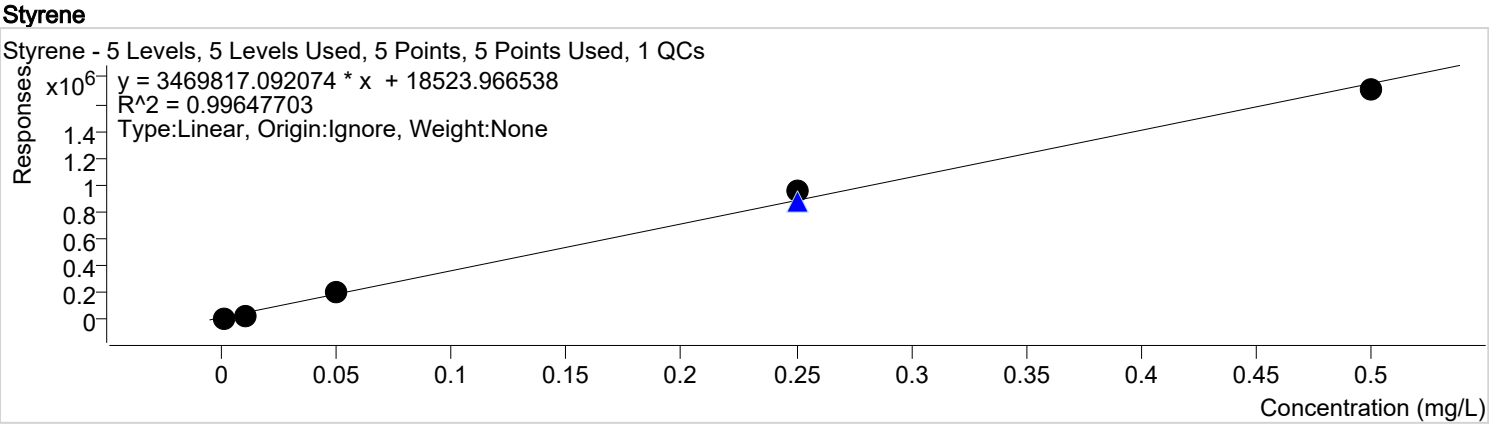

Cal. Path	Type	Level	Enable	Conc.	Response
V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\STY ST-01.d	Calibration	1	x	0.001	2014
V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\STY ST-02.d	Calibration	2	x	0.010	29921
V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\STY ST-03.d	Calibration	3	x	0.050	198512
V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\STY ST-04.d	Calibration	4	x	0.250	959833
V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\CCV S.d	QC	4	x	0.250	887056
V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\STY ST-05.d	Calibration	5	x	0.500	1716361

Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오전 11:50:12	**Data File**	STY ST-01.d
Type	Cal	**Name**	STY ST-01
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

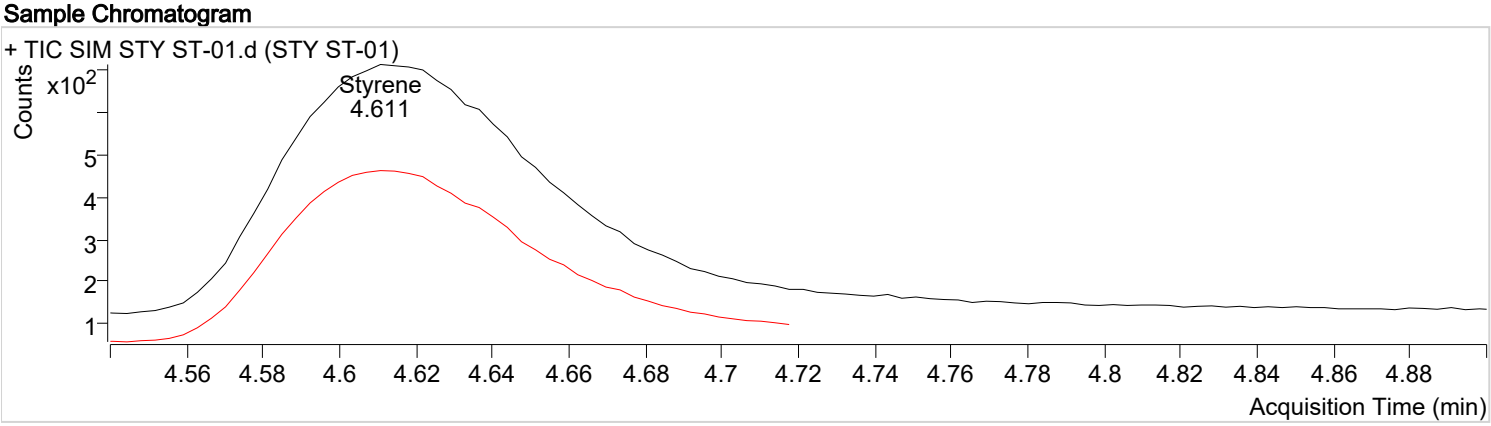

Name	RT	Resp.	Final Conc.	Units
Styrene	4.611	2014	0.000	mg/L

Styrene

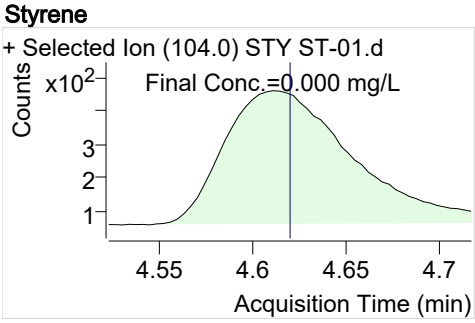



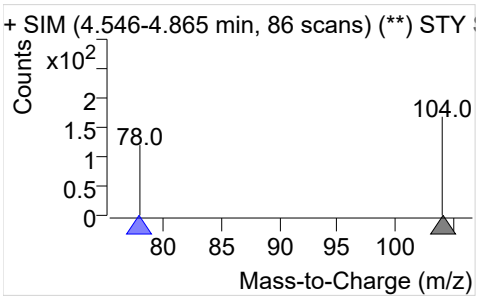

Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 12:07:19	**Data File**	STY ST-02.d
Type	Cal	**Name**	STY ST-02
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

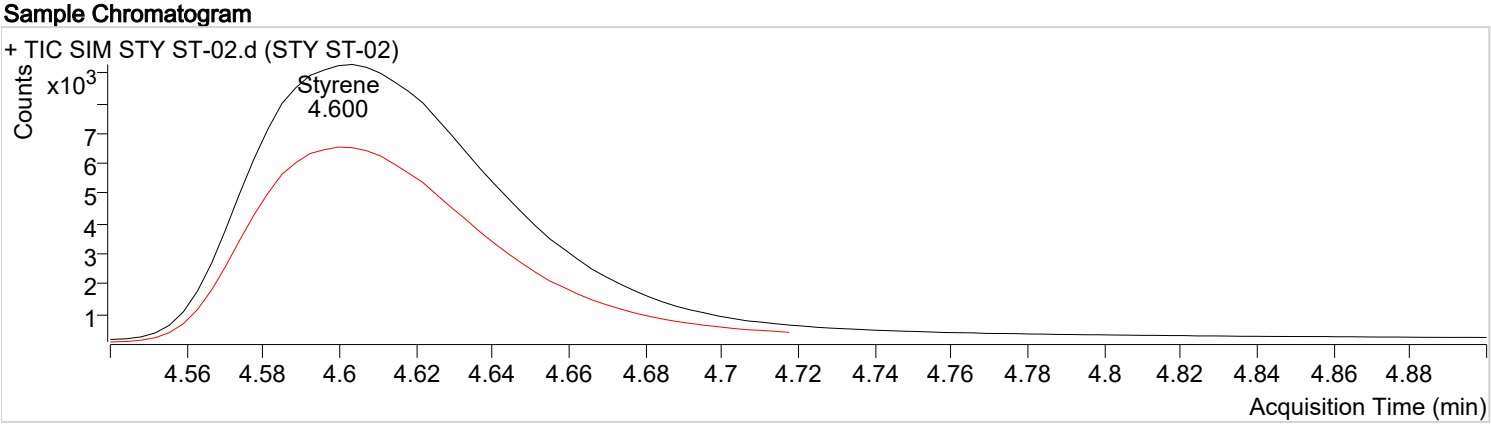

Name	RT	Resp.	Final Conc.	Units
Styrene	4.600	29921	0.003	mg/L

Styrene

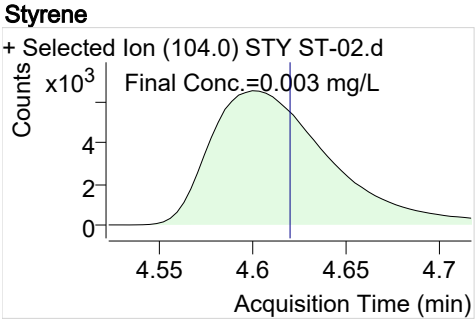



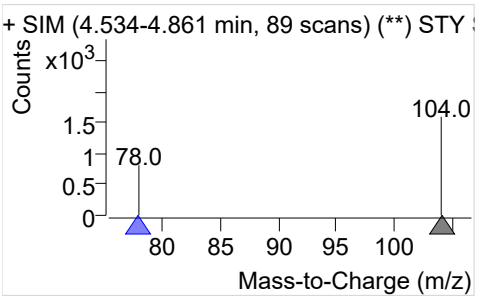

Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 12:24:21	**Data File**	STY ST-03.d
Type	Cal	**Name**	STY ST-03
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

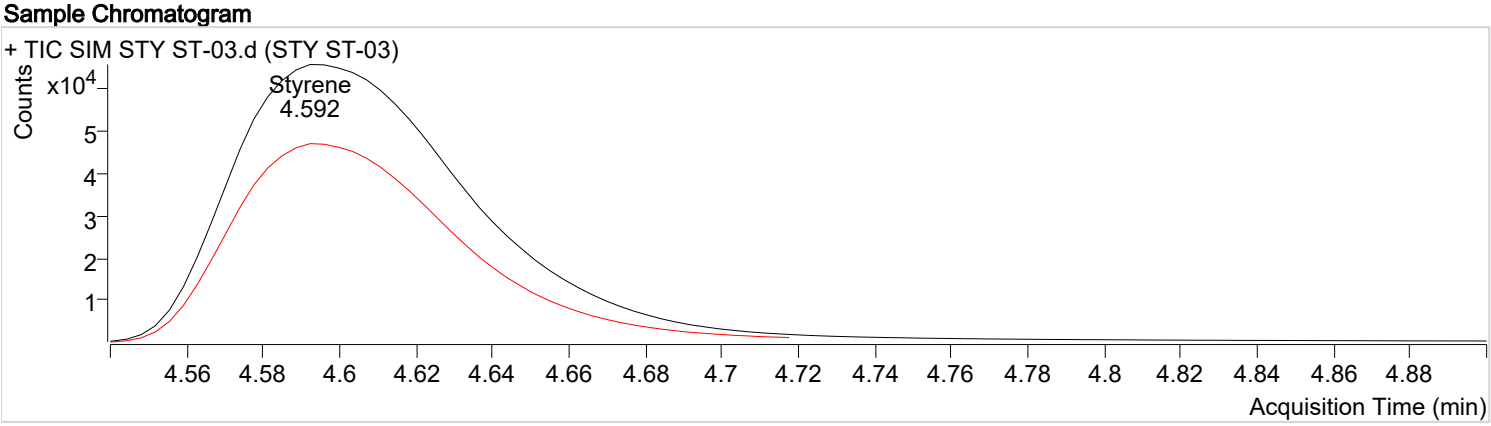

Name	RT	Resp.	Final Conc.	Units
Styrene	4.592	198512	0.052	mg/L

Styrene

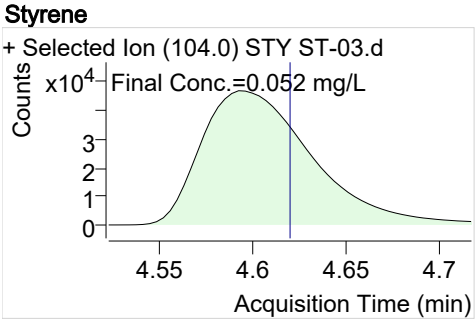



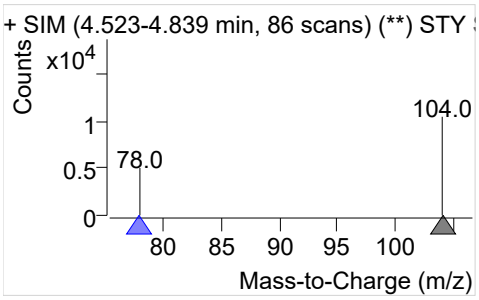

Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 12:41:27	**Data File**	STY ST-04.d
Type	Cal	**Name**	STY ST-04
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

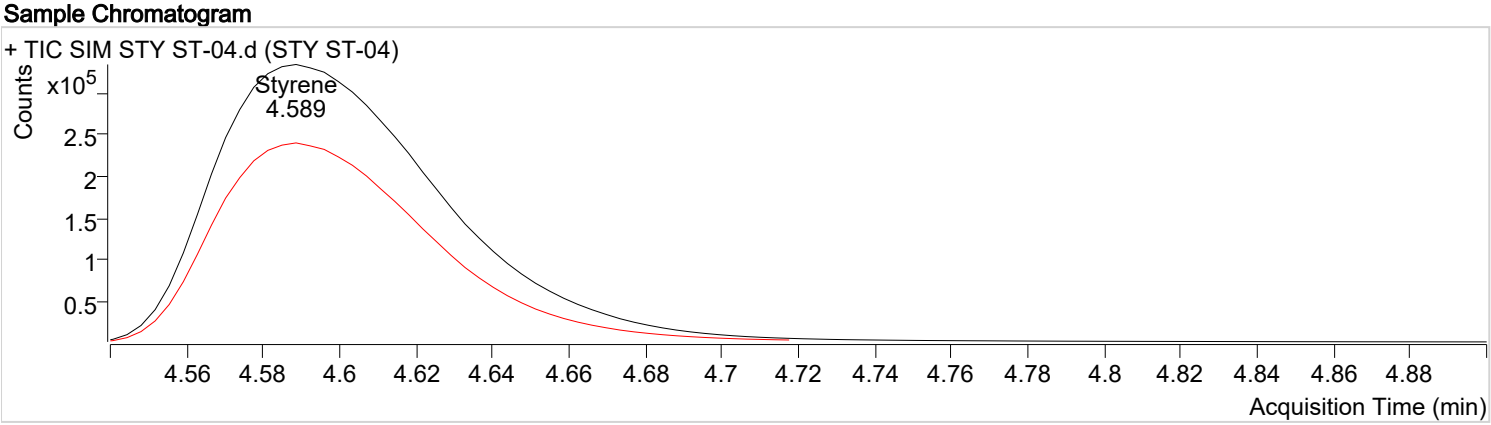

Name	RT	Resp.	Final Conc.	Units
Styrene	4.589	959833	0.271	mg/L

Styrene

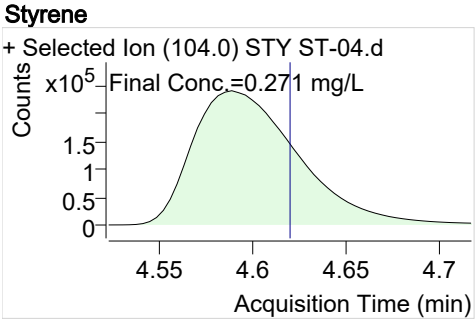

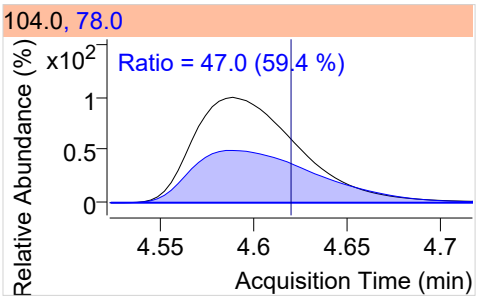

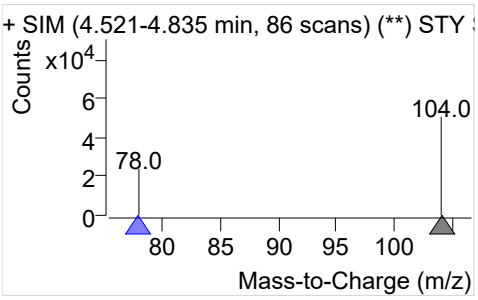

Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 12:58:39	**Data File**	STY ST-05.d
Type	Cal	**Name**	STY ST-05
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

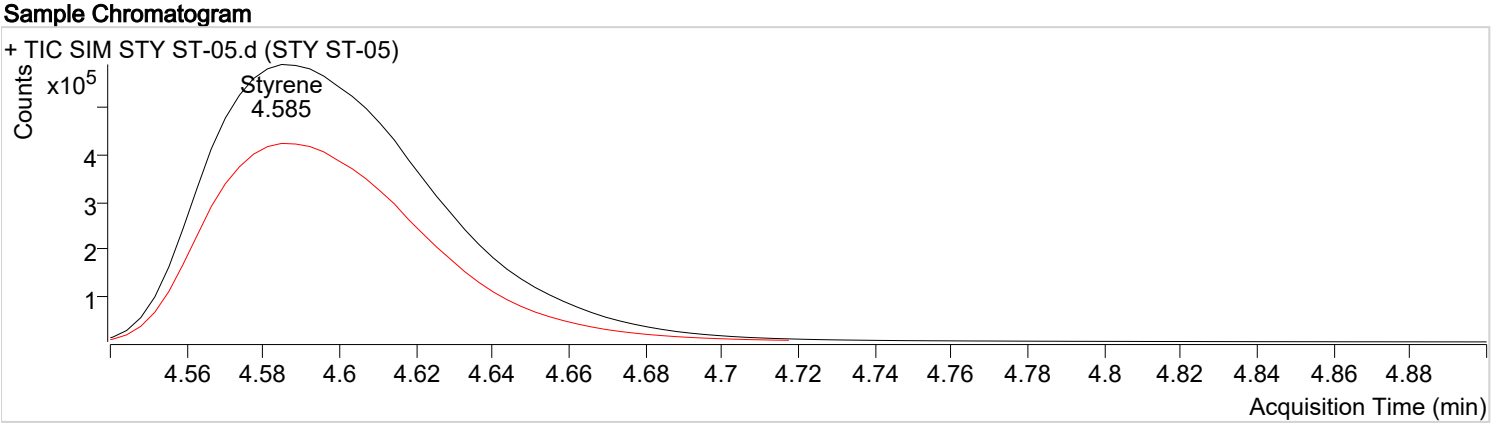

Name	RT	Resp.	Final Conc.	Units
Styrene	4.585	1716361	0.489	mg/L

Styrene

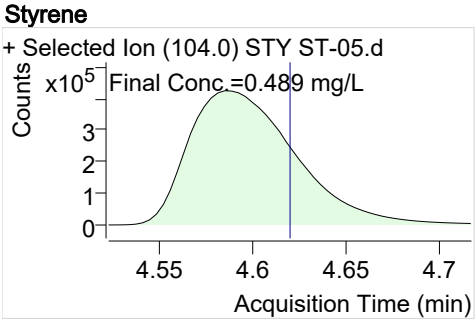



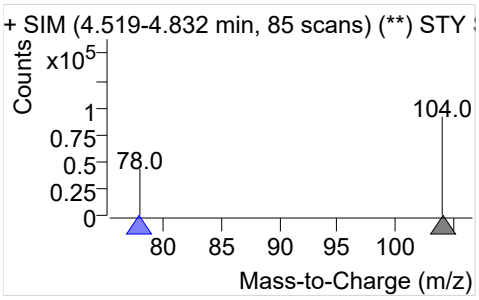

Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 1:32:46	**Data File**	BK-.d
Type	Blank	**Name**	BK-
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

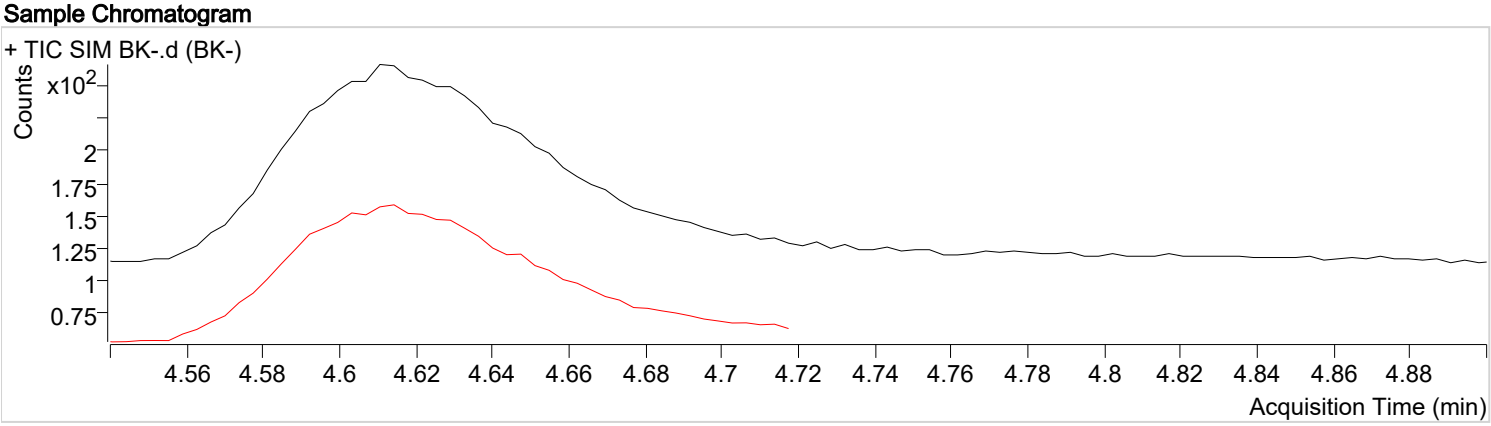

Styrene





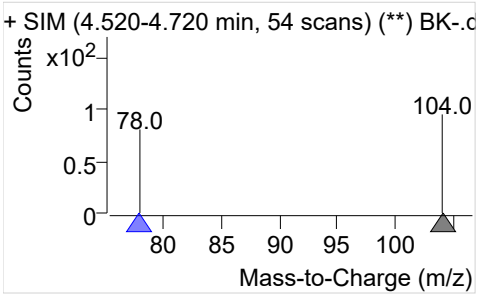

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 1:49:54	**Data File**	FBK(GS 26-02-10).d
Type	Blank	**Name**	FBK(GS 26-02-10)
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

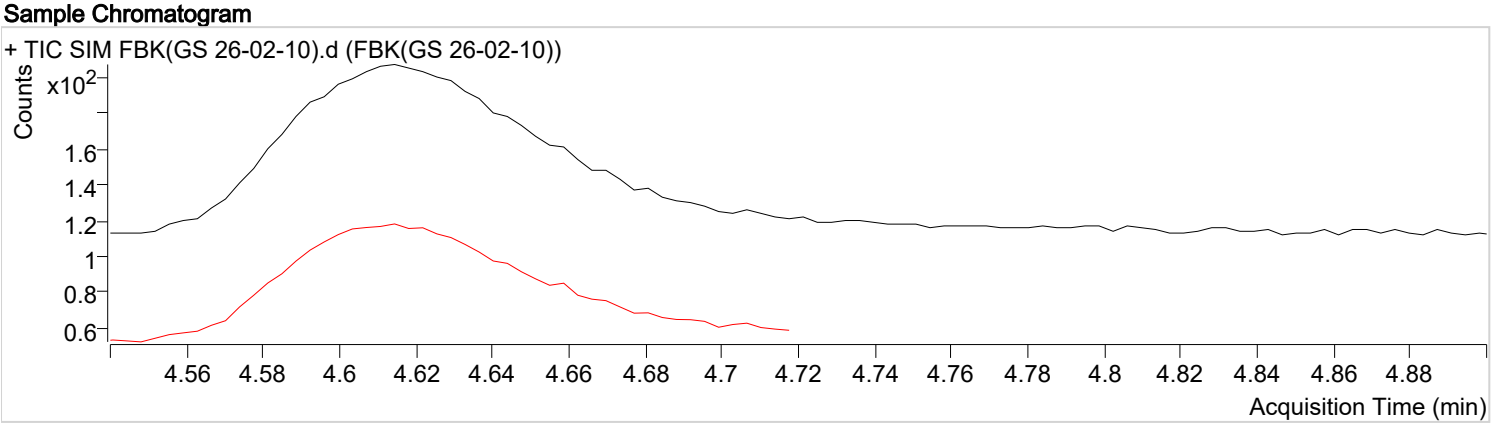

Styrene





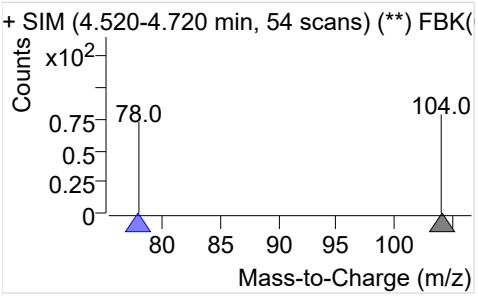

Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 2:07:03	**Data File**	KH (26-02-10).d
Type	Blank	**Name**	KH (26-02-10)
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

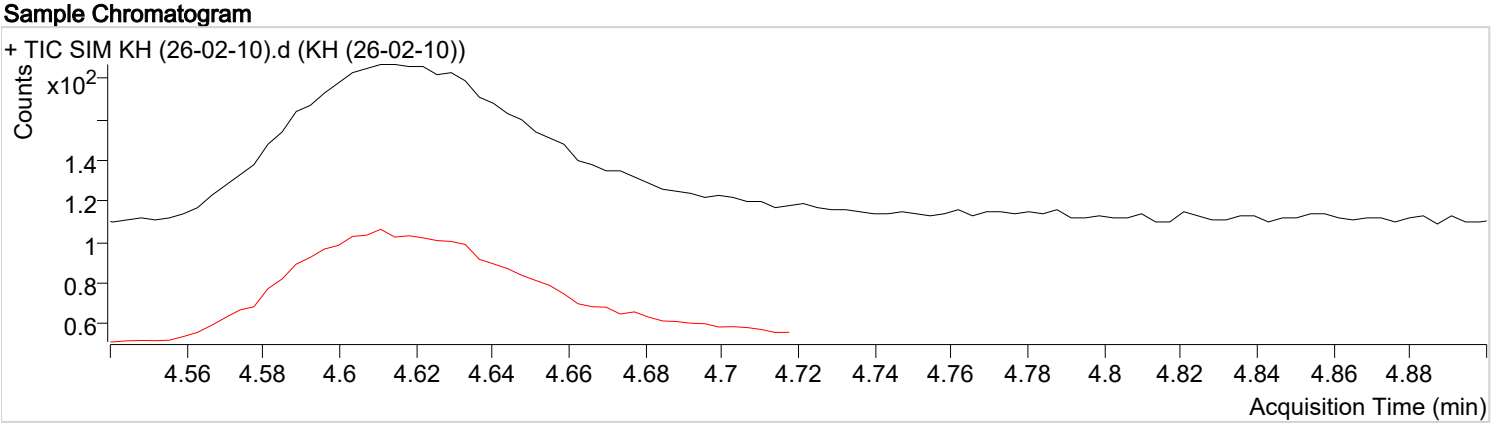

Styrene





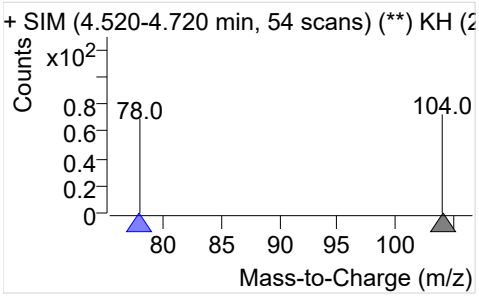

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 2:20:25	**Data File**	GS-01.d
Type	Sample	**Name**	GS-01
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

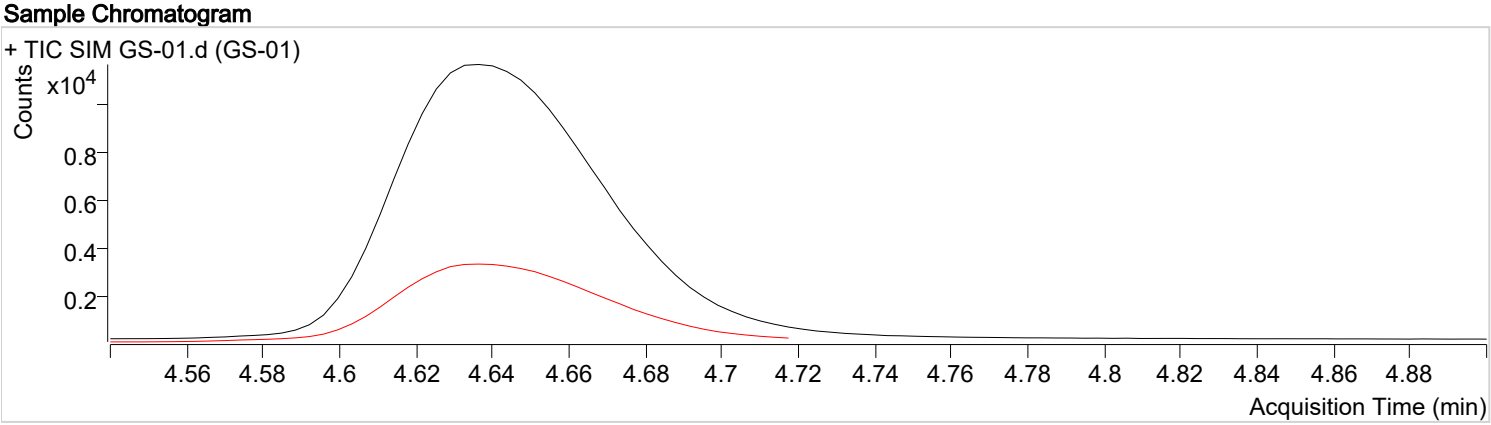

Name	RT	Resp.	Final Conc.	Units
Styrene	4.636	0	ND	mg/L

Styrene

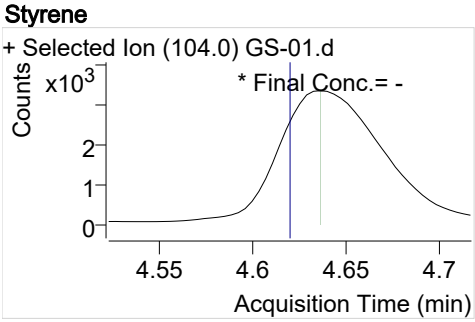





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 2:51:26	**Data File**	GS-02.d
Type	Sample	**Name**	GS-02
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

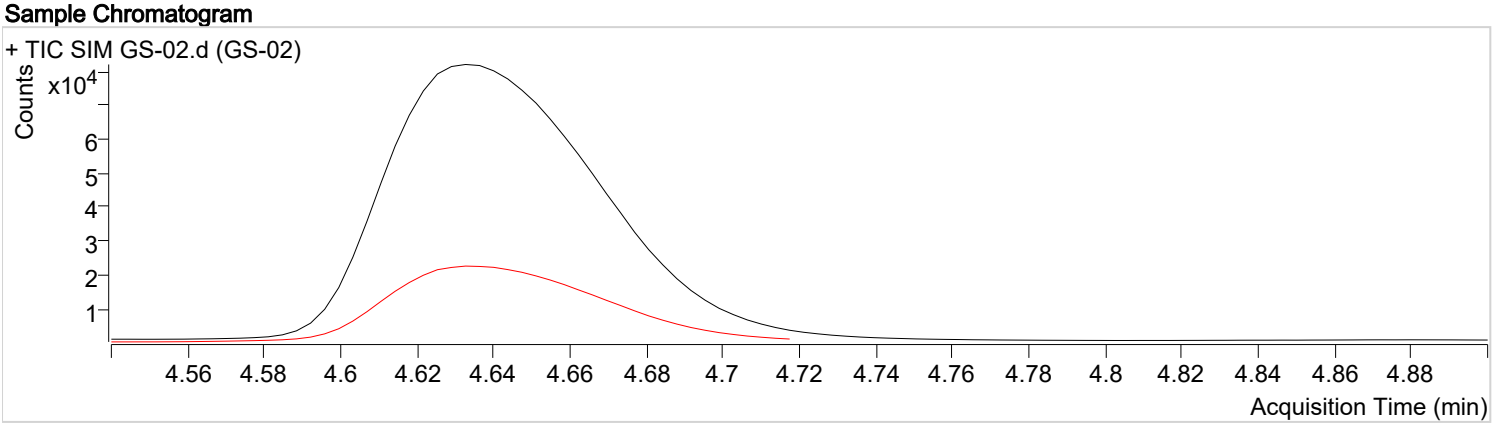

Name	RT	Resp.	Final Conc.	Units
Styrene	4.633	0	ND	mg/L

Styrene

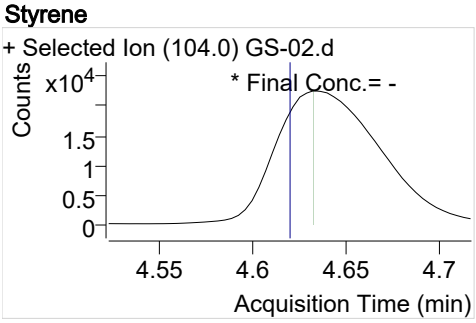

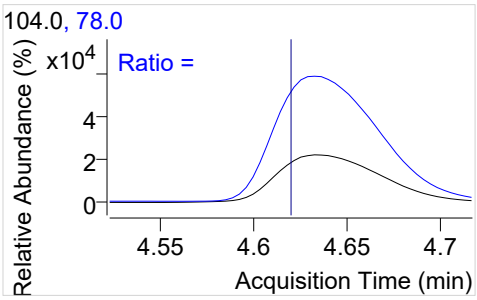

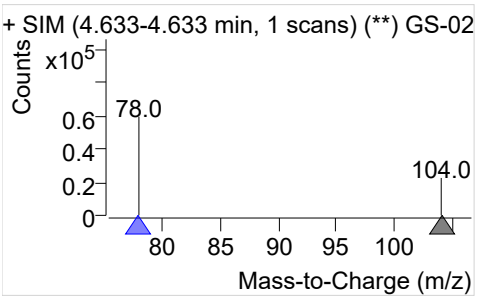

Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 3:08:21	**Data File**	GS-03.d
Type	Sample	**Name**	GS-03
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

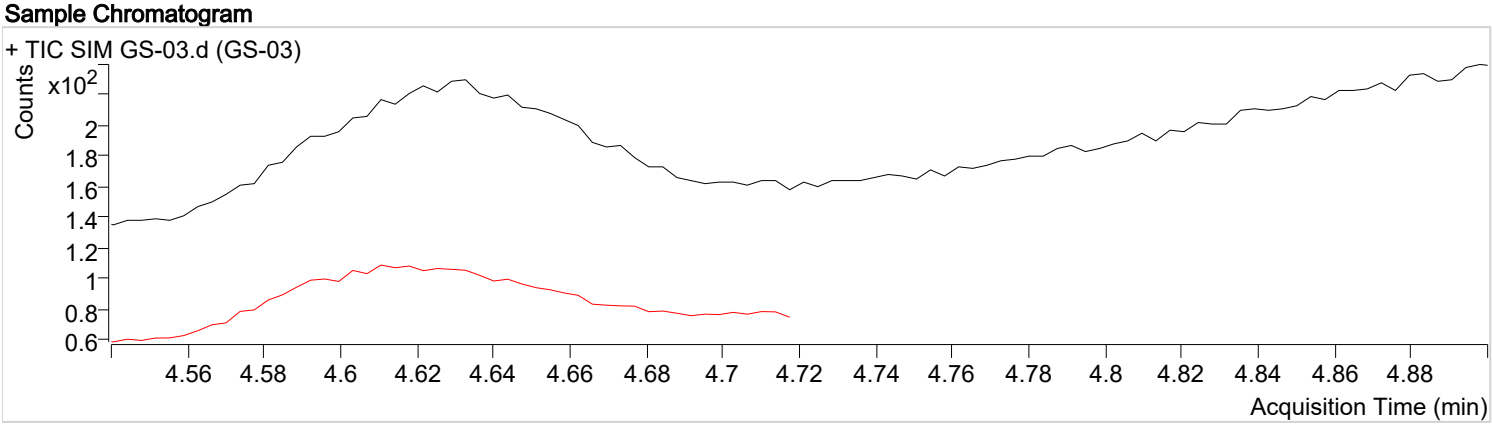

Styrene





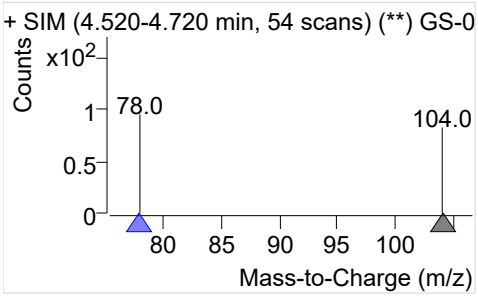

Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 3:25:25	**Data File**	GS-04.d
Type	Sample	**Name**	GS-04
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

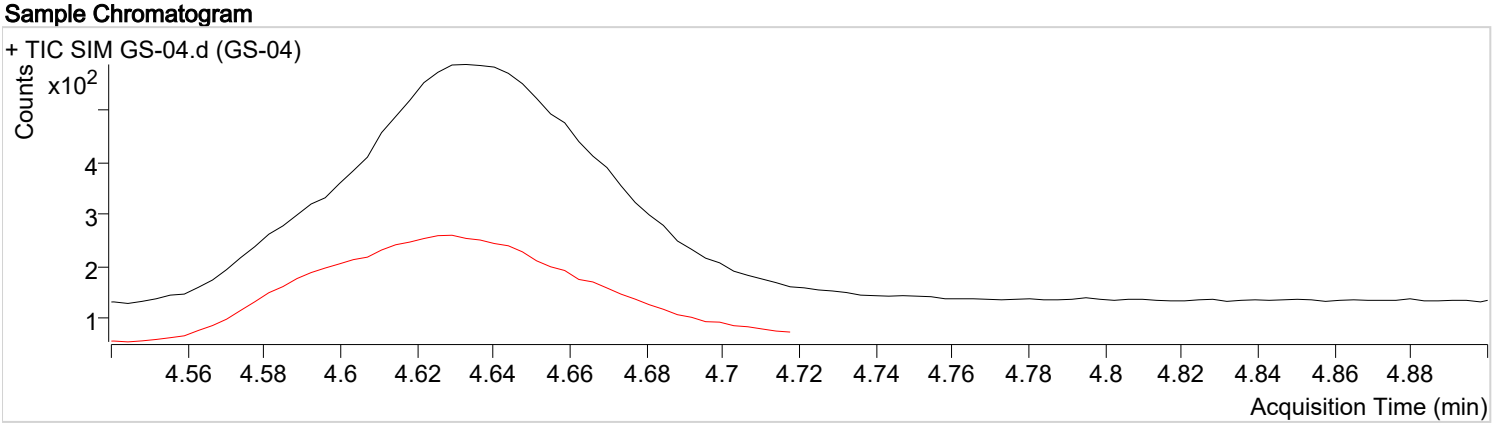

Name	RT	Resp.	Final Conc.	Units
Styrene	4.629	0	ND	mg/L

Styrene

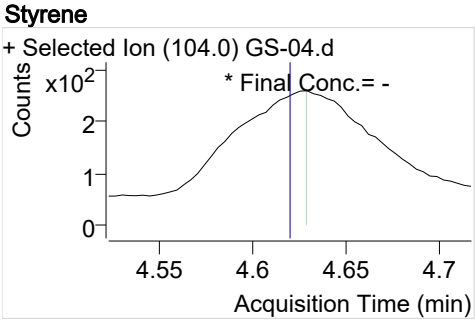

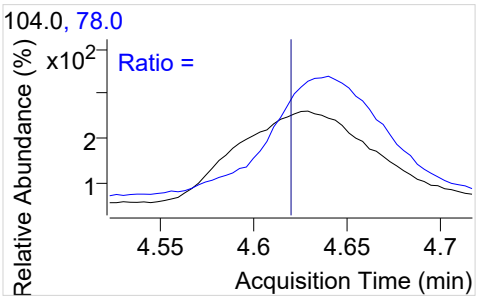

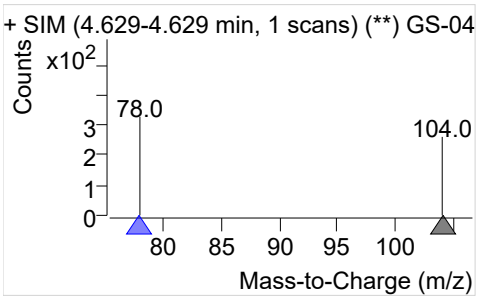

Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 3:38:49	**Data File**	GS-05.d
Type	Sample	**Name**	GS-05
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

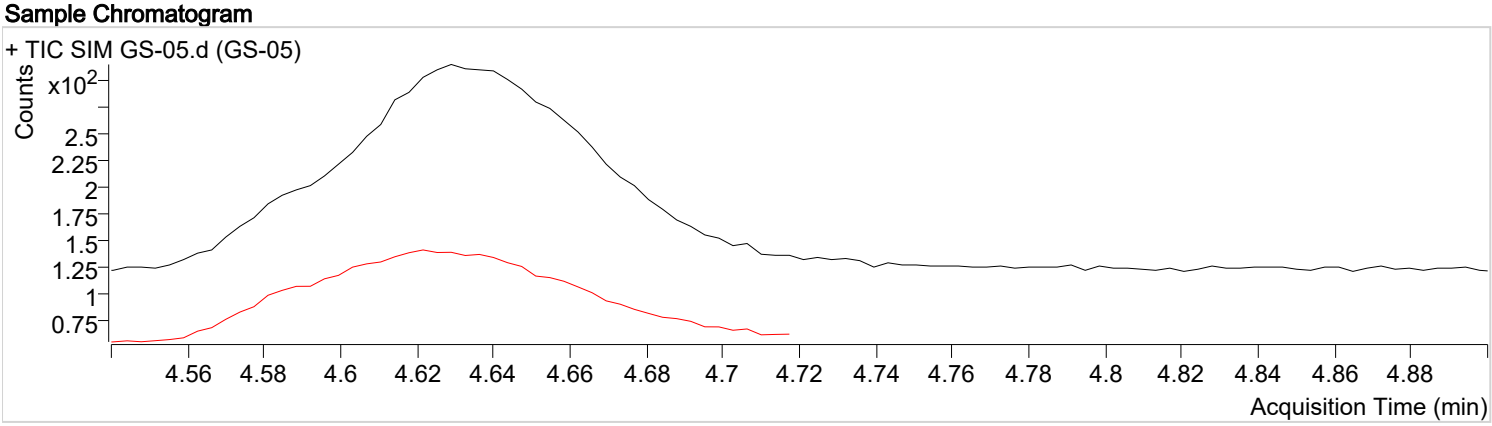

Styrene





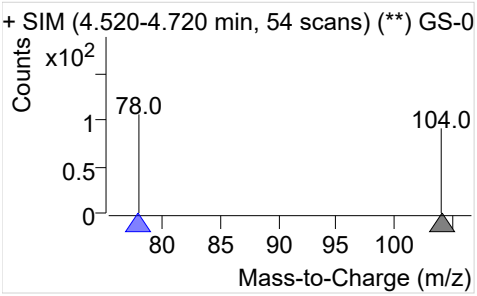

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 4:09:56	**Data File**	GS-06.d
Type	Sample	**Name**	GS-06
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

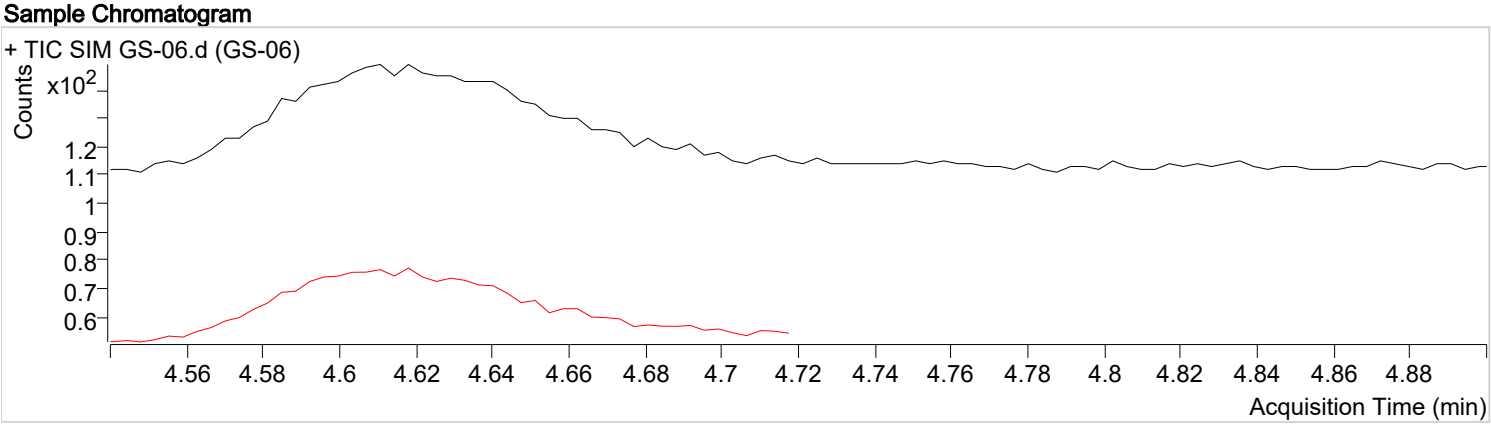

Styrene





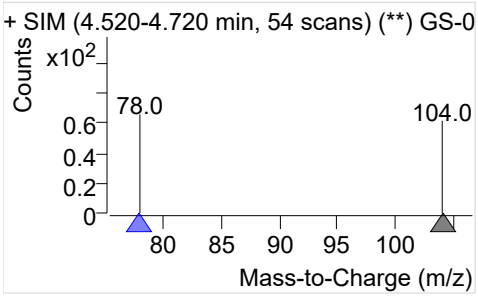

Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 4:27:05	**Data File**	GS-15.d
Type	Sample	**Name**	GS-15
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

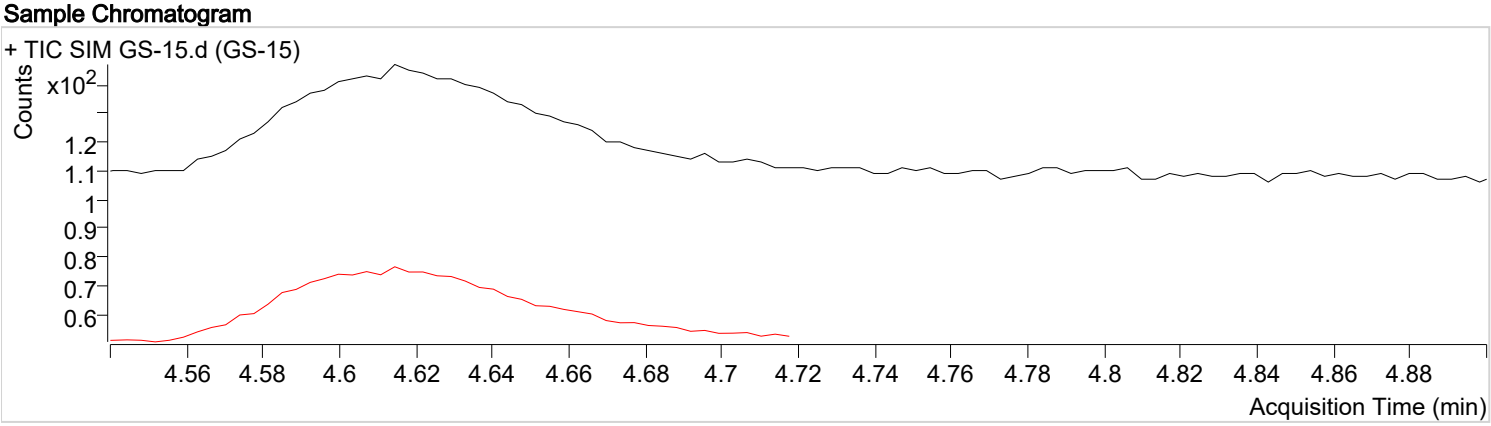

Styrene





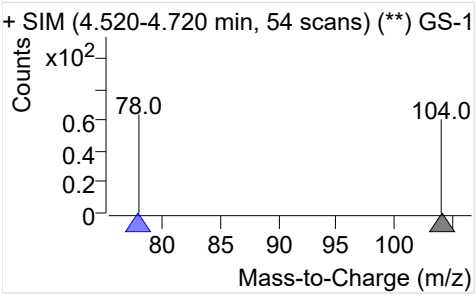

Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 5:01:21	**Data File**	MBK-1.d
Type	Blank	**Name**	MBK-1
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

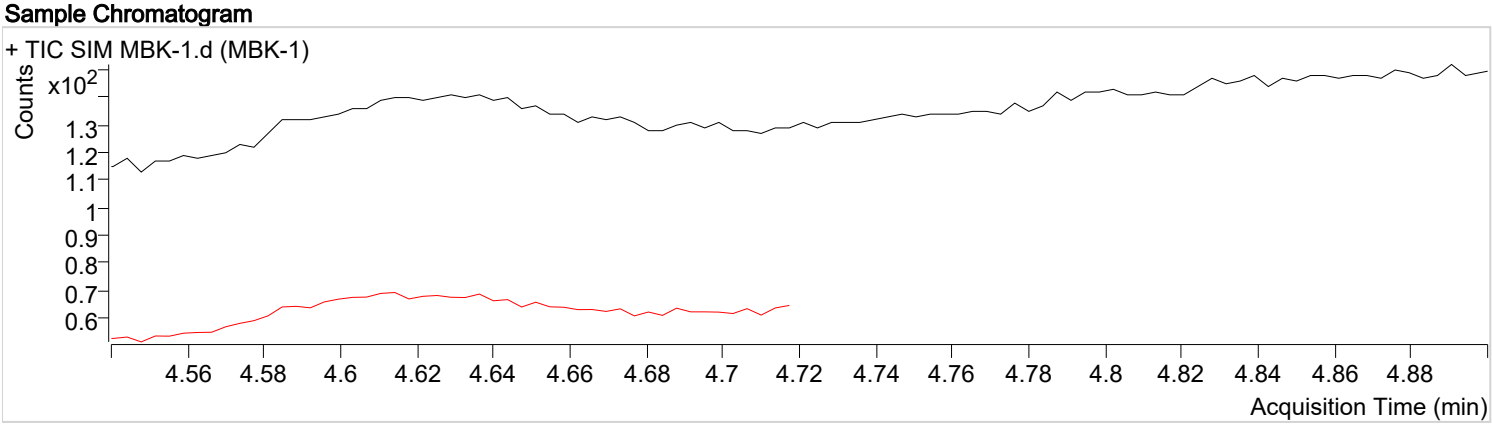

Styrene





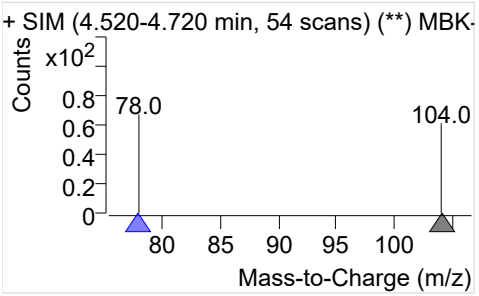

Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 5:52:32	**Data File**	CCV S.d
Type	QC	**Name**	CCV S
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

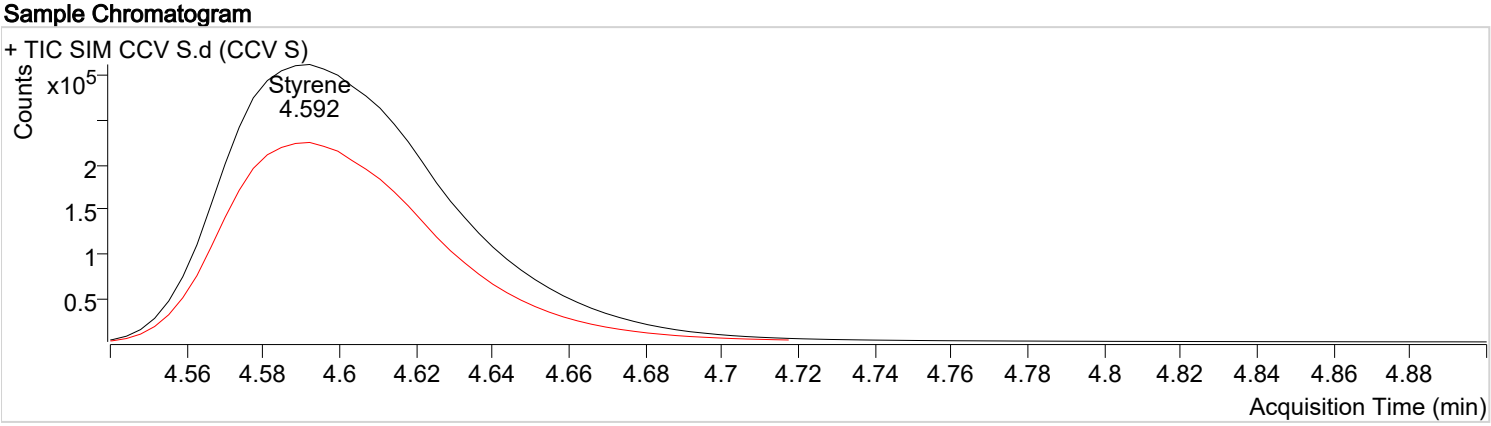

Name	RT	Resp.	Final Conc.	Units
Styrene	4.592	887056	0.250	mg/L

Styrene

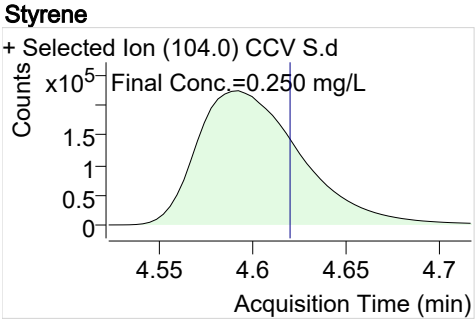

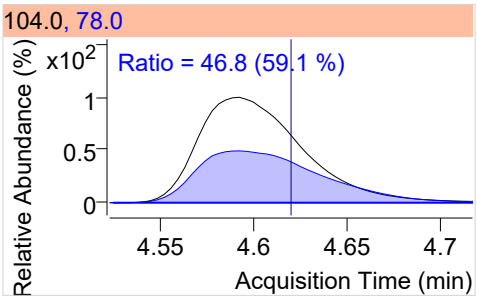

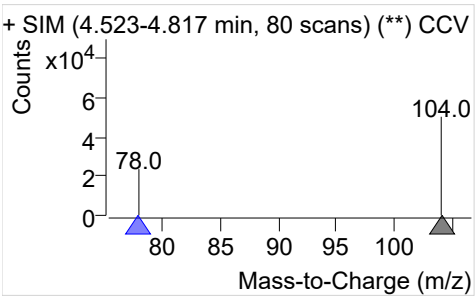

Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 6:26:37	**Data File**	SOL 1.d
Type	Sample	**Name**	SOL 1
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

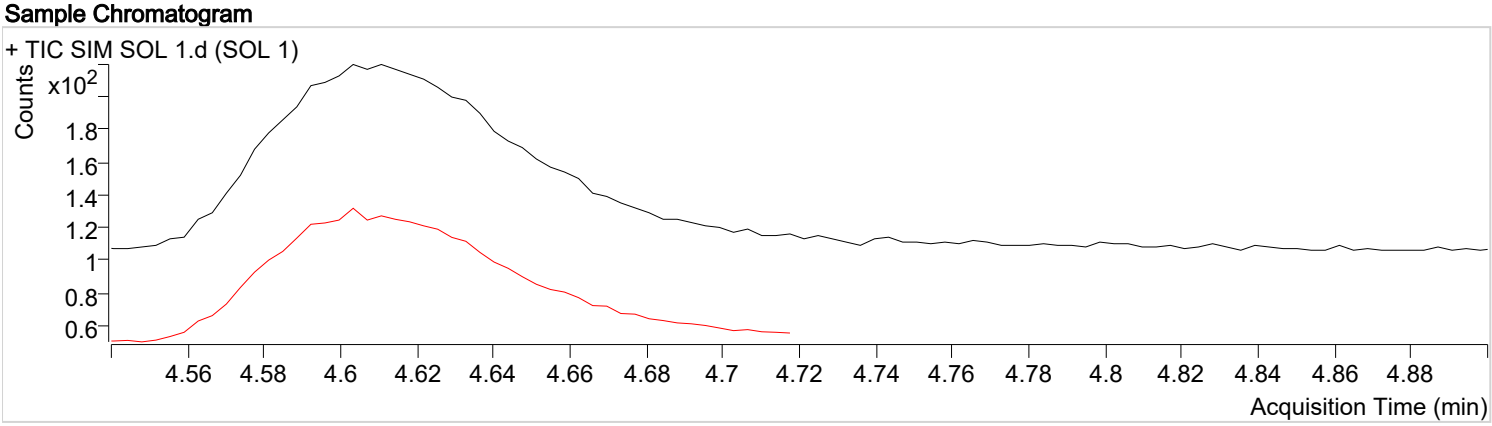

Styrene





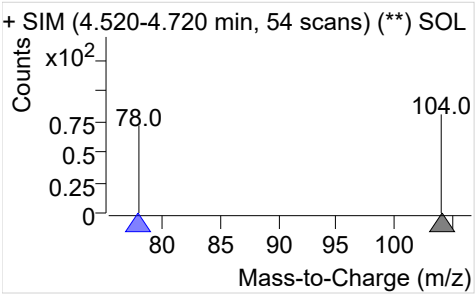

Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 6:43:33	**Data File**	SOL 2.d
Type	Sample	**Name**	SOL 2
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

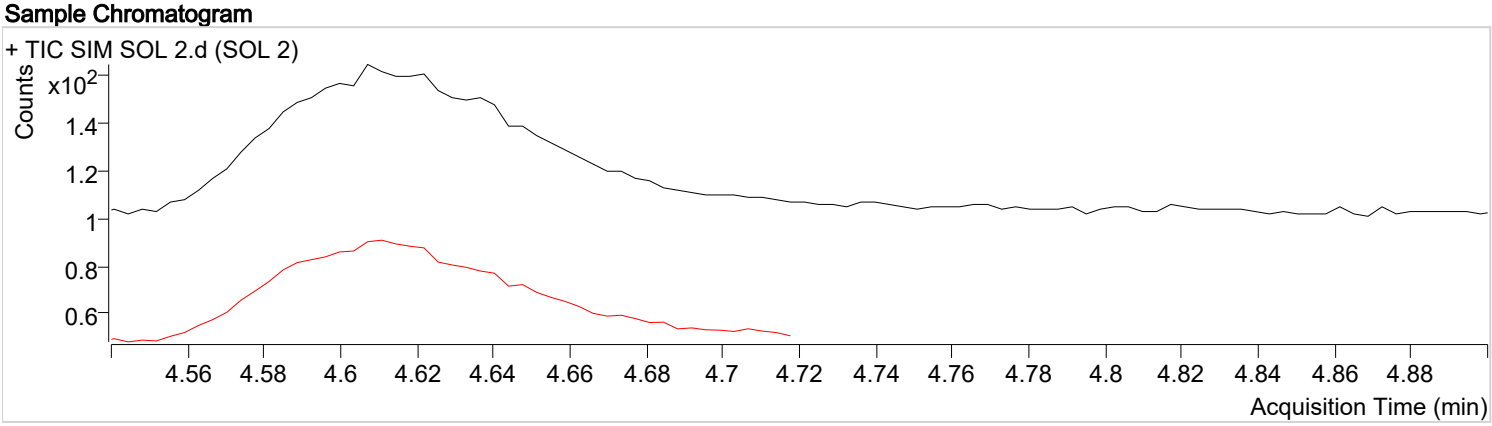

Styrene





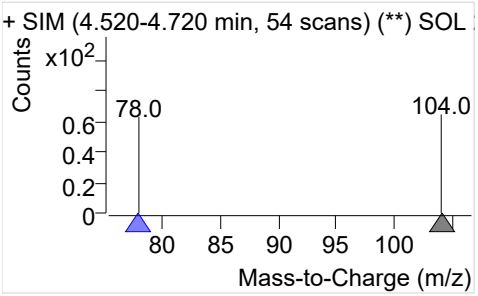

Quant Sample Report

Batch Data Path	V:\2026\2026-02\VOC2(GS 2.10, KH 2.10)\QuantResults\STY.batch.bin		
Analysis Time	2026-02-13 오후 12:47:09	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:13:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-13 오후 12:47:09	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-12 오후 7:00:29	**Data File**	SOL 3.d
Type	Sample	**Name**	SOL 3
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

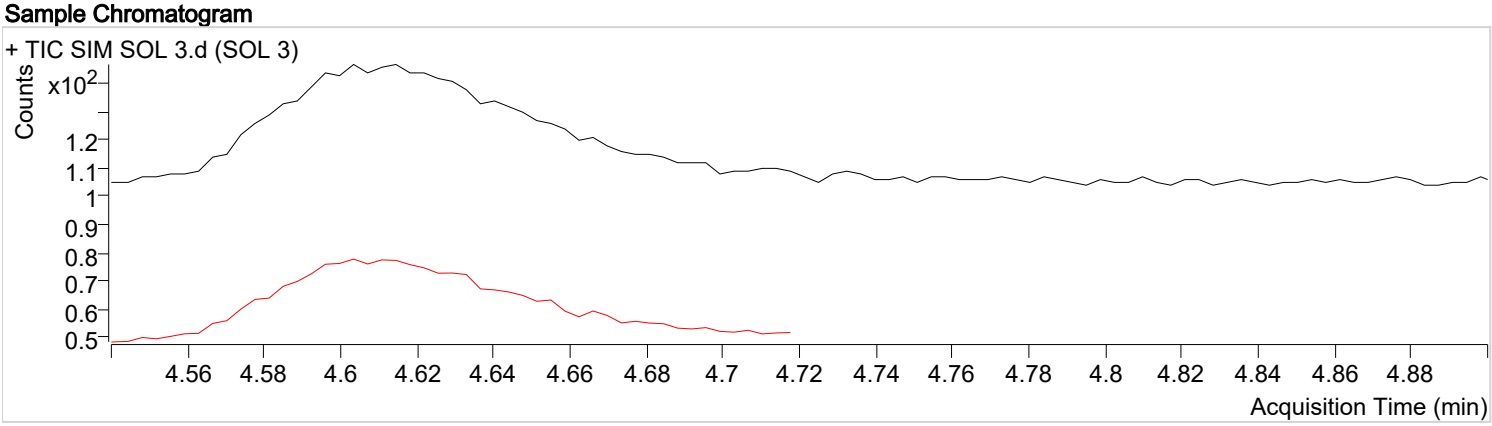
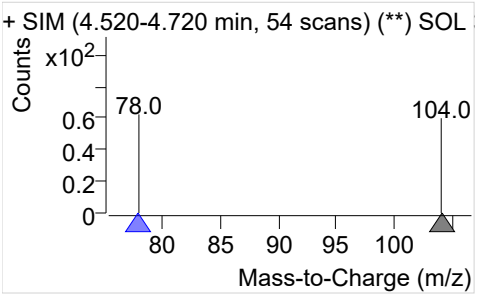
Styrene