Quantitative Analysis Results Summary Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin				
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Styrene

Data File	Type	RT	Resp.	Final Conc.
STY ST-01.d	Cal	4.607	9898	0.000
STY ST-02.d	Cal	4.600	52033	0.003
STY ST-03.d	Cal	4.592	265776	0.055
STY ST-04.d	Cal	4.588	1159585	0.270
STY ST-05.d	Cal	4.588	2075019	0.490
BK-.d	Blank	4.607	5022	0.000
FBK(RE 26-03-04).d	Blank	4.614	4746	0.000
FBK(KD 26-03-04).d	Blank	4.611	3893	0.000
RE-01.d	Sample	4.599	0	ND
RE-02.d	Sample	4.607	0	ND
RE-03.d	Sample	4.625	0	ND
RE-04.d	Sample	4.614	0	ND
RE-09.d	Sample	4.611	0	ND
RE-10.d	Sample			ND
RE-11.d	Sample			ND
RE-12.d	Sample			ND
KD-01.d	Sample			ND
KD-02.d	Sample			ND
KD-03.d	Sample			ND
MBK-1.d	Blank			ND
CCV S.d	QC	4.592	943522	0.218

Styrene

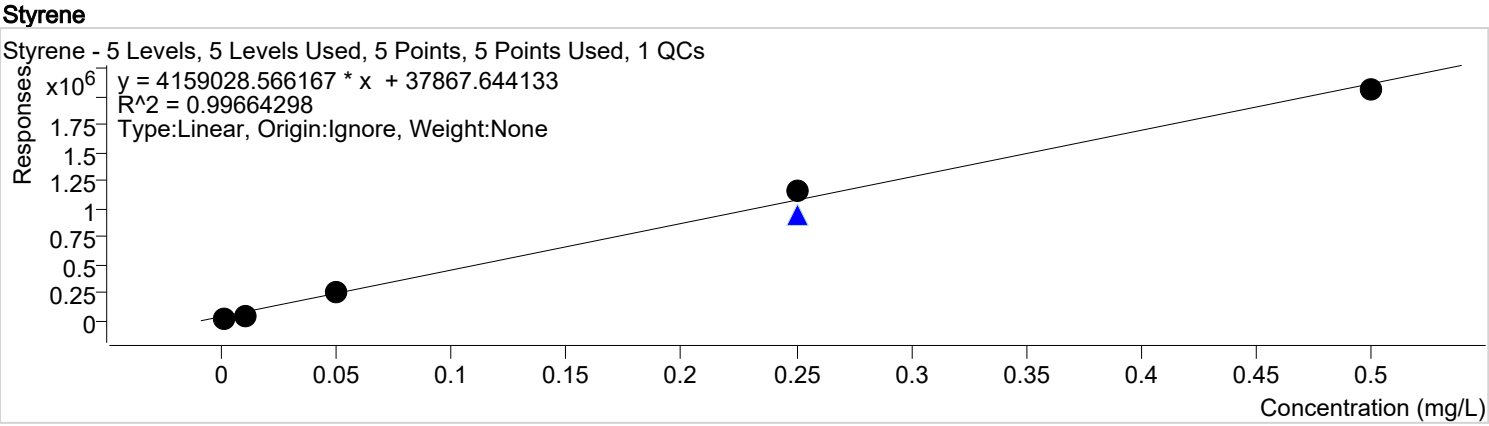

Cal. Path	Type	Level	Enable	Conc.	Response
V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\STY ST-01.d	Calibration	1	x	0.001	9898
V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\STY ST-02.d	Calibration	2	x	0.010	52033
V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\STY ST-03.d	Calibration	3	x	0.050	265776
V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\STY ST-04.d	Calibration	4	x	0.250	1159585
V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\CCV S.d	QC	4	x	0.250	943522
V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\STY ST-05.d	Calibration	5	x	0.500	2075019

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 3:53:03	**Data File**	STY ST-01.d
Type	Cal	**Name**	STY ST-01
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

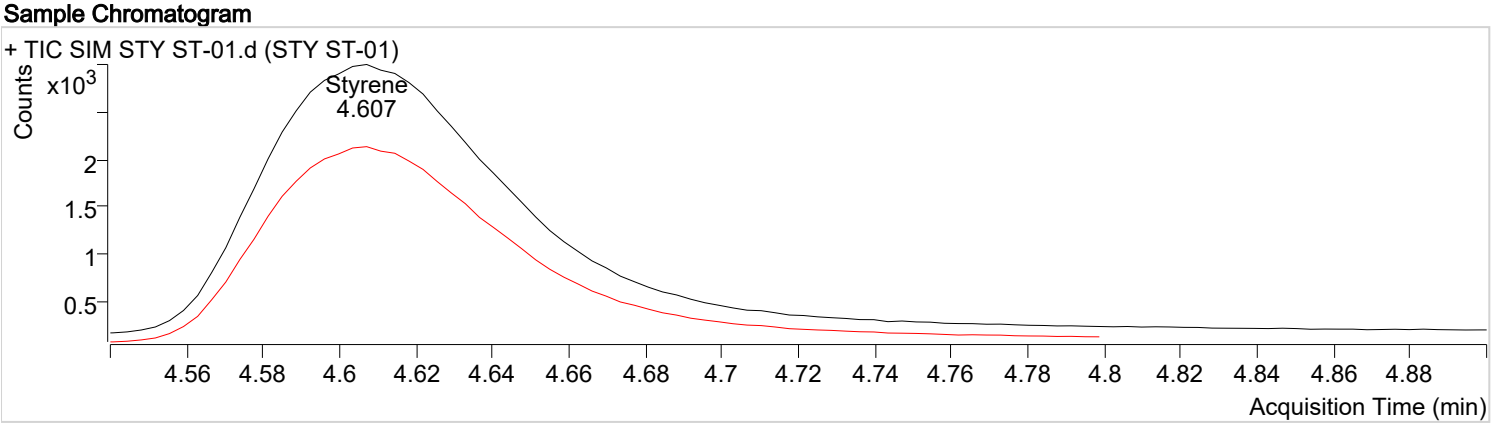

Name	RT	Resp.	Final Conc.	Units
Styrene	4.607	9898	0.000	mg/L

Styrene

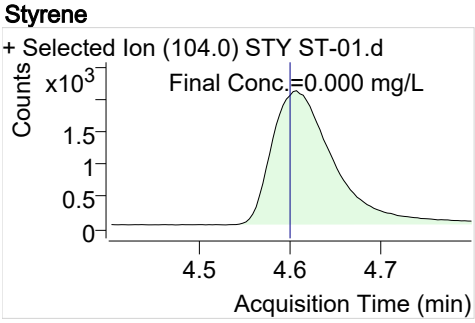

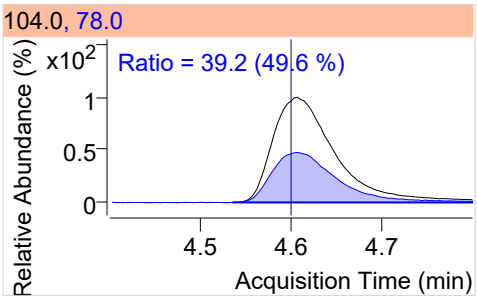

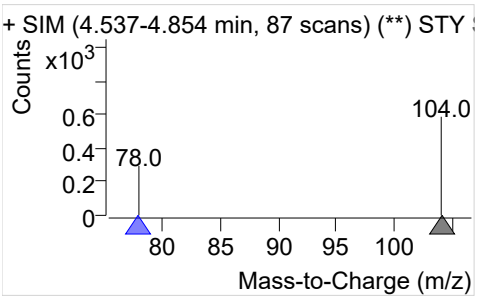

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 4:10:05	**Data File**	STY ST-02.d
Type	Cal	**Name**	STY ST-02
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

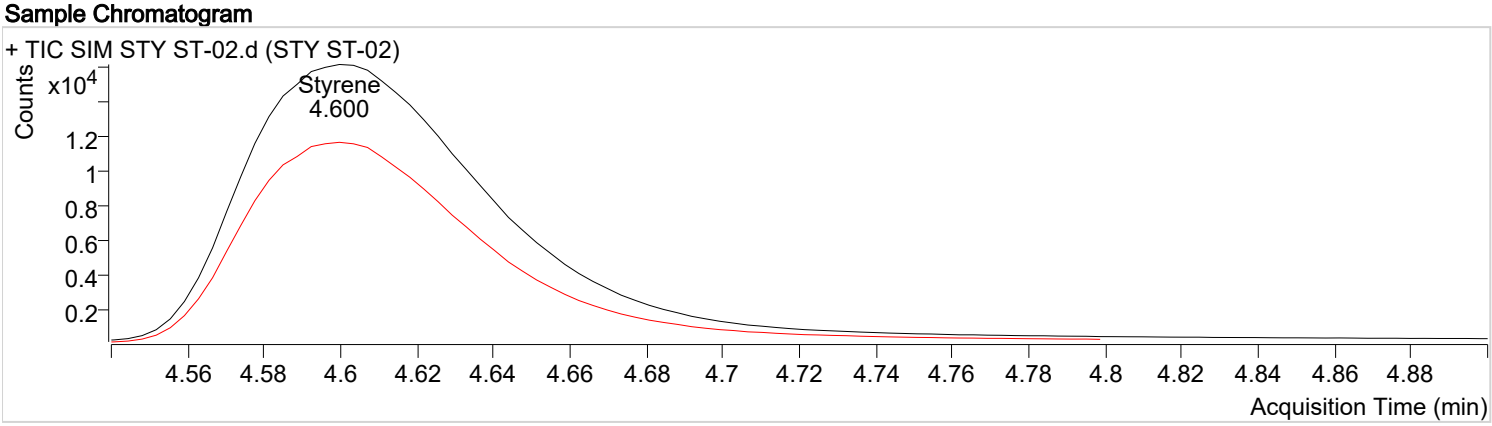

Name	RT	Resp.	Final Conc.	Units
Styrene	4.600	52033	0.003	mg/L

Styrene

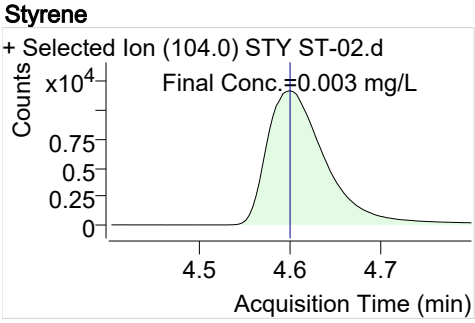

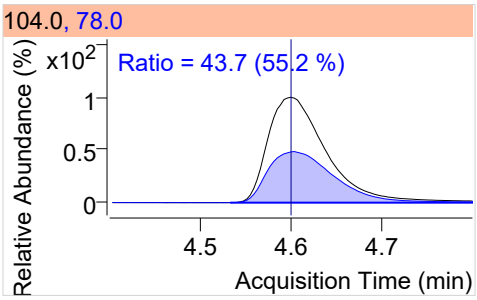

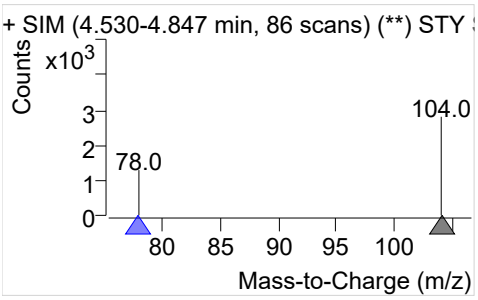

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 4:27:05	**Data File**	STY ST-03.d
Type	Cal	**Name**	STY ST-03
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

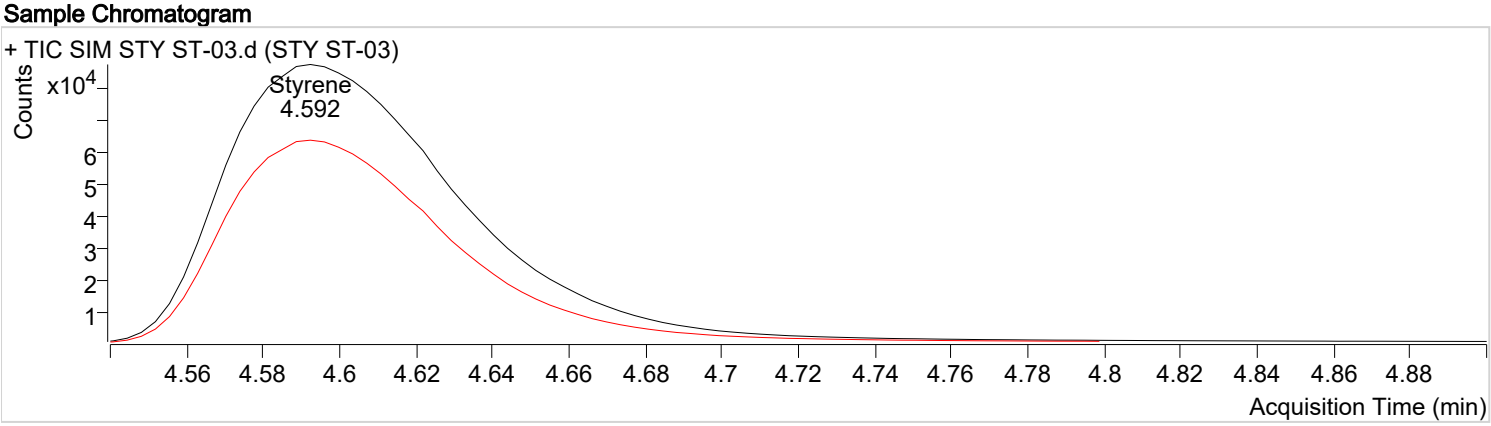

Name	RT	Resp.	Final Conc.	Units
Styrene	4.592	265776	0.055	mg/L

Styrene

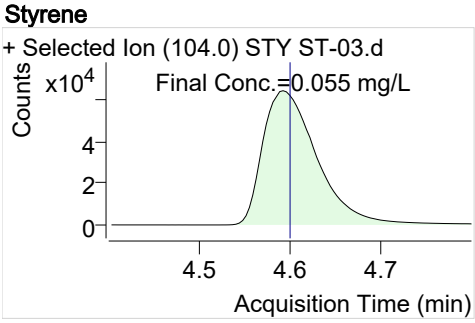



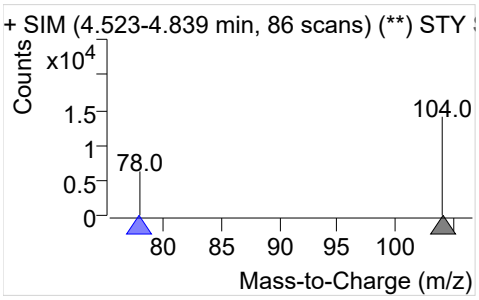

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 4:44:09	**Data File**	STY ST-04.d
Type	Cal	**Name**	STY ST-04
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

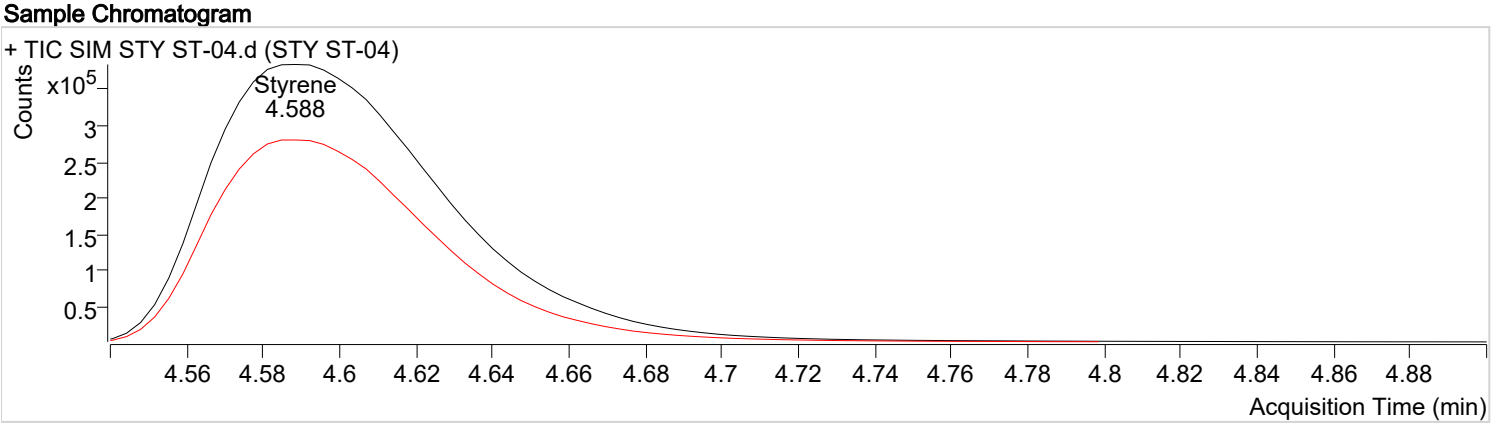

Name	RT	Resp.	Final Conc.	Units
Styrene	4.588	1159585	0.270	mg/L

Styrene

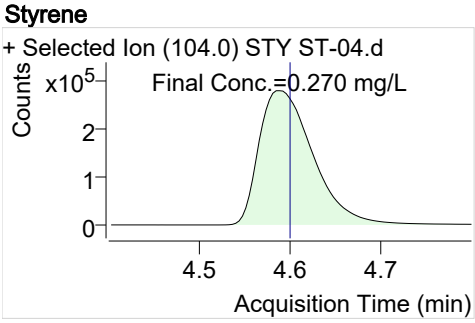



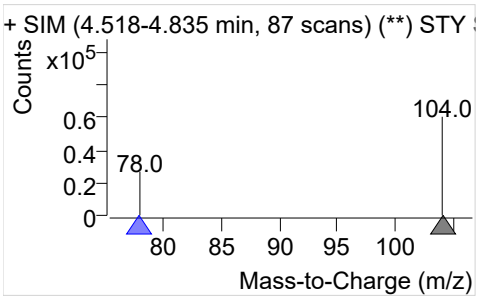

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 5:01:10	**Data File**	STY ST-05.d
Type	Cal	**Name**	STY ST-05
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

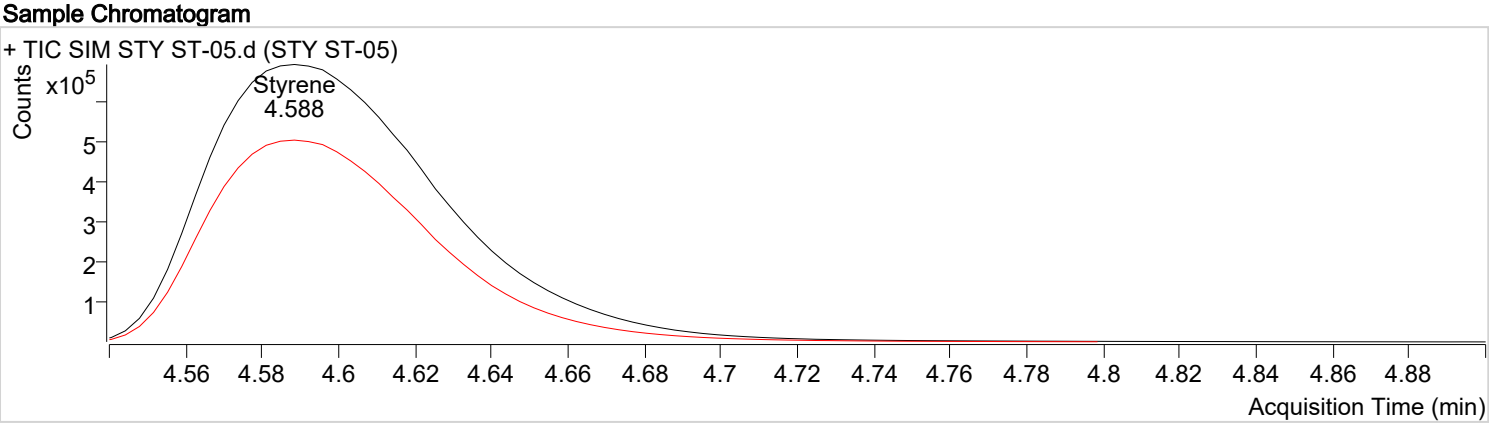

Name	RT	Resp.	Final Conc.	Units
Styrene	4.588	2075019	0.490	mg/L

Styrene

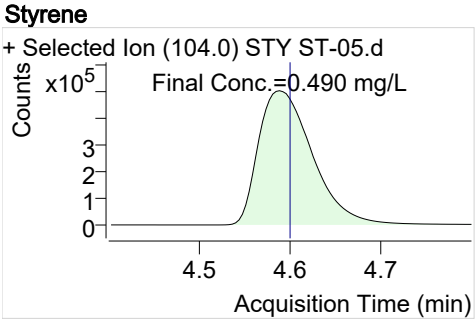

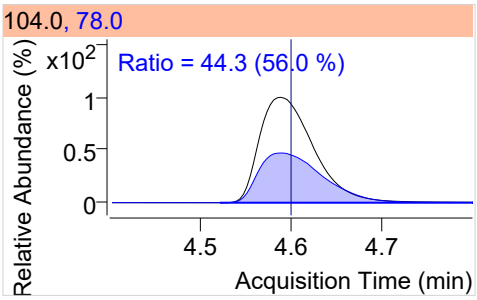

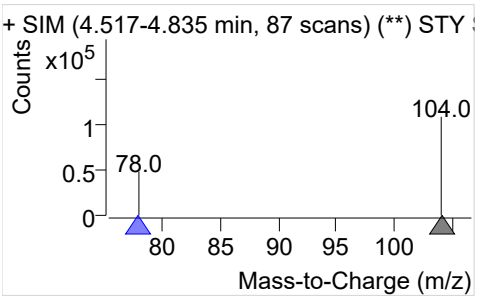

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 5:35:11	**Data File**	BK-.d
Type	Blank	**Name**	BK-
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

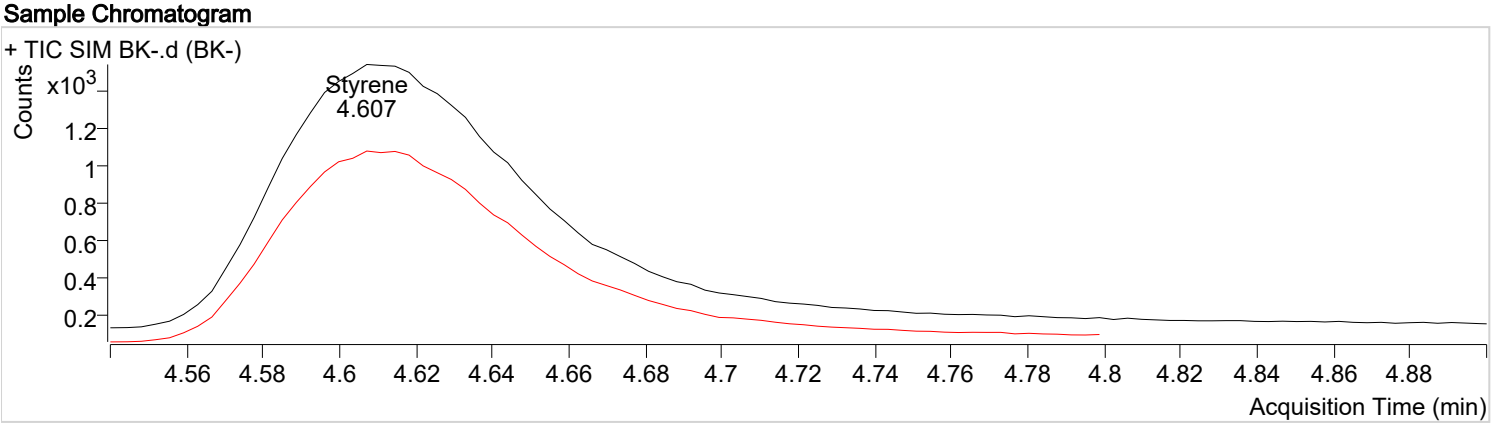

Styrene





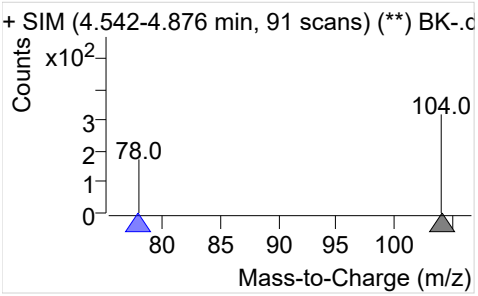

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 5:52:15	**Data File**	FBK(RE 26-03-04).d
Type	Blank	**Name**	FBK(RE 26-03-04)
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

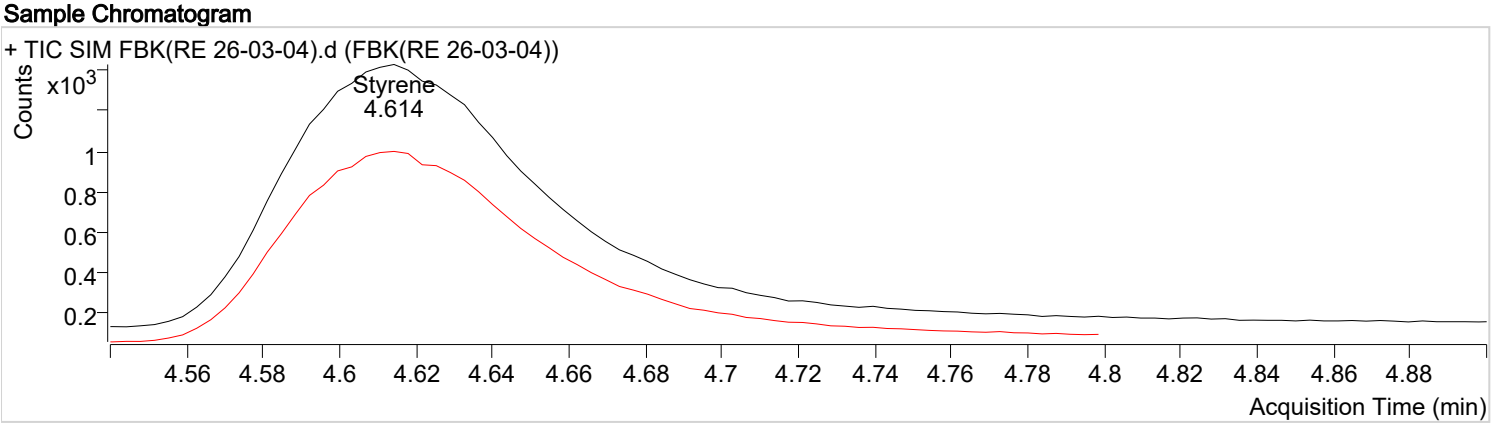

Styrene





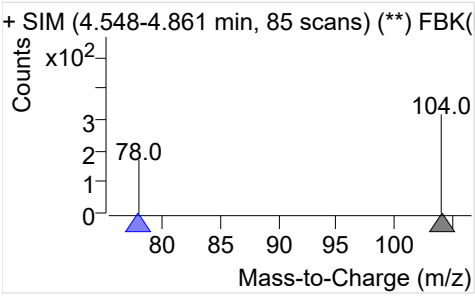

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 6:09:15	**Data File**	FBK(KD 26-03-04).d
Type	Blank	**Name**	FBK(KD 26-03-04)
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

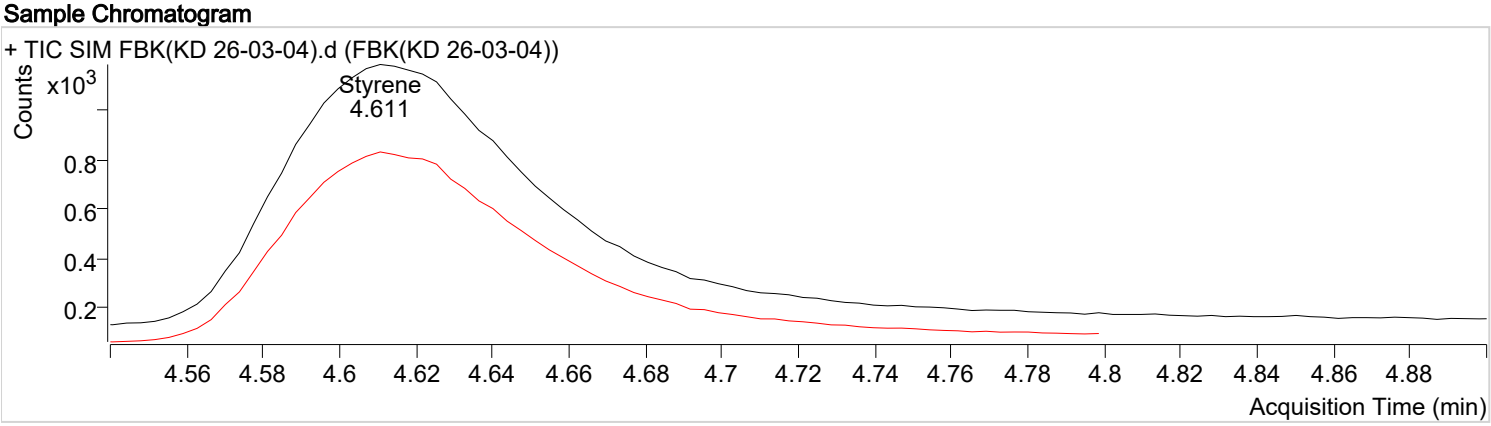

Styrene





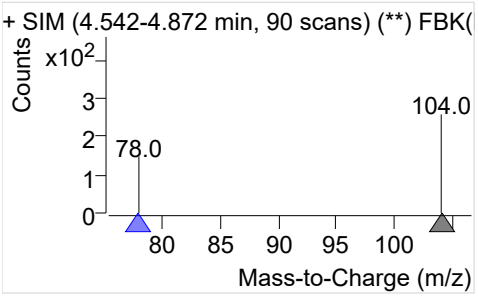

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 6:26:18	**Data File**	RE-01.d
Type	Sample	**Name**	RE-01
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

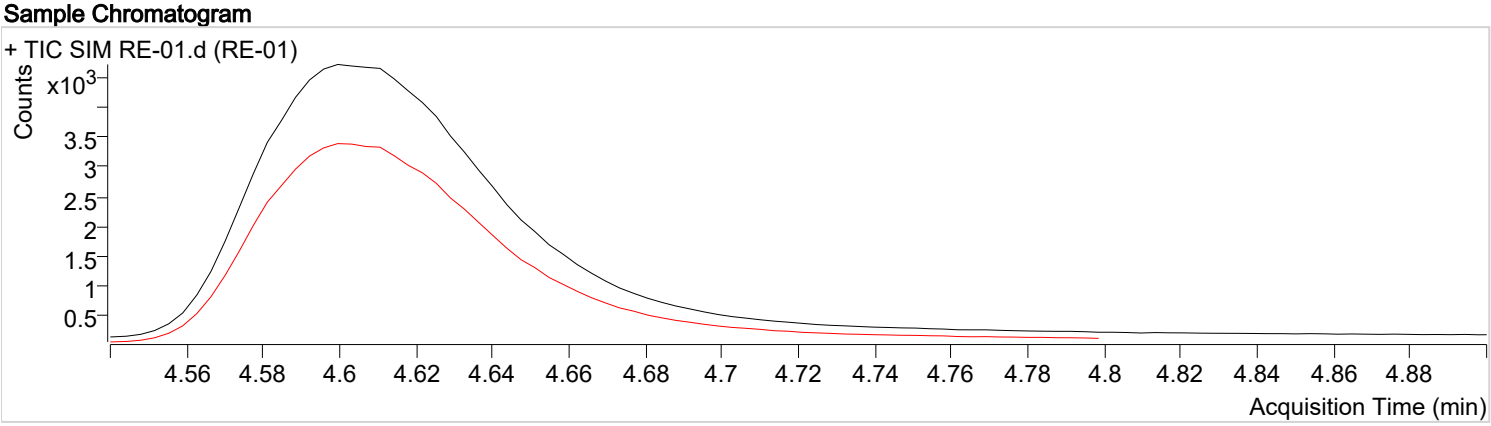

Name	RT	Resp.	Final Conc.	Units
Styrene	4.599	0	ND	mg/L

Styrene

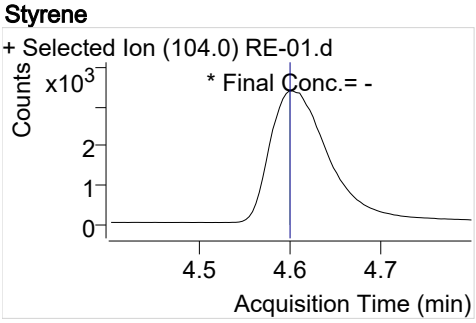

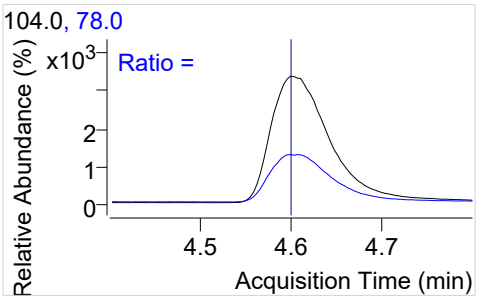



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 6:43:17	**Data File**	RE-02.d
Type	Sample	**Name**	RE-02
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

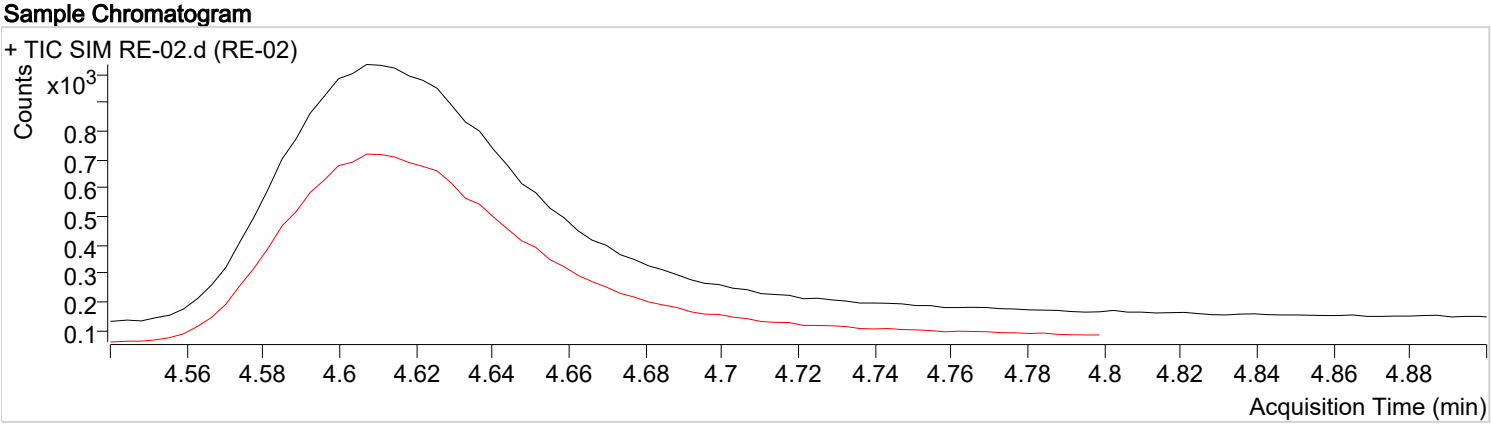

Styrene





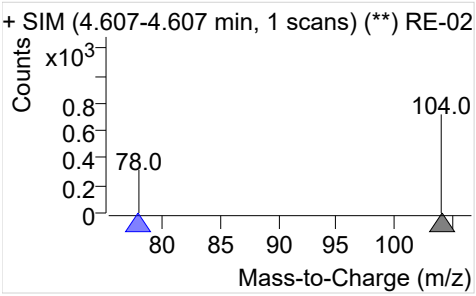

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 7:00:17	**Data File**	RE-03.d
Type	Sample	**Name**	RE-03
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

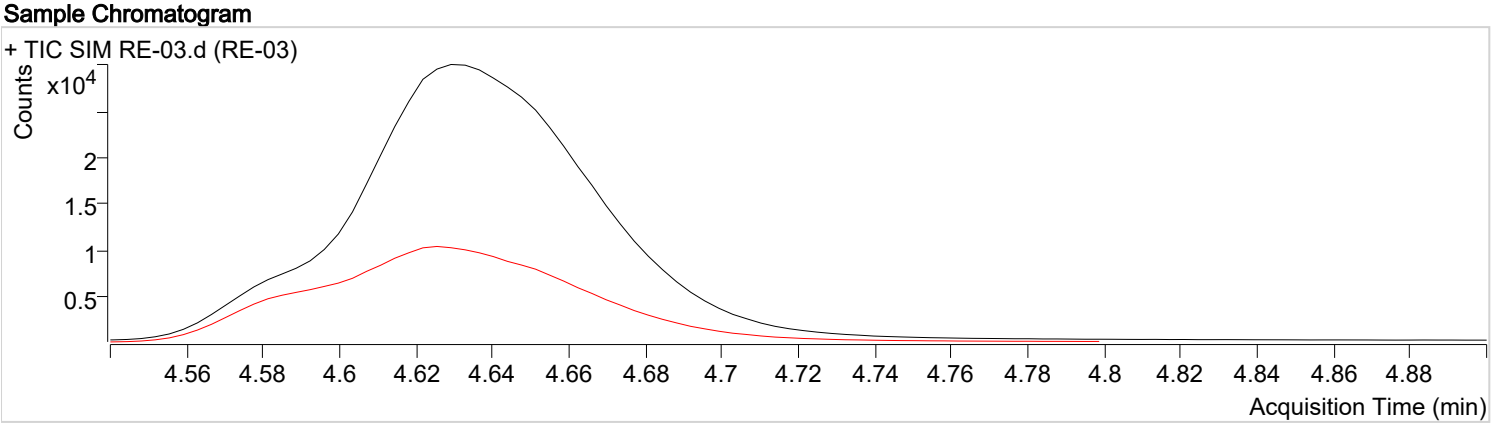

Name	RT	Resp.	Final Conc.	Units
Styrene	4.625	0	ND	mg/L

Styrene

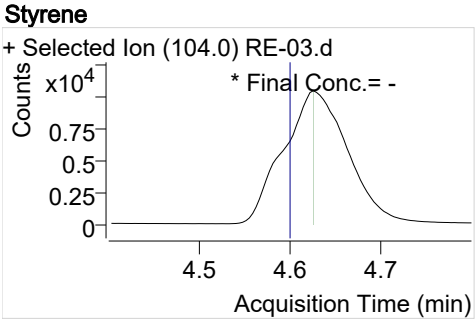





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 7:17:19	**Data File**	RE-04.d
Type	Sample	**Name**	RE-04
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

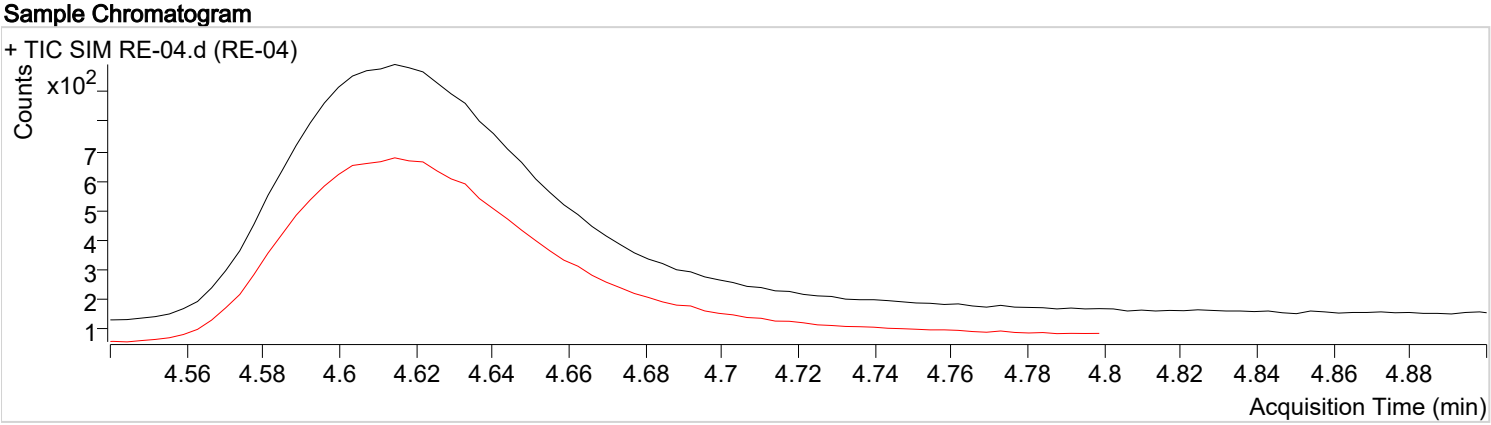

Styrene





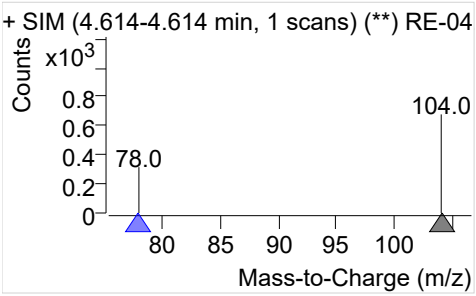

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 7:34:21	**Data File**	RE-09.d
Type	Sample	**Name**	RE-09
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

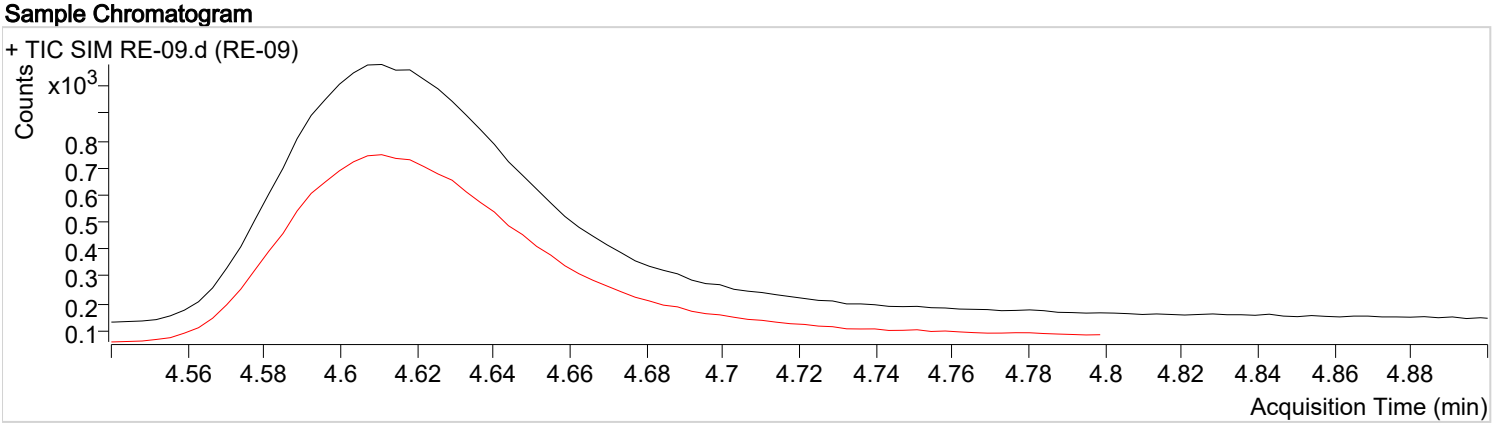

Styrene





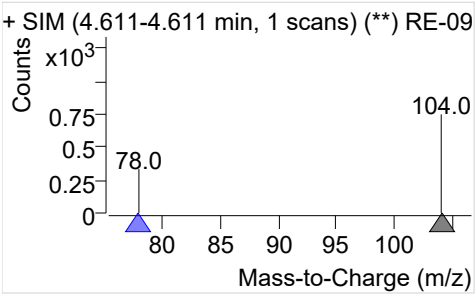

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 7:51:20	**Data File**	RE-10.d
Type	Sample	**Name**	RE-10
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

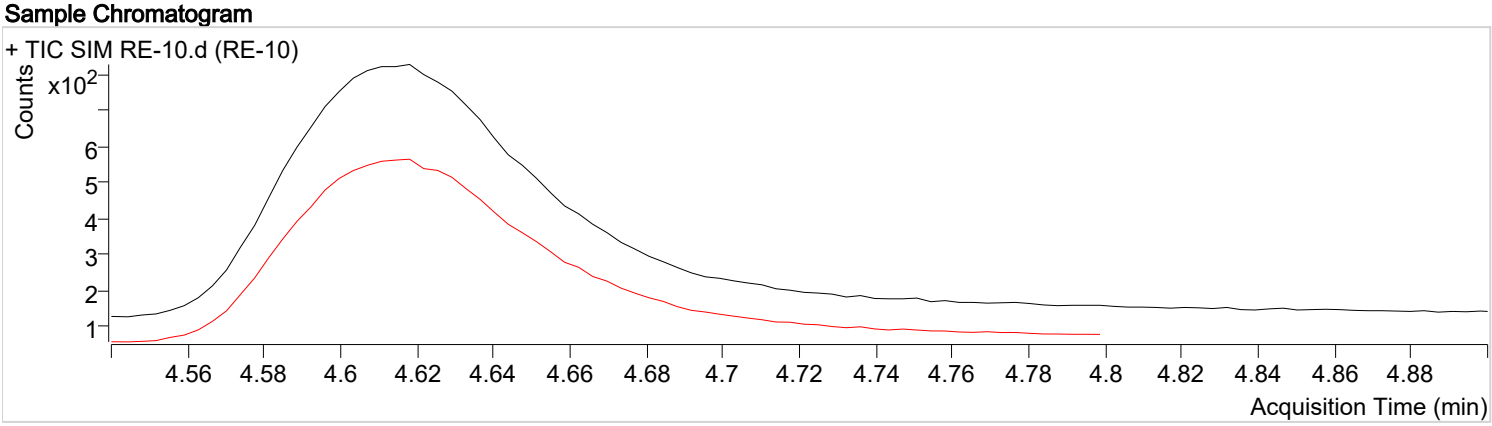

Styrene





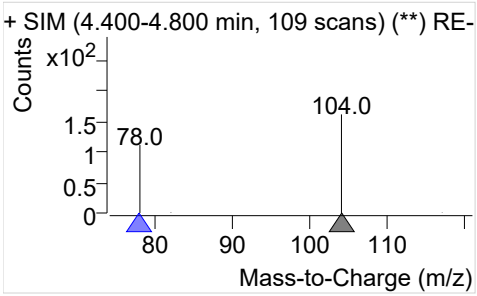

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 8:08:22	**Data File**	RE-11.d
Type	Sample	**Name**	RE-11
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

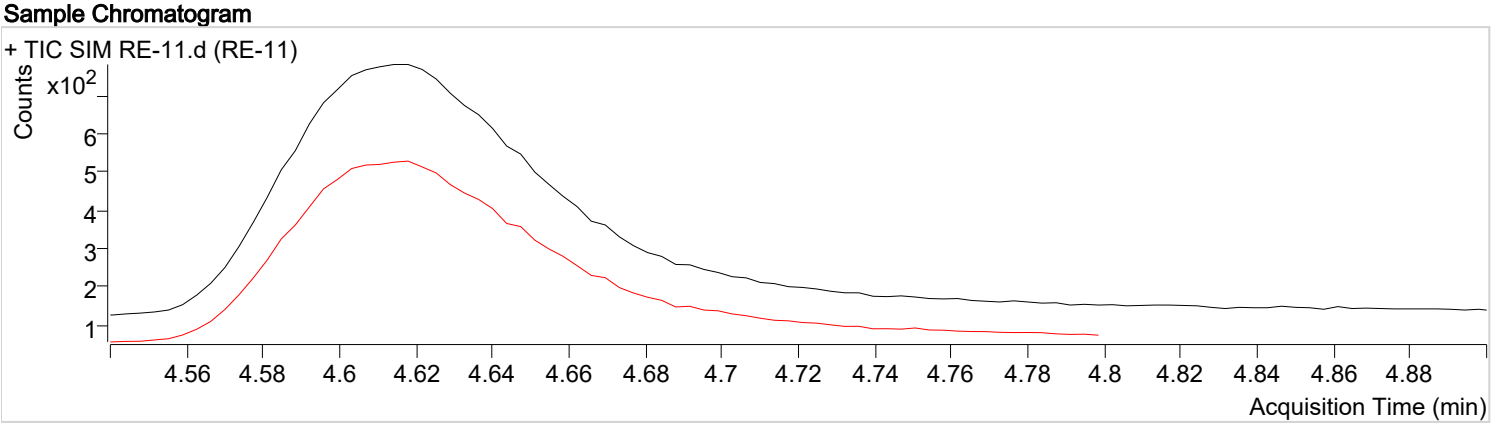

Styrene





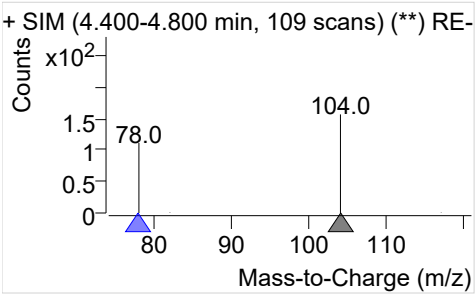

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 8:25:23	**Data File**	RE-12.d
Type	Sample	**Name**	RE-12
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

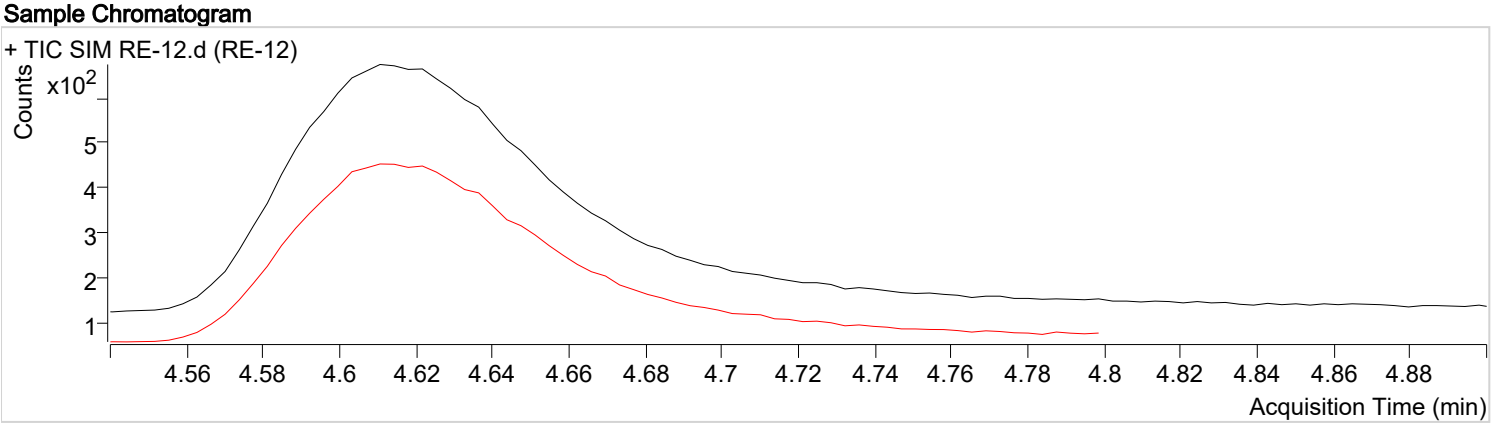

Styrene





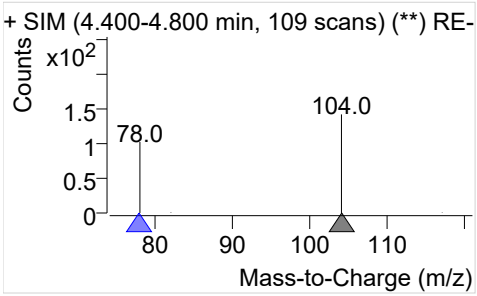

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 8:42:24	**Data File**	KD-01.d
Type	Sample	**Name**	KD-01
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

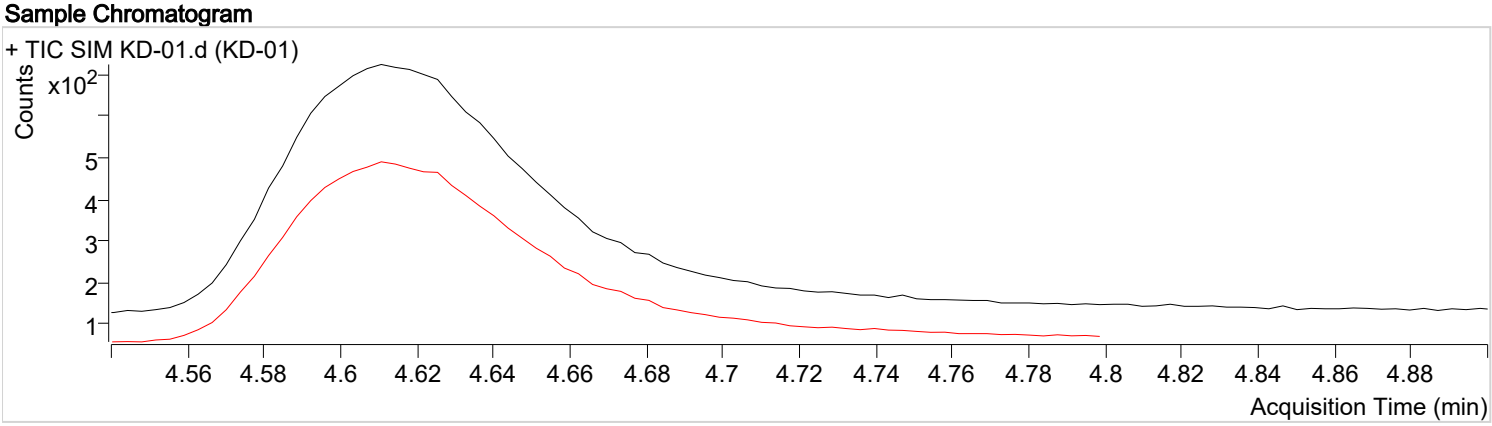

Styrene





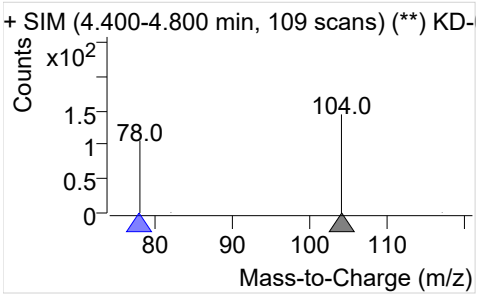

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 8:59:26	**Data File**	KD-02.d
Type	Sample	**Name**	KD-02
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

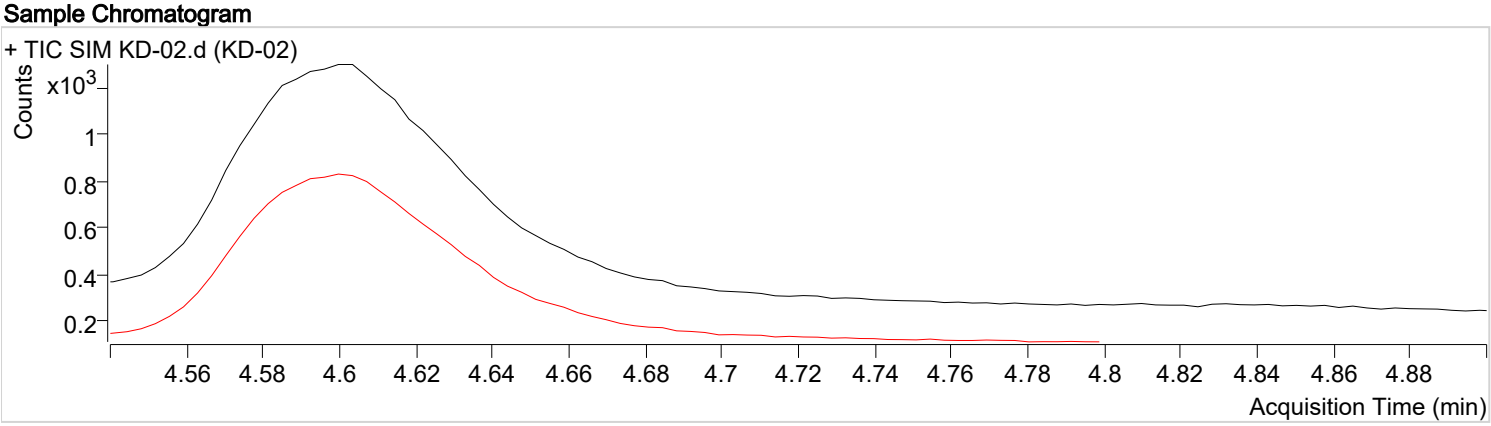

Styrene





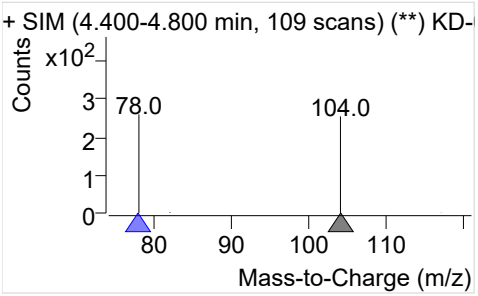

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 9:16:27	**Data File**	KD-03.d
Type	Sample	**Name**	KD-03
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

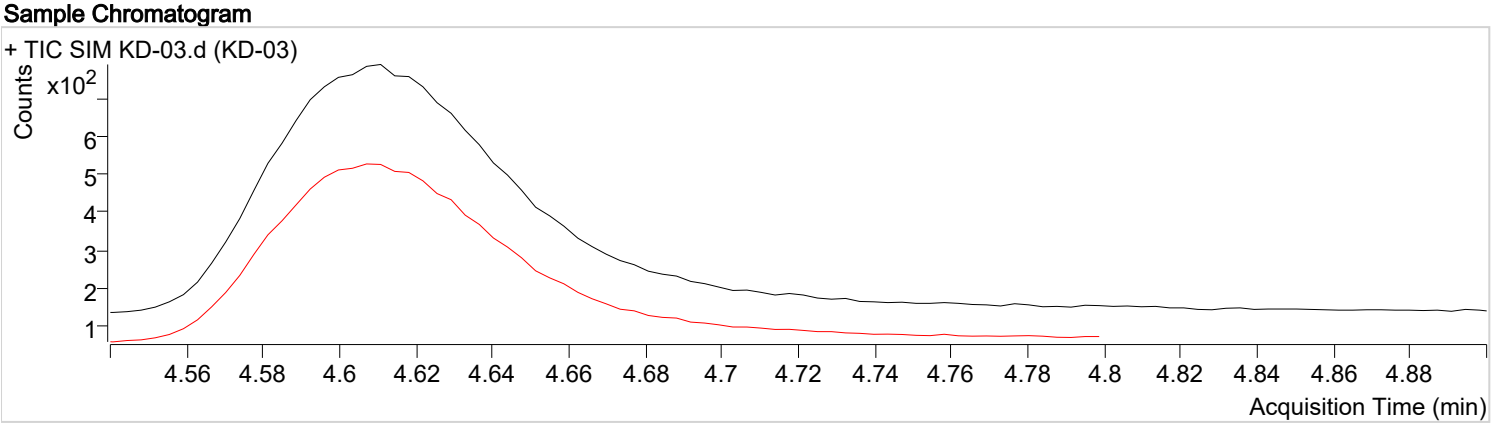

Styrene





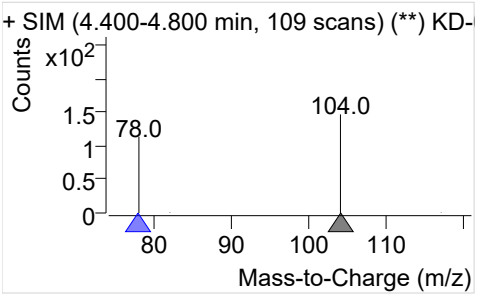

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 9:33:29	**Data File**	MBK-1.d
Type	Blank	**Name**	MBK-1
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

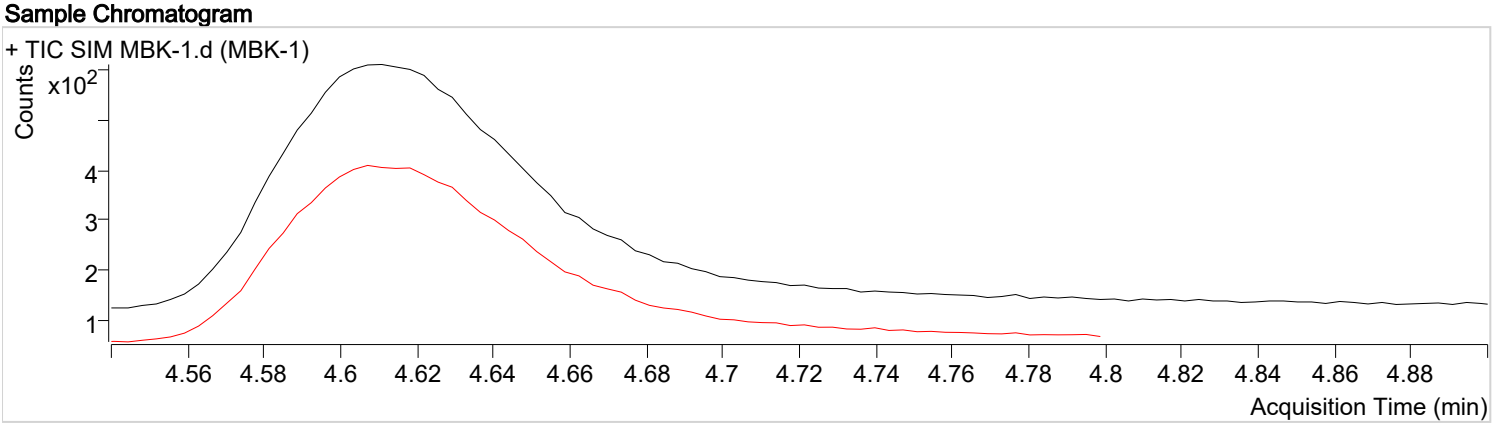

Styrene





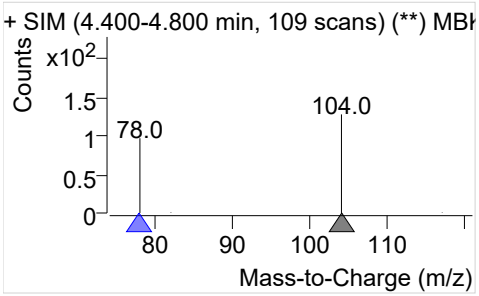

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.4 KD 3.4)\QuantResults\ST.batch.bin		
Analysis Time	2026-03-05 오후 3:43:41	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:15:52	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-05 오후 3:43:41	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-04 오후 10:07:23	**Data File**	CCV S.d
Type	QC	**Name**	CCV S
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

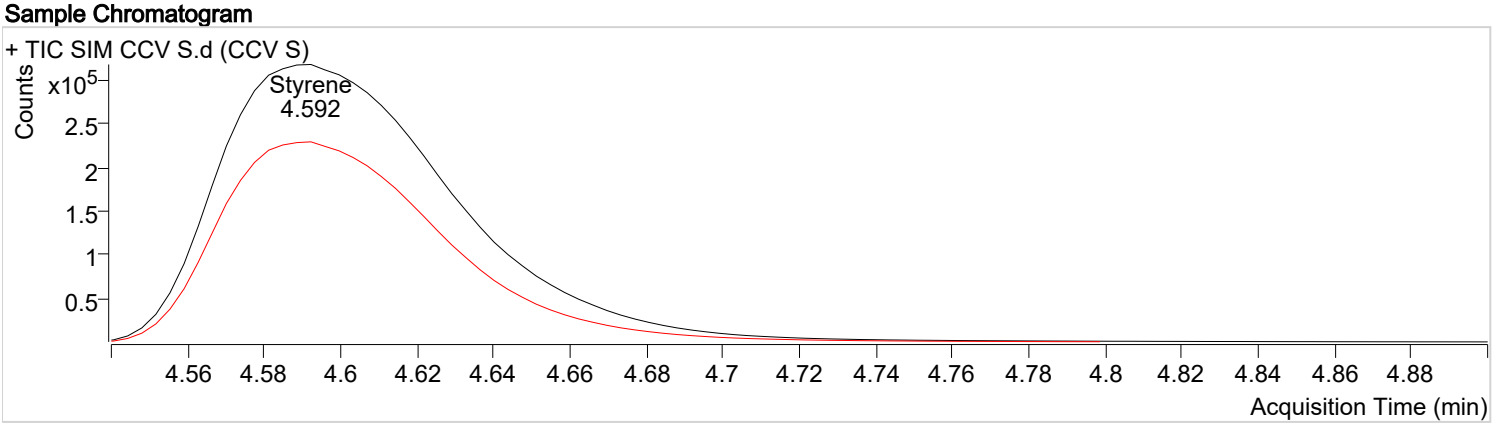

Name	RT	Resp.	Final Conc.	Units
Styrene	4.592	943522	0.218	mg/L
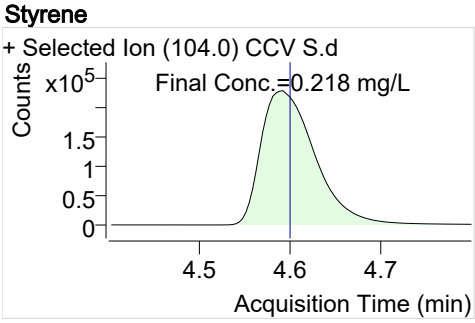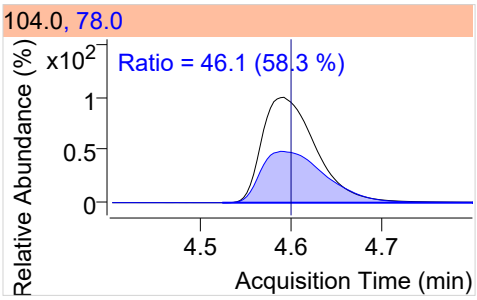
Styrene