Quantitative Analysis Results Summary Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\QuantResults\STY.batch.bin				
Analysis Time	2026-03-23 오전 11:22:43	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:22:43	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Styrene

Data File	Type	RT	Resp.	Final Conc.
STY ST-01.d	Cal	4.629	2826	0.007
STY ST-02.d	Cal	4.611	32858	0.016
STY ST-03.d	Cal	4.603	88015	0.032
STY ST-04.d	Cal	4.592	864272	0.257
STY ST-05.d	Cal	4.589	1694117	0.498
-BK-.d	Blank			ND
FBK(RE 26-03-17).d	Blank			ND
FBK(RE 26-03-18).d	Blank			ND
RE-05.d	Sample			ND
RE-06.d	Sample			ND
RE-13.d	Sample			ND
RE-14.d	Sample			ND
RE-24.d	Sample			ND
RE-25.d	Sample			ND
JR 26-03-19.d	Sample	4.625	0	ND
MBK.d	Blank			ND
STY CCV-.d	QC	4.592	840164	0.250

Styrene

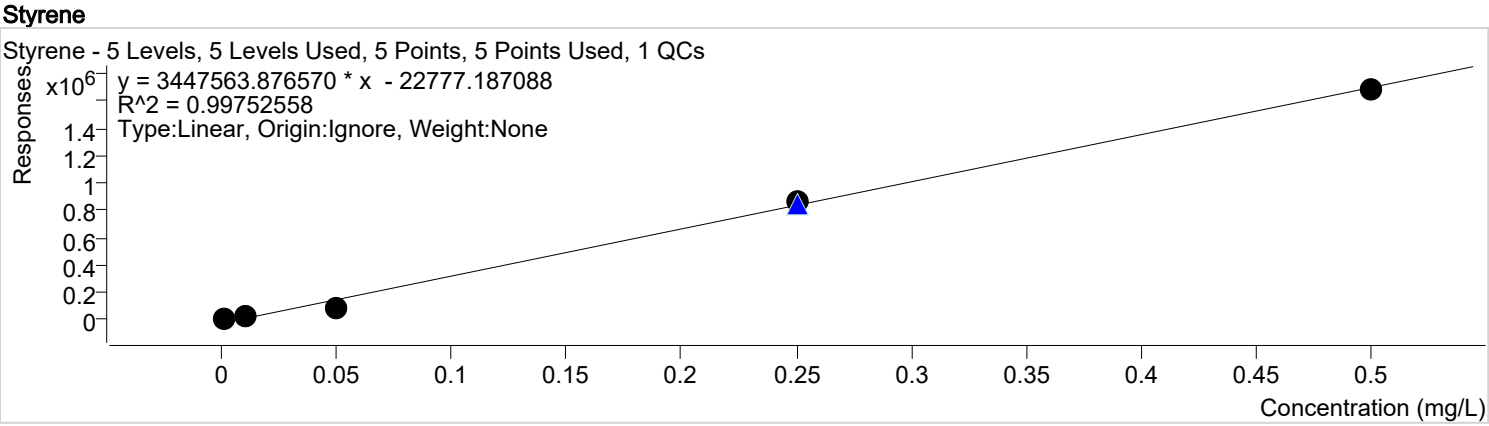

Cal. Path	Type	Level	Enable	Conc.	Response
V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\STY ST-01.d	Calibration	1	x	0.001	2826
V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\STY ST-02.d	Calibration	2	x	0.010	32858
V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\STY ST-03.d	Calibration	3	x	0.050	88015
V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\STY ST-04.d	Calibration	4	x	0.250	864272
V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\STY CCV-.d	QC	4	x	0.250	840164
V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\STY ST-05.d	Calibration	5	x	0.500	1694117

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\QuantResults\STY.batch.bin		
Analysis Time	2026-03-23 오전 11:22:43	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:17:22	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:22:43	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-19 오후 7:56:54	**Data File**	STY ST-01.d
Type	Cal	**Name**	STY ST-01
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

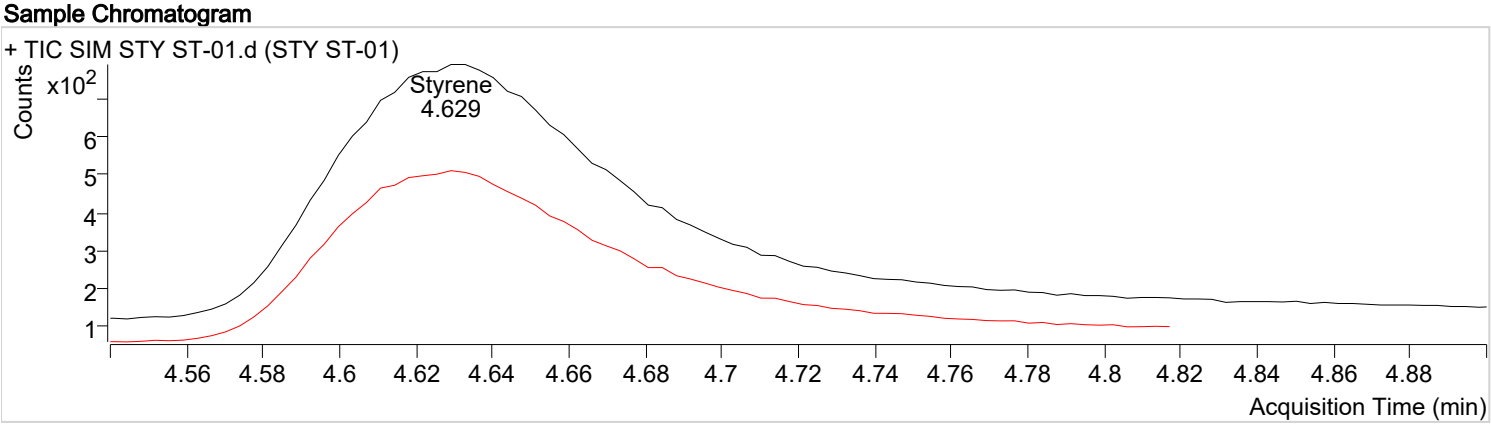

Name	RT	Resp.	Final Conc.	Units
Styrene	4.629	2826	0.007	mg/L

Styrene

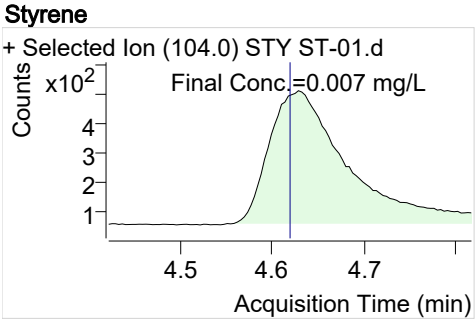

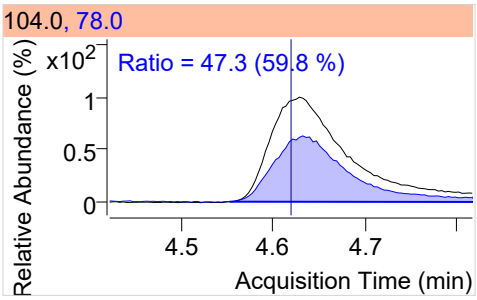

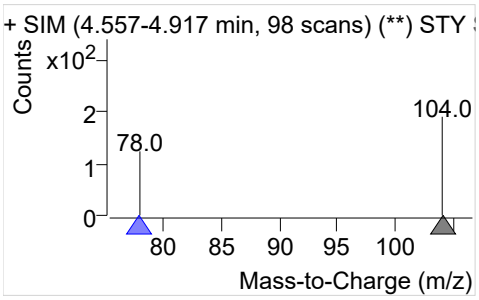

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\QuantResults\STY.batch.bin		
Analysis Time	2026-03-23 오전 11:22:43	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:17:22	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:22:43	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-19 오후 8:13:58	**Data File**	STY ST-02.d
Type	Cal	**Name**	STY ST-02
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

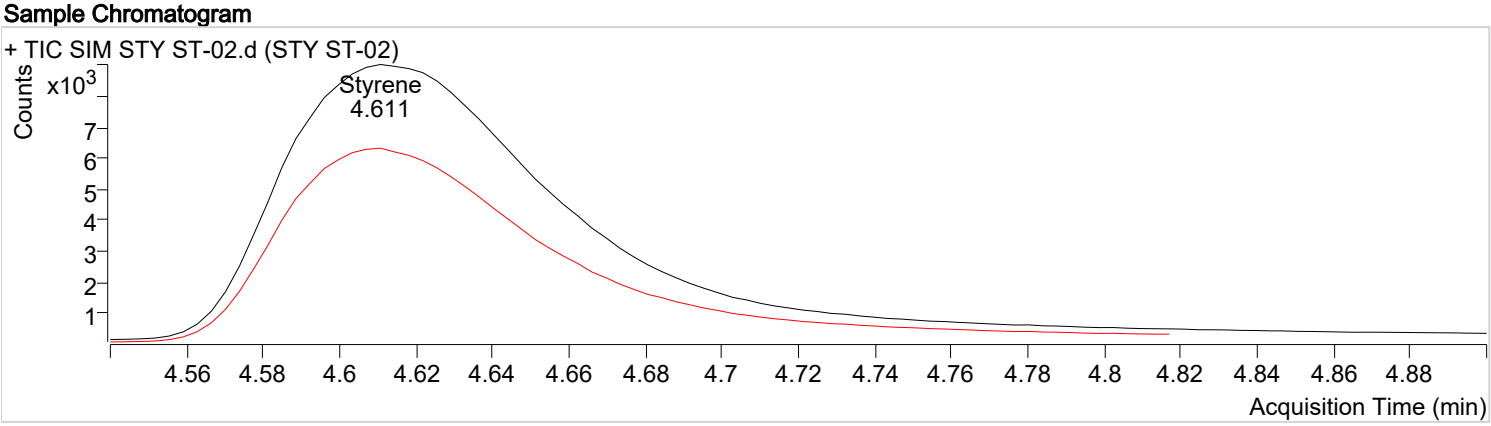

Name	RT	Resp.	Final Conc.	Units
Styrene	4.611	32858	0.016	mg/L

Styrene

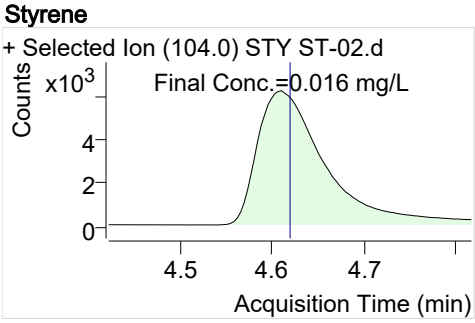



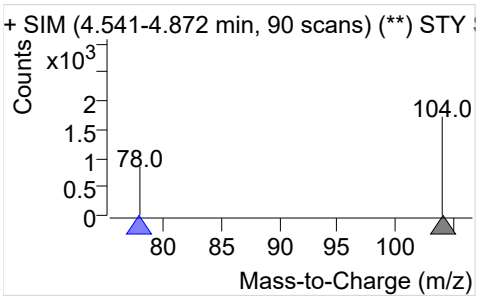

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\QuantResults\STY.batch.bin		
Analysis Time	2026-03-23 오전 11:22:43	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:17:22	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:22:43	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-19 오후 8:31:06	**Data File**	STY ST-03.d
Type	Cal	**Name**	STY ST-03
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

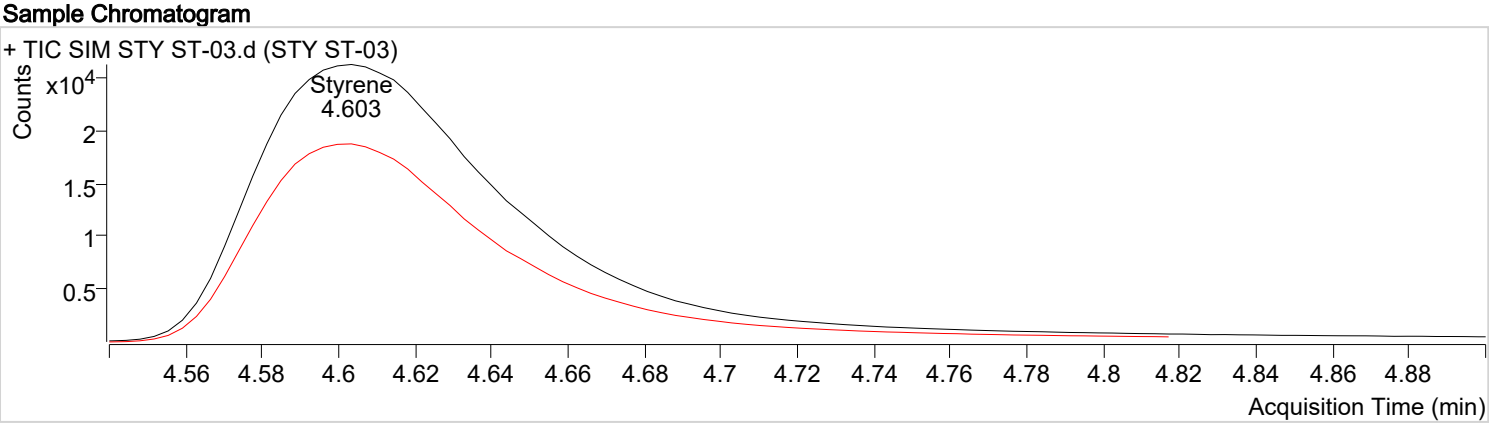

Name	RT	Resp.	Final Conc.	Units
Styrene	4.603	88015	0.032	mg/L

Styrene

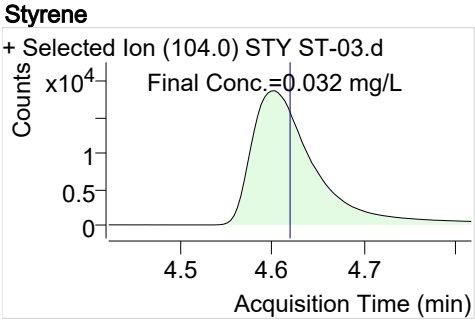



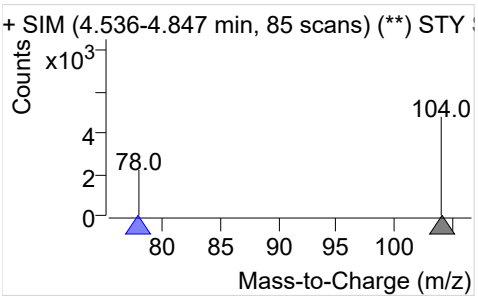

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\QuantResults\STY.batch.bin		
Analysis Time	2026-03-23 오전 11:22:43	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:17:22	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:22:43	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-19 오후 8:48:00	**Data File**	STY ST-04.d
Type	Cal	**Name**	STY ST-04
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

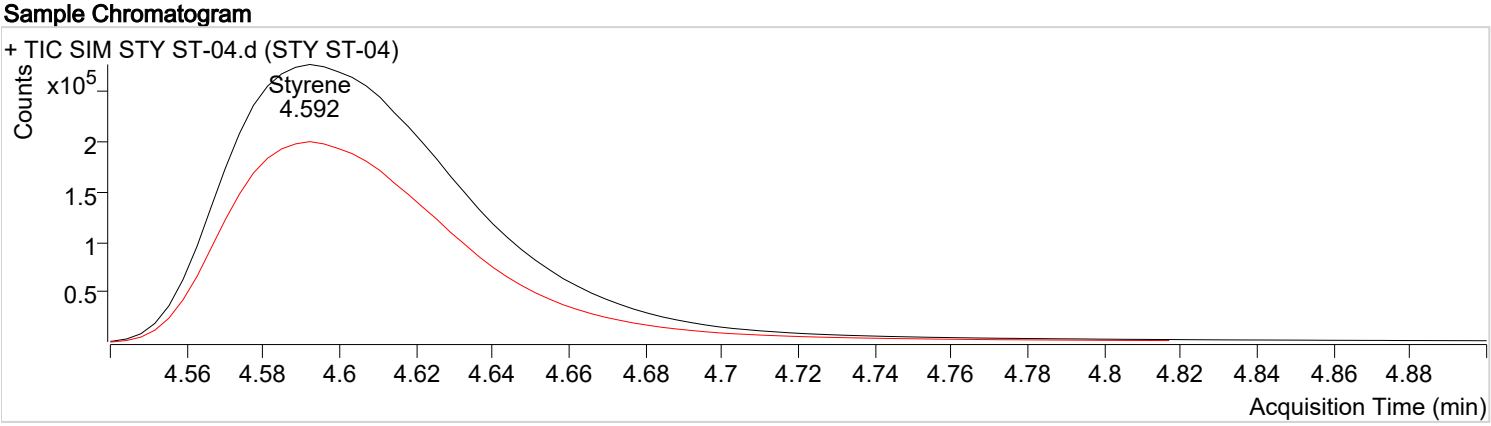

Name	RT	Resp.	Final Conc.	Units
Styrene	4.592	864272	0.257	mg/L

Styrene

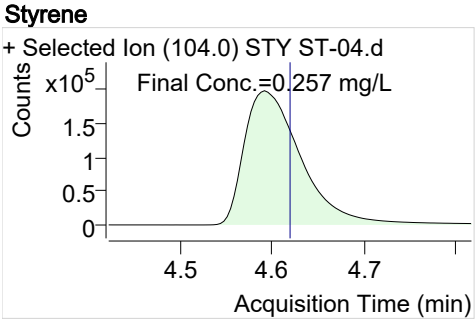

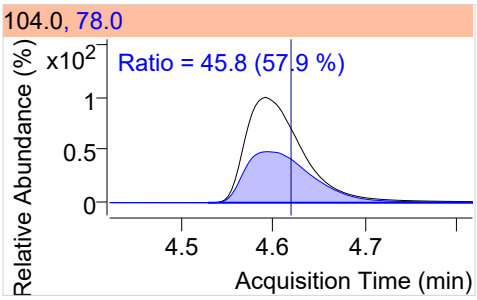

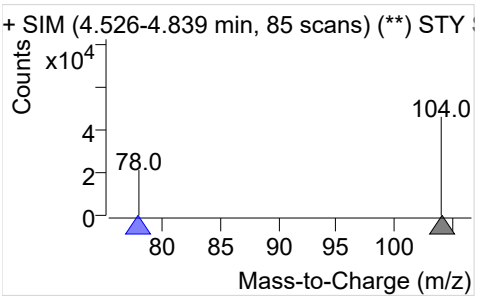

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\QuantResults\STY.batch.bin		
Analysis Time	2026-03-23 오전 11:22:43	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:17:22	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:22:43	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-19 오후 9:05:03	**Data File**	STY ST-05.d
Type	Cal	**Name**	STY ST-05
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

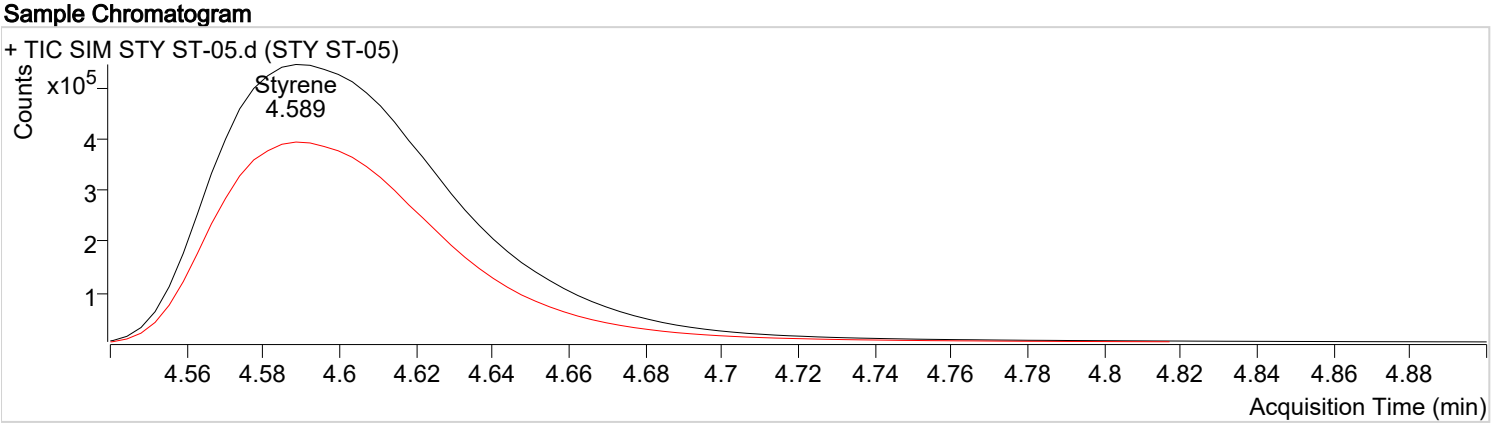

Name	RT	Resp.	Final Conc.	Units
Styrene	4.589	1694117	0.498	mg/L

Styrene

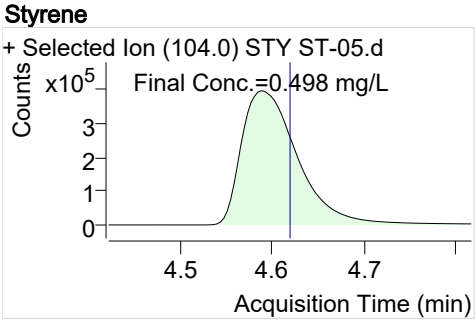

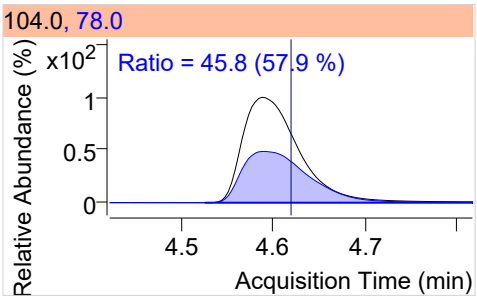

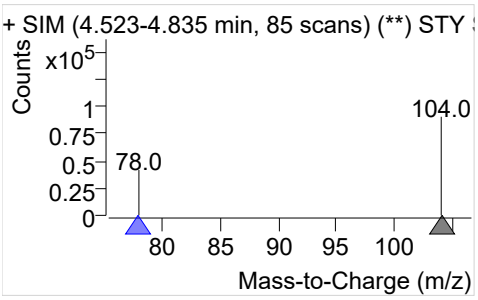

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\QuantResults\STY.batch.bin		
Analysis Time	2026-03-23 오전 11:22:43	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:17:22	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:22:43	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-19 오후 9:39:09	**Data File**	-BK-.d
Type	Blank	**Name**	-BK-
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

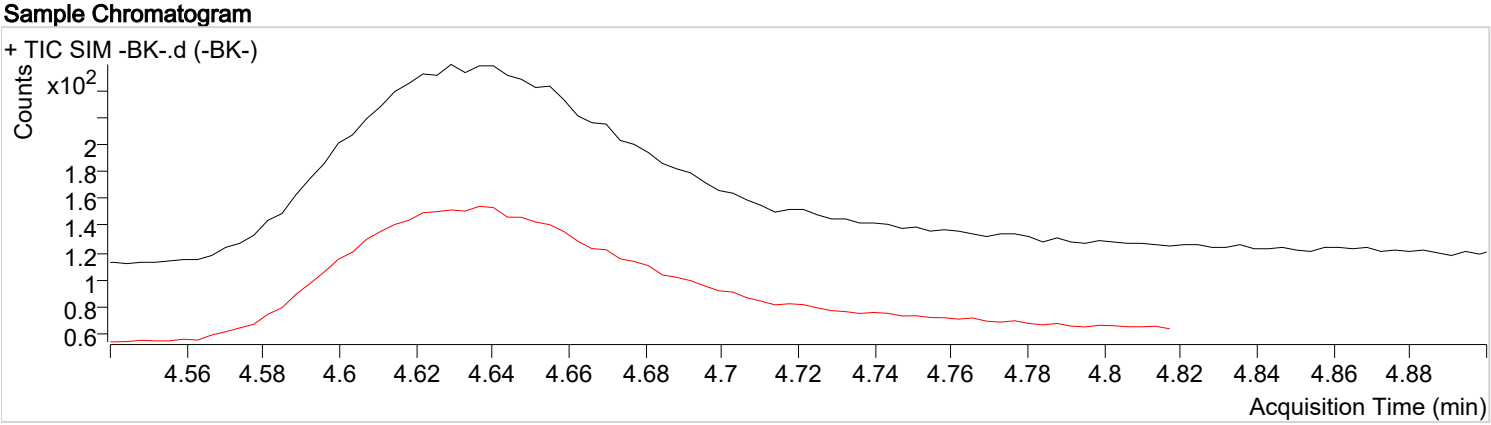

Styrene





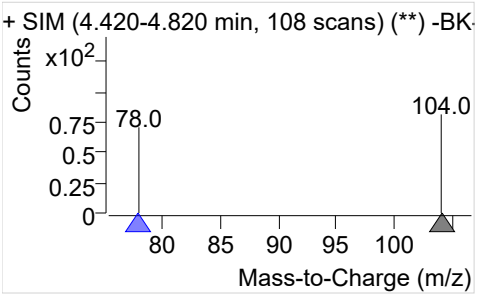

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\QuantResults\STY.batch.bin		
Analysis Time	2026-03-23 오전 11:22:43	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:17:22	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:22:43	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-19 오후 9:56:14	**Data File**	FBK(RE 26-03-17).d
Type	Blank	**Name**	FBK(RE 26-03-17)
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

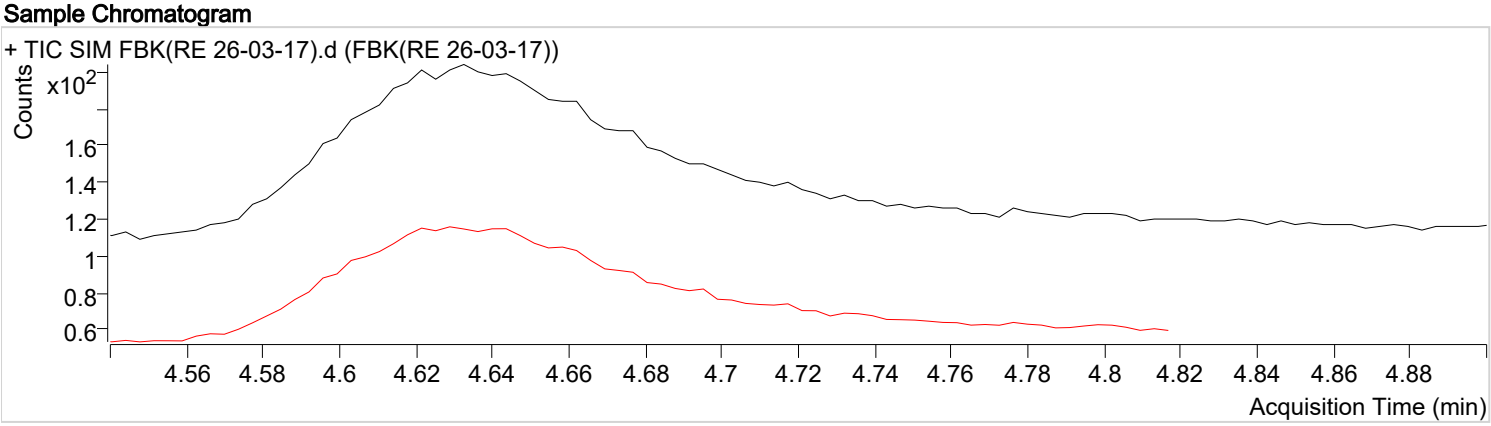

Styrene





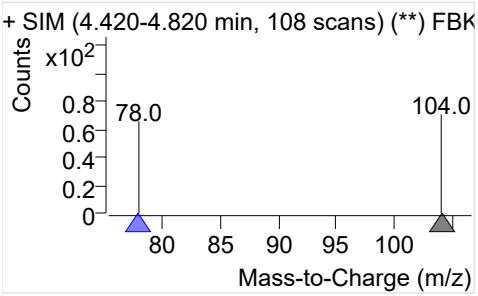

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\QuantResults\STY.batch.bin		
Analysis Time	2026-03-23 오전 11:22:43	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:17:22	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:22:43	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-19 오후 10:13:16	**Data File**	FBK(RE 26-03-18).d
Type	Blank	**Name**	FBK(RE 26-03-18)
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

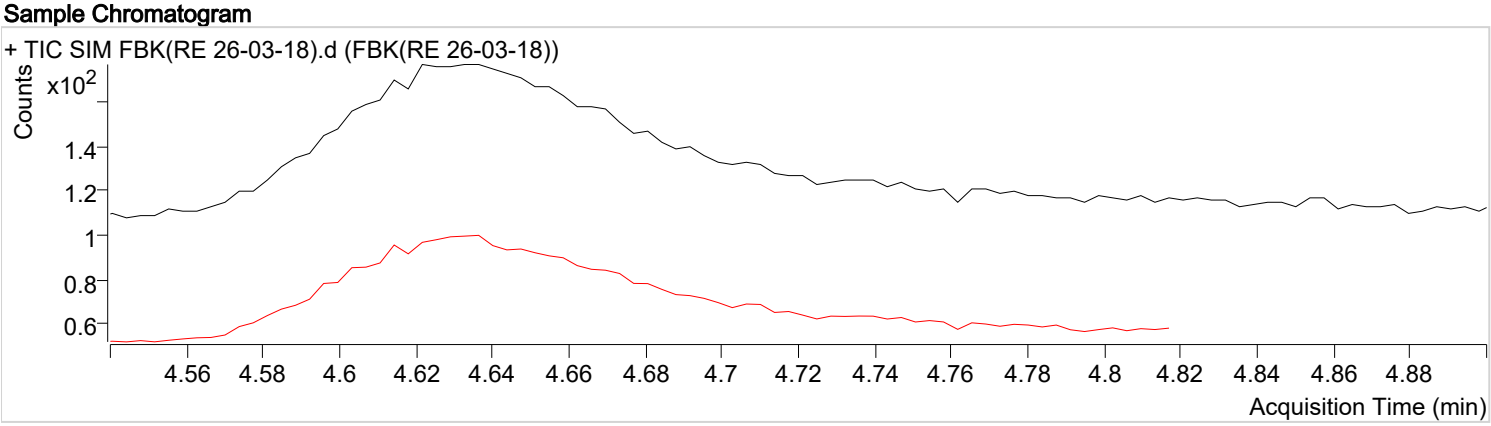

Styrene





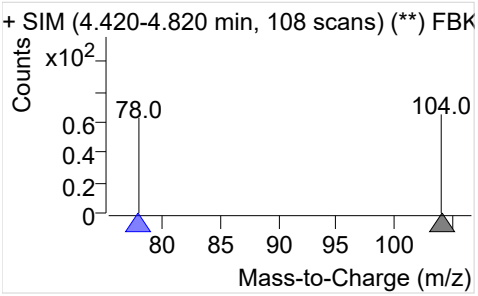

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\QuantResults\STY.batch.bin		
Analysis Time	2026-03-23 오전 11:22:43	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:17:22	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:22:43	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-19 오후 10:30:20	**Data File**	RE-05.d
Type	Sample	**Name**	RE-05
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

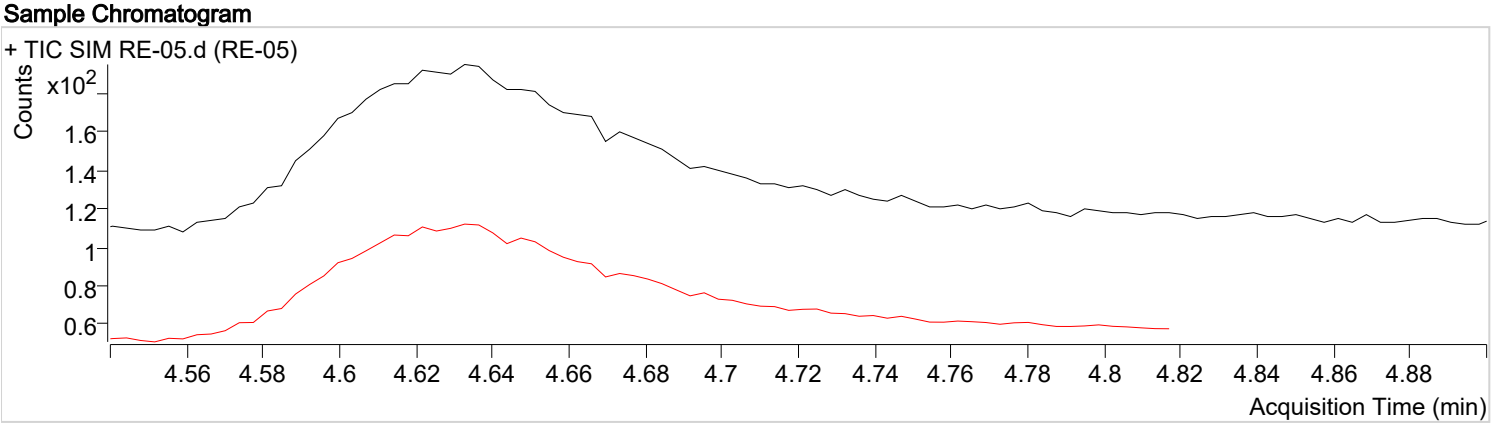

Styrene





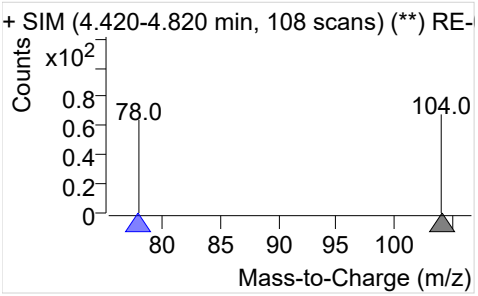

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\QuantResults\STY.batch.bin		
Analysis Time	2026-03-23 오전 11:22:43	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:17:22	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:22:43	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-19 오후 10:47:26	**Data File**	RE-06.d
Type	Sample	**Name**	RE-06
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

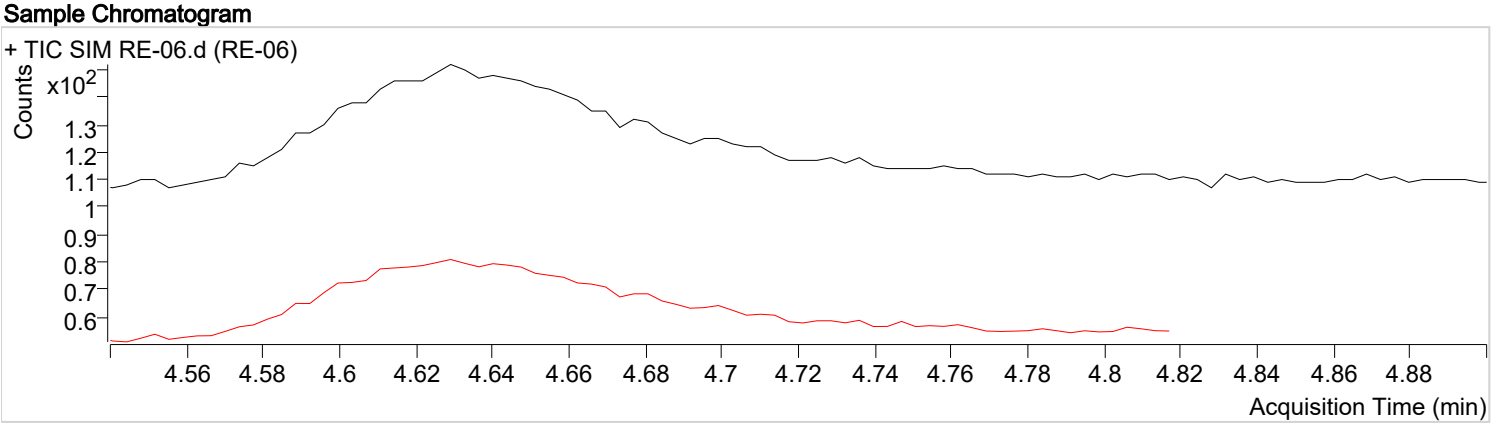

Styrene





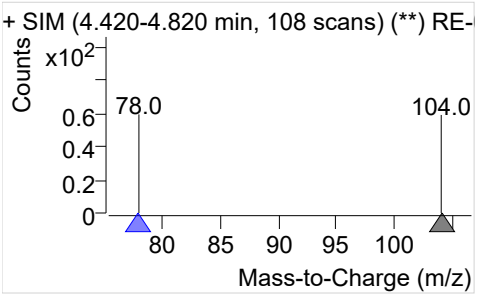

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\QuantResults\STY.batch.bin		
Analysis Time	2026-03-23 오전 11:22:43	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:17:22	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:22:43	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-19 오후 11:04:31	**Data File**	RE-13.d
Type	Sample	**Name**	RE-13
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

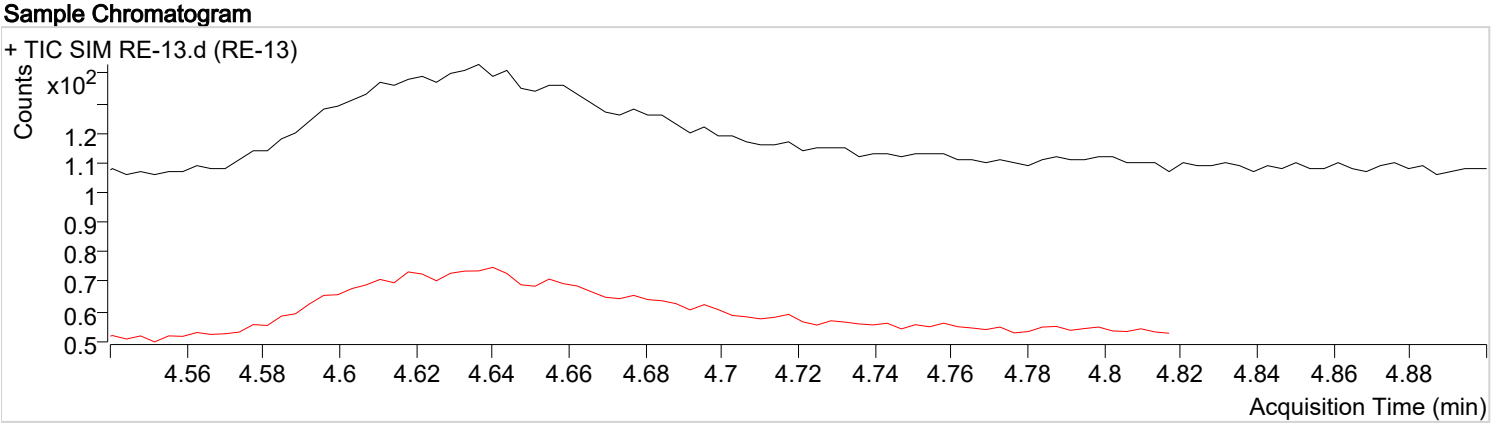

Styrene





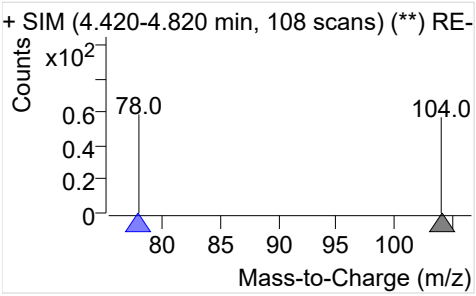

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\QuantResults\STY.batch.bin		
Analysis Time	2026-03-23 오전 11:22:43	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:17:22	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:22:43	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-19 오후 11:21:28	**Data File**	RE-14.d
Type	Sample	**Name**	RE-14
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

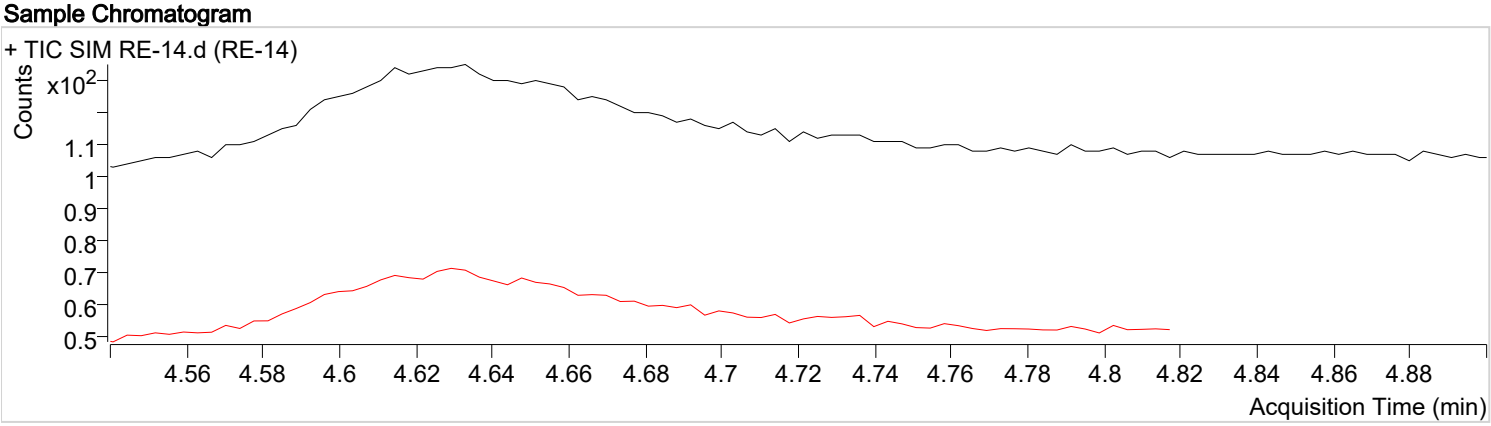

Styrene





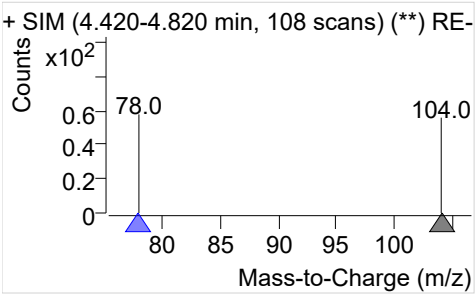

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\QuantResults\STY.batch.bin		
Analysis Time	2026-03-23 오전 11:22:43	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:17:22	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:22:43	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-19 오후 11:38:34	**Data File**	RE-24.d
Type	Sample	**Name**	RE-24
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

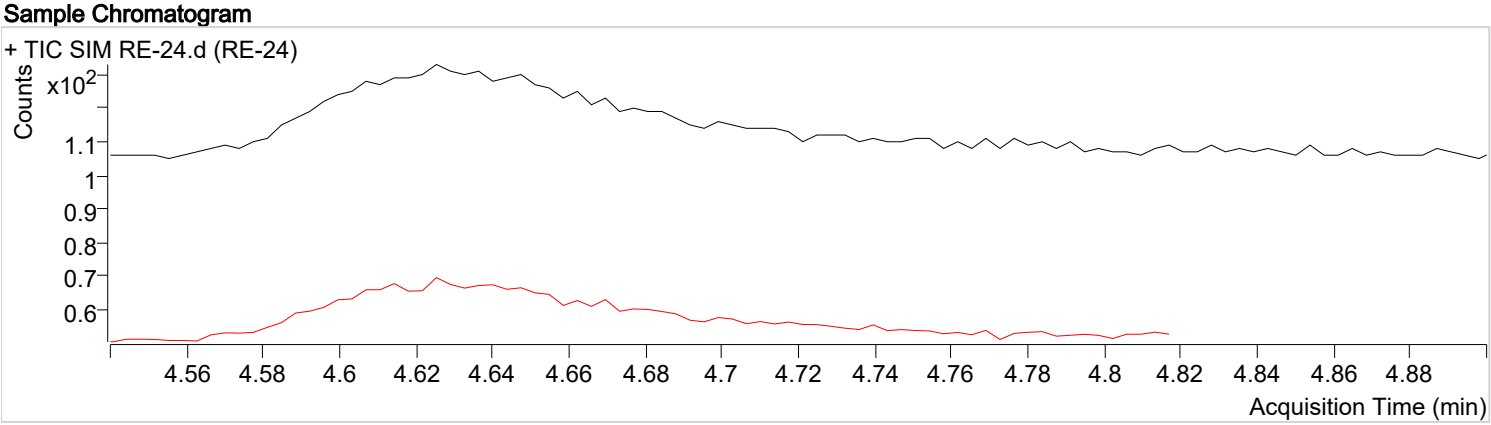

Styrene





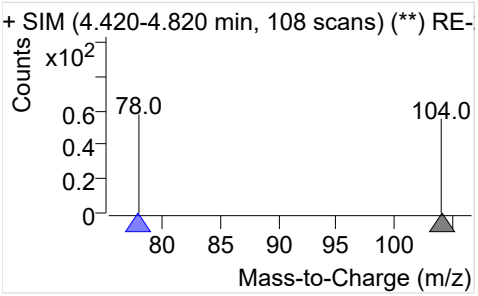

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\QuantResults\STY.batch.bin		
Analysis Time	2026-03-23 오전 11:22:43	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:17:22	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:22:43	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-19 오후 11:55:38	**Data File**	RE-25.d
Type	Sample	**Name**	RE-25
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

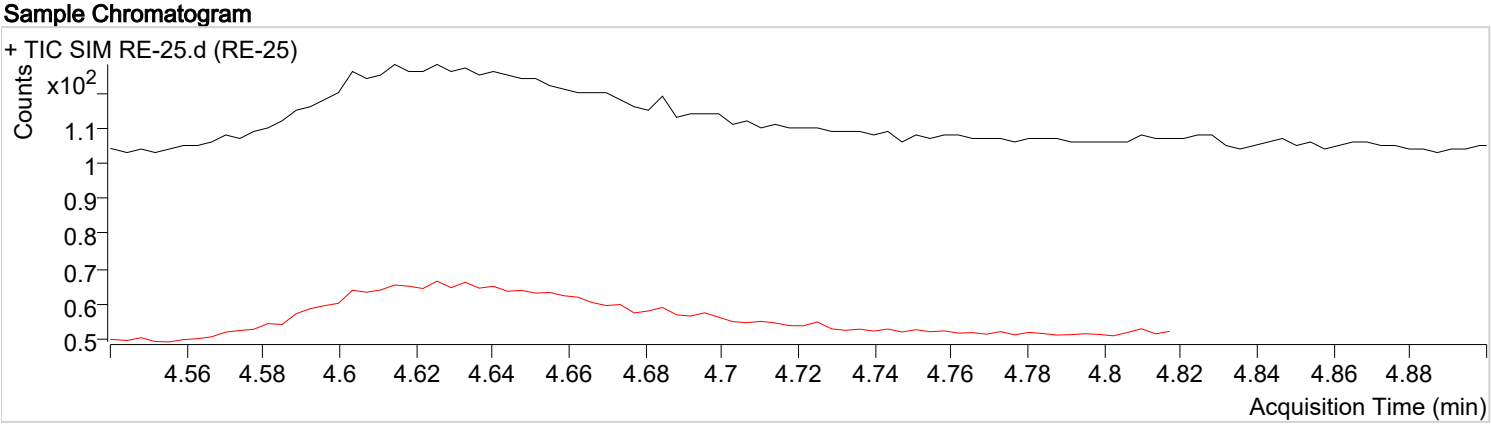

Styrene





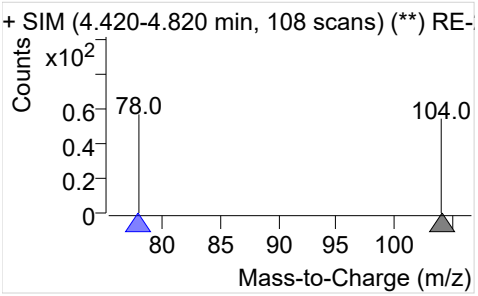

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\QuantResults\STY.batch.bin		
Analysis Time	2026-03-23 오전 11:22:43	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:17:22	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:22:43	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오전 12:12:42	**Data File**	JR 26-03-19.d
Type	Sample	**Name**	JR 26-03-19
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

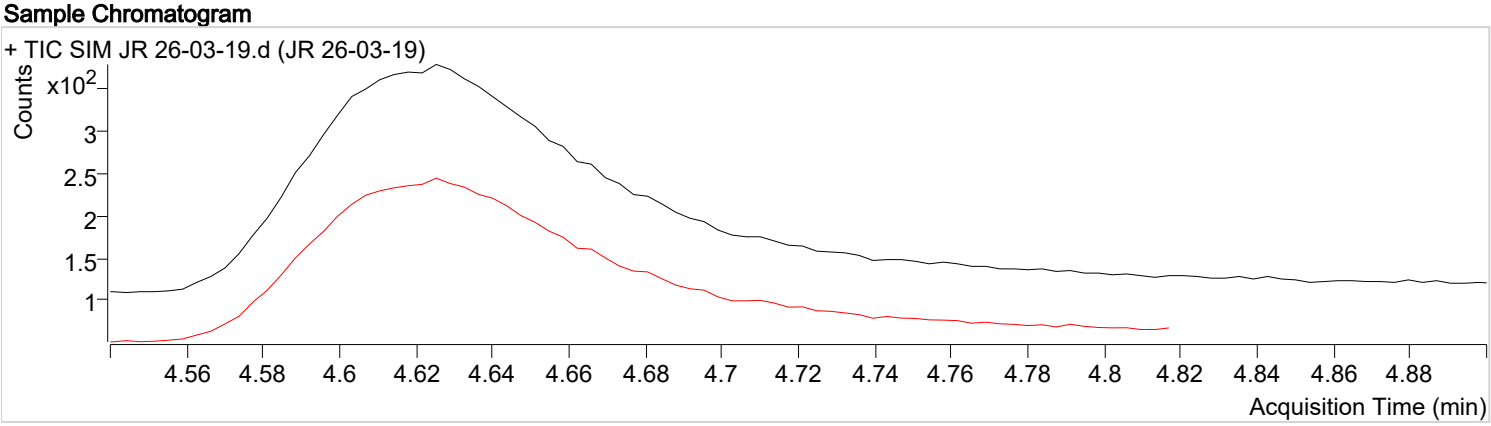

Styrene





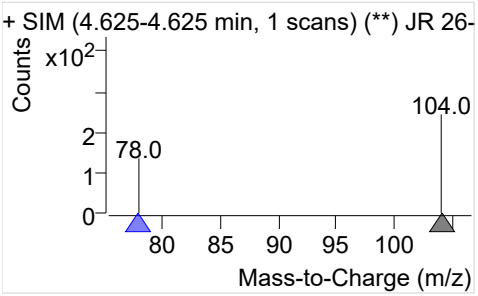

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\QuantResults\STY.batch.bin		
Analysis Time	2026-03-23 오전 11:22:43	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:17:22	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:22:43	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오전 12:29:48	**Data File**	MBK.d
Type	Blank	**Name**	MBK
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

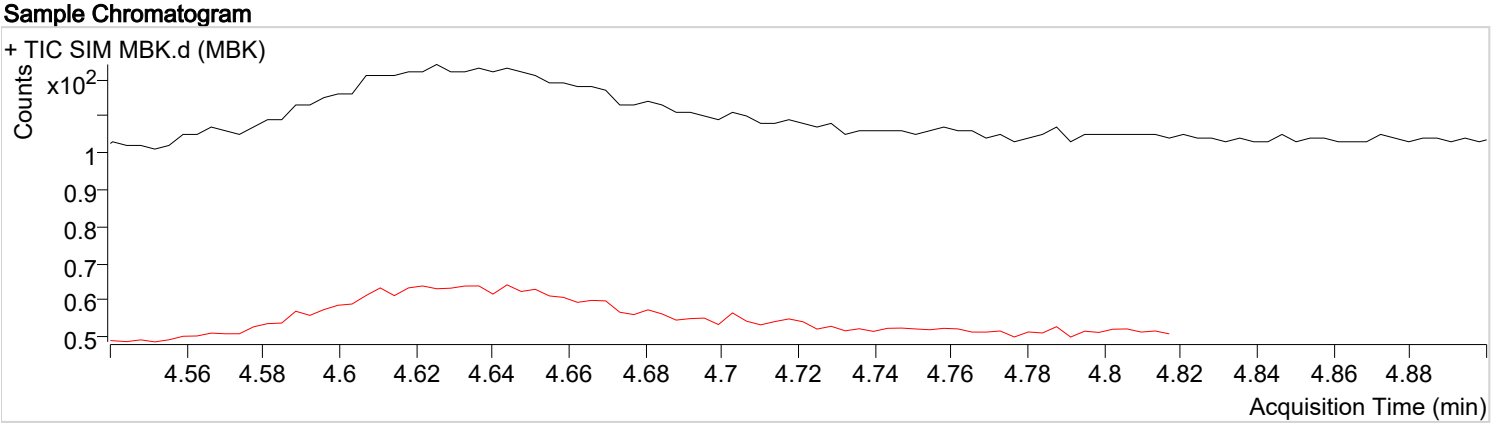

Styrene





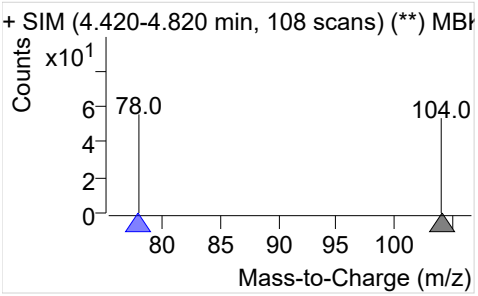

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(RE 3.17 RE3.18 JR 3.19)\QuantResults\STY.batch.bin		
Analysis Time	2026-03-23 오전 11:22:43	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:17:22	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:22:43	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오전 1:37:52	**Data File**	STY CCV-.d
Type	QC	**Name**	STY CCV-
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

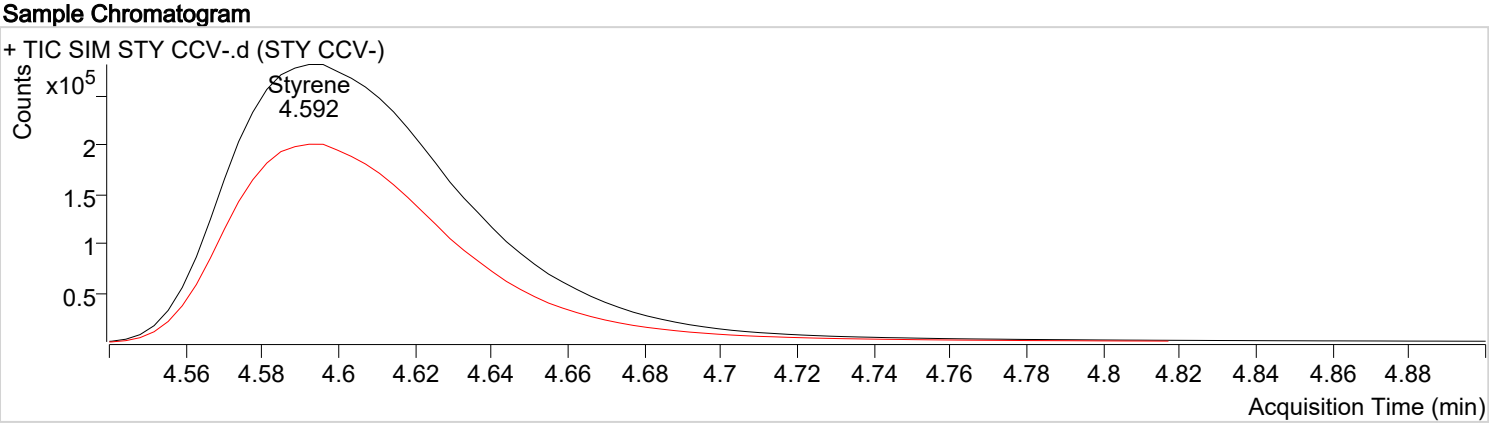

Name	RT	Resp.	Final Conc.	Units
Styrene	4.592	840164	0.250	mg/L
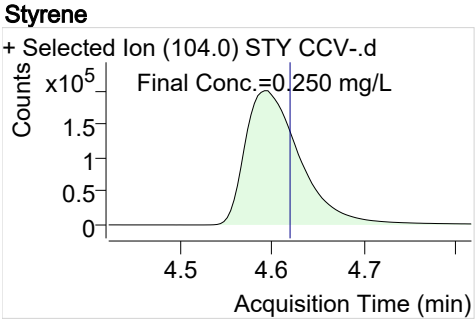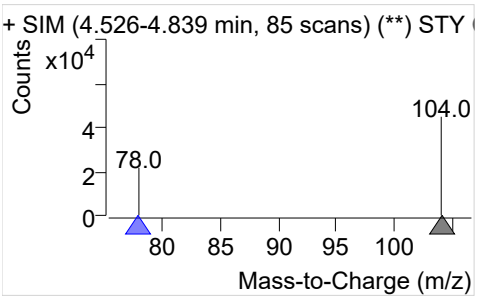
Styrene