Quantitative Analysis Results Summary Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\ST.batch.bin				
Analysis Time	2026-04-01 오후 4:42:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:42:37	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Styrene

Data File	Type	RT	Resp.	Final Conc.
STY ST-01.d	Cal	4.611	790	0.005
STY ST-02.d	Cal	4.603	8667	0.008
STY ST-03.d	Cal	4.603	99877	0.044
STY ST-04.d	Cal	4.596	641986	0.256
STY ST-05.d	Cal	4.589	1262924	0.498
BK-.d	Blank			ND
FBK(NK 26-03-26).d	Blank			ND
NJ-01.d	Sample			ND
NJ-02.d	Sample			ND
NJ-03.d	Sample			ND
NJ-04.d	Sample			ND
NJ-05.d	Sample			ND
NJ-06.d	Sample			ND
MBK.d	Blank			ND
-CCV-S.d	QC	4.596	685902	0.273

Styrene

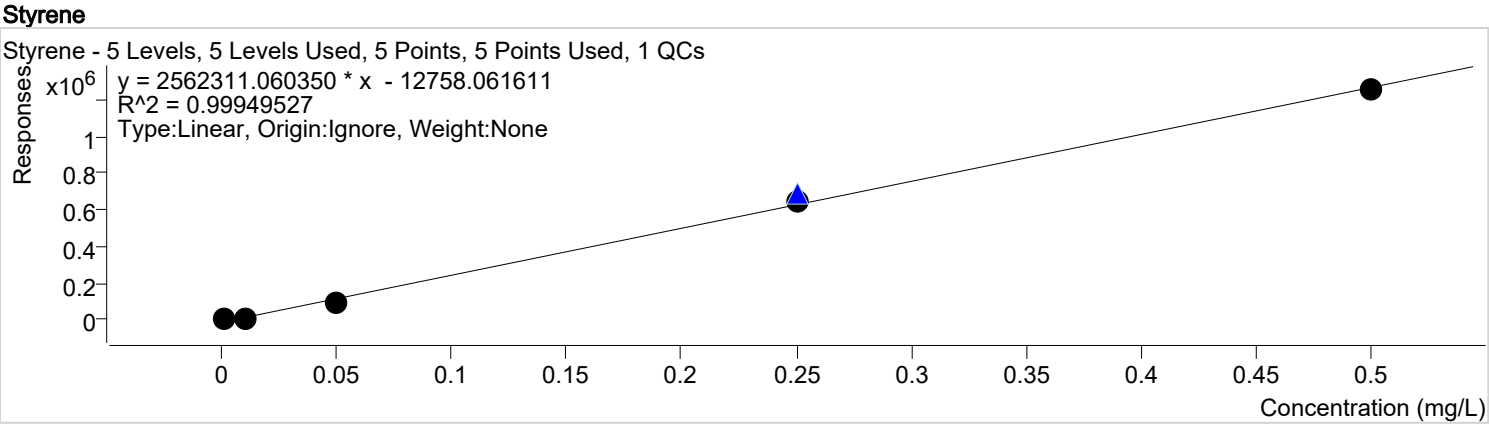

Cal. Path	Type	Level	Enable	Conc.	Response
V:\2026\2026-03\VOC2(NJ 3.26)\STY ST-01.d	Calibration	1	x	0.001	790
V:\2026\2026-03\VOC2(NJ 3.26)\STY ST-02.d	Calibration	2	x	0.010	8667
V:\2026\2026-03\VOC2(NJ 3.26)\STY ST-03.d	Calibration	3	x	0.050	99877
V:\2026\2026-03\VOC2(NJ 3.26)\STY ST-04.d	Calibration	4	x	0.250	641986
V:\2026\2026-03\VOC2(NJ 3.26)\-CCV-S.d	QC	4	x	0.250	685902
V:\2026\2026-03\VOC2(NJ 3.26)\STY ST-05.d	Calibration	5	x	0.500	1262924

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\ST.batch.bin		
Analysis Time	2026-04-01 오후 4:42:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:14:47	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:42:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-30 오후 4:17:03	**Data File**	STY ST-01.d
Type	Cal	**Name**	STY ST-01
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

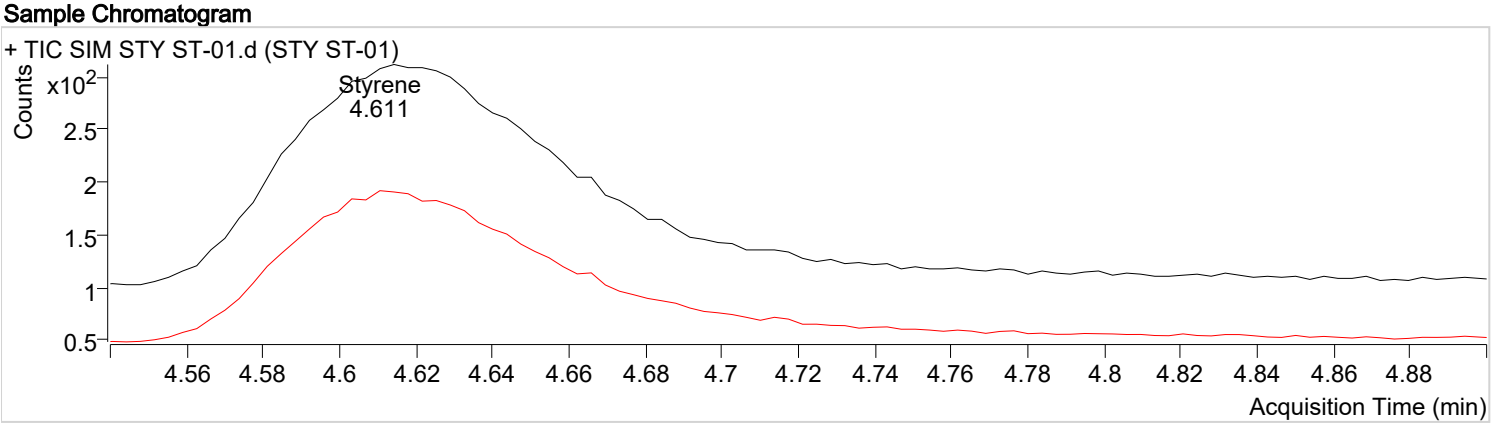

Name	RT	Resp.	Final Conc.	Units
Styrene	4.611	790	0.005	mg/L

Styrene

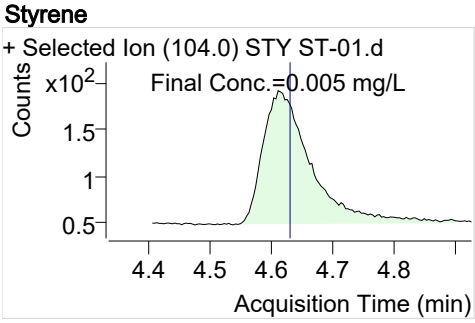



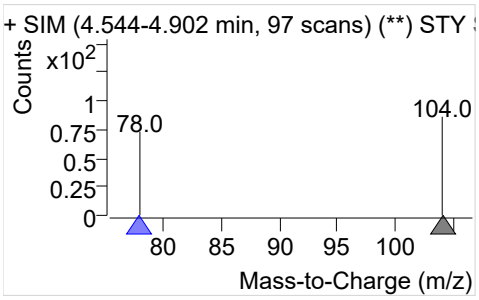

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\ST.batch.bin		
Analysis Time	2026-04-01 오후 4:42:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:14:47	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:42:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-30 오후 4:34:04	**Data File**	STY ST-02.d
Type	Cal	**Name**	STY ST-02
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

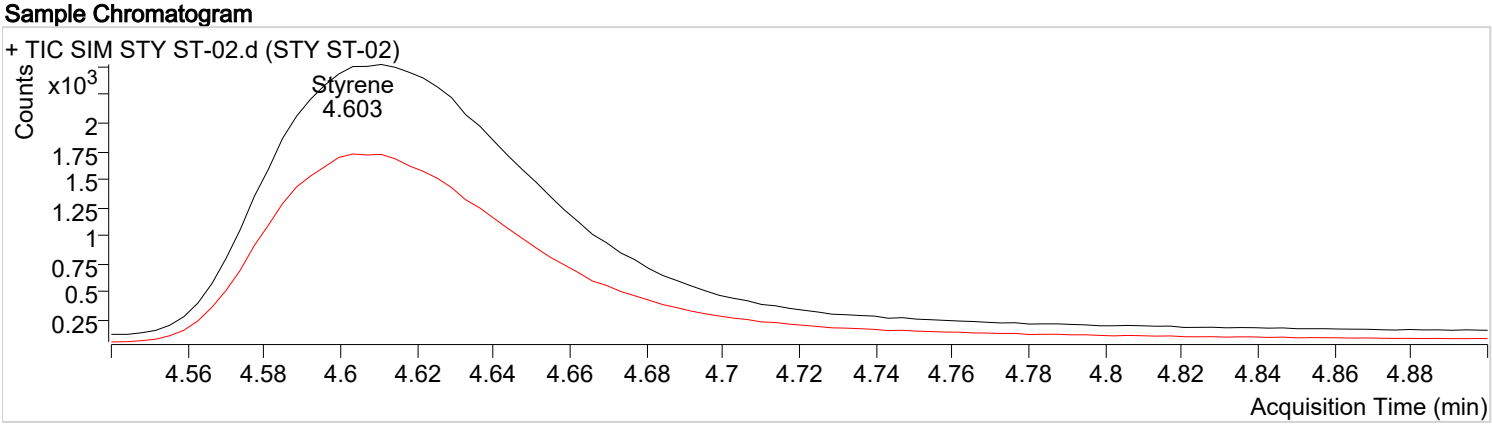

Name	RT	Resp.	Final Conc.	Units
Styrene	4.603	8667	0.008	mg/L

Styrene

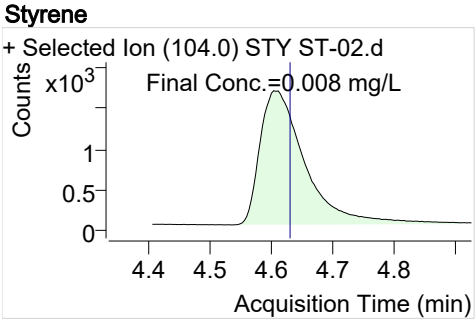

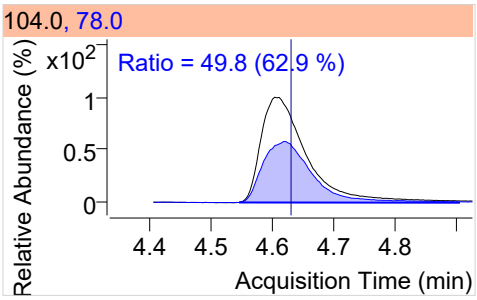

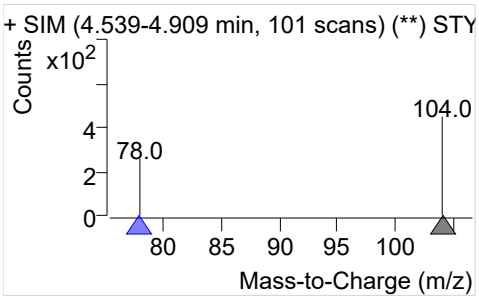

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\ST.batch.bin		
Analysis Time	2026-04-01 오후 4:42:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:14:47	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:42:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-30 오후 4:51:08	**Data File**	STY ST-03.d
Type	Cal	**Name**	STY ST-03
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

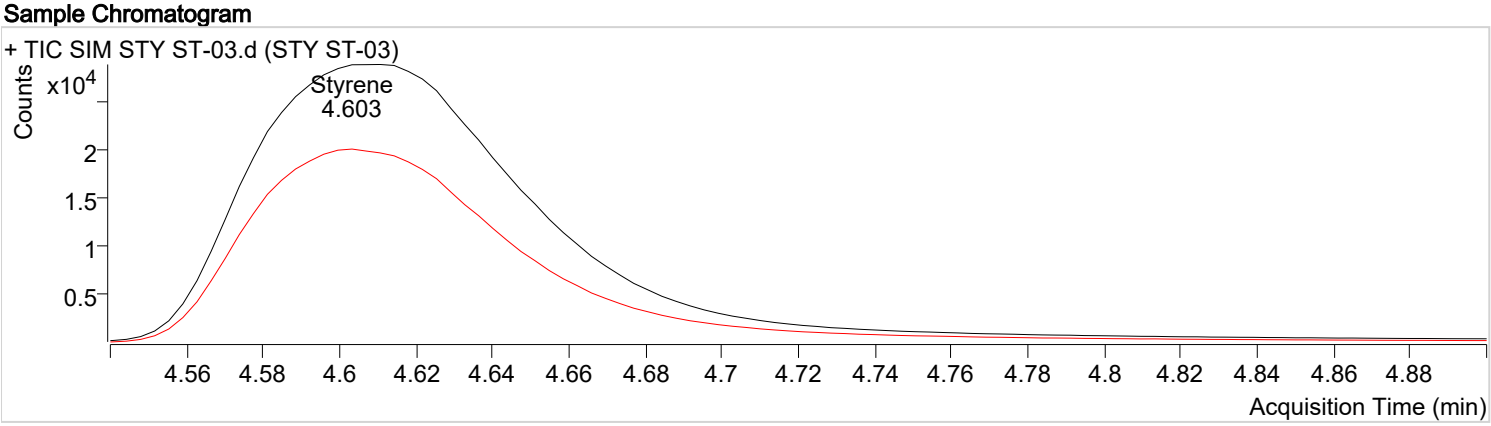

Name	RT	Resp.	Final Conc.	Units
Styrene	4.603	99877	0.044	mg/L

Styrene

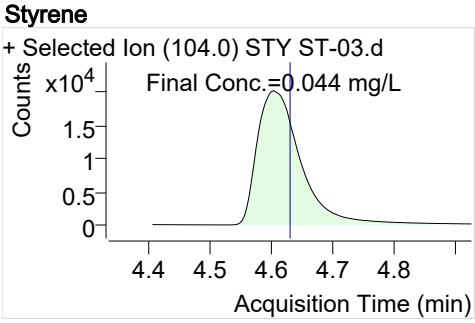

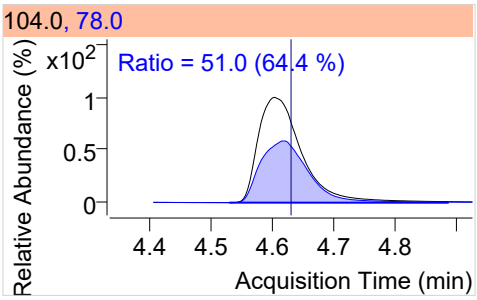

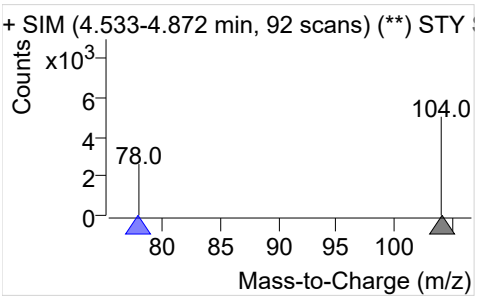

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\ST.batch.bin		
Analysis Time	2026-04-01 오후 4:42:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:14:47	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:42:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-30 오후 5:08:10	**Data File**	STY ST-04.d
Type	Cal	**Name**	STY ST-04
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

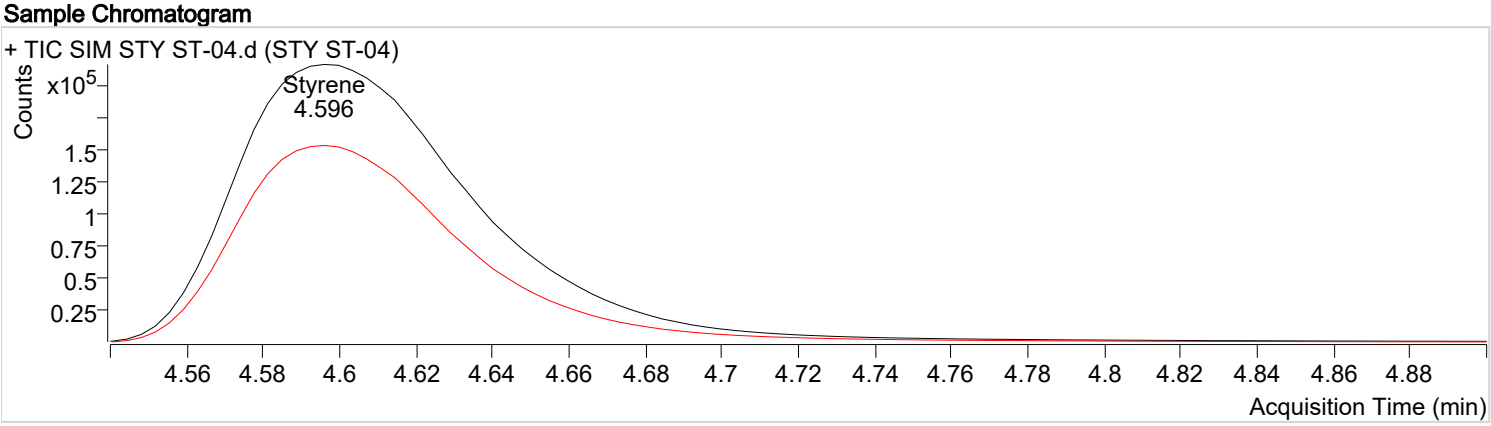

Name	RT	Resp.	Final Conc.	Units
Styrene	4.596	641986	0.256	mg/L

Styrene

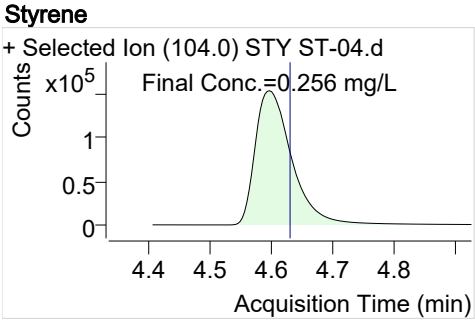



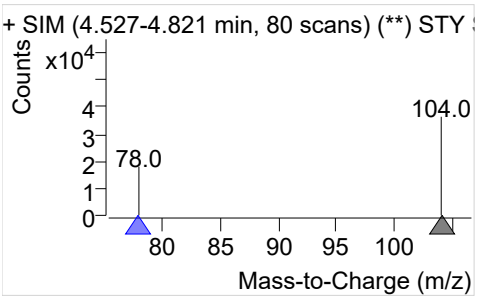

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\ST.batch.bin		
Analysis Time	2026-04-01 오후 4:42:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:14:47	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:42:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-30 오후 5:25:13	**Data File**	STY ST-05.d
Type	Cal	**Name**	STY ST-05
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

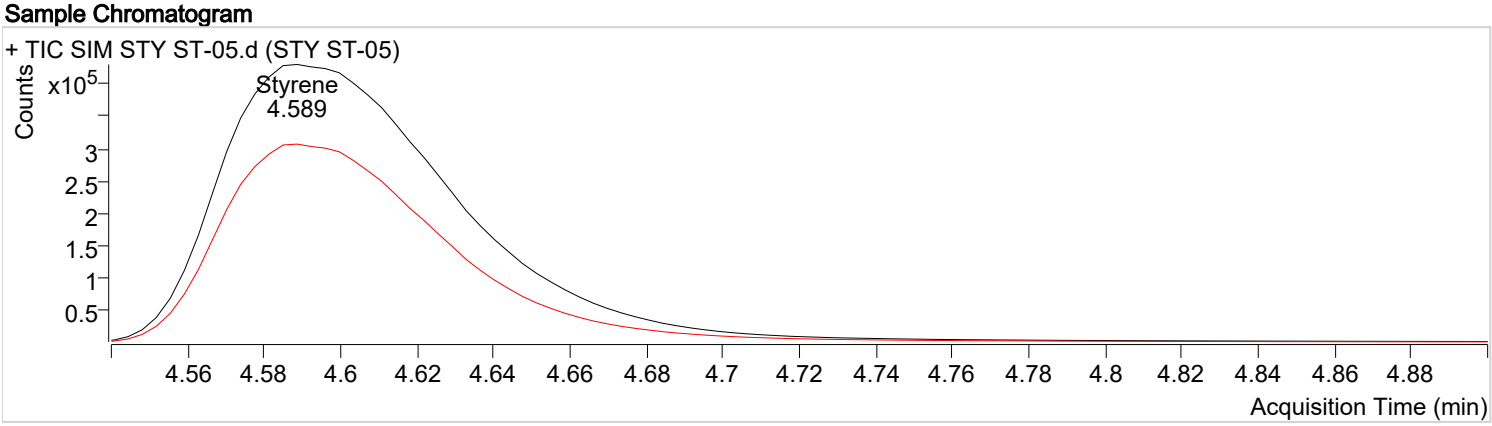

Name	RT	Resp.	Final Conc.	Units
Styrene	4.589	1262924	0.498	mg/L

Styrene

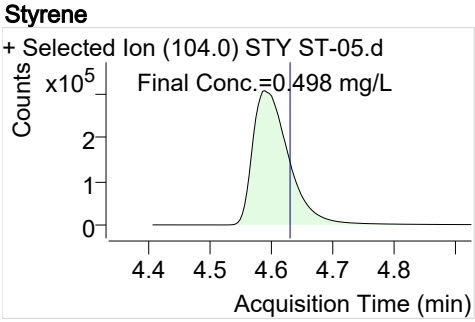

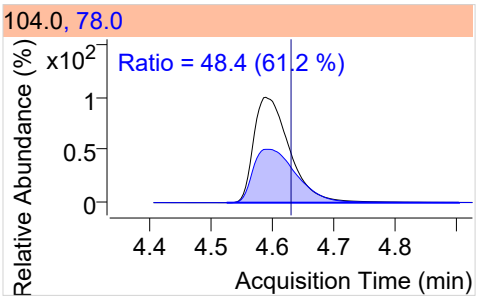

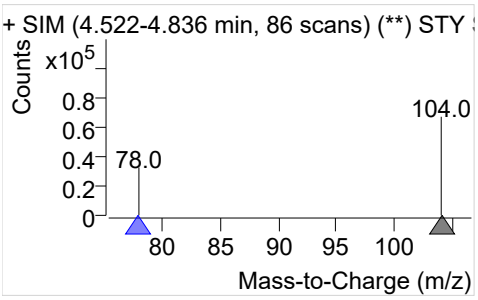

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\ST.batch.bin		
Analysis Time	2026-04-01 오후 4:42:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:14:47	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:42:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-30 오후 5:59:19	**Data File**	BK-.d
Type	Blank	**Name**	BK-
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

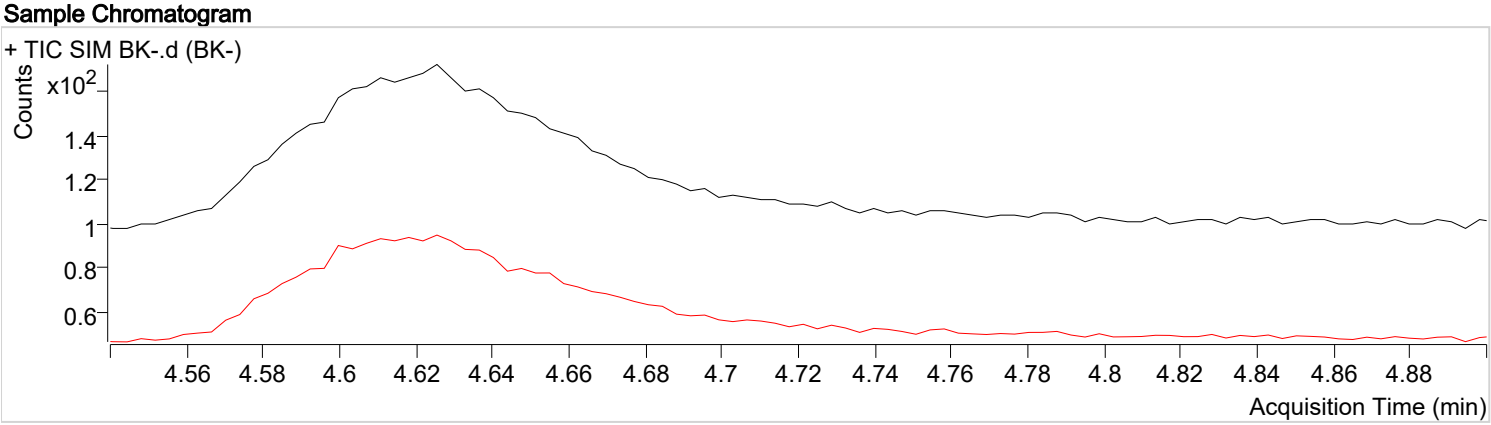

Styrene

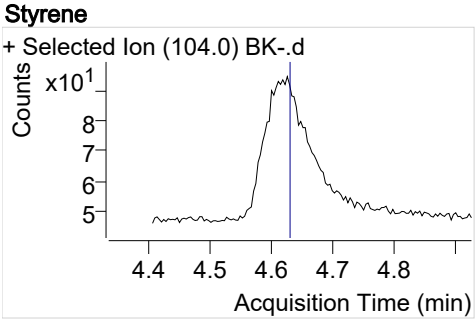



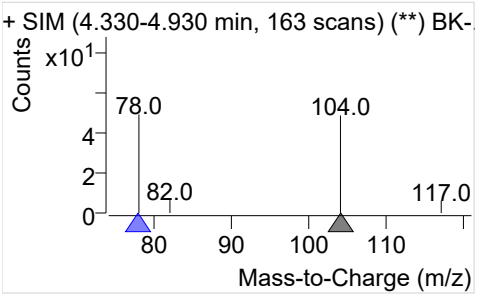

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\ST.batch.bin		
Analysis Time	2026-04-01 오후 4:42:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:14:47	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:42:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-30 오후 6:16:20	**Data File**	FBK(NK 26-03-26).d
Type	Blank	**Name**	FBK(NK 26-03-26)
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

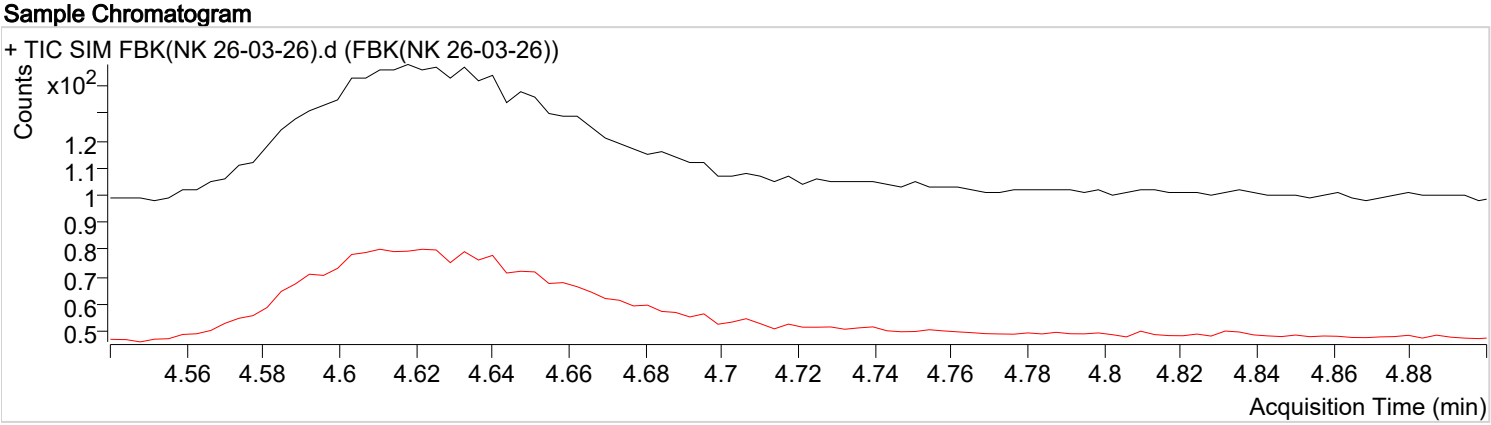

Styrene

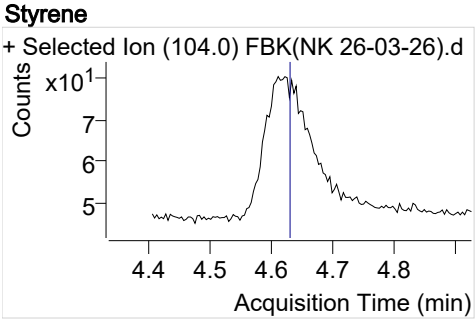



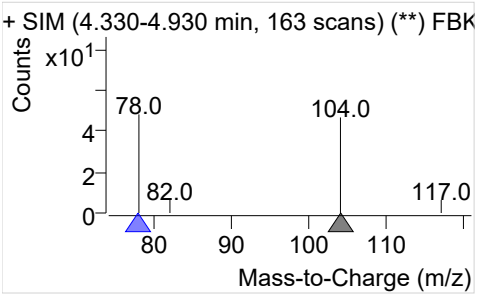

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\ST.batch.bin		
Analysis Time	2026-04-01 오후 4:42:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:14:47	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:42:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-30 오후 6:33:23	**Data File**	NJ-01.d
Type	Sample	**Name**	NJ-01
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

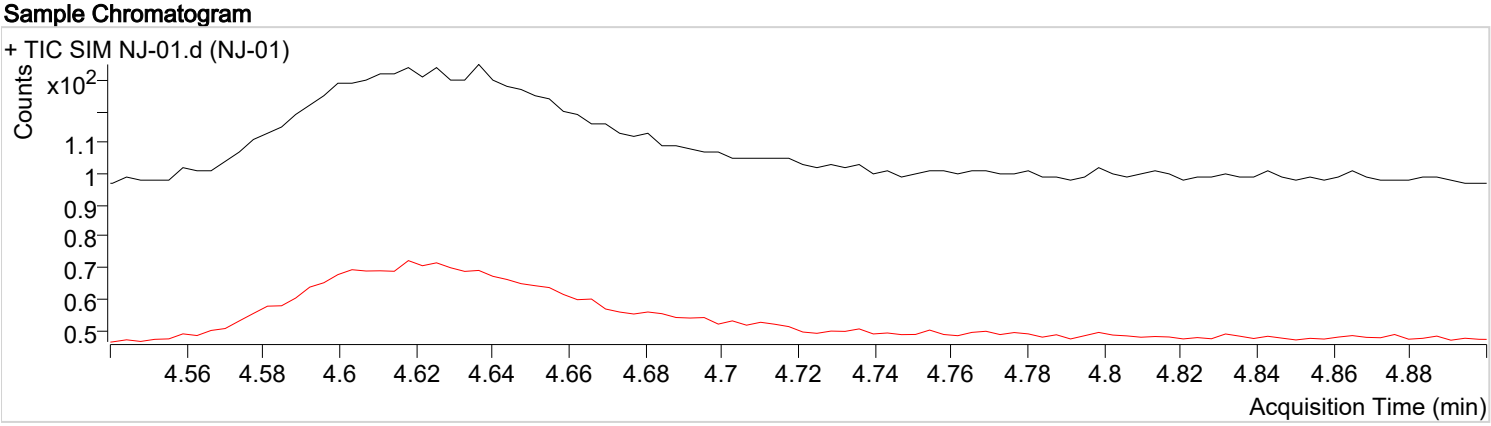

Styrene

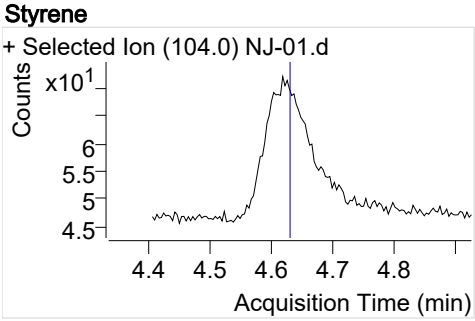



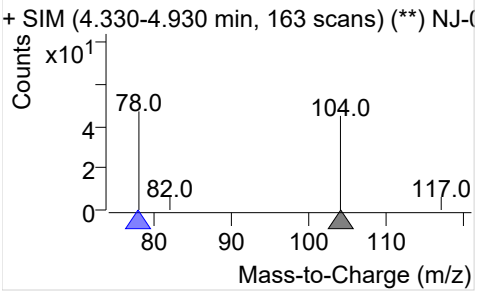

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\ST.batch.bin		
Analysis Time	2026-04-01 오후 4:42:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:14:47	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:42:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-30 오후 6:50:26	**Data File**	NJ-02.d
Type	Sample	**Name**	NJ-02
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

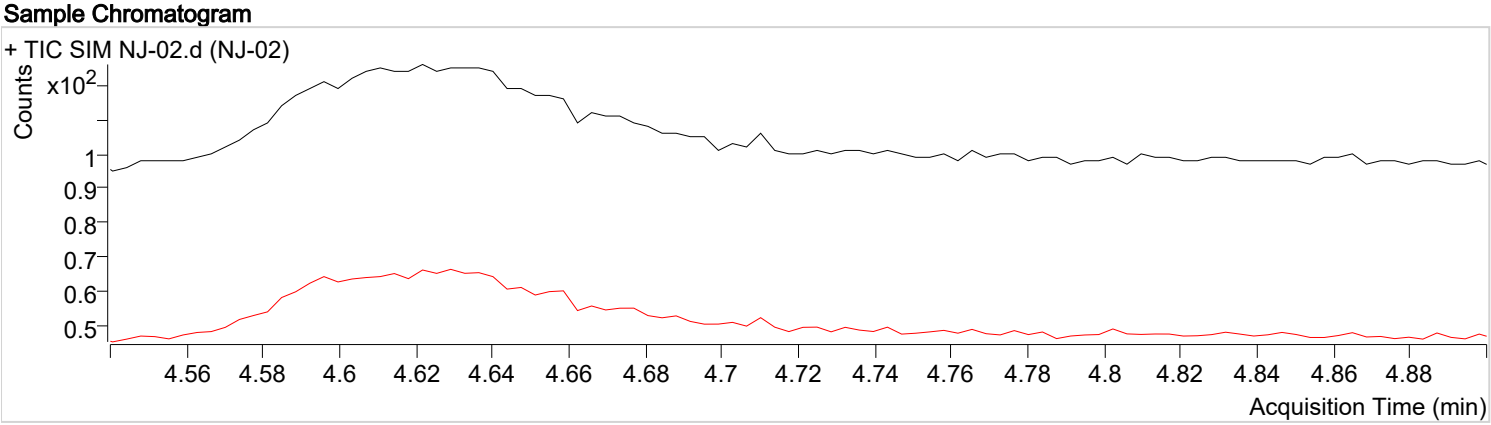

Styrene

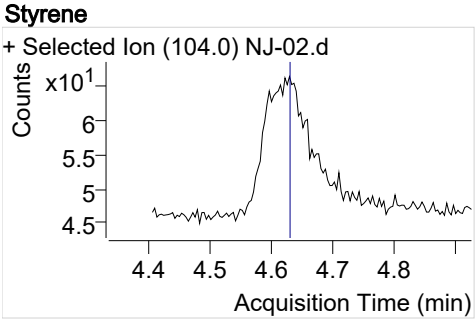



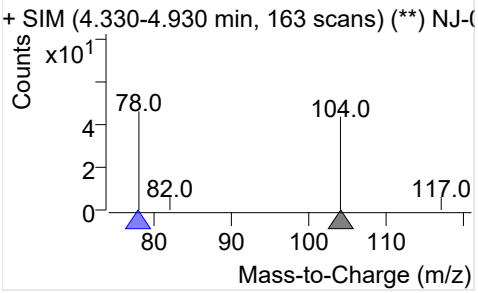

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\ST.batch.bin		
Analysis Time	2026-04-01 오후 4:42:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:14:47	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:42:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-30 오후 7:07:32	**Data File**	NJ-03.d
Type	Sample	**Name**	NJ-03
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

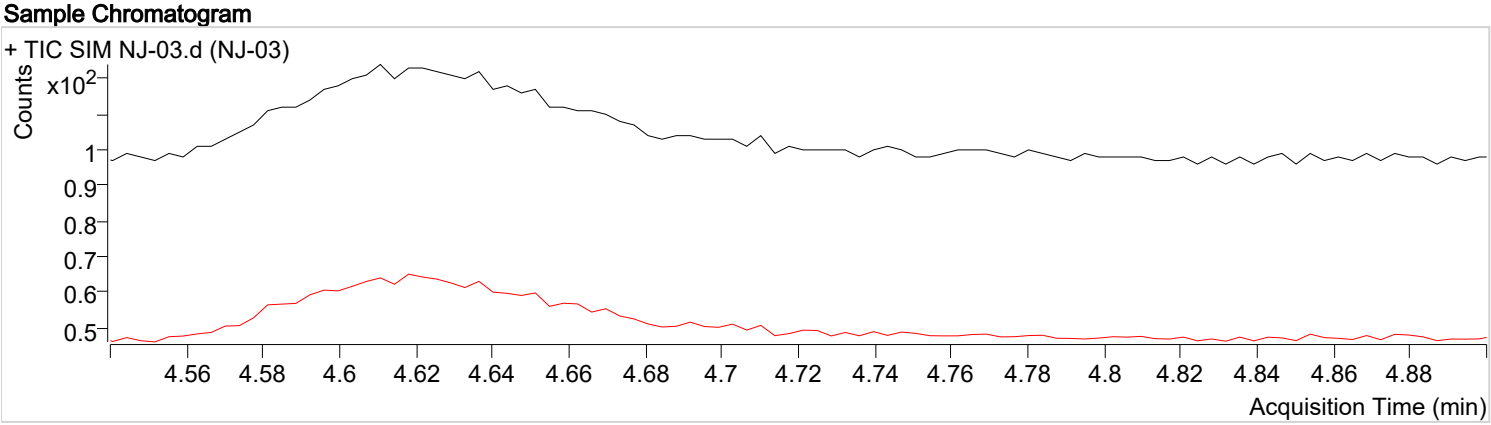

Styrene

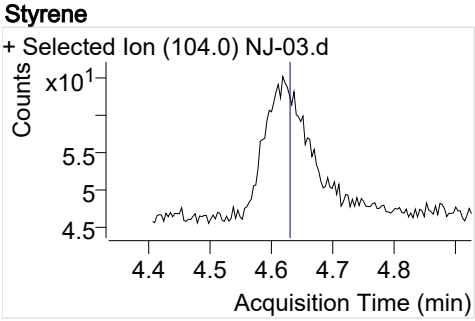



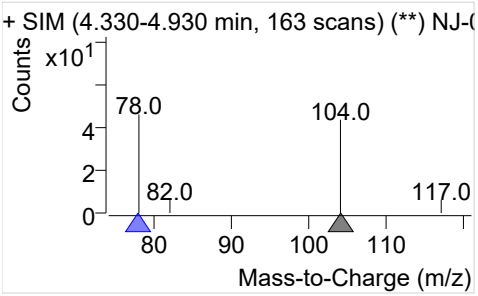

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\ST.batch.bin		
Analysis Time	2026-04-01 오후 4:42:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:14:47	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:42:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-30 오후 7:24:34	**Data File**	NJ-04.d
Type	Sample	**Name**	NJ-04
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

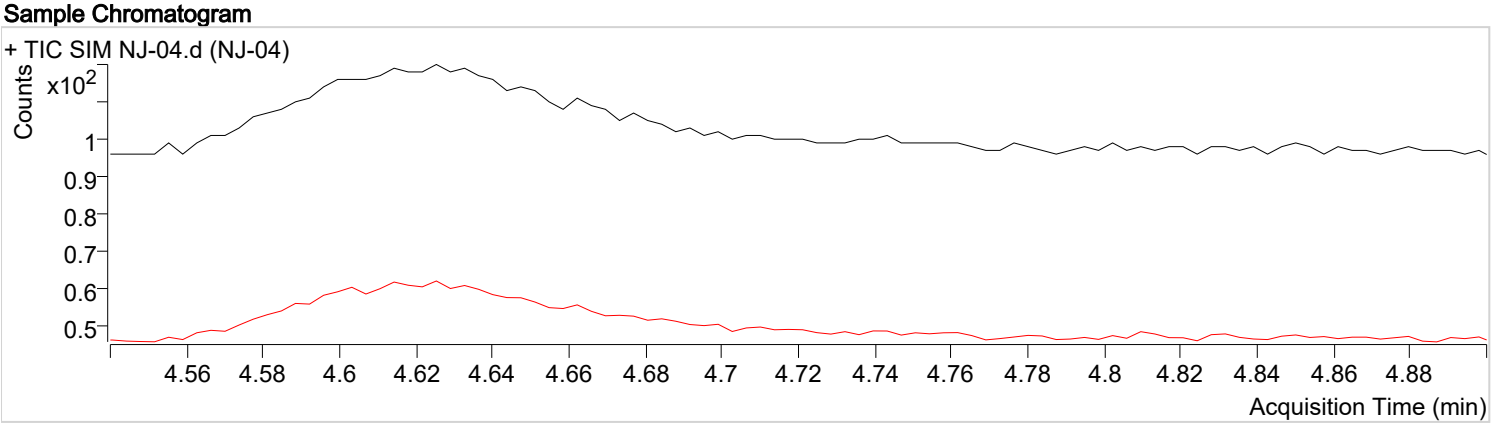

Styrene

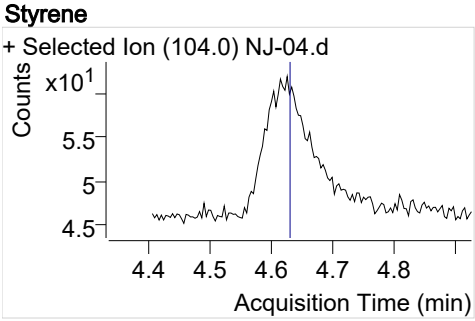



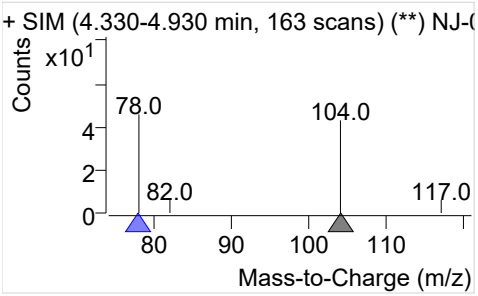

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\ST.batch.bin		
Analysis Time	2026-04-01 오후 4:42:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:14:47	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:42:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-30 오후 7:41:39	**Data File**	NJ-05.d
Type	Sample	**Name**	NJ-05
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

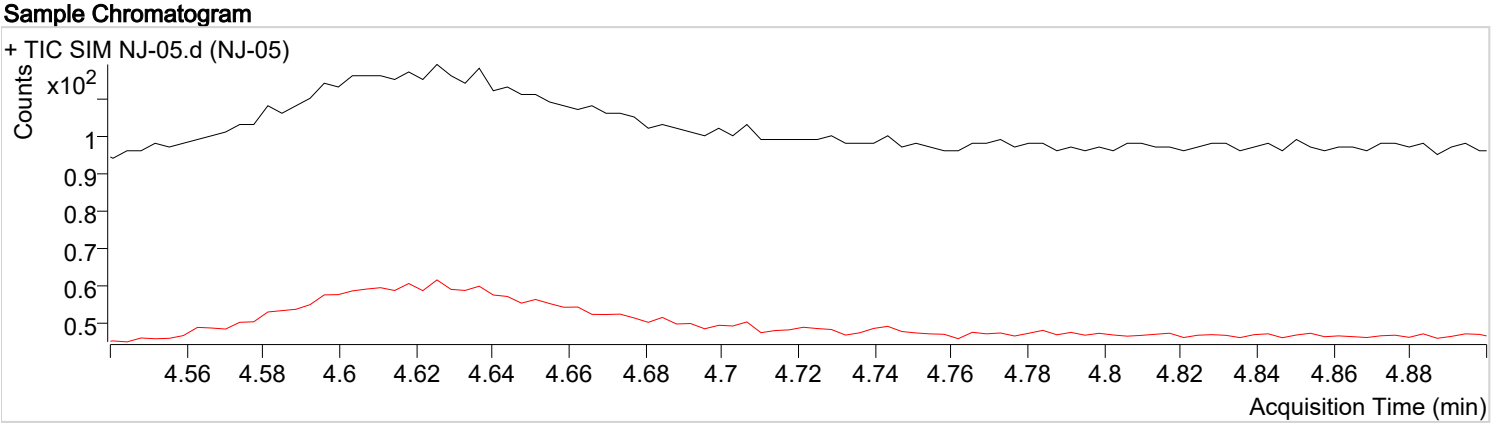

Styrene

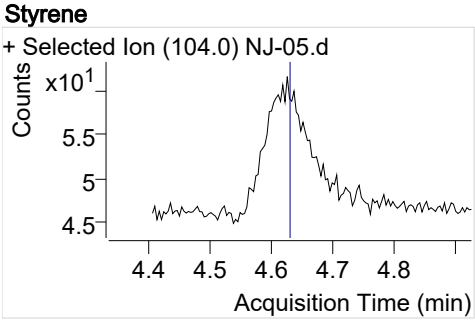



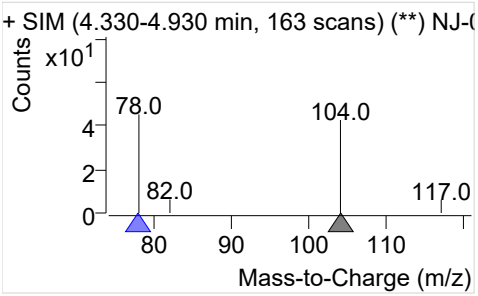

Quant Sample Report

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\ST.batch.bin		
Analysis Time	2026-04-01 오후 4:42:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:14:47	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:42:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-30 오후 7:58:51	**Data File**	NJ-06.d
Type	Sample	**Name**	NJ-06
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

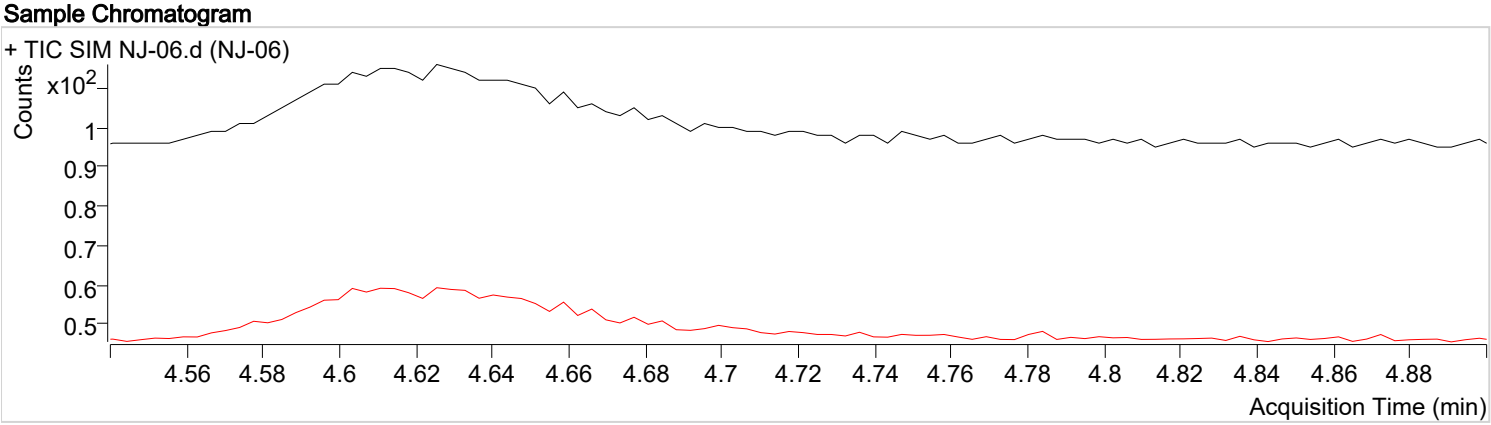

Styrene

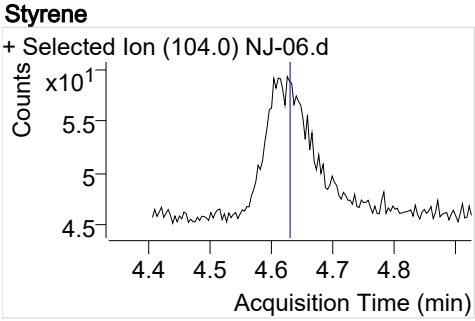



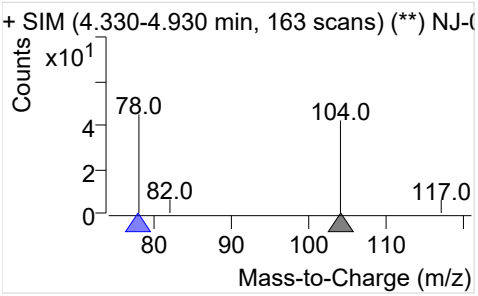

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\ST.batch.bin		
Analysis Time	2026-04-01 오후 4:42:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:14:47	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:42:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-30 오후 8:15:51	**Data File**	MBK.d
Type	Blank	**Name**	MBK
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

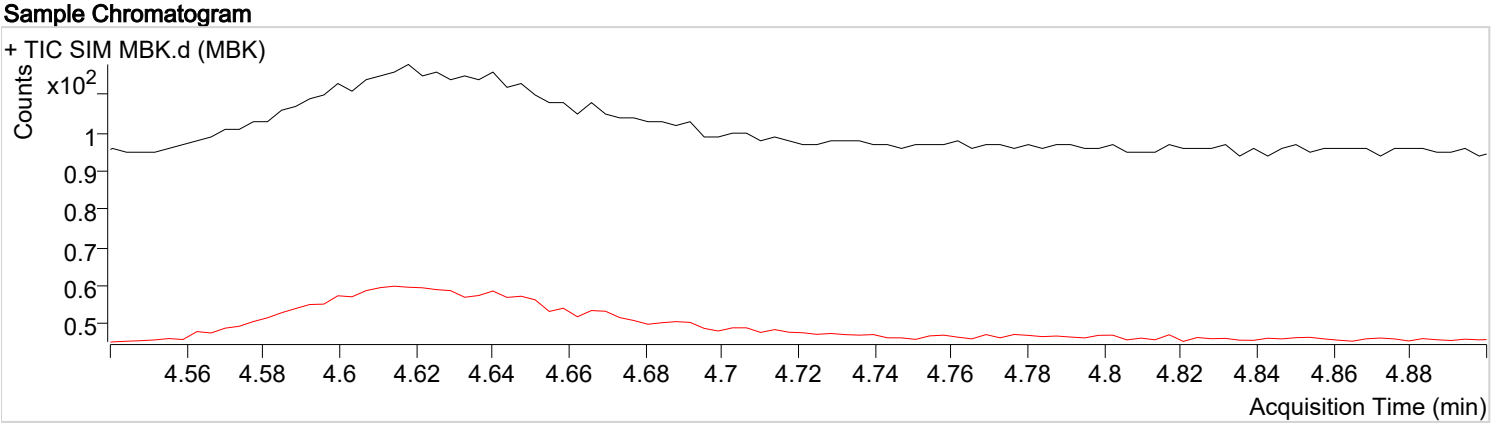

Styrene

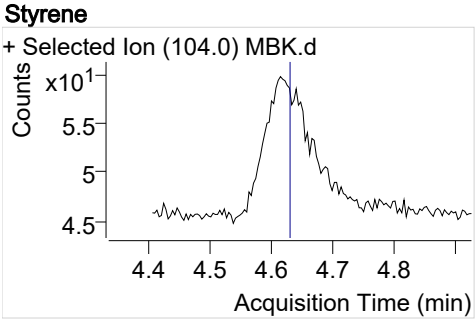



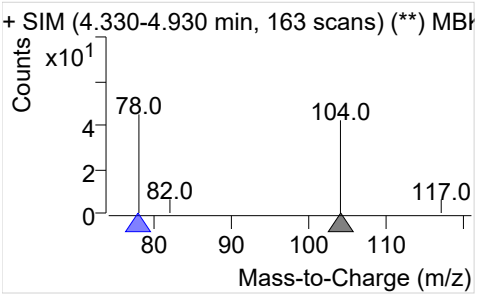

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\VOC2(NJ 3.26)\QuantResults\ST.batch.bin		
Analysis Time	2026-04-01 오후 4:42:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 3:14:47	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:42:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-30 오후 9:23:57	**Data File**	-CCV-S.d
Type	QC	**Name**	-CCV-S
Dil.	1	**Acq. Method File**	VOC2

Sample Chromatogram

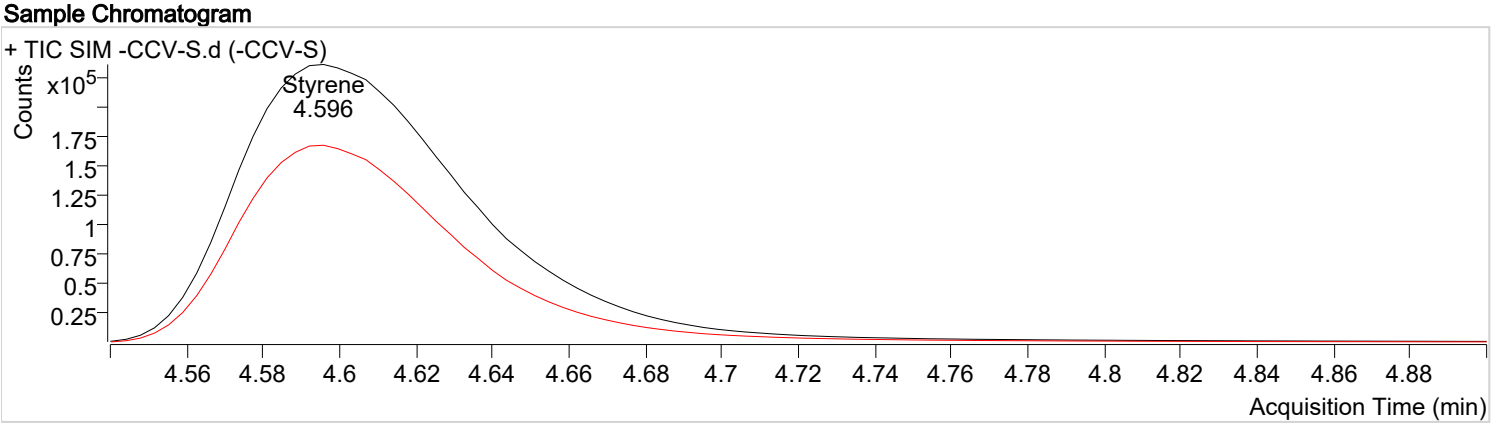

Name	RT	Resp.	Final Conc.	Units
Styrene	4.596	685902	0.273	mg/L

Styrene

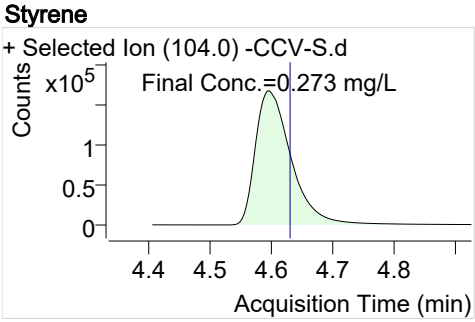



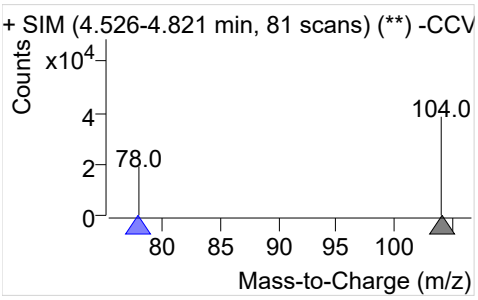

Generated at 오후 3:14 on 2026-04-10