Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\ACRYL(PL 12.30)\QuantResults\ACRYL.batch.bin				
Analysis Time	2026-01-08 오전 11:41:21	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:41:21	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Acrylamide

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
ACRYL ST-01.D	Cal	4.068	1474	15557	0.006
ACRYL ST-02.D	Cal	4.063	3557	15366	0.010
ACRYL ST-03.D	Cal	4.057	6641	15826	0.016
ACRYL ST-04.D	Cal	4.058	8068	14704	0.020
ACRYL ST-05.D	Cal	4.058	15363	16201	0.032
BK-.D	Blank			14208	ND
FBK(PL 25-12-30).D	Blank			15979	ND
PL-01.D	Sample			15911	ND
PL-02.D	Sample			15673	ND
MBK.D	Blank			15882	ND
-CCV-.D	QC	4.063	5677	15488	0.014

Acrylamide

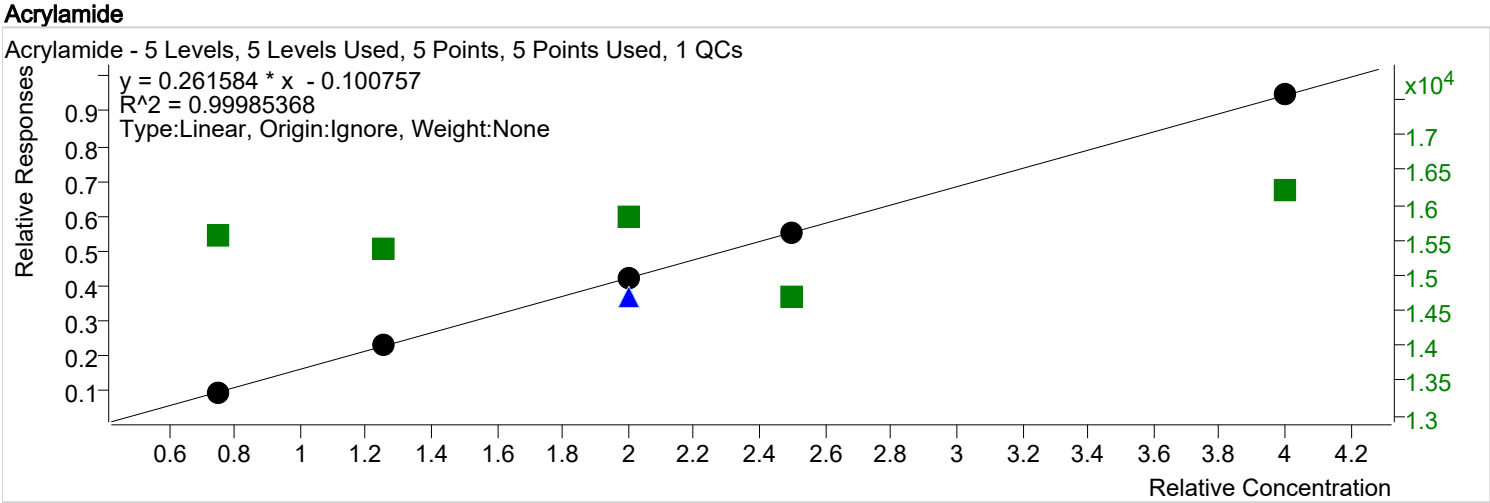

Cal. Path	Type	Level	Enable	Conc.	Response
W:\2026\1. 2026-01\ACRYL(PL 12.30)\ACRYL ST-01.D	Calibration	1	x	3.000	1474
W:\2026\1. 2026-01\ACRYL(PL 12.30)\ACRYL ST-02.D	Calibration	2	x	5.000	3557
W:\2026\1. 2026-01\ACRYL(PL 12.30)\ACRYL ST-03.D	Calibration	3	x	8.000	6641
W:\2026\1. 2026-01\ACRYL(PL 12.30)\-CCV-.D	QC	3	x	8.000	5677
W:\2026\1. 2026-01\ACRYL(PL 12.30)\ACRYL ST-04.D	Calibration	4	x	10.000	8068
W:\2026\1. 2026-01\ACRYL(PL 12.30)\ACRYL ST-05.D	Calibration	5	x	16.000	15363

Quant Sample Report

Batch Data Path	W:\2026\1. 2026-01\ACRYL(PL 12.30)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-08 오전 11:41:21	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:12:32	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:41:21	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-07 오후 4:20:08	**Data File**	ACRYL ST-01.D
Type	Cal	**Name**	ACRYL ST-01
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

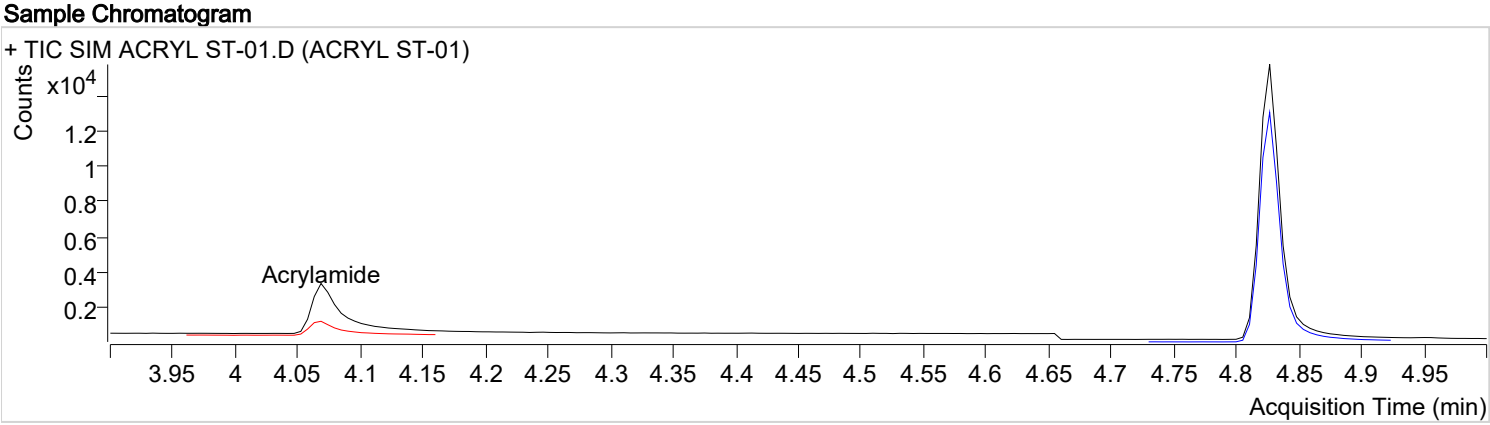

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.068	1474	15557	0.006 mg/L

Acrylamide

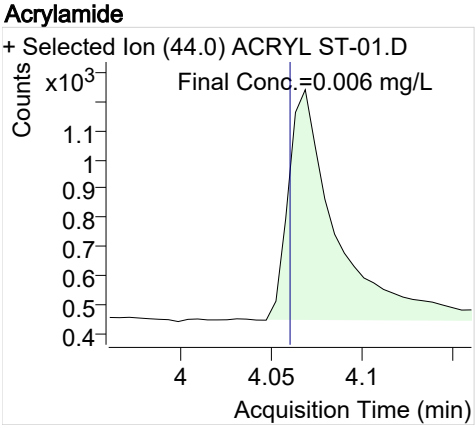

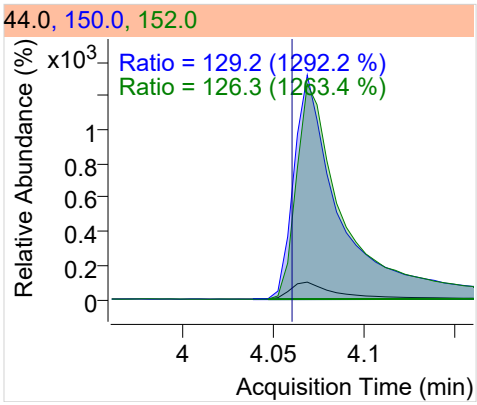



Quant Sample Report

Batch Data Path	W:\2026\1. 2026-01\ACRYL(PL 12.30)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-08 오전 11:41:21	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:12:32	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:41:21	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-07 오후 4:28:53	**Data File**	ACRYL ST-02.D
Type	Cal	**Name**	ACRYL ST-02
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

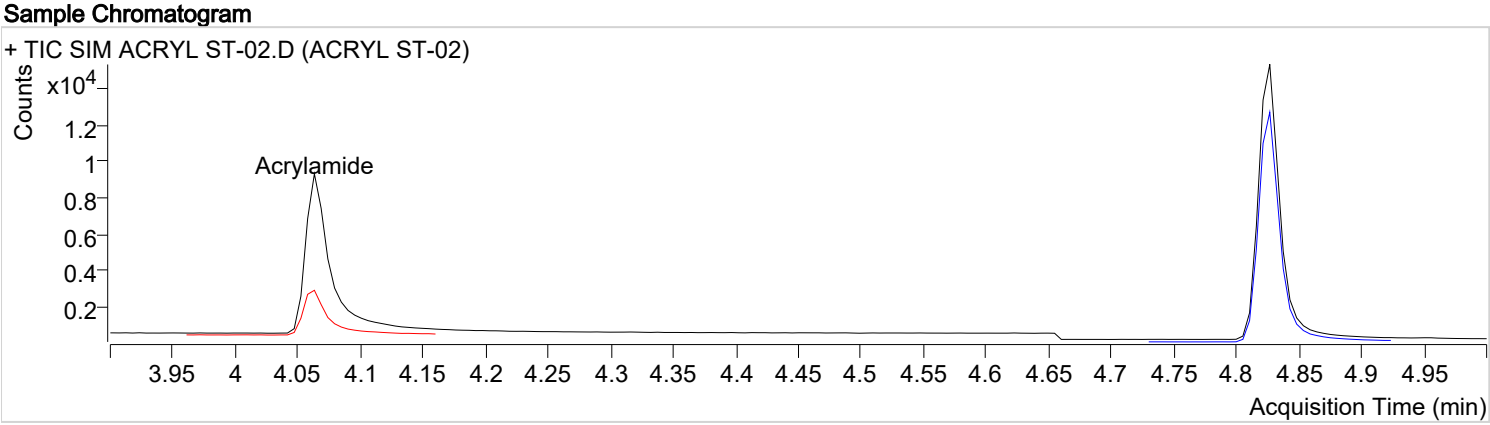

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.063	3557	15366	0.010 mg/L

Acrylamide

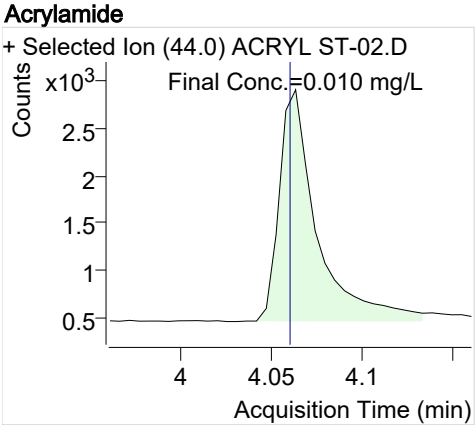

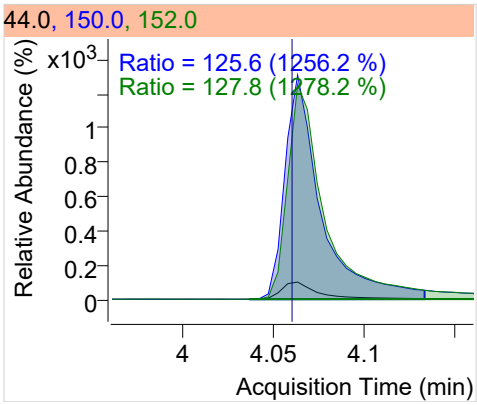



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\ACRYL(PL 12.30)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-08 오전 11:41:21	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:12:32	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:41:21	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-07 오후 4:37:39	**Data File**	ACRYL ST-03.D
Type	Cal	**Name**	ACRYL ST-03
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

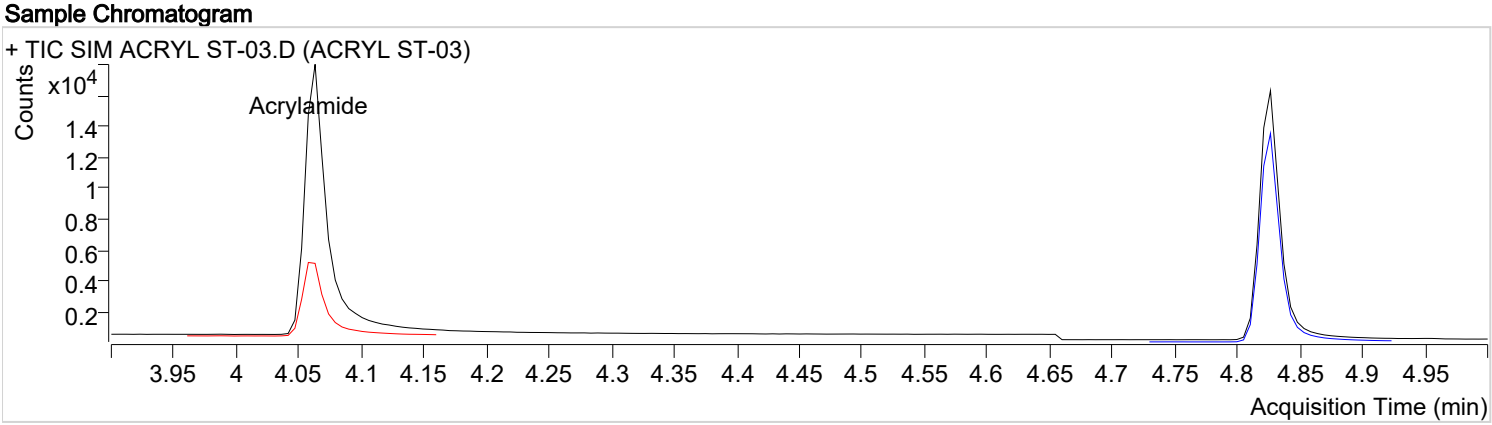

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.057	6641	15826	0.016 mg/L

Acrylamide

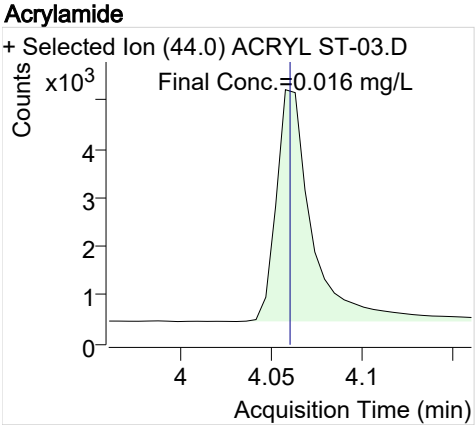





Quant Sample Report

Batch Data Path	W:\2026\1. 2026-01\ACRYL(PL 12.30)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-08 오전 11:41:21	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:12:32	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:41:21	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-07 오후 4:46:24	**Data File**	ACRYL ST-04.D
Type	Cal	**Name**	ACRYL ST-04
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

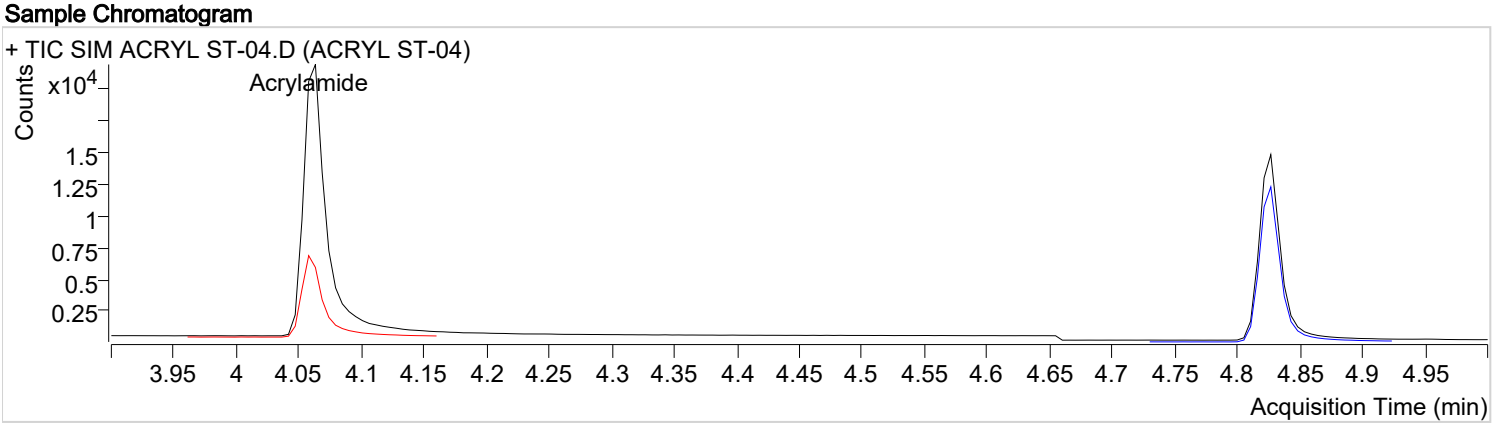

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.058	8068	14704	0.020 mg/L

Acrylamide

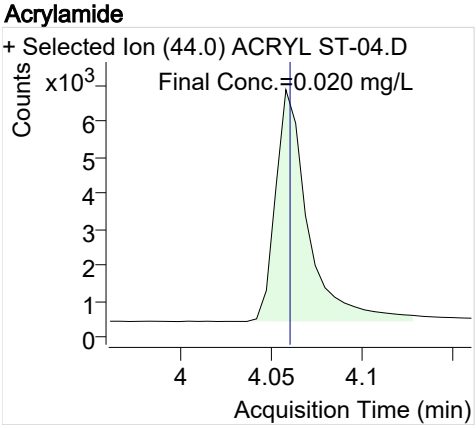





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\ACRYL(PL 12.30)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-08 오전 11:41:21	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:12:32	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:41:21	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-07 오후 4:55:11	**Data File**	ACRYL ST-05.D
Type	Cal	**Name**	ACRYL ST-05
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

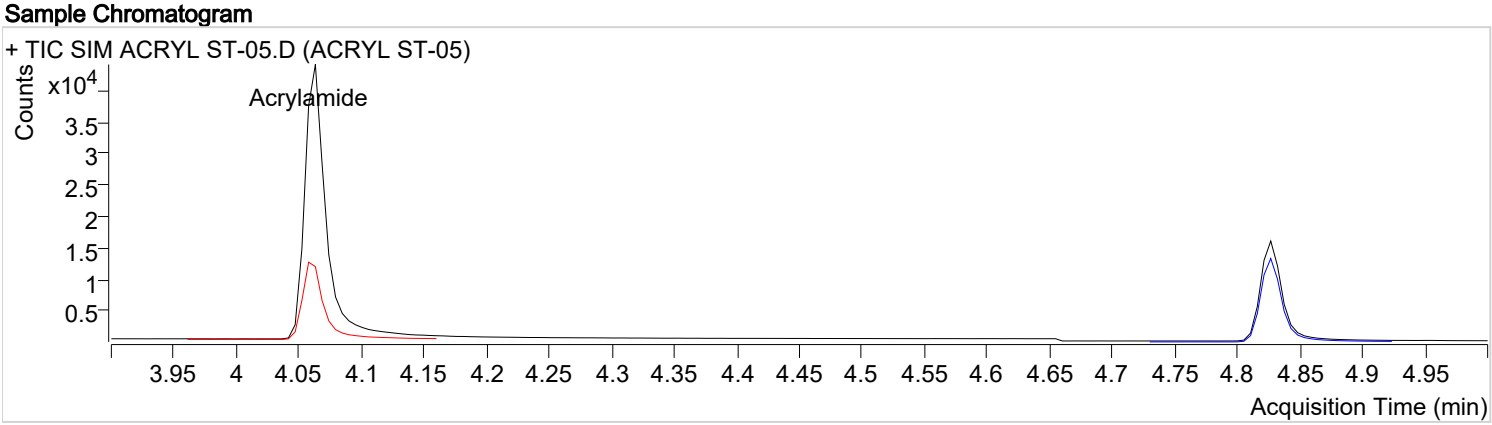

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.058	15363	16201	0.032 mg/L

Acrylamide

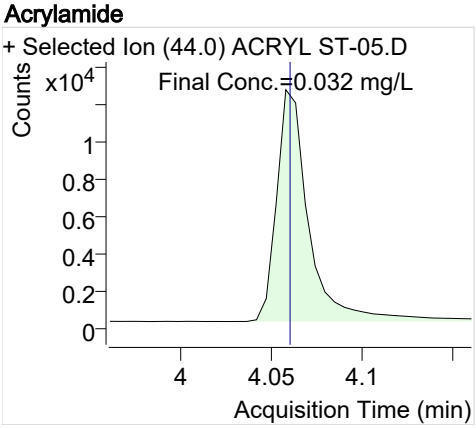





Quant Sample Report

Batch Data Path	W:\2026\1. 2026-01\ACRYL(PL 12.30)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-08 오전 11:41:21	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:12:32	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:41:21	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-07 오후 5:21:26	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

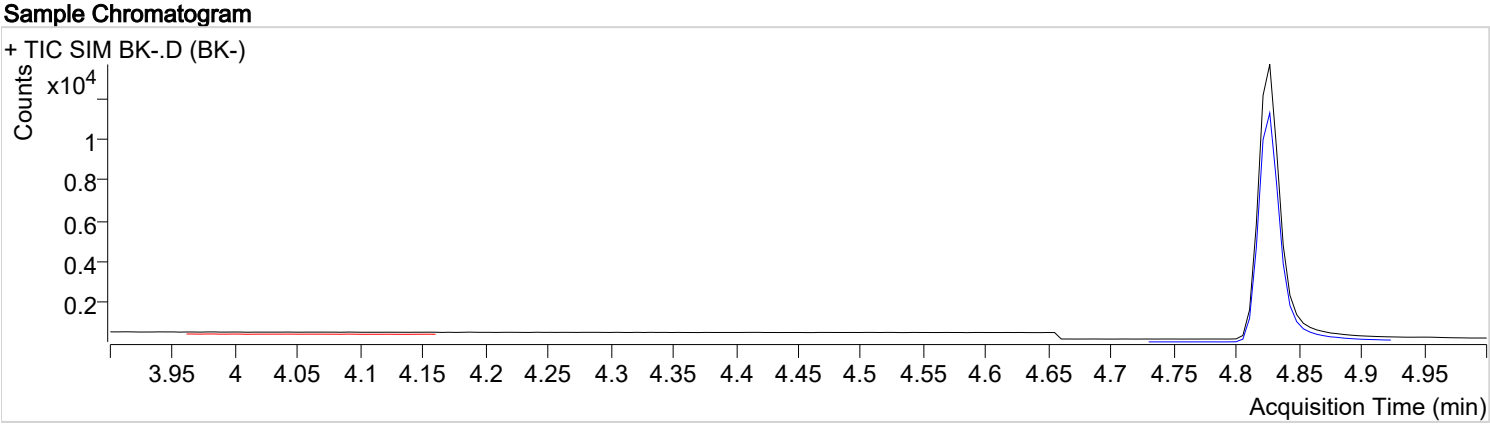

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide			14208	ND mg/L

Acrylamide

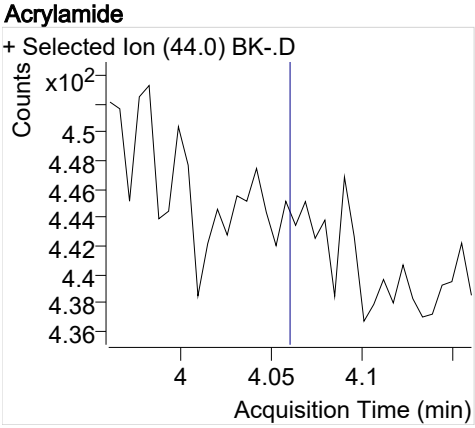

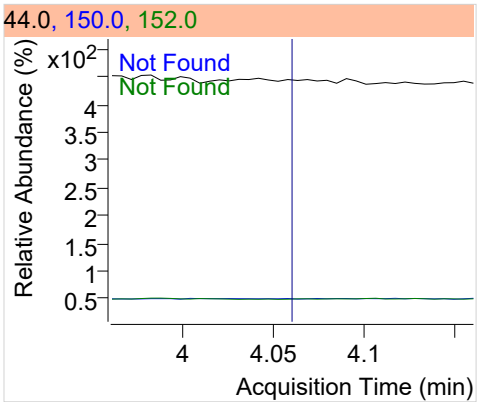



Quant Sample Report

Batch Data Path	W:\2026\1. 2026-01\ACRYL(PL 12.30)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-08 오전 11:41:21	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:12:32	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:41:21	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-07 오후 5:30:11	**Data File**	FBK(PL 25-12-30).D
Type	Blank	**Name**	FBK(PL 25-12-30)
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

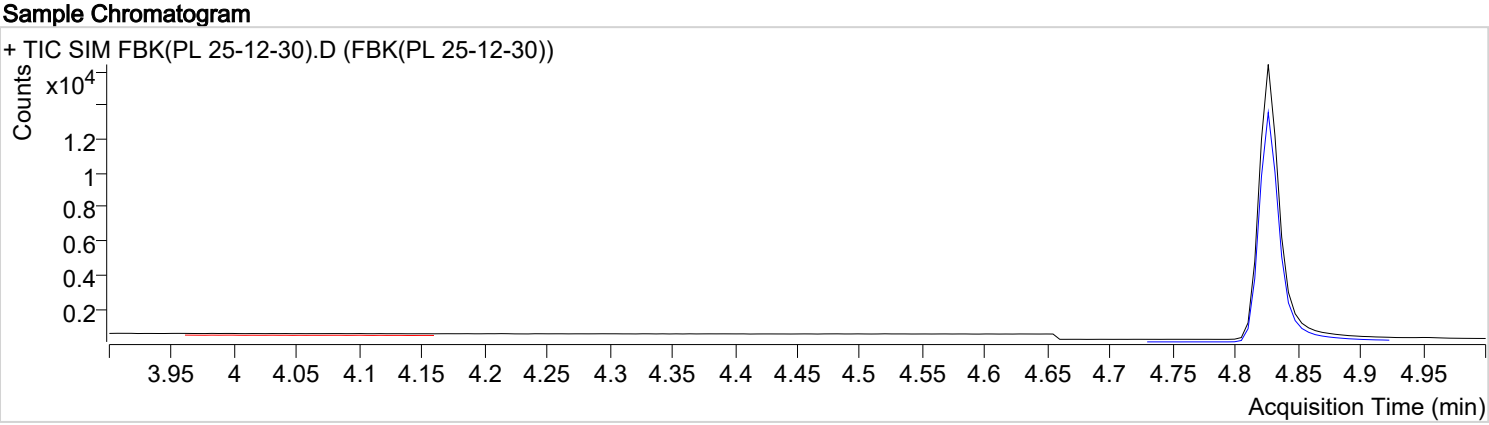

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide			15979	ND mg/L

Acrylamide

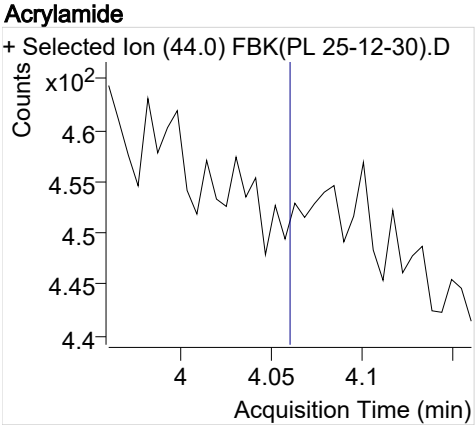



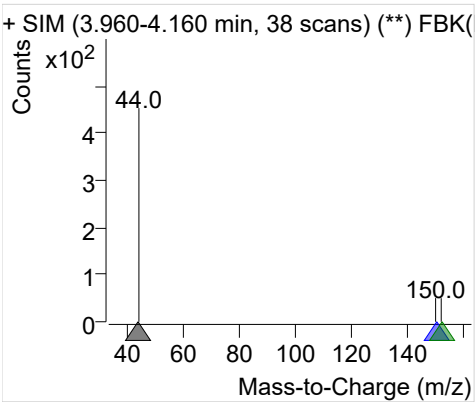

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\ACRYL(PL 12.30)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-08 오전 11:41:21	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:12:32	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:41:21	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-07 오후 5:38:57	**Data File**	PL-01.D
Type	Sample	**Name**	PL-01
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

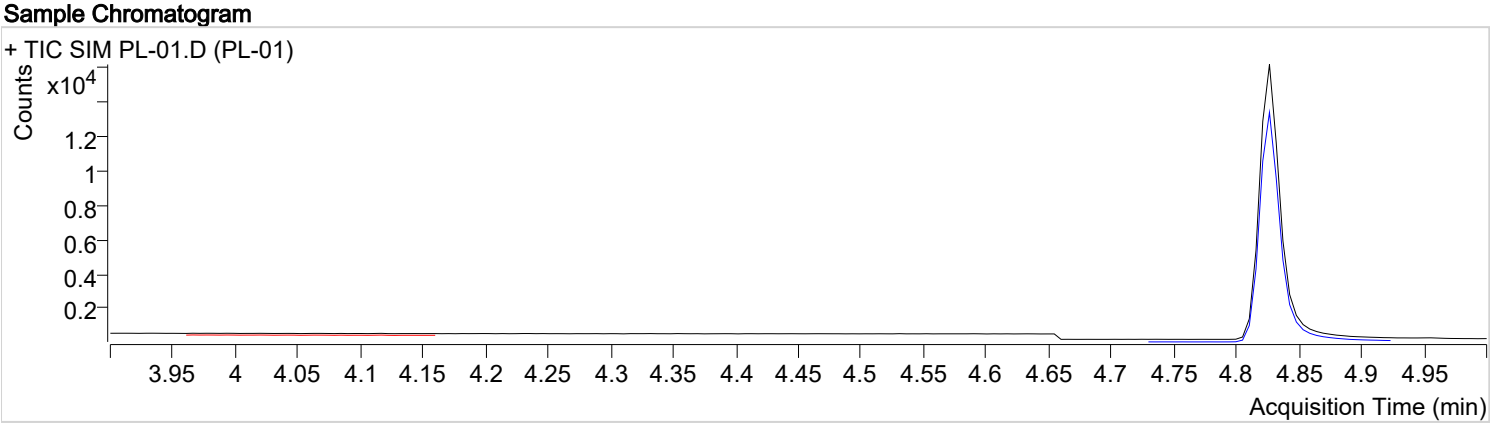

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide			15911	ND mg/L

Acrylamide

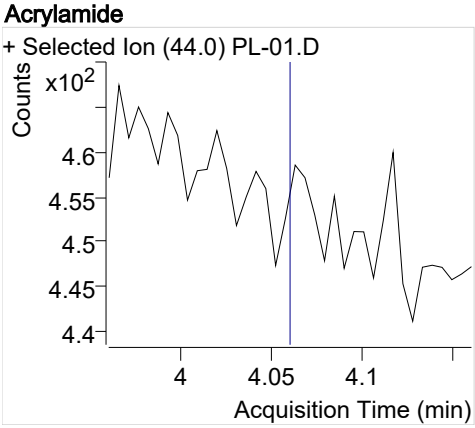

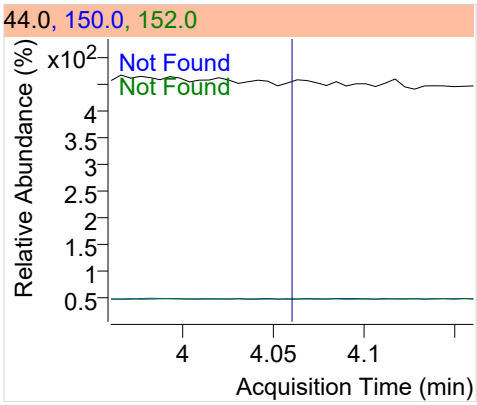



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\ACRYL(PL 12.30)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-08 오전 11:41:21	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:12:32	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:41:21	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-07 오후 5:47:40	**Data File**	PL-02.D
Type	Sample	**Name**	PL-02
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

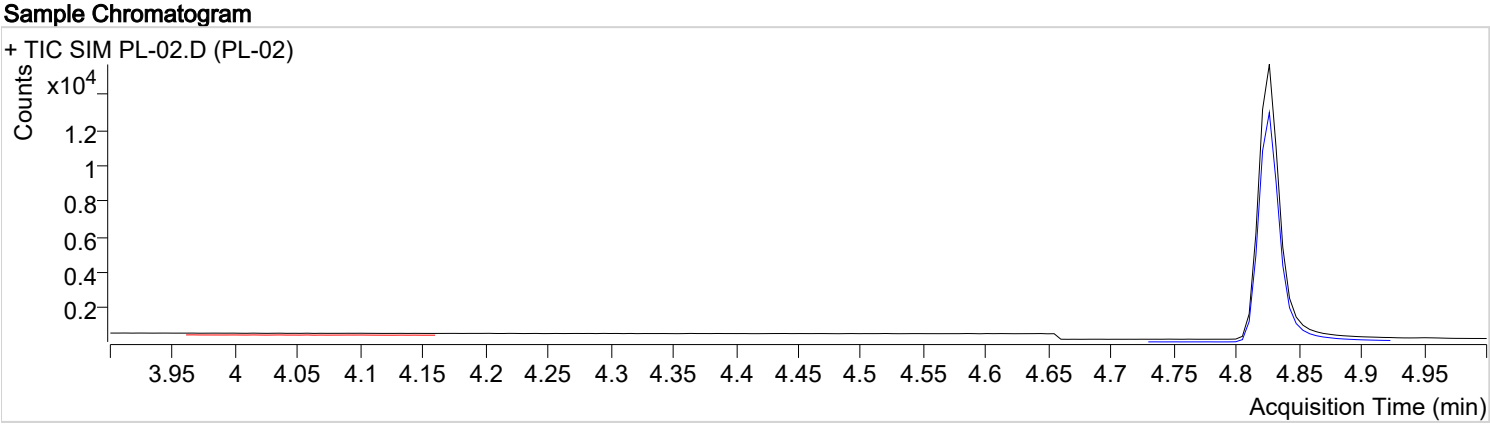

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide			15673	ND mg/L

Acrylamide

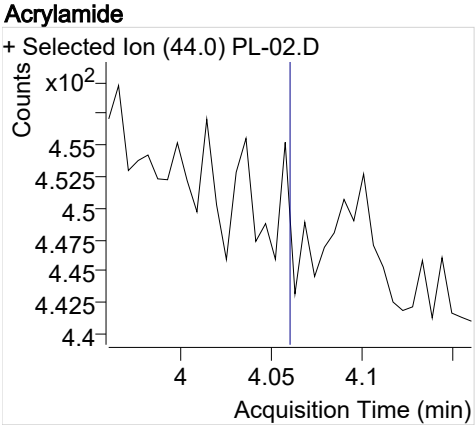

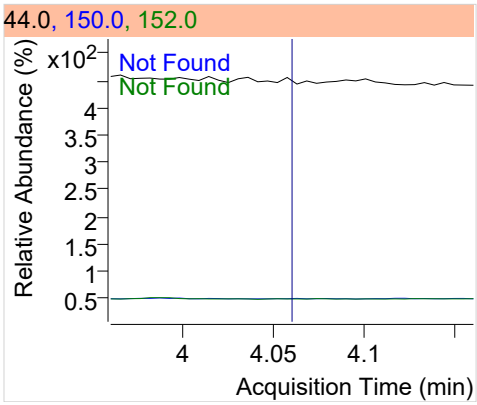



Quant Sample Report

Batch Data Path	W:\2026\1. 2026-01\ACRYL(PL 12.30)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-08 오전 11:41:21	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:12:32	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:41:21	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-07 오후 5:56:25	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

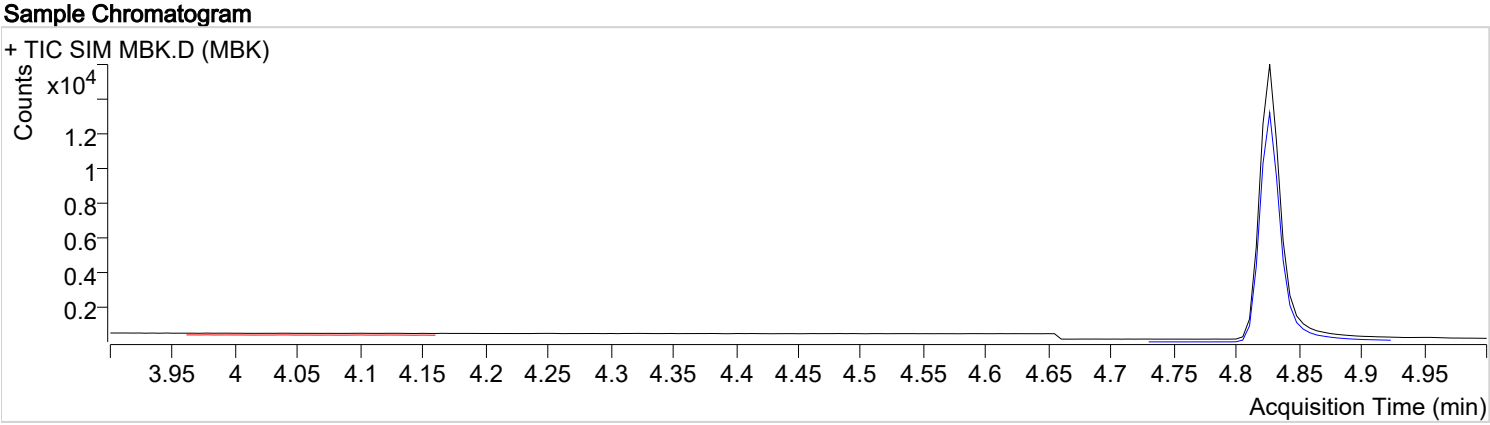

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide			15882	ND mg/L

Acrylamide

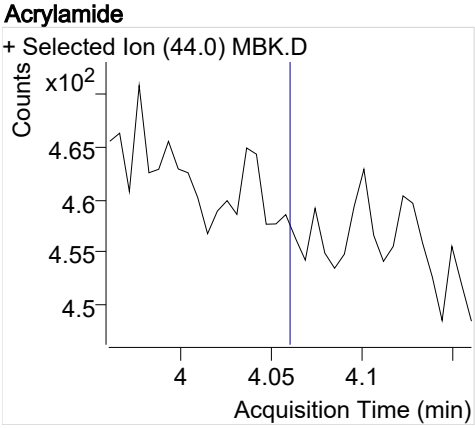

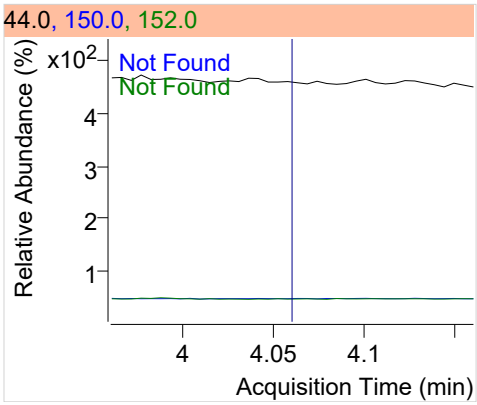



Quant Sample Report

Batch Data Path	W:\2026\1. 2026-01\ACRYL(PL 12.30)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-08 오전 11:41:21	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:12:32	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:41:21	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-07 오후 6:13:55	**Data File**	-CCV-.D
Type	QC	**Name**	-CCV-
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

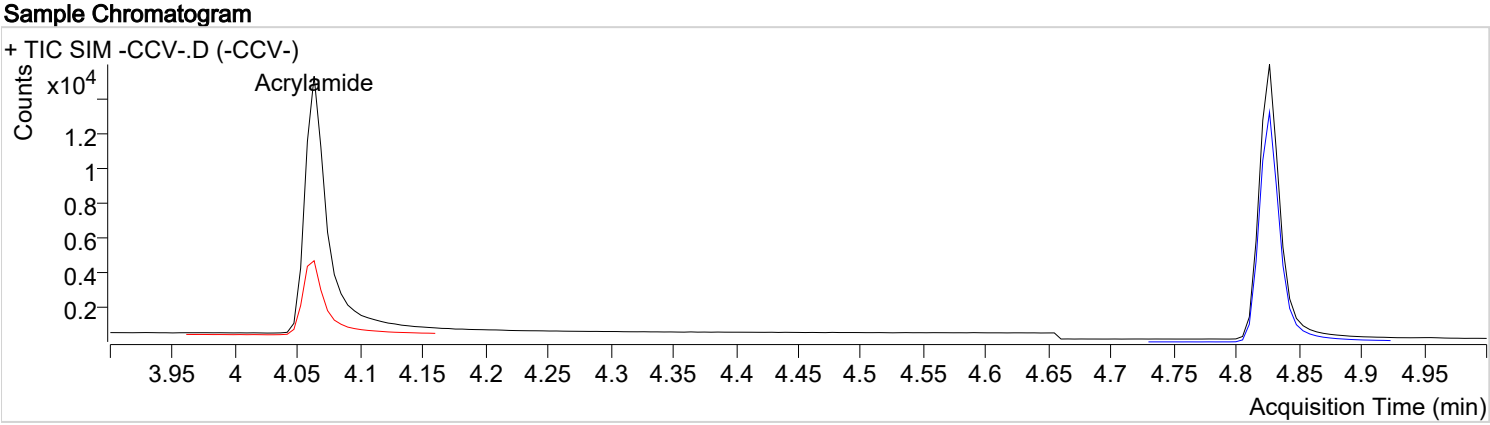

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.063	5677	15488	0.014 mg/L
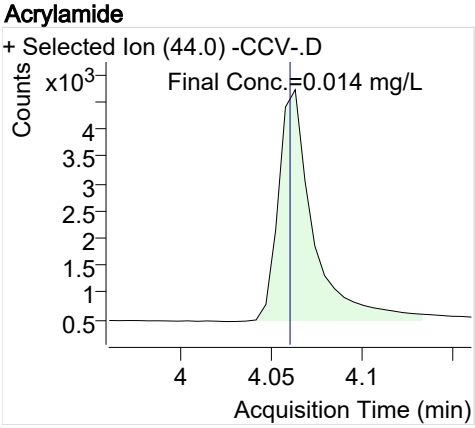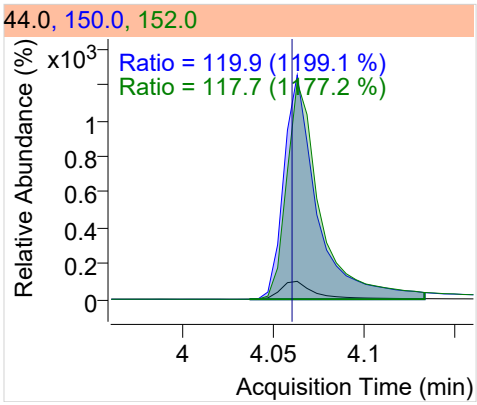
Acrylamide