Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\ACRYL(KD 1.15)\QuantResults\ACRYL.batch.bin				
Analysis Time	2026-01-21 오후 1:08:12	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 1:08:12	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Acrylamide

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
ACRYL ST-01.D	Cal	4.079	152	2026	0.005
ACRYL ST-02.D	Cal	4.068	310	2903	0.009
ACRYL ST-03.D	Cal	4.063	949	4829	0.018
ACRYL ST-04.D	Cal	4.058	1732	6069	0.028
ACRYL ST-05.D	Cal	4.057	1985	6124	0.032
ACRYL ST-06.D	Cal	4.058	2686	6943	0.039
BK-.D	Blank			7414	ND
FBK(KD 26-01-15).D	Blank			2004	ND
KD-01.D	Sample			5560	ND
MBK.D	Blank			6980	ND
CCV-.D	QC	4.057	1285	6899	0.017

Acrylamide

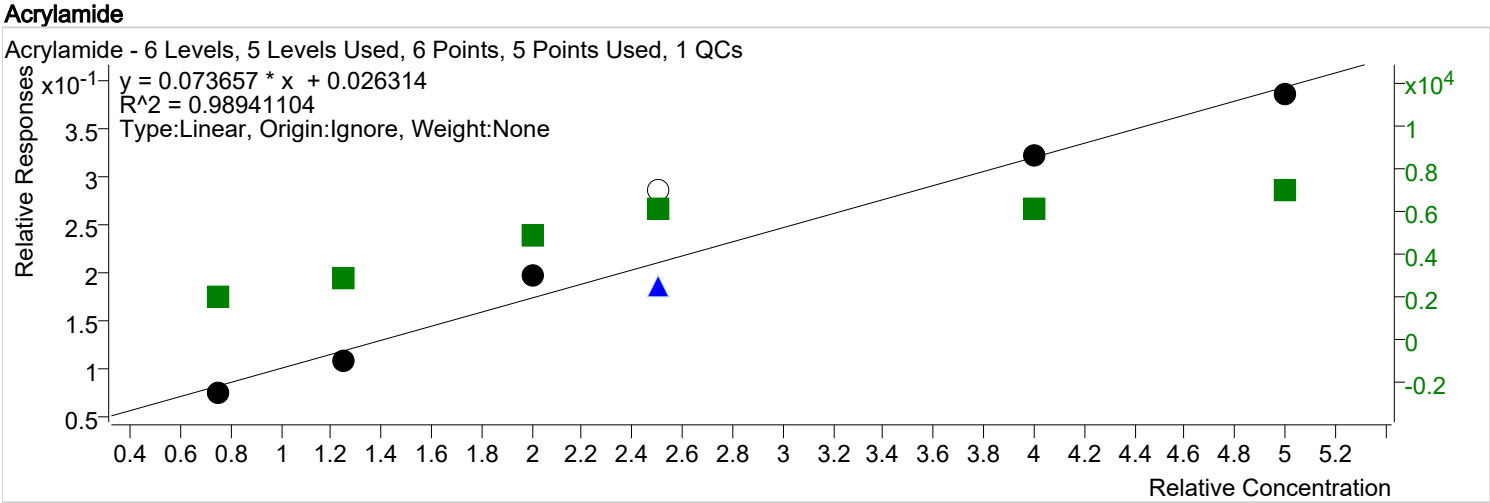

Cal. Path	Type	Level	Enable	Conc.	Response
W:\2026\1. 2026-01\ACRYL(KD 1.15)\ACRYL ST-01.D	Calibration	1	x	3.000	152
W:\2026\1. 2026-01\ACRYL(KD 1.15)\ACRYL ST-02.D	Calibration	2	x	5.000	310
W:\2026\1. 2026-01\ACRYL(KD 1.15)\ACRYL ST-03.D	Calibration	3	x	8.000	949
W:\2026\1. 2026-01\ACRYL(KD 1.15)\ACRYL ST-04.D	Calibration	4		10.000	1732
W:\2026\1. 2026-01\ACRYL(KD 1.15)\CCV-.D	QC	4	x	10.000	1285
W:\2026\1. 2026-01\ACRYL(KD 1.15)\ACRYL ST-05.D	Calibration	5	x	16.000	1985
W:\2026\1. 2026-01\ACRYL(KD 1.15)\ACRYL ST-06.D	Calibration	6	x	20.000	2686

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\ACRYL(KD 1.15)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-21 오후 1:08:12	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:11:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 1:08:12	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-21 오전 10:10:31	**Data File**	ACRYL ST-01.D
Type	Cal	**Name**	ACRYL ST-01
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

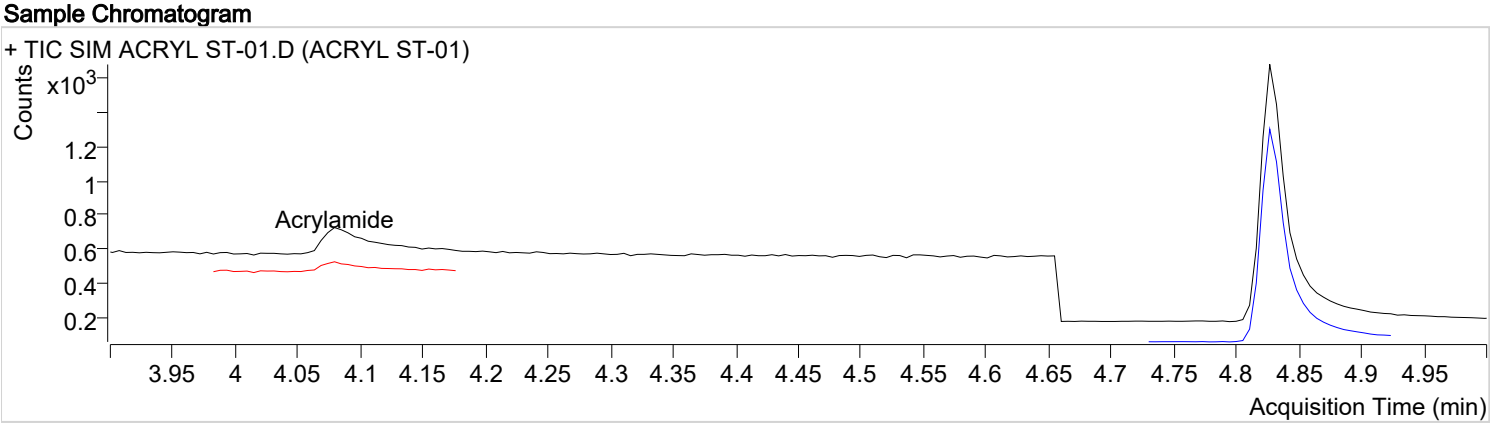

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.079	152	2026	0.005 mg/L

Acrylamide







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\ACRYL(KD 1.15)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-21 오후 1:08:12	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:11:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 1:08:12	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-21 오전 10:19:15	**Data File**	ACRYL ST-02.D
Type	Cal	**Name**	ACRYL ST-02
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

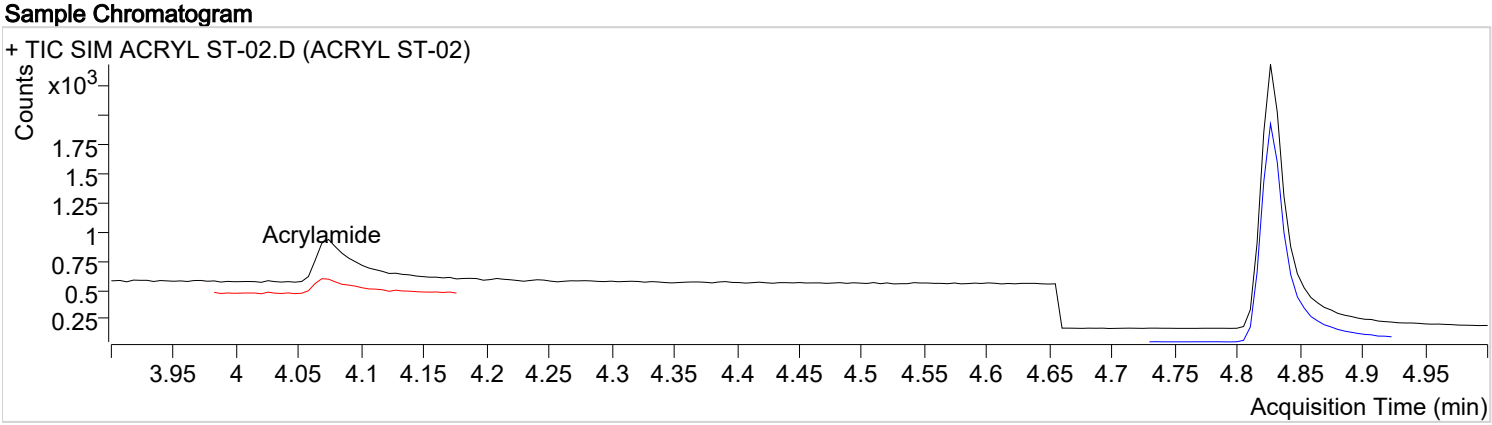

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.068	310	2903	0.009 mg/L

Acrylamide

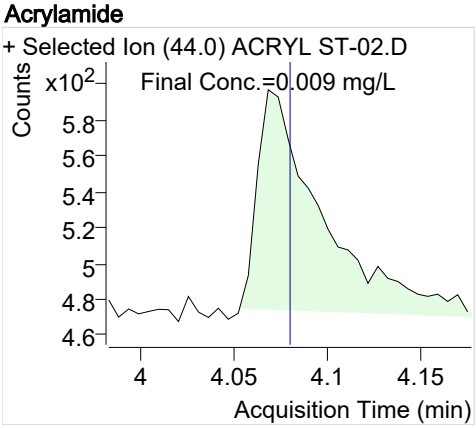





Quant Sample Report

Batch Data Path	W:\2026\1. 2026-01\ACRYL(KD 1.15)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-21 오후 1:08:12	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:11:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 1:08:12	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-21 오전 10:27:59	**Data File**	ACRYL ST-03.D
Type	Cal	**Name**	ACRYL ST-03
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

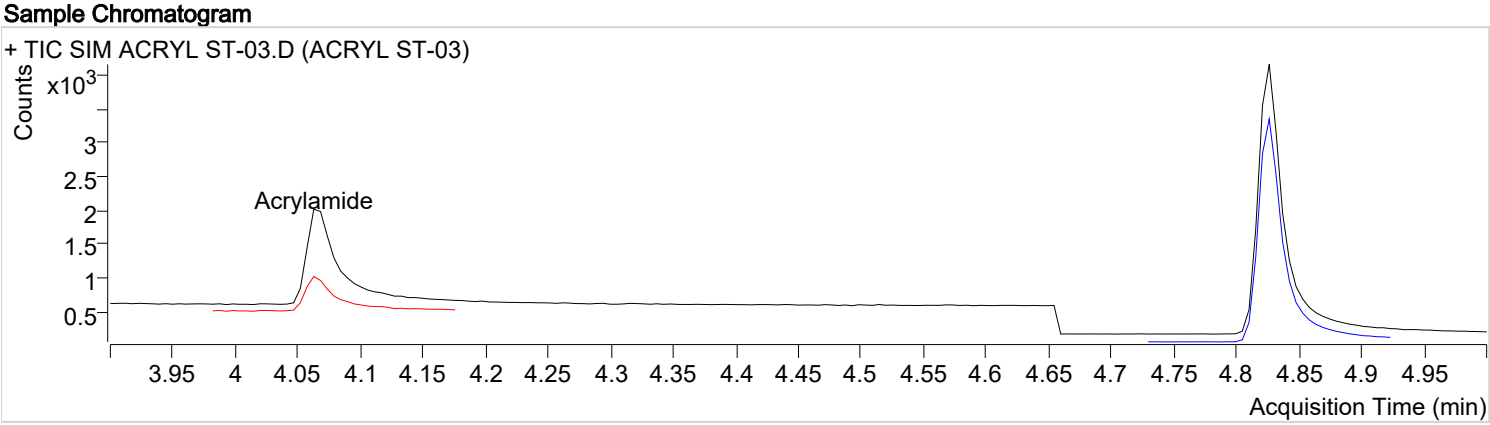

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.063	949	4829	0.018 mg/L

Acrylamide







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\ACRYL(KD 1.15)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-21 오후 1:08:12	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:11:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 1:08:12	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-21 오전 10:36:43	**Data File**	ACRYL ST-04.D
Type	Cal	**Name**	ACRYL ST-04
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

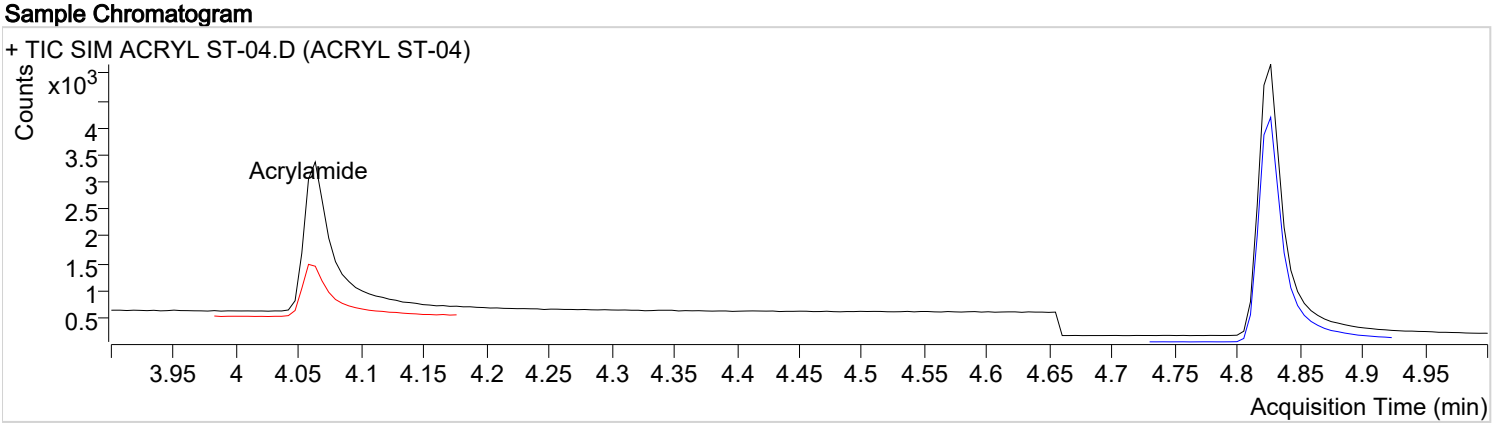

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.058	1732	6069	0.028 mg/L

Acrylamide







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\ACRYL(KD 1.15)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-21 오후 1:08:12	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:11:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 1:08:12	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-21 오전 10:45:27	**Data File**	ACRYL ST-05.D
Type	Cal	**Name**	ACRYL ST-05
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

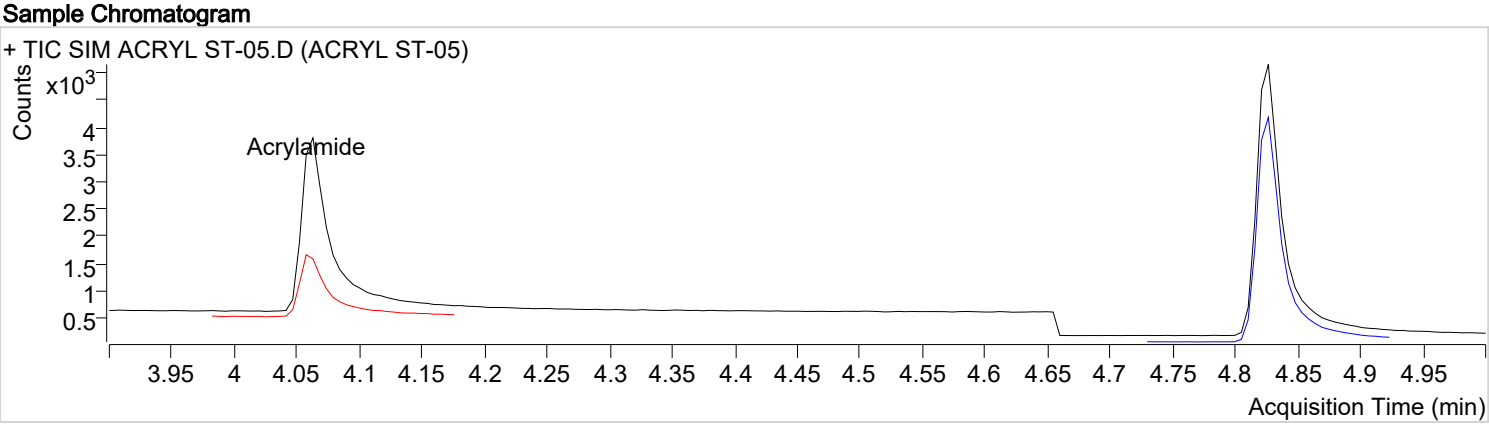

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.057	1985	6124	0.032 mg/L

Acrylamide







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\ACRYL(KD 1.15)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-21 오후 1:08:12	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:11:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 1:08:12	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-21 오전 10:54:14	**Data File**	ACRYL ST-06.D
Type	Cal	**Name**	ACRYL ST-06
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

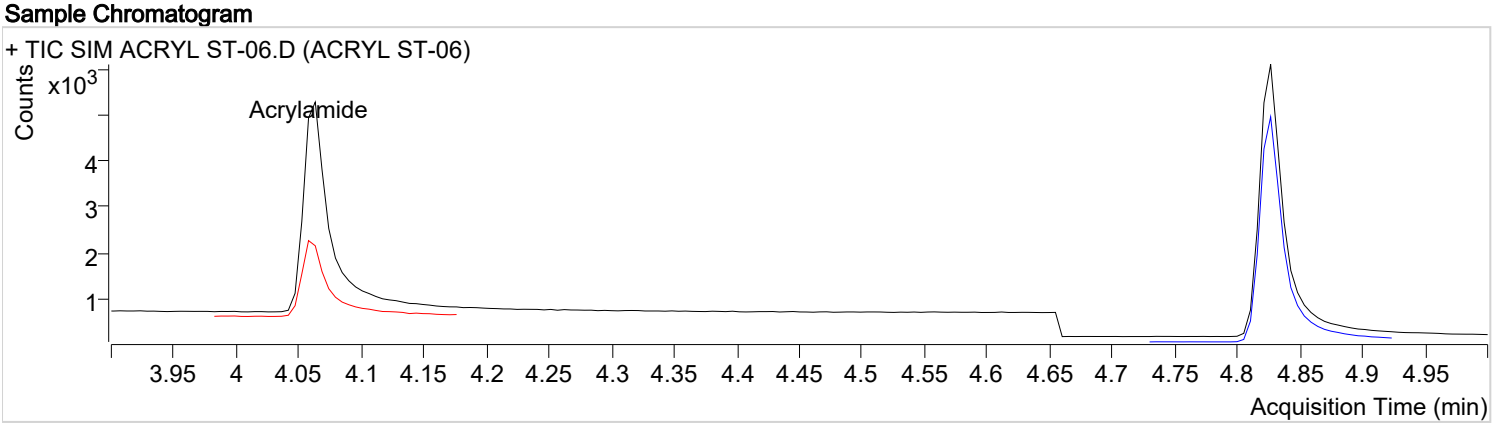

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.058	2686	6943	0.039 mg/L

Acrylamide







Quant Sample Report

Batch Data Path	W:\2026\1. 2026-01\ACRYL(KD 1.15)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-21 오후 1:08:12	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:11:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 1:08:12	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-21 오전 11:11:47	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

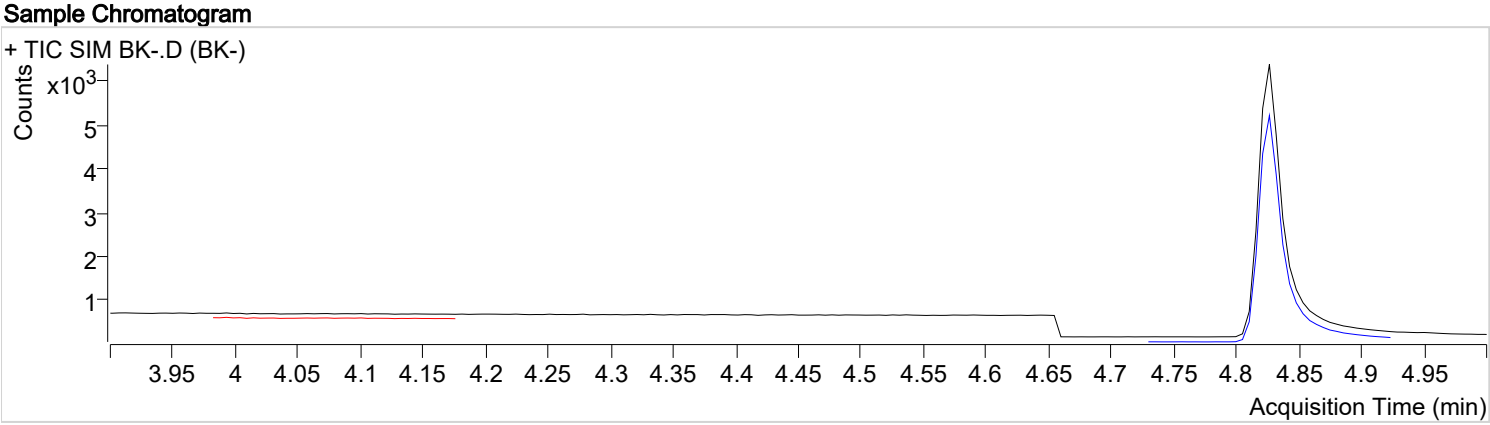

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide			7414	ND mg/L

Acrylamide







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\ACRYL(KD 1.15)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-21 오후 1:08:12	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:11:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 1:08:12	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-21 오전 11:20:34	**Data File**	FBK(KD 26-01-15).D
Type	Blank	**Name**	FBK(KD 26-01-15)
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

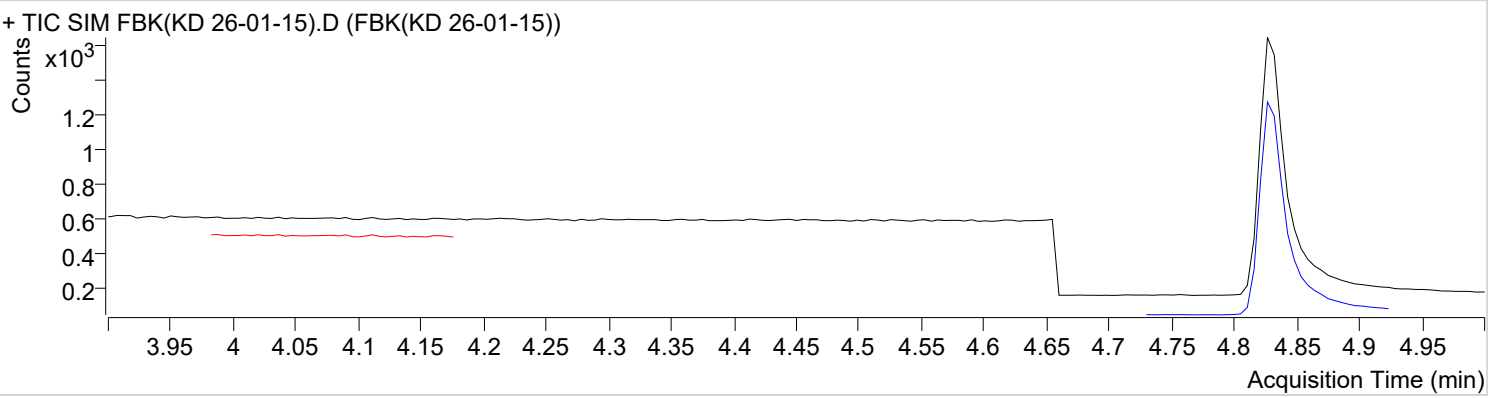

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide			2004	ND mg/L

Acrylamide







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\ACRYL(KD 1.15)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-21 오후 1:08:12	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:11:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 1:08:12	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-21 오전 11:29:21	**Data File**	KD-01.D
Type	Sample	**Name**	KD-01
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

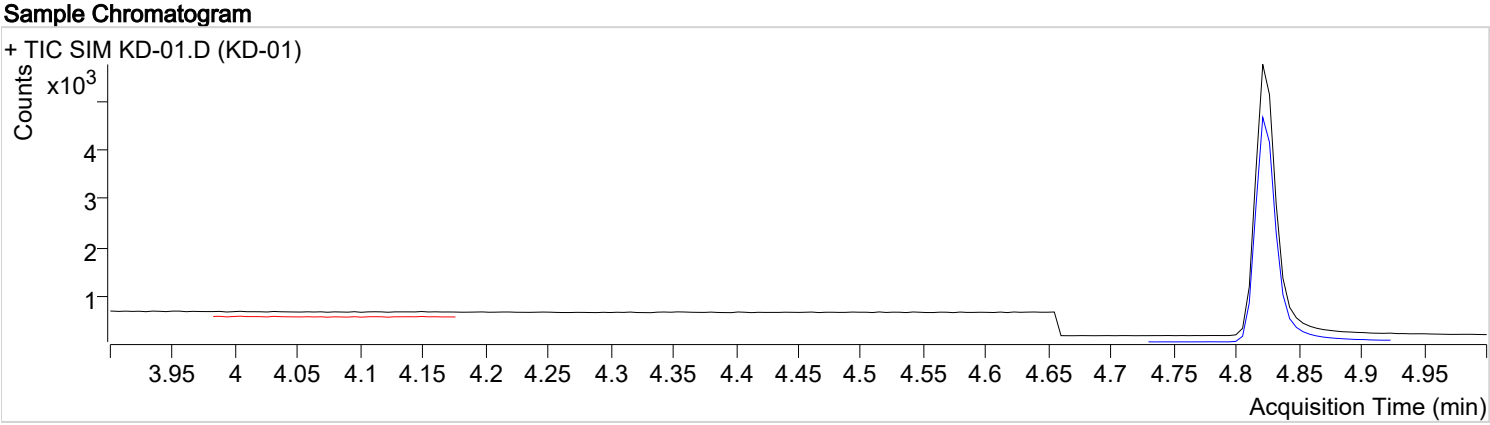

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide			5560	ND mg/L

Acrylamide





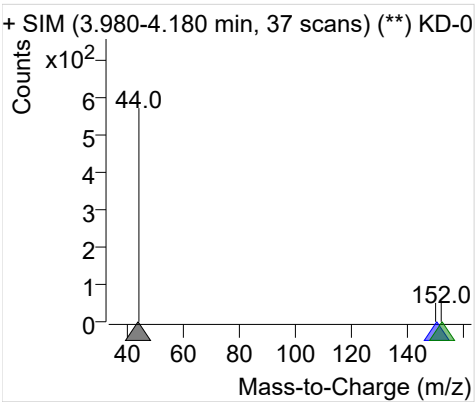

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	W:\2026\1. 2026-01\ACRYL(KD 1.15)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-21 오후 1:08:12	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:11:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 1:08:12	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-21 오전 11:38:11	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

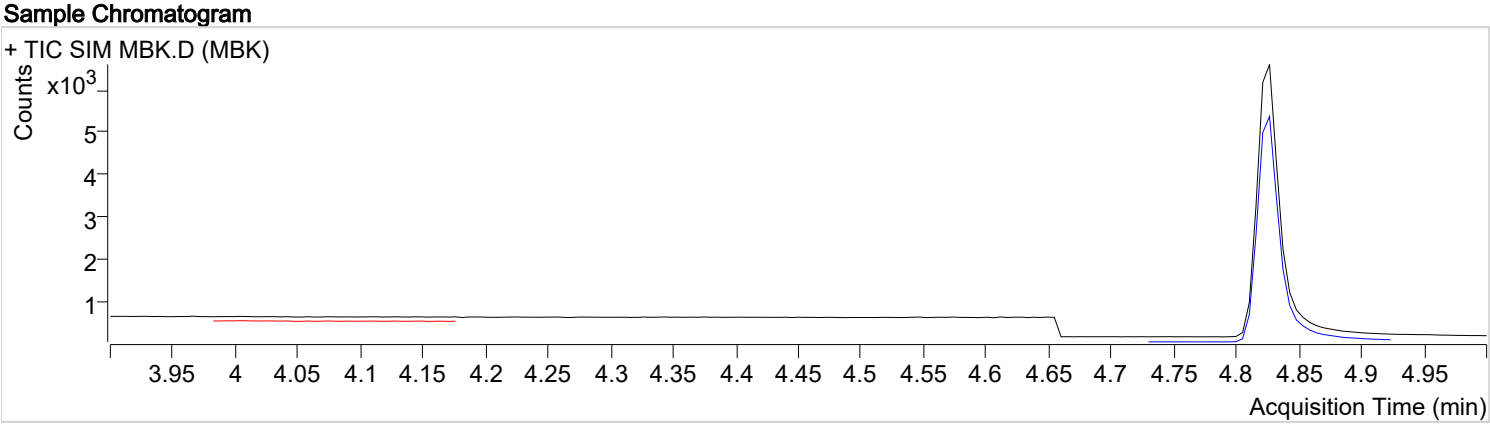

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide			6980	ND mg/L

Acrylamide







Quant Sample Report

Batch Data Path	W:\2026\1. 2026-01\ACRYL(KD 1.15)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-01-21 오후 1:08:12	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:11:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-21 오후 1:08:12	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-21 오전 11:55:42	**Data File**	CCV-.D
Type	QC	**Name**	CCV-
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

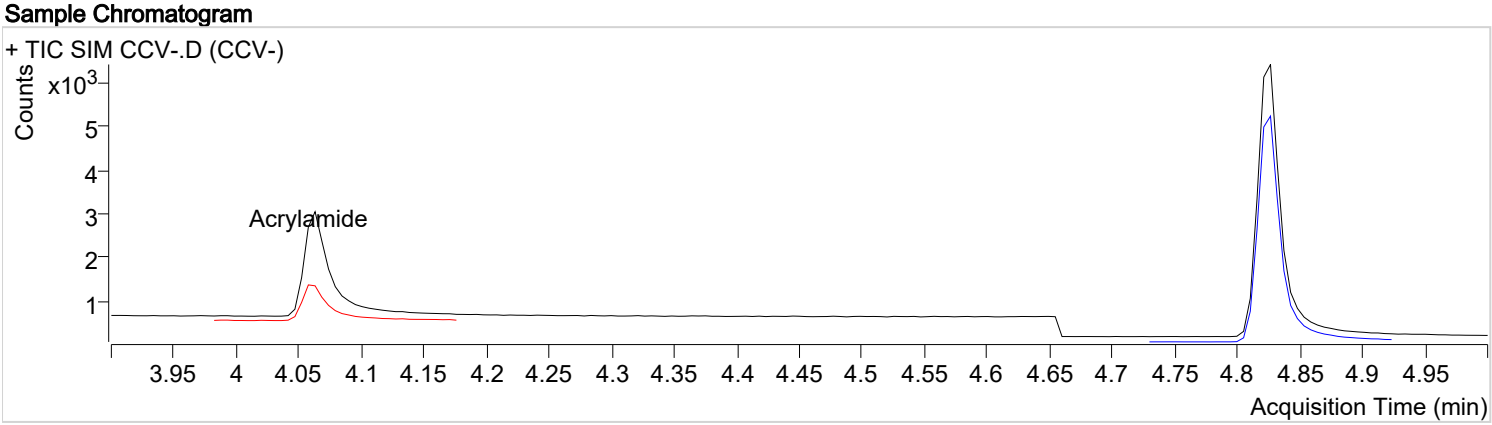

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.057	1285	6899	0.017 mg/L

Acrylamide