Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\QuantResults\ACRYL.batch.bin				
Analysis Time	2026-02-19 오후 5:34:56	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:34:56	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Acrylamide

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
ACRYL ST-01.D	Cal	4.085	126	8603	0.005
ACRYL ST-02.D	Cal	4.079	343	8418	0.012
ACRYL ST-03.D	Cal	4.074	613	8805	0.019
ACRYL ST-04.D	Cal	4.106	168	8692	0.006
ACRYL ST-05.D	Cal	4.068	879	7808	0.030
ACRYL ST-06.D	Cal	4.068	1264	8275	0.041
BK-.D	Blank			7060	ND
FBK(GS 26-02-10).D	Blank			7616	ND
KH 26-02-10.D	Sample			8344	ND
GS-01.D	Sample	4.138	0	9251	ND
GS-02.D	Sample			8950	ND
GS-03.D	Sample			9786	ND
GS-04.D	Sample			9637	ND
GS-05.D	Sample			8333	ND
GS-06.D	Sample			9358	ND
GS-15.D	Sample			6123	ND
MBK-1.D	Blank			8931	ND
CCV-1.D	QC	4.068	678	8153	0.023

Acrylamide

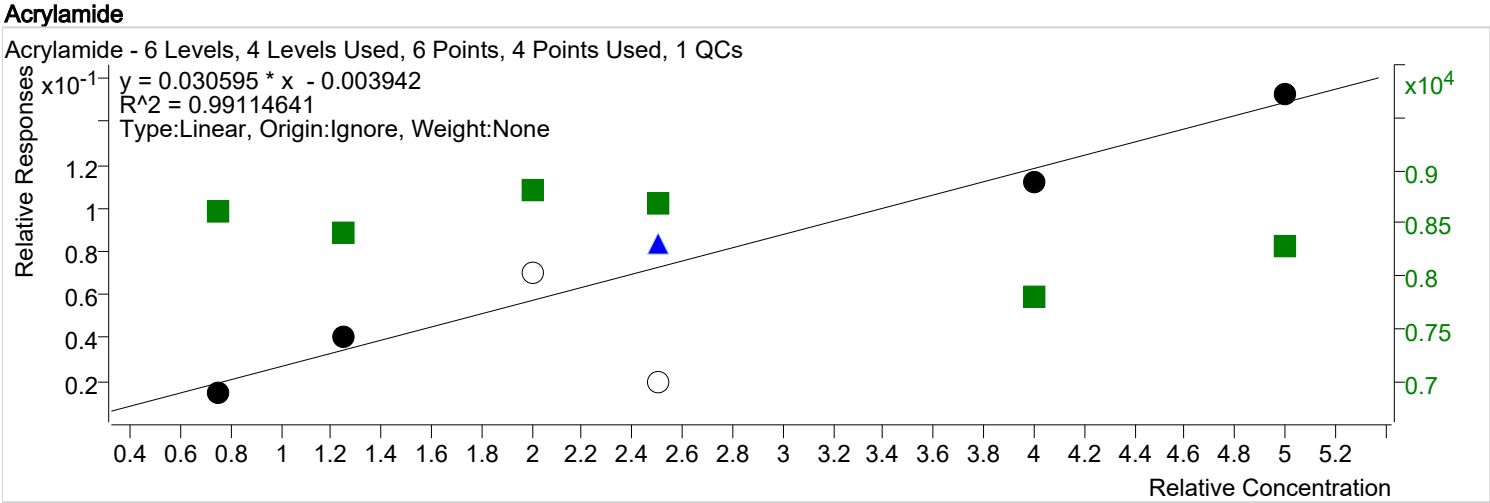

Cal. Path	Type	Level	Enable	Conc.	Response
\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\ACRYL ST-01.D	Calibration	1	x	3.000	126
\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\ACRYL ST-02.D	Calibration	2	x	5.000	343
\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\ACRYL ST-03.D	Calibration	3		8.000	613
\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\ACRYL ST-04.D	Calibration	4		10.000	168
\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\CCV-1.D	QC	4	x	10.000	678
\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\ACRYL ST-05.D	Calibration	5	x	16.000	879
\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\ACRYL ST-06.D	Calibration	6	x	20.000	1264

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-02-19 오후 5:34:56	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:13:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:34:56	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-13 오후 1:34:58	**Data File**	ACRYL ST-01.D
Type	Cal	**Name**	ACRYL ST-01
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

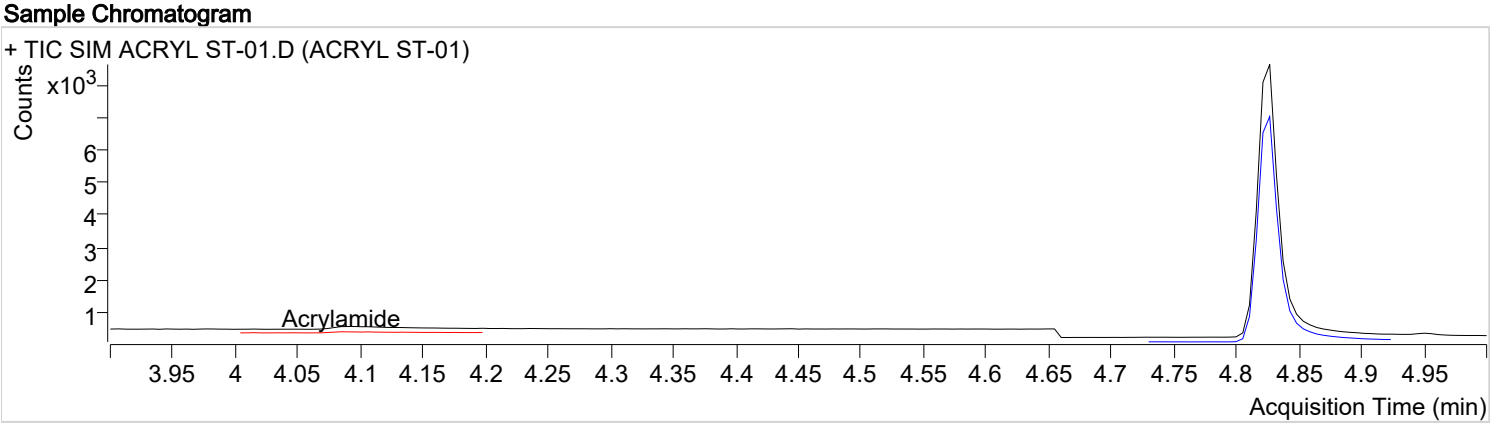

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.085	126	8603	0.005 mg/L

Acrylamide







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-02-19 오후 5:34:56	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:13:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:34:56	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-13 오후 1:43:43	**Data File**	ACRYL ST-02.D
Type	Cal	**Name**	ACRYL ST-02
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

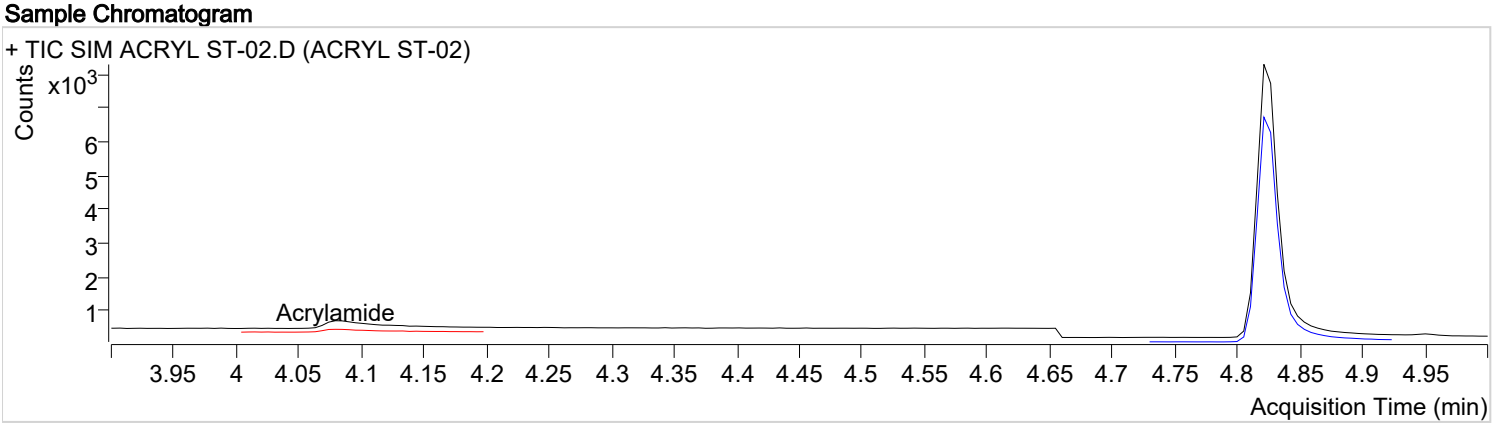

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.079	343	8418	0.012 mg/L

Acrylamide

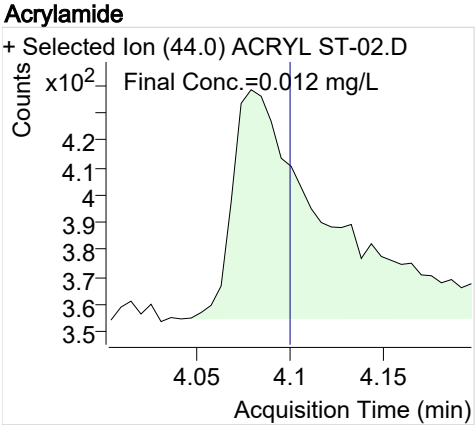





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-02-19 오후 5:34:56	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:13:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:34:56	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-13 오후 1:52:29	**Data File**	ACRYL ST-03.D
Type	Cal	**Name**	ACRYL ST-03
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

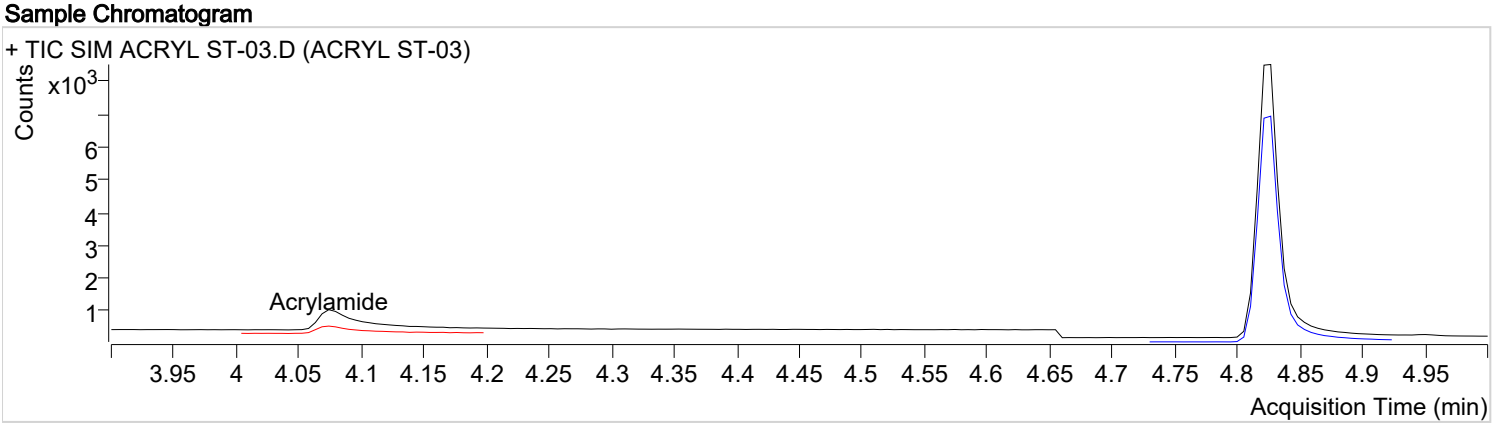

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.074	613	8805	0.019 mg/L

Acrylamide

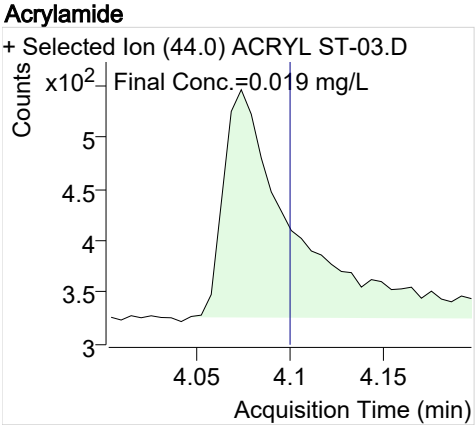





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-02-19 오후 5:34:56	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:13:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:34:56	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-13 오후 2:01:15	**Data File**	ACRYL ST-04.D
Type	Cal	**Name**	ACRYL ST-04
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

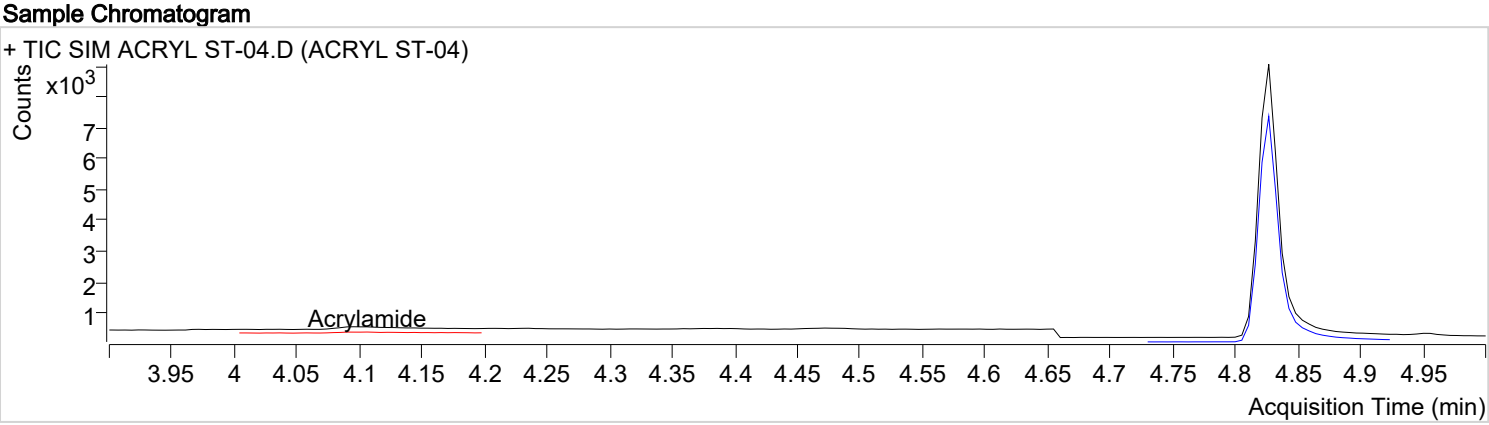

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.106	168	8692	0.006 mg/L

Acrylamide

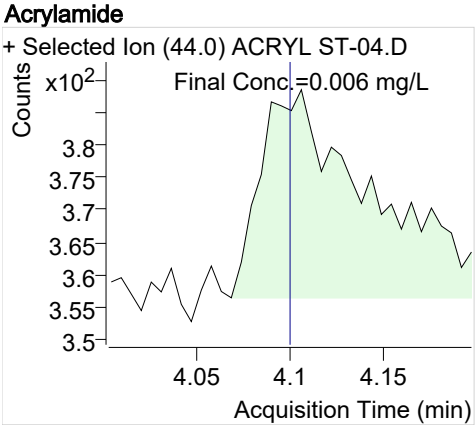





Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-02-19 오후 5:34:56	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:13:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:34:56	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-13 오후 2:10:03	**Data File**	ACRYL ST-05.D
Type	Cal	**Name**	ACRYL ST-05
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

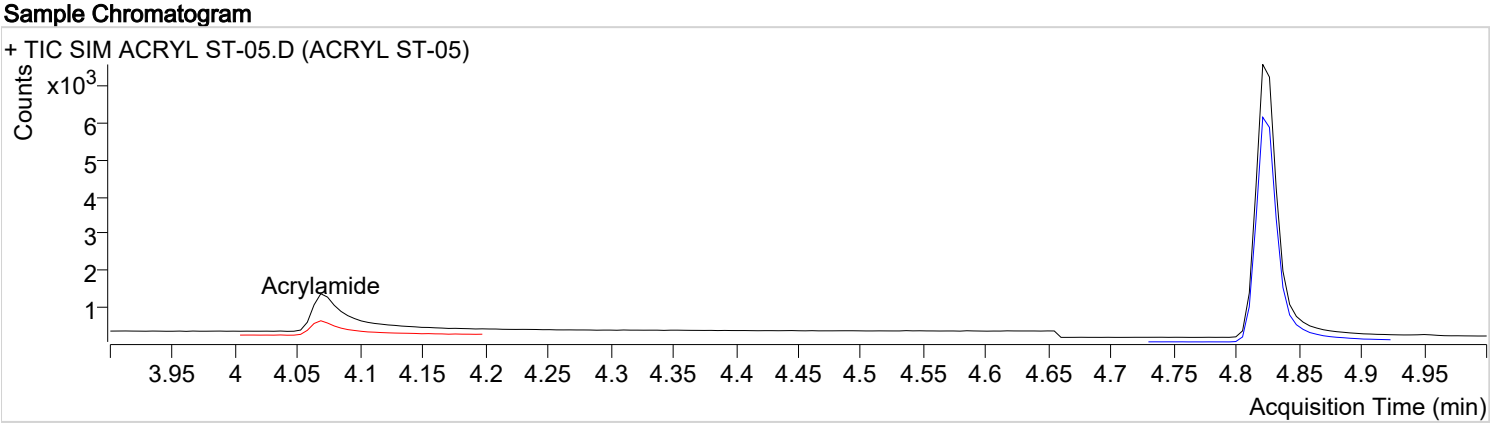

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.068	879	7808	0.030 mg/L

Acrylamide







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-02-19 오후 5:34:56	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:13:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:34:56	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-13 오후 2:18:53	**Data File**	ACRYL ST-06.D
Type	Cal	**Name**	ACRYL ST-06
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

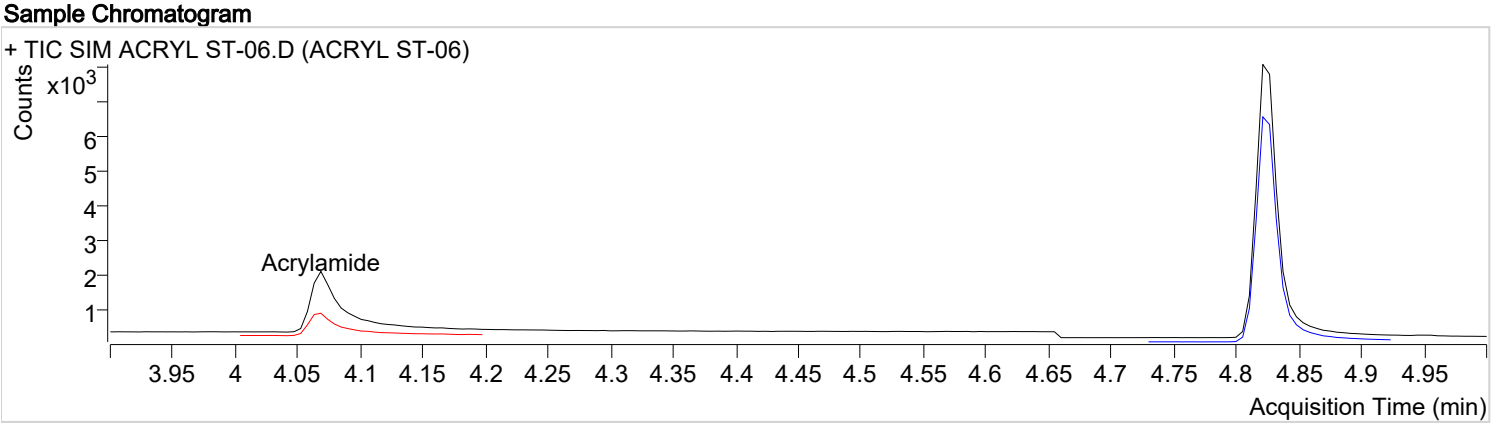

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.068	1264	8275	0.041 mg/L

Acrylamide

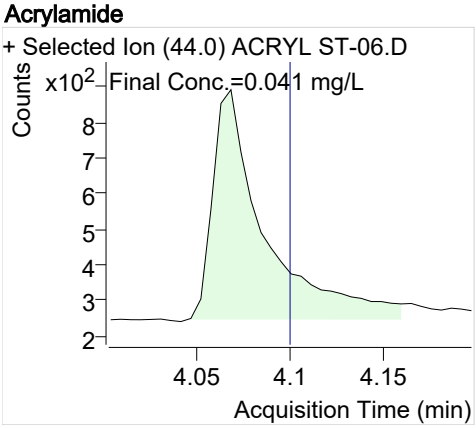





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-02-19 오후 5:34:56	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:13:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:34:56	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-13 오후 2:36:27	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

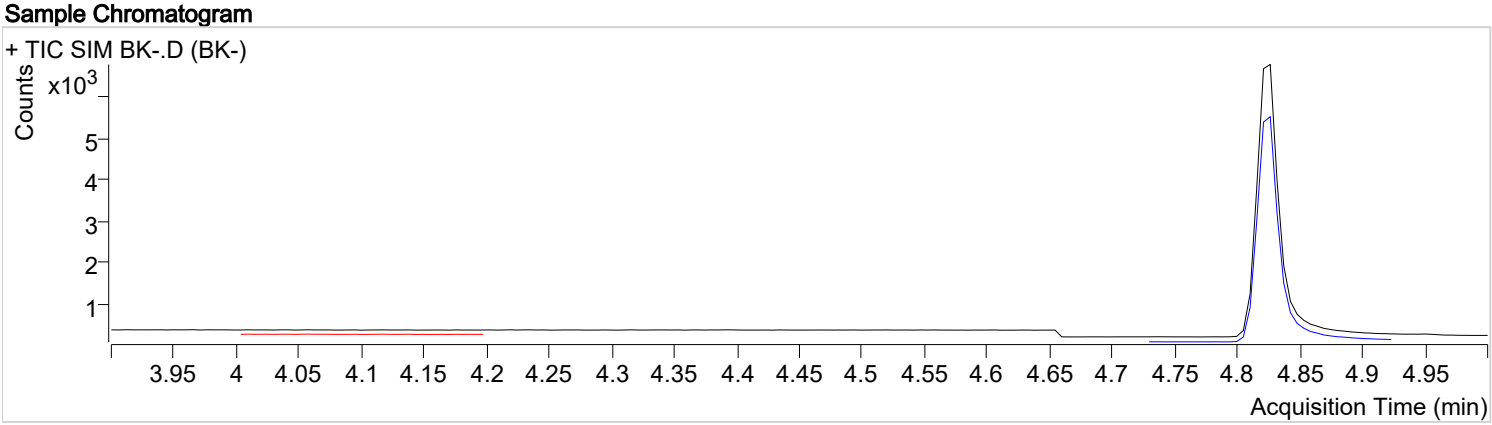

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide			7060	ND mg/L

Acrylamide

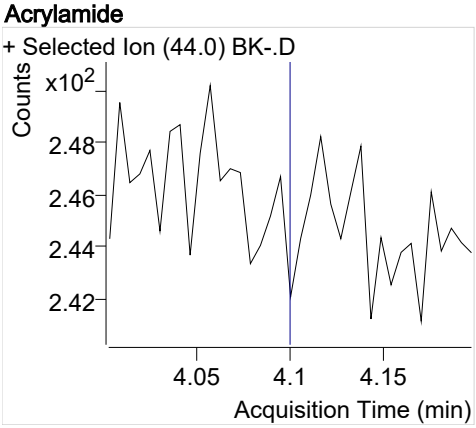





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-02-19 오후 5:34:56	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:13:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:34:56	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-13 오후 2:45:15	**Data File**	FBK(GS 26-02-10).D
Type	Blank	**Name**	FBK(GS 26-02-10)
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

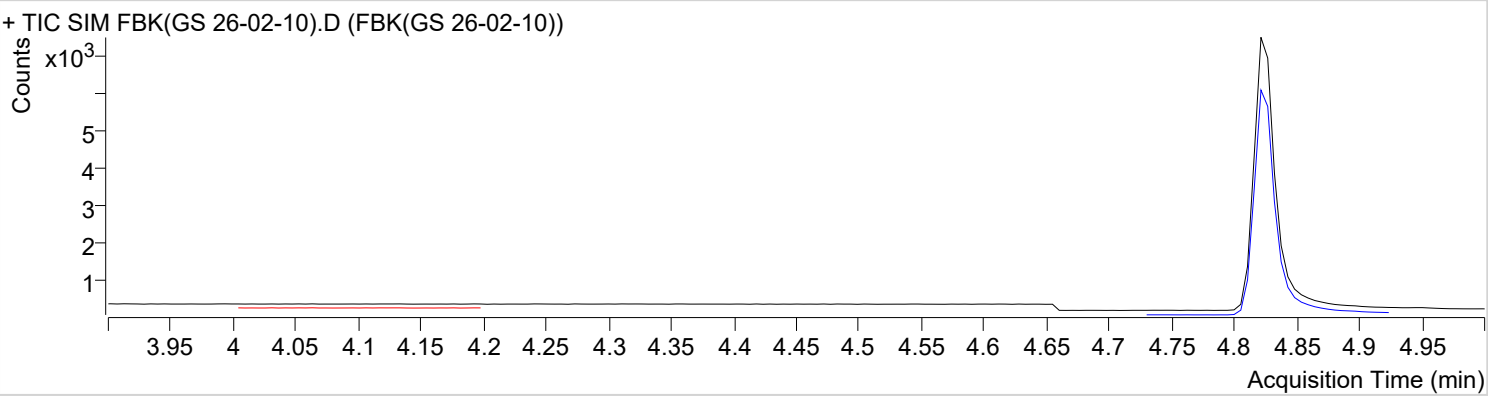

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide			7616	ND mg/L

Acrylamide







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-02-19 오후 5:34:56	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:13:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:34:56	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-13 오후 2:54:01	**Data File**	KH 26-02-10.D
Type	Sample	**Name**	KH 26-02-10
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

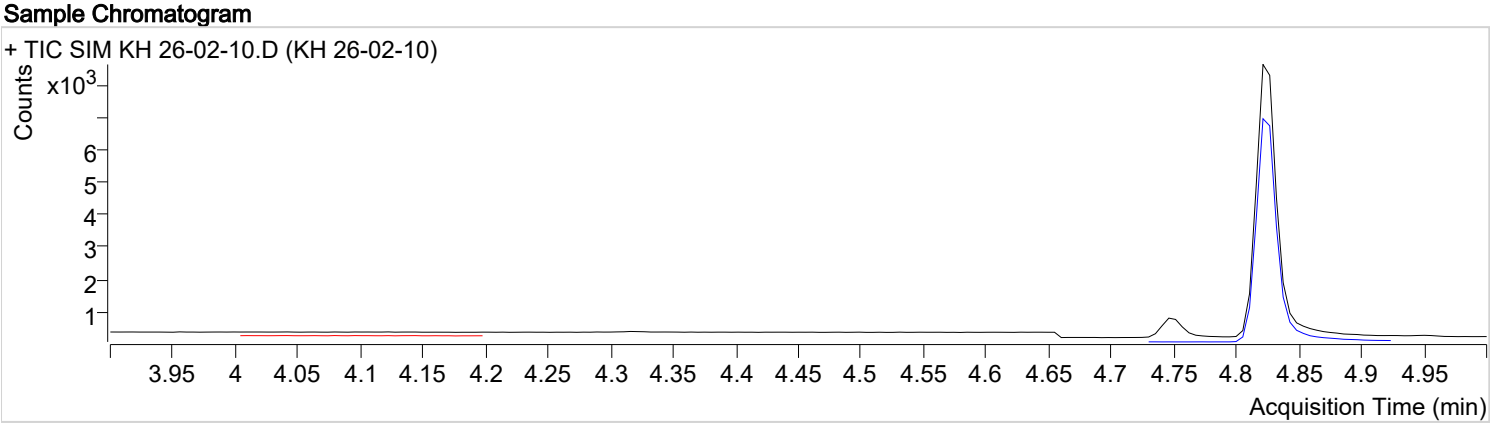

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide			8344	ND mg/L

Acrylamide







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-02-19 오후 5:34:56	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:13:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:34:56	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-13 오후 3:02:46	**Data File**	GS-01.D
Type	Sample	**Name**	GS-01
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

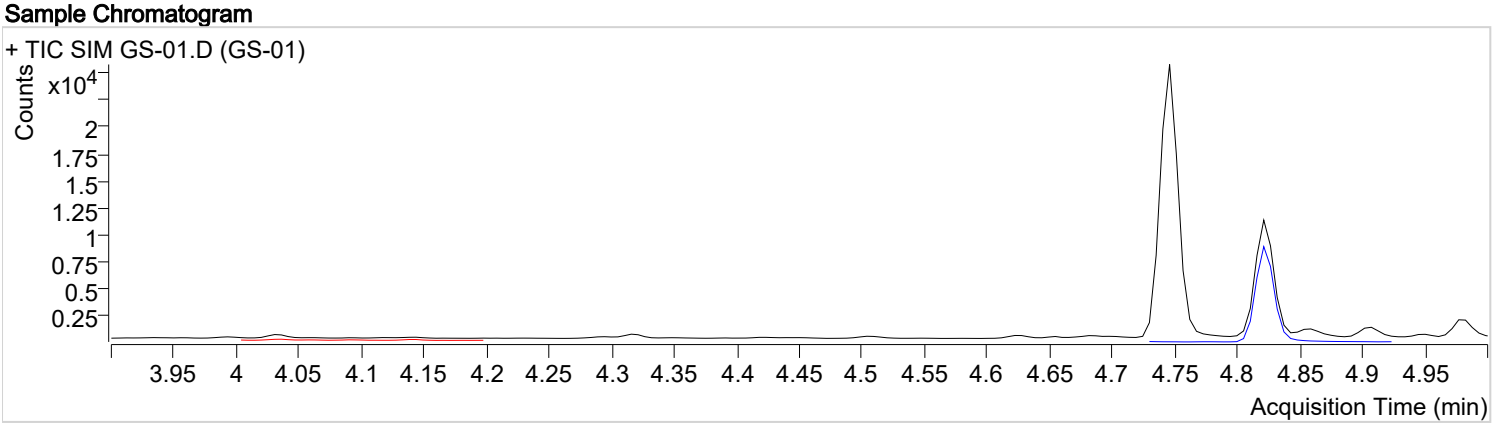

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.138	0	9251	ND mg/L

Acrylamide

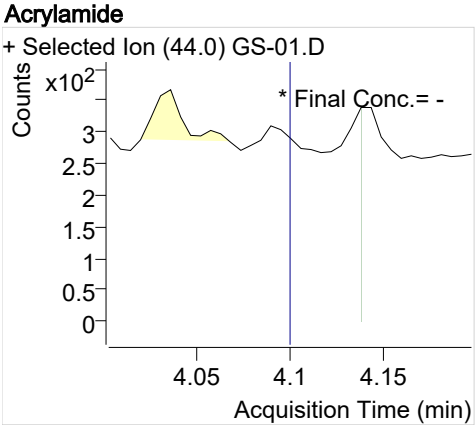





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-02-19 오후 5:34:56	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:13:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:34:56	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-13 오후 3:11:34	**Data File**	GS-02.D
Type	Sample	**Name**	GS-02
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

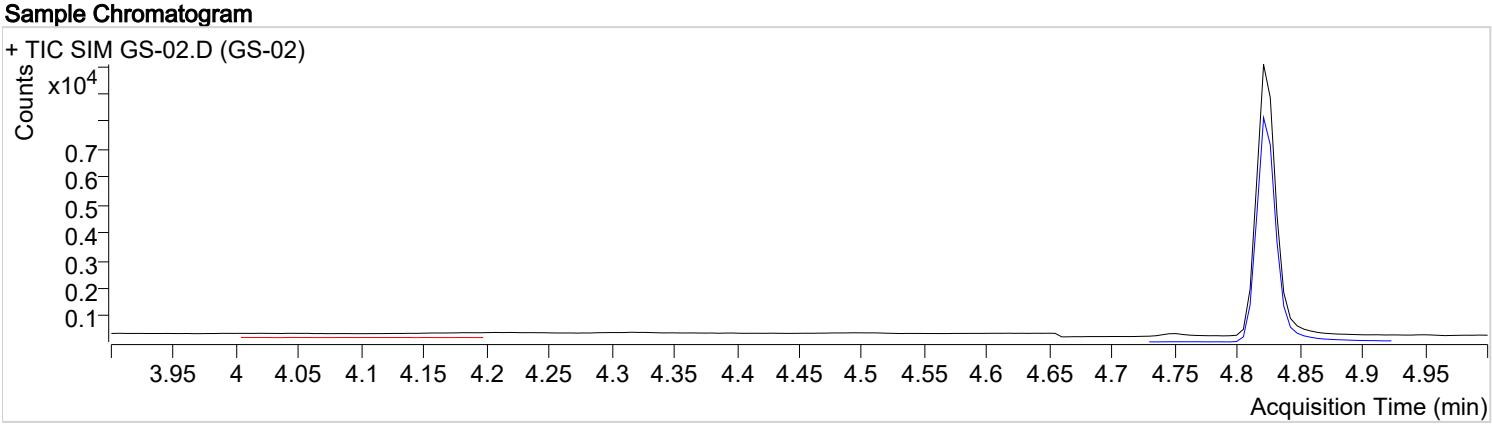

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide			8950	ND mg/L

Acrylamide







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-02-19 오후 5:34:56	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:13:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:34:56	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-13 오후 3:20:21	**Data File**	GS-03.D
Type	Sample	**Name**	GS-03
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

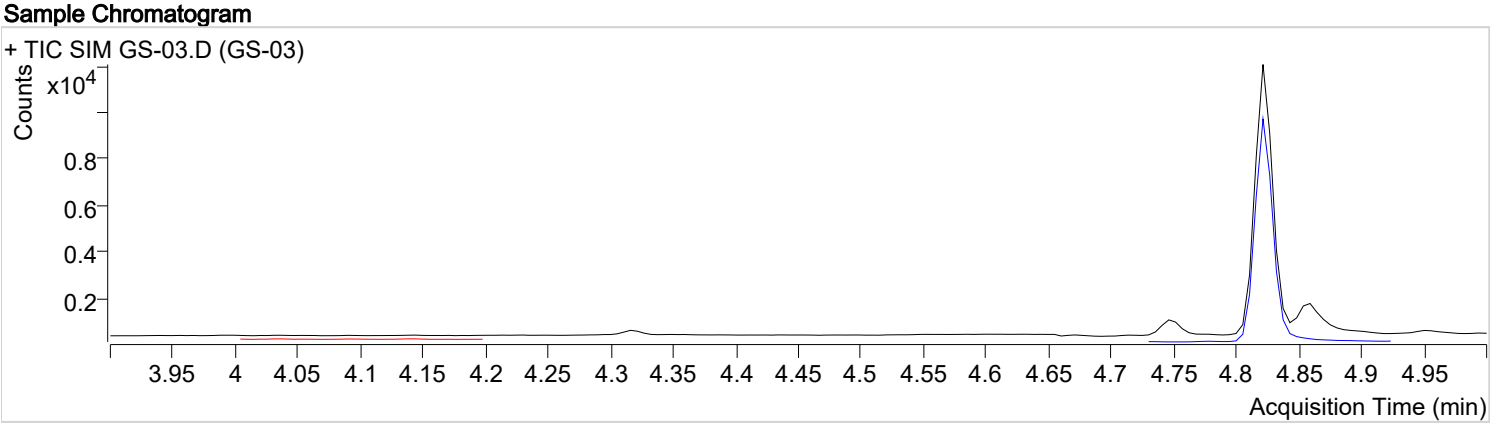

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide			9786	ND mg/L

Acrylamide







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-02-19 오후 5:34:56	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:13:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:34:56	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-13 오후 3:29:09	**Data File**	GS-04.D
Type	Sample	**Name**	GS-04
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

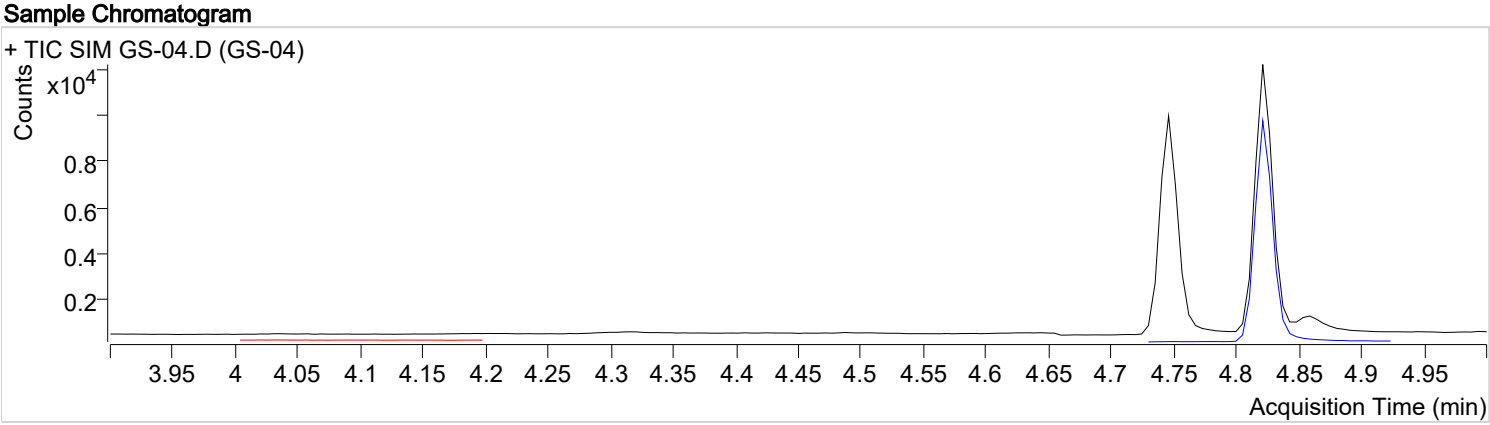

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide			9637	ND mg/L

Acrylamide







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-02-19 오후 5:34:56	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:13:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:34:56	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-13 오후 3:37:55	**Data File**	GS-05.D
Type	Sample	**Name**	GS-05
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

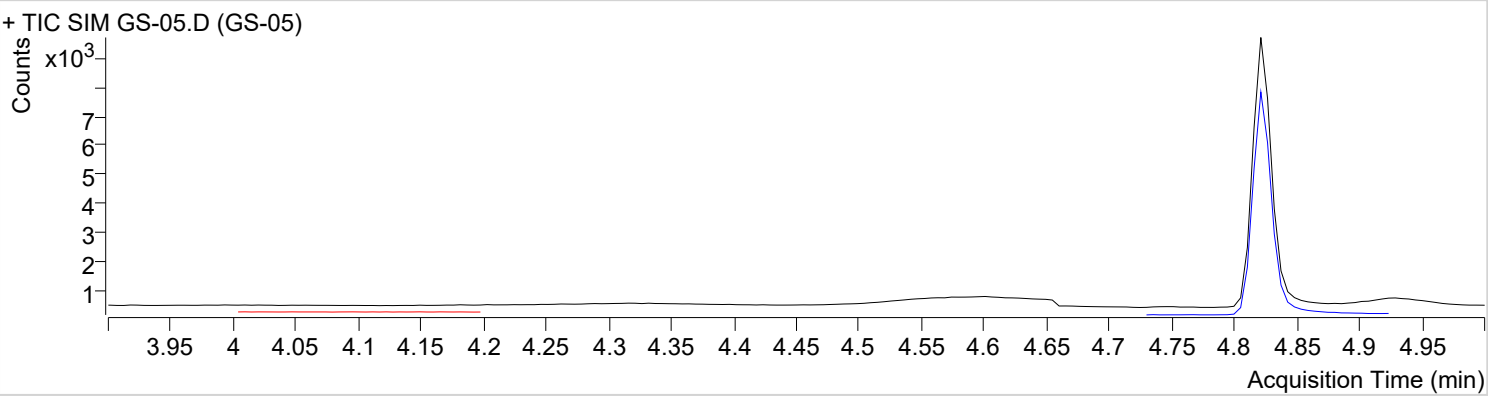

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide			8333	ND mg/L

Acrylamide

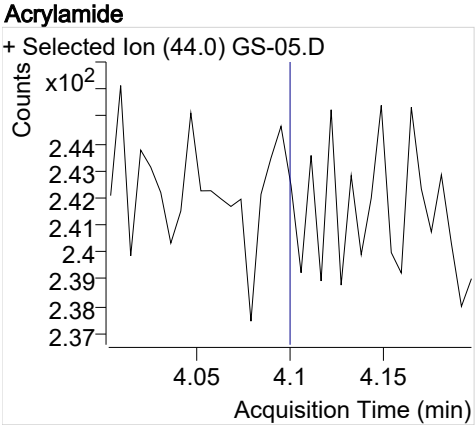





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-02-19 오후 5:34:56	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:13:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:34:56	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-13 오후 3:46:42	**Data File**	GS-06.D
Type	Sample	**Name**	GS-06
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

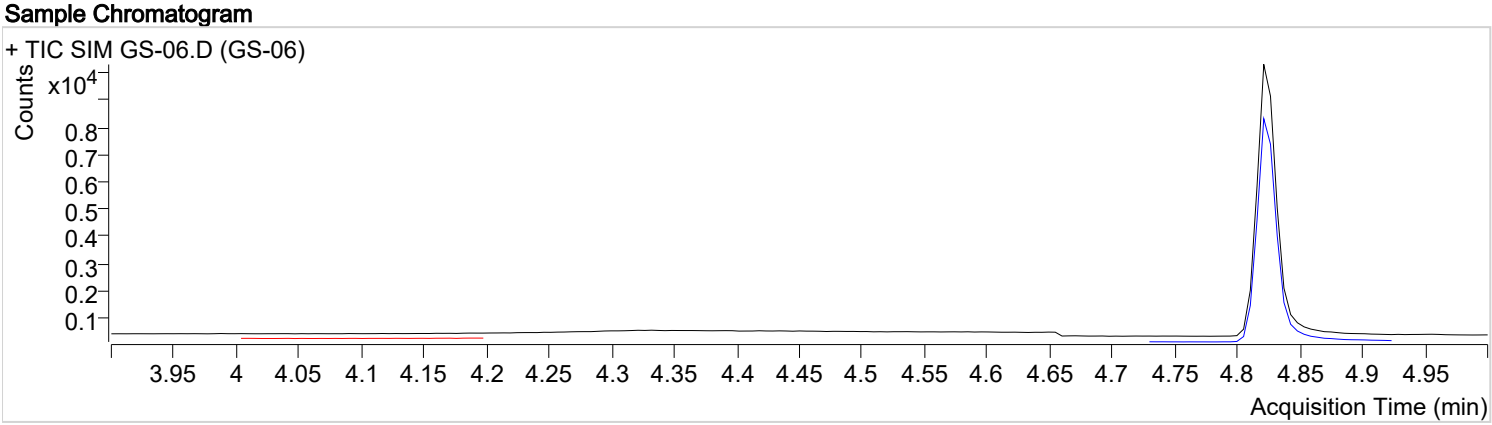

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide			9358	ND mg/L

Acrylamide







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-02-19 오후 5:34:56	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:13:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:34:56	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-13 오후 3:55:26	**Data File**	GS-15.D
Type	Sample	**Name**	GS-15
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

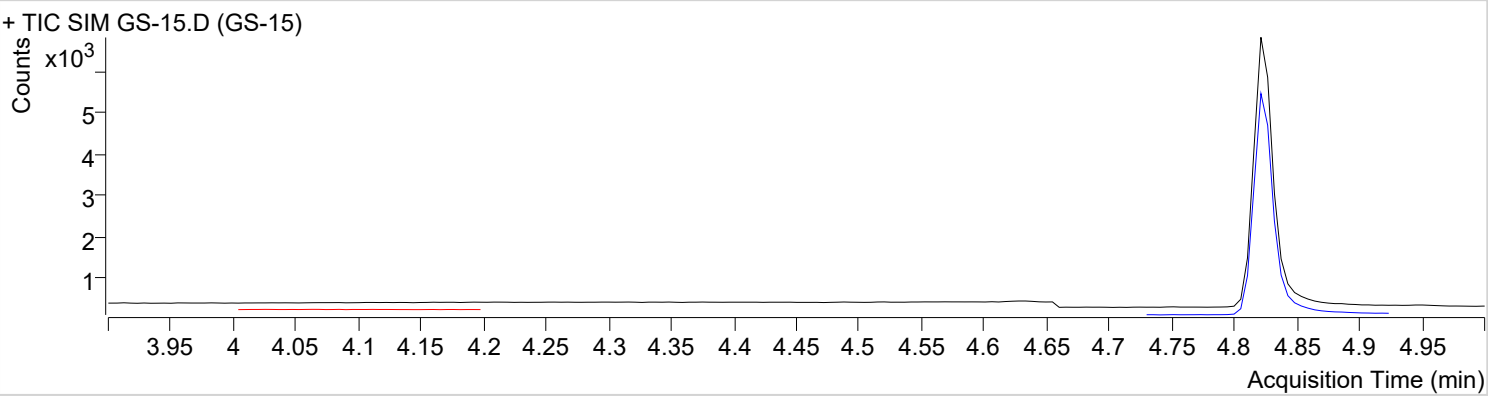

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide			6123	ND mg/L

Acrylamide

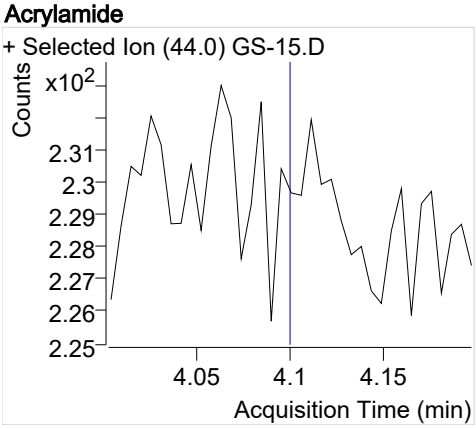



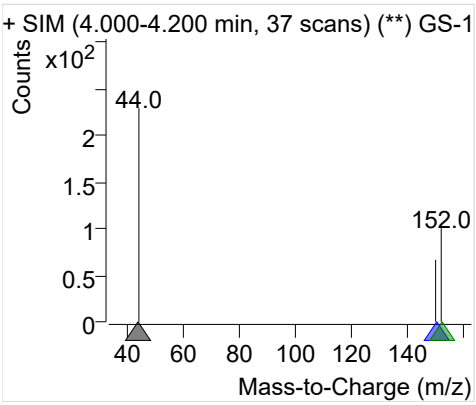

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-02-19 오후 5:34:56	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:13:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:34:56	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-13 오후 4:04:14	**Data File**	MBK-1.D
Type	Blank	**Name**	MBK-1
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

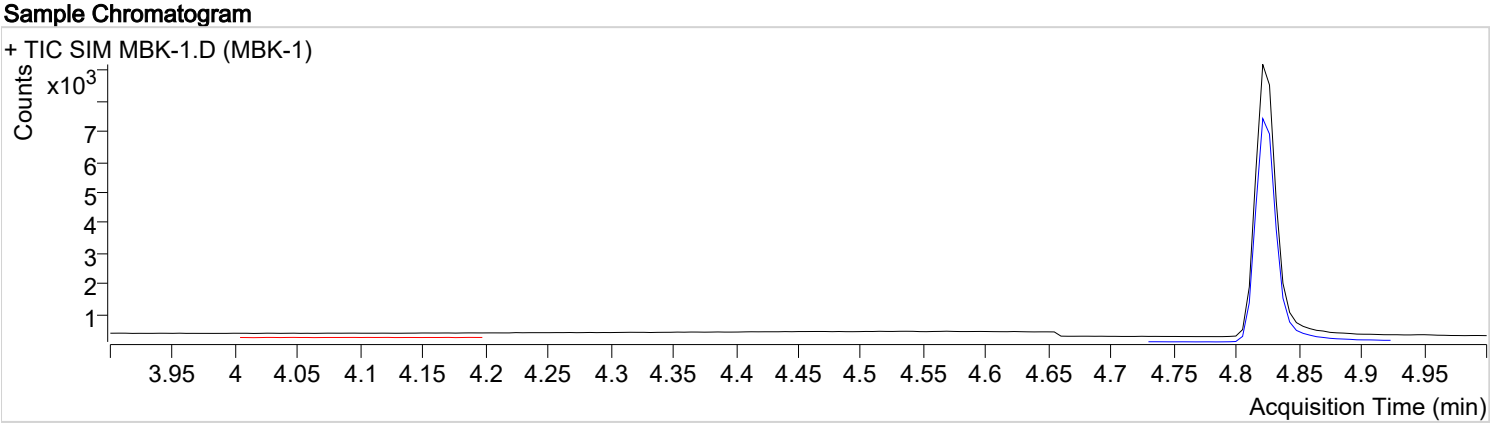

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide			8931	ND mg/L

Acrylamide







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\ACRYL(GS 2.10 KH 2.10)\QuantResults\ACRYL.batch.bin		
Analysis Time	2026-02-19 오후 5:34:56	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:13:08	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:34:56	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-13 오후 4:13:00	**Data File**	CCV-1.D
Type	QC	**Name**	CCV-1
Dil.	0.002	**Acq. Method File**	VOCs(Acrylamide)

Sample Chromatogram

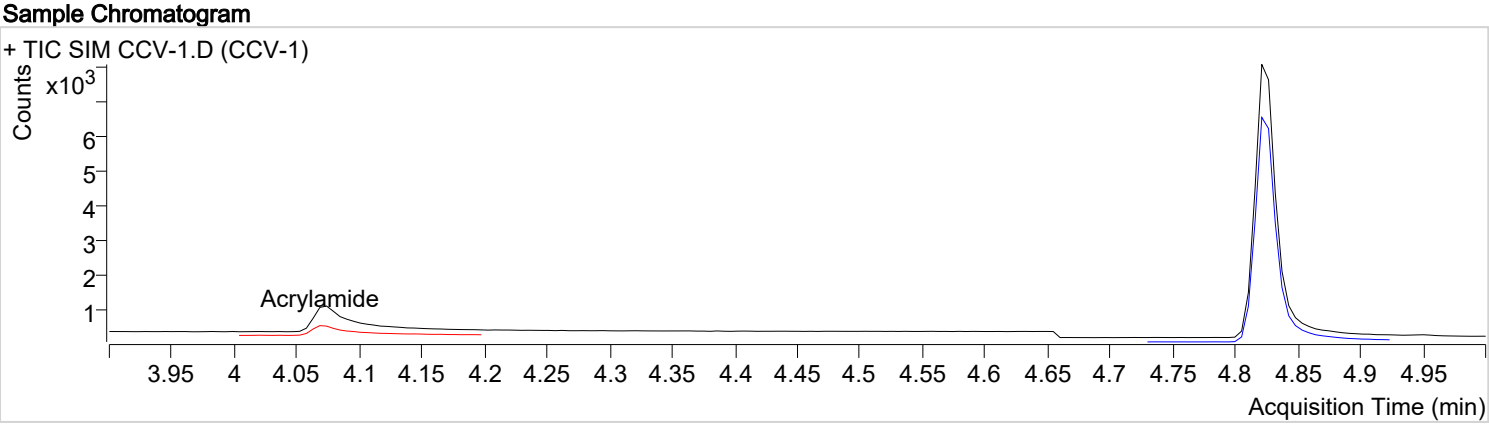

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Acrylamide	4.068	678	8153	0.023 mg/L

Acrylamide