Quantitative Analysis Results Summary Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\QuantResults\EPIC.batch.bin				
Analysis Time	2026-02-20 오후 1:14:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-20 오후 1:14:07	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Epichlorohydrin

Data File	Type	RT	Resp.	Final Conc.
EPIC ST-01.D	Cal	6.290	6069	0.195
EPIC ST-02.D	Cal	6.290	11683	0.462
EPIC ST-03.D	Cal	6.290	23430	1.021
EPIC ST-04.D	Cal	6.284	57451	2.639
EPIC ST-05.D	Cal	6.284	105664	4.933
BK-.D	Blank			ND
FBK(GS 26-02-10).D	Blank			ND
KH 26-02-10.D	Sample			ND
GS-01.D	Sample			ND
GS-02.D	Sample	6.290	61066	0.006
GS-03.D	Sample			ND
GS-04.D	Sample			ND
GS-05.D	Sample			ND
GS-06.D	Sample			ND
GS-15.D	Sample	6.290	0	ND
MBK.D	Blank			ND
CCV.D	QC	6.284	58311	2.680

Epichlorohydrin

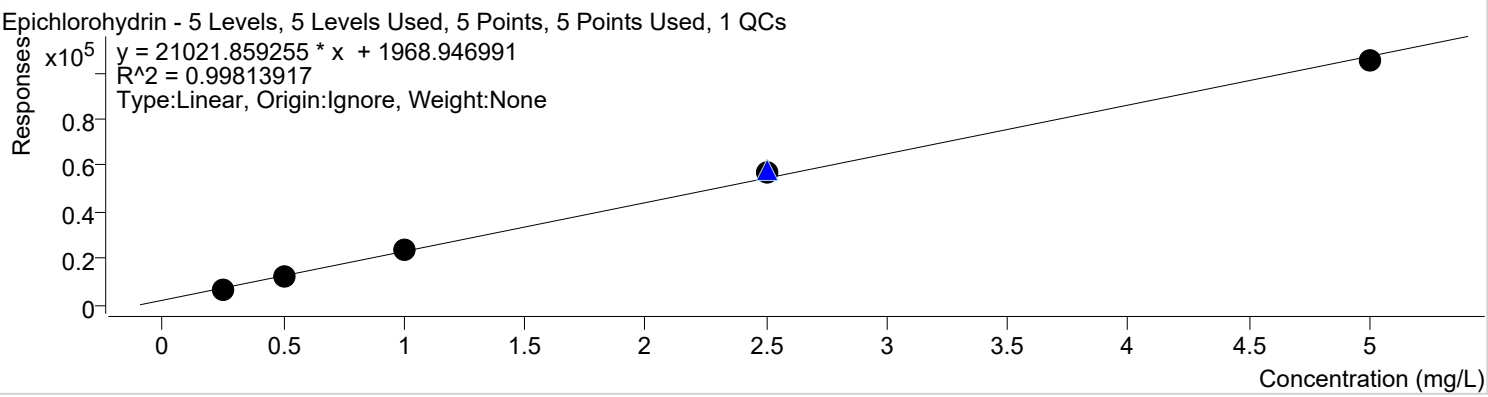

Cal. Path	Type	Level	Enable	Conc.	Response
D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\EPIC ST-01.D	Calibration	1	x	0.250	6069
D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\EPIC ST-02.D	Calibration	2	x	0.500	11683
D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\EPIC ST-03.D	Calibration	3	x	1.000	23430
D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\EPIC ST-04.D	Calibration	4	x	2.500	57451
D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\CCV.D	QC	4	x	2.500	58311
D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\EPIC ST-05.D	Calibration	5	x	5.000	105664

Quant Sample Report

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-02-20 오후 1:14:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:48:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-20 오후 1:14:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-20 오전 8:37:32	**Data File**	EPIC ST-01.D
Type	Cal	**Name**	EPIC ST-01
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

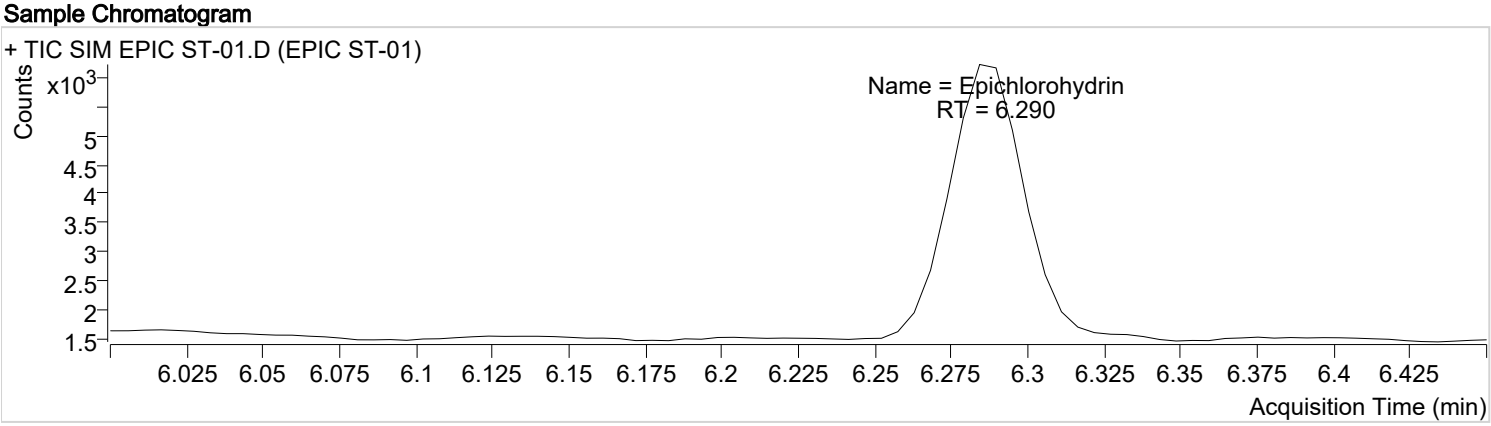

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	6069	0.195	mg/L

Epichlorohydrin

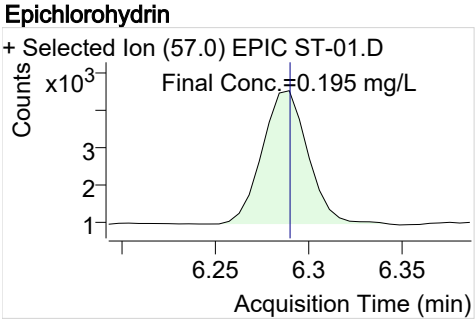

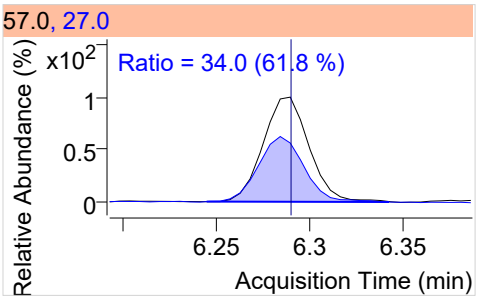

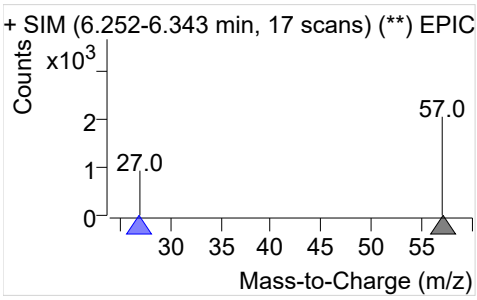

Quant Sample Report

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-02-20 오후 1:14:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:48:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-20 오후 1:14:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-20 오전 8:47:47	**Data File**	EPIC ST-02.D
Type	Cal	**Name**	EPIC ST-02
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

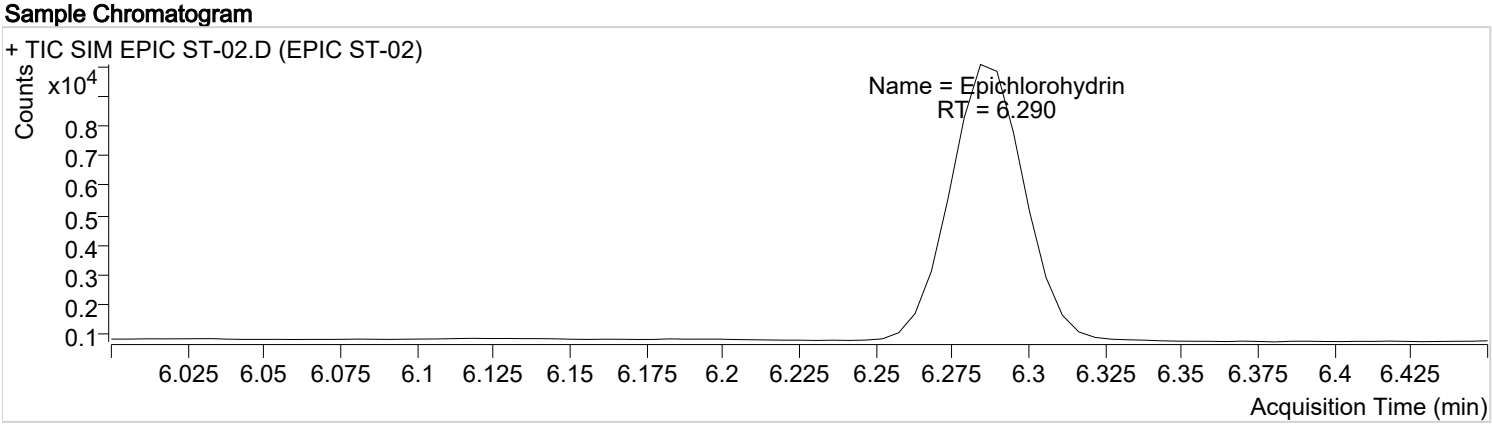

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	11683	0.462	mg/L

Epichlorohydrin

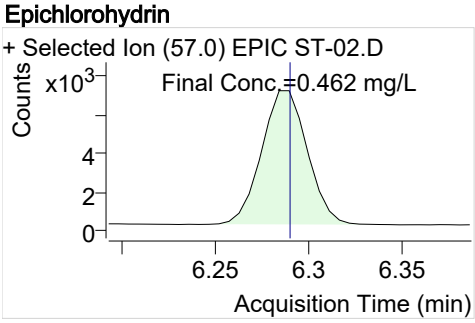

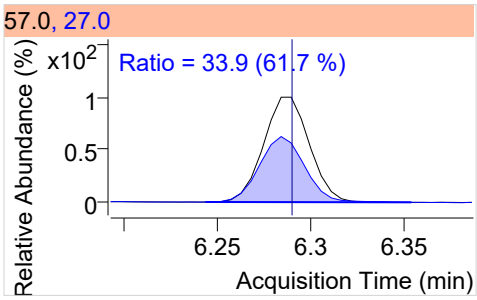

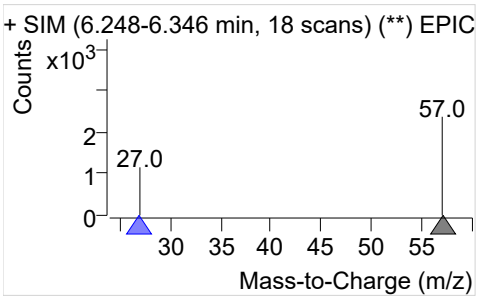

Quant Sample Report

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-02-20 오후 1:14:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:48:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-20 오후 1:14:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-20 오전 8:58:01	**Data File**	EPIC ST-03.D
Type	Cal	**Name**	EPIC ST-03
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

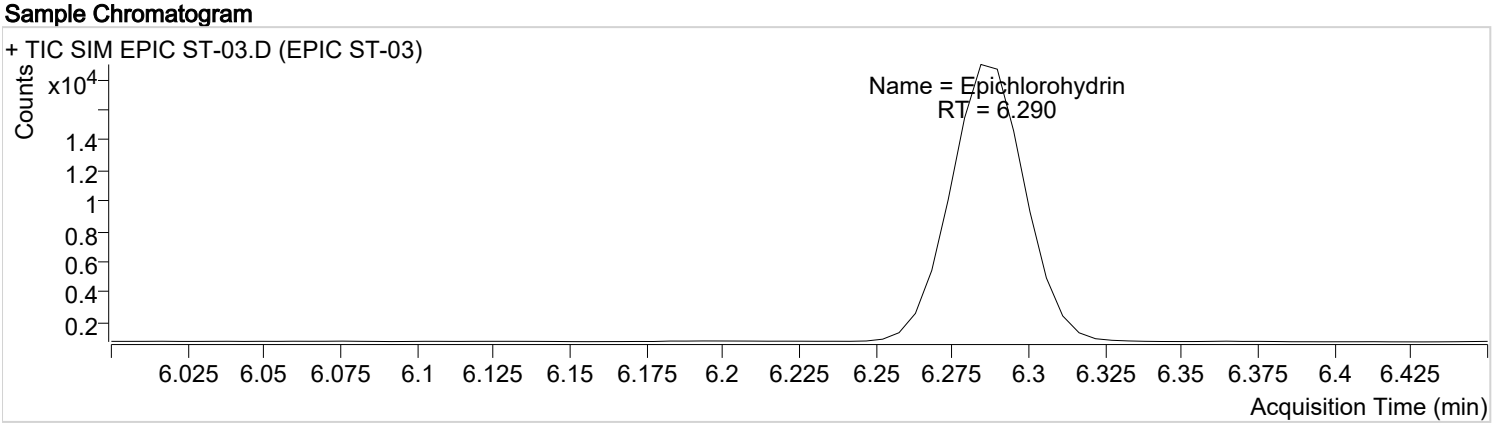

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	23430	1.021	mg/L

Epichlorohydrin

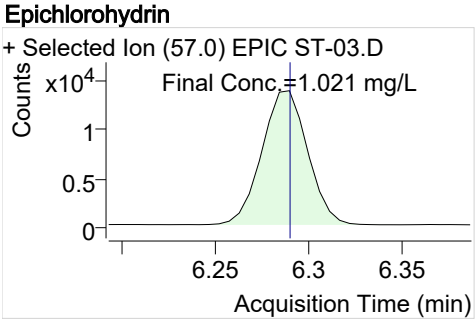

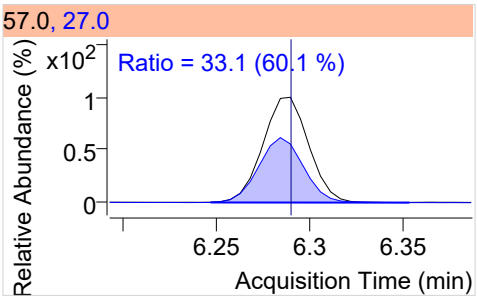

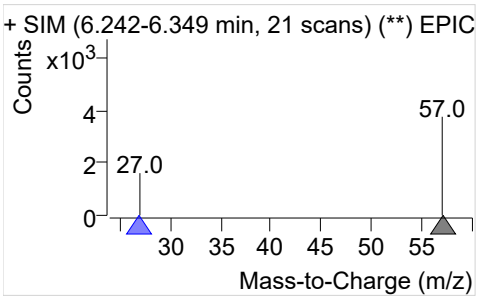

Quant Sample Report

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-02-20 오후 1:14:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:48:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-20 오후 1:14:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-20 오전 9:08:12	**Data File**	EPIC ST-04.D
Type	Cal	**Name**	EPIC ST-04
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

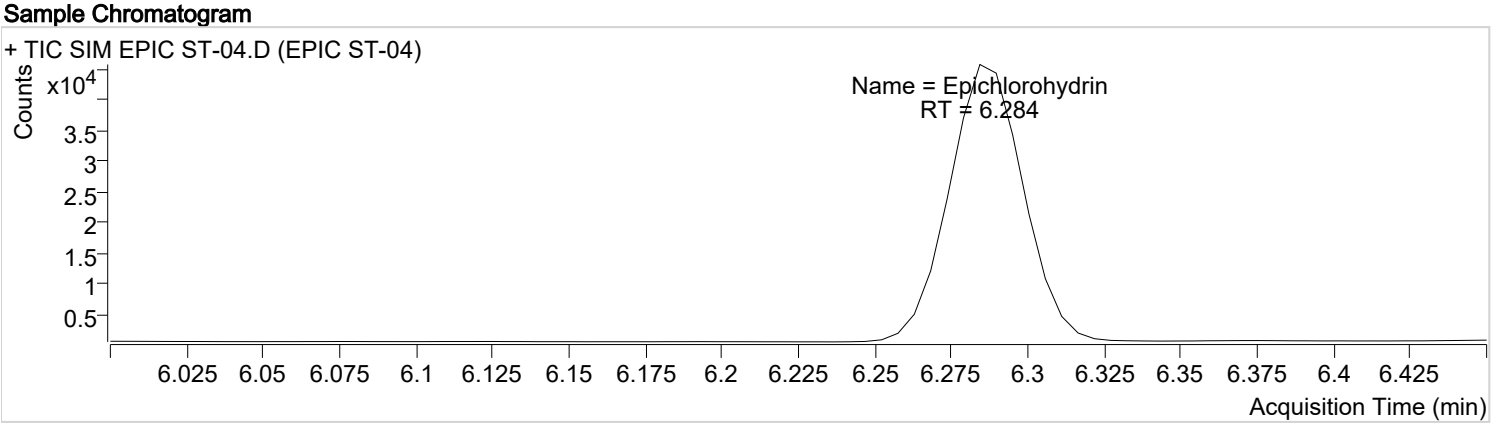

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.284	57451	2.639	mg/L

Epichlorohydrin

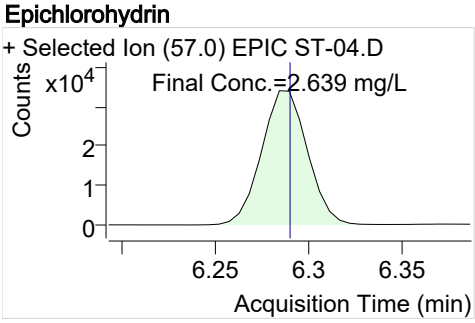



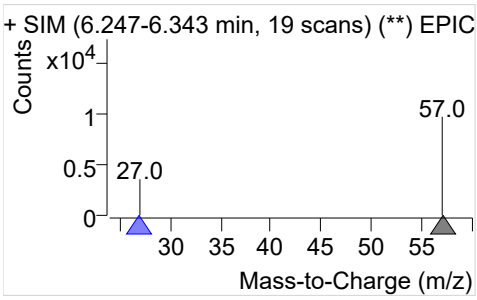

Quant Sample Report

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-02-20 오후 1:14:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:48:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-20 오후 1:14:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-20 오전 9:18:24	**Data File**	EPIC ST-05.D
Type	Cal	**Name**	EPIC ST-05
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

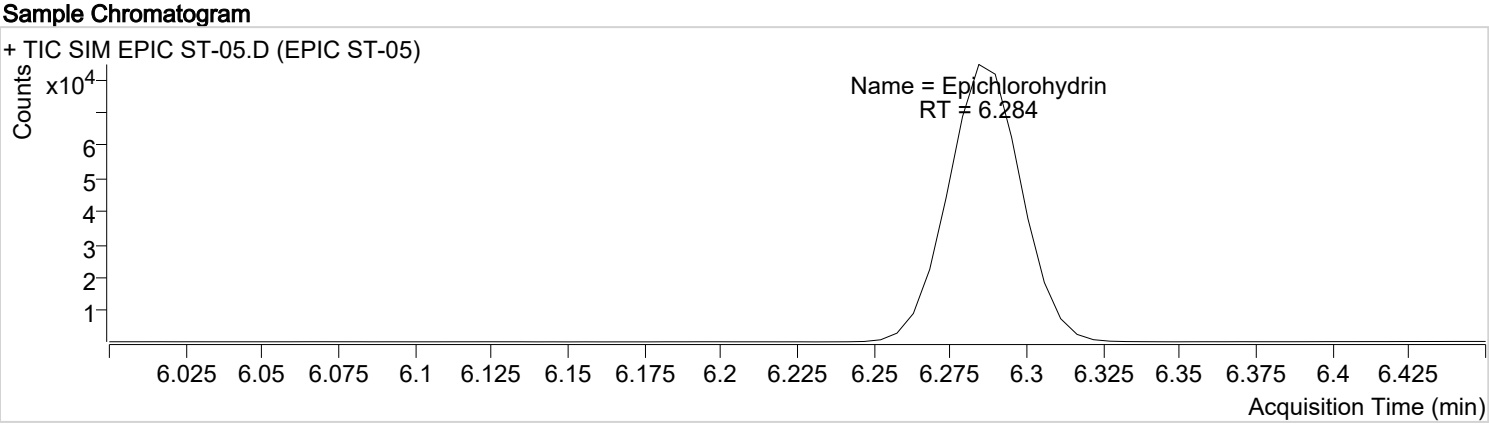

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.284	105664	4.933	mg/L

Epichlorohydrin

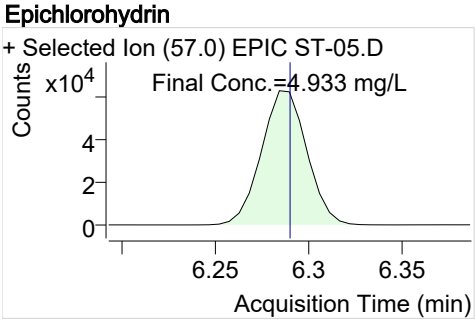





Quant Sample Report

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-02-20 오후 1:14:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:48:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-20 오후 1:14:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-20 오전 9:38:50	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

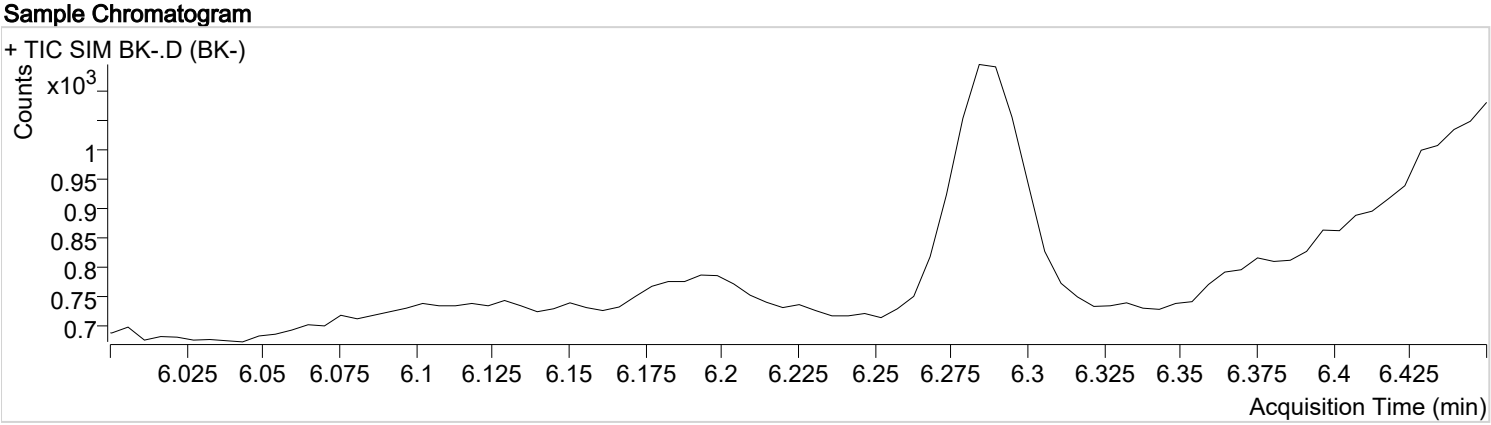

Epichlorohydrin

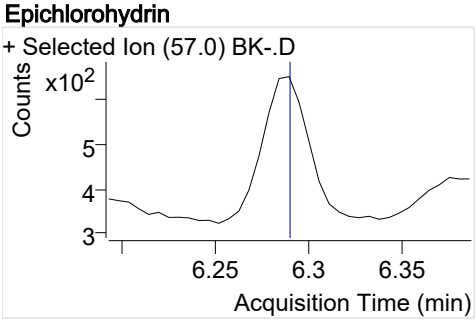



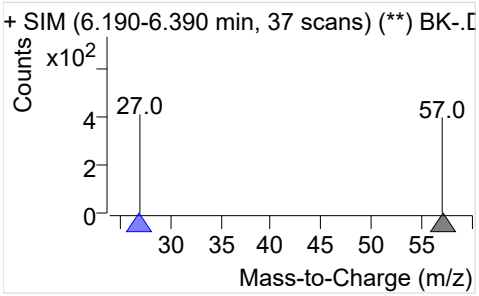

Quant Sample Report

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-02-20 오후 1:14:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:48:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-20 오후 1:14:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-20 오전 9:49:03	**Data File**	FBK(GS 26-02-10).D
Type	Blank	**Name**	FBK(GS 26-02-10)
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

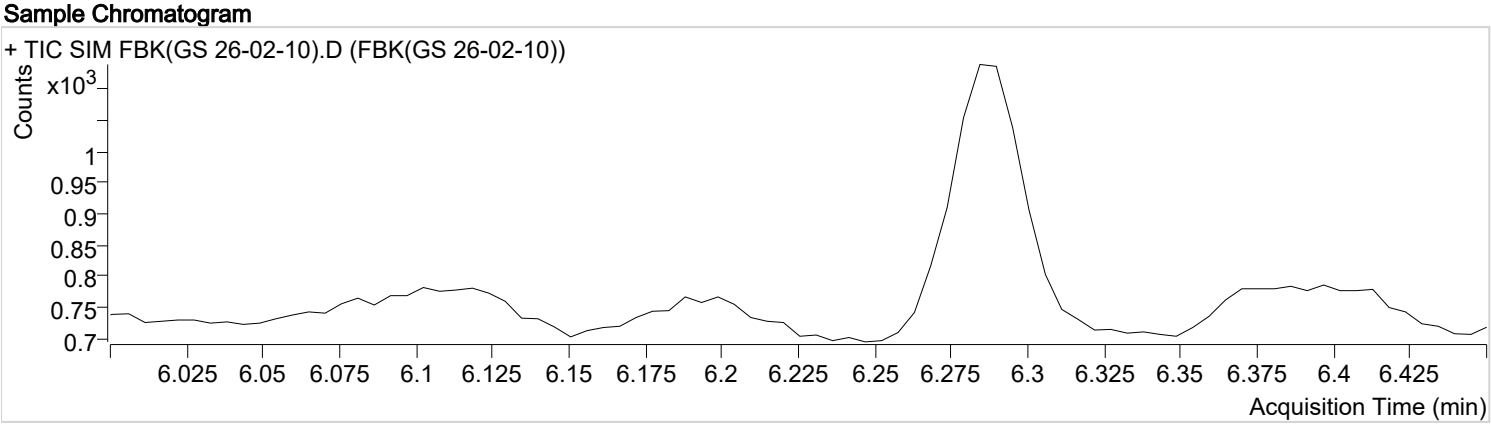

Epichlorohydrin

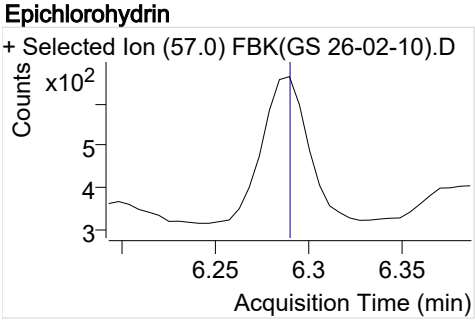



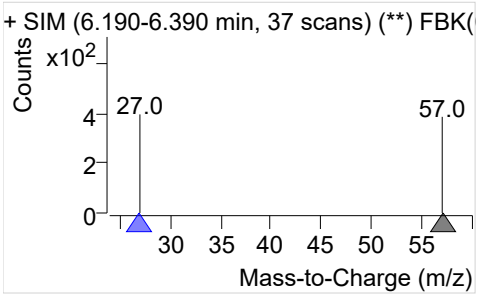

Quant Sample Report

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-02-20 오후 1:14:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:48:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-20 오후 1:14:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-20 오전 9:59:14	**Data File**	KH 26-02-10.D
Type	Sample	**Name**	KH 26-02-10
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

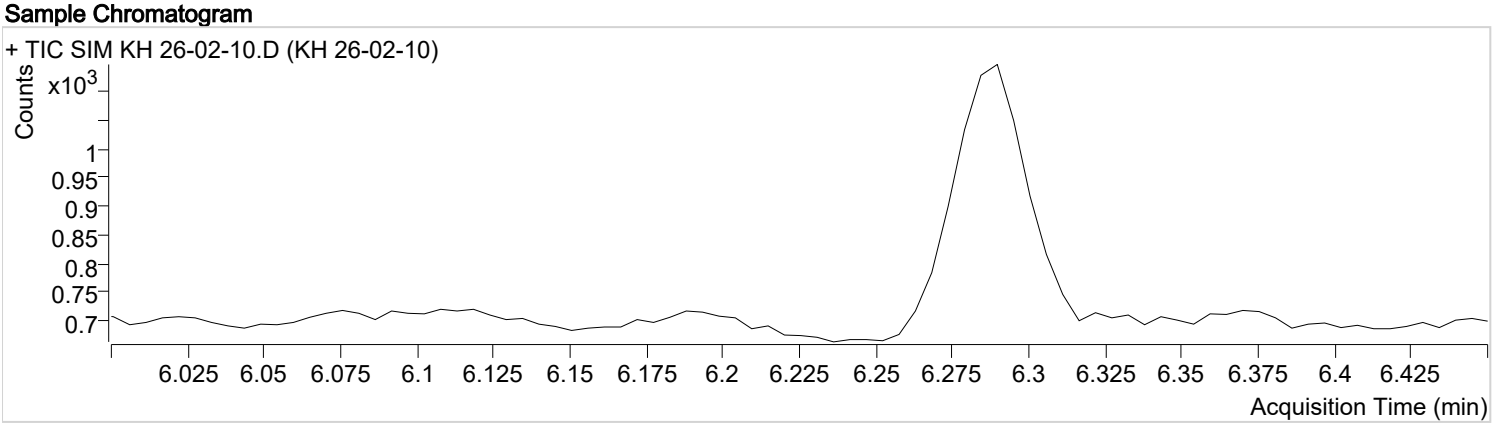

Epichlorohydrin

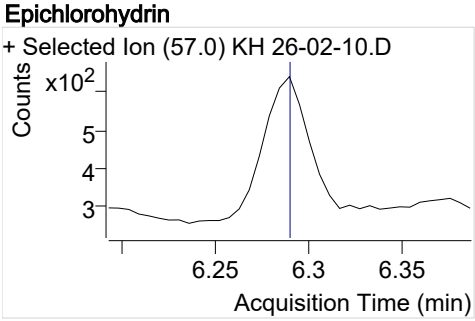



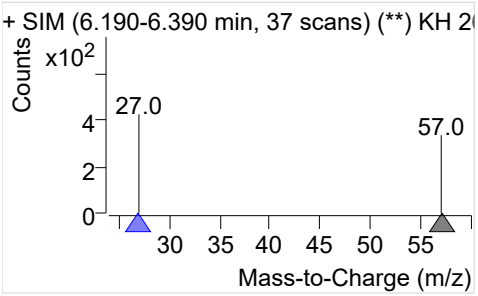

Quant Sample Report

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-02-20 오후 1:14:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:48:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-20 오후 1:14:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-20 오전 10:09:27	**Data File**	GS-01.D
Type	Sample	**Name**	GS-01
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

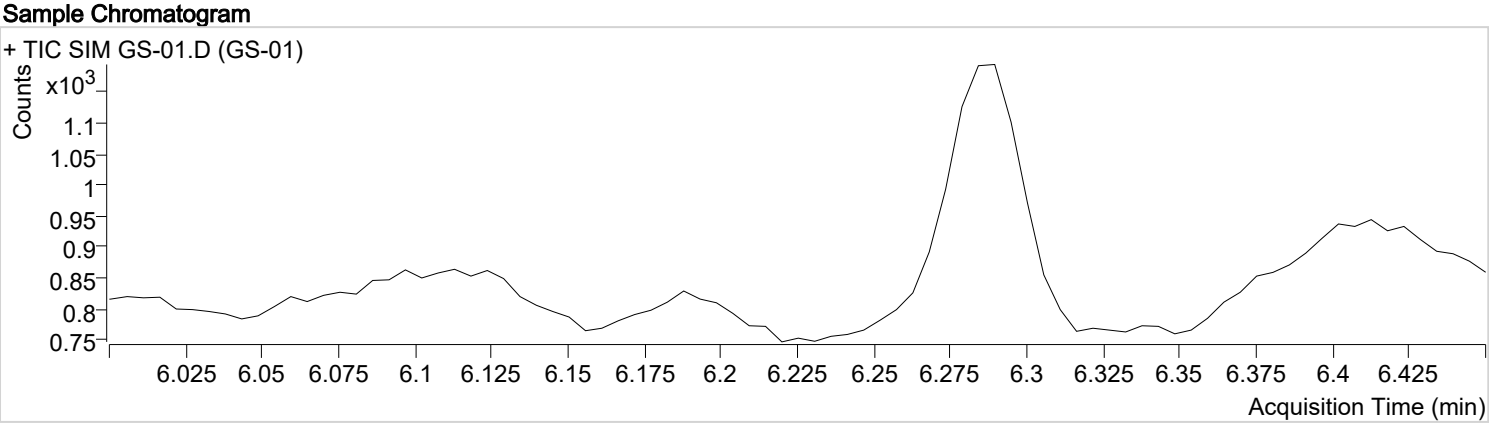

Epichlorohydrin

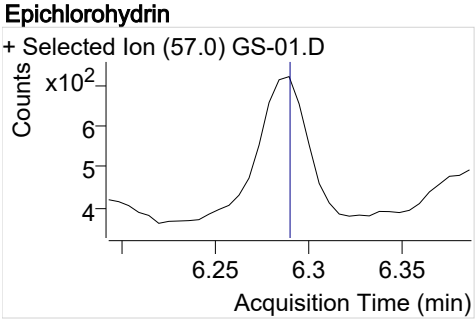



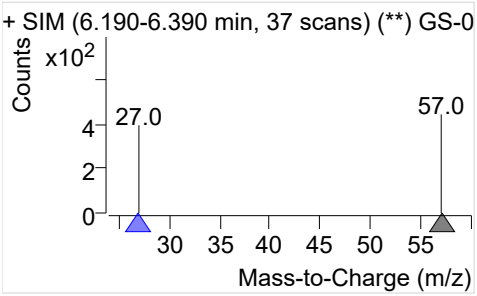

Quant Sample Report

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-02-20 오후 1:14:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:48:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-20 오후 1:14:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-20 오전 10:19:39	**Data File**	GS-02.D
Type	Sample	**Name**	GS-02
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

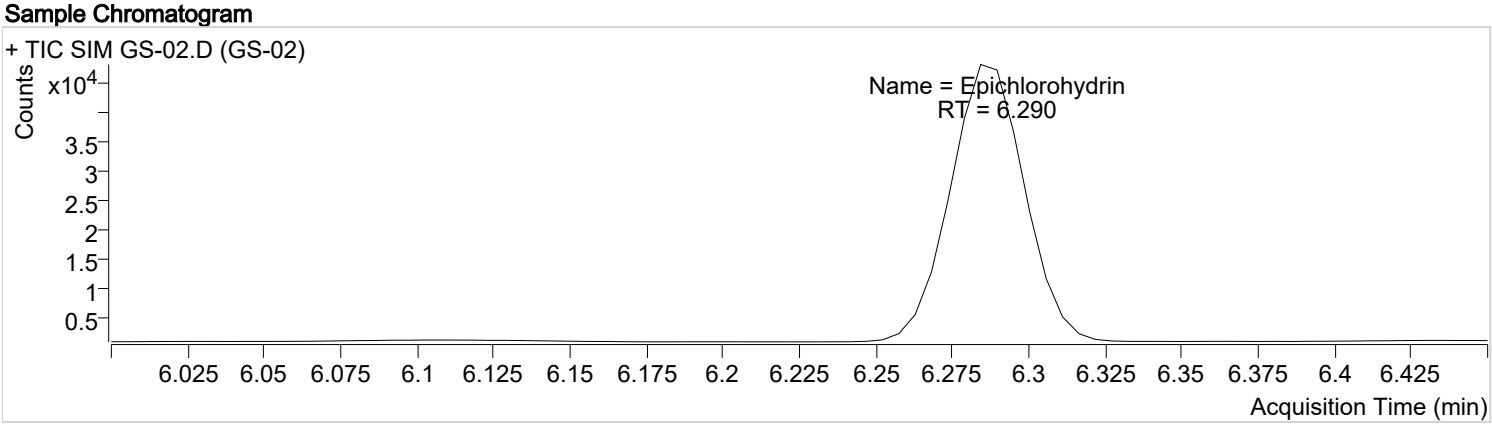

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	61066	0.006	mg/L

Epichlorohydrin

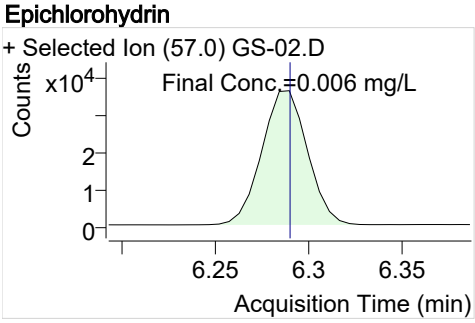



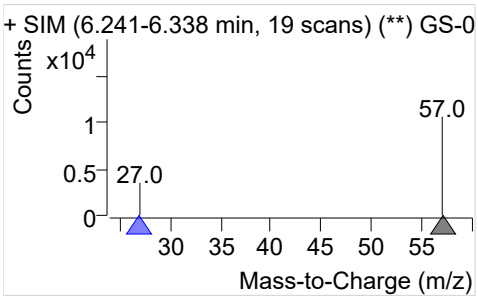

Quant Sample Report

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-02-20 오후 1:14:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:48:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-20 오후 1:14:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-20 오전 10:29:55	**Data File**	GS-03.D
Type	Sample	**Name**	GS-03
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

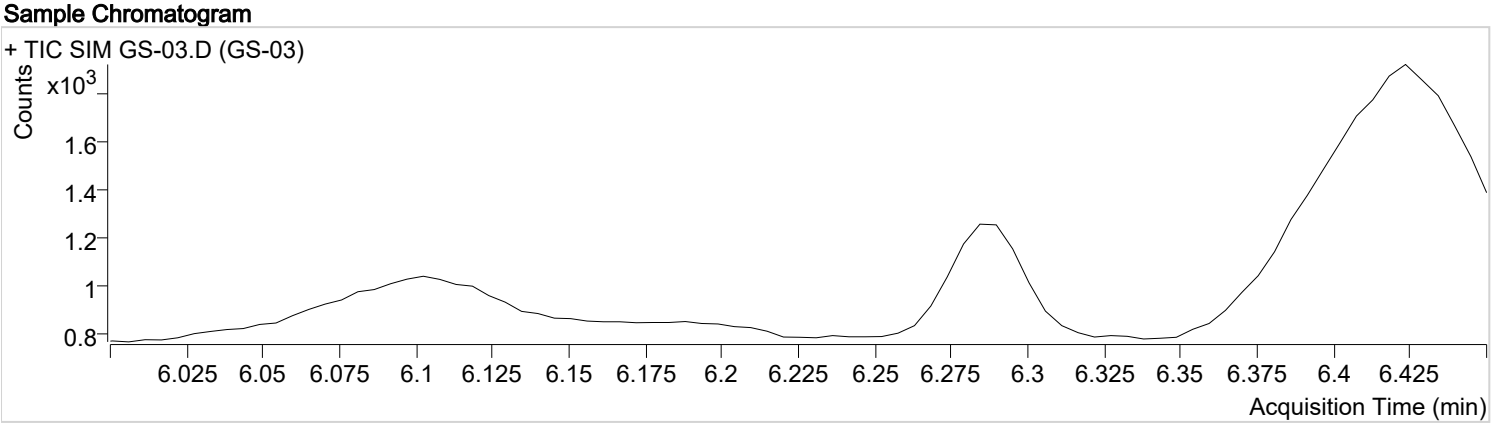

Epichlorohydrin

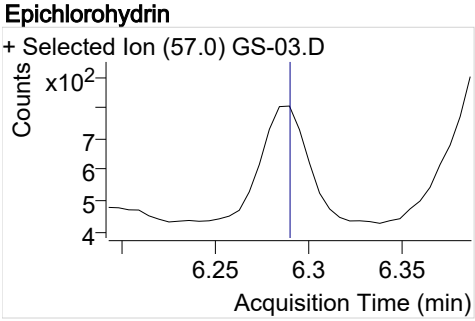



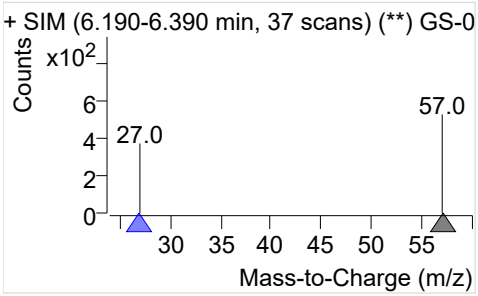

Quant Sample Report

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-02-20 오후 1:14:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:48:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-20 오후 1:14:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-20 오전 10:40:11	**Data File**	GS-04.D
Type	Sample	**Name**	GS-04
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

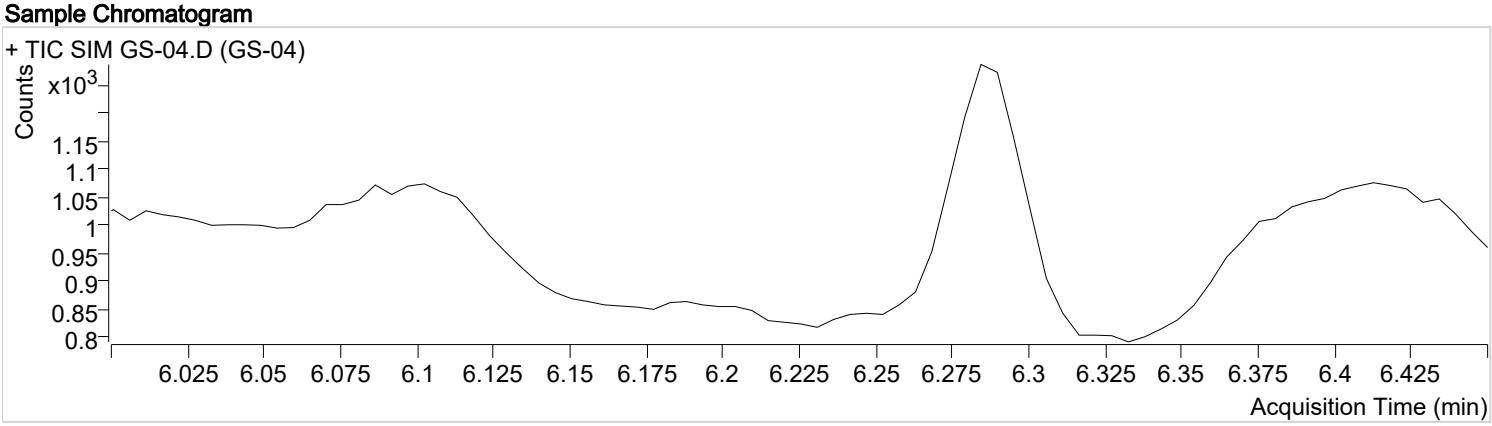

Epichlorohydrin

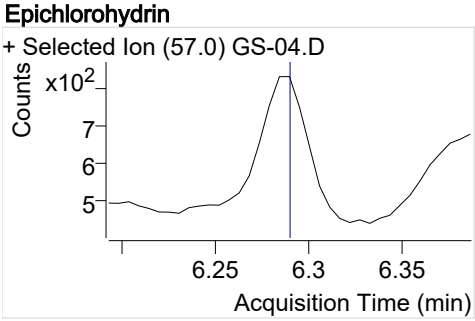



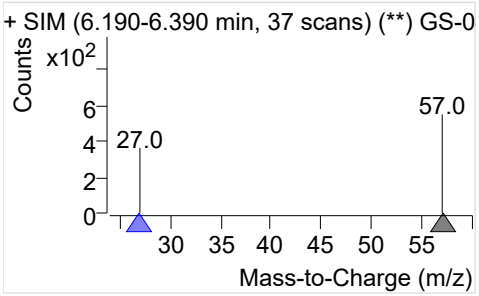

Quant Sample Report

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-02-20 오후 1:14:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:48:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-20 오후 1:14:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-20 오전 10:50:24	**Data File**	GS-05.D
Type	Sample	**Name**	GS-05
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

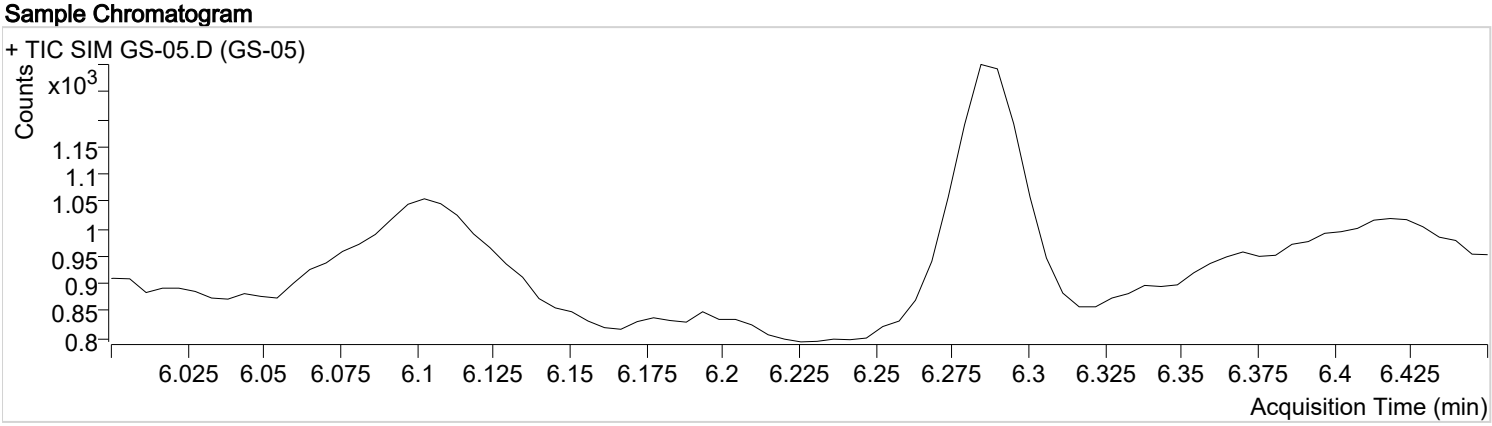

Epichlorohydrin

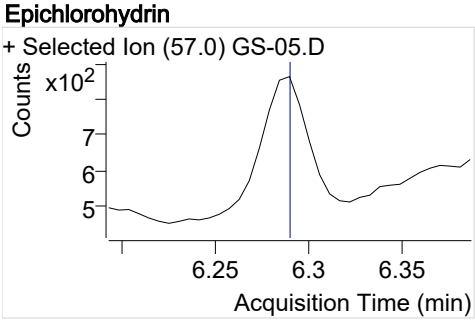



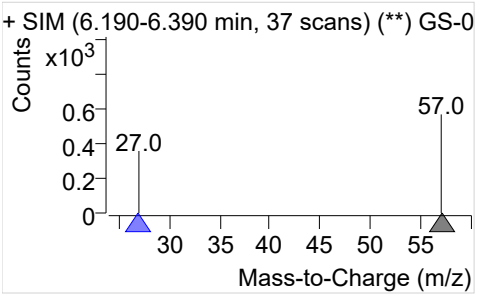

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-02-20 오후 1:14:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:48:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-20 오후 1:14:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-20 오전 11:00:37	**Data File**	GS-06.D
Type	Sample	**Name**	GS-06
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

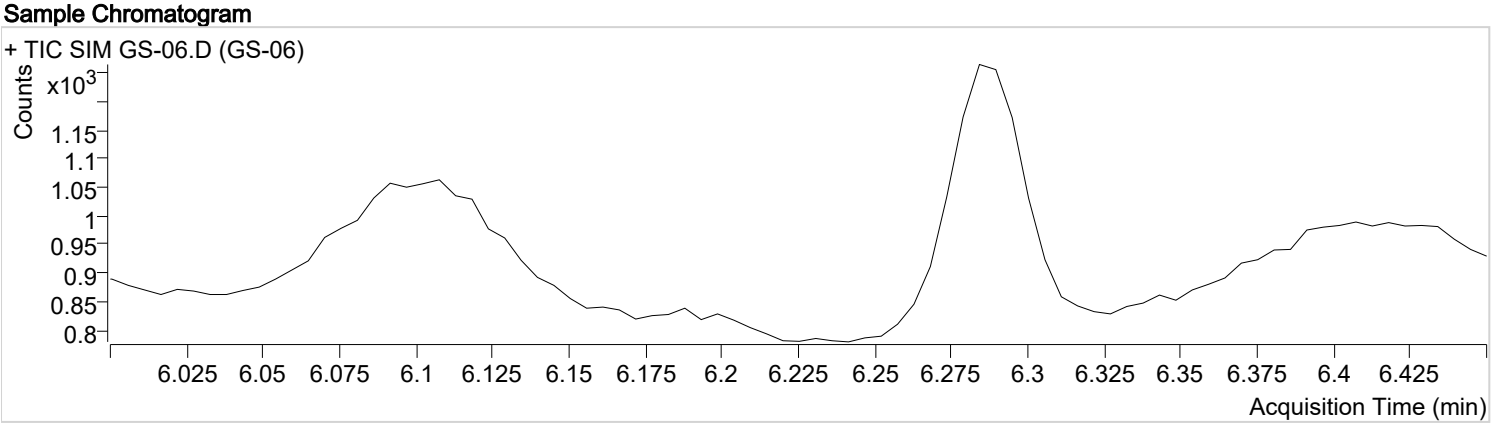

Epichlorohydrin

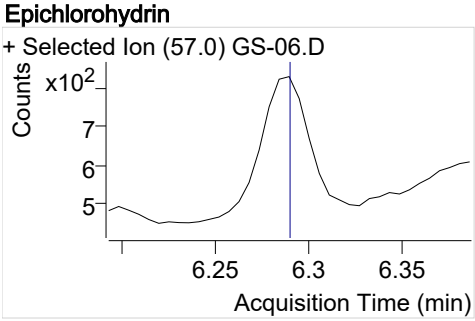



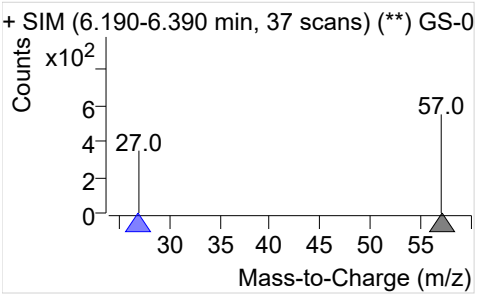

Quant Sample Report

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-02-20 오후 1:14:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:48:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-20 오후 1:14:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-20 오전 11:10:50	**Data File**	GS-15.D
Type	Sample	**Name**	GS-15
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

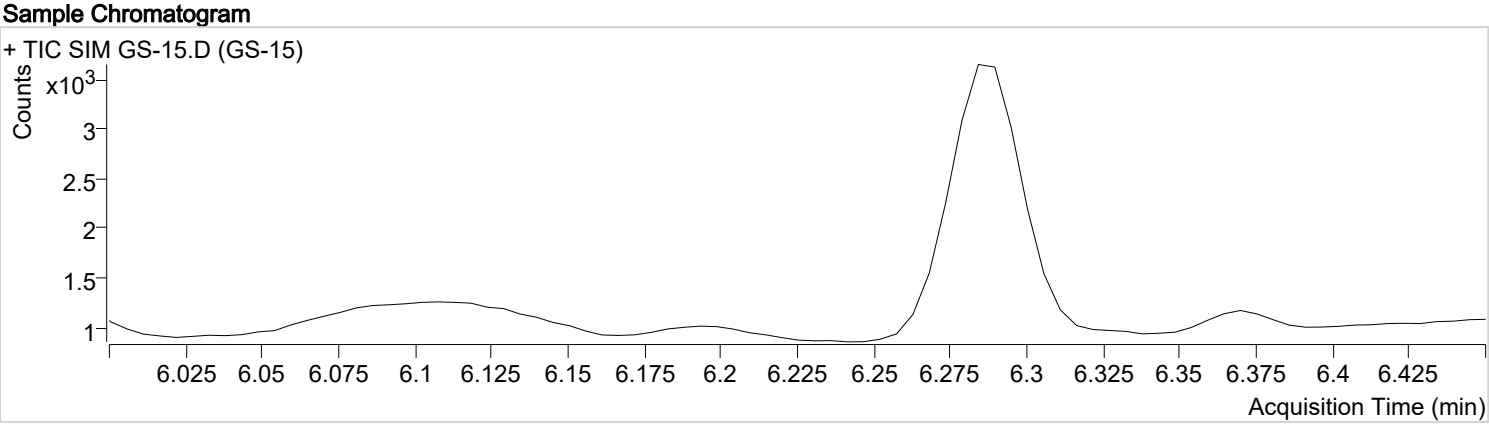

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	0	ND	mg/L

Epichlorohydrin

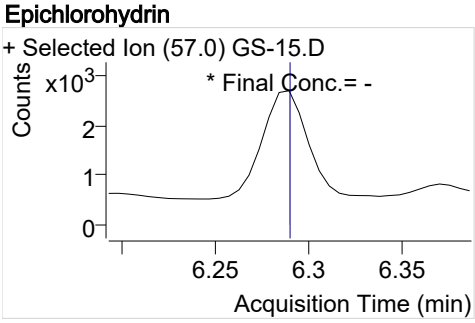

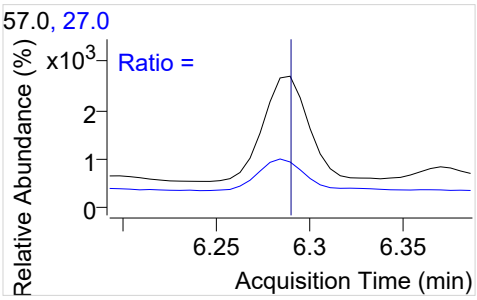

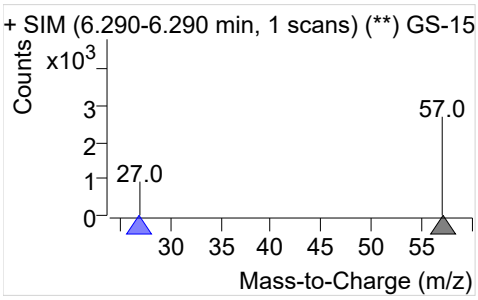

Quant Sample Report

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-02-20 오후 1:14:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:48:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-20 오후 1:14:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-20 오전 11:21:02	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

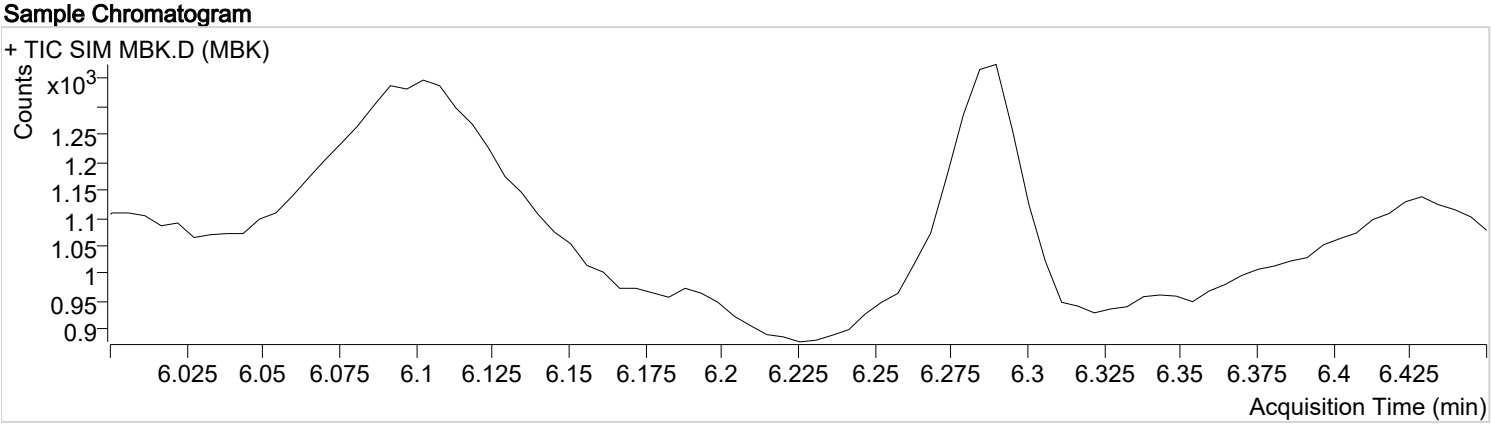

Epichlorohydrin

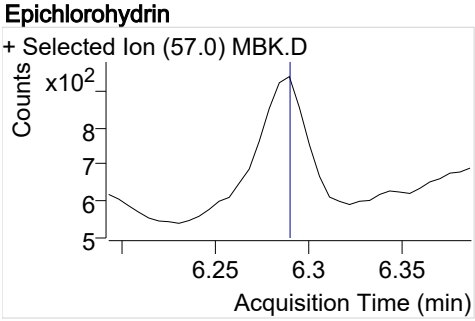



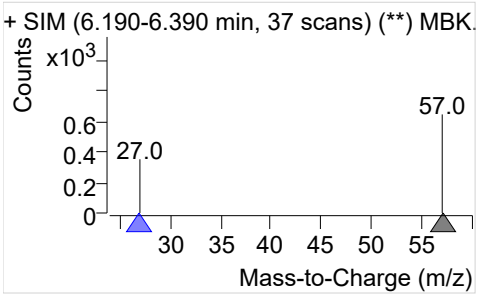

Quant Sample Report

Batch Data Path	D:\DATA\2026년\2. 2026년 2월\EPIC(GS 2.10, KH 2.10)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-02-20 오후 1:14:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:48:35	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-20 오후 1:14:07	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-02-20 오전 11:31:14	**Data File**	CCV.D
Type	QC	**Name**	CCV
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

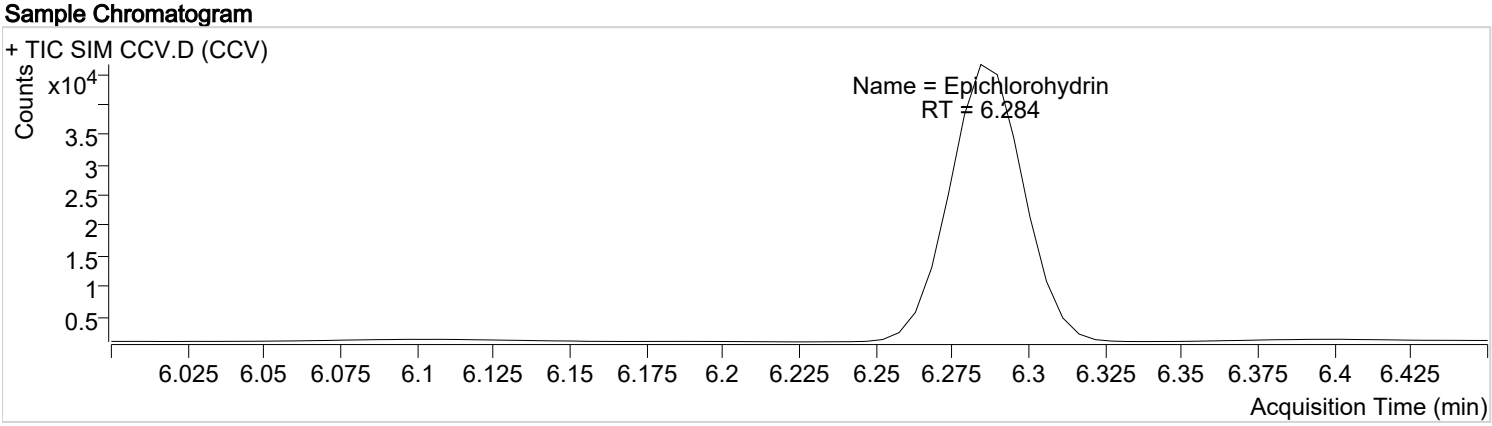

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.284	58311	2.680	mg/L
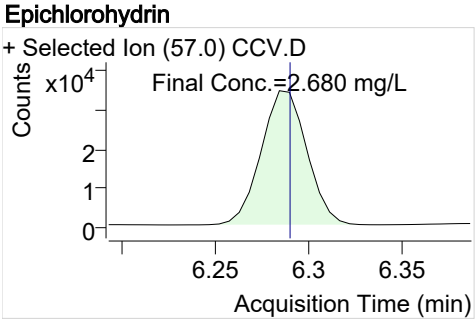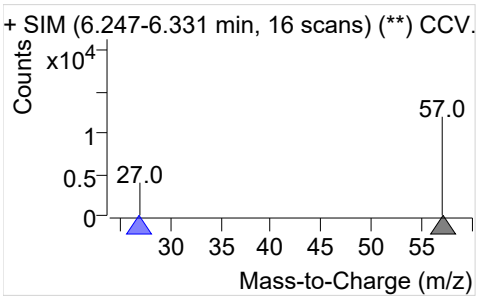
Epichlorohydrin