Quantitative Analysis Results Summary Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\QuantResults\EPIC.batch.bin				
Analysis Time	2026-03-03 오후 2:17:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-03 오후 2:17:15	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Epichlorohydrin

Data File	Type	RT	Resp.	Final Conc.
EPIC ST-01.D	Cal	6.290	3944	0.124
EPIC ST-02.D	Cal	6.289	8077	0.420
EPIC ST-03.D	Cal	6.290	16999	1.059
EPIC ST-04.D	Cal	6.289	41138	2.789
EPIC ST-05.D	Cal	6.290	70021	4.858
BK-.D	Blank			ND
FBK(DL 26-02-26).D	Blank			ND
FBK(LT 26-02-26).D	Blank			ND
FBK(PL 26-02-27).D	Blank			ND
DL-01.D	Sample			ND
LT-01.D	Sample	6.290	0	ND
LT-02.D	Sample	6.290	0	ND
LT-03.D	Sample	6.290	0	ND
PL-01.D	Sample	6.397	0	ND
PL-02.D	Sample			ND
MBK.D	Blank			ND
-CCV-.D	QC	6.290	29478	1.953

Epichlorohydrin

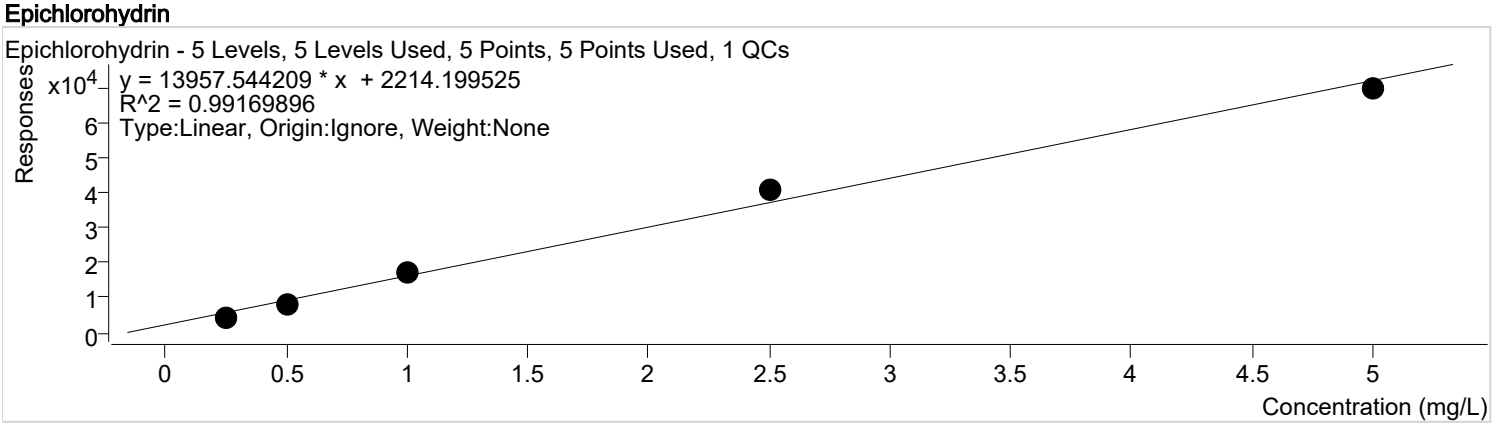

Cal. Path	Type	Level	Enable	Conc.	Response
D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\EPIC ST-01.D	Calibration	1	x	0.250	3944
D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\EPIC ST-02.D	Calibration	2	x	0.500	8077
D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\EPIC ST-03.D	Calibration	3	x	1.000	16999
D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\EPIC ST-04.D	Calibration	4	x	2.500	41138
D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\-CCV-.D	QC	4		2.500	29478
D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\EPIC ST-05.D	Calibration	5	x	5.000	70021

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-03 오후 2:17:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-03 오후 2:17:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-03 오전 9:16:50	**Data File**	EPIC ST-01.D
Type	Cal	**Name**	EPIC ST-01
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

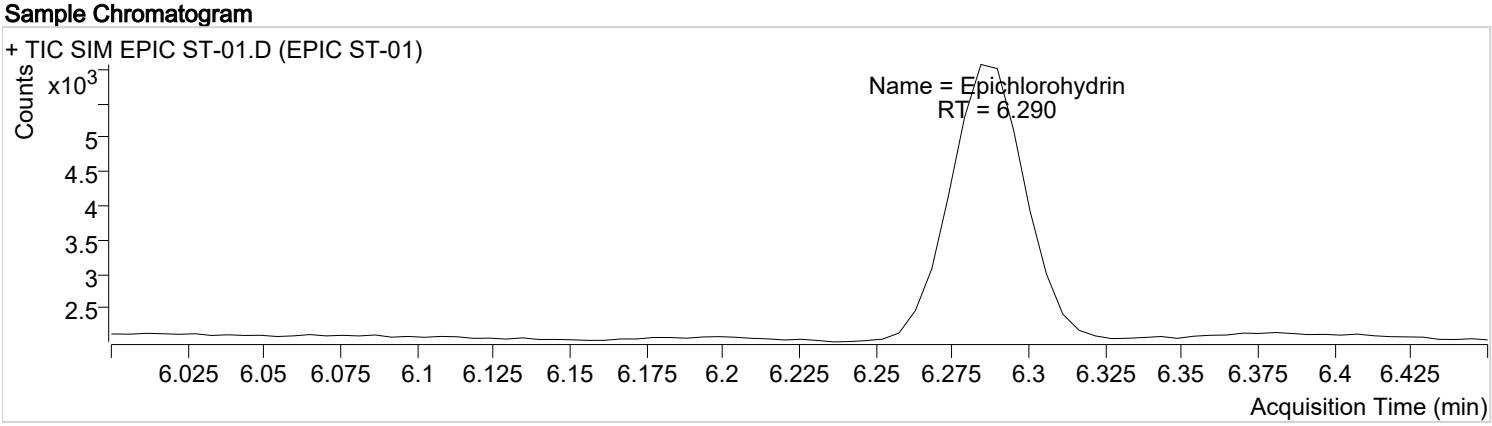

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	3944	0.124	mg/L

Epichlorohydrin

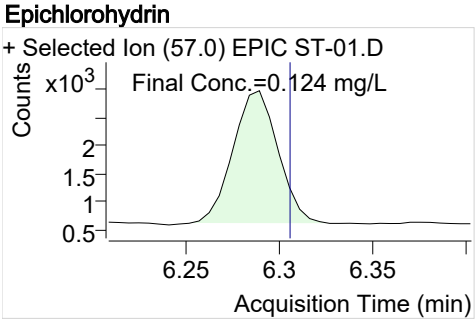

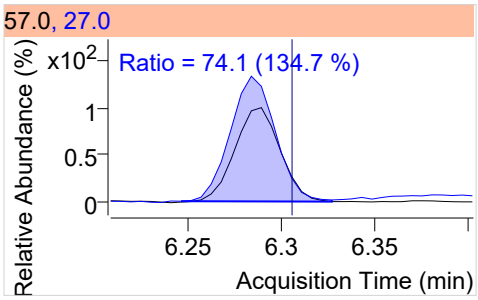

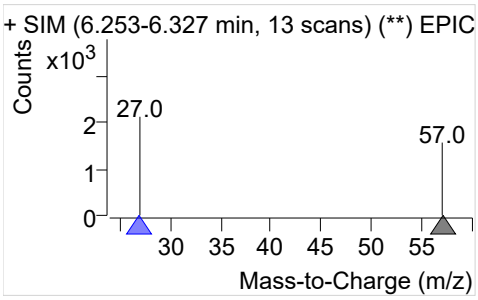

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-03 오후 2:17:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-03 오후 2:17:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-03 오전 9:27:03	**Data File**	EPIC ST-02.D
Type	Cal	**Name**	EPIC ST-02
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

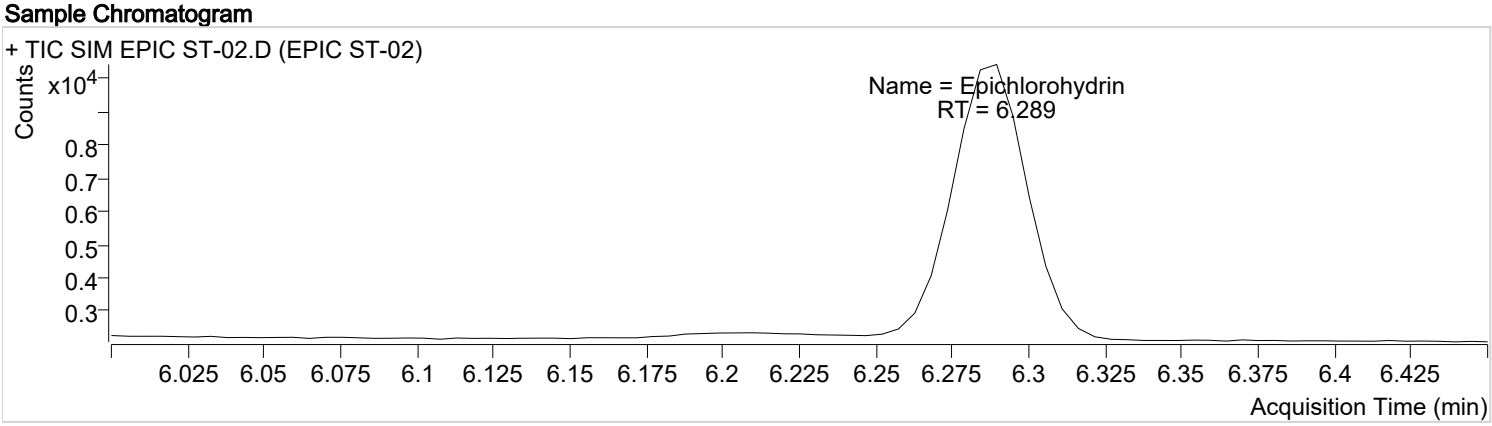

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.289	8077	0.420	mg/L

Epichlorohydrin

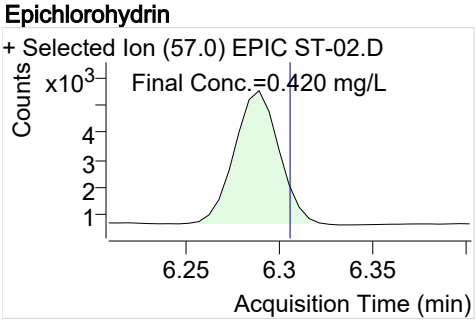

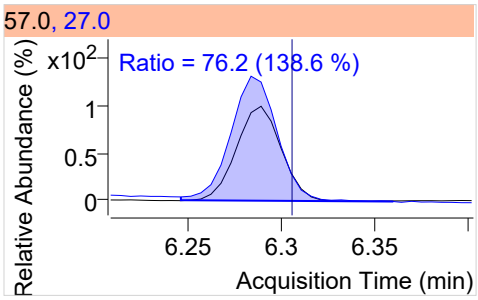



Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-03 오후 2:17:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-03 오후 2:17:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-03 오전 9:37:13	**Data File**	EPIC ST-03.D
Type	Cal	**Name**	EPIC ST-03
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

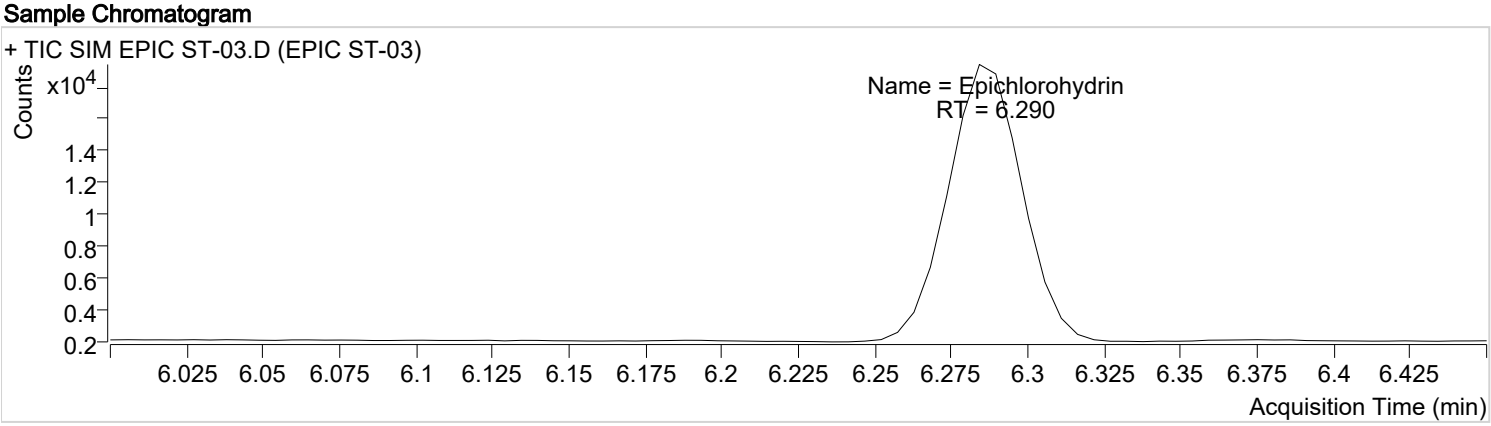

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	16999	1.059	mg/L

Epichlorohydrin

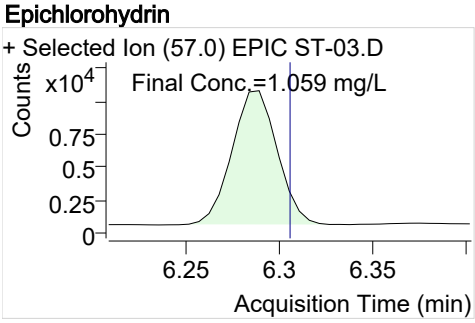





Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-03 오후 2:17:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-03 오후 2:17:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-03 오전 9:47:26	**Data File**	EPIC ST-04.D
Type	Cal	**Name**	EPIC ST-04
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

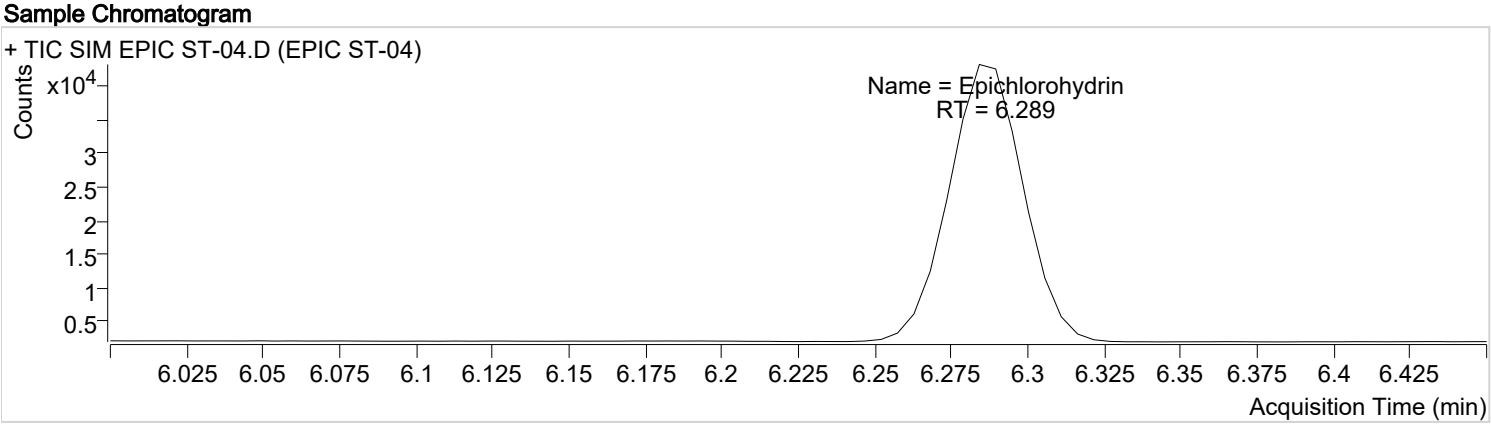

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.289	41138	2.789	mg/L

Epichlorohydrin

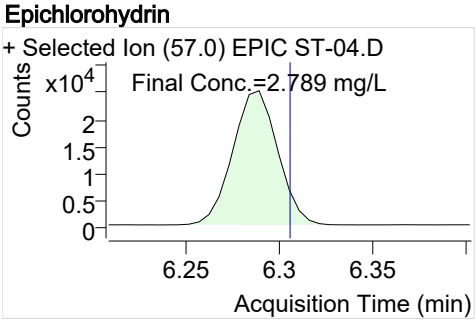





Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-03 오후 2:17:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-03 오후 2:17:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-03 오전 9:57:36	**Data File**	EPIC ST-05.D
Type	Cal	**Name**	EPIC ST-05
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

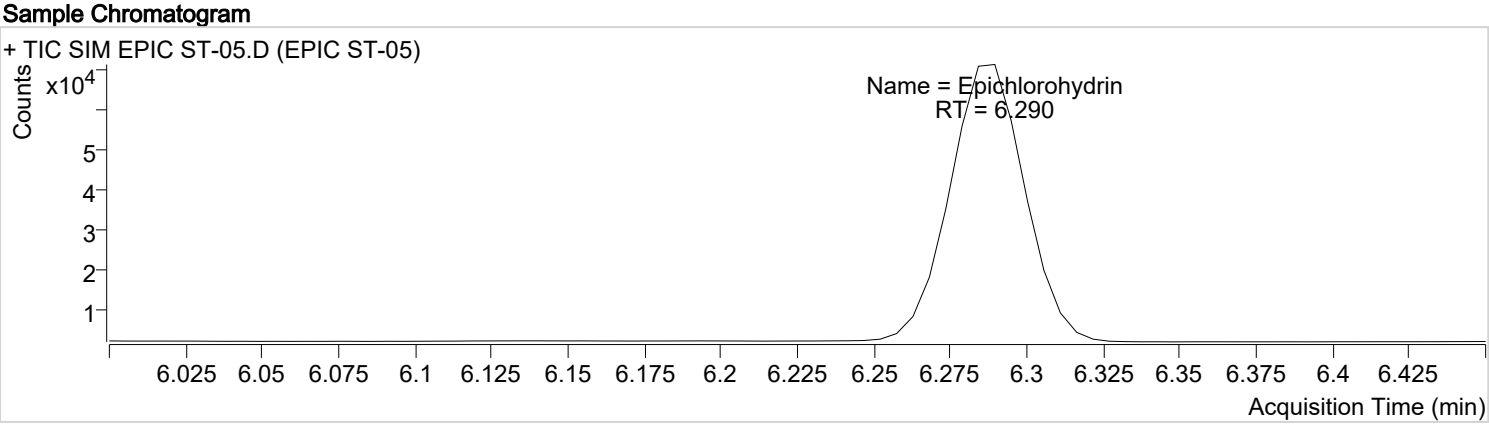

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	70021	4.858	mg/L

Epichlorohydrin

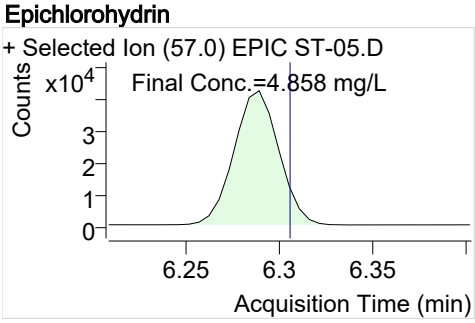





Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-03 오후 2:17:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-03 오후 2:17:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-03 오전 10:18:01	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

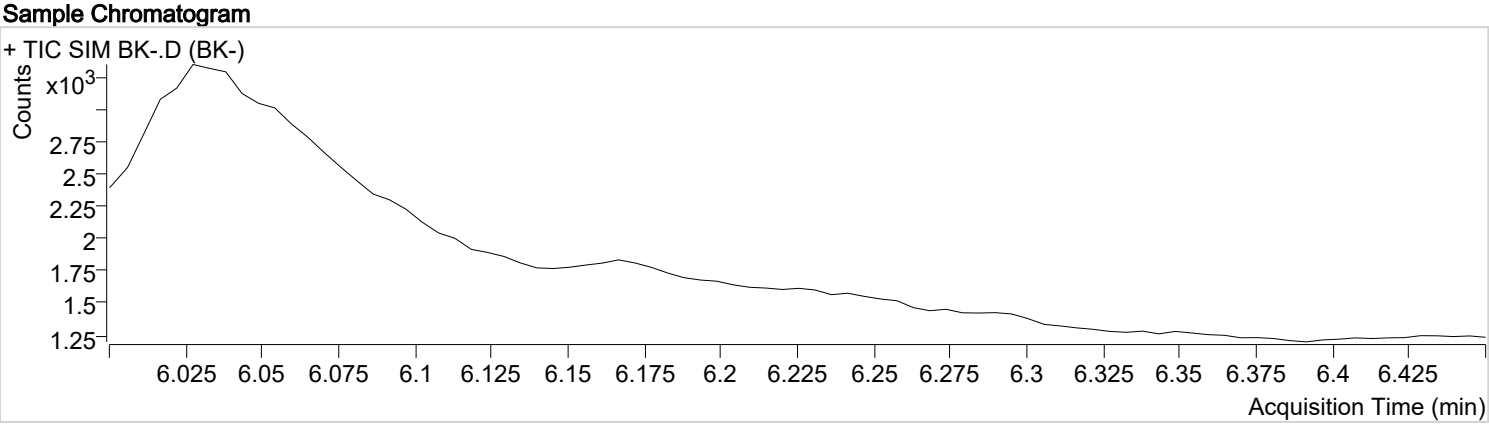

Epichlorohydrin

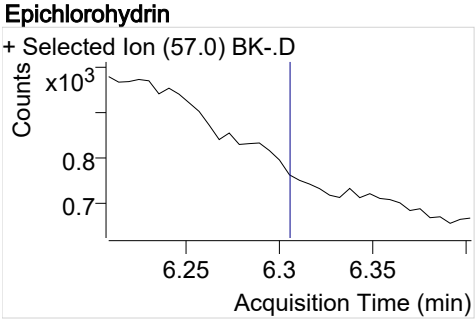



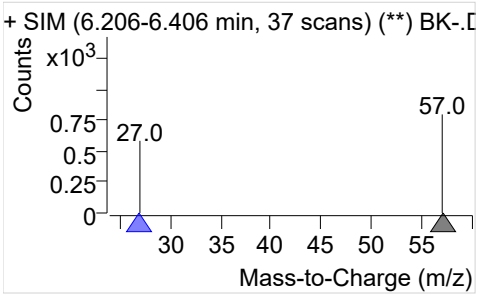

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-03 오후 2:17:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-03 오후 2:17:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-03 오전 10:28:12	**Data File**	FBK(DL 26-02-26).D
Type	Blank	**Name**	FBK(DL 26-02-26)
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

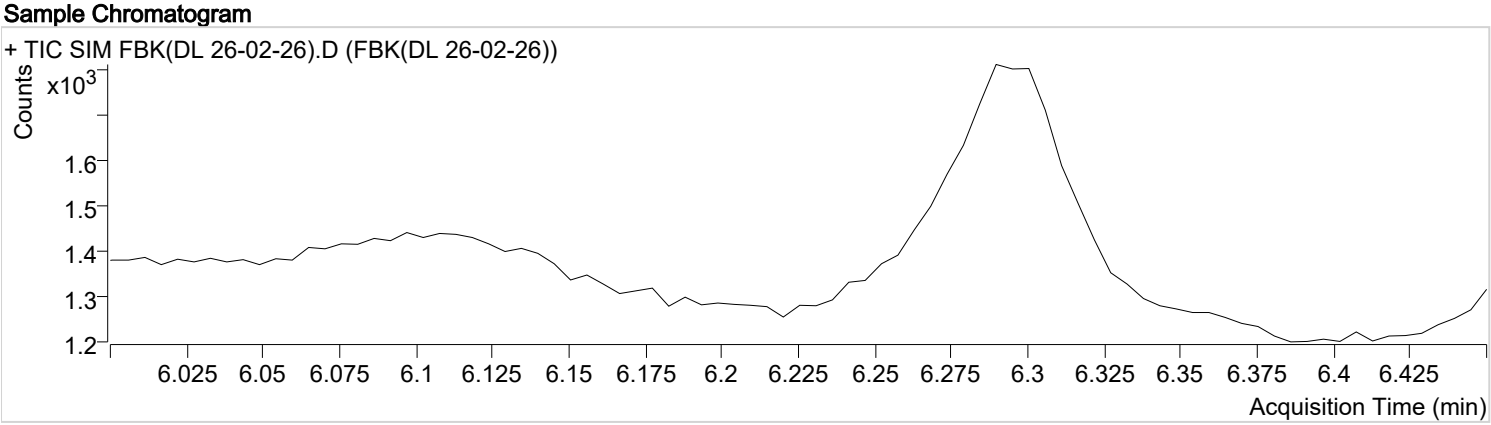

Epichlorohydrin

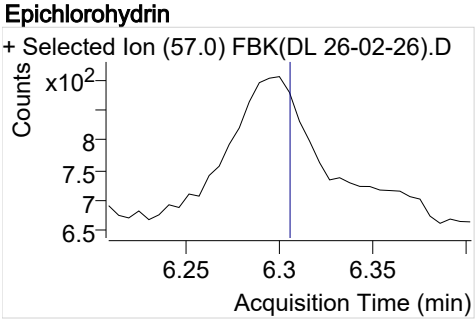



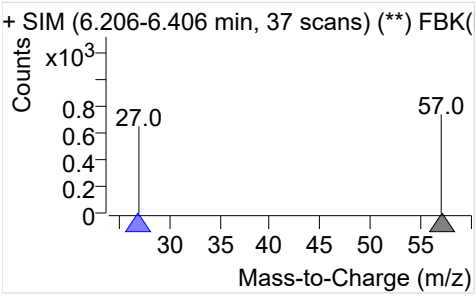

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-03 오후 2:17:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-03 오후 2:17:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-03 오전 10:38:24	**Data File**	FBK(LT 26-02-26).D
Type	Blank	**Name**	FBK(LT 26-02-26)
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

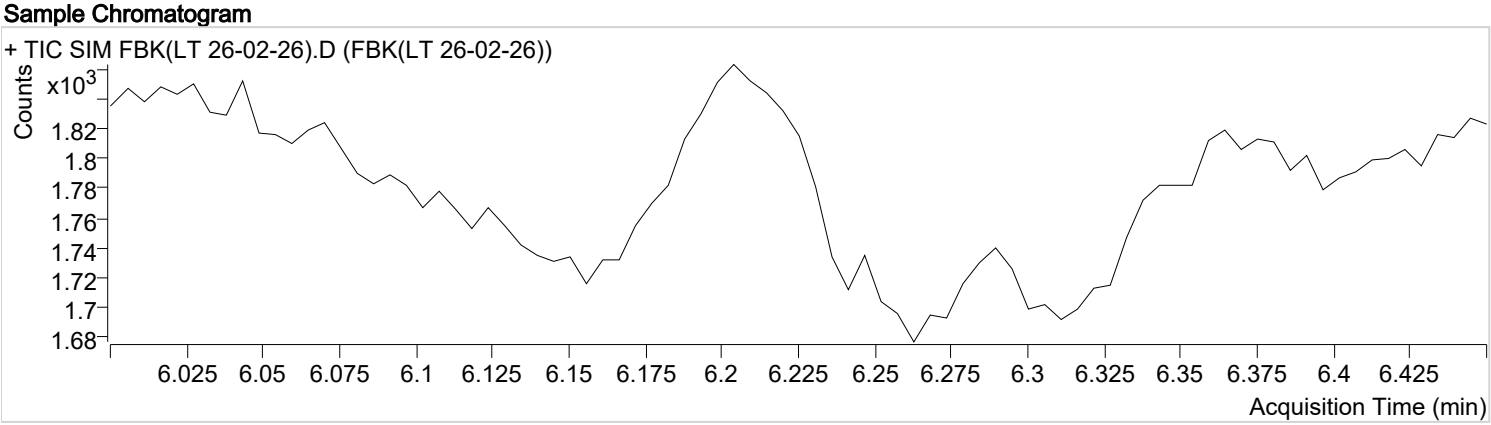

Epichlorohydrin

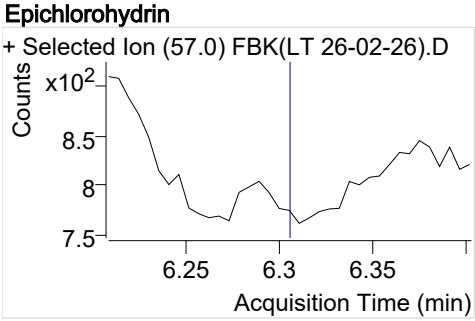



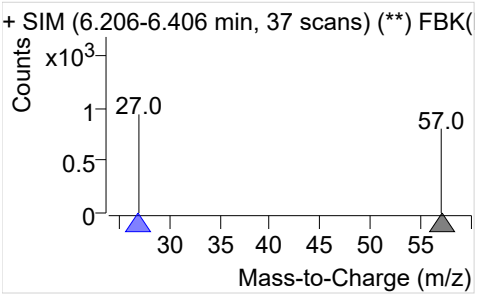

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-03 오후 2:17:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-03 오후 2:17:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-03 오전 10:48:34	**Data File**	FBK(PL 26-02-27).D
Type	Blank	**Name**	FBK(PL 26-02-27)
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

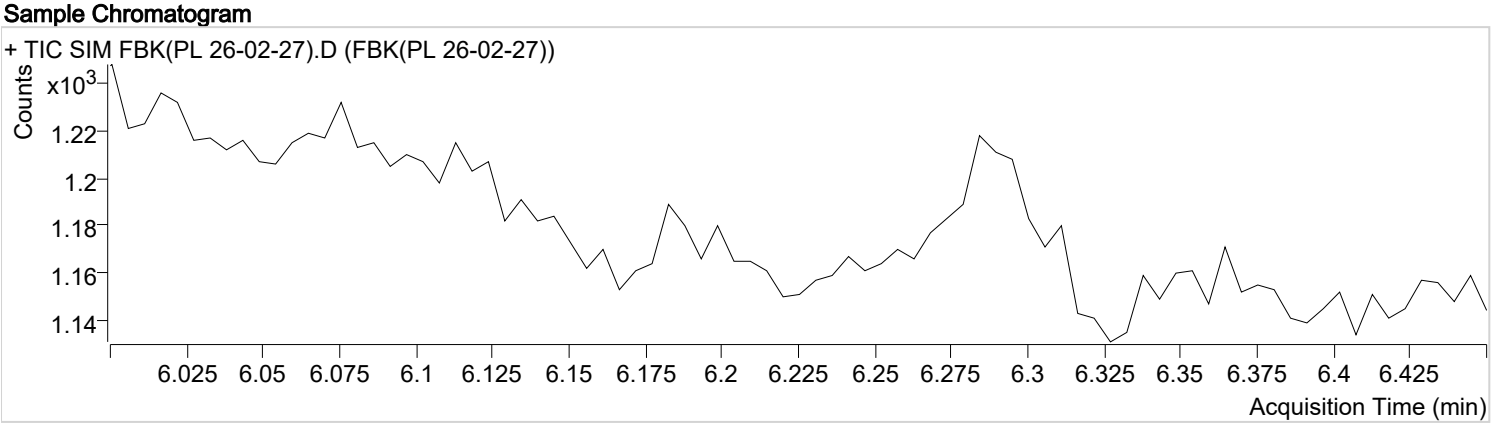

Epichlorohydrin

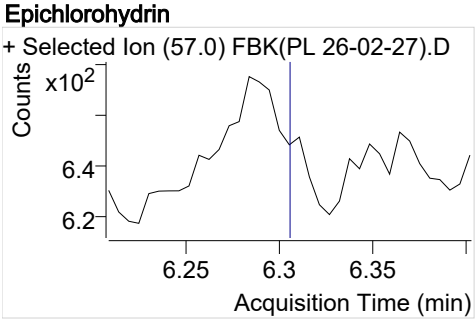



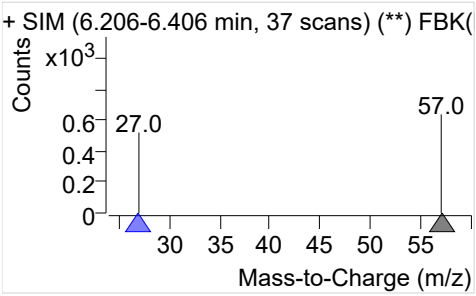

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-03 오후 2:17:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-03 오후 2:17:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-03 오전 10:58:48	**Data File**	DL-01.D
Type	Sample	**Name**	DL-01
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

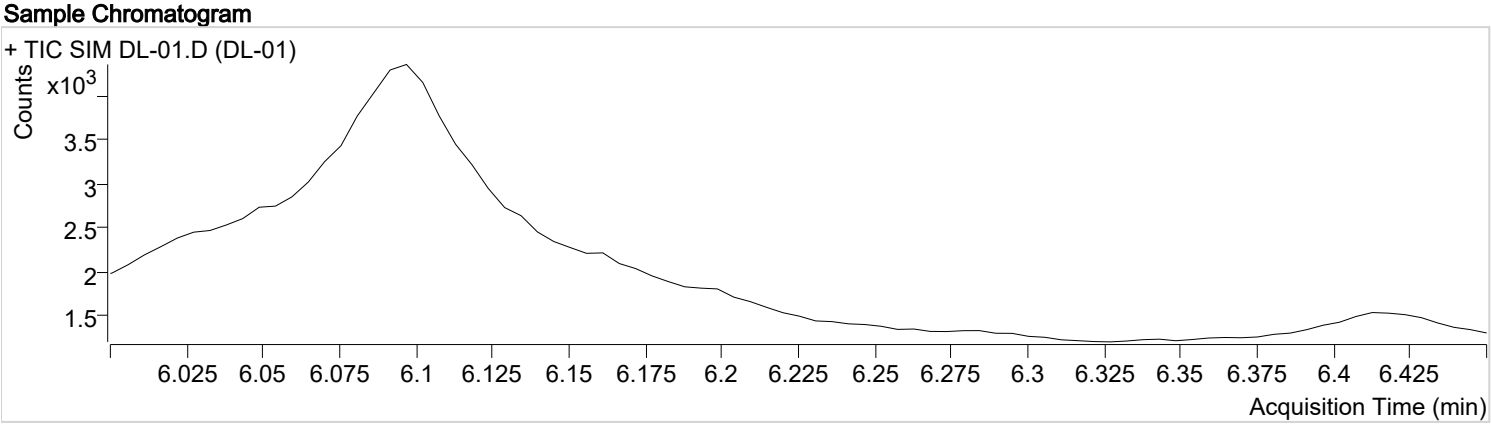

Epichlorohydrin

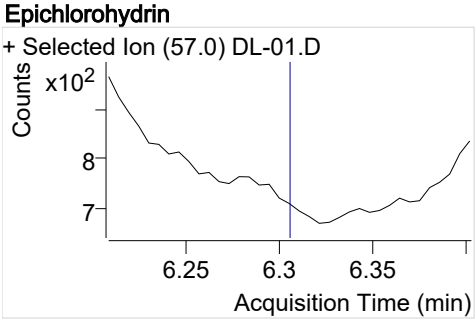



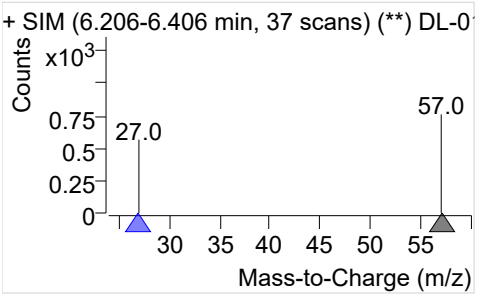

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-03 오후 2:17:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-03 오후 2:17:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-03 오전 11:09:01	**Data File**	LT-01.D
Type	Sample	**Name**	LT-01
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

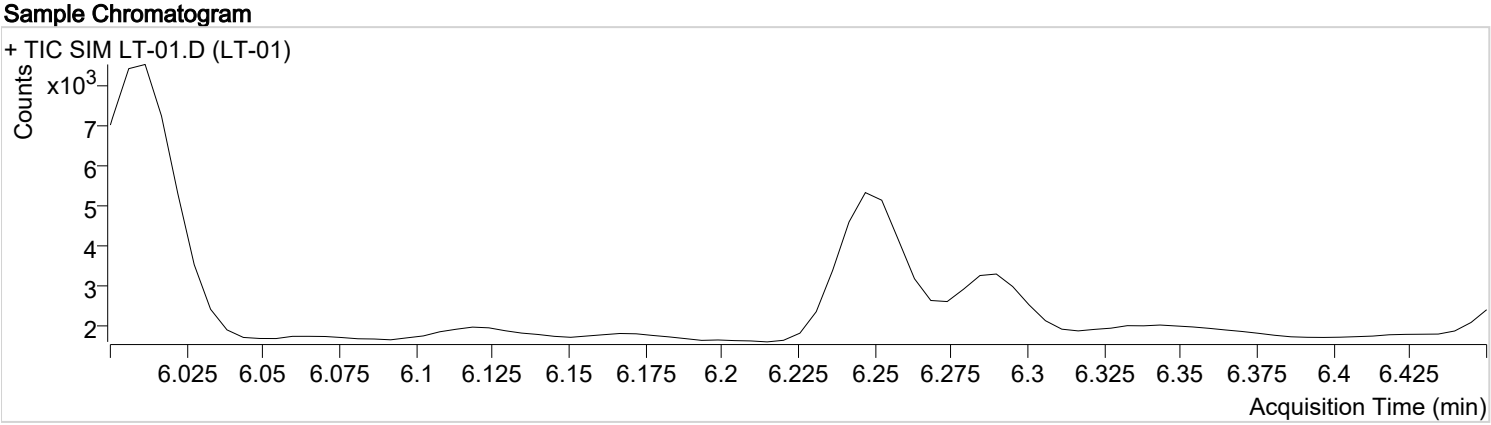

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	0	ND	mg/L

Epichlorohydrin

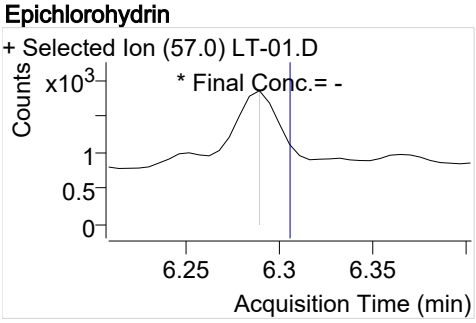





Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-03 오후 2:17:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-03 오후 2:17:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-03 오전 11:19:10	**Data File**	LT-02.D
Type	Sample	**Name**	LT-02
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

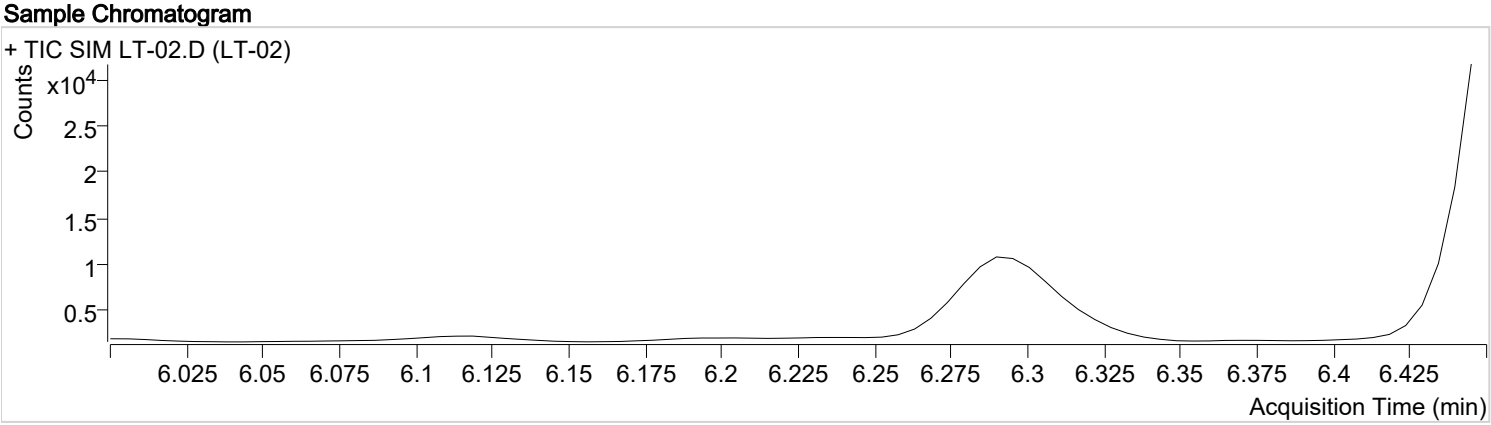

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	0	ND	mg/L

Epichlorohydrin

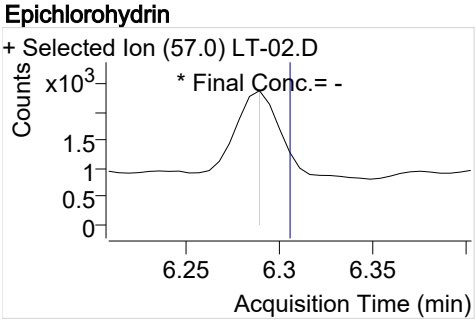





Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-03 오후 2:17:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-03 오후 2:17:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-03 오전 11:29:21	**Data File**	LT-03.D
Type	Sample	**Name**	LT-03
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

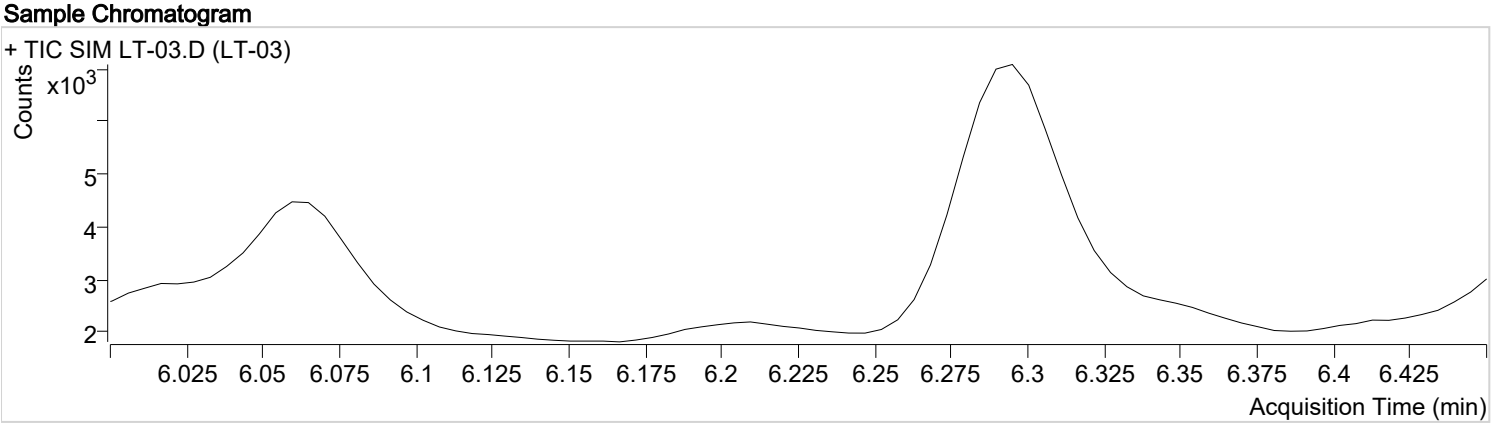

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	0	ND	mg/L

Epichlorohydrin

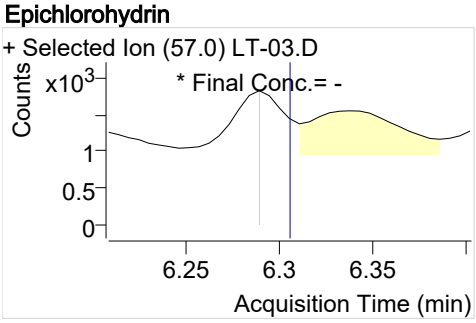





Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-03 오후 2:17:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-03 오후 2:17:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-03 오전 11:39:35	**Data File**	PL-01.D
Type	Sample	**Name**	PL-01
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

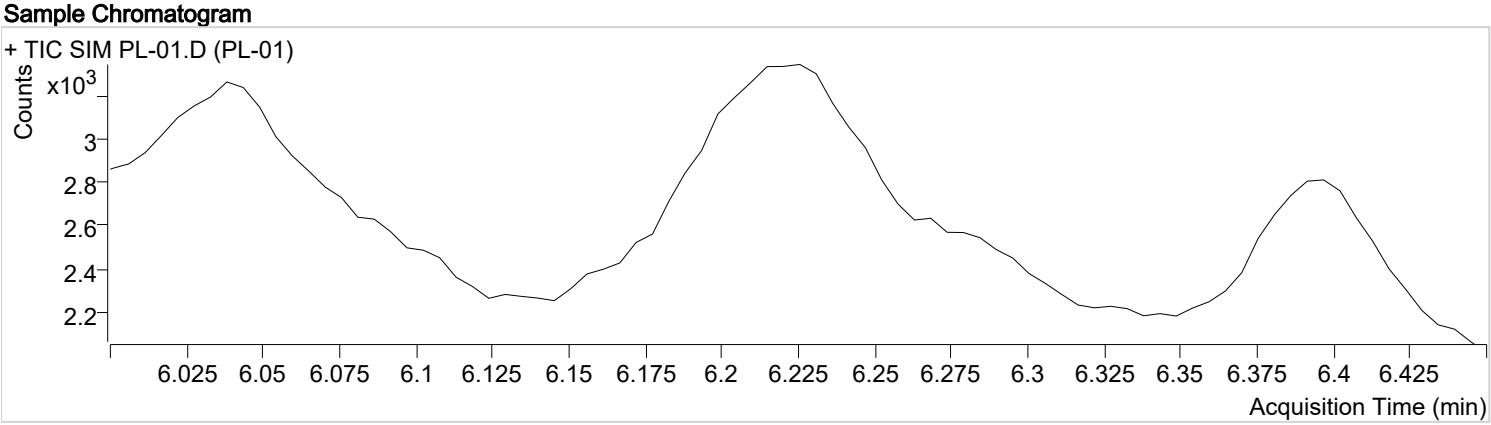

Epichlorohydrin

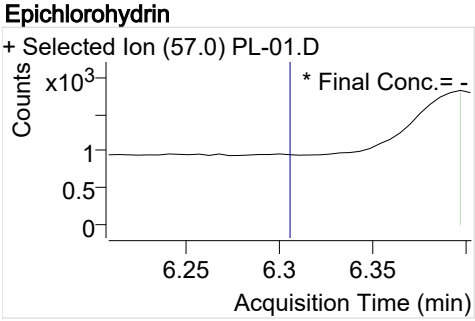



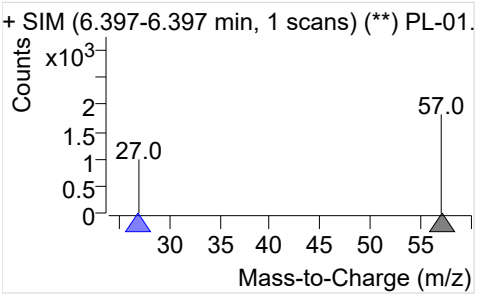

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-03 오후 2:17:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-03 오후 2:17:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-03 오전 11:49:45	**Data File**	PL-02.D
Type	Sample	**Name**	PL-02
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

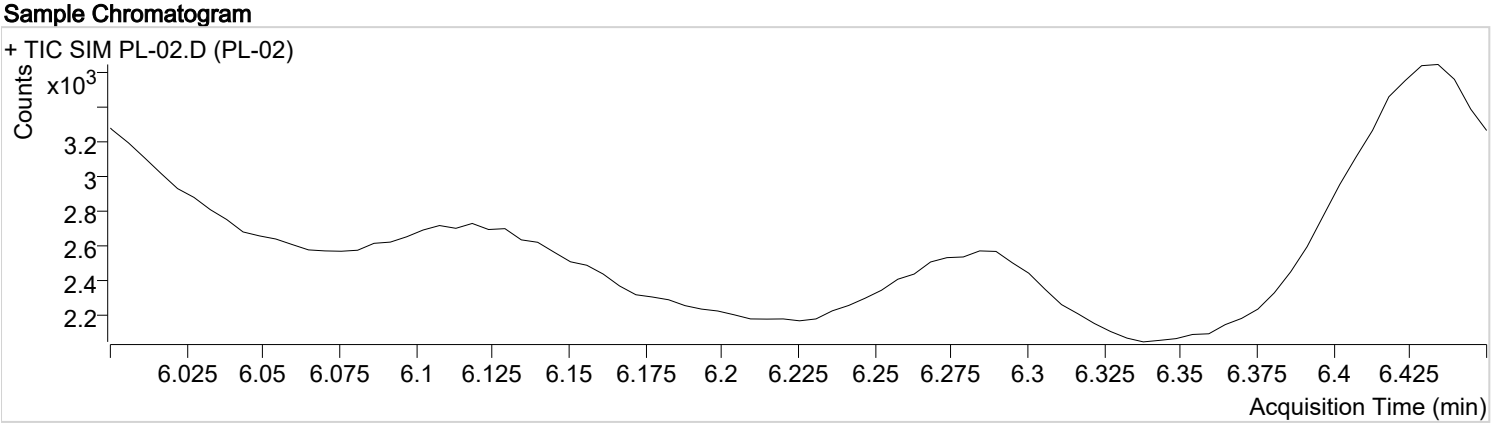

Epichlorohydrin

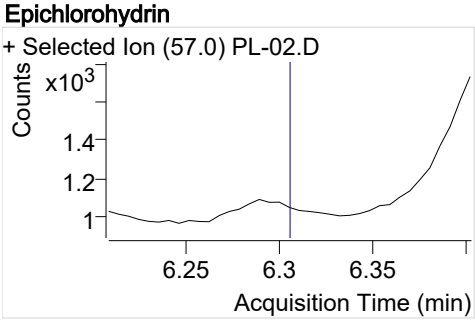



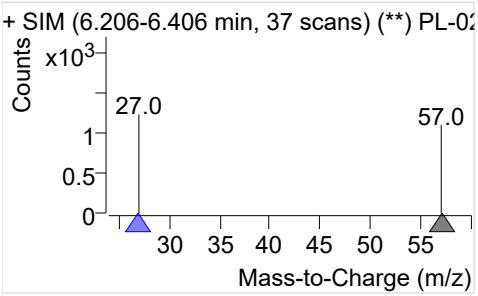

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-03 오후 2:17:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-03 오후 2:17:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-03 오전 11:59:55	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

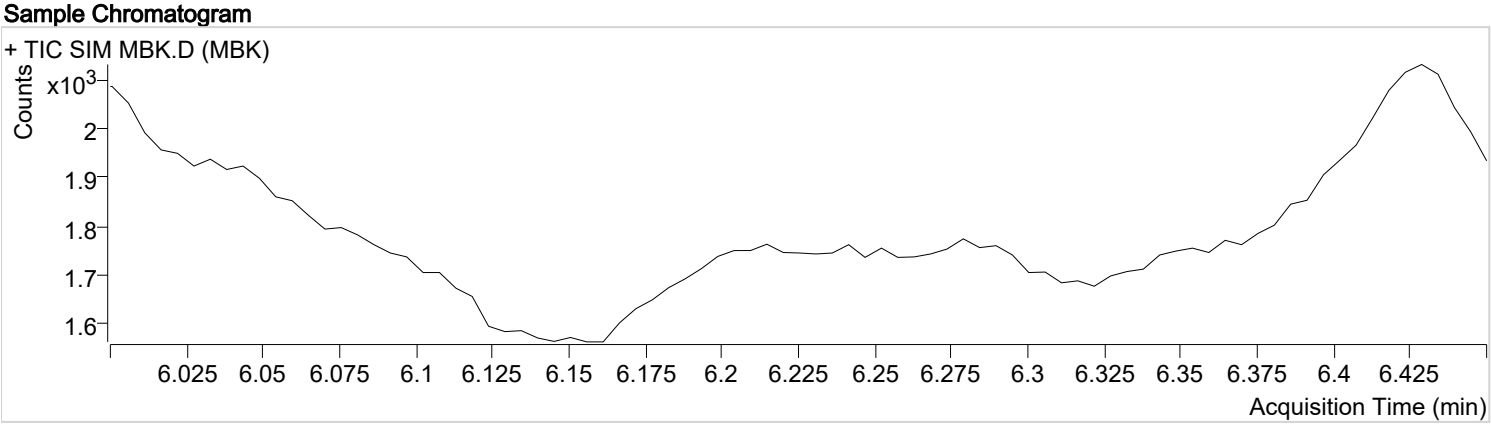

Epichlorohydrin

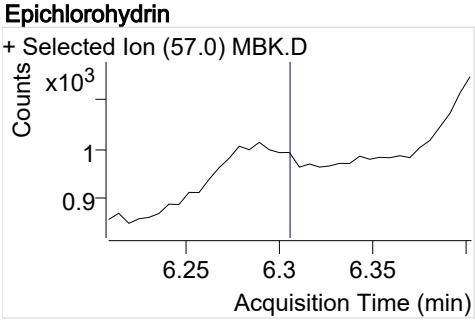



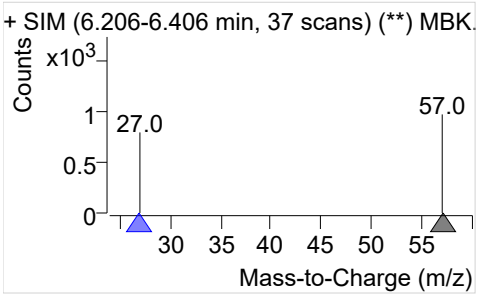

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(DL 2.26, LT 2.26, PL 2.27)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-03 오후 2:17:15	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:40	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-03 오후 2:17:15	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-03 오후 12:20:21	**Data File**	-CCV-.D
Type	QC	**Name**	-CCV-
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

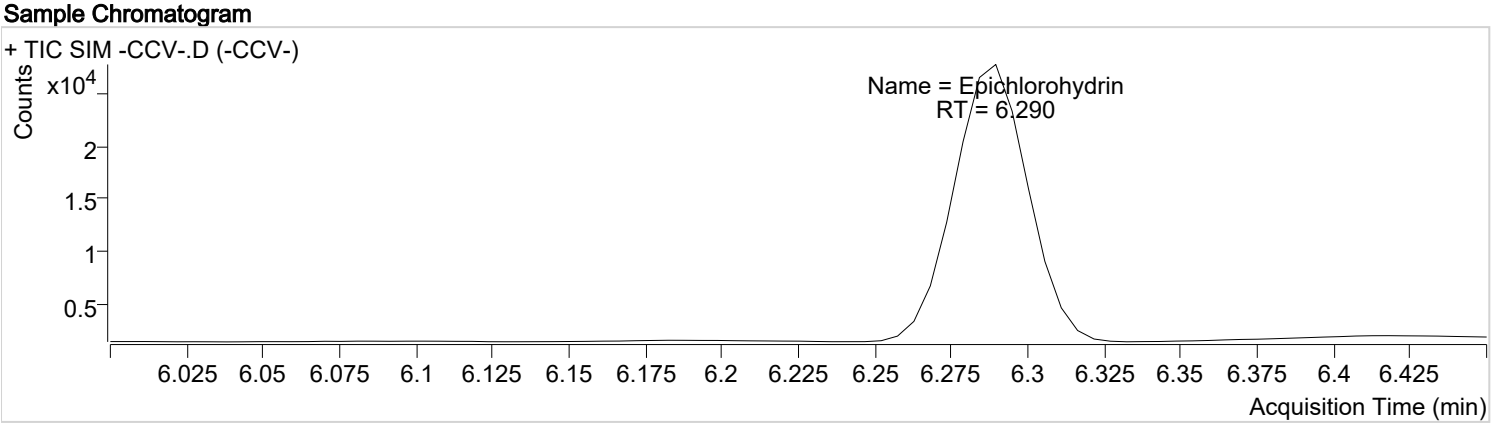

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	29478	1.953	mg/L
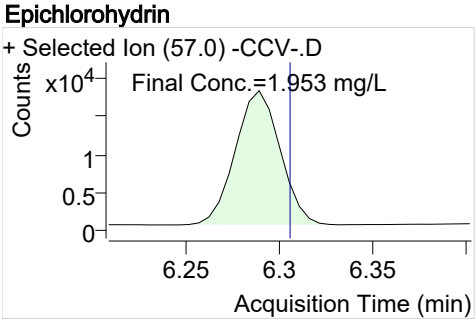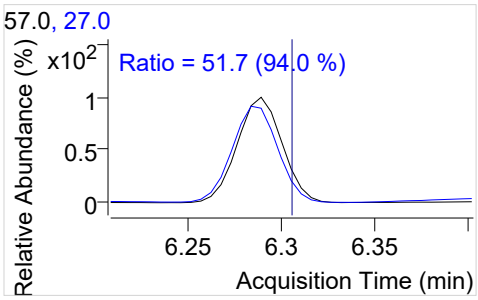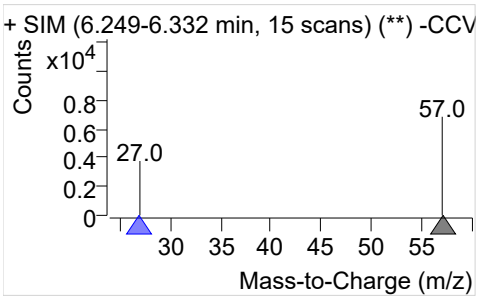
Epichlorohydrin