Quantitative Analysis Results Summary Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin				
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Epichlorohydrin

Data File	Type	RT	Resp.	Final Conc.
EPIC ST-01.D	Cal	6.290	1166	0.399
EPIC ST-02.D	Cal	6.290	1723	0.492
EPIC ST-03.D	Cal	6.290	4478	0.953
EPIC ST-04.D	Cal	6.290	12561	2.307
EPIC ST-05.D	Cal	6.290	29234	5.099
BK-.D	Blank			ND
FBK(RE 26-03-04).D	Blank			ND
FBK(KD 26-03-04).D	Blank			ND
RE-01.D	Sample			ND
RE-02.D	Sample			ND
RE-03.D	Sample			ND
RE-04.D	Sample	6.364	0	ND
RE-09.D	Sample	6.290	0	ND
RE-10.D	Sample			ND
RE-11.D	Sample			ND
RE-12.D	Sample			ND
KD-01.D	Sample	6.289	5388	0.002
KD-02.D	Sample	6.348	0	ND
KD-03.D	Sample	6.290	49773	0.017
MBK.D	Blank			ND
CCV.D	QC	6.289	12655	2.323
KD3-R.D	Sample	6.290	21371	0.015
MBK-2.D	Blank			ND
CCV-2.D	QC	6.289	12743	2.337

Epichlorohydrin

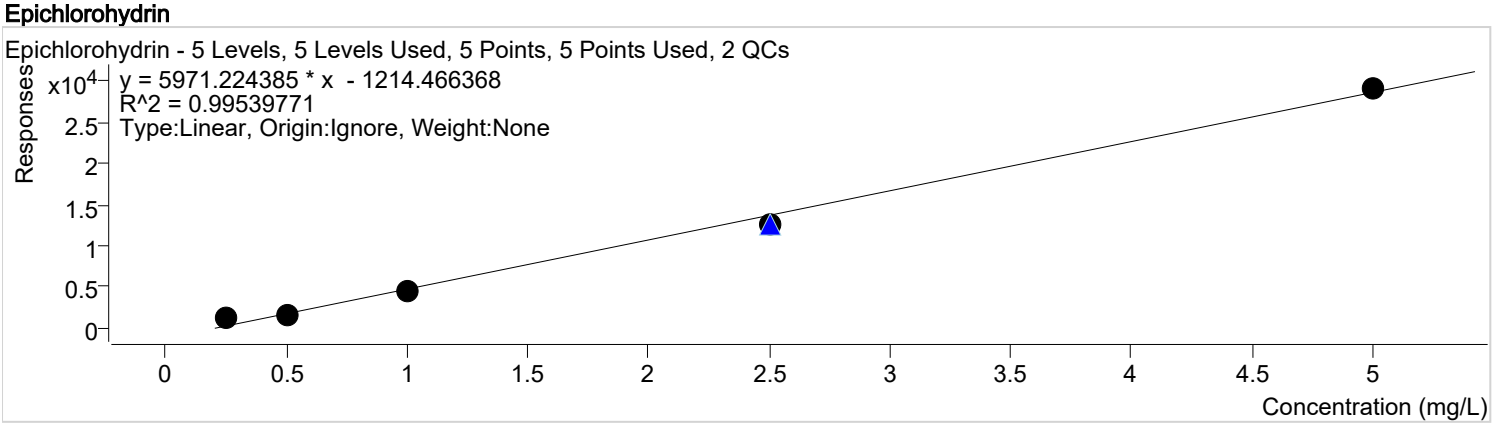

Cal. Path	Type	Level	Enable	Conc.	Response
D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\EPIC ST-01.D	Calibration	1	x	0.250	1166
D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\EPIC ST-02.D	Calibration	2	x	0.500	1723
D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\EPIC ST-03.D	Calibration	3	x	1.000	4478
D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\EPIC ST-04.D	Calibration	4	x	2.500	12561
D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\CCV.D	QC	4		2.500	12655
D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\CCV-2.D	QC	4	x	2.500	12743
D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\EPIC ST-05.D	Calibration	5	x	5.000	29234

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 5:30:26	**Data File**	EPIC ST-01.D
Type	Cal	**Name**	EPIC ST-01
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

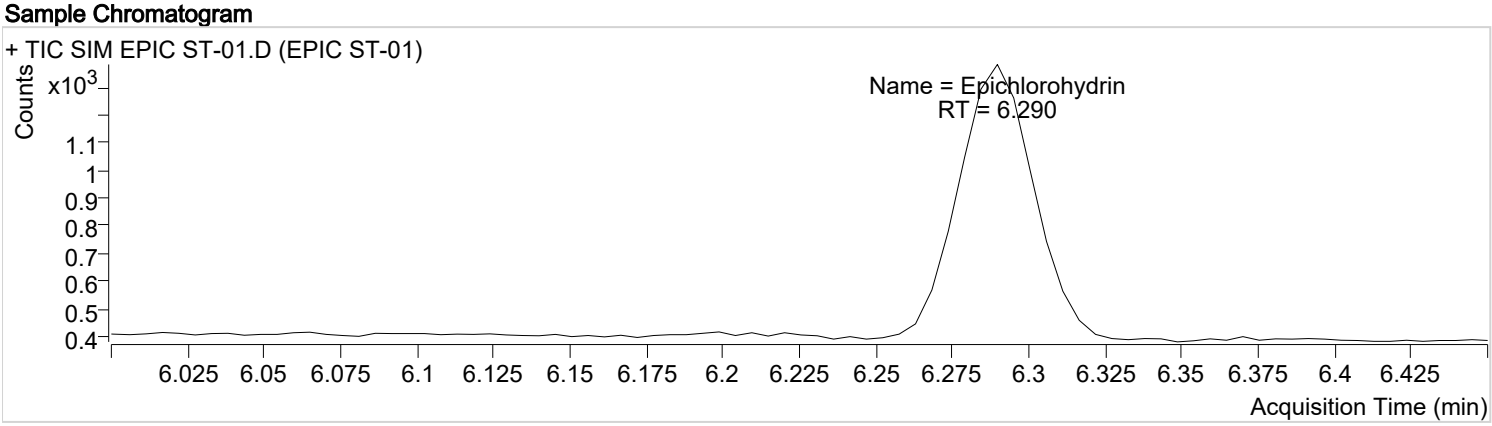

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	1166	0.399	mg/L

Epichlorohydrin

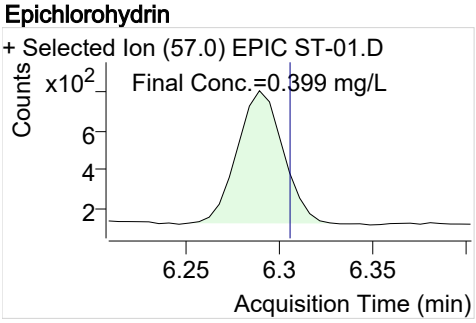





Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 5:40:39	**Data File**	EPIC ST-02.D
Type	Cal	**Name**	EPIC ST-02
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

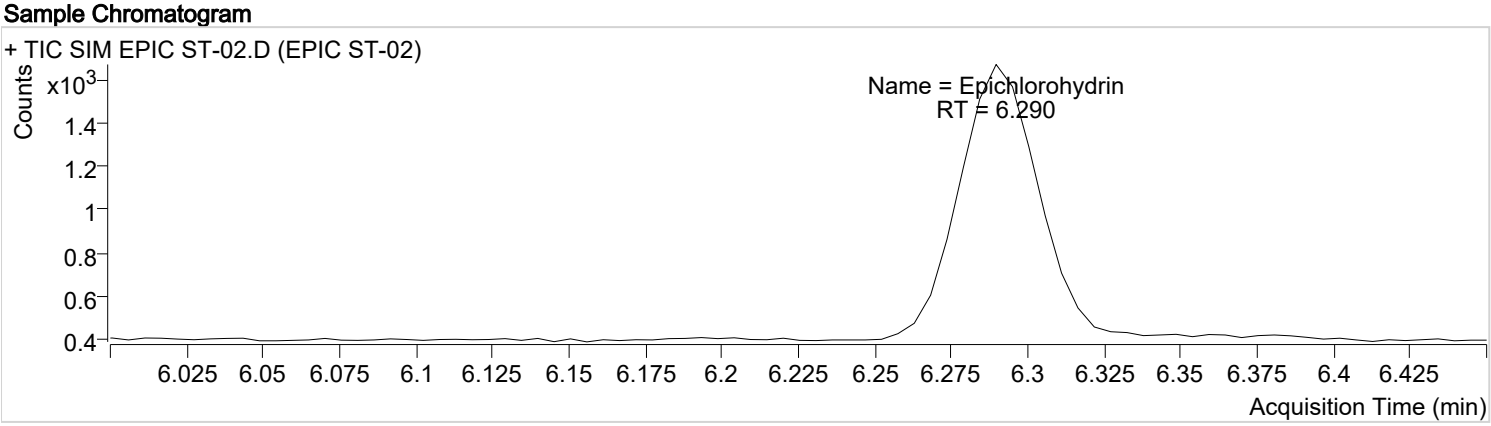

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	1723	0.492	mg/L

Epichlorohydrin

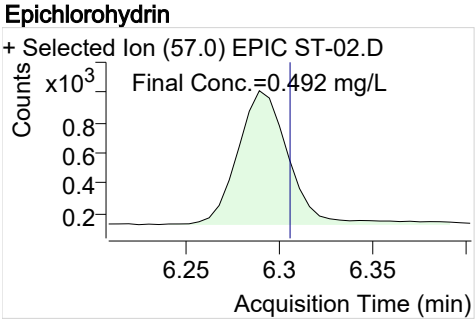





Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 5:50:53	**Data File**	EPIC ST-03.D
Type	Cal	**Name**	EPIC ST-03
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

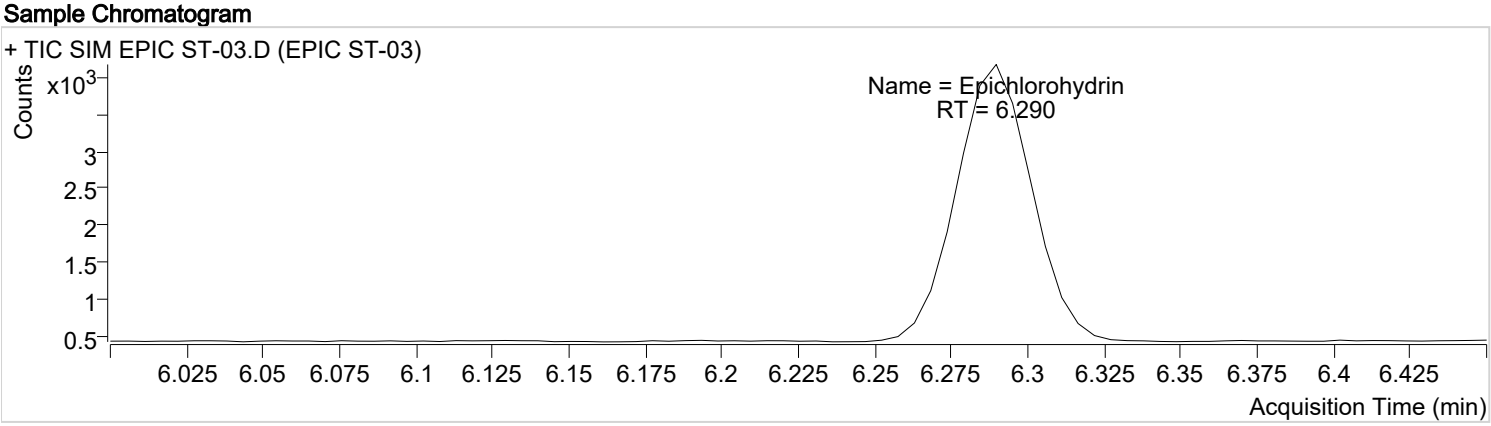

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	4478	0.953	mg/L

Epichlorohydrin

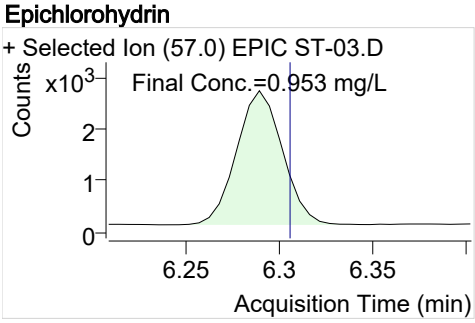





Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 6:01:03	**Data File**	EPIC ST-04.D
Type	Cal	**Name**	EPIC ST-04
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

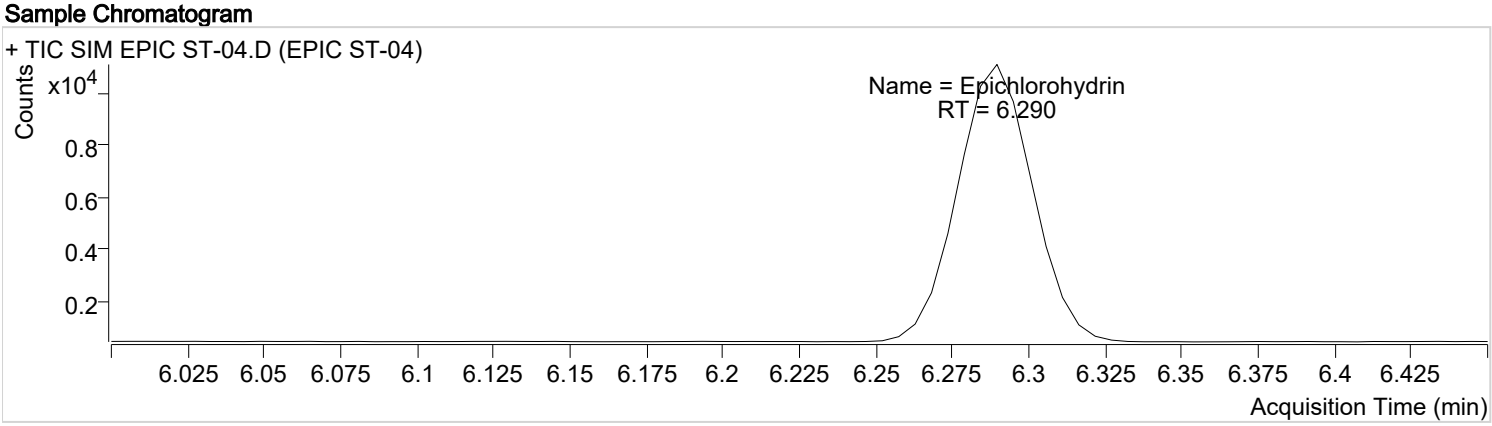

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	12561	2.307	mg/L

Epichlorohydrin

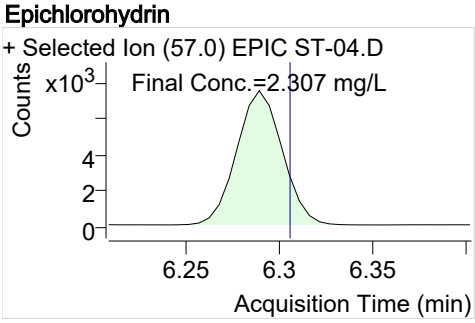





Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 6:11:17	**Data File**	EPIC ST-05.D
Type	Cal	**Name**	EPIC ST-05
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

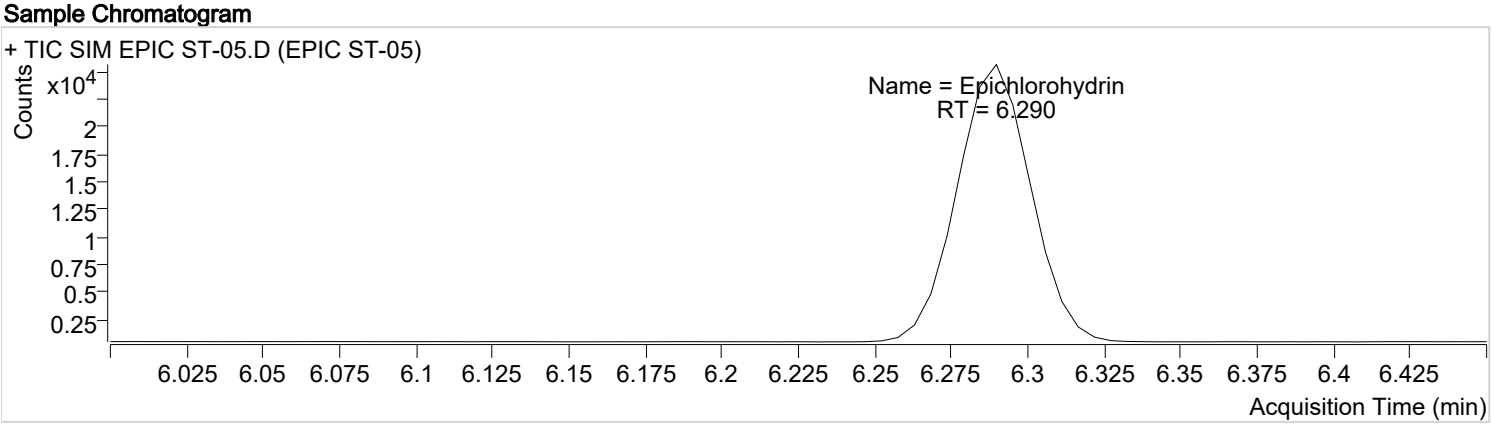

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	29234	5.099	mg/L

Epichlorohydrin

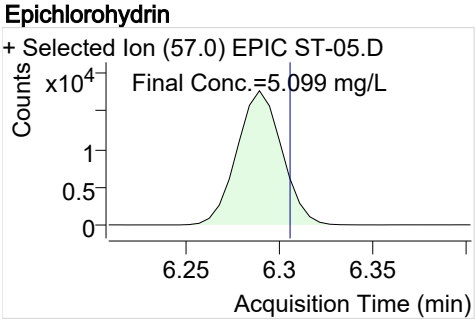





Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 6:31:47	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

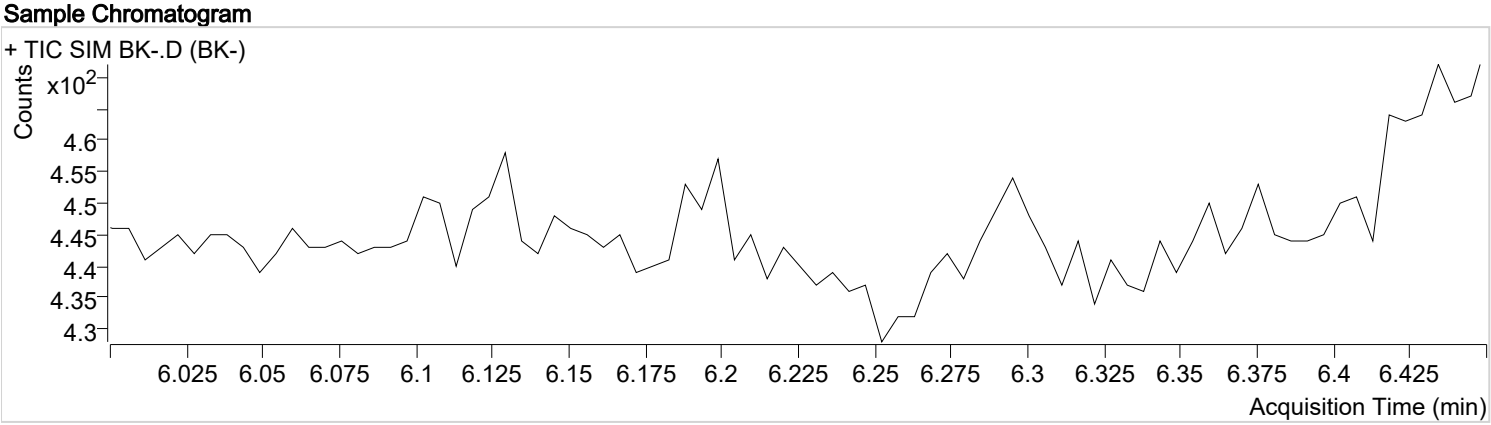

Epichlorohydrin





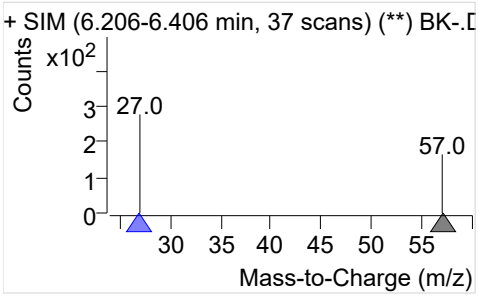

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 6:42:00	**Data File**	FBK(RE 26-03-04).D
Type	Blank	**Name**	FBK(RE 26-03-04)
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

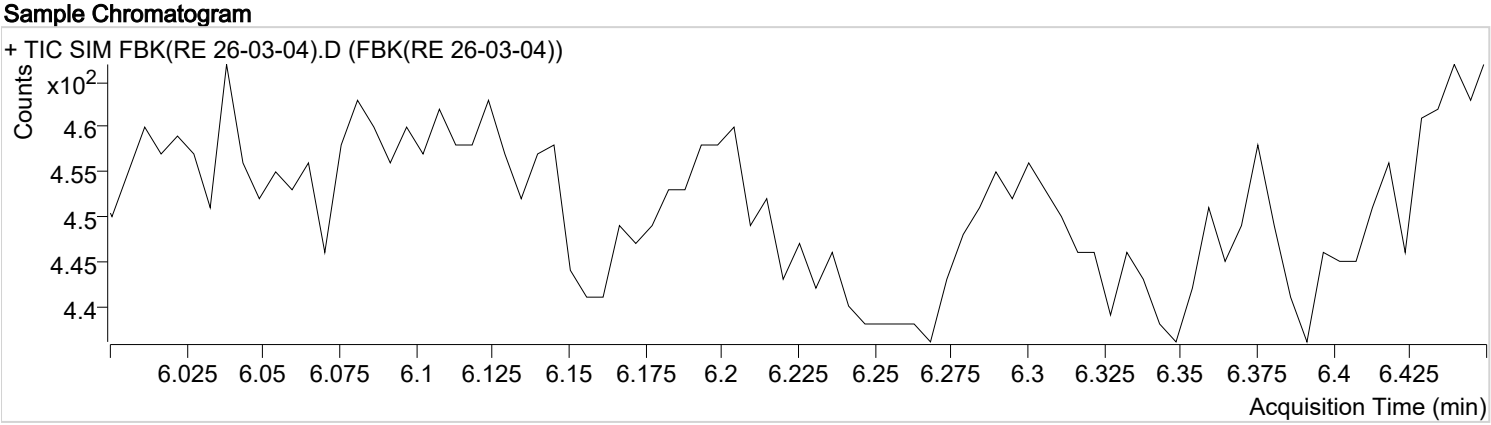

Epichlorohydrin





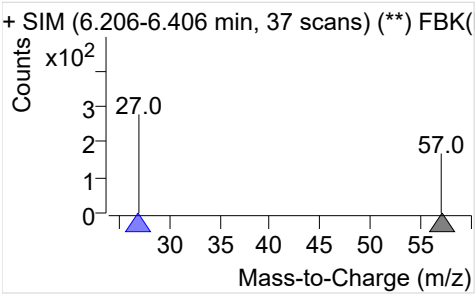

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 6:52:14	**Data File**	FBK(KD 26-03-04).D
Type	Blank	**Name**	FBK(KD 26-03-04)
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

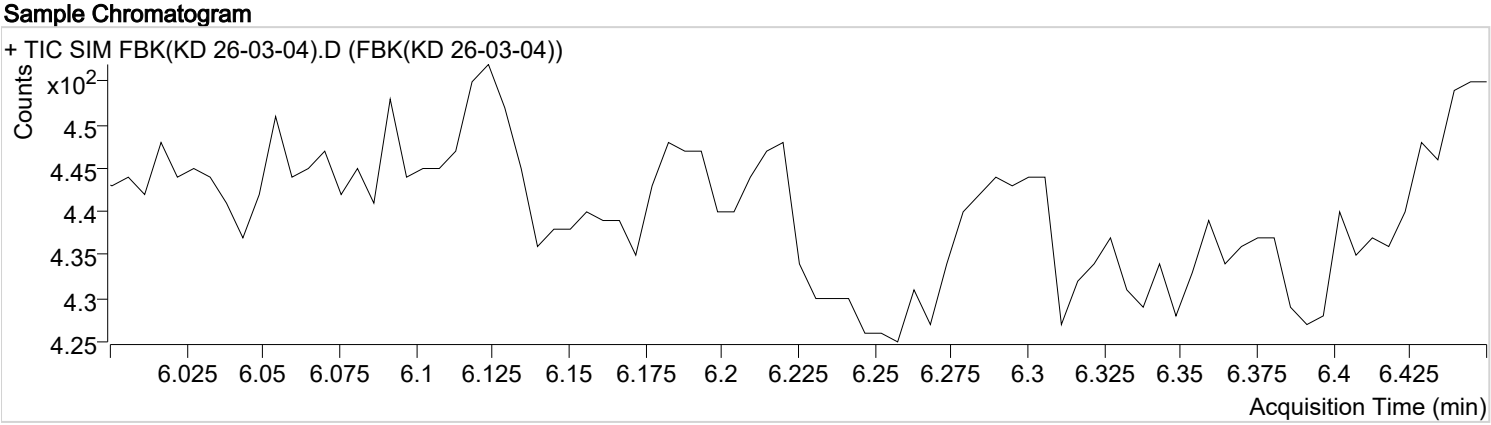

Epichlorohydrin





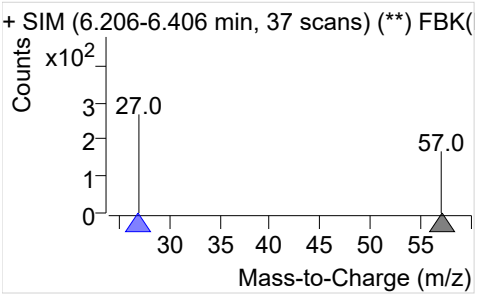

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 7:02:27	**Data File**	RE-01.D
Type	Sample	**Name**	RE-01
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

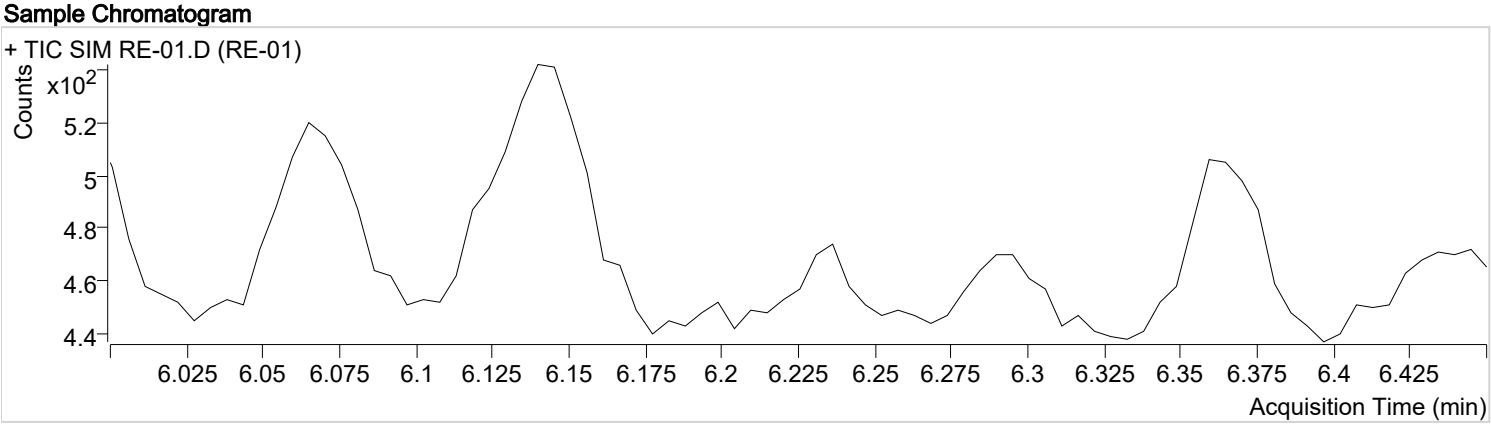

Epichlorohydrin





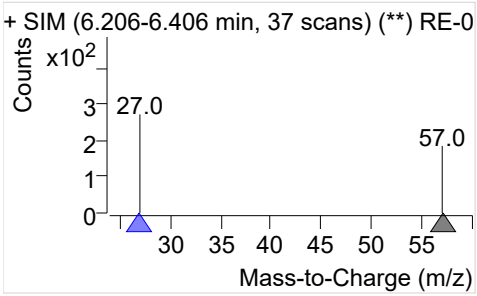

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 7:12:35	**Data File**	RE-02.D
Type	Sample	**Name**	RE-02
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

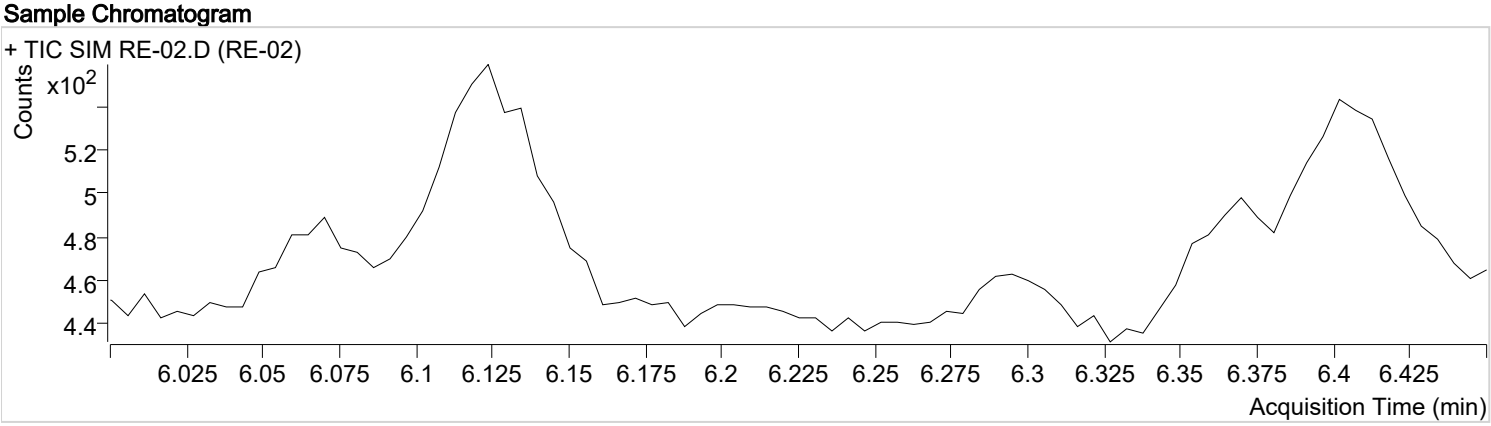

Epichlorohydrin





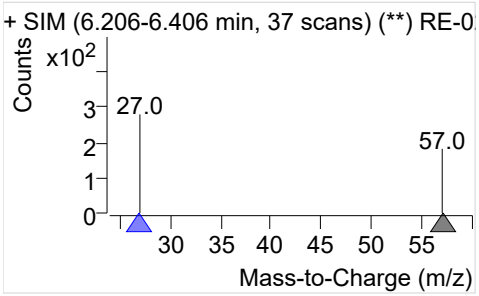

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 7:22:47	**Data File**	RE-03.D
Type	Sample	**Name**	RE-03
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

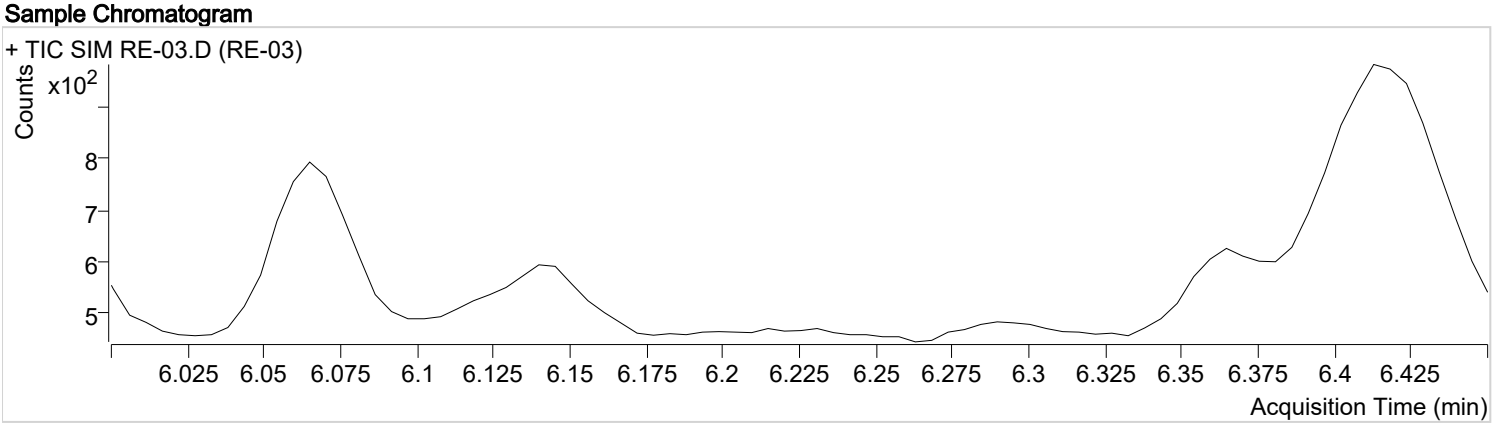

Epichlorohydrin





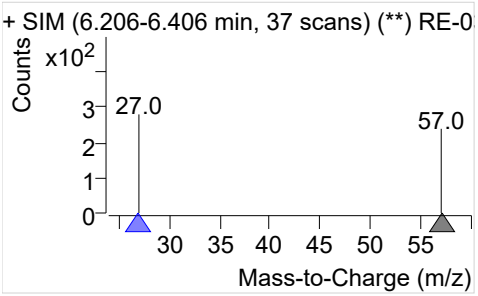

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 7:33:00	**Data File**	RE-04.D
Type	Sample	**Name**	RE-04
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

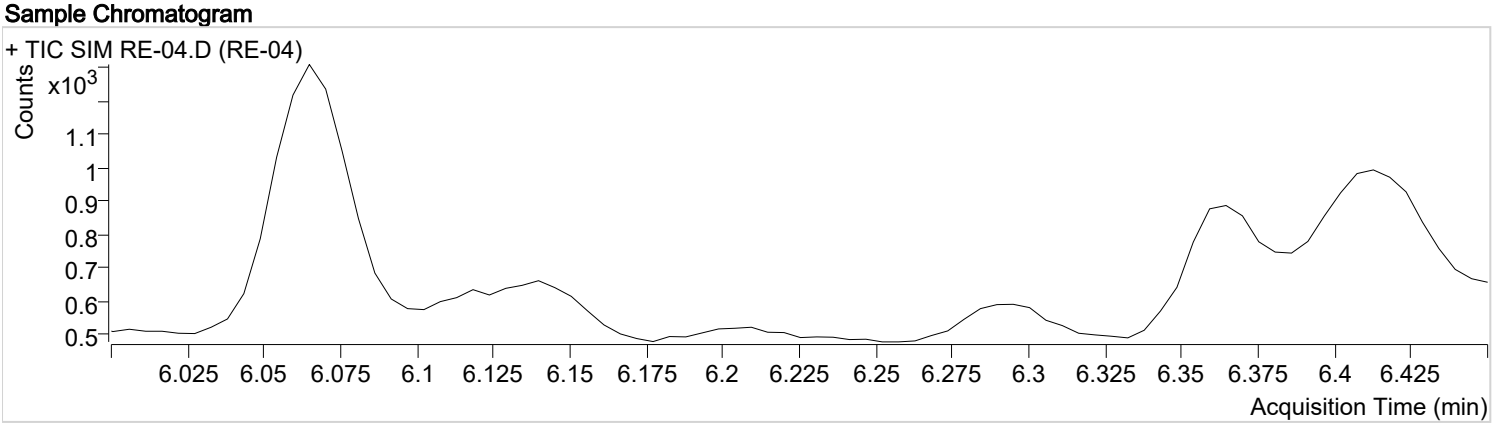

Epichlorohydrin





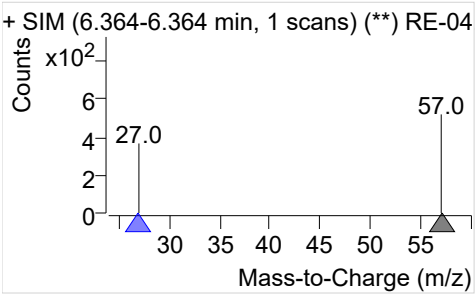

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 7:43:13	**Data File**	RE-09.D
Type	Sample	**Name**	RE-09
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

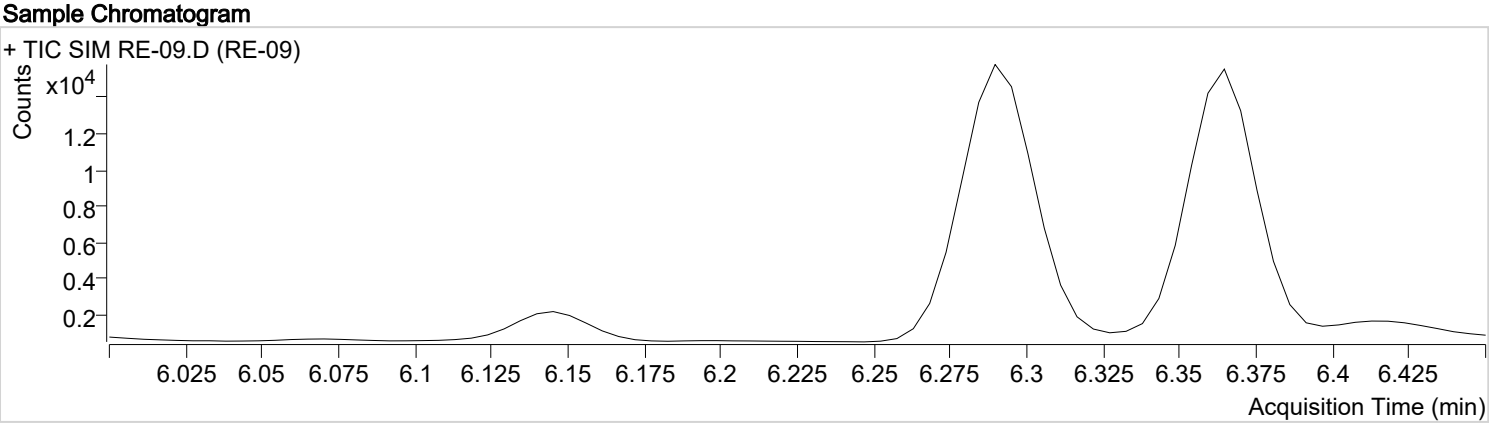

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	0	ND	mg/L

Epichlorohydrin

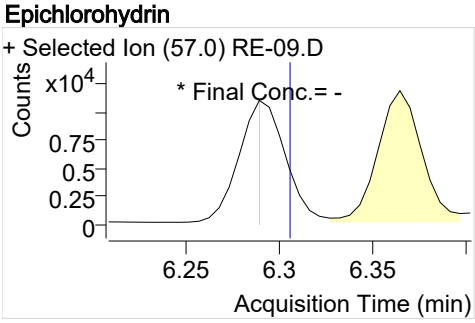





Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 7:53:26	**Data File**	RE-10.D
Type	Sample	**Name**	RE-10
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

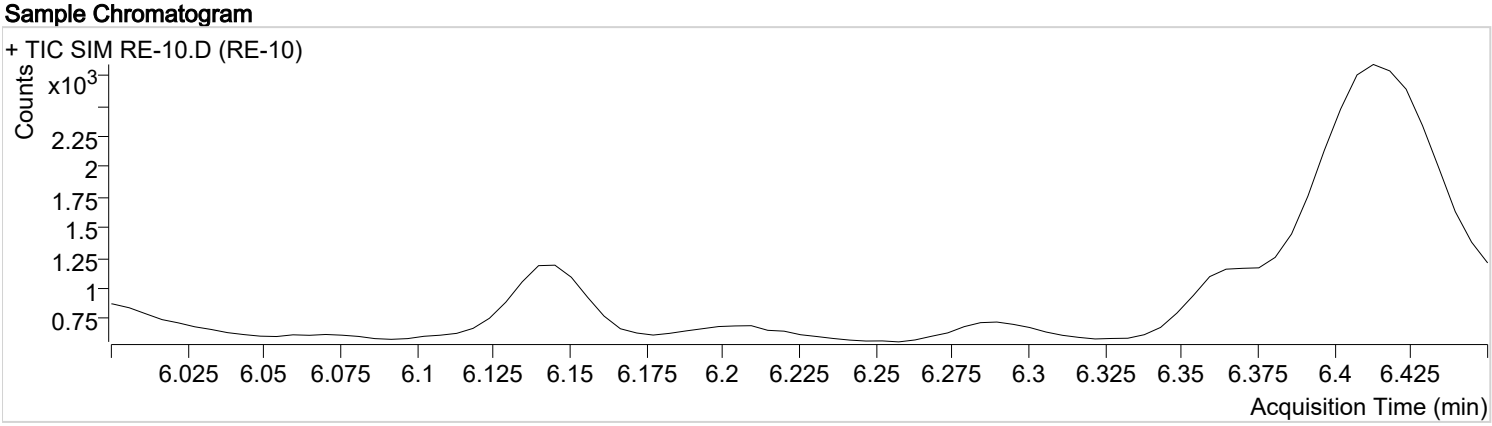

Epichlorohydrin





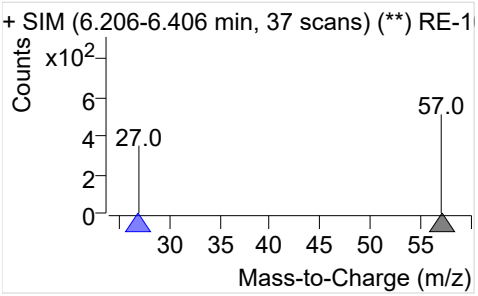

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 8:03:40	**Data File**	RE-11.D
Type	Sample	**Name**	RE-11
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

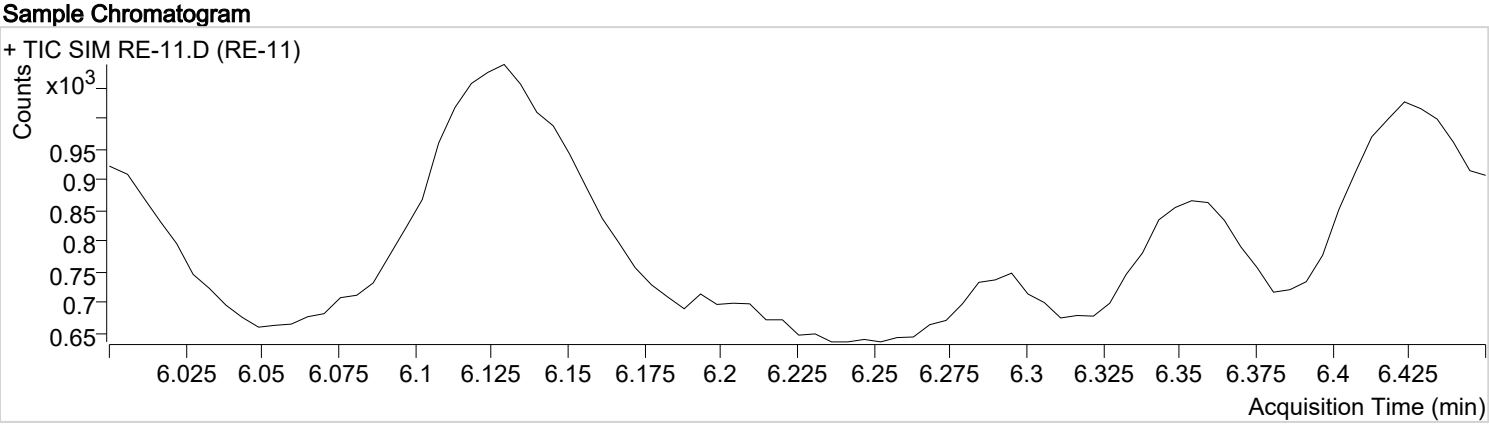

Epichlorohydrin





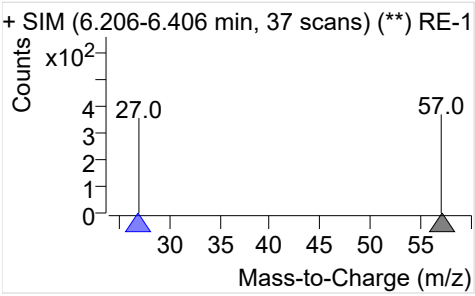

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 8:13:53	**Data File**	RE-12.D
Type	Sample	**Name**	RE-12
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

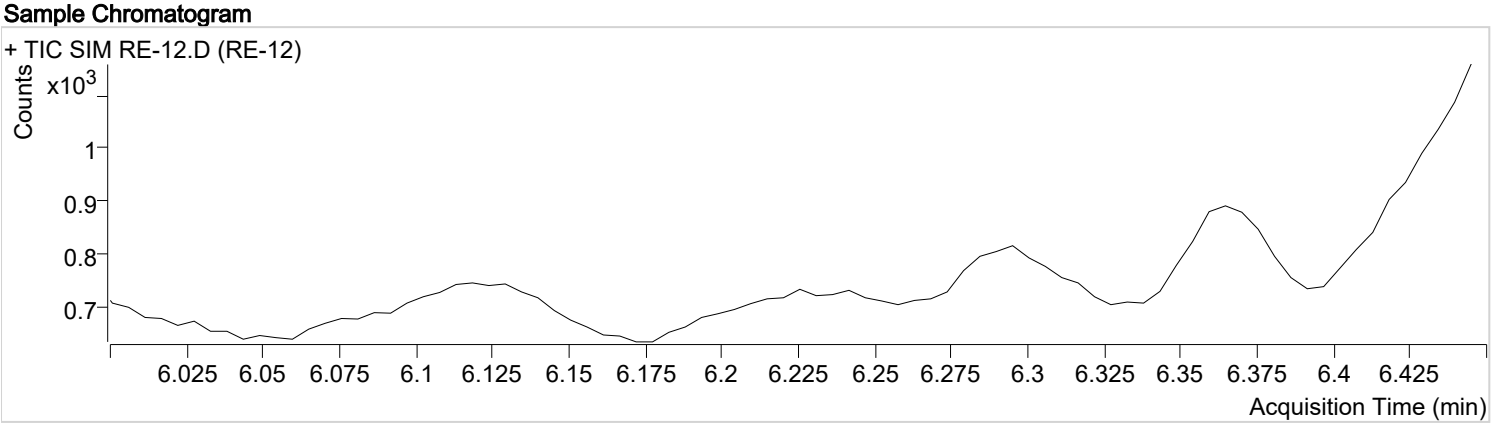

Epichlorohydrin





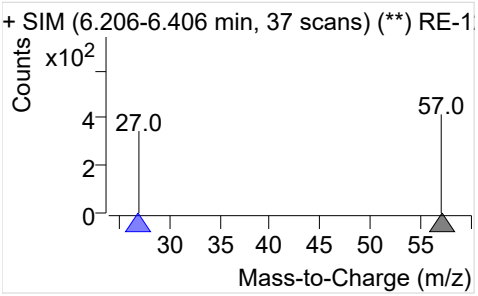

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 8:24:06	**Data File**	KD-01.D
Type	Sample	**Name**	KD-01
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

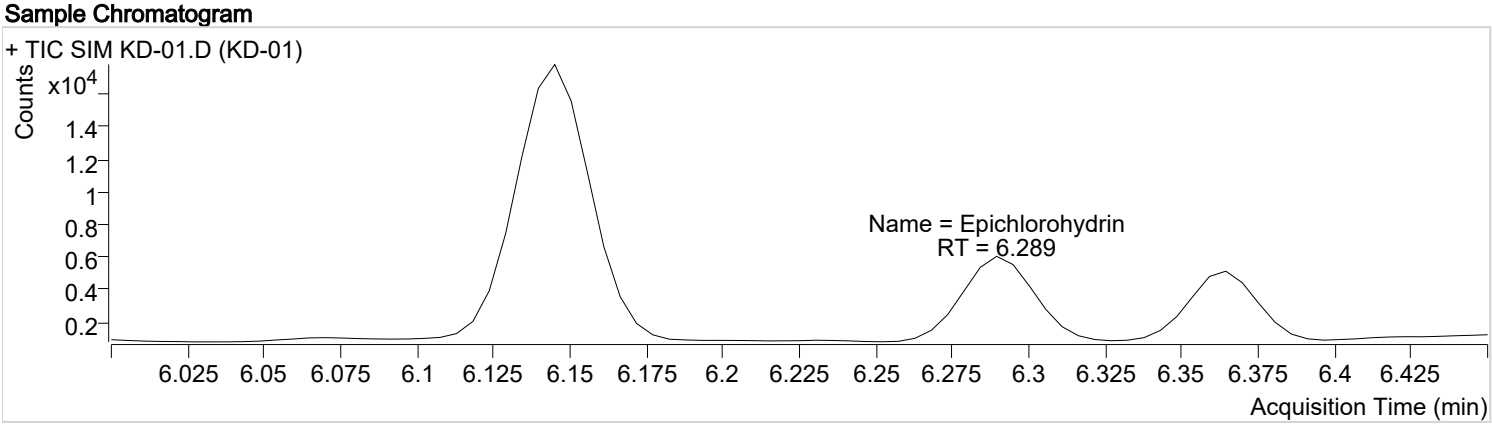

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.289	5388	0.002	mg/L

Epichlorohydrin

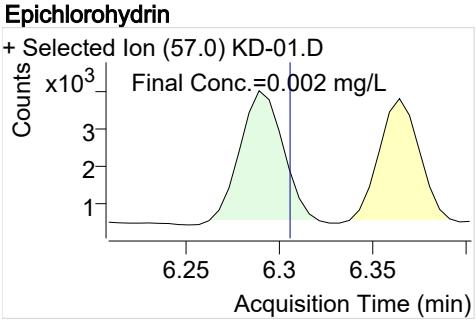





Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 8:34:18	**Data File**	KD-02.D
Type	Sample	**Name**	KD-02
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

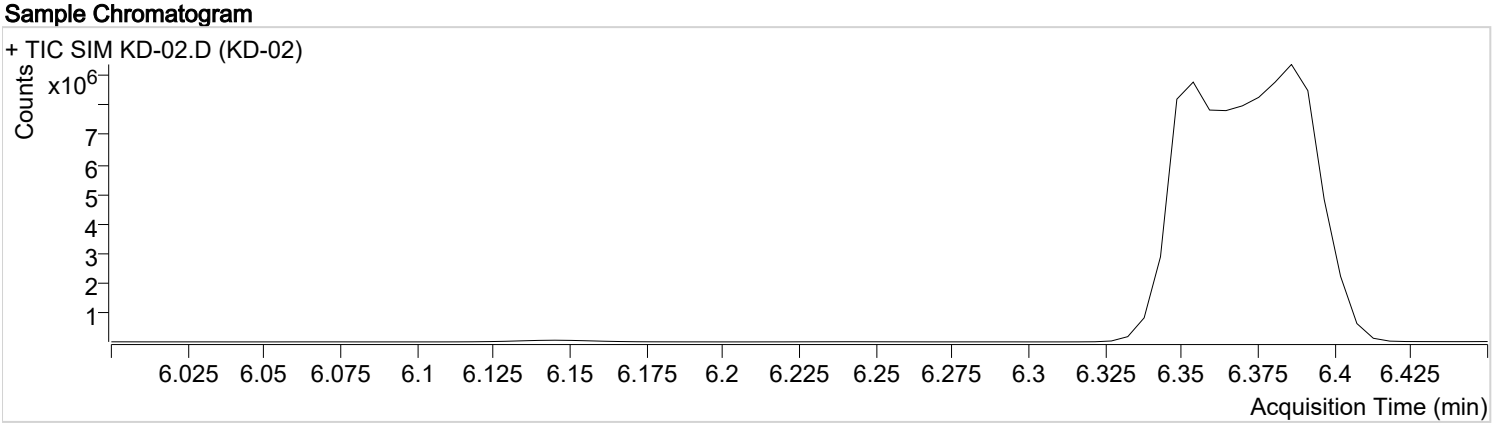

Epichlorohydrin





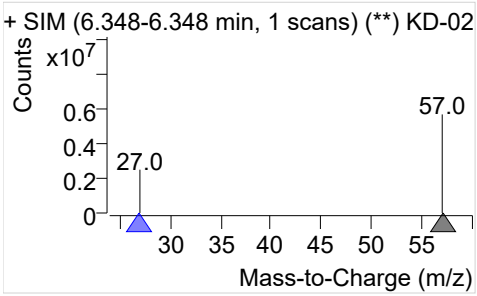

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 8:44:30	**Data File**	KD-03.D
Type	Sample	**Name**	KD-03
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

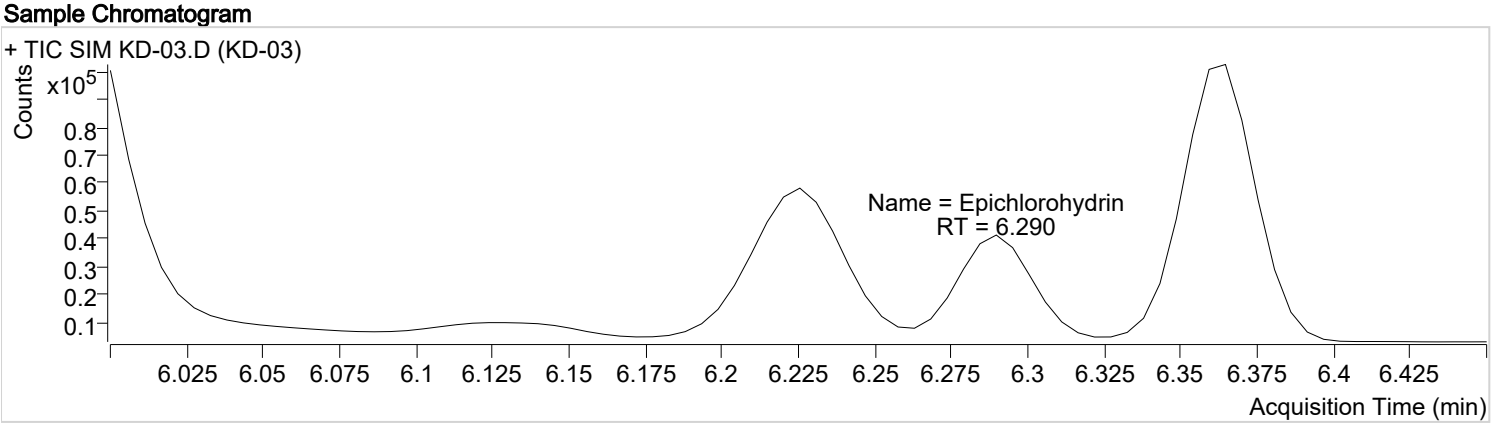

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	49773	0.017	mg/L

Epichlorohydrin

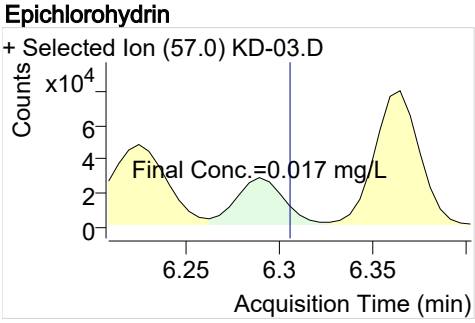



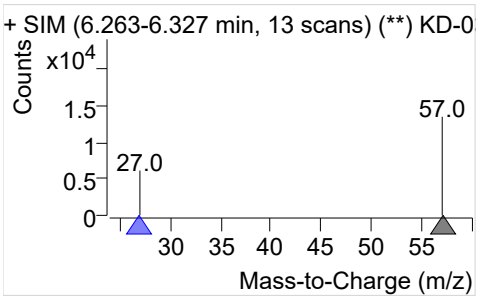

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 8:54:40	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

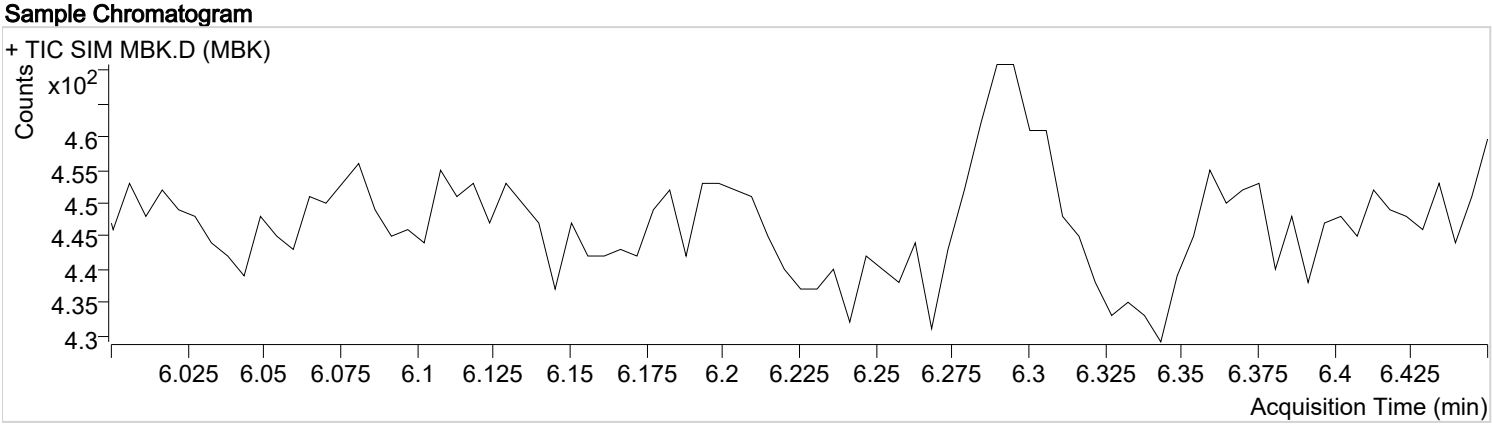

Epichlorohydrin





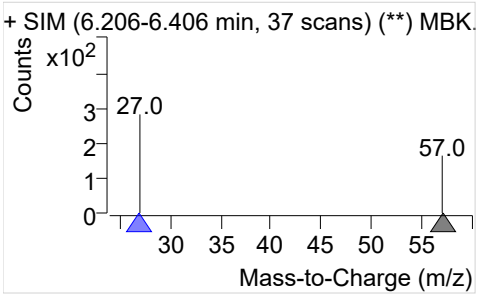

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 9:04:53	**Data File**	CCV.D
Type	QC	**Name**	CCV
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

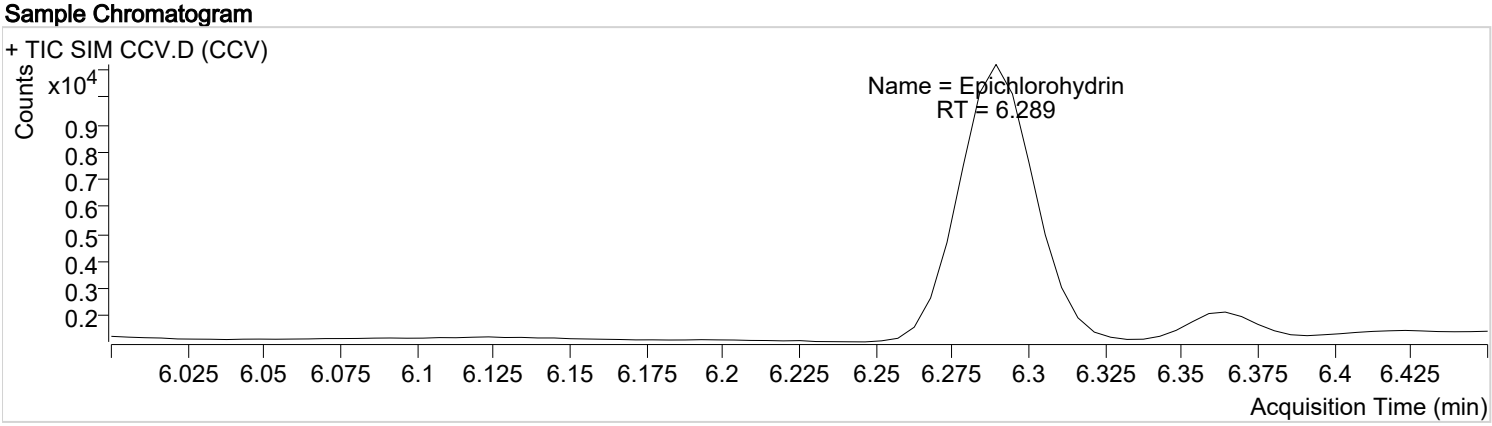

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.289	12655	2.323	mg/L

Epichlorohydrin

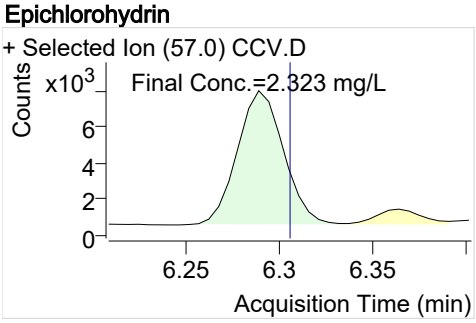



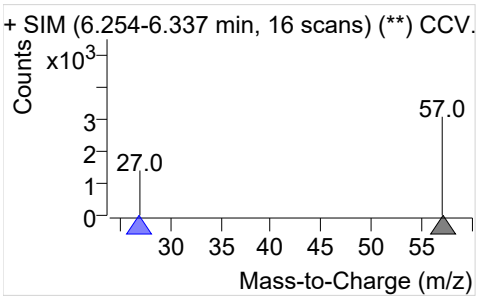

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 10:01:07	**Data File**	KD3-R.D
Type	Sample	**Name**	KD3-R
Dil.	0.004	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

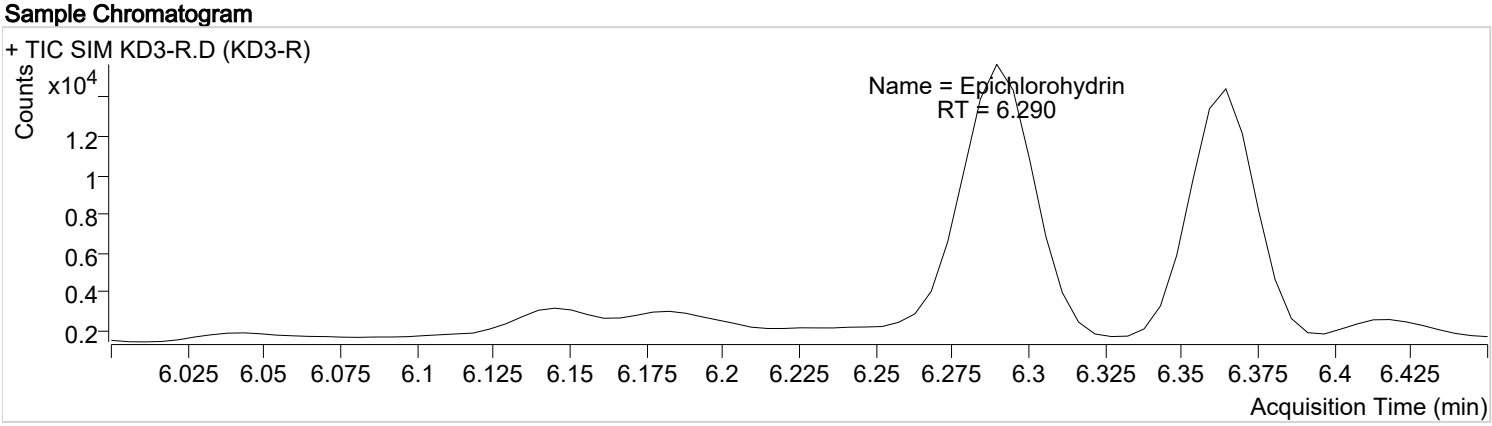

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	21371	0.015	mg/L

Epichlorohydrin

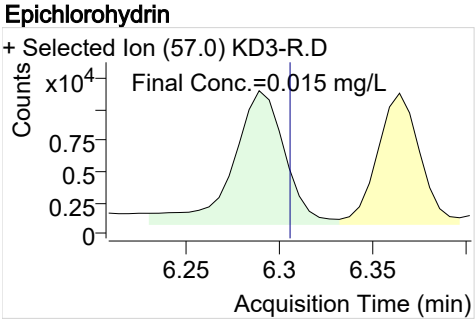





Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 10:11:33	**Data File**	MBK-2.D
Type	Blank	**Name**	MBK-2
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

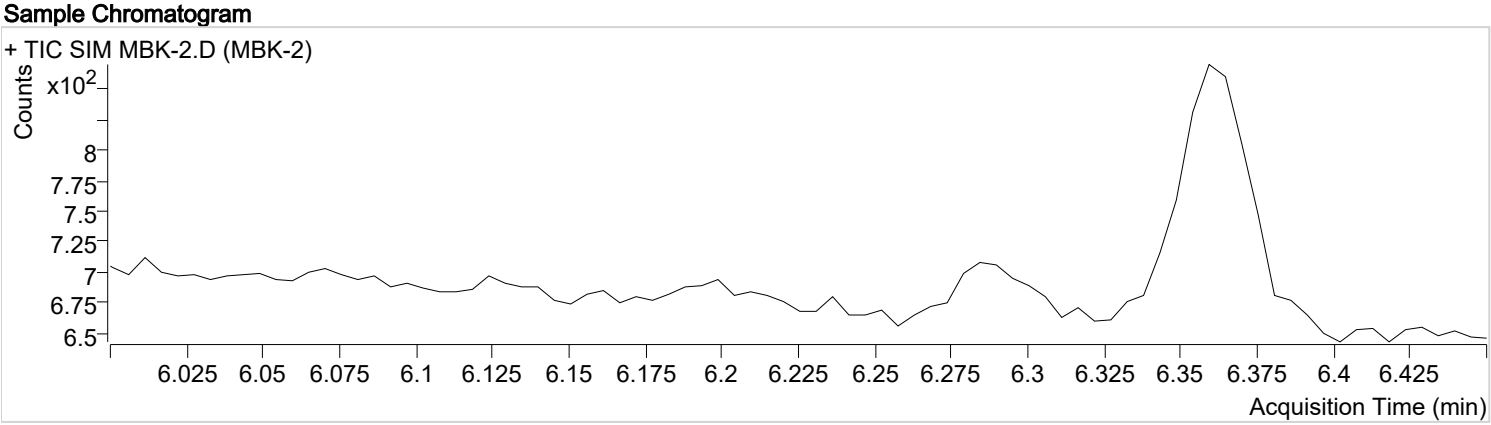

Epichlorohydrin





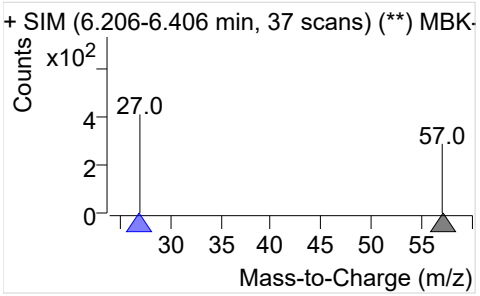

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(KD 3.4 RE 3.4)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-10 오후 4:48:39	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:53:09	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-10 오후 4:48:39	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-06 오후 10:21:46	**Data File**	CCV-2.D
Type	QC	**Name**	CCV-2
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

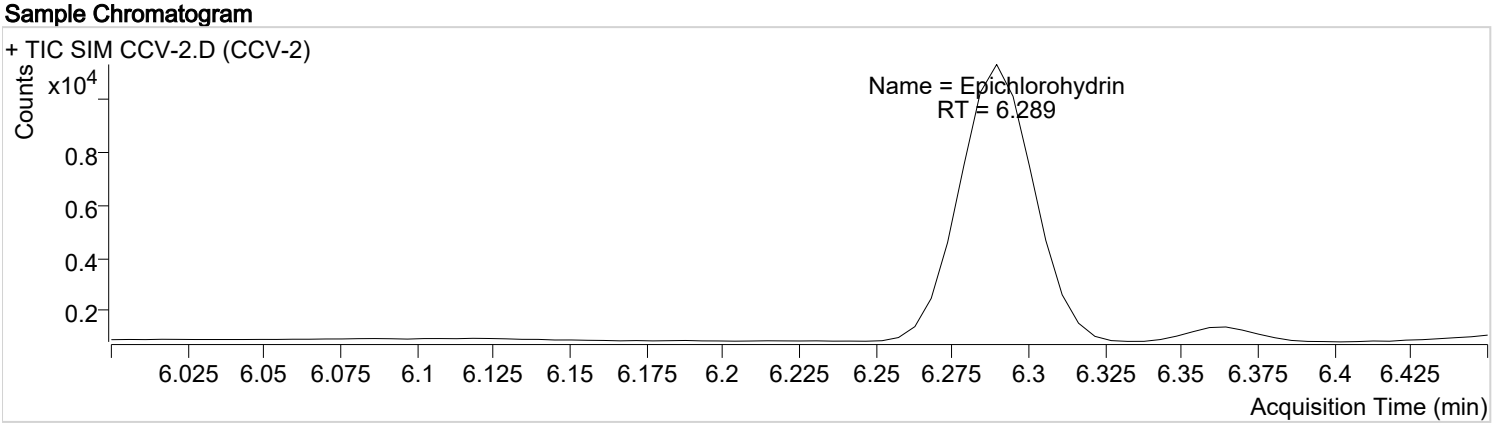

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.289	12743	2.337	mg/L
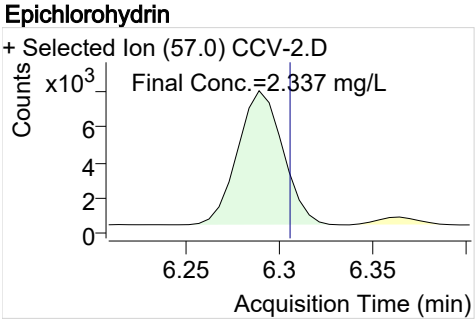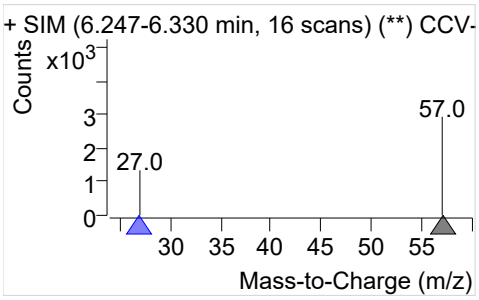
Epichlorohydrin