Quantitative Analysis Results Summary Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\QuantResults\EPIC.batch.bin				
Analysis Time	2026-03-23 오전 11:27:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:27:25	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Epichlorohydrin

Data File	Type	RT	Resp.	Final Conc.
EPIC ST-01.D	Cal	6.290	2228	0.211
EPIC ST-02.D	Cal	6.290	4702	0.483
EPIC ST-03.D	Cal	6.289	9802	1.042
EPIC ST-04.D	Cal	6.290	23429	2.538
EPIC ST-05.D	Cal	6.290	45649	4.976
BK-.D	Blank			ND
FBK(RE 26-03-17).D	Blank			ND
FBK(RE 26-03-18).D	Blank			ND
RE-05.D	Sample	6.290	4976	0.001
RE-06.D	Sample			ND
RE-13.D	Sample	6.364	0	ND
RE-14.D	Sample			ND
RE-24.D	Sample			ND
RE-25.D	Sample			ND
MBK.D	Blank			ND
CCV.D	QC	6.290	22598	2.447

Epichlorohydrin

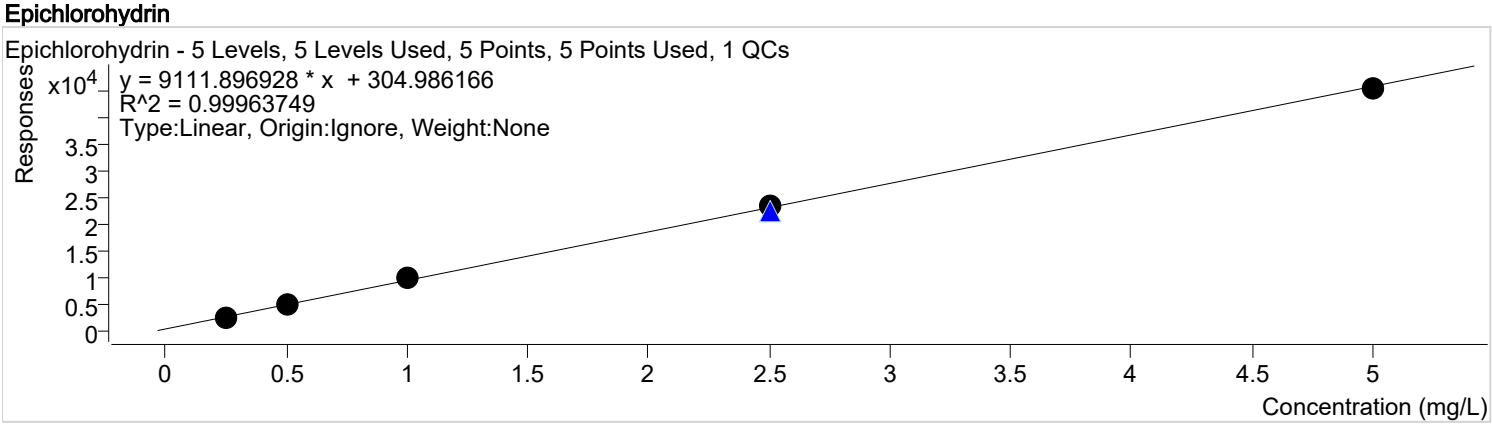

Cal. Path	Type	Level	Enable	Conc.	Response
D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\EPIC ST-01.D	Calibration	1	x	0.250	2228
D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\EPIC ST-02.D	Calibration	2	x	0.500	4702
D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\EPIC ST-03.D	Calibration	3	x	1.000	9802
D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\EPIC ST-04.D	Calibration	4	x	2.500	23429
D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\CCV.D	QC	4	x	2.500	22598
D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\EPIC ST-05.D	Calibration	5	x	5.000	45649

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-23 오전 11:27:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:50:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:27:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오전 11:08:41	**Data File**	EPIC ST-01.D
Type	Cal	**Name**	EPIC ST-01
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

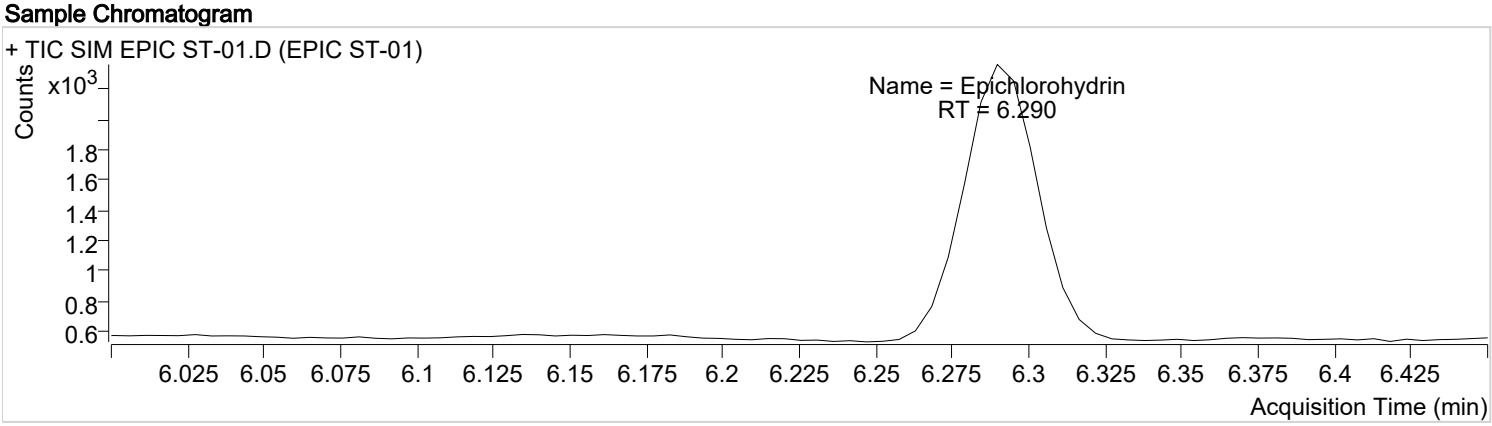

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	2228	0.211	mg/L

Epichlorohydrin

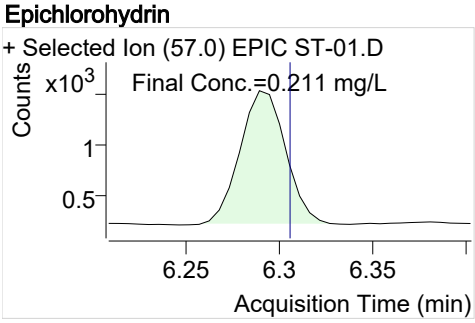





Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-23 오전 11:27:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:50:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:27:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오전 11:18:50	**Data File**	EPIC ST-02.D
Type	Cal	**Name**	EPIC ST-02
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

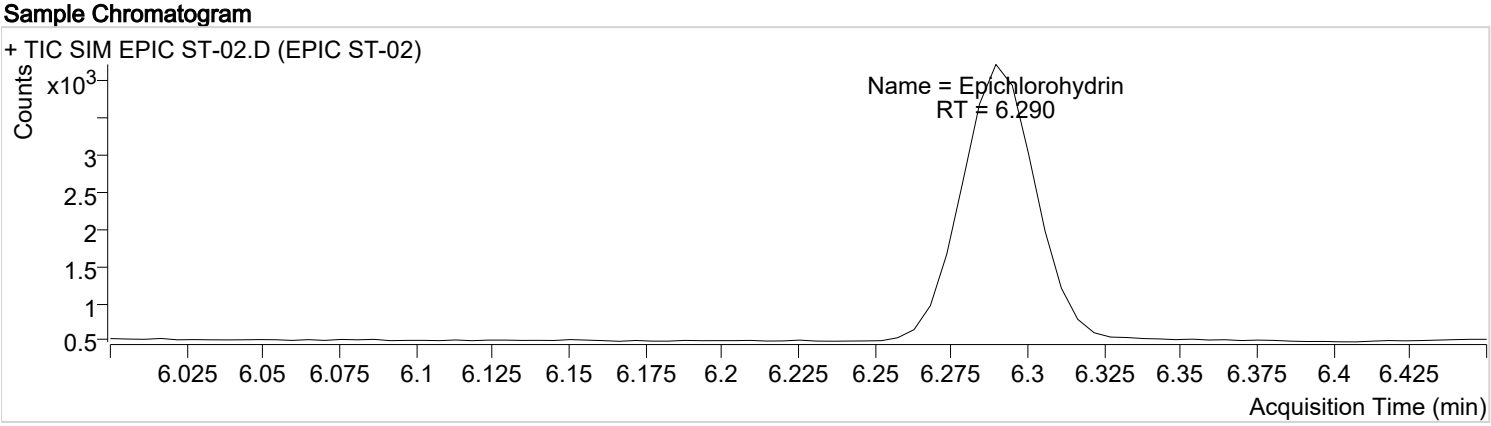

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	4702	0.483	mg/L

Epichlorohydrin

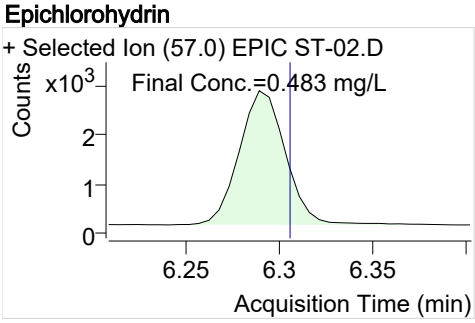



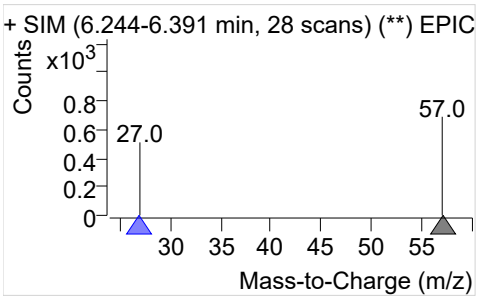

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-23 오전 11:27:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:50:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:27:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오전 11:29:00	**Data File**	EPIC ST-03.D
Type	Cal	**Name**	EPIC ST-03
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

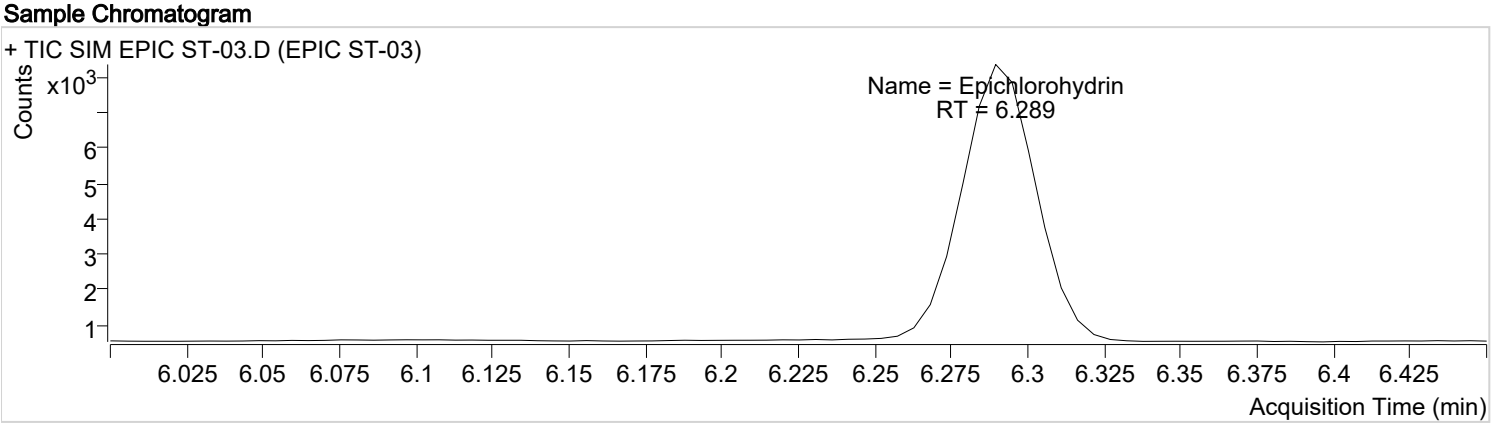

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.289	9802	1.042	mg/L

Epichlorohydrin

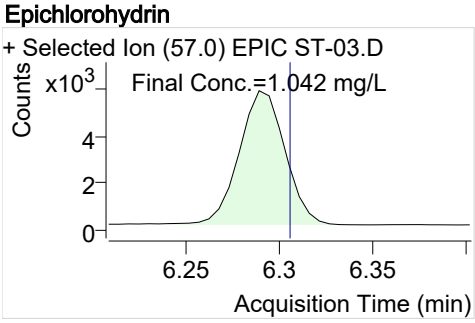



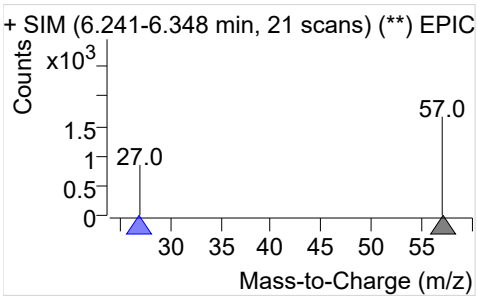

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-23 오전 11:27:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:50:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:27:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오전 11:39:14	**Data File**	EPIC ST-04.D
Type	Cal	**Name**	EPIC ST-04
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

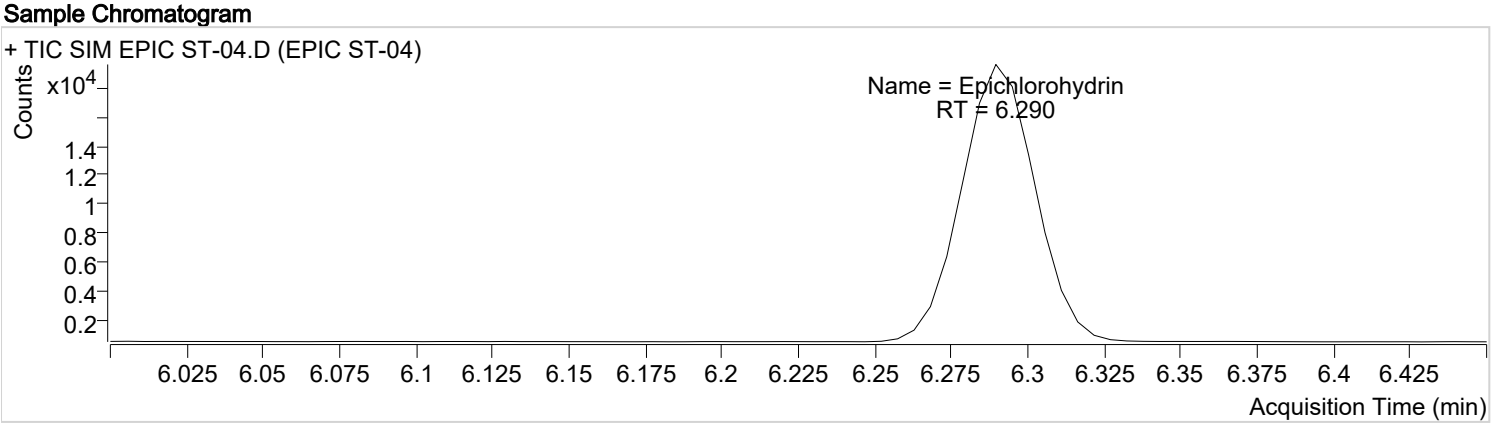

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	23429	2.538	mg/L

Epichlorohydrin

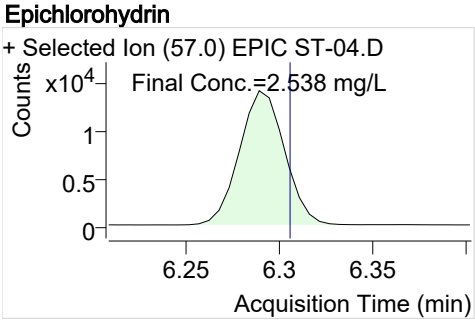



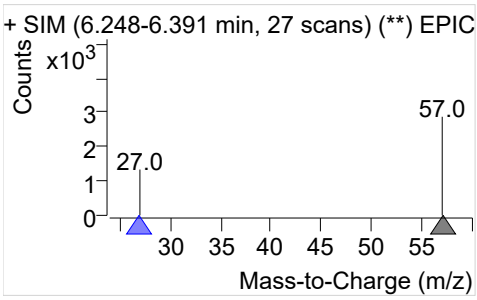

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-23 오전 11:27:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:50:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:27:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오전 11:49:29	**Data File**	EPIC ST-05.D
Type	Cal	**Name**	EPIC ST-05
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

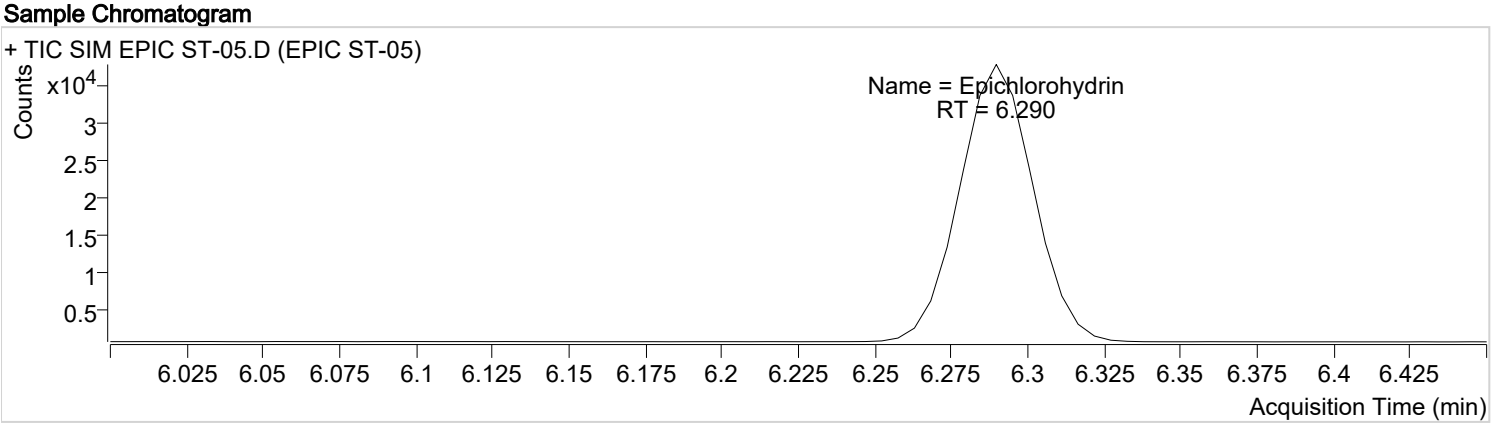

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	45649	4.976	mg/L

Epichlorohydrin

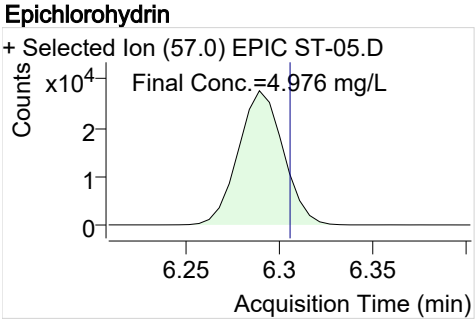

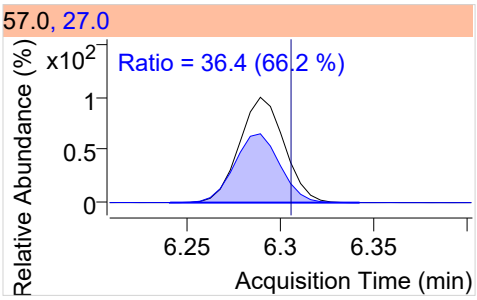

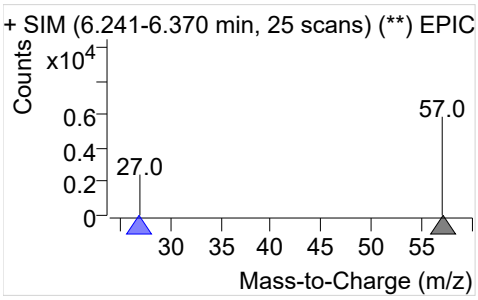

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-23 오전 11:27:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:50:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:27:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 12:09:55	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

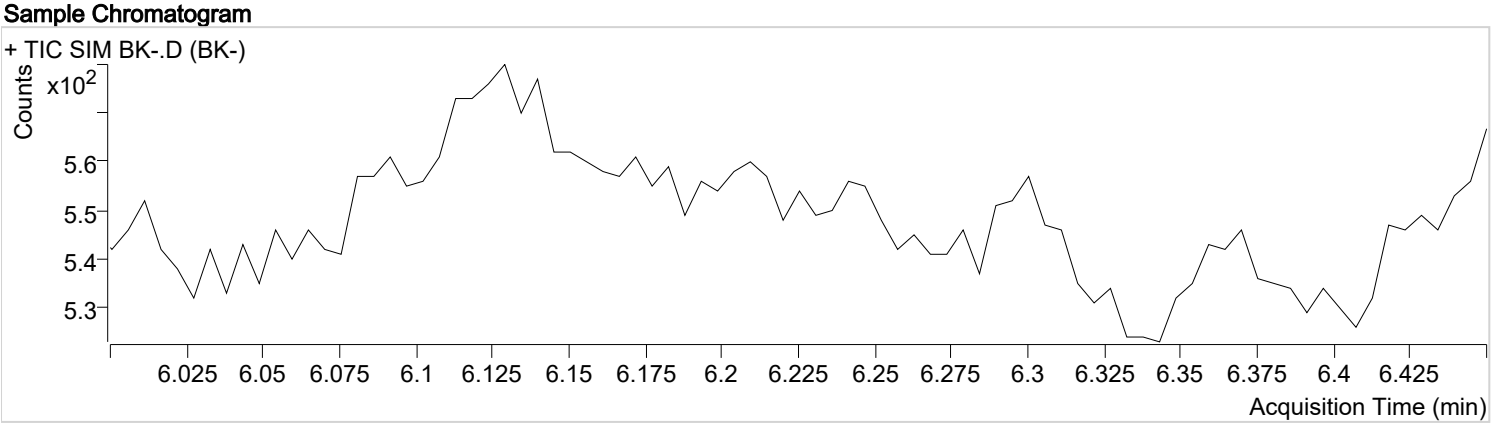

Epichlorohydrin

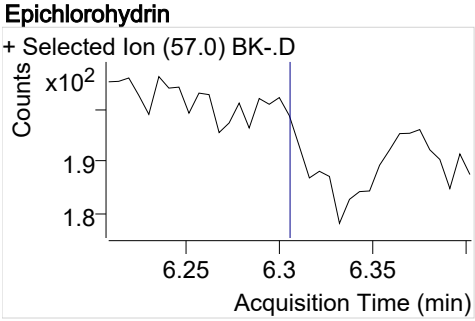



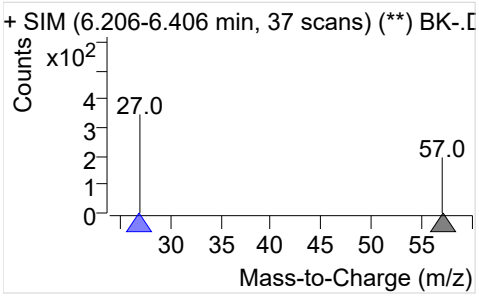

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-23 오전 11:27:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:50:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:27:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 12:20:07	**Data File**	FBK(RE 26-03-17).D
Type	Blank	**Name**	FBK(RE 26-03-17)
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

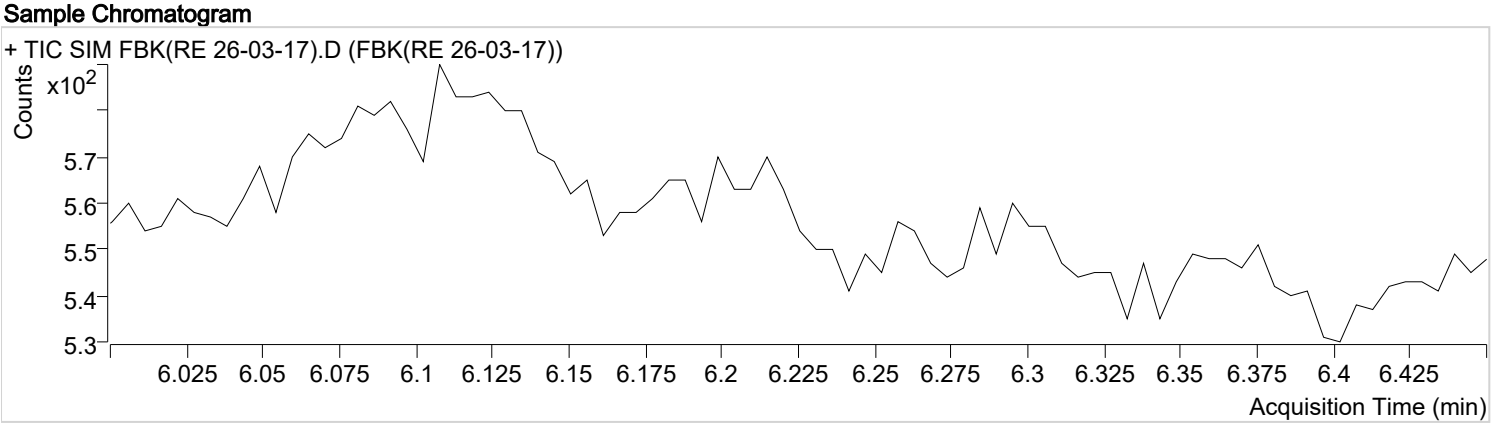

Epichlorohydrin

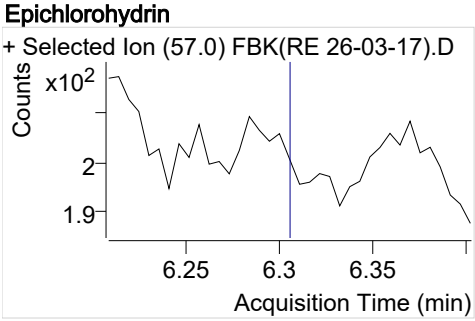



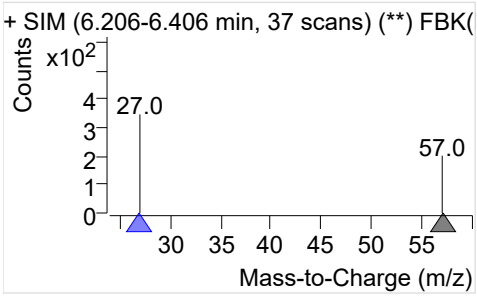

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-23 오전 11:27:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:50:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:27:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 12:44:42	**Data File**	FBK(RE 26-03-18).D
Type	Blank	**Name**	FBK(RE 26-03-18)
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

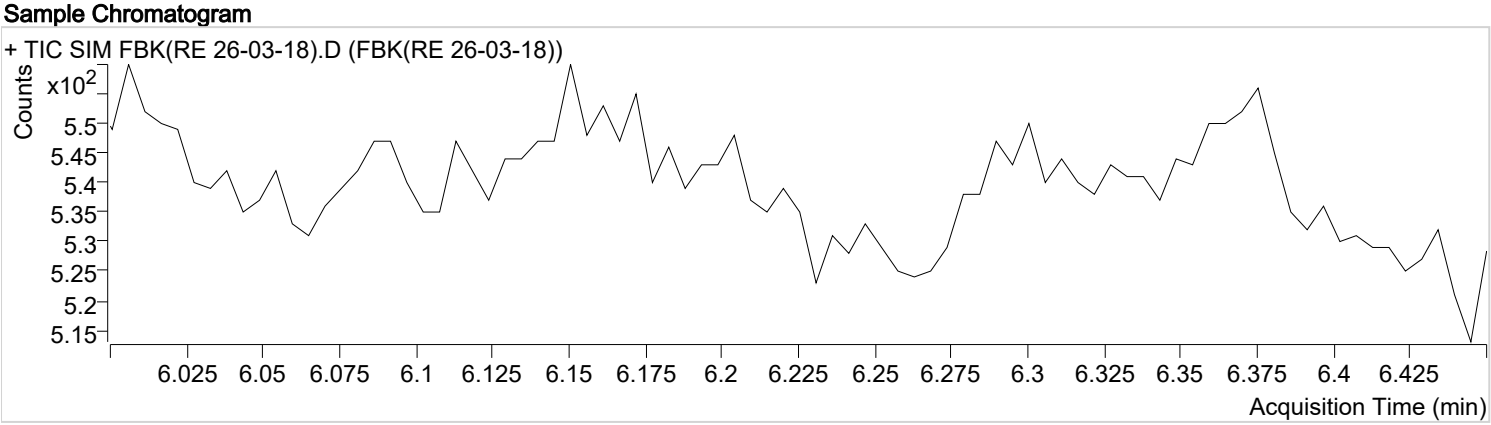

Epichlorohydrin

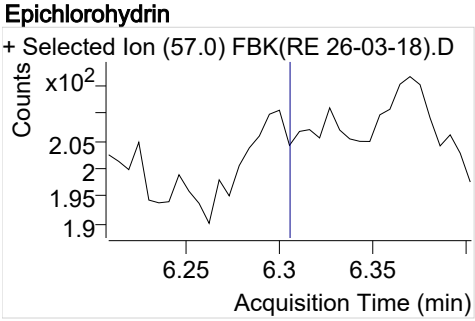



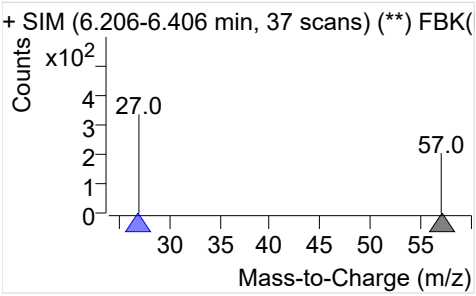

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-23 오전 11:27:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:50:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:27:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 12:54:55	**Data File**	RE-05.D
Type	Sample	**Name**	RE-05
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

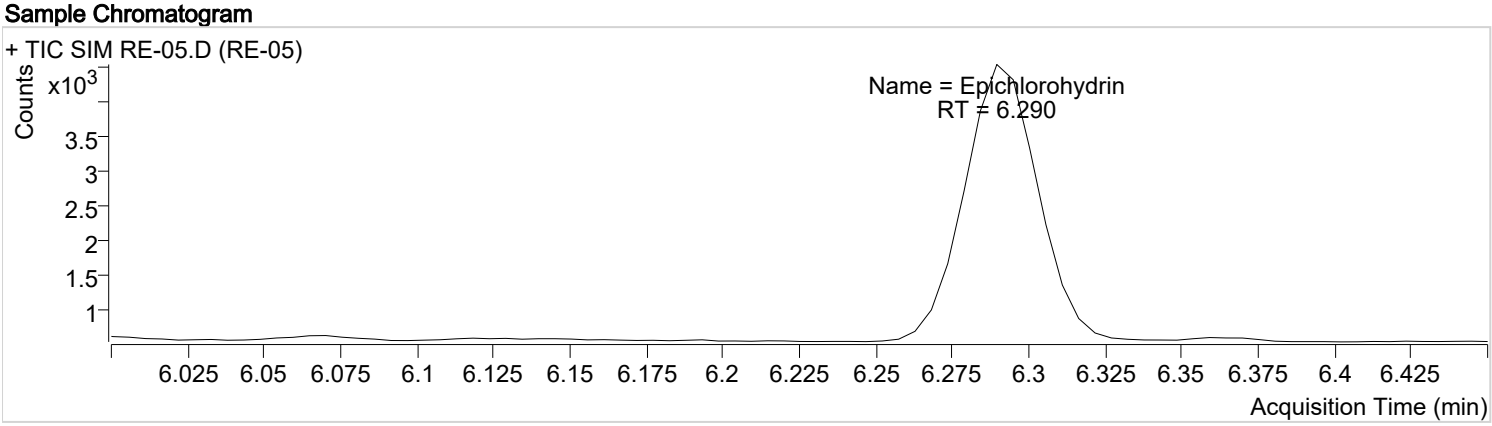

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	4976	0.001	mg/L

Epichlorohydrin

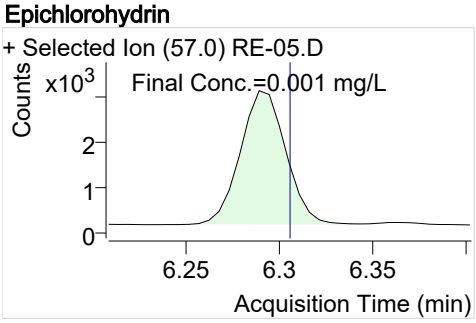

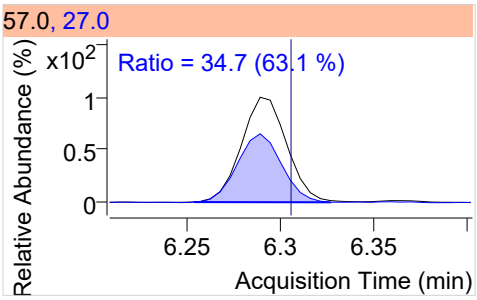

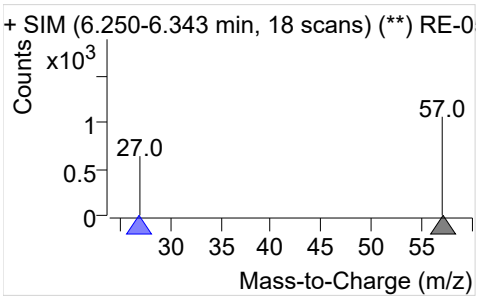

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-23 오전 11:27:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:50:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:27:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 2:03:19	**Data File**	RE-06.D
Type	Sample	**Name**	RE-06
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

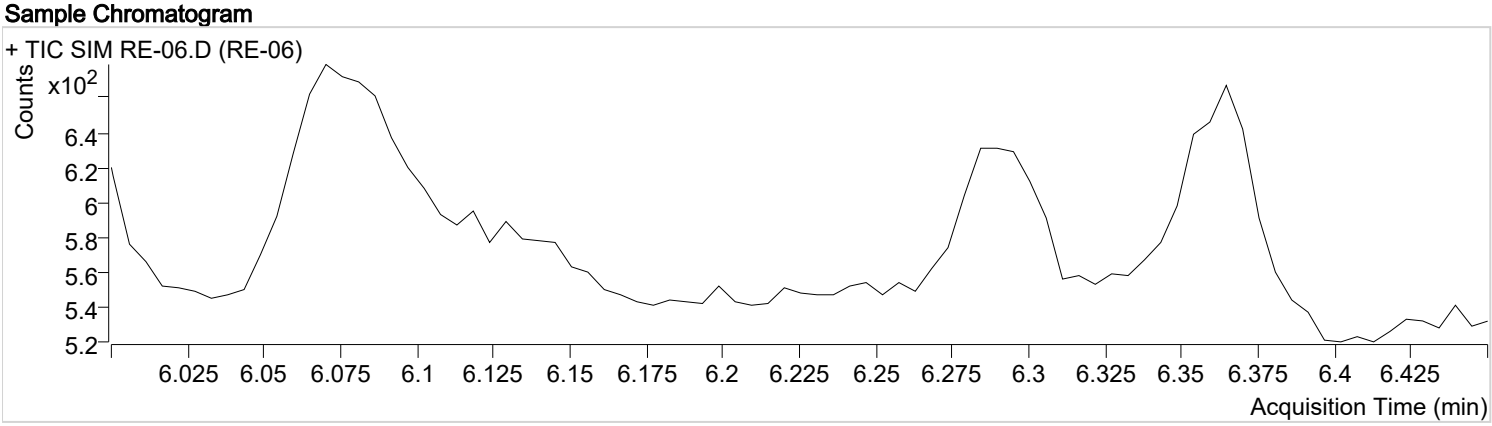

Epichlorohydrin

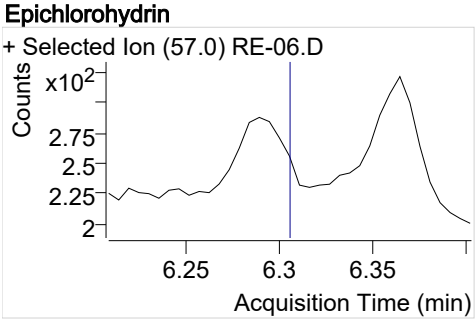



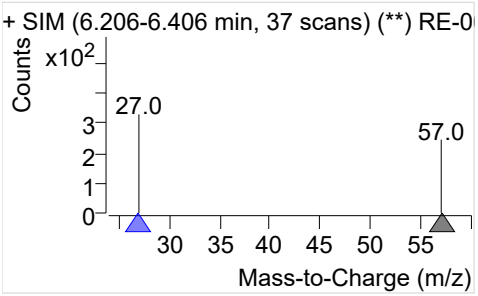

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-23 오전 11:27:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:50:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:27:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 2:13:28	**Data File**	RE-13.D
Type	Sample	**Name**	RE-13
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

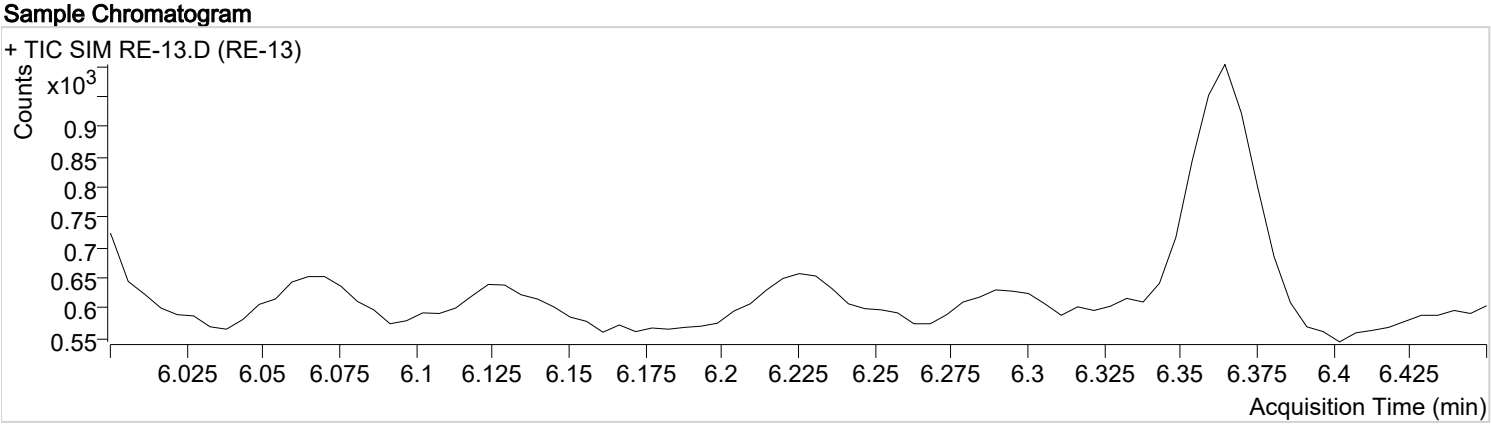

Epichlorohydrin

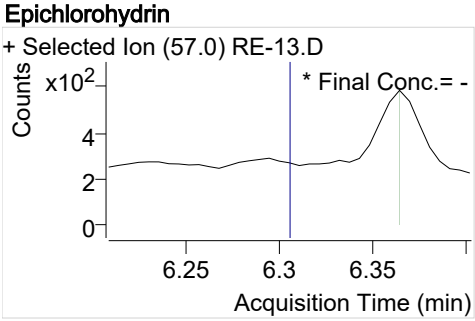



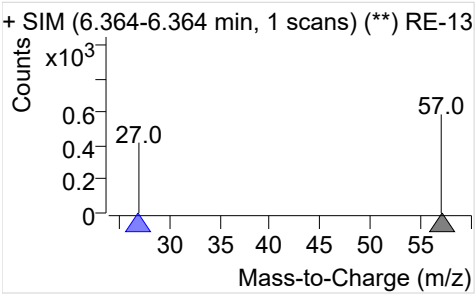

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-23 오전 11:27:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:50:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:27:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 2:23:38	**Data File**	RE-14.D
Type	Sample	**Name**	RE-14
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

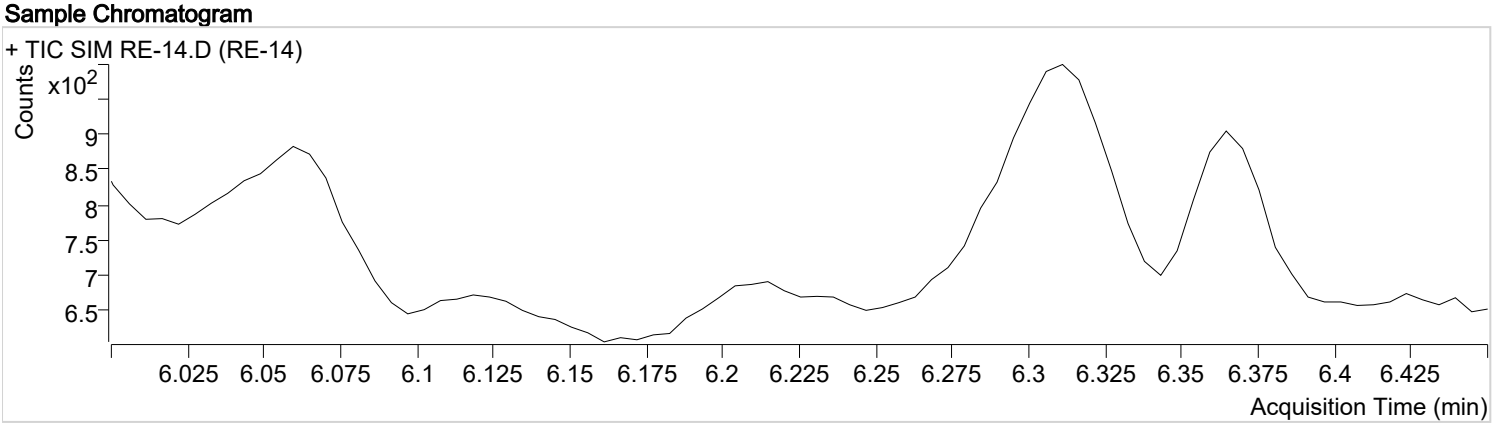

Epichlorohydrin

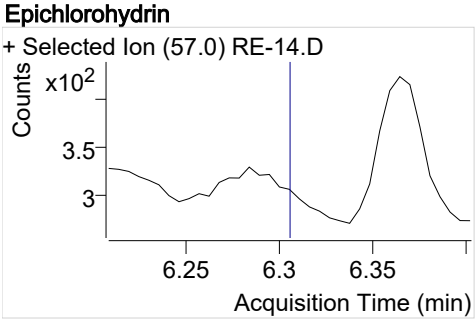

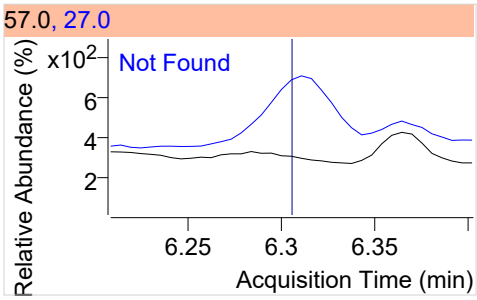

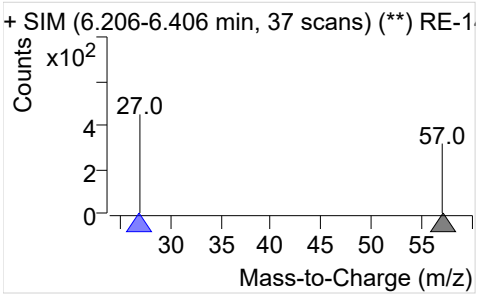

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-23 오전 11:27:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:50:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:27:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 2:33:50	**Data File**	RE-24.D
Type	Sample	**Name**	RE-24
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

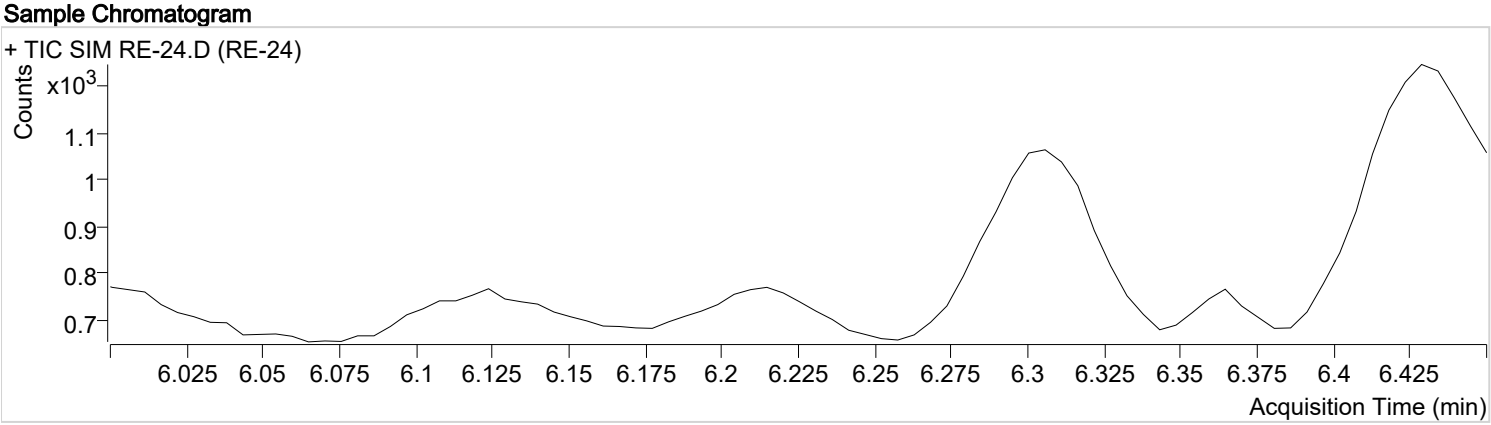

Epichlorohydrin

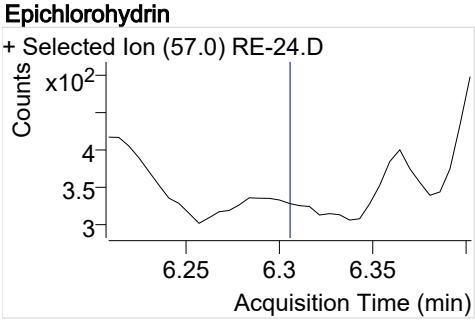



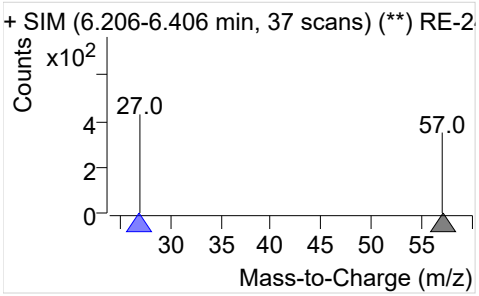

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-23 오전 11:27:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:50:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:27:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 3:40:49	**Data File**	RE-25.D
Type	Sample	**Name**	RE-25
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

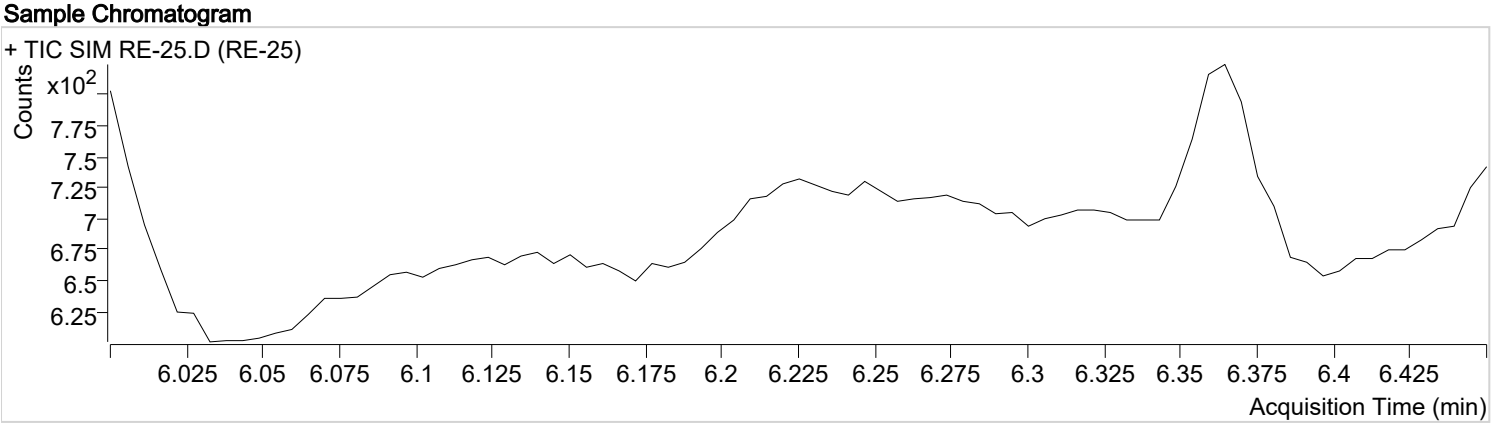

Epichlorohydrin

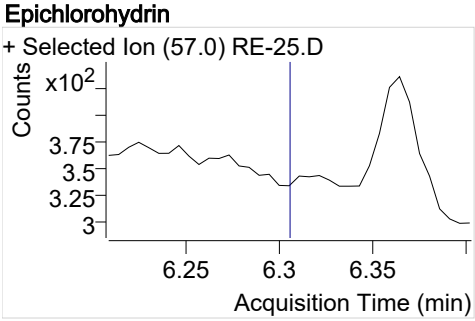



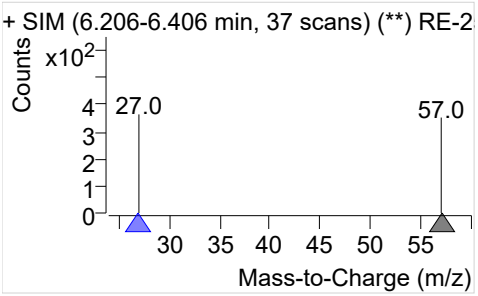

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-23 오전 11:27:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:50:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:27:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 3:51:03	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

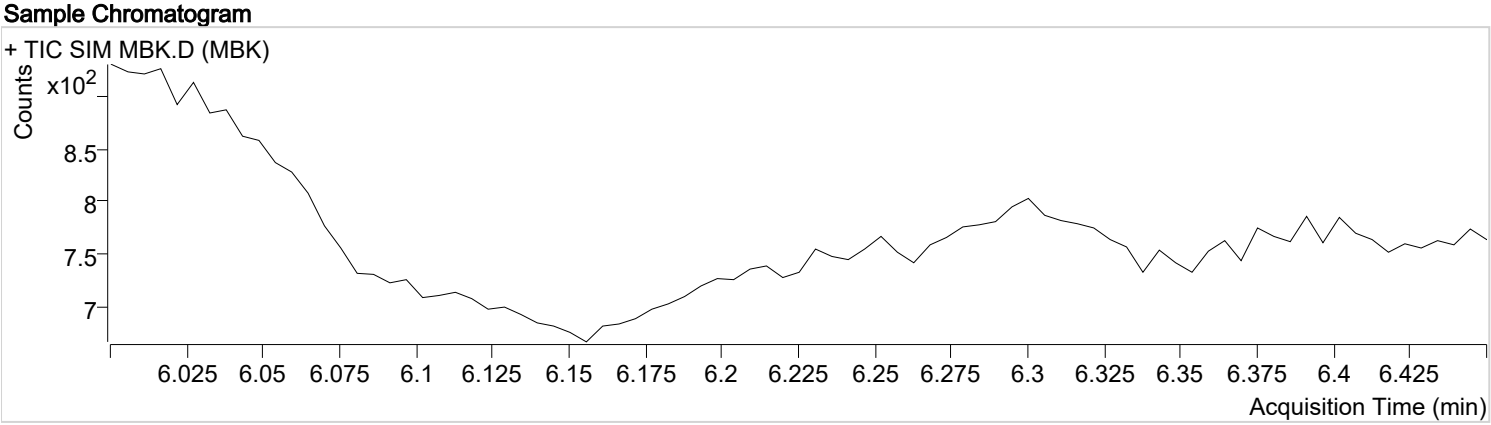

Epichlorohydrin

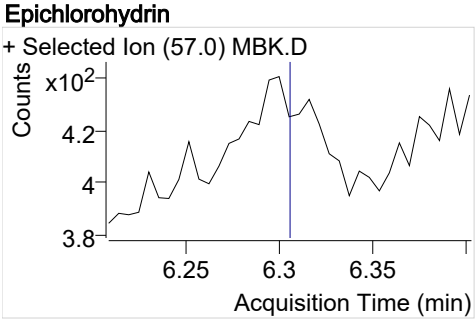



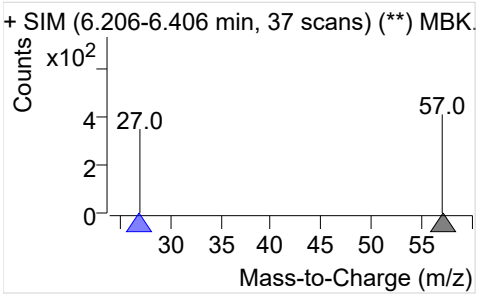

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(RE 3.17.18)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-03-23 오전 11:27:25	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:50:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-23 오전 11:27:25	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-20 오후 4:01:14	**Data File**	CCV.D
Type	QC	**Name**	CCV
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

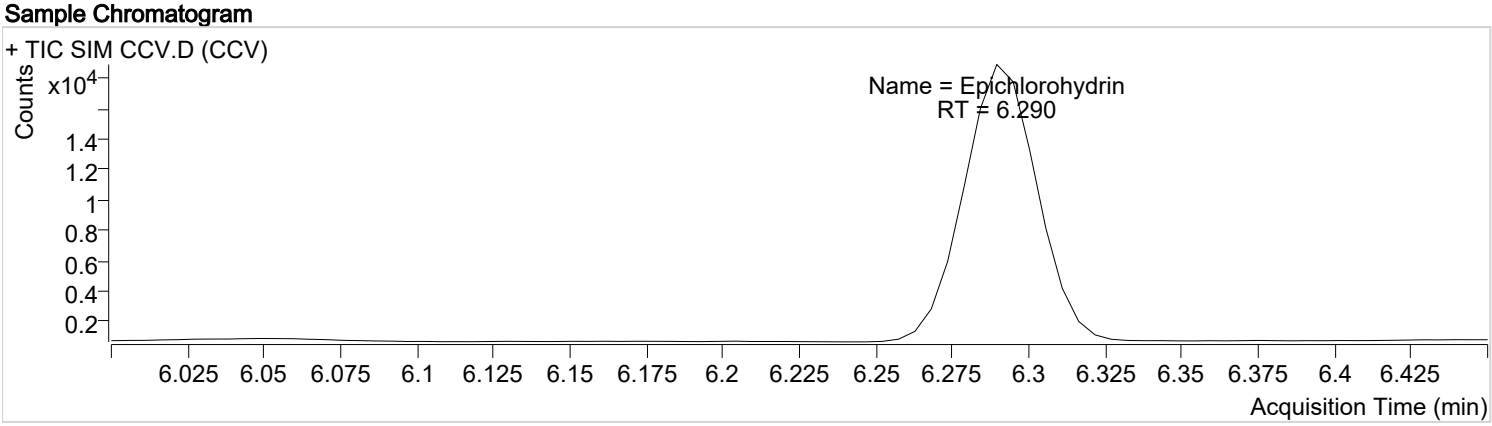

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	22598	2.447	mg/L
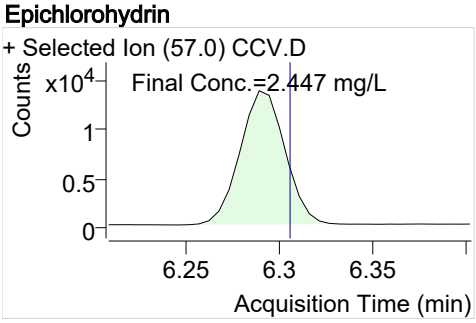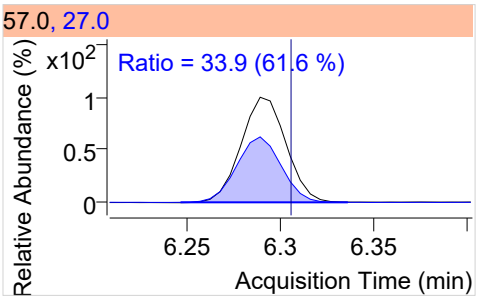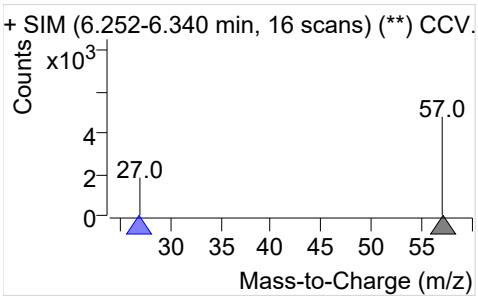
Epichlorohydrin