Quantitative Analysis Results Summary Report

Agilent | Trusted Answers

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\QuantResults\EPIC.batch.bin				
Analysis Time	2026-04-01 오후 4:31:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:31:23	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Epichlorohydrin

Data File	Type	RT	Resp.	Final Conc.
EPIC ST-01.D	Cal	6.290	2204	0.247
EPIC ST-02.D	Cal	6.290	5059	0.529
EPIC ST-03.D	Cal	6.290	9273	0.947
EPIC ST-04.D	Cal	6.290	25359	2.538
EPIC ST-05.D	Cal	6.290	50117	4.989
BK-.D	Blank			ND
FBK(LG NJ 26-03-26).D	Blank			ND
NJ-01.D	Sample			ND
NJ-02.D	Sample			ND
NJ-03.D	Sample	6.327	0	ND
NJ-04.D	Sample	6.333	0	ND
NJ-05.D	Sample	6.343	0	ND
NJ-06.D	Sample	6.365	0	ND
MBK.D	Blank			ND
CCV.D	QC	6.290	22785	2.284

Epichlorohydrin

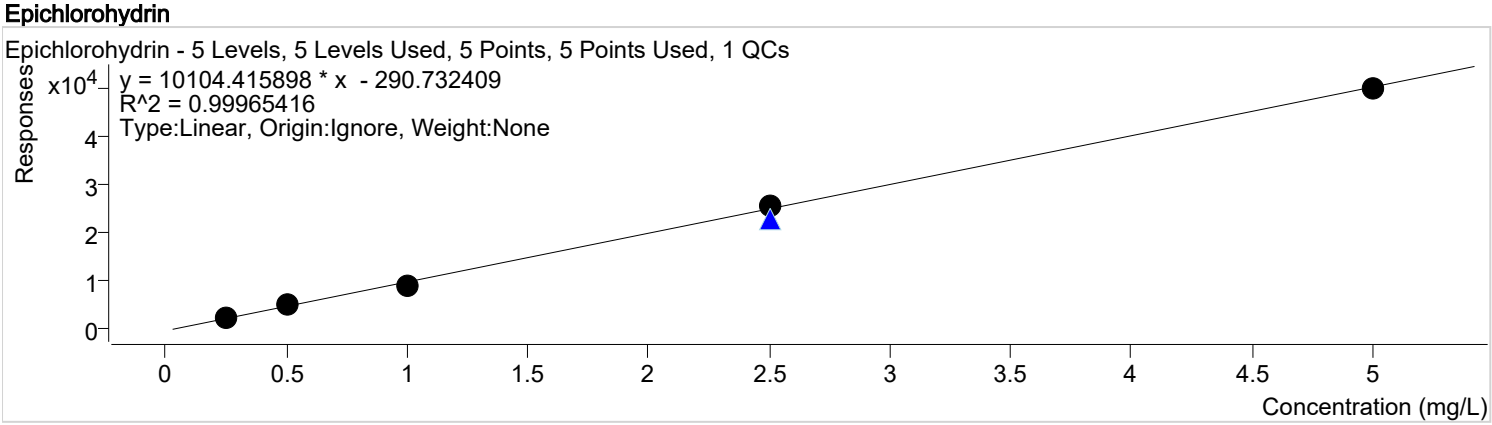

Cal. Path	Type	Level	Enable	Conc.	Response
D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\EPIC ST-01.D	Calibration	1	x	0.250	2204
D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\EPIC ST-02.D	Calibration	2	x	0.500	5059
D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\EPIC ST-03.D	Calibration	3	x	1.000	9273
D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\EPIC ST-04.D	Calibration	4	x	2.500	25359
D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\CCV.D	QC	4	x	2.500	22785
D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\EPIC ST-05.D	Calibration	5	x	5.000	50117

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-04-01 오후 4:31:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:51:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:31:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-31 오전 11:23:49	**Data File**	EPIC ST-01.D
Type	Cal	**Name**	EPIC ST-01
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

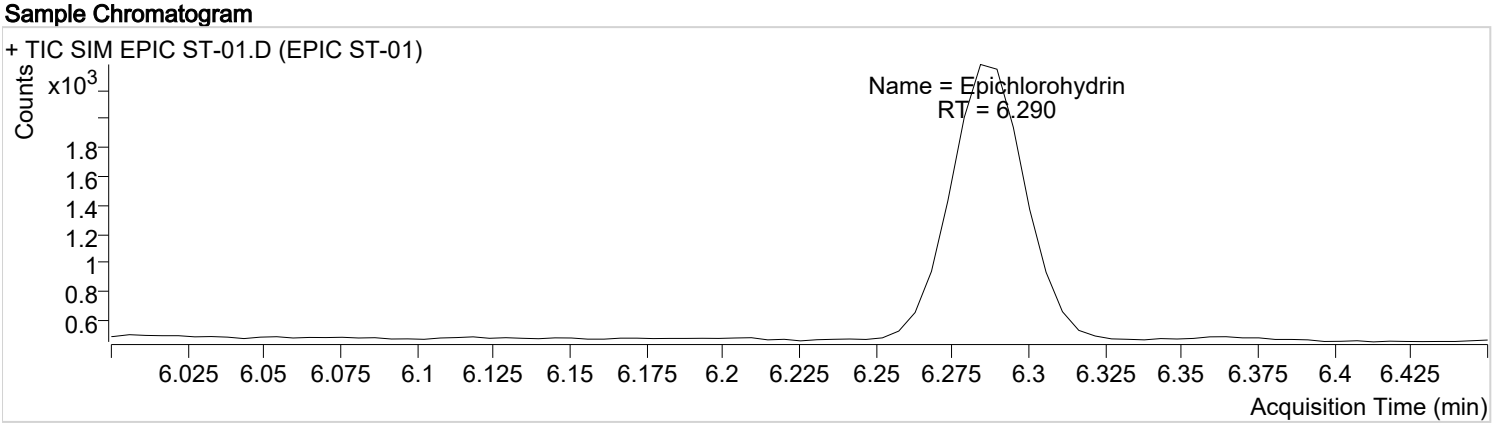

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	2204	0.247	mg/L

Epichlorohydrin

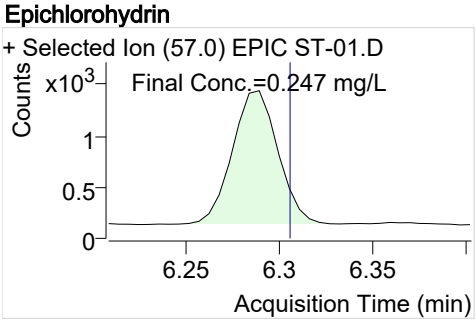



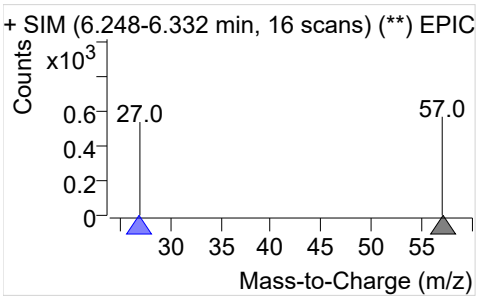

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-04-01 오후 4:31:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:51:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:31:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-31 오전 11:34:00	**Data File**	EPIC ST-02.D
Type	Cal	**Name**	EPIC ST-02
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

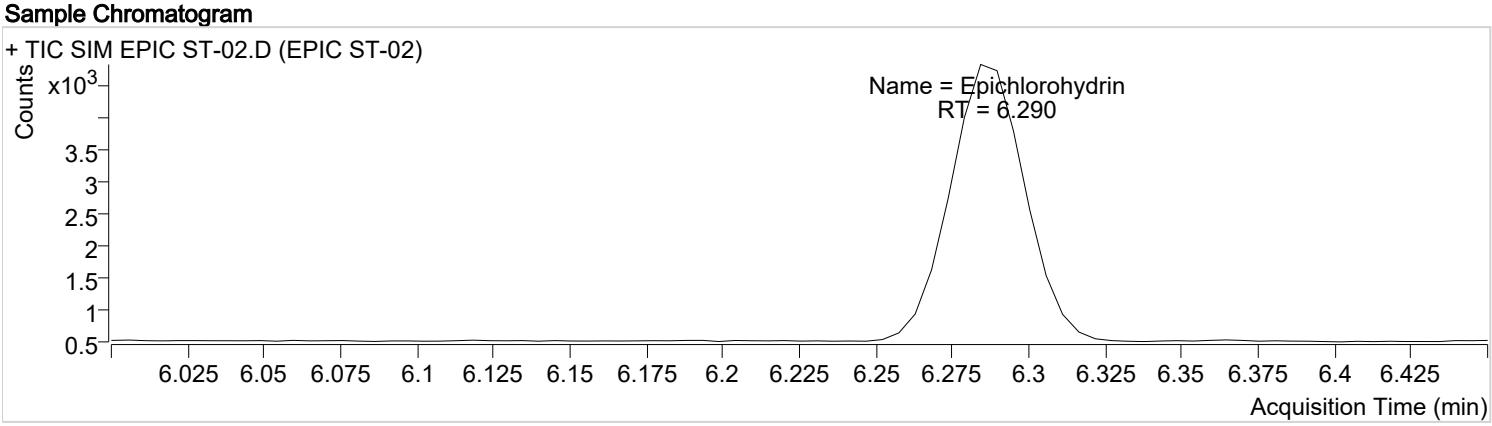

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	5059	0.529	mg/L

Epichlorohydrin

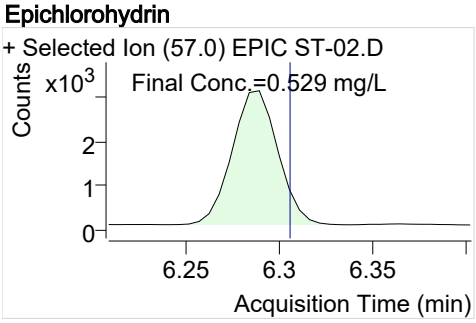





Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-04-01 오후 4:31:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:51:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:31:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-31 오전 11:44:12	**Data File**	EPIC ST-03.D
Type	Cal	**Name**	EPIC ST-03
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

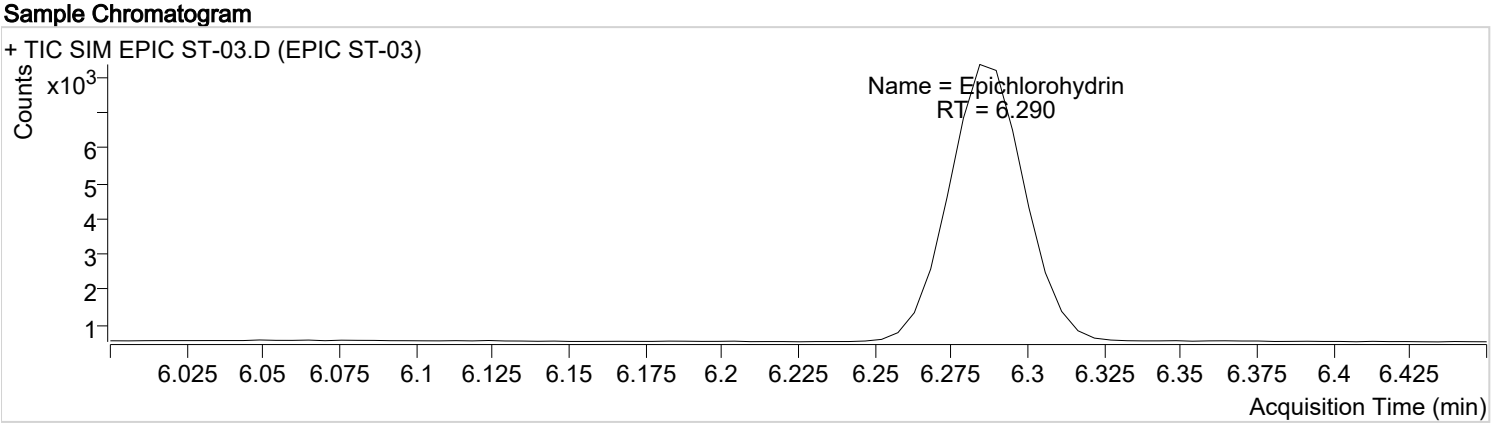

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	9273	0.947	mg/L

Epichlorohydrin

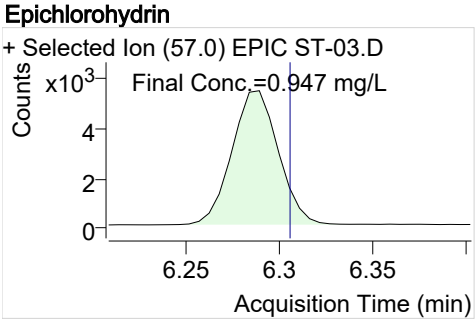

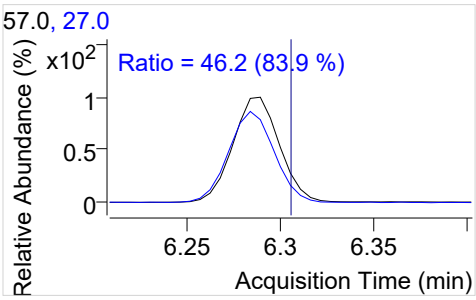



Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-04-01 오후 4:31:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:51:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:31:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-31 오전 11:54:24	**Data File**	EPIC ST-04.D
Type	Cal	**Name**	EPIC ST-04
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

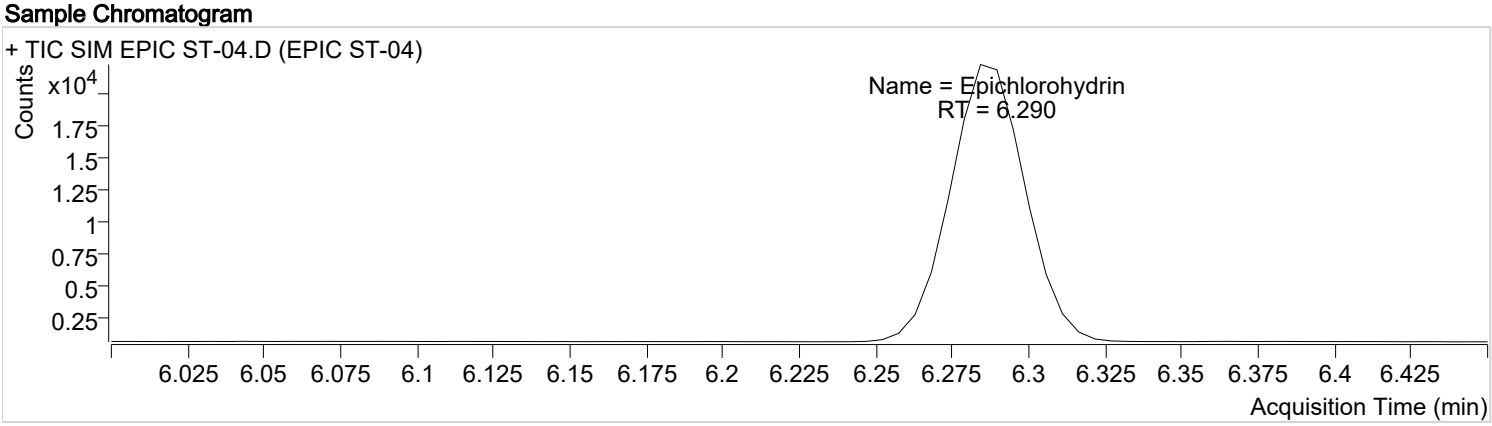

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	25359	2.538	mg/L

Epichlorohydrin

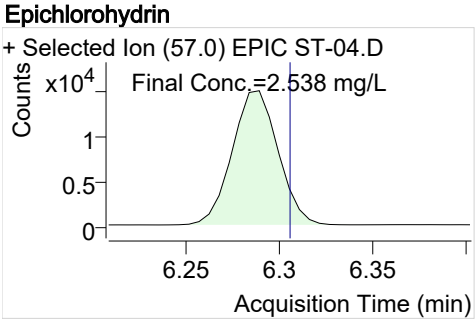



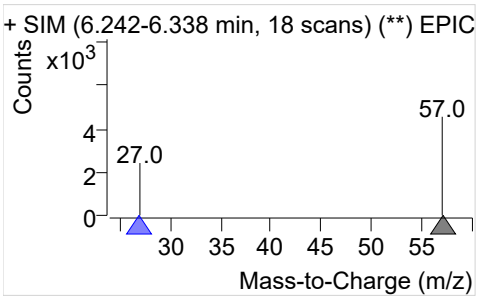

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-04-01 오후 4:31:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:51:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:31:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-31 오후 12:04:41	**Data File**	EPIC ST-05.D
Type	Cal	**Name**	EPIC ST-05
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

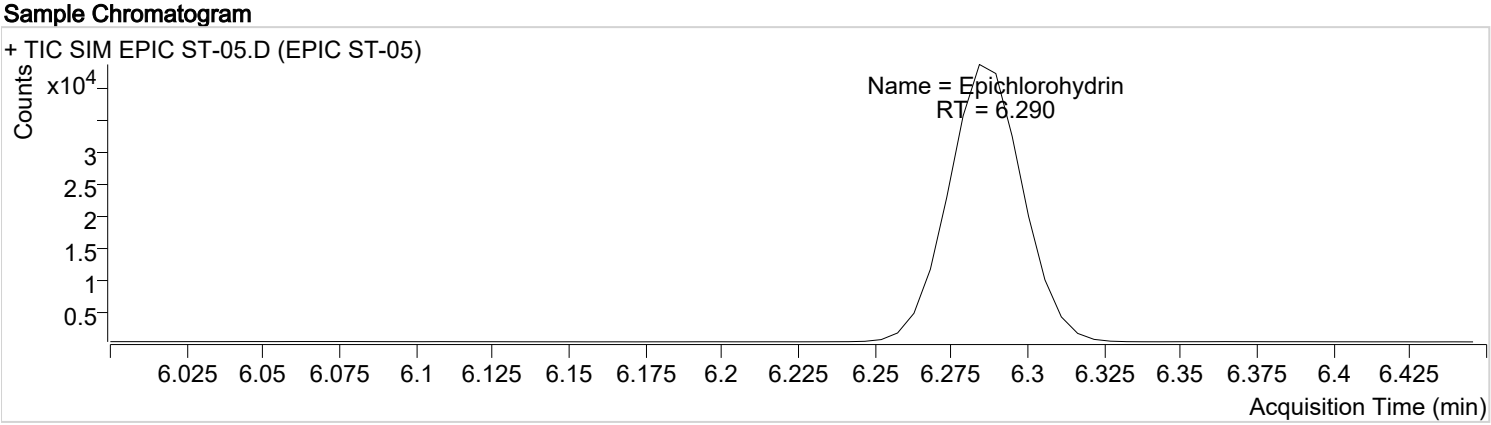

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	50117	4.989	mg/L

Epichlorohydrin

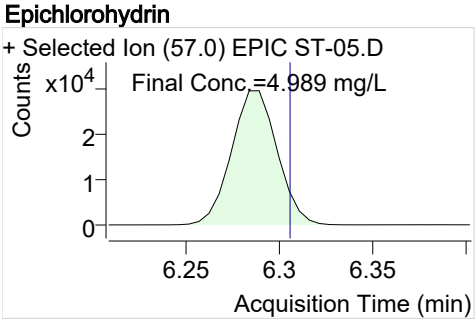





Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-04-01 오후 4:31:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:51:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:31:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-31 오후 12:25:05	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

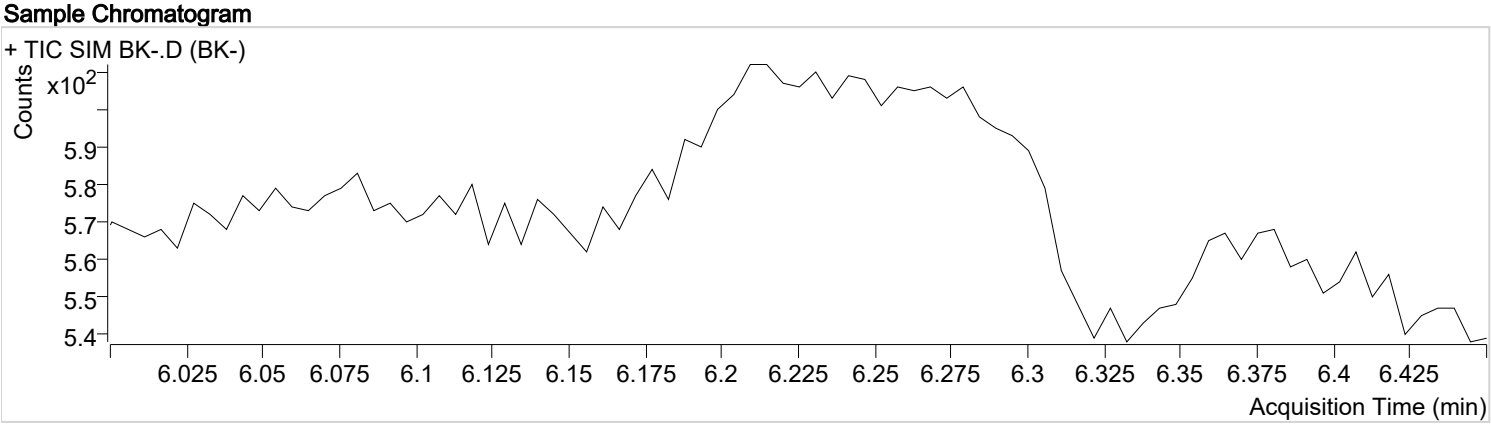

Epichlorohydrin

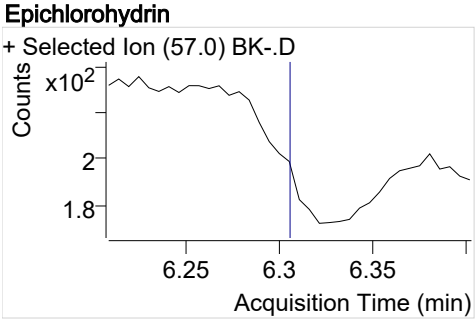

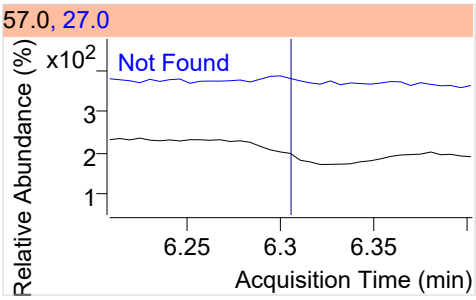

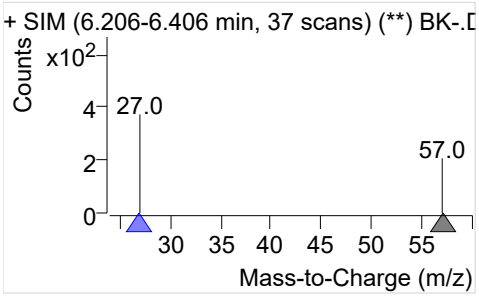

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-04-01 오후 4:31:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:51:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:31:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-31 오후 12:35:22	**Data File**	FBK(LG NJ 26-03-26).D
Type	Blank	**Name**	FBK(LG NJ 26-03-26)
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

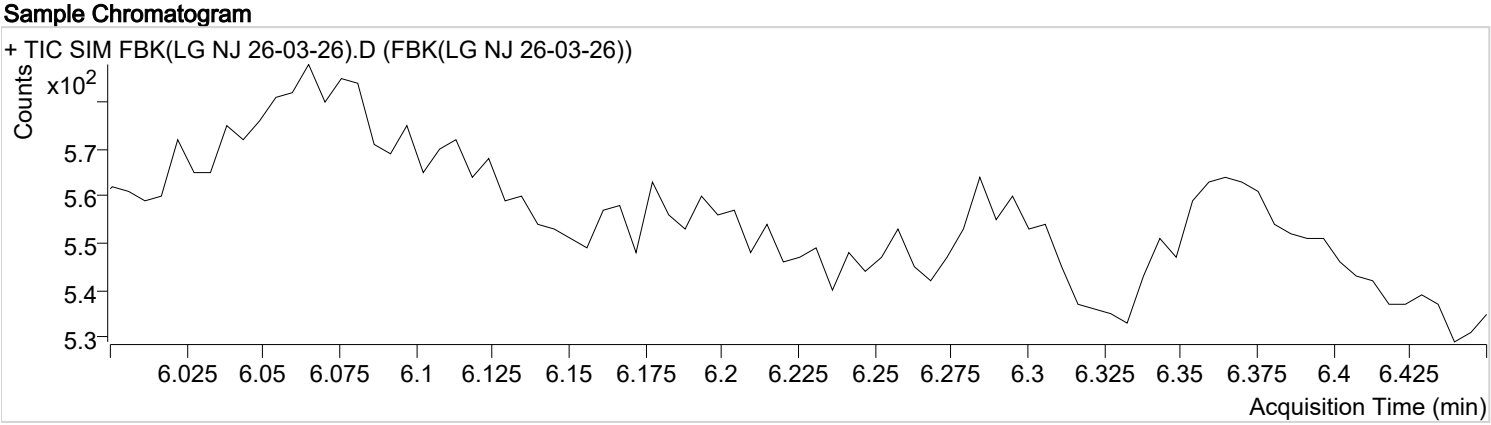

Epichlorohydrin

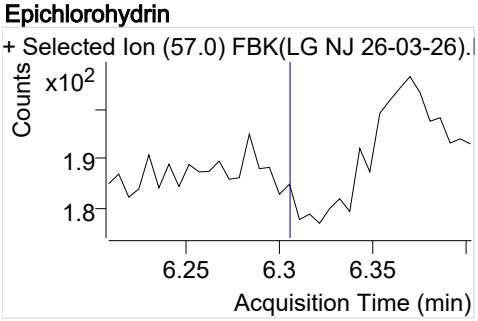

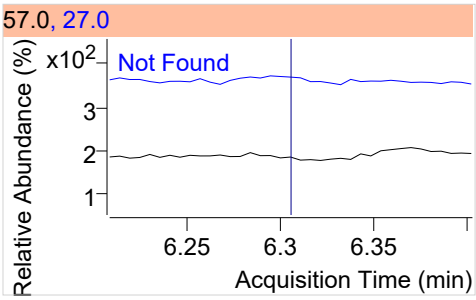

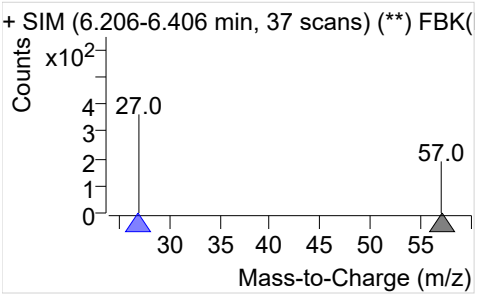

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-04-01 오후 4:31:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:51:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:31:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-31 오후 12:45:34	**Data File**	NJ-01.D
Type	Sample	**Name**	NJ-01
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

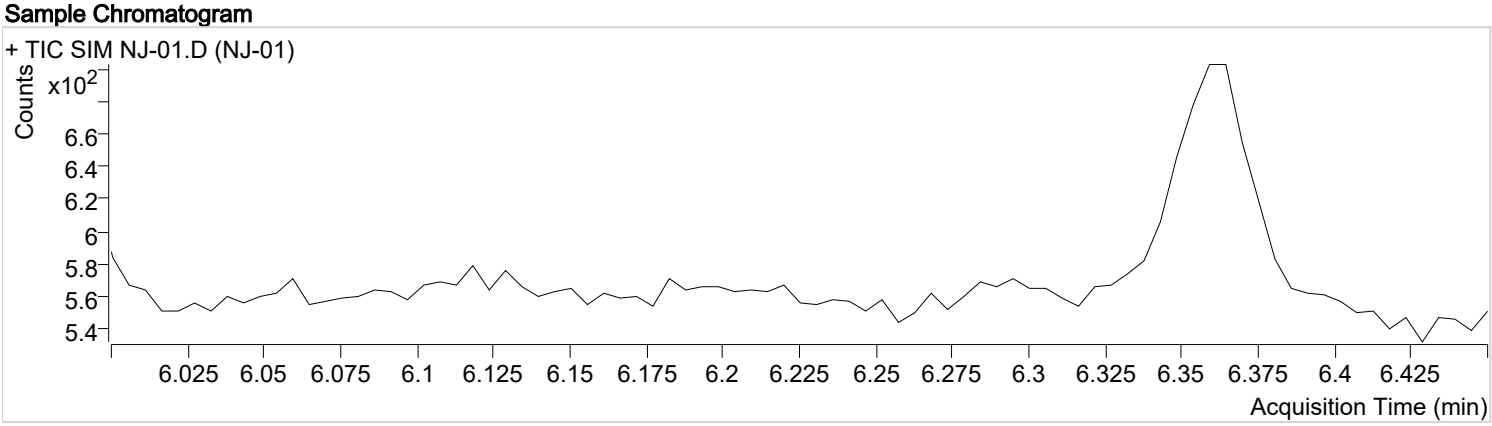

Epichlorohydrin

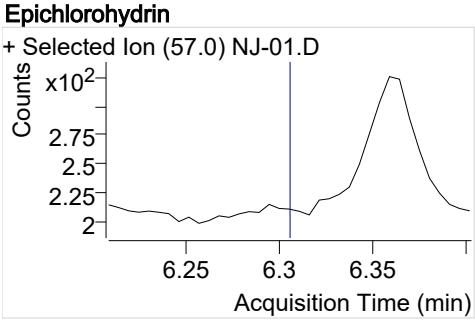

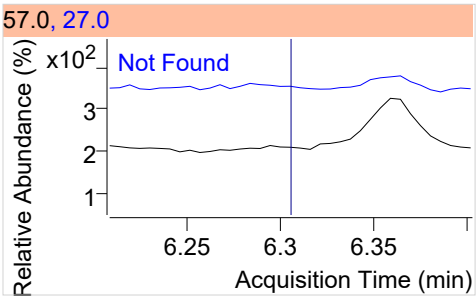

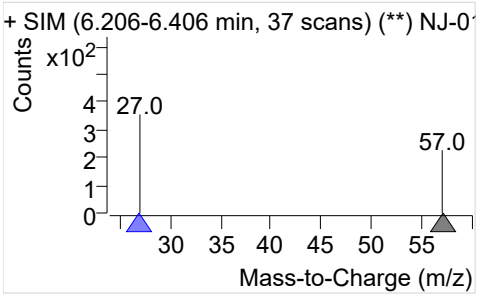

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-04-01 오후 4:31:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:51:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:31:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-31 오후 12:55:46	**Data File**	NJ-02.D
Type	Sample	**Name**	NJ-02
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

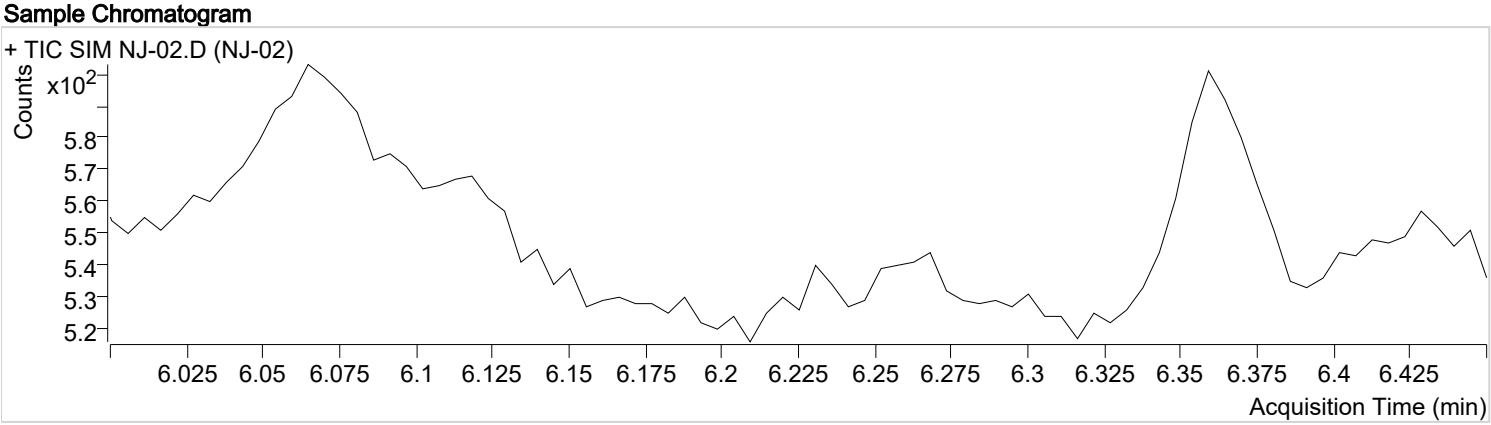

Epichlorohydrin

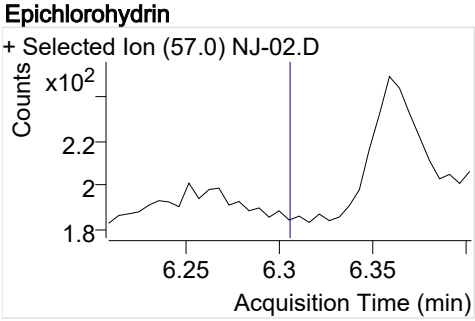

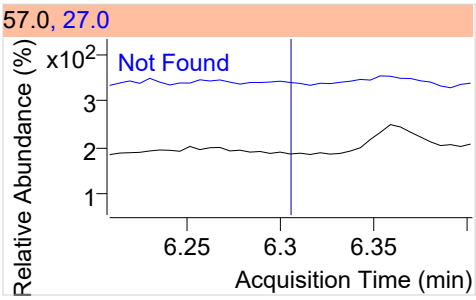

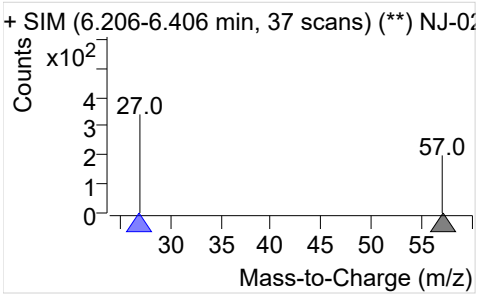

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-04-01 오후 4:31:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:51:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:31:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-31 오후 1:06:01	**Data File**	NJ-03.D
Type	Sample	**Name**	NJ-03
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

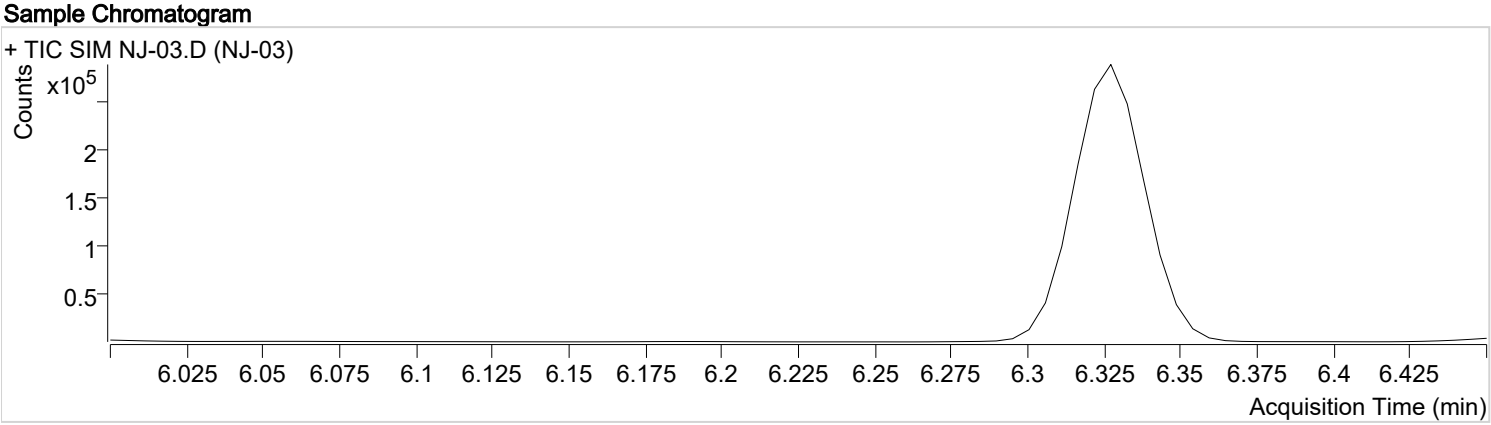

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.327	0	ND	mg/L

Epichlorohydrin

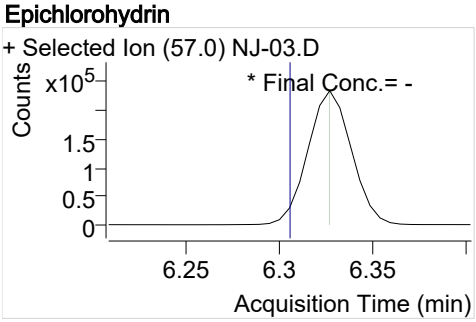





Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-04-01 오후 4:31:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:51:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:31:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-31 오후 1:16:17	**Data File**	NJ-04.D
Type	Sample	**Name**	NJ-04
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

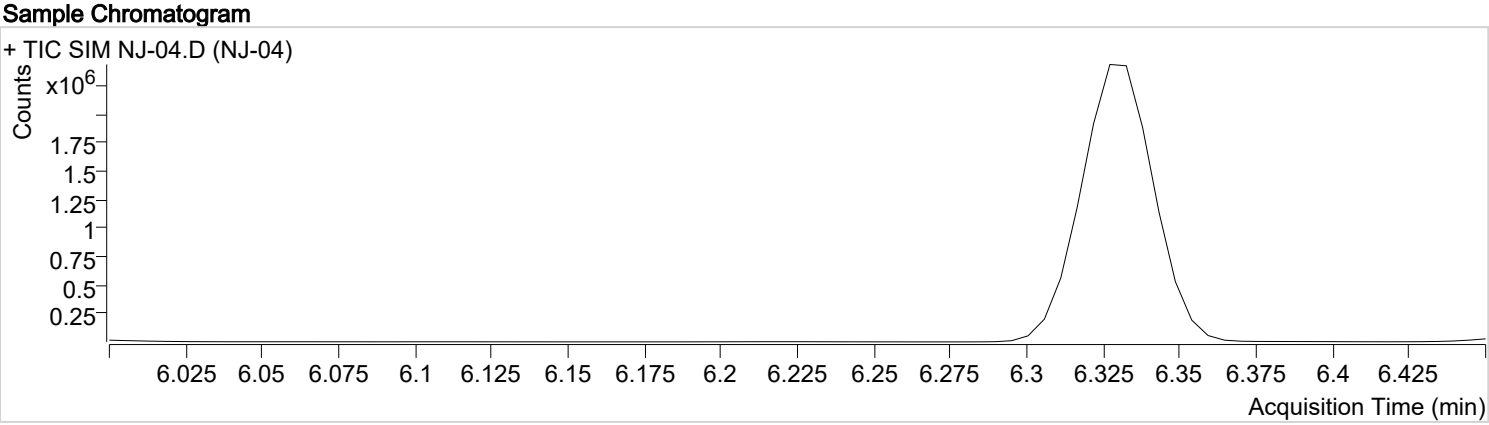

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.333	0	ND	mg/L

Epichlorohydrin

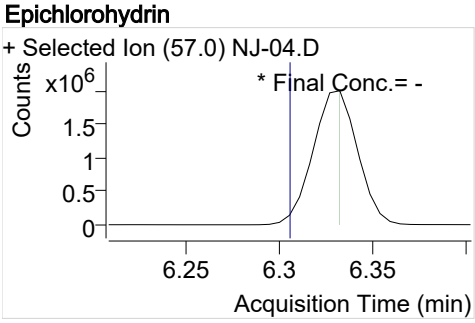

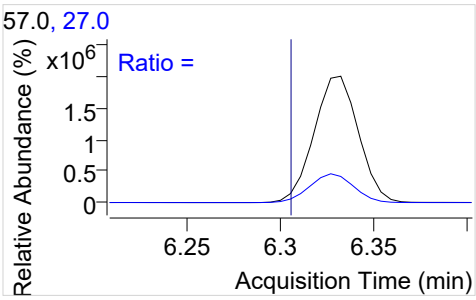



Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-04-01 오후 4:31:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:51:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:31:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-31 오후 1:26:33	**Data File**	NJ-05.D
Type	Sample	**Name**	NJ-05
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

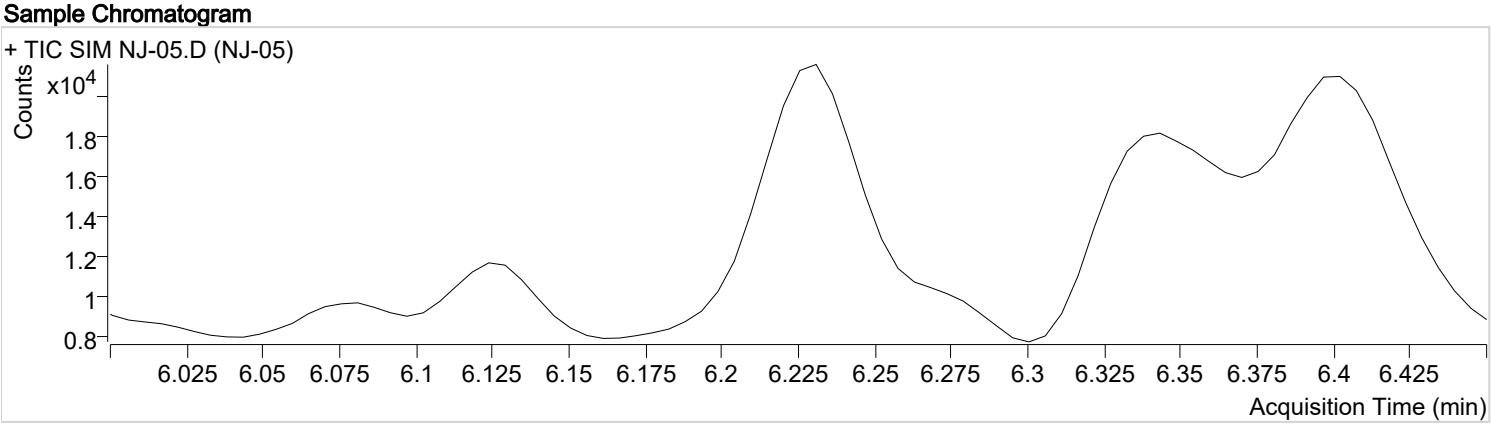

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.343	0	ND	mg/L

Epichlorohydrin

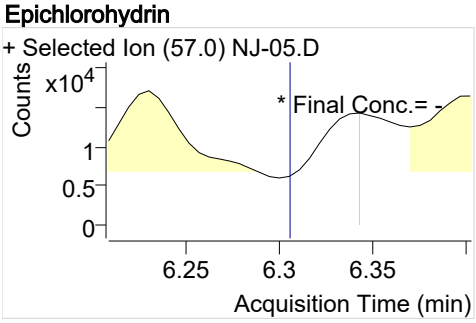



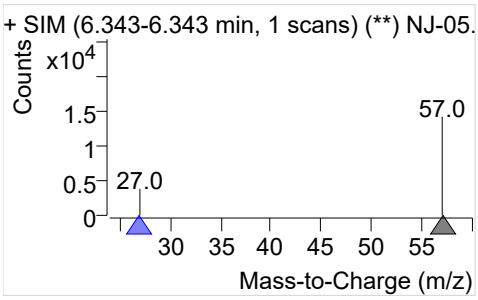

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-04-01 오후 4:31:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:51:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:31:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-31 오후 1:36:45	**Data File**	NJ-06.D
Type	Sample	**Name**	NJ-06
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

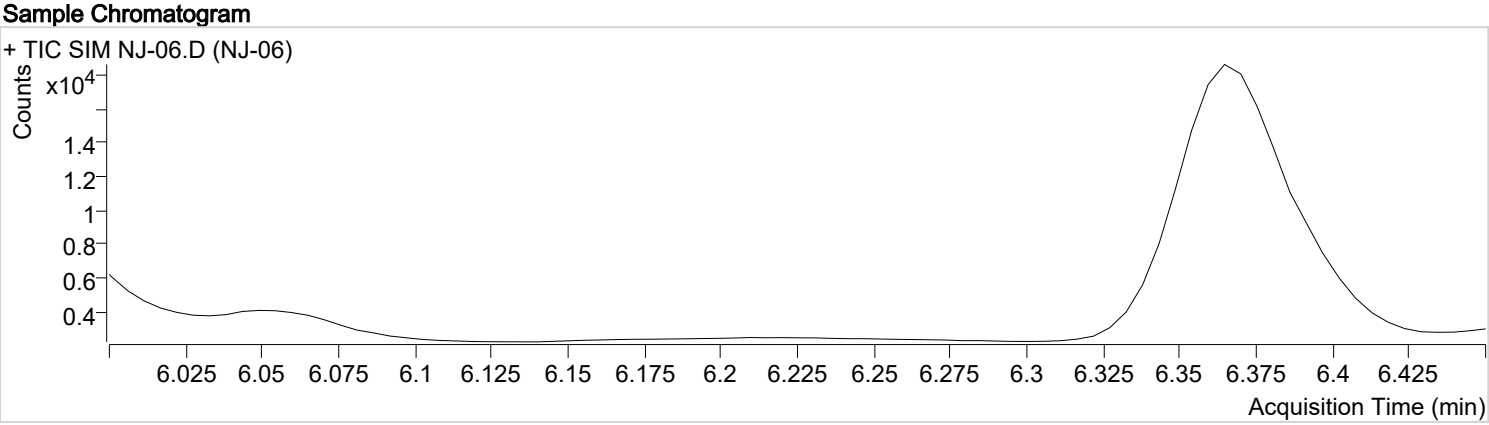

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.365	0	ND	mg/L

Epichlorohydrin

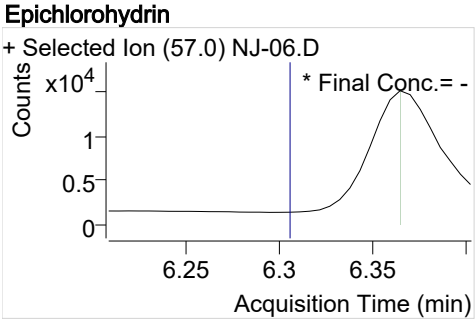

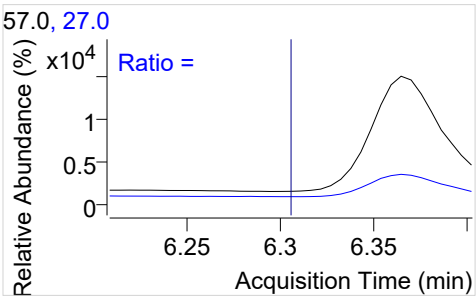

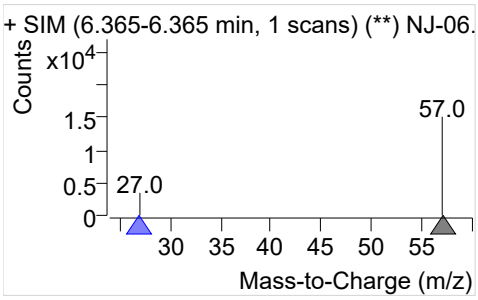

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-04-01 오후 4:31:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:51:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:31:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-31 오후 1:46:59	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

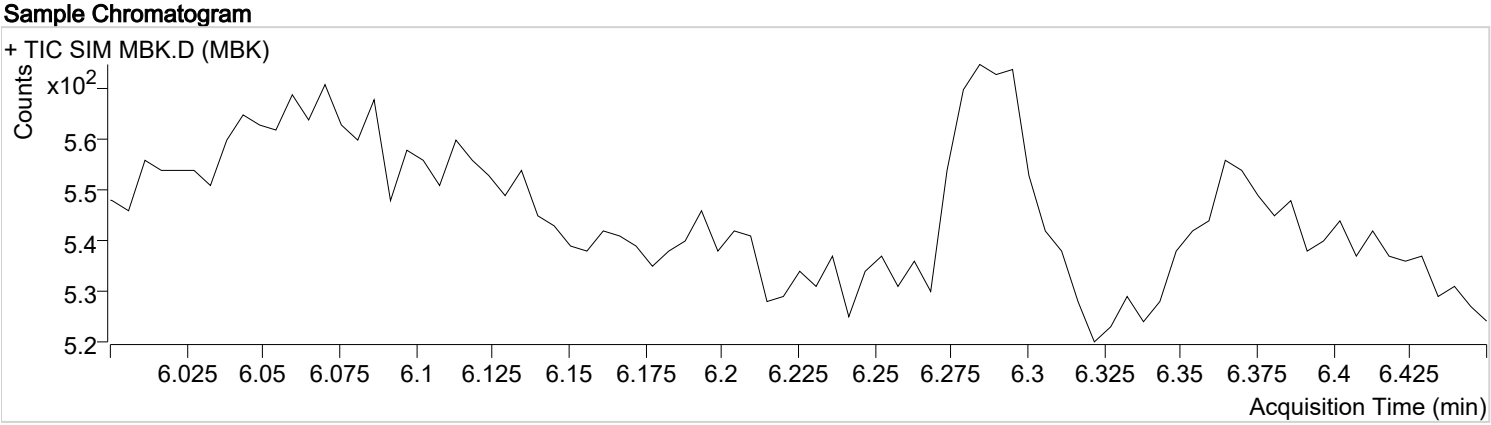

Epichlorohydrin

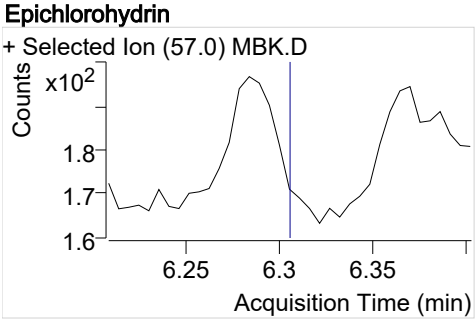

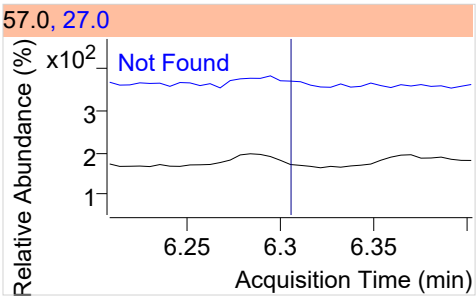

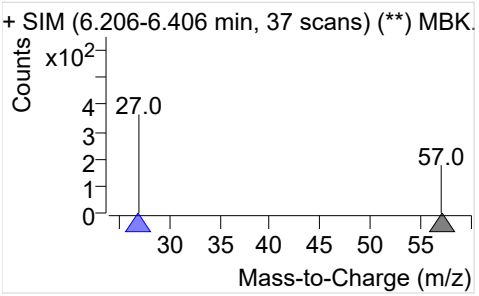

Quant Sample Report

Batch Data Path	D:\DATA\2026년\3. 2026년 3월\EPIC(NJ 3.26)\QuantResults\EPIC.batch.bin		
Analysis Time	2026-04-01 오후 4:31:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 2:51:38	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-04-01 오후 4:31:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2
Acq. Date-Time	2026-03-31 오후 1:57:12	**Data File**	CCV.D
Type	QC	**Name**	CCV
Dil.	1	**Acq. Method File**	VOC(EPIC) NEW

Sample Chromatogram

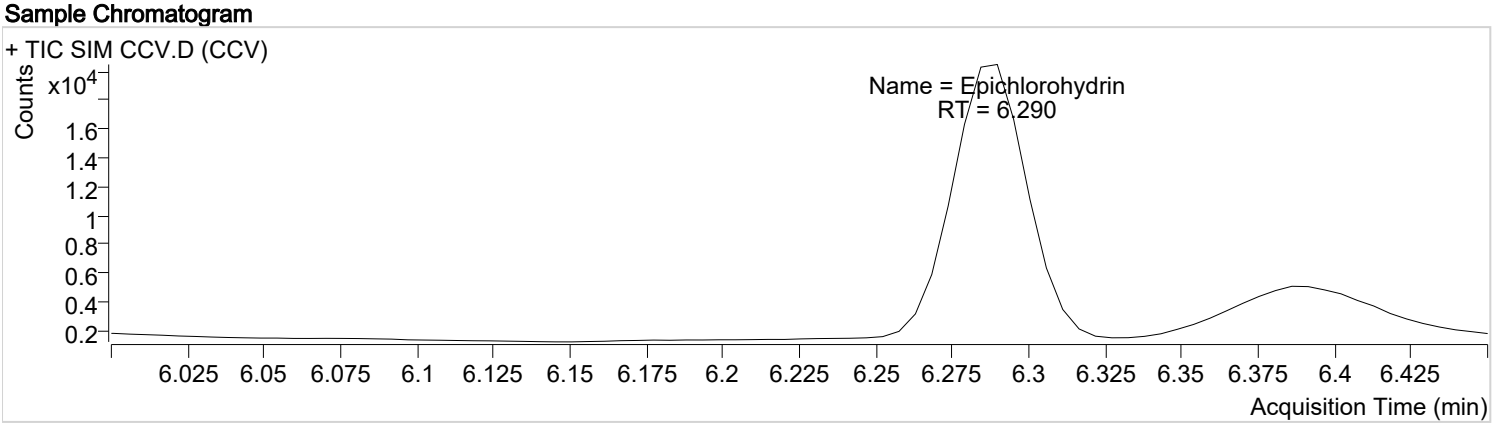

Name	RT	Resp.	Final Conc.	Units
Epichlorohydrin	6.290	22785	2.284	mg/L
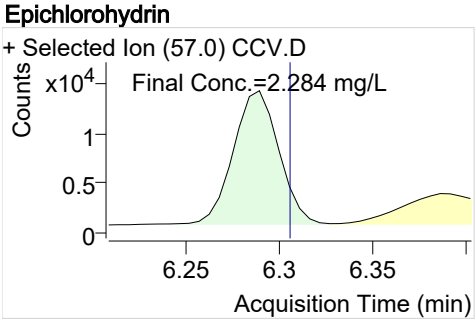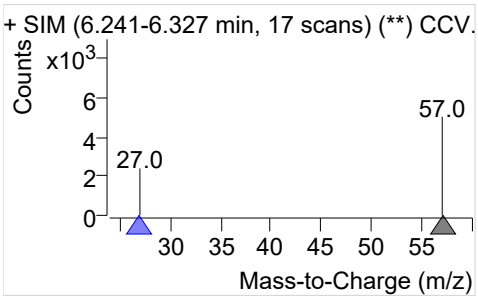
Epichlorohydrin