Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin				
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Phenol

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
PHENOL ST-01.D	Cal	2.080	40148	81329	0.006
PHENOL ST-02.D	Cal	2.080	85009	83004	0.010
PHENOL ST-03.D	Cal	2.080	126124	76727	0.014
PHENOL ST-04.D	Cal	2.075	195560	81016	0.020
PHENOL ST-05.D	Cal	2.080	268075	75361	0.029
PHENOL ST-06.D	Cal	2.075	362106	70179	0.041
BK-.D	Blank			74961	ND
FBK(GS 26-02-10).D	Blank			77143	ND
GS-01.D	Sample			63019	ND
GS-02.D	Sample	2.075	1191247	66946	0.136
GS-03.D	Sample	2.085	0	69754	ND
GS-04.D	Sample	2.085	0	67526	ND
GS-05.D	Sample	2.118	0	60458	ND
GS-06.D	Sample			70908	ND
GS-15.D	Sample			62060	ND
KH 26-02-10.D	Sample	2.118	0	70815	ND
GC-02 R.D	Sample	2.080	129248	80485	0.142
MBK-1.D	Blank			88073	ND
-CCV-.D	QC	2.075	196746	86962	0.019

Phenol

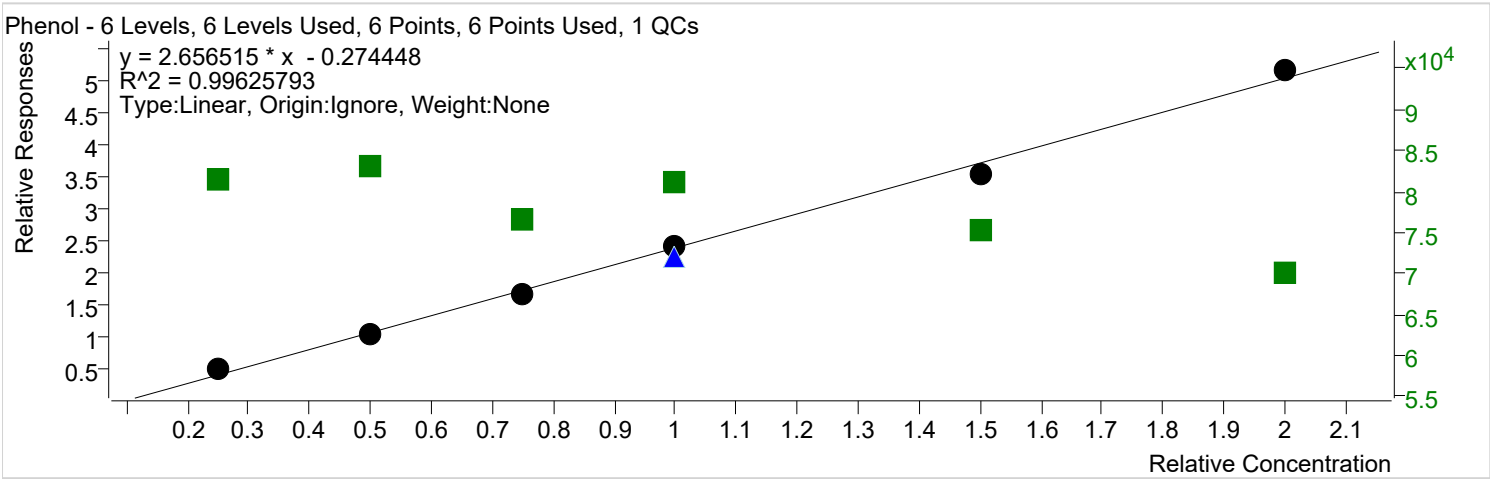

Cal. Path	Type	Level	Enable	Conc.	Response
\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\PHENOL ST-01.D	Calibration	1	x	2.500	40148
\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\PHENOL ST-02.D	Calibration	2	x	5.000	85009
\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\PHENOL ST-03.D	Calibration	3	x	7.500	126124
\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\PHENOL ST-04.D	Calibration	4	x	10.000	195560
\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\-CCV-.D	QC	4	x	10.000	196746
\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\PHENOL ST-05.D	Calibration	5	x	15.000	268075
\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\PHENOL ST-06.D	Calibration	6	x	20.000	362106

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:10:56	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-11 오전 11:53:56	**Data File**	PHENOL ST-01.D
Type	Cal	**Name**	PHENOL ST-01
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

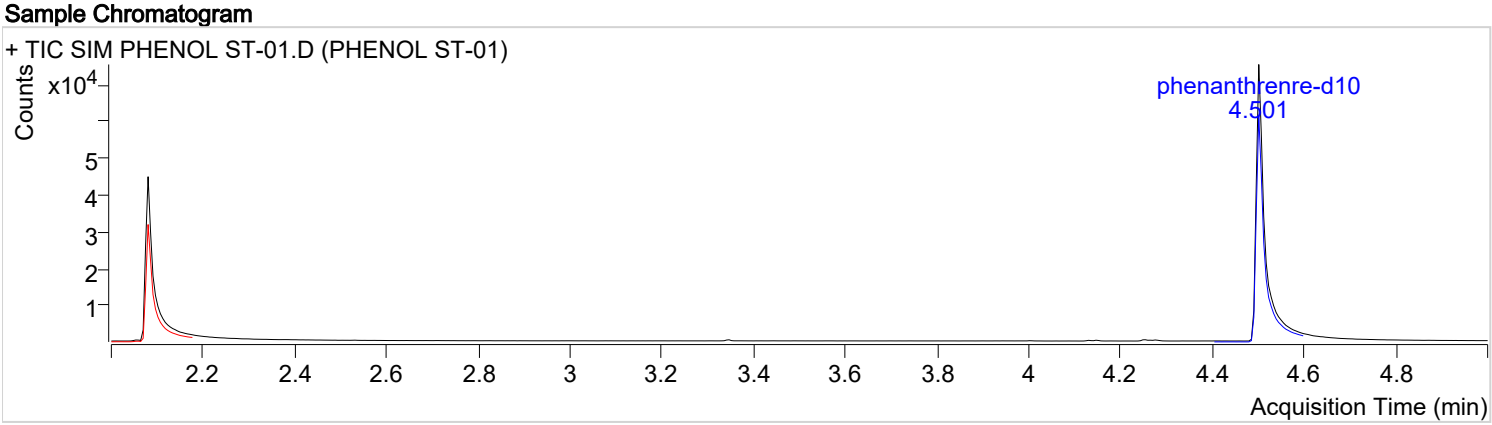

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.080	40148	81329	0.006 mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:10:56	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-11 오후 12:02:13	**Data File**	PHENOL ST-02.D
Type	Cal	**Name**	PHENOL ST-02
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

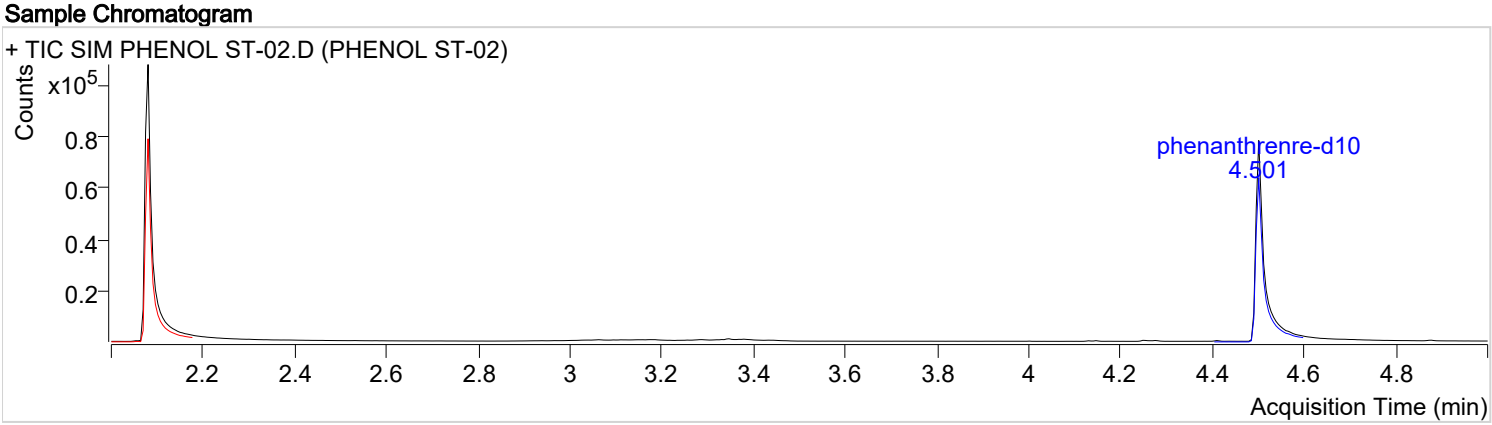

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.080	85009	83004	0.010 mg/L

Phenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:10:56	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-11 오후 12:10:34	**Data File**	PHENOL ST-03.D
Type	Cal	**Name**	PHENOL ST-03
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

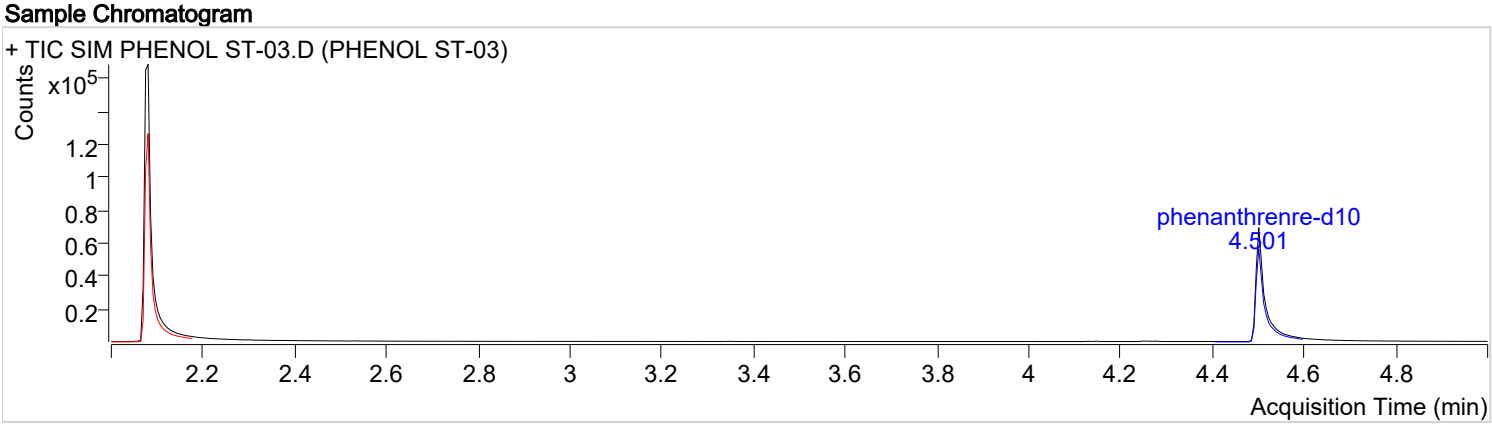

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.080	126124	76727	0.014 mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:10:56	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-11 오후 12:18:56	**Data File**	PHENOL ST-04.D
Type	Cal	**Name**	PHENOL ST-04
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

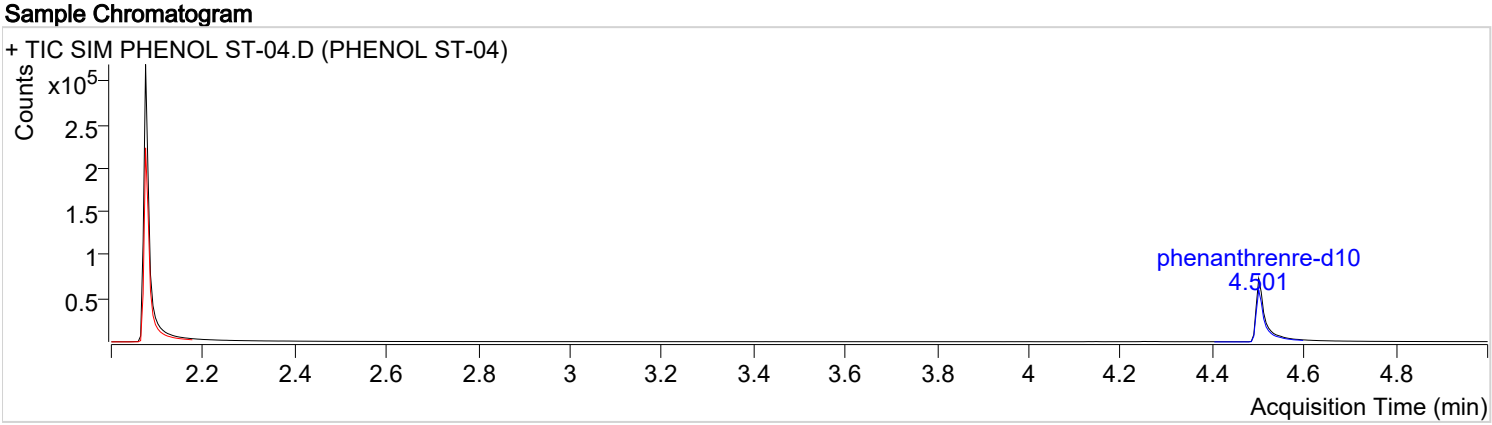

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	195560	81016	0.020 mg/L

Phenol





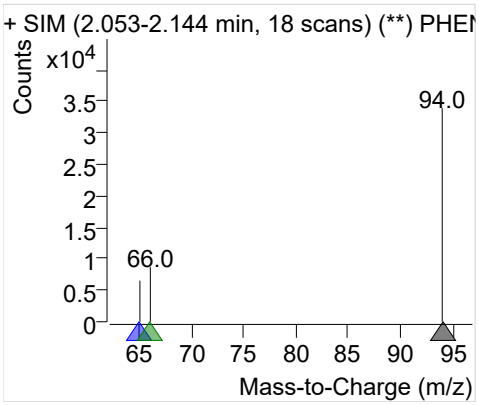

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:10:56	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-11 오후 12:27:17	**Data File**	PHENOL ST-05.D
Type	Cal	**Name**	PHENOL ST-05
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

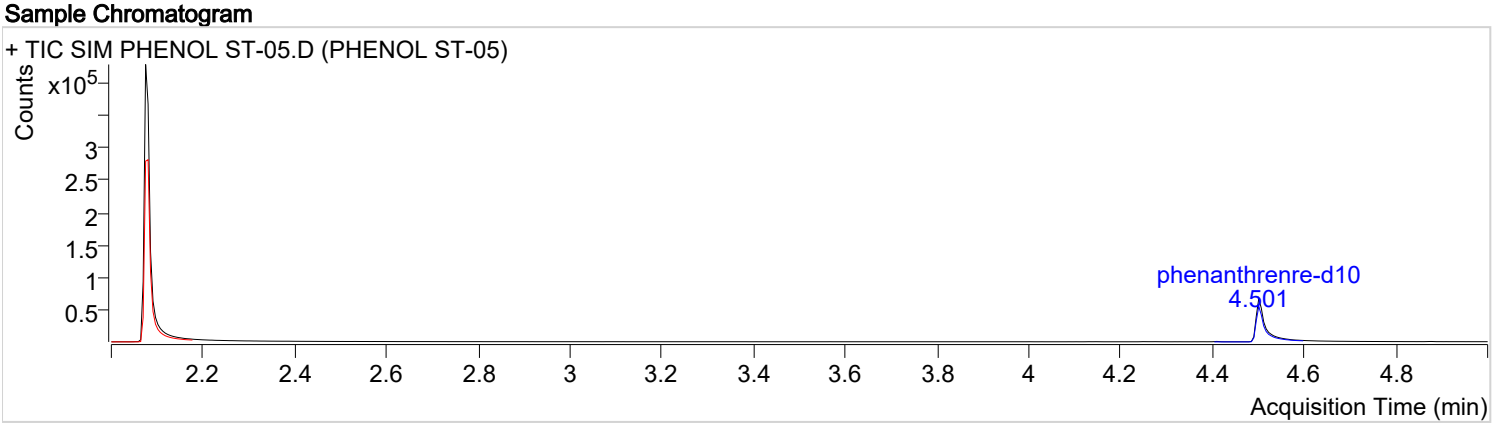

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.080	268075	75361	0.029 mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:10:56	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-11 오후 12:35:40	**Data File**	PHENOL ST-06.D
Type	Cal	**Name**	PHENOL ST-06
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

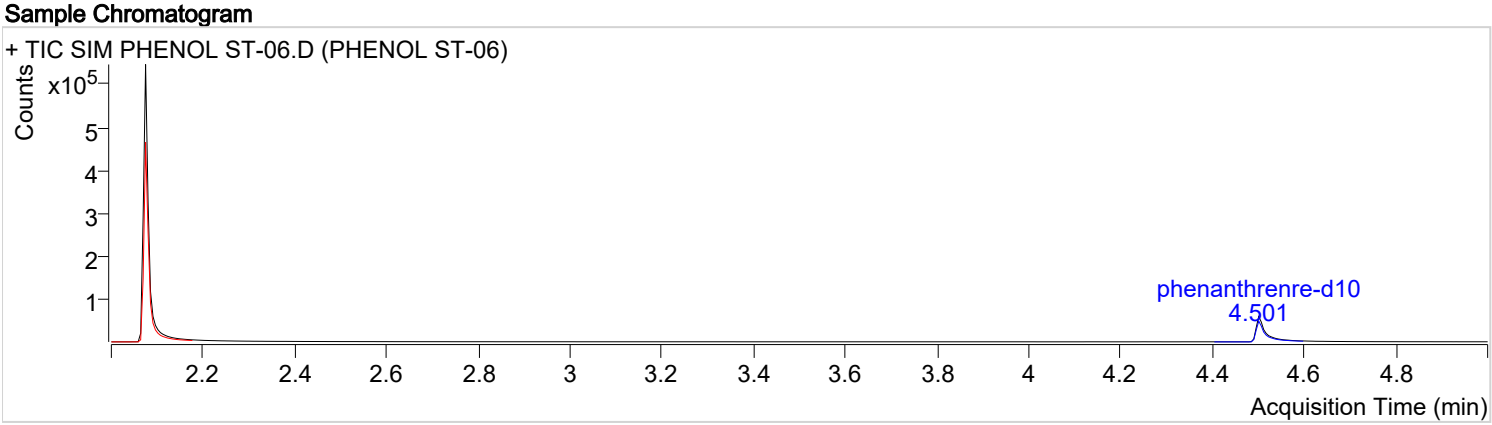

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	362106	70179	0.041 mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:10:56	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-11 오후 12:52:22	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

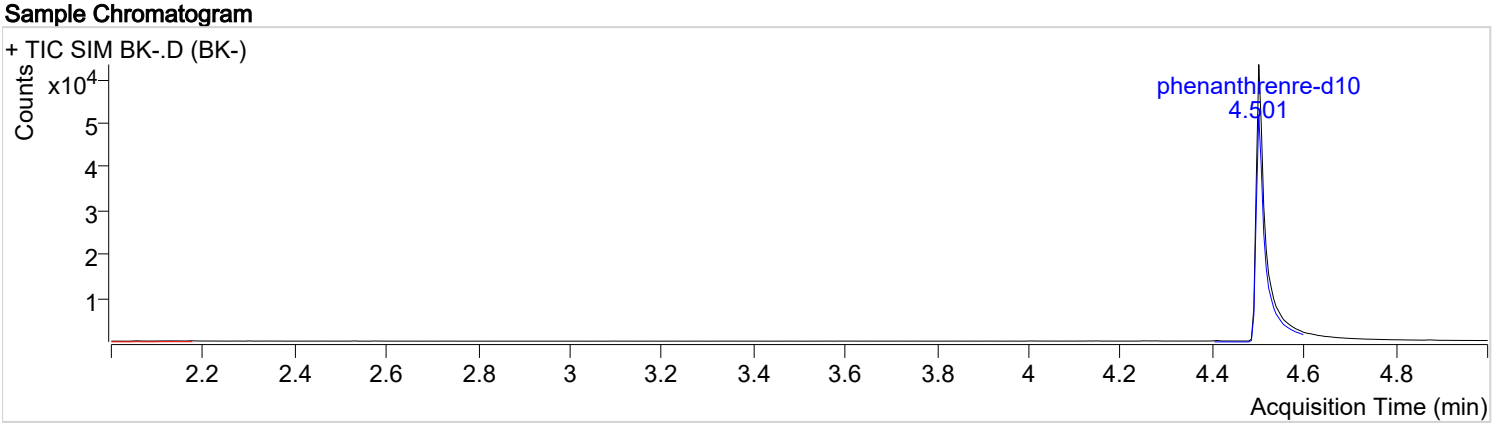

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			74961	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:10:56	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-11 오후 1:00:44	**Data File**	FBK(GS 26-02-10).D
Type	Blank	**Name**	FBK(GS 26-02-10)
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

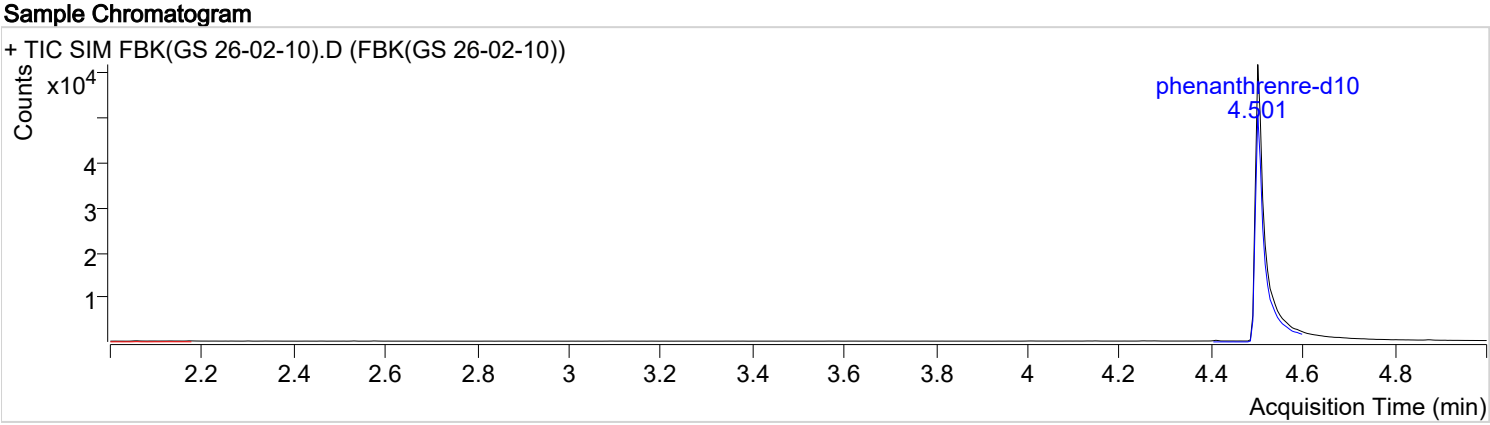

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			77143	ND mg/L

Phenol





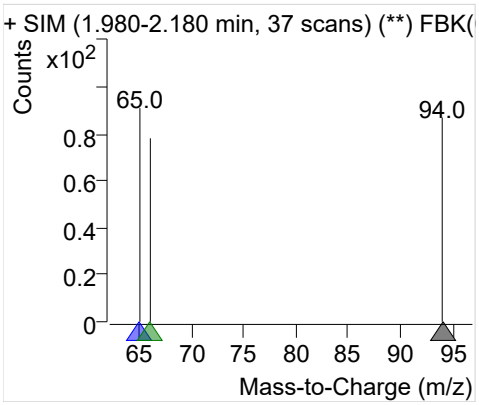

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:10:56	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-11 오후 1:09:07	**Data File**	GS-01.D
Type	Sample	**Name**	GS-01
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

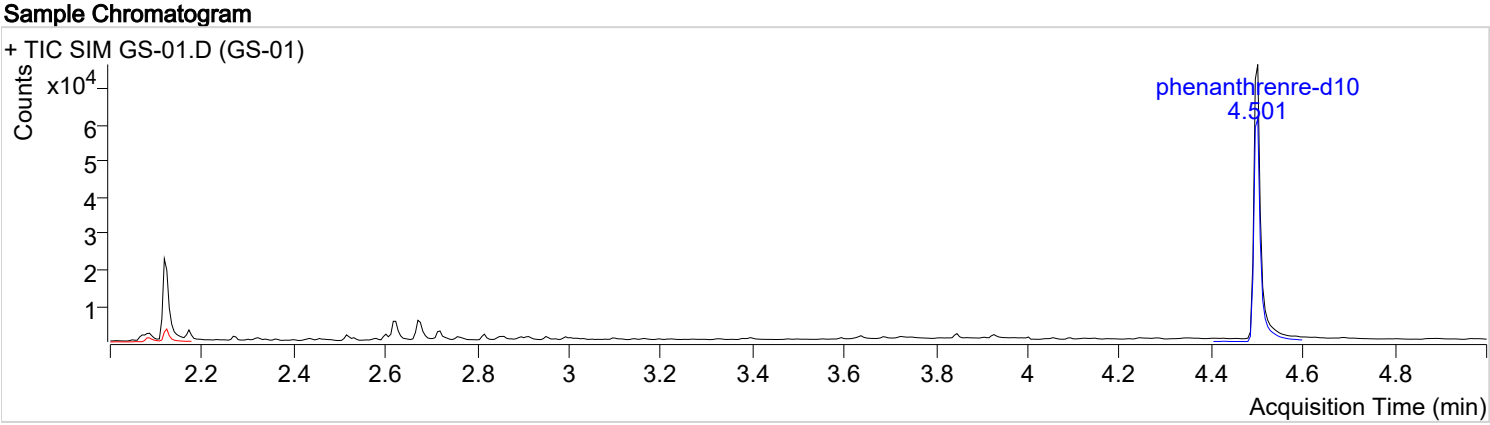

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			63019	ND mg/L

Phenol





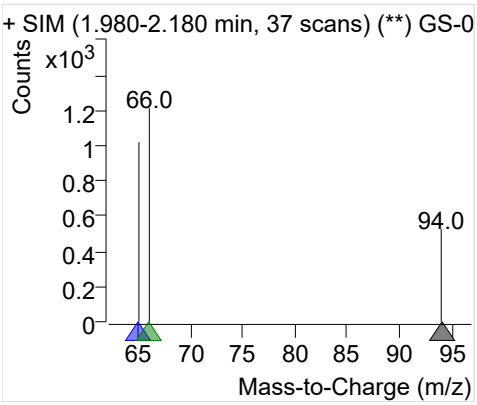

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:10:56	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-11 오후 1:17:30	**Data File**	GS-02.D
Type	Sample	**Name**	GS-02
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

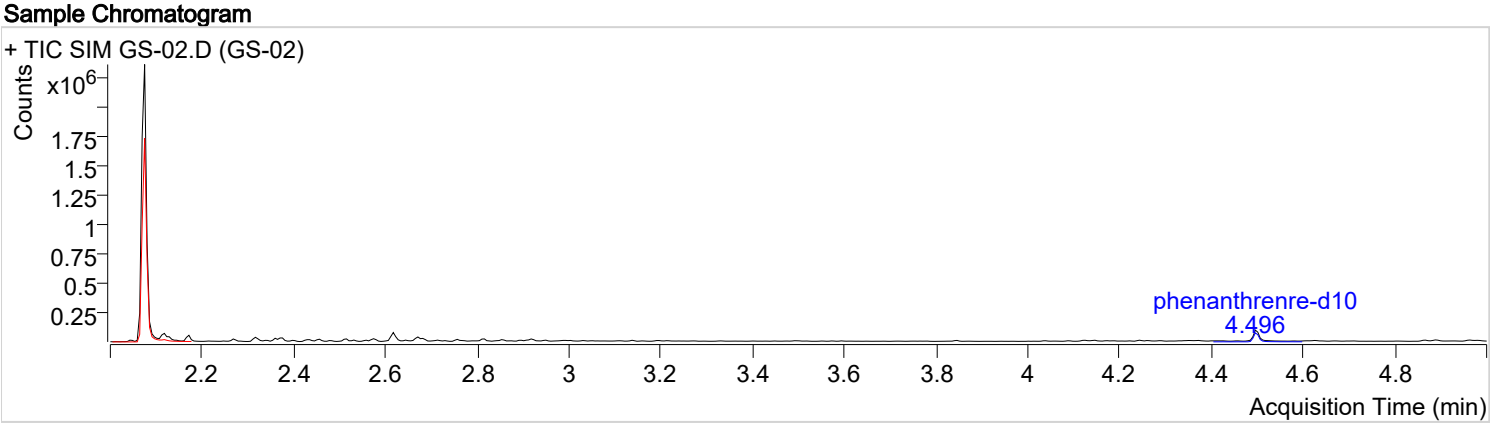

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	1191247	66946	0.136 mg/L

Phenol





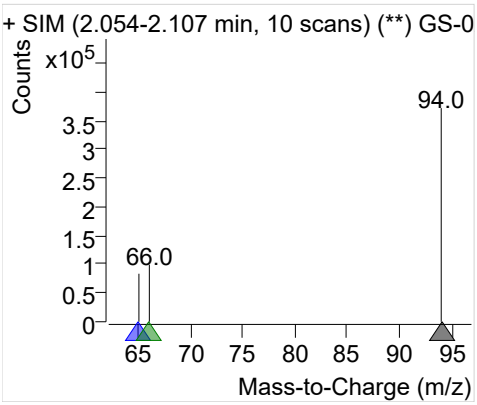

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:10:56	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-11 오후 1:25:54	**Data File**	GS-03.D
Type	Sample	**Name**	GS-03
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

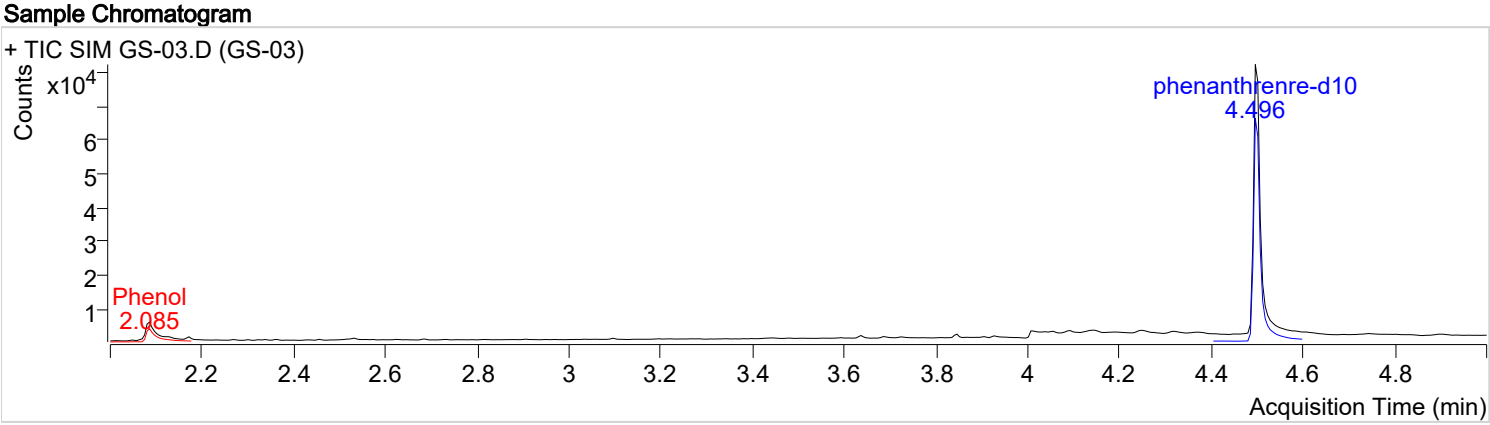

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.085	0	69754	ND mg/L

Phenol





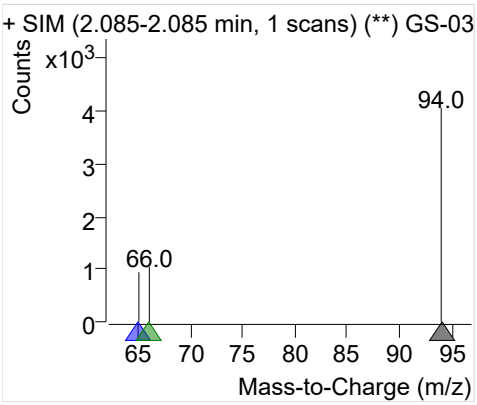

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:10:56	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-11 오후 1:34:17	**Data File**	GS-04.D
Type	Sample	**Name**	GS-04
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

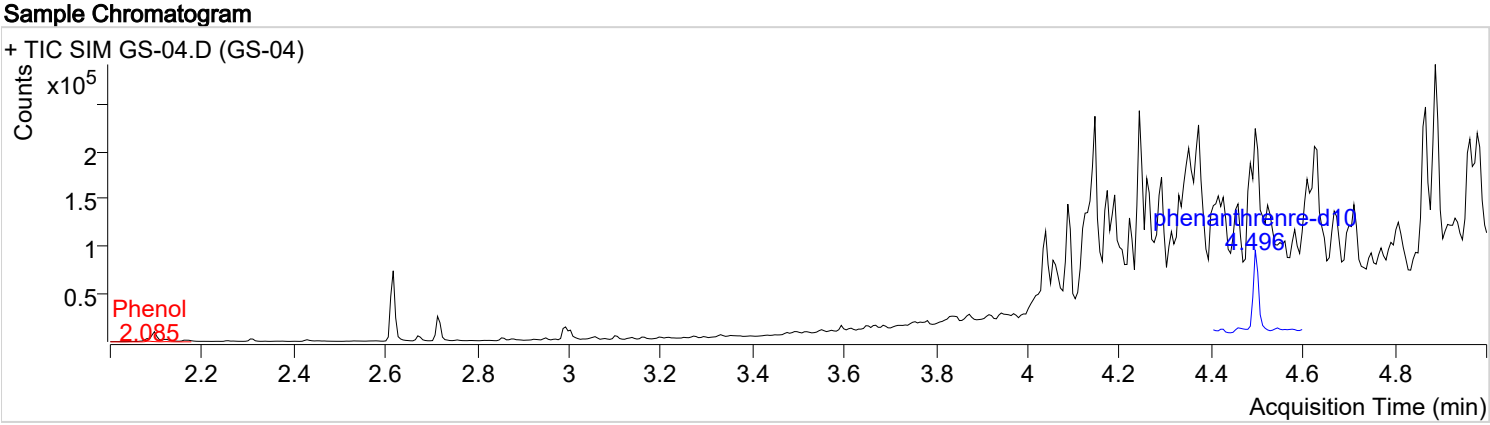

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.085	0	67526	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:10:56	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-11 오후 1:42:38	**Data File**	GS-05.D
Type	Sample	**Name**	GS-05
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

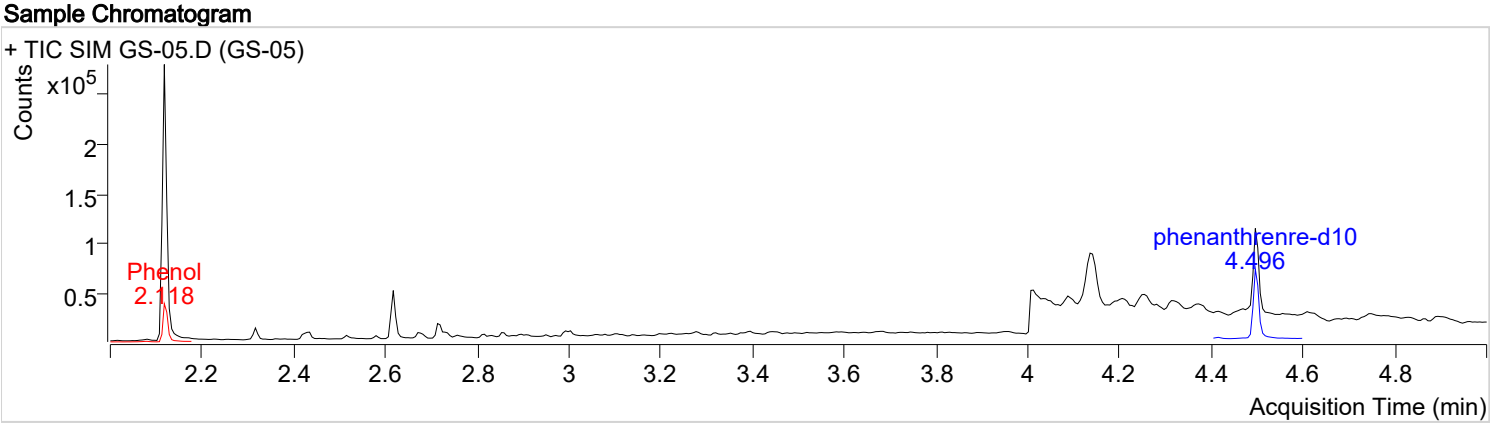

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.118	0	60458	ND mg/L

Phenol





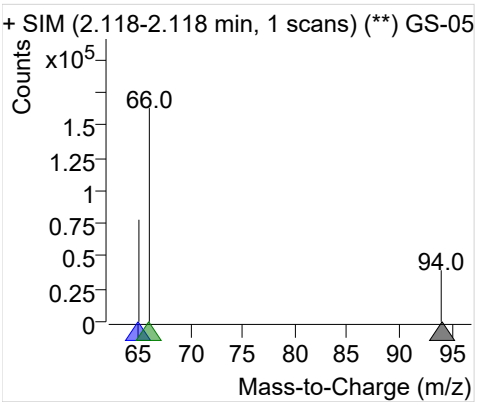

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:10:56	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-11 오후 1:51:00	**Data File**	GS-06.D
Type	Sample	**Name**	GS-06
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

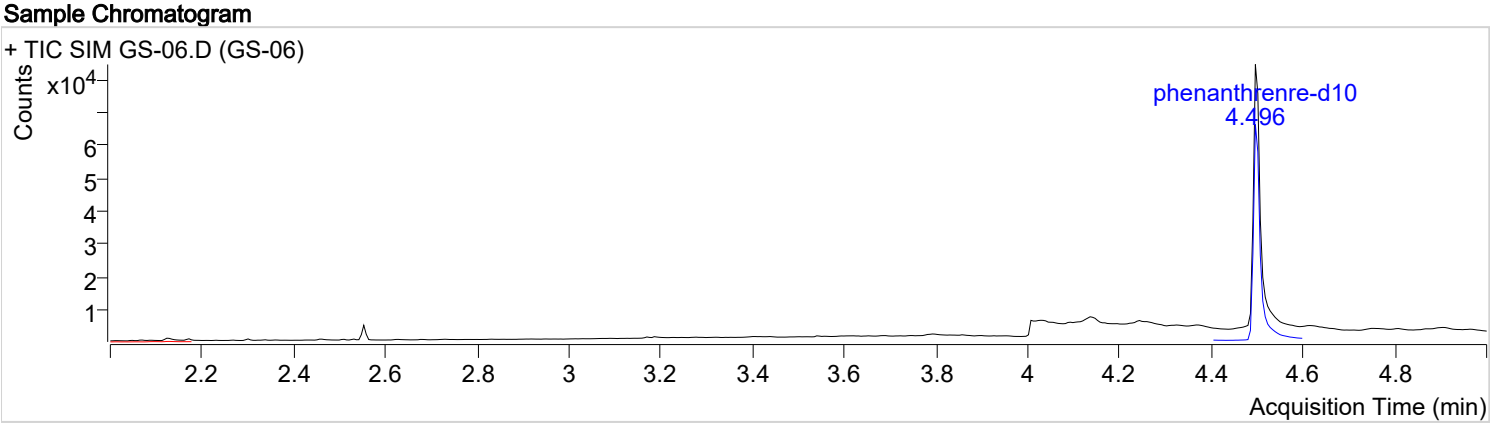

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			70908	ND mg/L

Phenol





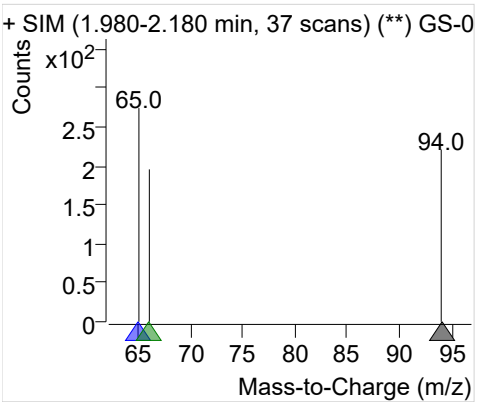

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:10:56	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-11 오후 1:59:23	**Data File**	GS-15.D
Type	Sample	**Name**	GS-15
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

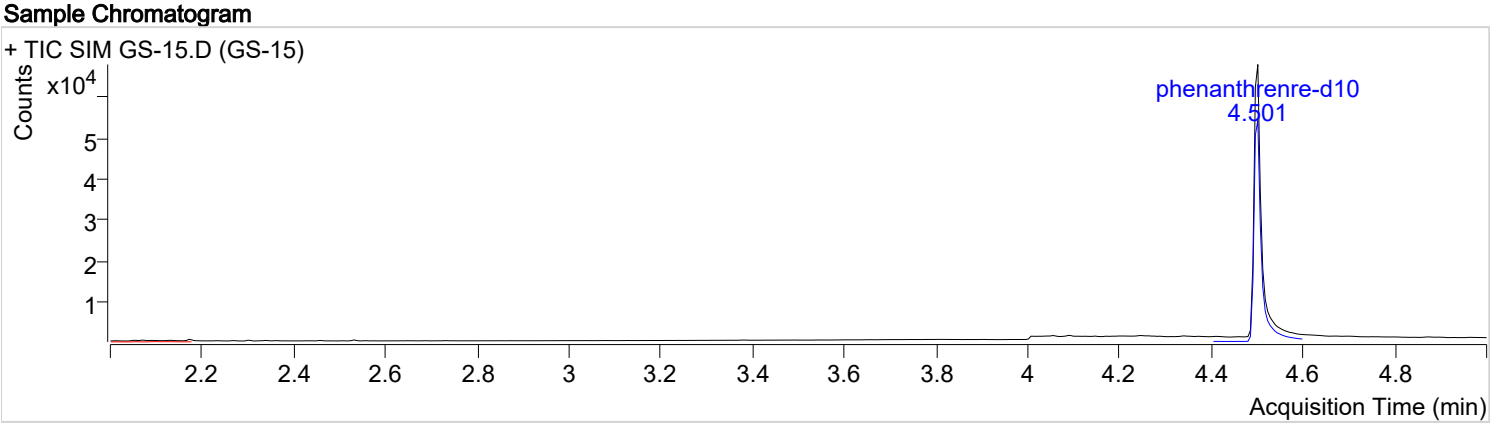

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			62060	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:10:56	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-11 오후 2:07:45	**Data File**	KH 26-02-10.D
Type	Sample	**Name**	KH 26-02-10
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

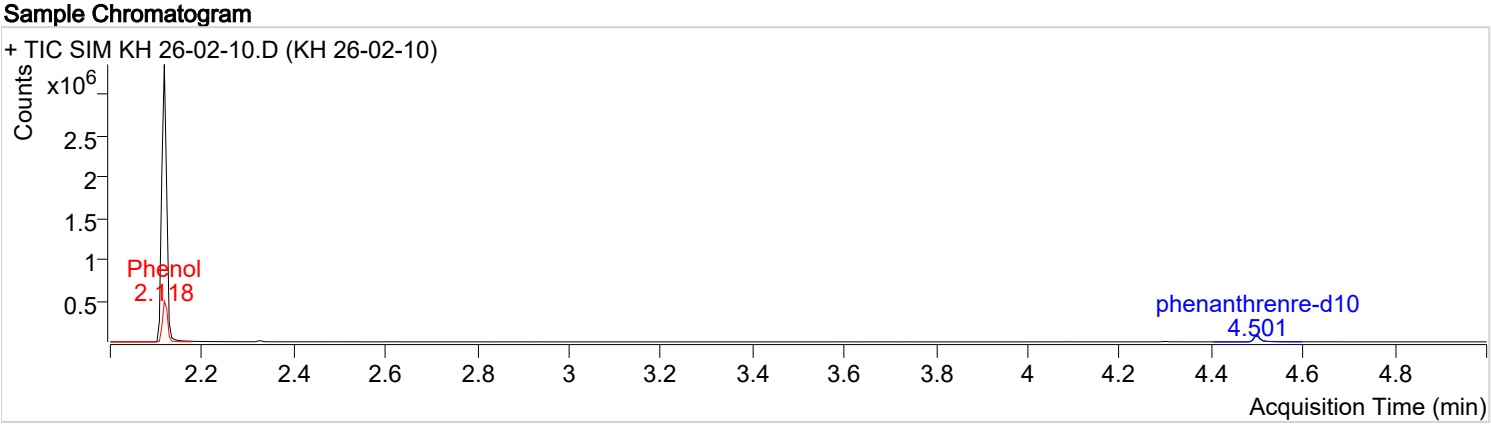

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.118	0	70815	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:10:56	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-11 오후 2:24:32	**Data File**	GC-02 R.D
Type	Sample	**Name**	GC-02 R
Dil.	0.02	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

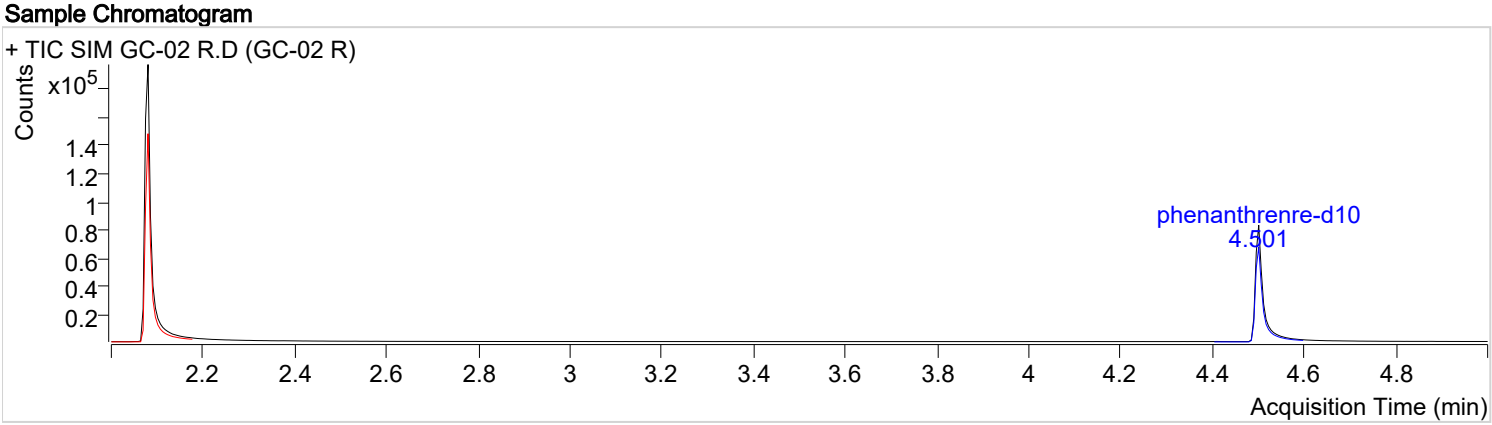

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.080	129248	80485	0.142 mg/L

Phenol



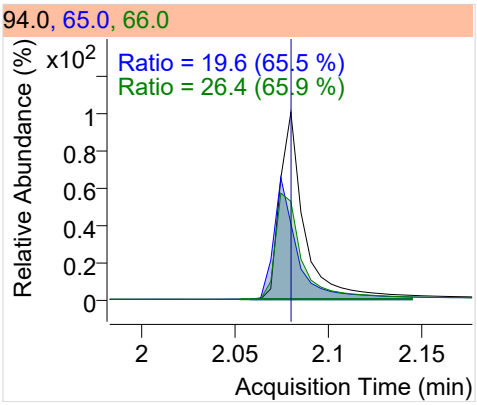

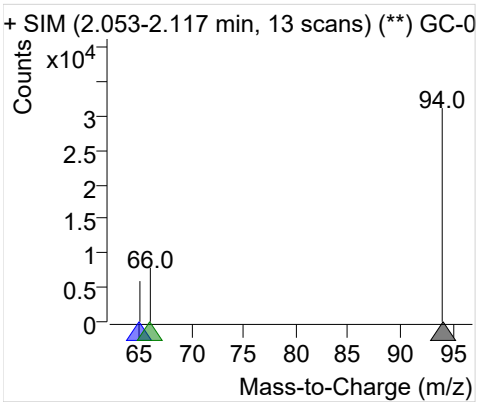

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:10:56	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-11 오후 2:32:54	**Data File**	MBK-1.D
Type	Blank	**Name**	MBK-1
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

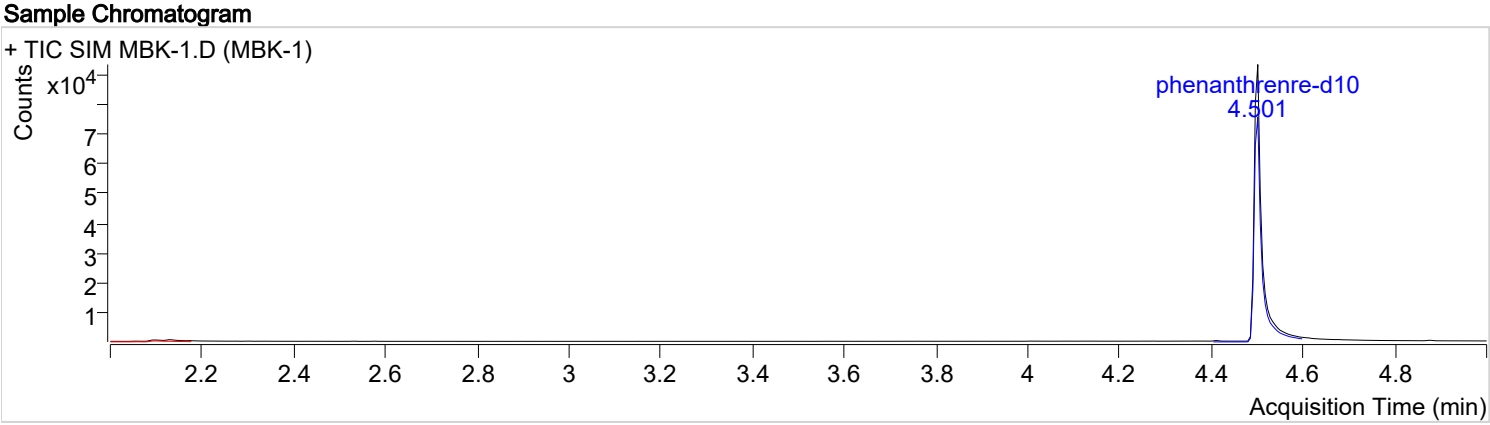

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			88073	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(GS 2.10, KH 2.10)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-11 오후 3:00:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:10:56	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-11 오후 3:00:54	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-11 오후 2:41:19	**Data File**	-CCV-.D
Type	QC	**Name**	-CCV-
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

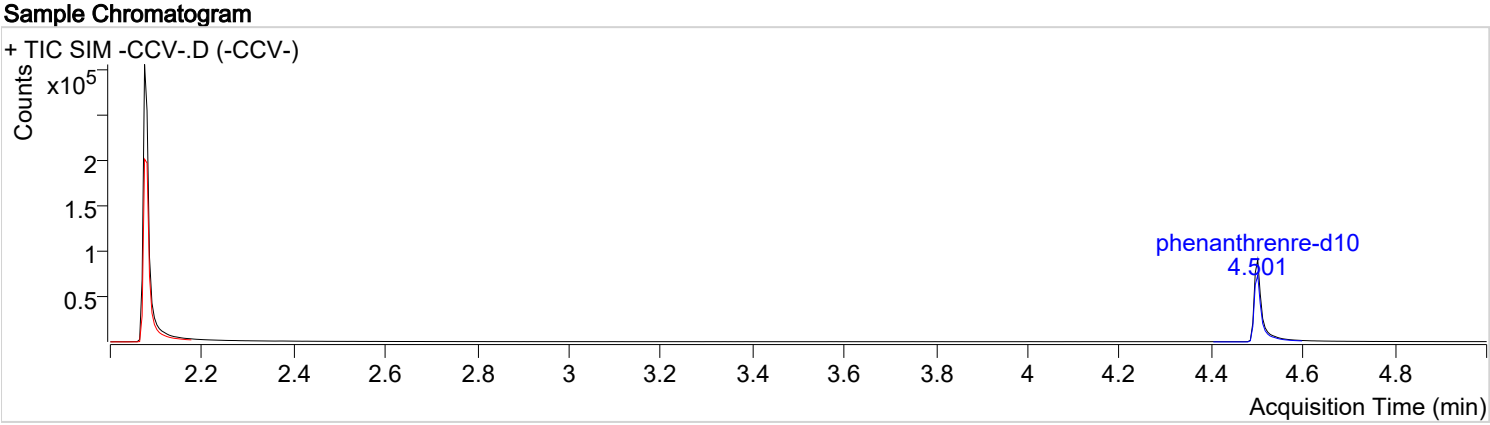

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	196746	86962	0.019 mg/L

Phenol