Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(JR 2.20)\QuantResults\PHENOL.batch.bin				
Analysis Time	2026-02-24 오전 8:47:32	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:47:32	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Phenol

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
PHENOL ST-01.D	Cal	2.075	46875	71569	0.005
PHENOL ST-02.D	Cal	2.075	99182	74073	0.010
PHENOL ST-03.D	Cal	2.075	160691	75698	0.015
PHENOL ST-04.D	Cal	2.075	209631	77672	0.019
PHENOL ST-05.D	Cal	2.075	293347	66303	0.031
PHENOL ST-06.D	Cal	2.075	385624	66938	0.040
BK-.D	Blank			75204	ND
JR 26-02-20.D	Sample			72487	ND
MBK.D	Blank			72725	ND
-CCV-.D	QC	2.075	211193	73279	0.020

Phenol

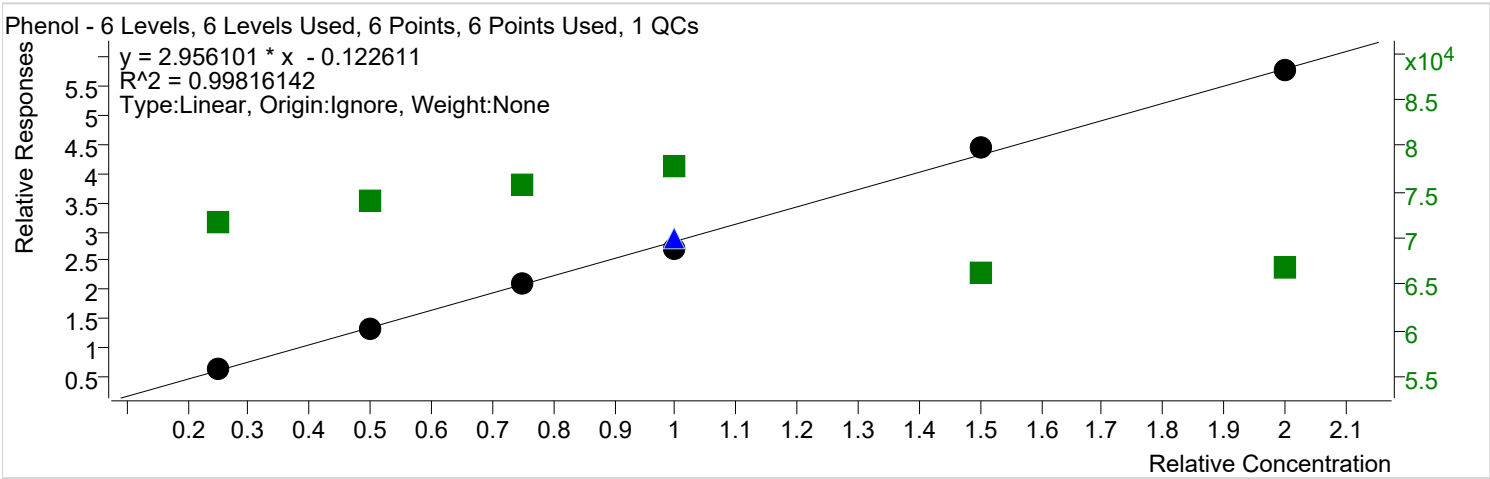

Cal. Path	Type	Level	Enable	Conc.	Response
\\192.168.254.121\data\2026\2. 2026-02\PHENOL(JR 2.20)\PHENOL ST-01.D	Calibration	1	x	2.500	46875
\\192.168.254.121\data\2026\2. 2026-02\PHENOL(JR 2.20)\PHENOL ST-02.D	Calibration	2	x	5.000	99182
\\192.168.254.121\data\2026\2. 2026-02\PHENOL(JR 2.20)\PHENOL ST-03.D	Calibration	3	x	7.500	160691
\\192.168.254.121\data\2026\2. 2026-02\PHENOL(JR 2.20)\PHENOL ST-04.D	Calibration	4	x	10.000	209631
\\192.168.254.121\data\2026\2. 2026-02\PHENOL(JR 2.20)\-CCV-.D	QC	4	x	10.000	211193
\\192.168.254.121\data\2026\2. 2026-02\PHENOL(JR 2.20)\PHENOL ST-05.D	Calibration	5	x	15.000	293347
\\192.168.254.121\data\2026\2. 2026-02\PHENOL(JR 2.20)\PHENOL ST-06.D	Calibration	6	x	20.000	385624

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(JR 2.20)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-24 오전 8:47:32	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:12:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:47:32	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 3:58:31	**Data File**	PHENOL ST-01.D
Type	Cal	**Name**	PHENOL ST-01
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

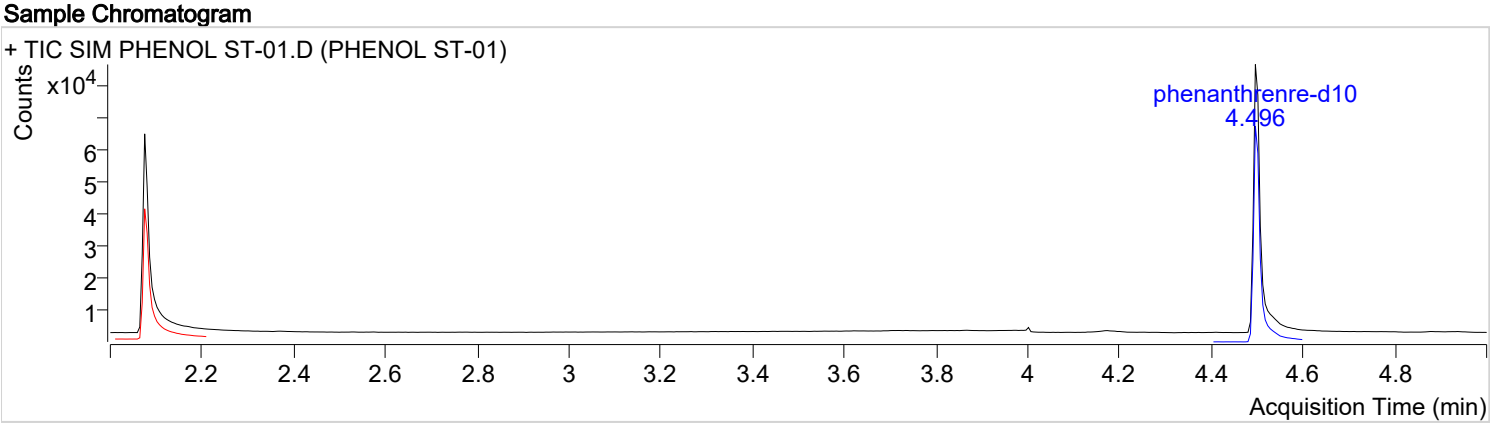

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	46875	71569	0.005 mg/L

Phenol

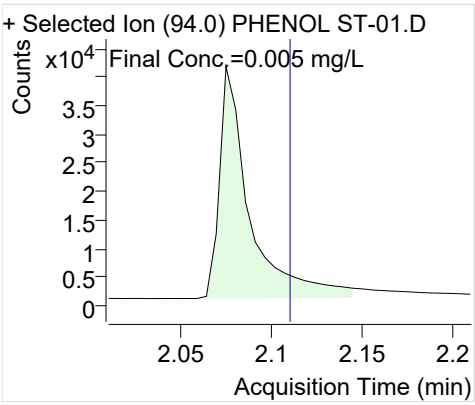





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(JR 2.20)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-24 오전 8:47:32	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:12:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:47:32	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 4:06:51	**Data File**	PHENOL ST-02.D
Type	Cal	**Name**	PHENOL ST-02
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

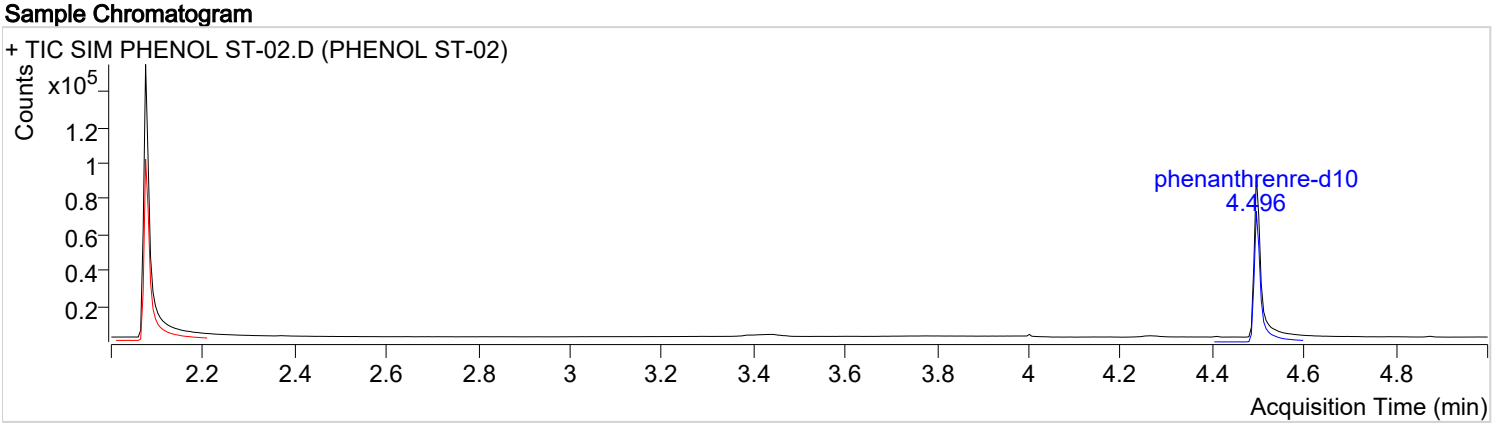

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	99182	74073	0.010 mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(JR 2.20)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-24 오전 8:47:32	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:12:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:47:32	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 4:15:11	**Data File**	PHENOL ST-03.D
Type	Cal	**Name**	PHENOL ST-03
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

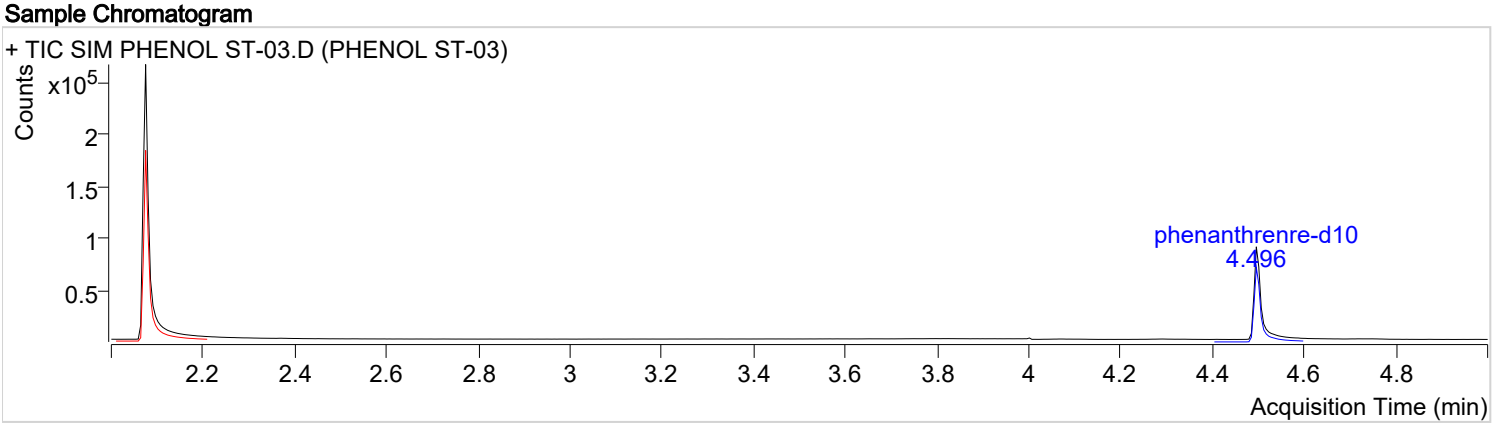

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	160691	75698	0.015 mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(JR 2.20)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-24 오전 8:47:32	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:12:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:47:32	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 4:23:32	**Data File**	PHENOL ST-04.D
Type	Cal	**Name**	PHENOL ST-04
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

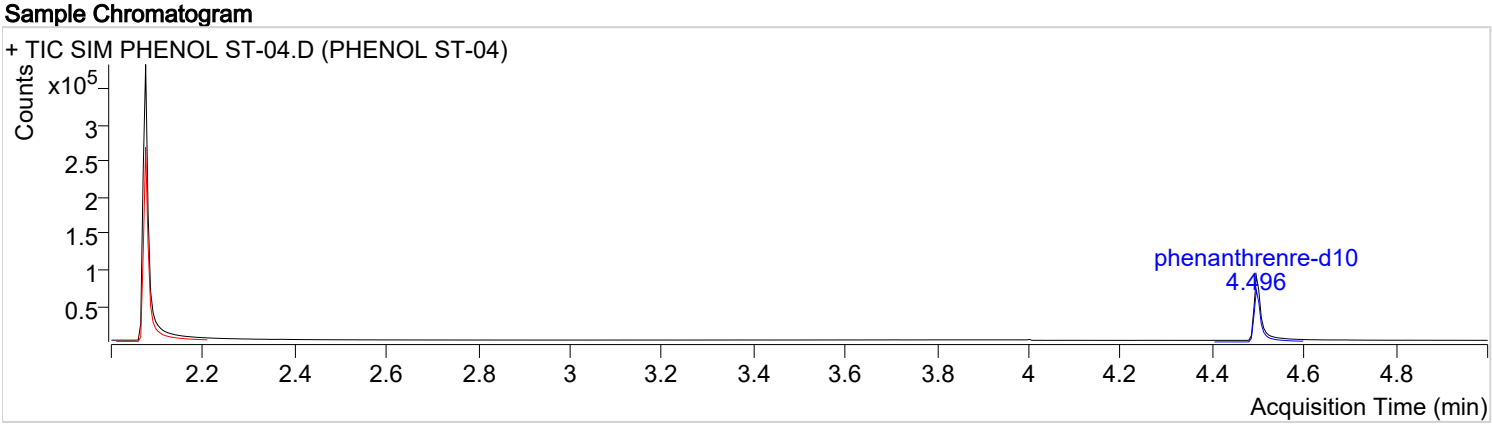

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	209631	77672	0.019 mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(JR 2.20)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-24 오전 8:47:32	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:12:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:47:32	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 4:31:57	**Data File**	PHENOL ST-05.D
Type	Cal	**Name**	PHENOL ST-05
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

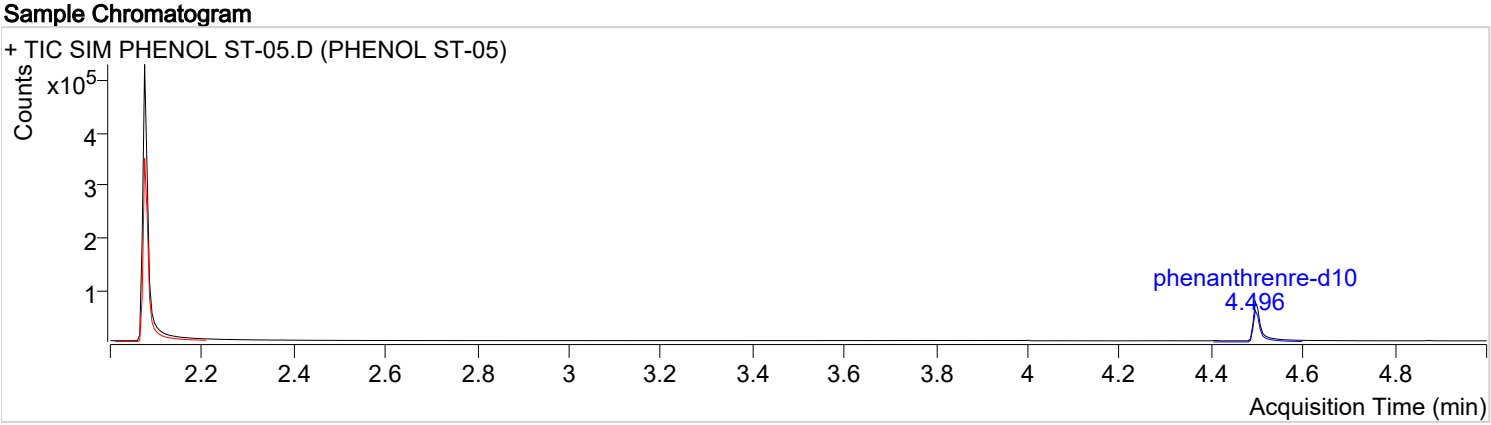

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	293347	66303	0.031 mg/L

Phenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(JR 2.20)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-24 오전 8:47:32	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:12:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:47:32	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 4:40:23	**Data File**	PHENOL ST-06.D
Type	Cal	**Name**	PHENOL ST-06
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

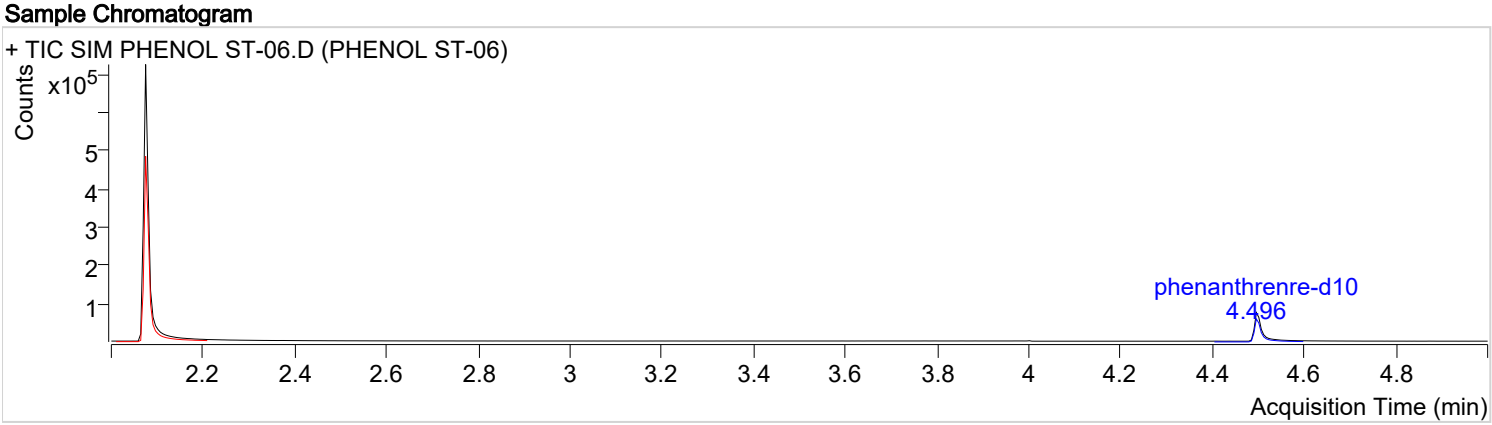

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	385624	66938	0.040 mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(JR 2.20)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-24 오전 8:47:32	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:12:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:47:32	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 4:57:09	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

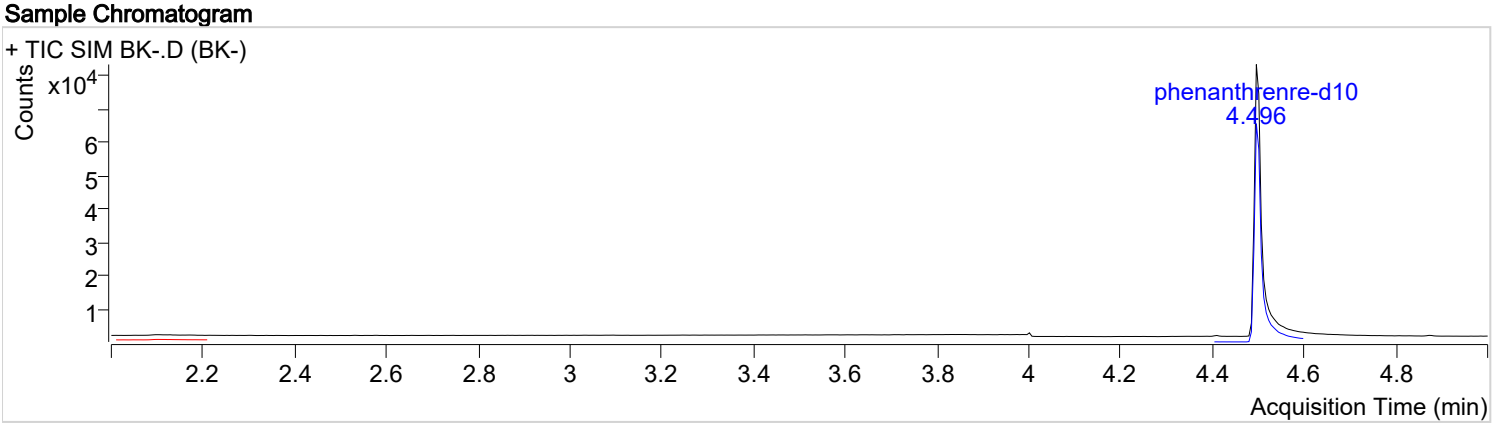

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			75204	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(JR 2.20)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-24 오전 8:47:32	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:12:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:47:32	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 5:05:32	**Data File**	JR 26-02-20.D
Type	Sample	**Name**	JR 26-02-20
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

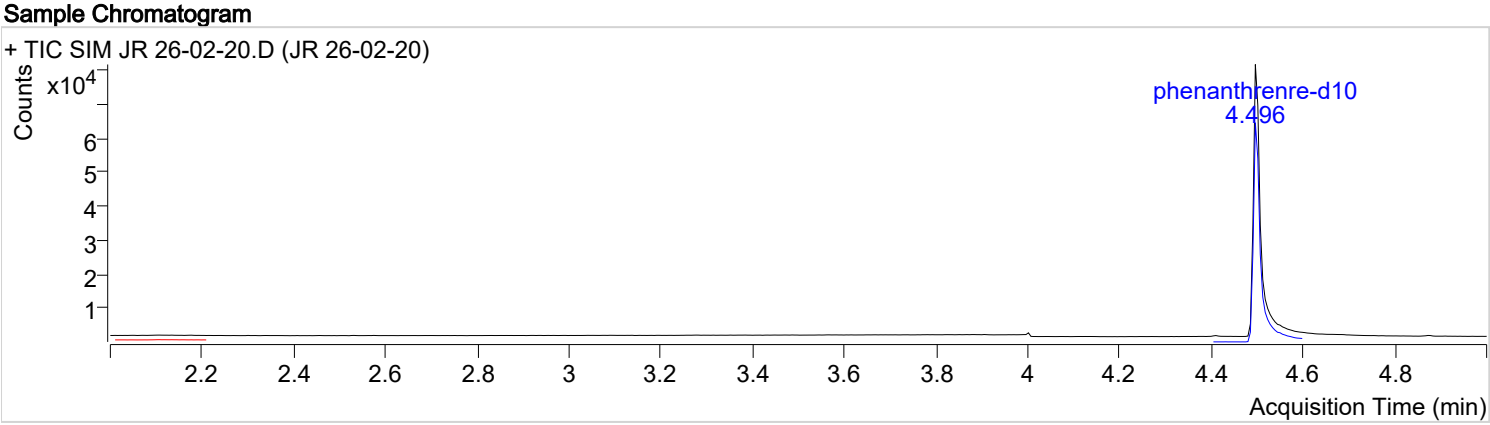

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			72487	ND mg/L

Phenol

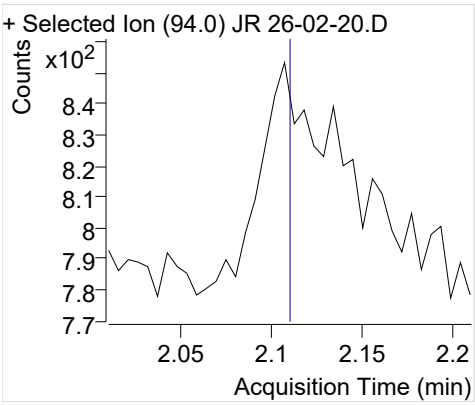





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(JR 2.20)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-24 오전 8:47:32	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:12:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:47:32	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 5:13:54	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

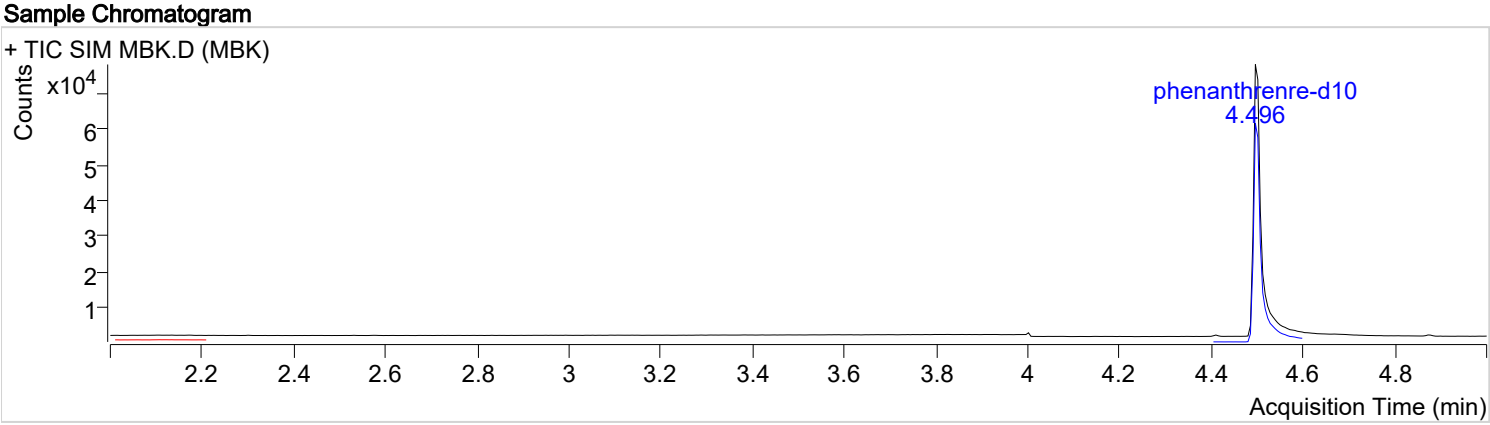

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			72725	ND mg/L

Phenol

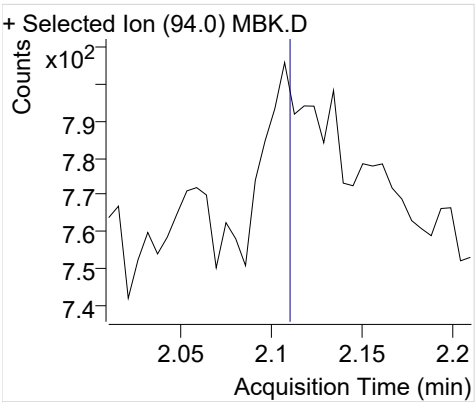





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PHENOL(JR 2.20)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-02-24 오전 8:47:32	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:12:11	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-24 오전 8:47:32	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-23 오후 5:30:44	**Data File**	-CCV-.D
Type	QC	**Name**	-CCV-
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

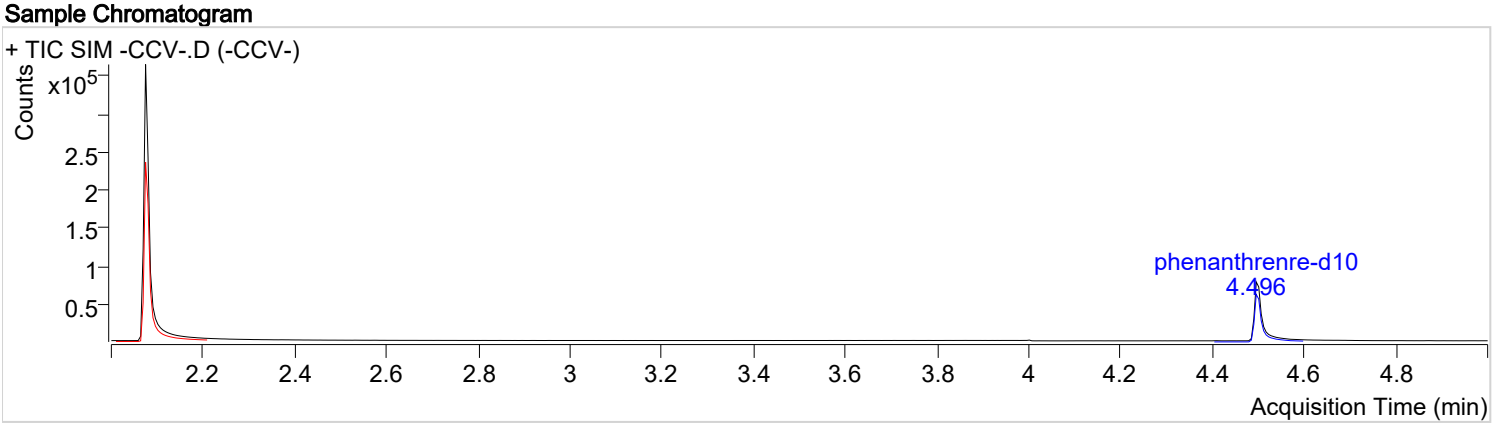

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	211193	73279	0.020 mg/L
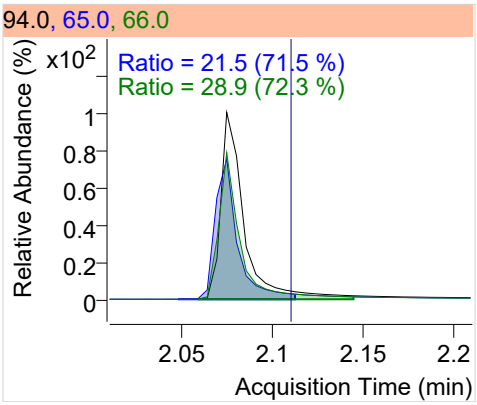
Phenol