Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin				
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Phenol

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
PHENOL ST-01.D	Cal	2.075	36679	62338	0.005
PHENOL ST-02.D	Cal	2.075	73893	62750	0.010
PHENOL ST-03.D	Cal	2.075	123083	71370	0.015
PHENOL ST-04.D	Cal	2.075	140788	63084	0.019
PHENOL ST-05.D	Cal	2.075	234944	60470	0.032
PHENOL ST-06.D	Cal	2.075	287517	59544	0.039
BK-.D	Blank			62289	ND
FBK(RE 26-03-11).D	Blank			61212	ND
RE-07.D	Sample	2.080	22332	49203	0.004
RE-08.D	Sample			44593	ND
RE-17.D	Sample			55619	ND
RE-18.D	Sample			53502	ND
RE-19.D	Sample	2.075	23170	61826	0.004
RE-20.D	Sample			56468	ND
RE-21.D	Sample			42737	ND
RE-22.D	Sample			58126	ND
RE-23.D	Sample			42775	ND
MBK.D	Blank			62575	ND
-C-C-V-.D	QC	2.075	133580	63388	0.018

Phenol

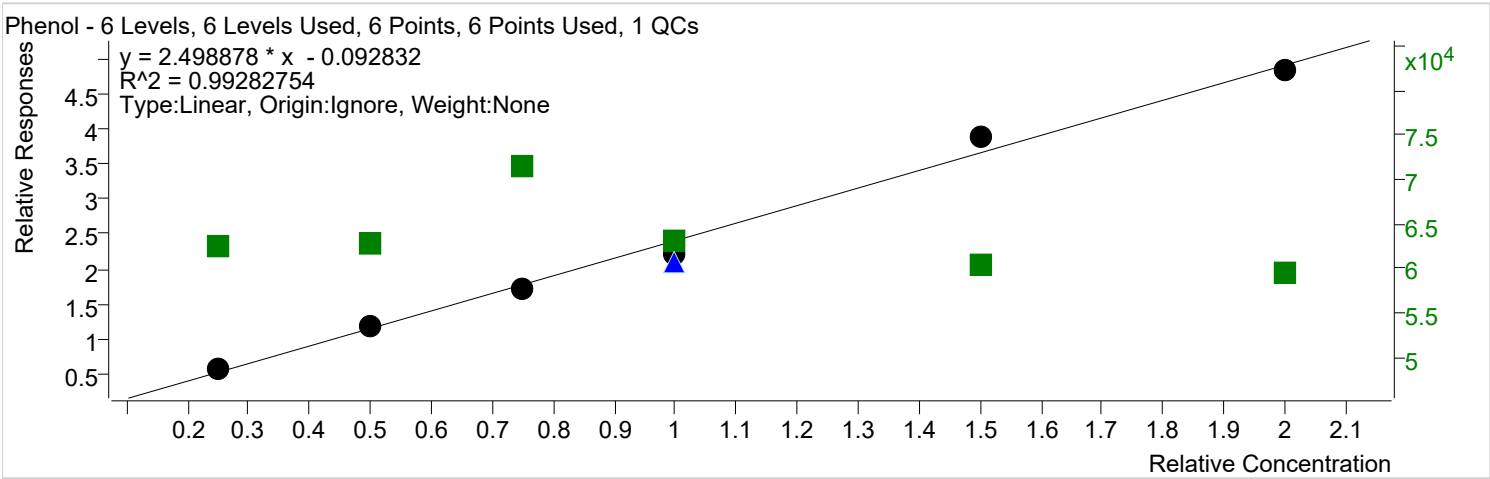

Cal. Path	Type	Level	Enable	Conc.	Response
\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\PHENOL ST-01.D	Calibration	1	x	2.500	36679
\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\PHENOL ST-02.D	Calibration	2	x	5.000	73893
\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\PHENOL ST-03.D	Calibration	3	x	7.500	123083
\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\PHENOL ST-04.D	Calibration	4	x	10.000	140788
\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\-C-C-V-.D	QC	4	x	10.000	133580
\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\PHENOL ST-05.D	Calibration	5	x	15.000	234944
\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\PHENOL ST-06.D	Calibration	6	x	20.000	287517

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 2:38:05	**Data File**	PHENOL ST-01.D
Type	Cal	**Name**	PHENOL ST-01
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

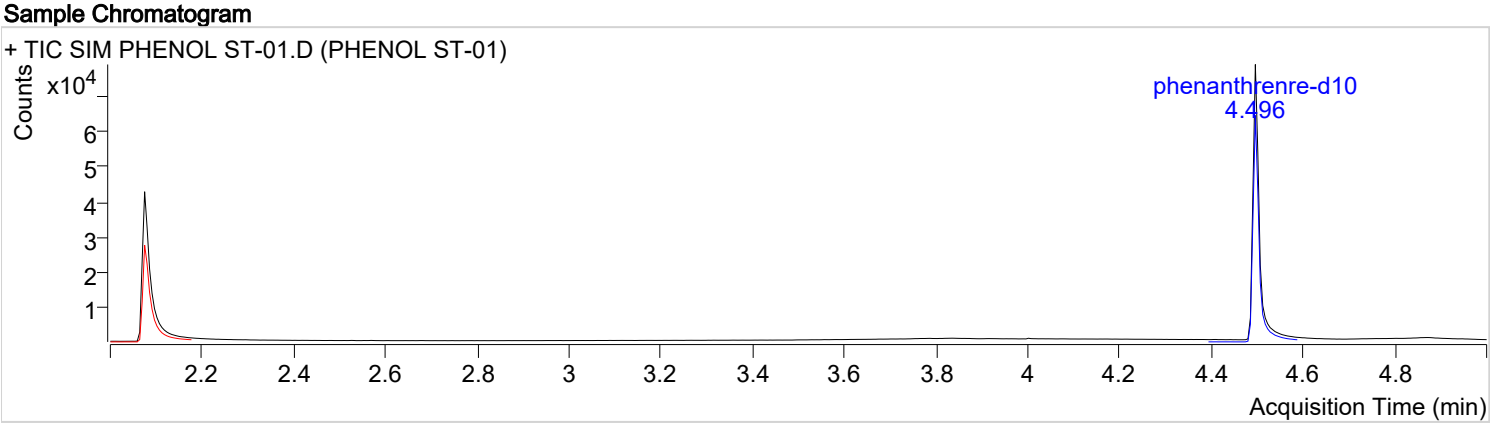

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	36679	62338	0.005 mg/L

Phenol







Generated at 오전 10:18 on 2026-04-10

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 2:46:19	**Data File**	PHENOL ST-02.D
Type	Cal	**Name**	PHENOL ST-02
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

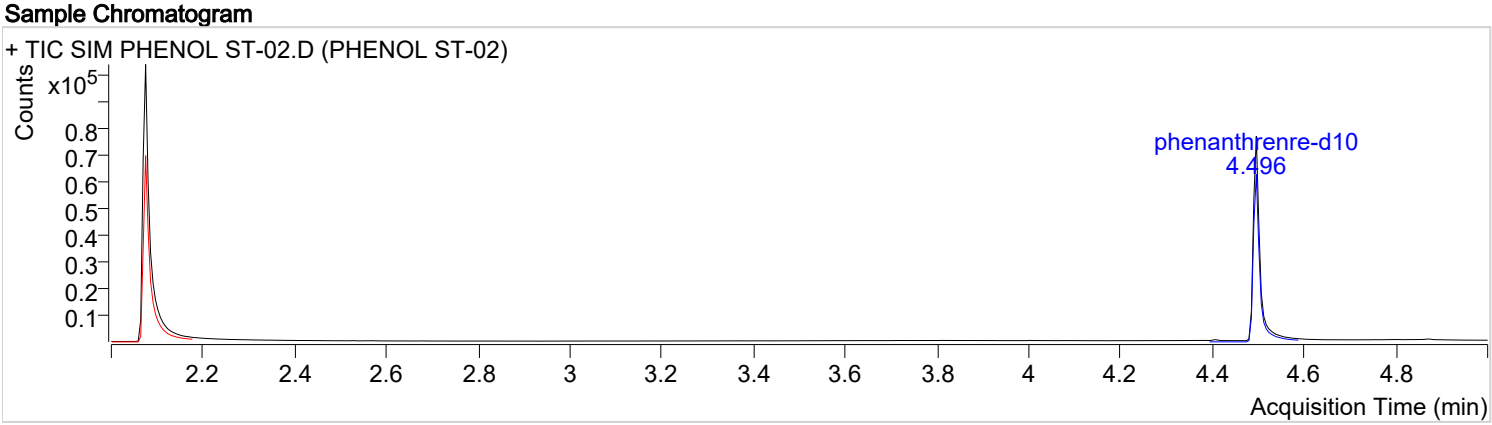

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	73893	62750	0.010 mg/L

Phenol



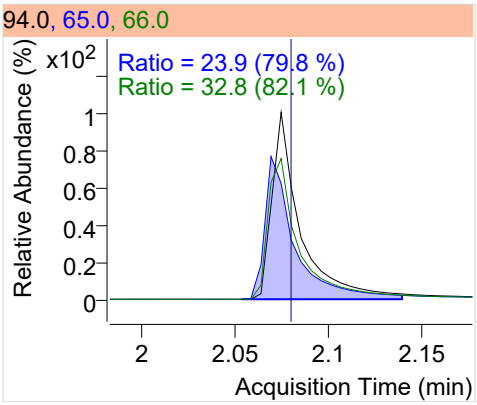



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 2:54:36	**Data File**	PHENOL ST-03.D
Type	Cal	**Name**	PHENOL ST-03
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

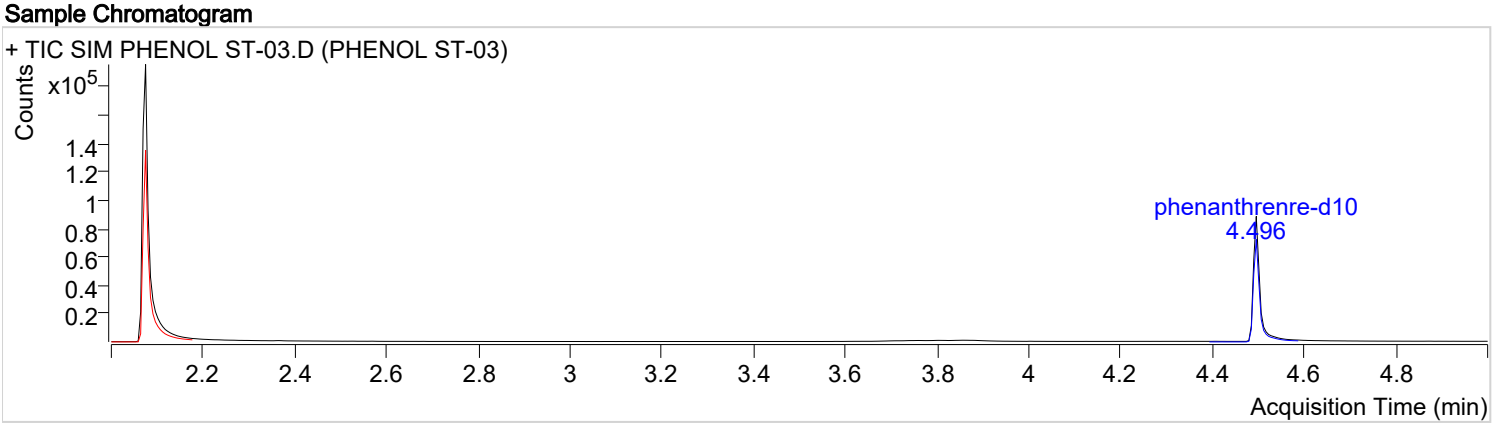

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	123083	71370	0.015 mg/L

Phenol



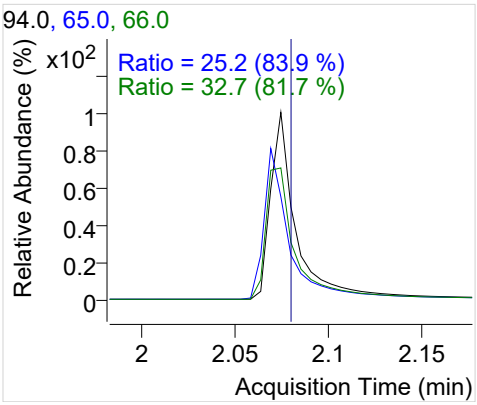



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 3:02:51	**Data File**	PHENOL ST-04.D
Type	Cal	**Name**	PHENOL ST-04
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

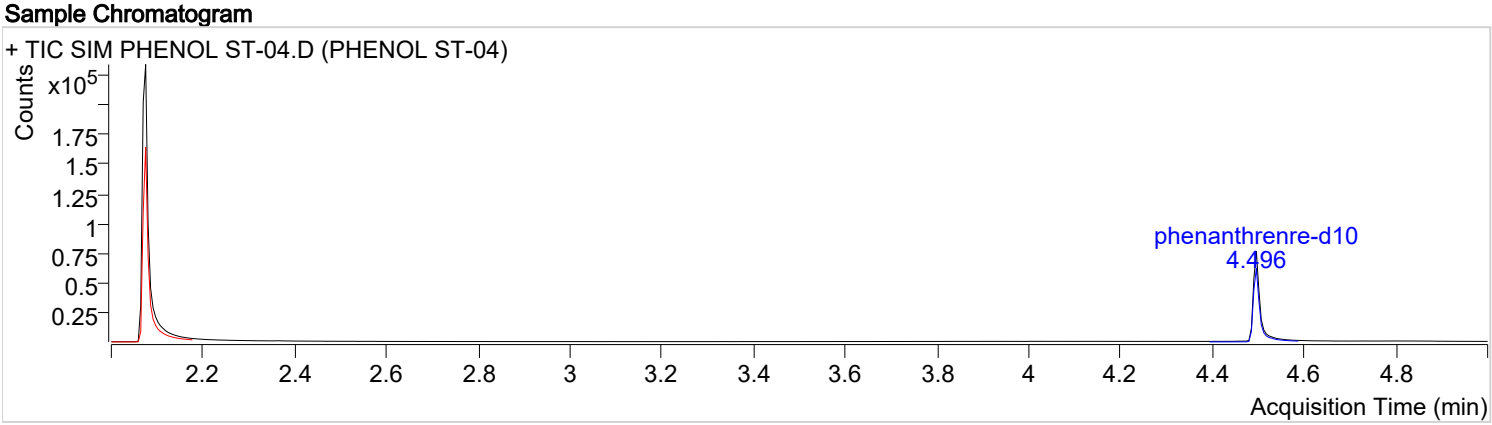

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	140788	63084	0.019 mg/L

Phenol



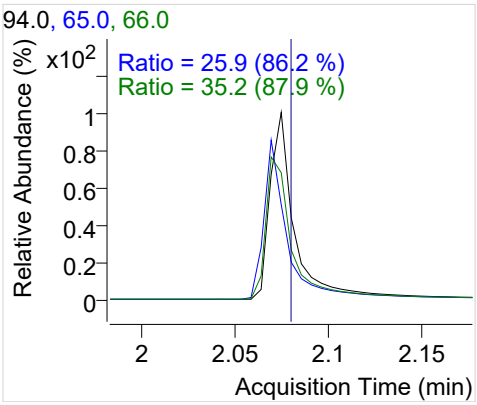



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 3:11:11	**Data File**	PHENOL ST-05.D
Type	Cal	**Name**	PHENOL ST-05
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

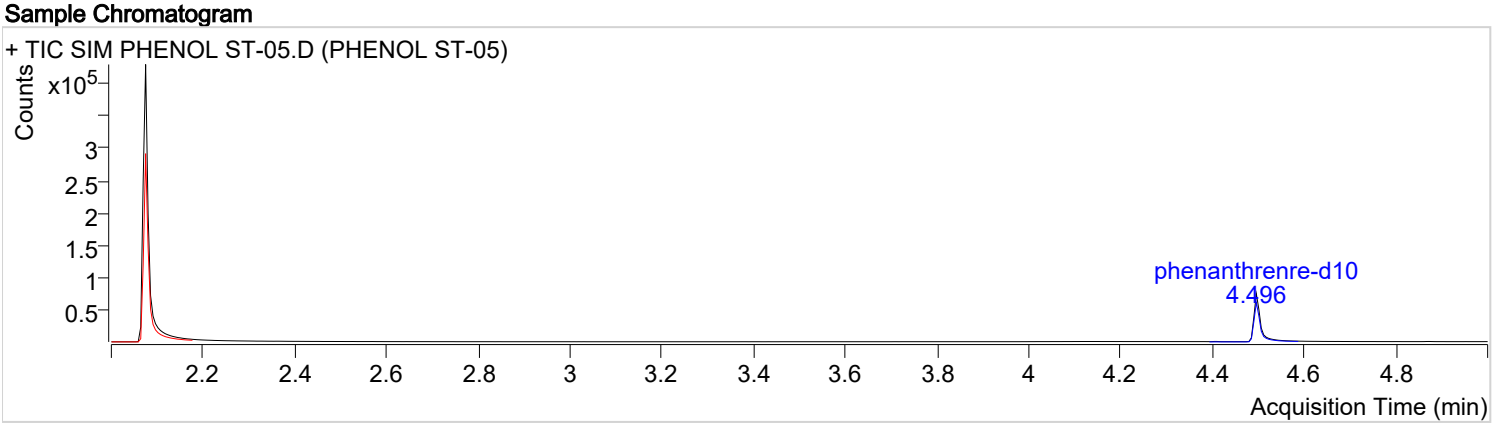

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	234944	60470	0.032 mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 3:19:30	**Data File**	PHENOL ST-06.D
Type	Cal	**Name**	PHENOL ST-06
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

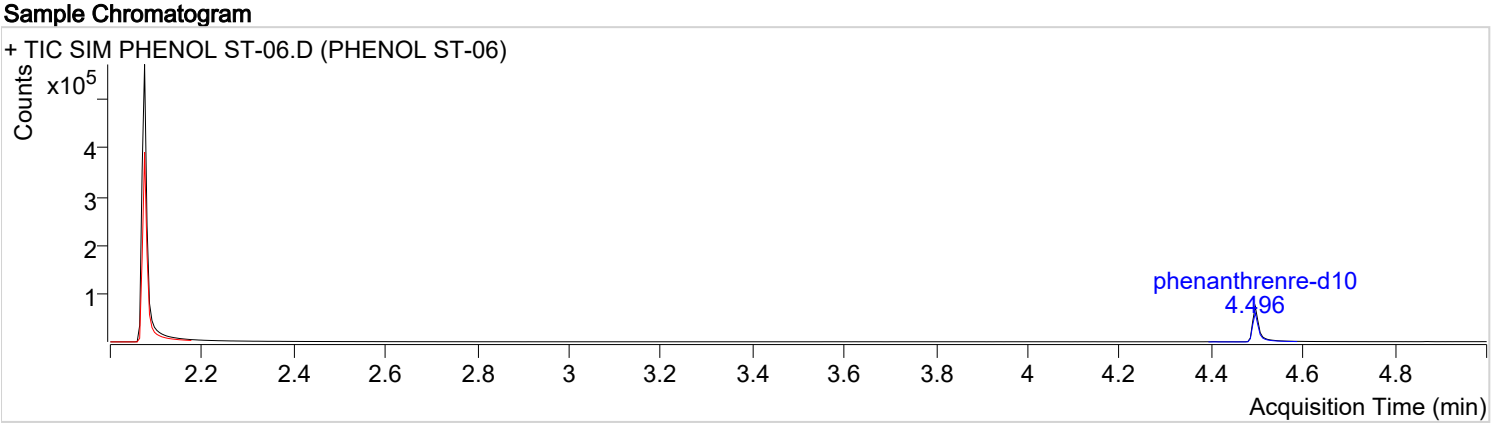

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	287517	59544	0.039 mg/L

Phenol



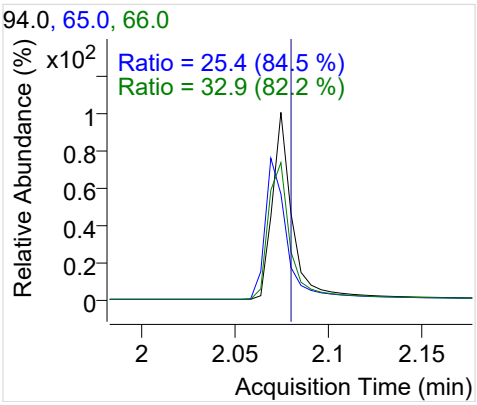

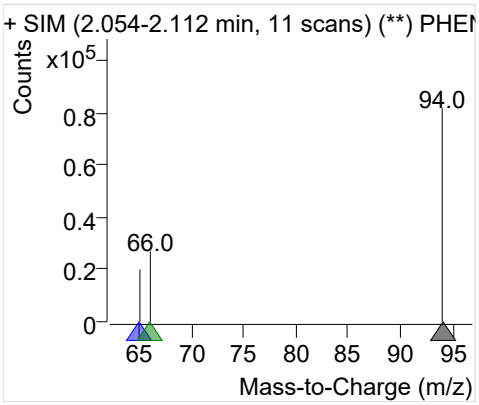

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 3:36:06	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

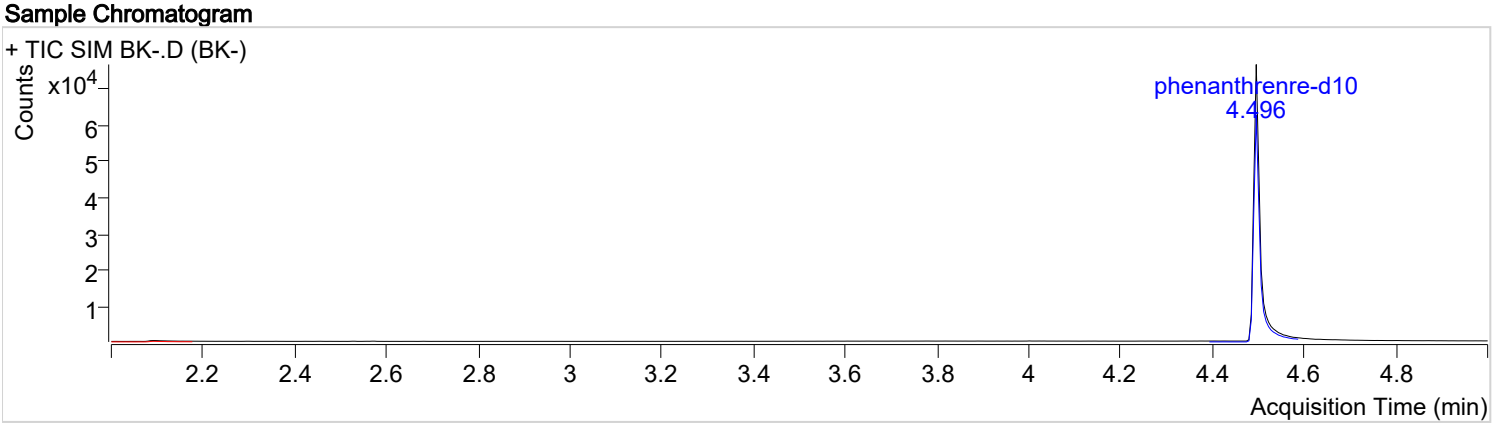

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			62289	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 3:44:26	**Data File**	FBK(RE 26-03-11).D
Type	Blank	**Name**	FBK(RE 26-03-11)
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

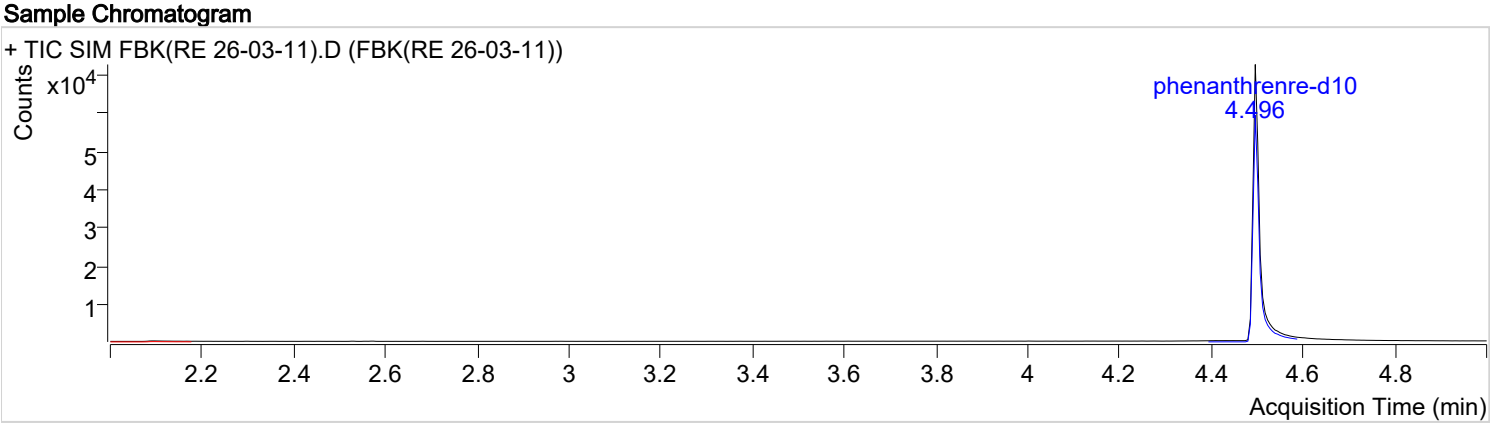

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			61212	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 3:52:45	**Data File**	RE-07.D
Type	Sample	**Name**	RE-07
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

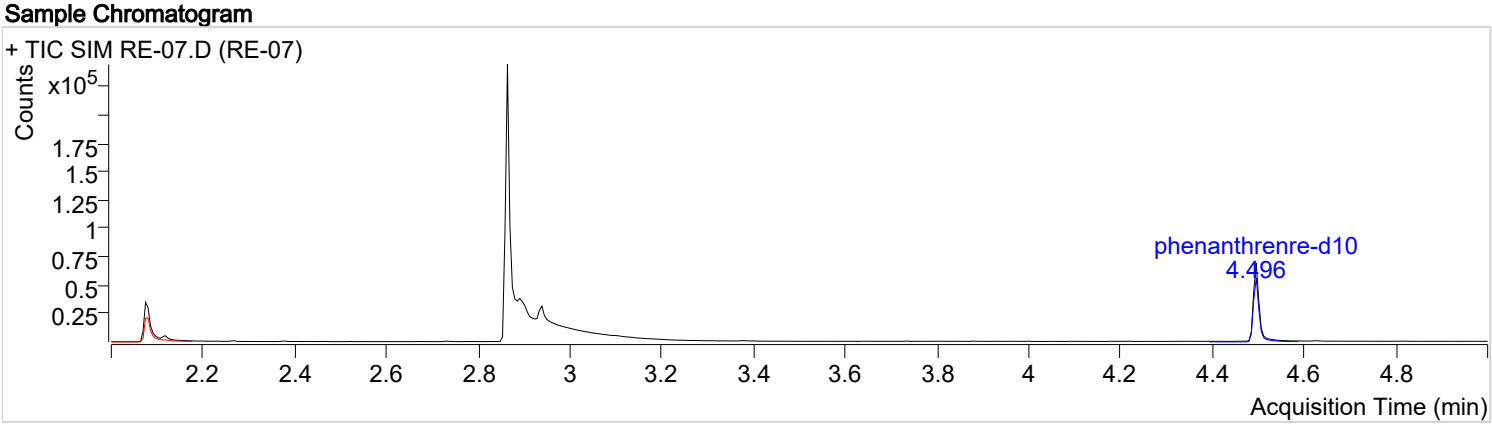

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.080	22332	49203	0.004 mg/L

Phenol



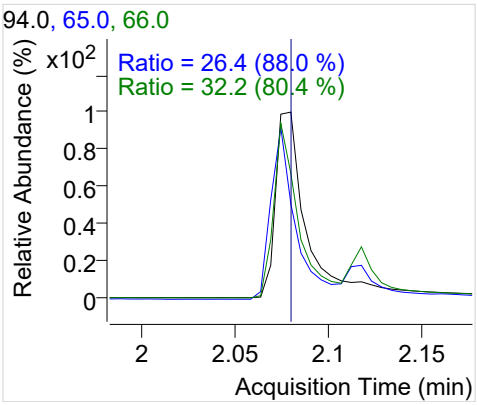

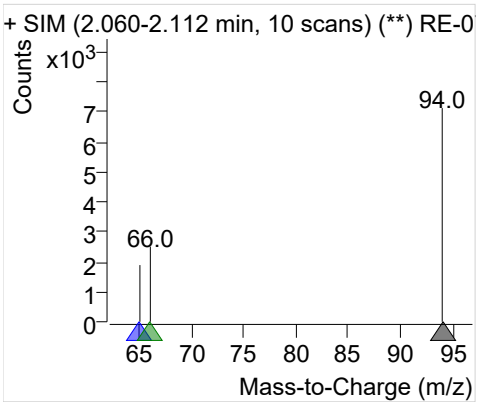

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 4:01:03	**Data File**	RE-08.D
Type	Sample	**Name**	RE-08
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

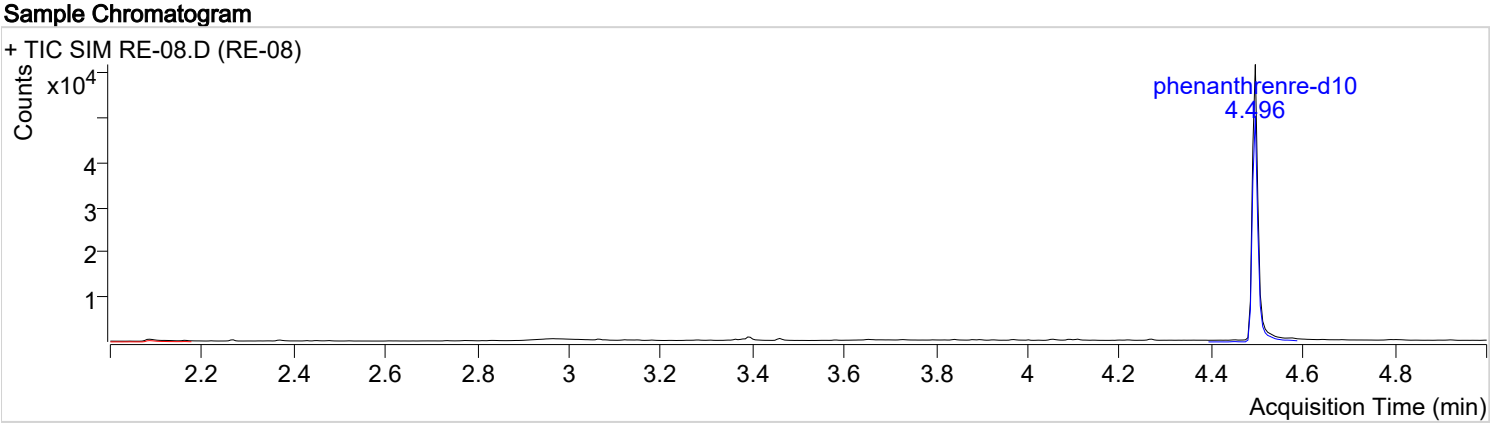

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			44593	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 4:09:23	**Data File**	RE-17.D
Type	Sample	**Name**	RE-17
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

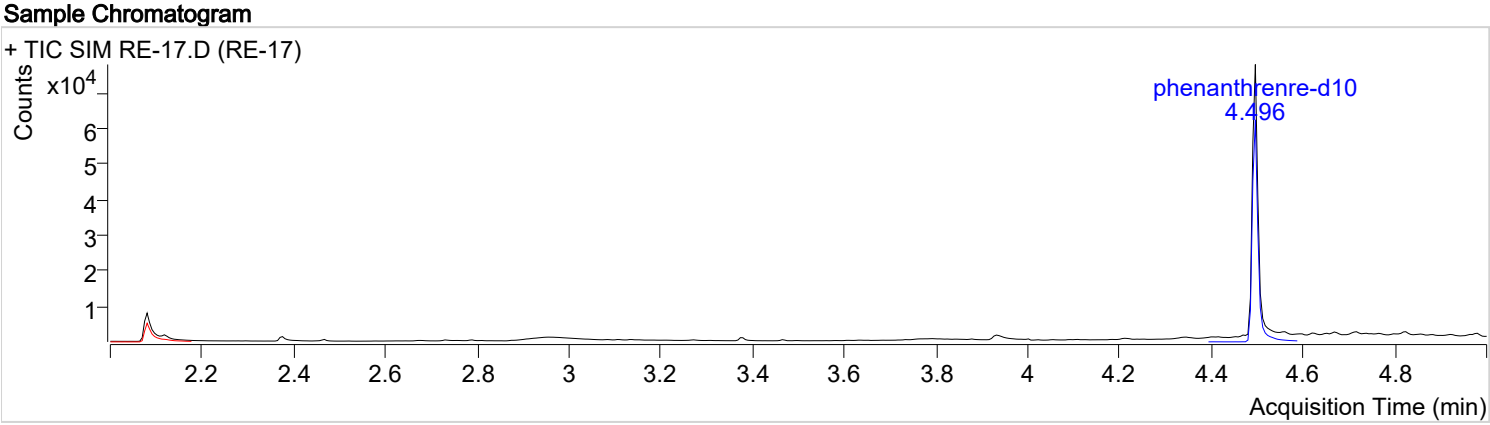

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			55619	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 4:17:43	**Data File**	RE-18.D
Type	Sample	**Name**	RE-18
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

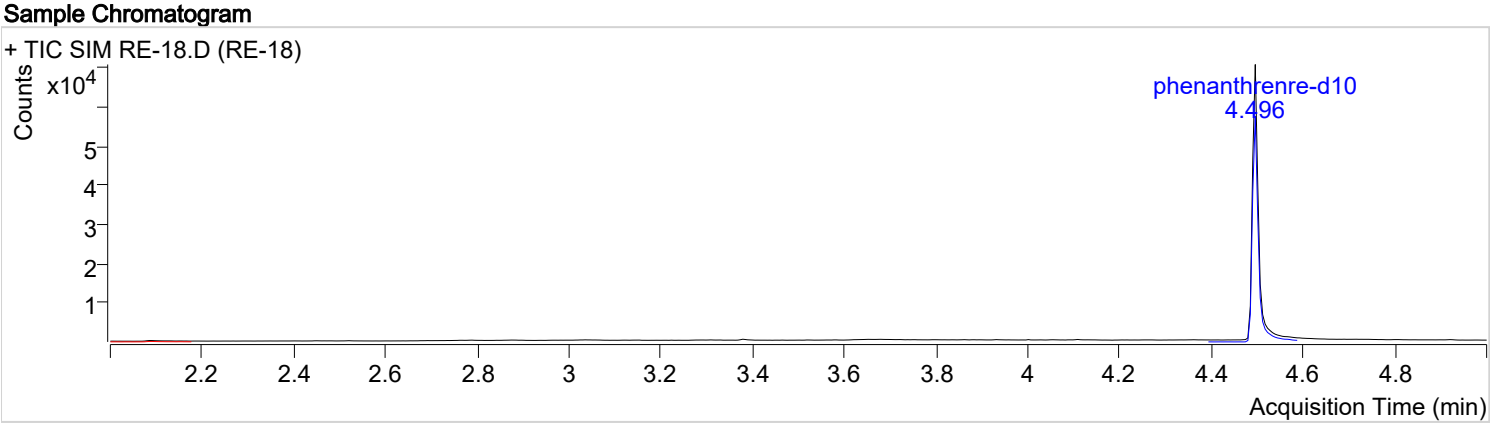

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			53502	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 4:26:03	**Data File**	RE-19.D
Type	Sample	**Name**	RE-19
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

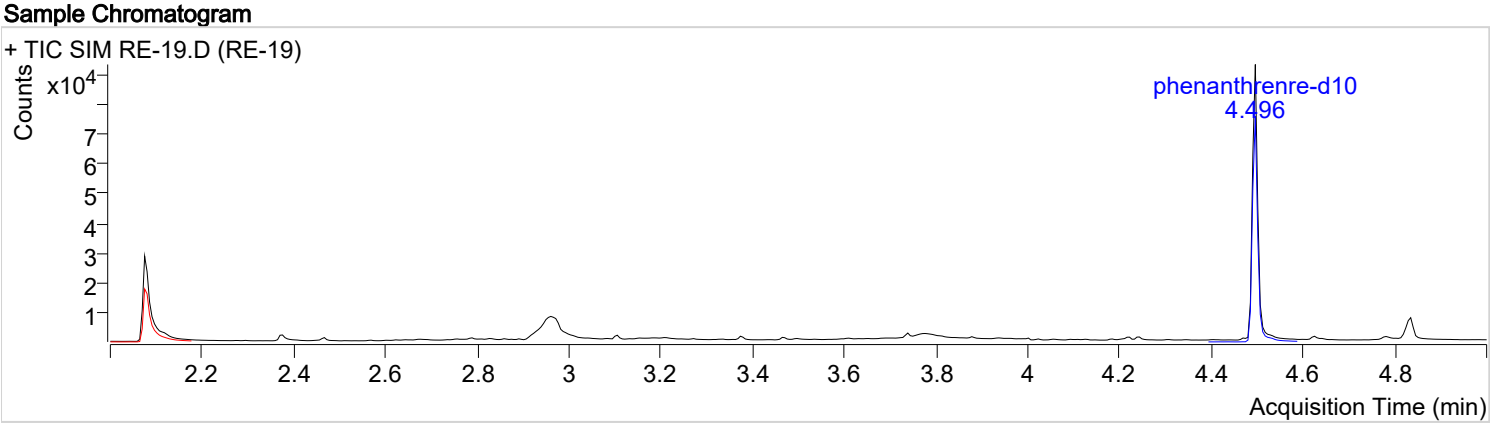

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	23170	61826	0.004 mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 4:34:21	**Data File**	RE-20.D
Type	Sample	**Name**	RE-20
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

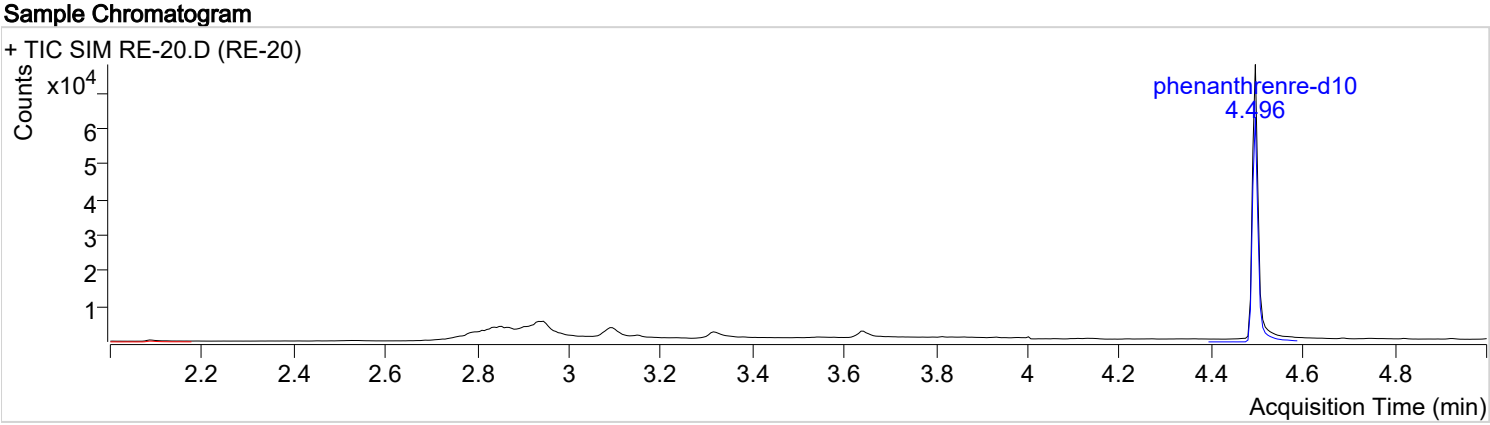

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			56468	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 4:42:41	**Data File**	RE-21.D
Type	Sample	**Name**	RE-21
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

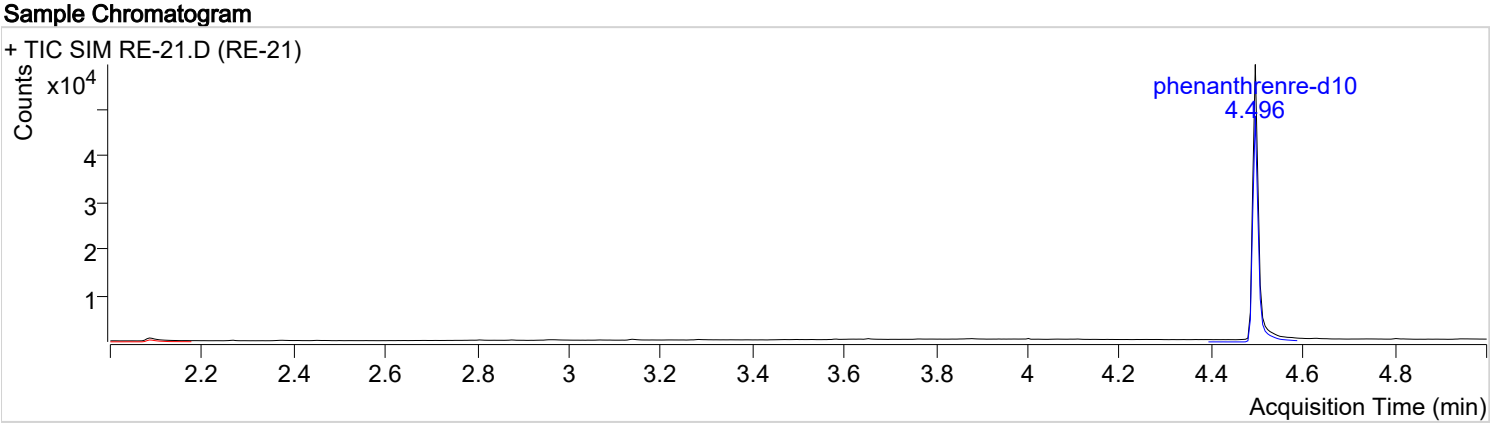

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			42737	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 4:50:58	**Data File**	RE-22.D
Type	Sample	**Name**	RE-22
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

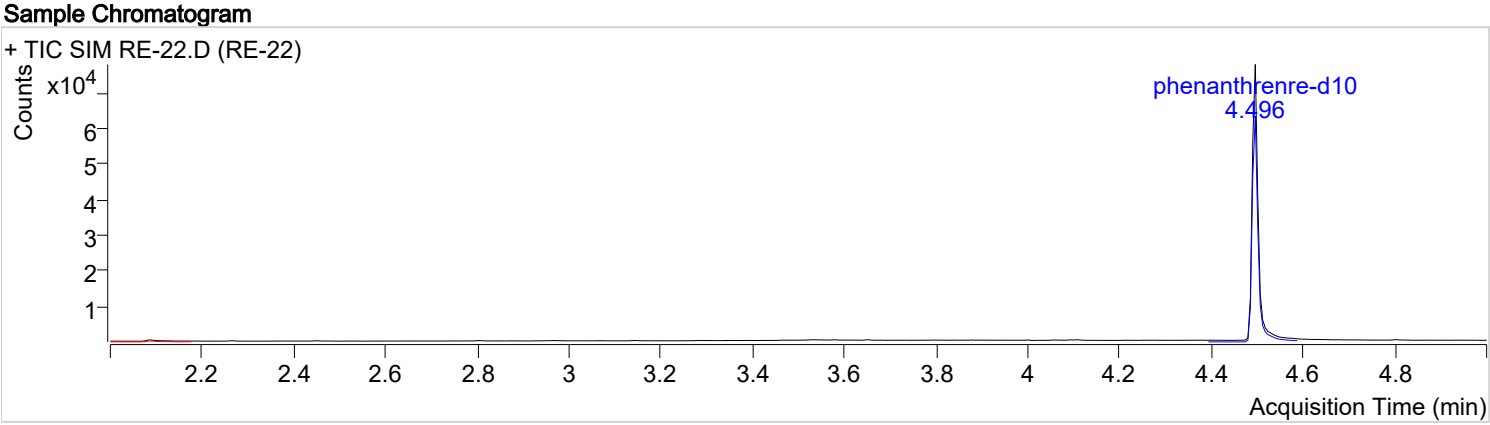

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			58126	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 4:59:18	**Data File**	RE-23.D
Type	Sample	**Name**	RE-23
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

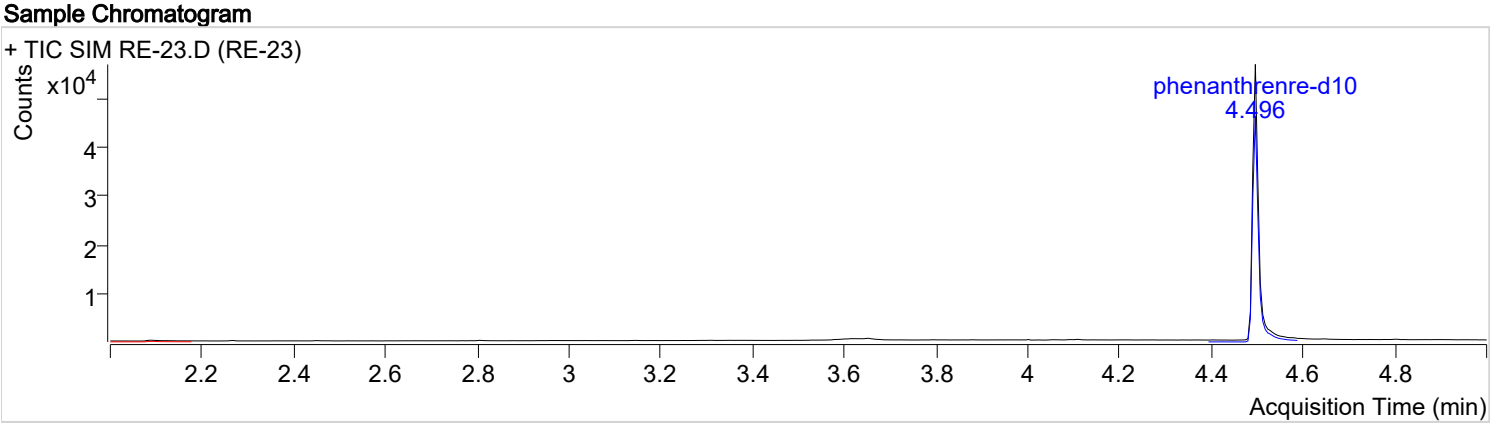

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			42775	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 5:07:42	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

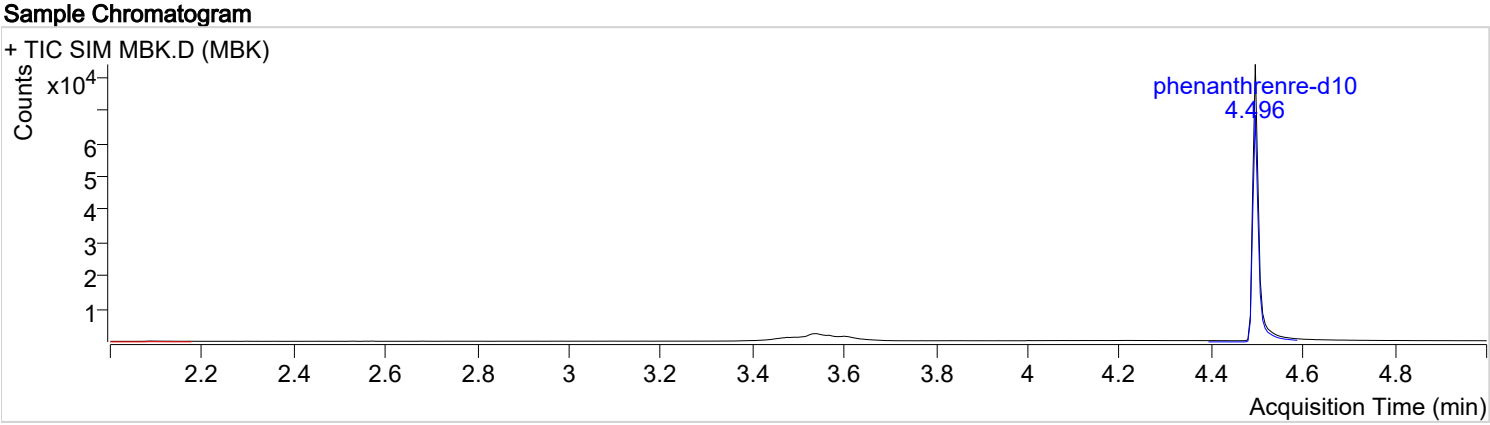

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			62575	ND mg/L

Phenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(RE 3.11)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-18 오후 12:40:23	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:18:44	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-18 오후 12:40:23	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-16 오후 5:32:37	**Data File**	-C-C-V-.D
Type	QC	**Name**	-C-C-V-
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

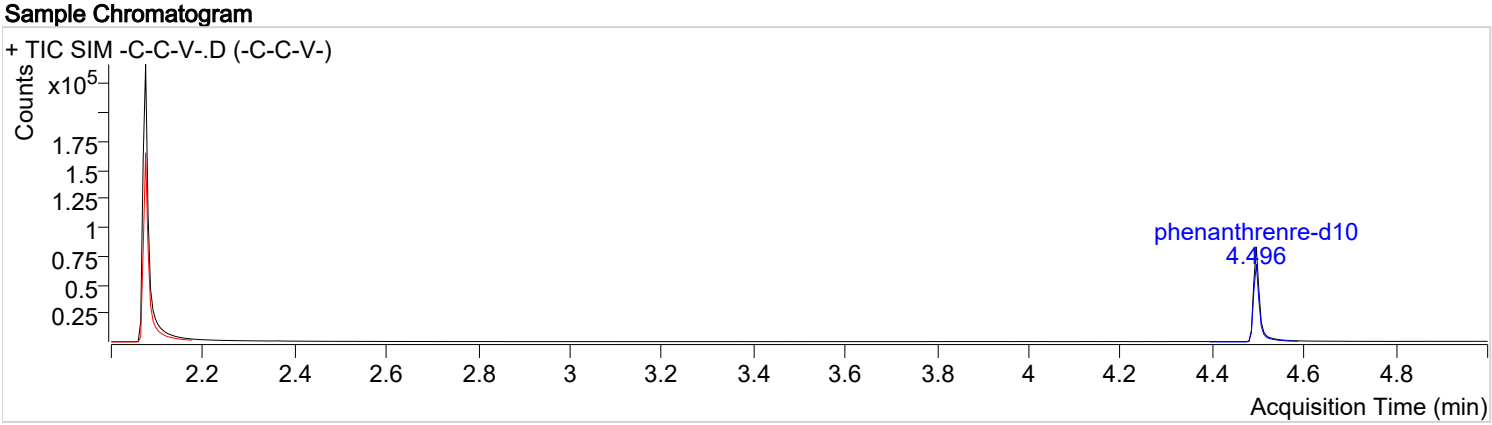

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	133580	63388	0.018 mg/L
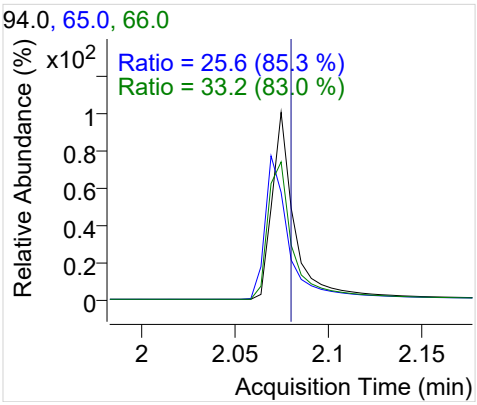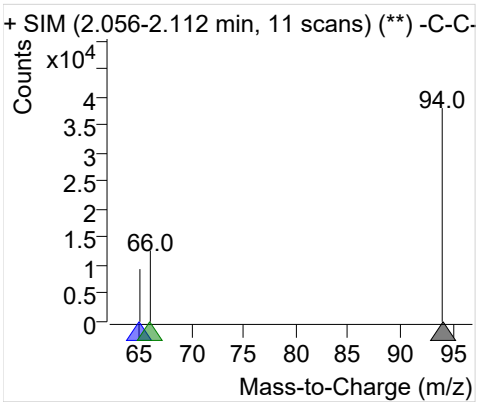
Phenol