Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\QuantResults\PHENOL.batch.bin				
Analysis Time	2026-03-31 오후 1:54:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:54:57	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Phenol

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
PHENOL ST-01.D	Cal	2.080	21850	37334	0.006
PHENOL ST-02.D	Cal	2.080	44505	35565	0.010
PHENOL ST-03.D	Cal	2.080	71251	36455	0.015
PHENOL ST-04.D	Cal	2.075	80113	32408	0.018
PHENOL ST-05.D	Cal	2.075	135974	33092	0.029
PHENOL ST-06.D	Cal	2.075	201189	32946	0.042
BK-.D	Blank			32522	ND
FBK(LG NJ 26-03-26).D	Blank			32236	ND
LG NJ-01.D	Sample			30001	ND
LG NJ-02.D	Sample			31800	ND
LG NJ-03.D	Sample	2.139	0	32739	ND
LG NJ-04.D	Sample			45705	ND
LG NJ-05.D	Sample			34019	ND
LG NJ-06.D	Sample			33268	ND
MBK.D	Blank			37179	ND
-CCV-.D	QC	2.080	83824	31582	0.019

Phenol

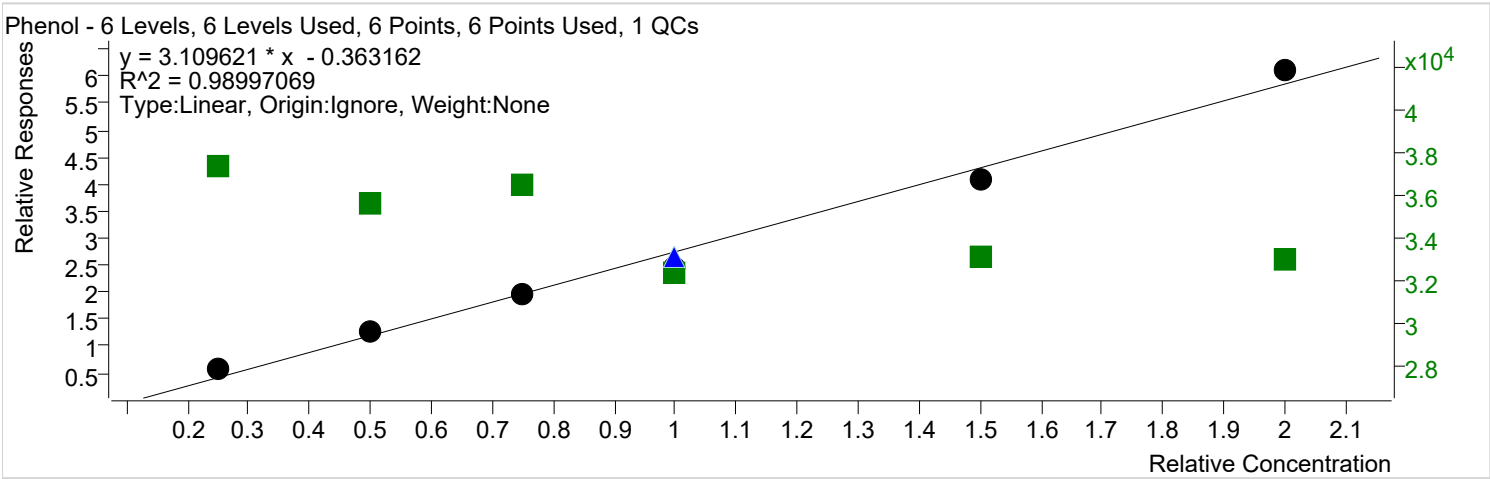

Cal. Path	Type	Level	Enable	Conc.	Response
\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\PHENOL ST-01.D	Calibration	1	x	2.500	21850
\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\PHENOL ST-02.D	Calibration	2	x	5.000	44505
\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\PHENOL ST-03.D	Calibration	3	x	7.500	71251
\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\PHENOL ST-04.D	Calibration	4	x	10.000	80113
\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\-CCV-.D	QC	4	x	10.000	83824
\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\PHENOL ST-05.D	Calibration	5	x	15.000	135974
\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\PHENOL ST-06.D	Calibration	6	x	20.000	201189

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-31 오후 1:54:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:17:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:54:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 9:20:06	**Data File**	PHENOL ST-01.D
Type	Cal	**Name**	PHENOL ST-01
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

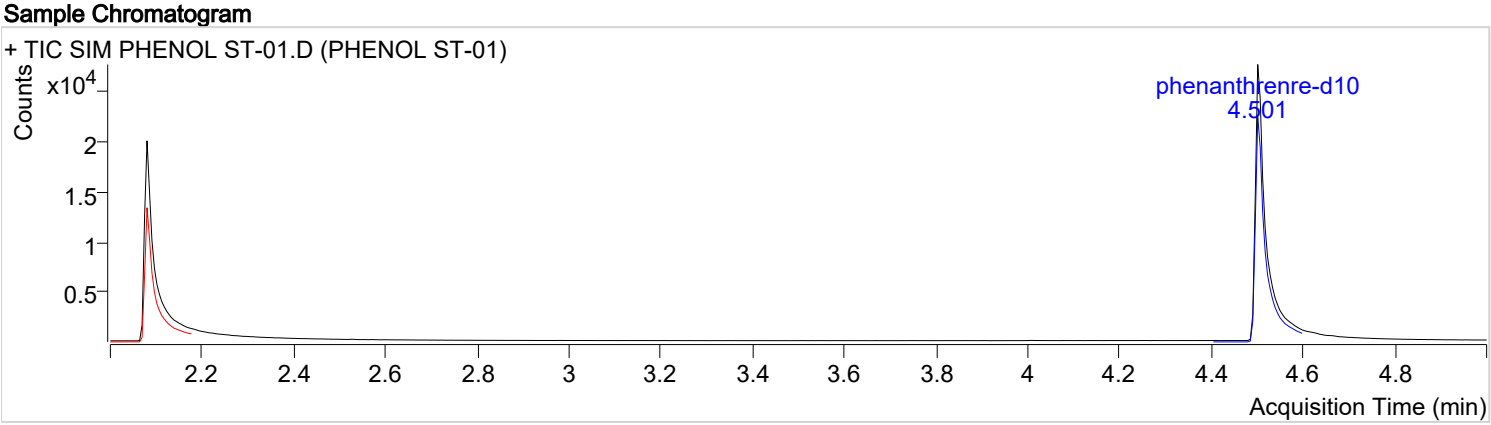

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.080	21850	37334	0.006 mg/L

Phenol





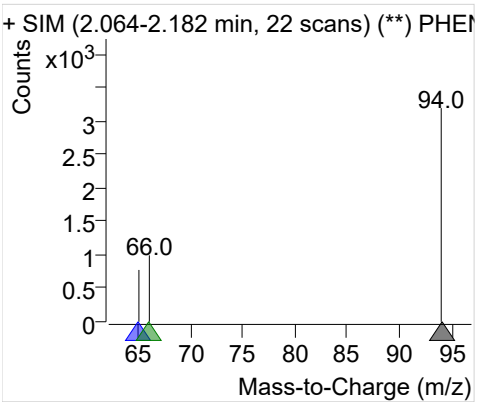

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-31 오후 1:54:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:17:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:54:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 9:28:23	**Data File**	PHENOL ST-02.D
Type	Cal	**Name**	PHENOL ST-02
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

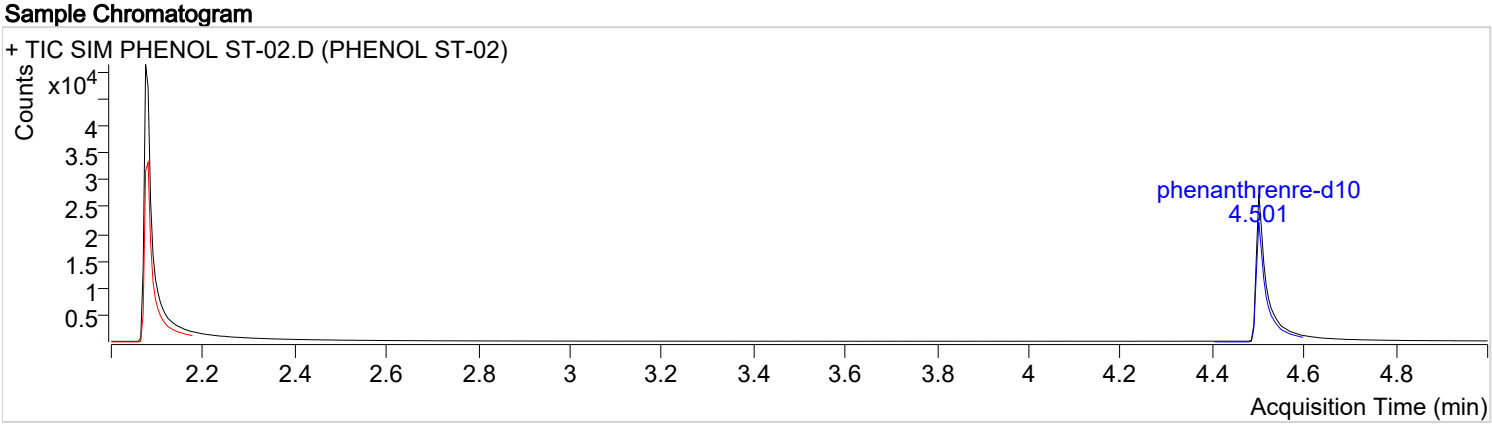

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.080	44505	35565	0.010 mg/L

Phenol





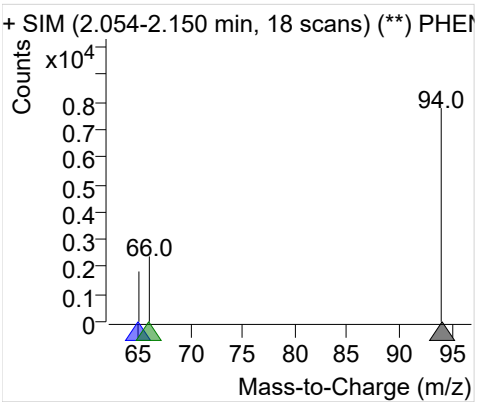

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-31 오후 1:54:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:17:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:54:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 9:36:44	**Data File**	PHENOL ST-03.D
Type	Cal	**Name**	PHENOL ST-03
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

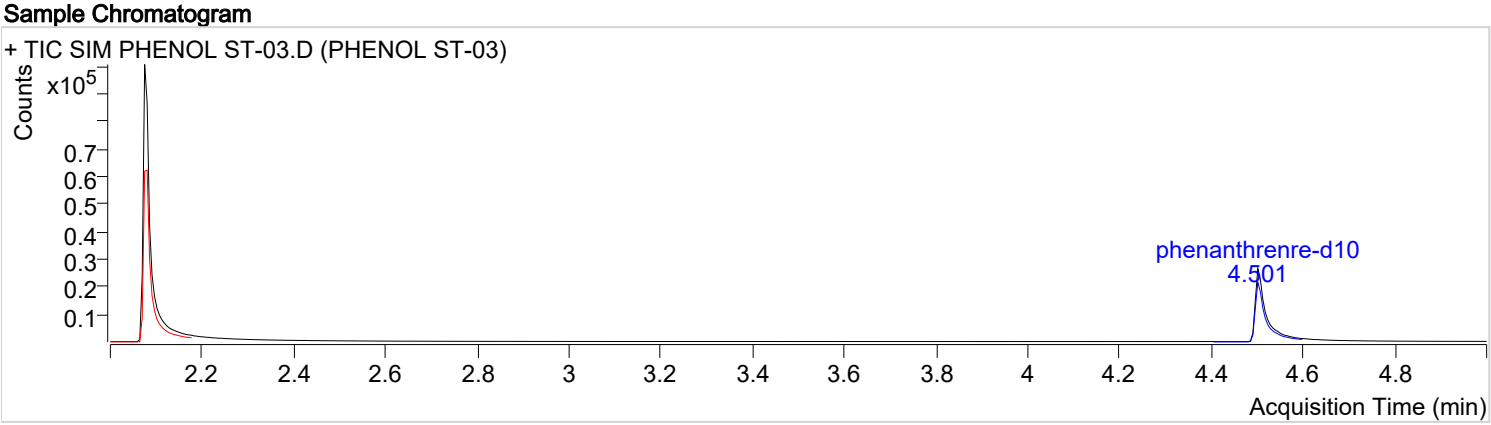

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.080	71251	36455	0.015 mg/L

Phenol



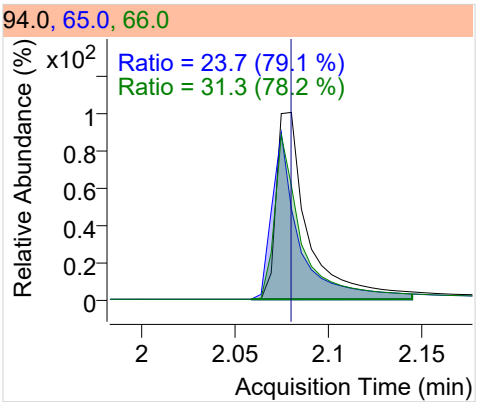

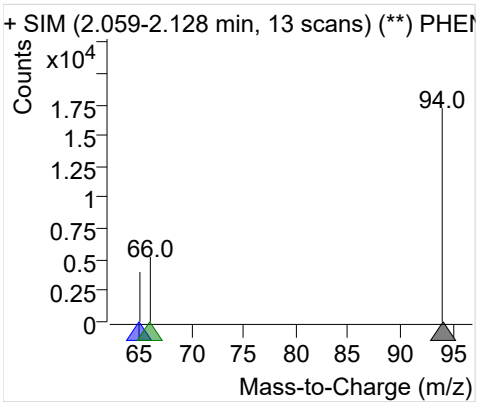

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-31 오후 1:54:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:17:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:54:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 9:45:02	**Data File**	PHENOL ST-04.D
Type	Cal	**Name**	PHENOL ST-04
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

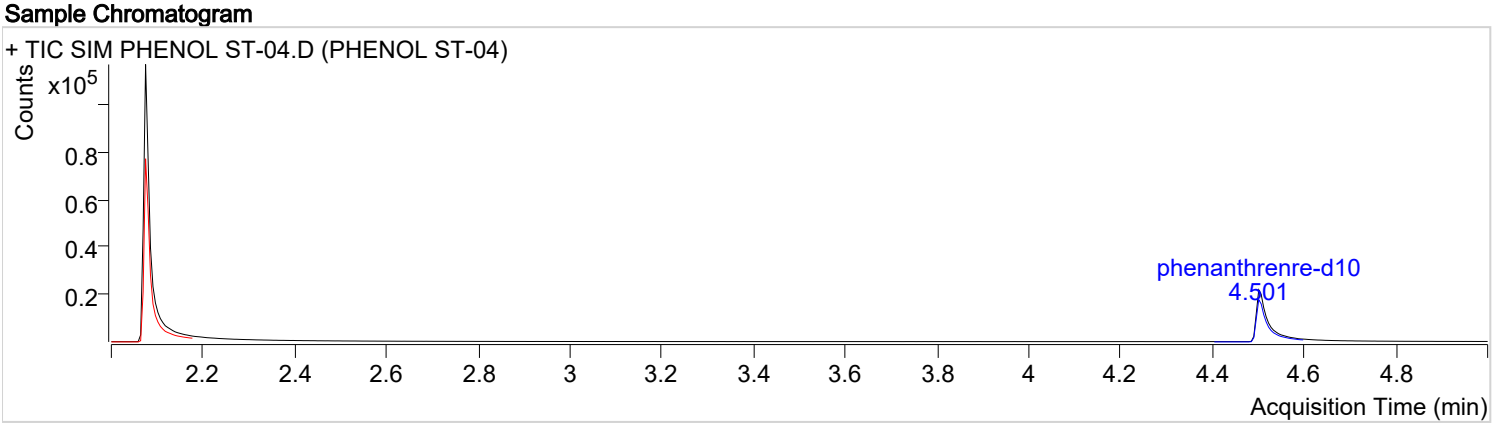

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	80113	32408	0.018 mg/L

Phenol





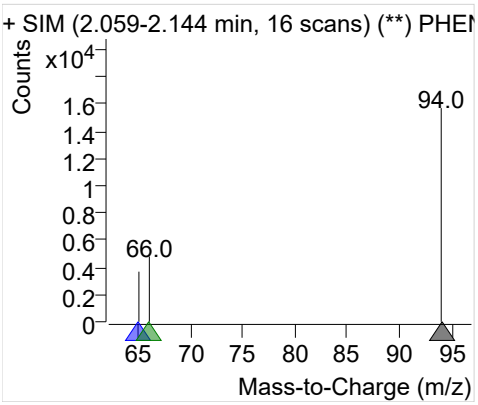

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-31 오후 1:54:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:17:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:54:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 9:53:21	**Data File**	PHENOL ST-05.D
Type	Cal	**Name**	PHENOL ST-05
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

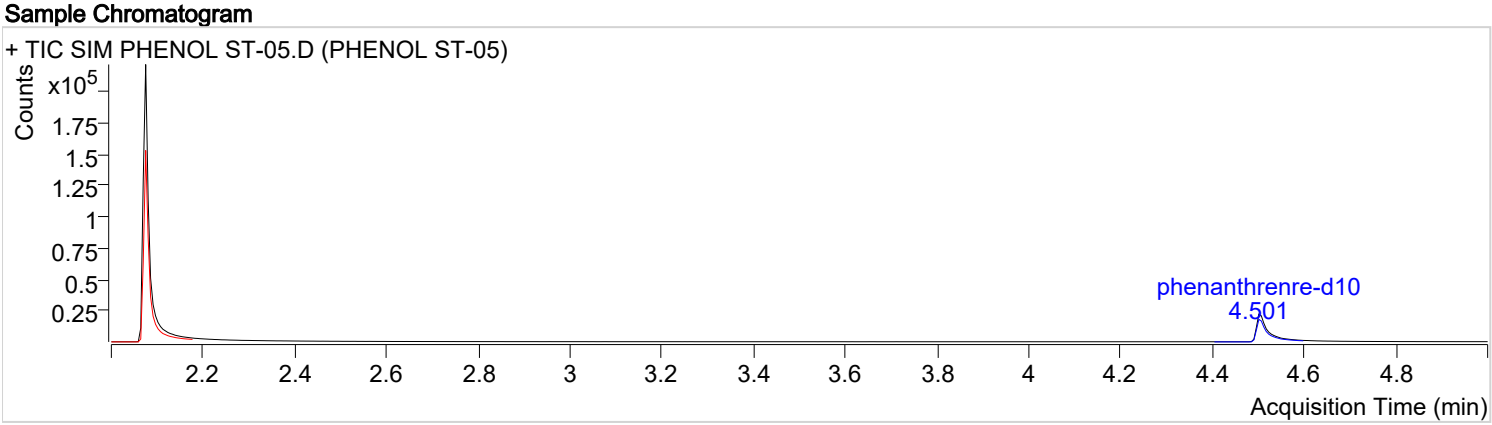

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	135974	33092	0.029 mg/L

Phenol



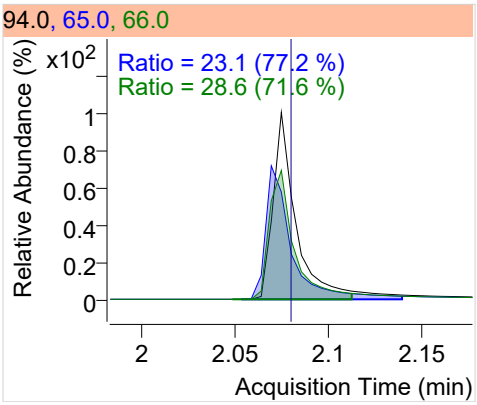

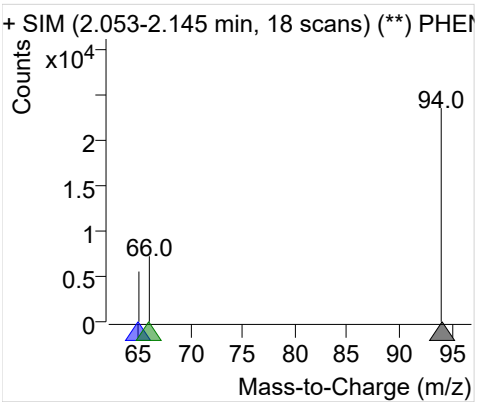

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-31 오후 1:54:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:17:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:54:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 10:01:42	**Data File**	PHENOL ST-06.D
Type	Cal	**Name**	PHENOL ST-06
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

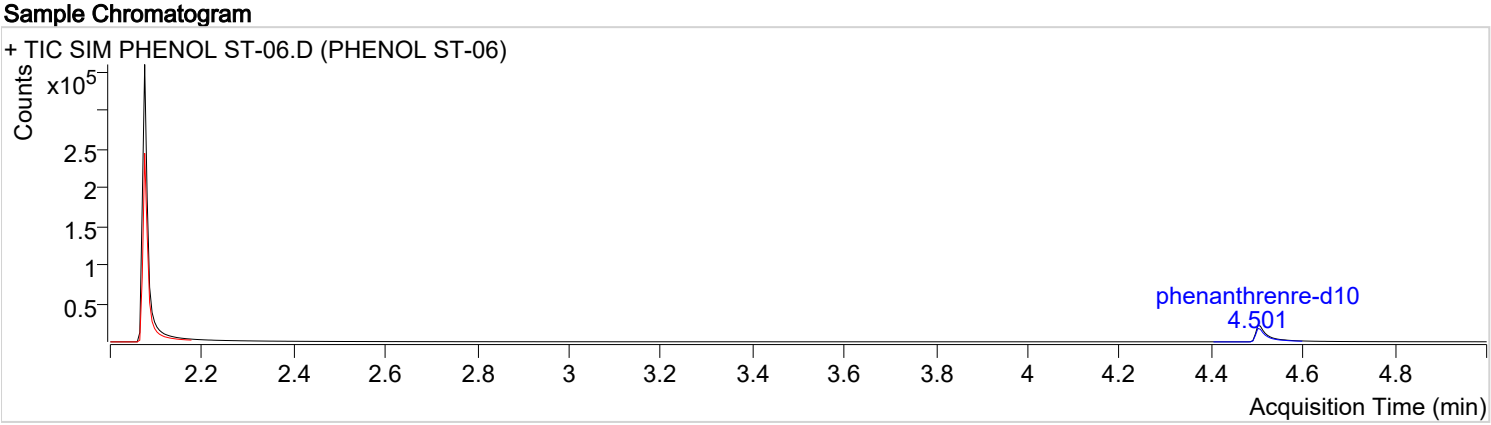

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.075	201189	32946	0.042 mg/L

Phenol

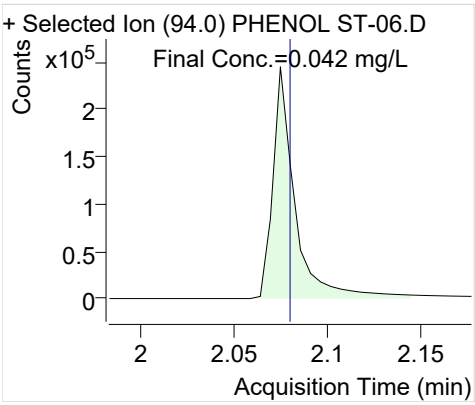



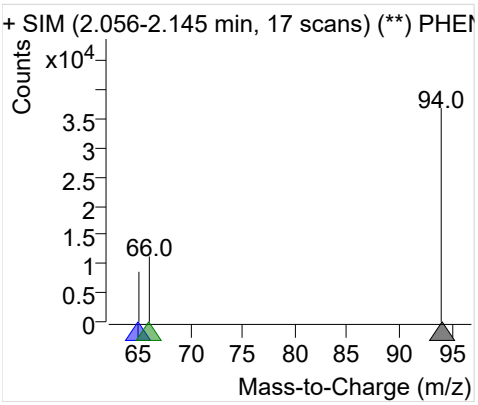

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-31 오후 1:54:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:17:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:54:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 10:18:23	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

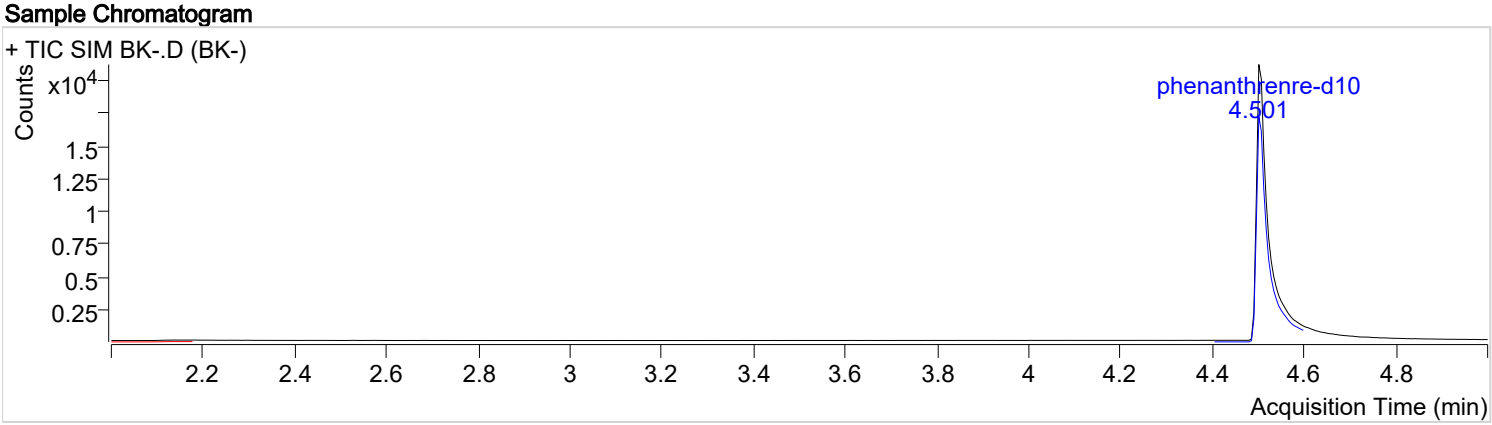

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			32522	ND mg/L

Phenol



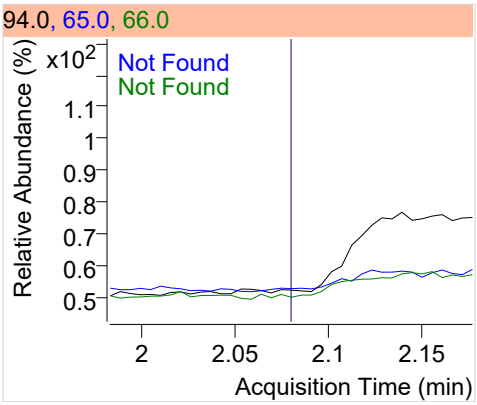

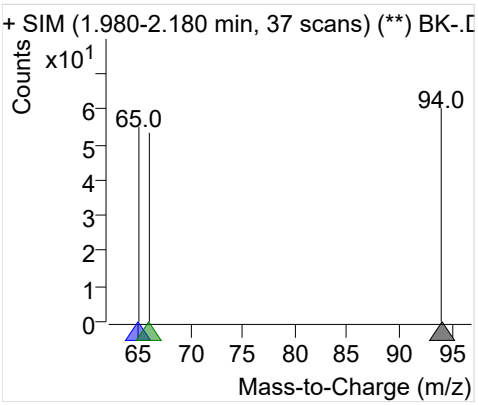

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-31 오후 1:54:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:17:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:54:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 10:26:44	**Data File**	FBK(LG NJ 26-03-26).D
Type	Blank	**Name**	FBK(LG NJ 26-03-26)
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

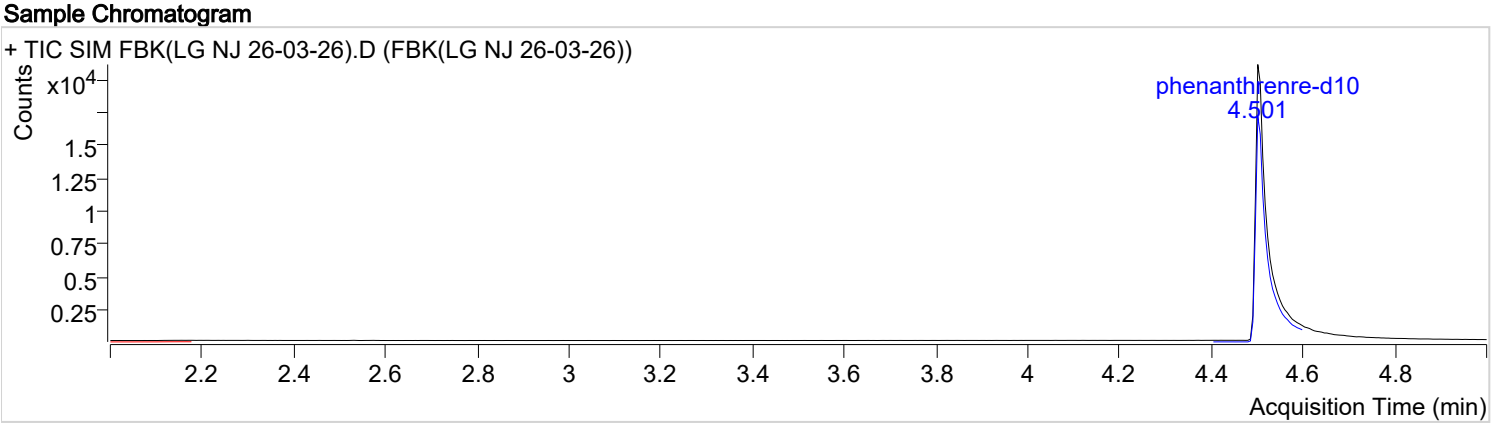

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			32236	ND mg/L

Phenol

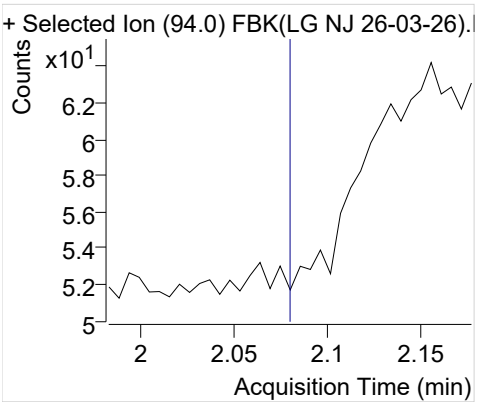

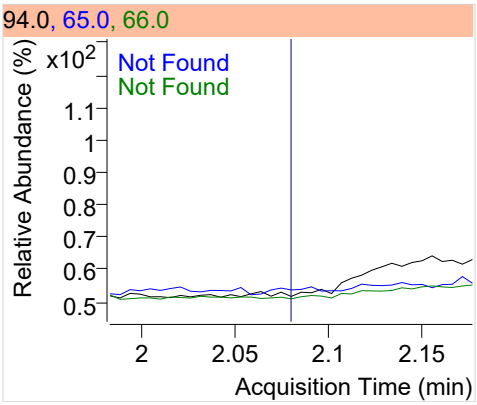

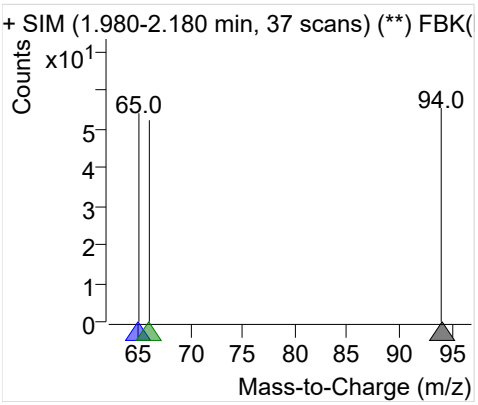

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-31 오후 1:54:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:17:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:54:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 10:35:07	**Data File**	LG NJ-01.D
Type	Sample	**Name**	LG NJ-01
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

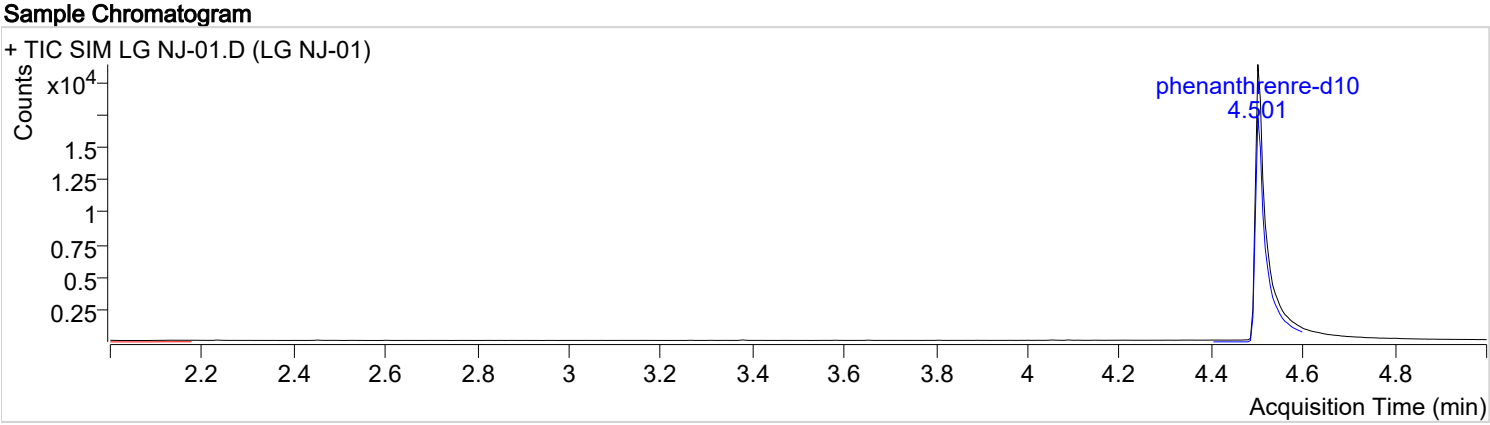

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			30001	ND mg/L

Phenol

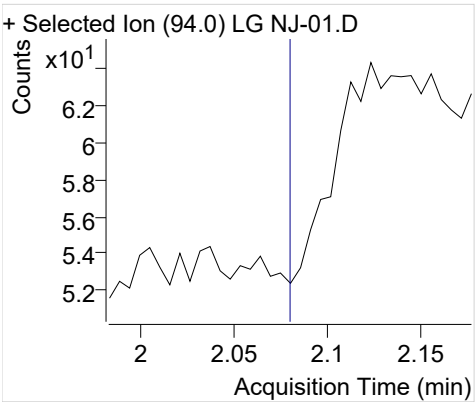





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-31 오후 1:54:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:17:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:54:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 10:43:30	**Data File**	LG NJ-02.D
Type	Sample	**Name**	LG NJ-02
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

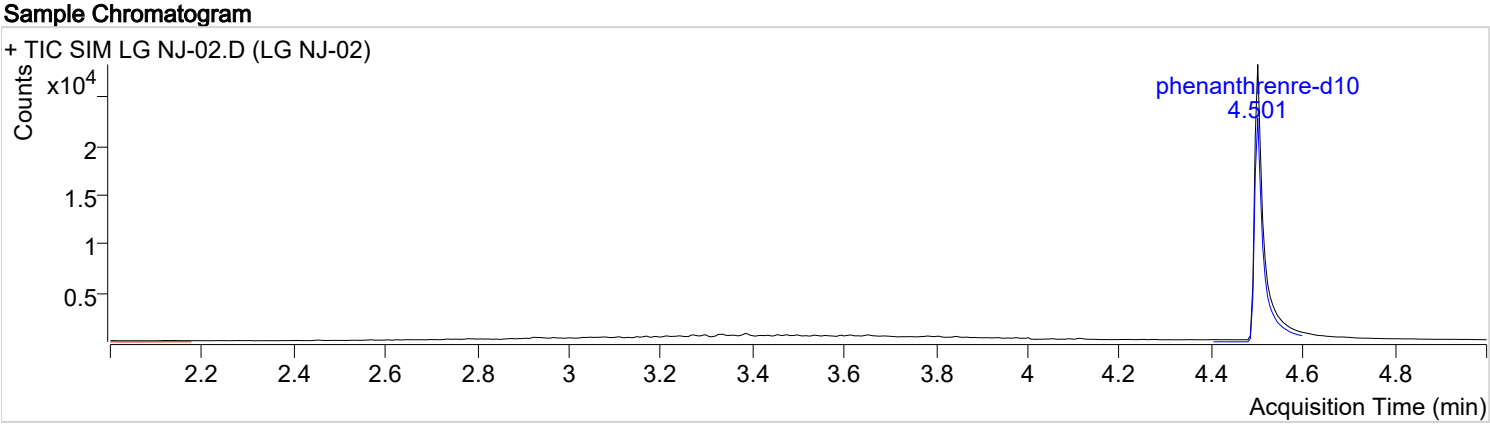

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			31800	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-31 오후 1:54:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:17:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:54:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 10:51:50	**Data File**	LG NJ-03.D
Type	Sample	**Name**	LG NJ-03
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

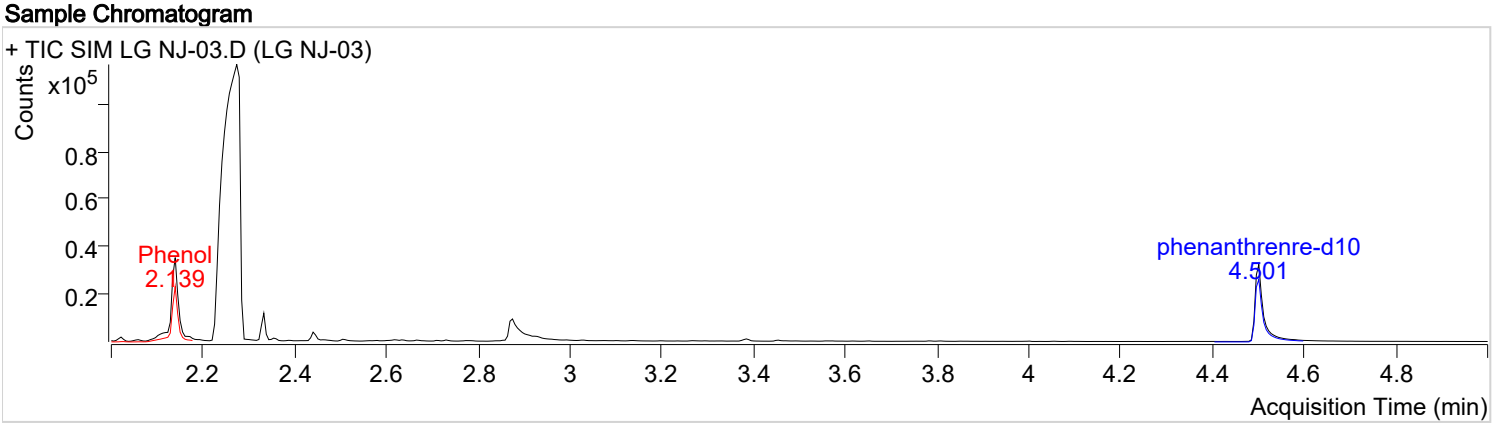

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.139	0	32739	ND mg/L

Phenol



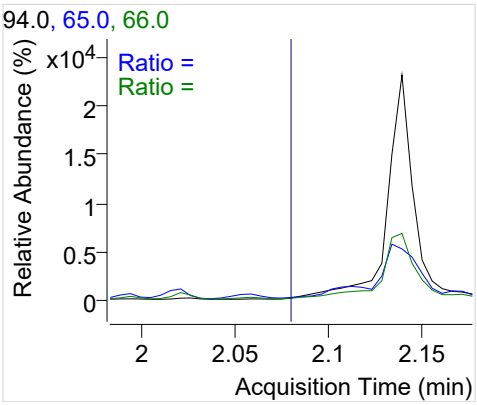

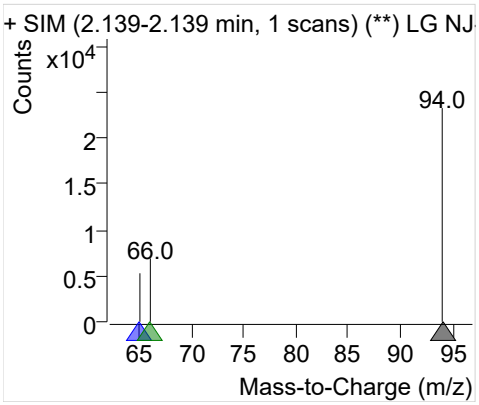

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-31 오후 1:54:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:17:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:54:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 11:00:11	**Data File**	LG NJ-04.D
Type	Sample	**Name**	LG NJ-04
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

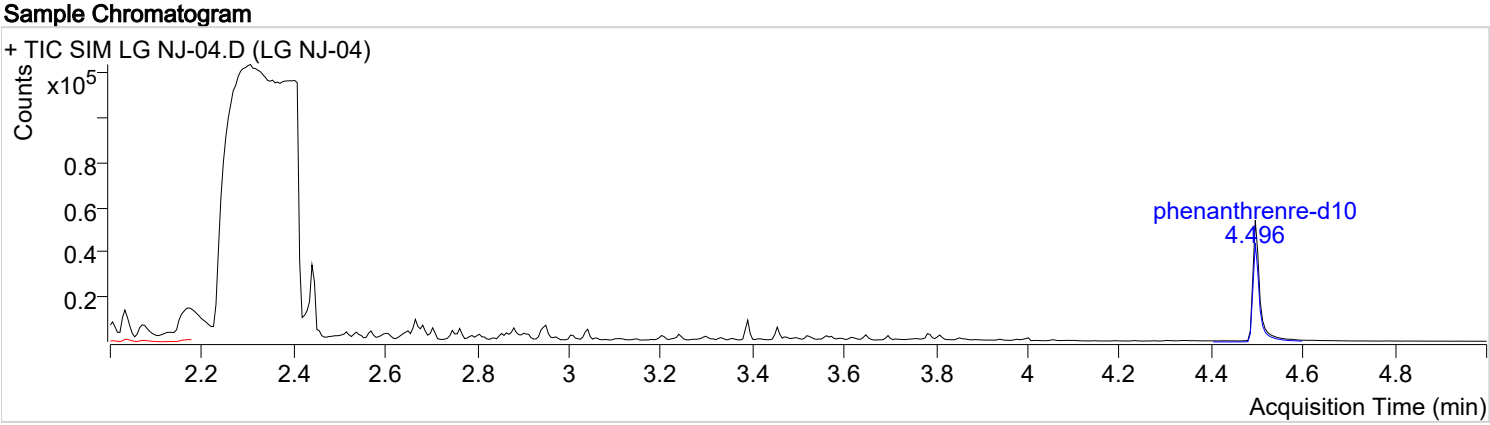

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			45705	ND mg/L

Phenol

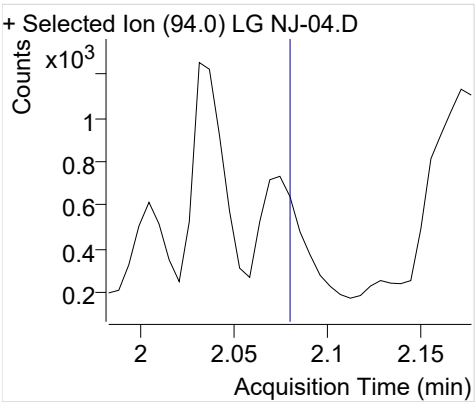





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-31 오후 1:54:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:17:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:54:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 11:08:32	**Data File**	LG NJ-05.D
Type	Sample	**Name**	LG NJ-05
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

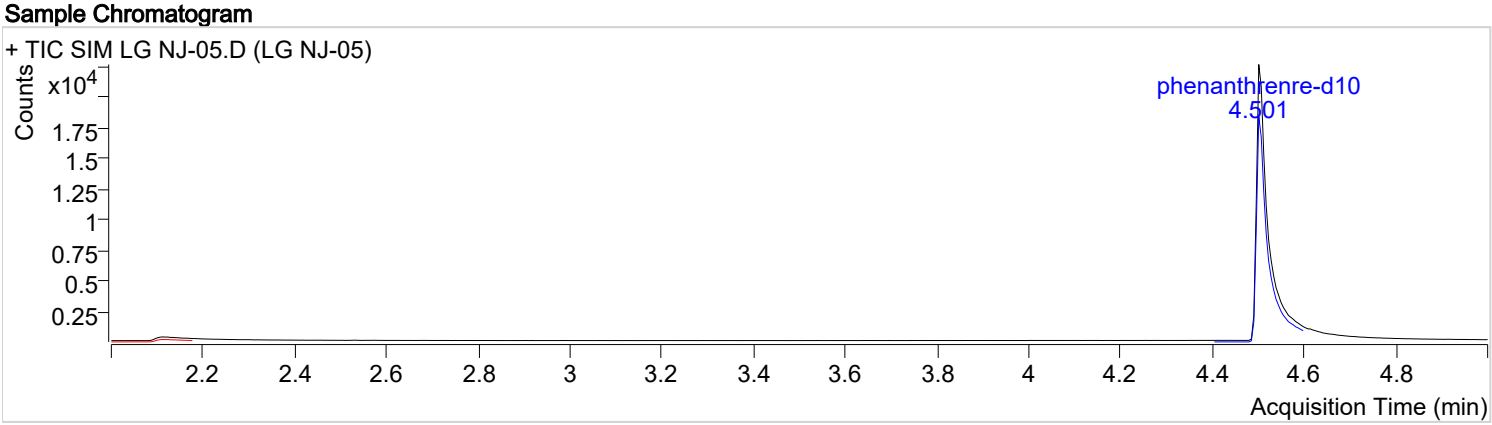

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			34019	ND mg/L

Phenol



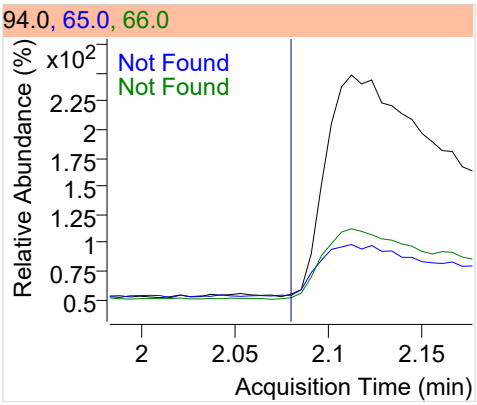

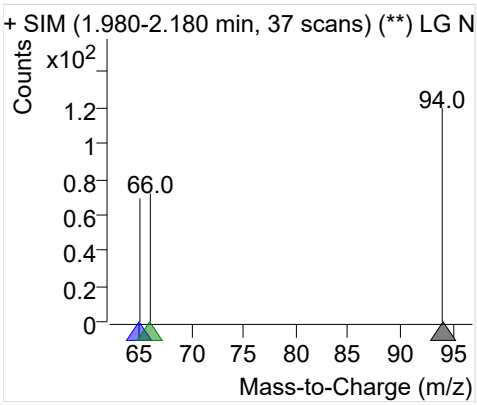

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-31 오후 1:54:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:17:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:54:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 11:16:55	**Data File**	LG NJ-06.D
Type	Sample	**Name**	LG NJ-06
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

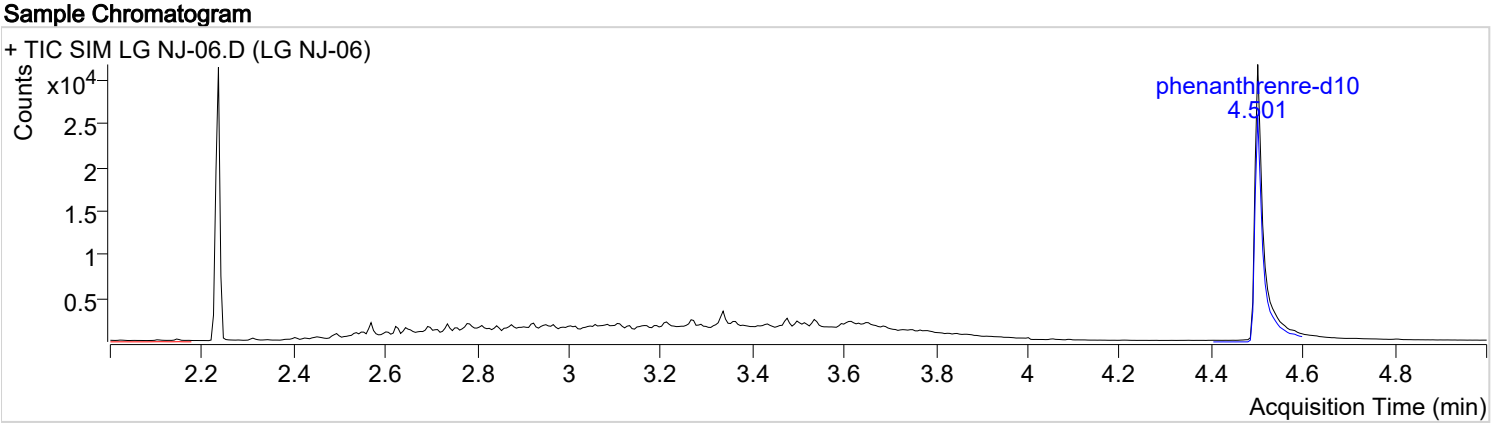

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			33268	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-31 오후 1:54:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:17:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:54:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 11:25:16	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

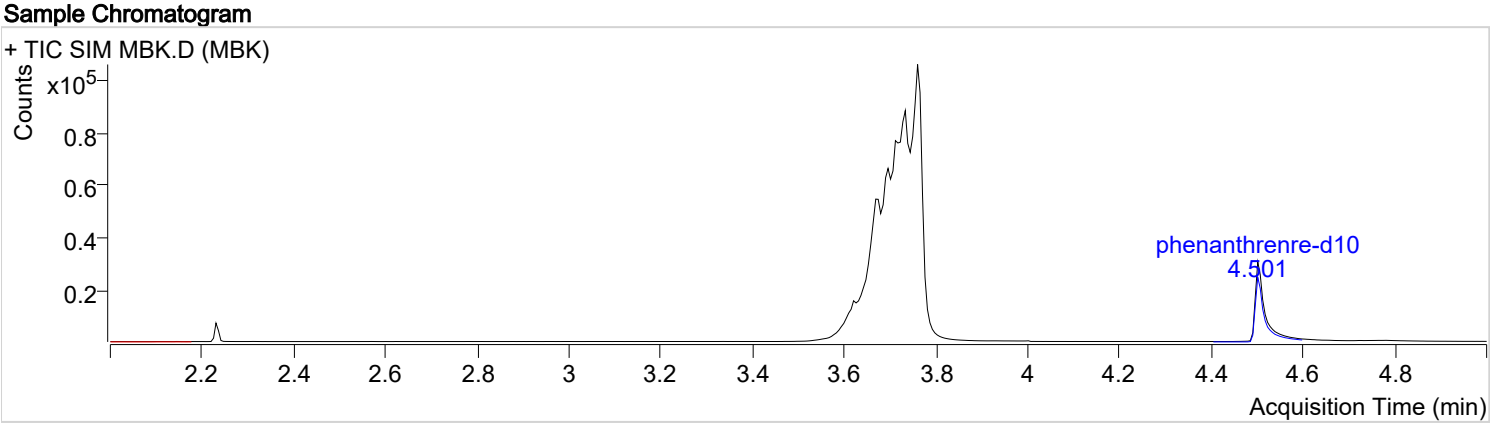

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			37179	ND mg/L

Phenol

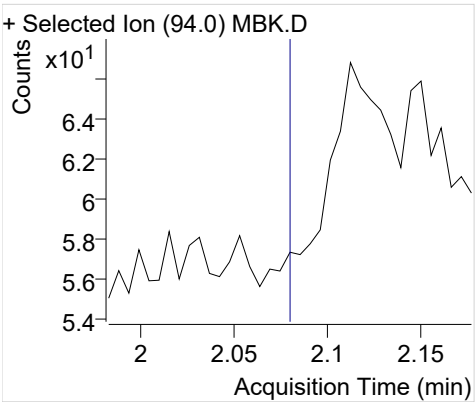



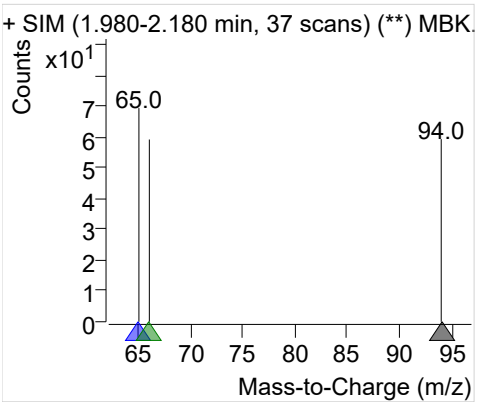

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PHENOL(NJ 3.26)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-31 오후 1:54:57	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:17:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-31 오후 1:54:57	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-31 오전 11:41:59	**Data File**	-CCV-.D
Type	QC	**Name**	-CCV-
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

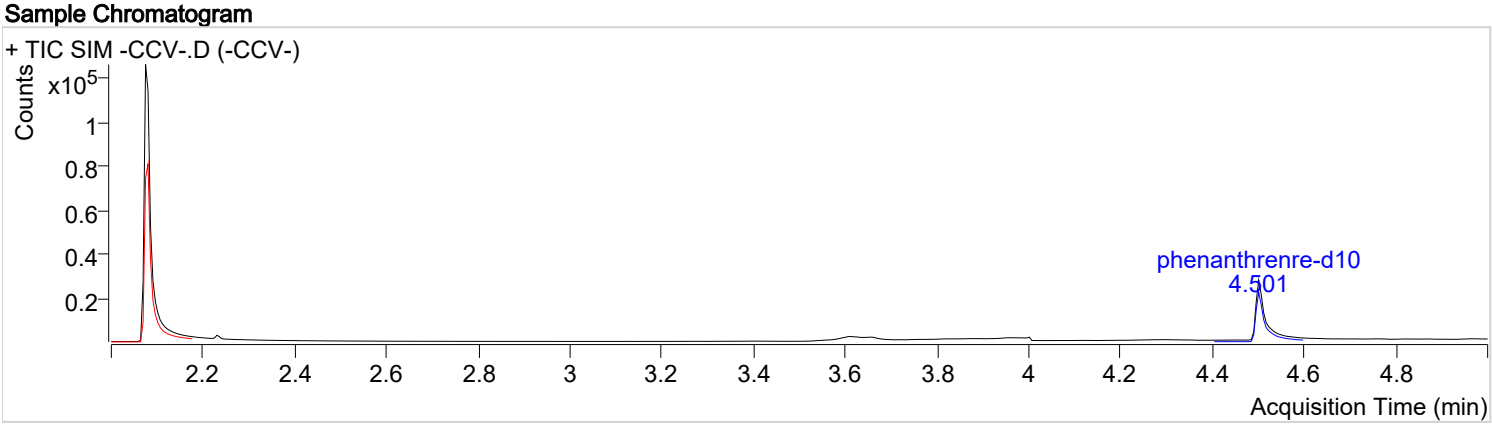

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.080	83824	31582	0.019 mg/L
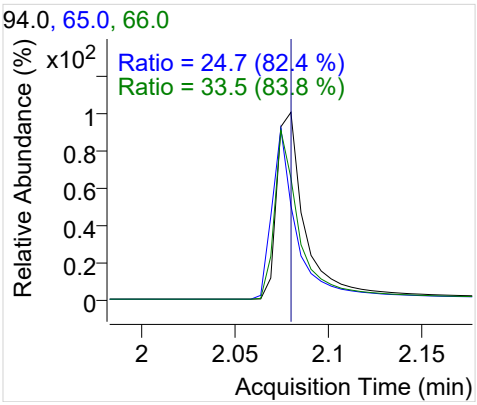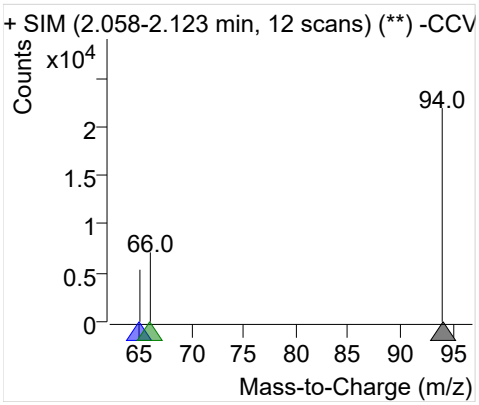
Phenol