Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\QuantResults\PHENOL.batch.bin				
Analysis Time	2026-01-08 오전 11:49:10	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:49:10	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Phenol

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
PHENOL ST-01.d	Cal	2.323	60378	73721	0.005
PHENOL ST-02.d	Cal	2.318	128792	72872	0.010
PHENOL ST-03.d	Cal	2.318	218506	158270	0.008
PHENOL ST-04.d	Cal	2.318	289044	75306	0.020
PHENOL ST-05.d	Cal	2.318	420004	72474	0.029
PHENOL ST-06.d	Cal	2.318	575964	71587	0.040
BK-.d	Blank			73789	ND
FBK(HN 25-12-29).d	Blank			71828	ND
HN 25-12-29.d	Sample			72394	ND
FBK(PL 25-12-30).d	Blank			78758	ND
PL-01.d	Sample			90806	ND
PL-02.d	Sample			71537	ND
JR 26-01-02.d	Sample			86985	ND
MBK.d	Blank			83320	ND
-C-C-V-.d	QC	2.318	292615	79359	0.019

Phenol

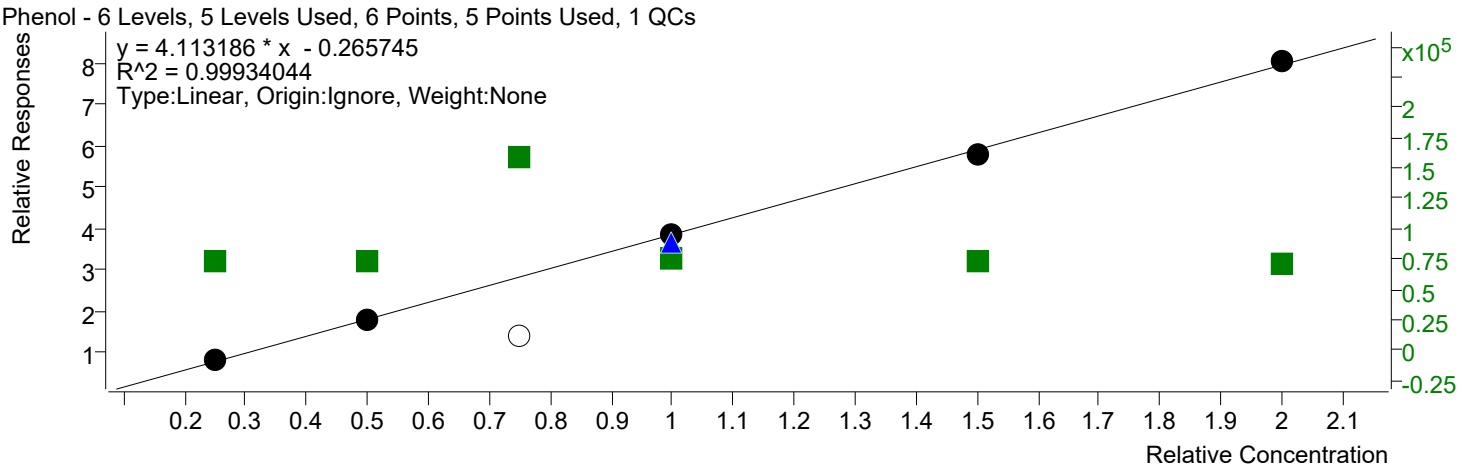

Cal. Path	Type	Level	Enable	Conc.	Response
V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\PHENOL ST-01.d	Calibration	1	x	2.500	60378
V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\PHENOL ST-02.d	Calibration	2	x	5.000	128792
V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\PHENOL ST-03.d	Calibration	3		7.500	218506
V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\PHENOL ST-04.d	Calibration	4	x	10.000	289044
V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\-C-C-V-.d	QC	4	x	10.000	292615
V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\PHENOL ST-05.d	Calibration	5	x	15.000	420004
V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\PHENOL ST-06.d	Calibration	6	x	20.000	575964

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-01-08 오전 11:49:10	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:19:37	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:49:10	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오전 10:03:35	**Data File**	PHENOL ST-01.d
Type	Cal	**Name**	PHENOL ST-01
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

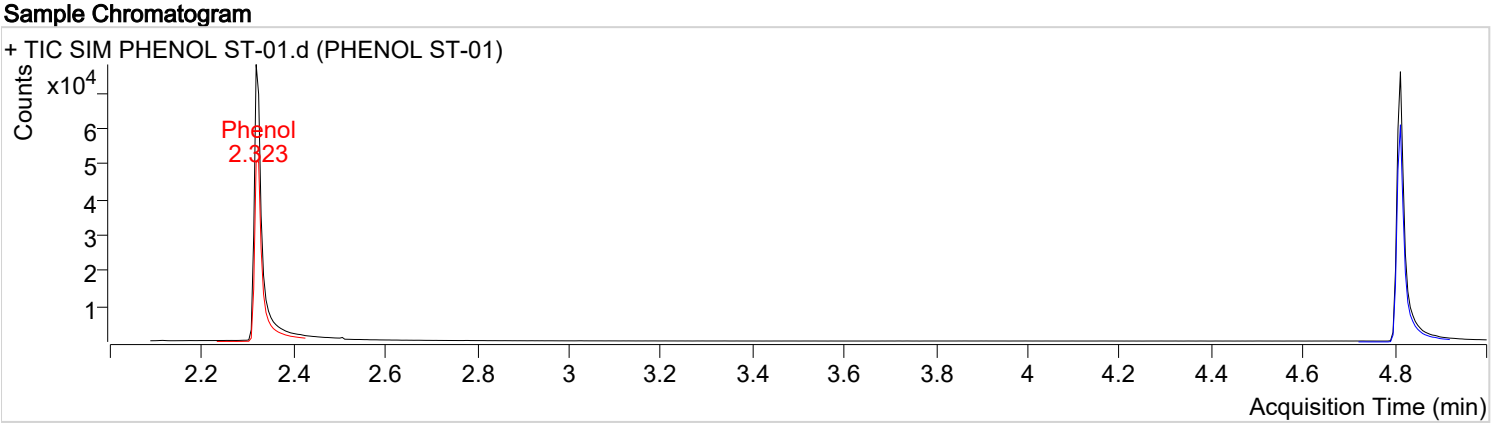

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.323	60378	73721	0.005 mg/L

Phenol







Generated at 오전 10:19 on 2026-04-10

Quant Sample Report

Batch Data Path	V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-01-08 오전 11:49:10	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:19:37	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:49:10	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오전 10:11:52	**Data File**	PHENOL ST-02.d
Type	Cal	**Name**	PHENOL ST-02
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

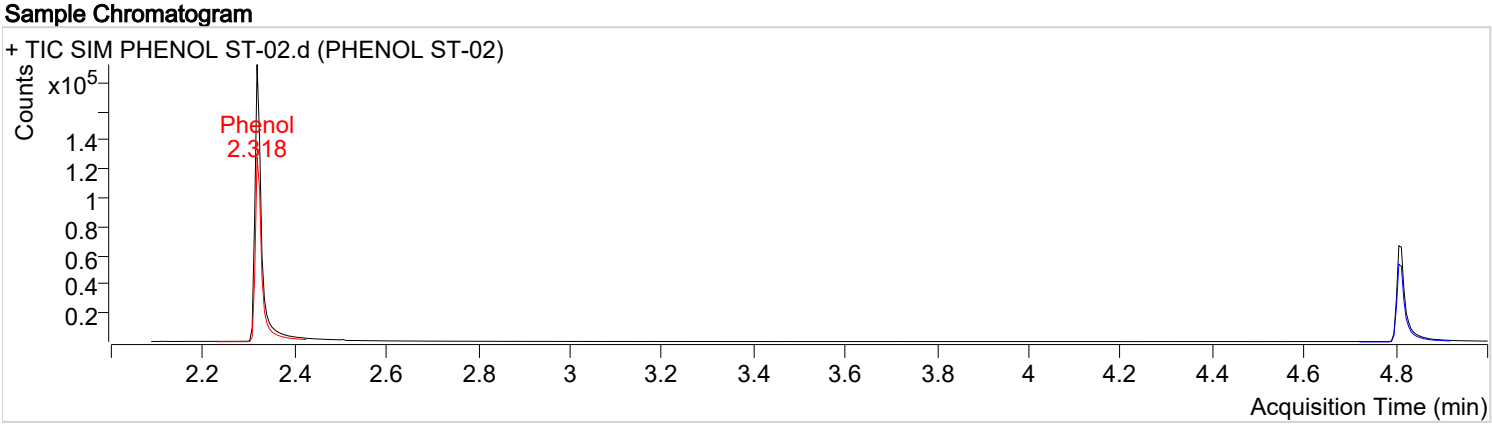

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.318	128792	72872	0.010 mg/L

Phenol



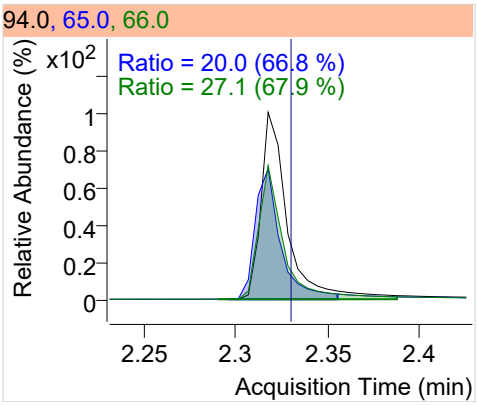



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-01-08 오전 11:49:10	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:19:37	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:49:10	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오전 10:20:10	**Data File**	PHENOL ST-03.d
Type	Cal	**Name**	PHENOL ST-03
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

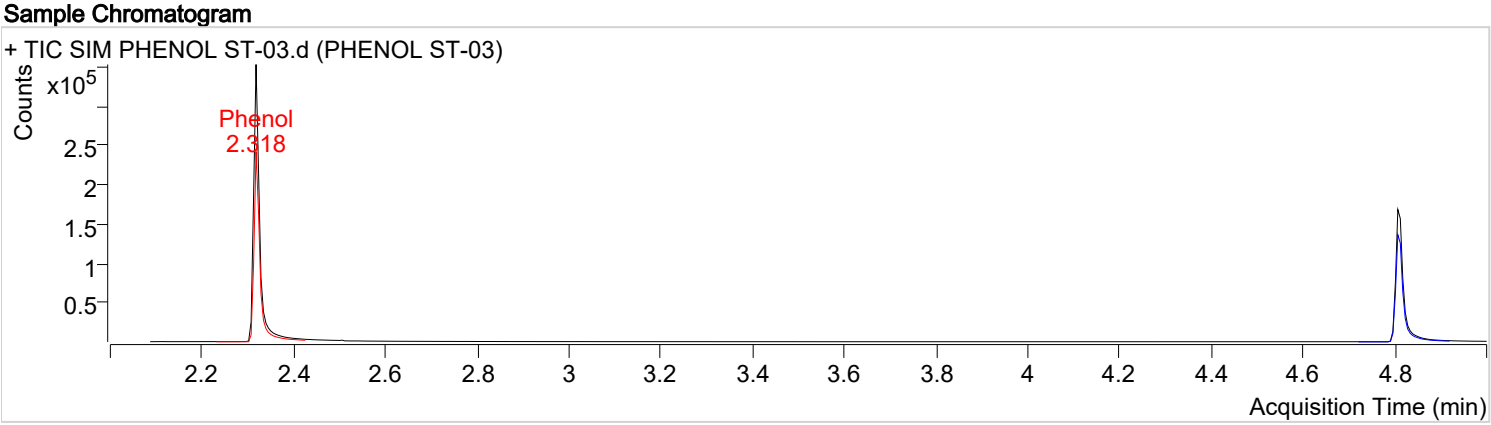

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.318	218506	158270	0.008 mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-01-08 오전 11:49:10	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:19:37	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:49:10	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오전 10:28:28	**Data File**	PHENOL ST-04.d
Type	Cal	**Name**	PHENOL ST-04
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

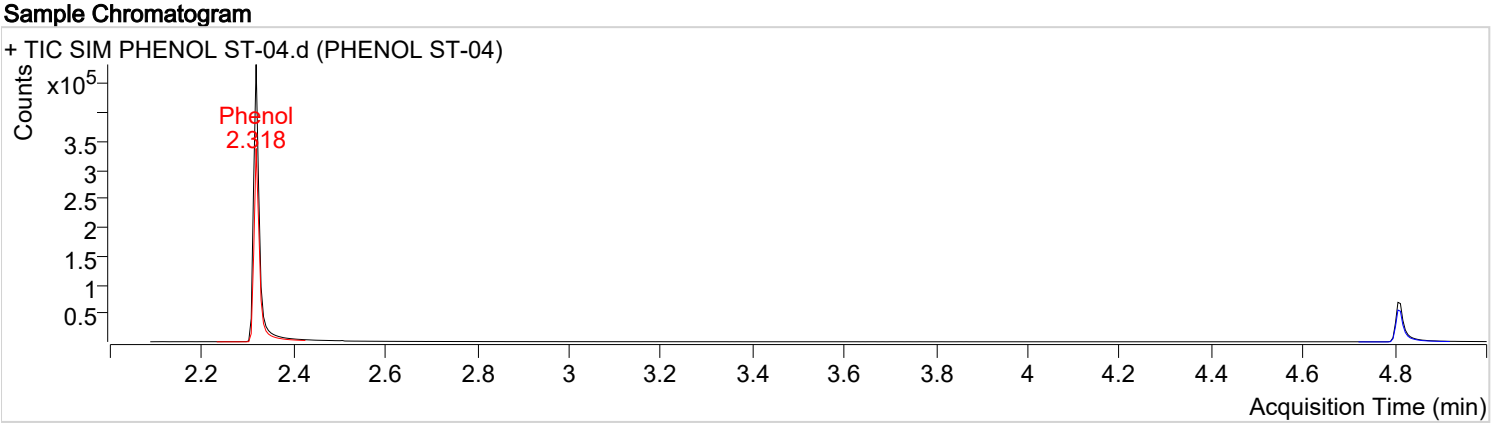

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.318	289044	75306	0.020 mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-01-08 오전 11:49:10	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:19:37	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:49:10	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오전 10:36:47	**Data File**	PHENOL ST-05.d
Type	Cal	**Name**	PHENOL ST-05
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

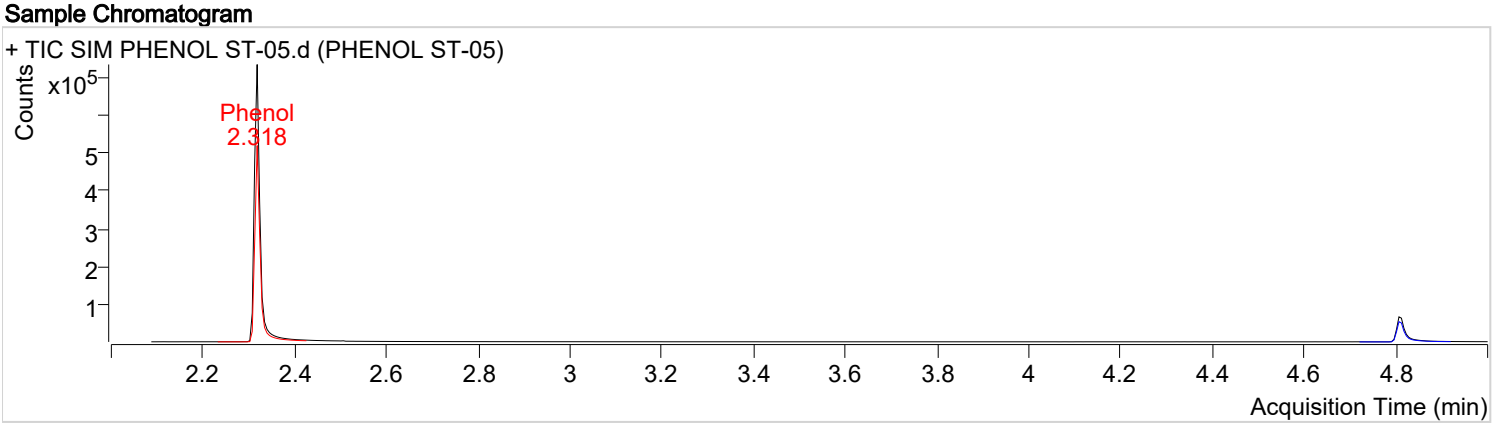

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.318	420004	72474	0.029 mg/L

Phenol







Quant Sample Report

Batch Data Path	V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-01-08 오전 11:49:10	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:19:37	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:49:10	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오전 10:45:11	**Data File**	PHENOL ST-06.d
Type	Cal	**Name**	PHENOL ST-06
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

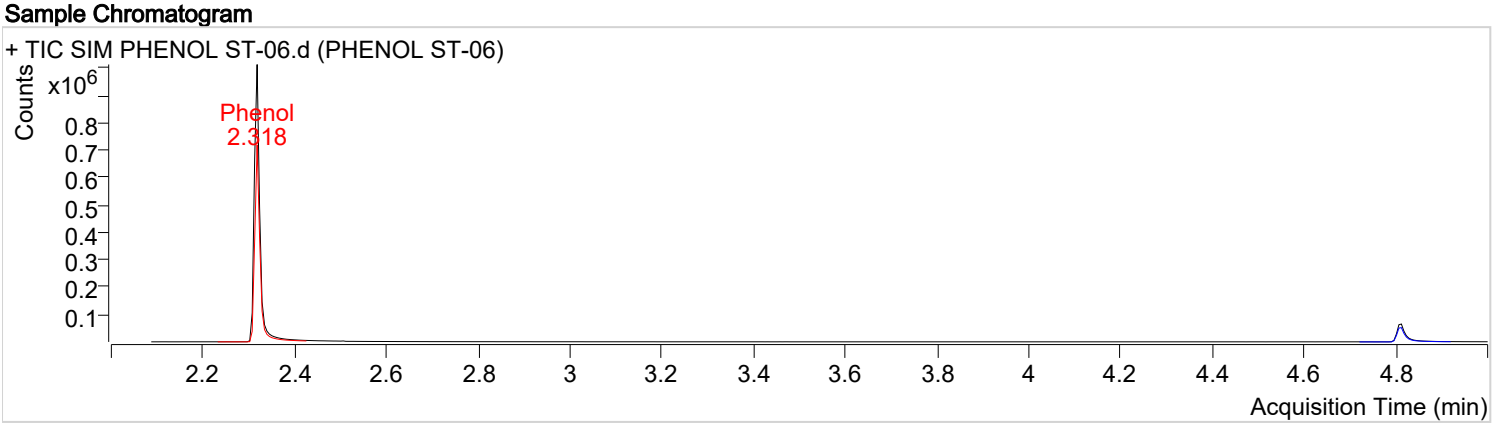

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.318	575964	71587	0.040 mg/L

Phenol







Quant Sample Report

Batch Data Path	V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-01-08 오전 11:49:10	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:19:37	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:49:10	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오전 11:01:50	**Data File**	BK-.d
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

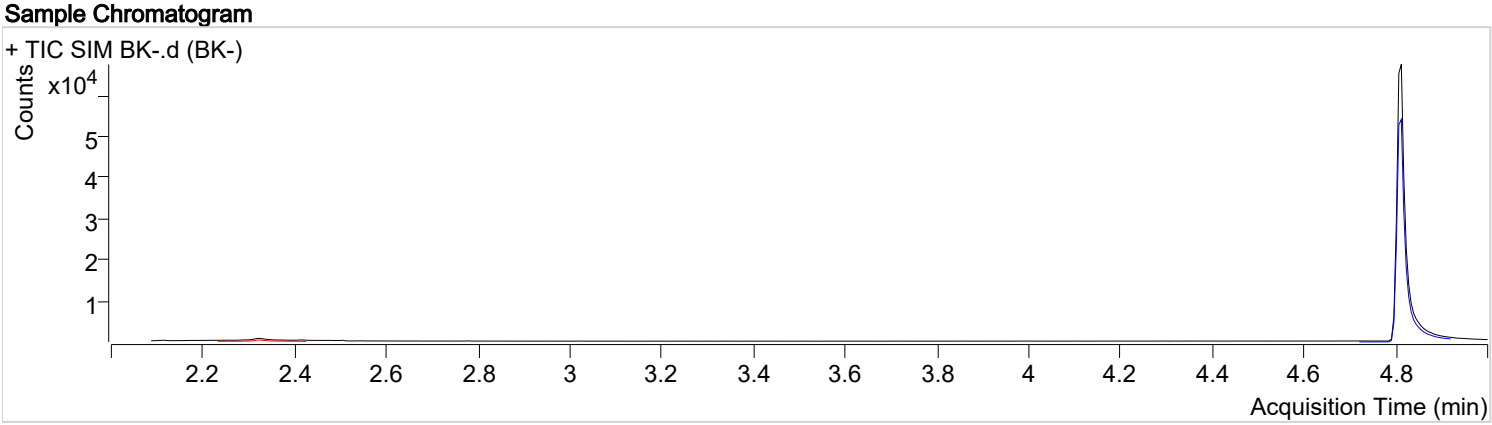

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			73789	ND mg/L

Phenol

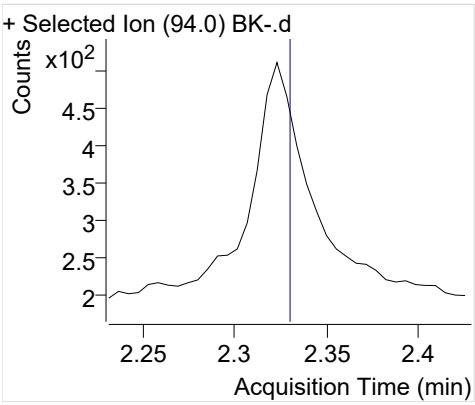





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-01-08 오전 11:49:10	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:19:37	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:49:10	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오전 11:10:12	**Data File**	FBK(HN 25-12-29).d
Type	Blank	**Name**	FBK(HN 25-12-29)
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

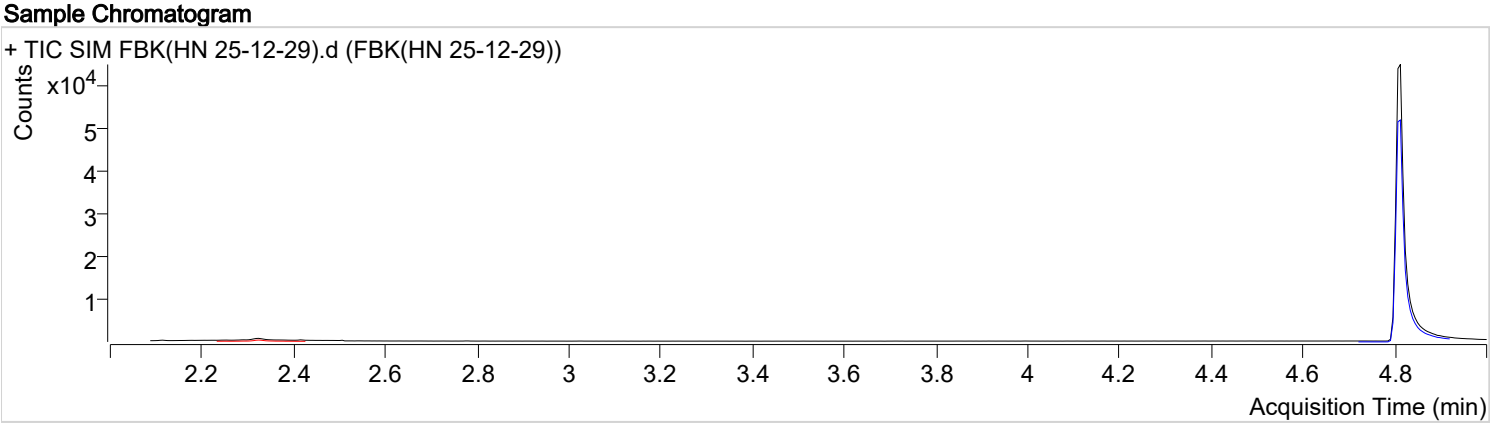

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			71828	ND mg/L

Phenol

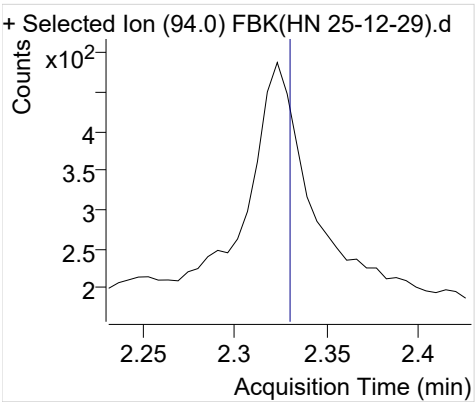





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-01-08 오전 11:49:10	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:19:37	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:49:10	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오전 11:18:31	**Data File**	HN 25-12-29.d
Type	Sample	**Name**	HN 25-12-29
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

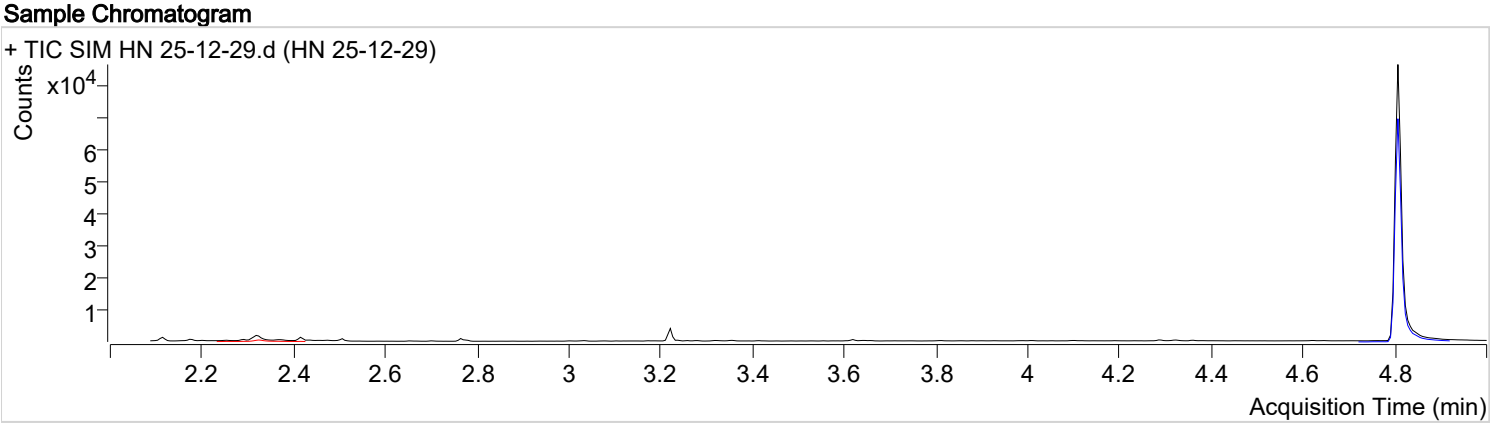

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			72394	ND mg/L

Phenol

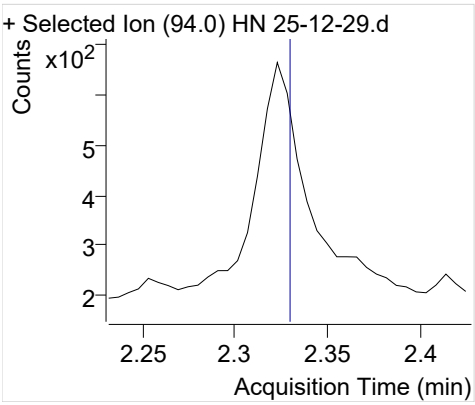





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-01-08 오전 11:49:10	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:19:37	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:49:10	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오전 11:26:54	**Data File**	FBK(PL 25-12-30).d
Type	Blank	**Name**	FBK(PL 25-12-30)
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

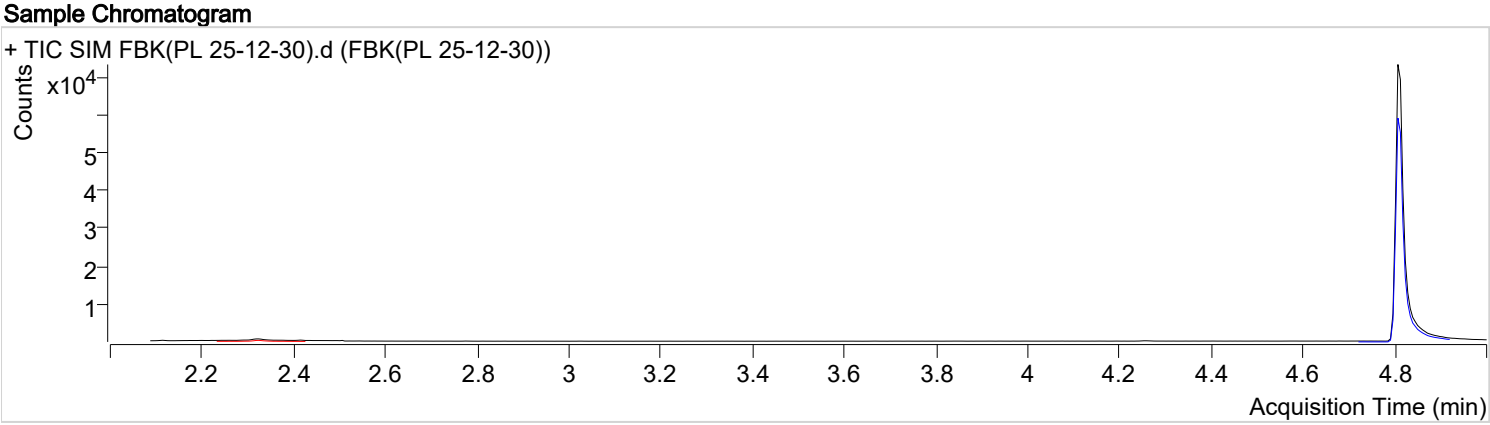

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			78758	ND mg/L

Phenol

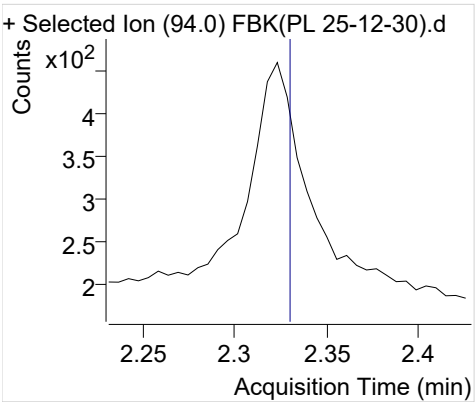





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-01-08 오전 11:49:10	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:19:37	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:49:10	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오전 11:35:13	**Data File**	PL-01.d
Type	Sample	**Name**	PL-01
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

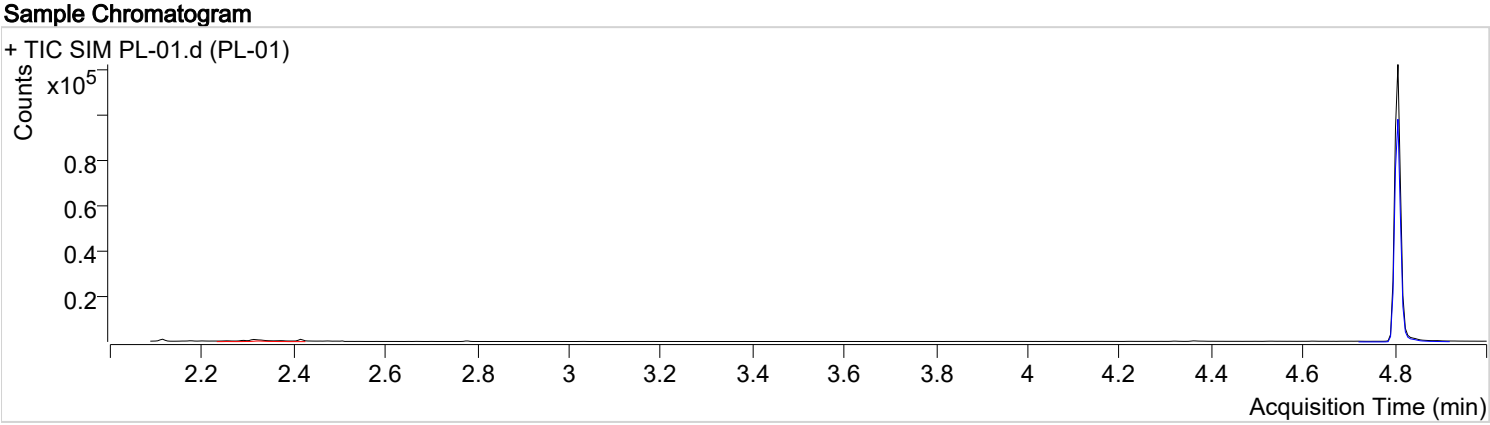

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			90806	ND mg/L

Phenol

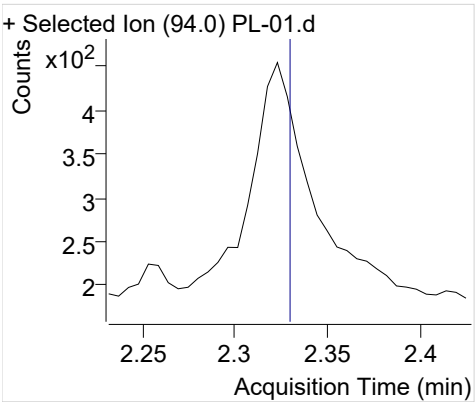





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-01-08 오전 11:49:10	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:19:37	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:49:10	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오전 11:43:31	**Data File**	PL-02.d
Type	Sample	**Name**	PL-02
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

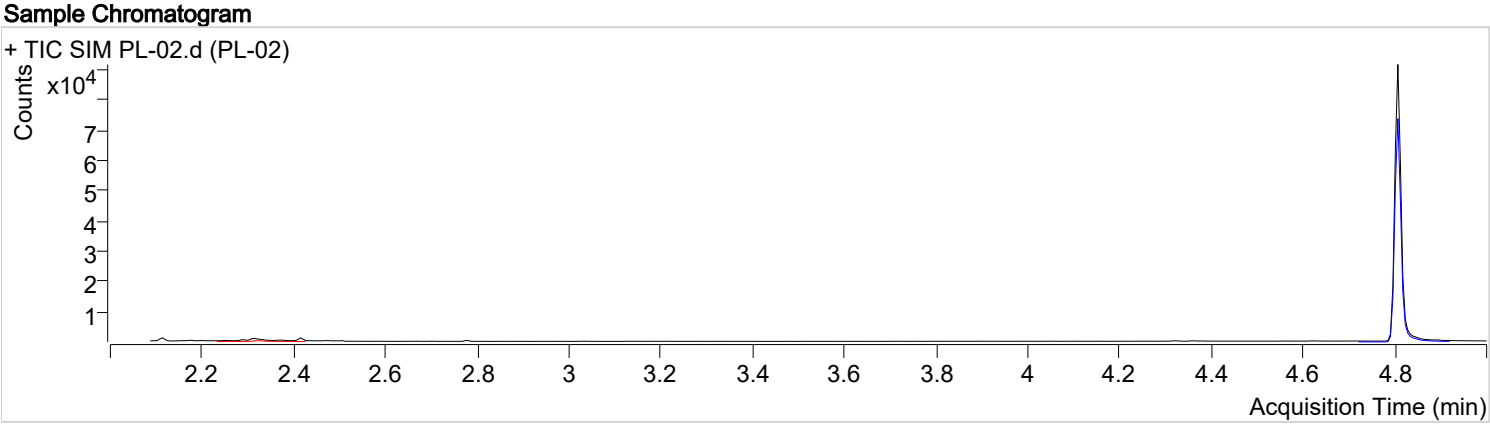

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			71537	ND mg/L

Phenol

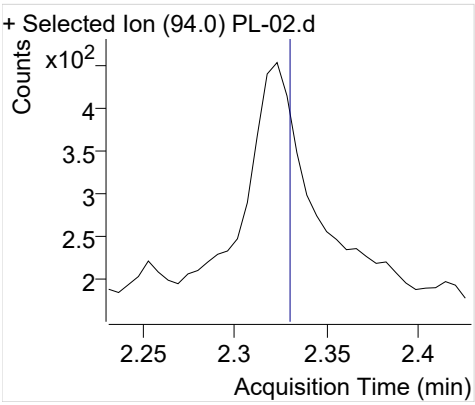

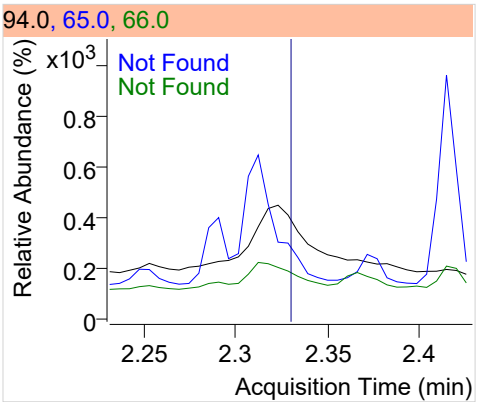



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-01-08 오전 11:49:10	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:19:37	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:49:10	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오전 11:51:52	**Data File**	JR 26-01-02.d
Type	Sample	**Name**	JR 26-01-02
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

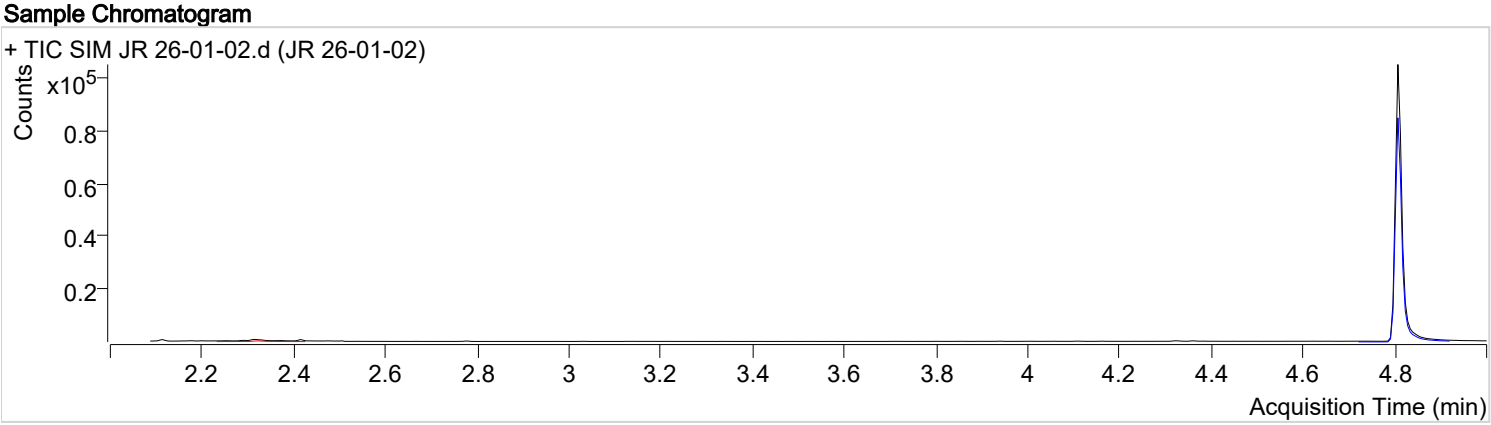

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			86985	ND mg/L

Phenol

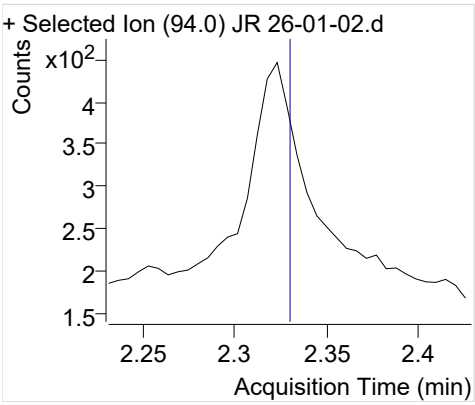





Quant Sample Report

Batch Data Path	V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-01-08 오전 11:49:10	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:19:37	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:49:10	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오후 12:00:13	**Data File**	MBK.d
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

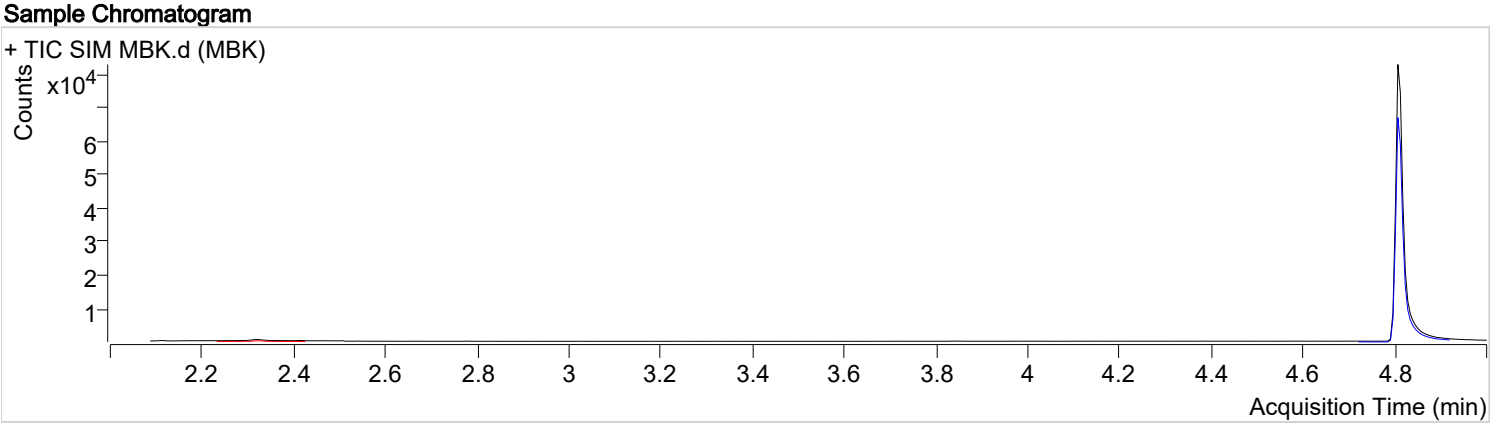

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			83320	ND mg/L

Phenol

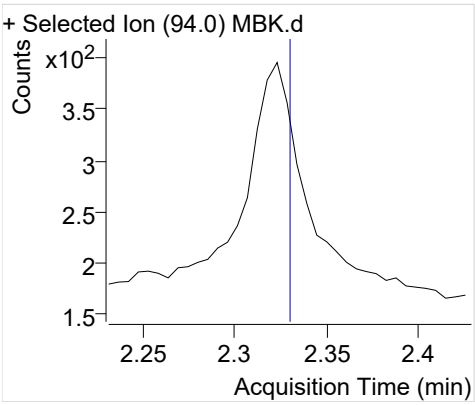





Quant Sample Report

Batch Data Path	V:\2026\2026-01\PHENOL(HN 12.29 PL 12.30 JR 1.2)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-01-08 오전 11:49:10	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:19:37	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-01-08 오전 11:49:10	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-01-06 오후 12:25:16	**Data File**	-C-C-V-.d
Type	QC	**Name**	-C-C-V-
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

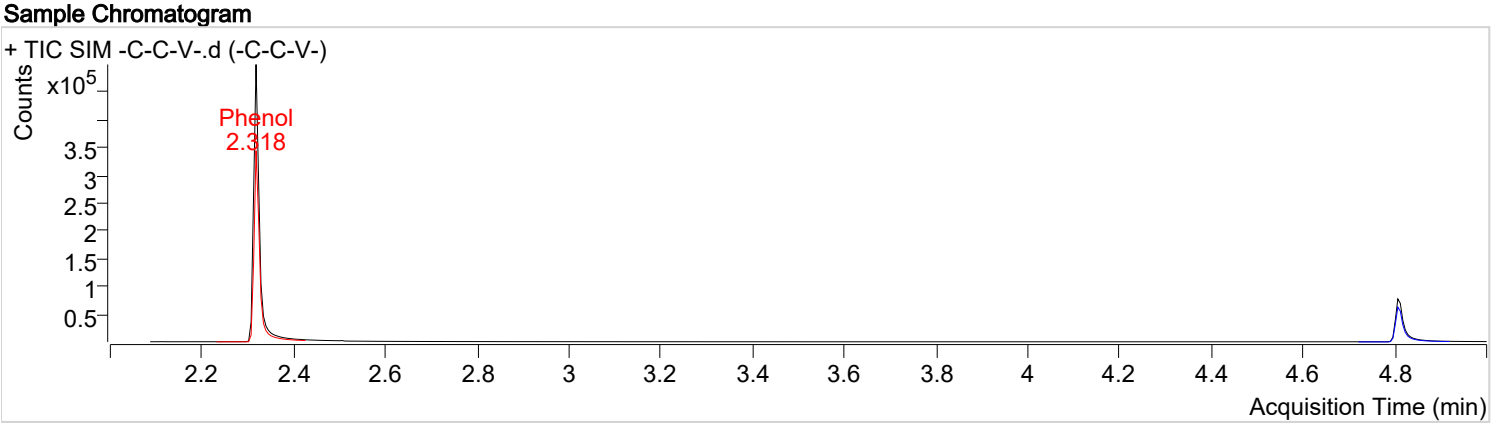

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.318	292615	79359	0.019 mg/L

Phenol