Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\QuantResults\PHENOL.batch.bin				
Analysis Time	2026-03-24 오전 11:19:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:19:37	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Phenol

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
PHENOL ST-01.d	Cal	2.339	46379	65022	0.005
PHENOL ST-02.d	Cal	2.334	81382	59718	0.010
PHENOL ST-03.d	Cal	2.328	130724	63038	0.015
PHENOL ST-04.d	Cal	2.323	182469	62386	0.020
PHENOL ST-05.d	Cal	2.323	269310	61688	0.030
PHENOL ST-06.d	Cal	2.323	349464	59987	0.040
BK-.d	Blank			60778	ND
FBK(RE 26-03-17).d	Blank			59692	ND
FBK(RE 26-03-18).d	Blank			61839	ND
RE-05.d	Sample			47907	ND
RE-06.d	Sample			53033	ND
RE-13.d	Sample			51513	ND
RE-14.d	Sample			65714	ND
RE-24.d	Sample			72061	ND
RE-25.d	Sample			47413	ND
JR 26-03-19.d	Sample			50772	ND
MBK.d	Blank			71308	ND
C-C-V.d	QC	2.323	189698	69773	0.019

Phenol

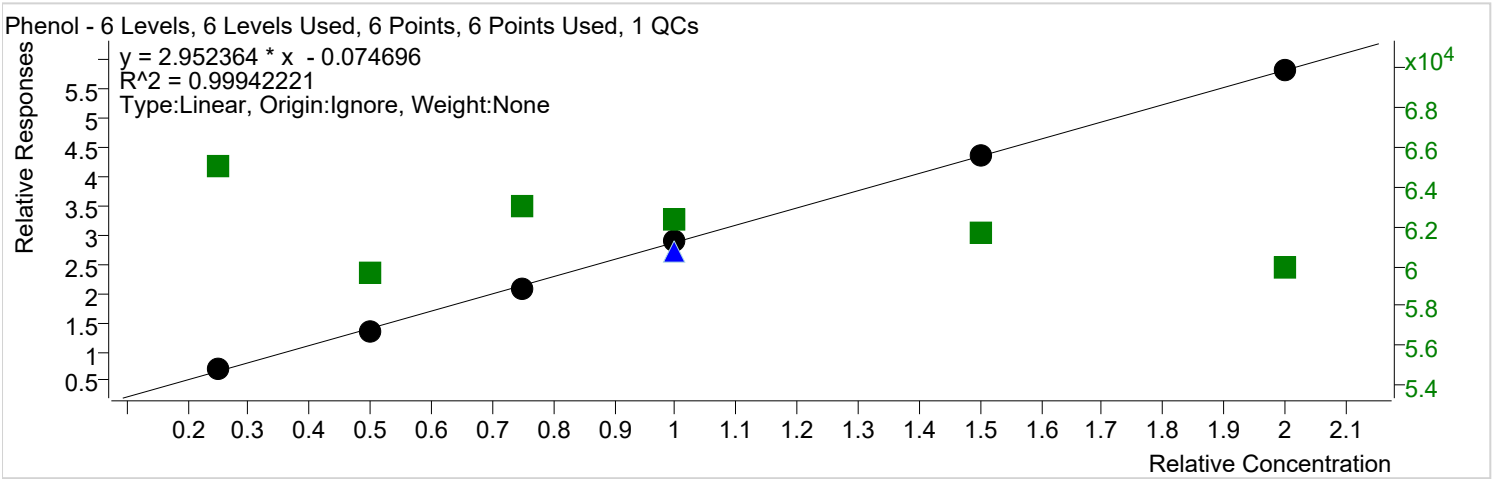

Cal. Path	Type	Level	Enable	Conc.	Response
V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\PHENOL ST-01.d	Calibration	1	x	2.500	46379
V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\PHENOL ST-02.d	Calibration	2	x	5.000	81382
V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\PHENOL ST-03.d	Calibration	3	x	7.500	130724
V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\PHENOL ST-04.d	Calibration	4	x	10.000	182469
V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\C-C-V.d	QC	4	x	10.000	189698
V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\PHENOL ST-05.d	Calibration	5	x	15.000	269310
V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\PHENOL ST-06.d	Calibration	6	x	20.000	349464

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-24 오전 11:19:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:21:04	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:19:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-20 오후 6:03:59	**Data File**	PHENOL ST-01.d
Type	Cal	**Name**	PHENOL ST-01
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

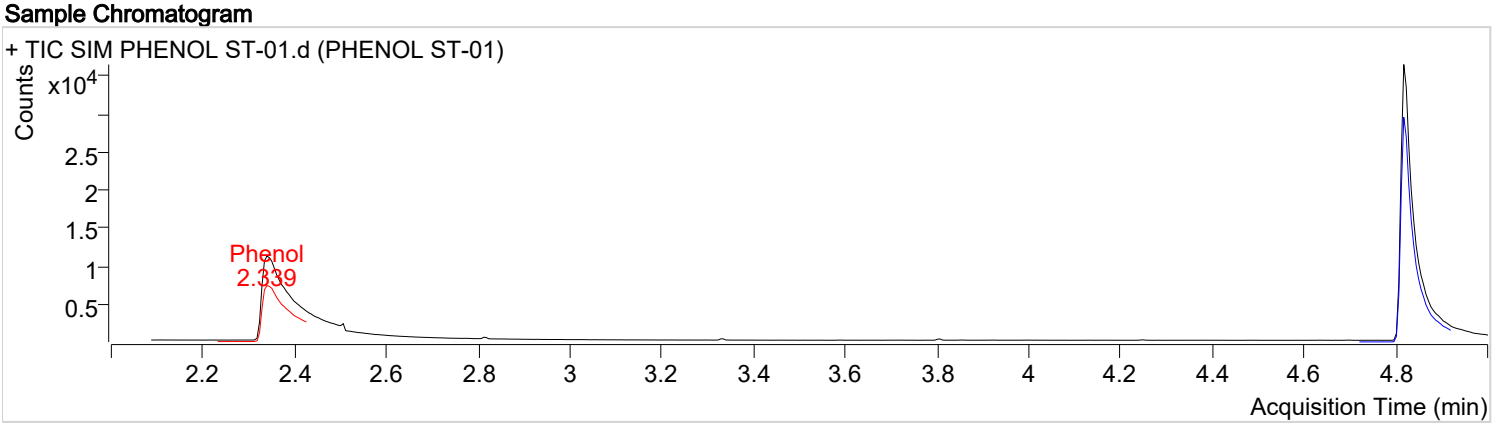

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.339	46379	65022	0.005 mg/L

Phenol



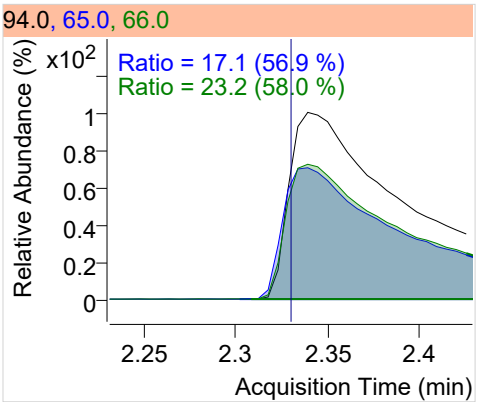



Quant Sample Report

Batch Data Path	V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-24 오전 11:19:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:21:04	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:19:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-20 오후 6:12:21	**Data File**	PHENOL ST-02.d
Type	Cal	**Name**	PHENOL ST-02
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

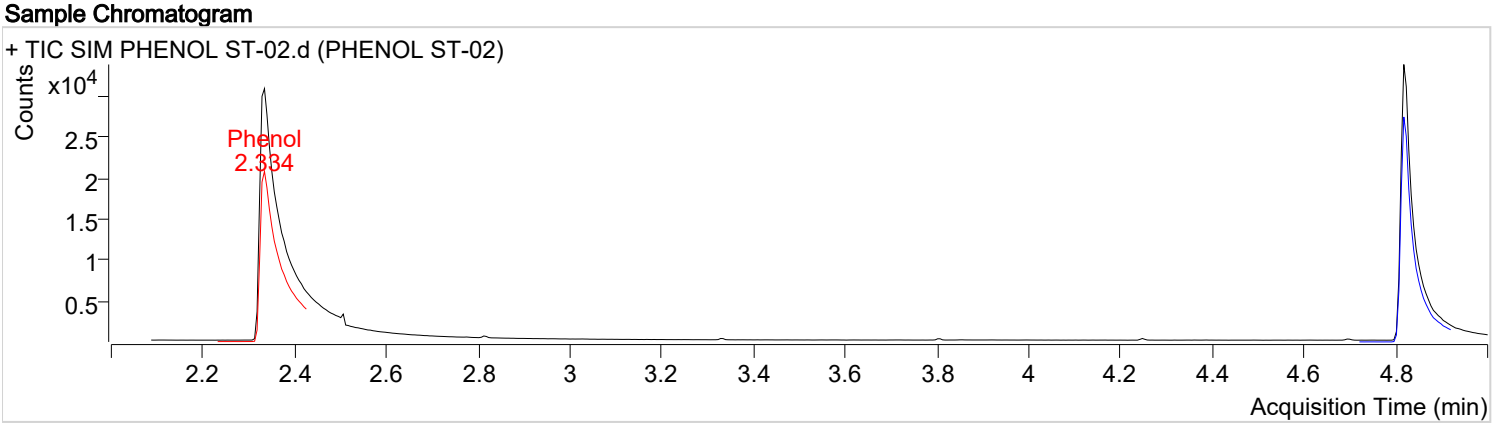

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.334	81382	59718	0.010 mg/L

Phenol



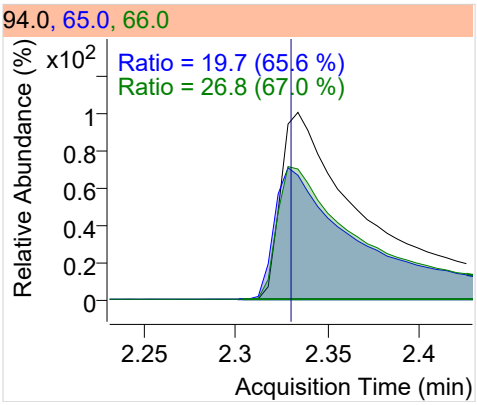



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-24 오전 11:19:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:21:04	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:19:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-20 오후 6:20:40	**Data File**	PHENOL ST-03.d
Type	Cal	**Name**	PHENOL ST-03
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

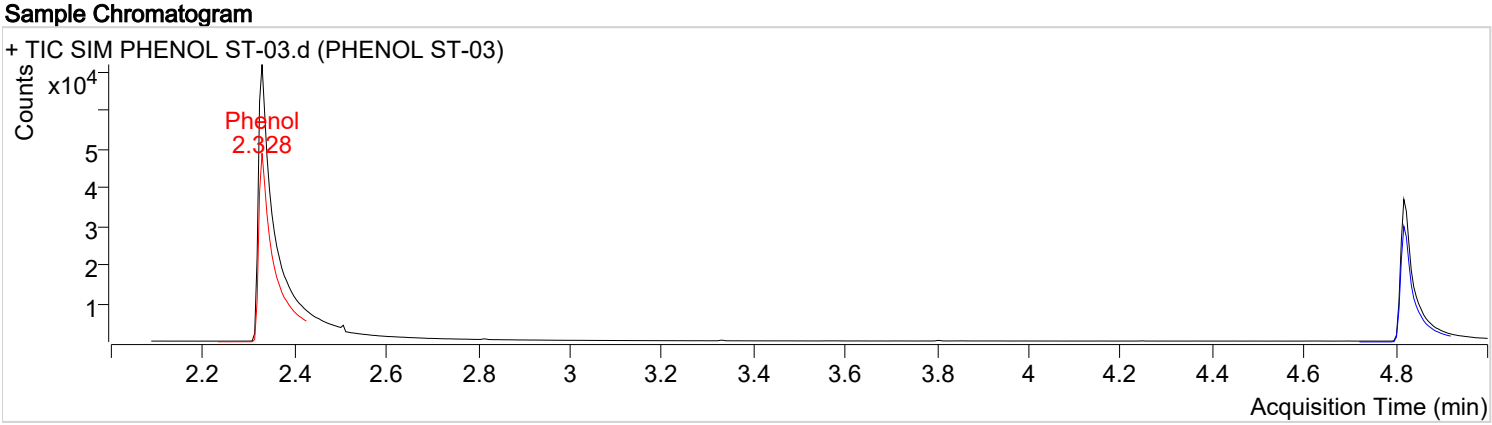

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.328	130724	63038	0.015 mg/L

Phenol



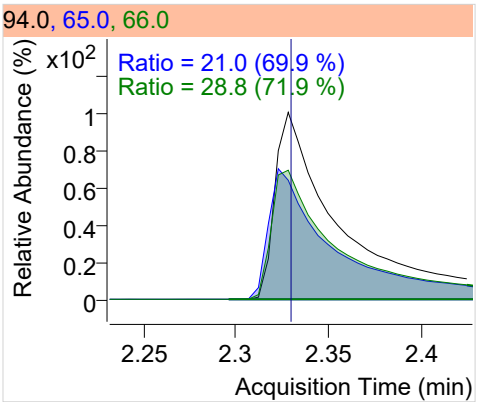



Quant Sample Report

Batch Data Path	V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-24 오전 11:19:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:21:04	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:19:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-20 오후 6:29:02	**Data File**	PHENOL ST-04.d
Type	Cal	**Name**	PHENOL ST-04
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

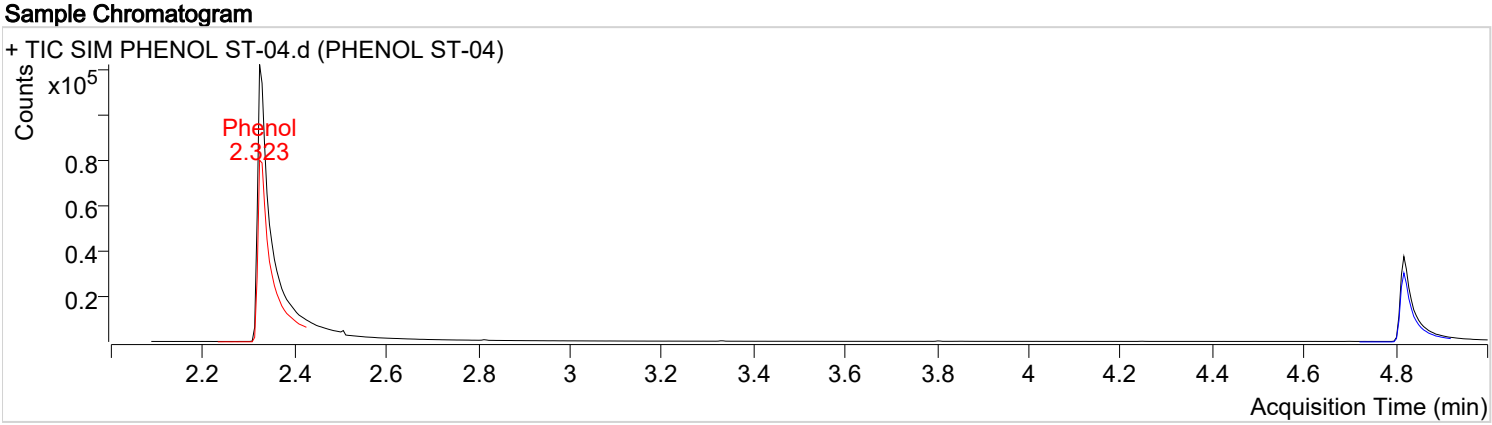

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.323	182469	62386	0.020 mg/L

Phenol



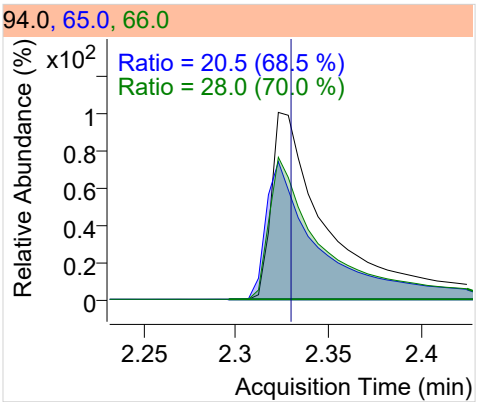



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-24 오전 11:19:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:21:04	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:19:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-20 오후 6:37:24	**Data File**	PHENOL ST-05.d
Type	Cal	**Name**	PHENOL ST-05
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

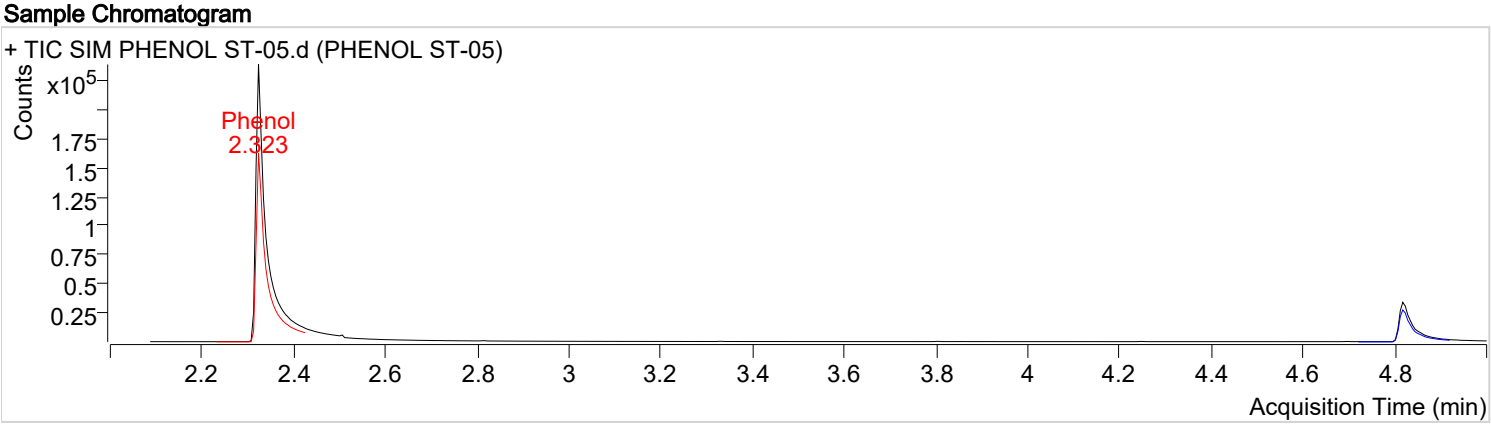

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.323	269310	61688	0.030 mg/L

Phenol







Quant Sample Report

Batch Data Path	V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-24 오전 11:19:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:21:04	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:19:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-20 오후 6:45:45	**Data File**	PHENOL ST-06.d
Type	Cal	**Name**	PHENOL ST-06
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

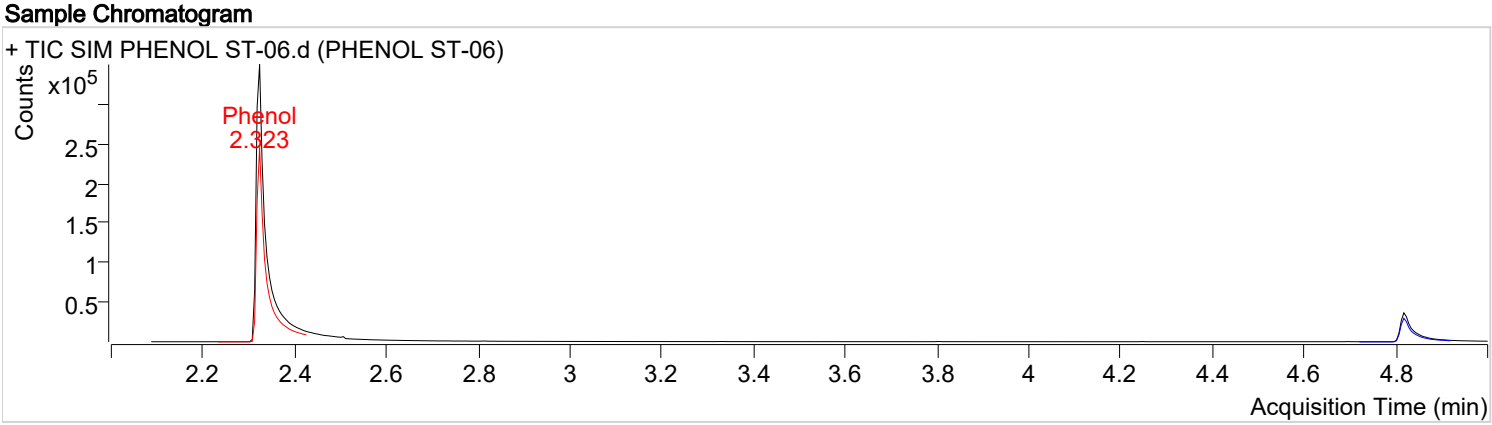

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.323	349464	59987	0.040 mg/L

Phenol



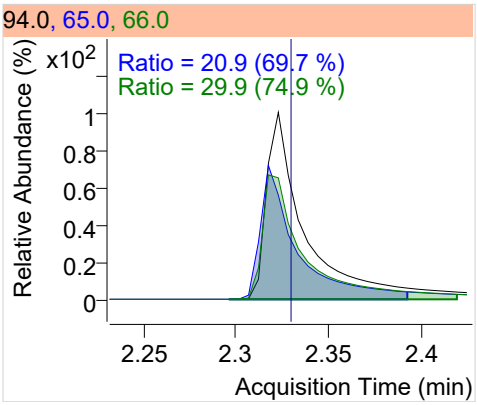



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-24 오전 11:19:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:21:04	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:19:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-20 오후 7:02:24	**Data File**	BK-.d
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

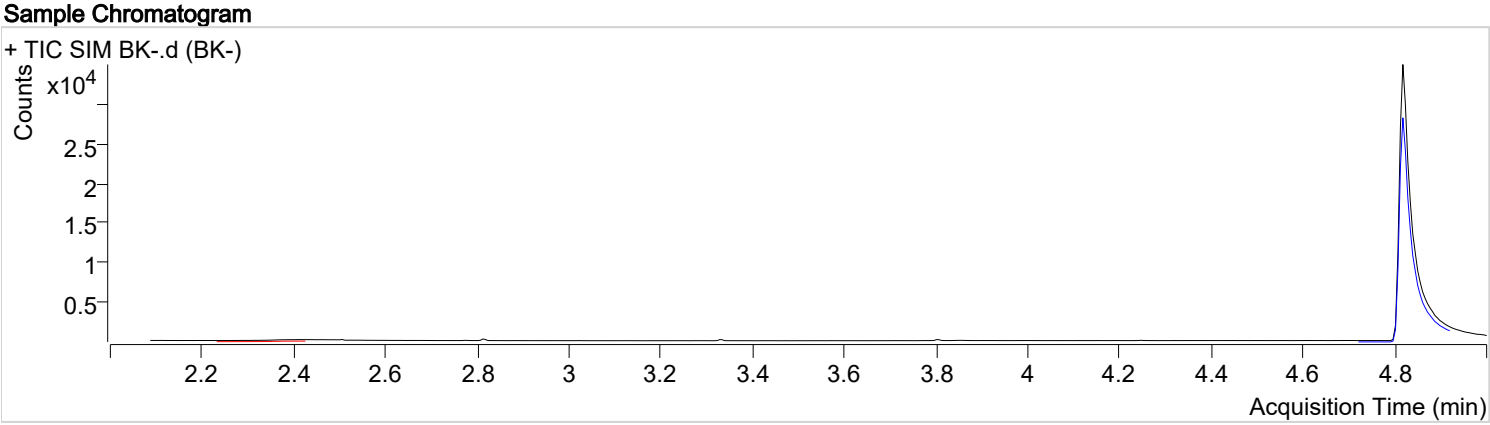

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			60778	ND mg/L

Phenol







Quant Sample Report

Batch Data Path	V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-24 오전 11:19:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:21:04	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:19:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-20 오후 7:10:46	**Data File**	FBK(RE 26-03-17).d
Type	Blank	**Name**	FBK(RE 26-03-17)
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

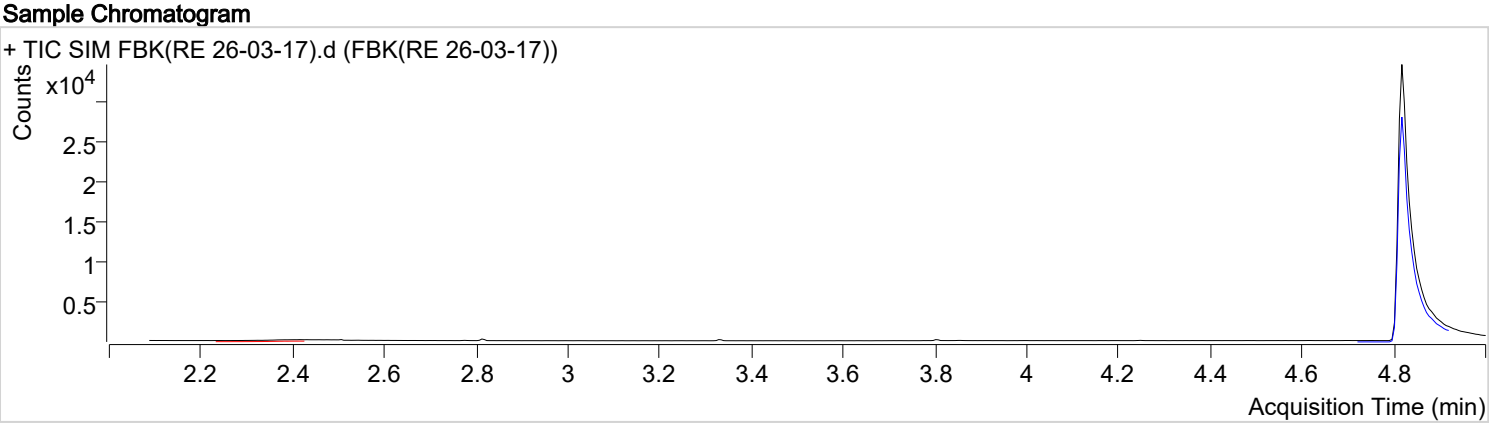

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			59692	ND mg/L

Phenol







Quant Sample Report

Batch Data Path	V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-24 오전 11:19:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:21:04	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:19:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-20 오후 7:19:05	**Data File**	FBK(RE 26-03-18).d
Type	Blank	**Name**	FBK(RE 26-03-18)
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

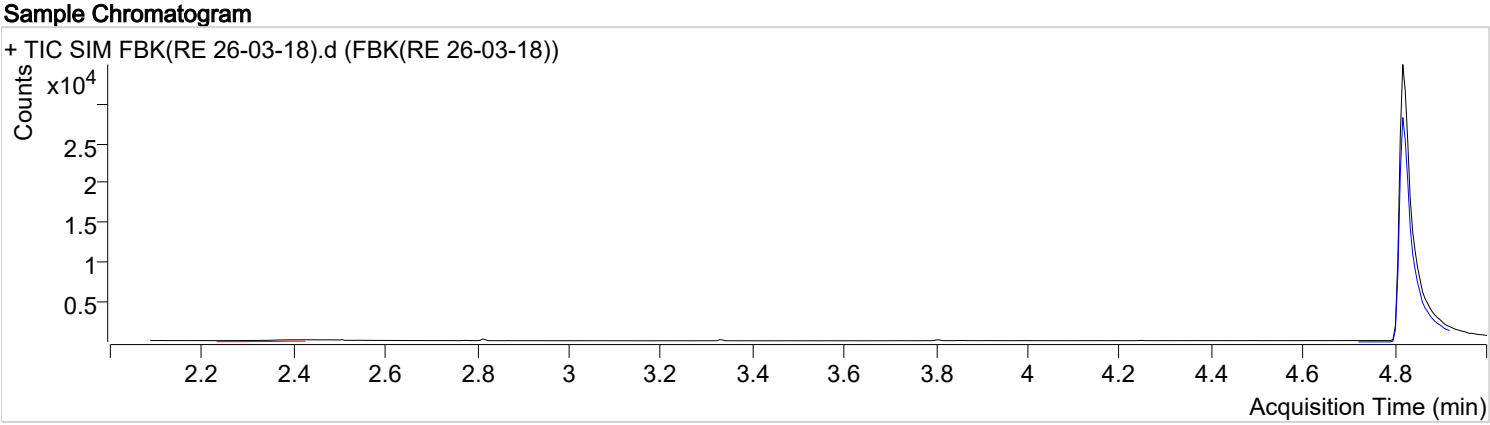

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			61839	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-24 오전 11:19:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:21:04	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:19:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-20 오후 7:27:24	**Data File**	RE-05.d
Type	Sample	**Name**	RE-05
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

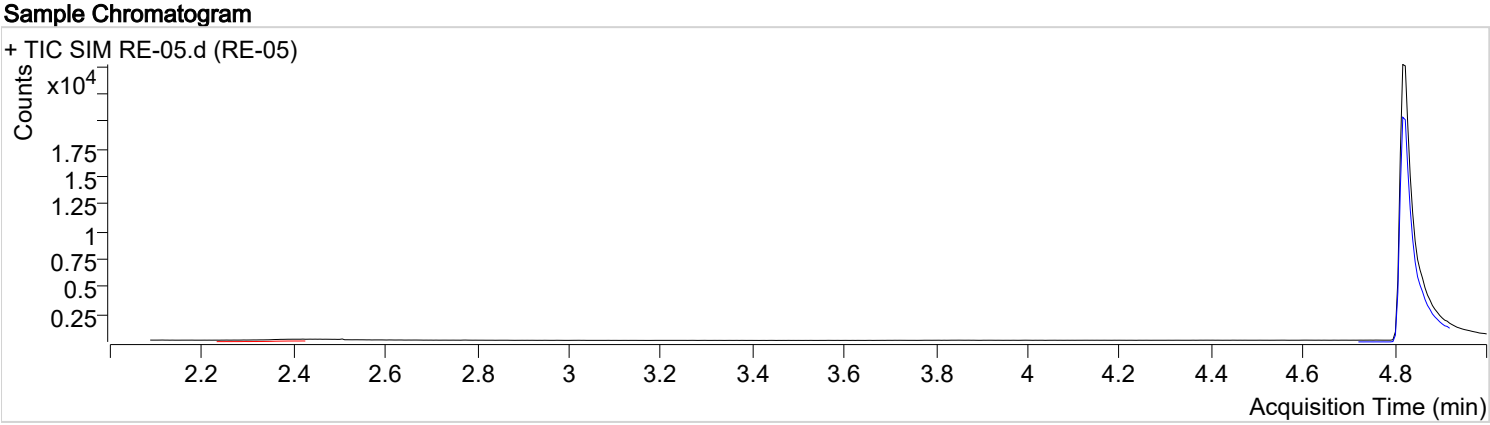

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			47907	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-24 오전 11:19:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:21:04	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:19:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-20 오후 7:35:48	**Data File**	RE-06.d
Type	Sample	**Name**	RE-06
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

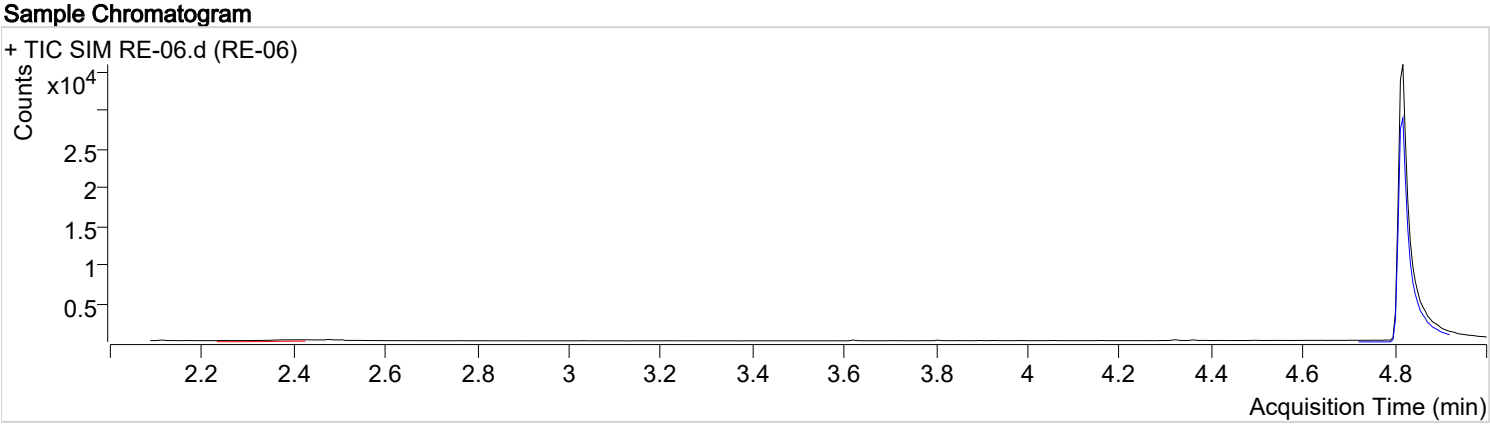

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			53033	ND mg/L

Phenol







Quant Sample Report

Batch Data Path	V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-24 오전 11:19:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:21:04	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:19:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-20 오후 7:44:09	**Data File**	RE-13.d
Type	Sample	**Name**	RE-13
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

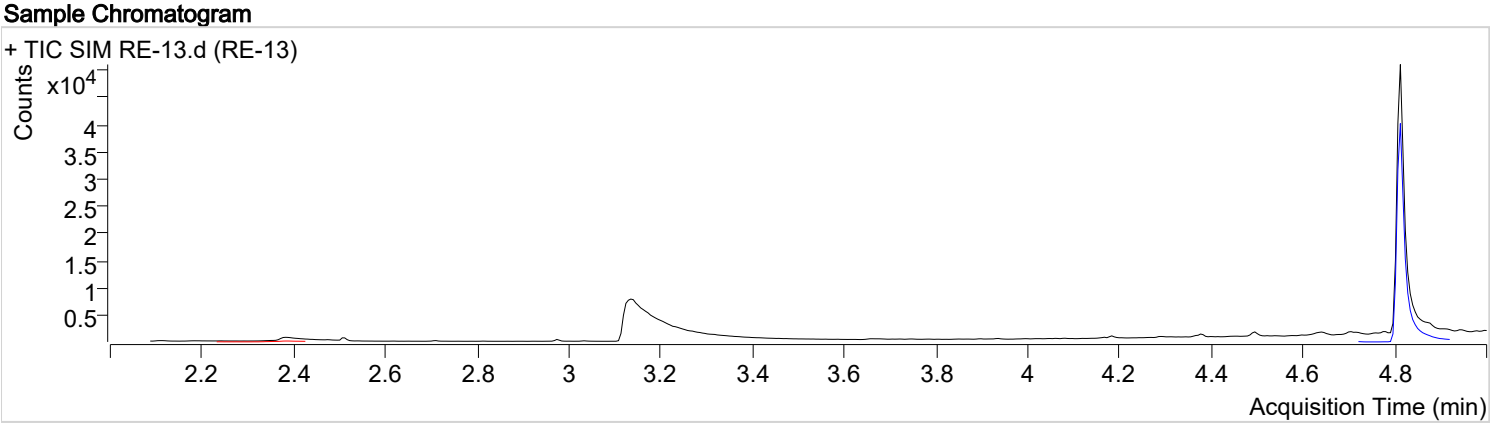

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			51513	ND mg/L

Phenol







Quant Sample Report

Batch Data Path	V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-24 오전 11:19:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:21:04	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:19:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-20 오후 7:52:30	**Data File**	RE-14.d
Type	Sample	**Name**	RE-14
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

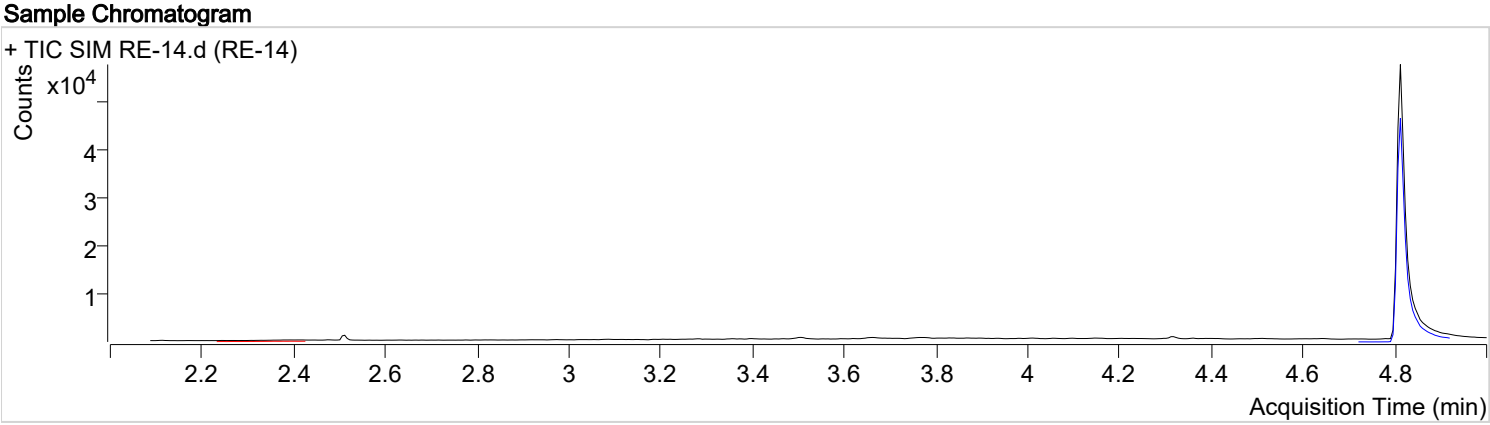

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			65714	ND mg/L

Phenol







Quant Sample Report

Batch Data Path	V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-24 오전 11:19:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:21:04	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:19:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-20 오후 8:00:55	**Data File**	RE-24.d
Type	Sample	**Name**	RE-24
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

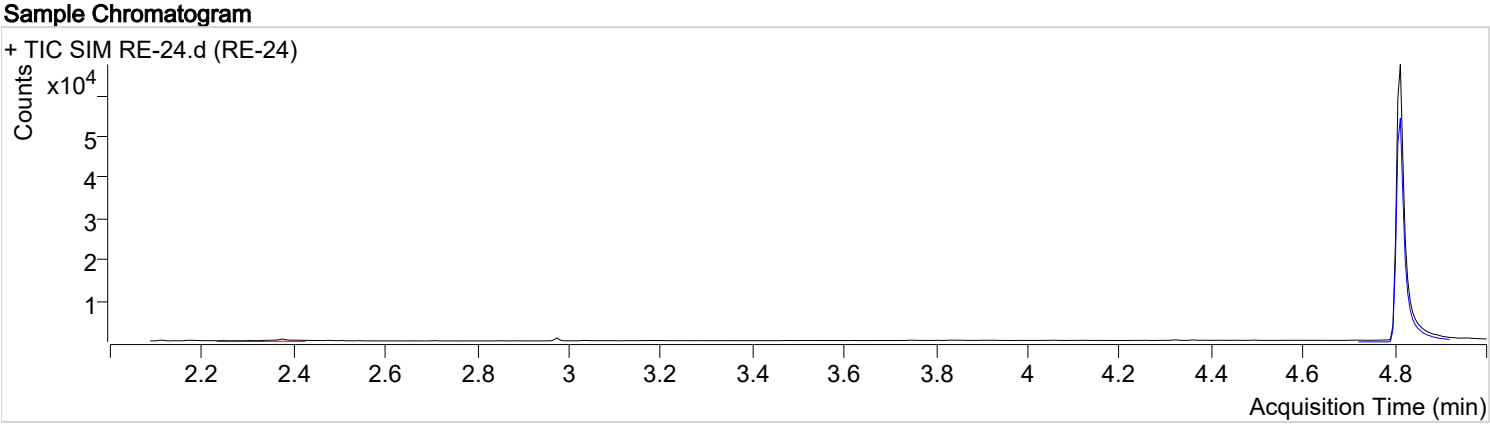

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			72061	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-24 오전 11:19:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:21:04	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:19:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-20 오후 8:09:18	**Data File**	RE-25.d
Type	Sample	**Name**	RE-25
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

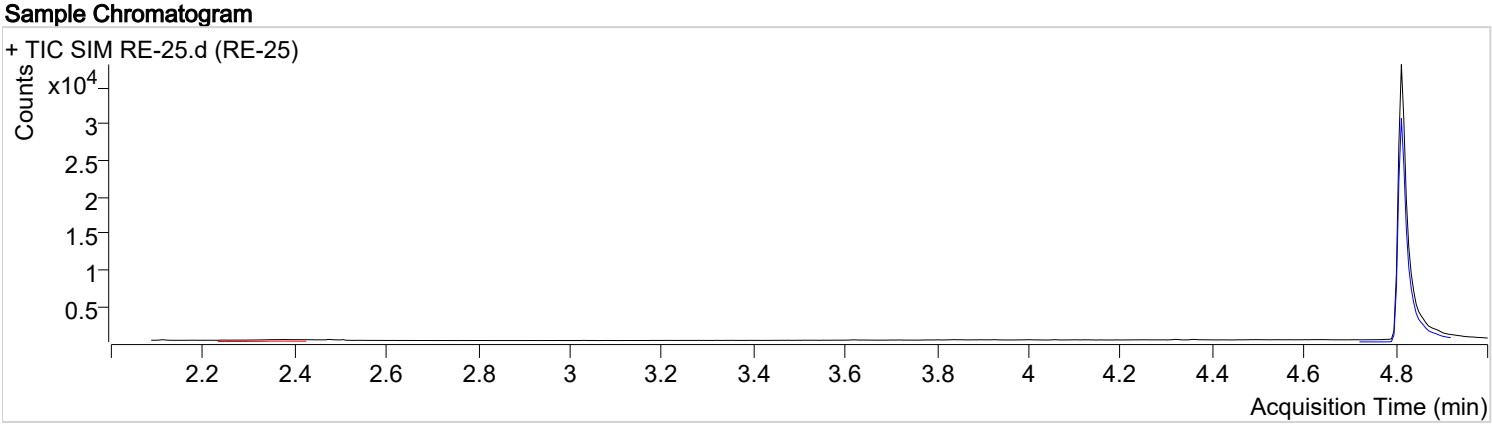

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			47413	ND mg/L

Phenol







Quant Sample Report

Batch Data Path	V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-24 오전 11:19:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:21:04	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:19:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-20 오후 8:17:34	**Data File**	JR 26-03-19.d
Type	Sample	**Name**	JR 26-03-19
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

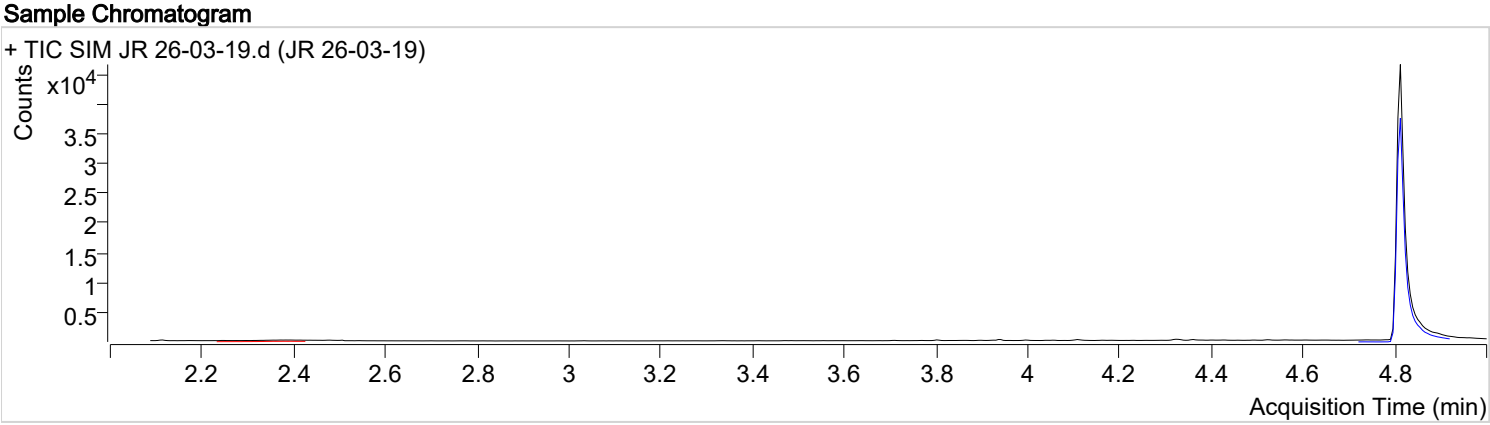

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			50772	ND mg/L

Phenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-24 오전 11:19:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:21:04	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:19:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-20 오후 8:25:55	**Data File**	MBK.d
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

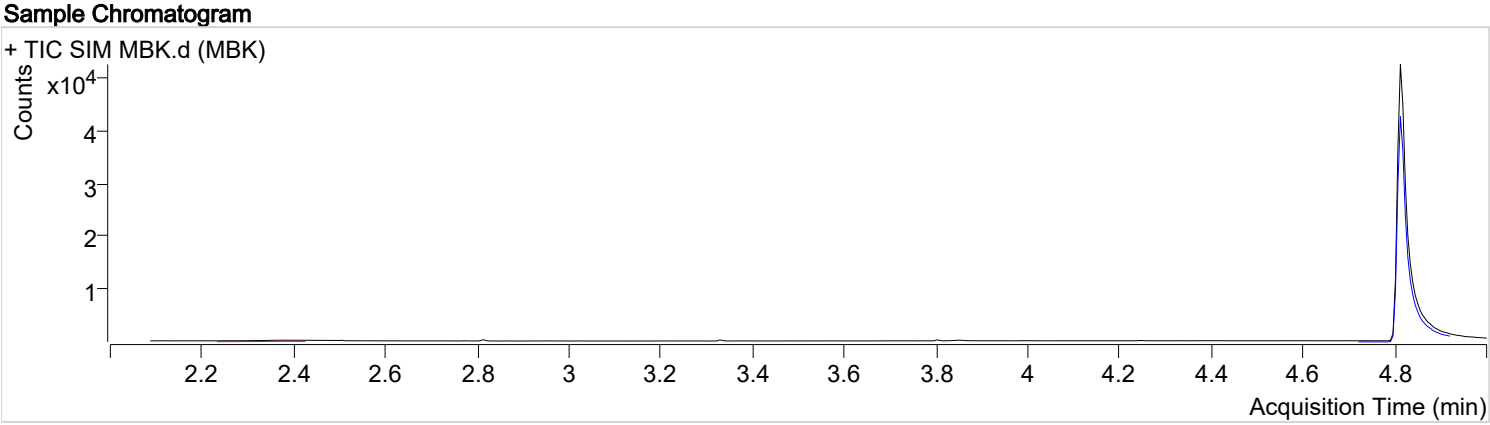

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol			71308	ND mg/L

Phenol







Quant Sample Report

Batch Data Path	V:\2026\2026-03\PHENOL(RE 3.17.18 JR 3.19)\QuantResults\PHENOL.batch.bin		
Analysis Time	2026-03-24 오전 11:19:37	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:21:04	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:19:37	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-20 오후 8:51:00	**Data File**	C-C-V.d
Type	QC	**Name**	C-C-V
Dil.	0.002	**Acq. Method File**	VOCs(Phenol)

Sample Chromatogram

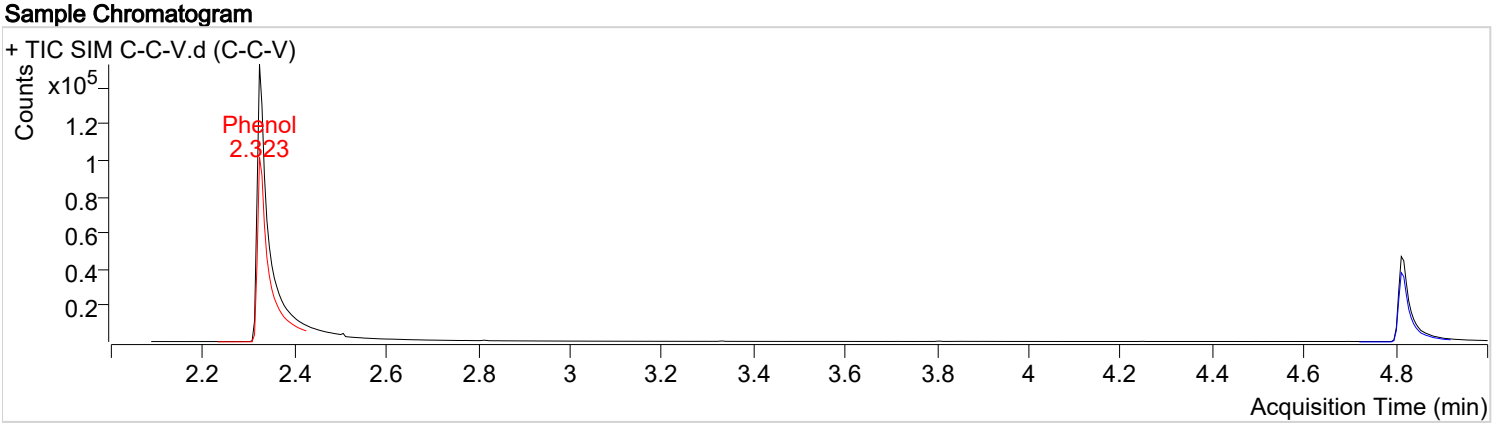

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Phenol	2.323	189698	69773	0.019 mg/L
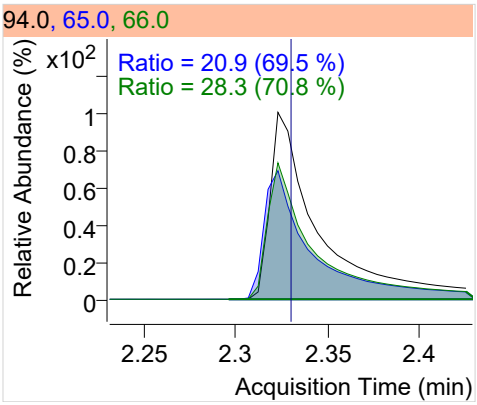
Phenol