Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin				
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Pentachlorophenol

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
PENTA ST-01.D	Cal	8.523	786	147283	0.0013
PENTA ST-02.D	Cal	8.523	1584	105268	0.0022
PENTA ST-03.D	Cal	8.523	2722	125661	0.0028
PENTA ST-04.D	Cal	8.523	3953	124933	0.0037
PENTA ST-05.D	Cal	8.523	5679	134290	0.0047
PENTA ST-06.D	Cal	8.523	6681	120447	0.0059
PENTA ST-07.D	Cal	8.523	10339	123619	0.0084
BK-.D	Blank			113330	ND
FBK(KD 26-02-04).D	Blank			95826	ND
FBK(JR 26-02-05).D	Blank			121608	ND
KD-01.D	Sample			141315	ND
KD-02.D	Sample			140645	ND
KD-04.D	Sample	8.566	0	156464	ND
JR-01.D	Sample	8.523	0	131428	ND
JR-02.D	Sample	8.523	0	135319	ND
JR-03.D	Sample	8.523	0	168676	ND
JR-04.D	Sample			139906	ND
JR-05.D	Sample			152182	ND
JR-06.D	Sample	8.523	0	134333	ND
JR-07.D	Sample			140803	ND
JR-08.D	Sample			142223	ND
MBK.D	Blank			104353	ND
C-C-V-.D	QC	8.523	5943	145245	0.0045

Pentachlorophenol

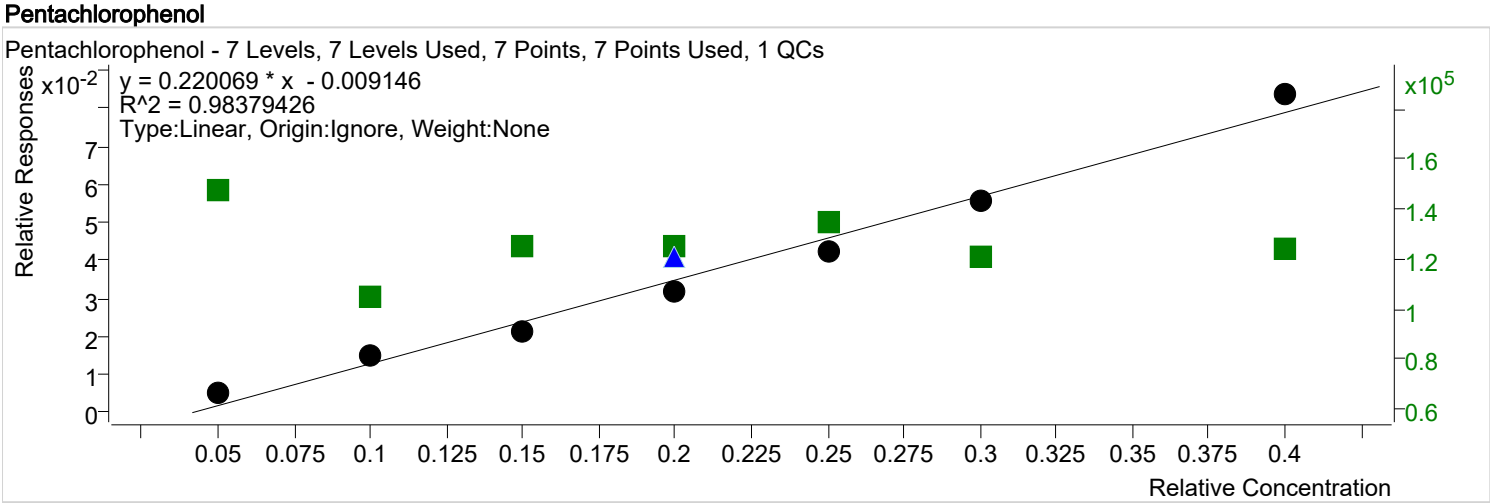

Cal. Path	Type	Level	Enable	Conc.	Response
\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\PENTA ST-01.D	Calibration	1	x	0.500	786
\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\PENTA ST-02.D	Calibration	2	x	1.000	1584
\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\PENTA ST-03.D	Calibration	3	x	1.500	2722
\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\PENTA ST-04.D	Calibration	4	x	2.000	3953
\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\C-C-V-.D	QC	4	x	2.000	5943
\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\PENTA ST-05.D	Calibration	5	x	2.500	5679
\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\PENTA ST-06.D	Calibration	6	x	3.000	6681
\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\PENTA ST-07.D	Calibration	7	x	4.000	10339

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오전 10:12:46	**Data File**	PENTA ST-01.D
Type	Cal	**Name**	PENTA ST-01
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

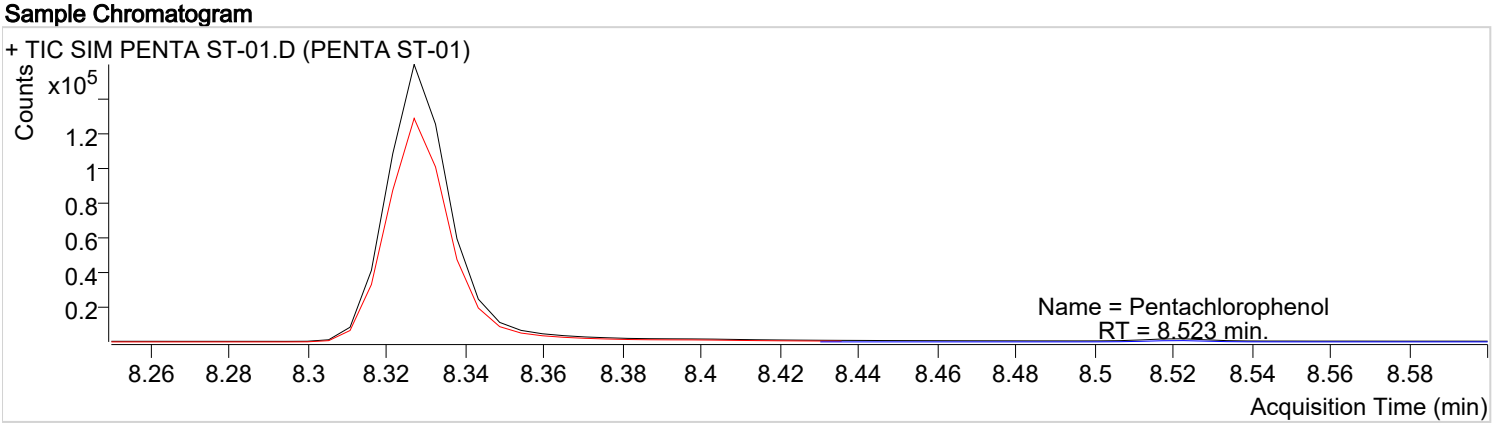

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	786	147283	0.0013 mg/L

Pentachlorophenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오전 10:26:09	**Data File**	PENTA ST-02.D
Type	Cal	**Name**	PENTA ST-02
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

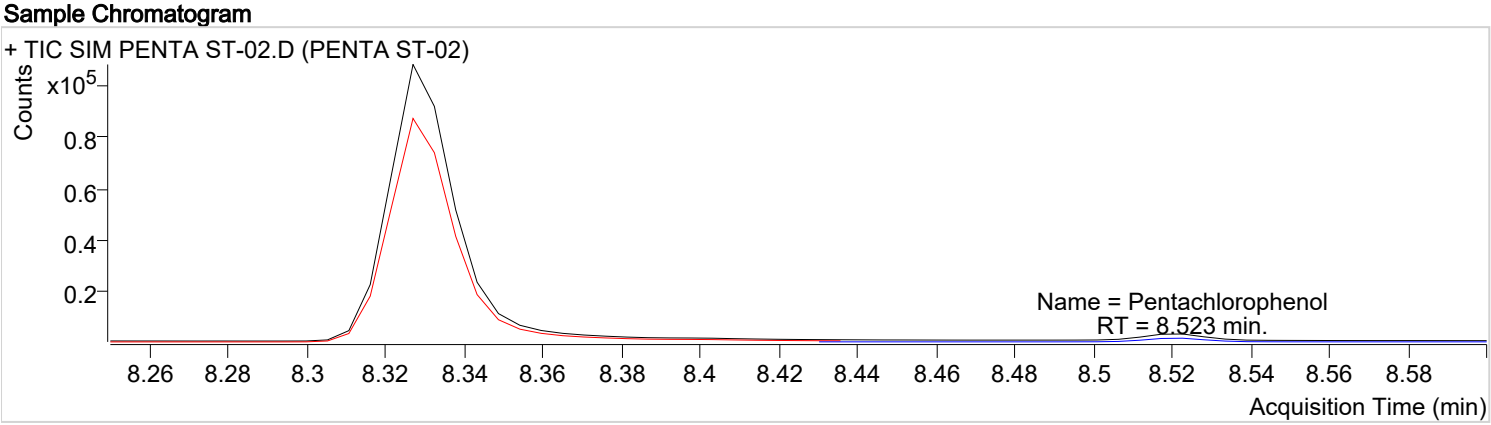

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	1584	105268	0.0022 mg/L

Pentachlorophenol

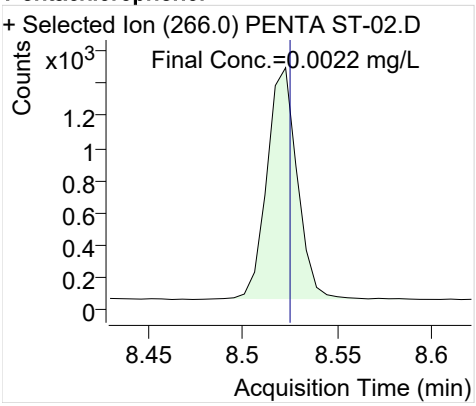

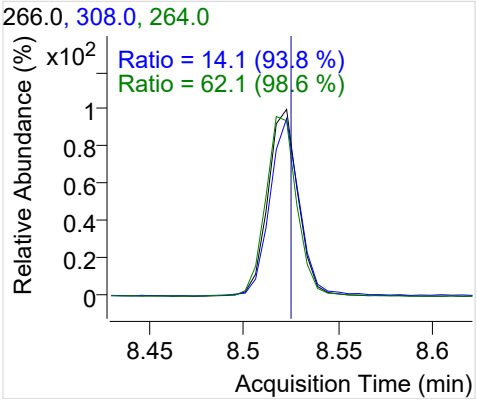

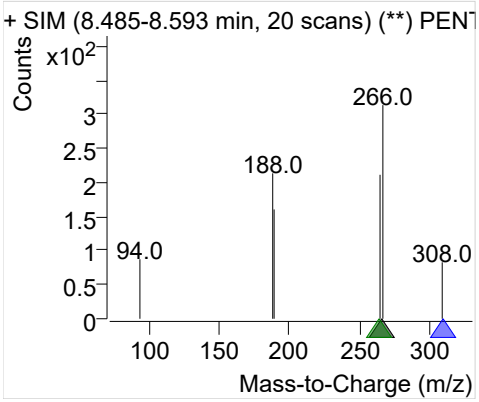

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오전 10:39:30	**Data File**	PENTA ST-03.D
Type	Cal	**Name**	PENTA ST-03
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

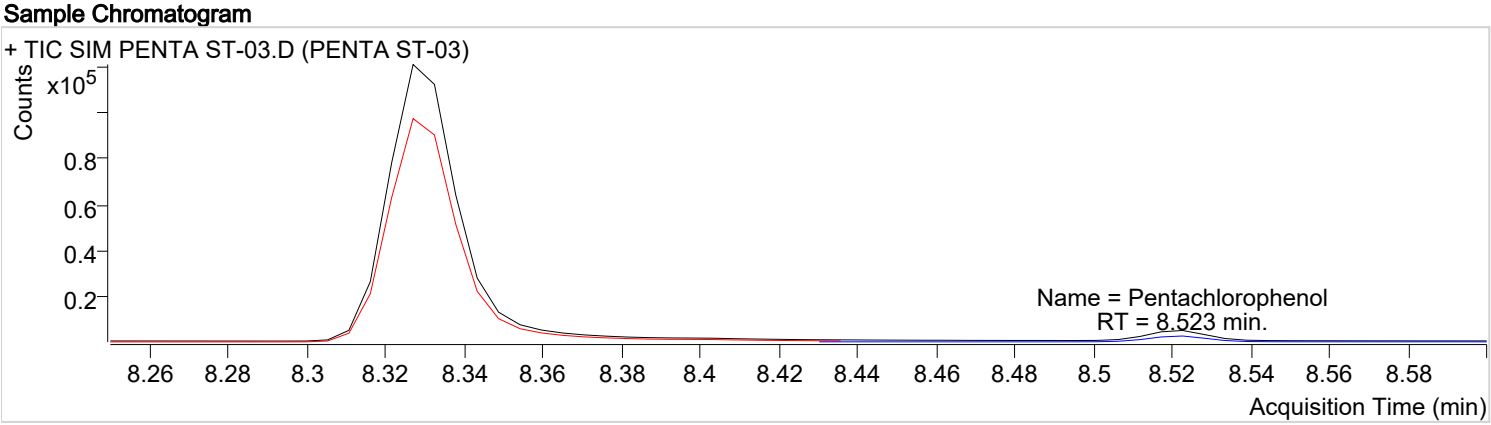

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	2722	125661	0.0028 mg/L

Pentachlorophenol





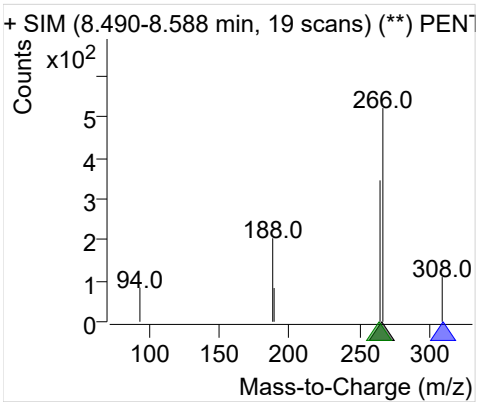

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오전 10:52:54	**Data File**	PENTA ST-04.D
Type	Cal	**Name**	PENTA ST-04
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

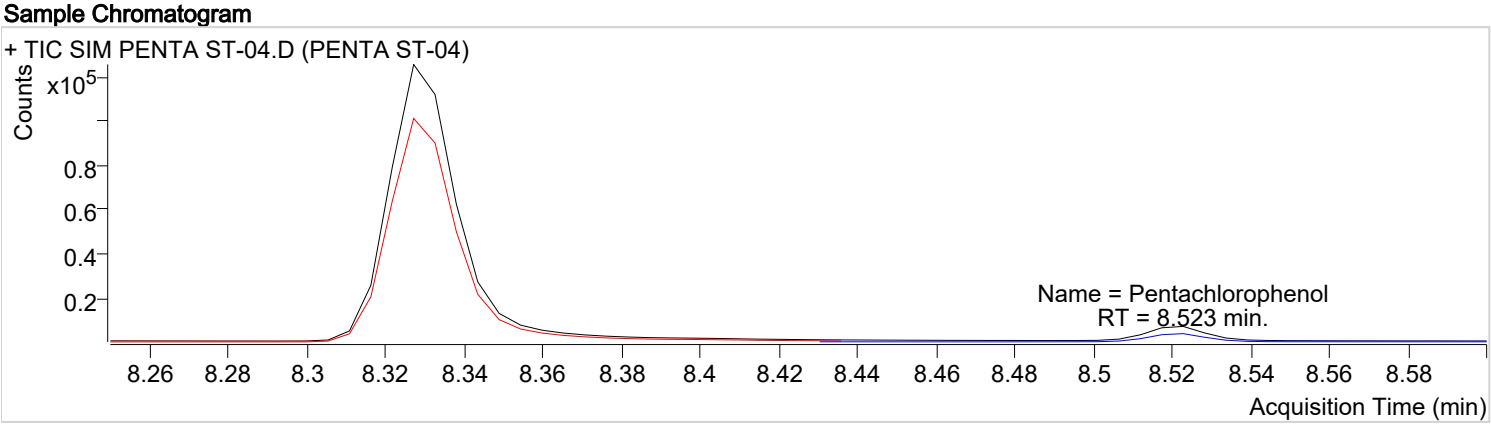

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	3953	124933	0.0037 mg/L

Pentachlorophenol





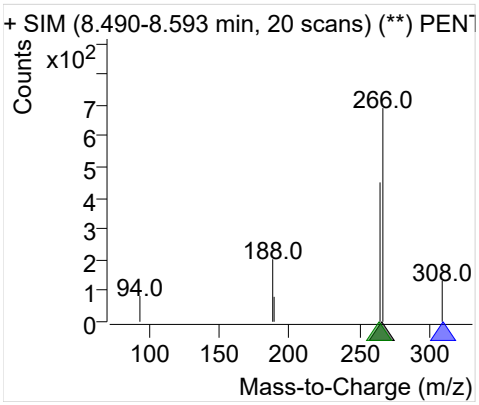

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오전 11:06:18	**Data File**	PENTA ST-05.D
Type	Cal	**Name**	PENTA ST-05
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

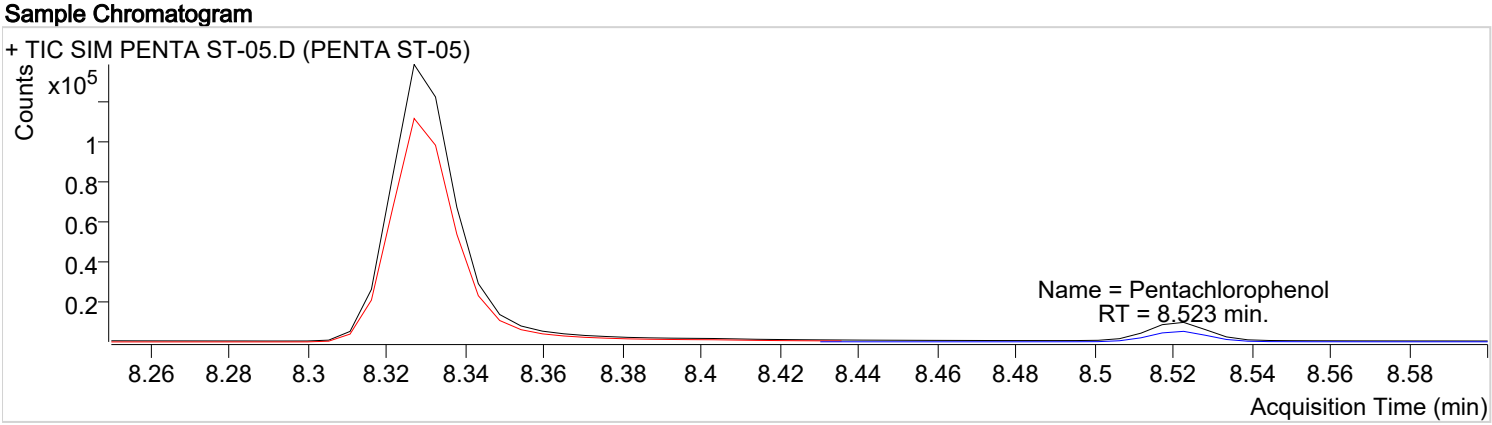

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	5679	134290	0.0047 mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오전 11:19:42	**Data File**	PENTA ST-06.D
Type	Cal	**Name**	PENTA ST-06
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

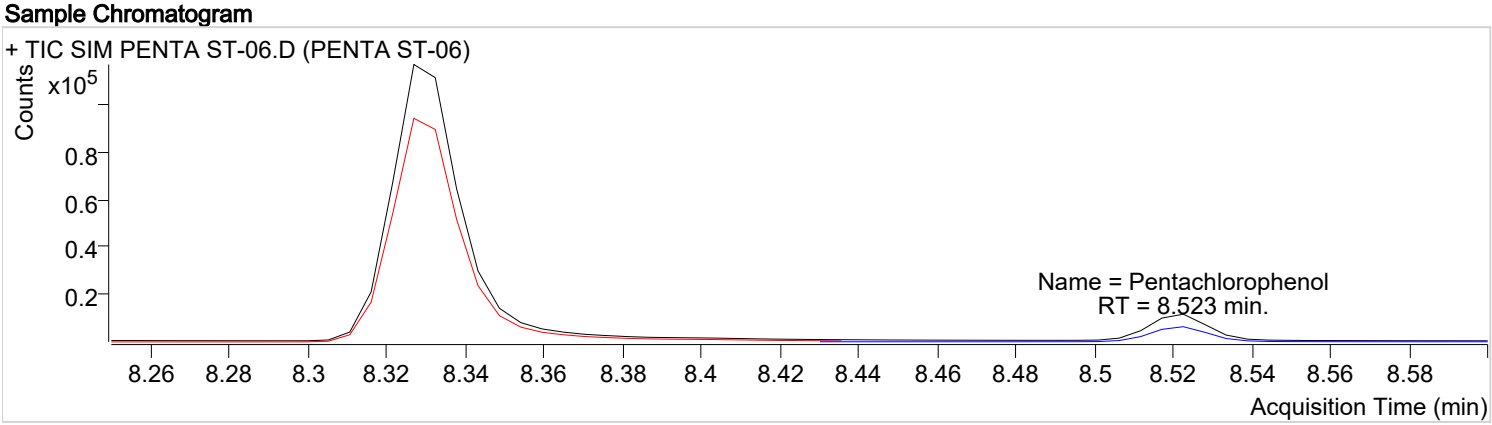

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	6681	120447	0.0059 mg/L

Pentachlorophenol





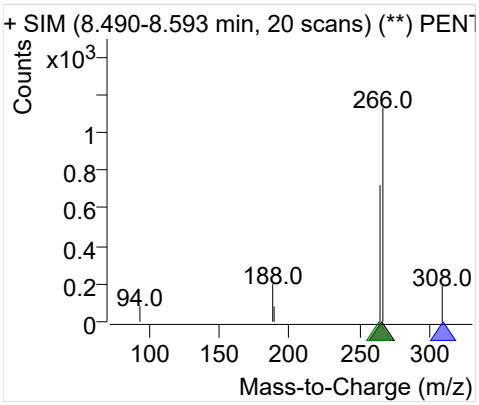

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오전 11:33:07	**Data File**	PENTA ST-07.D
Type	Cal	**Name**	PENTA ST-07
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

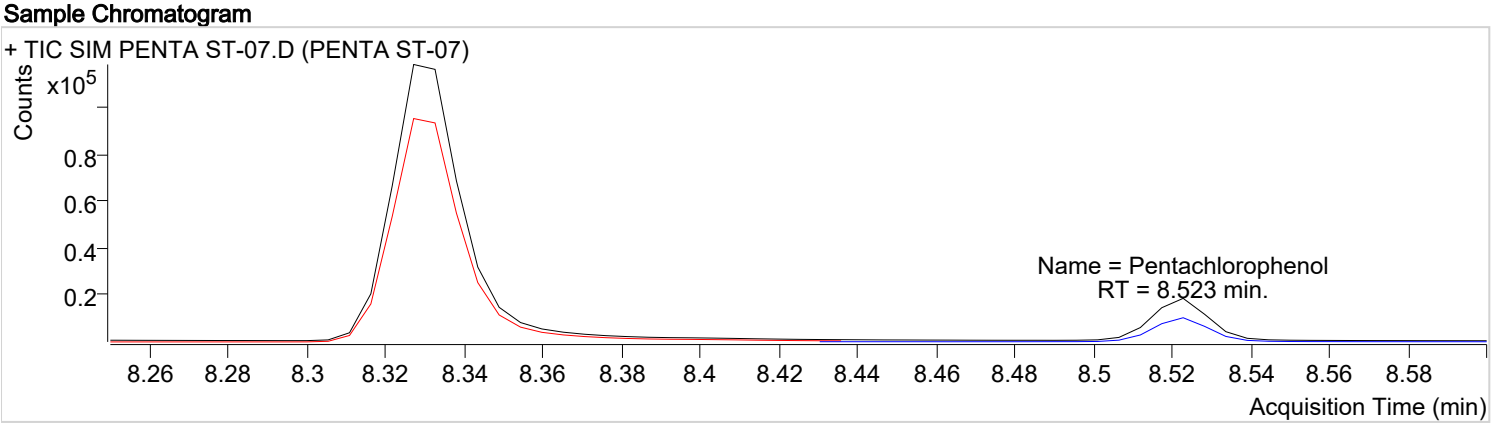

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	10339	123619	0.0084 mg/L

Pentachlorophenol





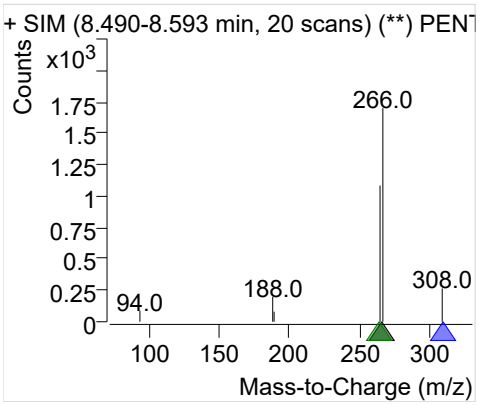

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오전 11:59:51	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

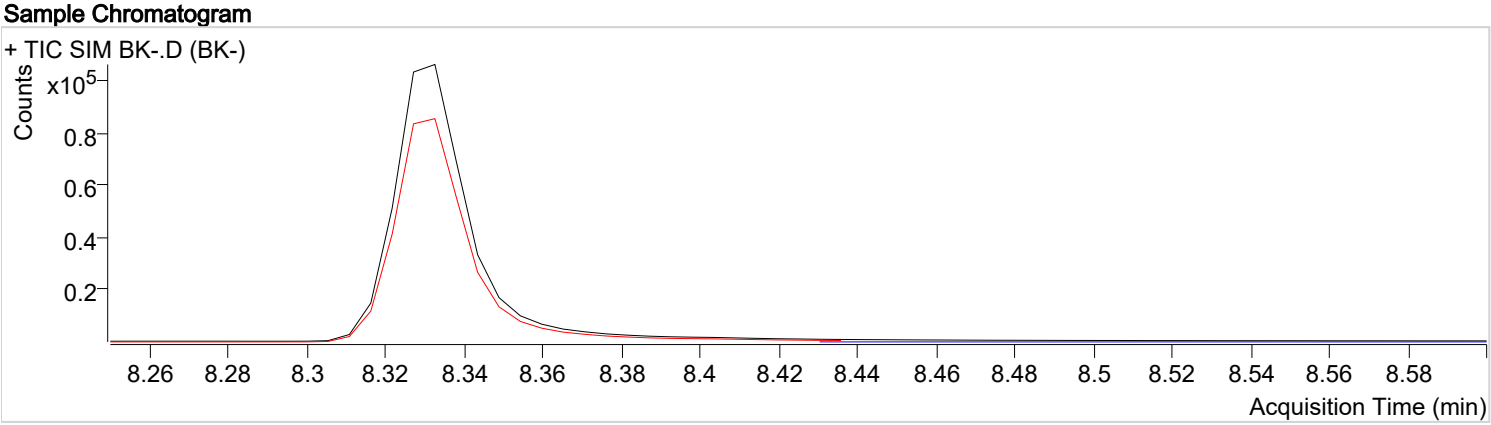

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			113330	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오후 12:13:13	**Data File**	FBK(KD 26-02-04).D
Type	Blank	**Name**	FBK(KD 26-02-04)
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

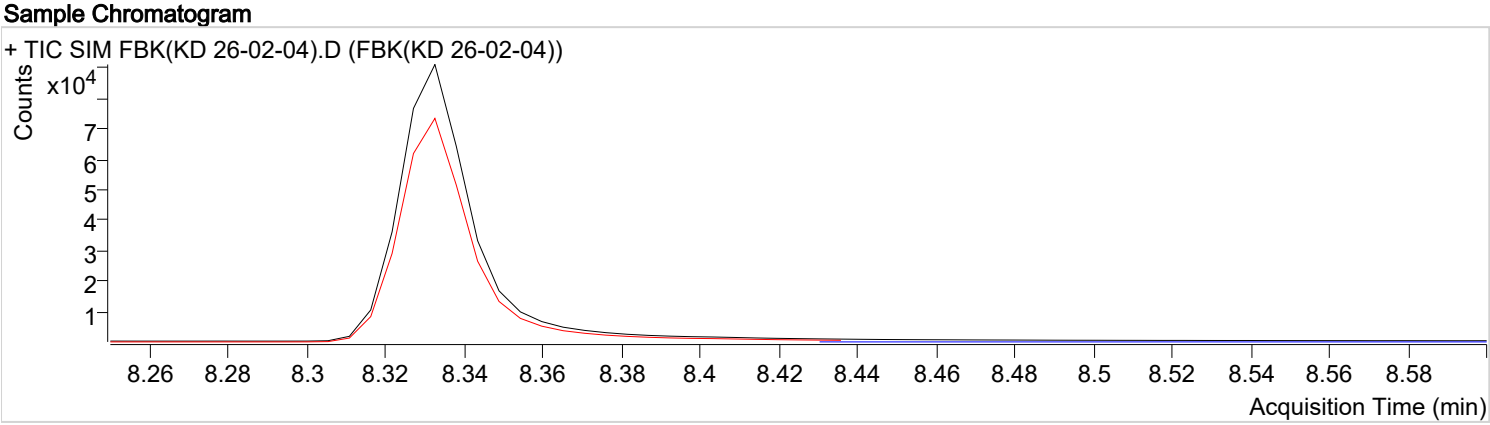

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			95826	ND mg/L

Pentachlorophenol

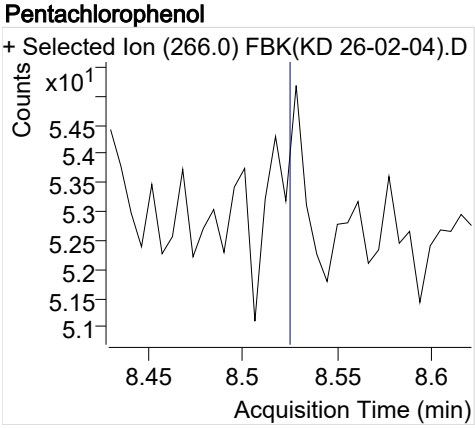

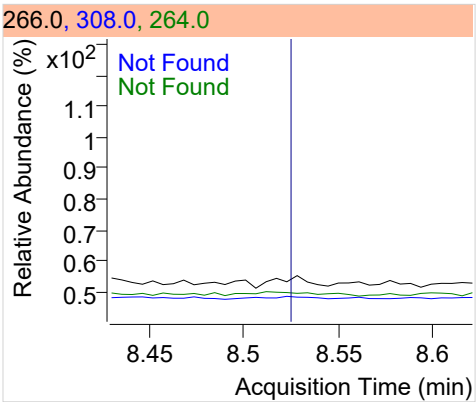



Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오후 12:26:35	**Data File**	FBK(JR 26-02-05).D
Type	Blank	**Name**	FBK(JR 26-02-05)
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

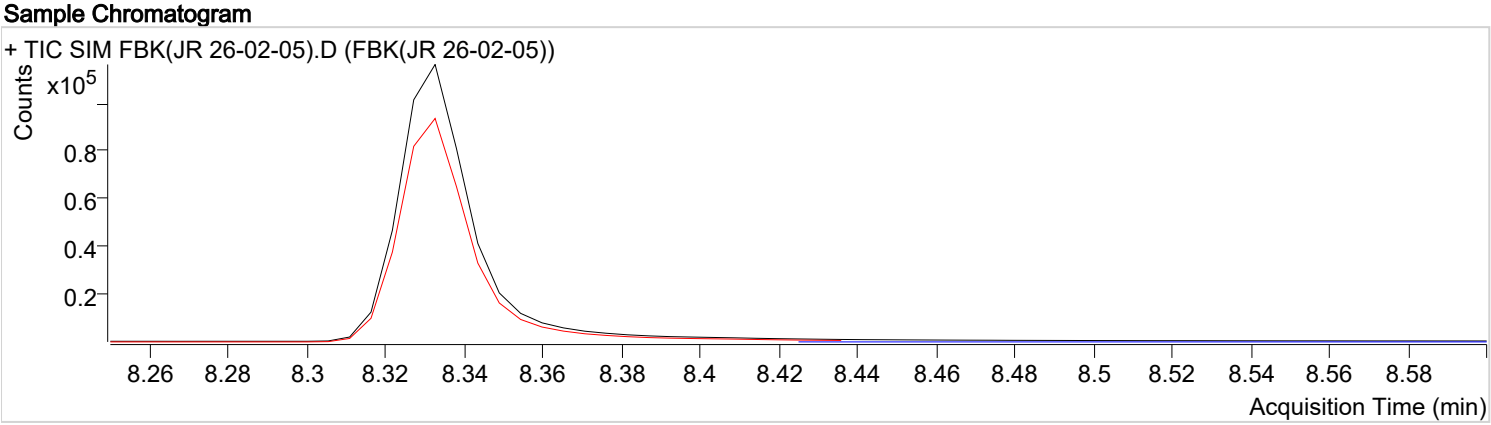

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			121608	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오후 12:39:59	**Data File**	KD-01.D
Type	Sample	**Name**	KD-01
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

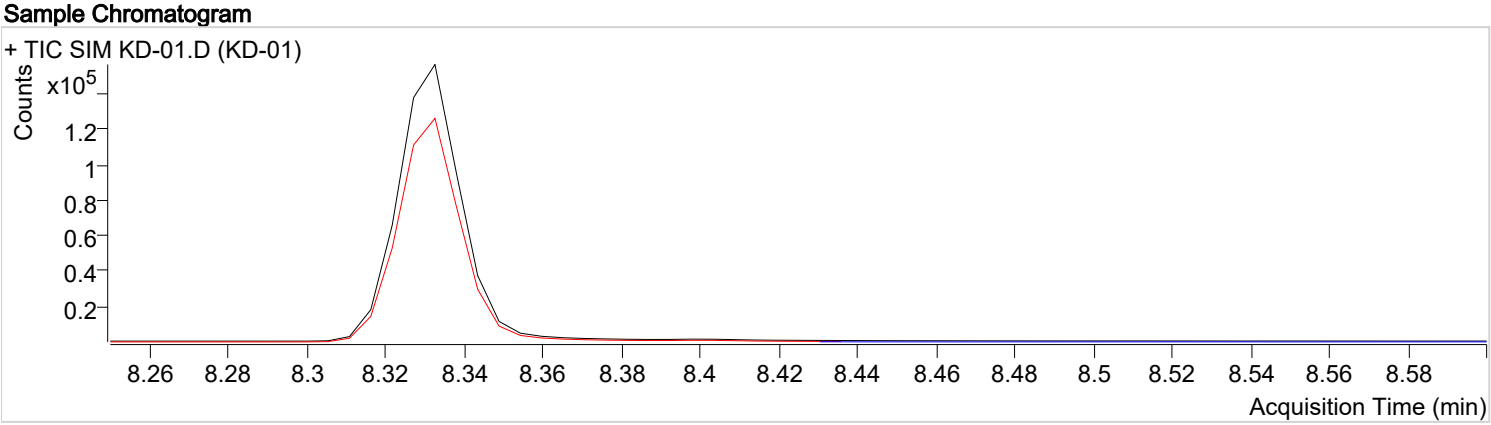

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			141315	ND mg/L

Pentachlorophenol





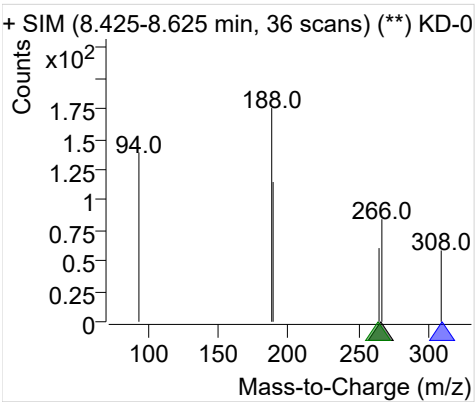

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오후 12:53:23	**Data File**	KD-02.D
Type	Sample	**Name**	KD-02
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

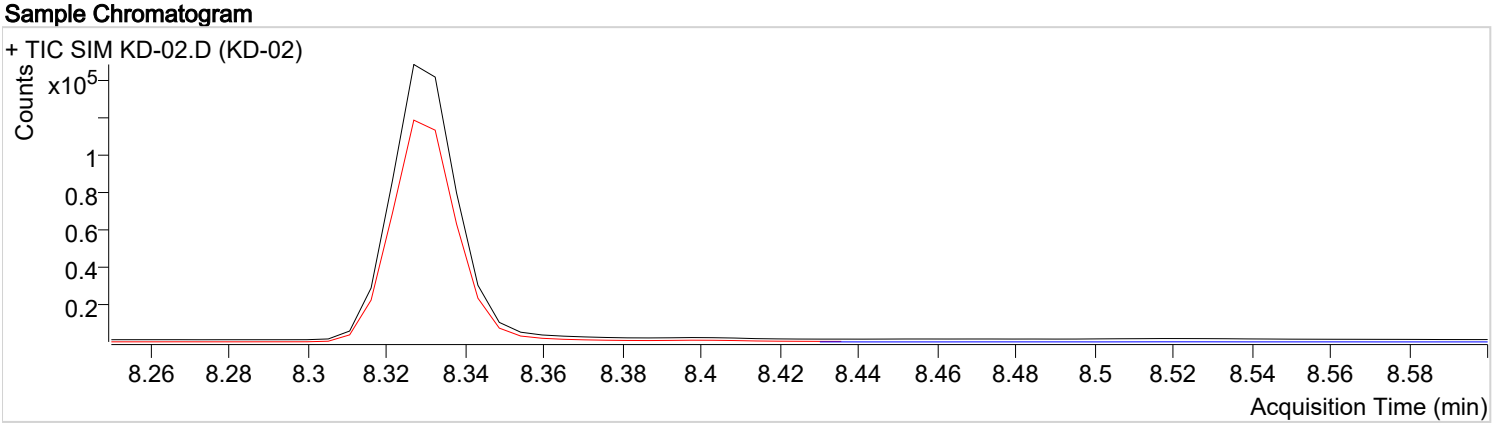

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			140645	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오후 1:06:47	**Data File**	KD-04.D
Type	Sample	**Name**	KD-04
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

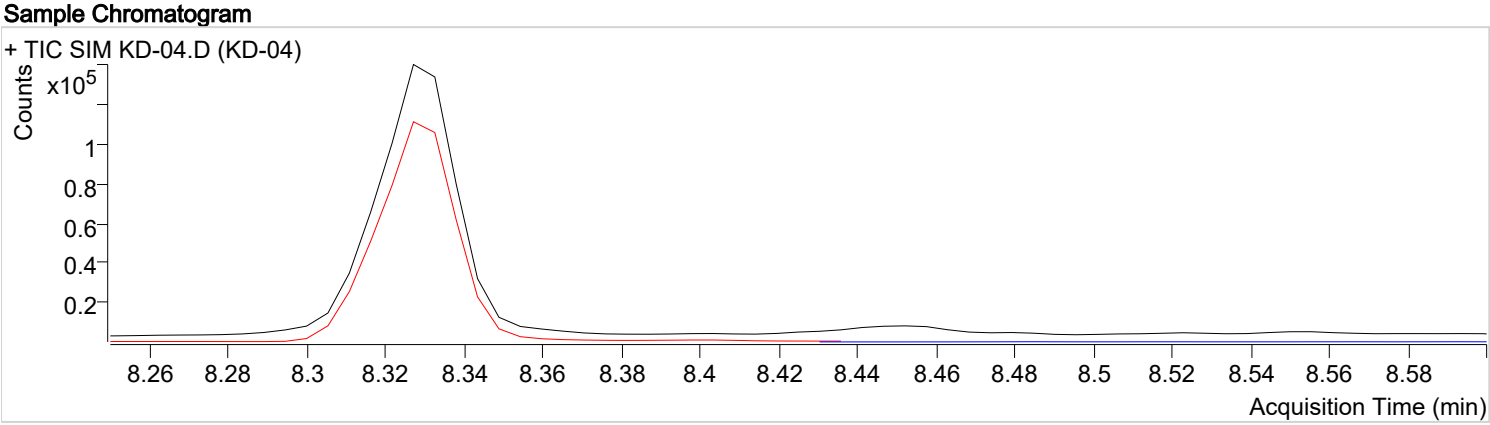

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.566	0	156464	ND mg/L

Pentachlorophenol

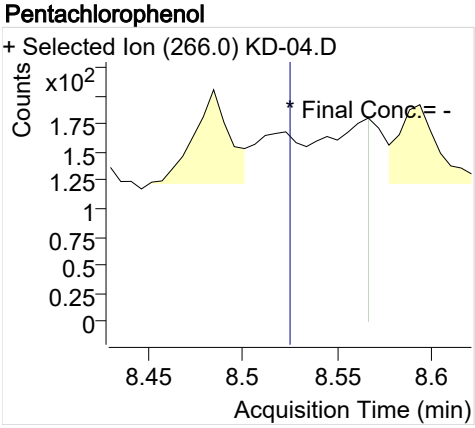

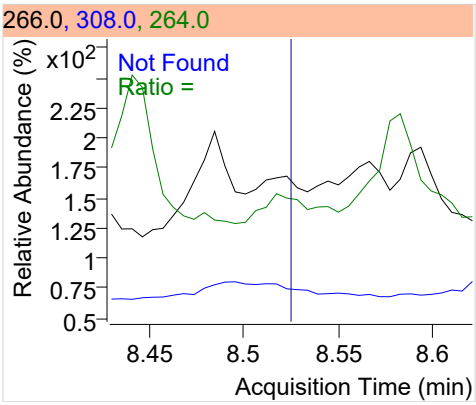

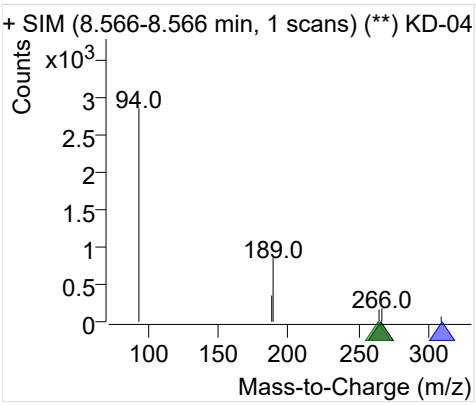

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오후 1:20:13	**Data File**	JR-01.D
Type	Sample	**Name**	JR-01
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

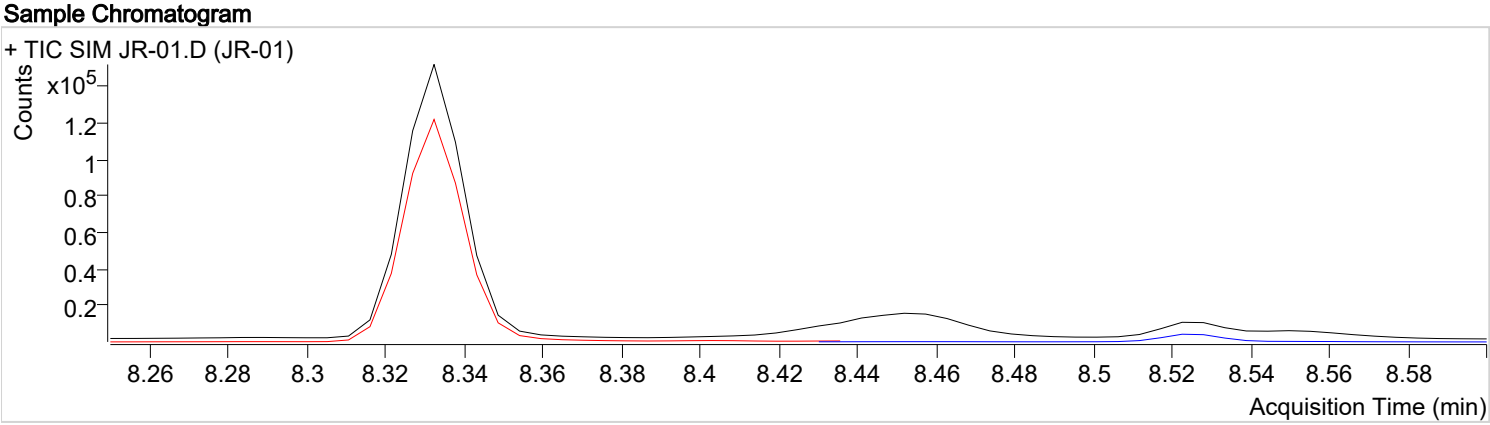

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	0	131428	ND mg/L

Pentachlorophenol

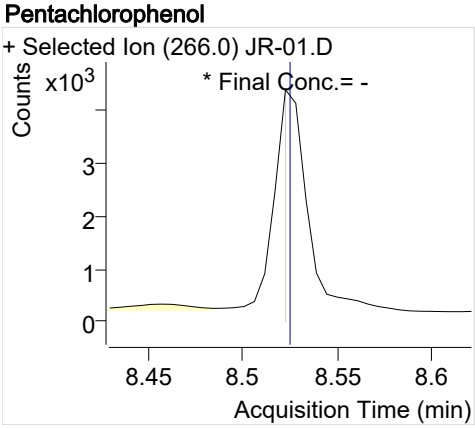





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오후 1:33:38	**Data File**	JR-02.D
Type	Sample	**Name**	JR-02
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

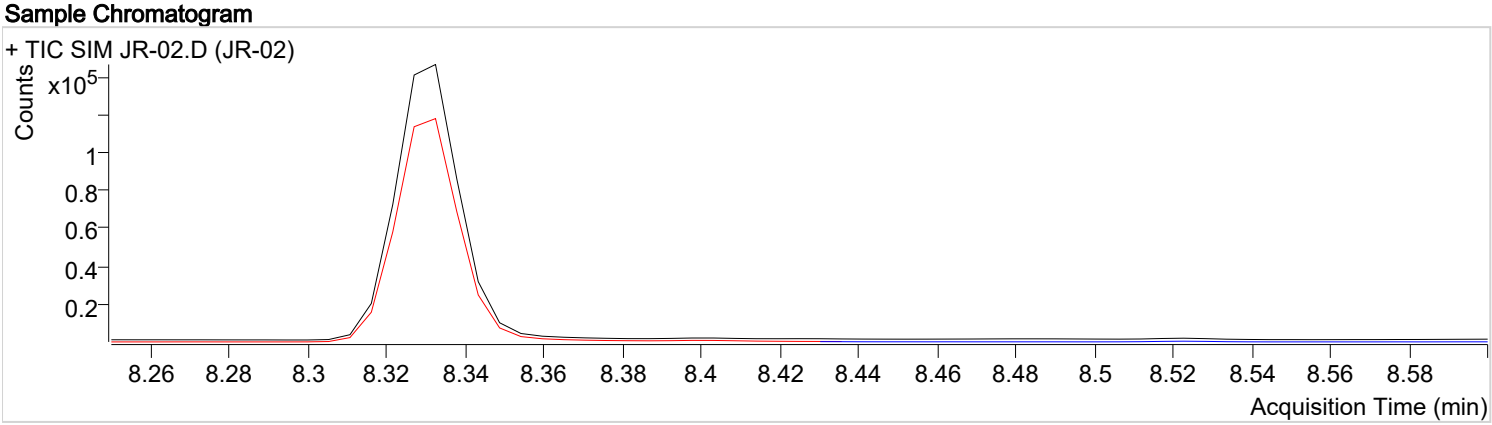

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	0	135319	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오후 1:47:02	**Data File**	JR-03.D
Type	Sample	**Name**	JR-03
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

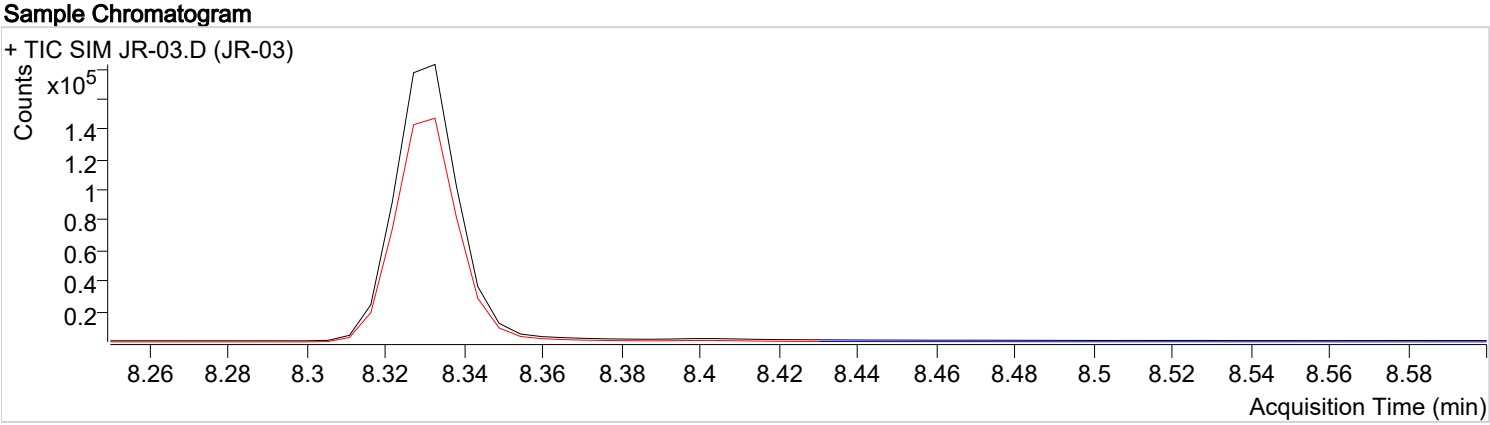

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	0	168676	ND mg/L

Pentachlorophenol

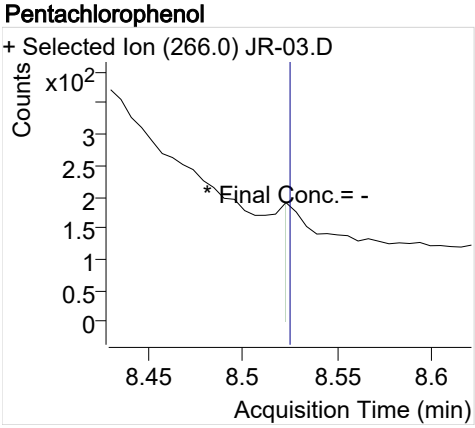

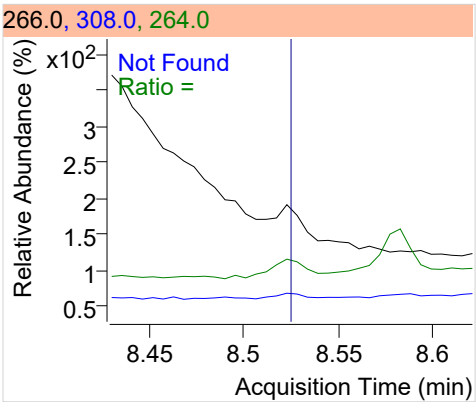



Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오후 2:00:24	**Data File**	JR-04.D
Type	Sample	**Name**	JR-04
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

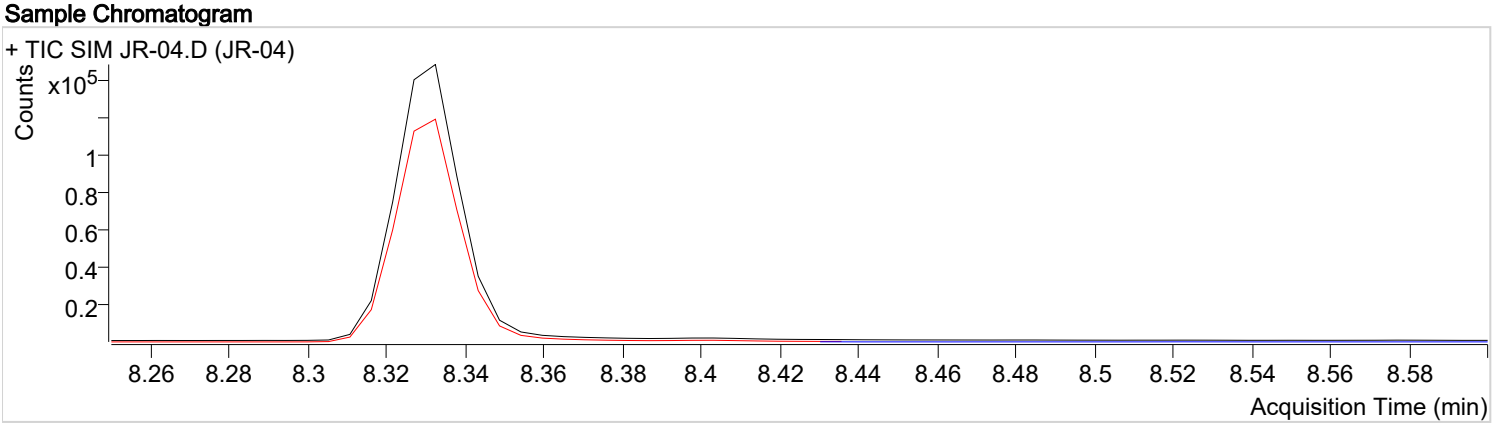

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			139906	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오후 2:13:48	**Data File**	JR-05.D
Type	Sample	**Name**	JR-05
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

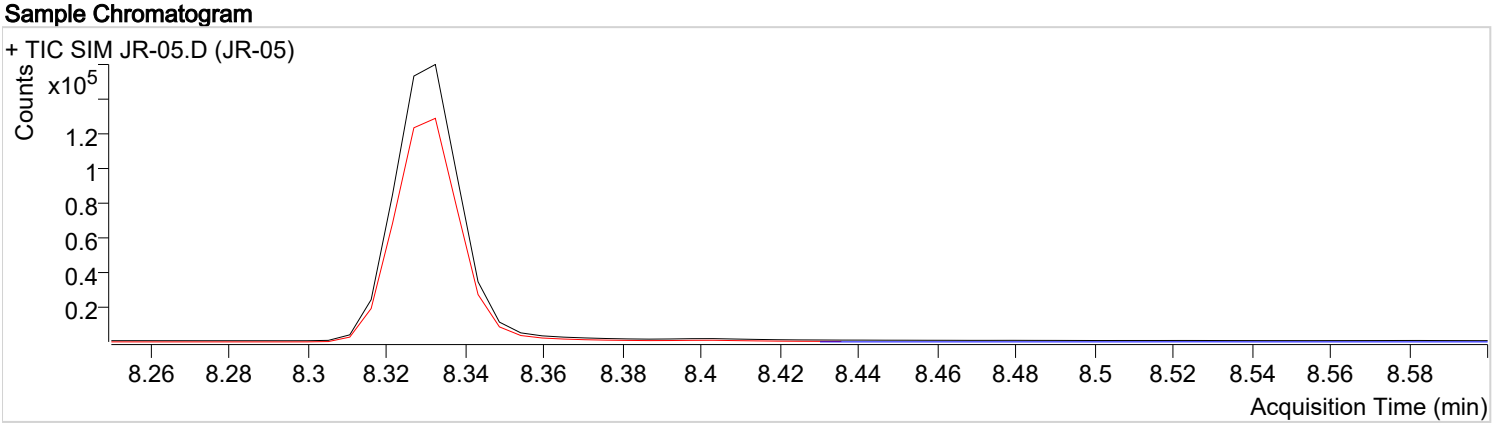

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			152182	ND mg/L

Pentachlorophenol

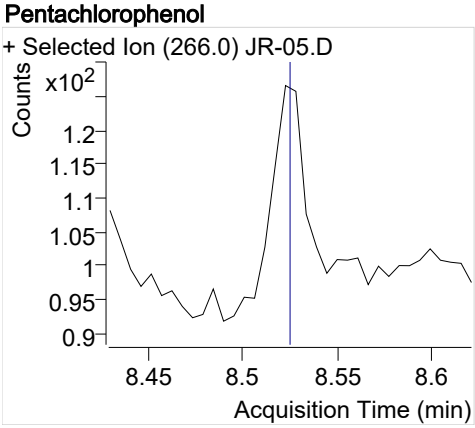

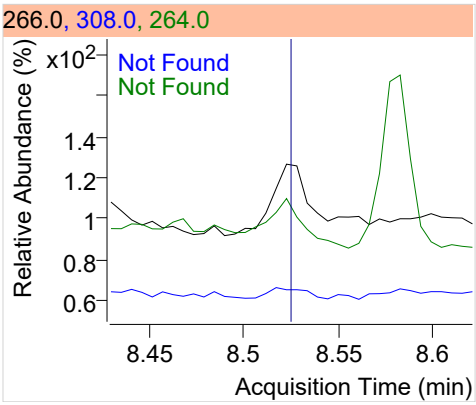



Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오후 2:27:12	**Data File**	JR-06.D
Type	Sample	**Name**	JR-06
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

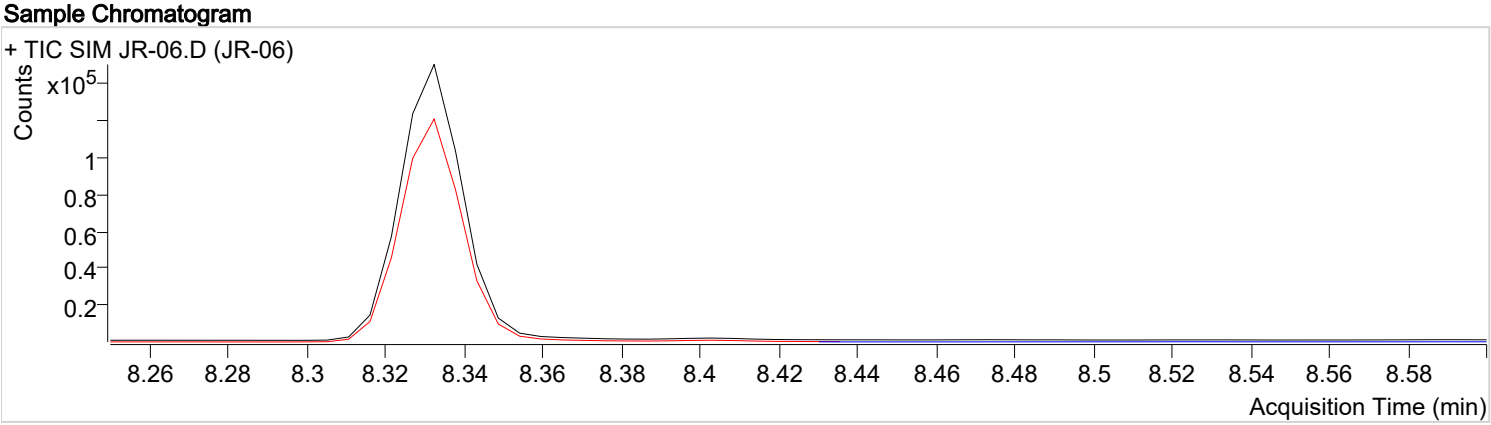

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	0	134333	ND mg/L

Pentachlorophenol

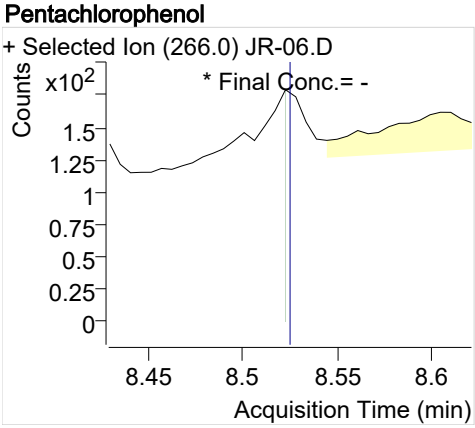





Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오후 2:40:37	**Data File**	JR-07.D
Type	Sample	**Name**	JR-07
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

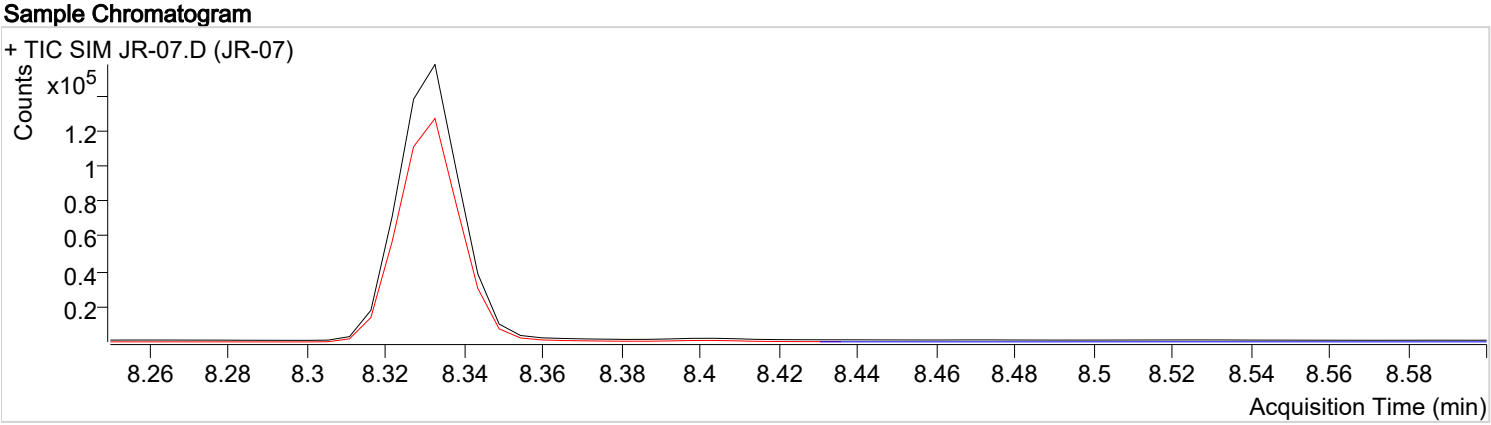

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			140803	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오후 2:54:01	**Data File**	JR-08.D
Type	Sample	**Name**	JR-08
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

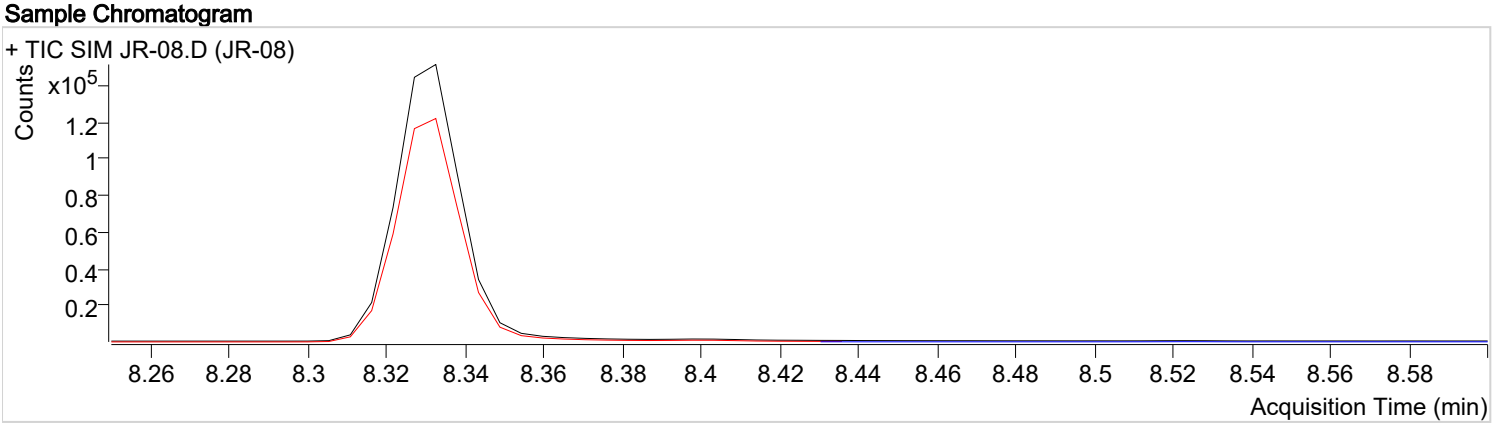

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			142223	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오후 3:08:43	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

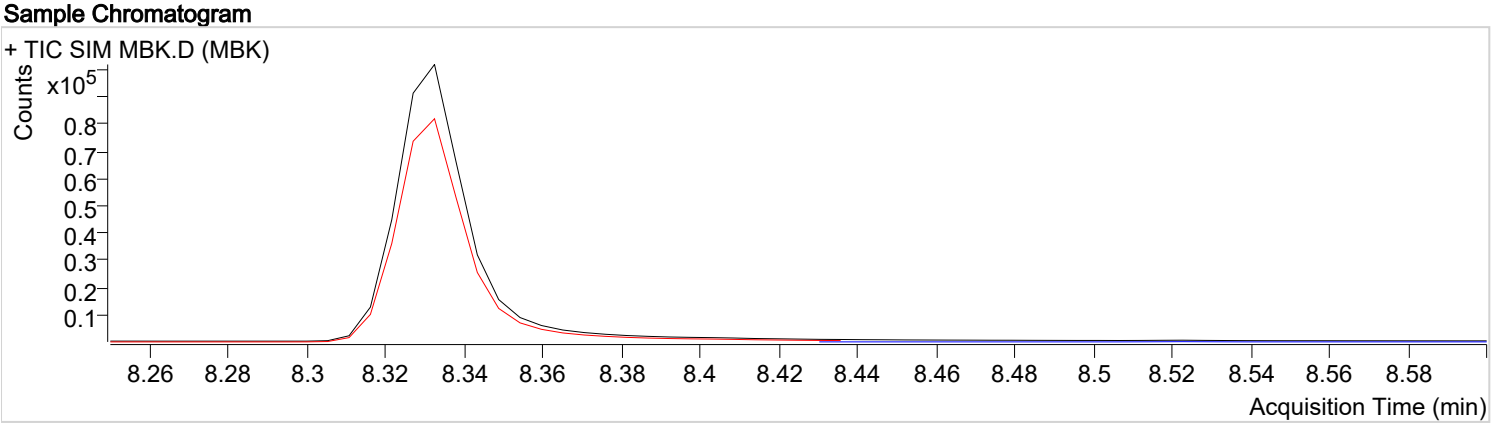

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			104353	ND mg/L

Pentachlorophenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(KD 2.4, JR 2.5)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-09 오후 4:27:14	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:41:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-09 오후 4:27:14	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-09 오후 3:35:34	**Data File**	C-C-V-.D
Type	QC	**Name**	C-C-V-
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

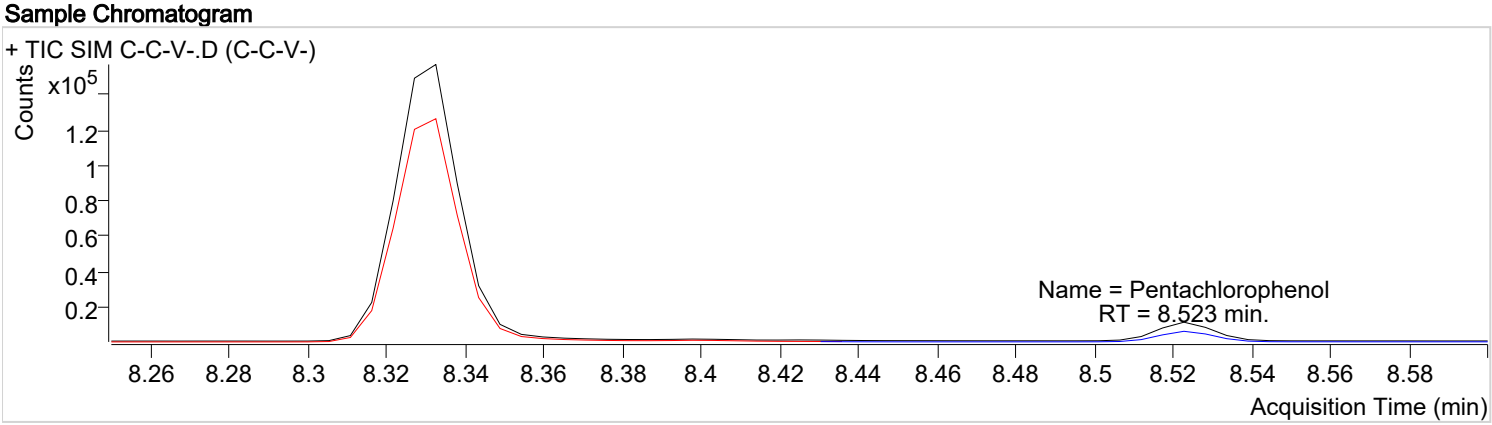

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	5943	145245	0.0045 mg/L
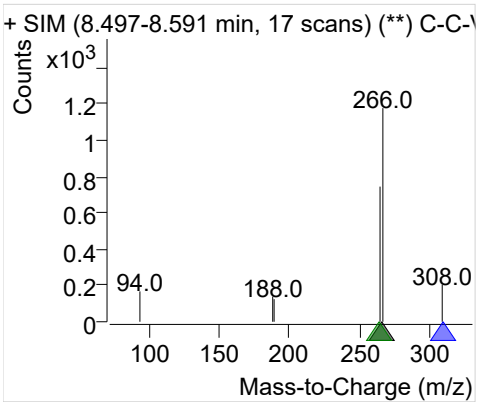
Pentachlorophenol