Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin				
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Pentachlorophenol

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
PENTA ST-01.D	Cal	8.523	890	110067	0.0012
PENTA ST-02.D	Cal	8.523	1999	112993	0.0019
PENTA ST-03.D	Cal	8.523	3635	142374	0.0025
PENTA ST-04.D	Cal	8.523	4550	104091	0.0039
PENTA ST-05.D	Cal	8.523	9551	180528	0.0046
PENTA ST-06.D	Cal	8.523	11864	176867	0.0057
PENTA ST-07.D	Cal	8.523	10573	105784	0.0082
BK-.D	Blank			110780	ND
FBK(DL 26-02-26).D	Blank			128402	ND
FBK(LT 26-02-26).D	Blank			108408	ND
FBK(PL 26-02-27).D	Blank			166878	ND
DL-01.D	Sample			142432	ND
LT-01.D	Sample	8.523	0	161958	ND
LT-02.D	Sample			177964	ND
LT-03.D	Sample			135135	ND
PL-01.D	Sample			160062	ND
PL-02.D	Sample			136954	ND
MBK.D	Blank			182114	ND
-CCV-.D	QC	8.523	7632	134719	0.0049

Pentachlorophenol

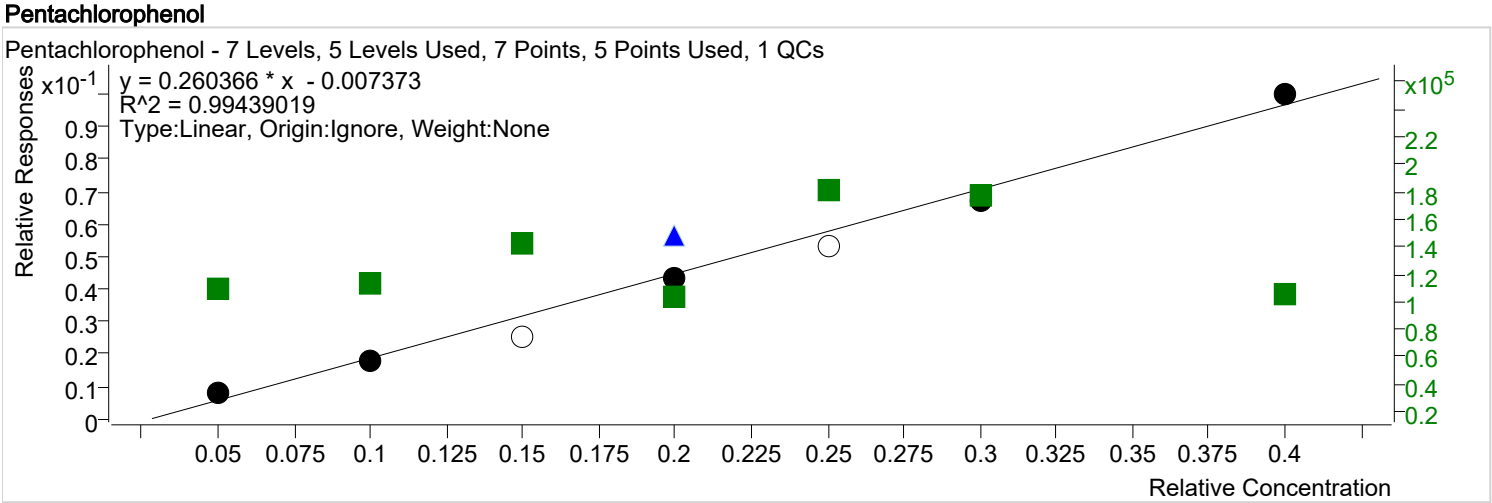

Cal. Path	Type	Level	Enable	Conc.	Response
\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\PENTA ST-01.D	Calibration	1	x	0.500	890
\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\PENTA ST-02.D	Calibration	2	x	1.000	1999
\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\PENTA ST-03.D	Calibration	3		1.500	3635
\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\PENTA ST-04.D	Calibration	4	x	2.000	4550
\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\-CCV-.D	QC	4	x	2.000	7632
\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\PENTA ST-05.D	Calibration	5		2.500	9551
\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\PENTA ST-06.D	Calibration	6	x	3.000	11864
\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\PENTA ST-07.D	Calibration	7	x	4.000	10573

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:39:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 6:06:53	**Data File**	PENTA ST-01.D
Type	Cal	**Name**	PENTA ST-01
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

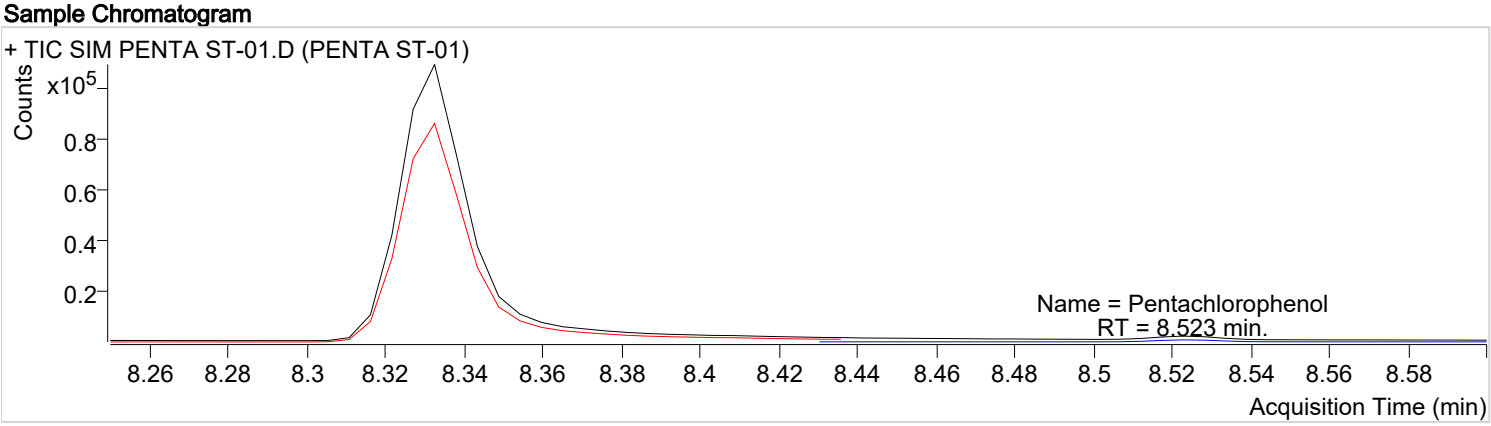

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	890	110067	0.0012 mg/L

Pentachlorophenol

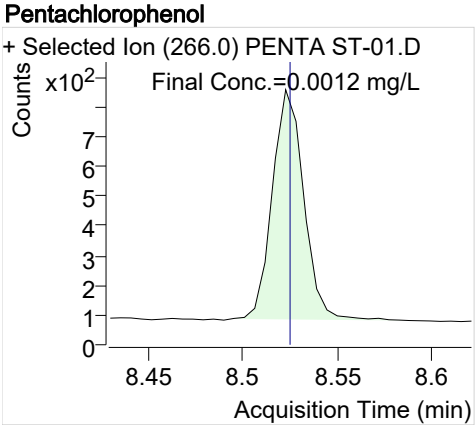

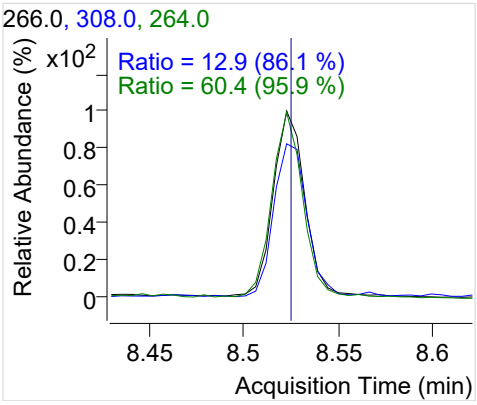

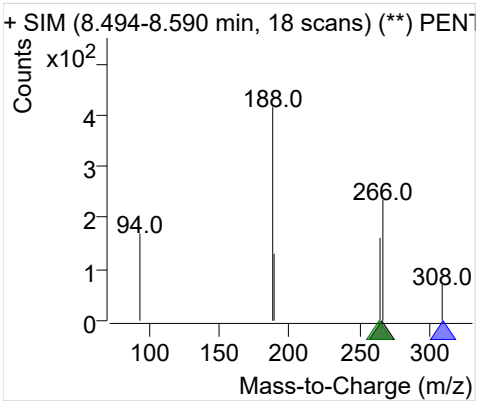

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:39:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 6:20:17	**Data File**	PENTA ST-02.D
Type	Cal	**Name**	PENTA ST-02
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

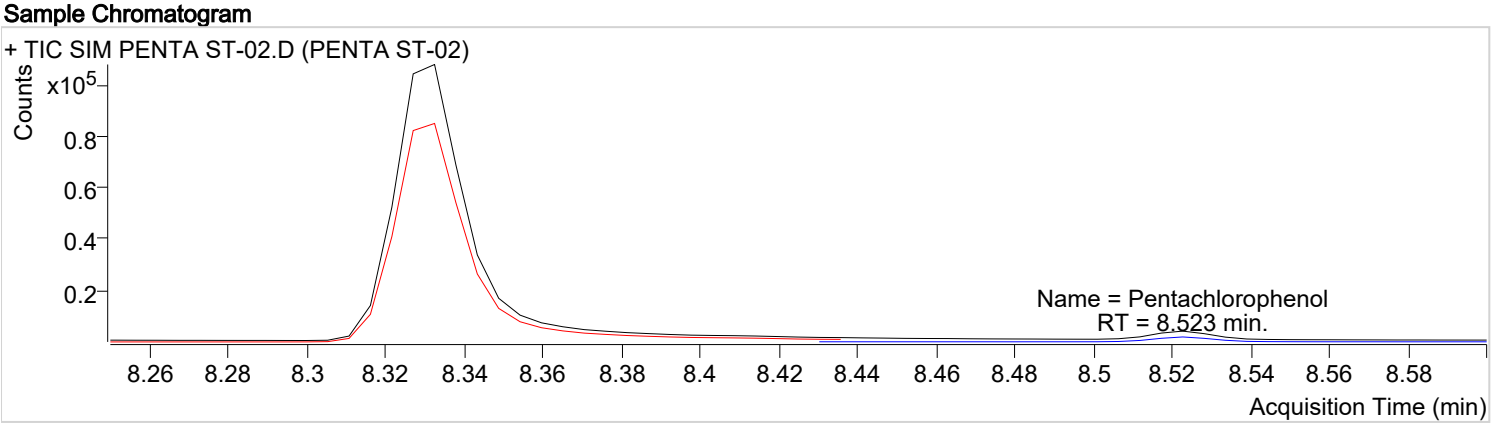

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	1999	112993	0.0019 mg/L

Pentachlorophenol

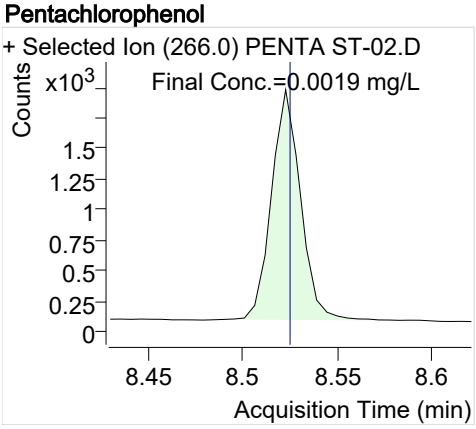

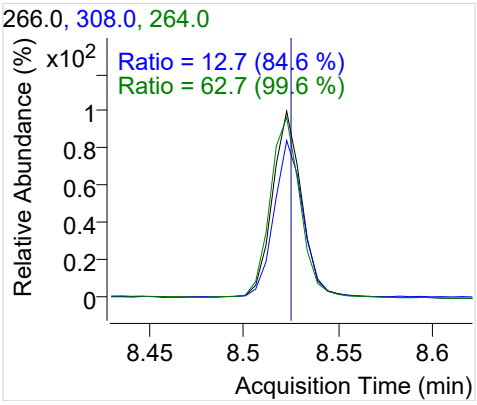

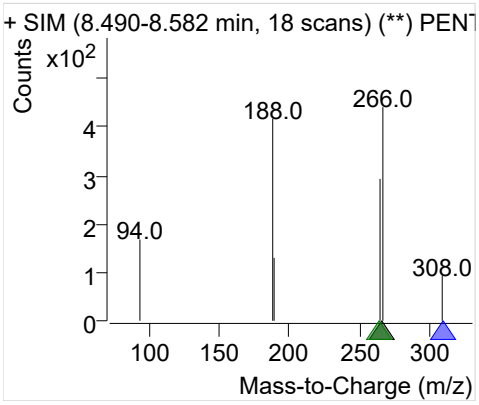

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:39:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 6:33:45	**Data File**	PENTA ST-03.D
Type	Cal	**Name**	PENTA ST-03
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

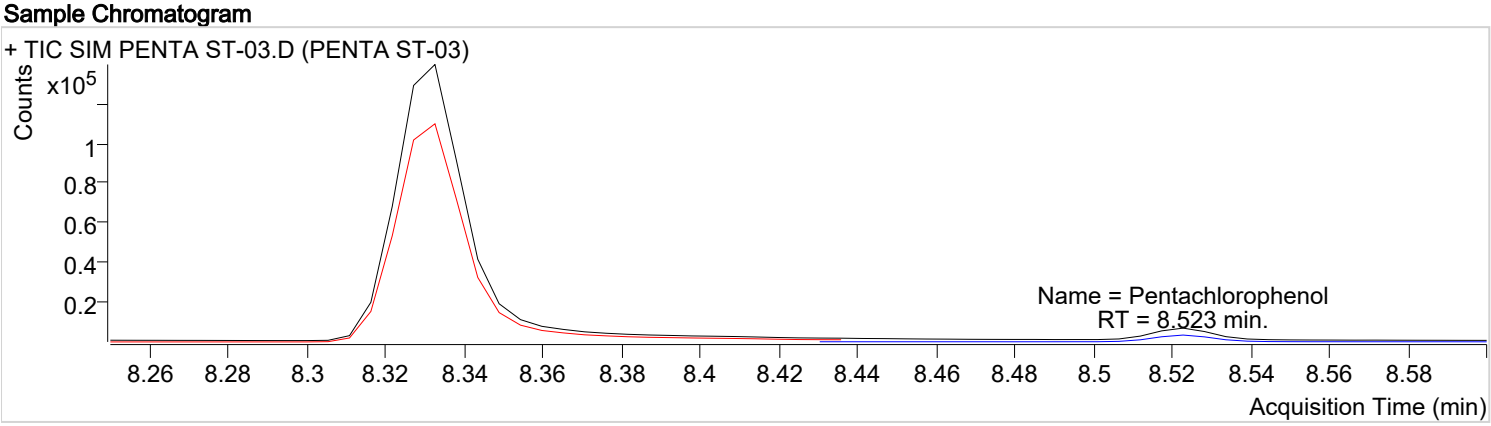

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	3635	142374	0.0025 mg/L

Pentachlorophenol

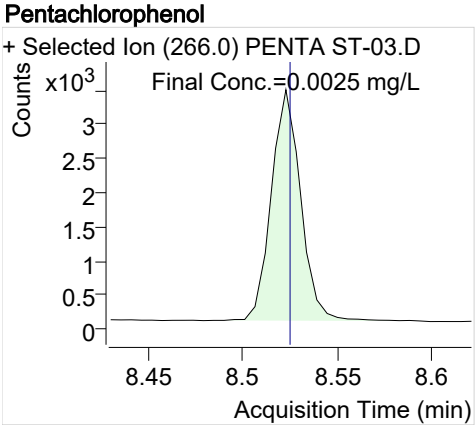

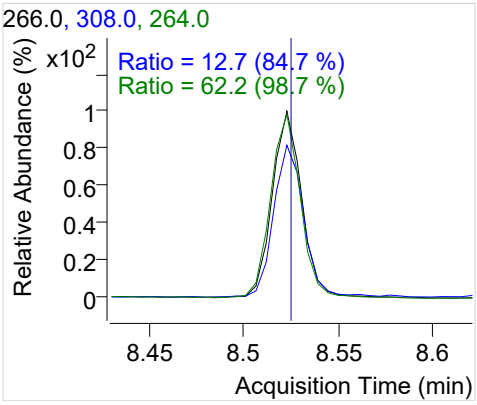

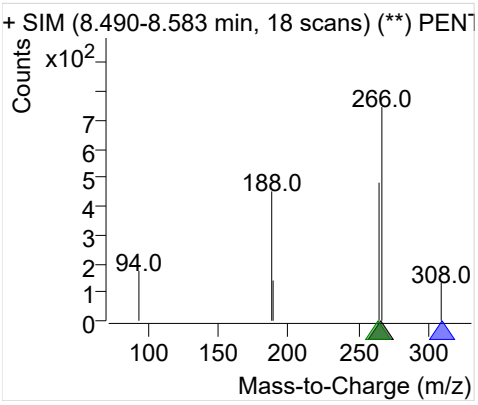

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:39:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 6:47:10	**Data File**	PENTA ST-04.D
Type	Cal	**Name**	PENTA ST-04
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

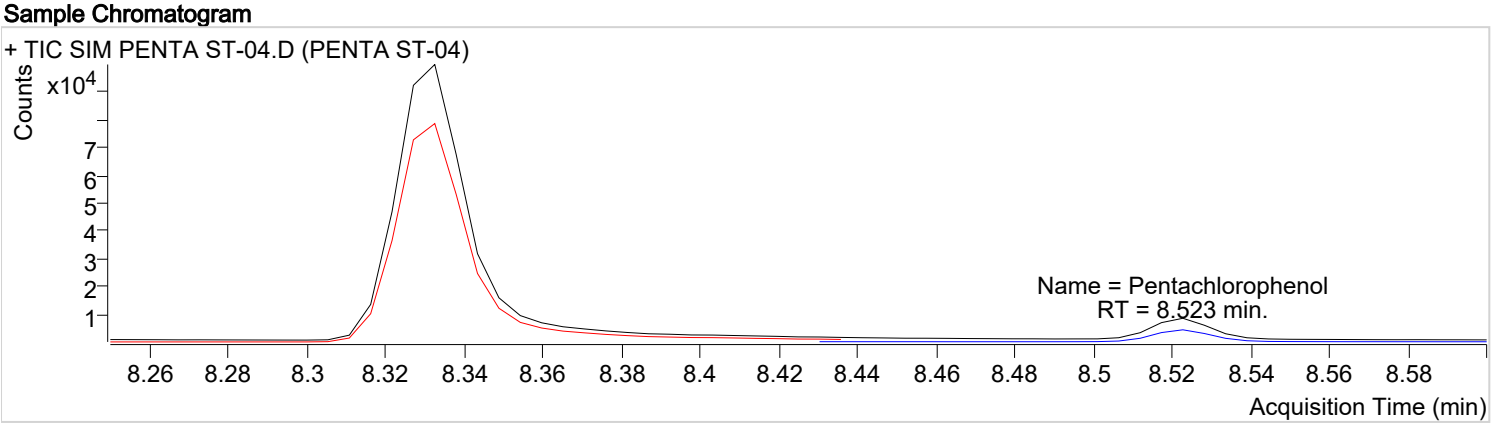

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	4550	104091	0.0039 mg/L

Pentachlorophenol

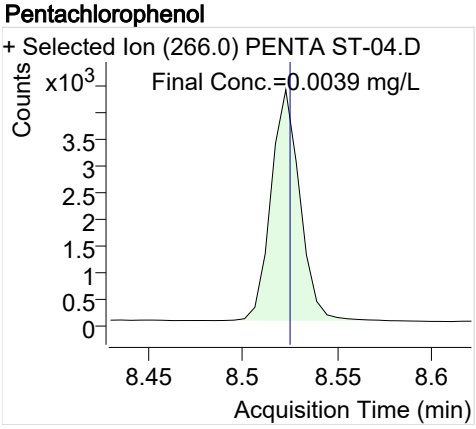

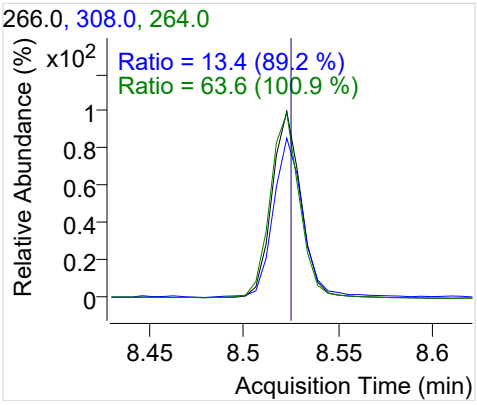

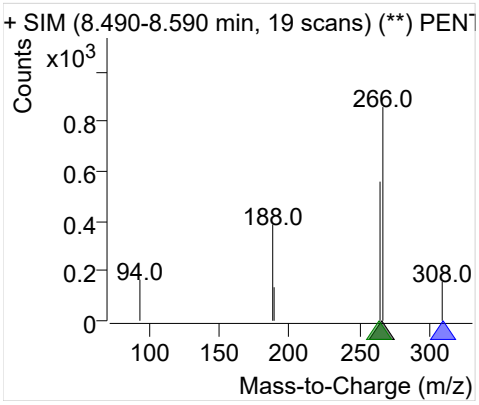

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:39:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 7:00:37	**Data File**	PENTA ST-05.D
Type	Cal	**Name**	PENTA ST-05
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

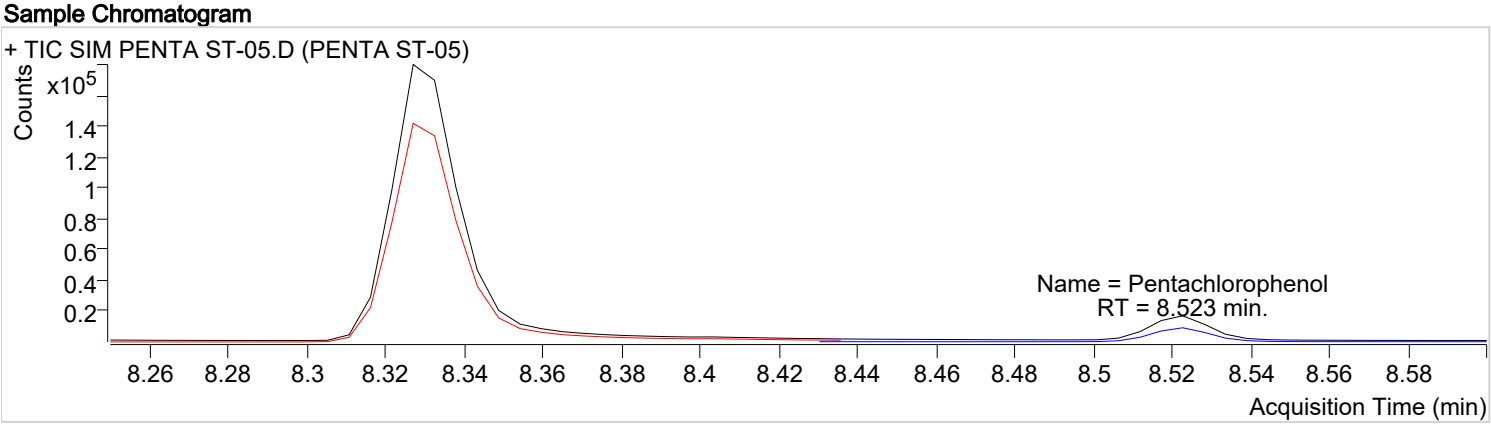

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	9551	180528	0.0046 mg/L

Pentachlorophenol

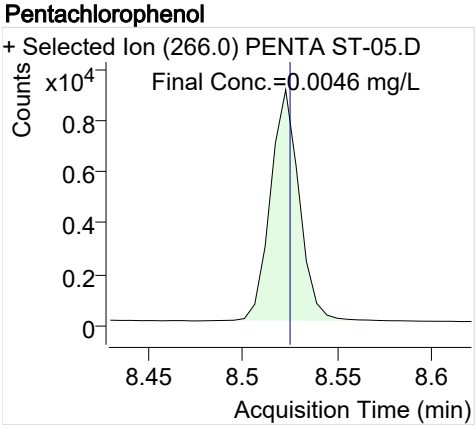

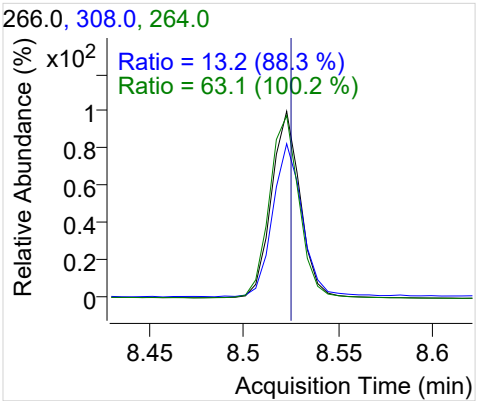

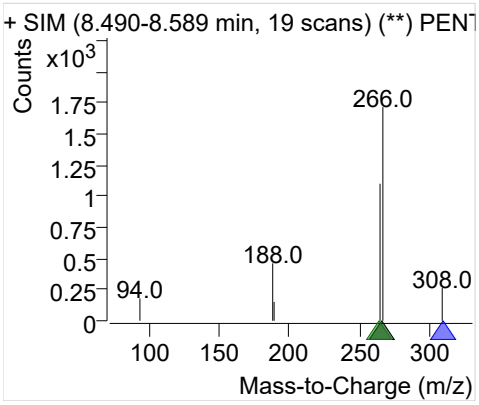

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:39:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 7:14:02	**Data File**	PENTA ST-06.D
Type	Cal	**Name**	PENTA ST-06
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

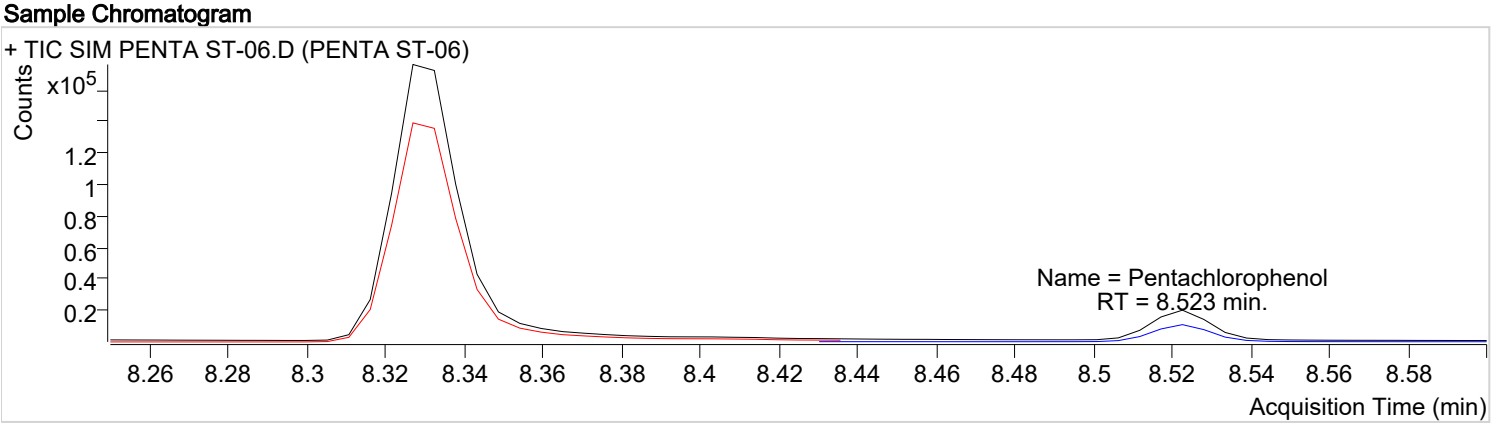

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	11864	176867	0.0057 mg/L

Pentachlorophenol

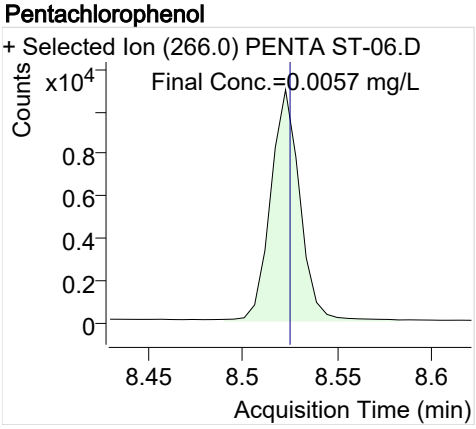

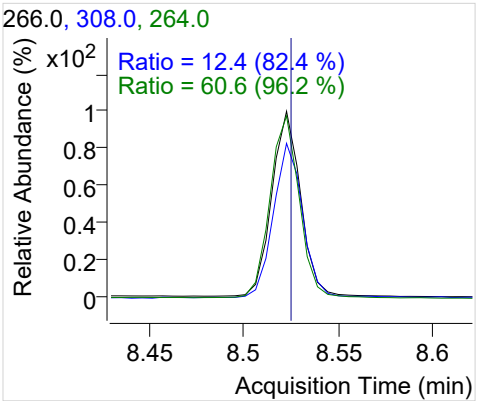

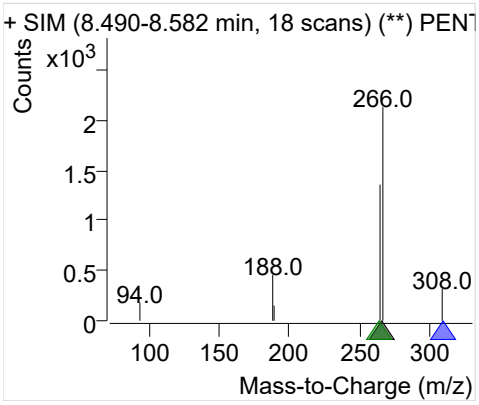

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:39:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 7:27:27	**Data File**	PENTA ST-07.D
Type	Cal	**Name**	PENTA ST-07
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

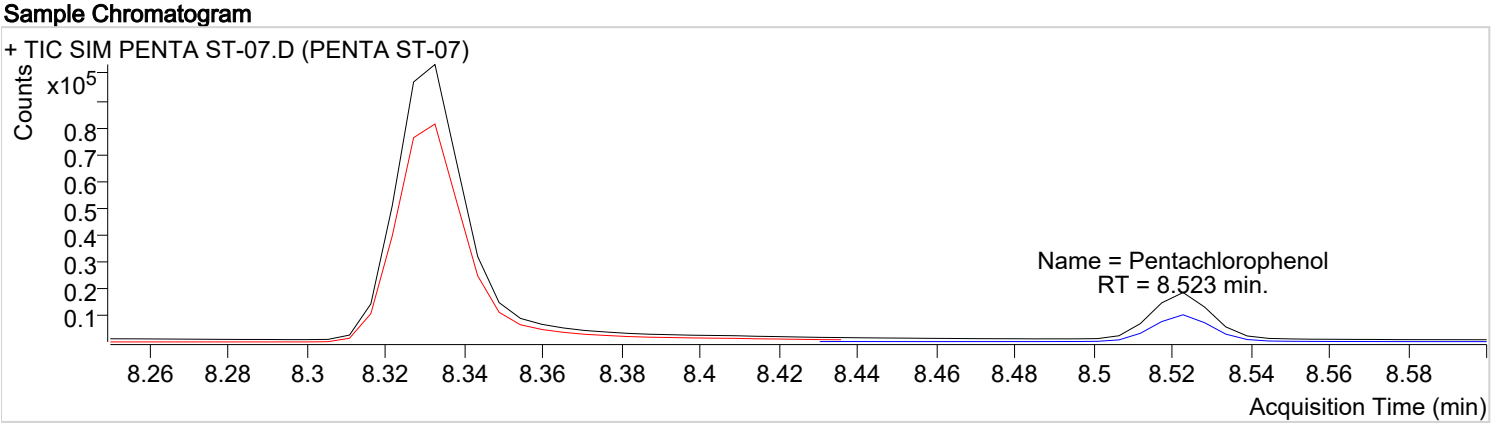

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	10573	105784	0.0082 mg/L

Pentachlorophenol

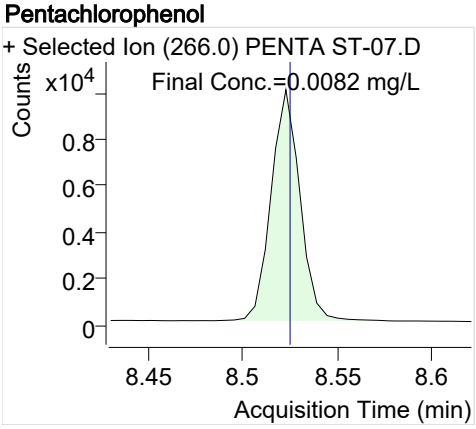

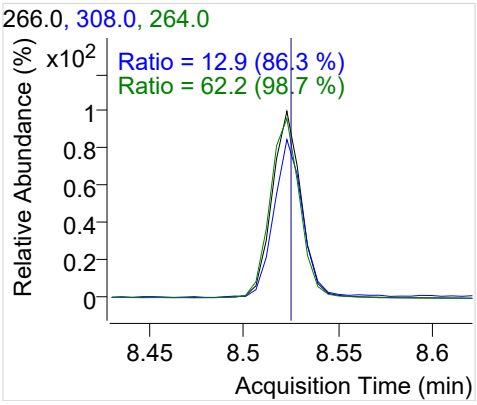

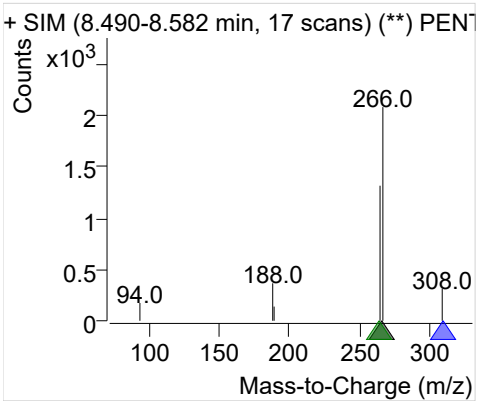

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:39:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 7:54:16	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

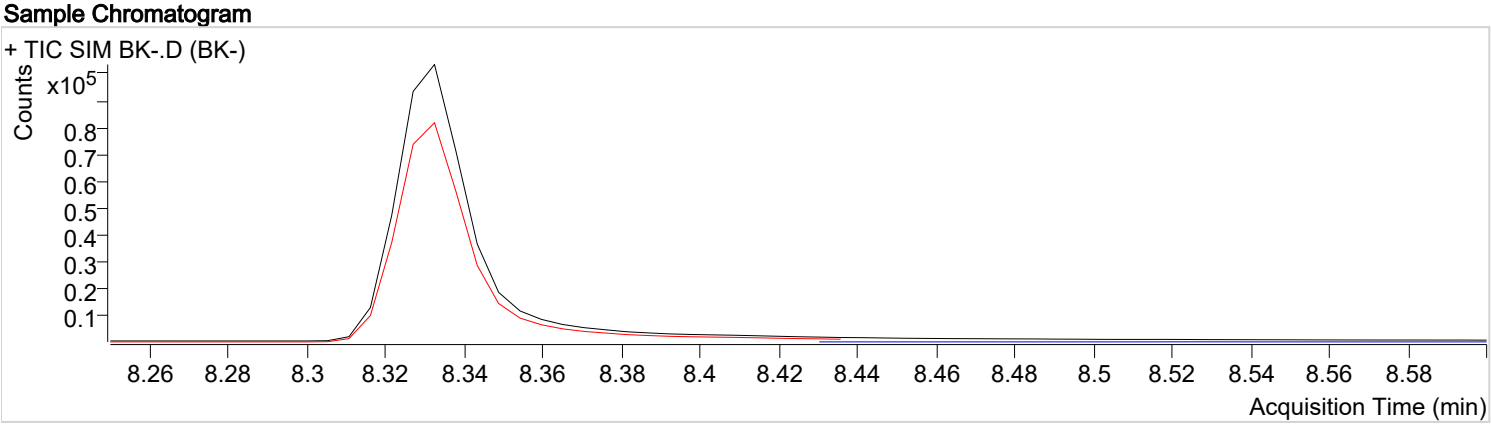

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			110780	ND mg/L

Pentachlorophenol

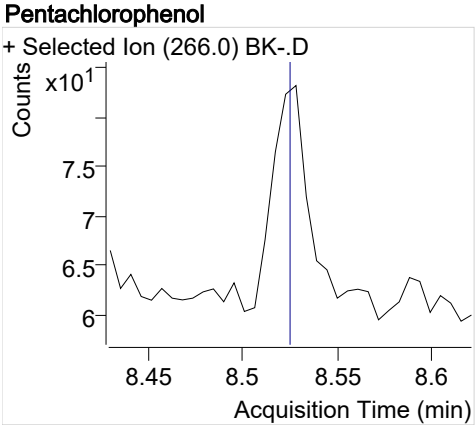



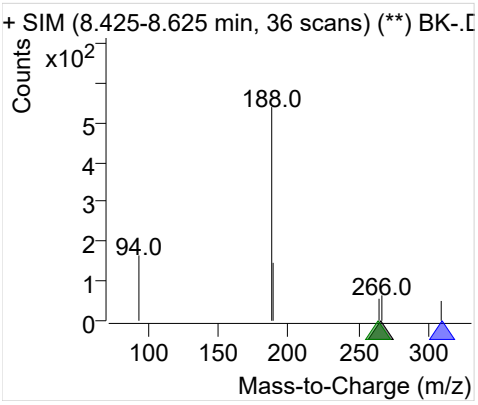

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:39:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 8:07:42	**Data File**	FBK(DL 26-02-26).D
Type	Blank	**Name**	FBK(DL 26-02-26)
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

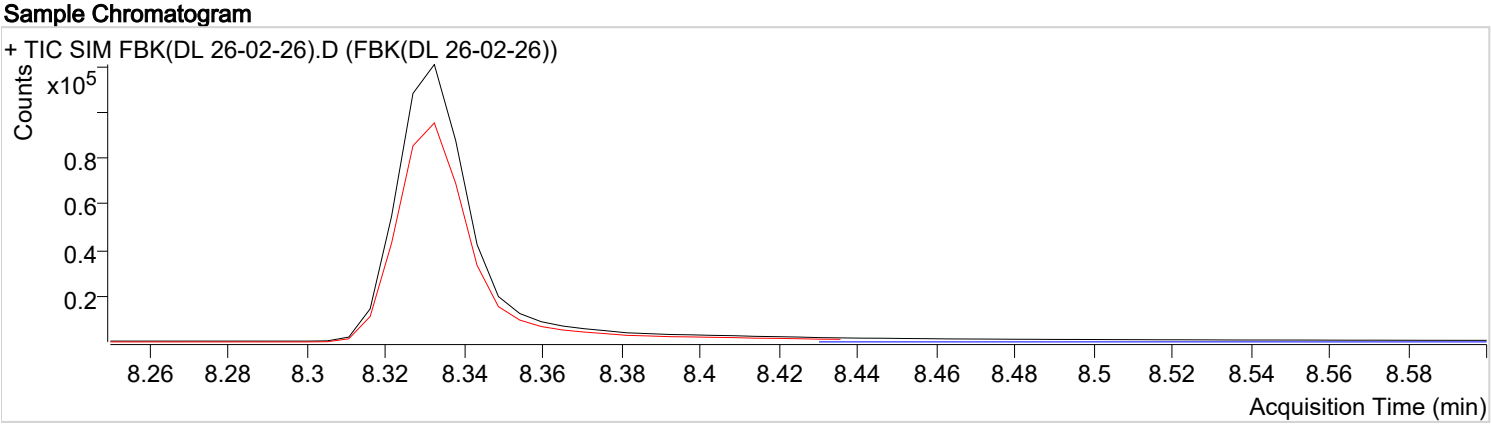

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			128402	ND mg/L

Pentachlorophenol

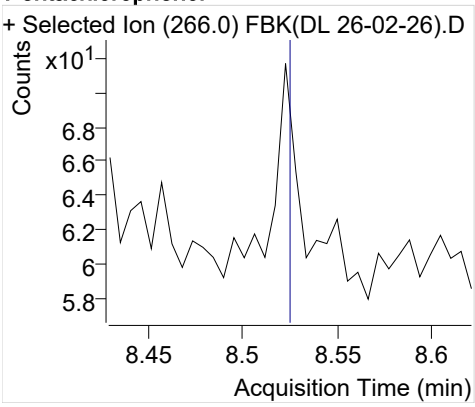



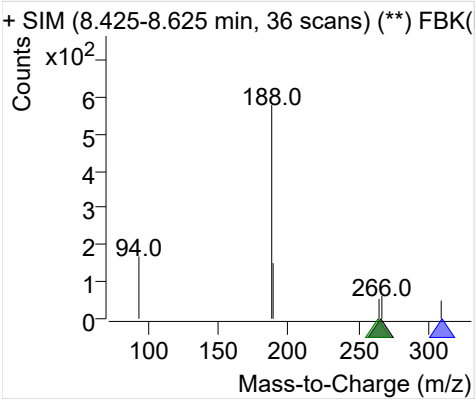

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:39:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 8:21:07	**Data File**	FBK(LT 26-02-26).D
Type	Blank	**Name**	FBK(LT 26-02-26)
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

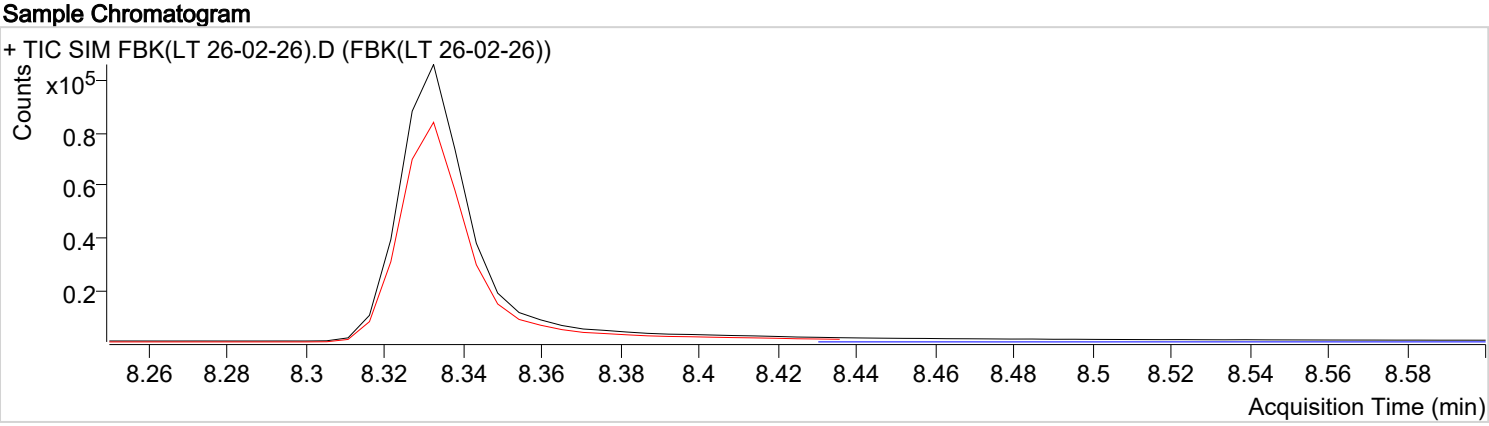

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			108408	ND mg/L

Pentachlorophenol

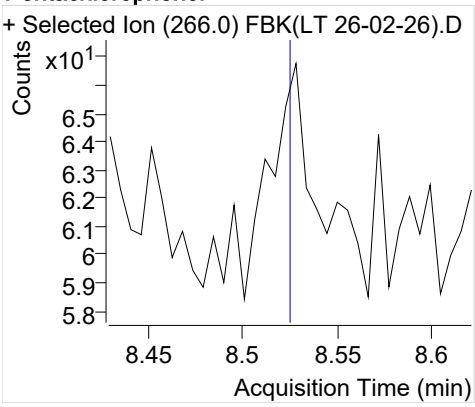



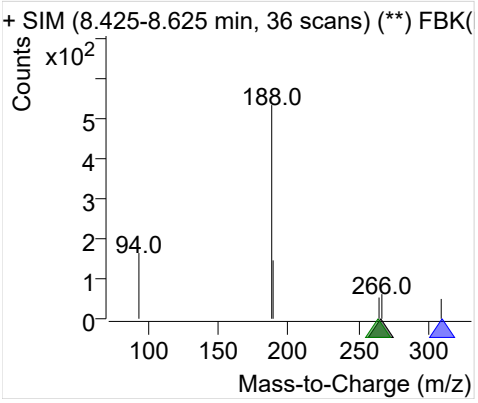

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:39:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 8:34:31	**Data File**	FBK(PL 26-02-27).D
Type	Blank	**Name**	FBK(PL 26-02-27)
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

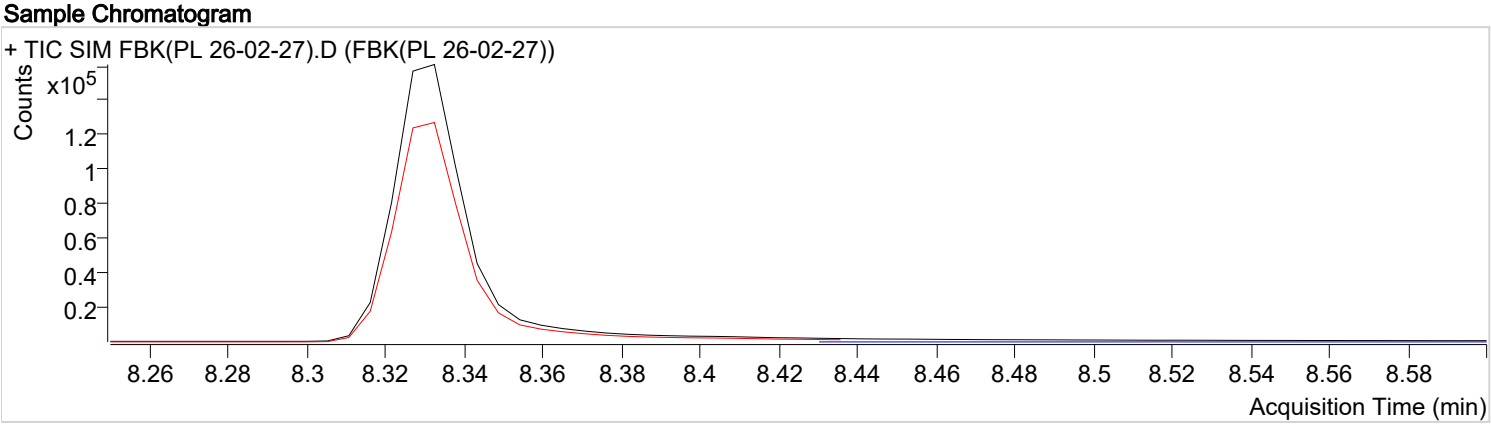

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			166878	ND mg/L

Pentachlorophenol

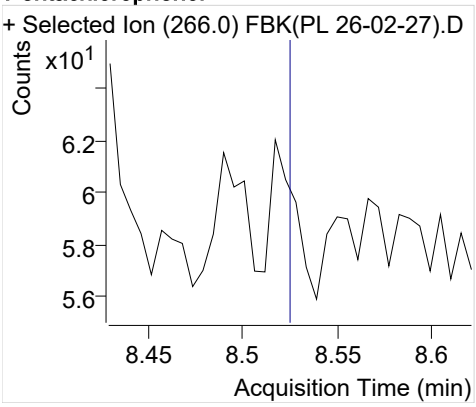

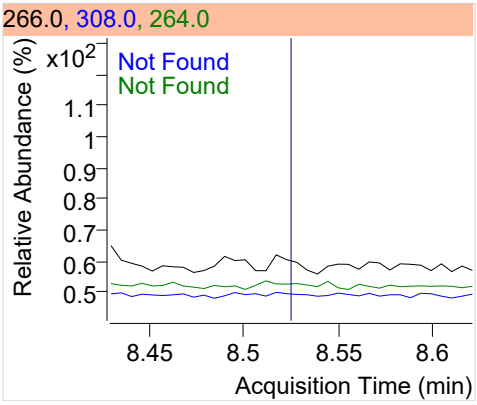

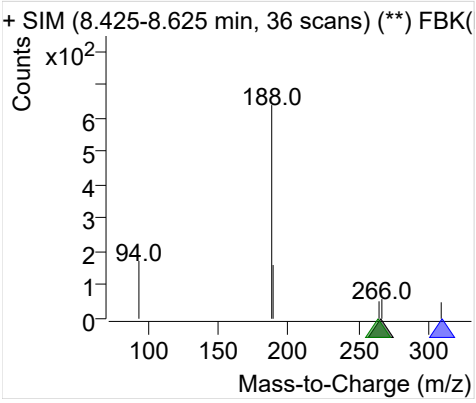

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:39:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 8:47:55	**Data File**	DL-01.D
Type	Sample	**Name**	DL-01
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

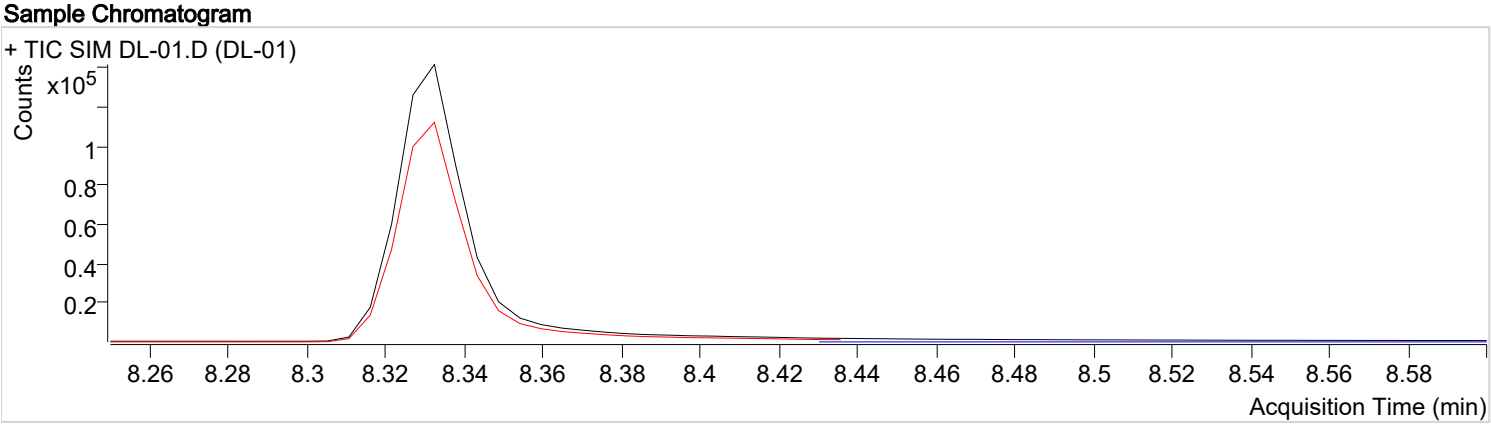

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			142432	ND mg/L

Pentachlorophenol

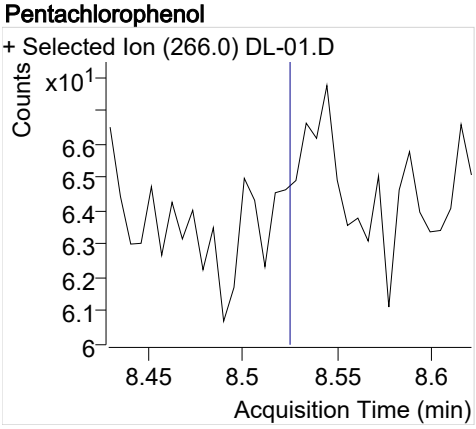



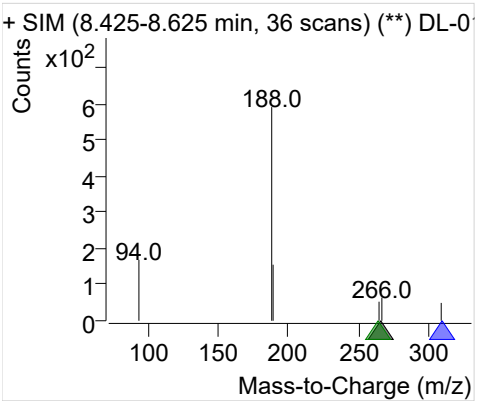

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:39:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 9:01:19	**Data File**	LT-01.D
Type	Sample	**Name**	LT-01
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

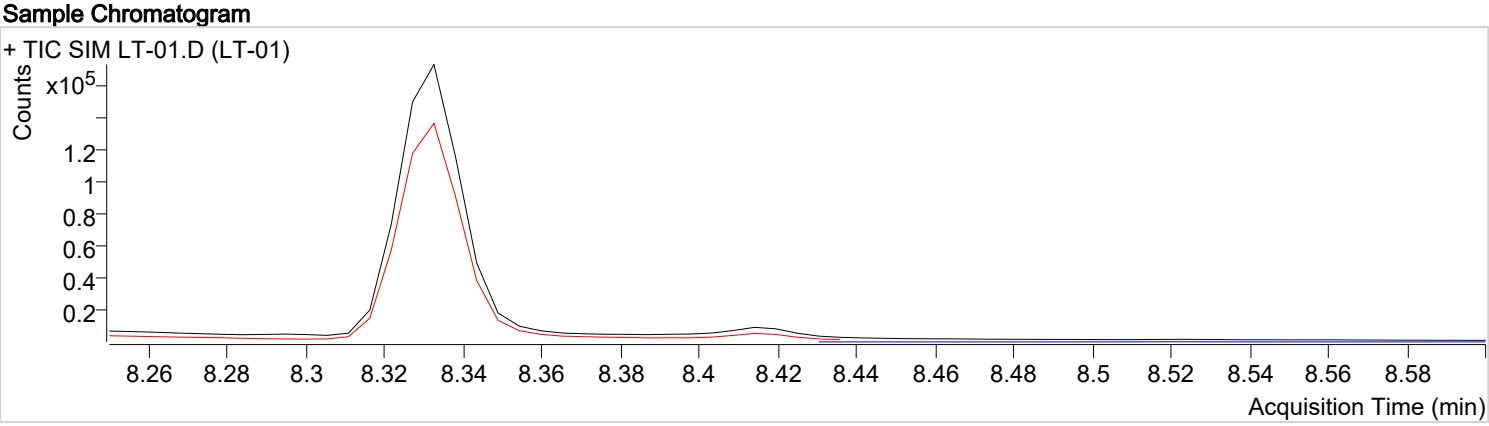

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	0	161958	ND mg/L

Pentachlorophenol

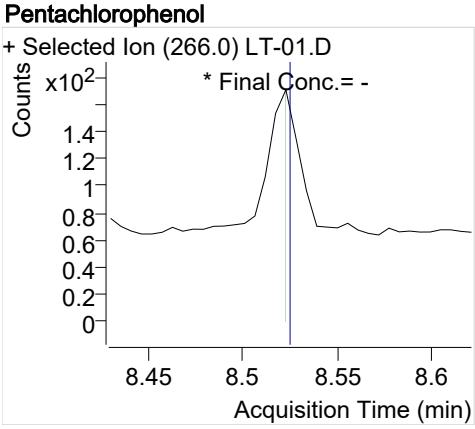





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:39:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 9:14:44	**Data File**	LT-02.D
Type	Sample	**Name**	LT-02
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

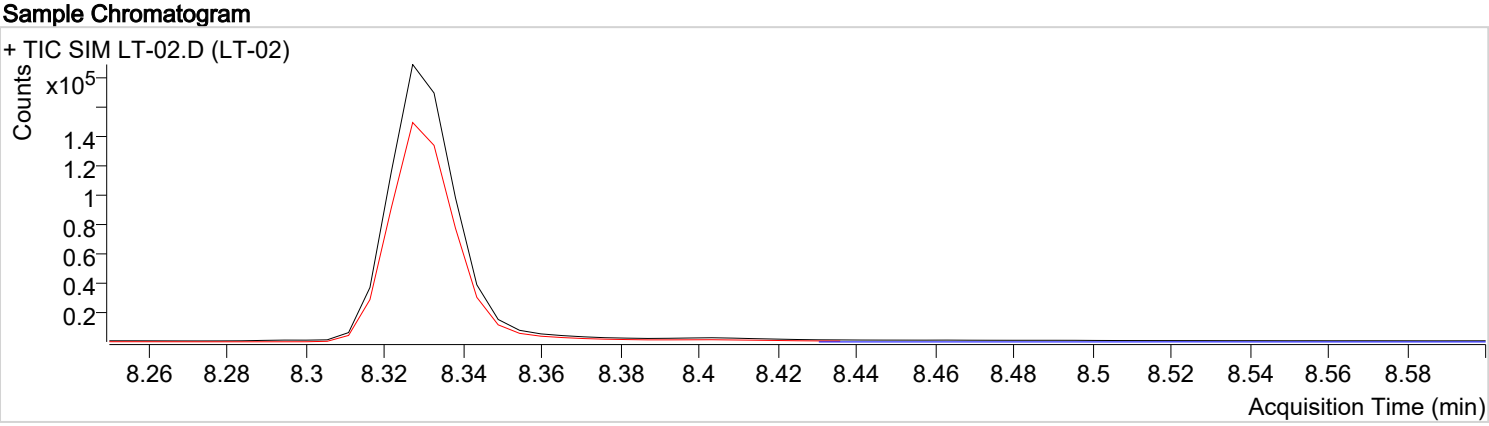

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			177964	ND mg/L

Pentachlorophenol

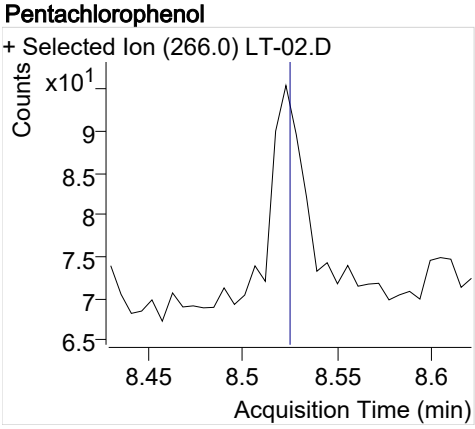



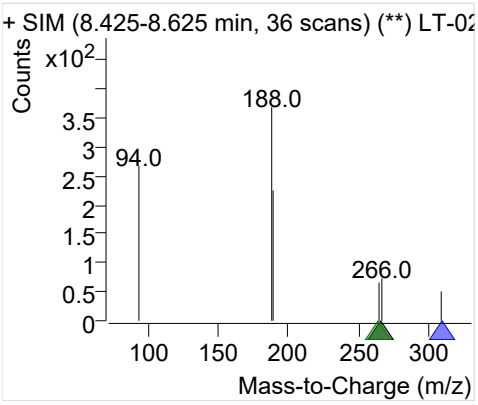

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:39:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 9:28:11	**Data File**	LT-03.D
Type	Sample	**Name**	LT-03
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

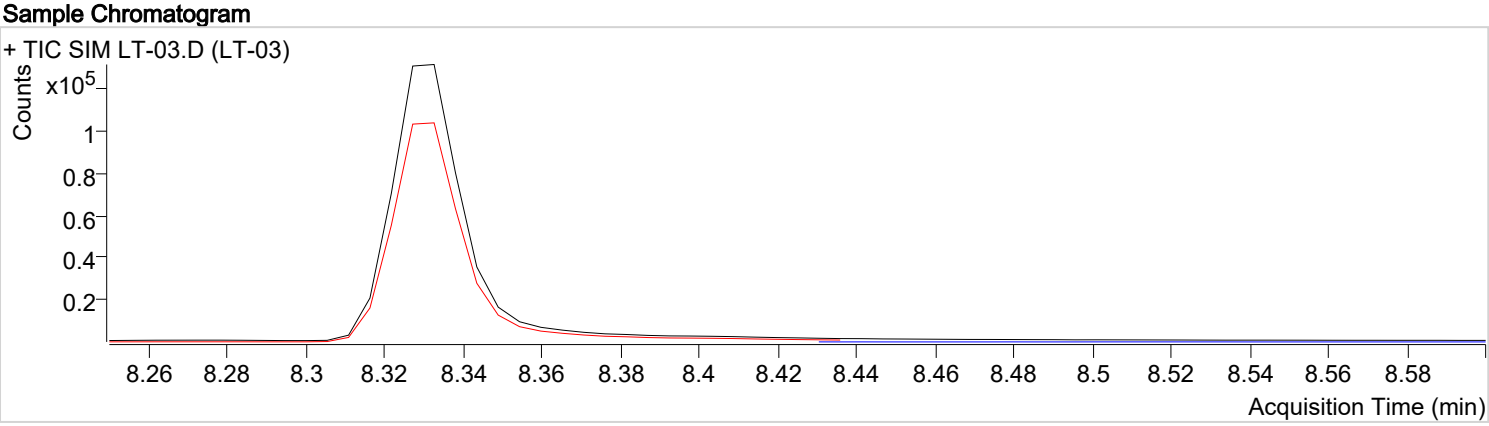

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			135135	ND mg/L

Pentachlorophenol

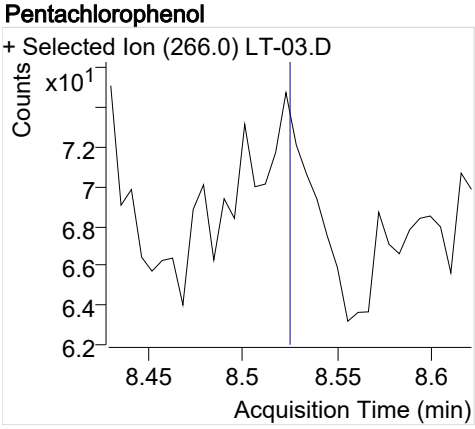



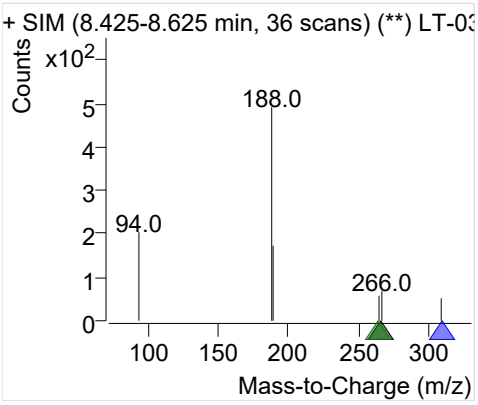

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:39:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 9:41:36	**Data File**	PL-01.D
Type	Sample	**Name**	PL-01
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

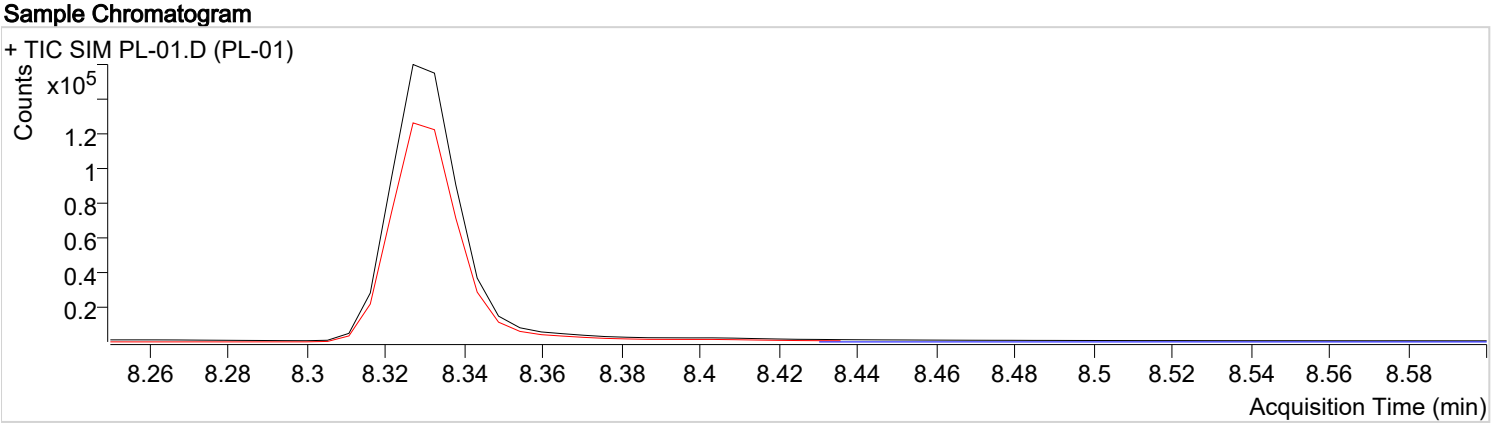

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			160062	ND mg/L

Pentachlorophenol

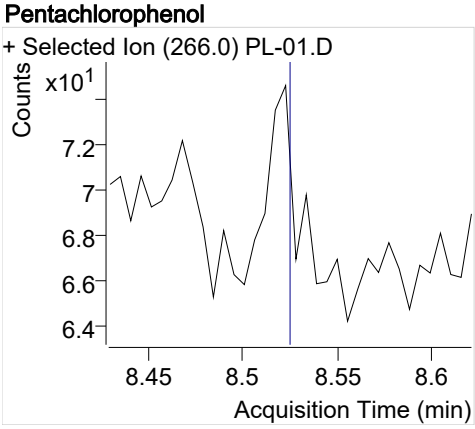



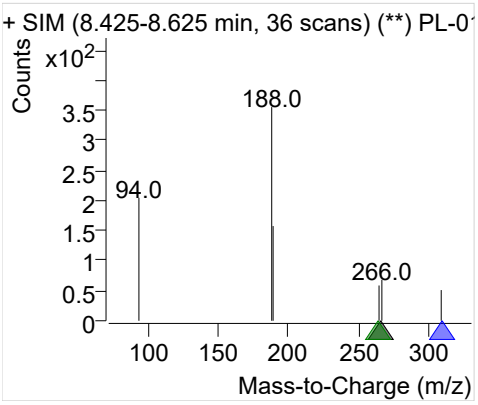

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:39:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 9:55:01	**Data File**	PL-02.D
Type	Sample	**Name**	PL-02
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

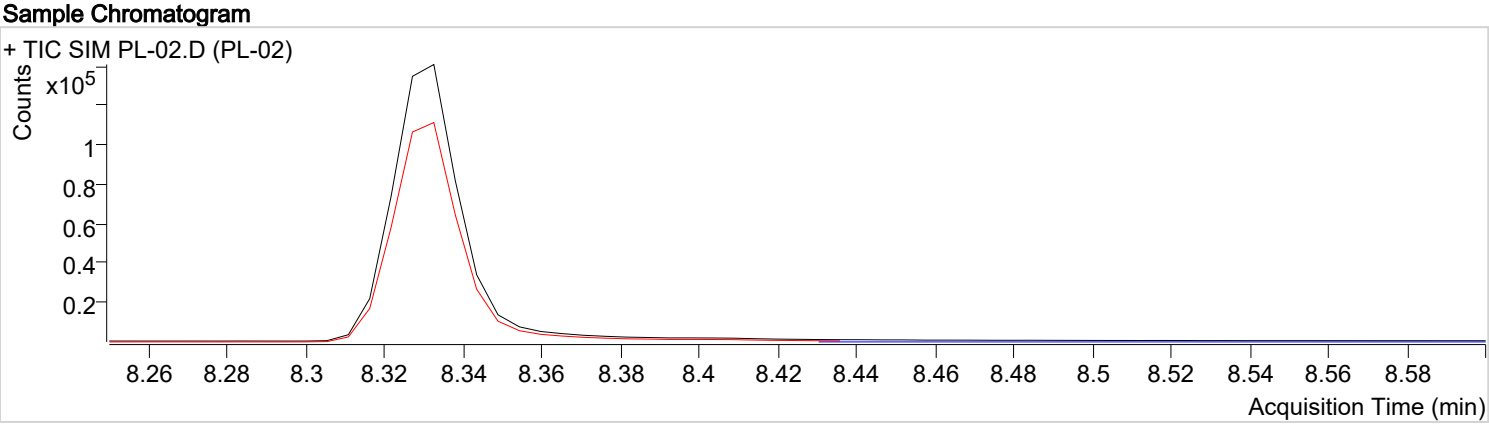

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			136954	ND mg/L

Pentachlorophenol

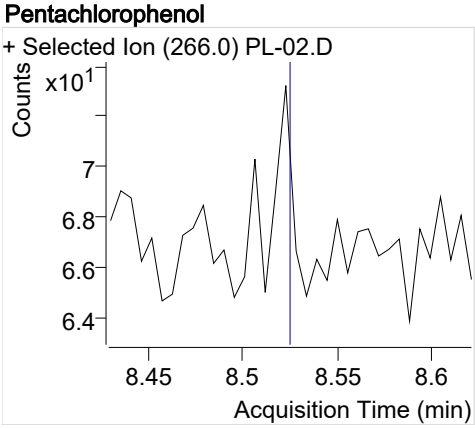



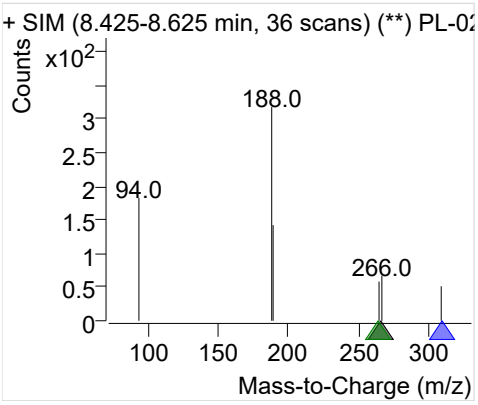

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:39:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 10:08:26	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

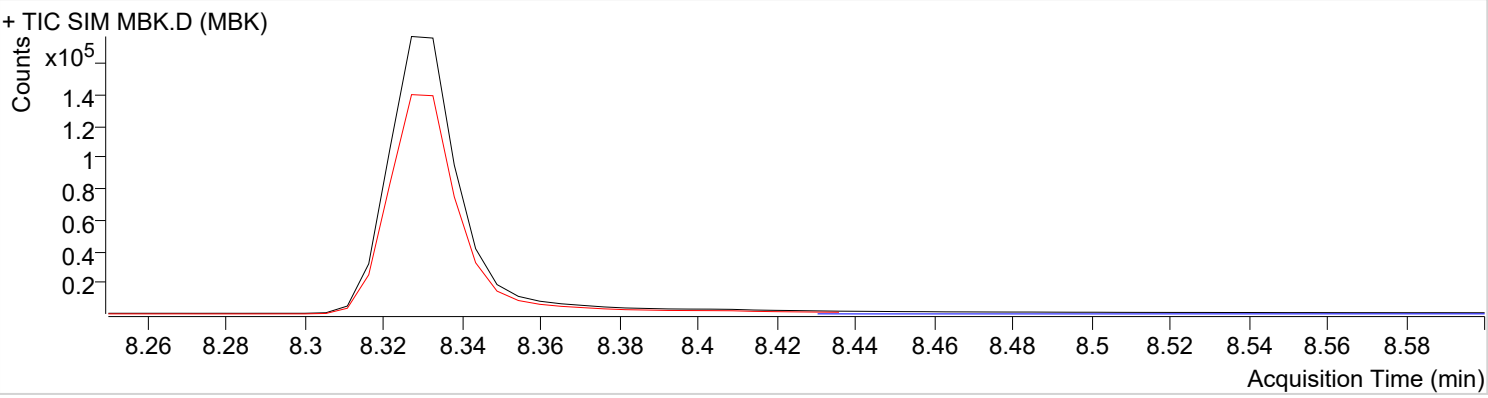

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			182114	ND mg/L

Pentachlorophenol

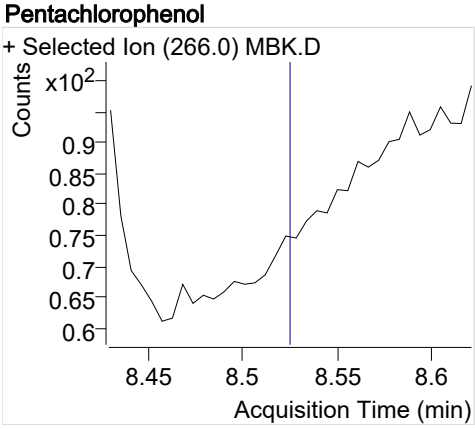



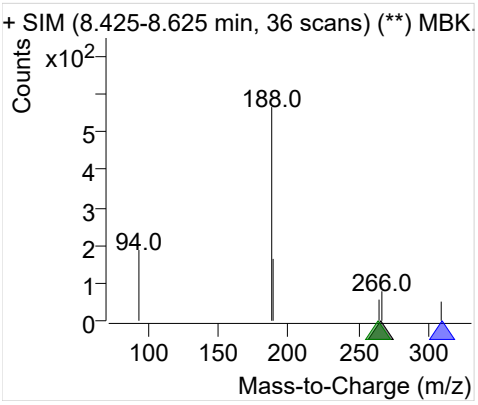

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\2. 2026-02\PENTA(DL 2.26 LT 2.26 PL 2.27)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-02-28 오전 9:58:20	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:39:05	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-28 오전 9:58:20	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-27 오후 10:35:16	**Data File**	-CCV-.D
Type	QC	**Name**	-CCV-
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

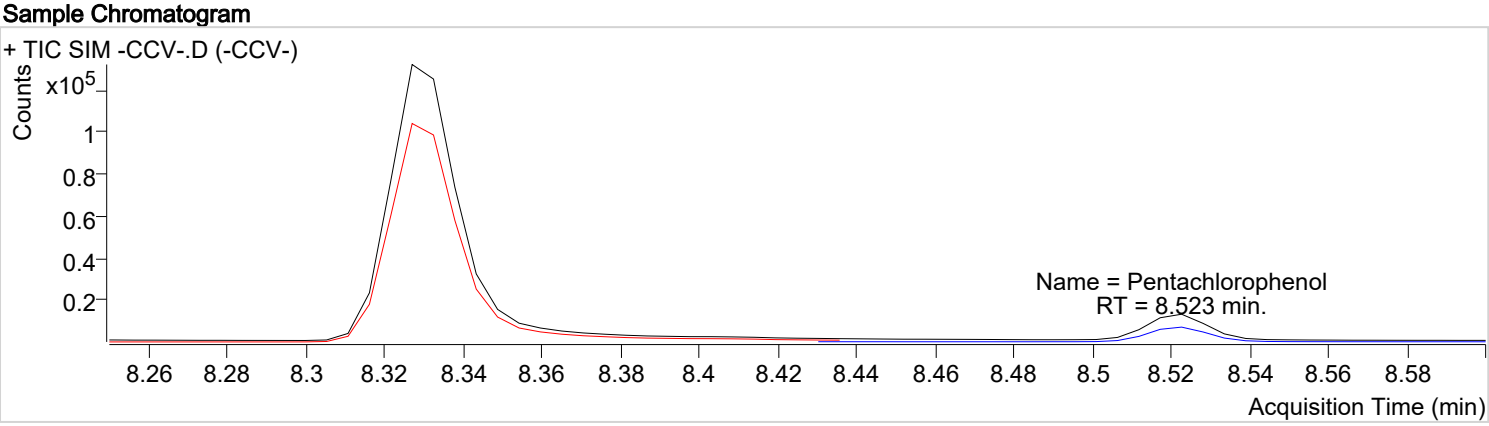

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	7632	134719	0.0049 mg/L
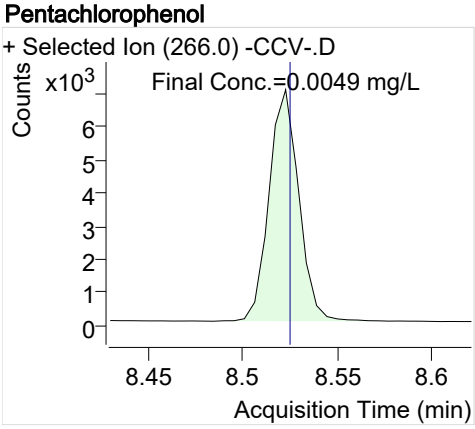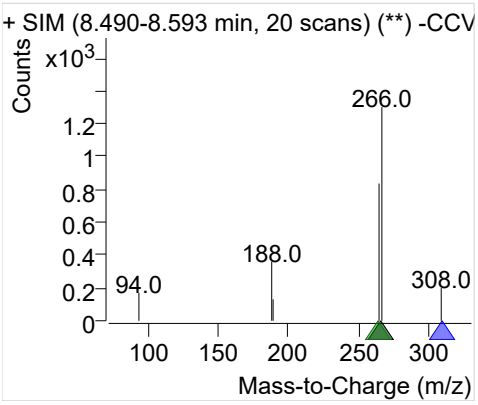
Pentachlorophenol