Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin				
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Pentachlorophenol

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
PENTA ST-01.D	Cal	8.523	1383	131184	0.0013
PENTA ST-02.D	Cal	8.523	3497	122372	0.0019
PENTA ST-03.D	Cal	8.523	5820	96758	0.0029
PENTA ST-04.D	Cal	8.523	11110	130378	0.0036
PENTA ST-05.D	Cal	8.523	15986	127419	0.0049
PENTA ST-06.D	Cal	8.523	22698	128956	0.0064
PENTA ST-07.D	Cal	8.523	33665	147406	0.0080
BK-.D	Blank			137921	ND
FBK(RE 26-03-04).D	Blank			123185	ND
FBK(KD 26-03-04).D	Blank			126837	ND
RE-01.D	Sample	8.523	3248	126669	0.0018
RE-02.D	Sample			131472	ND
RE-03.D	Sample			99413	ND
RE-04.D	Sample	8.517	1436	124077	0.0014
RE-09.D	Sample			124807	ND
RE-10.D	Sample			112072	ND
RE-11.D	Sample			126187	ND
RE-12.D	Sample			116712	ND
KD-01.D	Sample			123791	ND
KD-02.D	Sample			133801	ND
KD-03.D	Sample			120648	ND
MBK.D	Blank			149422	ND
-CCV-.D	QC	8.523	11853	141582	0.0036

Pentachlorophenol

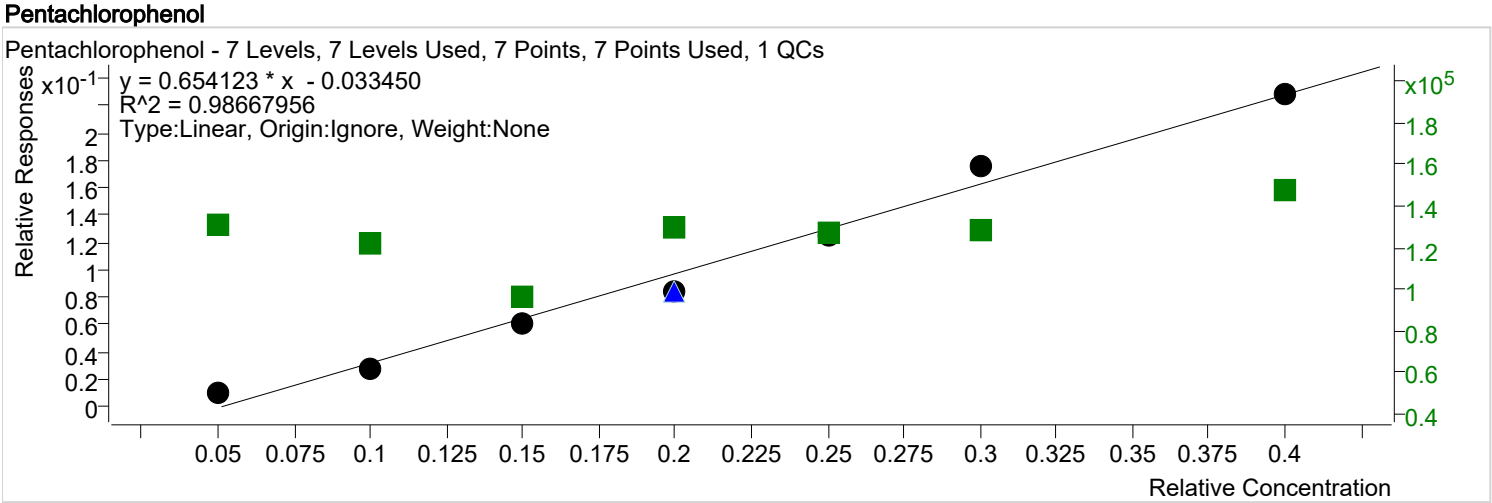

Cal. Path	Type	Level	Enable	Conc.	Response
\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\PENTA ST-01.D	Calibration	1	x	0.500	1383
\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\PENTA ST-02.D	Calibration	2	x	1.000	3497
\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\PENTA ST-03.D	Calibration	3	x	1.500	5820
\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\PENTA ST-04.D	Calibration	4	x	2.000	11110
\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\-CCV-.D	QC	4	x	2.000	11853
\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\PENTA ST-05.D	Calibration	5	x	2.500	15986
\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\PENTA ST-06.D	Calibration	6	x	3.000	22698
\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\PENTA ST-07.D	Calibration	7	x	4.000	33665

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 3:09:08	**Data File**	PENTA ST-01.D
Type	Cal	**Name**	PENTA ST-01
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

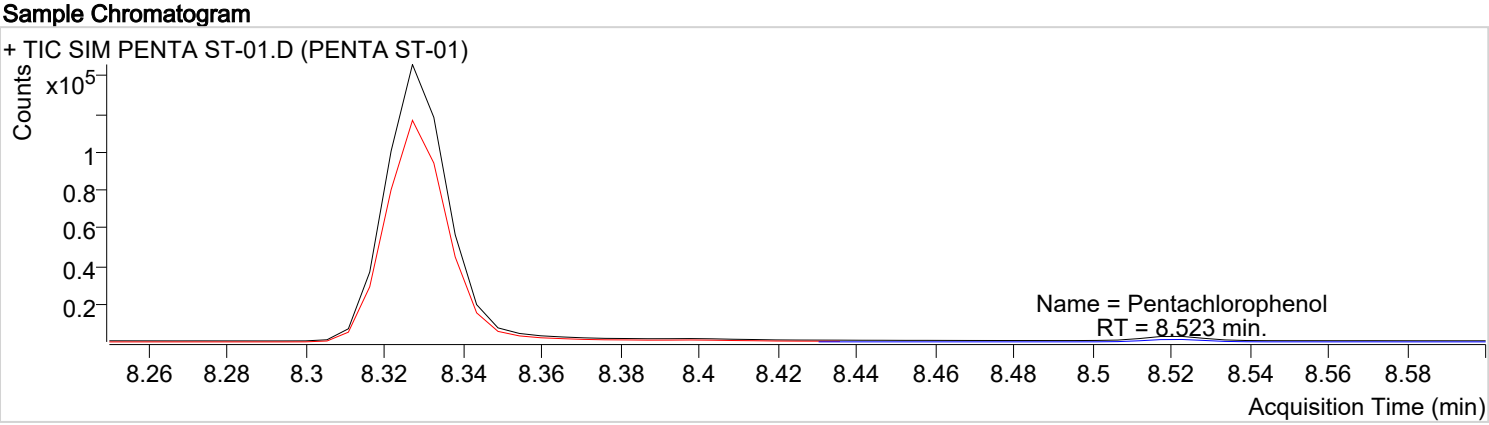

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	1383	131184	0.0013 mg/L

Pentachlorophenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 3:22:30	**Data File**	PENTA ST-02.D
Type	Cal	**Name**	PENTA ST-02
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

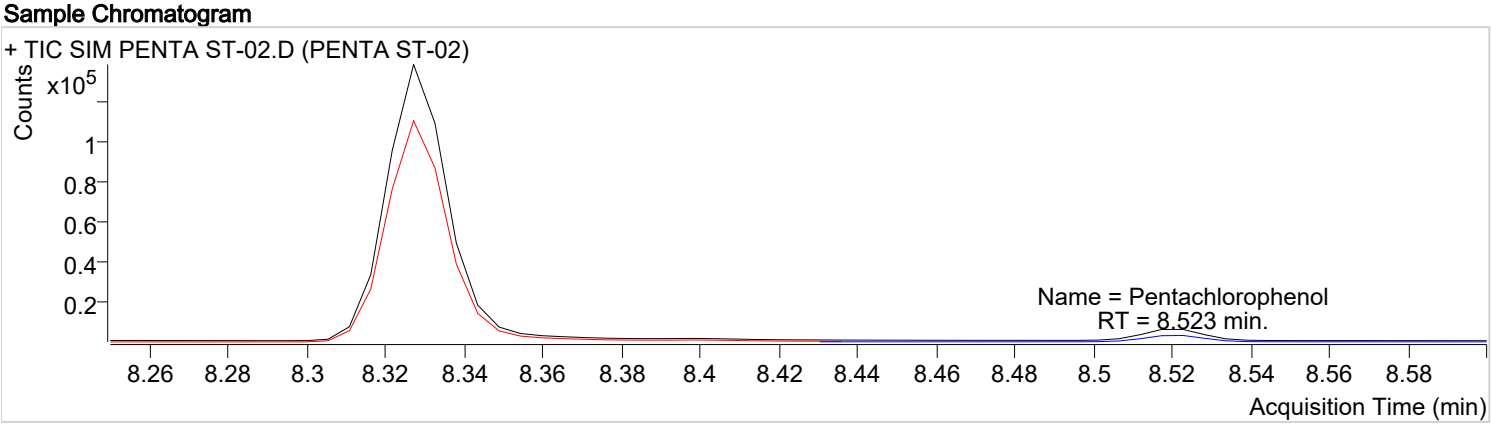

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	3497	122372	0.0019 mg/L

Pentachlorophenol





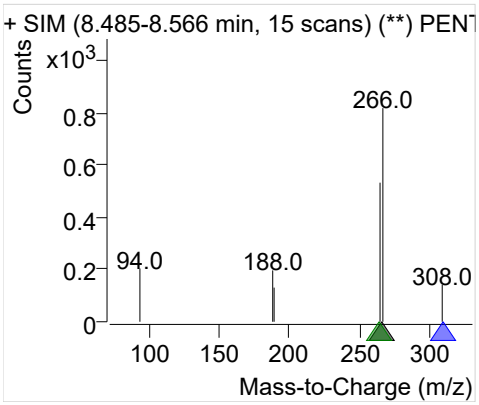

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 3:35:50	**Data File**	PENTA ST-03.D
Type	Cal	**Name**	PENTA ST-03
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

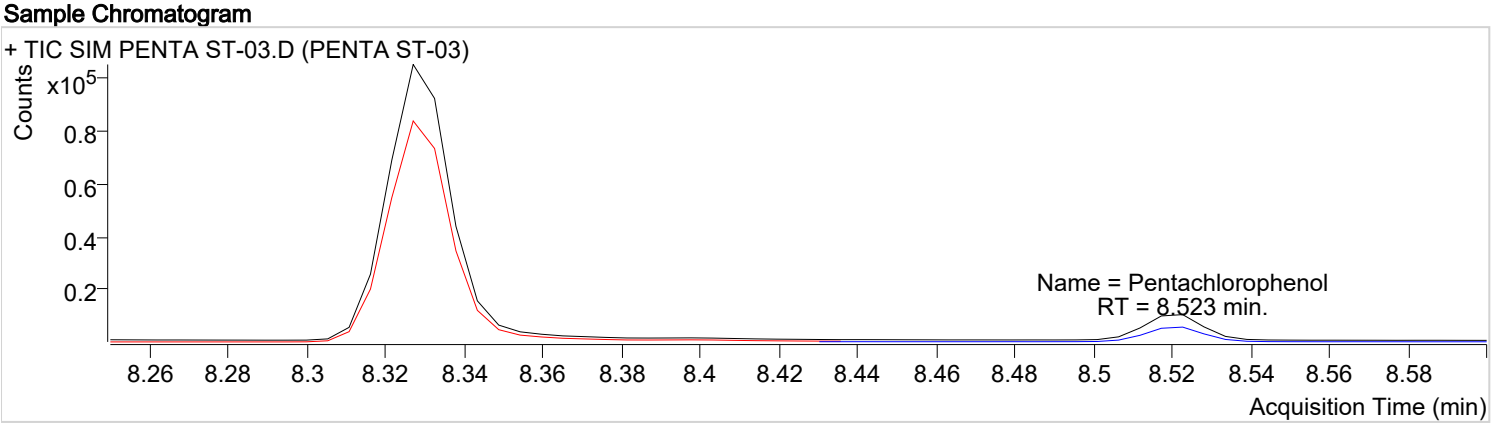

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	5820	96758	0.0029 mg/L

Pentachlorophenol





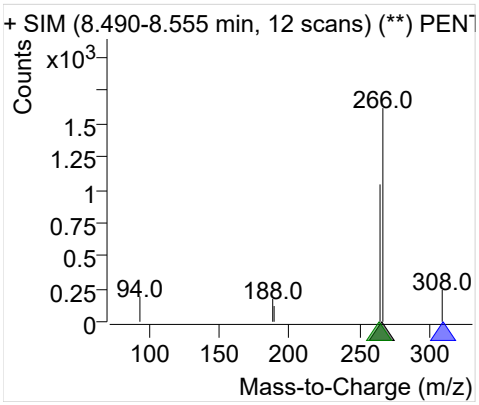

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 3:49:13	**Data File**	PENTA ST-04.D
Type	Cal	**Name**	PENTA ST-04
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

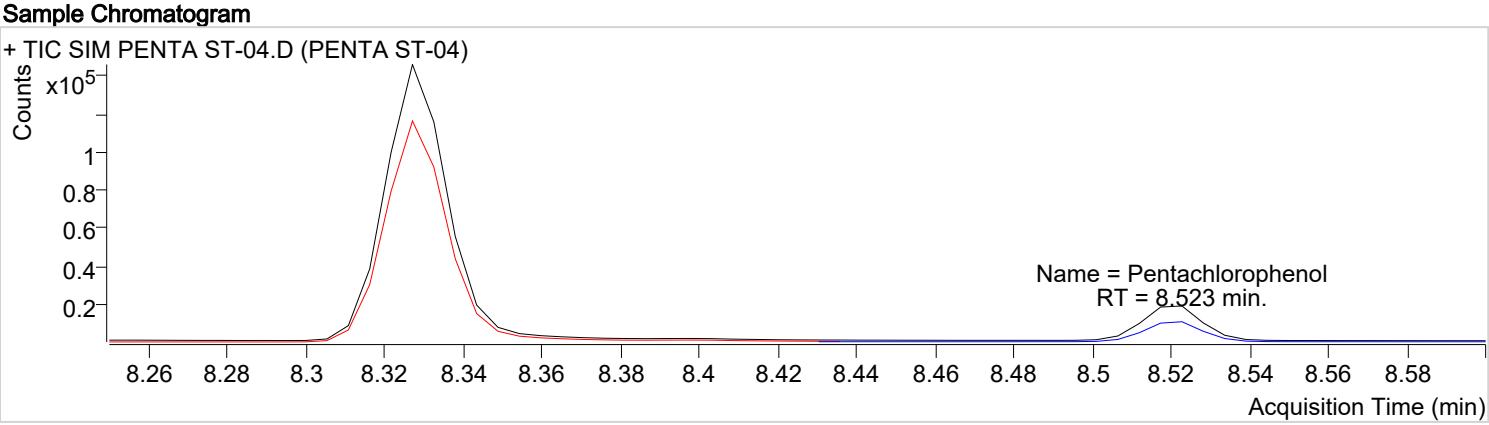

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	11110	130378	0.0036 mg/L

Pentachlorophenol

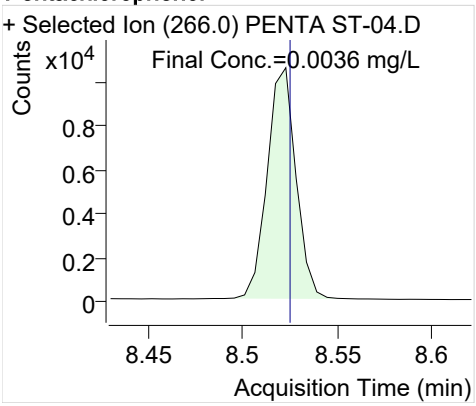

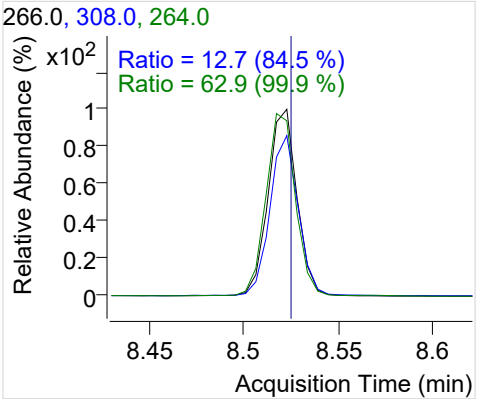

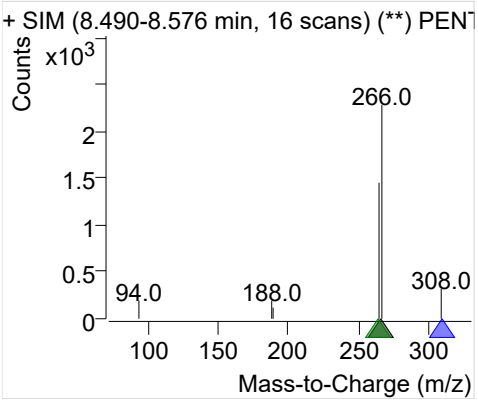

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 4:02:35	**Data File**	PENTA ST-05.D
Type	Cal	**Name**	PENTA ST-05
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

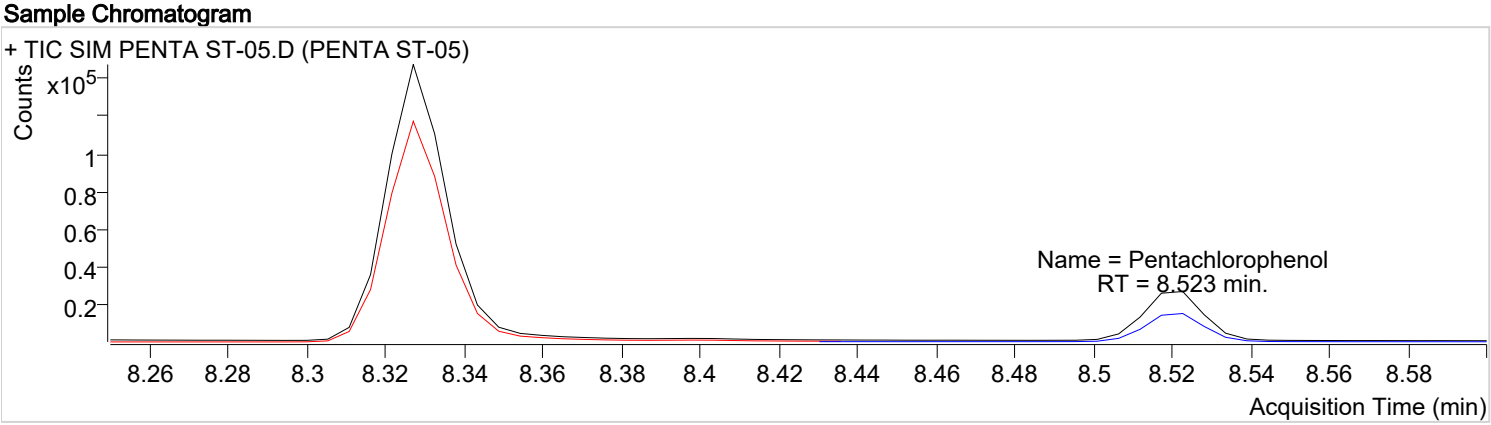

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	15986	127419	0.0049 mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 4:15:57	**Data File**	PENTA ST-06.D
Type	Cal	**Name**	PENTA ST-06
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

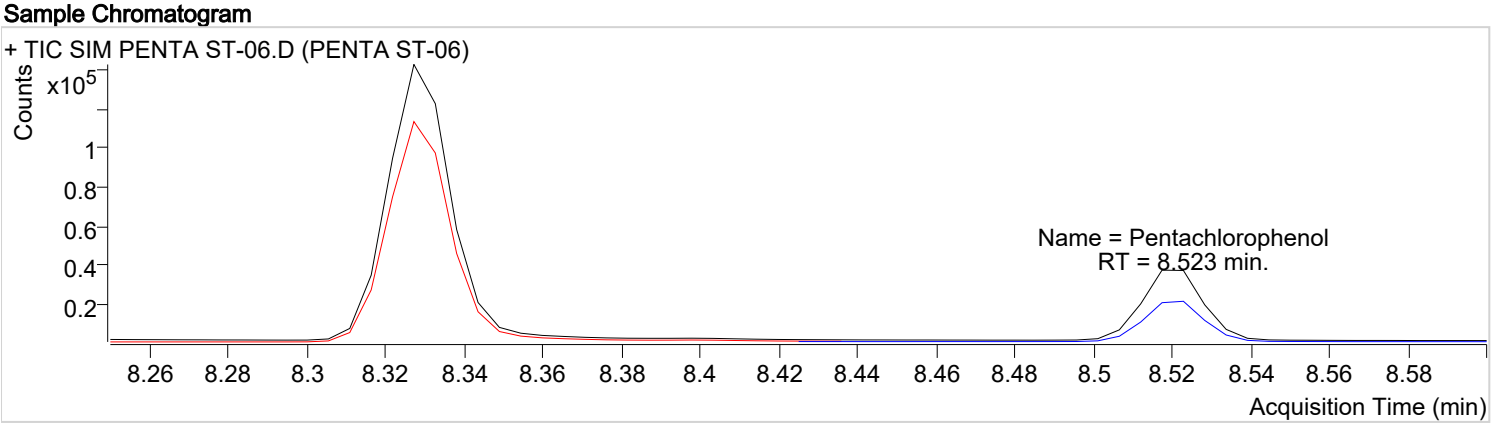

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	22698	128956	0.0064 mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 4:29:20	**Data File**	PENTA ST-07.D
Type	Cal	**Name**	PENTA ST-07
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

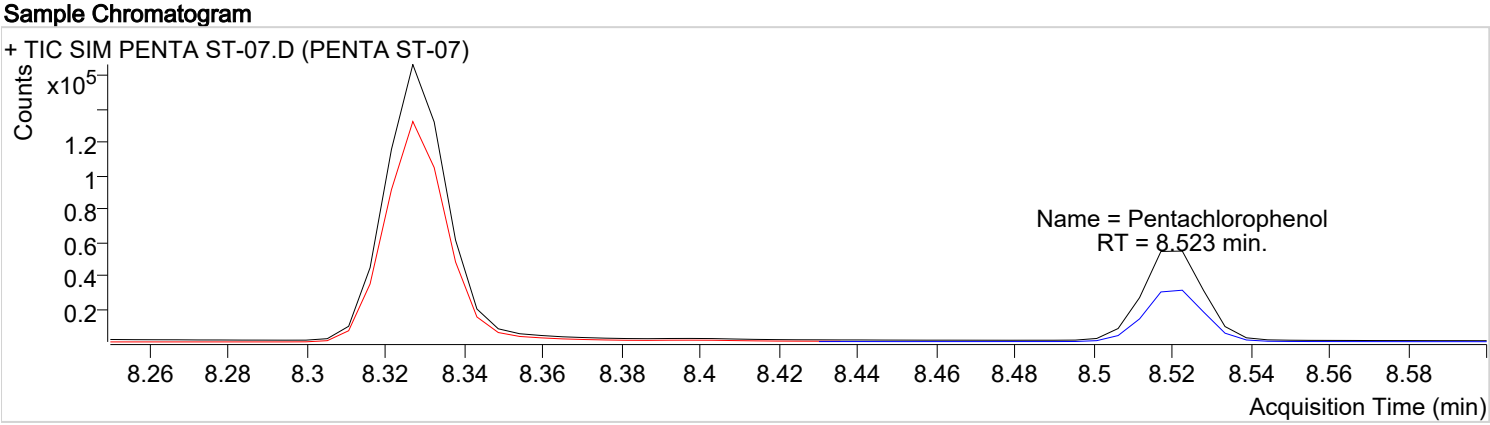

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	33665	147406	0.0080 mg/L

Pentachlorophenol





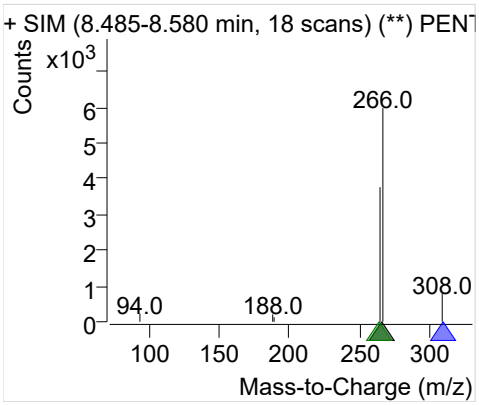

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 4:56:06	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

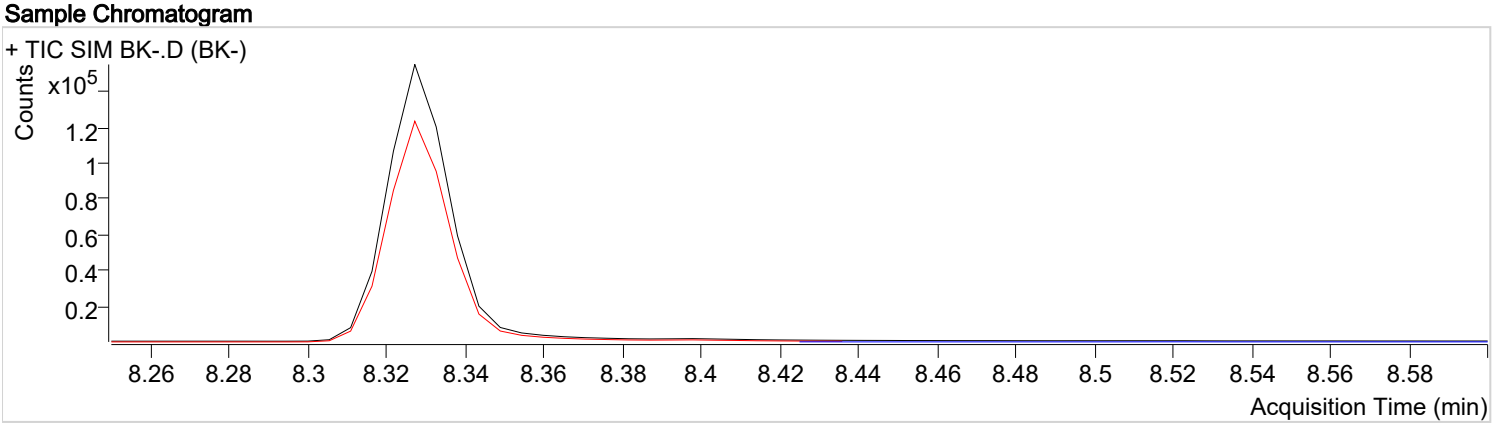

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			137921	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 5:09:31	**Data File**	FBK(RE 26-03-04).D
Type	Blank	**Name**	FBK(RE 26-03-04)
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

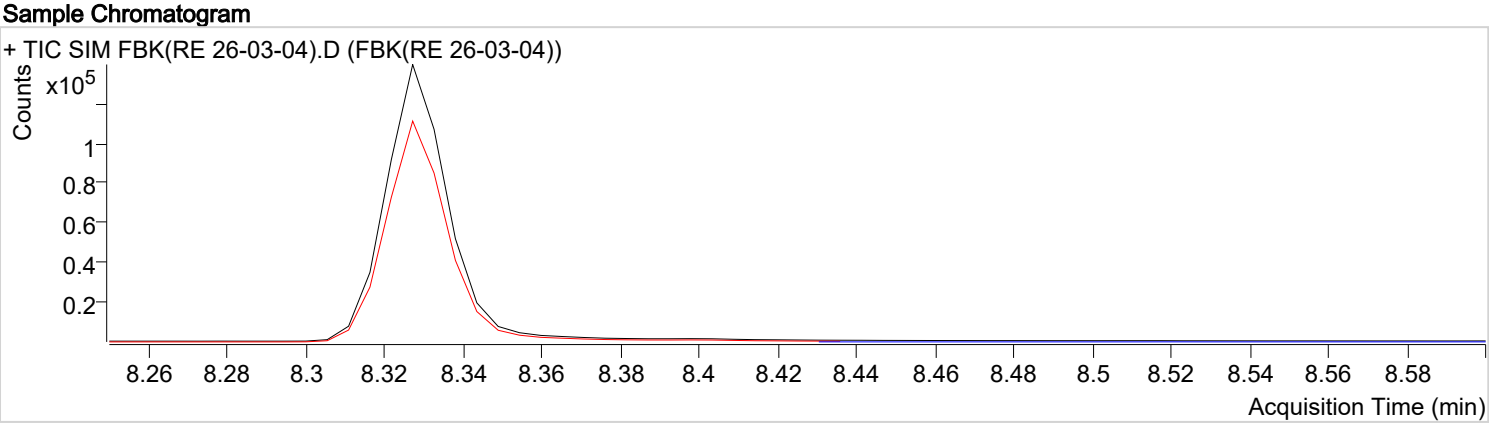

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			123185	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 5:22:52	**Data File**	FBK(KD 26-03-04).D
Type	Blank	**Name**	FBK(KD 26-03-04)
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

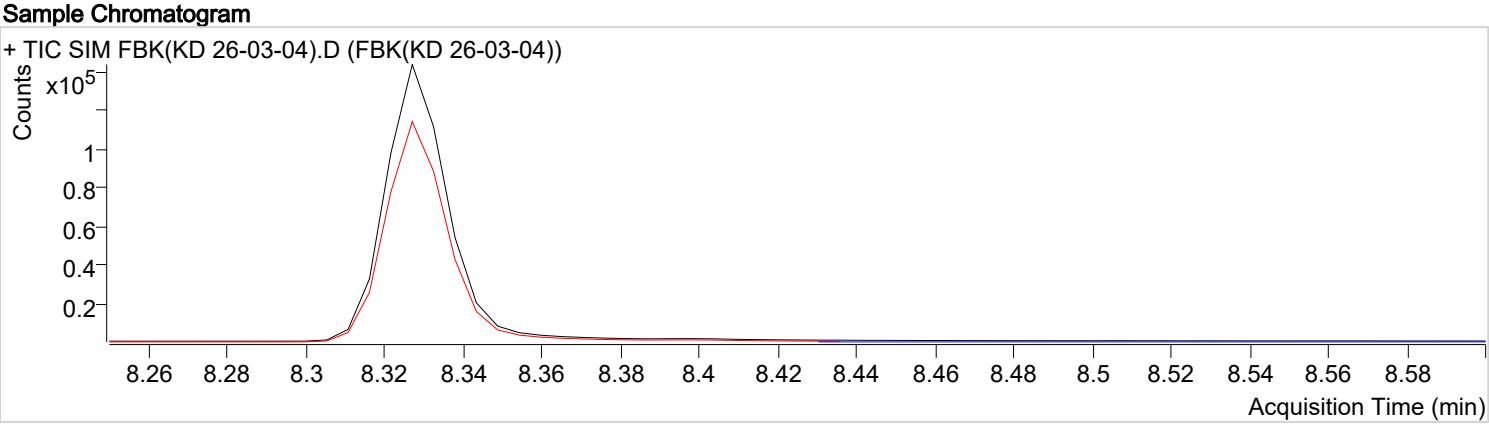

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			126837	ND mg/L

Pentachlorophenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 5:36:14	**Data File**	RE-01.D
Type	Sample	**Name**	RE-01
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

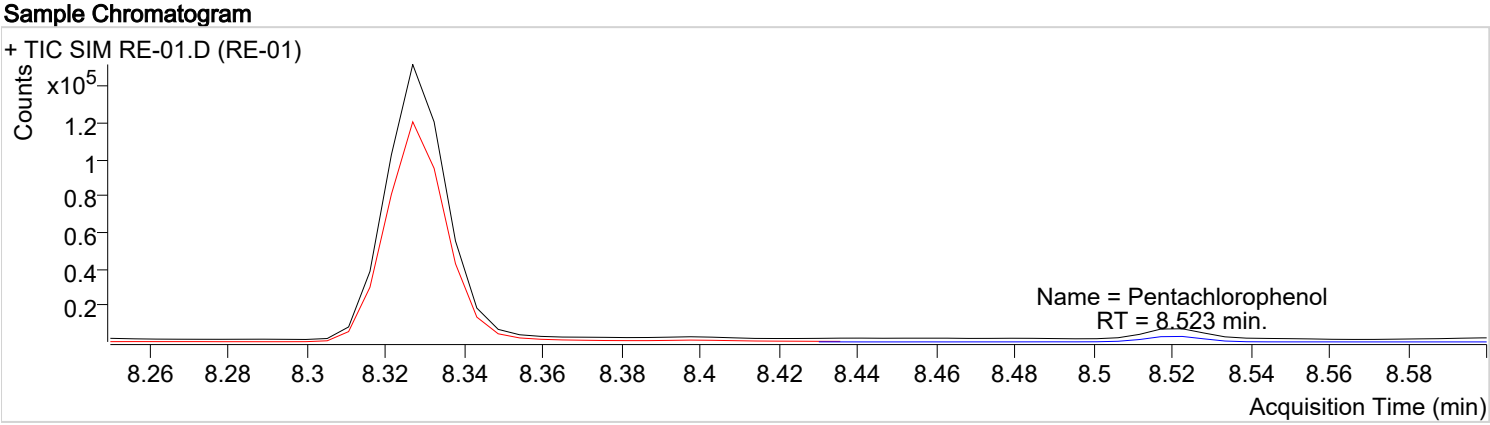

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	3248	126669	0.0018 mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 5:49:37	**Data File**	RE-02.D
Type	Sample	**Name**	RE-02
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

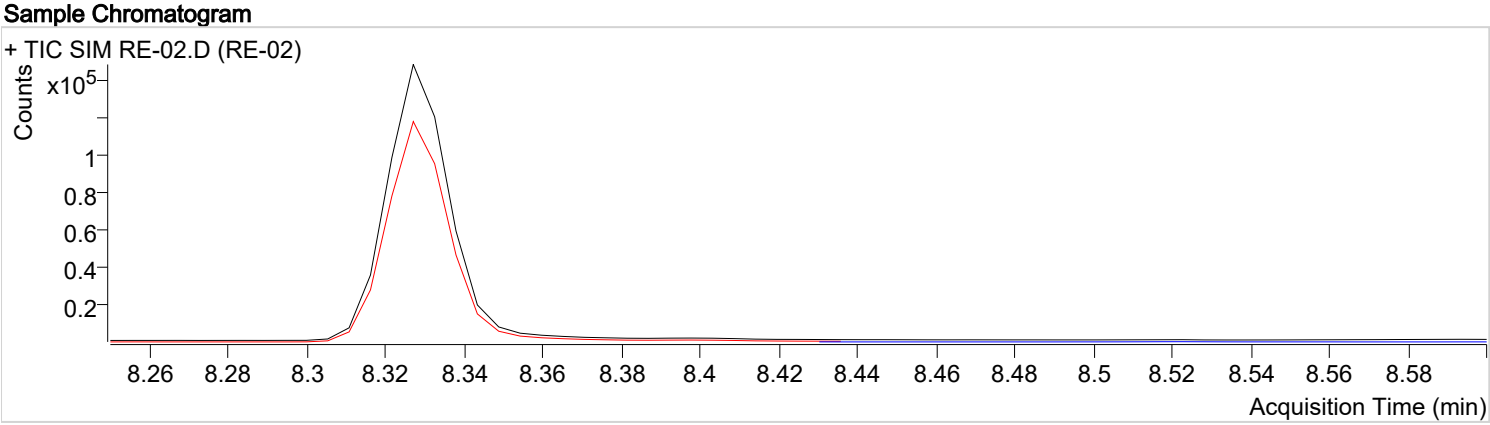

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			131472	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 6:02:58	**Data File**	RE-03.D
Type	Sample	**Name**	RE-03
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

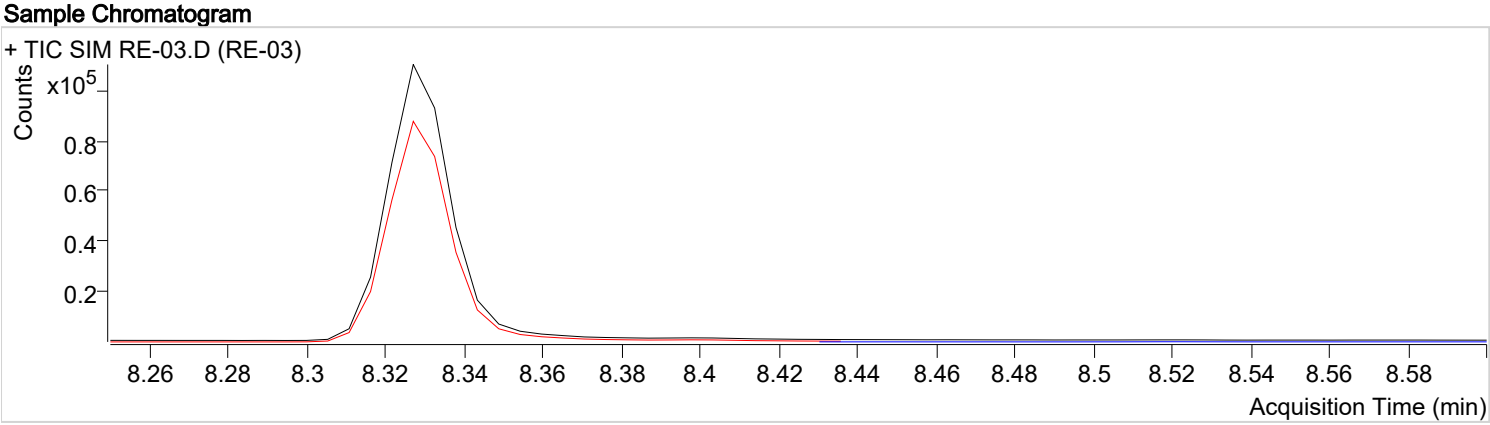

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			99413	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 6:16:20	**Data File**	RE-04.D
Type	Sample	**Name**	RE-04
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

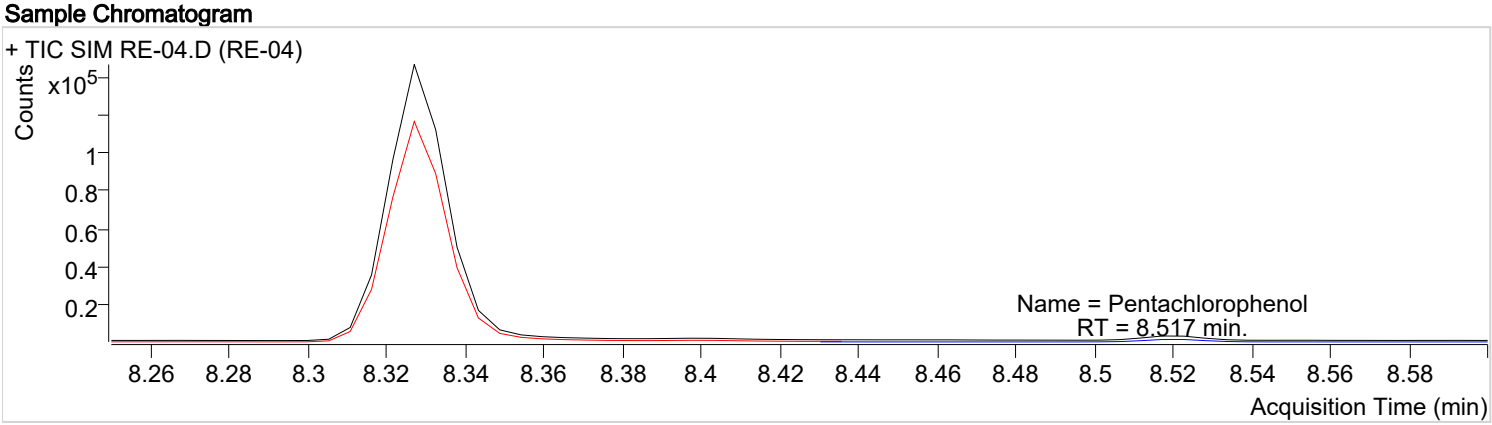

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.517	1436	124077	0.0014 mg/L

Pentachlorophenol





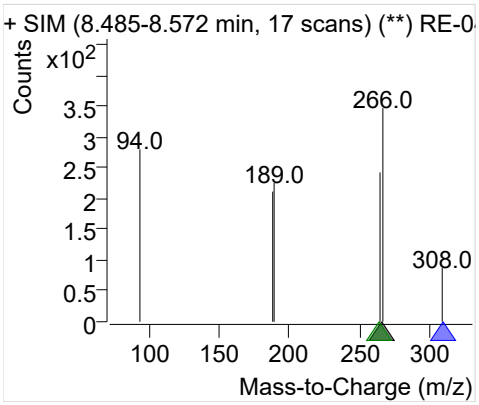

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 6:29:41	**Data File**	RE-09.D
Type	Sample	**Name**	RE-09
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

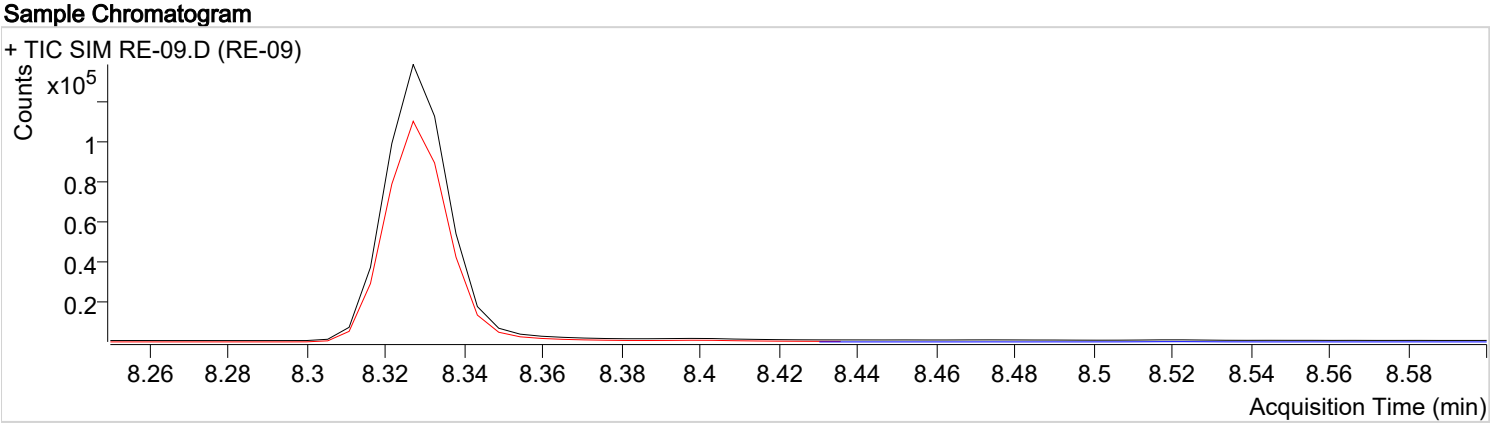

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			124807	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 6:43:03	**Data File**	RE-10.D
Type	Sample	**Name**	RE-10
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

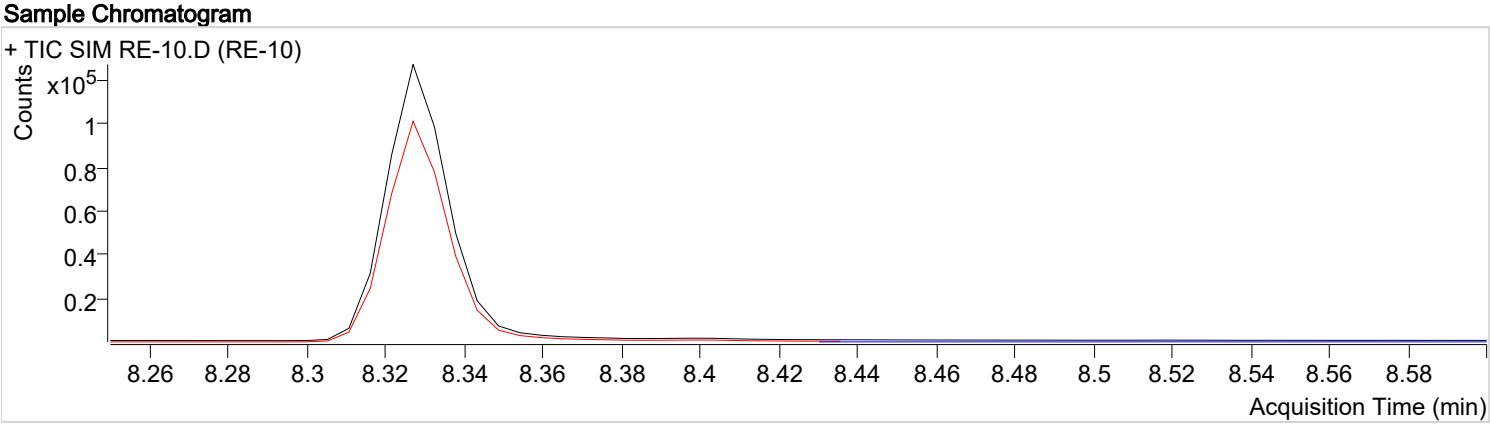

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			112072	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 6:56:25	**Data File**	RE-11.D
Type	Sample	**Name**	RE-11
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

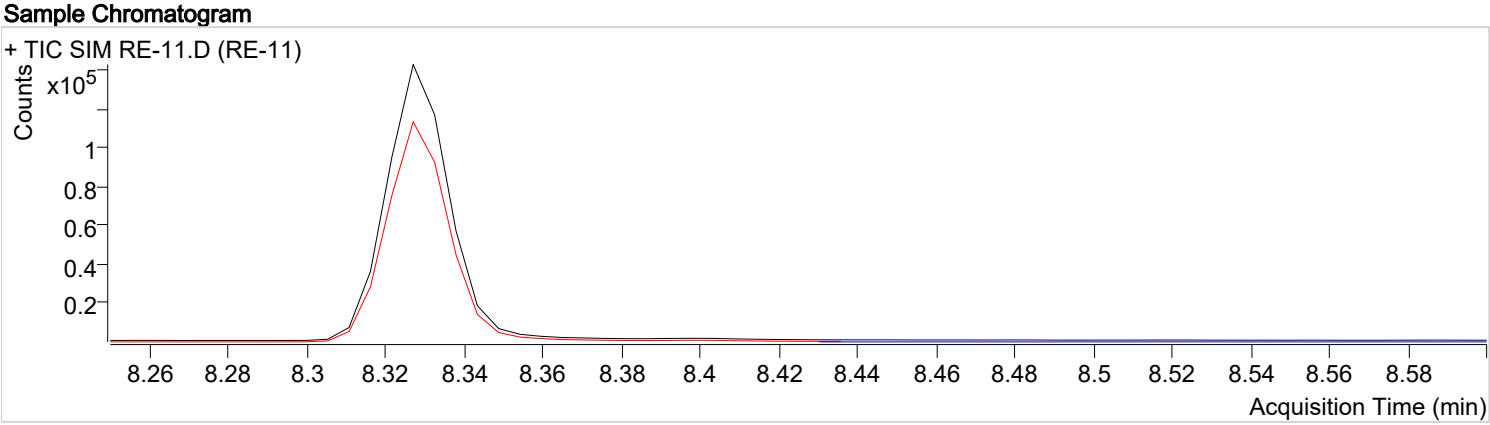

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			126187	ND mg/L

Pentachlorophenol





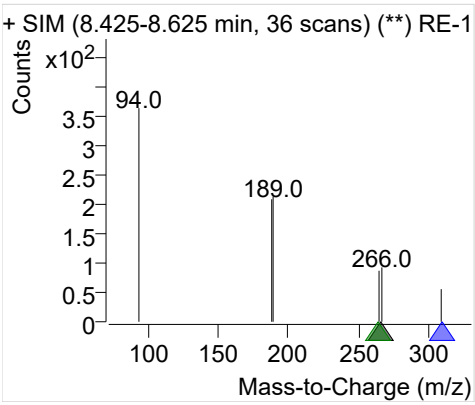

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 7:09:46	**Data File**	RE-12.D
Type	Sample	**Name**	RE-12
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

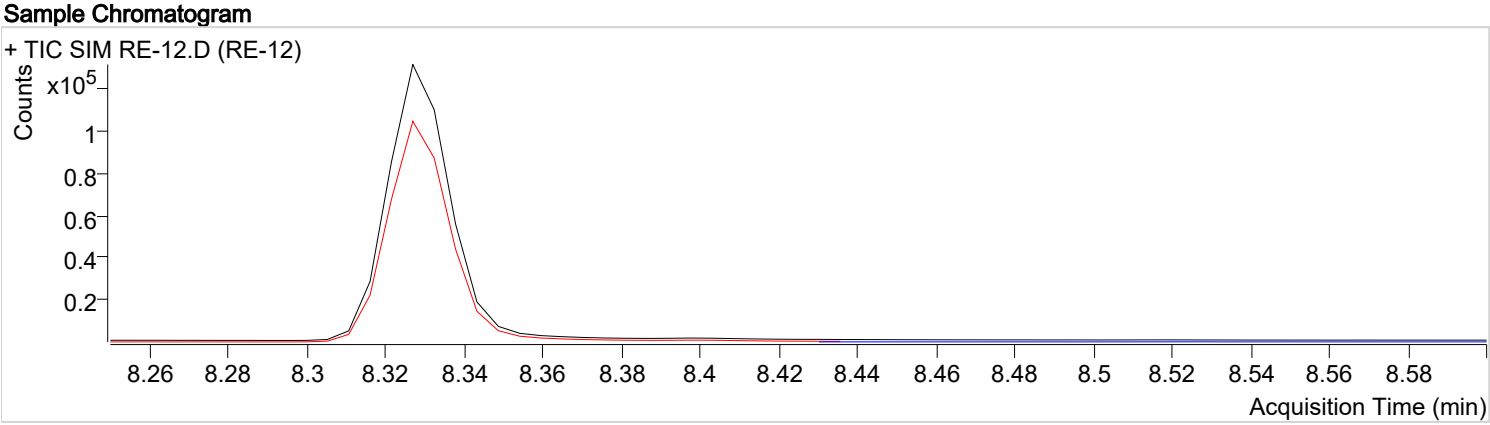

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			116712	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 7:23:10	**Data File**	KD-01.D
Type	Sample	**Name**	KD-01
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

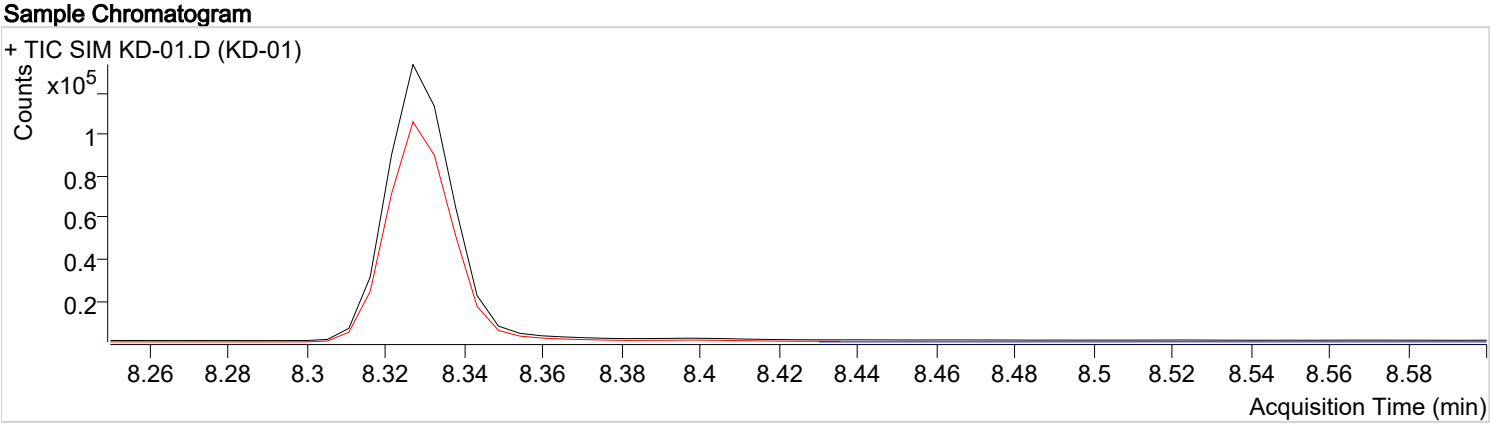

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			123791	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 7:36:31	**Data File**	KD-02.D
Type	Sample	**Name**	KD-02
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

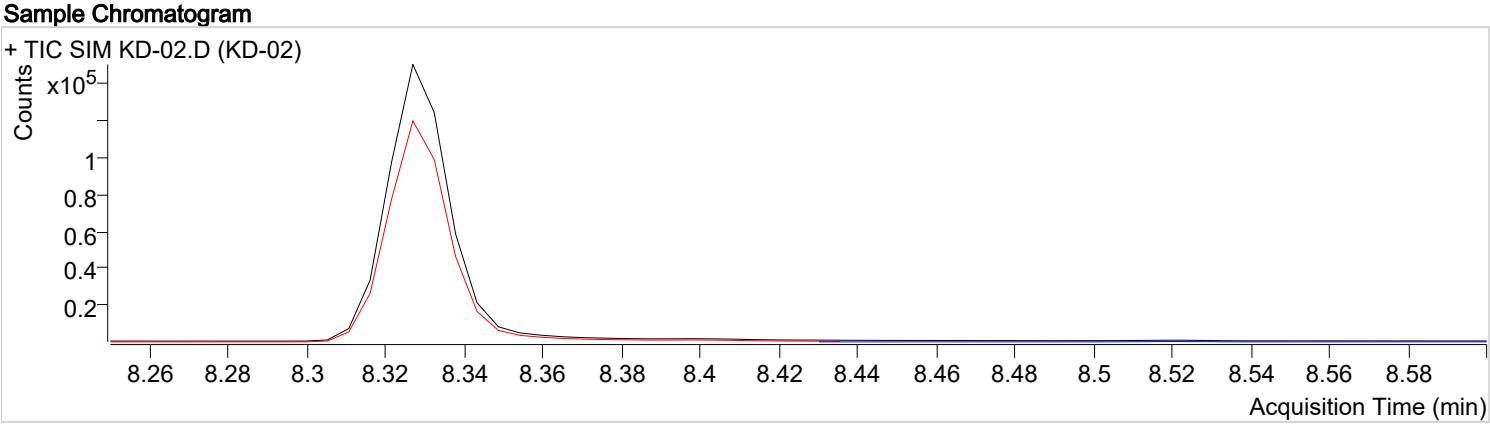

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			133801	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 7:49:53	**Data File**	KD-03.D
Type	Sample	**Name**	KD-03
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

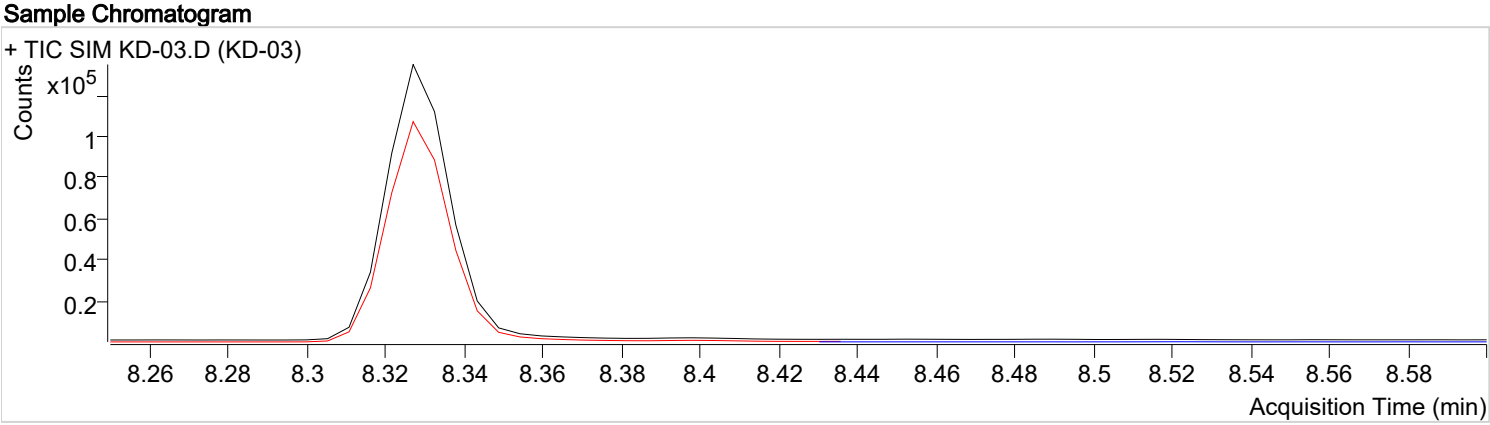

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			120648	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 8:03:15	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

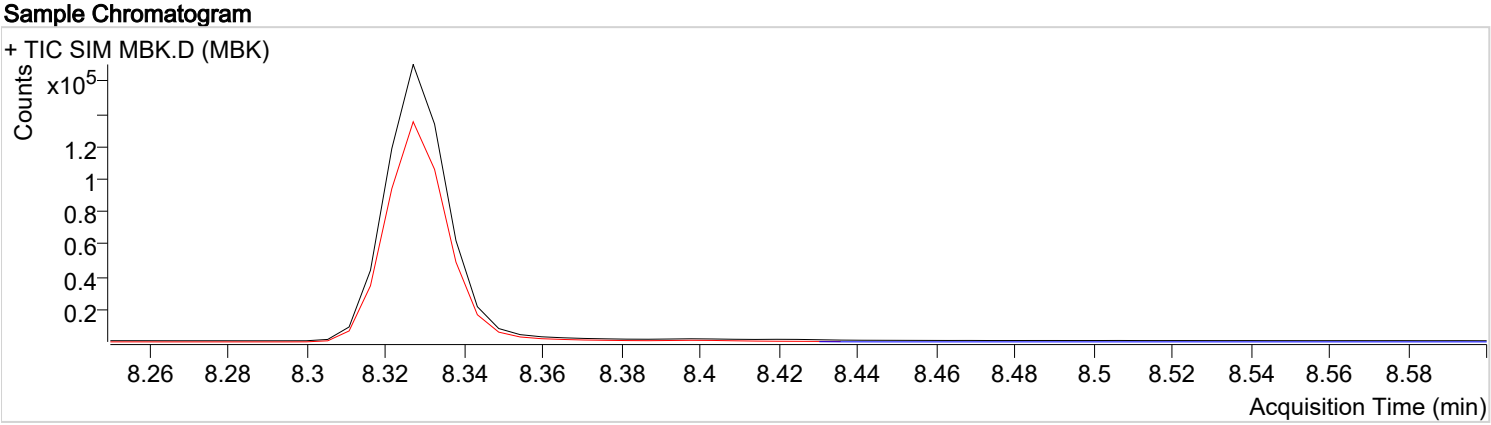

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			149422	ND mg/L

Pentachlorophenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.4, KD 3.4)\QuantResults\PENTQA.batch.bin		
Analysis Time	2026-03-06 오후 2:58:19	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:44:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 2:58:19	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 8:29:59	**Data File**	-CCV-.D
Type	QC	**Name**	-CCV-
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

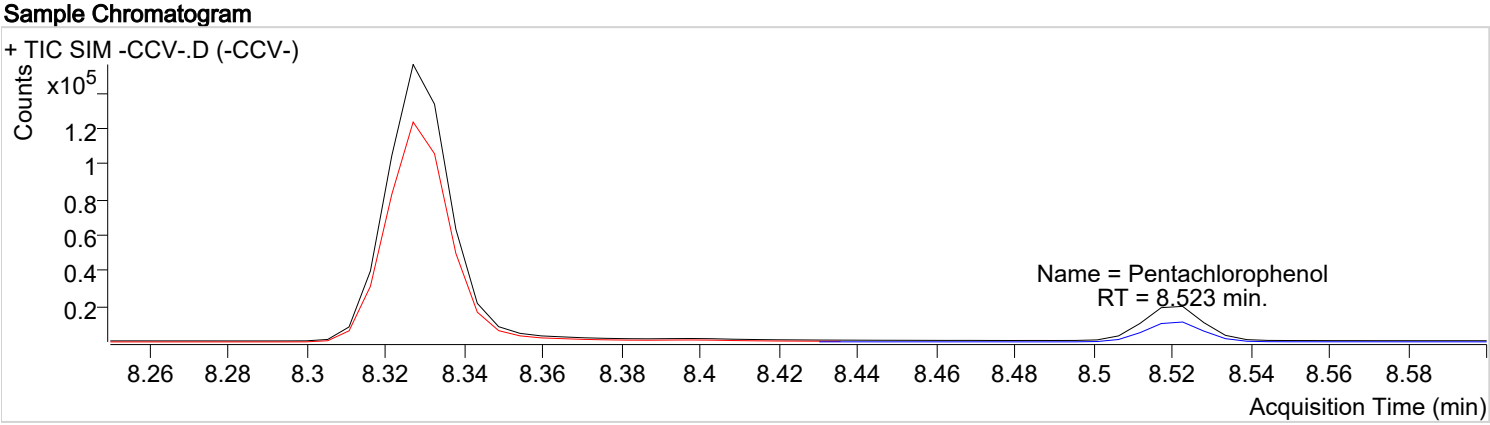

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	11853	141582	0.0036 mg/L
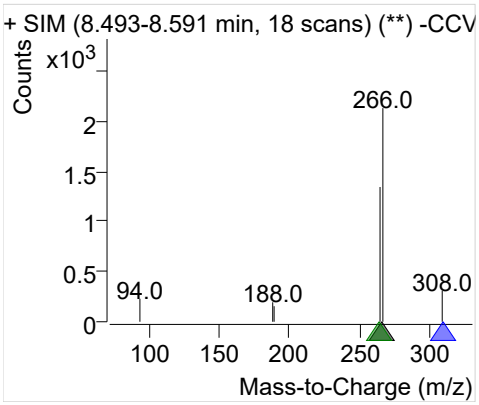
Pentachlorophenol