Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\QuantResults\PENTA.batch.bin				
Analysis Time	2026-03-24 오전 11:26:26	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:26:26	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Pentachlorophenol

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
PENTA ST-01.D	Cal	8.523	1466	82727	0.0012
PENTA ST-02.D	Cal	8.523	2776	71820	0.0020
PENTA ST-03.D	Cal	8.523	4004	67839	0.0028
PENTA ST-04.D	Cal	8.523	6374	74999	0.0038
PENTA ST-05.D	Cal	8.523	7024	61007	0.0050
PENTA ST-06.D	Cal	8.523	9011	64531	0.0059
PENTA ST-07.D	Cal	8.523	13245	67195	0.0082
BK-.D	Blank			59522	ND
FBK(RE 26-03-17).D	Blank			48326	ND
FBK(RE 26-03-18).D	Blank			57767	ND
RE-05.D	Sample			48493	ND
RE-06.D	Sample			54388	ND
RE-13.D	Sample			64560	ND
RE-14.D	Sample			73498	ND
RE-24.D	Sample			72495	ND
RE-25.D	Sample			81558	ND
MBK.D	Blank			72042	ND
-CCV-.D	QC	8.523	6419	71453	0.0040

Pentachlorophenol

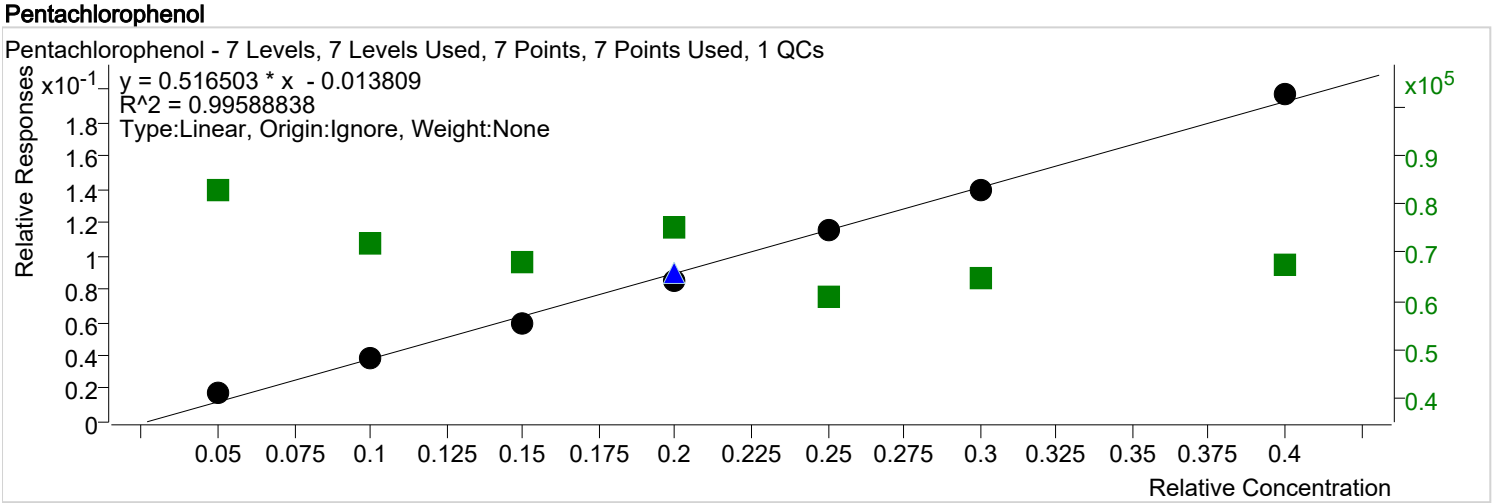

Cal. Path	Type	Level	Enable	Conc.	Response
\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\PENTAST-01.D	Calibration	1	x	0.500	1466
\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\PENTAST-02.D	Calibration	2	x	1.000	2776
\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\PENTAST-03.D	Calibration	3	x	1.500	4004
\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\PENTAST-04.D	Calibration	4	x	2.000	6374
\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\-CCV-.D	QC	4	x	2.000	6419
\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\PENTAST-05.D	Calibration	5	x	2.500	7024
\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\PENTAST-06.D	Calibration	6	x	3.000	9011
\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\PENTAST-07.D	Calibration	7	x	4.000	13245

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-24 오전 11:26:26	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:26:26	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-19 오후 5:55:07	**Data File**	PENTA ST-01.D
Type	Cal	**Name**	PENTA ST-01
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

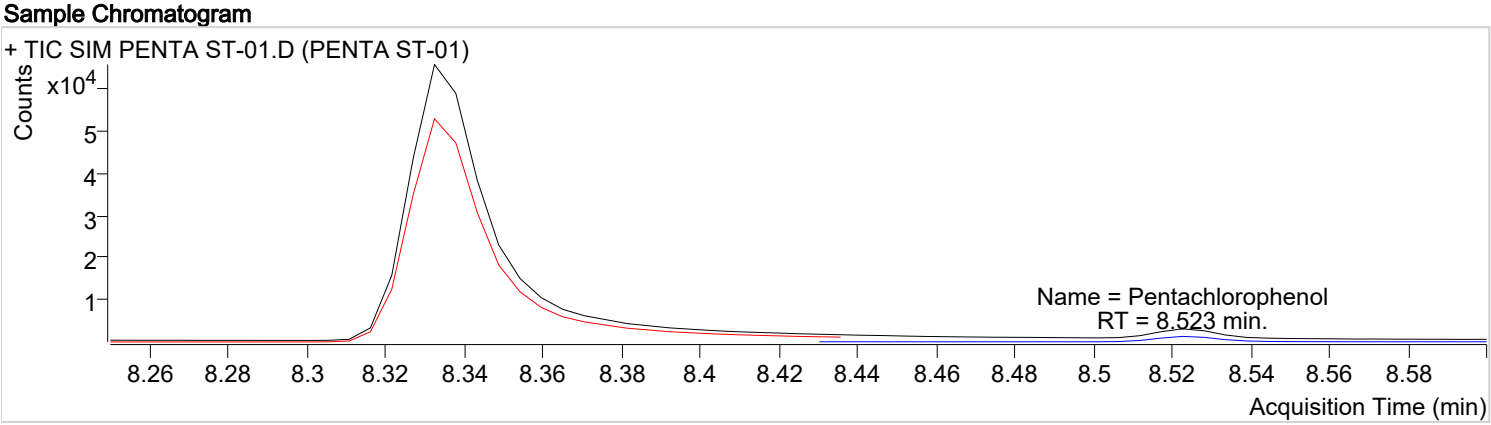

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	1466	82727	0.0012 mg/L

Pentachlorophenol





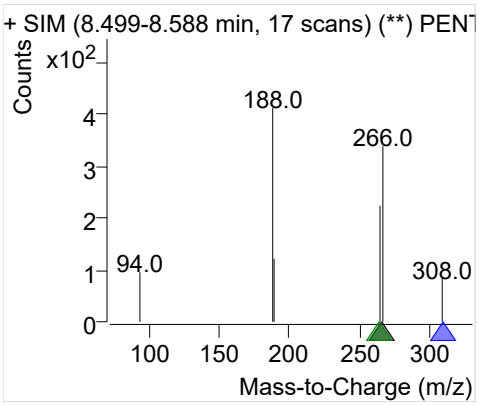

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-24 오전 11:26:26	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:26:26	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-19 오후 6:08:29	**Data File**	PENTA ST-02.D
Type	Cal	**Name**	PENTA ST-02
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

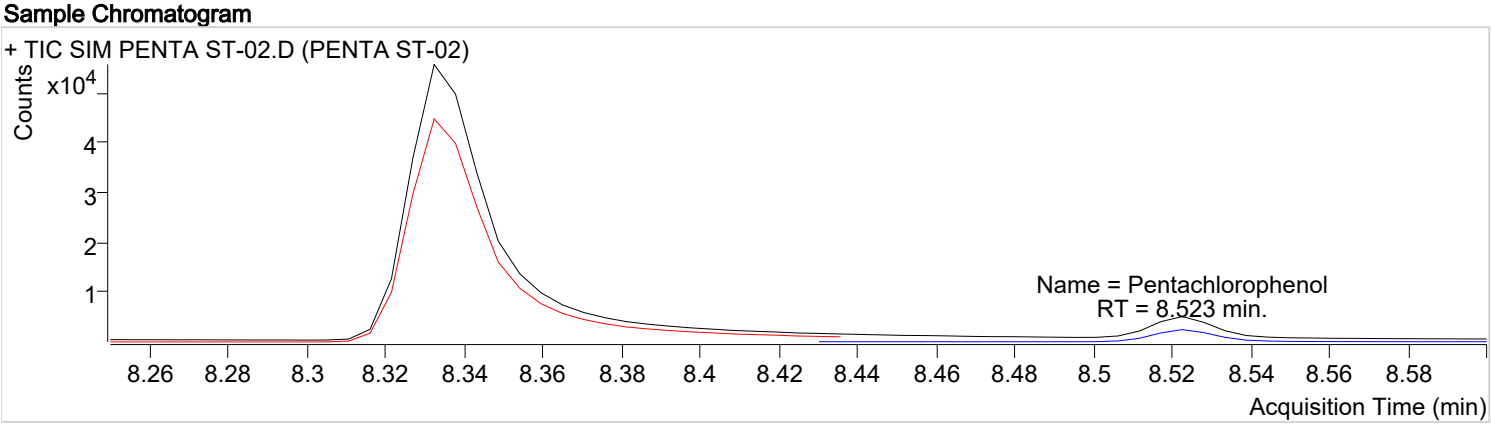

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	2776	71820	0.0020 mg/L

Pentachlorophenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-24 오전 11:26:26	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:26:26	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-19 오후 6:21:54	**Data File**	PENTA ST-03.D
Type	Cal	**Name**	PENTA ST-03
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

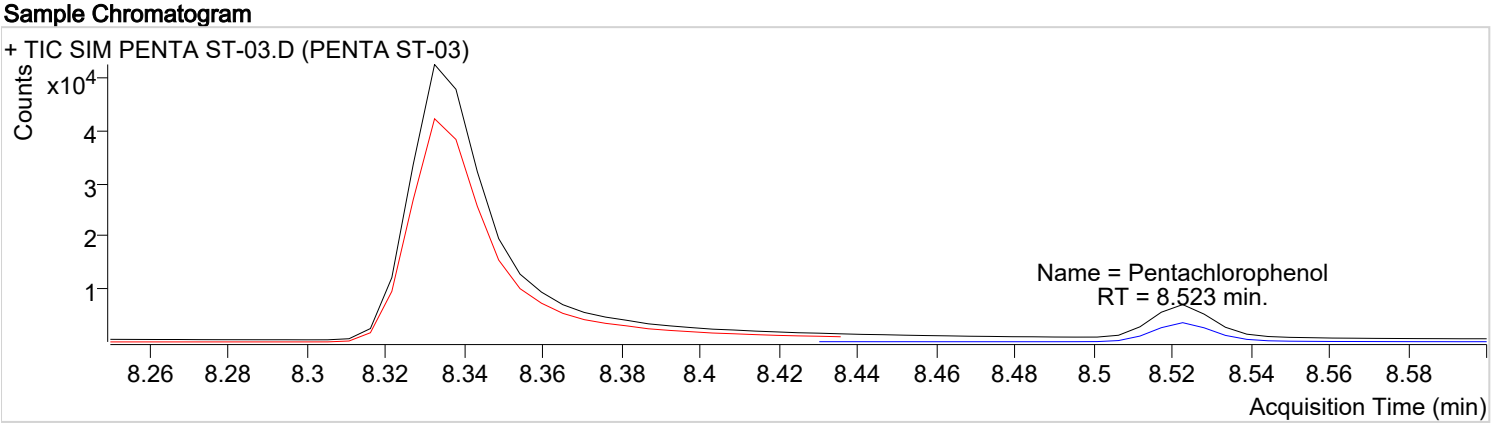

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	4004	67839	0.0028 mg/L

Pentachlorophenol

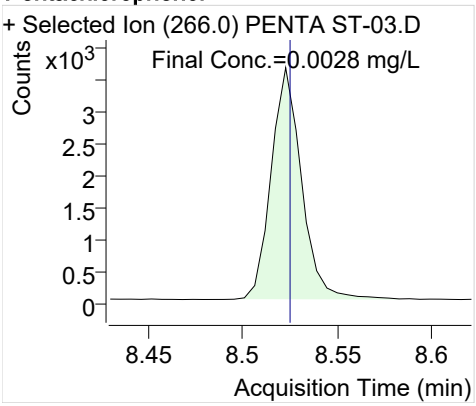

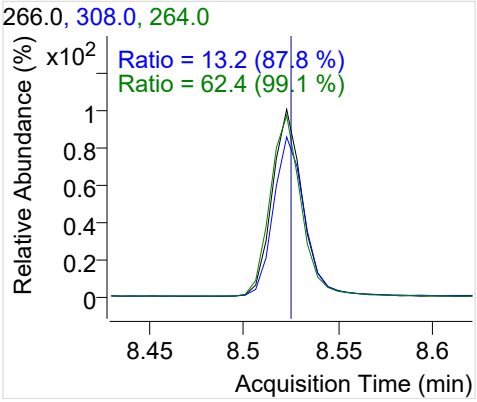

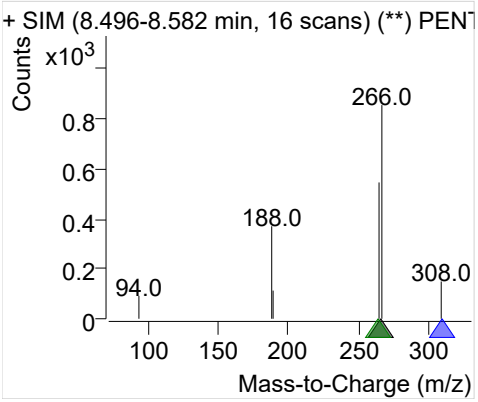

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-24 오전 11:26:26	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:26:26	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-19 오후 6:35:15	**Data File**	PENTA ST-04.D
Type	Cal	**Name**	PENTA ST-04
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

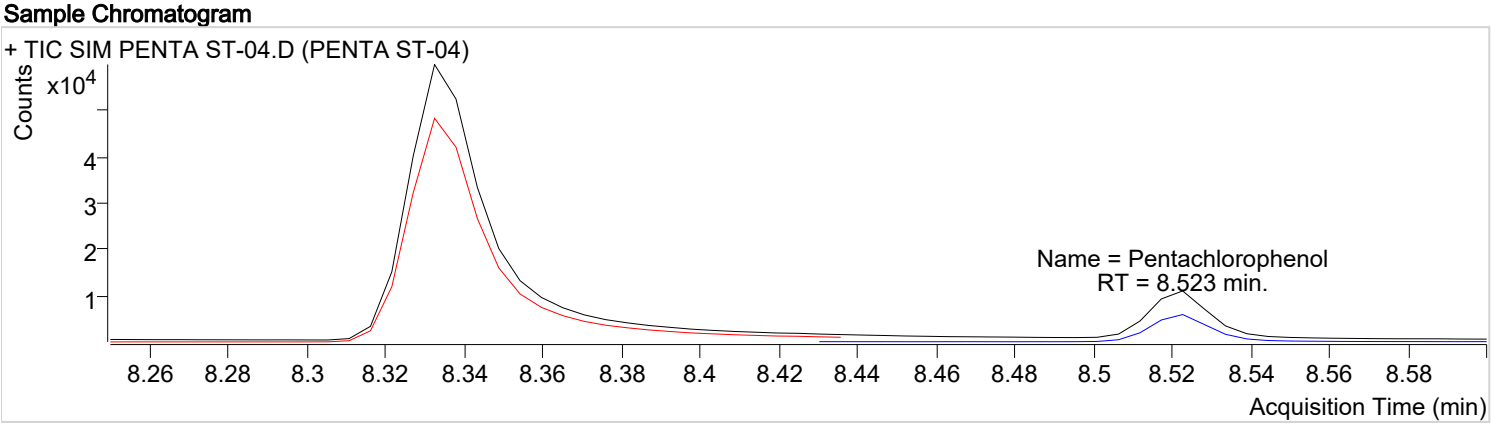

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	6374	74999	0.0038 mg/L

Pentachlorophenol





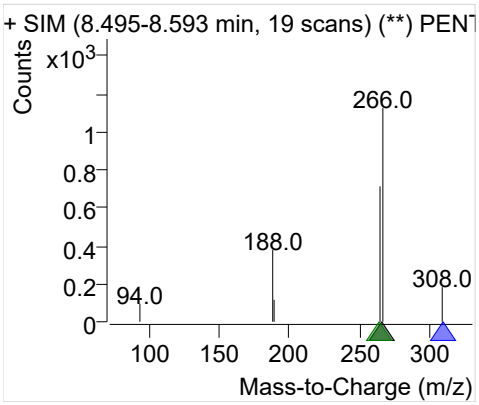

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-24 오전 11:26:26	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:26:26	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-19 오후 6:48:38	**Data File**	PENTA ST-05.D
Type	Cal	**Name**	PENTA ST-05
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

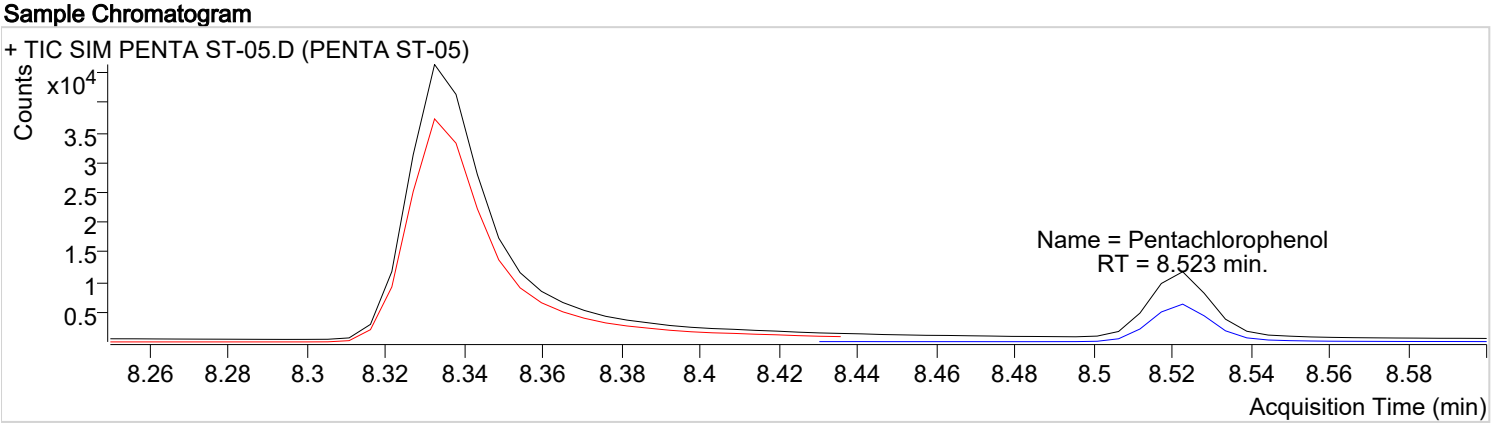

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	7024	61007	0.0050 mg/L

Pentachlorophenol



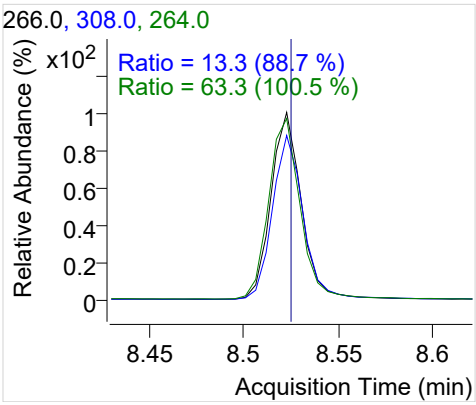



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-24 오전 11:26:26	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:26:26	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-19 오후 7:02:00	**Data File**	PENTA ST-06.D
Type	Cal	**Name**	PENTA ST-06
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

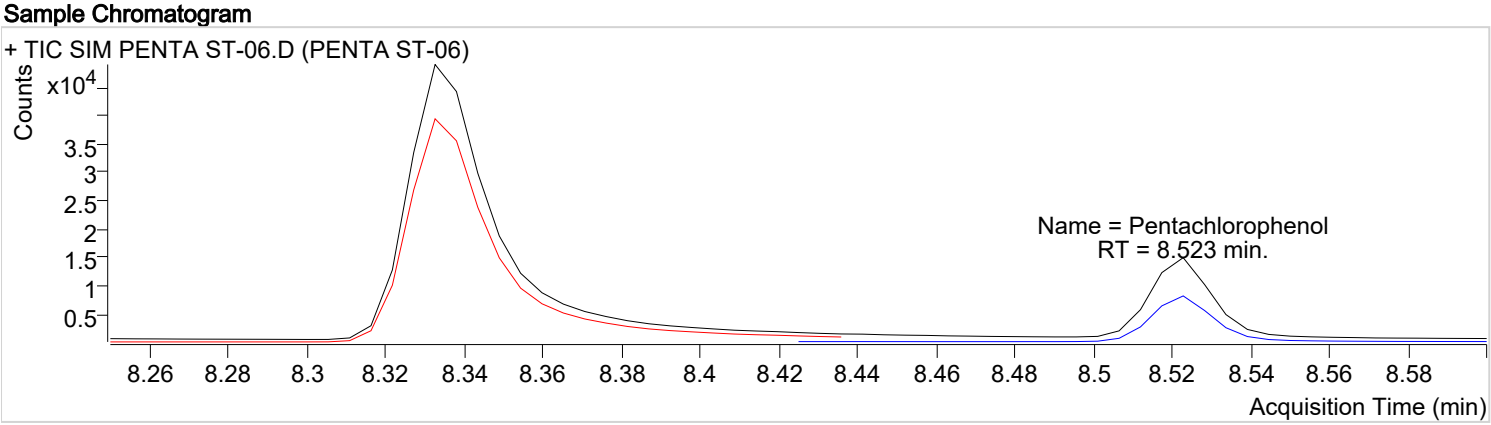

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	9011	64531	0.0059 mg/L

Pentachlorophenol





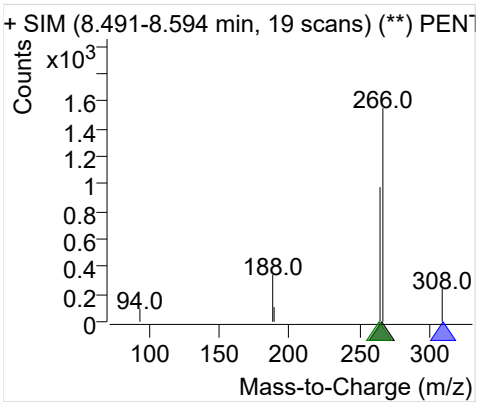

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-24 오전 11:26:26	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:26:26	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-19 오후 7:15:24	**Data File**	PENTA ST-07.D
Type	Cal	**Name**	PENTA ST-07
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

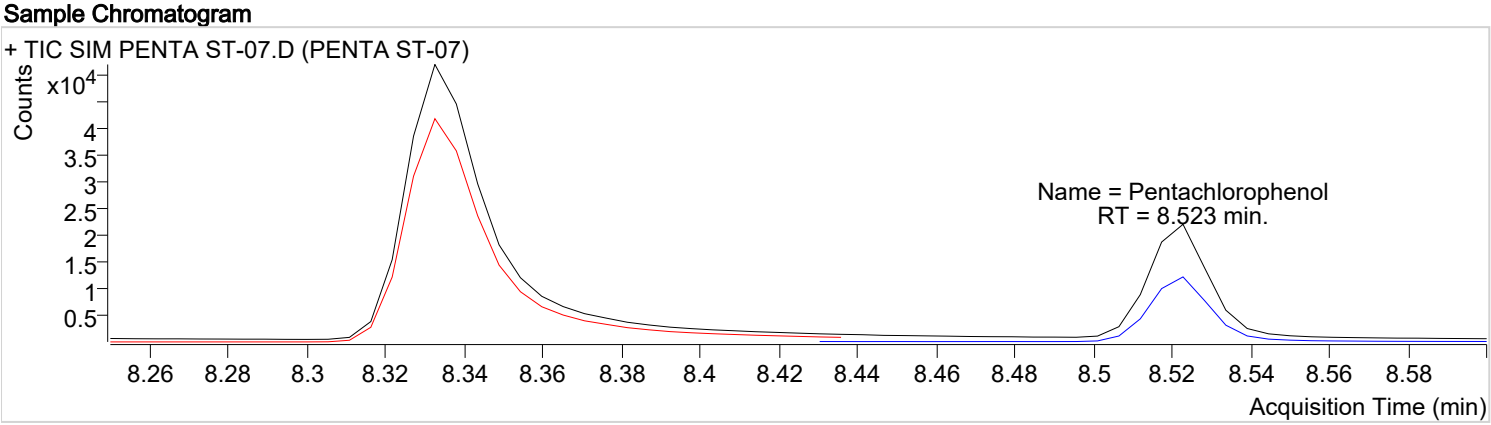

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	13245	67195	0.0082 mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-24 오전 11:26:26	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:26:26	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-19 오후 7:42:11	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

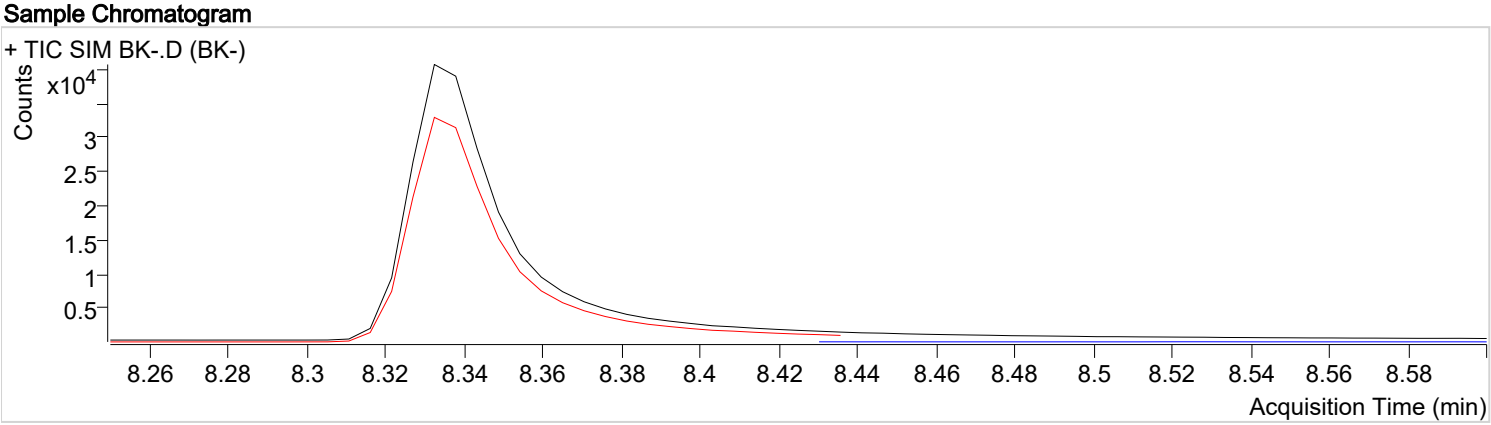

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			59522	ND mg/L

Pentachlorophenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-24 오전 11:26:26	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:26:26	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-19 오후 7:55:33	**Data File**	FBK(RE 26-03-17).D
Type	Blank	**Name**	FBK(RE 26-03-17)
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

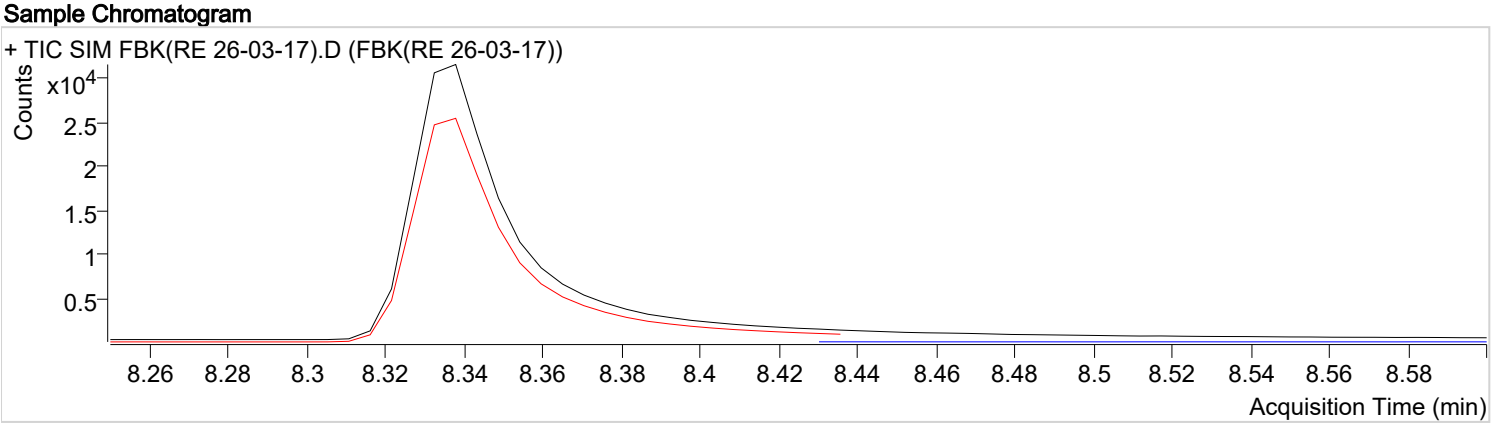

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			48326	ND mg/L

Pentachlorophenol





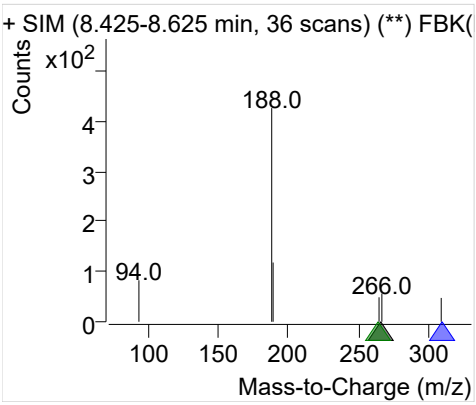

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-24 오전 11:26:26	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:26:26	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-19 오후 8:08:56	**Data File**	FBK(RE 26-03-18).D
Type	Blank	**Name**	FBK(RE 26-03-18)
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

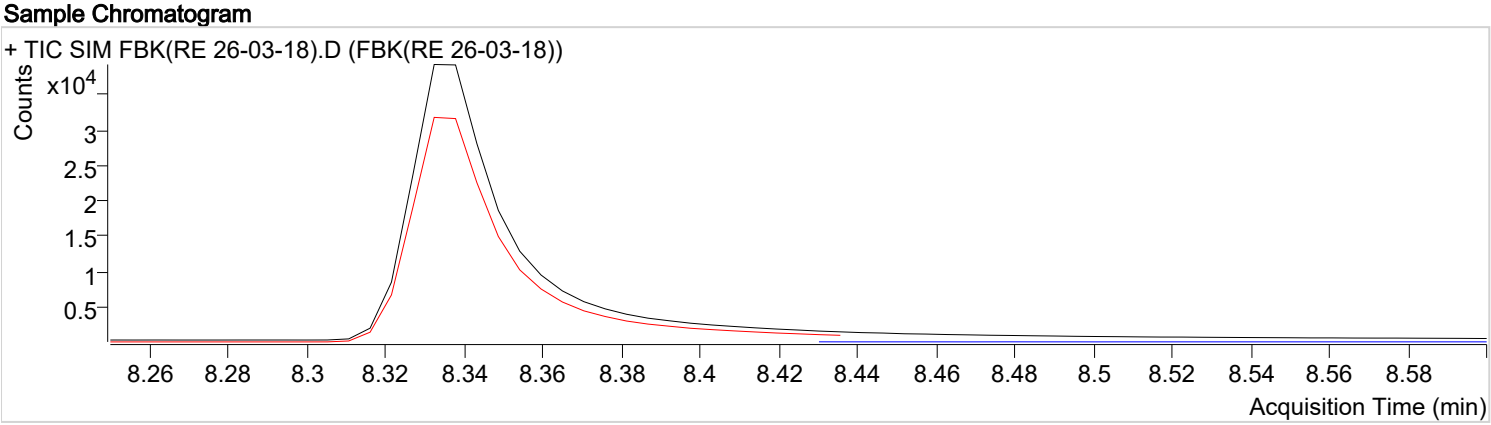

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			57767	ND mg/L

Pentachlorophenol





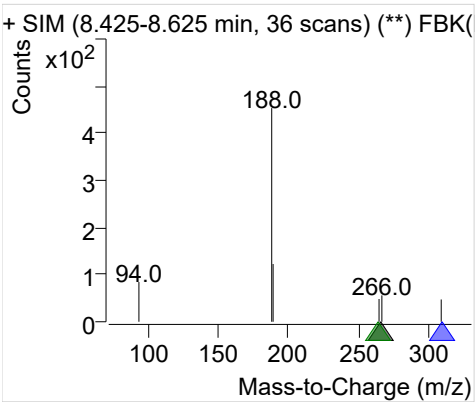

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-24 오전 11:26:26	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:26:26	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-19 오후 8:22:18	**Data File**	RE-05.D
Type	Sample	**Name**	RE-05
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

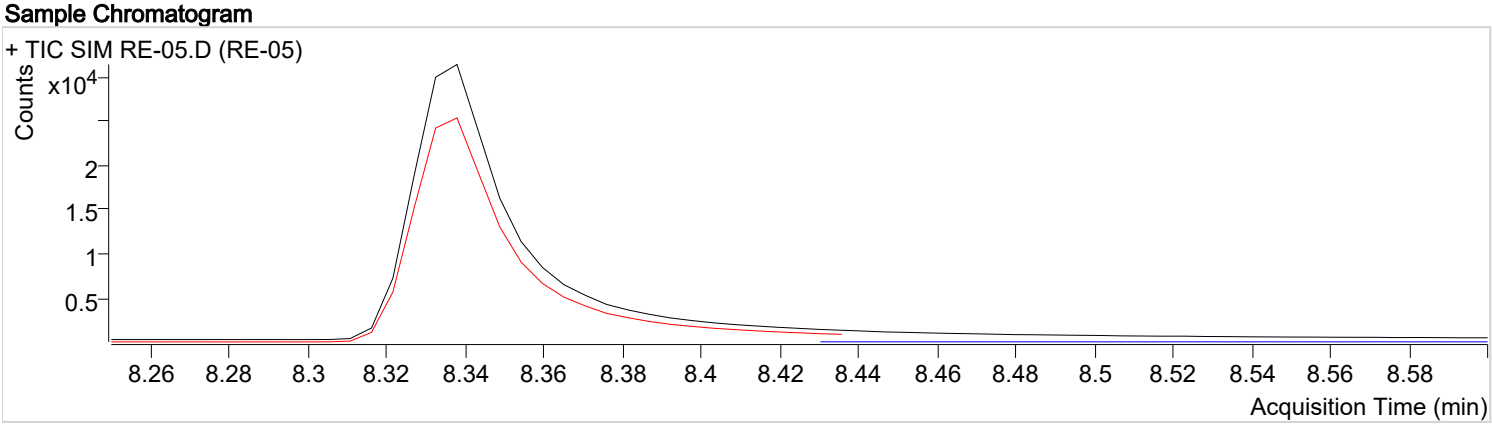

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			48493	ND mg/L

Pentachlorophenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-24 오전 11:26:26	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:26:26	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-19 오후 8:35:40	**Data File**	RE-06.D
Type	Sample	**Name**	RE-06
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

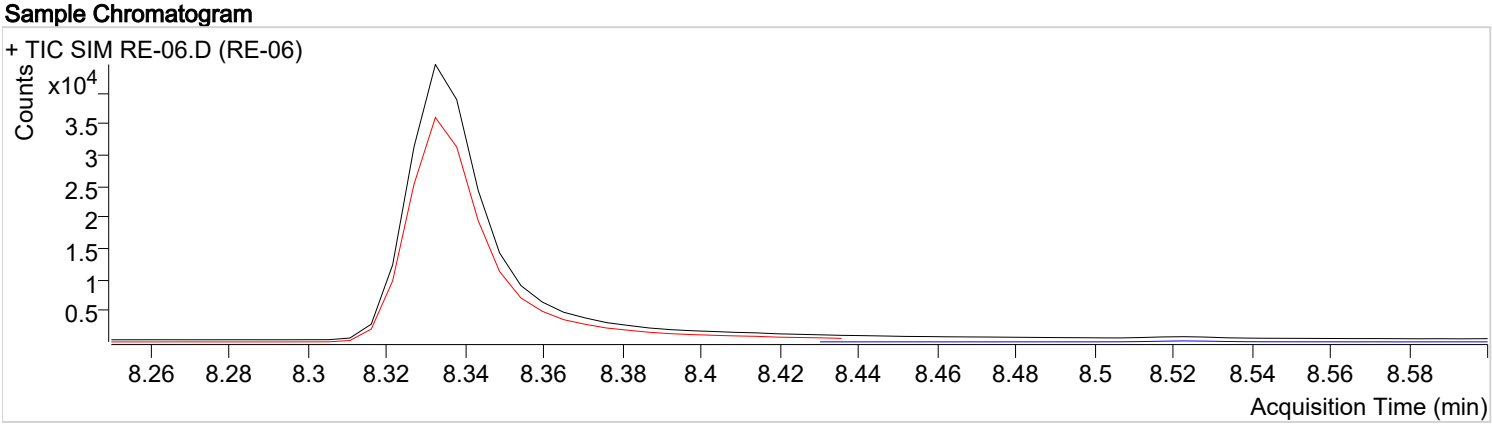

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			54388	ND mg/L

Pentachlorophenol

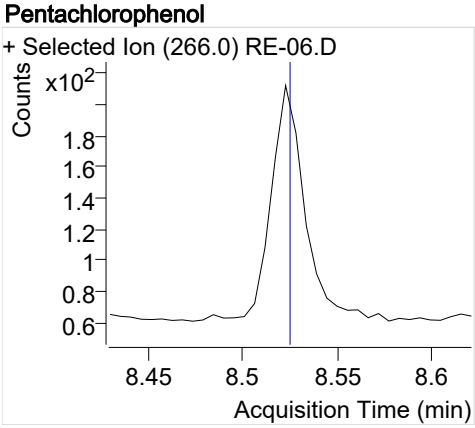

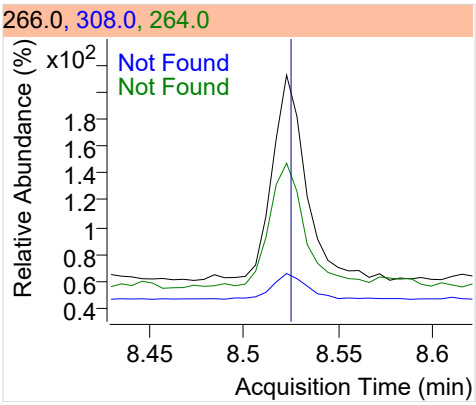



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-24 오전 11:26:26	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:26:26	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-19 오후 8:49:02	**Data File**	RE-13.D
Type	Sample	**Name**	RE-13
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

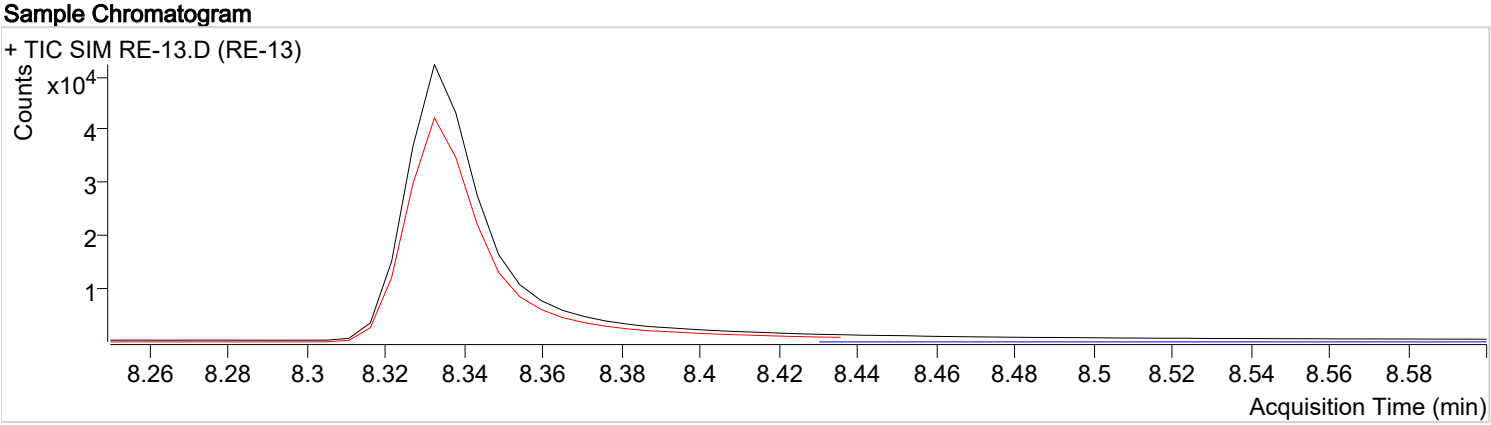

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			64560	ND mg/L

Pentachlorophenol

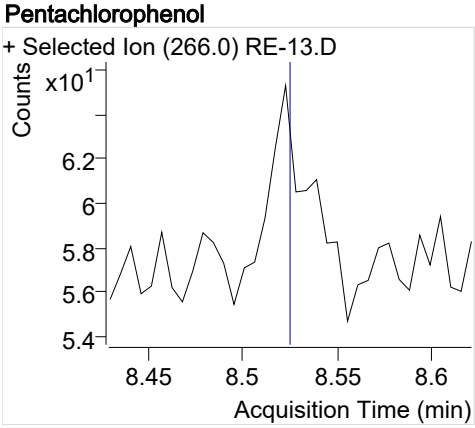

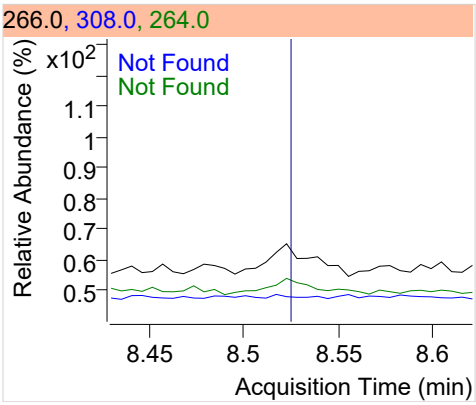



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-24 오전 11:26:26	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:26:26	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-19 오후 9:02:23	**Data File**	RE-14.D
Type	Sample	**Name**	RE-14
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

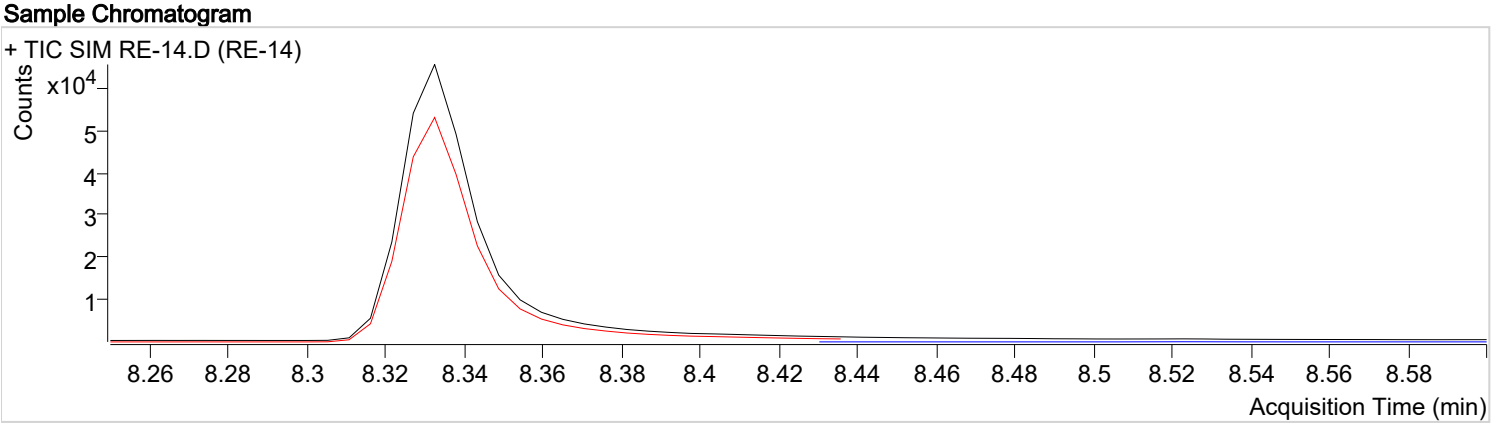

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			73498	ND mg/L

Pentachlorophenol



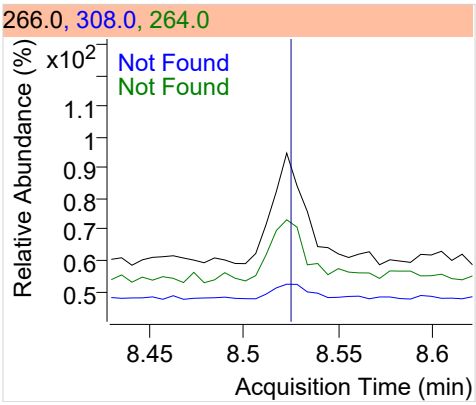



Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-24 오전 11:26:26	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:26:26	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-19 오후 9:15:46	**Data File**	RE-24.D
Type	Sample	**Name**	RE-24
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

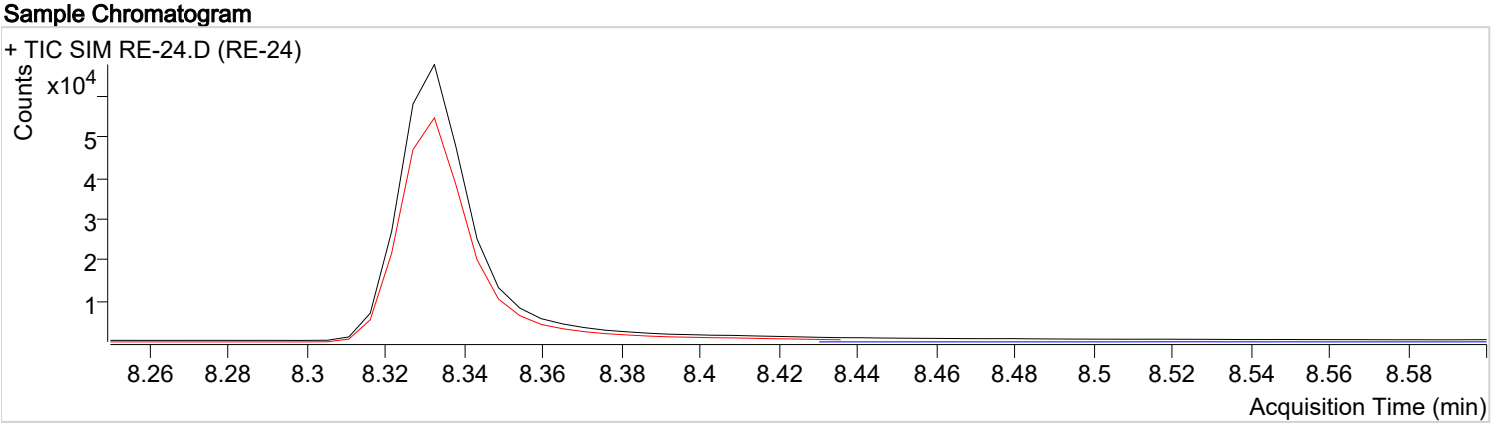

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			72495	ND mg/L

Pentachlorophenol







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-24 오전 11:26:26	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:26:26	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-19 오후 9:29:10	**Data File**	RE-25.D
Type	Sample	**Name**	RE-25
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

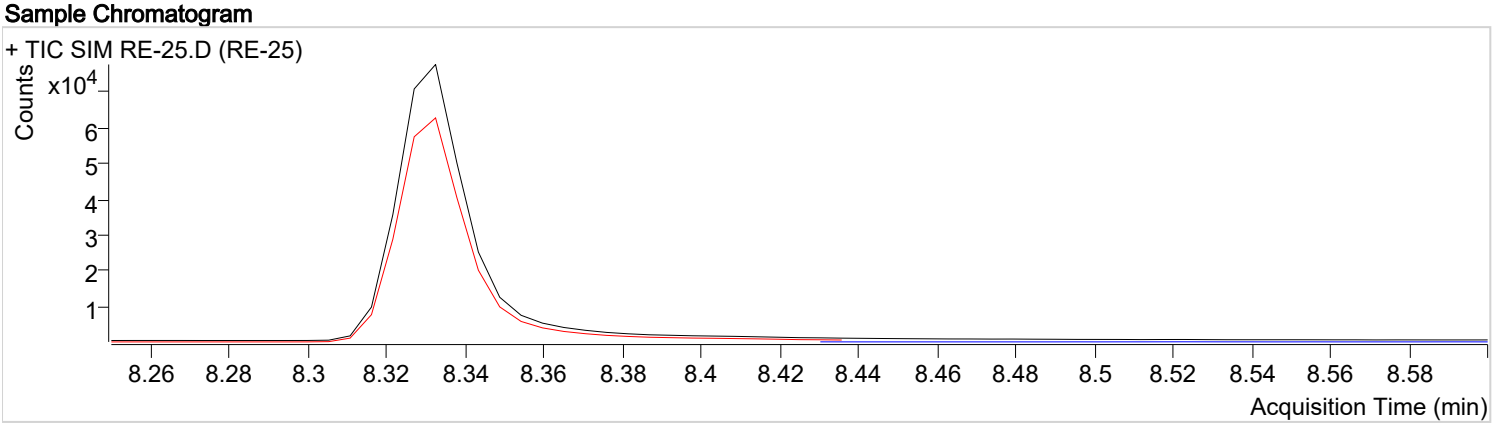

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			81558	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-24 오전 11:26:26	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:26:26	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-19 오후 9:42:33	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

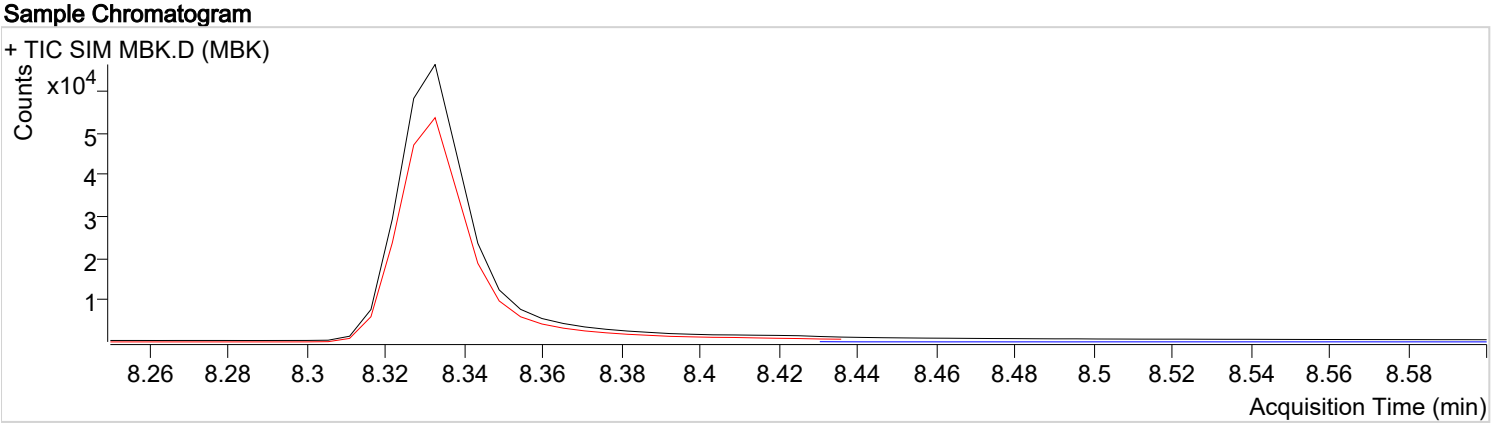

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			72042	ND mg/L

Pentachlorophenol

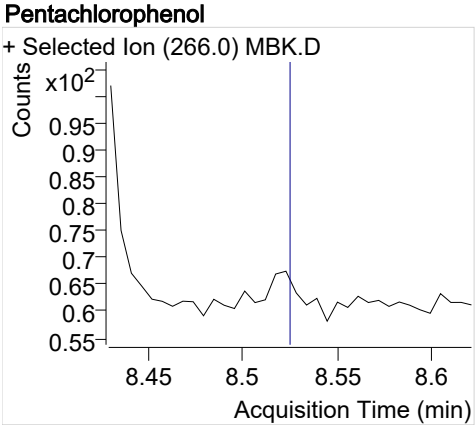

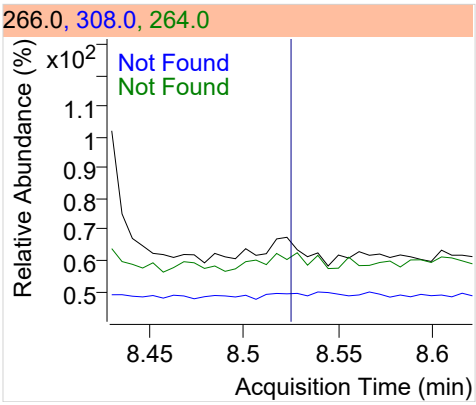



Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(RE 3.17 RE 3.18)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-24 오전 11:26:26	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:00	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-24 오전 11:26:26	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-19 오후 10:09:17	**Data File**	-CCV-.D
Type	QC	**Name**	-CCV-
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

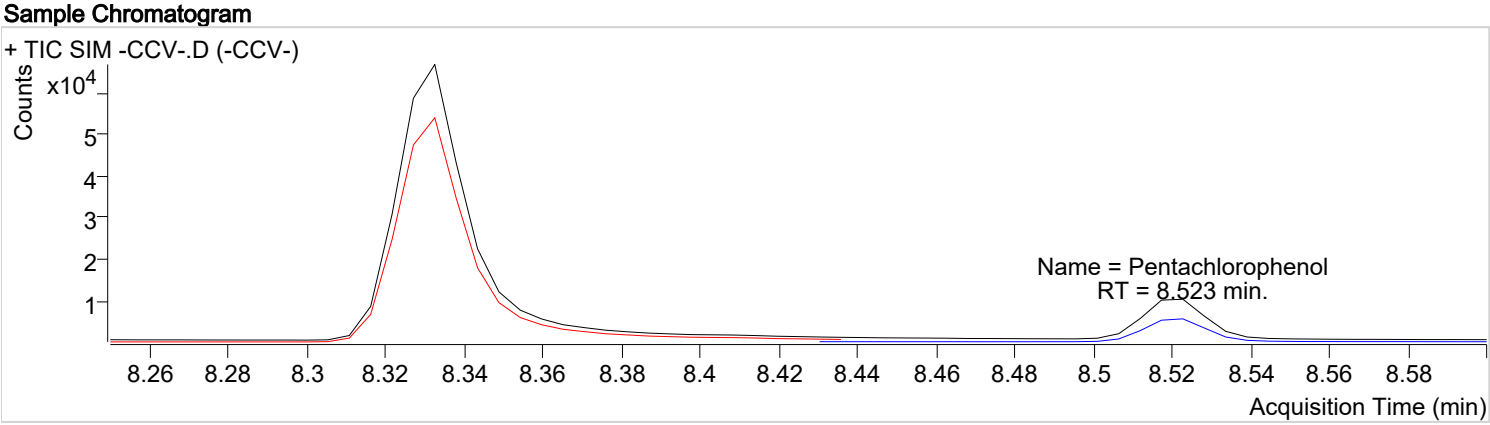

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	6419	71453	0.0040 mg/L
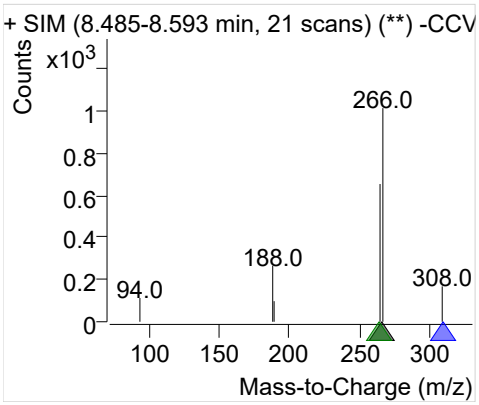
Pentachlorophenol